


Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY081325\
Data File : VY023058.D
Acq On : 13 Aug 2025 08:21
Operator : SY/MD
Sample : BFB
Misc : 5.00g/5.0mL/MSVOA_Y/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_Y
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y081225S.M
Title : SW846 8260
Last Update : Wed Aug 13 02:10:11 2025

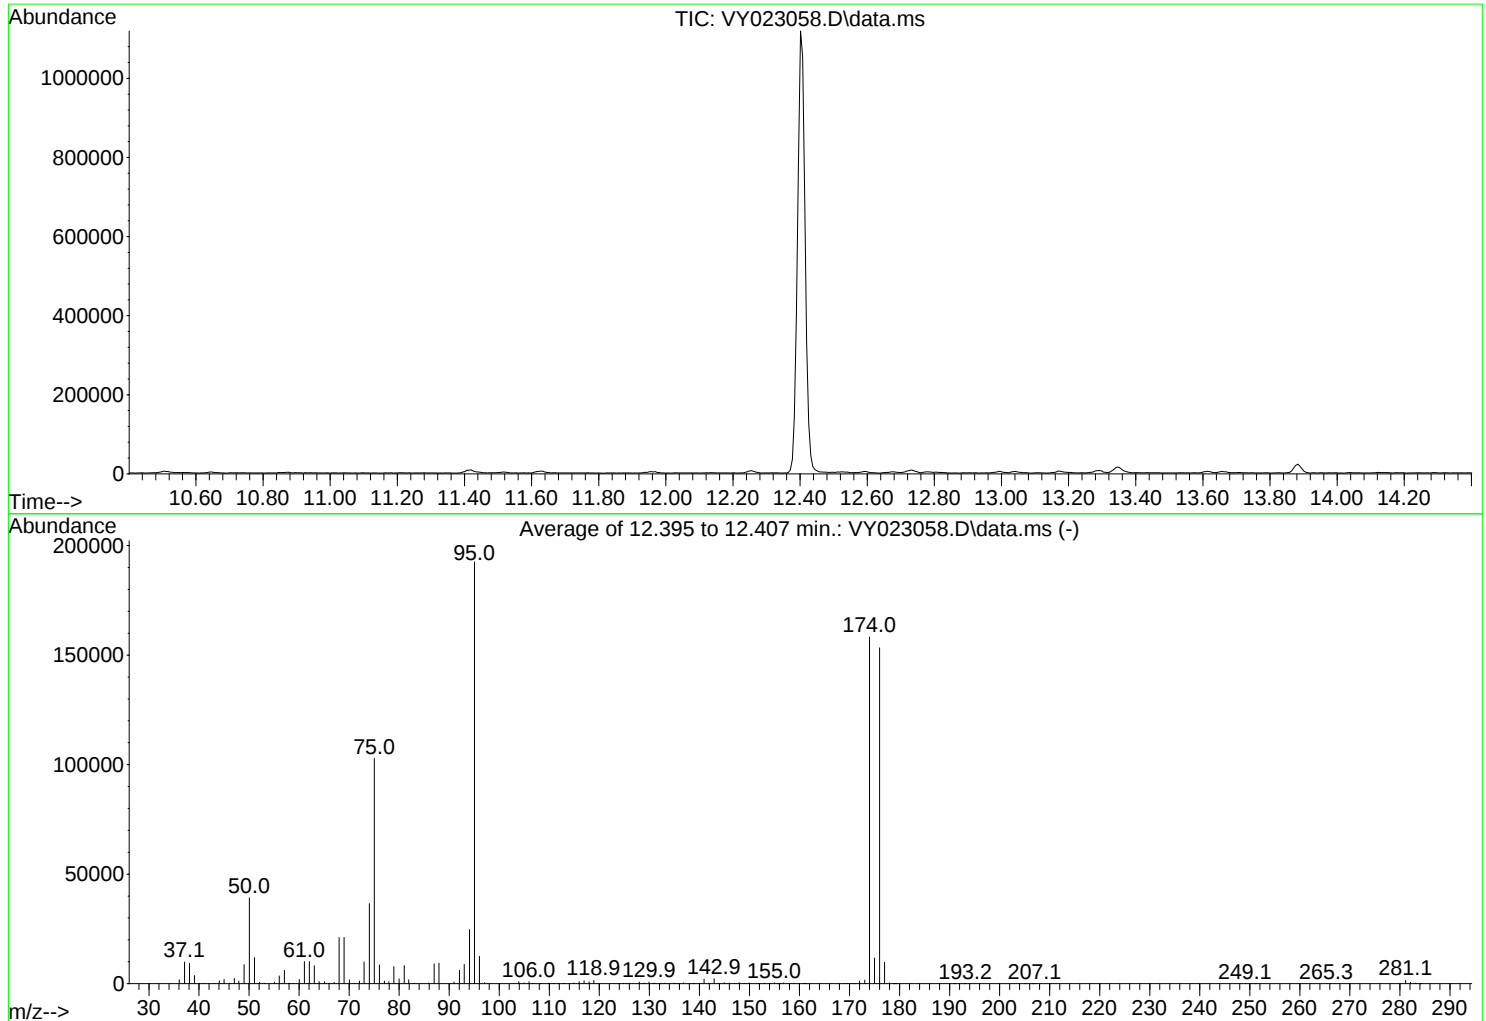

AutoFind: Scans 1751, 1752, 1753; Background Corrected with Scan 1743

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	20.3	39163	PASS
75	95	30	60	53.4	102800	PASS
95	95	100	100	100.0	192597	PASS
96	95	5	9	6.4	12401	PASS
173	174	0.00	2	1.0	1625	PASS
174	95	50	100	82.2	158224	PASS
175	174	5	9	7.4	11707	PASS
176	174	95	101	96.9	153344	PASS
177	176	5	9	6.4	9830	PASS