

Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY081325\
 Data File : VY023081.D
 Acq On : 13 Aug 2025 19:38
 Operator : SY/MD
 Sample : Q2819-19
 Misc : 6.73g/5.0mL/MSVOA_Y/SOIL/A
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 MSVOA_Y
 ClientSampleId :
 38M-E

Quant Time: Aug 14 01:29:07 2025
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y081225S.M
 Quant Title : SW846 8260
 QLast Update : Wed Aug 13 02:10:11 2025
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Pentafluorobenzene	7.707	168	641351	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	8.610	114	1276856	50.000	ug/l	0.00
63) Chlorobenzene-d5	11.414	117	1106347	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.340	152	424298	50.000	ug/l	0.00

System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	8.055	65	379278	62.049	ug/l	0.00
Spiked Amount	50.000	Range	50 - 163	Recovery	=	124.100%
35) Dibromofluoromethane	7.628	113	407347	53.316	ug/l	0.00
Spiked Amount	50.000	Range	54 - 147	Recovery	=	106.640%
50) Toluene-d8	10.103	98	1563625	52.387	ug/l	0.00
Spiked Amount	50.000	Range	58 - 134	Recovery	=	104.780%
62) 4-Bromofluorobenzene	12.402	95	438170	45.648	ug/l	0.00
Spiked Amount	50.000	Range	30 - 143	Recovery	=	91.300%


Target Compounds	Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY081325\
Data File : VY023081.D
Acq On : 13 Aug 2025 19:38
Operator : SY/MD
Sample : Q2819-19
Misc : 6.73g/5.0mL/MSVOA_Y/SOIL/A
ALS Vial : 24 Sample Multiplier: 1

Instrument :
MSVOA_Y
ClientSampleId :
38M-E

Quant Time: Aug 14 01:29:07 2025
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y081225S.M
Quant Title : SW846 8260
QLast Update : Wed Aug 13 02:10:11 2025
Response via : Initial Calibration




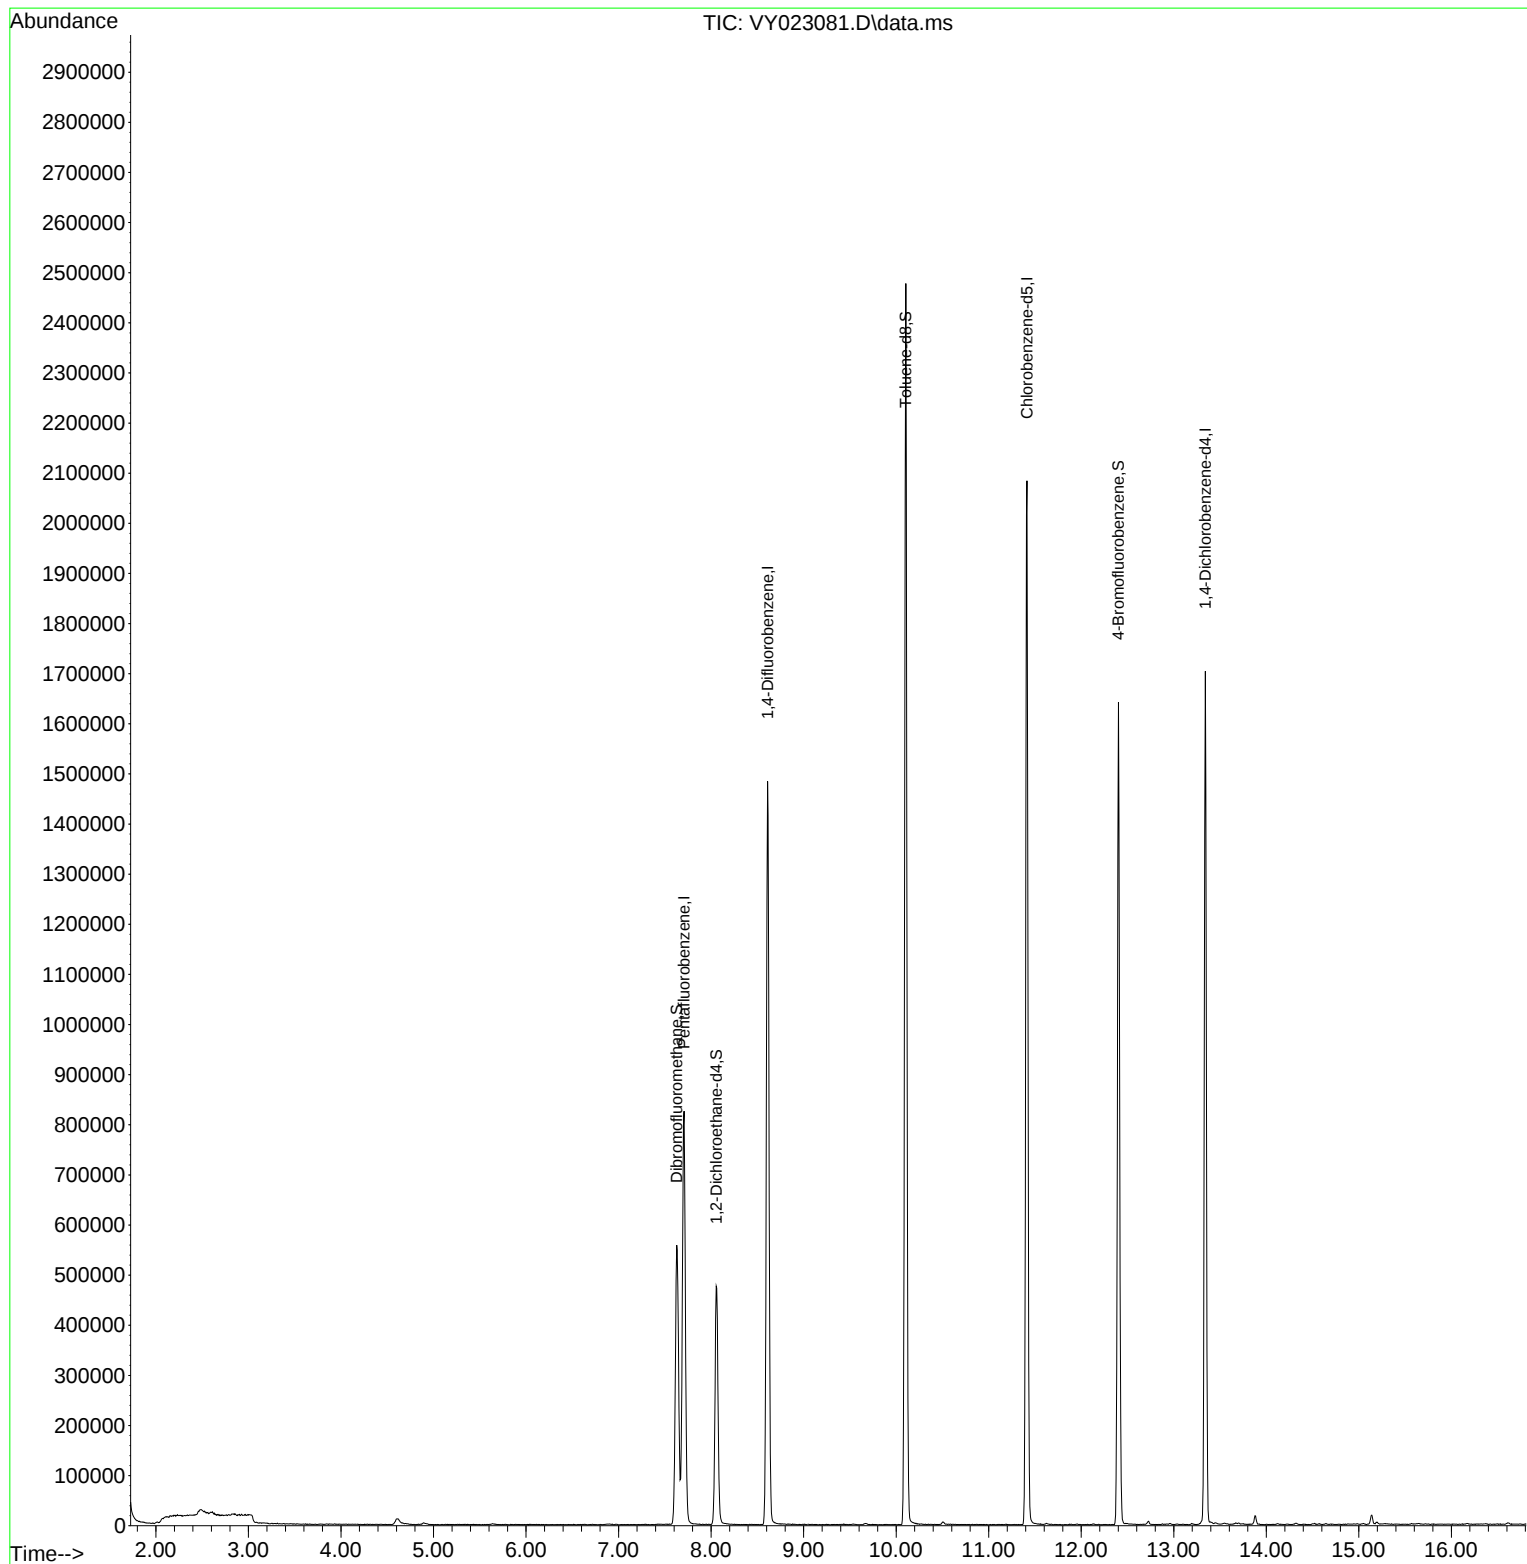


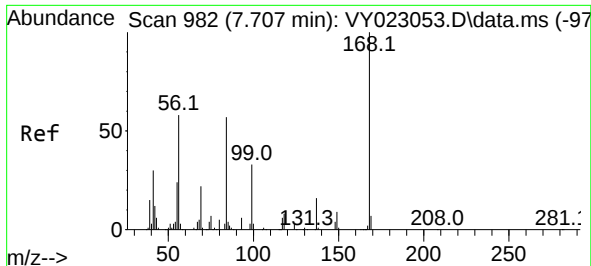

#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 7.707 min Scan# 91
Delta R.T. 0.000 min
Lab File: VY023081.D
Acq: 13 Aug 2025 19:38




Instrument :
MSVOA_Y
ClientSampleId :
38M-E


Tgt Ion:168 Resp: 641351
Ion Ratio Lower Upper
168 100
99 54.7 42.8 64.2

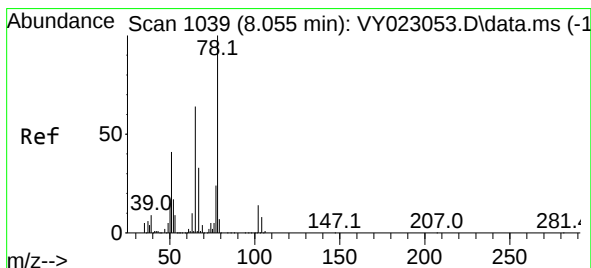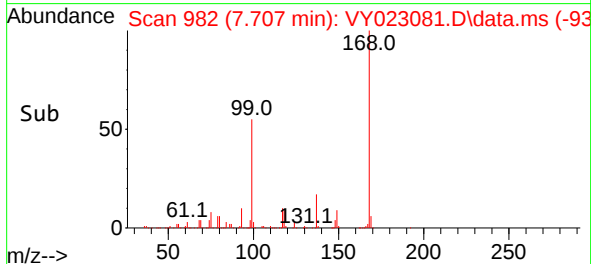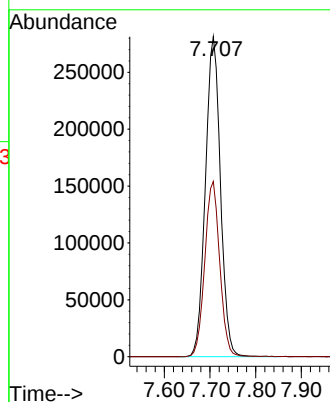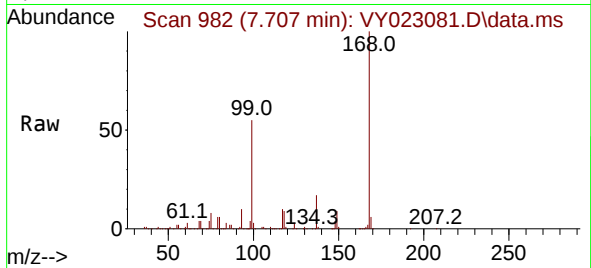

#33
1,2-Dichloroethane-d4
Concen: 62.049 ug/l
RT: 8.055 min Scan# 1039
Delta R.T. 0.000 min
Lab File: VY023081.D
Acq: 13 Aug 2025 19:38

Tgt Ion: 65 Resp: 379278
Ion Ratio Lower Upper
65 100
67 53.2 0.0 106.8


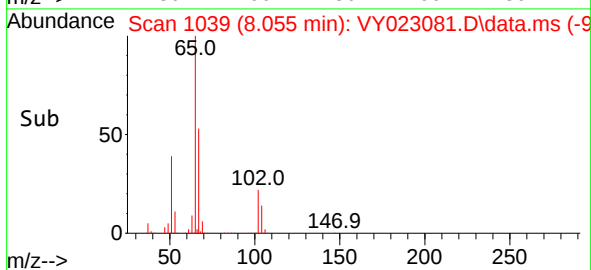
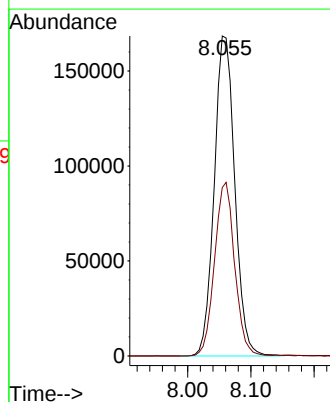
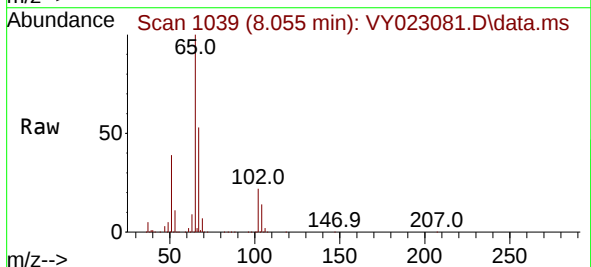


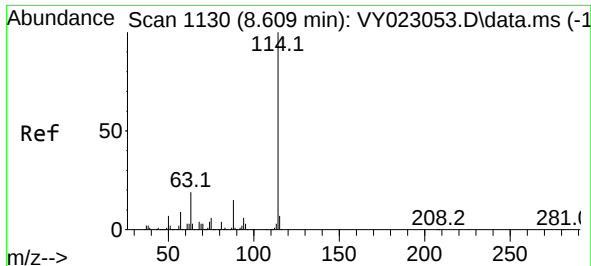

#34
1,4-Difluorobenzene
Concen: 50.000 ug/l
RT: 8.610 min Scan# 1130
Delta R.T. 0.000 min
Lab File: VY023081.D
Acq: 13 Aug 2025 19:38




Instrument :
MSVOA_Y
ClientSampleId :
38M-E


Tgt Ion:114 Resp: 1276856
Ion Ratio Lower Upper
114 100
63 19.8 0.0 38.4
88 15.3 0.0 30.0

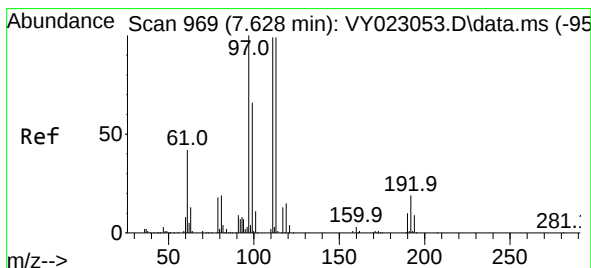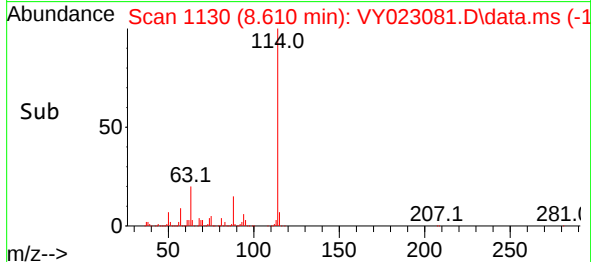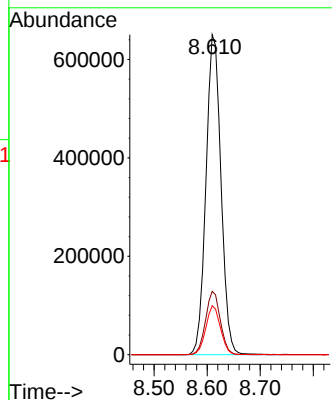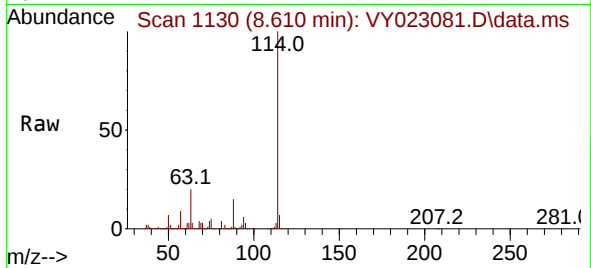

#35
Dibromofluoromethane
Concen: 53.316 ug/l
RT: 7.628 min Scan# 969
Delta R.T. 0.000 min
Lab File: VY023081.D
Acq: 13 Aug 2025 19:38

Tgt Ion:113 Resp: 407347
Ion Ratio Lower Upper
113 100
111 102.4 81.1 121.7
192 19.6 16.2 24.4


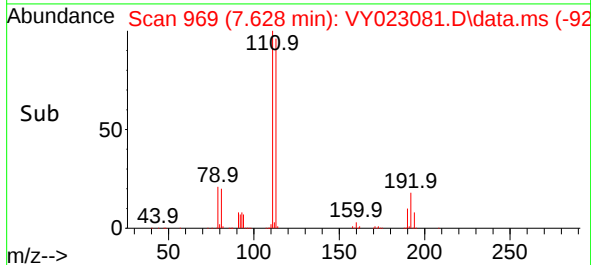
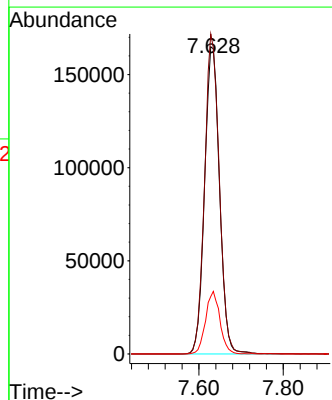
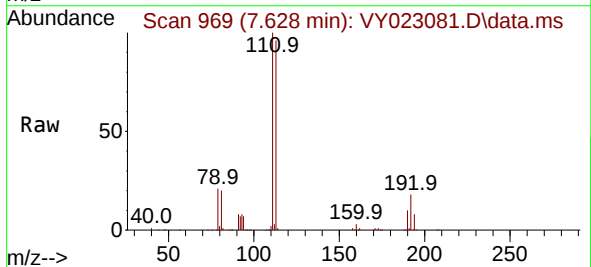


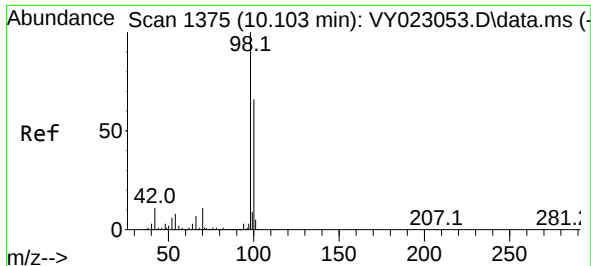

#50
Toluene-d8
Concen: 52.387 ug/l
RT: 10.103 min Scan# 1375
Delta R.T. 0.000 min
Lab File: VY023081.D
Acq: 13 Aug 2025 19:38




Instrument :
MSVOA_Y
ClientSampleId :
38M-E


Tgt Ion: 98 Resp: 1563625
Ion Ratio Lower Upper
98 100
100 64.9 52.3 78.5

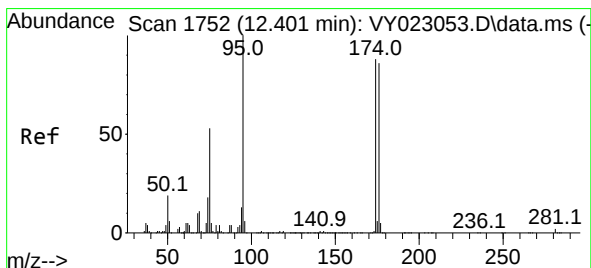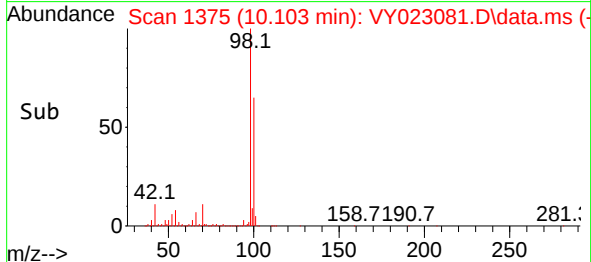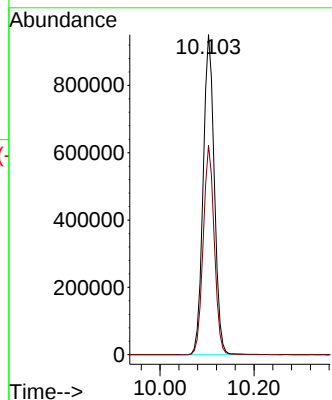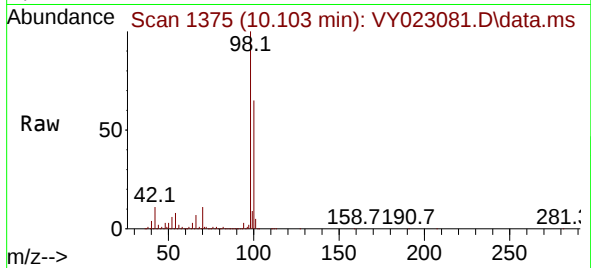

#62
4-Bromofluorobenzene
Concen: 45.648 ug/l
RT: 12.402 min Scan# 1752
Delta R.T. 0.000 min
Lab File: VY023081.D
Acq: 13 Aug 2025 19:38

Tgt Ion: 95 Resp: 438170
Ion Ratio Lower Upper
95 100
174 86.1 0.0 171.6
176 83.5 0.0 167.6


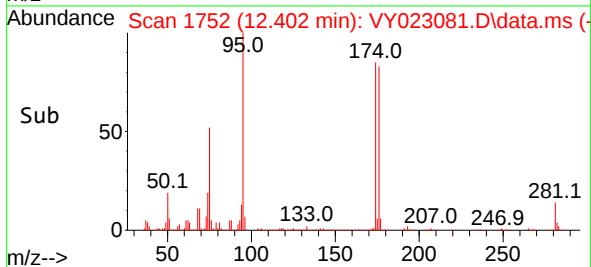
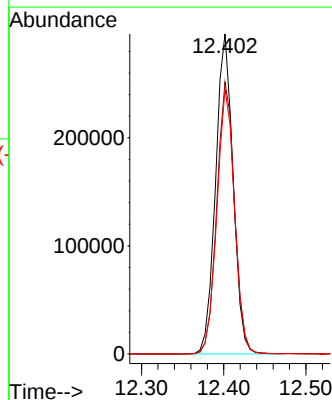
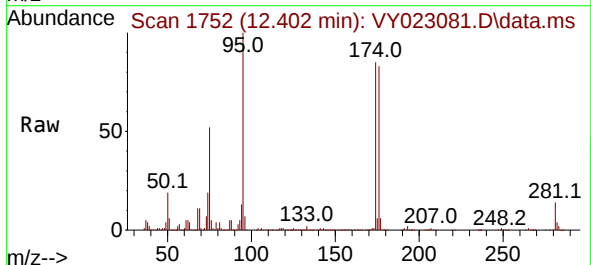


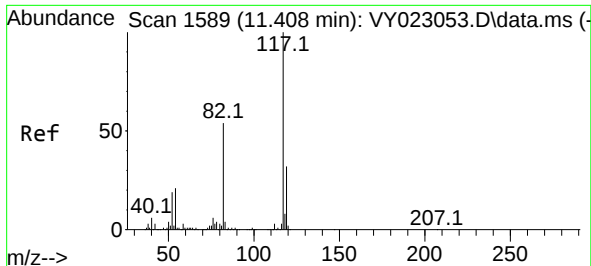

#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 11.414 min Scan# 11
Delta R.T. 0.006 min
Lab File: VY023081.D
Acq: 13 Aug 2025 19:38

Instrument :
MSVOA_Y
ClientSampleId :
38M-E

Tgt Ion:117 Resp: 1106347
Ion Ratio Lower Upper
117 100
82 53.6 43.4 65.0
119 31.9 25.6 38.4

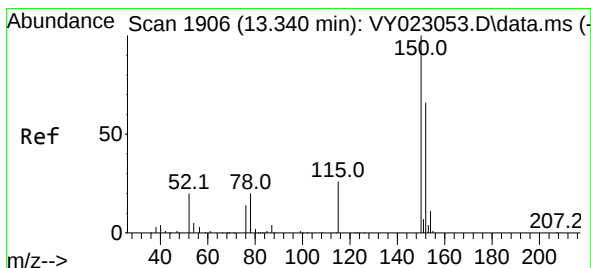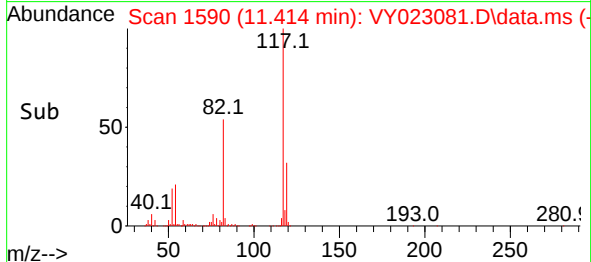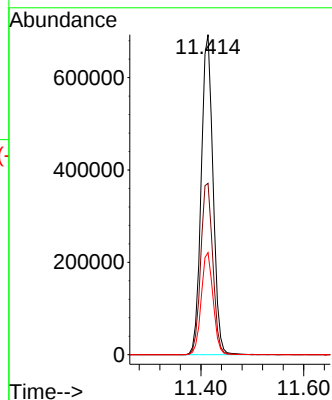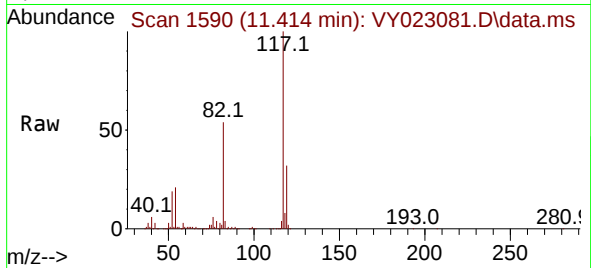

#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 13.340 min Scan# 1906
Delta R.T. 0.000 min
Lab File: VY023081.D
Acq: 13 Aug 2025 19:38

Tgt Ion:152 Resp: 424298
Ion Ratio Lower Upper
152 100
115 57.3 28.2 84.6
150 156.7 0.0 348.0

