
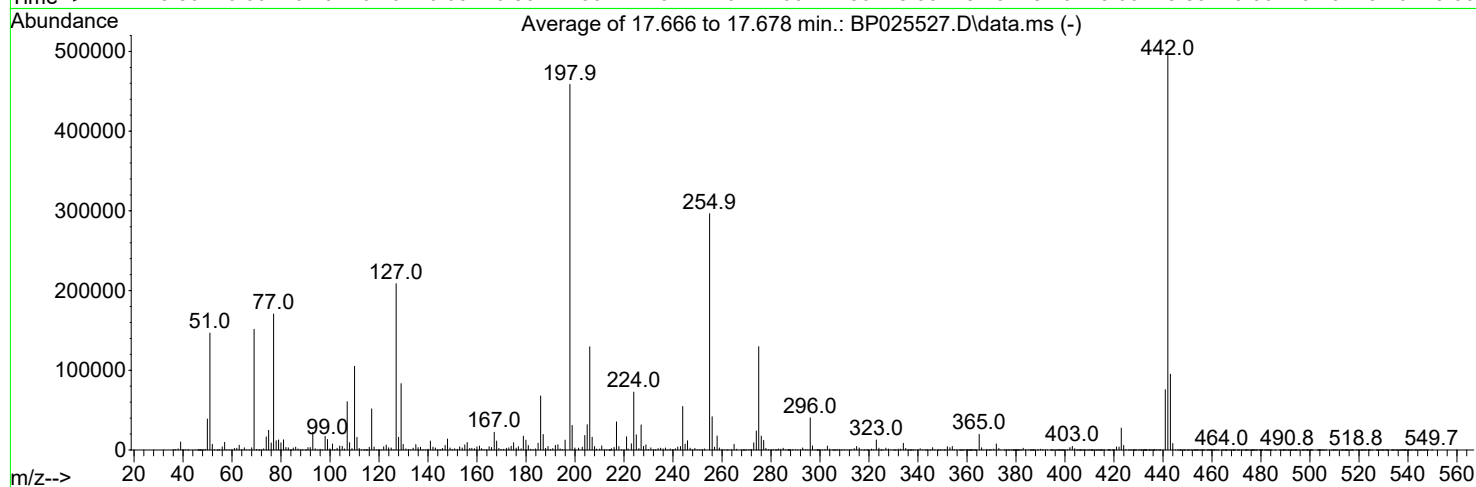


Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP082025\
Data File : BP025527.D
Acq On : 21 Aug 2025 06:01
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP081425.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Thu Aug 14 18:14:31 2025

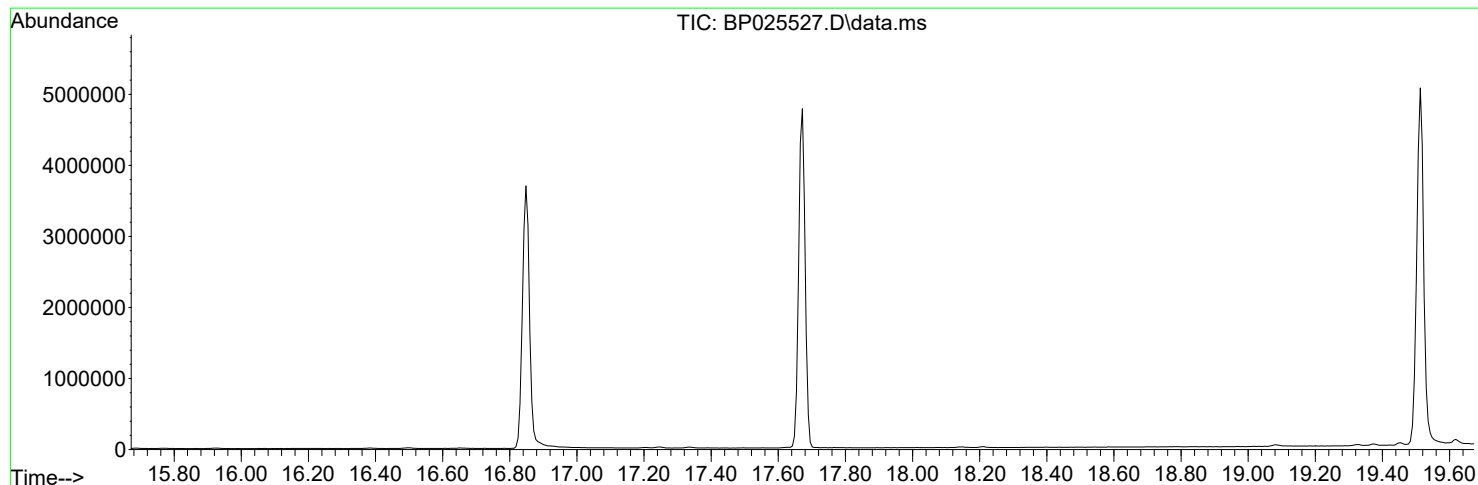

AutoFind: Scans 2504, 2505, 2506; Background Corrected with Scan 2495

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
68	69	0.00	2	1.9	2866	PASS
69	69	100	100	100.0	151600	PASS
70	69	0.00	2	0.5	829	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	458631	PASS
199	198	5	9	6.7	30834	PASS
365	198	1	100	4.3	19700	PASS
441	443	0.01	150	79.6	75722	PASS
442	442	100	100	100.0	495296	PASS
443	442	15	24	19.2	95153	PASS

DDT Breakdown




Date	Instrument Name	DFTPP Data File
8/20/2025	BNA_P	<u>BP025527.D</u>
Compound Name	Response	Retention Time
DDT	2180101	20.813
DDD	63141	20.348
DDE	5921	19.825
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
69062	2249163	3.07

Instrument :
BNA_P
ClientSampleId :
DFTPP

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP082025\
Data File : BP025527.D
Acq On : 21 Aug 2025 05:20
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DFTPP

Quant Time: Aug 21 06:28:41 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP081425.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Aug 14 18:14:31 2025
Response via : Initial Calibration

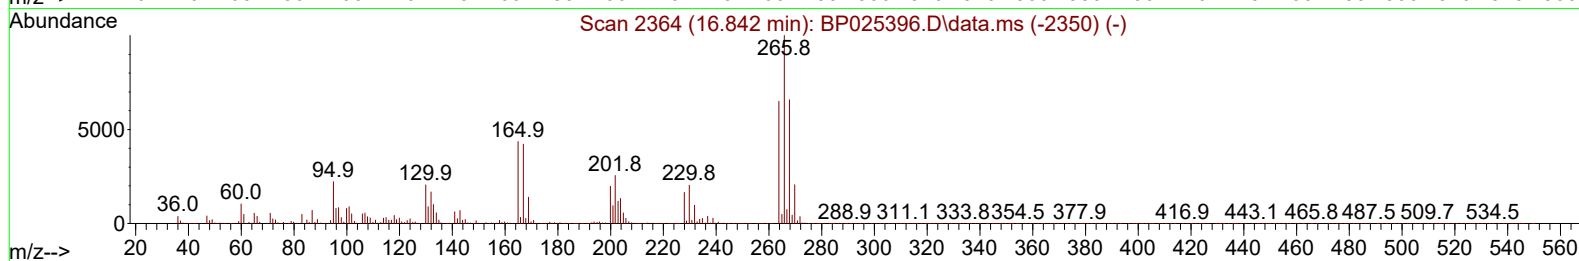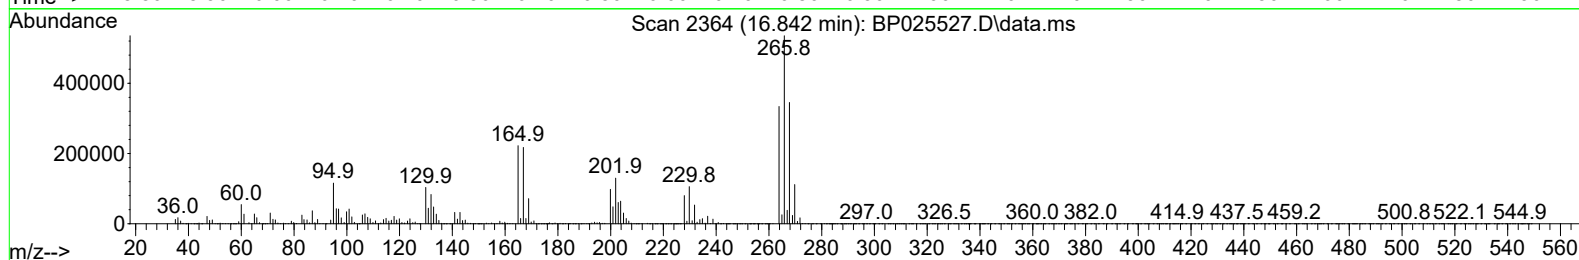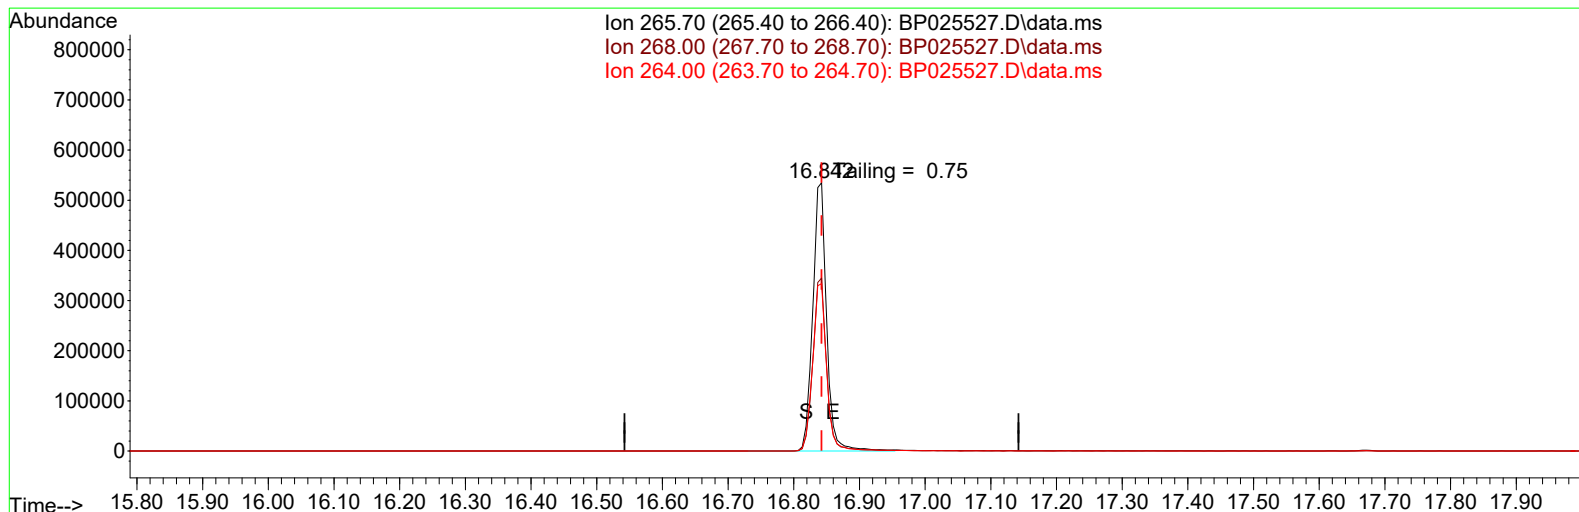

TIC: BP025527.D\data.ms

(70) Pentachlorophenol (C)

16.842min (+ 0.000) 14024.53 ng




response 784998

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	65.80	64.48
264.00	65.00	62.40
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP082025\
Data File : BP025527.D
Acq On : 21 Aug 2025 05:20
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DFTPP

Quant Time: Aug 21 06:28:41 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP081425.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Aug 14 18:14:31 2025
Response via : Initial Calibration

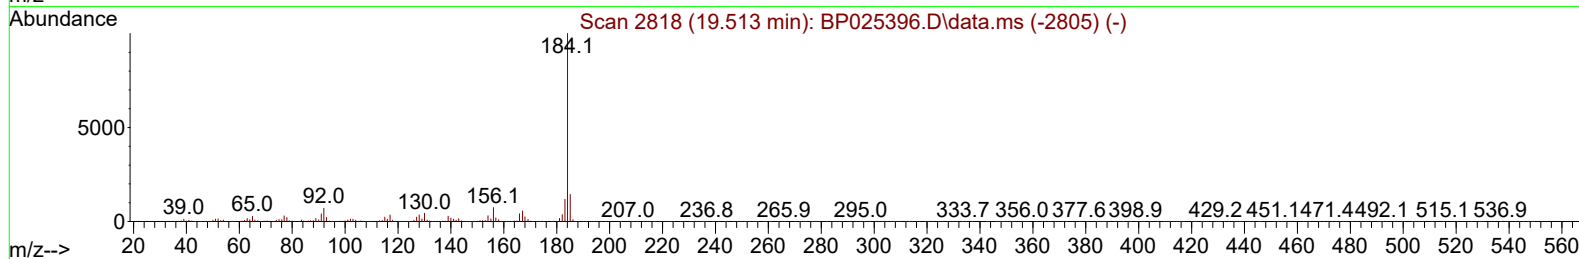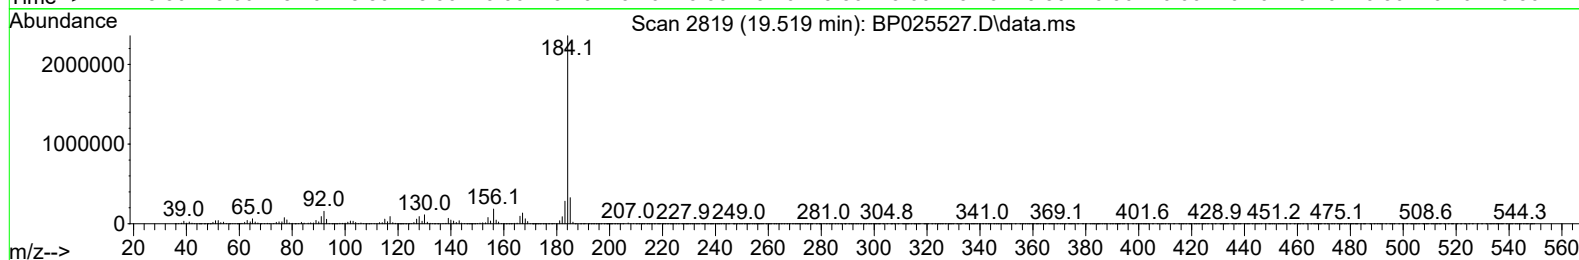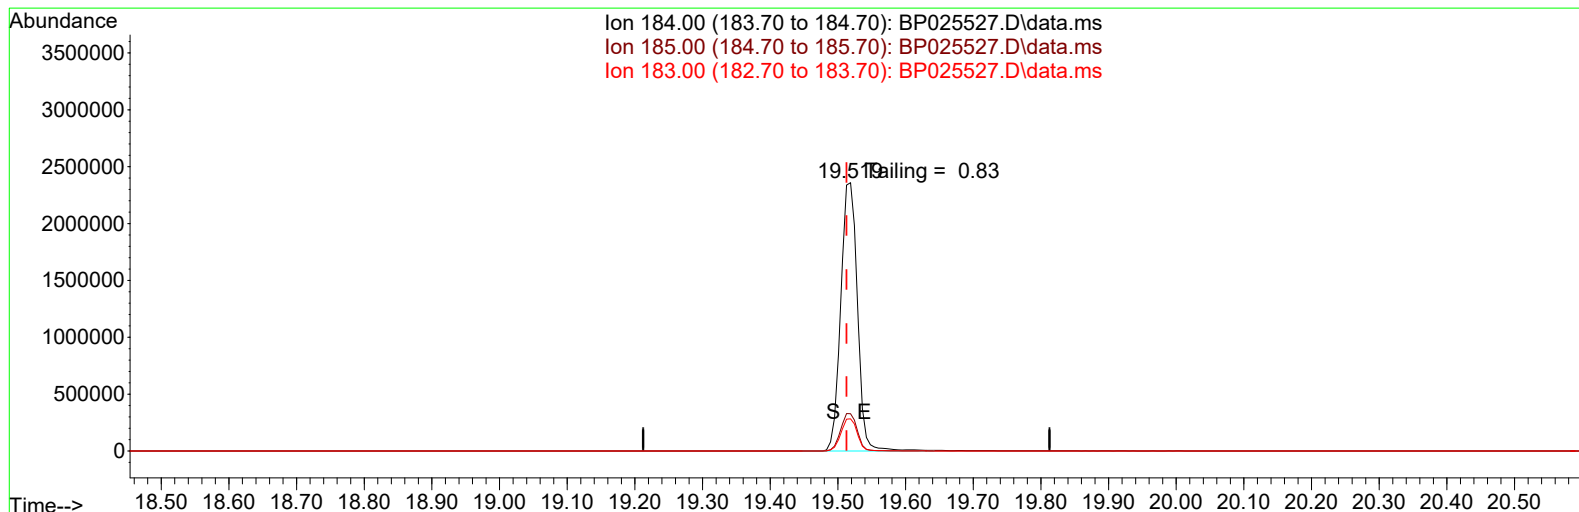

TIC: BP025527.D\data.ms

(77) Benzidine

19.519min (+ 0.006) 13689.91 ng

response 4033404

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.40	13.90
183.00	11.80	11.97
0.00	0.00	0.00