
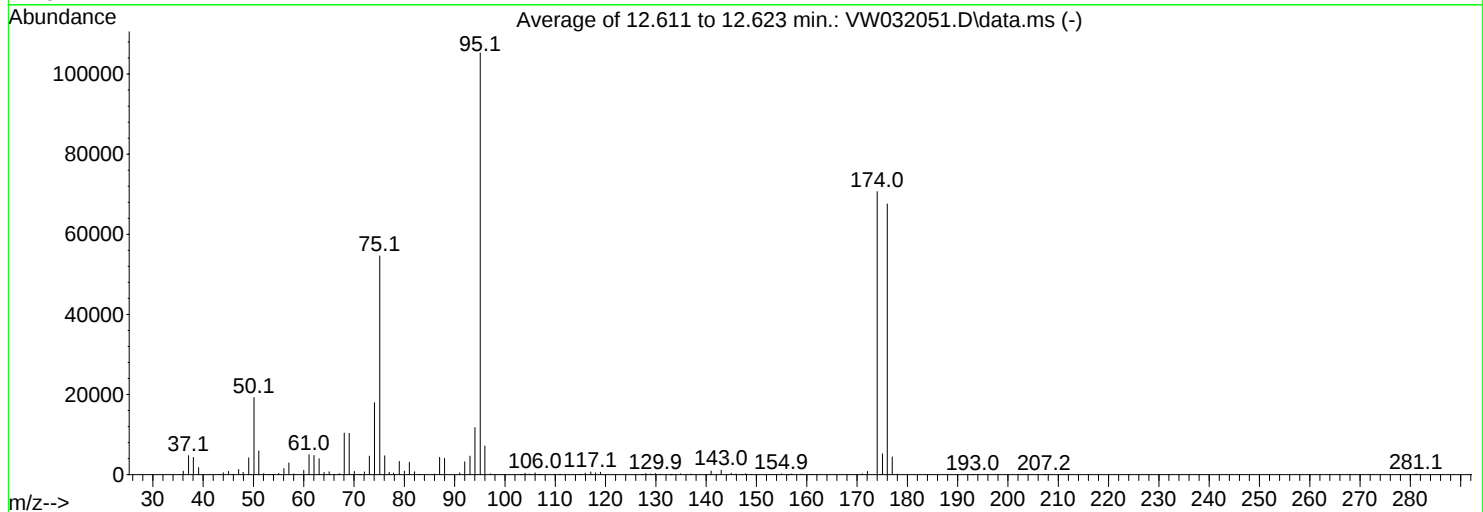


Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW081125\
Data File : VW032051.D
Acq On : 11 Aug 2025 07:53
Operator : SY/MD
Sample : BFB
Misc : 5.00g/5mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\82W081125S.M
Title : SW846 8260
Last Update : Tue Aug 12 04:04:48 2025

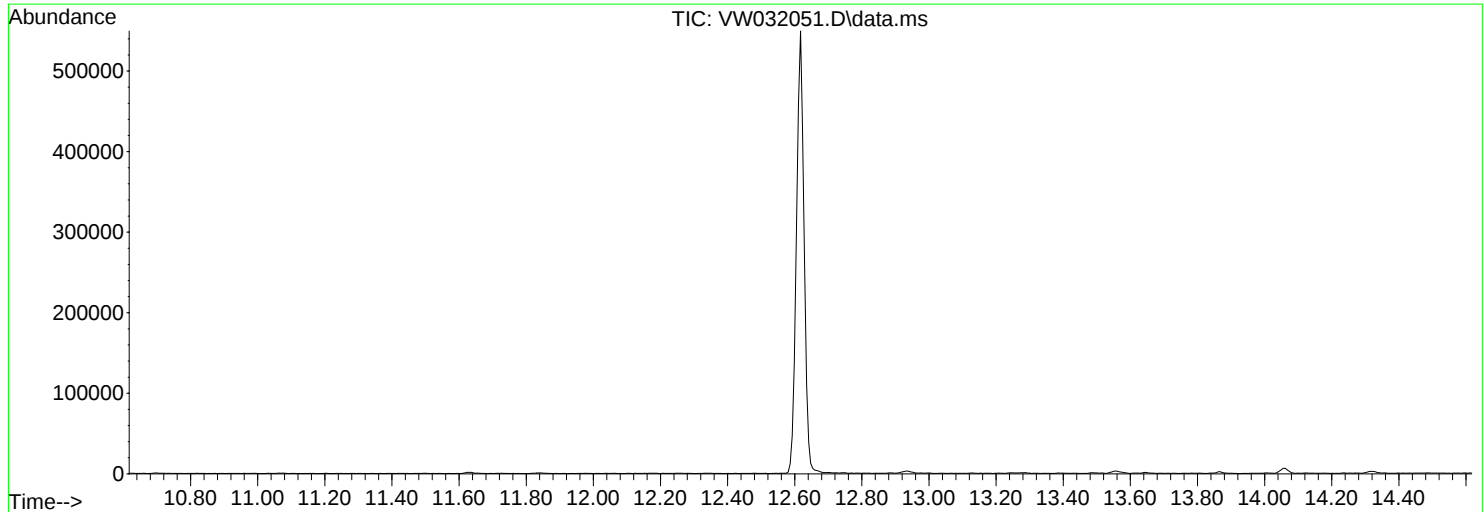

AutoFind: Scans 1759, 1760, 1761; Background Corrected with Scan 1750

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	15	40	18.3	19253	PASS
75	95	30	60	51.9	54621	PASS
95	95	100	100	100.0	105291	PASS
96	95	5	9	6.8	7140	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	100	67.1	70667	PASS
175	174	5	9	7.3	5189	PASS
176	174	95	101	95.6	67573	PASS
177	176	5	9	6.5	4421	PASS