

Method Path : Z:\svoasrv\HPCHEM1\BNA_N\Methods\
 Method File : 8270-SIM-BN081225.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Wed Aug 13 05:00:58 2025
 Response Via : Initial Calibration

Calibration Files

0.1 =BN037578.D 0.2 =BN037579.D 0.4 =BN037580.D 0.8 =BN037581.D 1.6 =BN037582.D 3.2 =BN037583.D 5 =BN037584.D

	Compound	0.1	0.2	0.4	0.8	1.6	3.2	5	Avg	%RSD
1) I	1,4-Dichlorobenzen...	-----ISTD-----								
2)	1,4-Dioxane	0.413	0.395	0.368	0.397	0.375	0.348	0.383	6.08	
3)	n-Nitrosodimet...	0.471	0.488	0.471	0.493	0.503	0.508	0.489	3.19	
4) S	2-Fluorophenol	0.922	0.945	0.888	0.823	0.886	0.906	0.977	0.907	5.41
5) S	Phenol-d6	1.045	1.051	1.044	0.983	1.198	1.117	1.201	1.091	7.66
6)	bis(2-Chloroet...	0.935	0.987	0.976	0.936	1.020	1.008	1.022	0.983	3.75
7) I	Naphthalene-d8	-----ISTD-----								
8) S	Nitrobenzene-d5	0.270	0.257	0.262	0.264	0.292	0.301	0.326	0.282	9.03
9)	Naphthalene	1.044	1.050	1.037	1.012	1.089	1.096	1.127	1.065	3.78
10)	Hexachlorobuta...	0.252	0.258	0.262	0.253	0.267	0.264	0.265	0.260	2.22
11) SURR	2-Methylnaphth...	0.488	0.492	0.508	0.493	0.543	0.578	0.705	0.544	14.39
12)	2-Methylnaphth...	0.589	0.631	0.635	0.629	0.701	0.731	0.760	0.668	9.39
13) I	Acenaphthene-d10	-----ISTD-----								
14) S	2,4,6-Tribromo...	0.139	0.149	0.156	0.160	0.185	0.203	0.234	0.175	19.39
15) S	2-Fluorobiphenyl	2.226	2.243	2.300	2.251	2.341	2.391	2.440	2.313	3.50
16)	Acenaphthylene	1.740	1.760	1.710	1.653	1.850	1.858	1.980	1.793	6.15
17)	Acenaphthene	1.144	1.150	1.172	1.154	1.283	1.286	1.348	1.220	6.86
18)	Fluorene	1.466	1.510	1.524	1.521	1.686	1.693	1.770	1.596	7.38
19) I	Phenanthrene-d10	-----ISTD-----								
20)	4,6-Dinitro-2-...	0.042	0.046	0.047	0.061	0.070		0.053	22.37	
21)	4-Bromophenyl-...	0.226	0.236	0.234	0.237	0.265	0.271	0.292	0.251	9.77
22)	Hexachlorobenzene	0.360	0.360	0.356	0.332	0.364	0.354	0.370	0.356	3.37
23)	Atrazine	0.127	0.126	0.130	0.134	0.160	0.176		0.142	14.76
24)	Pentachlorophenol		0.108	0.113	0.113	0.139	0.152		0.125	15.36
25)	Phenanthrene	1.146	1.162	1.170	1.138	1.281	1.269	1.347	1.216	6.72
26)	Anthracene	0.950	0.985	0.995	0.988	1.145	1.186	1.286	1.077	11.93
27) SURR	Fluoranthene-d10	0.932	0.966	0.954	0.935	1.050	1.110	1.419	1.052	16.61
28)	Fluoranthene	1.241	1.264	1.299	1.291	1.503	1.533	1.648	1.397	11.53
29) I	Chrysene-d12	-----ISTD-----								
30)	Pyrene	1.539	1.486	1.464	1.403	1.502	1.520	1.552	1.495	3.38
31) S	Terphenyl-d14	0.814	0.801	0.796	0.763	0.833	0.853	0.901	0.823	5.45
32)	Benzo(a)anthra...	1.266	1.275	1.263	1.253	1.351	1.458	1.487	1.336	7.40
33)	Chrysene	1.547	1.515	1.433	1.379	1.511	1.489	1.551	1.489	4.21
34)	Bis(2-ethylhex...	0.518	0.522	0.483	0.522	0.593	0.671	0.551	12.47	
35) I	Perylene-d12	-----ISTD-----								


Method Path : Z:\svoasrv\HPCHEM1\BNA_N\Methods\

Method File : 8270-SIM-BN081225.M

36)	Indeno(1,2,3-c...	1.446	1.462	1.612	1.568	1.816	1.883	2.011	1.686	13.01
37)	Benzo(b)fluora...	1.351	1.375	1.338	1.432	1.615	1.674	1.825	1.516	12.52
38)	Benzo(k)fluora...	1.597	1.580	1.651	1.628	1.821	1.797	1.898	1.710	7.36
39) C	Benzo(a)pyrene	1.146	1.136	1.149	1.157	1.322	1.382	1.508	1.257	11.77
40)	Dibenzo(a,h)an...	1.023	1.118	1.222	1.215	1.439	1.516	1.621	1.308	16.85
41)	Benzo(g,h,i)pe...	1.207	1.274	1.262	1.261	1.467	1.532	1.643	1.378	12.17

(#) = Out of Range

4,6-Dinitro-2-methylphenol

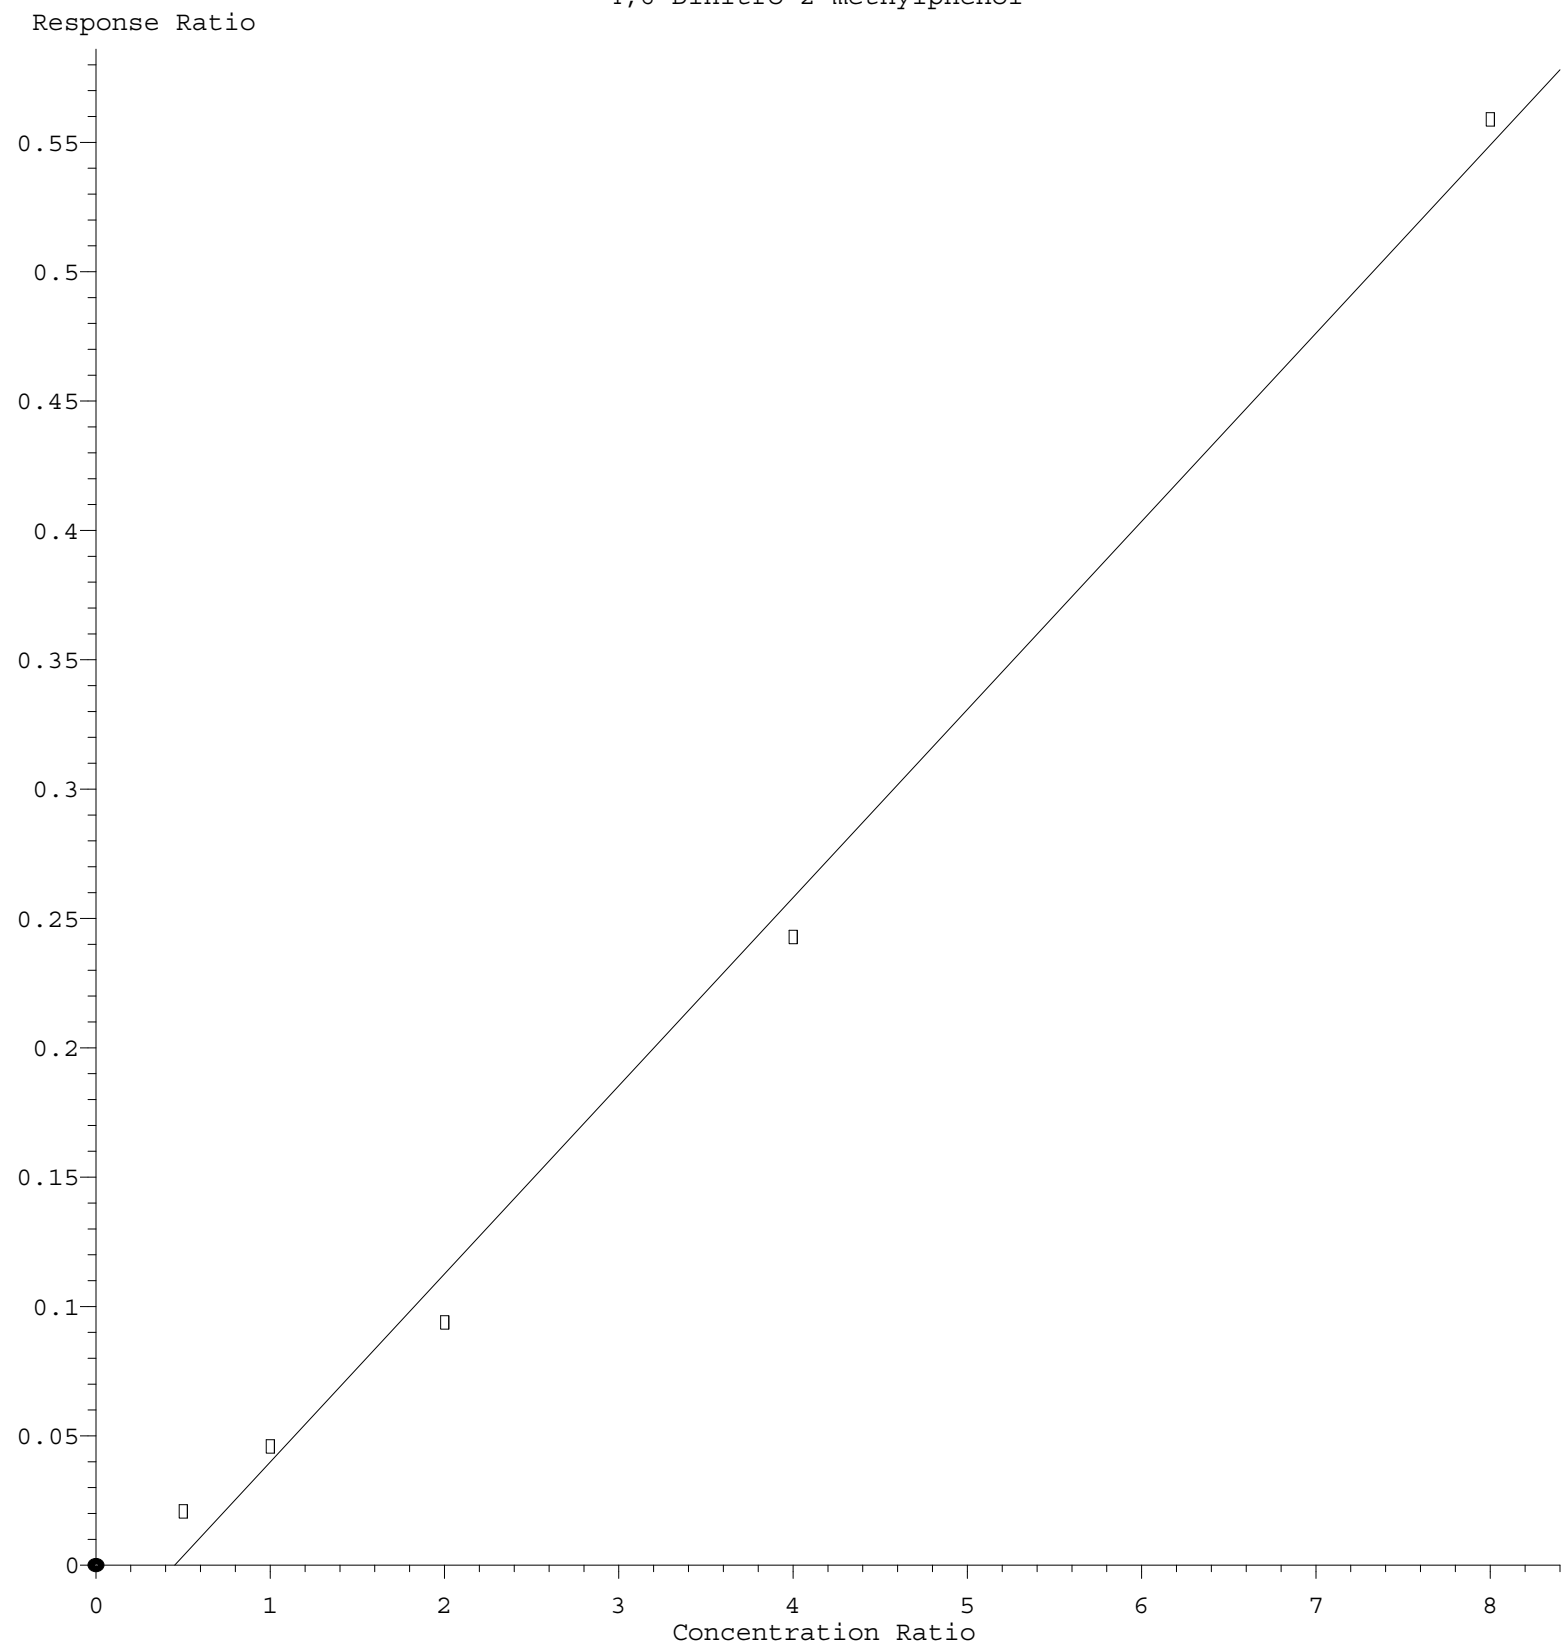

Response = $7.267 \times 10^{-2} \times \text{Amt} - 3.284 \times 10^{-2}$
 Coef of Det (r^2) = 0.994845 Curve Fit: Linear
 Method Name: Z:\svoasrv\HPCHEM1\BNA N\Methods\8270-SIM-BN081225.M
 Calibration Table Last Updated: Wed Aug 13 05:00:58 2025