


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN081225\
Data File : BN037576.D
Acq On : 12 Aug 2025 15:05
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270-SIM-BN081225.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Wed Aug 13 05:00:58 2025

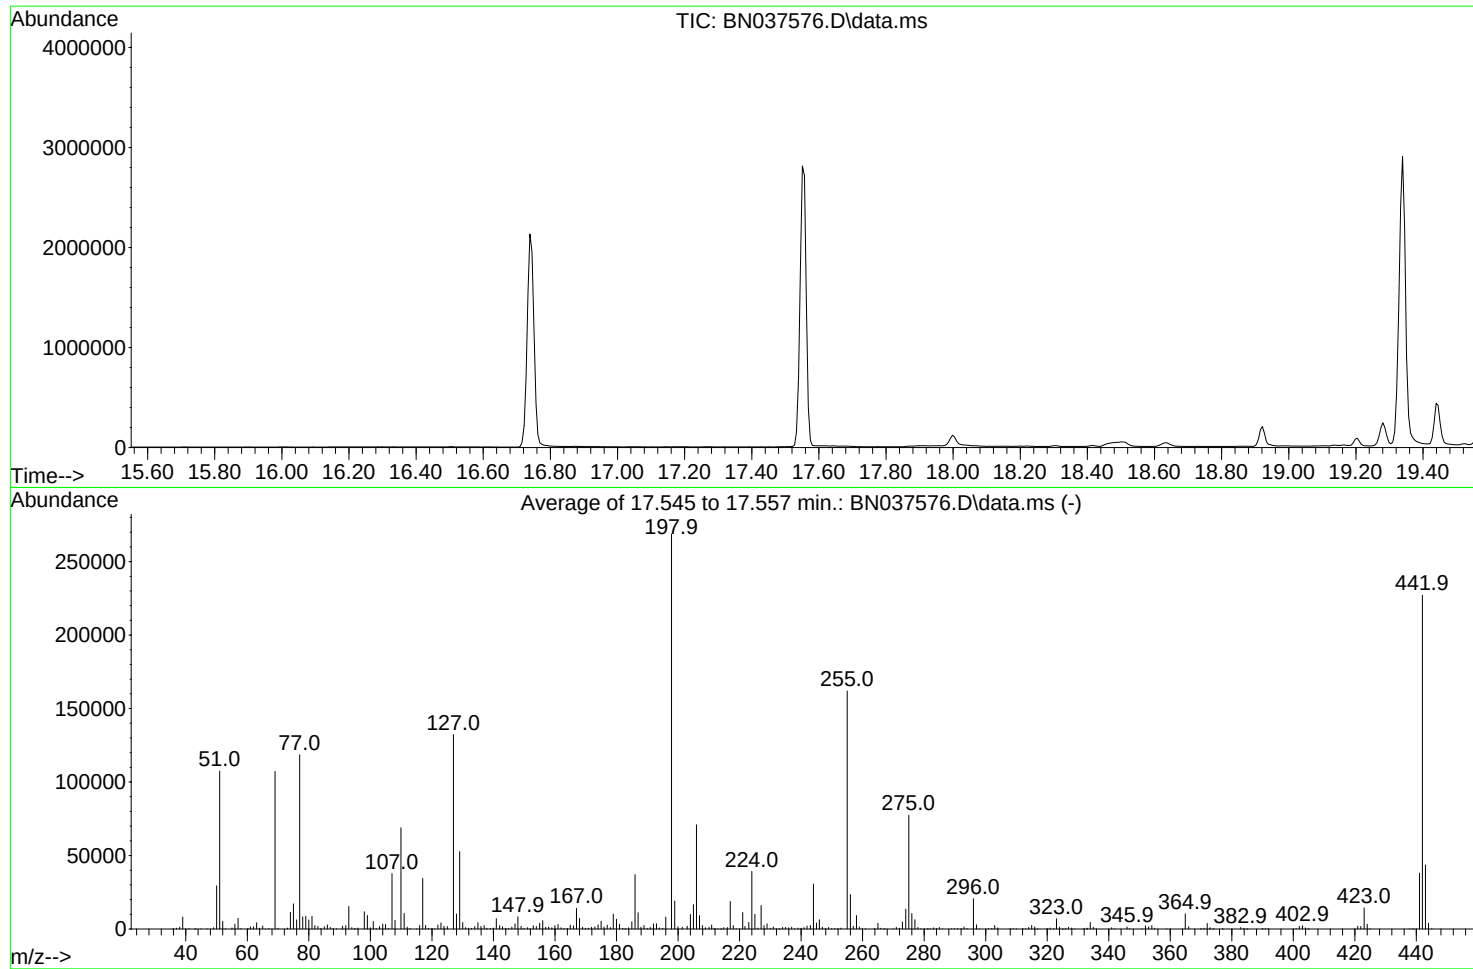

AutoFind: Scans 2458, 2459, 2460; Background Corrected with Scan 2451

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
68	69	0.00	2	0.0	0	PASS
69	69	100	100	100.0	107227	PASS
70	69	0.00	2	0.6	598	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	268651	PASS
199	198	5	9	7.1	19058	PASS
365	198	1	100	3.9	10363	PASS
441	443	0.01	150	87.2	38019	PASS
442	442	100	100	100.0	227139	PASS
443	442	15	24	19.2	43589	PASS

DDT Breakdown




Date	Instrument Name	DFTPP Data File
8/12/2025	BNA_N	<u>BN037576.D</u>
Compound Name	Response	Retention Time
DDT	903527	20.586
DDD	9291	20.192
DDE	170	19.633
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
9461	912988	1.04

Instrument :
BNA_N
ClientSampleId :
DFTPP

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN081225\
Data File : BN037576.D
Acq On : 12 Aug 2025 15:05
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: Aug 13 06:28:28 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Aug 06 01:49:15 2025
Response via : Initial Calibration

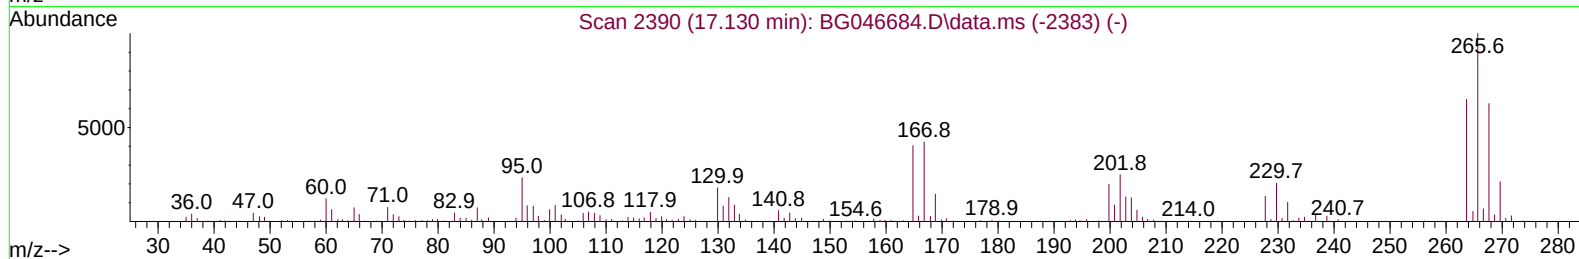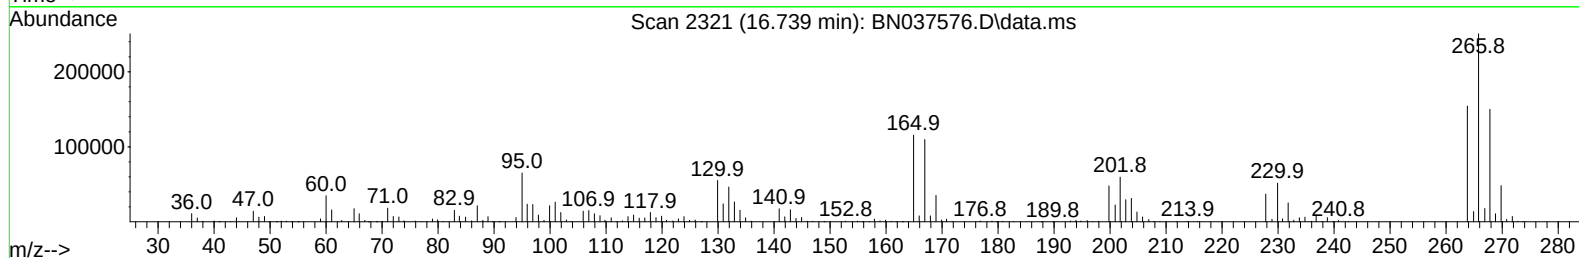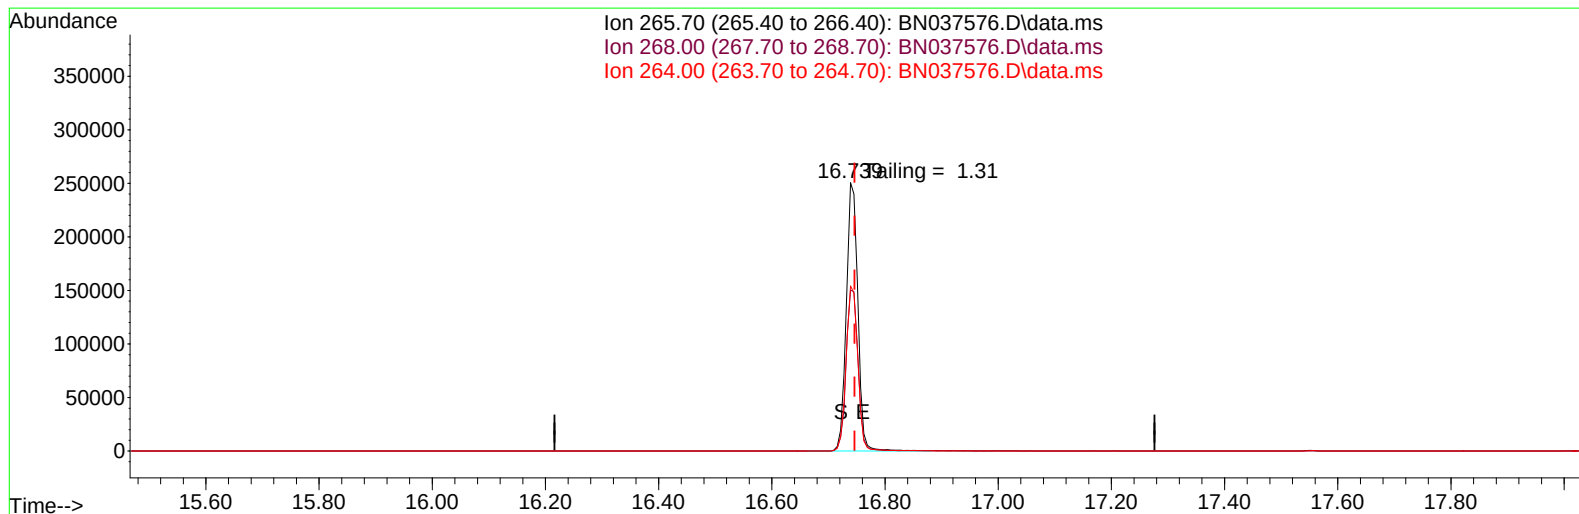

TIC: BN037576.D\data.ms

(70) Pentachlorophenol (C)

16.739min (-0.007) 29662.60 ng




response 357790

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	59.87
264.00	61.60	61.53
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN081225\
Data File : BN037576.D
Acq On : 12 Aug 2025 15:05
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: Aug 13 06:28:28 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Aug 06 01:49:15 2025
Response via : Initial Calibration

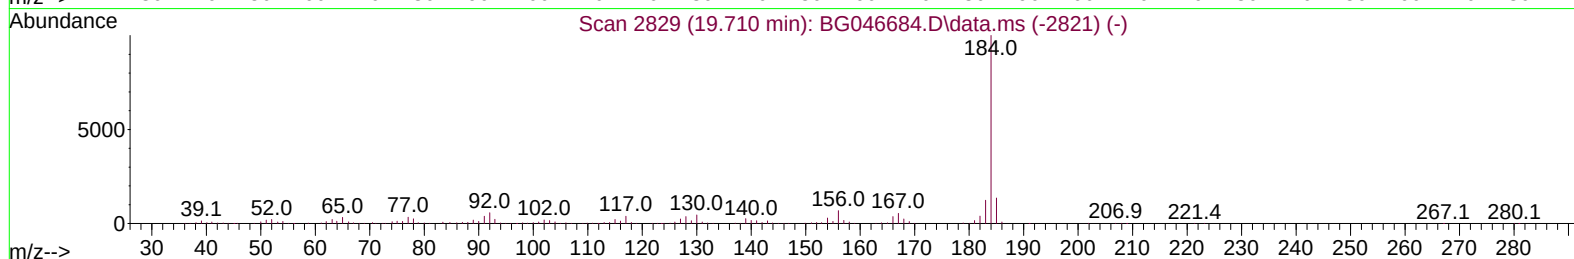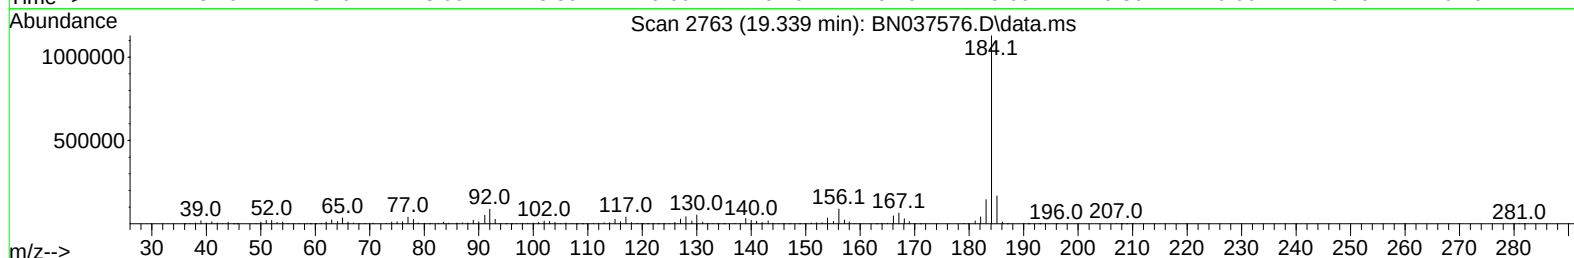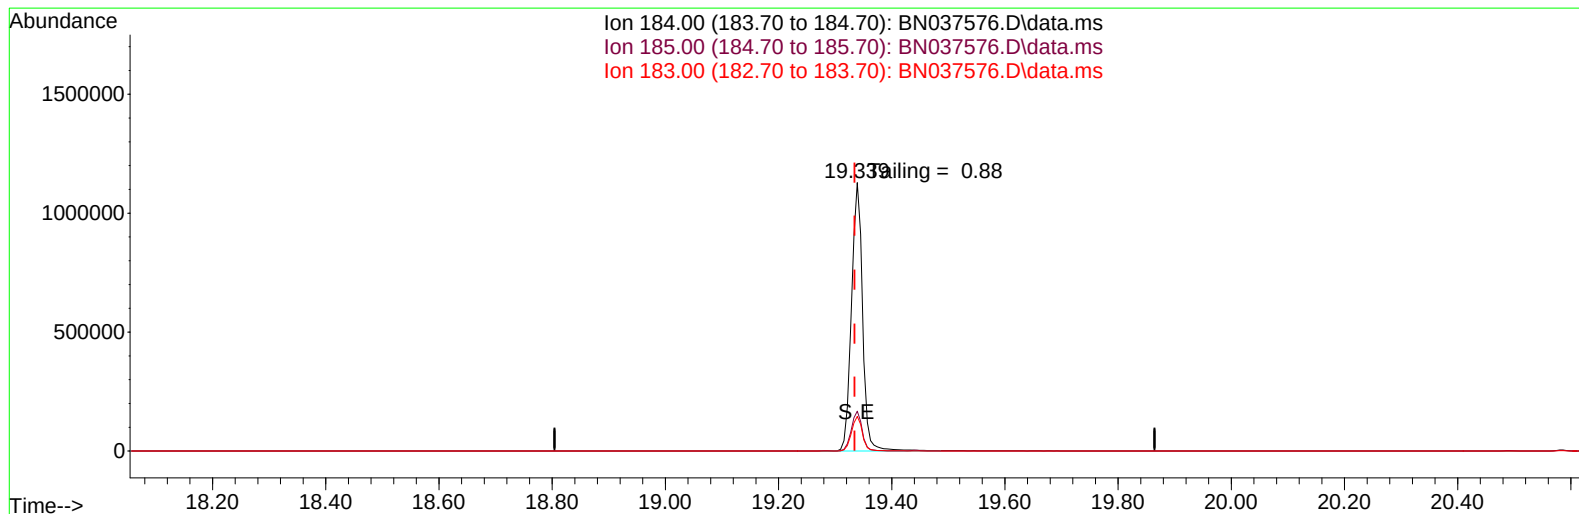

TIC: BN037576.D\data.ms

(77) Benzidine

19.339min (+ 0.005) 0.00 ng

response 1542567

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	14.86
183.00	13.20	12.90
0.00	0.00	0.00