


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN081325\
Data File : BN037587.D
Acq On : 13 Aug 2025 09:48
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270-SIM-BN081225.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Wed Aug 13 05:00:58 2025

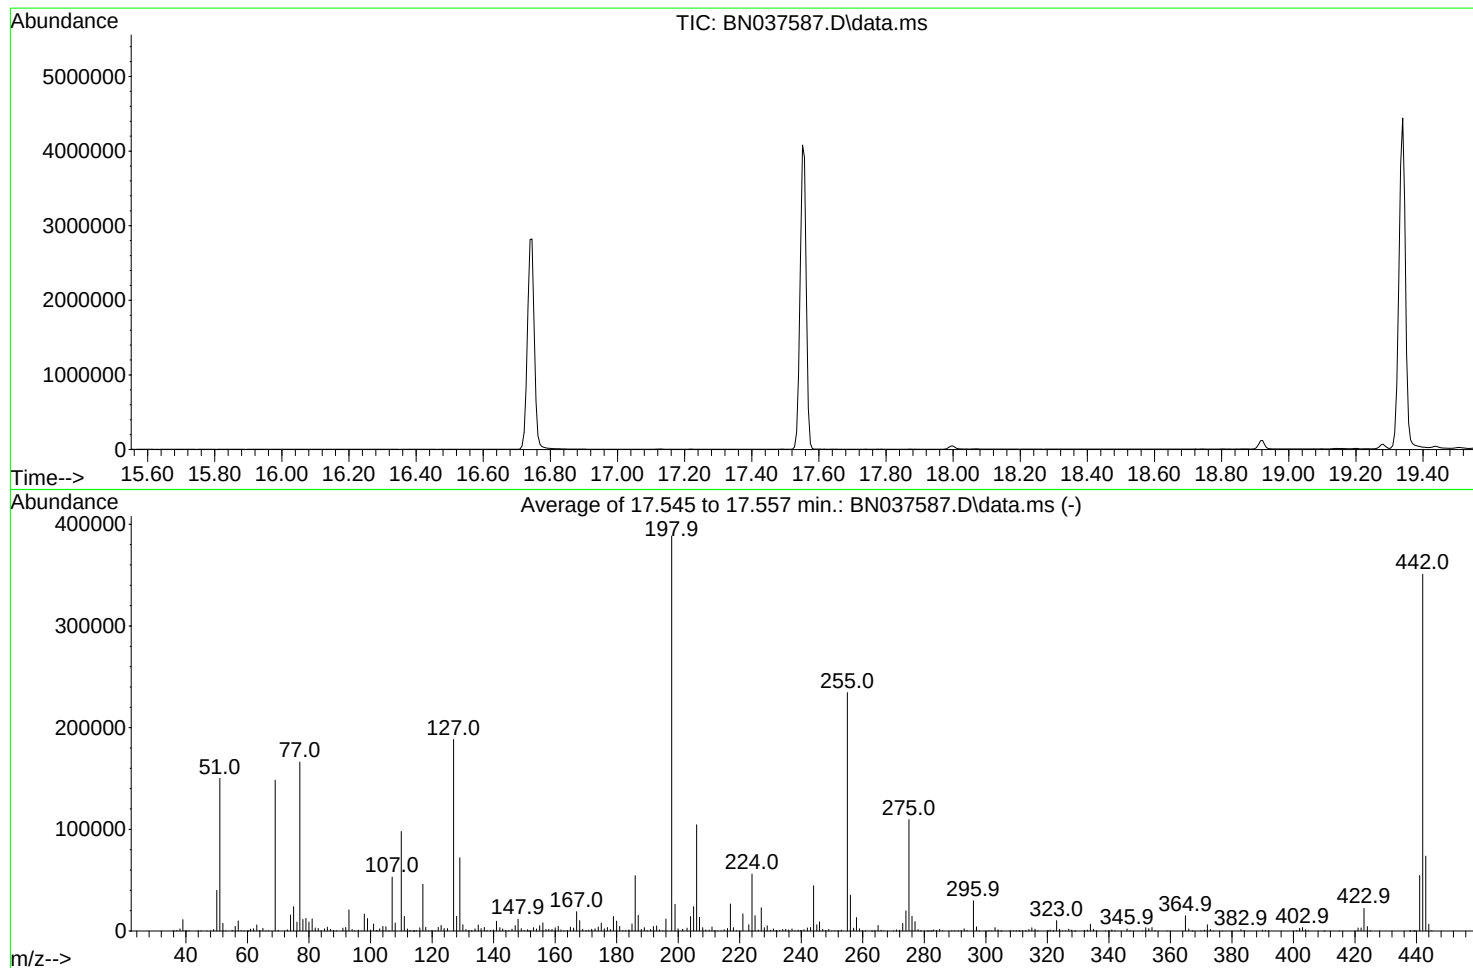




AutoFind: Scans 2458, 2459, 2460; Background Corrected with Scan 2451

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
68	69	0.00	2	0.0	0	PASS
69	69	100	100	100.0	148448	PASS
70	69	0.00	2	0.5	736	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	388309	PASS
199	198	5	9	6.8	26275	PASS
365	198	1	100	3.9	15039	PASS
441	443	0.01	150	74.2	54659	PASS
442	442	100	100	100.0	350869	PASS
443	442	15	24	21.0	73643	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN081325\
Data File : BN037587.D
Acq On : 13 Aug 2025 09:48
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: Aug 13 12:38:31 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Aug 06 01:49:15 2025
Response via : Initial Calibration

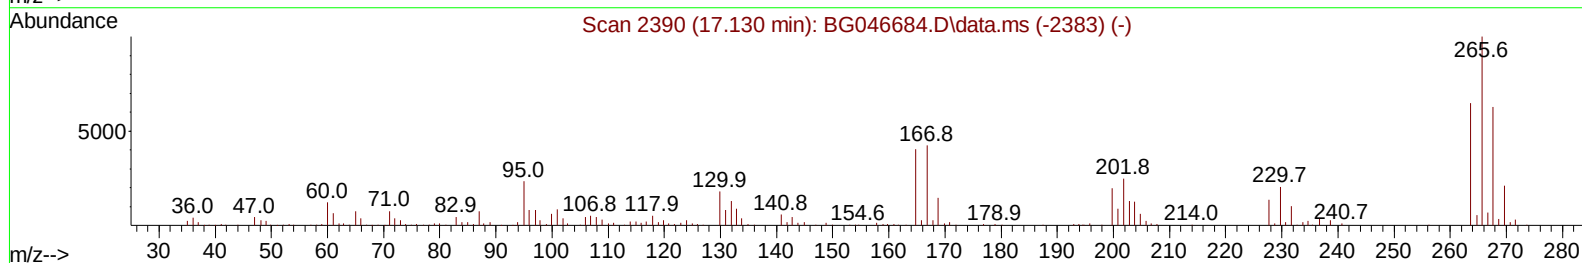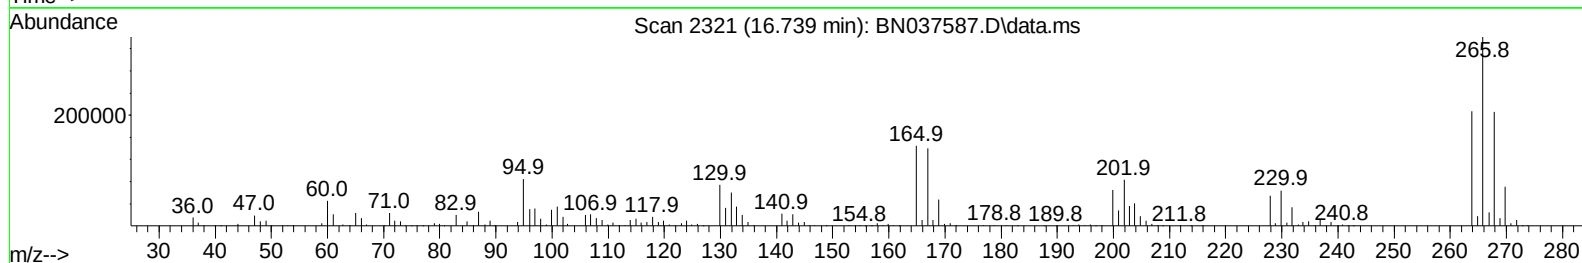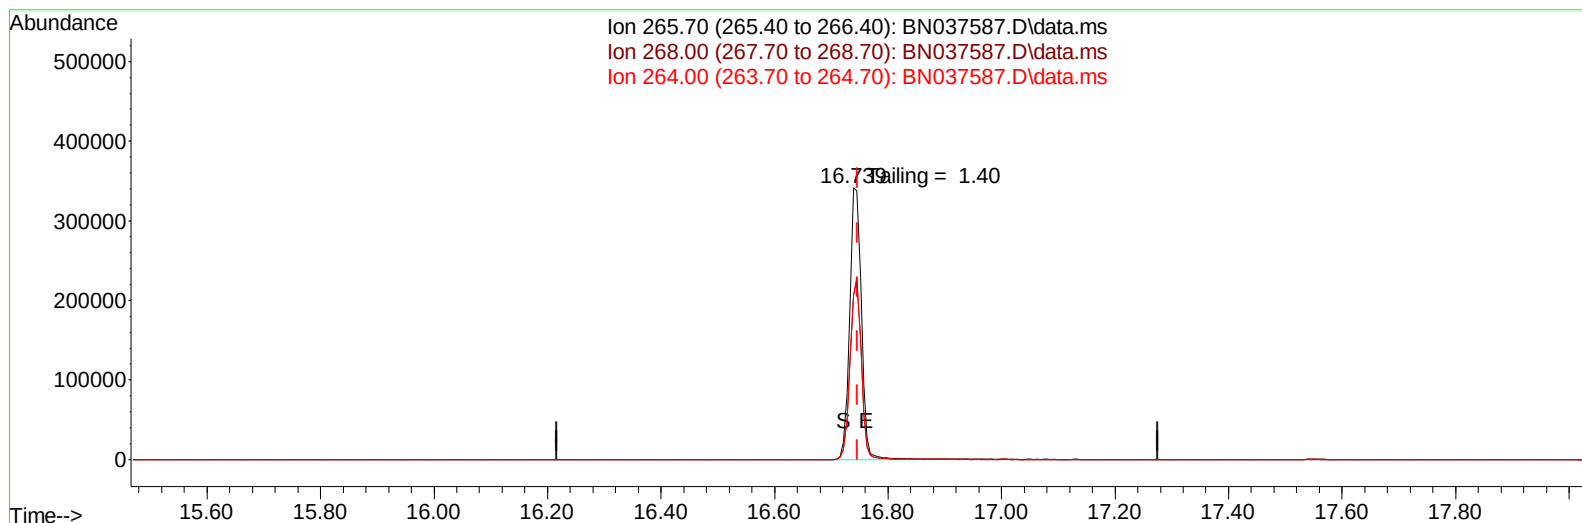

TIC: BN037587.D\data.ms

(70) Pentachlorophenol (C)

16.739min (-0.007) 26359.62 ng




response 484061

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	60.50
264.00	61.60	60.78
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN081325\
Data File : BN037587.D
Acq On : 13 Aug 2025 09:48
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: Aug 13 12:38:31 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Aug 06 01:49:15 2025
Response via : Initial Calibration

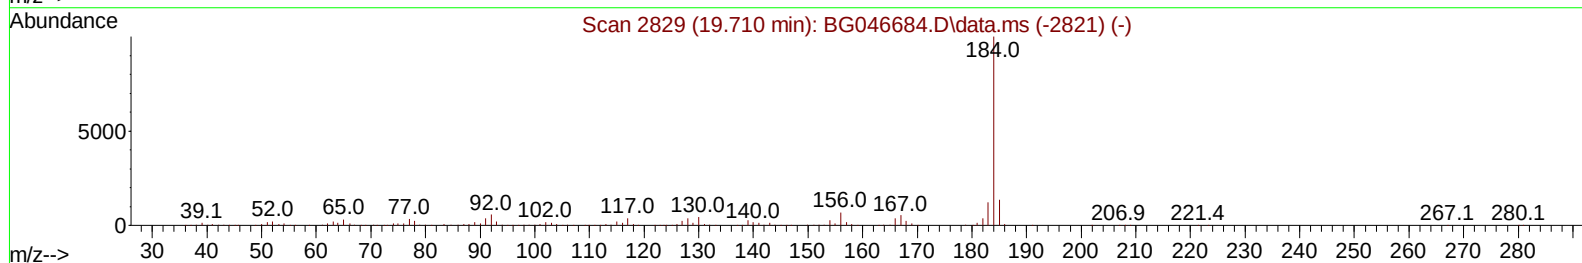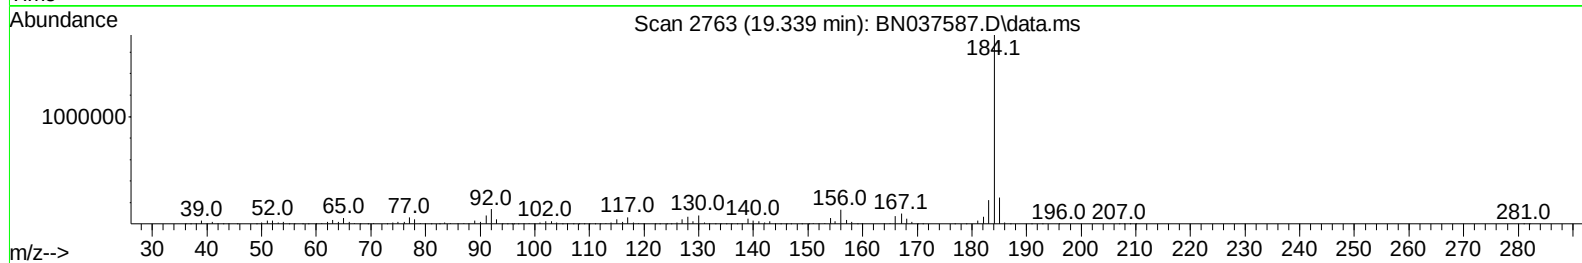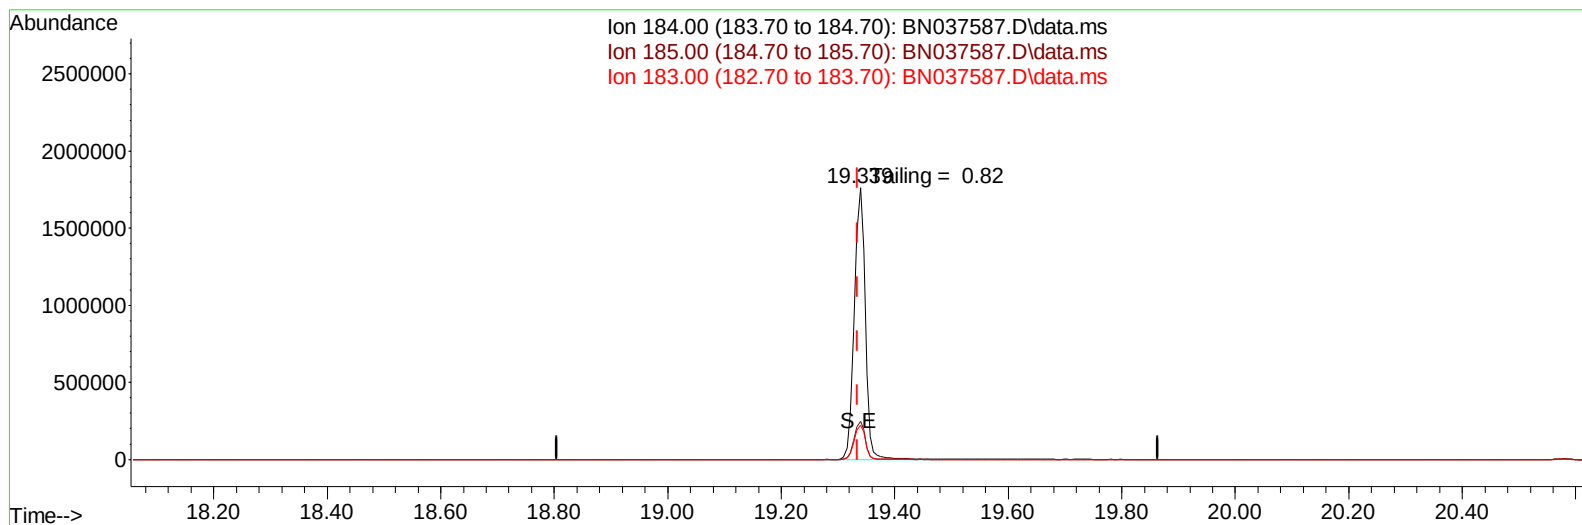

TIC: BN037587.D\data.ms

(77) Benzidine

19.339min (+ 0.005) 0.00 ng

response 2377211

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	14.03
183.00	13.20	12.54
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
8/13/2025	BNA_N	<u>BN037587.D</u>
Compound Name	Response	Retention Time
DDT	1163963	20.58
DDD	16801	20.192
DDE	162	19.627
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
16963	1180926	1.44

Instrument :
BNA_N
ClientSampleId :
DFTPP