
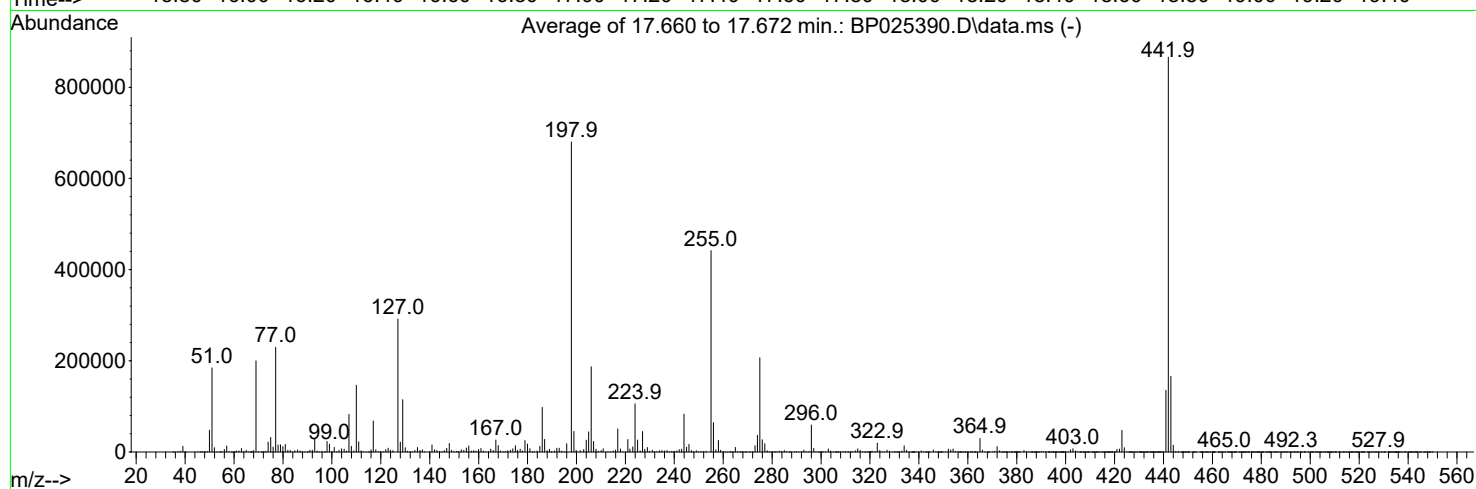


Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP081425\
Data File : BP025390.D
Acq On : 14 Aug 2025 10:30
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP081425.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Thu Aug 14 18:14:31 2025

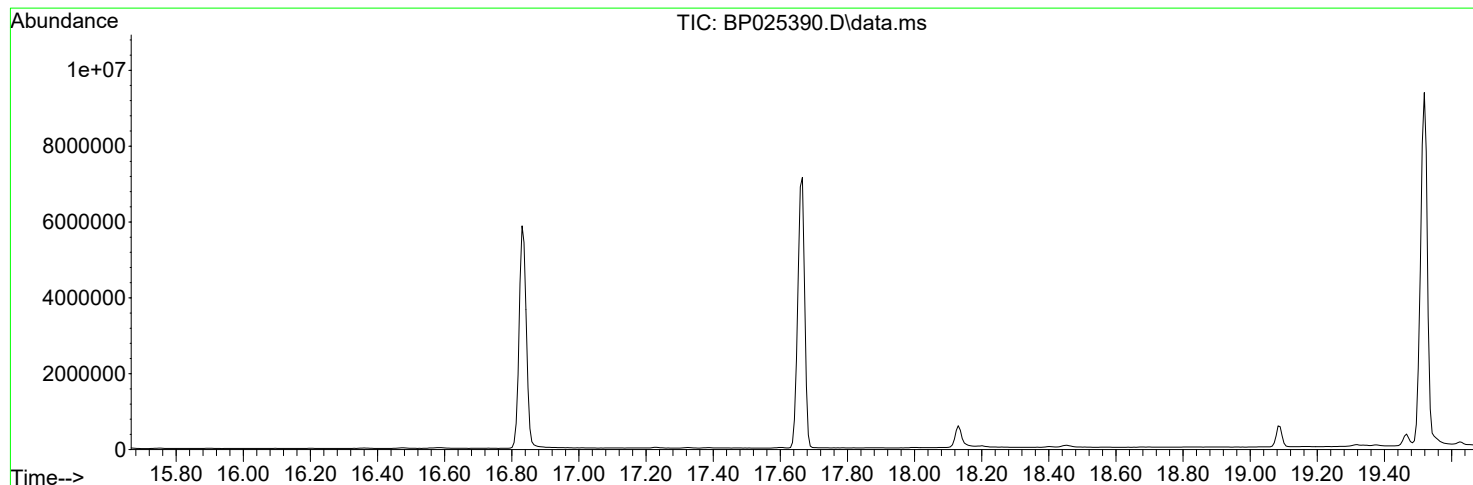

AutoFind: Scans 2503, 2504, 2505; Background Corrected with Scan 2494

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
68	69	0.00	2	1.6	3290	PASS
69	69	100	100	100.0	199967	PASS
70	69	0.00	2	0.4	716	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	680138	PASS
199	198	5	9	6.7	45247	PASS
365	198	1	100	4.4	29981	PASS
441	443	0.01	150	81.3	135091	PASS
442	442	100	100	100.0	866023	PASS
443	442	15	24	19.2	166133	PASS

DDT Breakdown




Date	Instrument Name	DFTPP Data File
8/14/2025	BNA_P	<u>BP025390.D</u>
Compound Name	Response	Retention Time
DDT	2976098	20.818
DDD	52170	20.407
DDE	9165	19.824
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
61335	3037433	2.02

Instrument :
BNA_P
ClientSampleId :
DFTPP

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP081425\
Data File : BP025390.D
Acq On : 14 Aug 2025 10:30
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DFTPP

Quant Time: Aug 14 18:17:37 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP081425.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Aug 14 18:14:31 2025
Response via : Initial Calibration

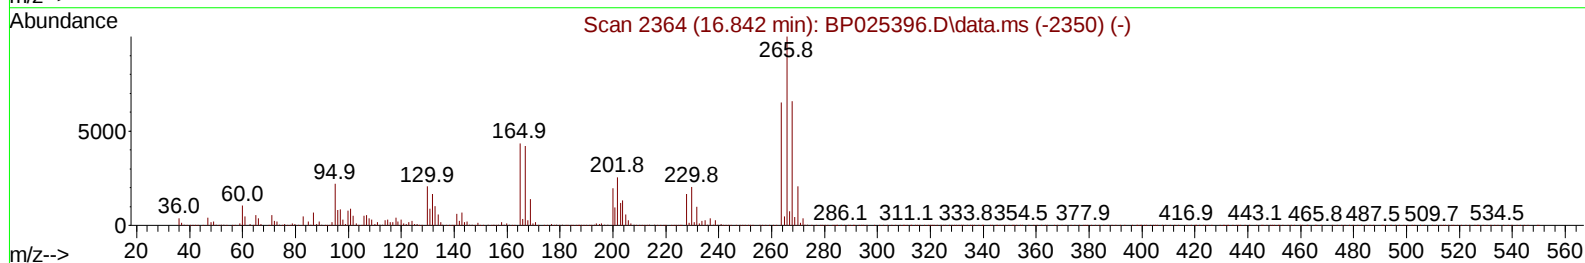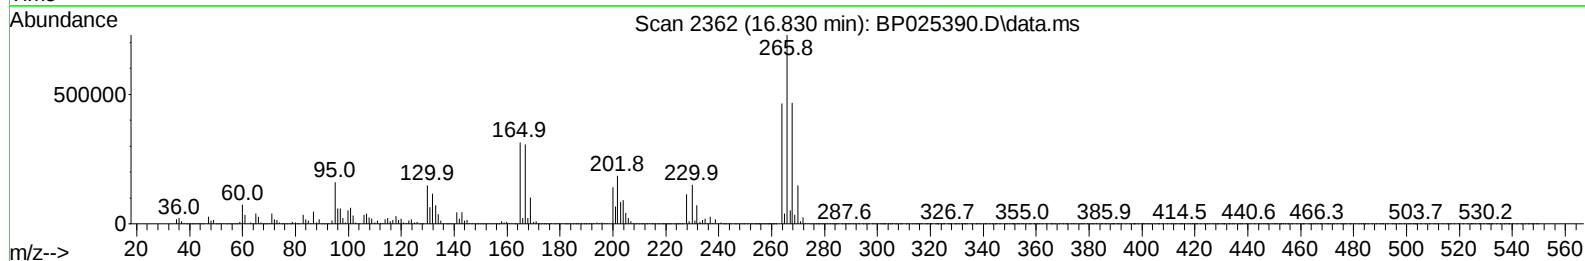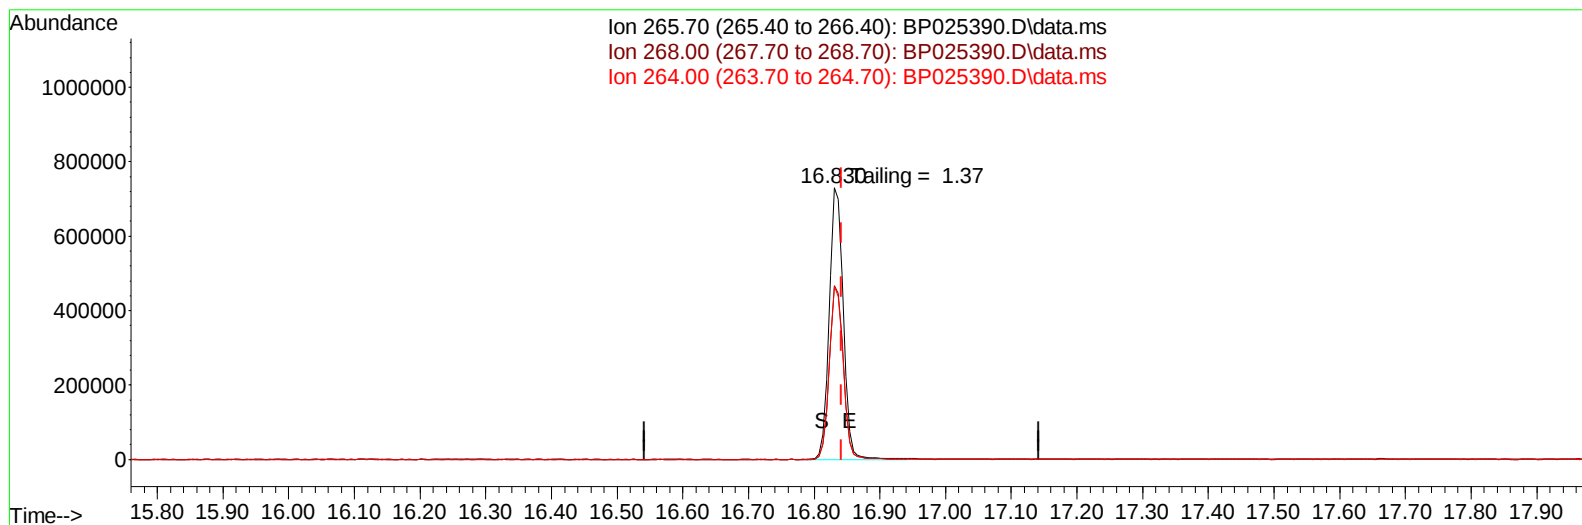

TIC: BP025390.D\data.ms

(70) Pentachlorophenol (C)

16.830min (-0.012) 61985.64 ng




response 1096483

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	65.80	64.04
264.00	65.00	63.79
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP081425\
Data File : BP025390.D
Acq On : 14 Aug 2025 10:30
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DFTPP

Quant Time: Aug 14 18:17:37 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP081425.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Aug 14 18:14:31 2025
Response via : Initial Calibration

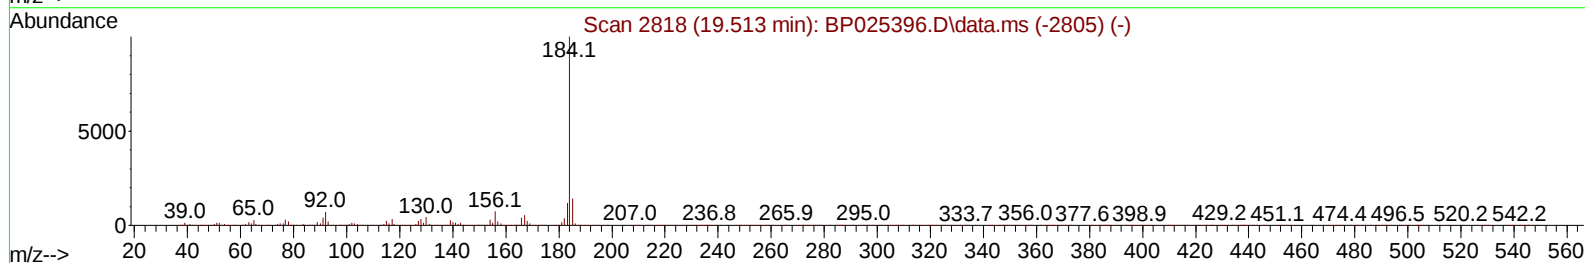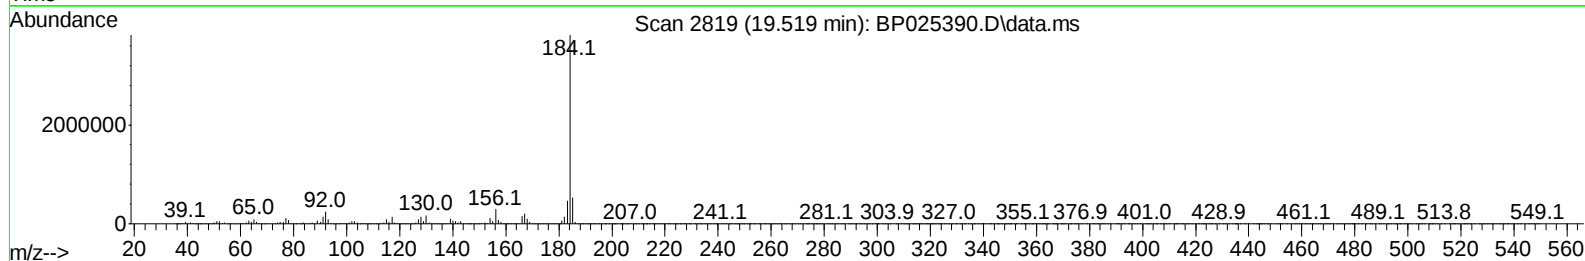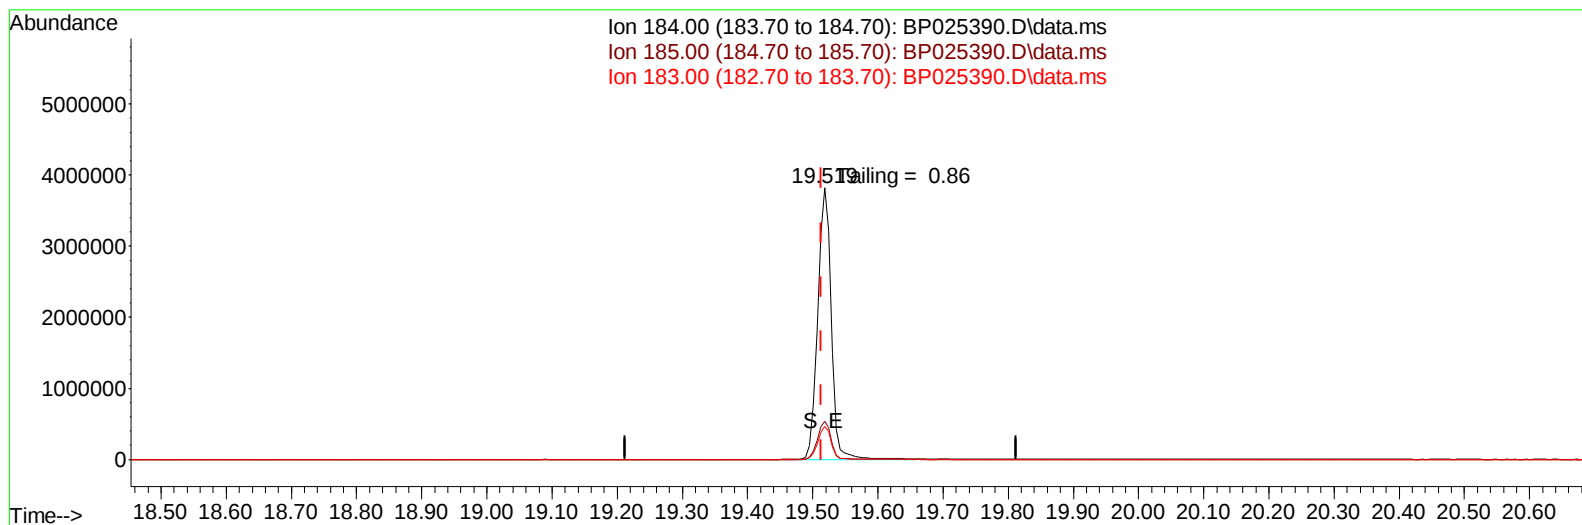

TIC: BP025390.D\data.ms

(77) Benzidine

19.519min (+ 0.006) 64482.34 ng

response 5499416

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.40	14.03
183.00	11.80	12.10
0.00	0.00	0.00