
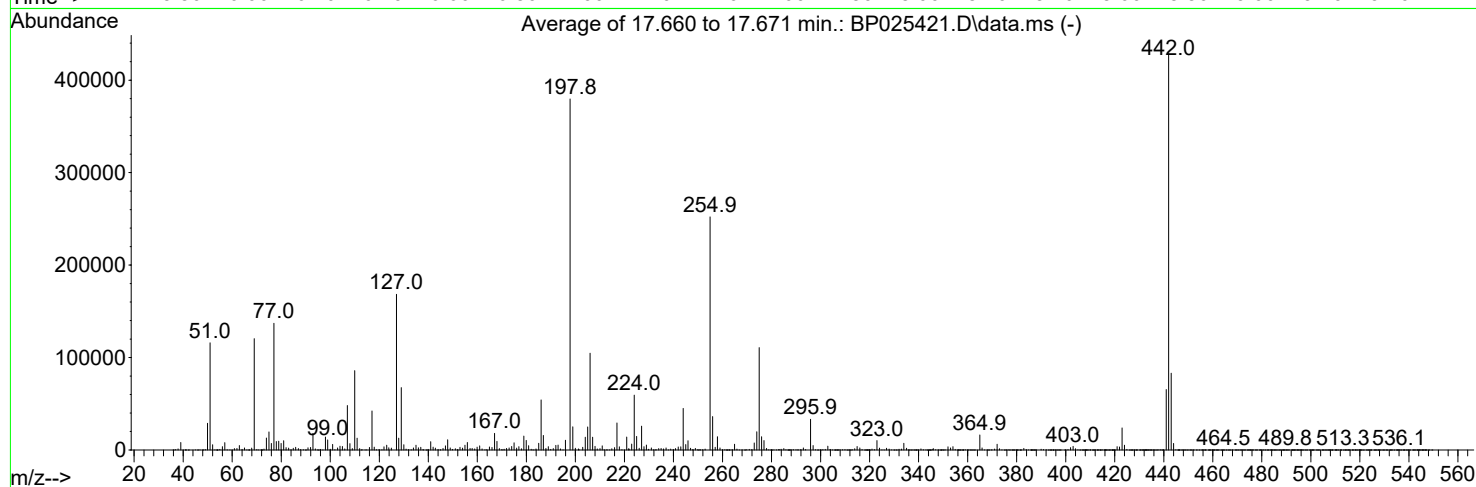


Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP081525\
Data File : BP025421.D
Acq On : 15 Aug 2025 09:55
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP081425.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Thu Aug 14 18:14:31 2025

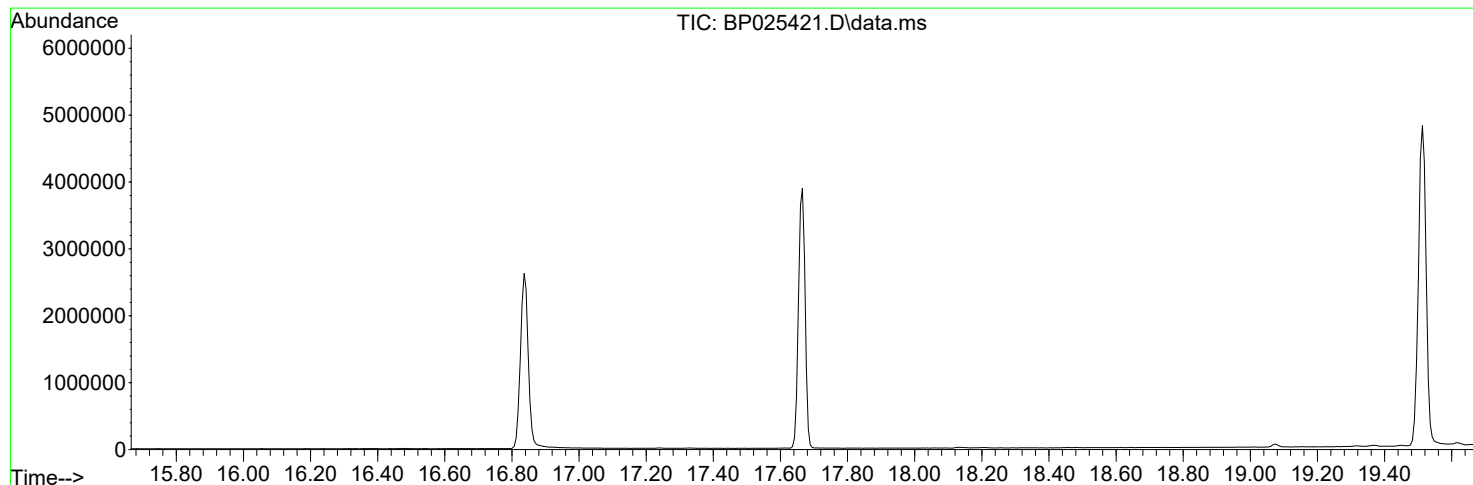

AutoFind: Scans 2503, 2504, 2505; Background Corrected with Scan 2494

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
68	69	0.00	2	1.8	2159	PASS
69	69	100	100	100.0	120418	PASS
70	69	0.00	2	0.5	621	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	379747	PASS
199	198	5	9	6.6	25040	PASS
365	198	1	100	4.3	16274	PASS
441	443	0.01	150	78.6	65352	PASS
442	442	100	100	100.0	427047	PASS
443	442	15	24	19.5	83115	PASS

DDT Breakdown




Date	Instrument Name	DFTPP Data File
8/15/2025	BNA_P	<u>BP025421.D</u>
Compound Name	Response	Retention Time
DDT	1519310	20.812
DDD	29585	20.348
DDE	4915	19.818
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
34500	1553810	2.22

Instrument :
BNA_P
ClientSampleId :
DFTPP

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP081525\
Data File : BP025421.D
Acq On : 15 Aug 2025 09:55
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DFTPP

Quant Time: Aug 15 11:28:21 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP081425.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Aug 14 18:14:31 2025
Response via : Initial Calibration

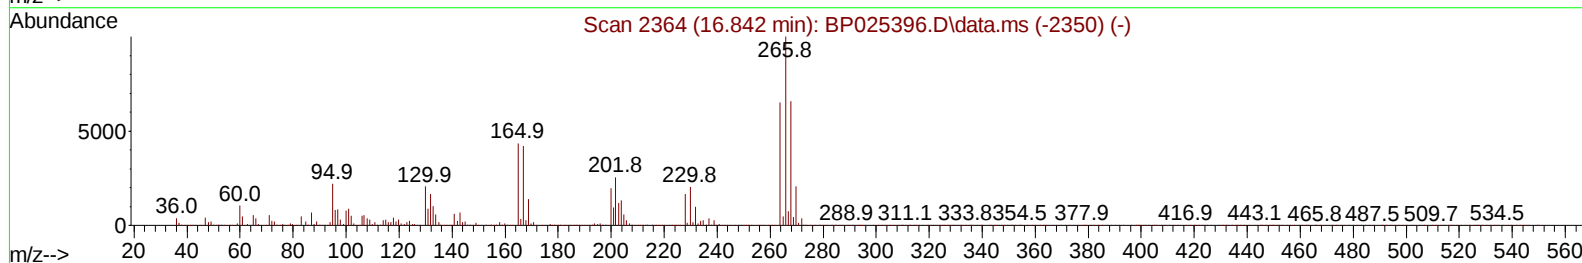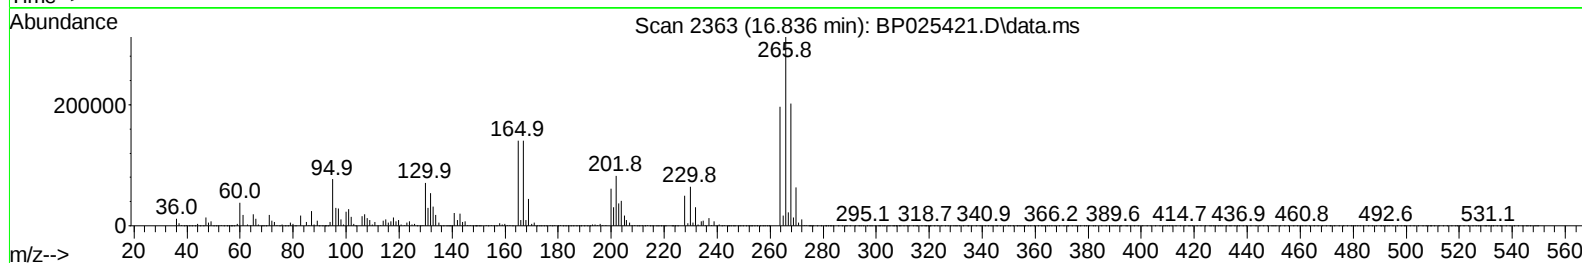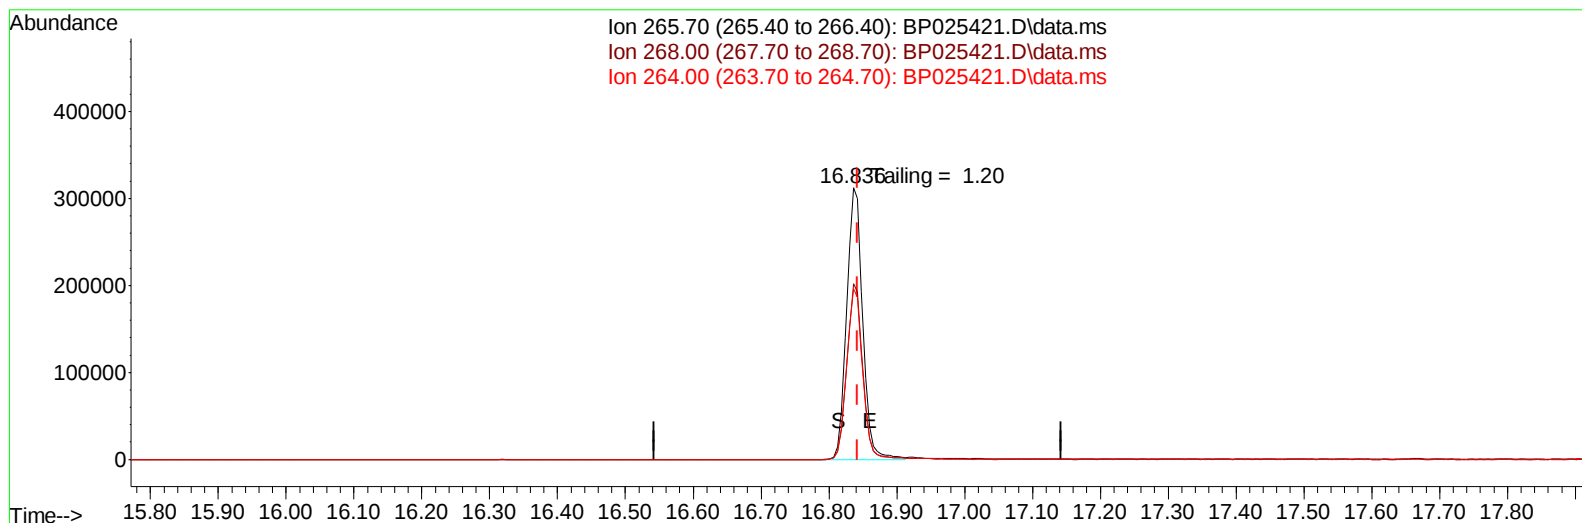

TIC: BP025421.D\data.ms

(70) Pentachlorophenol (C)

16.836min (-0.006) 99008.85 ng




response 510758

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	65.80	64.63
264.00	65.00	62.91
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP081525\
Data File : BP025421.D
Acq On : 15 Aug 2025 09:55
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DFTPP

Quant Time: Aug 15 11:28:21 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP081425.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Aug 14 18:14:31 2025
Response via : Initial Calibration

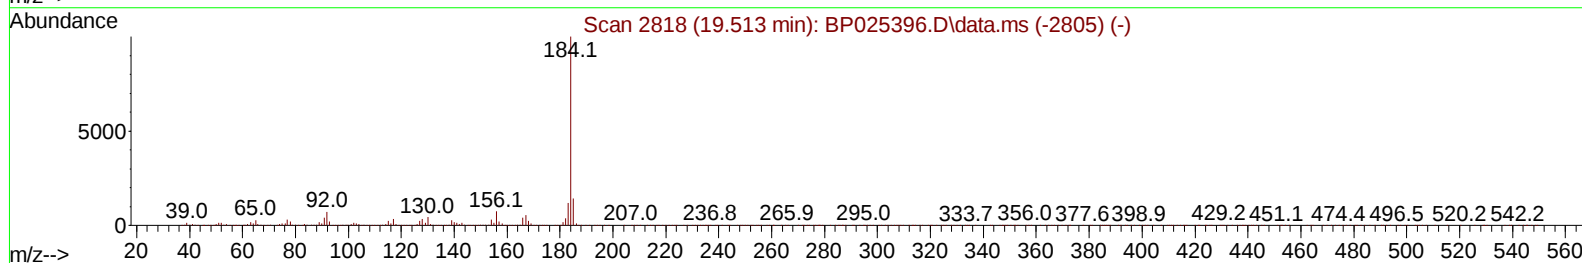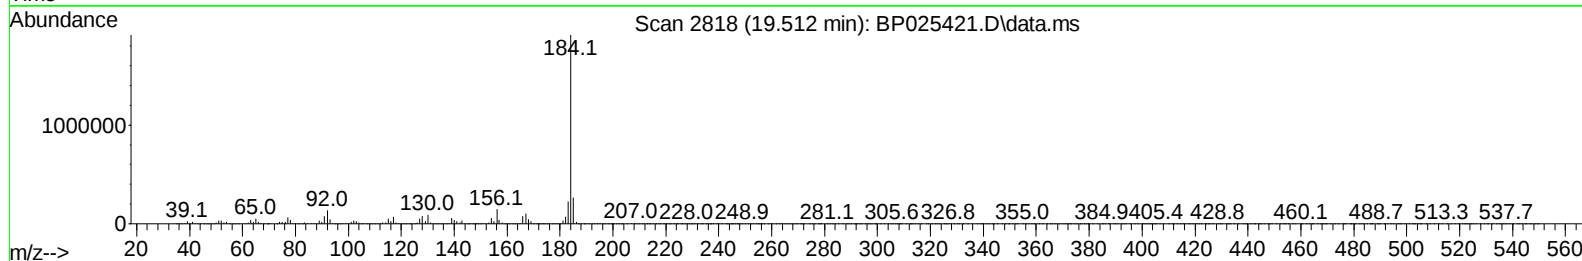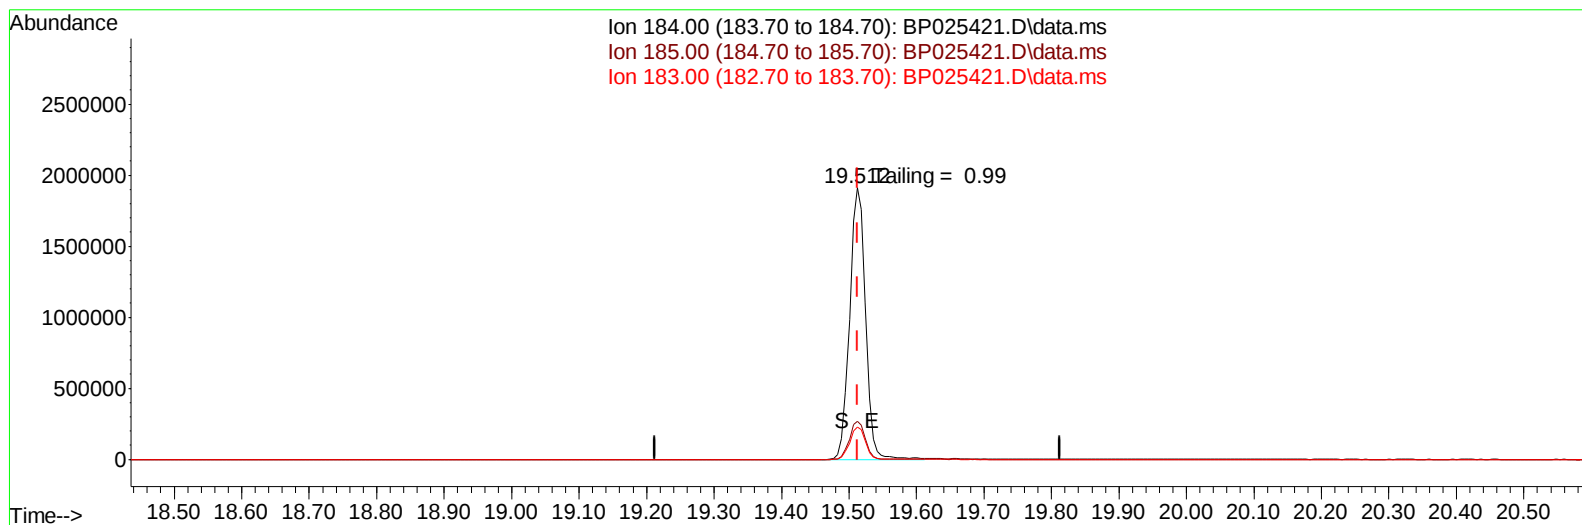

TIC: BP025421.D\data.ms

(77) Benzidine

19.512min (-0.000) 55650.72 ng

response 3124253

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.40	14.04
183.00	11.80	11.97
0.00	0.00	0.00