
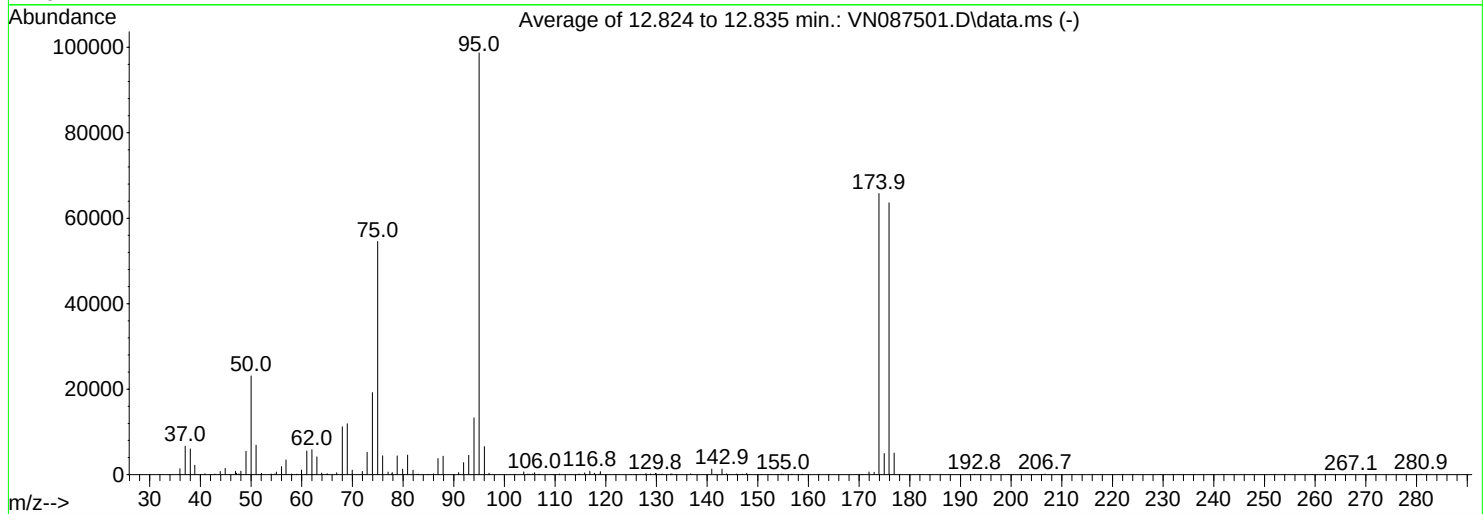


Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN081225\
Data File : VN087501.D
Acq On : 12 Aug 2025 07:57
Operator : JC\MD
Sample : BFB
Misc : 5.0mL/MSVOA_N/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N071625W.M
Title : SW846 8260
Last Update : Thu Jul 17 02:56:13 2025

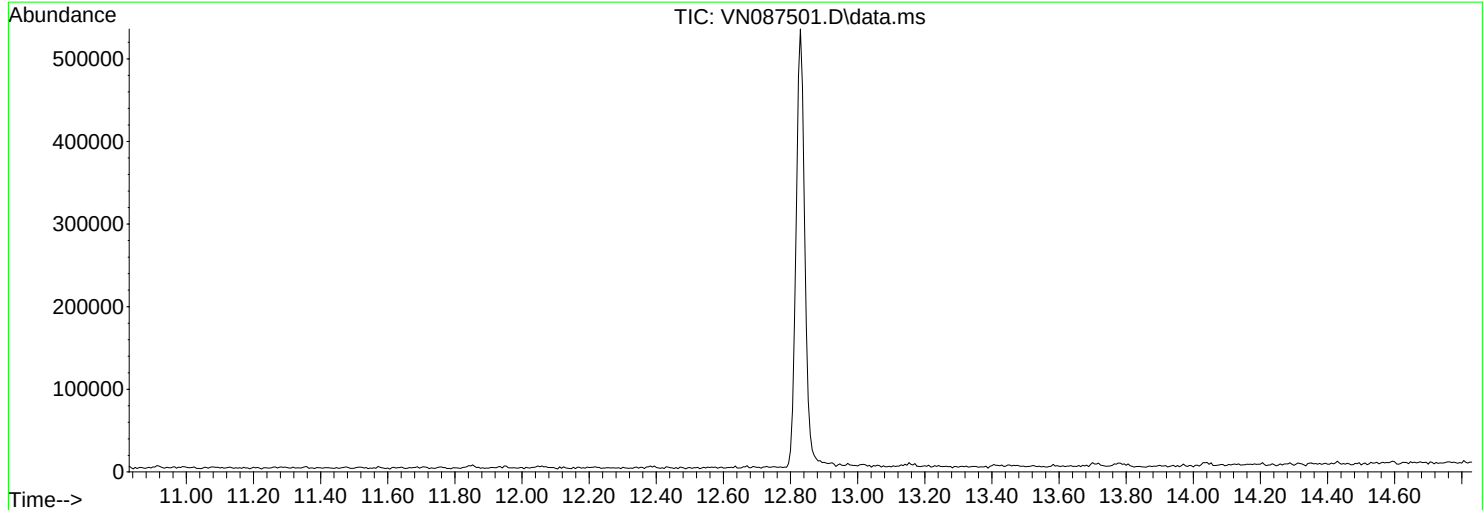

AutoFind: Scans 1848, 1849, 1850; Background Corrected with Scan 1839

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	23.4	23109	PASS
75	95	30	60	55.3	54557	PASS
95	95	100	100	100.0	98707	PASS
96	95	5	9	6.6	6558	PASS
173	174	0.00	2	0.9	578	PASS
174	95	50	100	66.6	65784	PASS
175	174	5	9	7.5	4946	PASS
176	174	95	101	96.7	63619	PASS
177	176	5	9	7.9	5043	PASS

Average of 12.824 to 12.835 min.: VN087501.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
35.95	1378	48.00	814	58.00	138	68.00	1118
37.00	6658	49.00	5460	58.20	52	69.00	1190
38.00	6021	50.00	23109	59.05	128	69.95	105
38.90	2198	51.00	6903	59.95	1106	71.95	73
40.90	221	51.80	79	61.00	5542	72.90	5237
42.85	147	52.05	311	62.00	5833	73.95	19221
43.90	745	54.00	144	63.00	4154	75.00	54557
44.90	1459	54.70	162	63.95	383	75.95	4438
46.90	792	55.00	617	64.80	60	77.05	606
47.10	351	56.00	1893	65.05	235	77.70	168
47.60	197	56.90	3430	66.90	453	77.85	498

Average of 12.824 to 12.835 min.: VN087501.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
78.85	4387	91.95	2794	106.85	130	125.80	53
79.90	1279	92.95	4531	109.70	58	127.80	88
80.90	4553	94.00	13294	110.85	141	127.95	227
81.95	1068	95.00	98707	114.75	139	128.85	191
82.70	60	96.05	6558	115.85	397	129.80	284
83.00	130	96.95	328	116.85	803	130.00	233
84.90	67	103.80	636	117.75	340	130.60	63
86.00	193	104.65	167	118.00	93	131.10	136
86.90	3799	105.00	96	118.70	165	132.80	148
87.90	4303	105.60	183	118.95	717	133.05	196
90.95	488	105.95	442	125.00	51	136.75	199

Average of 12.824 to 12.835 min.: VN087501.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
137.00	81	155.00	135	192.80	98		
140.90	1325	156.75	130	206.70	164		
141.70	57	158.75	107	267.10	74		
142.95	1327	170.60	52	280.90	121		
143.85	205	171.95	644				
145.85	138	172.95	578				
146.95	121	173.90	65784				
147.80	285	174.95	4946				
149.90	54	175.90	63619				
150.80	60	176.90	5043				
154.70	127	177.90	75				

Instrument :

MSVOA_N

ClientSampleId :

BFB