
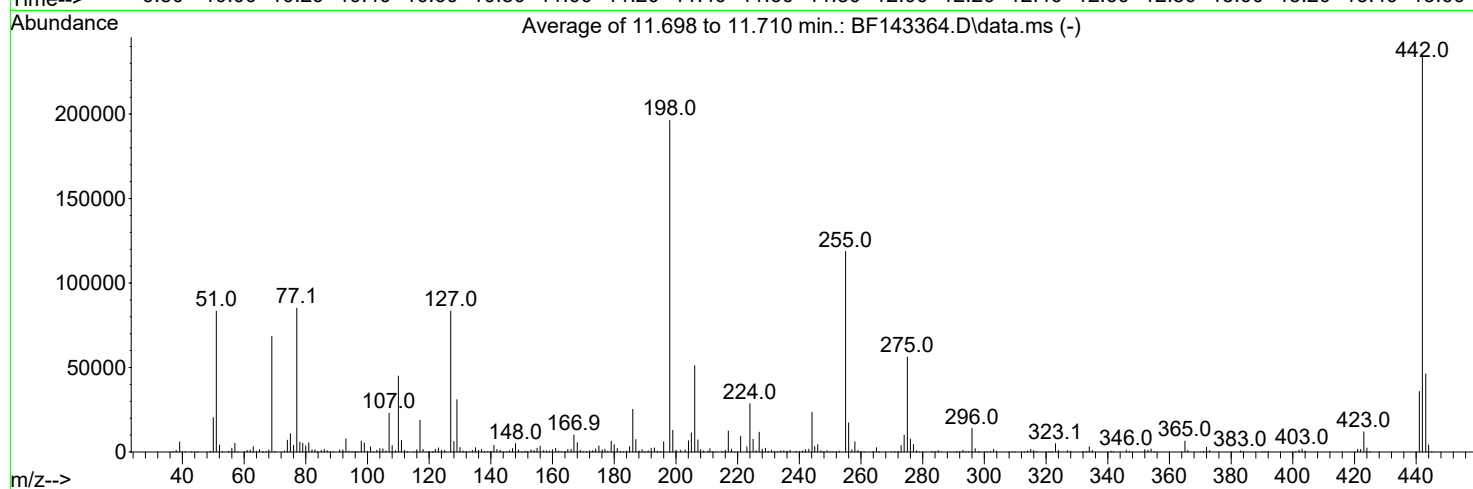


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF081325\
Data File : BF143364.D
Acq On : 13 Aug 2025 08:59
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF081225.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Tue Aug 12 13:25:39 2025

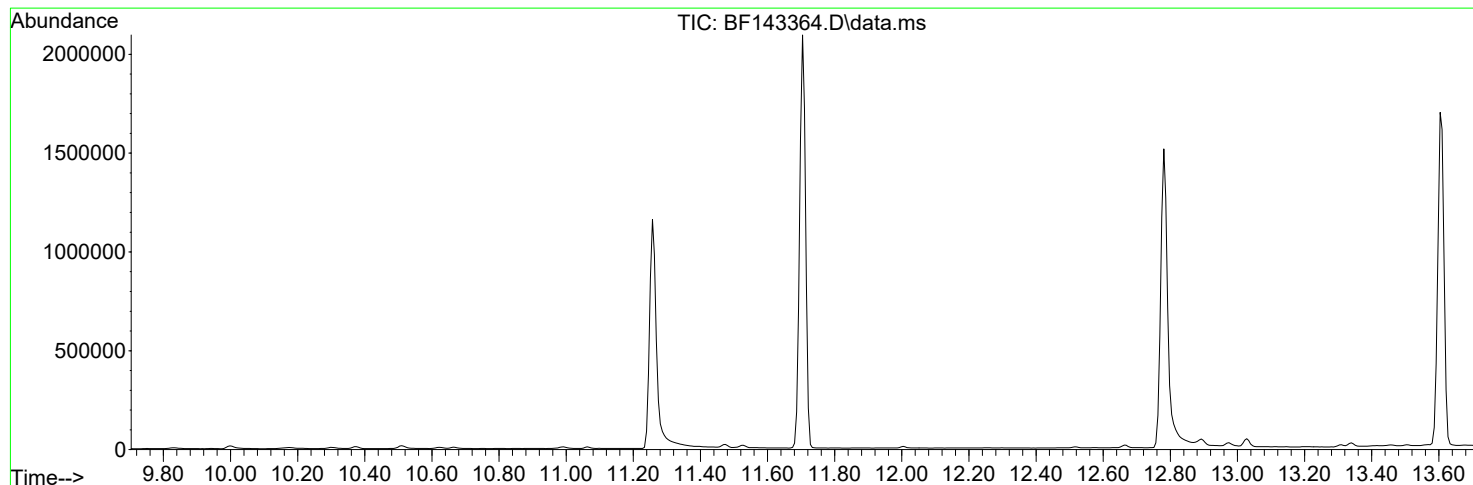

AutoFind: Scans 1616, 1617, 1618; Background Corrected with Scan 1610

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
68	69	0.00	2	1.9	1286	PASS
69	69	100	100	100.0	68336	PASS
70	69	0.00	2	0.6	395	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	196331	PASS
199	198	5	9	6.6	12910	PASS
365	198	1	100	3.3	6489	PASS
441	443	0.01	150	77.5	35787	PASS
442	442	100	100	100.0	233685	PASS
443	442	15	24	19.8	46192	PASS

DDT Breakdown




Date	Instrument Name	DFTPP Data File
8/13/2025	BNA_F	<u>BF143364.D</u>
Compound Name	Response	Retention Time
DDT	428873	13.604
DDD	10022	13.339
DDE	6725	12.975
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
16747	445620	3.76

Instrument :
BNA_F
ClientSampleId :
DFTPP

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF081325\
Data File : BF143364.D
Acq On : 13 Aug 2025 08:59
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Aug 13 11:48:18 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF081225.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Aug 12 13:25:39 2025
Response via : Initial Calibration

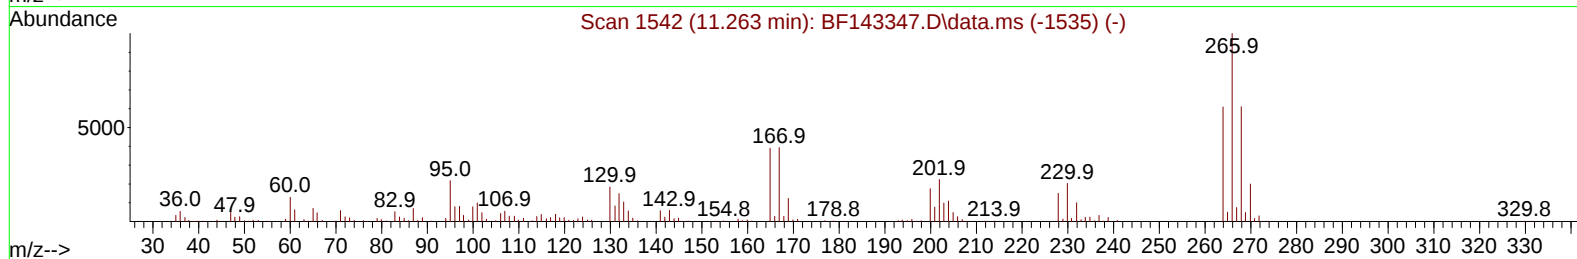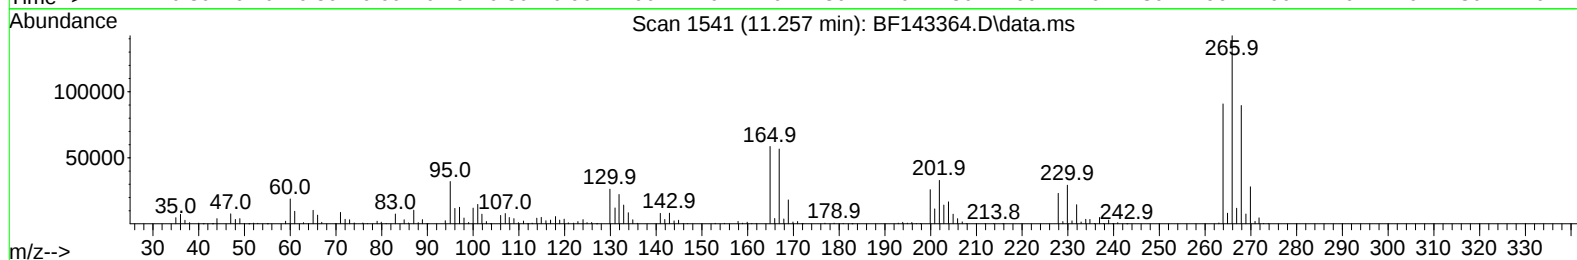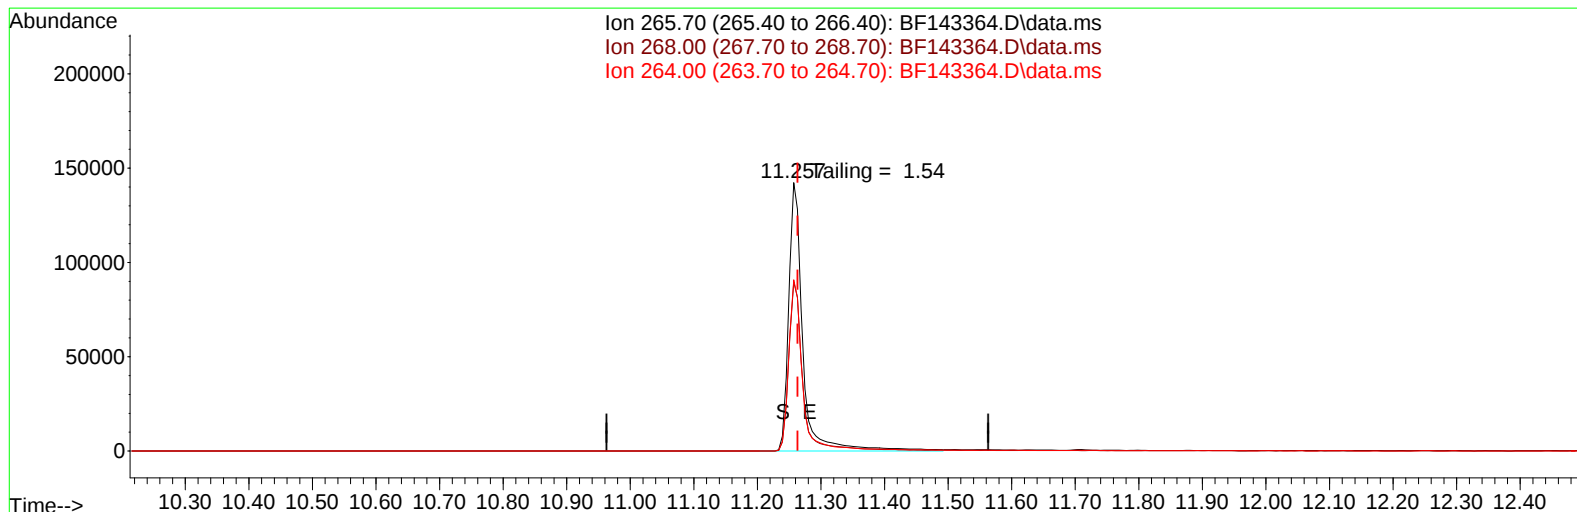

TIC: BF143364.D\data.ms

(70) Pentachlorophenol (C)

11.257min (-0.006) 27752.57 ng




response 221678

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	61.00	62.96
264.00	61.00	63.80
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF081325\
Data File : BF143364.D
Acq On : 13 Aug 2025 08:59
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Aug 13 11:48:18 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF081225.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Aug 12 13:25:39 2025
Response via : Initial Calibration

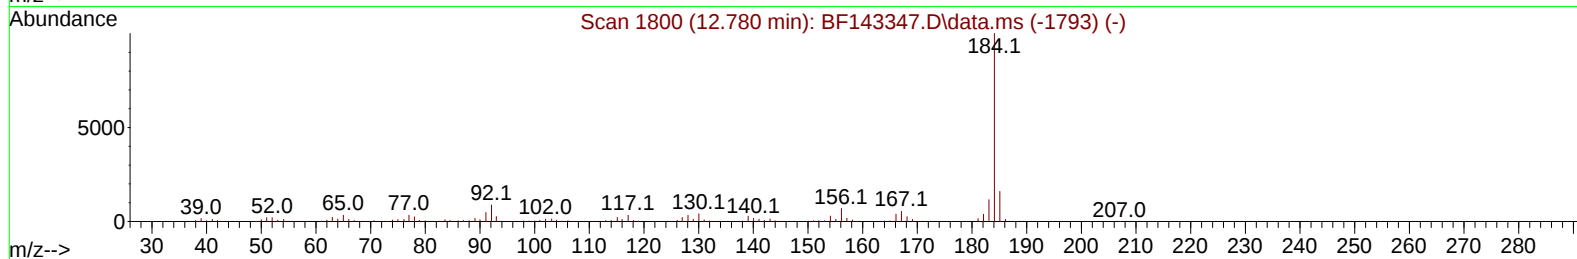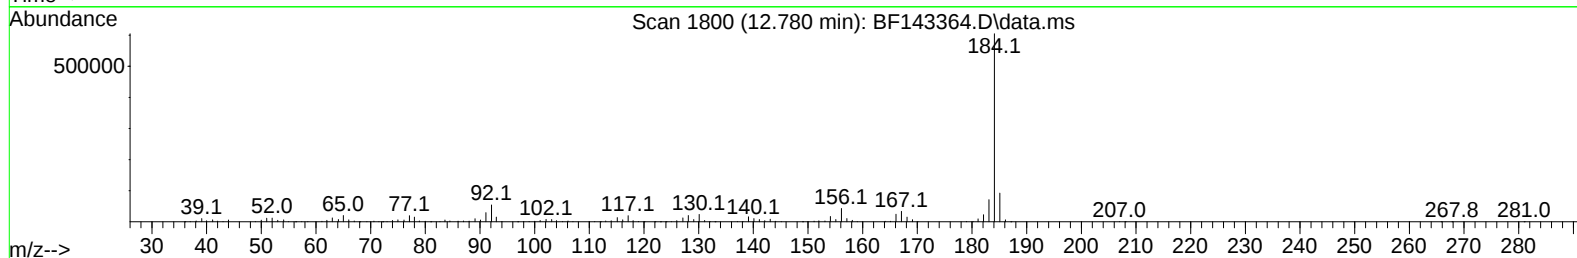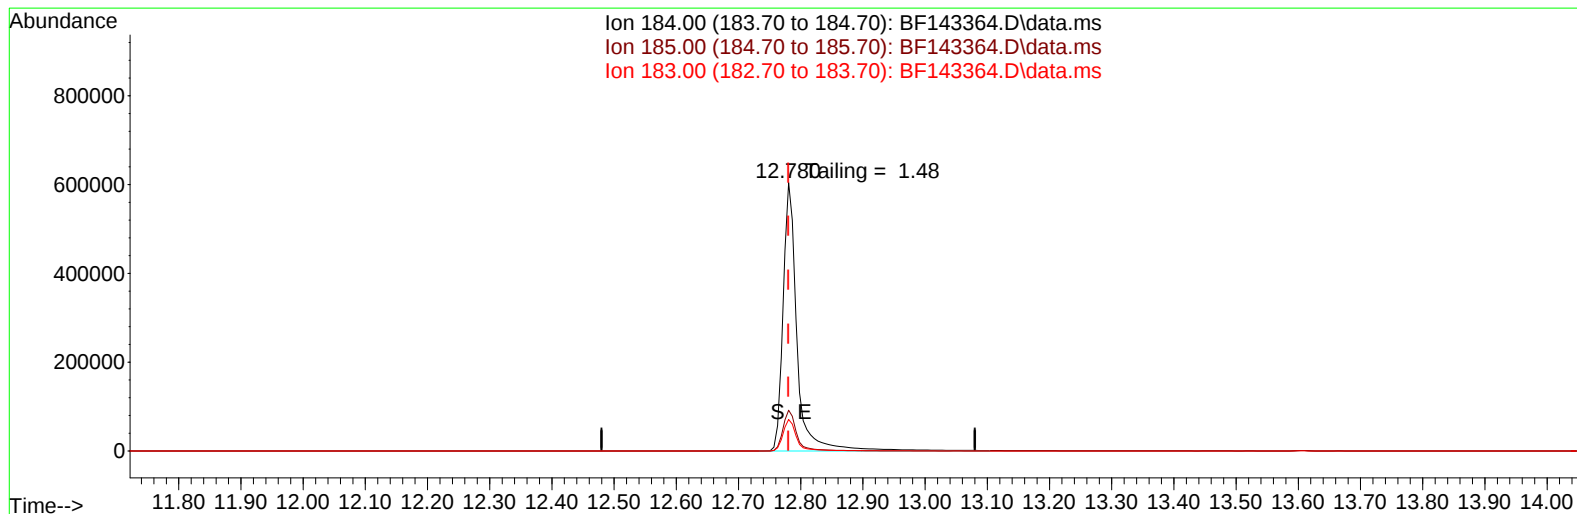

TIC: BF143364.D\data.ms

(77) Benzidine

12.780min (+ 0.000) 0.00 ng

response 949077

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	16.00	15.22
183.00	11.60	11.79
0.00	0.00	0.00