
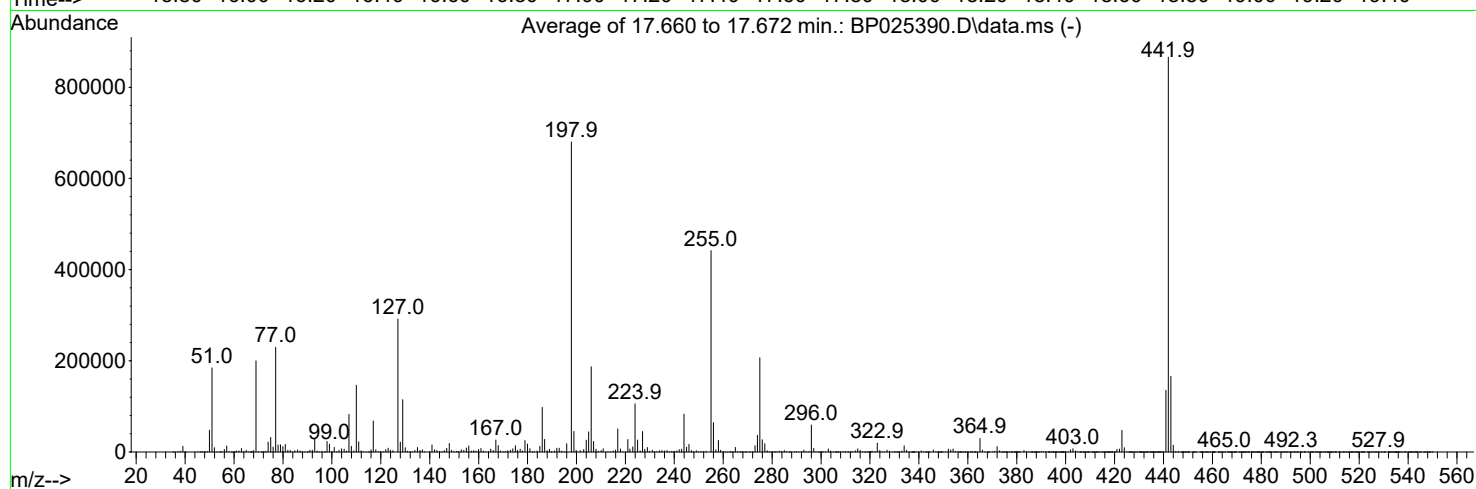


Data Path : Z:\svoasrv\HPCHEM1\BNA\_P\Data\BP081425\  
Data File : BP025390.D  
Acq On : 14 Aug 2025 10:30  
Operator : CG/JU  
Sample : DFTPP  
Misc :  
ALS Vial : 1 Sample Multiplier: 1

Instrument :  
BNA\_P  
ClientSampleId :  
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA\_P\Methods\8270E-BP081425.M  
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
Last Update : Thu Aug 14 18:14:31 2025

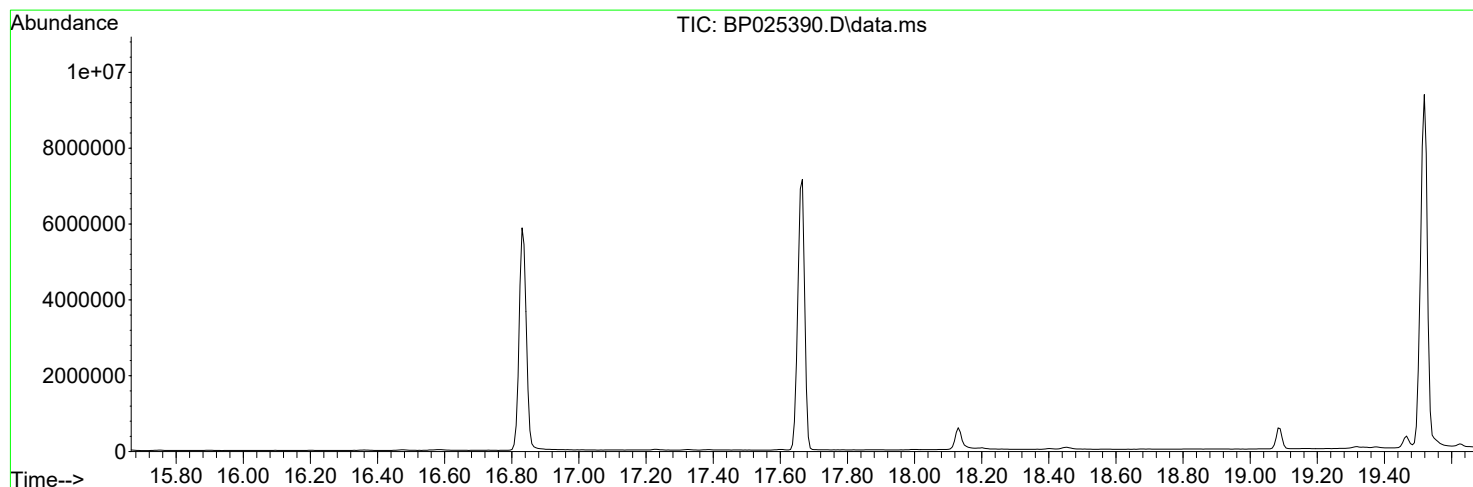

AutoFind: Scans 2503, 2504, 2505; Background Corrected with Scan 2494

| Target | Rel. to | Lower  | Upper  | Rel.  | Raw    | Result    |
|--------|---------|--------|--------|-------|--------|-----------|
| Mass   | Mass    | Limit% | Limit% | Abn%  | Abn    | Pass/Fail |
| 68     | 69      | 0.00   | 2      | 1.6   | 3290   | PASS      |
| 69     | 69      | 100    | 100    | 100.0 | 199967 | PASS      |
| 70     | 69      | 0.00   | 2      | 0.4   | 716    | PASS      |
| 197    | 198     | 0.00   | 2      | 0.0   | 0      | PASS      |
| 198    | 198     | 100    | 100    | 100.0 | 680138 | PASS      |
| 199    | 198     | 5      | 9      | 6.7   | 45247  | PASS      |
| 365    | 198     | 1      | 100    | 4.4   | 29981  | PASS      |
| 441    | 443     | 0.01   | 150    | 81.3  | 135091 | PASS      |
| 442    | 442     | 100    | 100    | 100.0 | 866023 | PASS      |
| 443    | 442     | 15     | 24     | 19.2  | 166133 | PASS      |

# DDT Breakdown




| Date          | Instrument Name  | DFTPP Data File    |
|---------------|------------------|--------------------|
| 8/14/2025     | BNA_P            | <u>BP025390.D</u>  |
|               |                  |                    |
|               |                  |                    |
| Compound Name | Response         | Retention Time     |
|               |                  |                    |
| DDT           | 2976098          | 20.818             |
| DDD           | 52170            | 20.407             |
| DDE           | 9165             | 19.824             |
|               |                  |                    |
|               |                  |                    |
| SUM(DDD+DDE)  | SUM(DDT+DDD+DDE) | % Breakdown Of DDT |
|               |                  |                    |
| 61335         | 3037433          | 2.02               |
|               |                  |                    |

Instrument :  
BNA\_P  
ClientSampleId :  
DFTPP

Data Path : Z:\svoasrv\HPCHEM1\BNA\_P\Data\BP081425\  
Data File : BP025390.D  
Acq On : 14 Aug 2025 10:30  
Operator : CG/JU  
Sample : DFTPP  
Misc :  
ALS Vial : 1 Sample Multiplier: 1

Instrument :  
BNA\_P  
ClientSampleId :  
DFTPP

Quant Time: Aug 14 18:17:37 2025  
Quant Method : Z:\svoasrv\HPCHEM1\BNA\_P\Methods\8270E-BP081425.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
QLast Update : Thu Aug 14 18:14:31 2025  
Response via : Initial Calibration

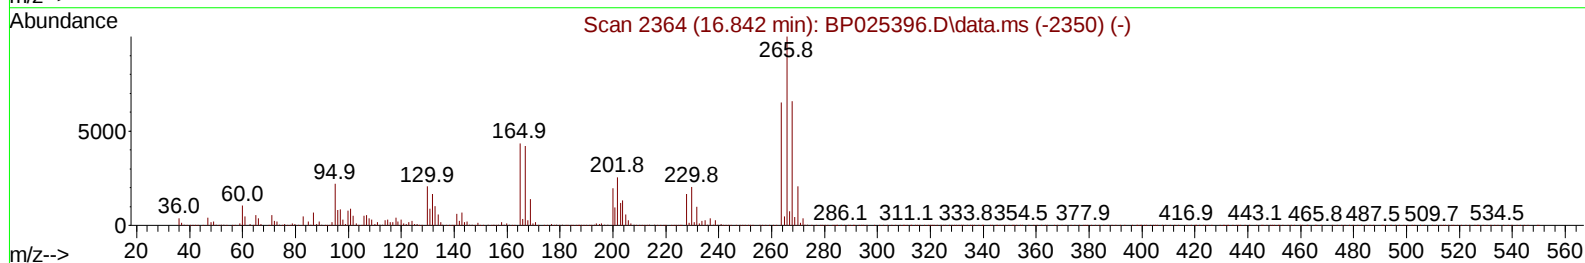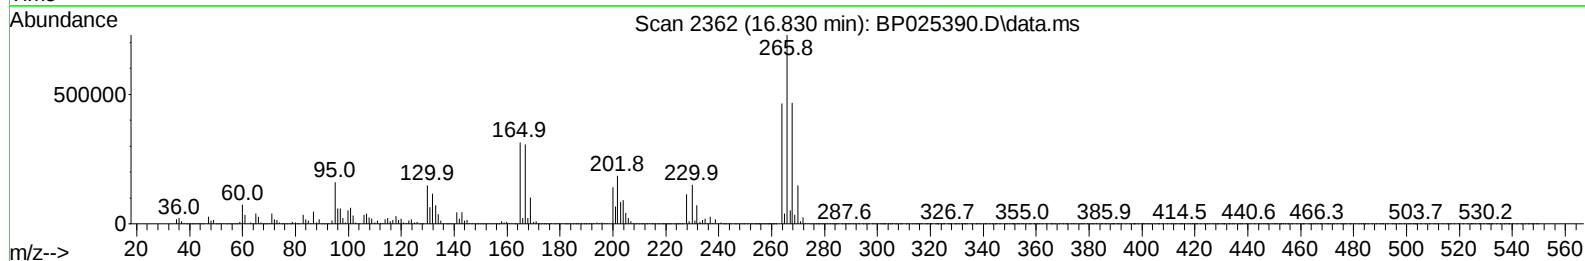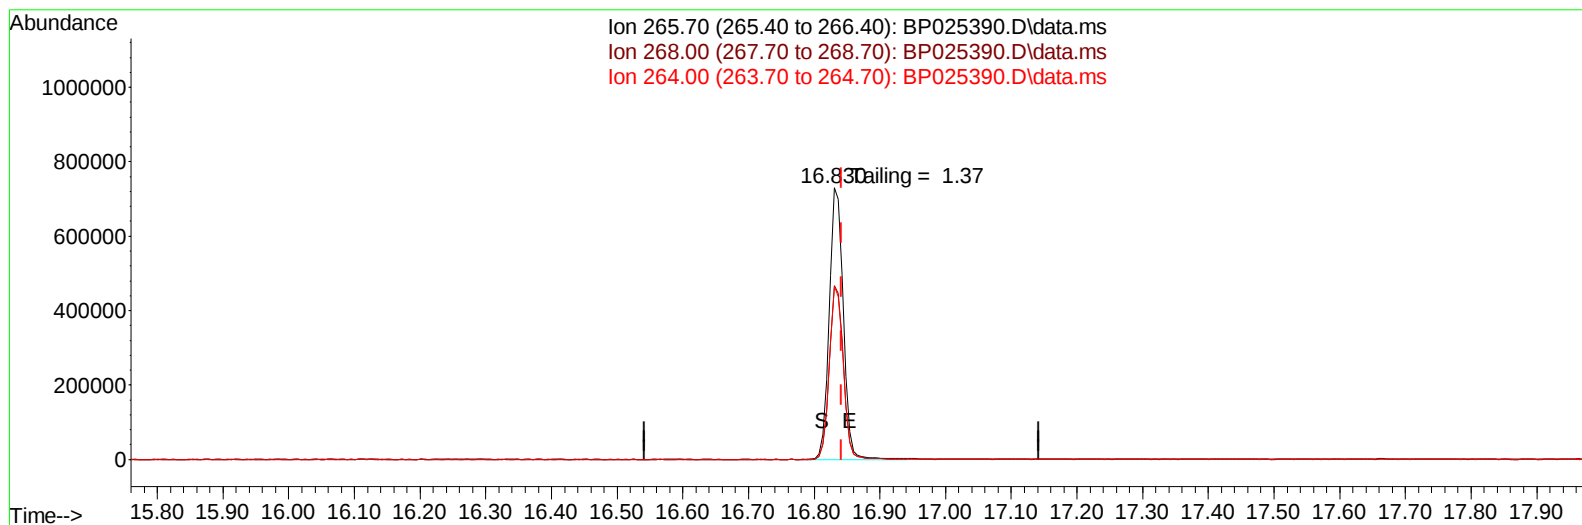

TIC: BP025390.D\data.ms

**(70) Pentachlorophenol (C)**

**16.830min (-0.012) 61985.64 ng**




**response 1096483**

| Ion    | Exp%   | Act%   |
|--------|--------|--------|
| 265.70 | 100.00 | 100.00 |
| 268.00 | 65.80  | 64.04  |
| 264.00 | 65.00  | 63.79  |
| 0.00   | 0.00   | 0.00   |

Data Path : Z:\svoasrv\HPCHEM1\BNA\_P\Data\BP081425\  
Data File : BP025390.D  
Acq On : 14 Aug 2025 10:30  
Operator : CG/JU  
Sample : DFTPP  
Misc :  
ALS Vial : 1 Sample Multiplier: 1

Instrument :  
BNA\_P  
ClientSampleId :  
DFTPP

Quant Time: Aug 14 18:17:37 2025  
Quant Method : Z:\svoasrv\HPCHEM1\BNA\_P\Methods\8270E-BP081425.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
QLast Update : Thu Aug 14 18:14:31 2025  
Response via : Initial Calibration

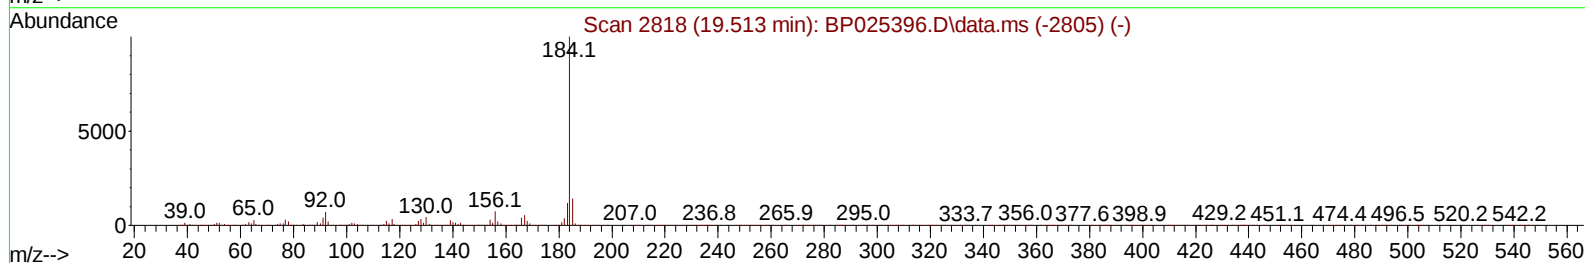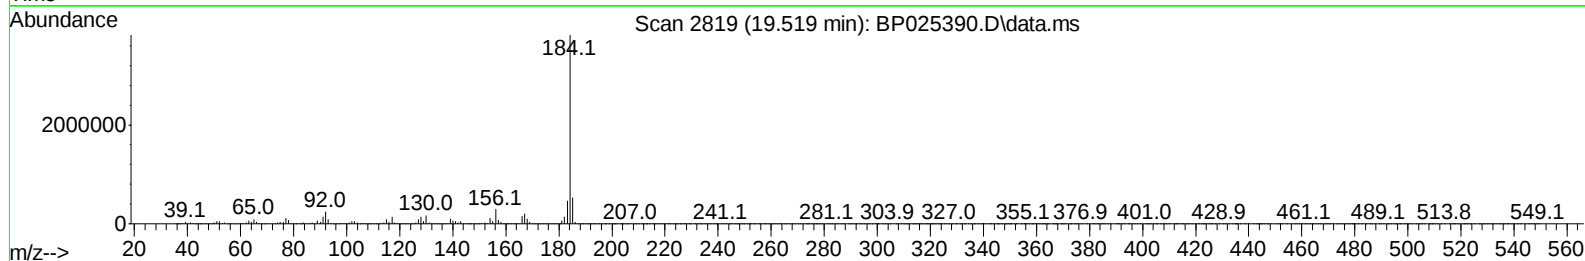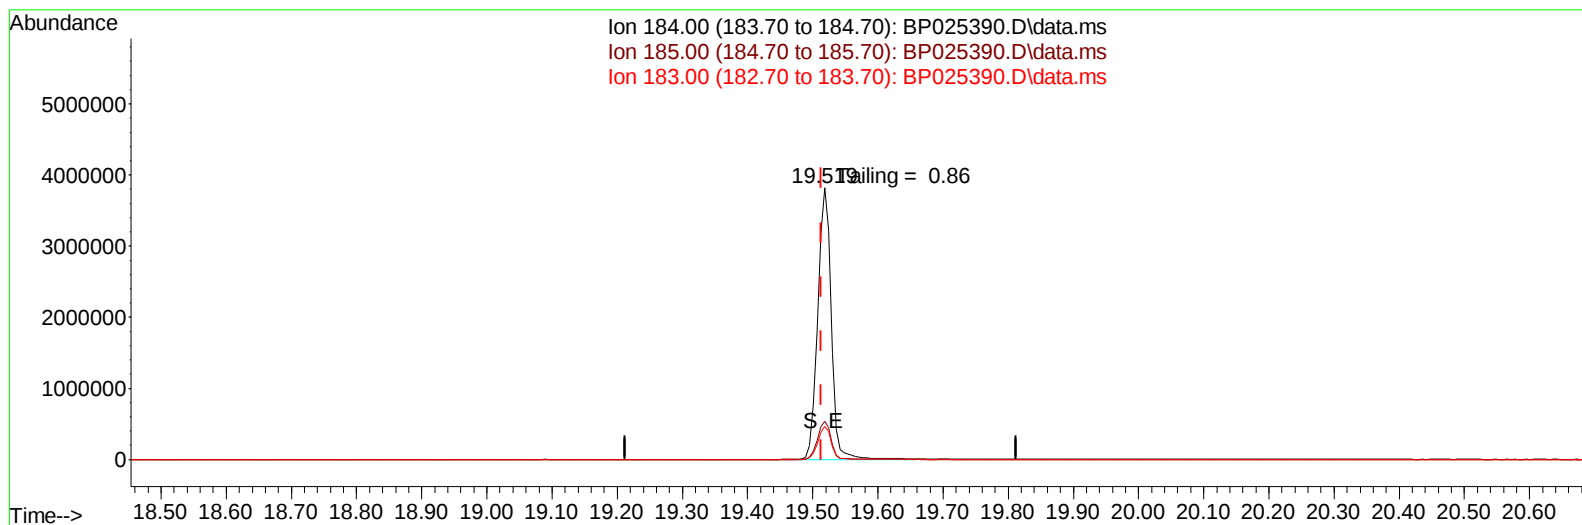

TIC: BP025390.D\data.ms

(77) Benzidine

19.519min (+ 0.006) 64482.34 ng

response 5499416

| Ion    | Exp%   | Act%   |
|--------|--------|--------|
| 184.00 | 100.00 | 100.00 |
| 185.00 | 14.40  | 14.03  |
| 183.00 | 11.80  | 12.10  |
| 0.00   | 0.00   | 0.00   |