

Instrume IC-1		Analyst : NF		Method: 300.0 / 9056A						
Ident	Con F-	Con CL-	Con NO2	Con BR-	Con NO	Con HPC	Con SO4	Method name	date time	Initial Analyst
STD1	0.000	0.000	0.000	0.000	0.000	0.000	0.000	IC1-080625	8/6/2025 10:18	10 RM/IZ
STD2	0.413	0.620	0.623	2.052	0.515	1.033	3.185	IC1-080625	8/6/2025 10:40	10 RM/IZ
STD3	0.794	1.184	1.185	3.953	0.990	2.067	5.931	IC1-080625	8/6/2025 11:01	10 RM/IZ
STD4	1.023	1.524	1.519	5.070	1.270	2.633	7.597	IC1-080625	8/6/2025 11:23	10 RM/IZ
STD5	1.972	2.981	2.982	9.960	2.483	4.695	14.838	IC1-080625	8/6/2025 11:44	10 RM/IZ
STD6	3.956	5.938	5.934	19.801	4.945	9.953	29.505	IC1-080625	8/6/2025 12:06	10 RM/IZ
STD7	5.041	7.553	7.556	25.165	6.298	12.620	37.443	IC1-080625	8/6/2025 12:27	10 RM/IZ
ICV	2.038	3.184	3.095	10.343	2.641	4.970	15.425	IC1-080625	8/6/2025 12:48	10 RM/IZ
ICB	0.000	0.000	0.000	0.000	0.000	0.000	0.000	IC1-080625	8/6/2025 13:10	10 RM/IZ
CCV	1.992	2.992	2.985	10.019	2.495	4.852	14.924	IC1-080625	8/13/2025 9:19	10 RM/IZ
CCB	0.000	0.000	0.000	0.000	0.000	0.000	0.000	IC1-080625	8/13/2025 9:40	10 RM/IZ
LB136803BLW	0.000	0.000	0.000	0.000	0.000	0.000	0.000	IC1-080625	8/13/2025 10:02	10 RM/IZ
LB136803BSW	1.994	2.998	2.989	10.027	2.504	5.009	14.969	IC1-080625	8/13/2025 10:23	10 RM/IZ
Q2842-01	0.285	18.656	0.000	0.000	0.000	0.000	2.402	IC1-080625	8/13/2025 13:42	10 RM/IZ
Q2842-03	0.230	20.610	0.000	0.236	0.000	0.000	41.007	IC1-080625	8/13/2025 14:25	10 RM/IZ
Q2842-04MS	2.300	23.450	3.027	10.347	2.555	3.053	55.132	IC1-080625	8/13/2025 15:08	10 RM/IZ
Q2842-05MSD	2.369	23.289	3.072	10.483	2.600	3.296	55.367	IC1-080625	8/13/2025 15:51	10 RM/IZ
Q2842-01DLX5	0.086	3.604	0.000	0.000	0.000	0.000	0.760	IC1-080625	8/13/2025 16:13	10 RM/IZ
Q2842-03DLX5	0.074	3.882	0.000	0.000	0.000	0.000	8.127	IC1-080625	8/13/2025 16:34	10 RM/IZ
CCV	1.978	2.973	2.960	9.963	2.482	5.051	14.657	IC1-080625	8/13/2025 17:39	10 RM/IZ
CCB	0.000	0.000	0.000	0.000	0.000	0.000	0.000	IC1-080625	8/13/2025 18:00	10 RM/IZ

Clear table


Instrument ID: IC-2 Analyst : IZ Method: 300.0 / 9056A											
ident	concentra tion F-	concentratio n CL-	concentratio on NO2	concentratio on BR-	concentratio on NO3	concentratio n HPO4	concentratio on SO4	file name	date time	Initial wt/ Final	Analyst
		0.0000 0.6200 1.1840 1.5240 2.9810 5.9380 7.5530	0.0000 0.6230 1.1850 1.5190 2.9820 5.9340 7.5560	0.0000 2.0520 3.9530 5.0700 9.9600 19.8010 25.1650	0.0000 0.5150 0.9900 1.2700 2.4830 4.9450 6.2980	0.0000 1.0330 2.0670 2.6330 4.6950 9.9530 12.6200	0.0000 3.1850 5.9310 7.5970 14.8380 29.5050 37.4430	IC1-080625 IC1-080625 IC1-080625 IC1-080625 IC1-080625 IC1-080625 IC1-080625			
STD1	0.0000								8/6/2025 10:18	10	RM/IZ
STD2	0.4130								8/6/2025 10:40	10	RM/IZ
STD3	0.7940								8/6/2025 11:01	10	RM/IZ
STD4	1.0230								8/6/2025 11:23	10	RM/IZ
STD5	1.9720								8/6/2025 11:44	10	RM/IZ
STD6	3.9560								8/6/2025 12:06	10	RM/IZ
STD7	5.0410								8/6/2025 12:27	10	RM/IZ

ident	True Value F-	True Value CL-	True Value NO2	True Value BR-	True Value NO3	True Value HPO4	True Value SO4
		0.0000 0.6000 1.2000 1.5000 3.0000 6.0000 7.5000	0.0000 0.6000 1.2000 1.5000 3.0000 6.0000 7.5000	0.0000 2.0000 4.0000 5.0000 10.0000 20.0000 25.0000	0.0000 0.5000 1.0000 1.2500 2.5000 5.0000 6.2500	0.0000 1.0000 2.0000 2.5000 5.0000 10.0000 12.5000	0.0000 3.0000 6.0000 7.5000 15.0000 30.0000 37.0000
STD1	0.0000						
STD2	0.4000						
STD3	0.8000						
STD4	1.0000						
STD5	2.0000						
STD6	4.0000						
STD7	5.0000						

ident	Relative Error F-	Relative Error CL-	Relative Error NO2	Relative Error BR-	Relative Error NO3	Relative Error HPO4	Relative Error SO4
		3.3333 -1.3333 1.6000 -0.6333 -1.0333 0.7067	3.8333 -1.2500 1.2667 -0.6000 -1.1000 0.7467	2.6000 -1.1750 1.4000 -0.4000 -0.9950 0.6600	3.0000 -1.0000 1.6000 -0.6800 -1.1000 0.7680	3.3000 3.3500 5.3200 -6.1000 -0.4700 0.9600	6.1667 -1.1500 1.2933 -1.0800 -1.6500 1.1973
STD1							
STD2	3.2500						
STD3	-0.7500						
STD4	2.3000						
STD5	-1.4000						
STD6	-1.1000						
STD7	0.8200						

Fluoride (Anions)

($\mu\text{S}/\text{cm}$) x min

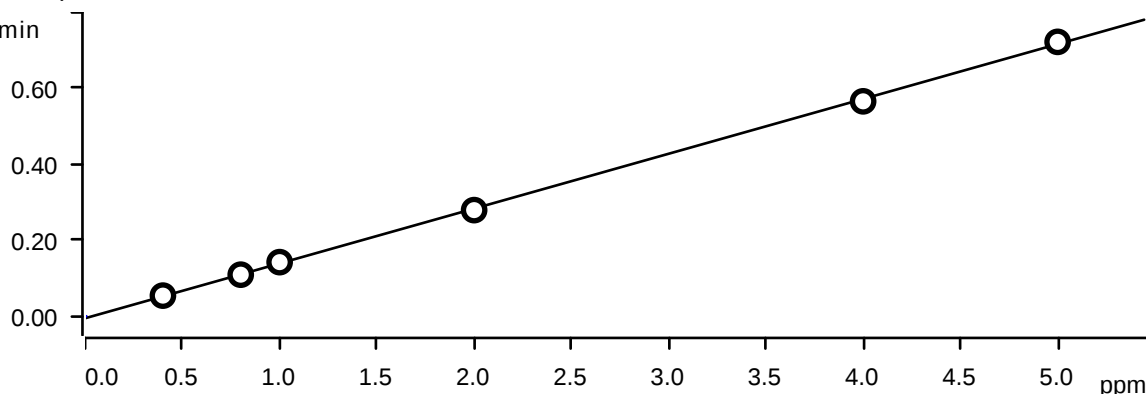

Function: $A = -5.18233\text{E-}3 + 0.0144368 \times Q$


Relative standard deviation 1.650446 %

Correlation coefficient 0.999856

Sample type	Index	Conc.	Volume	Dilution	Sample amount	Area	Ident	Date	Used
Standard 1	1	0.000	10.0	1.0	1.0	n. d.	STD1	2025-08-06 10:18:54 UTC-4	used
Standard 2	1	0.400	10.0	1.0	1.0	0.054	STD2	2025-08-06 10:40:18 UTC-4	used
Standard 3	1	0.800	10.0	1.0	1.0	0.110	STD3	2025-08-06 11:01:42 UTC-4	used
Standard 4	1	1.000	10.0	1.0	1.0	0.143	STD4	2025-08-06 11:23:08 UTC-4	used
Standard 5	1	2.000	10.0	1.0	1.0	0.280	STD5	2025-08-06 11:44:33 UTC-4	used
Standard 6	1	4.000	10.0	1.0	1.0	0.566	STD6	2025-08-06 12:06:00 UTC-4	used
Standard 7	1	5.000	10.0	1.0	1.0	0.723	STD7	2025-08-06 12:27:27 UTC-4	used

Chloride (Anions)

($\mu\text{S}/\text{cm}$) x min

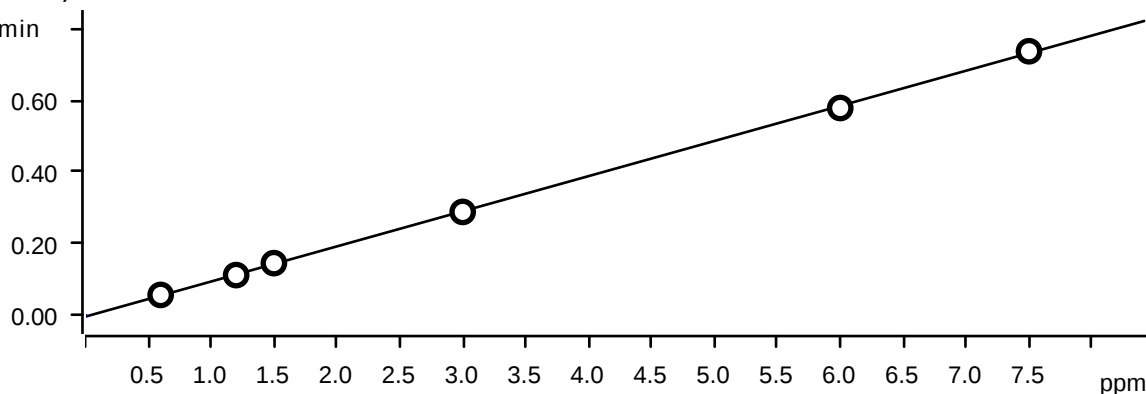

Function: $A = -3.45407\text{E-}3 + 9.79772\text{E-}3 \times Q$


Relative standard deviation 1.384132 %

Correlation coefficient 0.999898

Sample type	Index	Conc.	Volume	Dilution	Sample amount	Area	Ident	Date	Used
Standard 1	1	0.000	10.0	1.0	1.0	n. d.	STD1	2025-08-06 10:18:54 UTC-4	used
Standard 2	1	0.600	10.0	1.0	1.0	0.057	STD2	2025-08-06 10:40:18 UTC-4	used
Standard 3	1	1.200	10.0	1.0	1.0	0.113	STD3	2025-08-06 11:01:42 UTC-4	used
Standard 4	1	1.500	10.0	1.0	1.0	0.146	STD4	2025-08-06 11:23:08 UTC-4	used
Standard 5	1	3.000	10.0	1.0	1.0	0.289	STD5	2025-08-06 11:44:33 UTC-4	used
Standard 6	1	6.000	10.0	1.0	1.0	0.578	STD6	2025-08-06 12:06:00 UTC-4	used
Standard 7	1	7.500	10.0	1.0	1.0	0.737	STD7	2025-08-06 12:27:27 UTC-4	used

Nitrite (Anions)

(μS/cm) x min

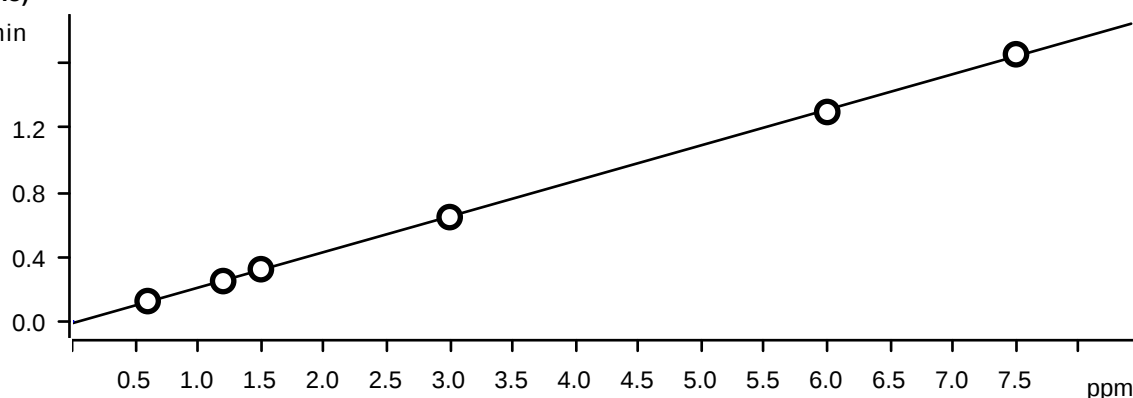Function: $A = -0.0116303 + 0.0220561 \times Q$


Relative standard deviation 1.449488 %

Correlation coefficient 0.999889

Sample type	Index	Conc.	Volume	Dilution	Sample amount	Area	Ident	Date	Used
Standard 1	1	0.000	10.0	1.0	1.0	n. d.	STD1	2025-08-06 10:18:54 UTC-4	used
Standard 2	1	0.600	10.0	1.0	1.0	0.126	STD2	2025-08-06 10:40:18 UTC-4	used
Standard 3	1	1.200	10.0	1.0	1.0	0.250	STD3	2025-08-06 11:01:42 UTC-4	used
Standard 4	1	1.500	10.0	1.0	1.0	0.323	STD4	2025-08-06 11:23:08 UTC-4	used
Standard 5	1	3.000	10.0	1.0	1.0	0.646	STD5	2025-08-06 11:44:33 UTC-4	used
Standard 6	1	6.000	10.0	1.0	1.0	1.297	STD6	2025-08-06 12:06:00 UTC-4	used
Standard 7	1	7.500	10.0	1.0	1.0	1.655	STD7	2025-08-06 12:27:27 UTC-4	used

Bromide (Anions)

($\mu\text{S}/\text{cm}$) $\times$ min

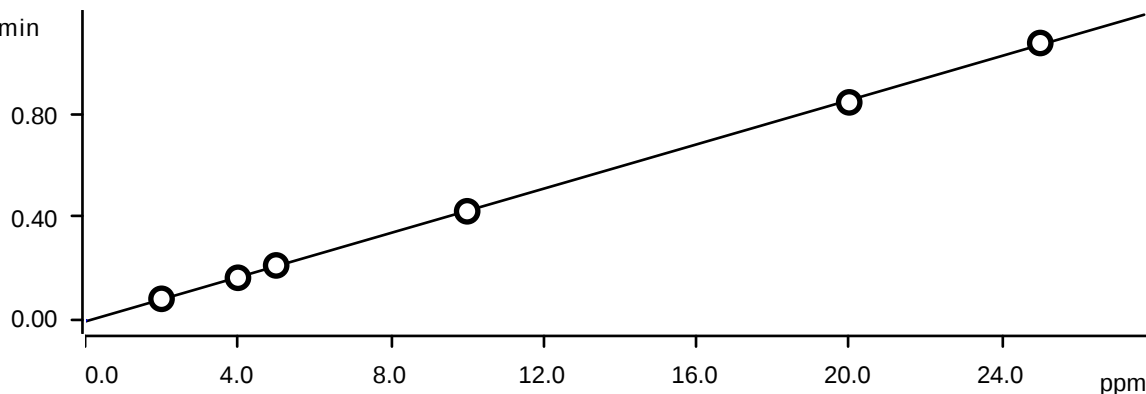

Function: $A = -4.59233\text{E-}3 + 4.28617\text{E-}3 \times Q$


Relative standard deviation 1.283698 %

Correlation coefficient 0.999912

Sample type	Index	Conc.	Volume	Dilution	Sample amount	Area	Ident	Date	Used
Standard 1	1	0.000	10.0	1.0	1.0	n. d.	STD1	2025-08-06 10:18:54 UTC-4	used
Standard 2	1	2.000	10.0	1.0	1.0	0.083	STD2	2025-08-06 10:40:18 UTC-4	used
Standard 3	1	4.000	10.0	1.0	1.0	0.165	STD3	2025-08-06 11:01:42 UTC-4	used
Standard 4	1	5.000	10.0	1.0	1.0	0.213	STD4	2025-08-06 11:23:08 UTC-4	used
Standard 5	1	10.000	10.0	1.0	1.0	0.422	STD5	2025-08-06 11:44:33 UTC-4	used
Standard 6	1	20.000	10.0	1.0	1.0	0.844	STD6	2025-08-06 12:06:00 UTC-4	used
Standard 7	1	25.000	10.0	1.0	1.0	1.074	STD7	2025-08-06 12:27:27 UTC-4	used

Nitrate (Anions)

($\mu\text{S}/\text{cm}$) $\times$ min

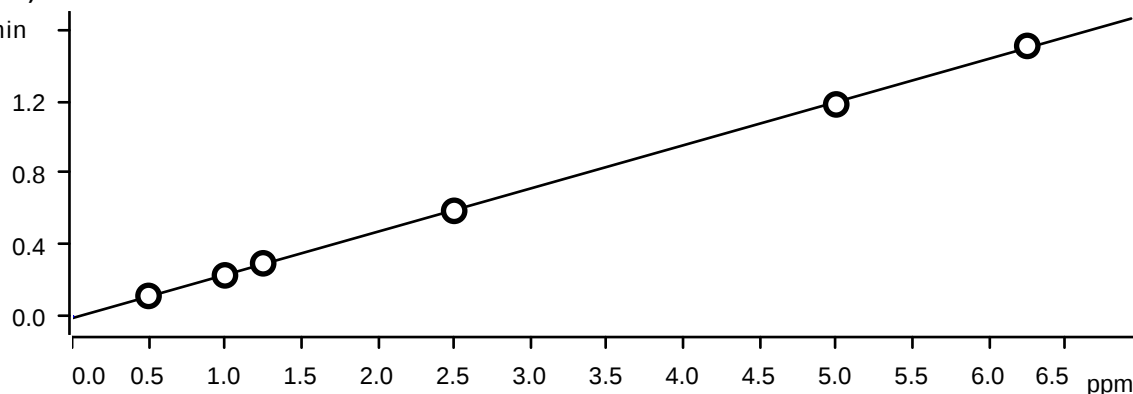

Function: $A = -9.68516\text{E-}3 + 0.0241085 \times Q$


Relative standard deviation 1.469135 %

Correlation coefficient 0.999886

Sample type	Index	Conc.	Volume	Dilution	Sample amount	Area	Ident	Date	Used
Standard 1	1	0.000	10.0	1.0	1.0	n. d.	STD1	2025-08-06 10:18:54 UTC-4	used
Standard 2	1	0.500	10.0	1.0	1.0	0.115	STD2	2025-08-06 10:40:18 UTC-4	used
Standard 3	1	1.000	10.0	1.0	1.0	0.229	STD3	2025-08-06 11:01:42 UTC-4	used
Standard 4	1	1.250	10.0	1.0	1.0	0.296	STD4	2025-08-06 11:23:08 UTC-4	used
Standard 5	1	2.500	10.0	1.0	1.0	0.589	STD5	2025-08-06 11:44:33 UTC-4	used
Standard 6	1	5.000	10.0	1.0	1.0	1.182	STD6	2025-08-06 12:06:00 UTC-4	used
Standard 7	1	6.250	10.0	1.0	1.0	1.509	STD7	2025-08-06 12:27:27 UTC-4	used

Phosphate (Anions)

(μS/cm) x min

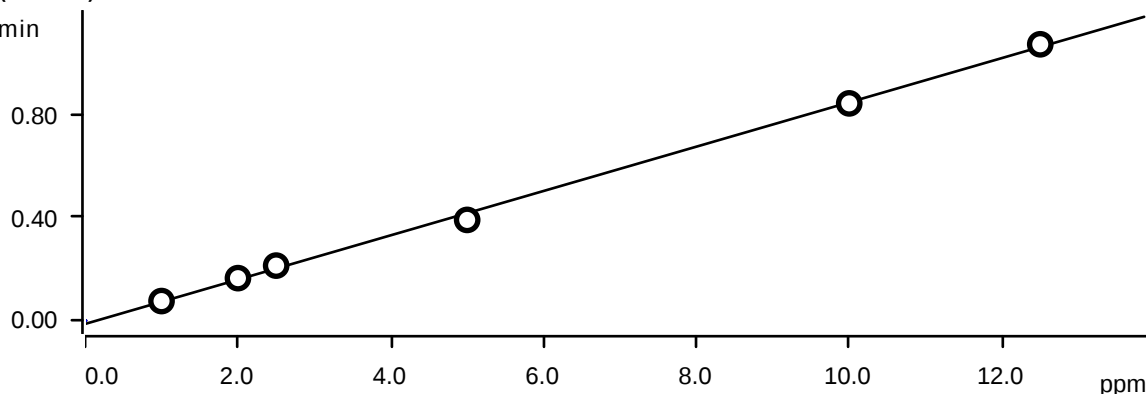
Function: $A = -0.0128563 + 8.58091E-3 \times Q$

Relative standard deviation 3.406332 %

Correlation coefficient 0.999402

Sample type	Index	Conc.	Volume	Dilution	Sample amount	Area	Ident	Date	Used
Standard 1	1	0.000	10.0	1.0	1.0	n. d.	STD1	2025-08-06 10:18:54 UTC-4	used
Standard 2	1	1.000	10.0	1.0	1.0	0.076	STD2	2025-08-06 10:40:18 UTC-4	used
Standard 3	1	2.000	10.0	1.0	1.0	0.164	STD3	2025-08-06 11:01:42 UTC-4	used
Standard 4	1	2.500	10.0	1.0	1.0	0.213	STD4	2025-08-06 11:23:08 UTC-4	used
Standard 5	1	5.000	10.0	1.0	1.0	0.390	STD5	2025-08-06 11:44:33 UTC-4	used
Standard 6	1	10.000	10.0	1.0	1.0	0.841	STD6	2025-08-06 12:06:00 UTC-4	used
Standard 7	1	12.500	10.0	1.0	1.0	1.070	STD7	2025-08-06 12:27:27 UTC-4	used

Sulfate (Anions)

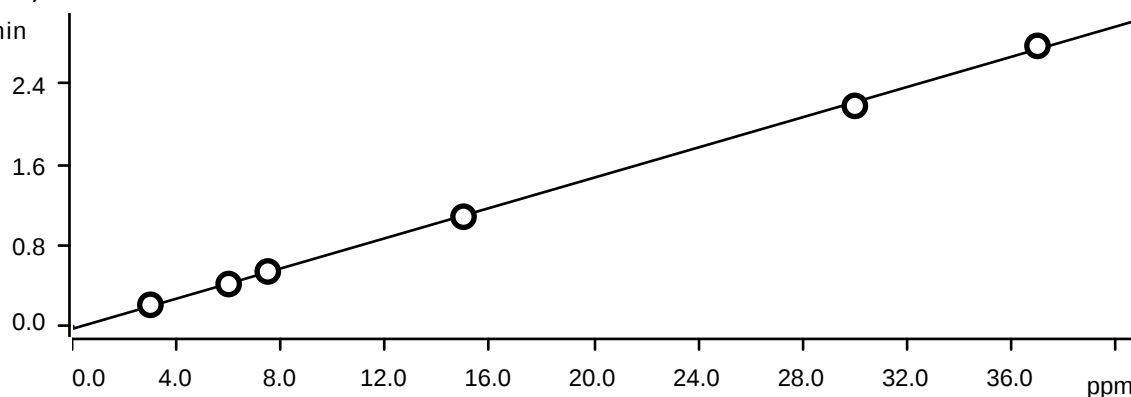 $(\mu\text{S}/\text{cm}) \times \text{min}$ Function: $A = -0.0267558 + 7.49232E-3 \times Q$

Relative standard deviation 2.236460 %

Correlation coefficient 0.999736


Sample type	Index	Conc.	Volume	Dilution	Sample amount	Area	Ident	Date	Used
Standard 1	1	0.000	10.0	1.0	1.0	n. d.	STD1	2025-08-06 10:18:54 UTC-4	used
Standard 2	1	3.000	10.0	1.0	1.0	0.212	STD2	2025-08-06 10:40:18 UTC-4	used
Standard 3	1	6.000	10.0	1.0	1.0	0.418	STD3	2025-08-06 11:01:42 UTC-4	used
Standard 4	1	7.500	10.0	1.0	1.0	0.542	STD4	2025-08-06 11:23:08 UTC-4	used
Standard 5	1	15.000	10.0	1.0	1.0	1.085	STD5	2025-08-06 11:44:33 UTC-4	used
Standard 6	1	30.000	10.0	1.0	1.0	2.184	STD6	2025-08-06 12:06:00 UTC-4	used
Standard 7	1	37.000	10.0	1.0	1.0	2.779	STD7	2025-08-06 12:27:27 UTC-4	used

Sample data

Ident STD1
Sample type Standard 1
Determination start 2025-08-06 10:18:54 UTC-4
Method IC1-080625
Operator

Anions

Data source Conductivity detector 1 (Eco IC 1)
Channel Conductivity
Recording time 19.0 min
Integration Automatically
Column type Metrosep A Supp 19 - 150/4.0
Eluent composition not defined
Flow 0.700 mL/min
Maximum flow monitored yes
Pressure 12.73 MPa
Maximum pressure monitored yes
Temperature ---- °C

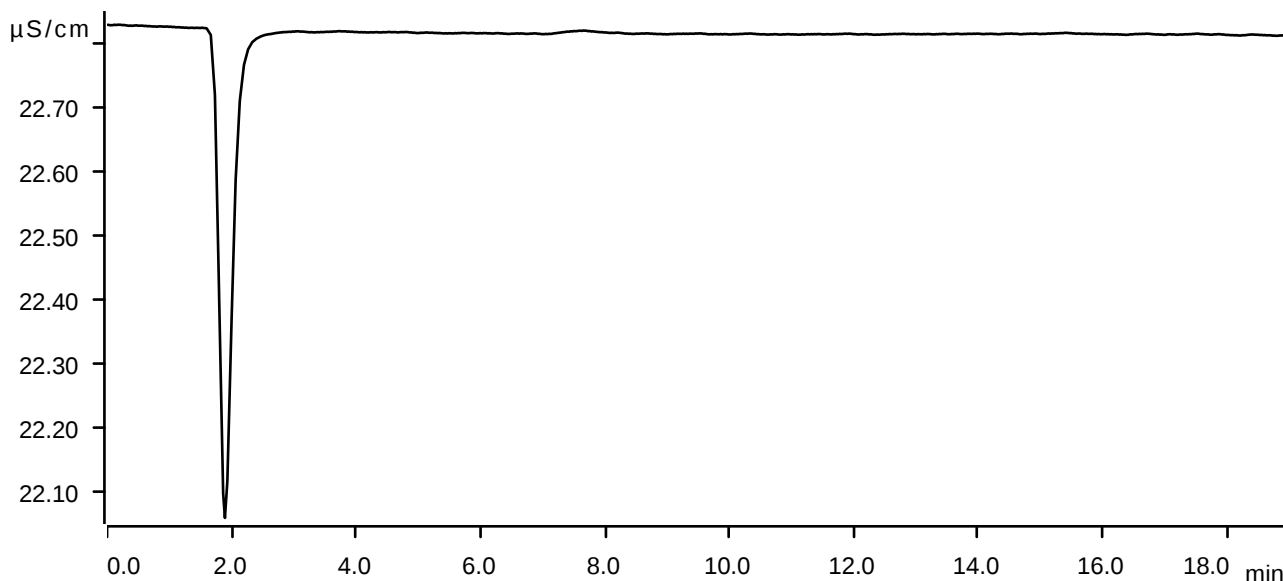Anions


Sample data

Ident STD2
Sample type Standard 2
Determination start 2025-08-06 10:40:18 UTC-4
Method IC1-080625
Operator

Anions

Data source Conductivity detector 1 (Eco IC 1)
Channel Conductivity
Recording time 19.0 min
Integration Automatically
Column type Metrosep A Supp 19 - 150/4.0
Eluent composition not defined
Flow 0.700 mL/min
Maximum flow monitored yes
Pressure 12.61 MPa
Maximum pressure monitored yes
Temperature ---- °C

Anions

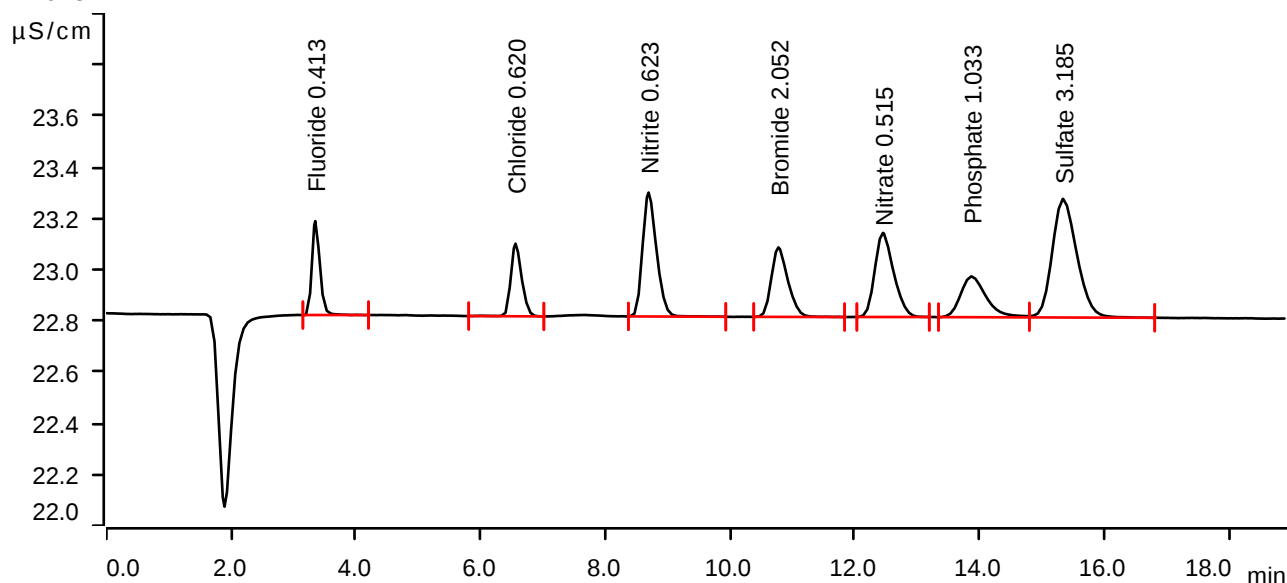

Peak number	Retention time min	Area (µS/cm) x min	Height µS/cm	Concentration ppm	Component name
1	3.350	0.0544	0.367	0.413	Fluoride
2	6.560	0.0573	0.284	0.620	Chloride
3	8.693	0.1258	0.484	0.623	Nitrite
4	10.775	0.0833	0.271	2.052	Bromide
5	12.452	0.1145	0.328	0.515	Nitrate
6	13.870	0.0758	0.159	1.033	Phosphate
7	15.340	0.2119	0.463	3.185	Sulfate


Sample data

Ident STD3
Sample type Standard 3
Determination start 2025-08-06 11:01:42 UTC-4
Method IC1-080625
Operator

Anions

Data source Conductivity detector 1 (Eco IC 1)
Channel Conductivity
Recording time 19.0 min
Integration Automatically
Column type Metrosep A Supp 19 - 150/4.0
Eluent composition not defined
Flow 0.700 mL/min
Maximum flow monitored yes
Pressure 12.61 MPa
Maximum pressure monitored yes
Temperature ---- °C

Anions

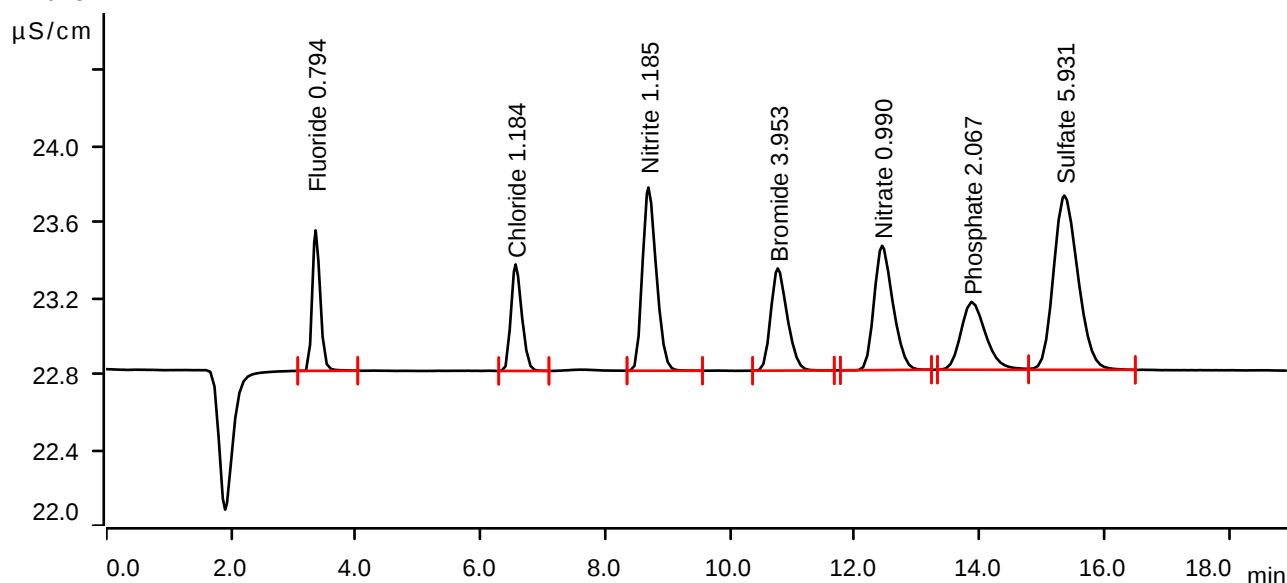

Peak number	Retention time min	Area (µS/cm) x min	Height µS/cm	Concentration ppm	Component name
1	3.357	0.1095	0.740	0.794	Fluoride
2	6.562	0.1125	0.561	1.184	Chloride
3	8.692	0.2498	0.966	1.185	Nitrite
4	10.765	0.1649	0.539	3.953	Bromide
5	12.438	0.2291	0.655	0.990	Nitrate
6	13.875	0.1645	0.358	2.067	Phosphate
7	15.360	0.4176	0.918	5.931	Sulfate


Sample data

Ident STD4
Sample type Standard 4
Determination start 2025-08-06 11:23:08 UTC-4
Method IC1-080625
Operator

Anions

Data source Conductivity detector 1 (Eco IC 1)
Channel Conductivity
Recording time 19.0 min
Integration Automatically
Column type Metrosep A Supp 19 - 150/4.0
Eluent composition not defined
Flow 0.700 mL/min
Maximum flow monitored yes
Pressure 12.44 MPa
Maximum pressure monitored yes
Temperature ---- °C

Anions

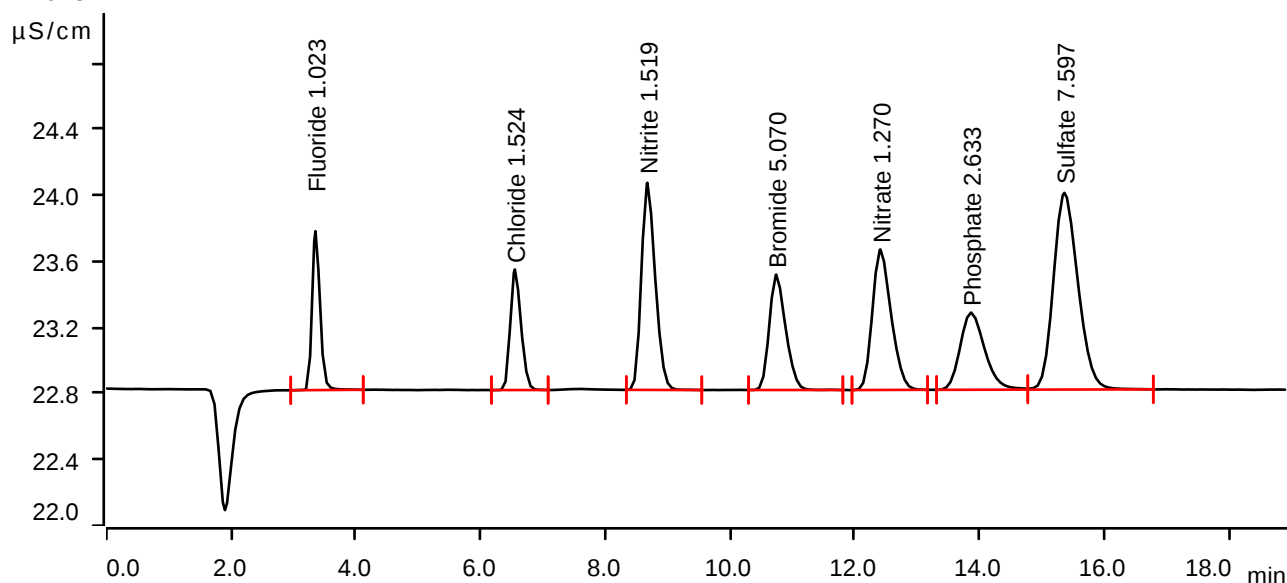

Peak number	Retention time min	Area (µS/cm) x min	Height µS/cm	Concentration ppm	Component name
1	3.353	0.1425	0.962	1.023	Fluoride
2	6.552	0.1459	0.730	1.524	Chloride
3	8.675	0.3233	1.254	1.519	Nitrite
4	10.740	0.2127	0.698	5.070	Bromide
5	12.410	0.2964	0.850	1.270	Nitrate
6	13.862	0.2131	0.467	2.633	Phosphate
7	15.360	0.5424	1.191	7.597	Sulfate


Sample data

Ident STD5
 Sample type Standard 5
 Determination start 2025-08-06 11:44:33 UTC-4
 Method IC1-080625
 Operator

Anions

Data source Conductivity detector 1 (Eco IC 1)
 Channel Conductivity
 Recording time 19.0 min
 Integration Automatically
 Column type Metrosep A Supp 19 - 150/4.0
 Eluent composition not defined
 Flow 0.700 mL/min
 Maximum flow monitored yes
 Pressure 12.44 MPa
 Maximum pressure monitored yes
 Temperature ---- °C

Anions

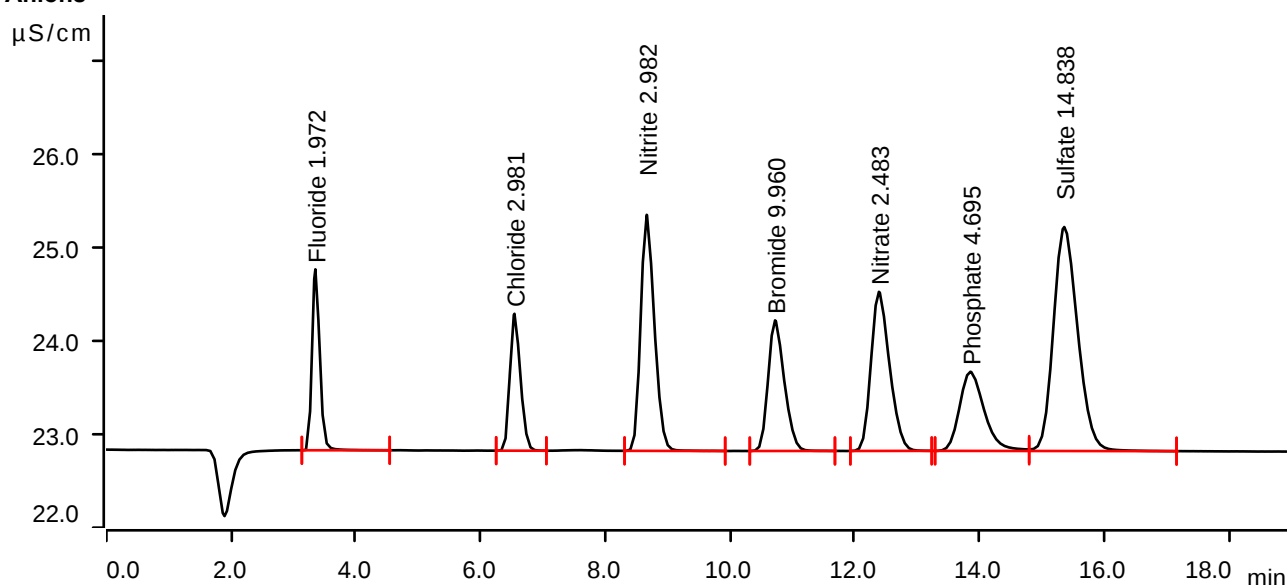

Peak number	Retention time min	Area (µS/cm) x min	Height µS/cm	Concentration ppm	Component name
1	3.352	0.2796	1.943	1.972	Fluoride
2	6.543	0.2887	1.470	2.981	Chloride
3	8.663	0.6461	2.534	2.982	Nitrite
4	10.722	0.4223	1.403	9.960	Bromide
5	12.387	0.5889	1.709	2.483	Nitrate
6	13.853	0.3900	0.850	4.695	Phosphate
7	15.358	1.0850	2.405	14.838	Sulfate


Sample data

Ident STD6
Sample type Standard 6
Determination start 2025-08-06 12:06:00 UTC-4
Method IC1-080625
Operator

Anions

Data source Conductivity detector 1 (Eco IC 1)
Channel Conductivity
Recording time 19.0 min
Integration Automatically
Column type Metrosep A Supp 19 - 150/4.0
Eluent composition not defined
Flow 0.700 mL/min
Maximum flow monitored yes
Pressure 12.39 MPa
Maximum pressure monitored yes
Temperature ---- °C

Anions

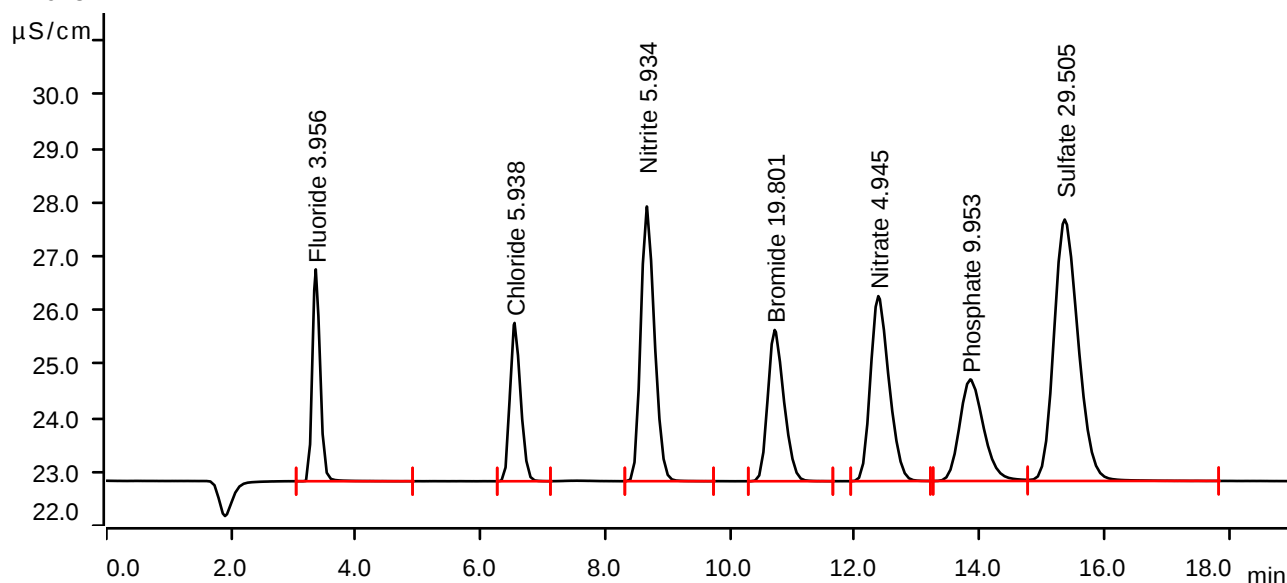

Peak number	Retention time min	Area (µS/cm) x min	Height µS/cm	Concentration ppm	Component name
1	3.358	0.5660	3.928	3.956	Fluoride
2	6.545	0.5784	2.936	5.938	Chloride
3	8.665	1.2973	5.095	5.934	Nitrite
4	10.715	0.8441	2.805	19.801	Bromide
5	12.377	1.1824	3.431	4.945	Nitrate
6	13.852	0.8412	1.884	9.953	Phosphate
7	15.365	2.1839	4.849	29.505	Sulfate


Sample data

Ident STD7
Sample type Standard 7
Determination start 2025-08-06 12:27:27 UTC-4
Method IC1-080625
Operator

Anions

Data source Conductivity detector 1 (Eco IC 1)
Channel Conductivity
Recording time 19.0 min
Integration Automatically
Column type Metrosep A Supp 19 - 150/4.0
Eluent composition not defined
Flow 0.700 mL/min
Maximum flow monitored yes
Pressure 12.39 MPa
Maximum pressure monitored yes
Temperature ---- °C

Anions

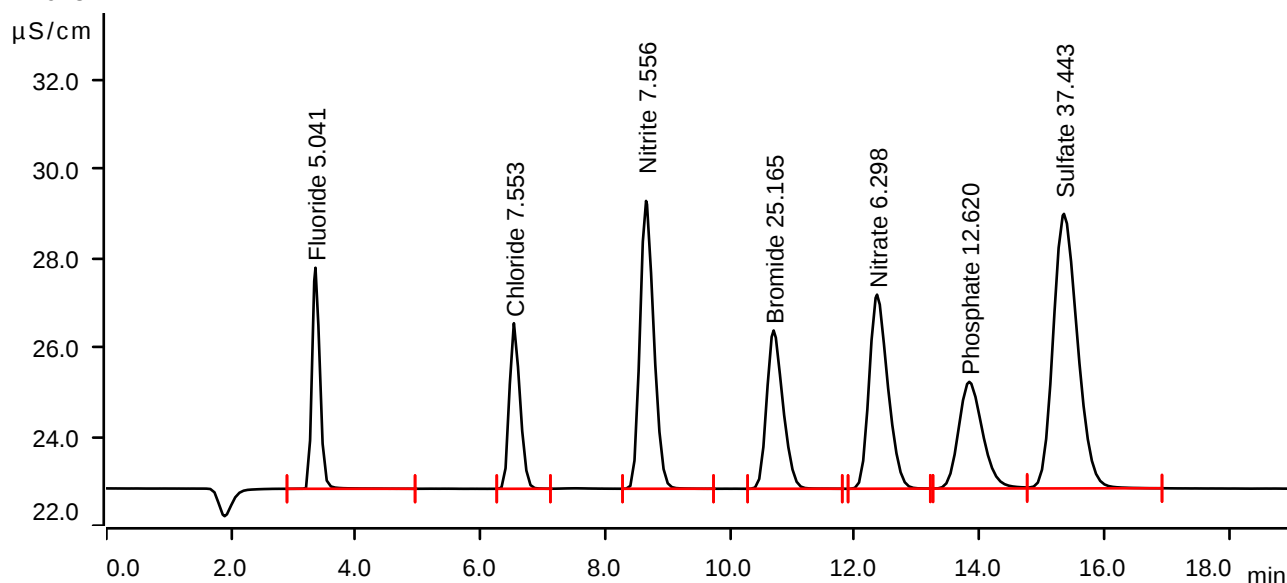

Peak number	Retention time min	Area (µS/cm) x min	Height µS/cm	Concentration ppm	Component name
1	3.353	0.7226	4.963	5.041	Fluoride
2	6.535	0.7366	3.716	7.553	Chloride
3	8.653	1.6550	6.462	7.556	Nitrite
4	10.698	1.0740	3.554	25.165	Bromide
5	12.357	1.5086	4.357	6.298	Nitrate
6	13.835	1.0700	2.396	12.620	Phosphate
7	15.353	2.7786	6.163	37.443	Sulfate


Sample data

Ident ICV
Sample type Check standard 1
Determination start 2025-08-06 12:48:56 UTC-4
Method IC1-080625
Operator

Anions

Data source Conductivity detector 1 (Eco IC 1)
Channel Conductivity
Recording time 19.0 min
Integration Automatically
Column type Metrosep A Supp 19 - 150/4.0
Eluent composition not defined
Flow 0.700 mL/min
Maximum flow monitored yes
Pressure 12.44 MPa
Maximum pressure monitored yes
Temperature ---- °C

Anions

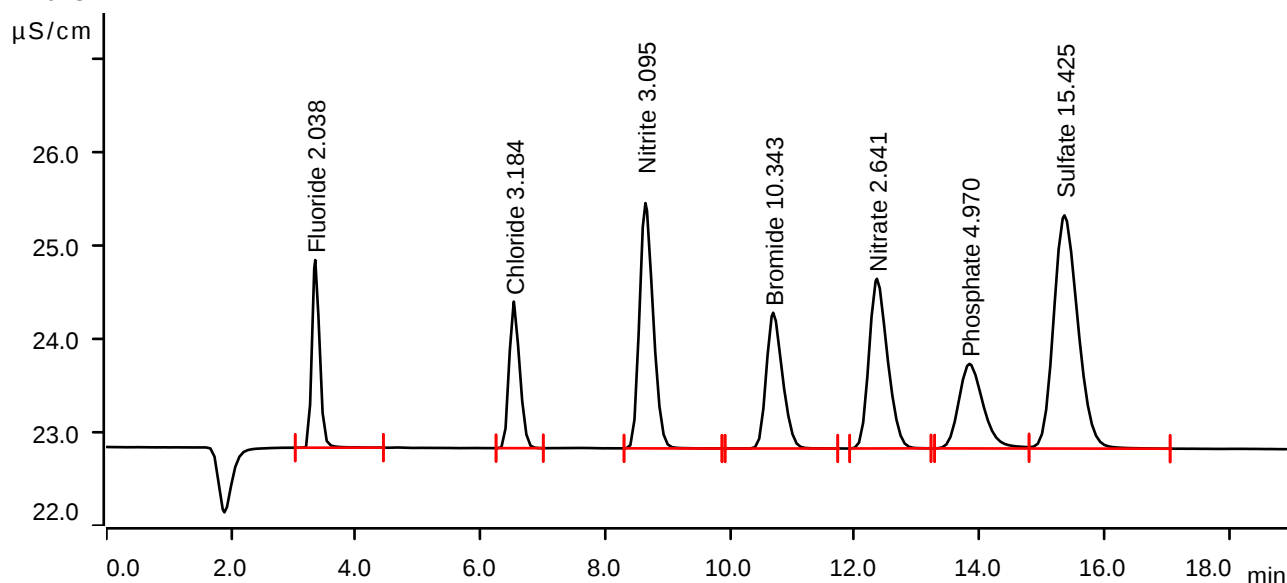

Peak number	Retention time min	Area (µS/cm) x min	Height µS/cm	Concentration ppm	Component name
1	3.350	0.2890	2.015	2.038	Fluoride
2	6.532	0.3085	1.574	3.184	Chloride
3	8.643	0.6711	2.634	3.095	Nitrite
4	10.692	0.4387	1.458	10.343	Bromide
5	12.355	0.6270	1.822	2.641	Nitrate
6	13.838	0.4136	0.908	4.970	Phosphate
7	15.362	1.1289	2.504	15.425	Sulfate


Sample data

Ident ICB
Sample type Sample
Determination start 2025-08-06 13:10:25 UTC-4
Method IC1-080625
Operator

Anions

Data source Conductivity detector 1 (Eco IC 1)
Channel Conductivity
Recording time 19.0 min
Integration Automatically
Column type Metrosep A Supp 19 - 150/4.0
Eluent composition not defined
Flow 0.700 mL/min
Maximum flow monitored yes
Pressure 12.33 MPa
Maximum pressure monitored yes
Temperature ---- °C

Anions

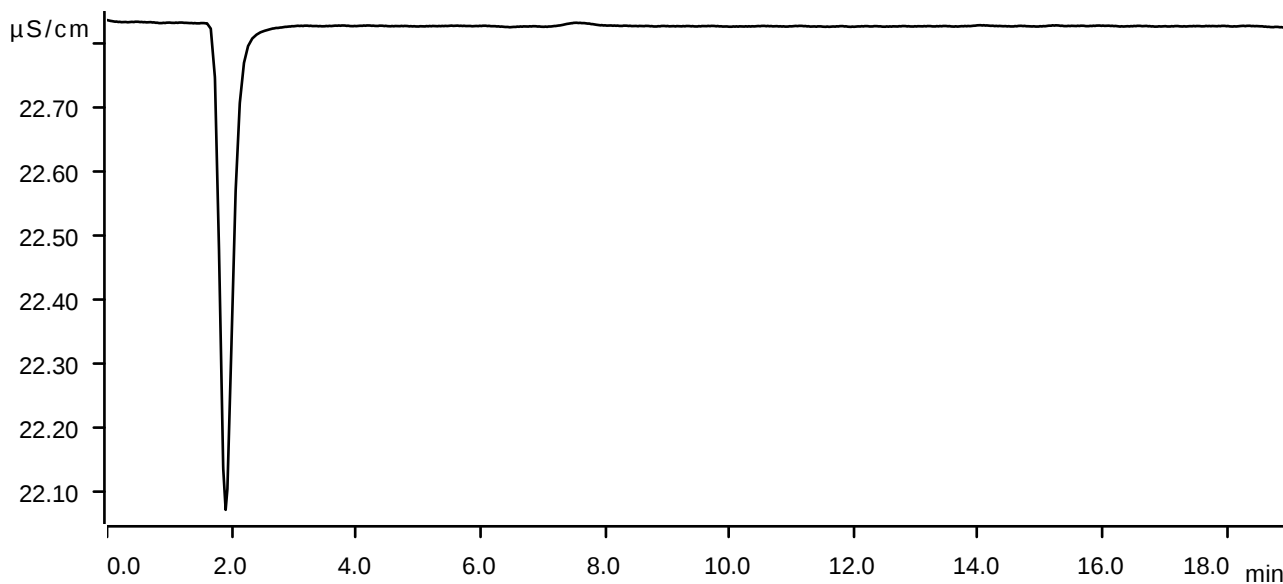


Sample data

Ident CCV
Sample type Check standard 1
Determination start 2025-08-13 09:19:09 UTC-4
Method IC1-080625
Operator

Anions

Data source Conductivity detector 1 (Eco IC 1)
Channel Conductivity
Recording time 19.0 min
Integration Automatically
Column type Metrosep A Supp 19 - 150/4.0
Eluent composition not defined
Flow 0.700 mL/min
Maximum flow monitored yes
Pressure 12.16 MPa
Maximum pressure monitored yes
Temperature ---- °C

Anions

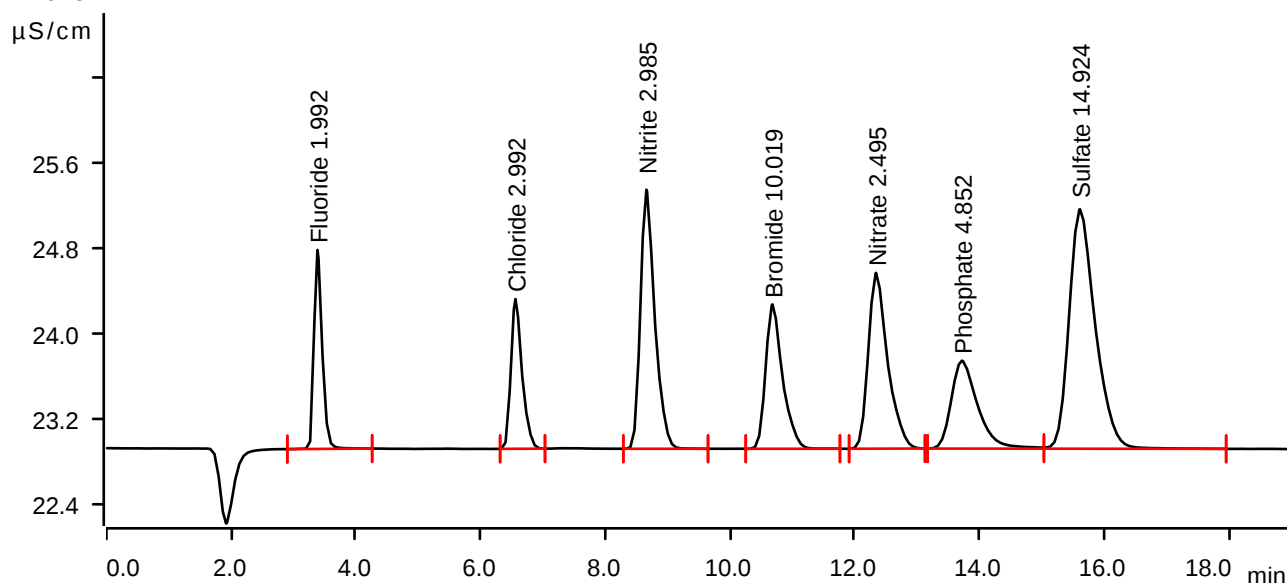

Peak number	Retention time min	Area (µS/cm) x min	Height µS/cm	Concentration ppm	Component name
1	3.385	0.2824	1.864	1.992	Fluoride
2	6.560	0.2897	1.403	2.992	Chloride
3	8.658	0.6468	2.428	2.985	Nitrite
4	10.680	0.4249	1.353	10.019	Bromide
5	12.342	0.5918	1.647	2.495	Nitrate
6	13.717	0.4035	0.824	4.852	Phosphate
7	15.610	1.0914	2.244	14.924	Sulfate


Sample data

Ident CCB
Sample type Sample
Determination start 2025-08-13 09:40:39 UTC-4
Method IC1-080625
Operator

Anions

Data source Conductivity detector 1 (Eco IC 1)
Channel Conductivity
Recording time 19.0 min
Integration Automatically
Column type Metrosep A Supp 19 - 150/4.0
Eluent composition not defined
Flow 0.700 mL/min
Maximum flow monitored yes
Pressure 11.88 MPa
Maximum pressure monitored yes
Temperature ---- °C

Anions

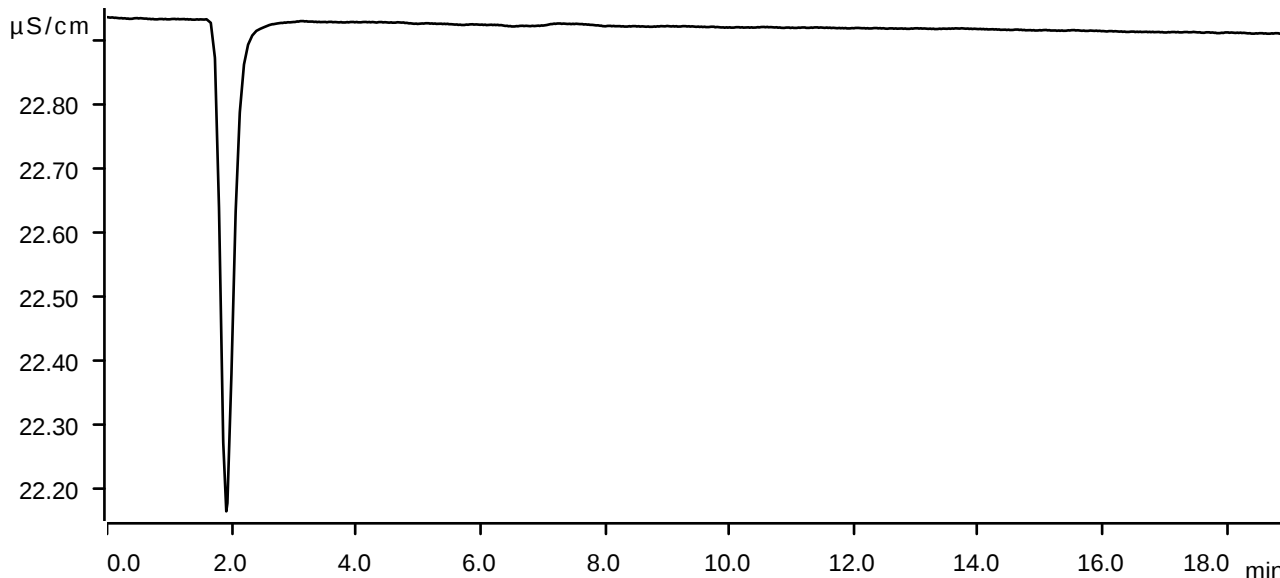


Sample data

Ident LB136803BLW
Sample type Sample
Determination start 2025-08-13 10:02:10 UTC-4
Method IC1-080625
Operator

Anions

Data source Conductivity detector 1 (Eco IC 1)
Channel Conductivity
Recording time 19.0 min
Integration Automatically
Column type Metrosep A Supp 19 - 150/4.0
Eluent composition not defined
Flow 0.700 mL/min
Maximum flow monitored yes
Pressure 11.77 MPa
Maximum pressure monitored yes
Temperature ---- °C

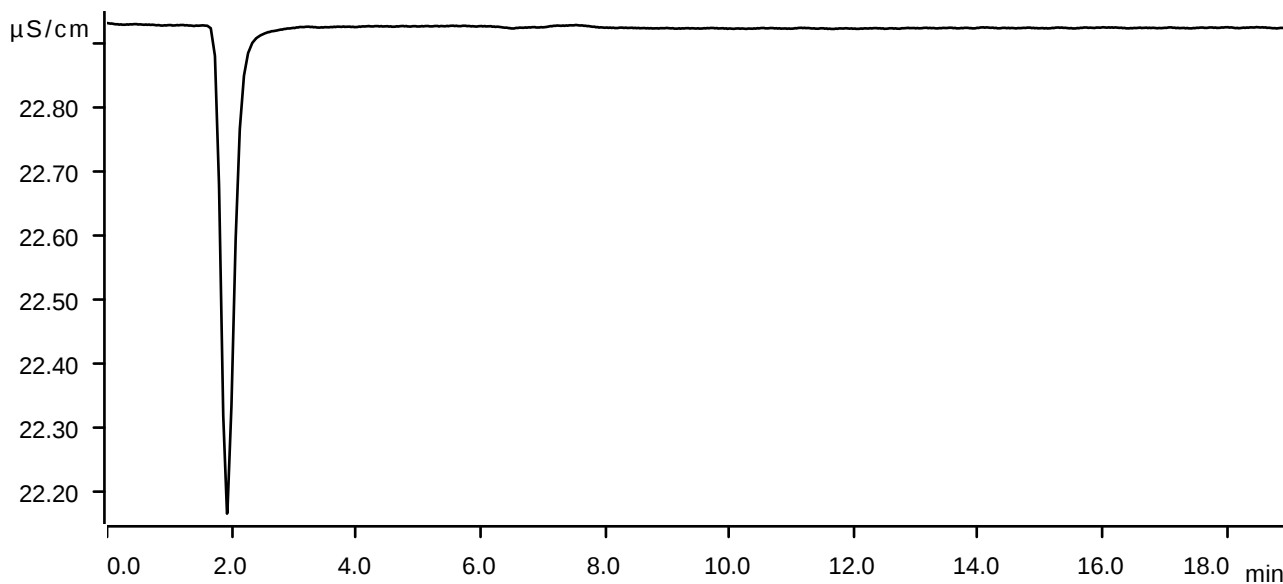Anions


Sample data

Ident LB136803BSW
Sample type Check standard 1
Determination start 2025-08-13 10:23:41 UTC-4
Method IC1-080625
Operator

Anions

Data source Conductivity detector 1 (Eco IC 1)
Channel Conductivity
Recording time 19.0 min
Integration Automatically
Column type Metrosep A Supp 19 - 150/4.0
Eluent composition not defined
Flow 0.700 mL/min
Maximum flow monitored yes
Pressure 11.71 MPa
Maximum pressure monitored yes
Temperature ---- °C

Anions

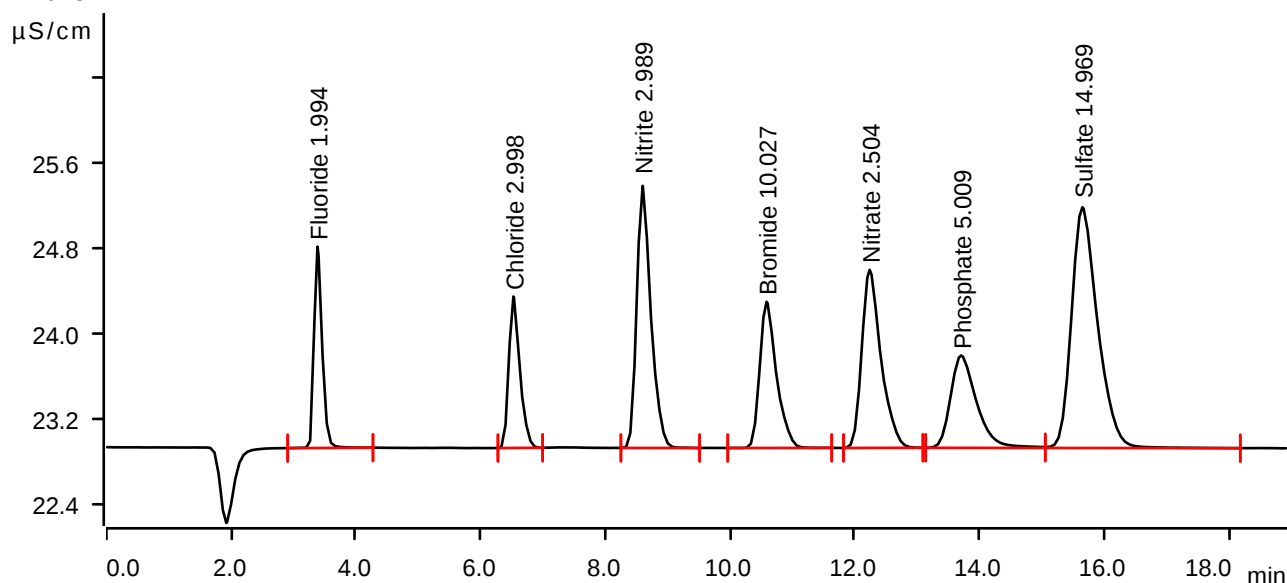

Peak number	Retention time min	Area (µS/cm) x min	Height µS/cm	Concentration ppm	Component name
1	3.385	0.2827	1.887	1.994	Fluoride
2	6.527	0.2903	1.419	2.998	Chloride
3	8.598	0.6477	2.457	2.989	Nitrite
4	10.585	0.4252	1.370	10.027	Bromide
5	12.238	0.5939	1.668	2.504	Nitrate
6	13.705	0.4170	0.865	5.009	Phosphate
7	15.648	1.0948	2.257	14.969	Sulfate


Sample data

Ident Q2842-01
Sample type Sample
Determination start 2025-08-13 13:42:41 UTC-4
Method IC1-080625
Operator

Anions

Data source Conductivity detector 1 (Eco IC 1)
Channel Conductivity
Recording time 19.0 min
Integration Automatically
Column type Metrosep A Supp 19 - 150/4.0
Eluent composition not defined
Flow 0.700 mL/min
Maximum flow monitored yes
Pressure 11.49 MPa
Maximum pressure monitored yes
Temperature ---- °C

Anions

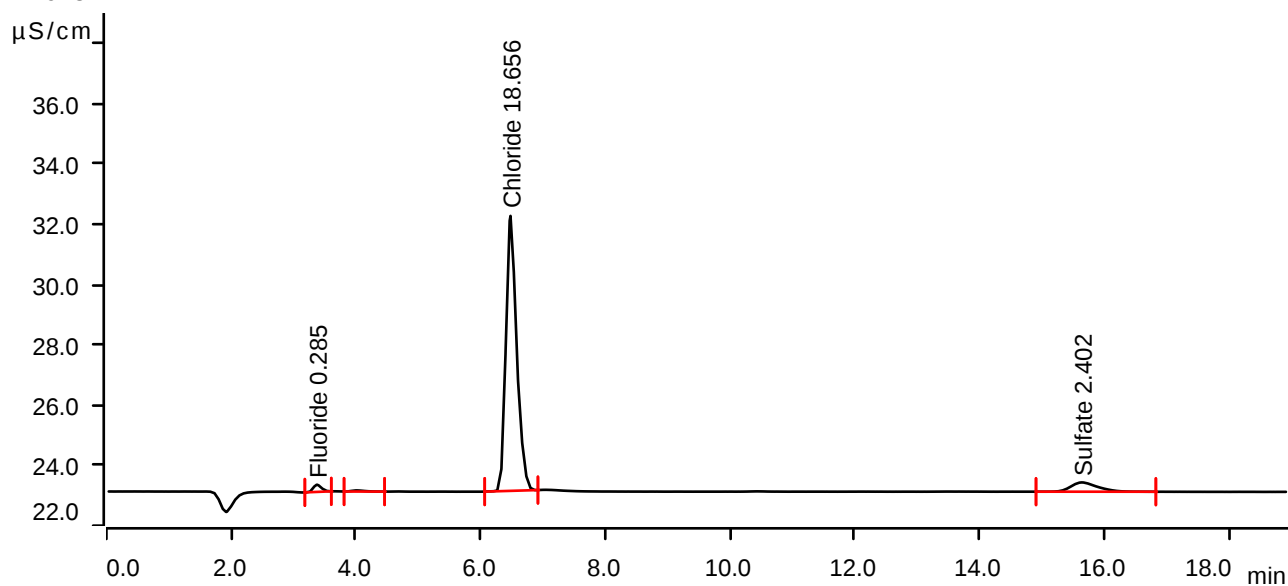

Peak number	Retention time min	Area (µS/cm) x min	Height µS/cm	Concentration ppm	Component name
1	3.375	0.0359	0.241	0.285	Fluoride
2	4.020	0.0087	0.037	invalid	
3	6.480	1.8244	9.126	18.656	Chloride
4	15.638	0.1532	0.309	2.402	Sulfate


Sample data

Ident Q2842-03
Sample type Sample
Determination start 2025-08-13 14:25:37 UTC-4
Method IC1-080625
Operator

Anions

Data source Conductivity detector 1 (Eco IC 1)
Channel Conductivity
Recording time 19.0 min
Integration Automatically
Column type Metrosep A Supp 19 - 150/4.0
Eluent composition not defined
Flow 0.700 mL/min
Maximum flow monitored yes
Pressure 11.43 MPa
Maximum pressure monitored yes
Temperature ---- °C

Anions

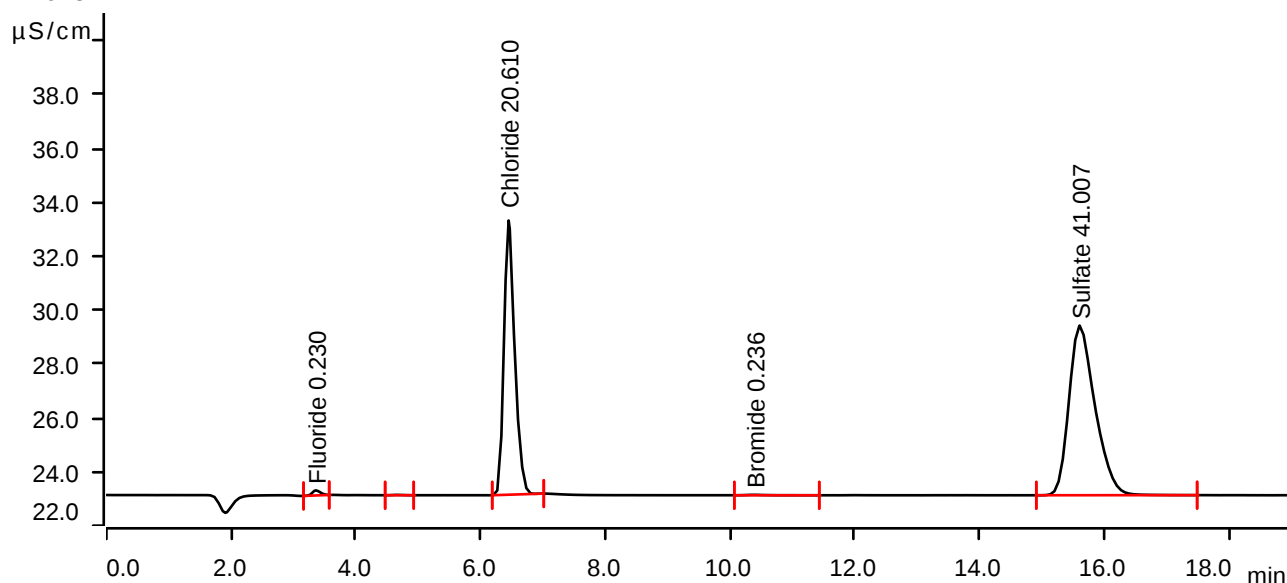

Peak number	Retention time min	Area (µS/cm) x min	Height µS/cm	Concentration ppm	Component name
1	3.360	0.0280	0.189	0.230	Fluoride
2	4.662	0.0024	0.013	invalid	
3	6.450	2.0158	10.171	20.610	Chloride
4	10.390	0.0055	0.016	0.236	Bromide
5	15.605	3.0456	6.293	41.007	Sulfate


Sample data

Ident Q2842-04MS
Sample type Sample
Determination start 2025-08-13 15:08:32 UTC-4
Method IC1-080625
Operator

Anions

Data source Conductivity detector 1 (Eco IC 1)
Channel Conductivity
Recording time 19.0 min
Integration Automatically
Column type Metrosep A Supp 19 - 150/4.0
Eluent composition not defined
Flow 0.700 mL/min
Maximum flow monitored yes
Pressure 11.54 MPa
Maximum pressure monitored yes
Temperature ---- °C

Anions

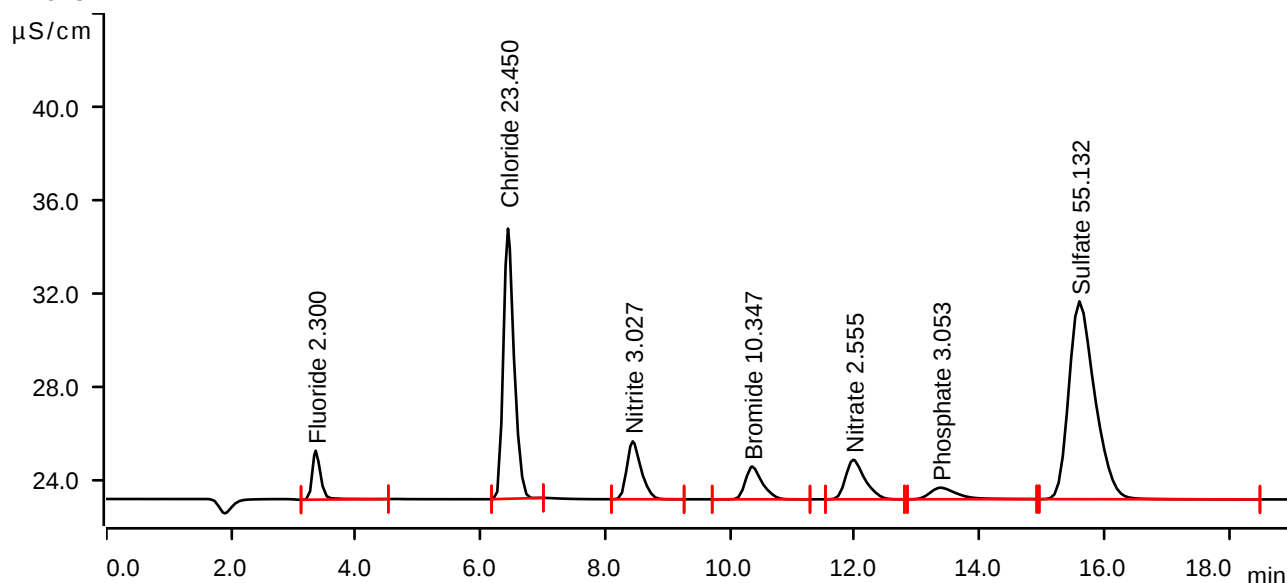

Peak number	Retention time min	Area (µS/cm) x min	Height µS/cm	Concentration ppm	Component name
1	3.357	0.3268	2.103	2.300	Fluoride
2	6.440	2.2941	11.606	23.450	Chloride
3	8.440	0.6561	2.486	3.027	Nitrite
4	10.355	0.4389	1.409	10.347	Bromide
5	11.977	0.6062	1.700	2.555	Nitrate
6	13.375	0.2491	0.496	3.053	Phosphate
7	15.602	4.1039	8.496	55.132	Sulfate


Sample data

Ident Q2842-05MSD
Sample type Sample
Determination start 2025-08-13 15:51:29 UTC-4
Method IC1-080625
Operator

Anions

Data source Conductivity detector 1 (Eco IC 1)
Channel Conductivity
Recording time 19.0 min
Integration Automatically
Column type Metrosep A Supp 19 - 150/4.0
Eluent composition not defined
Flow 0.700 mL/min
Maximum flow monitored yes
Pressure 11.37 MPa
Maximum pressure monitored yes
Temperature ---- °C

Anions

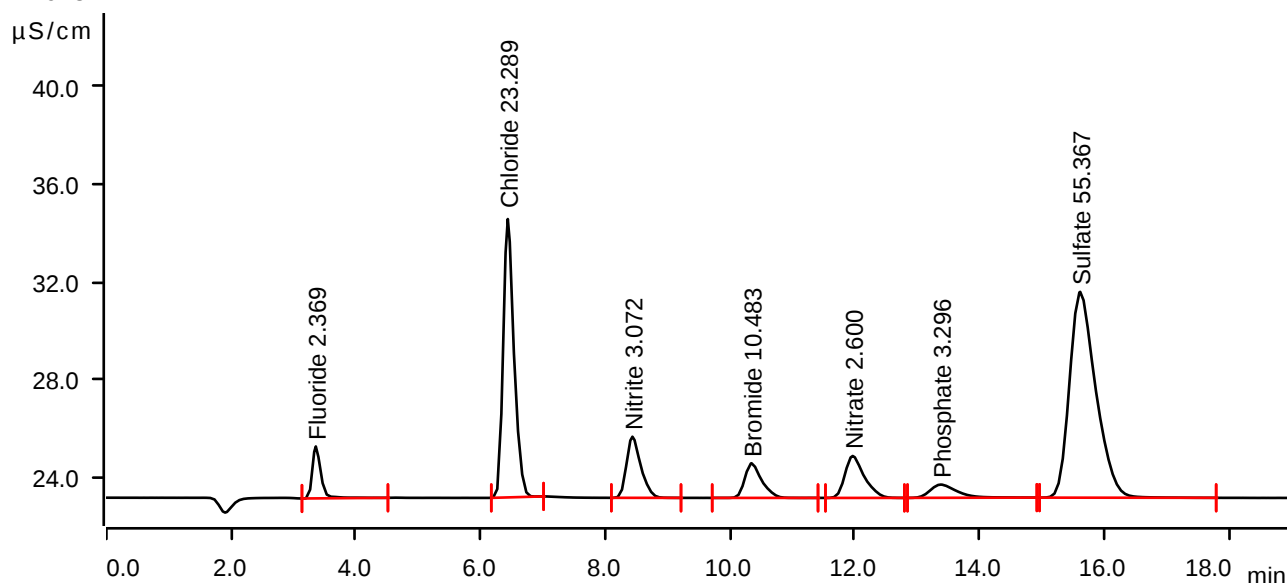

Peak number	Retention time min	Area (µS/cm) x min	Height µS/cm	Concentration ppm	Component name
1	3.358	0.3369	2.129	2.369	Fluoride
2	6.437	2.2783	11.412	23.289	Chloride
3	8.435	0.6659	2.506	3.072	Nitrite
4	10.345	0.4447	1.420	10.483	Bromide
5	11.967	0.6171	1.719	2.600	Nitrate
6	13.378	0.2700	0.543	3.296	Phosphate
7	15.613	4.1215	8.438	55.367	Sulfate


Sample data

Ident Q2842-01DLX5
Sample type Sample
Determination start 2025-08-13 16:13:04 UTC-4
Method IC1-080625
Operator

Anions

Data source Conductivity detector 1 (Eco IC 1)
Channel Conductivity
Recording time 19.0 min
Integration Automatically
Column type Metrosep A Supp 19 - 150/4.0
Eluent composition not defined
Flow 0.700 mL/min
Maximum flow monitored yes
Pressure 11.37 MPa
Maximum pressure monitored yes
Temperature ---- °C

Anions

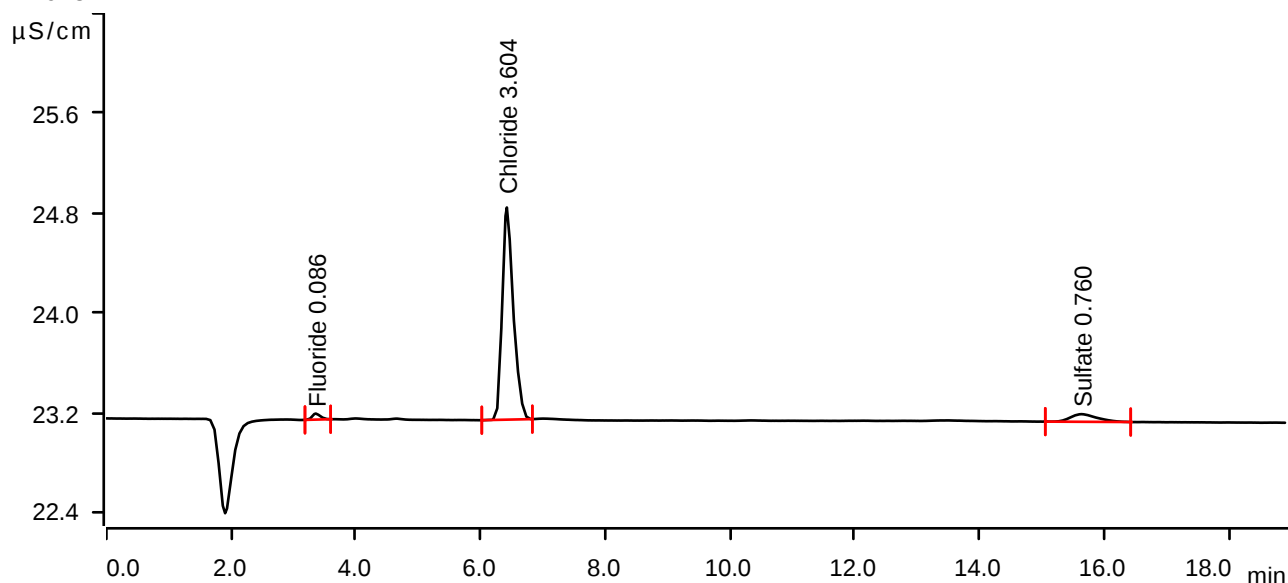

Peak number	Retention time min	Area (µS/cm) x min	Height µS/cm	Concentration ppm	Component name
1	3.358	0.0073	0.048	0.086	Fluoride
2	6.422	0.3497	1.698	3.604	Chloride
3	15.633	0.0302	0.061	0.760	Sulfate


Sample data

Ident Q2842-03DLX5
Sample type Sample
Determination start 2025-08-13 16:34:38 UTC-4
Method IC1-080625
Operator

Anions

Data source Conductivity detector 1 (Eco IC 1)
Channel Conductivity
Recording time 19.0 min
Integration Automatically
Column type Metrosep A Supp 19 - 150/4.0
Eluent composition not defined
Flow 0.700 mL/min
Maximum flow monitored yes
Pressure 11.43 MPa
Maximum pressure monitored yes
Temperature ---- °C

Anions

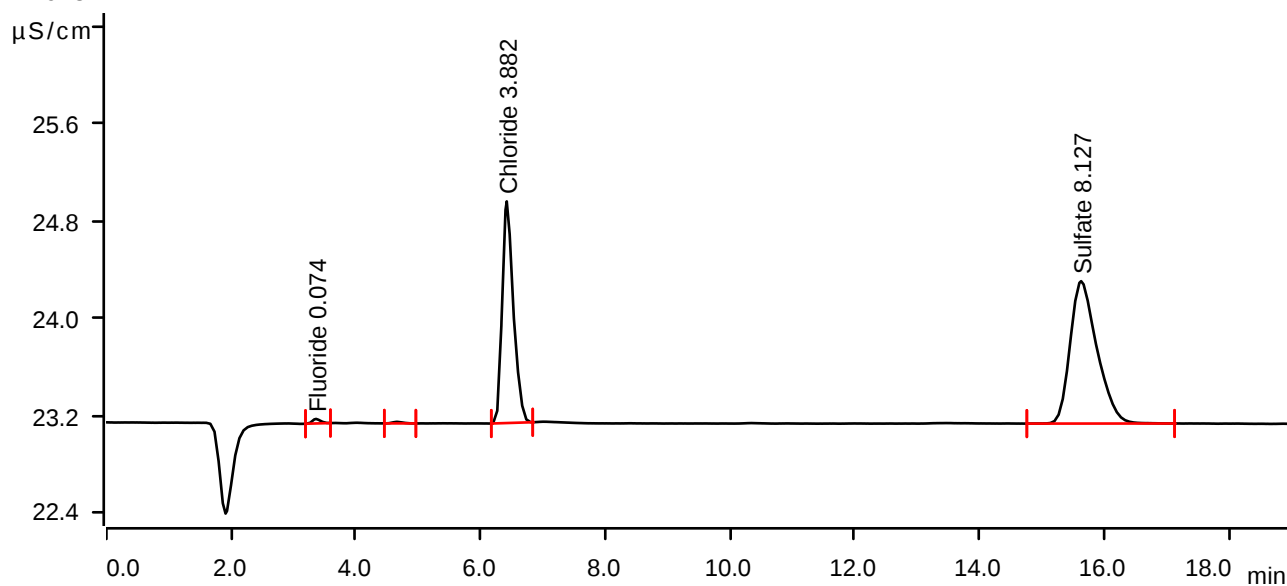

Peak number	Retention time min	Area (µS/cm) x min	Height µS/cm	Concentration ppm	Component name
1	3.363	0.0055	0.037	0.074	Fluoride
2	4.653	0.0024	0.013	invalid	
3	6.420	0.3769	1.818	3.882	Chloride
4	15.628	0.5822	1.167	8.127	Sulfate


Sample data

Ident CCV
Sample type Check standard 1
Determination start 2025-08-13 17:39:04 UTC-4
Method IC1-080625
Operator

Anions

Data source Conductivity detector 1 (Eco IC 1)
Channel Conductivity
Recording time 19.0 min
Integration Automatically
Column type Metrosep A Supp 19 - 150/4.0
Eluent composition not defined
Flow 0.700 mL/min
Maximum flow monitored yes
Pressure 11.49 MPa
Maximum pressure monitored yes
Temperature ---- °C

Anions

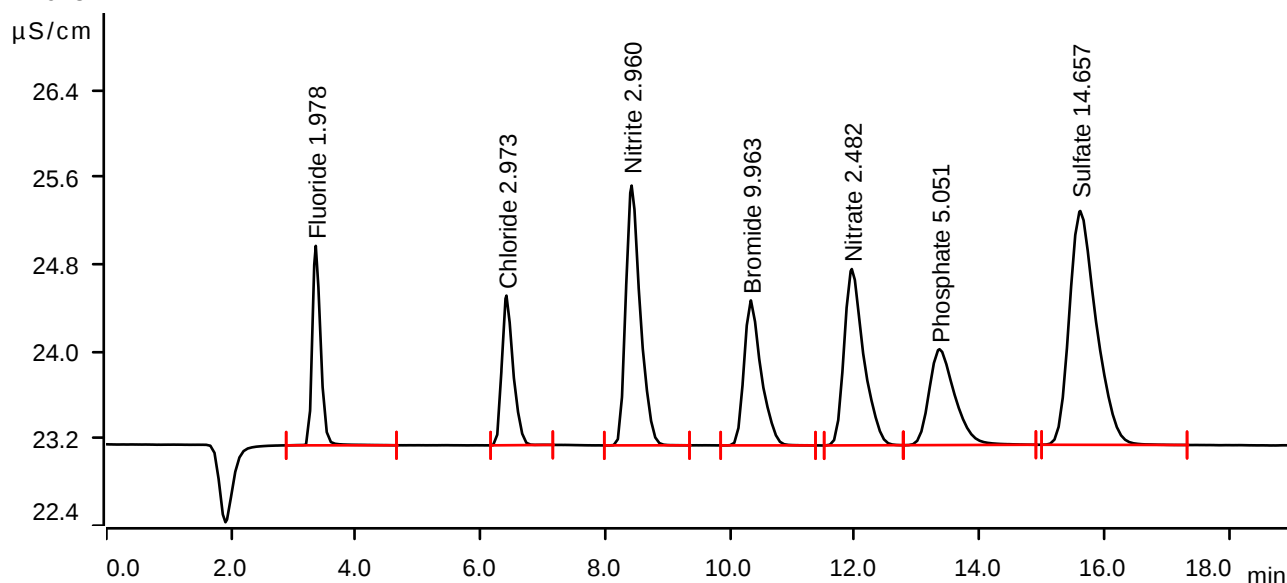

Peak number	Retention time min	Area (µS/cm) x min	Height µS/cm	Concentration ppm	Component name
1	3.358	0.2804	1.830	1.978	Fluoride
2	6.415	0.2878	1.373	2.973	Chloride
3	8.422	0.6413	2.384	2.960	Nitrite
4	10.332	0.4224	1.330	9.963	Bromide
5	11.952	0.5888	1.618	2.482	Nitrate
6	13.358	0.4206	0.880	5.051	Phosphate
7	15.615	1.0714	2.145	14.657	Sulfate

Sample data

Ident CCB
Sample type Sample
Determination start 2025-08-13 18:00:34 UTC-4
Method IC1-080625
Operator

Anions

Data source Conductivity detector 1 (Eco IC 1)
Channel Conductivity
Recording time 19.0 min
Integration Automatically
Column type Metrosep A Supp 19 - 150/4.0
Eluent composition not defined
Flow 0.700 mL/min
Maximum flow monitored yes
Pressure 11.43 MPa
Maximum pressure monitored yes
Temperature ---- °C

Anions