

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN081425\
 Data File : VN087554.D
 Acq On : 14 Aug 2025 10:32
 Operator : JC\MD
 Sample : VN0814WBL01
 Misc : 5.0mL/MSVOA_N/WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_N
 ClientSampleId :
 VN0814WBL01

Quant Time: Aug 14 15:23:32 2025
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N071625W.M
 Quant Title : SW846 8260
 QLast Update : Thu Jul 17 02:56:13 2025
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Pentafluorobenzene	8.206	168	284398	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	9.083	114	560321	50.000	ug/l	0.00
63) Chlorobenzene-d5	11.847	117	503771	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.771	152	234765	50.000	ug/l	0.00

System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	8.565	65	255137	52.871	ug/l	0.00
Spiked Amount	50.000	Range	74 - 125	Recovery	=	105.740%
35) Dibromofluoromethane	8.153	113	170840	44.201	ug/l	0.00
Spiked Amount	50.000	Range	75 - 124	Recovery	=	88.400%
50) Toluene-d8	10.547	98	608969	44.169	ug/l	0.00
Spiked Amount	50.000	Range	86 - 113	Recovery	=	88.340%
62) 4-Bromofluorobenzene	12.829	95	222642	43.709	ug/l	0.00
Spiked Amount	50.000	Range	77 - 121	Recovery	=	87.420%


Target Compounds	Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN081425\
Data File : VN087554.D
Acq On : 14 Aug 2025 10:32
Operator : JC\MD
Sample : VN0814WBL01
Misc : 5.0mL/MSVOA_N/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
VN0814WBL01

Quant Time: Aug 14 15:23:32 2025
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N071625W.M
Quant Title : SW846 8260
QLast Update : Thu Jul 17 02:56:13 2025
Response via : Initial Calibration




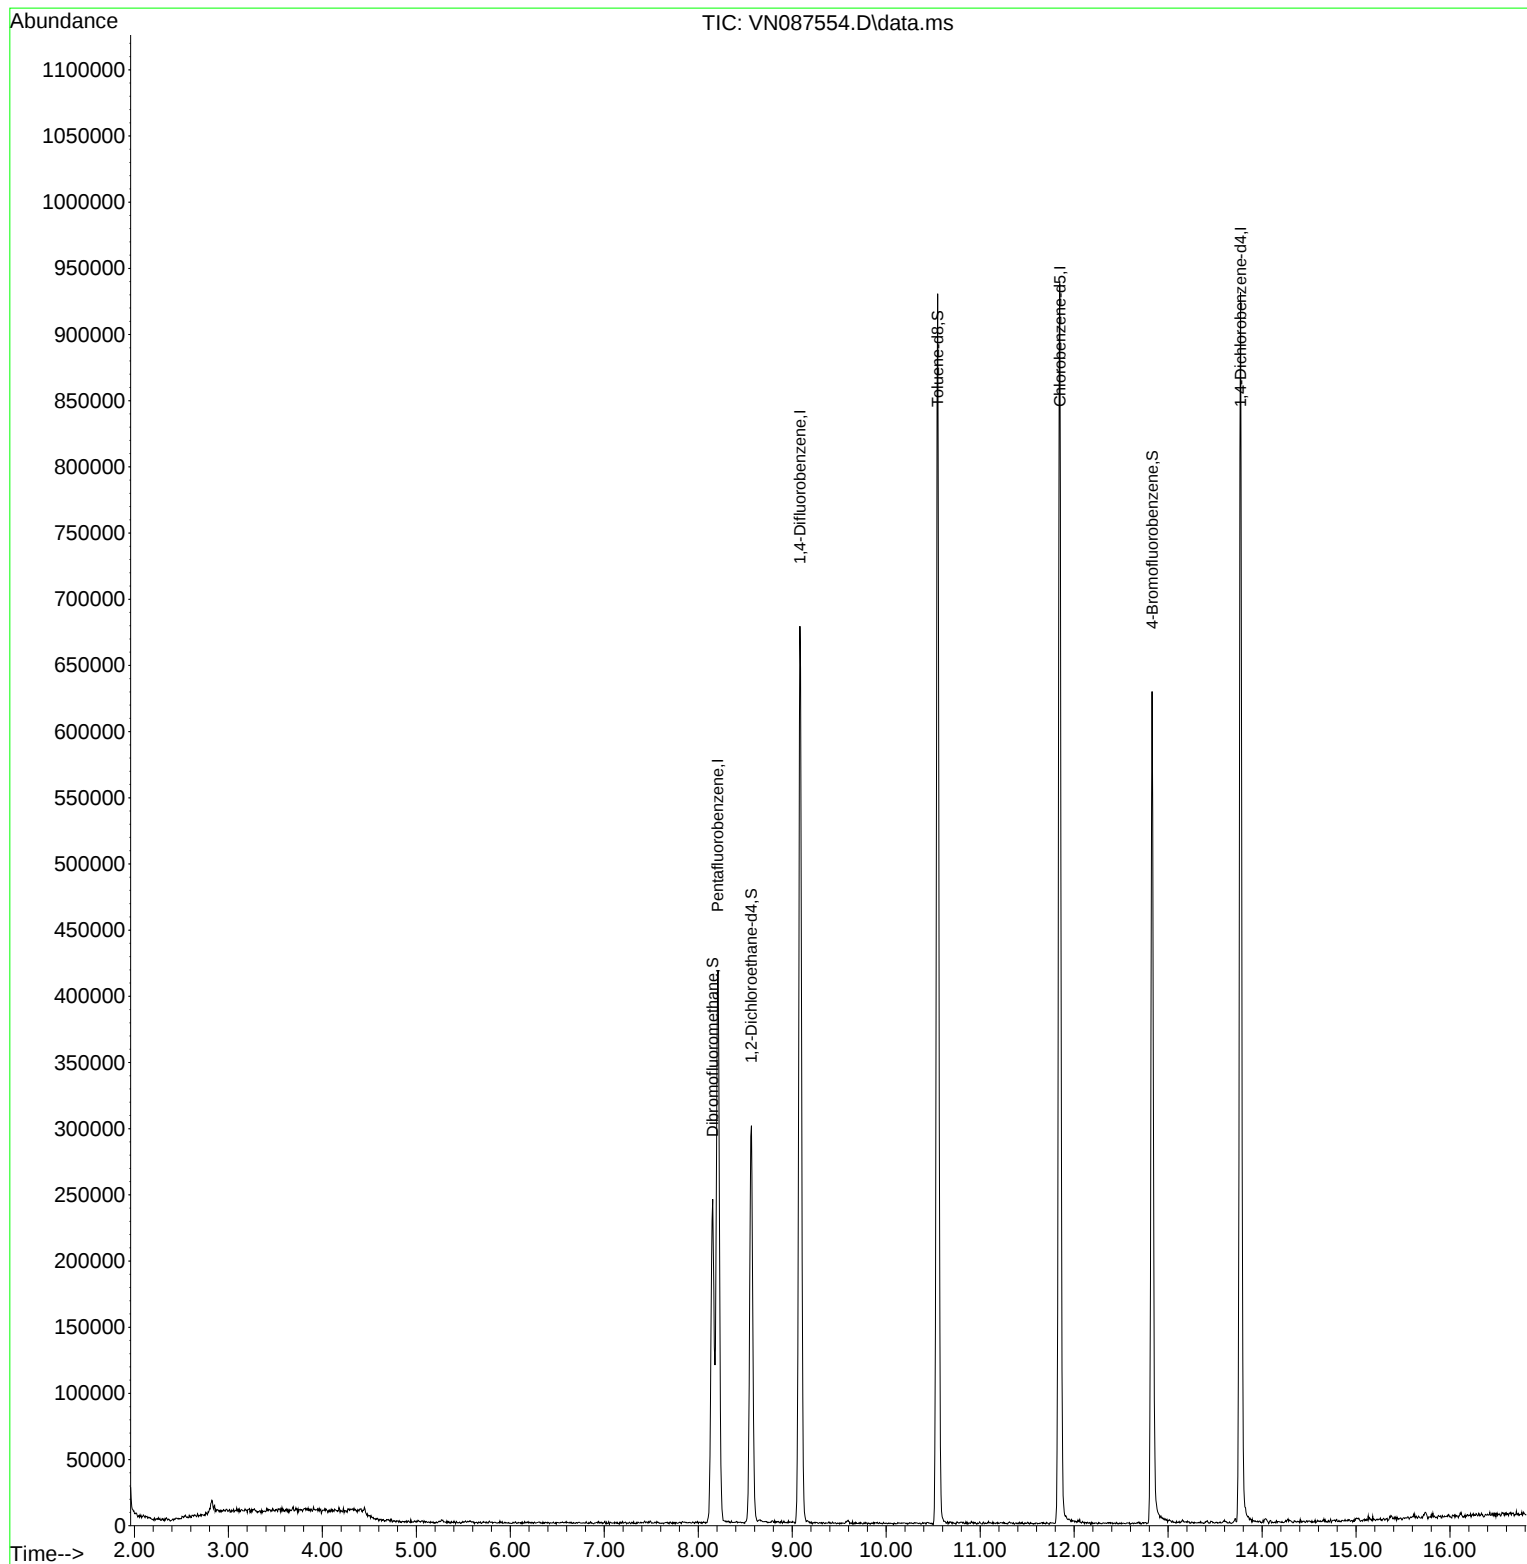


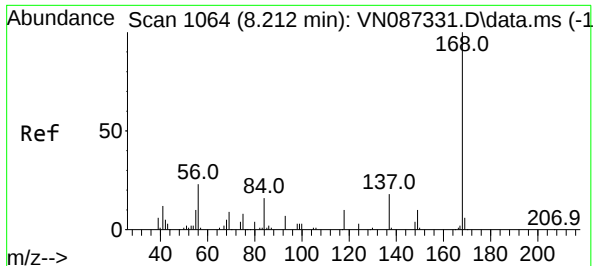

#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 8.206 min Scan# 1106
Delta R.T. -0.006 min
Lab File: VN087554.D
Acq: 14 Aug 2025 10:32




Instrument :
MSVOA_N
ClientSampleId :
VN0814WBL01


Tgt Ion:168 Resp: 284398
Ion Ratio Lower Upper
168 100
99 67.0 47.9 71.9

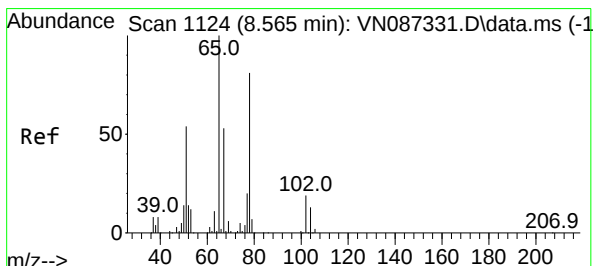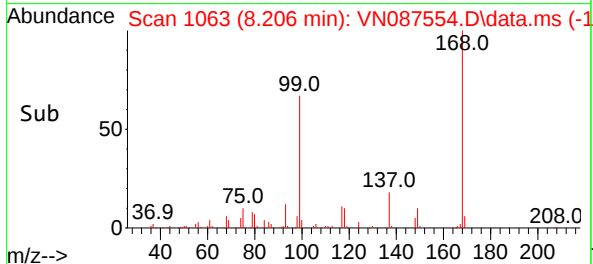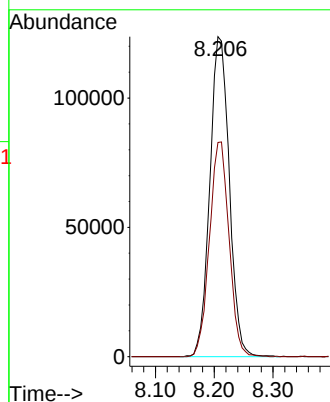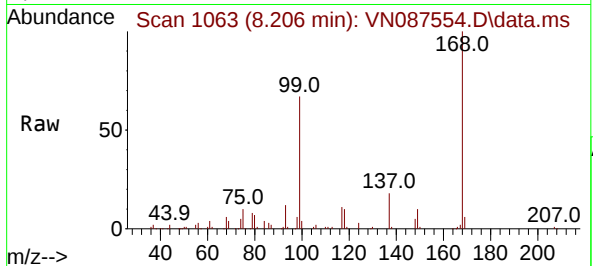

#33
1,2-Dichloroethane-d4
Concen: 52.871 ug/l
RT: 8.565 min Scan# 1124
Delta R.T. 0.000 min
Lab File: VN087554.D
Acq: 14 Aug 2025 10:32

Tgt Ion: 65 Resp: 255137
Ion Ratio Lower Upper
65 100
67 50.2 0.0 104.0

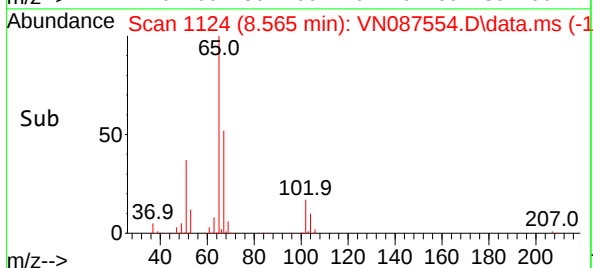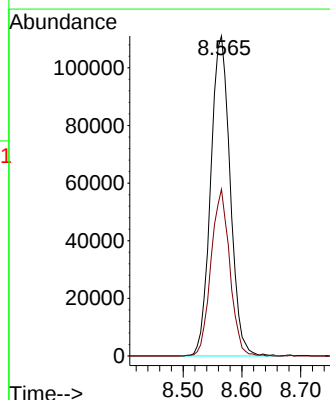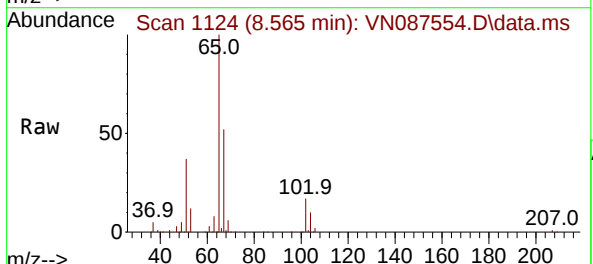

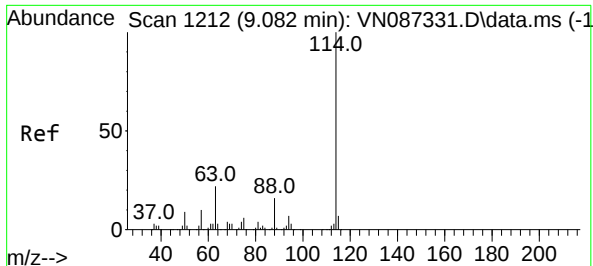

#34

1,4-Difluorobenzene

Concen: 50.000 ug/l

RT: 9.083 min Scan# 1

Delta R.T. 0.001 min

Lab File: VN087554.D

Acq: 14 Aug 2025 10:32

Instrument :

MSVOA_N

ClientSampleId :

VN0814WBL01





Tgt Ion:114 Resp: 560321

Ion Ratio Lower Upper

114 100

63 23.2 0.0 44.6

88 16.3 0.0 32.8

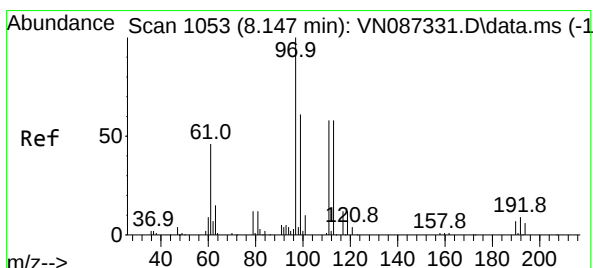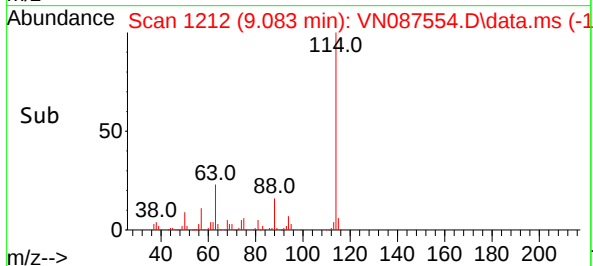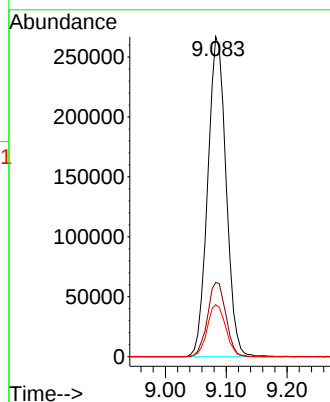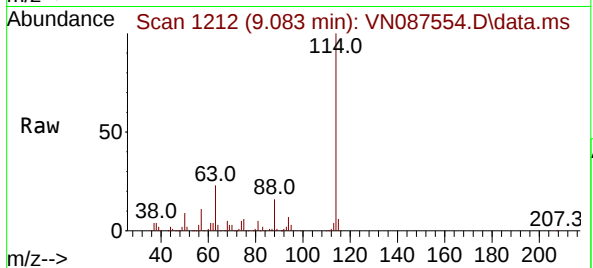

#35

Dibromofluoromethane

Concen: 44.201 ug/l

RT: 8.153 min Scan# 1054

Delta R.T. 0.006 min

Lab File: VN087554.D

Acq: 14 Aug 2025 10:32




Tgt Ion:113 Resp: 170840


Ion Ratio Lower Upper

113 100

111 103.1 82.5 123.7

192 16.3 13.7 20.5


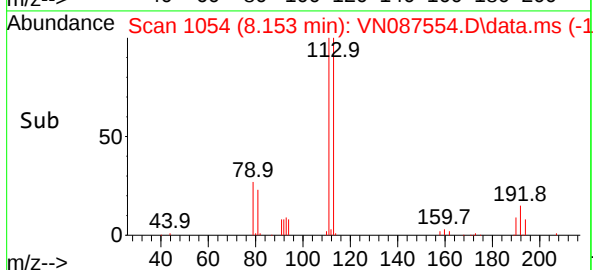
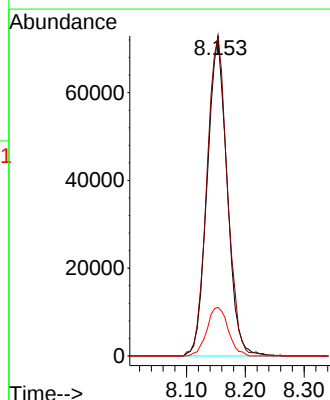
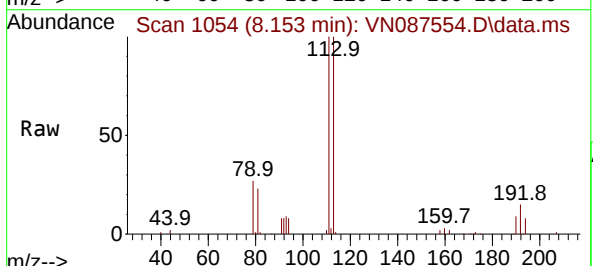


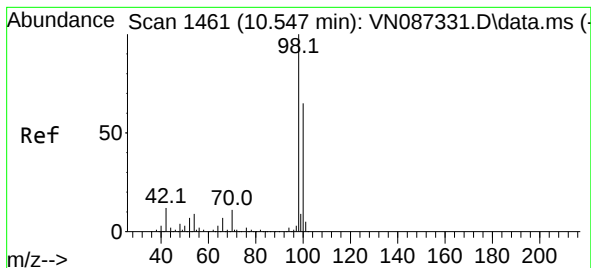

#50
Toluene-d8
Concen: 44.169 ug/l
RT: 10.547 min Scan# 1461
Delta R.T. 0.000 min
Lab File: VN087554.D
Acq: 14 Aug 2025 10:32




Instrument :
MSVOA_N
ClientSampleId :
VN0814WBL01


Tgt Ion: 98 Resp: 608969
Ion Ratio Lower Upper
98 100
100 64.2 52.1 78.1

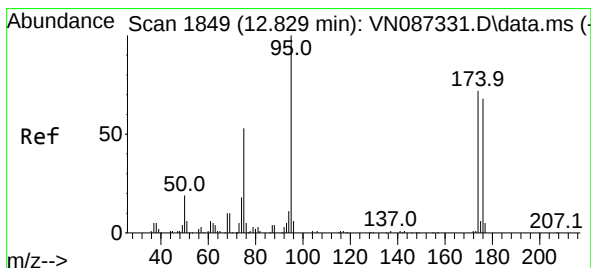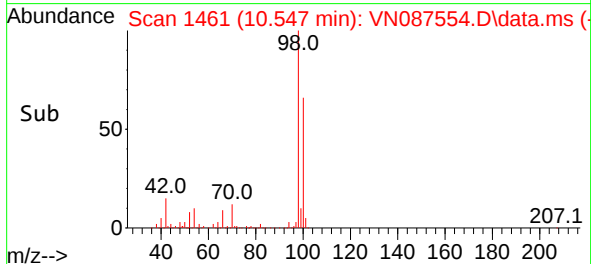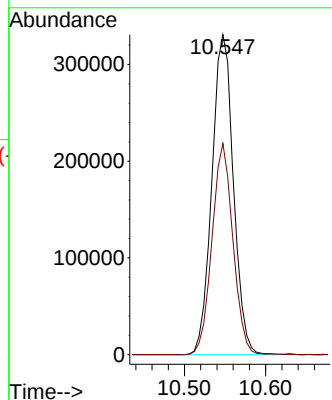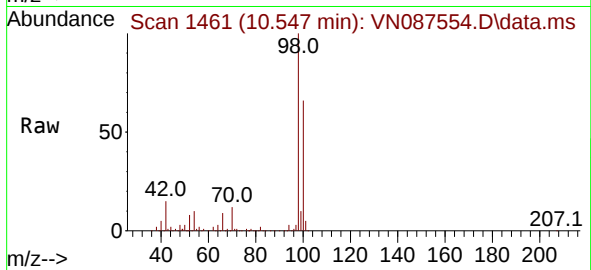

#62
4-Bromofluorobenzene
Concen: 43.709 ug/l
RT: 12.829 min Scan# 1849
Delta R.T. 0.000 min
Lab File: VN087554.D
Acq: 14 Aug 2025 10:32

Tgt Ion: 95 Resp: 222642
Ion Ratio Lower Upper
95 100
174 66.5 0.0 149.4
176 64.9 0.0 141.2


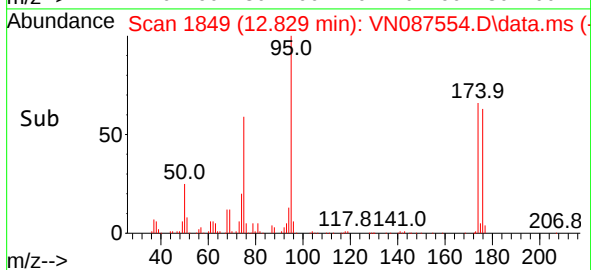
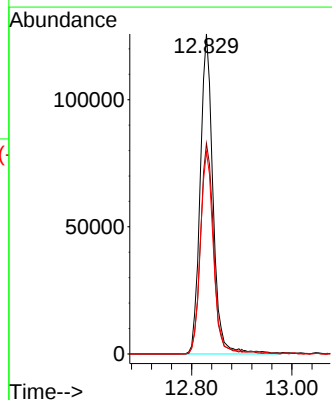
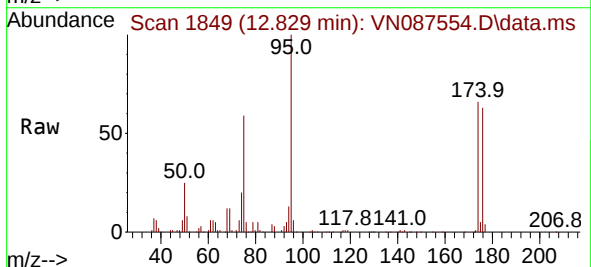


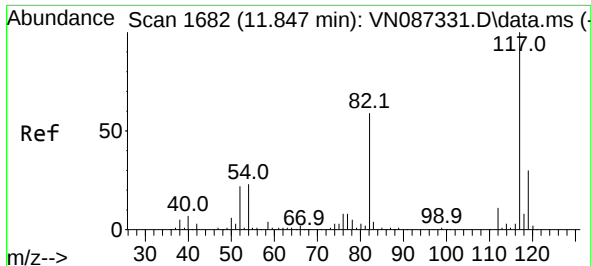

#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 11.847 min Scan# 117
Delta R.T. 0.000 min
Lab File: VN087554.D
Acq: 14 Aug 2025 10:32

Instrument :
MSVOA_N
ClientSampleId :
VN0814WBL01

Tgt Ion:117 Resp: 503771
Ion Ratio Lower Upper
117 100
82 60.7 47.4 71.2
119 31.6 23.8 35.8

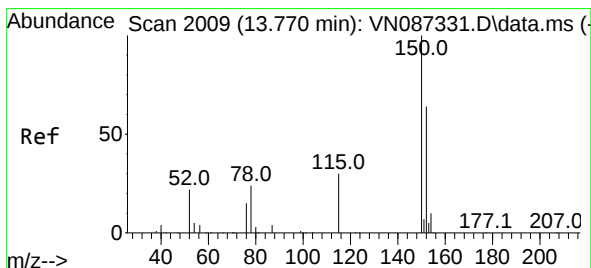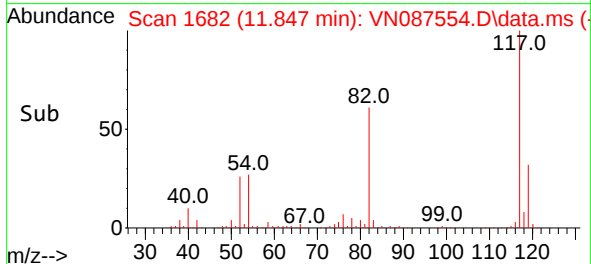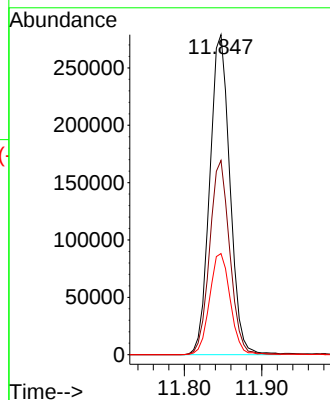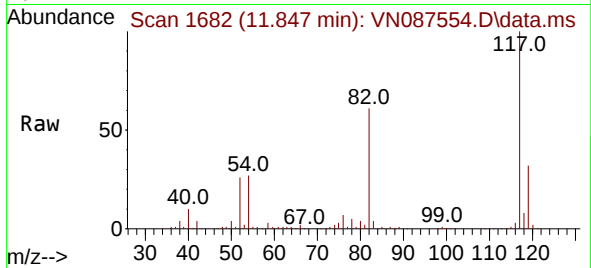

#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 13.771 min Scan# 2009
Delta R.T. 0.000 min
Lab File: VN087554.D
Acq: 14 Aug 2025 10:32

Tgt Ion:152 Resp: 234765
Ion Ratio Lower Upper
152 100
115 64.5 31.1 93.5
150 156.1 0.0 349.0

