

DATA REPORTING QUALIFIERS- ORGANIC

For reporting results, the following “Results Qualifiers” are used:

Value	If the result is a value greater than or equal to the detection limit, report the value
U	Indicates the compound was analyzed for but was not detected. Report the minimum detection limit for the sample with the U, i.e. “10 U”. This is not necessarily the instrument detection limit attainable for this particular sample based on any concentration or dilution that may have been required.
ND	Indicates the analyte was analyzed for, but not detected
J	Indicates an estimated value. This flag is used: (1) When estimating a concentration for a tentatively identified compound (library search hits, where a 1:1 response is assumed.) (2) When the mass spectral data indicated the identification, however the result was less than the specified detection limit greater than zero. If the detection limit was 10ug/L and a concentration of 3 ug/L was calculated report as 3 J. This flag is used when similar situation arise on any organic parameter i.e. Pest, PCB and others.
B	Indicates the analyte was found in the blank as well as the sample report as “12 B”.
E	Indicates the analyte ‘s concentration exceeds the calibrated range of the instrument for that specific analysis.
D	This flag identifies all compounds identified in an analysis at a secondary dilution factor.
P	This flag is used for Pesticide/PCB target analyte when there is >25% difference for detected concentrations between the two GC columns. The lower of the two values is reported on Form 1 and flagged with a “P”.
N	This flag indicates presumptive evidence of a compound. This is only used for tentatively identified compounds (TICs), where the identification is based on a mass spectral library search. It applies to all TIC results. For generic characterization of a TIC, such as chlorinated hydrocarbon, the flag is not used.
A	This flag indicates that a Tentatively Identified Compound is a suspected aldol-condensation product.
Q	Indicates the LCS did not meet the control limits requirements

LAB CHRONICLE

OrderID:	Q2868	OrderDate:	8/14/2025 9:08:00 AM
Client:	Sciacca General Contractors, LLC	Project:	507 Franklin Ave
Contact:	Rosanne Scirica	Location:	J23,VOA Lab

LabID	ClientID	Matrix	Test	Method	Sample Date	Prep Date	Anal Date	Received
Q2868-02	VOC	SOIL	VOC-TCLVOA-10	8260D	08/12/25		08/15/25	08/13/25



284 Sheffield Street, Mountainside, New Jersey 07092, Phone : 908 789 8900,
Fax : 908 789 8922

Hit Summary Sheet
SW-846

SDG No.: Q2868

Client: Sciacca General Contractors, LLC

Sample ID	Client ID	Matrix	Parameter	Concentration	C	MDL	RDL	Units
-----------	-----------	--------	-----------	---------------	---	-----	-----	-------

Client ID:

0

Total Voc :

Total Concentration:



QC SUMMARY

Surrogate Summary

SDG No.: Q2868

Client: Sciacca General Contractors, LLC

Analytical Method: SW8260D

Lab Sample ID	Client ID	Parameter	Spike	Result	Recovery (%)	Qual	Limits (%)	
							Low	High
Q2868-02	VOC	1,2-Dichloroethane-d4	50	58.5	117		63	155
		Dibromofluoromethane	50	51.9	104		70	134
		Toluene-d8	50	52.2	104		74	123
		4-Bromofluorobenzene	50	49.9	100		17	146
VY0815SBL01	VY0815SBL01	1,2-Dichloroethane-d4	50	59.8	120		63	155
		Dibromofluoromethane	50	52.7	105		70	134
		Toluene-d8	50	52.4	105		74	123
		4-Bromofluorobenzene	50	47.5	95		17	146
VY0815SBS01	VY0815SBS01	1,2-Dichloroethane-d4	50	51.7	103		63	155
		Dibromofluoromethane	50	49.3	99		70	134
		Toluene-d8	50	50.2	100		74	123
		4-Bromofluorobenzene	50	48.5	97		17	146
VY0815BSD01	VY0815BSD01	1,2-Dichloroethane-d4	50	52.1	104		63	155
		Dibromofluoromethane	50	50.3	101		70	134
		Toluene-d8	50	50.5	101		74	123
		4-Bromofluorobenzene	50	48.7	97		17	146

Laboratory Control Sample/Laboratory Control Sample Duplicate Summary

SW-846

SDG No.:	<u>Q2868</u>	Analytical Method:	<u>SW8260D</u>
Client:	<u>Sciacca General Contractors, LLC</u>	Datafile :	<u>VY023113.D</u>

Lab Sample ID	Parameter	Spike	Result	Unit	Rec	RPD	Qual	Low	Limits High	RPD
VY0815SBS01	Dichlorodifluoromethane	20	19.7	ug/Kg	99			64	136	
	Chloromethane	20	22.2	ug/Kg	111			52	151	
	Vinyl chloride	20	22.5	ug/Kg	113			56	148	
	Bromomethane	20	25.5	ug/Kg	128			58	141	
	Chloroethane	20	22.7	ug/Kg	114			69	130	
	Trichlorofluoromethane	20	21.1	ug/Kg	106			69	134	
	1,1,2-Trichlorotrifluoroethane	20	20.2	ug/Kg	101			81	123	
	1,1-Dichloroethene	20	19.8	ug/Kg	99			79	121	
	Acetone	100	110	ug/Kg	110			40	171	
	Carbon disulfide	20	20.1	ug/Kg	101			59	130	
	Methyl tert-butyl Ether	20	19.5	ug/Kg	98			77	129	
	Methyl Acetate	20	18.5	ug/Kg	93			69	149	
	Methylene Chloride	20	20.8	ug/Kg	104			72	131	
	trans-1,2-Dichloroethene	20	19.9	ug/Kg	100			80	123	
	1,1-Dichloroethane	20	20.4	ug/Kg	102			82	123	
	Cyclohexane	20	18.9	ug/Kg	95			76	122	
	2-Butanone	100	110	ug/Kg	110			69	131	
	Carbon Tetrachloride	20	19.6	ug/Kg	98			76	129	
	cis-1,2-Dichloroethene	20	20.1	ug/Kg	101			82	123	
	Bromochloromethane	20	21.9	ug/Kg	110			80	127	
	Chloroform	20	20.9	ug/Kg	104			82	125	
	1,1,1-Trichloroethane	20	20.3	ug/Kg	102			80	126	
	Methylcyclohexane	20	18.7	ug/Kg	94			77	123	
	Benzene	20	20.4	ug/Kg	102			84	121	
	1,2-Dichloroethane	20	20.6	ug/Kg	103			81	126	
	Trichloroethene	20	20.5	ug/Kg	103			83	122	
	1,2-Dichloropropane	20	20.5	ug/Kg	103			83	122	
	Bromodichloromethane	20	20.8	ug/Kg	104			82	123	
	4-Methyl-2-Pentanone	100	97.9	ug/Kg	98			70	135	
	Toluene	20	20.2	ug/Kg	101			83	122	
	t-1,3-Dichloropropene	20	19.9	ug/Kg	100			78	124	
	cis-1,3-Dichloropropene	20	19.6	ug/Kg	98			81	122	
	1,1,2-Trichloroethane	20	20.2	ug/Kg	101			82	125	
	2-Hexanone	100	100	ug/Kg	100			66	138	
	Dibromochloromethane	20	20.1	ug/Kg	101			79	125	
	1,2-Dibromoethane	20	20.1	ug/Kg	101			80	125	
	Tetrachloroethene	20	21.8	ug/Kg	109			83	125	
	Chlorobenzene	20	19.5	ug/Kg	98			84	122	
	Ethyl Benzene	20	18.8	ug/Kg	94			82	124	
	m/p-Xylenes	40	38.6	ug/Kg	97			83	124	
	o-Xylene	20	18.6	ug/Kg	93			83	123	
	Styrene	20	19.4	ug/Kg	97			82	124	
	Bromoform	20	18.7	ug/Kg	94			75	127	
	Isopropylbenzene	20	18.8	ug/Kg	94			82	124	
	1,1,2,2-Tetrachloroethane	20	18.1	ug/Kg	91			77	127	
	1,3-Dichlorobenzene	20	19.1	ug/Kg	96			83	122	
	1,4-Dichlorobenzene	20	19.3	ug/Kg	97			84	121	
	1,2-Dichlorobenzene	20	18.9	ug/Kg	95			83	124	

Laboratory Control Sample/Laboratory Control Sample Duplicate Summary

SW-846

SDG No.:	<u>Q2868</u>	Analytical Method:	<u>SW8260D</u>
Client:	<u>Sciacca General Contractors, LLC</u>	Datafile :	<u>VY023113.D</u>

Lab Sample ID	Parameter	Spike	Result	Unit	Rec	RPD	Qual	Low	Limits High	RPD
VY0815SBS01	1,2-Dibromo-3-Chloropropane	20	19.8	ug/Kg	99			66	134	
	1,2,4-Trichlorobenzene	20	18.2	ug/Kg	91			78	127	
	1,2,3-Trichlorobenzene	20	17.9	ug/Kg	90			70	137	

Laboratory Control Sample/Laboratory Control Sample Duplicate Summary

SW-846

SDG No.:	<u>Q2868</u>	Analytical Method:	<u>SW8260D</u>
Client:	<u>Sciacca General Contractors, LLC</u>	Datafile :	<u>VY023114.D</u>

Lab Sample ID	Parameter	Spike	Result	Unit	Rec	RPD	Qual	Low	Limits High	RPD
VY0815SBSD01	Dichlorodifluoromethane	20	21.3	ug/Kg	106	7		64	136	20
	Chloromethane	20	22.8	ug/Kg	114	3		52	151	20
	Vinyl chloride	20	23.3	ug/Kg	117	3		56	148	20
	Bromomethane	20	25.5	ug/Kg	128	0		58	141	20
	Chloroethane	20	23.9	ug/Kg	119	4		69	130	20
	Trichlorofluoromethane	20	22.3	ug/Kg	112	6		69	134	20
	1,1,2-Trichlorotrifluoroethane	20	21.7	ug/Kg	109	8		81	123	20
	1,1-Dichloroethene	20	20.9	ug/Kg	104	5		79	121	20
	Acetone	100	110	ug/Kg	110	0		40	171	20
	Carbon disulfide	20	20.8	ug/Kg	104	3		59	130	20
	Methyl tert-butyl Ether	20	20.3	ug/Kg	102	4		77	129	20
	Methyl Acetate	20	21.2	ug/Kg	106	13		69	149	20
	Methylene Chloride	20	22.1	ug/Kg	111	7		72	131	20
	trans-1,2-Dichloroethene	20	21.0	ug/Kg	105	5		80	123	20
	1,1-Dichloroethane	20	21.0	ug/Kg	105	3		82	123	20
	Cyclohexane	20	19.7	ug/Kg	99	4		76	122	20
	2-Butanone	100	100	ug/Kg	100	10		69	131	20
	Carbon Tetrachloride	20	20.5	ug/Kg	103	5		76	129	20
	cis-1,2-Dichloroethene	20	20.5	ug/Kg	103	2		82	123	20
	Bromochloromethane	20	21.8	ug/Kg	109	1		80	127	20
	Chloroform	20	21.6	ug/Kg	108	4		82	125	20
	1,1,1-Trichloroethane	20	21.0	ug/Kg	105	3		80	126	20
	Methylcyclohexane	20	19.5	ug/Kg	98	4		77	123	20
	Benzene	20	20.6	ug/Kg	103	1		84	121	20
	1,2-Dichloroethane	20	20.9	ug/Kg	104	1		81	126	20
	Trichloroethene	20	21.1	ug/Kg	106	3		83	122	20
	1,2-Dichloropropane	20	20.6	ug/Kg	103	0		83	122	20
	Bromodichloromethane	20	20.7	ug/Kg	104	0		82	123	20
	4-Methyl-2-Pentanone	100	99.3	ug/Kg	99	1		70	135	20
	Toluene	20	20.5	ug/Kg	103	2		83	122	20
	t-1,3-Dichloropropene	20	19.7	ug/Kg	99	1		78	124	20
	cis-1,3-Dichloropropene	20	20.2	ug/Kg	101	3		81	122	20
	1,1,2-Trichloroethane	20	20.4	ug/Kg	102	1		82	125	20
	2-Hexanone	100	99.7	ug/Kg	100	0		66	138	20
	Dibromochloromethane	20	20.6	ug/Kg	103	2		79	125	20
	1,2-Dibromoethane	20	20.2	ug/Kg	101	0		80	125	20
	Tetrachloroethene	20	22.8	ug/Kg	114	4		83	125	20
	Chlorobenzene	20	21.1	ug/Kg	106	8		84	122	20
	Ethyl Benzene	20	20.2	ug/Kg	101	7		82	124	20
	m/p-Xylenes	40	41.1	ug/Kg	103	6		83	124	20
	o-Xylene	20	20.1	ug/Kg	101	8		83	123	20
	Styrene	20	20.5	ug/Kg	103	6		82	124	20
	Bromoform	20	19.8	ug/Kg	99	5		75	127	20
	Isopropylbenzene	20	19.4	ug/Kg	97	3		82	124	20
	1,1,2,2-Tetrachloroethane	20	19.0	ug/Kg	95	4		77	127	20
	1,3-Dichlorobenzene	20	20.1	ug/Kg	101	5		83	122	20
	1,4-Dichlorobenzene	20	19.8	ug/Kg	99	2		84	121	20
	1,2-Dichlorobenzene	20	19.7	ug/Kg	99	4		83	124	20

Laboratory Control Sample/Laboratory Control Sample Duplicate Summary

SW-846

SDG No.:	<u>Q2868</u>	Analytical Method:	<u>SW8260D</u>
Client:	<u>Sciacca General Contractors, LLC</u>	Datafile :	<u>VY023114.D</u>

Lab Sample ID	Parameter	Spike	Result	Unit	Rec	RPD	Qual	Low	Limits	RPD
									High	
VY0815SBSD01	1,2-Dibromo-3-Chloropropane	20	20.0	ug/Kg	100	1		66	134	20
	1,2,4-Trichlorobenzene	20	18.5	ug/Kg	93	2		78	127	20
	1,2,3-Trichlorobenzene	20	18.6	ug/Kg	93	3		70	137	20

VOLATILE METHOD BLANK SUMMARY

Client ID

VY0815SBL01

Lab Name: Alliance

Contract: SCIA01

Lab Code: ACE

SDG NO.: Q2868

Lab File ID: VY023112.D

Lab Sample ID: VY0815SBL01

Date Analyzed: 08/15/2025

Time Analyzed: 09:08

GC Column: RXI-624 ID: 0.25 (mm)

Heated Purge: (Y/N) Y

Instrument ID: MSVOA_Y

THIS METHOD BLANK APPLIES TO THE FOLLOWING SAMPLES, MS AND MSD:

EPA SAMPLE NO.	LAB SAMPLE ID	LAB FILE ID	DATE ANALYZED
VY0815SBS01	VY0815SBS01	VY023113.D	08/15/2025
VY0815SBSD01	VY0815SBSD01	VY023114.D	08/15/2025
VOC	Q2868-02	VY023131.D	08/15/2025

COMMENTS: _____



284 Sheffield Street, Mountainside, New Jersey 07092, Phone : 908 789 8900,
Fax : 908 789 8922

VOLATILE ORGANIC INSTRUMENT PERFORMANCE CHECK
BROMOFLUOROBENZENE (BFB)

Lab Name: Alliance

Contract: SCIA01

Lab Code: ACE

SDG NO.: Q2868

Lab File ID: VY023048.D

BFB Injection Date: 08/12/2025

Instrument ID: MSVOA_Y

BFB Injection Time: 08:26

GC Column: RXI-624 ID: 0.25 (mm)

Heated Purge: Y/N Y

m/e	ION ABUNDANCE CRITERIA	% RELATIVE ABUNDANCE
50	15.0 - 40.0% of mass 95	19.2
75	30.0 - 60.0% of mass 95	51.9
95	Base Peak, 100% relative abundance	100
96	5.0 - 9.0% of mass 95	6.8
173	Less than 2.0% of mass 174	0.9 (1.1) 1
174	50.0 - 100.0% of mass 95	83.2
175	5.0 - 9.0% of mass 174	6.3 (7.6) 1
176	95.0 - 101.0% of mass 174	80.9 (97.2) 1
177	5.0 - 9.0% of mass 176	5.1 (6.4) 2

1-Value is % mass 174

2-Value is % mass 176

THIS CHECK APPLIES TO THE FOLLOWING SAMPLES, MS, MSD, BLANKS, AND STANDARDS:

CLIENT ID	LAB SAMPLE ID	LAB FILE ID	DATE ANALYZED	TIME ANALYZED
VSTDIC005	VSTDIC005	VY023050.D	08/12/2025	14:54
VSTDIC010	VSTDIC010	VY023051.D	08/12/2025	15:17
VSTDIC020	VSTDIC020	VY023052.D	08/12/2025	15:40
VSTDIC050	VSTDIC050	VY023053.D	08/12/2025	16:02
VSTDIC100	VSTDIC100	VY023054.D	08/12/2025	16:25
VSTDIC150	VSTDIC150	VY023055.D	08/12/2025	16:47



284 Sheffield Street, Mountainside, New Jersey 07092, Phone : 908 789 8900,
Fax : 908 789 8922

VOLATILE ORGANIC INSTRUMENT PERFORMANCE CHECK
BROMOFLUOROBENZENE (BFB)

Lab Name: Alliance

Contract: SCIA01

Lab Code: ACE

SDG NO.: Q2868

Lab File ID: VY023110.D

BFB Injection Date: 08/15/2025

Instrument ID: MSVOA_Y

BFB Injection Time: 08:07

GC Column: RXI-624 ID: 0.25 (mm)

Heated Purge: Y/N Y

m/e	ION ABUNDANCE CRITERIA	% RELATIVE ABUNDANCE
50	15.0 - 40.0% of mass 95	19.6
75	30.0 - 60.0% of mass 95	52.7
95	Base Peak, 100% relative abundance	100
96	5.0 - 9.0% of mass 95	6.8
173	Less than 2.0% of mass 174	1.1 (1.2) 1
174	50.0 - 100.0% of mass 95	88.9
175	5.0 - 9.0% of mass 174	6.6 (7.4) 1
176	95.0 - 101.0% of mass 174	85.3 (96) 1
177	5.0 - 9.0% of mass 176	5.6 (6.5) 2

1-Value is % mass 174

2-Value is % mass 176

THIS CHECK APPLIES TO THE FOLLOWING SAMPLES, MS, MSD, BLANKS, AND STANDARDS:

CLIENT ID	LAB SAMPLE ID	LAB FILE ID	DATE ANALYZED	TIME ANALYZED
VSTDCCC050	VSTDCCC050	VY023111.D	08/15/2025	08:39
VY0815SBL01	VY0815SBL01	VY023112.D	08/15/2025	09:08
VY0815SBS01	VY0815SBS01	VY023113.D	08/15/2025	09:37
VY0815SBSD01	VY0815SBSD01	VY023114.D	08/15/2025	09:59
VOC	Q2868-02	VY023131.D	08/15/2025	17:33

VOLATILE INTERNAL STANDARD AREA AND RT SUMMARY

Lab Name: Alliance Contract: SCIA01
 Lab Code: ACE SDG NO.: Q2868
 Lab File ID: VY023111.D Date Analyzed: 08/15/2025
 Instrument ID: MSVOA_Y Time Analyzed: 08:39
 GC Column: RXI-624 ID: 0.25 (mm) Heated Purge: (Y/N) Y

	IS1 AREA #	RT #	IS2 AREA #	RT #	IS3 AREA #	RT #
12 HOUR STD	443799	7.71	696916	8.62	607348	11.41
UPPER LIMIT	887598	8.207	1393830	9.116	1214700	11.914
LOWER LIMIT	221900	7.207	348458	8.116	303674	10.914
EPA SAMPLE NO.						
VOC	496911	7.70	931727	8.61	853505	11.41
VY0815SBL01	550500	7.71	1049087	8.62	953139	11.41
VY0815SBS01	452403	7.71	727202	8.62	654458	11.41
VY0815SBSD01	440097	7.71	718363	8.62	623331	11.41

IS1 = Pentafluorobenzene
 IS2 = 1,4-Difluorobenzene
 IS3 = Chlorobenzene-d5

AREA UPPER LIMIT = +100% of internal standard area
 AREA LOWER LIMIT = -50% of internal standard area
 RT UPPER LIMIT = +0.50 minutes of internal standard RT
 RT LOWER LIMIT = -0.50 minutes of internal standard RT

Column used to flag values outside QC limits with an asterisk.
 * Values outside of QC limits.

VOLATILE INTERNAL STANDARD AREA AND RT SUMMARY

Lab Name: Alliance Contract: SCIA01
 Lab Code: ACE SDG NO.: Q2868
 Lab File ID: VY023111.D Date Analyzed: 08/15/2025
 Instrument ID: MSVOA_Y Time Analyzed: 08:39
 GC Column: RXI-624 ID: 0.25 (mm) Heated Purge: (Y/N) Y

	IS4 AREA #	RT #				
12 HOUR STD	306948	13.347				
UPPER LIMIT	613896	13.847				
LOWER LIMIT	153474	12.847				
EPA SAMPLE NO.						
VOC	359140	13.34				
VY0815SBL01	370974	13.35				
VY0815SBS01	327154	13.34				
VY0815SBSD01	315352	13.34				

IS4 = 1,4-Dichlorobenzene-d4

AREA UPPER LIMIT = +100% of internal standard area
 AREA LOWER LIMIT = -50% of internal standard area
 RT UPPER LIMIT = +0.50 minutes of internal standard RT
 RT LOWER LIMIT = -0.50 minutes of internal standard RT

Column used to flag values outside QC limits with an asterisk.
 * Values outside of QC limits.



SAMPLE DATA

Report of Analysis

Client:	Sciacca General Contractors, LLC		Date Collected:	08/12/25	
Project:	507 Franklin Ave		Date Received:	08/13/25	
Client Sample ID:	VOC		SDG No.:	Q2868	
Lab Sample ID:	Q2868-02		Matrix:	SOIL	
Analytical Method:	8260D		% Solid:	97.5	
Sample Wt/Vol:	5.18	Units: g	Final Vol:	5000	uL
Soil Aliquot Vol:		uL	Test:	VOC-TCLVOA-10	
GC Column:	RXI-624	ID : 0.25	Level :	LOW	
Prep Method :					

File ID/Qc Batch:	Dilution:	Date Analyzed	Prep Batch ID
VY023131.D	1	08/15/25 17:33	VY081525

CAS Number	Parameter	Conc.	Qualifier	MDL	LOQ / CRQL	Units(Dry Weight)
TARGETS						
75-71-8	Dichlorodifluoromethane	1.10	U	1.10	5.00	ug/Kg
74-87-3	Chloromethane	1.10	U	1.10	5.00	ug/Kg
75-01-4	Vinyl Chloride	0.78	U	0.78	5.00	ug/Kg
74-83-9	Bromomethane	1.10	U	1.10	5.00	ug/Kg
75-00-3	Chloroethane	1.20	U	1.20	5.00	ug/Kg
75-69-4	Trichlorofluoromethane	1.20	U	1.20	5.00	ug/Kg
76-13-1	1,1,2-Trichlorotrifluoroethane	1.00	U	1.00	5.00	ug/Kg
75-35-4	1,1-Dichloroethene	0.99	U	0.99	5.00	ug/Kg
67-64-1	Acetone	4.70	U	4.70	24.8	ug/Kg
75-15-0	Carbon Disulfide	1.00	U	1.00	5.00	ug/Kg
1634-04-4	Methyl tert-butyl Ether	0.72	U	0.72	5.00	ug/Kg
79-20-9	Methyl Acetate	1.50	U	1.50	5.00	ug/Kg
75-09-2	Methylene Chloride	3.50	U	3.50	9.90	ug/Kg
156-60-5	trans-1,2-Dichloroethene	0.85	U	0.85	5.00	ug/Kg
75-34-3	1,1-Dichloroethane	0.79	U	0.79	5.00	ug/Kg
110-82-7	Cyclohexane	0.78	U	0.78	5.00	ug/Kg
78-93-3	2-Butanone	6.50	U	6.50	24.8	ug/Kg
56-23-5	Carbon Tetrachloride	0.96	U	0.96	5.00	ug/Kg
156-59-2	cis-1,2-Dichloroethene	0.74	U	0.74	5.00	ug/Kg
74-97-5	Bromochloromethane	1.10	U	1.10	5.00	ug/Kg
67-66-3	Chloroform	0.83	U	0.83	5.00	ug/Kg
71-55-6	1,1,1-Trichloroethane	0.92	U	0.92	5.00	ug/Kg
108-87-2	Methylcyclohexane	0.90	U	0.90	5.00	ug/Kg
71-43-2	Benzene	0.78	U	0.78	5.00	ug/Kg
107-06-2	1,2-Dichloroethane	0.78	U	0.78	5.00	ug/Kg
79-01-6	Trichloroethene	0.80	U	0.80	5.00	ug/Kg
78-87-5	1,2-Dichloropropane	0.90	U	0.90	5.00	ug/Kg
75-27-4	Bromodichloromethane	0.77	U	0.77	5.00	ug/Kg
108-10-1	4-Methyl-2-Pentanone	3.50	U	3.50	24.8	ug/Kg
108-88-3	Toluene	0.77	U	0.77	5.00	ug/Kg

Report of Analysis

Client:	Sciacca General Contractors, LLC		Date Collected:	08/12/25	
Project:	507 Franklin Ave		Date Received:	08/13/25	
Client Sample ID:	VOC		SDG No.:	Q2868	
Lab Sample ID:	Q2868-02		Matrix:	SOIL	
Analytical Method:	8260D		% Solid:	97.5	
Sample Wt/Vol:	5.18	Units: g	Final Vol:	5000	uL
Soil Aliquot Vol:		uL	Test:	VOC-TCLVOA-10	
GC Column:	RXI-624	ID : 0.25	Level :	LOW	
Prep Method :					

File ID/Qc Batch:	Dilution:	Date Analyzed	Prep Batch ID
VY023131.D	1	08/15/25 17:33	VY081525

CAS Number	Parameter	Conc.	Qualifier	MDL	LOQ / CRQL	Units(Dry Weight)
10061-02-6	t-1,3-Dichloropropene	0.64	U	0.64	5.00	ug/Kg
10061-01-5	cis-1,3-Dichloropropene	0.61	U	0.61	5.00	ug/Kg
79-00-5	1,1,2-Trichloroethane	0.91	U	0.91	5.00	ug/Kg
591-78-6	2-Hexanone	3.70	U	3.70	24.8	ug/Kg
124-48-1	Dibromochloromethane	0.86	U	0.86	5.00	ug/Kg
106-93-4	1,2-Dibromoethane	0.87	U	0.87	5.00	ug/Kg
127-18-4	Tetrachloroethene	1.00	U	1.00	5.00	ug/Kg
108-90-7	Chlorobenzene	0.90	U	0.90	5.00	ug/Kg
100-41-4	Ethyl Benzene	0.66	U	0.66	5.00	ug/Kg
179601-23-1	m/p-Xylenes	1.20	U	1.20	9.90	ug/Kg
95-47-6	o-Xylene	0.81	U	0.81	5.00	ug/Kg
100-42-5	Styrene	0.70	U	0.70	5.00	ug/Kg
75-25-2	Bromoform	0.85	U	0.85	5.00	ug/Kg
98-82-8	Isopropylbenzene	0.77	U	0.77	5.00	ug/Kg
79-34-5	1,1,2,2-Tetrachloroethane	1.20	U	1.20	5.00	ug/Kg
541-73-1	1,3-Dichlorobenzene	1.70	U	1.70	5.00	ug/Kg
106-46-7	1,4-Dichlorobenzene	1.50	U	1.50	5.00	ug/Kg
95-50-1	1,2-Dichlorobenzene	1.40	U	1.40	5.00	ug/Kg
96-12-8	1,2-Dibromo-3-Chloropropane	1.80	U	1.80	5.00	ug/Kg
120-82-1	1,2,4-Trichlorobenzene	2.90	U	2.90	5.00	ug/Kg
87-61-6	1,2,3-Trichlorobenzene	3.10	U	3.10	5.00	ug/Kg
SURROGATES						
17060-07-0	1,2-Dichloroethane-d4	58.5		63 - 155	117%	SPK: 50
1868-53-7	Dibromofluoromethane	51.9		70 - 134	104%	SPK: 50
2037-26-5	Toluene-d8	52.2		74 - 123	104%	SPK: 50
460-00-4	4-Bromofluorobenzene	49.9		17 - 146	100%	SPK: 50
INTERNAL STANDARDS						
363-72-4	Pentafluorobenzene	497000	7.701			
540-36-3	1,4-Difluorobenzene	932000	8.61			
3114-55-4	Chlorobenzene-d5	854000	11.414			
3855-82-1	1,4-Dichlorobenzene-d4	359000	13.34			

Report of Analysis

Client:	Sciacca General Contractors, LLC	Date Collected:	08/12/25
Project:	507 Franklin Ave	Date Received:	08/13/25
Client Sample ID:	VOC	SDG No.:	Q2868
Lab Sample ID:	Q2868-02	Matrix:	SOIL
Analytical Method:	8260D	% Solid:	97.5
Sample Wt/Vol:	5.18 Units: g	Final Vol:	5000 uL
Soil Aliquot Vol:	uL	Test:	VOC-TCLVOA-10
GC Column:	RXI-624 ID : 0.25	Level :	LOW
Prep Method :			

File ID/Qc Batch:	Dilution:	Date Analyzed	Prep Batch ID
VY023131.D	1	08/15/25 17:33	VY081525

CAS Number	Parameter	Conc.	Qualifier	MDL	LOQ / CRQL	Units
------------	-----------	-------	-----------	-----	------------	-------

U = Not Detected

LOQ = Limit of Quantitation

MDL = Method Detection Limit

LOD = Limit of Detection

E = Value Exceeds Calibration Range

Q = indicates LCS control criteria did not meet requirements

M = MS/MSD acceptance criteria did not meet requirements

J = Estimated Value

B = Analyte Found in Associated Method Blank

N = Presumptive Evidence of a Compound

* = Values outside of QC limits

D = Dilution

() = Laboratory InHouse Limit

A = Aldol-Condensation Reaction Products

Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY081525\
 Data File : VY023131.D
 Acq On : 15 Aug 2025 17:33
 Operator : SY/MD
 Sample : Q2868-02
 Misc : 5.18g/5.0mL/MSVOA_Y/SOIL/A
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 MSVOA_Y
 ClientSampleId :
 VOC

Quant Time: Aug 18 02:32:28 2025
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y081225S.M
 Quant Title : SW846 8260
 QLast Update : Wed Aug 13 02:10:11 2025
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Pentafluorobenzene	7.701	168	496911	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	8.610	114	931727	50.000	ug/l	0.00
63) Chlorobenzene-d5	11.414	117	853505	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.340	152	359140	50.000	ug/l	0.00

System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	8.055	65	276979	58.485	ug/l	0.00
Spiked Amount	50.000	Range	50 - 163	Recovery	=	116.960%
35) Dibromofluoromethane	7.634	113	289457	51.919	ug/l	0.00
Spiked Amount	50.000	Range	54 - 147	Recovery	=	103.840%
50) Toluene-d8	10.103	98	1137267	52.217	ug/l	0.00
Spiked Amount	50.000	Range	58 - 134	Recovery	=	104.440%
62) 4-Bromofluorobenzene	12.402	95	349218	49.857	ug/l	0.00
Spiked Amount	50.000	Range	30 - 143	Recovery	=	99.720%


Target Compounds	Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY081525\
Data File : VY023131.D
Acq On : 15 Aug 2025 17:33
Operator : SY/MD
Sample : Q2868-02
Misc : 5.18g/5.0mL/MSVOA_Y/SOIL/A
ALS Vial : 23 Sample Multiplier: 1

Instrument :
MSVOA_Y
ClientSampleId :
VOC

Quant Time: Aug 18 02:32:28 2025
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y081225S.M
Quant Title : SW846 8260
QLast Update : Wed Aug 13 02:10:11 2025
Response via : Initial Calibration




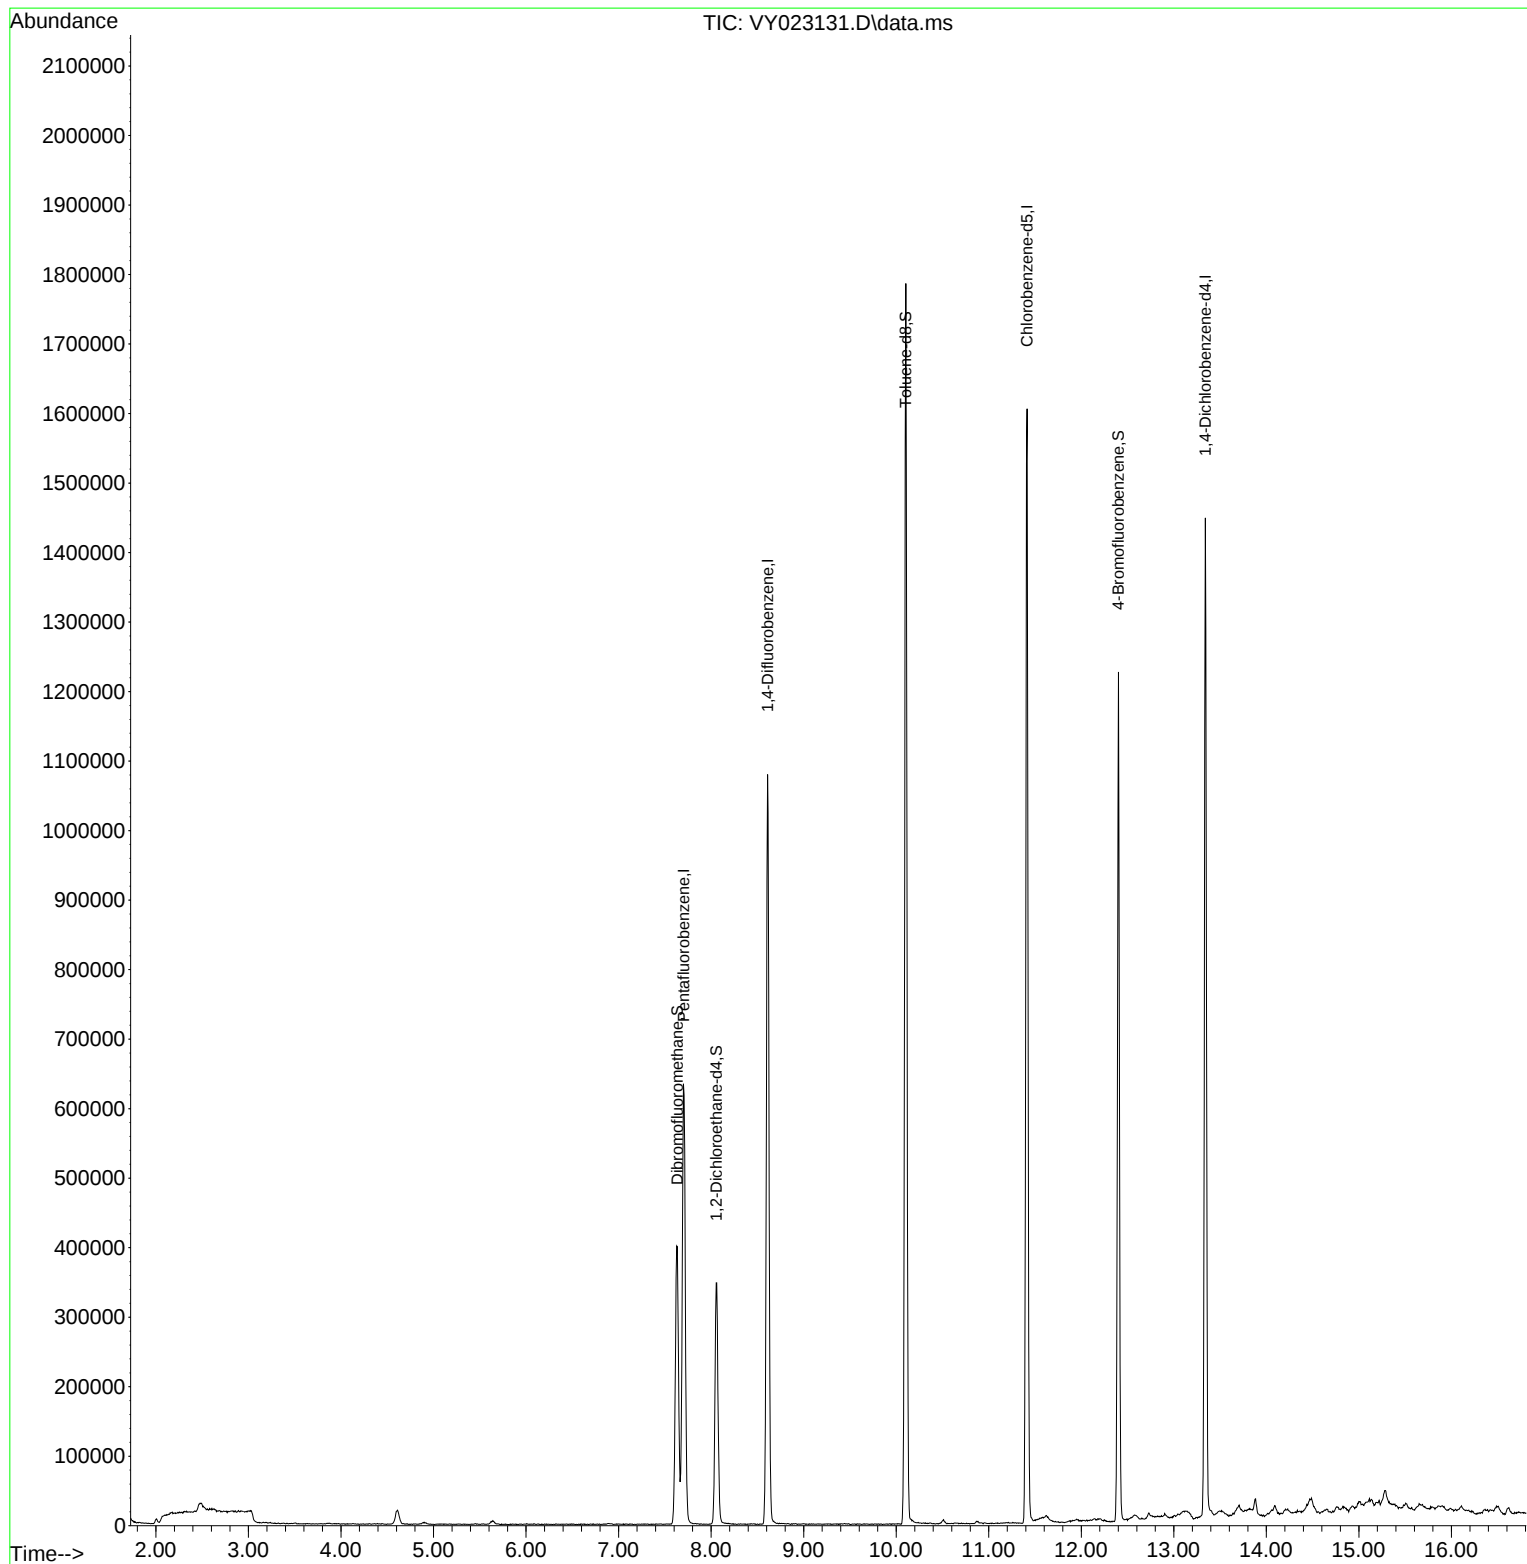


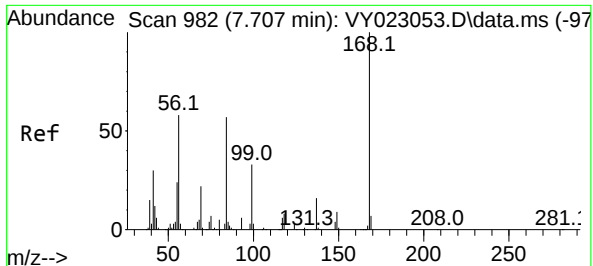

#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 7.701 min Scan# 91
Delta R.T. -0.006 min
Lab File: VY023131.D
Acq: 15 Aug 2025 17:33




Instrument :
MSVOA_Y
ClientSampleId :
VOC


Tgt Ion:168 Resp: 496911
Ion Ratio Lower Upper
168 100
99 54.2 42.8 64.2

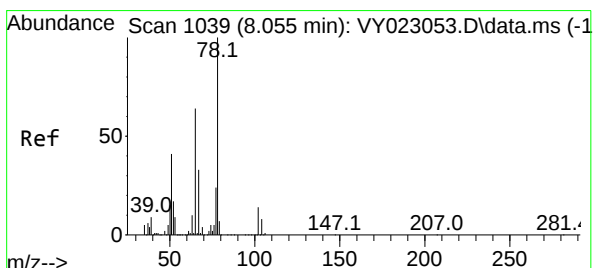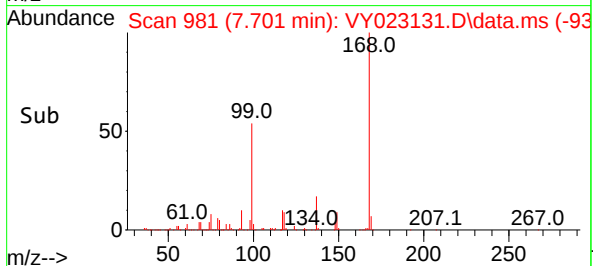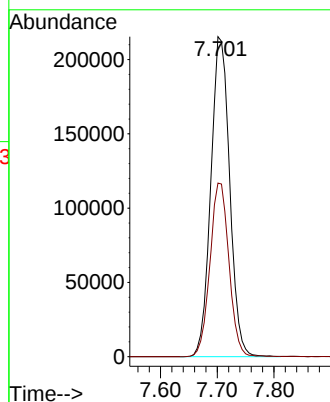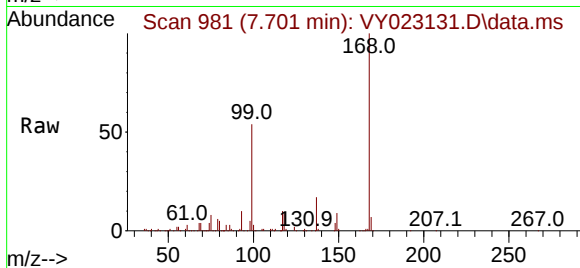

#33
1,2-Dichloroethane-d4
Concen: 58.485 ug/l
RT: 8.055 min Scan# 1039
Delta R.T. 0.000 min
Lab File: VY023131.D
Acq: 15 Aug 2025 17:33

Tgt Ion: 65 Resp: 276979
Ion Ratio Lower Upper
65 100
67 52.7 0.0 106.8

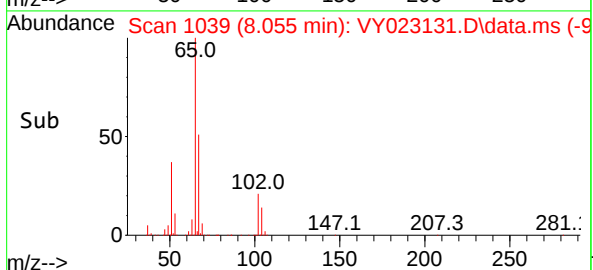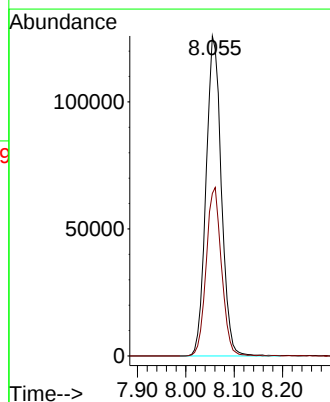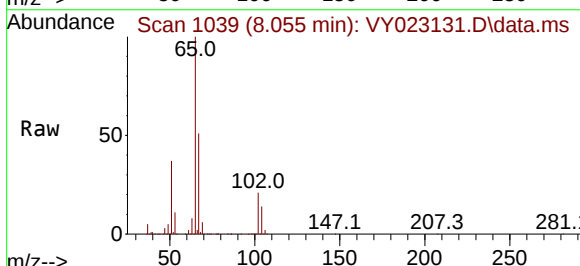

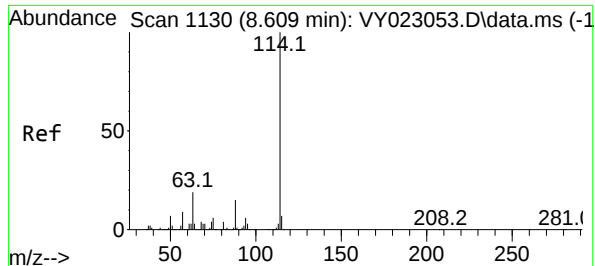

#34

1,4-Difluorobenzene

Concen: 50.000 ug/l

RT: 8.610 min Scan# 1130

Delta R.T. 0.000 min

Lab File: VY023131.D

Acq: 15 Aug 2025 17:33

Instrument :

MSVOA_Y

ClientSampleId :

VOC





Tgt Ion:114 Resp: 931727

Ion Ratio Lower Upper

114 100

63 19.7 0.0 38.4

88 14.6 0.0 30.0

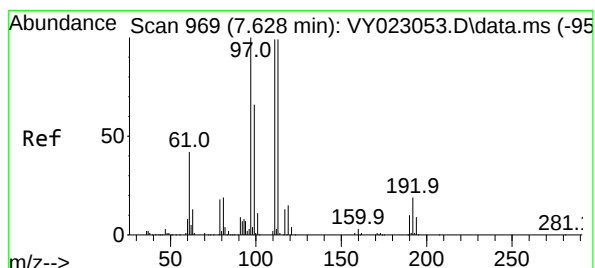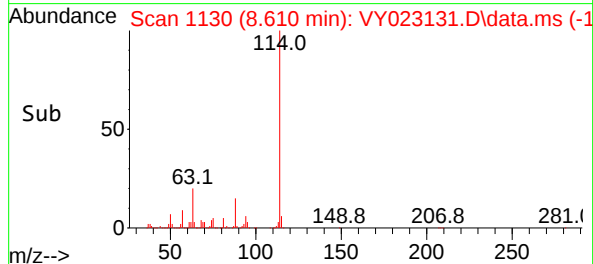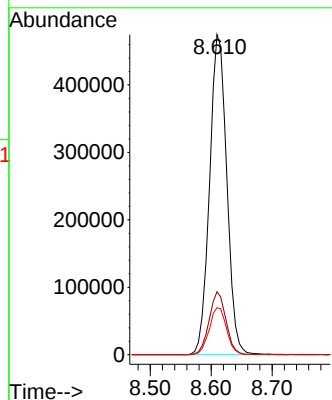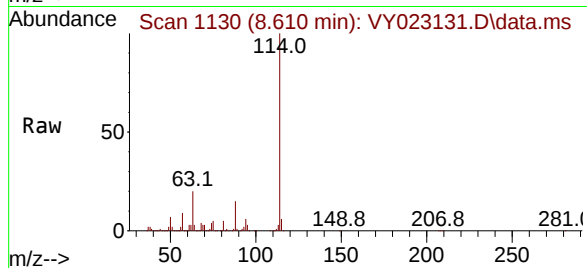

#35

Dibromofluoromethane

Concen: 51.919 ug/l

RT: 7.634 min Scan# 970

Delta R.T. 0.006 min

Lab File: VY023131.D

Acq: 15 Aug 2025 17:33




Tgt Ion:113 Resp: 289457


Ion Ratio Lower Upper

113 100

111 102.3 81.1 121.7

192 19.4 16.2 24.4


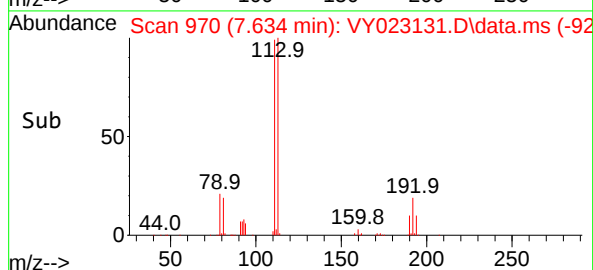
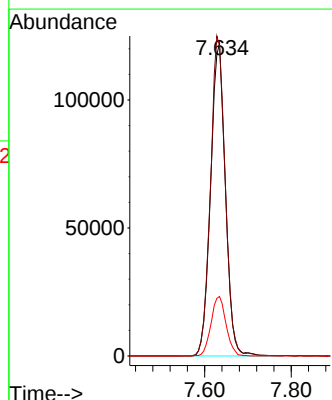
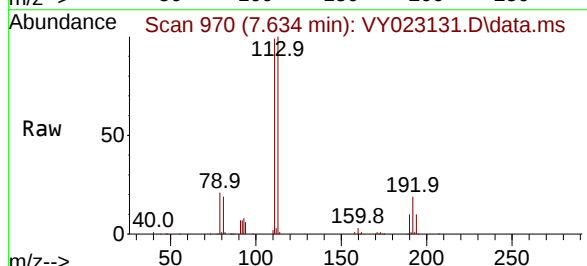


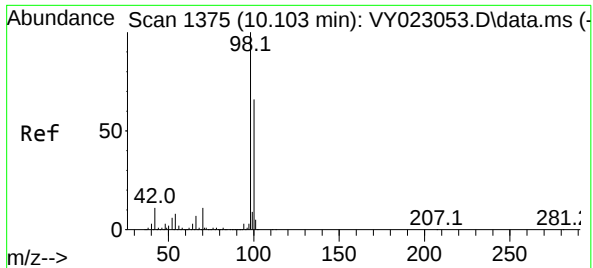

#50
Toluene-d8
Concen: 52.217 ug/l
RT: 10.103 min Scan# 11
Delta R.T. 0.000 min
Lab File: VY023131.D
Acq: 15 Aug 2025 17:33




Instrument :
MSVOA_Y
ClientSampleId :
VOC


Tgt Ion: 98 Resp: 1137267
Ion Ratio Lower Upper
98 100
100 65.3 52.3 78.5

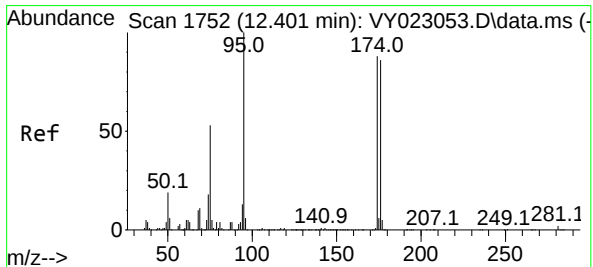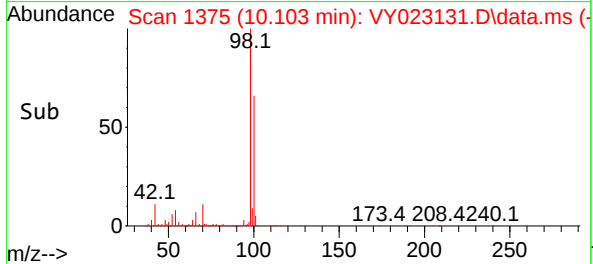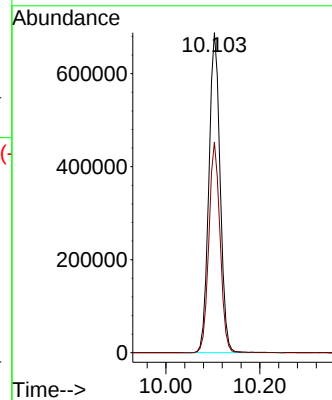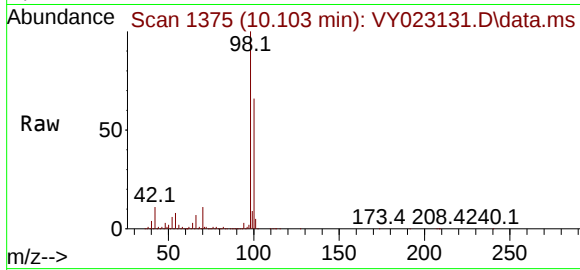

#62
4-Bromofluorobenzene
Concen: 49.857 ug/l
RT: 12.402 min Scan# 1752
Delta R.T. 0.000 min
Lab File: VY023131.D
Acq: 15 Aug 2025 17:33

Tgt Ion: 95 Resp: 349218
Ion Ratio Lower Upper
95 100
174 84.9 0.0 171.6
176 81.9 0.0 167.6


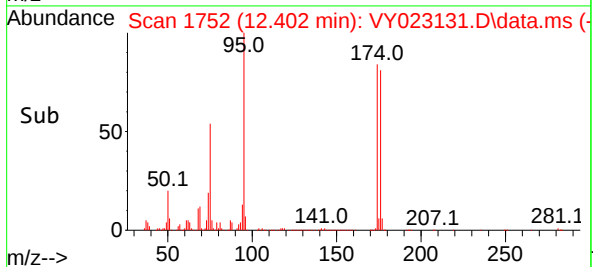
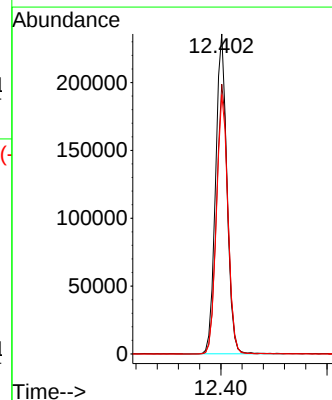
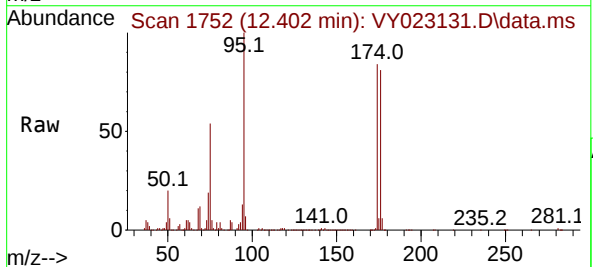


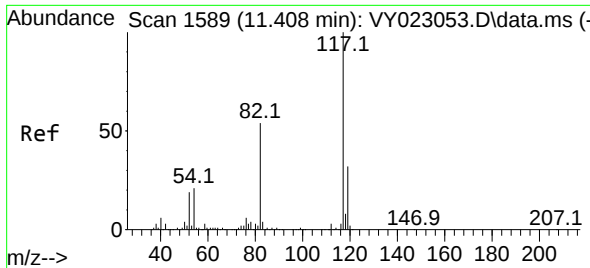

#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 11.414 min Scan# 11
Delta R.T. 0.006 min
Lab File: VY023131.D
Acq: 15 Aug 2025 17:33




Instrument :
MSVOA_Y
ClientSampleId :
VOC

Tgt Ion:117 Resp: 853505
Ion Ratio Lower Upper
117 100
82 52.1 43.4 65.0
119 31.7 25.6 38.4

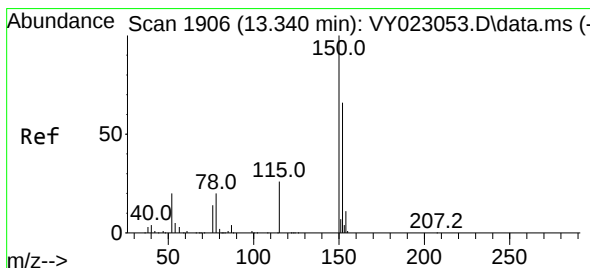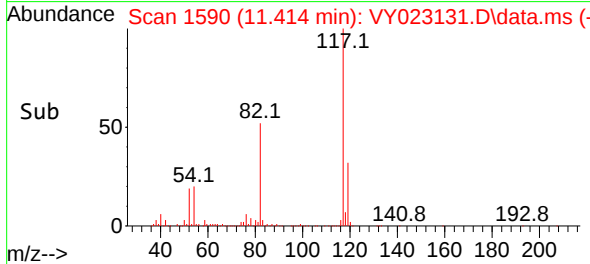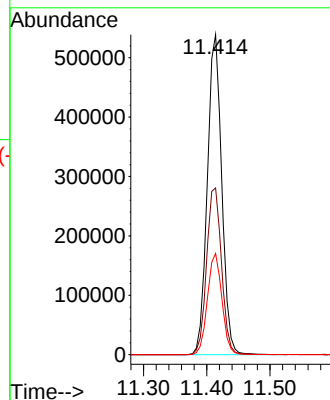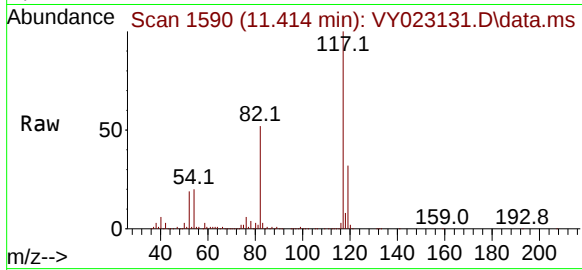

#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 13.340 min Scan# 1906
Delta R.T. 0.000 min
Lab File: VY023131.D
Acq: 15 Aug 2025 17:33

Tgt Ion:152 Resp: 359140
Ion Ratio Lower Upper
152 100
115 57.5 28.2 84.6
150 156.6 0.0 348.0

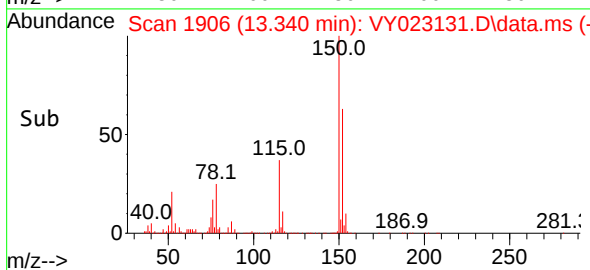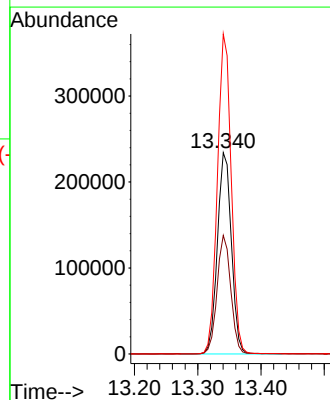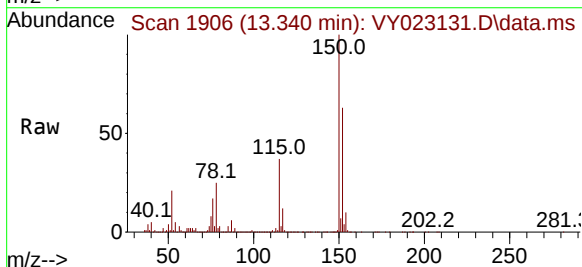

Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY081525\
 Data File : VY023131.D
 Acq On : 15 Aug 2025 17:33
 Operator : SY/MD
 Sample : Q2868-02
 Misc : 5.18g/5.0mL/MSVOA_Y/SOIL/A
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 MSVOA_Y
 ClientSampleId :
 VOC

Integration Parameters: RTEINT.P

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y081225S.M

Title : SW846 8260

Signal : TIC: VY023131.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	4.610	463	474	483	rBV2	19940	59062	1.98%	0.389%
2	7.628	959	969	975	rBV	400597	960637	32.20%	6.322%
3	7.701	975	981	997	rVB	632801	1462844	49.04%	9.627%
4	8.055	1028	1039	1054	rBV	347296	793836	26.61%	5.224%
5	8.610	1121	1130	1146	rBV	1078176	2124378	71.22%	13.980%
6	10.103	1367	1375	1384	rBV	1785086	2982997	100.00%	19.631%
7	11.414	1582	1590	1601	rBV	1603306	2599645	87.15%	17.108%
8	12.402	1744	1752	1762	rBV	1222338	1838349	61.63%	12.098%
9	12.572	1768	1780	1789	rBV	7807	35116	1.18%	0.231%
10	13.340	1899	1906	1921	rBV	1435734	2199363	73.73%	14.474%
11	13.706	1957	1966	1973	rBV	13050	41798	1.40%	0.275%
12	13.883	1990	1995	2003	rVB2	23989	48811	1.64%	0.321%
13	15.279	2220	2224	2234	rVB6	19278	48752	1.63%	0.321%


Sum of corrected areas: 15195588

Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY081525\
Data File : VY023131.D
Acq On : 15 Aug 2025 17:33
Operator : SY/MD
Sample : Q2868-02
Misc : 5.18g/5.0mL/MSVOA_Y/SOIL/A
ALS Vial : 23 Sample Multiplier: 1

Instrument :
MSVOA_Y
ClientSampleId :
VOC

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y081225S.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

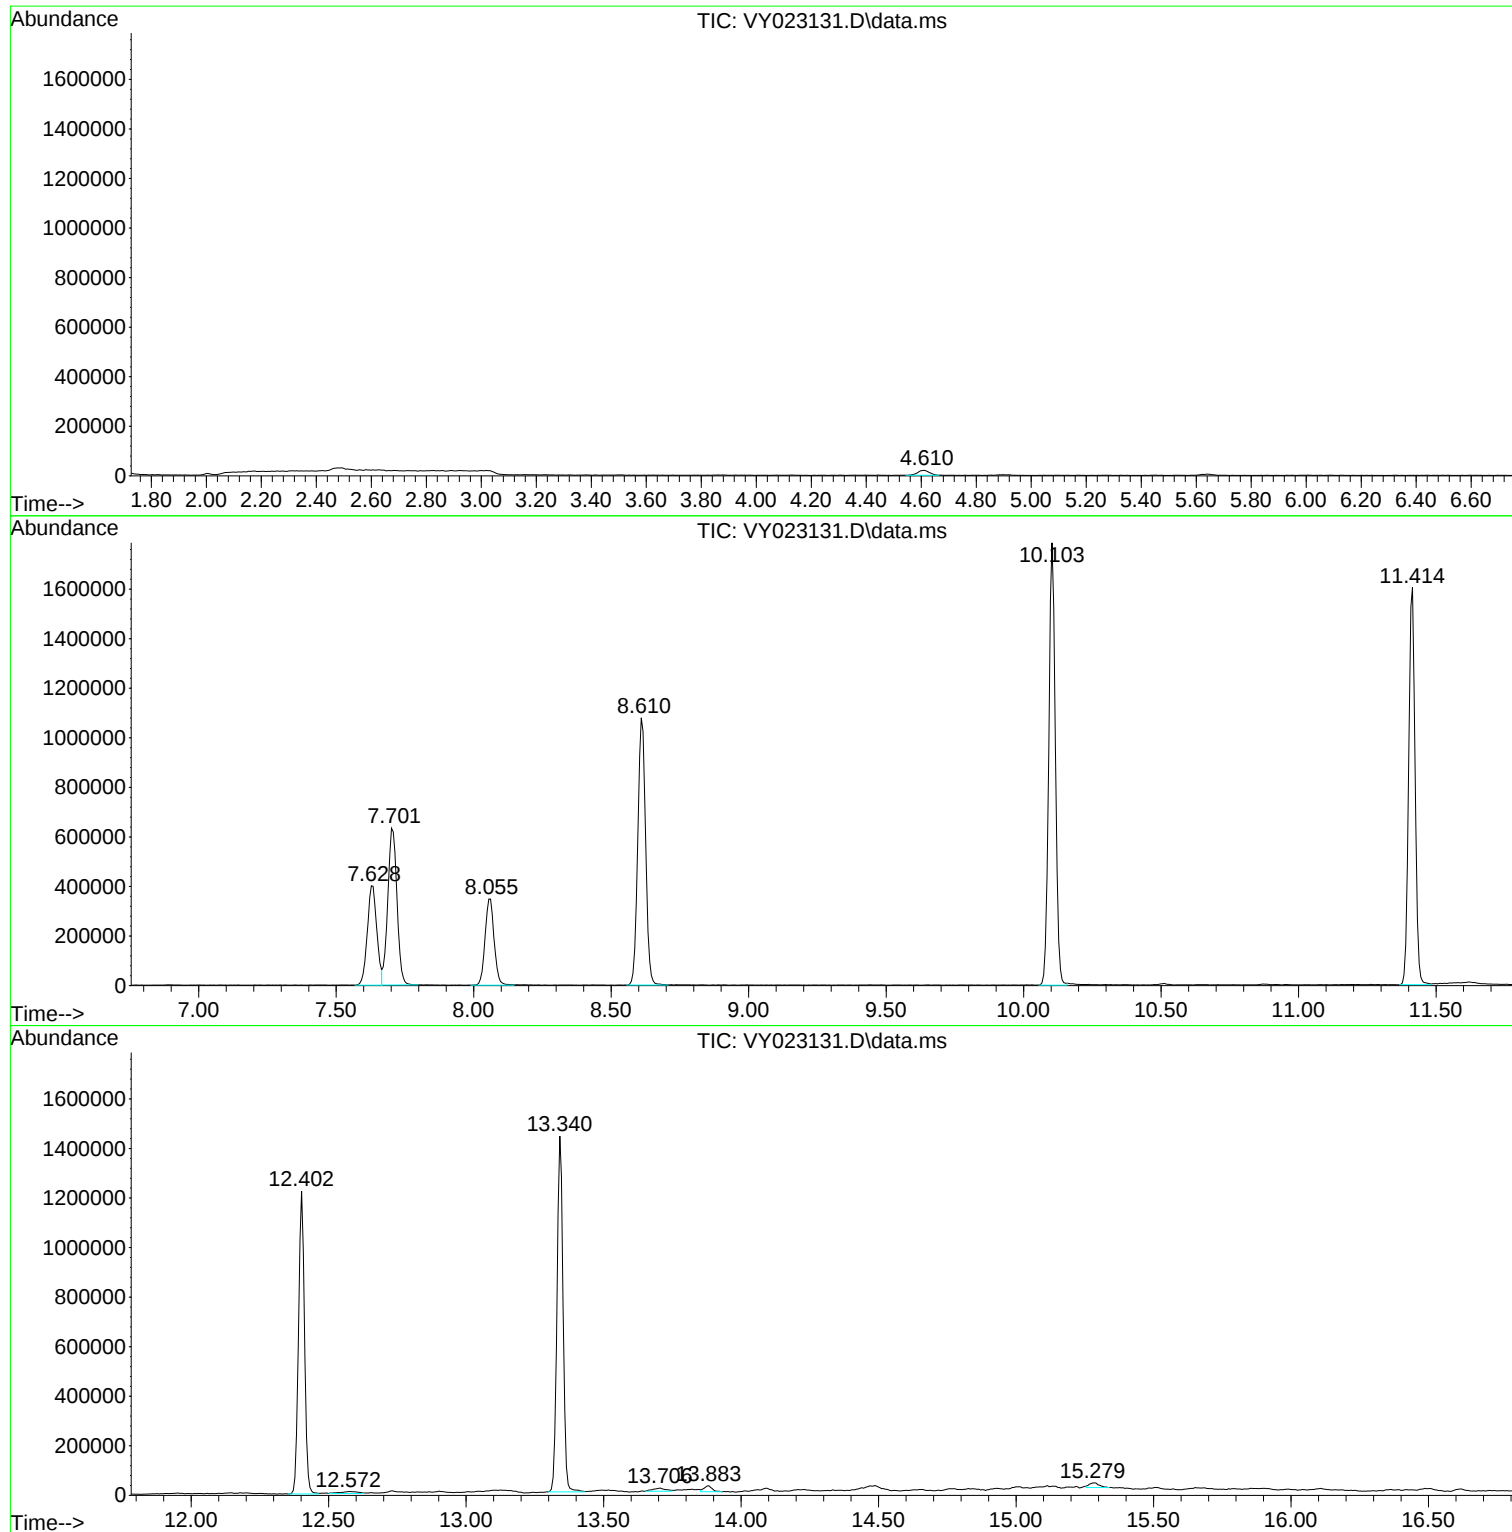

Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY081525\
Data File : VY023131.D
Acq On : 15 Aug 2025 17:33
Operator : SY/MD
Sample : Q2868-02
Misc : 5.18g/5.0mL/MSVOA_Y/SOIL/A
ALS Vial : 23 Sample Multiplier: 1

Instrument :
MSVOA_Y
ClientSampleId :
VOC

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y081225S.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY081525\
Data File : VY023131.D
Acq On : 15 Aug 2025 17:33
Operator : SY/MD
Sample : Q2868-02
Misc : 5.18g/5.0mL/MSVOA_Y/SOIL/A
ALS Vial : 23 Sample Multiplier: 1

Instrument :
MSVOA_Y
ClientSampleId :
VOC

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y081225S.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc



CALIBRATION SUMMARY



284 Sheffield Street, Mountainside, New Jersey 07092, Phone : 908 789 8900,
Fax : 908 789 8922

VOLATILE ORGANICS INITIAL CALIBRATION DATA

Lab Name: Alliance

Contract: SCIA01

Lab Code: ACE

SDG No.: Q2868

Instrument ID: MSVOA_Y

Calibration Date(s): 08/12/2025 08/12/2025

Heated Purge: (Y/N) Y

Calibration Time(s): 14:54 16:47

GC Column: RXI-624 ID: 0.25 (mm)

LAB FILE ID:		RRF005 = VY023050.D		RRF010 = VY023051.D		RRF020 = VY023052.D			
		RRF050 = VY023053.D		RRF100 = VY023054.D		RRF150 = VY023055.D			
COMPOUND	RRF005	RRF010	RRF020	RRF050	RRF100	RRF150	RRF	% RSD	
Dichlorodifluoromethane	0.487	0.463	0.460	0.348	0.337	0.354	0.408	16.8	
Chloromethane	0.699	0.707	0.736	0.607	0.603	0.613	0.661	9	
Vinyl Chloride	0.868	0.870	0.875	0.769	0.754	0.766	0.817	7.3	
Bromomethane	0.673	0.638	0.653	0.540	0.576	0.581	0.610	8.5	
Chloroethane	0.585	0.567	0.569	0.515	0.508	0.516	0.543	6.2	
Trichlorofluoromethane	1.059	1.044	1.048	0.937	0.900	0.974	0.994	6.7	
1,1,2-Trichlorotrifluoroethane	0.522	0.519	0.521	0.462	0.445	0.472	0.490	7	
1,1-Dichloroethene	0.492	0.505	0.502	0.463	0.454	0.475	0.482	4.4	
Acetone	0.110	0.111	0.106	0.103	0.094	0.096	0.103	6.9	
Carbon Disulfide	1.656	1.663	1.662	1.491	1.453	1.501	1.571	6.3	
Methyl tert-butyl Ether	1.181	1.268	1.296	1.236	1.202	1.308	1.249	4.1	
Methyl Acetate	0.299	0.308	0.325	0.322	0.280	0.309	0.307	5.4	
Methylene Chloride	0.861	0.706	0.606	0.510	0.511	0.524	0.620	22.7	
trans-1,2-Dichloroethene	0.535	0.561	0.559	0.523	0.520	0.550	0.541	3.3	
1,1-Dichloroethane	0.929	0.969	0.984	0.918	0.907	0.945	0.942	3.1	
Cyclohexane	1.040	0.934	0.905	0.816	0.792	0.838	0.888	10.4	
2-Butanone	0.135	0.152	0.143	0.142	0.129	0.142	0.140	5.5	
Carbon Tetrachloride	0.490	0.486	0.505	0.466	0.466	0.484	0.483	3.1	
cis-1,2-Dichloroethene	0.621	0.624	0.645	0.607	0.610	0.648	0.626	2.8	
Bromochloromethane	0.367	0.379	0.393	0.365	0.367	0.371	0.374	2.9	
Chloroform	0.969	0.997	1.002	0.943	0.936	0.981	0.971	2.8	
1,1,1-Trichloroethane	0.862	0.877	0.899	0.837	0.833	0.864	0.862	2.8	
Methylcyclohexane	0.574	0.579	0.605	0.566	0.575	0.614	0.586	3.3	
Benzene	1.354	1.375	1.430	1.334	1.334	1.395	1.370	2.8	
1,2-Dichloroethane	0.353	0.370	0.371	0.347	0.339	0.359	0.356	3.6	
Trichloroethene	0.354	0.355	0.373	0.341	0.342	0.359	0.354	3.3	
1,2-Dichloropropane	0.303	0.321	0.326	0.309	0.309	0.325	0.315	3.1	
Bromodichloromethane	0.446	0.464	0.489	0.459	0.456	0.481	0.466	3.5	
4-Methyl-2-Pentanone	0.168	0.201	0.200	0.199	0.190	0.211	0.195	7.7	
Toluene	0.817	0.851	0.902	0.858	0.873	0.921	0.870	4.3	

* Compounds with required minimum RRF and maximum %RSD values.
All other compounds must meet a minimum RRF of 0.010.
RRF of 1,4-Dioxane = Value should be divide by 1000.



284 Sheffield Street, Mountainside, New Jersey 07092, Phone : 908 789 8900,
Fax : 908 789 8922

VOLATILE ORGANICS INITIAL CALIBRATION DATA

Lab Name: Alliance Contract: SCIA01
 Lab Code: ACE SDG No.: Q2868
 Instrument ID: MSVOA_Y Calibration Date(s): 08/12/2025 08/12/2025
 Heated Purge: (Y/N) Y Calibration Time(s): 14:54 16:47
 GC Column: RXI-624 ID: 0.25 (mm)

LAB FILE ID:		RRF005 = VY023050.D		RRF010 = VY023051.D		RRF020 = VY023052.D			
		RRF050 = VY023053.D		RRF100 = VY023054.D		RRF150 = VY023055.D			
COMPOUND	RRF005	RRF010	RRF020	RRF050	RRF100	RRF150	RRF	% RSD	
t-1,3-Dichloropropene	0.377	0.410	0.435	0.420	0.428	0.459	0.422	6.5	
cis-1,3-Dichloropropene	0.457	0.486	0.513	0.496	0.500	0.540	0.499	5.5	
1,1,2-Trichloroethane	0.230	0.242	0.253	0.239	0.236	0.254	0.242	4	
2-Hexanone	0.112	0.134	0.137	0.136	0.131	0.146	0.133	8.6	
Dibromochloromethane	0.300	0.317	0.326	0.318	0.316	0.340	0.320	4.1	
1,2-Dibromoethane	0.206	0.232	0.237	0.226	0.222	0.242	0.228	5.6	
Tetrachloroethene	0.477	0.463	0.475	0.435	0.393	0.437	0.446	7.2	
Chlorobenzene	1.062	1.070	1.116	1.055	1.057	1.111	1.079	2.6	
Ethyl Benzene	1.775	1.795	1.894	1.859	1.858	1.956	1.856	3.6	
m/p-Xylenes	0.676	0.699	0.745	0.718	0.737	0.774	0.725	4.8	
o-Xylene	0.605	0.643	0.696	0.686	0.702	0.742	0.679	7.1	
Styrene	0.945	1.023	1.140	1.123	1.176	1.254	1.110	10	
Bromoform	0.197	0.213	0.216	0.214	0.213	0.231	0.214	5	
Isopropylbenzene	3.420	3.483	3.602	3.505	3.514	3.650	3.529	2.4	
1,1,2,2-Tetrachloroethane	0.584	0.647	0.605	0.585	0.581	0.613	0.603	4.2	
1,3-Dichlorobenzene	1.600	1.642	1.701	1.610	1.656	1.752	1.660	3.5	
1,4-Dichlorobenzene	1.687	1.657	1.680	1.601	1.597	1.660	1.647	2.3	
1,2-Dichlorobenzene	1.410	1.472	1.496	1.420	1.438	1.499	1.456	2.7	
1,2-Dibromo-3-Chloropropane	0.093	0.096	0.094	0.095	0.086	0.098	0.094	4.3	
1,2,4-Trichlorobenzene	0.788	0.839	0.881	0.847	0.856	0.955	0.861	6.4	
1,2,3-Trichlorobenzene	0.685	0.733	0.752	0.720	0.727	0.834	0.742	6.7	
1,2-Dichloroethane-d4	0.491	0.490	0.482	0.462	0.472	0.462	0.477	2.7	
Dibromofluoromethane	0.290	0.299	0.301	0.293	0.307	0.305	0.299	2.1	
Toluene-d8	1.151	1.157	1.173	1.143	1.202	1.186	1.169	1.9	
4-Bromofluorobenzene	0.358	0.367	0.367	0.370	0.399	0.394	0.376	4.4	

* Compounds with required minimum RRF and maximum %RSD values.
 All other compounds must meet a minimum RRF of 0.010.
 RRF of 1,4-Dioxane = Value should be divide by 1000.

Method Path : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\
 Method File : 82Y081225S.M
 Title : SW846 8260
 Last Update : Wed Aug 13 02:10:11 2025
 Response Via : Initial Calibration

Calibration Files

5 =VY023050.D 10 =VY023051.D 20 =VY023052.D 50 =VY023053.D 100 =VY023054.D 150 =VY023055.D

	Compound	5	10	20	50	100	150	Avg	%RSD
1) I	Pentafluorobenzene	-----ISTD-----							
2) T	Dichlorodifluo...	0.487	0.463	0.460	0.348	0.337	0.354	0.408	16.79
3) P	Chloromethane	0.699	0.707	0.736	0.607	0.603	0.613	0.661	9.01
4) C	Vinyl Chloride	0.868	0.870	0.875	0.769	0.754	0.766	0.817	7.29#
5) T	Bromomethane	0.673	0.638	0.653	0.540	0.576	0.581	0.610	8.52
6) T	Chloroethane	0.585	0.567	0.569	0.515	0.508	0.516	0.543	6.19
7) T	Trichlorofluor...	1.059	1.044	1.048	0.937	0.900	0.974	0.994	6.68
8) T	Diethyl Ether	0.271	0.276	0.271	0.251	0.245	0.264	0.263	4.69
9) T	1,1,2-Trichlor...	0.522	0.519	0.521	0.462	0.445	0.472	0.490	7.01
10) T	Methyl Iodide	0.468	0.491	0.539	0.549	0.564	0.563	0.529	7.57
11) T	Tert butyl alc...	0.033	0.037	0.033	0.032	0.029	0.033	0.033	7.44
12) CM	1,1-Dichloroet...	0.492	0.505	0.502	0.463	0.454	0.475	0.482	4.38#
13) T	Acrolein	0.048	0.055	0.050	0.045	0.043	0.046	0.048	8.57
14) T	Allyl chloride	0.734	0.718	0.724	0.686	0.681	0.712	0.709	3.01
15) T	Acrylonitrile	0.101	0.114	0.112	0.106	0.100	0.109	0.107	5.51
16) T	Acetone	0.110	0.111	0.106	0.103	0.094	0.096	0.103	6.89
17) T	Carbon Disulfide	1.656	1.663	1.662	1.491	1.453	1.501	1.571	6.30
18) T	Methyl Acetate	0.299	0.308	0.325	0.322	0.280	0.309	0.307	5.37
19) T	Methyl tert-bu...	1.181	1.268	1.296	1.236	1.202	1.308	1.249	4.09
20) T	Methylene Chlo...	0.861	0.706	0.606	0.510	0.511	0.524	0.620	22.69
21) T	trans-1,2-Dich...	0.535	0.561	0.559	0.523	0.520	0.550	0.541	3.28
22) T	Diisopropyl ether	1.442	1.565	1.609	1.512	1.510	1.605	1.541	4.21
23) T	Vinyl Acetate	0.790	0.875	0.875	0.841	0.830	0.899	0.852	4.62
24) P	1,1-Dichloroet...	0.929	0.969	0.984	0.918	0.907	0.945	0.942	3.15
25) T	2-Butanone	0.135	0.152	0.143	0.142	0.129	0.142	0.140	5.51
26) T	2,2-Dichloropr...	0.837	0.830	0.844	0.790	0.776	0.800	0.813	3.43
27) T	cis-1,2-Dichlo...	0.621	0.624	0.645	0.607	0.610	0.648	0.626	2.77
28) T	Bromochloromet...	0.367	0.379	0.393	0.365	0.367	0.371	0.374	2.88
29) T	Tetrahydrofuran	0.084	0.091	0.089	0.087	0.081	0.091	0.087	4.62
30) C	Chloroform	0.969	0.997	1.002	0.943	0.936	0.981	0.971	2.81#
31) T	Cyclohexane	1.040	0.934	0.905	0.816	0.792	0.838	0.888	10.35
32) T	1,1,1-Trichlor...	0.862	0.877	0.899	0.837	0.833	0.864	0.862	2.85
33) S	1,2-Dichloroet...	0.491	0.490	0.482	0.462	0.472	0.462	0.477	2.74
34) I	1,4-Difluorobenzene	-----ISTD-----							
35) S	Dibromofluorom...	0.290	0.299	0.301	0.293	0.307	0.305	0.299	2.14
36) T	1,1-Dichloropr...	0.442	0.455	0.461	0.433	0.429	0.447	0.445	2.81
37) T	Ethyl Acetate	0.167	0.197	0.196	0.188	0.178	0.195	0.187	6.52
38) T	Carbon Tetrach...	0.490	0.486	0.505	0.466	0.466	0.484	0.483	3.08
39) T	Methylcyclohexane	0.574	0.579	0.605	0.566	0.575	0.614	0.586	3.35
40) TM	Benzene	1.354	1.375	1.430	1.334	1.334	1.395	1.370	2.76
41) T	Methacrylonitrile	0.113	0.107	0.111	0.110	0.102	0.103	0.108	4.05
42) TM	1,2-Dichloroet...	0.353	0.370	0.371	0.347	0.339	0.359	0.356	3.59
43) T	Isopropyl Acetate	0.352	0.383	0.388	0.373	0.362	0.407	0.378	5.16
44) TM	Trichloroethene	0.354	0.355	0.373	0.341	0.342	0.359	0.354	3.35
45) C	1,2-Dichloropr...	0.303	0.321	0.326	0.309	0.309	0.325	0.315	3.08#
46) T	Dibromomethane	0.166	0.189	0.187	0.178	0.176	0.190	0.181	5.14
47) T	Bromodichlorom...	0.446	0.464	0.489	0.459	0.456	0.481	0.466	3.47
48) T	Methyl methacr...	0.149	0.180	0.189	0.188	0.182	0.196	0.181	9.18
49) T	1,4-Dioxane	0.002	0.002	0.002	0.002	0.002	0.002	0.002	6.71
50) S	Toluene-d8	1.151	1.157	1.173	1.143	1.202	1.186	1.169	1.92
51) T	4-Methyl-2-Pen...	0.168	0.201	0.200	0.199	0.190	0.211	0.195	7.67
52) CM	Toluene	0.817	0.851	0.902	0.858	0.873	0.921	0.870	4.28#
53) T	t-1,3-Dichloro...	0.377	0.410	0.435	0.420	0.428	0.459	0.422	6.47
54) T	cis-1,3-Dichlo...	0.457	0.486	0.513	0.496	0.500	0.540	0.499	5.54
55) T	1,1,2-Trichlor...	0.230	0.242	0.253	0.239	0.236	0.254	0.242	3.96
56) T	Ethyl methacry...	0.247	0.298	0.312	0.320	0.323	0.359	0.310	11.84


Method Path : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\
 Method File : 82Y081225S.M

57)	T	1,3-Dichloropr...	0.385	0.421	0.429	0.405	0.395	0.429	0.411	4.52
58)	T	2-Chloroethyl ...	0.114	0.135	0.144	0.155	0.158	0.171	0.146	13.68
59)	T	2-Hexanone	0.112	0.134	0.137	0.136	0.131	0.146	0.133	8.57
60)	T	Dibromochlorom...	0.300	0.317	0.326	0.318	0.316	0.340	0.320	4.09
61)	T	1,2-Dibromoethane	0.206	0.232	0.237	0.226	0.222	0.242	0.228	5.60
62)	S	4-Bromofluorob...	0.358	0.367	0.367	0.370	0.399	0.394	0.376	4.41
63)	I	Chlorobenzene-d5	-----ISTD-----							
64)	T	Tetrachloroethene	0.477	0.463	0.475	0.435	0.393	0.437	0.446	7.16
65)	PM	Chlorobenzene	1.062	1.070	1.116	1.055	1.057	1.111	1.079	2.55
66)	T	1,1,1,2-Tetrac...	0.347	0.360	0.378	0.362	0.365	0.384	0.366	3.58
67)	C	Ethyl Benzene	1.775	1.795	1.894	1.859	1.858	1.956	1.856	3.56#
68)	T	m/p-Xylenes	0.676	0.699	0.745	0.718	0.737	0.774	0.725	4.80
69)	T	o-Xylene	0.605	0.643	0.696	0.686	0.702	0.742	0.679	7.13
70)	T	Styrene	0.945	1.023	1.140	1.123	1.176	1.254	1.110	9.96
71)	P	Bromoform	0.197	0.213	0.216	0.214	0.213	0.231	0.214	5.03
72)	I	1,4-Dichlorobenzen...	-----ISTD-----							
73)	T	Isopropylbenzene	3.420	3.483	3.602	3.505	3.514	3.650	3.529	2.36
74)	T	N-amyl acetate	0.633	0.738	0.757	0.767	0.756	0.840	0.748	8.89
75)	P	1,1,2,2-Tetrac...	0.584	0.647	0.605	0.585	0.581	0.613	0.603	4.20
76)	T	1,2,3-Trichlor...	0.551	0.483	0.472	0.535	0.409	0.444	0.483	11.18
77)	T	Bromobenzene	0.824	0.830	0.866	0.828	0.831	0.873	0.842	2.58
78)	T	n-propylbenzene	4.052	4.149	4.317	4.217	4.158	4.315	4.201	2.46
79)	T	2-Chlorotoluene	2.349	2.398	2.464	2.382	2.390	2.461	2.407	1.90
80)	T	1,3,5-Trimethy...	2.672	2.811	2.932	2.859	2.872	2.966	2.852	3.64
81)	T	trans-1,4-Dich...	0.181	0.215	0.203	0.197	0.190	0.210	0.199	6.43
82)	T	4-Chlorotoluene	2.427	2.486	2.600	2.462	2.460	2.548	2.497	2.59
83)	T	tert-Butylbenzene	2.428	2.481	2.626	2.588	2.630	2.702	2.576	3.98
84)	T	1,2,4-Trimethy...	2.596	2.760	2.955	2.837	2.894	2.993	2.839	5.12
85)	T	sec-Butylbenzene	3.637	3.749	3.881	3.773	3.781	3.882	3.784	2.42
86)	T	p-Isopropyltol...	2.878	2.978	3.241	3.167	3.230	3.350	3.141	5.66
87)	T	1,3-Dichlorobe...	1.600	1.642	1.701	1.610	1.656	1.752	1.660	3.46
88)	T	1,4-Dichlorobe...	1.687	1.657	1.680	1.601	1.597	1.660	1.647	2.35
89)	T	n-Butylbenzene	2.625	2.809	2.972	2.911	2.933	3.059	2.885	5.24
90)	T	Hexachloroethane	0.638	0.648	0.650	0.630	0.632	0.660	0.643	1.83
91)	T	1,2-Dichlorobe...	1.410	1.472	1.496	1.420	1.438	1.499	1.456	2.65
92)	T	1,2-Dibromo-3-...	0.093	0.096	0.094	0.095	0.086	0.098	0.094	4.27
93)	T	1,2,4-Trichlor...	0.788	0.839	0.881	0.847	0.856	0.955	0.861	6.43
94)	T	Hexachlorobuta...	0.533	0.506	0.522	0.491	0.480	0.504	0.506	3.85
95)	T	Naphthalene	1.204	1.364	1.462	1.488	1.500	1.791	1.468	13.14
96)	T	1,2,3-Trichlor...	0.685	0.733	0.752	0.720	0.727	0.834	0.742	6.73

(#) = Out of Range

Methylene Chloride

Response Ratio

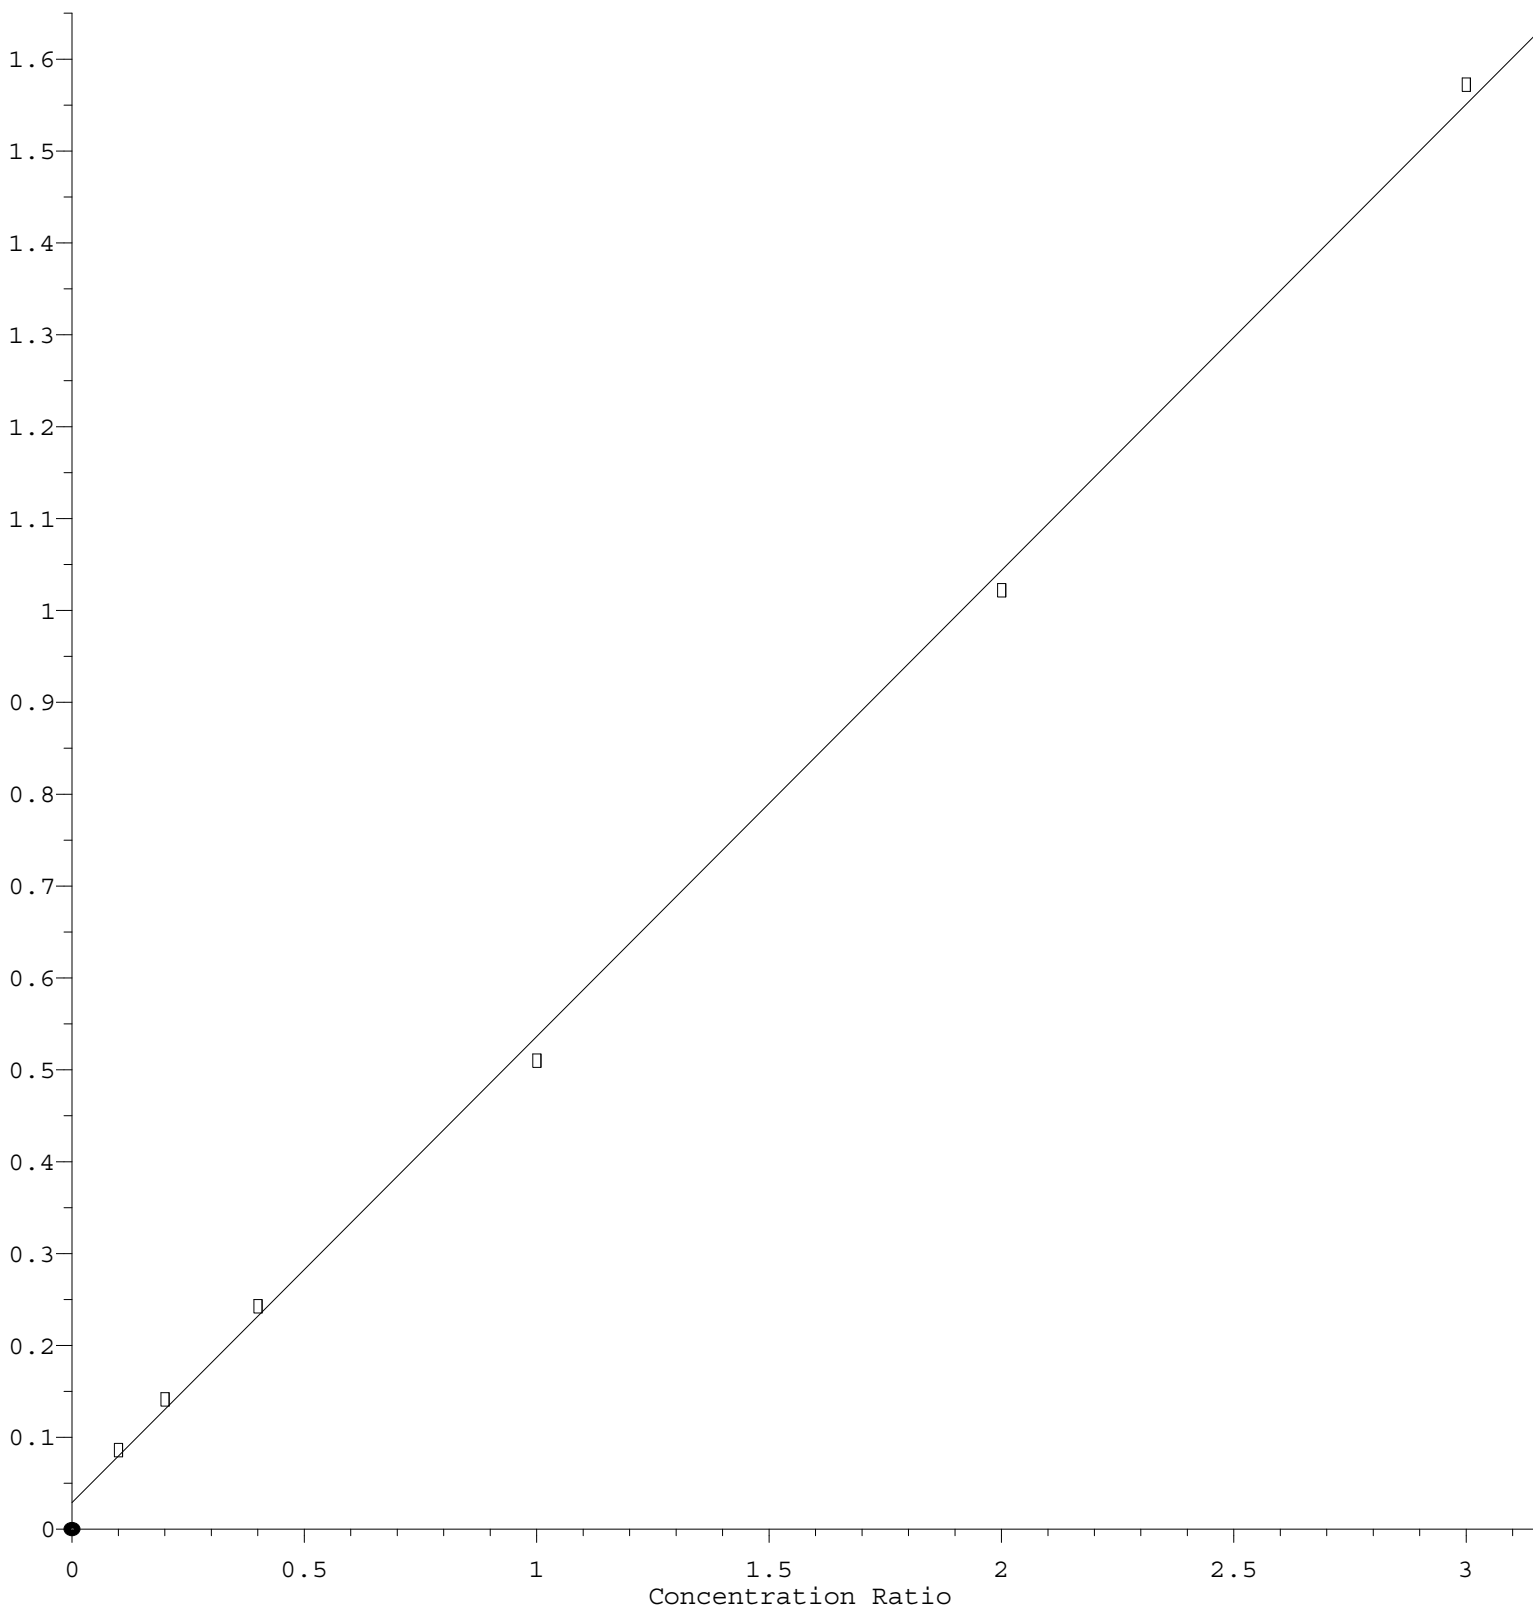

$$\text{Response} = 5.073\text{e-}001 * \text{Amt} + 2.916\text{e-}002$$

Coef of Det (r^2) = 0.998910 Curve Fit: Linear

Method Name: Z:\voasrv\HPCHEM1\MSVOA Y\methods\82Y081225S.M

Calibration Table Last Updated: Wed Aug 13 02:10:11 2025

Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY081225\
 Data File : VY023050.D
 Acq On : 12 Aug 2025 14:54
 Operator : SY/MD
 Sample : VSTDICC005
 Misc : 5.00g/5.0mL/MSVOA_Y/SOIL
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 MSVOA_Y
 ClientSampleId :
 VSTDICC005

Manual Integrations
 APPROVED

Reviewed By :Mahesh Dadoda 08/14/2025
 Supervised By :Semsettin Yesilyurt 08/14/2025

Quant Time: Aug 13 01:50:18 2025
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y081225S.M
 Quant Title : SW846 8260
 QLast Update : Wed Aug 13 01:46:43 2025
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Pentafluorobenzene	7.707	168	561390	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	8.610	114	904866	50.000	ug/l	0.00
63) Chlorobenzene-d5	11.414	117	759914	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.340	152	360397	50.000	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	8.055	65	27563	5.152	ug/l	0.00
Spiked Amount 50.000	Range 50 - 163		Recovery =	10.300%#		
35) Dibromofluoromethane	7.634	113	26265	4.851	ug/l	0.00
Spiked Amount 50.000	Range 54 - 147		Recovery =	9.700%#		
50) Toluene-d8	10.103	98	104144	4.924	ug/l	0.00
Spiked Amount 50.000	Range 58 - 134		Recovery =	9.840%#		
62) 4-Bromofluorobenzene	12.402	95	32420	4.766	ug/l	0.00
Spiked Amount 50.000	Range 30 - 143		Recovery =	9.540%#		
Target Compounds					Qvalue	
2) Dichlorodifluoromethane	1.861	85	27351	5.969	ug/l	96
3) Chloromethane	2.068	50	39269	5.291	ug/l	98
4) Vinyl Chloride	2.202	62	48736	5.312	ug/l	99
5) Bromomethane	2.592	94	37773	5.513	ug/l	97
6) Chloroethane	2.732	64	32816	5.380	ug/l	98
7) Trichlorofluoromethane	3.050	101	59438	5.328	ug/l	99
8) Diethyl Ether	3.452	74	15231	5.160	ug/l	99
9) 1,1,2-Trichlorotrifluo...	3.812	101	29291	5.322	ug/l	98
10) Methyl Iodide	3.994	142	26272	4.424	ug/l	98
11) Tert butyl alcohol	4.866	59	9219	25.147	ug/l #	92
12) 1,1-Dichloroethene	3.787	96	27635	5.108	ug/l	87
13) Acrolein	3.647	56	13391	24.941	ug/l	95
14) Allyl chloride	4.372	41	41201	5.176	ug/l	94
15) Acrylonitrile	5.061	53	28255	23.547	ug/l	95
16) Acetone	3.866	43	30803	26.574	ug/l	98
17) Carbon Disulfide	4.098	76	92964	5.270	ug/l	96
18) Methyl Acetate	4.379	43	16806	4.872	ug/l	99
19) Methyl tert-butyl Ether	5.116	73	66308	4.730	ug/l	98
20) Methylene Chloride	4.604	84	48322	5.657	ug/l	97
21) trans-1,2-Dichloroethene	5.110	96	30021	4.938	ug/l	97
22) Diisopropyl ether	6.012	45	80938	4.679	ug/l	91
23) Vinyl Acetate	5.958	43	221862	23.196	ug/l	97
24) 1,1-Dichloroethane	5.909	63	52152	4.931	ug/l	99
25) 2-Butanone	6.890	43	37821	23.991	ug/l	97
26) 2,2-Dichloropropane	6.878	77	46964	5.147	ug/l	99
27) cis-1,2-Dichloroethene	6.884	96	34877	4.962	ug/l	97
28) Bromochloromethane	7.238	49	20615	4.913	ug/l	96
29) Tetrahydrofuran	7.256	42	23487	24.035	ug/l	96
30) Chloroform	7.415	83	54392	4.987	ug/l	96
31) Cyclohexane	7.701	56	58362	5.856	ug/l #	83
32) 1,1,1-Trichloroethane	7.610	97	48413	5.003	ug/l	99
36) 1,1-Dichloropropene	7.829	75	39978	4.968	ug/l	99
37) Ethyl Acetate	6.982	43	15080	4.461	ug/l #	95
38) Carbon Tetrachloride	7.811	117	44360	5.076	ug/l	99
39) Methylcyclohexane	9.103	83	51931	4.901	ug/l	99
40) Benzene	8.073	78	122482	4.939	ug/l	99

Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY081225\
 Data File : VY023050.D
 Acq On : 12 Aug 2025 14:54
 Operator : SY/MD
 Sample : VSTDICC005
 Misc : 5.00g/5.0mL/MSVOA_Y/SOIL
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 MSVOA_Y
 ClientSampleId :
 VSTDICC005

Manual Integrations
 APPROVED

Reviewed By :Mahesh Dadoda 08/14/2025
 Supervised By :Semsettin Yesilyurt 08/14/2025

Quant Time: Aug 13 01:50:18 2025
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y081225S.M
 Quant Title : SW846 8260
 QLast Update : Wed Aug 13 01:46:43 2025
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
41) Methacrylonitrile	7.232	41	10246m	5.247	ug/l	
42) 1,2-Dichloroethane	8.152	62	31902	4.946	ug/l	98
43) Isopropyl Acetate	8.195	43	31890	4.668	ug/l	100
44) Trichloroethene	8.859	130	32050	5.001	ug/l	93
45) 1,2-Dichloropropane	9.134	63	27418	4.805	ug/l	93
46) Dibromomethane	9.225	93	15033	4.590	ug/l	97
47) Bromodichloromethane	9.420	83	40327	4.785	ug/l	98
48) Methyl methacrylate	9.219	41	13477	4.122	ug/l	90
49) 1,4-Dioxane	9.231	88	3454	89.939	ug/l #	91
51) 4-Methyl-2-Pentanone	9.993	43	75891	21.535	ug/l	100
52) Toluene	10.164	92	73910	4.692	ug/l	100
53) t-1,3-Dichloropropene	10.390	75	34154	4.475	ug/l	99
54) cis-1,3-Dichloropropene	9.853	75	41326	4.579	ug/l	97
55) 1,1,2-Trichloroethane	10.566	97	20795	4.745	ug/l	98
56) Ethyl methacrylate	10.432	69	22376	3.990	ug/l	99
57) 1,3-Dichloropropane	10.713	76	34835	4.687	ug/l	99
58) 2-Chloroethyl Vinyl ether	9.707	63	51585	19.500	ug/l	100
59) 2-Hexanone	10.755	43	50604	21.088	ug/l	97
60) Dibromochloromethane	10.908	129	27141	4.693	ug/l	100
61) 1,2-Dibromoethane	11.012	107	18652	4.528	ug/l	97
64) Tetrachloroethene	10.640	164	36210	5.336	ug/l	97
65) Chlorobenzene	11.438	112	80684	4.922	ug/l	93
66) 1,1,1,2-Tetrachloroethane	11.511	131	26397	4.745	ug/l	94
67) Ethyl Benzene	11.511	91	134854	4.781	ug/l	99
68) m/p-Xylenes	11.621	106	102783	9.329	ug/l	97
69) o-Xylene	11.950	106	45944	4.453	ug/l	94
70) Styrene	11.963	104	71801	4.255	ug/l	97
71) Bromoform	12.127	173	14954	4.599	ug/l #	94
73) Isopropylbenzene	12.249	105	123246	4.845	ug/l	99
74) N-amyl acetate	12.066	43	22829	4.232	ug/l	96
75) 1,1,2,2-Tetrachloroethane	12.499	83	21057	4.848	ug/l	98
76) 1,2,3-Trichloropropane	12.554	75	19875m	5.710	ug/l	
77) Bromobenzene	12.530	156	29681	4.891	ug/l	100
78) n-propylbenzene	12.590	91	146043	4.822	ug/l	99
79) 2-Chlorotoluene	12.670	91	84671	4.880	ug/l	99
80) 1,3,5-Trimethylbenzene	12.731	105	96308	4.685	ug/l	100
81) trans-1,4-Dichloro-2-b...	12.298	75	6514	4.533	ug/l	89
82) 4-Chlorotoluene	12.773	91	87454	4.859	ug/l	99
83) tert-Butylbenzene	12.993	119	87496	4.712	ug/l	99
84) 1,2,4-Trimethylbenzene	13.036	105	93551	4.571	ug/l	100
85) sec-Butylbenzene	13.170	105	131079	4.806	ug/l	99
86) p-Isopropyltoluene	13.285	119	103731	4.582	ug/l	99
87) 1,3-Dichlorobenzene	13.279	146	57668	4.819	ug/l	99
88) 1,4-Dichlorobenzene	13.359	146	60781	5.120	ug/l	97
89) n-Butylbenzene	13.609	91	94594	4.549	ug/l	98
90) Hexachloroethane	13.871	117	22980	4.958	ug/l	97
91) 1,2-Dichlorobenzene	13.651	146	50829	4.843	ug/l	99
92) 1,2-Dibromo-3-Chloropr...	14.267	75	3369	4.982	ug/l	93
93) 1,2,4-Trichlorobenzene	14.913	180	28399	4.576	ug/l	98
94) Hexachlorobutadiene	15.017	225	19196	5.263	ug/l	96
95) Naphthalene	15.133	128	43395	4.100	ug/l	99
96) 1,2,3-Trichlorobenzene	15.322	180	24703	4.619	ug/l	98

Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY081225\
Data File : VY023050.D
Acq On : 12 Aug 2025 14:54
Operator : SY/MD
Sample : VSTDICC005
Misc : 5.00g/5.0mL/MSVOA_Y/SOIL
ALS Vial : 3 Sample Multiplier: 1

Instrument :
MSVOA_Y
ClientSampleId :
VSTDICC005

Manual Integrations
APPROVED

Reviewed By :Mahesh Dadoda 08/14/2025
Supervised By :Semsettin Yesilyurt 08/14/2025

Quant Time: Aug 13 01:50:18 2025
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y081225S.M
Quant Title : SW846 8260
QLast Update : Wed Aug 13 01:46:43 2025
Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
----------	------	------	----------	------	-------	----------

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY081225\
Data File : VY023050.D
Acq On : 12 Aug 2025 14:54
Operator : SY/MD
Sample : VSTDIC005
Misc : 5.00g/5.0mL/MSVOA_Y/SOIL
ALS Vial : 3 Sample Multiplier: 1

Instrument :
MSVOA_Y
ClientSampleId :
VSTDICC005

Manual Integrations APPROVED

Reviewed By :Mahesh Dadoda 08/14/2025
Supervised By :Semsettin Yesilyurt 08/14/2025

Quant Time: Aug 13 01:50:18 2025
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y081225S.M
Quant Title : SW846 8260
QLast Update : Wed Aug 13 01:46:43 2025
Response via : Initial Calibration

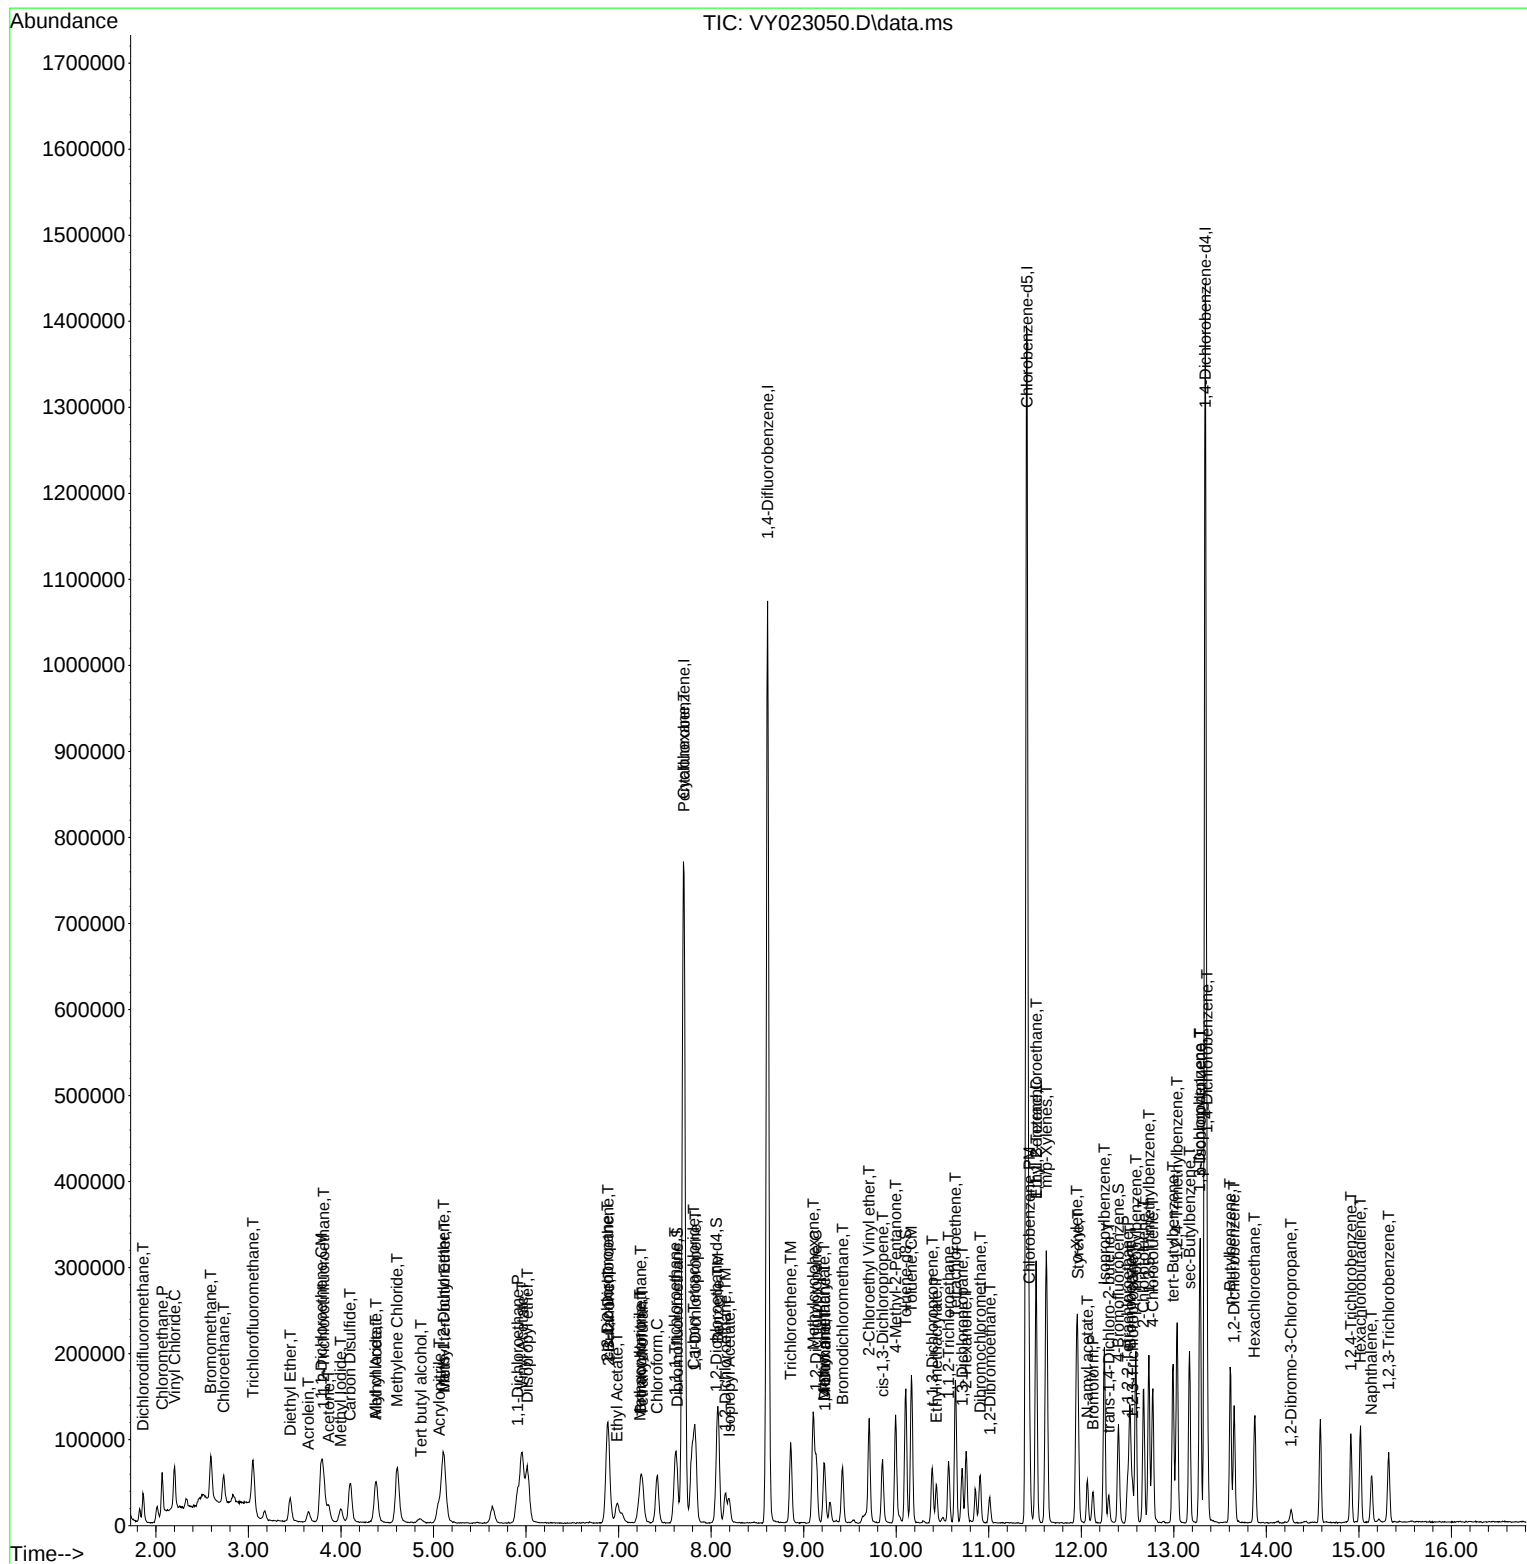

Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY081225\
 Data File : VY023051.D
 Acq On : 12 Aug 2025 15:17
 Operator : SY/MD
 Sample : VSTDICC010
 Misc : 5.00g/5.0mL/MSVOA_Y/SOIL
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_Y
 ClientSampleId :
 VSTDICC010

Manual Integrations
 APPROVED

Reviewed By :Mahesh Dadoda 08/14/2025
 Supervised By :Semsettin Yesilyurt 08/14/2025

Quant Time: Aug 13 01:51:22 2025
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y081225S.M
 Quant Title : SW846 8260
 QLast Update : Wed Aug 13 01:46:43 2025
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Pentafluorobenzene	7.701	168	551522	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	8.609	114	883548	50.000	ug/l	0.00
63) Chlorobenzene-d5	11.408	117	761327	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.340	152	365647	50.000	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	8.061	65	54002	10.274	ug/l	0.00
Spiked Amount 50.000	Range 50 - 163		Recovery =	20.540%#		
35) Dibromofluoromethane	7.628	113	52916	10.009	ug/l	0.00
Spiked Amount 50.000	Range 54 - 147		Recovery =	20.020%#		
50) Toluene-d8	10.103	98	204532	9.903	ug/l	0.00
Spiked Amount 50.000	Range 58 - 134		Recovery =	19.800%#		
62) 4-Bromofluorobenzene	12.401	95	64927	9.775	ug/l	0.00
Spiked Amount 50.000	Range 30 - 143		Recovery =	19.540%#		
Target Compounds						
					Qvalue	
2) Dichlorodifluoromethane	1.861	85	51022	11.334	ug/l	95
3) Chloromethane	2.068	50	77982	10.695	ug/l	97
4) Vinyl Chloride	2.202	62	95983	10.649	ug/l	99
5) Bromomethane	2.592	94	70415	10.461	ug/l	99
6) Chloroethane	2.732	64	62514	10.432	ug/l	97
7) Trichlorofluoromethane	3.049	101	115150	10.507	ug/l	94
8) Diethyl Ether	3.452	74	30390	10.481	ug/l	99
9) 1,1,2-Trichlorotrifluo...	3.812	101	57210	10.581	ug/l	100
10) Methyl Iodide	4.001	142	54184	9.287	ug/l	99
11) Tert butyl alcohol	4.866	59	20212	56.119	ug/l	99
12) 1,1-Dichloroethene	3.781	96	55669	10.475	ug/l	92
13) Acrolein	3.647	56	30081	57.030	ug/l	97
14) Allyl chloride	4.372	41	79145	10.121	ug/l	98
15) Acrylonitrile	5.049	53	62889	53.349	ug/l	99
16) Acetone	3.873	43	61290	53.821	ug/l	94
17) Carbon Disulfide	4.098	76	183399	10.583	ug/l	98
18) Methyl Acetate	4.385	43	33996	10.032	ug/l	99
19) Methyl tert-butyl Ether	5.110	73	139820	10.153	ug/l	95
20) Methylene Chloride	4.604	84	77920	11.095	ug/l	97
21) trans-1,2-Dichloroethene	5.110	96	61826	10.352	ug/l	100
22) Diisopropyl ether	6.012	45	172602	10.157	ug/l	93
23) Vinyl Acetate	5.957	43	482714	51.372	ug/l	98
24) 1,1-Dichloroethane	5.903	63	106831	10.282	ug/l	99
25) 2-Butanone	6.896	43	83923	54.187	ug/l	96
26) 2,2-Dichloropropane	6.878	77	91579	10.215	ug/l	100
27) cis-1,2-Dichloroethene	6.884	96	68839	9.970	ug/l	99
28) Bromochloromethane	7.238	49	41820	10.146	ug/l	100
29) Tetrahydrofuran	7.262	42	49926	52.005	ug/l	99
30) Chloroform	7.415	83	109942	10.260	ug/l	93
31) Cyclohexane	7.701	56	103068	10.527	ug/l #	89
32) 1,1,1-Trichloroethane	7.616	97	96693	10.170	ug/l	98
36) 1,1-Dichloropropene	7.829	75	80479	10.243	ug/l	99
37) Ethyl Acetate	6.982	43	34854	10.560	ug/l	97
38) Carbon Tetrachloride	7.811	117	85932	10.070	ug/l	97
39) Methylcyclohexane	9.103	83	102275	9.885	ug/l	99
40) Benzene	8.073	78	243060	10.037	ug/l	100

Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY081225\
 Data File : VY023051.D
 Acq On : 12 Aug 2025 15:17
 Operator : SY/MD
 Sample : VSTDICC010
 Misc : 5.00g/5.0mL/MSVOA_Y/SOIL
 ALS Vial : 4 Sample Multiplier: 1

Instrument :

MSVOA_Y

ClientSampleId :

VSTDICC010

Manual Integrations

APPROVED

Reviewed By :Mahesh Dadoda 08/14/2025

Supervised By :Semsettin Yesilyurt 08/14/2025

Quant Time: Aug 13 01:51:22 2025

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y081225S.M

Quant Title : SW846 8260

QLast Update : Wed Aug 13 01:46:43 2025

Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
41) Methacrylonitrile	7.213	41	18825	9.872	ug/l #	89
42) 1,2-Dichloroethane	8.152	62	65350	10.376	ug/l	99
43) Isopropyl Acetate	8.195	43	67669	10.144	ug/l	99
44) Trichloroethene	8.859	130	62689	10.017	ug/l	98
45) 1,2-Dichloropropane	9.134	63	56720	10.179	ug/l	97
46) Dibromomethane	9.225	93	33460	10.462	ug/l	98
47) Bromodichloromethane	9.420	83	81951	9.959	ug/l	97
48) Methyl methacrylate	9.213	41	31851	9.978	ug/l	96
49) 1,4-Dioxane	9.231	88	7705	205.471	ug/l	94
51) 4-Methyl-2-Pentanone	9.993	43	177157	51.484	ug/l	98
52) Toluene	10.164	92	150422	9.780	ug/l	99
53) t-1,3-Dichloropropene	10.390	75	72507	9.730	ug/l	99
54) cis-1,3-Dichloropropene	9.853	75	85945	9.753	ug/l	100
55) 1,1,2-Trichloroethane	10.566	97	42712	9.981	ug/l	97
56) Ethyl methacrylate	10.432	69	52746	9.632	ug/l	98
57) 1,3-Dichloropropane	10.713	76	74433	10.256	ug/l	99
58) 2-Chloroethyl Vinyl ether	9.707	63	119417	46.232	ug/l	98
59) 2-Hexanone	10.755	43	118452	50.553	ug/l	99
60) Dibromochloromethane	10.902	129	56045	9.925	ug/l	99
61) 1,2-Dibromoethane	11.011	107	41009	10.196	ug/l	99
64) Tetrachloroethene	10.640	164	70502	10.371	ug/l	98
65) Chlorobenzene	11.438	112	162985	9.925	ug/l	97
66) 1,1,1,2-Tetrachloroethane	11.511	131	54856	9.842	ug/l	97
67) Ethyl Benzene	11.511	91	273281	9.670	ug/l	99
68) m/p-Xylenes	11.621	106	212766	19.277	ug/l	99
69) o-Xylene	11.950	106	97841	9.465	ug/l	98
70) Styrene	11.963	104	155809	9.216	ug/l	99
71) Bromoform	12.127	173	32470	9.968	ug/l #	97
73) Isopropylbenzene	12.249	105	254745	9.871	ug/l	99
74) N-amyl acetate	12.066	43	53943	9.857	ug/l	98
75) 1,1,2,2-Tetrachloroethane	12.499	83	47304	10.735	ug/l	99
76) 1,2,3-Trichloropropane	12.548	75	35353m	10.012	ug/l	
77) Bromobenzene	12.523	156	60728	9.864	ug/l	96
78) n-propylbenzene	12.590	91	303440	9.876	ug/l	100
79) 2-Chlorotoluene	12.676	91	175364	9.962	ug/l	99
80) 1,3,5-Trimethylbenzene	12.731	105	205544	9.855	ug/l	100
81) trans-1,4-Dichloro-2-b...	12.298	75	15715	10.780	ug/l	96
82) 4-Chlorotoluene	12.767	91	181812	9.956	ug/l	99
83) tert-Butylbenzene	12.993	119	181408	9.630	ug/l	99
84) 1,2,4-Trimethylbenzene	13.035	105	201812	9.720	ug/l	100
85) sec-Butylbenzene	13.170	105	274178	9.908	ug/l	99
86) p-Isopropyltoluene	13.285	119	217799	9.482	ug/l	98
87) 1,3-Dichlorobenzene	13.279	146	120109	9.893	ug/l	99
88) 1,4-Dichlorobenzene	13.359	146	121160	10.060	ug/l	97
89) n-Butylbenzene	13.609	91	205420	9.737	ug/l	98
90) Hexachloroethane	13.871	117	47353	10.071	ug/l	98
91) 1,2-Dichlorobenzene	13.651	146	107656	10.110	ug/l	100
92) 1,2-Dibromo-3-Chloropr...	14.267	75	7032	10.250	ug/l	98
93) 1,2,4-Trichlorobenzene	14.913	180	61323	9.739	ug/l	99
94) Hexachlorobutadiene	15.017	225	37011	10.003	ug/l	99
95) Naphthalene	15.139	128	99780	9.293	ug/l	99
96) 1,2,3-Trichlorobenzene	15.322	180	53626	9.883	ug/l	96

Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY081225\
Data File : VY023051.D
Acq On : 12 Aug 2025 15:17
Operator : SY/MD
Sample : VSTDICC010
Misc : 5.00g/5.0mL/MSVOA_Y/SOIL
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_Y
ClientSampleId :
VSTDICC010

Manual Integrations
APPROVED

Reviewed By :Mahesh Dadoda 08/14/2025
Supervised By :Semsettin Yesilyurt 08/14/2025

Quant Time: Aug 13 01:51:22 2025
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y081225S.M
Quant Title : SW846 8260
QLast Update : Wed Aug 13 01:46:43 2025
Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
----------	------	------	----------	------	-------	----------

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY081225\
Data File : VY023051.D
Acq On : 12 Aug 2025 15:17
Operator : SY/MD
Sample : VSTDIC010
Misc : 5.00g/5.0mL/MSVOA_Y/SOIL
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_Y
ClientSampleId :
VSTDICC010

Manual Integrations APPROVED

Reviewed By :Mahesh Dadoda 08/14/2025
Supervised By :Semsettin Yesilyurt 08/14/2025

Quant Time: Aug 13 01:51:22 2025
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y081225S.M
Quant Title : SW846 8260
QLast Update : Wed Aug 13 01:46:43 2025
Response via : Initial Calibration

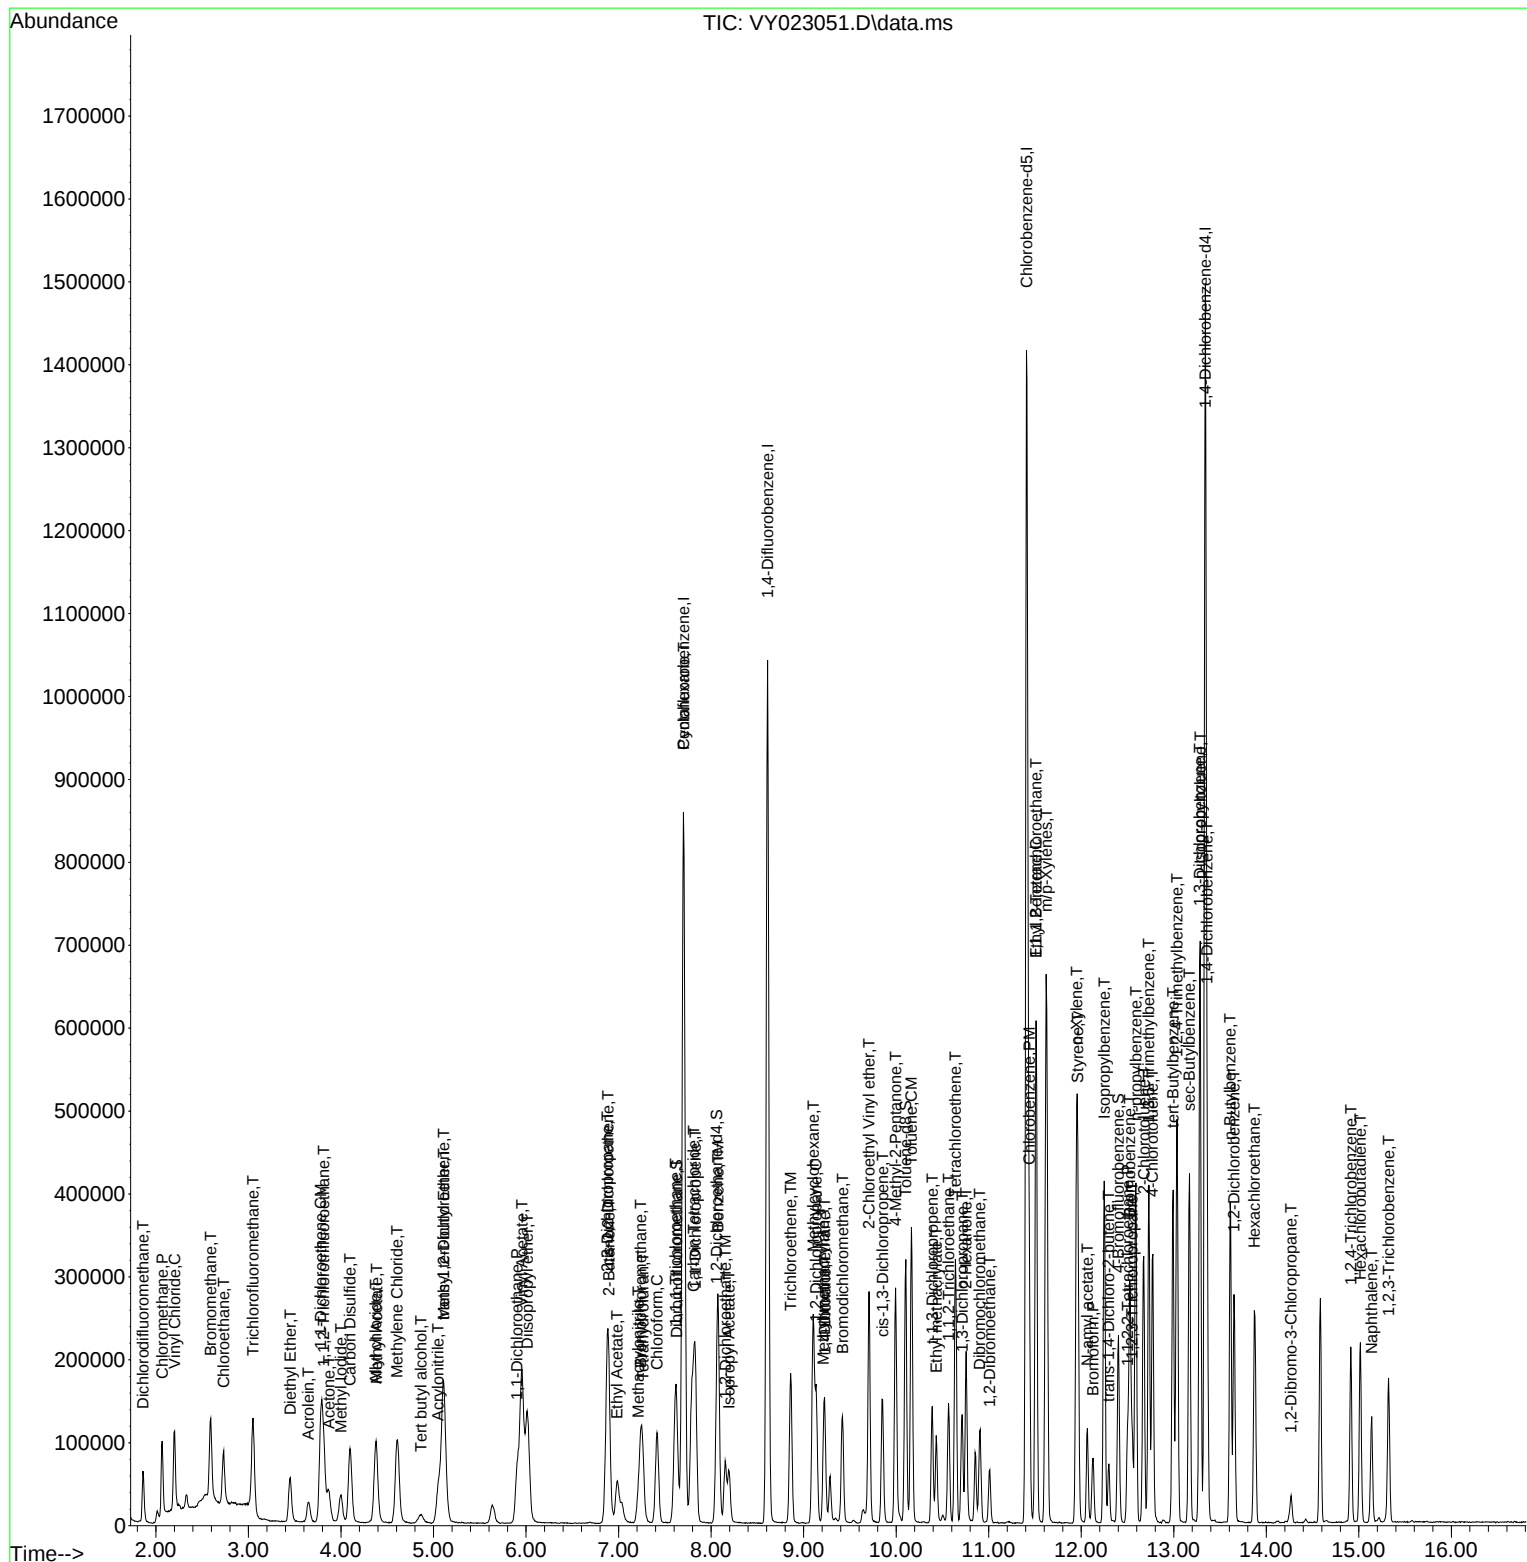

Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY081225\
 Data File : VY023052.D
 Acq On : 12 Aug 2025 15:40
 Operator : SY/MD
 Sample : VSTDICC020
 Misc : 5.00g/5.0mL/MSVOA_Y/SOIL
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_Y
 ClientSampleId :
 VSTDICC020

Manual Integrations
 APPROVED

Reviewed By :Mahesh Dadoda 08/14/2025
 Supervised By :Semsettin Yesilyurt 08/14/2025

Quant Time: Aug 13 01:52:25 2025
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y081225S.M
 Quant Title : SW846 8260
 QLast Update : Wed Aug 13 01:46:43 2025
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Pentafluorobenzene	7.707	168	537748	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	8.610	114	848953	50.000	ug/l	0.00
63) Chlorobenzene-d5	11.414	117	745484	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.340	152	370932	50.000	ug/l	0.00

System Monitoring Compounds

33) 1,2-Dichloroethane-d4	8.055	65	103755	20.244	ug/l	0.00
Spiked Amount	50.000	Range	50 - 163	Recovery	=	40.480%#
35) Dibromofluoromethane	7.628	113	102068	20.093	ug/l	0.00
Spiked Amount	50.000	Range	54 - 147	Recovery	=	40.180%#
50) Toluene-d8	10.103	98	398394	20.075	ug/l	0.00
Spiked Amount	50.000	Range	58 - 134	Recovery	=	40.160%#
62) 4-Bromofluorobenzene	12.402	95	124467	19.503	ug/l	0.00
Spiked Amount	50.000	Range	30 - 143	Recovery	=	39.000%

Target Compounds

						Qvalue
2) Dichlorodifluoromethane	1.861	85	98926	22.537	ug/l	98
3) Chloromethane	2.068	50	158310	22.268	ug/l	99
4) Vinyl Chloride	2.202	62	188307	21.427	ug/l	99
5) Bromomethane	2.586	94	140517	21.410	ug/l	99
6) Chloroethane	2.726	64	122310	20.934	ug/l	99
7) Trichlorofluoromethane	3.050	101	225373	21.090	ug/l	99
8) Diethyl Ether	3.452	74	58245	20.602	ug/l	99
9) 1,1,2-Trichlorotrifluo...	3.805	101	112116	21.267	ug/l	99
10) Methyl Iodide	3.994	142	115879	20.370	ug/l	99
11) Tert butyl alcohol	4.860	59	35192	100.214	ug/l	98
12) 1,1-Dichloroethene	3.781	96	107992	20.840	ug/l	99
13) Acrolein	3.653	56	54065	105.126	ug/l	100
14) Allyl chloride	4.379	41	155709	20.421	ug/l	97
15) Acrylonitrile	5.055	53	120151	104.535	ug/l	97
16) Acetone	3.866	43	113468	102.193	ug/l	96
17) Carbon Disulfide	4.098	76	357484	21.157	ug/l	98
18) Methyl Acetate	4.379	43	69853	21.141	ug/l	99
19) Methyl tert-butyl Ether	5.110	73	278863	20.767	ug/l	99
20) Methylene Chloride	4.610	84	130416	21.069	ug/l	96
21) trans-1,2-Dichloroethene	5.104	96	120321	20.661	ug/l	96
22) Diisopropyl ether	6.012	45	346195	20.894	ug/l	95
23) Vinyl Acetate	5.951	43	941364	102.748	ug/l	97
24) 1,1-Dichloroethane	5.909	63	211558	20.884	ug/l	98
25) 2-Butanone	6.890	43	153363	101.559	ug/l	100
26) 2,2-Dichloropropane	6.878	77	181528	20.767	ug/l	100
27) cis-1,2-Dichloroethene	6.884	96	138775	20.613	ug/l	99
28) Bromochloromethane	7.244	49	84540	21.035	ug/l	99
29) Tetrahydrofuran	7.262	42	95795	102.341	ug/l	99
30) Chloroform	7.415	83	215585	20.635	ug/l	98
31) Cyclohexane	7.701	56	194671	20.393	ug/l	96
32) 1,1,1-Trichloroethane	7.610	97	193268	20.848	ug/l	99
36) 1,1-Dichloropropene	7.835	75	156617	20.746	ug/l	98
37) Ethyl Acetate	6.982	43	66420	20.944	ug/l	100
38) Carbon Tetrachloride	7.817	117	171344	20.897	ug/l	98
39) Methylcyclohexane	9.103	83	205594	20.680	ug/l	98
40) Benzene	8.079	78	485631	20.871	ug/l	100

Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY081225\
 Data File : VY023052.D
 Acq On : 12 Aug 2025 15:40
 Operator : SY/MD
 Sample : VSTDICC020
 Misc : 5.00g/5.0mL/MSVOA_Y/SOIL
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_Y
 ClientSampleId :
 VSTDICC020

Manual Integrations
 APPROVED

Reviewed By :Mahesh Dadoda 08/14/2025
 Supervised By :Semsettin Yesilyurt 08/14/2025

Quant Time: Aug 13 01:52:25 2025
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y081225S.M
 Quant Title : SW846 8260
 QLast Update : Wed Aug 13 01:46:43 2025
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
41) Methacrylonitrile	7.226	41	37785m	20.623	ug/l	
42) 1,2-Dichloroethane	8.152	62	126111	20.839	ug/l	100
43) Isopropyl Acetate	8.195	43	131854	20.571	ug/l	98
44) Trichloroethene	8.859	130	126772	21.083	ug/l	98
45) 1,2-Dichloropropane	9.134	63	110699	20.677	ug/l	99
46) Dibromomethane	9.225	93	63410	20.635	ug/l	98
47) Bromodichloromethane	9.420	83	165954	20.988	ug/l	96
48) Methyl methacrylate	9.219	41	64120	20.905	ug/l	98
49) 1,4-Dioxane	9.225	88	14826	411.480	ug/l	98
51) 4-Methyl-2-Pentanone	9.993	43	339298	102.622	ug/l	100
52) Toluene	10.164	92	306193	20.719	ug/l	100
53) t-1,3-Dichloropropene	10.390	75	147696	20.627	ug/l	100
54) cis-1,3-Dichloropropene	9.853	75	174243	20.580	ug/l	96
55) 1,1,2-Trichloroethane	10.566	97	86022	20.920	ug/l	99
56) Ethyl methacrylate	10.432	69	105816	20.111	ug/l	99
57) 1,3-Dichloropropane	10.713	76	145621	20.882	ug/l	99
58) 2-Chloroethyl Vinyl ether	9.707	63	244340	98.450	ug/l	99
59) 2-Hexanone	10.755	43	231872	102.992	ug/l	99
60) Dibromochloromethane	10.908	129	110810	20.424	ug/l	99
61) 1,2-Dibromoethane	11.012	107	80549	20.842	ug/l	97
64) Tetrachloroethene	10.640	164	141609	21.273	ug/l	99
65) Chlorobenzene	11.438	112	332700	20.690	ug/l	97
66) 1,1,1,2-Tetrachloroethane	11.511	131	112677	20.647	ug/l	99
67) Ethyl Benzene	11.511	91	564855	20.412	ug/l	99
68) m/p-Xylenes	11.621	106	444361	41.115	ug/l	98
69) o-Xylene	11.950	106	207639	20.513	ug/l	99
70) Styrene	11.963	104	339891	20.532	ug/l	99
71) Bromoform	12.127	173	64275	20.151	ug/l #	98
73) Isopropylbenzene	12.249	105	534421	20.413	ug/l	100
74) N-amyl acetate	12.066	43	112297	20.227	ug/l	98
75) 1,1,2,2-Tetrachloroethane	12.499	83	89782	20.085	ug/l	100
76) 1,2,3-Trichloropropane	12.548	75	70070m	19.560	ug/l	
77) Bromobenzene	12.523	156	128501	20.574	ug/l	99
78) n-propylbenzene	12.590	91	640528	20.550	ug/l	99
79) 2-Chlorotoluene	12.670	91	365577	20.471	ug/l	100
80) 1,3,5-Trimethylbenzene	12.731	105	435074	20.563	ug/l	99
81) trans-1,4-Dichloro-2-b...	12.298	75	30153	20.389	ug/l	97
82) 4-Chlorotoluene	12.773	91	385755	20.822	ug/l	99
83) tert-Butylbenzene	12.993	119	389621	20.389	ug/l	100
84) 1,2,4-Trimethylbenzene	13.036	105	438392	20.814	ug/l	98
85) sec-Butylbenzene	13.170	105	575804	20.512	ug/l	100
86) p-Isopropyltoluene	13.285	119	480937	20.640	ug/l	100
87) 1,3-Dichlorobenzene	13.279	146	252452	20.497	ug/l	99
88) 1,4-Dichlorobenzene	13.359	146	249280	20.403	ug/l	99
89) n-Butylbenzene	13.609	91	440963	20.605	ug/l	99
90) Hexachloroethane	13.871	117	96478	20.226	ug/l	98
91) 1,2-Dichlorobenzene	13.651	146	222000	20.552	ug/l	99
92) 1,2-Dibromo-3-Chloropr...	14.267	75	13973	20.076	ug/l	98
93) 1,2,4-Trichlorobenzene	14.913	180	130718	20.464	ug/l	98
94) Hexachlorobutadiene	15.017	225	77511	20.650	ug/l	99
95) Naphthalene	15.139	128	216923	19.915	ug/l	100
96) 1,2,3-Trichlorobenzene	15.322	180	111506	20.258	ug/l	99

Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY081225\
Data File : VY023052.D
Acq On : 12 Aug 2025 15:40
Operator : SY/MD
Sample : VSTDICC020
Misc : 5.00g/5.0mL/MSVOA_Y/SOIL
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_Y
ClientSampleId :
VSTDICC020

Manual Integrations
APPROVED

Reviewed By :Mahesh Dadoda 08/14/2025
Supervised By :Semsettin Yesilyurt 08/14/2025

Quant Time: Aug 13 01:52:25 2025
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y081225S.M
Quant Title : SW846 8260
QLast Update : Wed Aug 13 01:46:43 2025
Response via : Initial Calibration


Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
----------	------	------	----------	------	-------	----------

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Instrument :
MSVOA_Y
ClientSampleId :
VSTDICC020

Manual Integrations APPROVED

Reviewed By :Mahesh Dadoda 08/14/2025
Supervised By :Semsettin Yesilyurt 08/14/2025

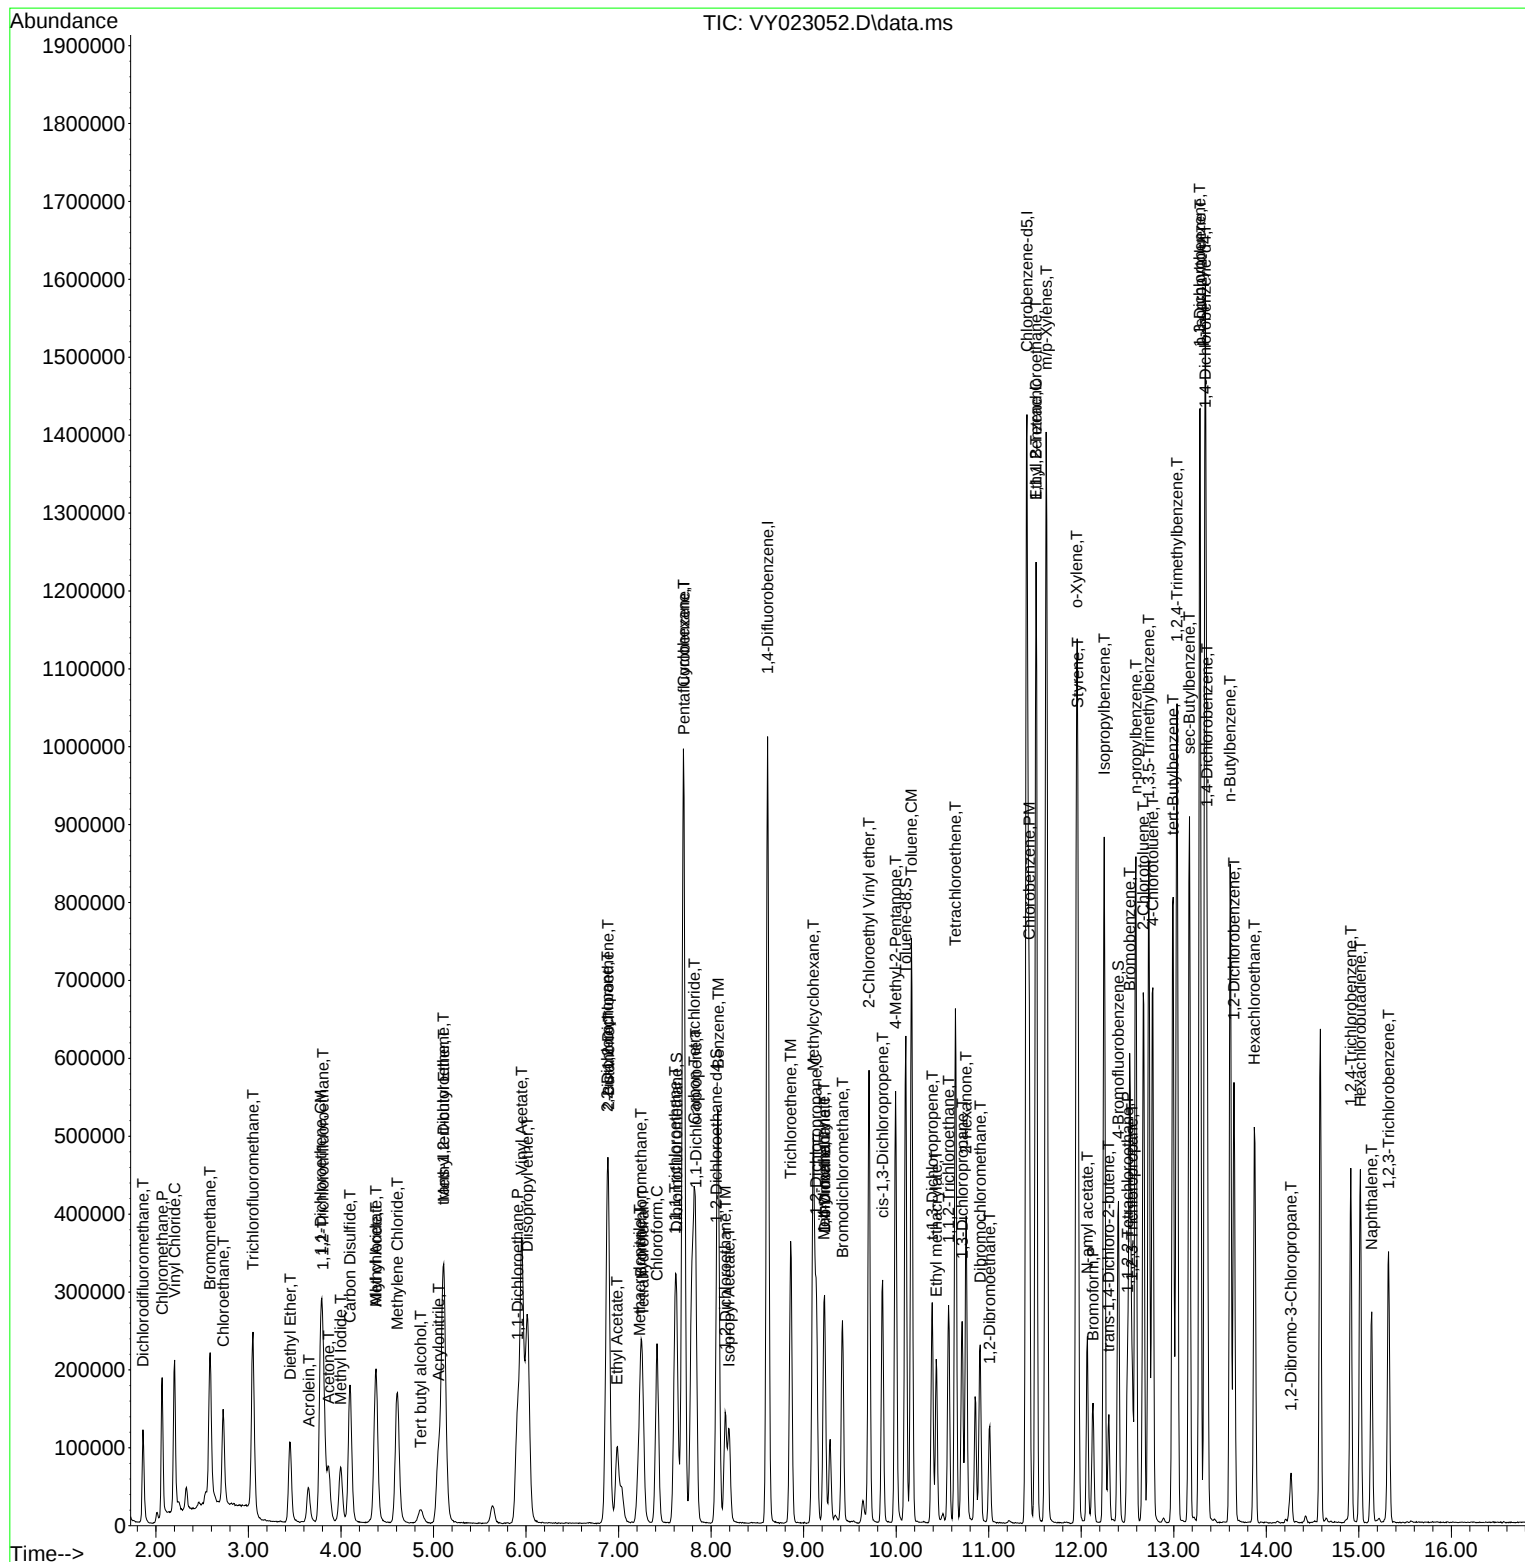

Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY081225\
 Data File : VY023053.D
 Acq On : 12 Aug 2025 16:02
 Operator : SY/MD
 Sample : VSTDICCC050
 Misc : 5.00g/5.0mL/MSVOA_Y/SOIL
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_Y
 ClientSampleId :
 VSTDICCC050

Manual Integrations
 APPROVED

Reviewed By :Mahesh Dadoda 08/14/2025
 Supervised By :Semsettin Yesilyurt 08/14/2025

Quant Time: Aug 13 01:53:26 2025
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y081225S.M
 Quant Title : SW846 8260
 QLast Update : Wed Aug 13 01:46:43 2025
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Pentafluorobenzene	7.707	168	539282	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	8.609	114	856556	50.000	ug/l	0.00
63) Chlorobenzene-d5	11.408	117	751969	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.340	152	377839	50.000	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	8.055	65	249044	48.455	ug/l	0.00
Spiked Amount 50.000	Range 50 - 163		Recovery =	96.900%		
35) Dibromofluoromethane	7.628	113	251193	49.010	ug/l	0.00
Spiked Amount 50.000	Range 54 - 147		Recovery =	98.020%		
50) Toluene-d8	10.103	98	979082	48.899	ug/l	0.00
Spiked Amount 50.000	Range 58 - 134		Recovery =	97.800%		
62) 4-Bromofluorobenzene	12.401	95	316770	49.194	ug/l	0.00
Spiked Amount 50.000	Range 30 - 143		Recovery =	98.380%		
Target Compounds					Qvalue	
2) Dichlorodifluoromethane	1.861	85	187863	42.677	ug/l	100
3) Chloromethane	2.068	50	327481	45.932	ug/l	100
4) Vinyl Chloride	2.196	62	414609	47.044	ug/l	100
5) Bromomethane	2.592	94	291336	44.263	ug/l	100
6) Chloroethane	2.726	64	277698	47.394	ug/l	100
7) Trichlorofluoromethane	3.049	101	505137	47.136	ug/l	100
8) Diethyl Ether	3.446	74	135373	47.747	ug/l	100
9) 1,1,2-Trichlorotrifluo...	3.805	101	249063	47.109	ug/l	100
10) Methyl Iodide	3.994	142	296087	51.899	ug/l	100
11) Tert butyl alcohol	4.860	59	85712	243.383	ug/l	100
12) 1,1-Dichloroethene	3.781	96	249492	48.009	ug/l	100
13) Acrolein	3.647	56	121185	234.966	ug/l	100
14) Allyl chloride	4.378	41	369720	48.350	ug/l	100
15) Acrylonitrile	5.049	53	285675	247.839	ug/l	100
16) Acetone	3.860	43	278510	250.122	ug/l	100
17) Carbon Disulfide	4.098	76	804119	47.456	ug/l	100
18) Methyl Acetate	4.378	43	173642	52.403	ug/l	100
19) Methyl tert-butyl Ether	5.110	73	666514	49.495	ug/l	100
20) Methylene Chloride	4.604	84	275004	47.415	ug/l	100
21) trans-1,2-Dichloroethene	5.104	96	282272	48.334	ug/l	100
22) Diisopropyl ether	6.018	45	815359	49.070	ug/l	100
23) Vinyl Acetate	5.951	43	2268046	246.849	ug/l	100
24) 1,1-Dichloroethane	5.909	63	495073	48.732	ug/l	100
25) 2-Butanone	6.884	43	382711	252.715	ug/l	100
26) 2,2-Dichloropropane	6.884	77	425773	48.571	ug/l	100
27) cis-1,2-Dichloroethene	6.884	96	327272	48.474	ug/l	100
28) Bromochloromethane	7.244	49	196667	48.795	ug/l	100
29) Tetrahydrofuran	7.256	42	235169	250.523	ug/l	100
30) Chloroform	7.415	83	508641	48.547	ug/l	100
31) Cyclohexane	7.695	56	440266	45.989	ug/l	100
32) 1,1,1-Trichloroethane	7.616	97	451521	48.569	ug/l	100
36) 1,1-Dichloropropene	7.829	75	371204	48.734	ug/l	100
37) Ethyl Acetate	6.982	43	160980	50.311	ug/l	100
38) Carbon Tetrachloride	7.817	117	399463	48.285	ug/l	100
39) Methylcyclohexane	9.103	83	484691	48.321	ug/l	100
40) Benzene	8.073	78	1142910	48.683	ug/l	100

Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY081225\
 Data File : VY023053.D
 Acq On : 12 Aug 2025 16:02
 Operator : SY/MD
 Sample : VSTDICCC050
 Misc : 5.00g/5.0mL/MSVOA_Y/SOIL
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_Y
 ClientSampleId :
 VSTDICCC050

Manual Integrations
 APPROVED

Reviewed By :Mahesh Dadoda 08/14/2025
 Supervised By :Semsettin Yesilyurt 08/14/2025

Quant Time: Aug 13 01:53:26 2025
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y081225S.M
 Quant Title : SW846 8260
 QLast Update : Wed Aug 13 01:46:43 2025
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
41) Methacrylonitrile	7.219	41	94123	50.916	ug/l	100
42) 1,2-Dichloroethane	8.152	62	296907	48.627	ug/l	100
43) Isopropyl Acetate	8.195	43	319600	49.419	ug/l	100
44) Trichloroethene	8.859	130	292421	48.199	ug/l	100
45) 1,2-Dichloropropane	9.140	63	264354	48.938	ug/l	100
46) Dibromomethane	9.225	93	152822	49.291	ug/l	100
47) Bromodichloromethane	9.420	83	393523	49.327	ug/l	100
48) Methyl methacrylate	9.213	41	160792	51.958	ug/l	100
49) 1,4-Dioxane	9.225	88	36249	997.124	ug/l	100
51) 4-Methyl-2-Pentanone	9.993	43	853025	255.710	ug/l	100
52) Toluene	10.164	92	735326	49.315	ug/l	100
53) t-1,3-Dichloropropene	10.390	75	359698	49.790	ug/l	100
54) cis-1,3-Dichloropropene	9.853	75	424834	49.731	ug/l	100
55) 1,1,2-Trichloroethane	10.566	97	204368	49.261	ug/l	100
56) Ethyl methacrylate	10.432	69	273801	51.576	ug/l	100
57) 1,3-Dichloropropane	10.713	76	346510	49.249	ug/l	100
58) 2-Chloroethyl Vinyl ether	9.707	63	663351	264.906	ug/l	100
59) 2-Hexanone	10.755	43	584223	257.194	ug/l	100
60) Dibromochloromethane	10.908	129	272171	49.719	ug/l	100
61) 1,2-Dibromoethane	11.005	107	193398	49.598	ug/l	100
64) Tetrachloroethene	10.640	164	327271	48.740	ug/l	100
65) Chlorobenzene	11.438	112	793490	48.920	ug/l	100
66) 1,1,1,2-Tetrachloroethane	11.511	131	271839	49.381	ug/l	100
67) Ethyl Benzene	11.511	91	1397704	50.073	ug/l	100
68) m/p-Xylenes	11.621	106	1080401	99.103	ug/l	100
69) o-Xylene	11.950	106	516002	50.536	ug/l	100
70) Styrene	11.962	104	844409	50.569	ug/l	100
71) Bromoform	12.127	173	160769	49.969	ug/l #	100
73) Isopropylbenzene	12.249	105	1324313	49.660	ug/l	100
74) N-amyl acetate	12.066	43	289914	51.264	ug/l	100
75) 1,1,2,2-Tetrachloroethane	12.499	83	220853	48.503	ug/l	100
76) 1,2,3-Trichloropropane	12.548	75	202260m	55.430	ug/l	
77) Bromobenzene	12.523	156	312706	49.152	ug/l	100
78) n-propylbenzene	12.590	91	1593368	50.186	ug/l	100
79) 2-Chlorotoluene	12.670	91	899967	49.473	ug/l	100
80) 1,3,5-Trimethylbenzene	12.731	105	1080333	50.126	ug/l	100
81) trans-1,4-Dichloro-2-b...	12.298	75	74567	49.500	ug/l	100
82) 4-Chlorotoluene	12.767	91	930329	49.299	ug/l	100
83) tert-Butylbenzene	12.993	119	978031	50.244	ug/l	100
84) 1,2,4-Trimethylbenzene	13.035	105	1071926	49.963	ug/l	100
85) sec-Butylbenzene	13.170	105	1425553	49.854	ug/l	100
86) p-Isopropyltoluene	13.285	119	1196645	50.417	ug/l	100
87) 1,3-Dichlorobenzene	13.279	146	608249	48.481	ug/l	100
88) 1,4-Dichlorobenzene	13.359	146	605079	48.618	ug/l	100
89) n-Butylbenzene	13.609	91	1099864	50.454	ug/l	100
90) Hexachloroethane	13.871	117	238005	48.984	ug/l	100
91) 1,2-Dichlorobenzene	13.651	146	536637	48.772	ug/l	100
92) 1,2-Dibromo-3-Chloropr...	14.267	75	35867	50.592	ug/l	100
93) 1,2,4-Trichlorobenzene	14.913	180	320080	49.192	ug/l	100
94) Hexachlorobutadiene	15.017	225	185604	48.543	ug/l	100
95) Naphthalene	15.139	128	562363	50.685	ug/l	100
96) 1,2,3-Trichlorobenzene	15.322	180	272154	48.540	ug/l	100

Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY081225\
Data File : VY023053.D
Acq On : 12 Aug 2025 16:02
Operator : SY/MD
Sample : VSTDICCC050
Misc : 5.00g/5.0mL/MSVOA_Y/SOIL
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_Y
ClientSampleId :
VSTDICCC050

Manual Integrations
APPROVED

Reviewed By :Mahesh Dadoda 08/14/2025
Supervised By :Semsettin Yesilyurt 08/14/2025

Quant Time: Aug 13 01:53:26 2025
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y081225S.M
Quant Title : SW846 8260
QLast Update : Wed Aug 13 01:46:43 2025
Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
----------	------	------	----------	------	-------	----------

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY081225\
 Data File : VY023053.D
 Acq On : 12 Aug 2025 16:02
 Operator : SY/MD
 Sample : VSTDICCC050
 Misc : 5.00g/5.0mL/MSVOA_Y/SOIL
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_Y
 ClientSampleId :
 VSTDICCC050

Quant Time: Aug 13 01:53:26 2025
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y081225S.M
 Quant Title : SW846 8260
 QLast Update : Wed Aug 13 01:46:43 2025
 Response via : Initial Calibration

Manual Integrations APPROVED

Reviewed By :Mahesh Dadoda 08/14/2025
 Supervised By :Semsettin Yesilyurt 08/14/2025

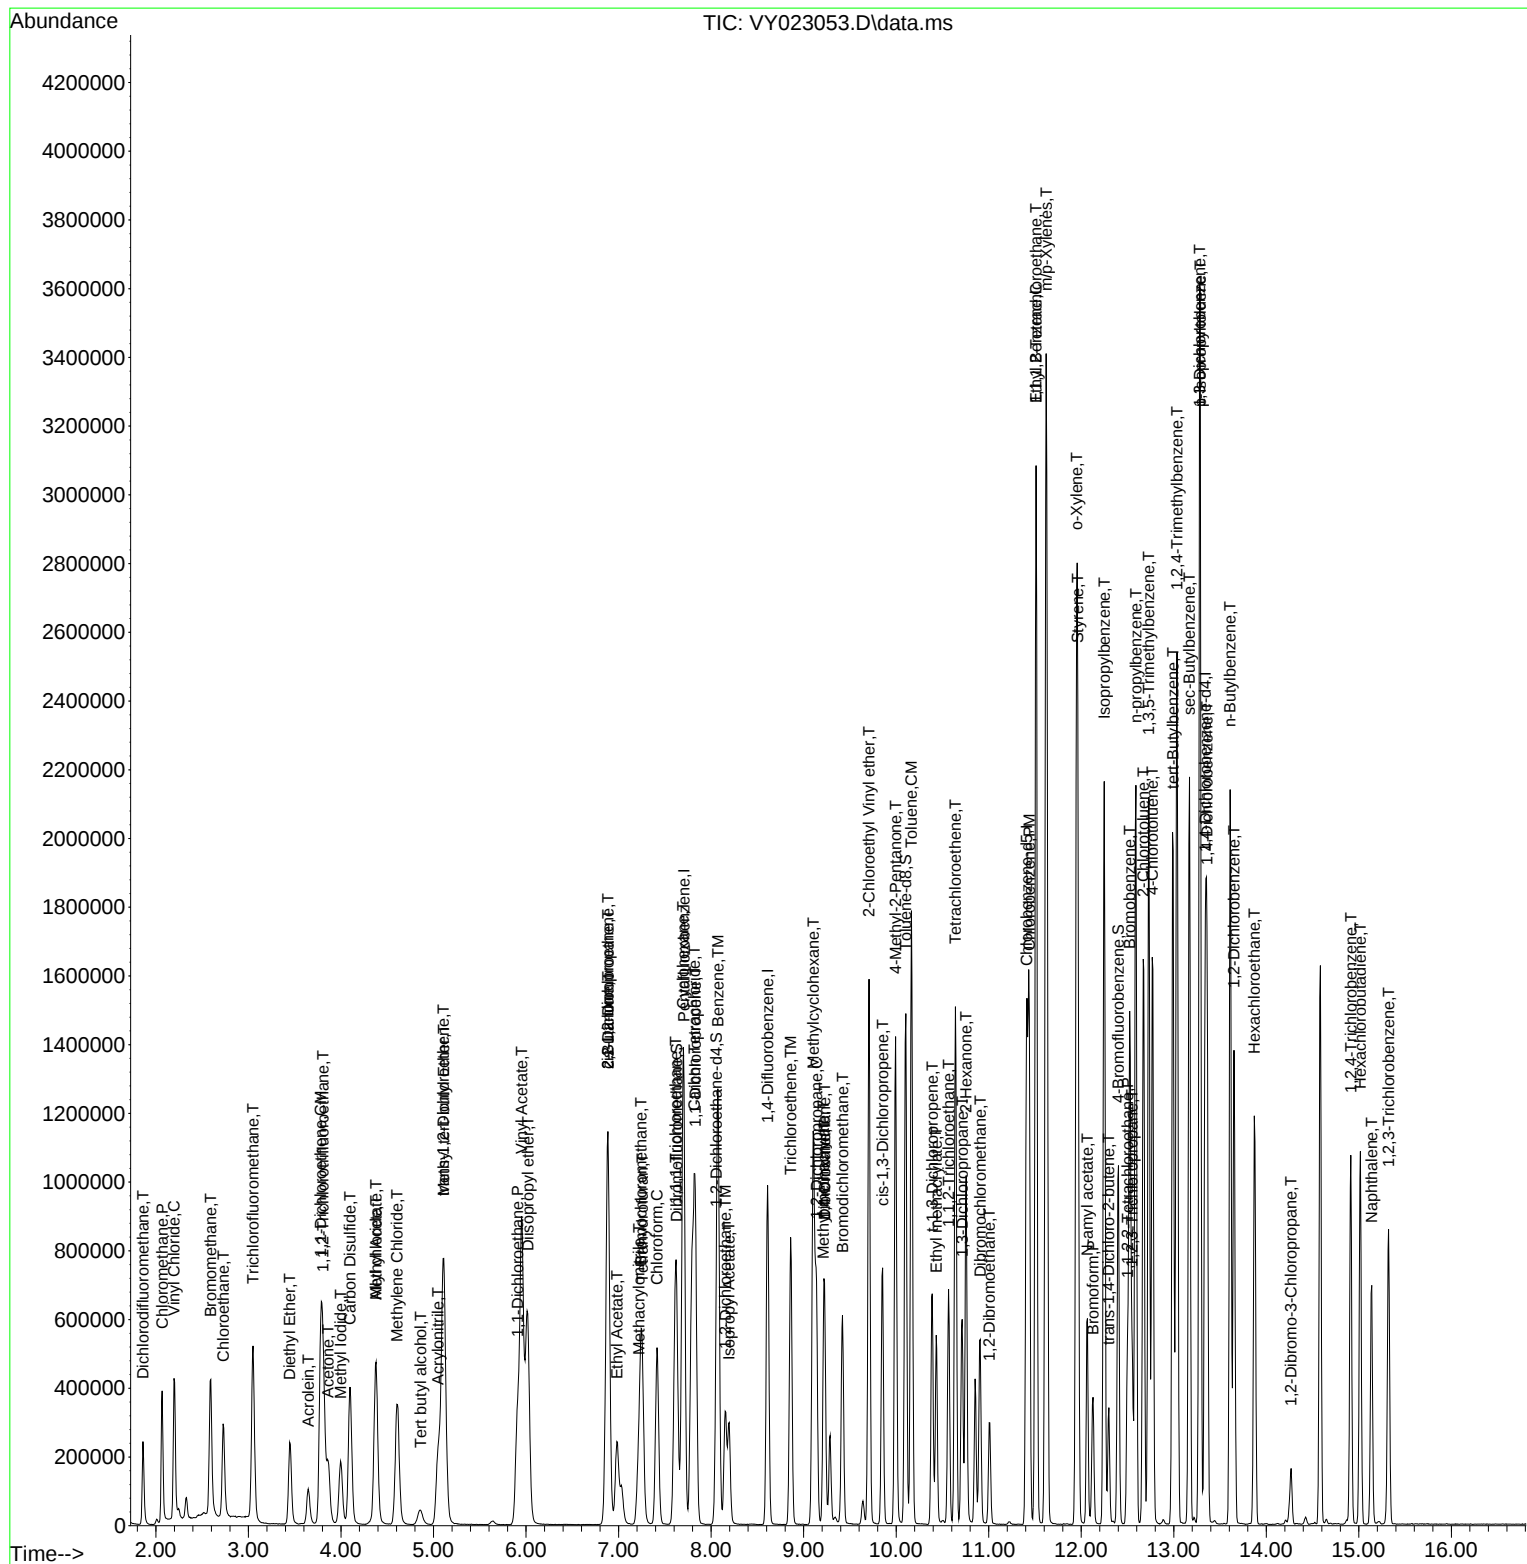

Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY081225\
 Data File : VY023054.D
 Acq On : 12 Aug 2025 16:25
 Operator : SY/MD
 Sample : VSTDICC100
 Misc : 5.00g/5.0mL/MSVOA_Y/SOIL
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_Y
 ClientSampleId :
 VSTDICC100

Manual Integrations
 APPROVED

Reviewed By :Mahesh Dadoda 08/14/2025
 Supervised By :Semsettin Yesilyurt 08/14/2025

Quant Time: Aug 13 01:54:25 2025
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y081225S.M
 Quant Title : SW846 8260
 QLast Update : Wed Aug 13 01:46:43 2025
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Pentafluorobenzene	7.707	168	558266	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	8.610	114	880463	50.000	ug/l	0.00
63) Chlorobenzene-d5	11.408	117	784385	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.340	152	404136	50.000	ug/l	0.00

System Monitoring Compounds

33) 1,2-Dichloroethane-d4	8.061	65	527356	99.115	ug/l	0.00
Spiked Amount	50.000	Range	50 - 163	Recovery	= 198.220%#	
35) Dibromofluoromethane	7.628	113	540106	102.518	ug/l	0.00
Spiked Amount	50.000	Range	54 - 147	Recovery	= 205.040%#	
50) Toluene-d8	10.103	98	2116445	102.832	ug/l	0.00
Spiked Amount	50.000	Range	58 - 134	Recovery	= 205.660%#	
62) 4-Bromofluorobenzene	12.402	95	702583	106.147	ug/l	0.00
Spiked Amount	50.000	Range	30 - 143	Recovery	= 212.300%#	

Target Compounds

						Qvalue
2) Dichlorodifluoromethane	1.867	85	376261	82.570	ug/l	98
3) Chloromethane	2.068	50	673475	91.248	ug/l	99
4) Vinyl Chloride	2.202	62	841648	92.250	ug/l	98
5) Bromomethane	2.586	94	643103	94.384	ug/l	100
6) Chloroethane	2.727	64	567515	93.563	ug/l	99
7) Trichlorofluoromethane	3.050	101	1005284	90.617	ug/l	99
8) Diethyl Ether	3.452	74	273400	93.150	ug/l	99
9) 1,1,2-Trichlorotrifluo...	3.812	101	497408	90.882	ug/l	99
10) Methyl Iodide	4.001	142	629775	106.635	ug/l	99
11) Tert butyl alcohol	4.866	59	162373	445.387	ug/l	99
12) 1,1-Dichloroethene	3.787	96	506919	94.229	ug/l	95
13) Acrolein	3.647	56	240580	450.599	ug/l	100
14) Allyl chloride	4.379	41	759925	96.000	ug/l	99
15) Acrylonitrile	5.049	53	555815	465.802	ug/l	99
16) Acetone	3.867	43	522178	453.007	ug/l	97
17) Carbon Disulfide	4.098	76	1622451	92.494	ug/l	100
18) Methyl Acetate	4.379	43	312127	90.993	ug/l	99
19) Methyl tert-butyl Ether	5.116	73	1342237	96.284	ug/l	100
20) Methylene Chloride	4.610	84	570465	97.847	ug/l	98
21) trans-1,2-Dichloroethene	5.110	96	580972	96.098	ug/l	99
22) Diisopropyl ether	6.019	45	1686285	98.033	ug/l	99
23) Vinyl Acetate	5.958	43	4632278	487.023	ug/l	100
24) 1,1-Dichloroethane	5.909	63	1012815	96.306	ug/l	100
25) 2-Butanone	6.890	43	722555	460.899	ug/l	97
26) 2,2-Dichloropropane	6.878	77	866598	95.497	ug/l	99
27) cis-1,2-Dichloroethene	6.884	96	681242	97.472	ug/l	100
28) Bromochloromethane	7.244	49	409677	98.188	ug/l	100
29) Tetrahydrofuran	7.256	42	451254	464.370	ug/l	100
30) Chloroform	7.415	83	1045381	96.383	ug/l	96
31) Cyclohexane	7.695	56	884707	89.271	ug/l	98
32) 1,1,1-Trichloroethane	7.610	97	929858	96.620	ug/l	99
36) 1,1-Dichloropropene	7.829	75	755114	96.443	ug/l	99
37) Ethyl Acetate	6.982	43	313447	95.302	ug/l	99
38) Carbon Tetrachloride	7.811	117	819941	96.419	ug/l	98
39) Methylcyclohexane	9.103	83	1011944	98.146	ug/l	99
40) Benzene	8.073	78	2348617	97.324	ug/l	99

Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY081225\
 Data File : VY023054.D
 Acq On : 12 Aug 2025 16:25
 Operator : SY/MD
 Sample : VSTDICC100
 Misc : 5.00g/5.0mL/MSVOA_Y/SOIL
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_Y
 ClientSampleId :
 VSTDICC100

Manual Integrations
 APPROVED

Reviewed By :Mahesh Dadoda 08/14/2025
 Supervised By :Semsettin Yesilyurt 08/14/2025

Quant Time: Aug 13 01:54:25 2025
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y081225S.M
 Quant Title : SW846 8260
 QLast Update : Wed Aug 13 01:46:43 2025
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
41) Methacrylonitrile	7.220	41	180468	94.973	ug/l	98
42) 1,2-Dichloroethane	8.152	62	597215	95.155	ug/l	100
43) Isopropyl Acetate	8.195	43	636710	95.780	ug/l	99
44) Trichloroethene	8.860	130	602322	96.584	ug/l	97
45) 1,2-Dichloropropane	9.140	63	543589	97.899	ug/l	99
46) Dibromomethane	9.225	93	309302	97.052	ug/l	99
47) Bromodichloromethane	9.420	83	802532	97.864	ug/l	98
48) Methyl methacrylate	9.219	41	319906	100.567	ug/l	99
49) 1,4-Dioxane	9.225	88	71300	1908.039	ug/l	94
51) 4-Methyl-2-Pentanone	9.994	43	1669668	486.924	ug/l	100
52) Toluene	10.164	92	1537088	100.288	ug/l	100
53) t-1,3-Dichloropropene	10.390	75	754278	101.574	ug/l	99
54) cis-1,3-Dichloropropene	9.853	75	880571	100.281	ug/l	99
55) 1,1,2-Trichloroethane	10.567	97	415556	97.446	ug/l	99
56) Ethyl methacrylate	10.432	69	569556	104.375	ug/l	100
57) 1,3-Dichloropropane	10.713	76	696130	96.253	ug/l	99
58) 2-Chloroethyl Vinyl ether	9.707	63	1389847	539.957	ug/l	99
59) 2-Hexanone	10.756	43	1151000	492.950	ug/l	100
60) Dibromochloromethane	10.902	129	557205	99.024	ug/l	99
61) 1,2-Dibromoethane	11.012	107	391650	97.713	ug/l	98
64) Tetrachloroethene	10.640	164	615871	87.931	ug/l	98
65) Chlorobenzene	11.438	112	1658154	98.004	ug/l	97
66) 1,1,1,2-Tetrachloroethane	11.512	131	573131	99.810	ug/l	99
67) Ethyl Benzene	11.512	91	2914020	100.082	ug/l	98
68) m/p-Xylenes	11.621	106	2312597	203.363	ug/l	98
69) o-Xylene	11.950	106	1100998	103.373	ug/l	99
70) Styrene	11.963	104	1845480	105.953	ug/l	99
71) Bromoform	12.127	173	334886	99.786	ug/l #	99
73) Isopropylbenzene	12.249	105	2839999	99.567	ug/l	99
74) N-amyl acetate	12.066	43	610668	100.955	ug/l	99
75) 1,1,2,2-Tetrachloroethane	12.499	83	469810	96.464	ug/l	100
76) 1,2,3-Trichloropropane	12.548	75	330554m	84.695	ug/l	
77) Bromobenzene	12.524	156	671329	98.655	ug/l	98
78) n-propylbenzene	12.591	91	3360679	98.963	ug/l	99
79) 2-Chlorotoluene	12.670	91	1931460	99.268	ug/l	100
80) 1,3,5-Trimethylbenzene	12.731	105	2321527	100.707	ug/l	99
81) trans-1,4-Dichloro-2-b...	12.298	75	153260	95.118	ug/l	100
82) 4-Chlorotoluene	12.767	91	1988544	98.519	ug/l	100
83) tert-Butylbenzene	12.993	119	2125785	102.102	ug/l	98
84) 1,2,4-Trimethylbenzene	13.036	105	2339432	101.946	ug/l	100
85) sec-Butylbenzene	13.170	105	3056373	99.932	ug/l	100
86) p-Isopropyltoluene	13.286	119	2610936	102.846	ug/l	100
87) 1,3-Dichlorobenzene	13.280	146	1338547	99.748	ug/l	99
88) 1,4-Dichlorobenzene	13.359	146	1290840	96.970	ug/l	99
89) n-Butylbenzene	13.609	91	2370706	101.675	ug/l	100
90) Hexachloroethane	13.871	117	510900	98.308	ug/l	99
91) 1,2-Dichlorobenzene	13.651	146	1162152	98.749	ug/l	99
92) 1,2-Dibromo-3-Chloropr...	14.267	75	69736	91.965	ug/l	97
93) 1,2,4-Trichlorobenzene	14.913	180	692201	99.460	ug/l	98
94) Hexachlorobutadiene	15.017	225	387707	94.803	ug/l	99
95) Naphthalene	15.133	128	1212227	102.147	ug/l	100
96) 1,2,3-Trichlorobenzene	15.322	180	587990	98.046	ug/l	100

Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY081225\
Data File : VY023054.D
Acq On : 12 Aug 2025 16:25
Operator : SY/MD
Sample : VSTDICC100
Misc : 5.00g/5.0mL/MSVOA_Y/SOIL
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_Y
ClientSampleId :
VSTDICC100

Manual Integrations
APPROVED

Reviewed By :Mahesh Dadoda 08/14/2025
Supervised By :Semsettin Yesilyurt 08/14/2025

Quant Time: Aug 13 01:54:25 2025
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y081225S.M
Quant Title : SW846 8260
QLast Update : Wed Aug 13 01:46:43 2025
Response via : Initial Calibration


Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
----------	------	------	----------	------	-------	----------

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Instrument :
MSVOA_Y
ClientSampleId :
VSTDICC100

Manual Integrations APPROVED

Reviewed By :Mahesh Dadoda 08/14/2025
Supervised By :Semsettin Yesilyurt 08/14/2025

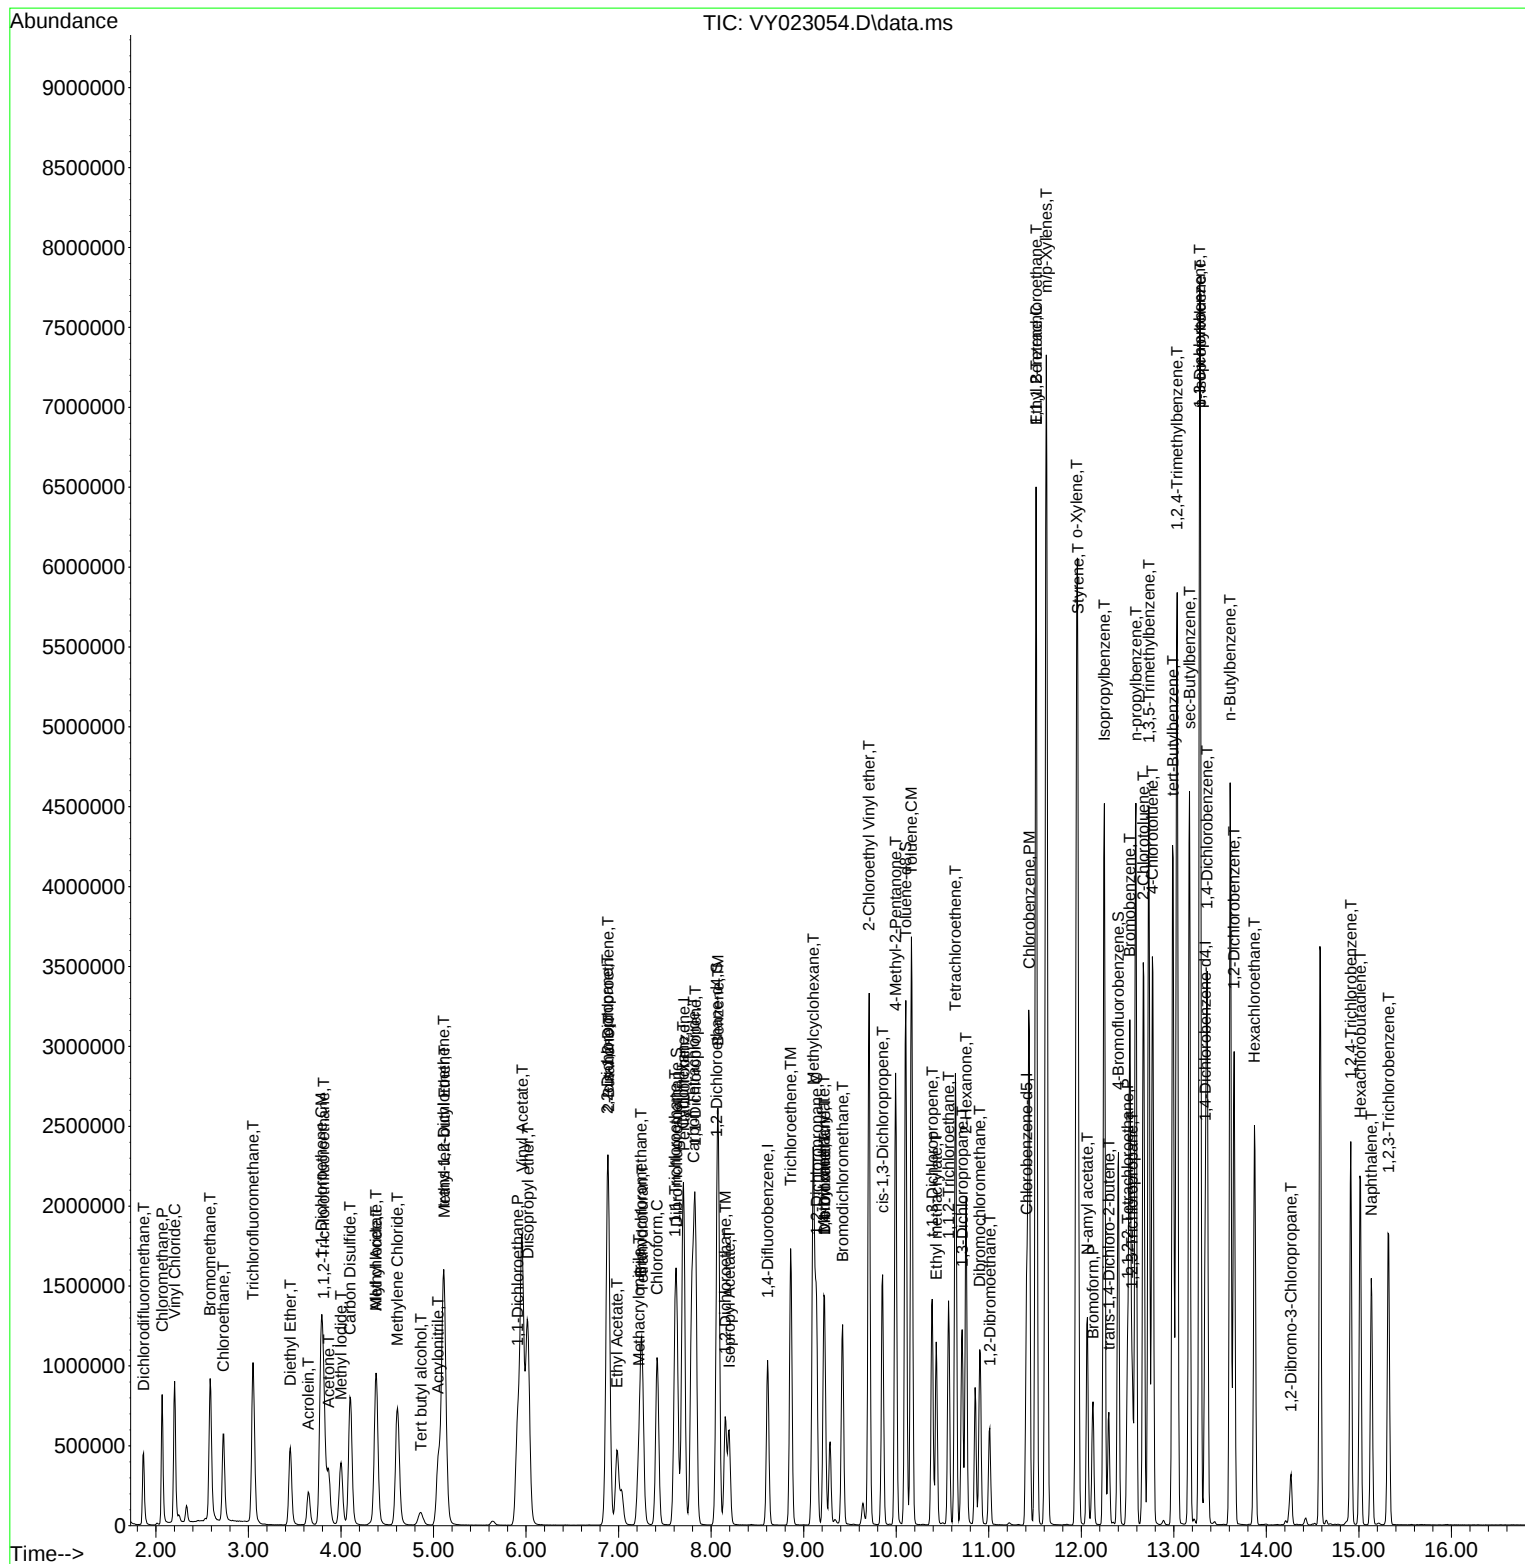

Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY081225\
 Data File : VY023055.D
 Acq On : 12 Aug 2025 16:47
 Operator : SY/MD
 Sample : VSTDICC150
 Misc : 5.00g/5.0mL/MSVOA_Y/SOIL
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 MSVOA_Y
 ClientSampleId :
 VSTDICC150

Manual Integrations
 APPROVED

Reviewed By :Mahesh Dadoda 08/14/2025
 Supervised By :Semsettin Yesilyurt 08/14/2025

Quant Time: Aug 13 01:55:24 2025
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y081225S.M
 Quant Title : SW846 8260
 QLast Update : Wed Aug 13 01:46:43 2025
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Pentafluorobenzene	7.701	168	538712	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	8.610	114	844092	50.000	ug/l	0.00
63) Chlorobenzene-d5	11.408	117	756365	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.340	152	389949	50.000	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	8.055	65	746936	145.480	ug/l	0.00
Spiked Amount 50.000	Range 50 - 163		Recovery = 290.960%#			
35) Dibromofluoromethane	7.628	113	771944	152.837	ug/l	0.00
Spiked Amount 50.000	Range 54 - 147		Recovery = 305.680%#			
50) Toluene-d8	10.103	98	3003834	152.237	ug/l	0.00
Spiked Amount 50.000	Range 58 - 134		Recovery = 304.480%#			
62) 4-Bromofluorobenzene	12.402	95	998318	157.326	ug/l	0.00
Spiked Amount 50.000	Range 30 - 143		Recovery = 314.660%#			
Target Compounds						Qvalue
2) Dichlorodifluoromethane	1.861	85	571723	130.017	ug/l	98
3) Chloromethane	2.062	50	991215	139.173	ug/l	99
4) Vinyl Chloride	2.202	62	1238646	140.692	ug/l	99
5) Bromomethane	2.580	94	938717	142.770	ug/l	100
6) Chloroethane	2.720	64	834547	142.581	ug/l	100
7) Trichlorofluoromethane	3.043	101	1574213	147.051	ug/l	99
8) Diethyl Ether	3.446	74	426242	150.496	ug/l	100
9) 1,1,2-Trichlorotrifluo...	3.806	101	763053	144.479	ug/l	99
10) Methyl Iodide	3.995	142	909378	159.567	ug/l	100
11) Tert butyl alcohol	4.860	59	265243	753.967	ug/l	100
12) 1,1-Dichloroethene	3.781	96	768098	147.960	ug/l	95
13) Acrolein	3.647	56	374594	727.070	ug/l	98
14) Allyl chloride	4.372	41	1151194	150.707	ug/l	99
15) Acrylonitrile	5.049	53	883293	767.115	ug/l	99
16) Acetone	3.866	43	777658	699.133	ug/l	100
17) Carbon Disulfide	4.098	76	2426564	143.357	ug/l	99
18) Methyl Acetate	4.379	43	500151	151.100	ug/l	99
19) Methyl tert-butyl Ether	5.110	73	2113920	157.144	ug/l	99
20) Methylene Chloride	4.604	84	846955	152.064	ug/l	99
21) trans-1,2-Dichloroethene	5.110	96	889517	152.474	ug/l	97
22) Diisopropyl ether	6.012	45	2594499	156.307	ug/l	99
23) Vinyl Acetate	5.951	43	7267824	791.851	ug/l	99
24) 1,1-Dichloroethane	5.909	63	1527663	150.534	ug/l	99
25) 2-Butanone	6.890	43	1144112	756.289	ug/l	97
26) 2,2-Dichloropropane	6.878	77	1293043	147.663	ug/l	99
27) cis-1,2-Dichloroethene	6.884	96	1047717	155.348	ug/l	98
28) Bromochloromethane	7.238	49	599841	148.984	ug/l	98
29) Tetrahydrofuran	7.256	42	734408	783.186	ug/l	99
30) Chloroform	7.415	83	1585686	151.505	ug/l	95
31) Cyclohexane	7.695	56	1354021	141.586	ug/l	98
32) 1,1,1-Trichloroethane	7.610	97	1396470	150.372	ug/l	100
36) 1,1-Dichloropropene	7.829	75	1132306	150.850	ug/l	99
37) Ethyl Acetate	6.982	43	494371	156.788	ug/l	99
38) Carbon Tetrachloride	7.811	117	1226800	150.478	ug/l	96
39) Methylcyclohexane	9.103	83	1556004	157.417	ug/l	98
40) Benzene	8.073	78	3533174	152.720	ug/l	100

Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY081225\
 Data File : VY023055.D
 Acq On : 12 Aug 2025 16:47
 Operator : SY/MD
 Sample : VSTDICC150
 Misc : 5.00g/5.0mL/MSVOA_Y/SOIL
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 MSVOA_Y
 ClientSampleId :
 VSTDICC150

Manual Integrations
 APPROVED

Reviewed By :Mahesh Dadoda 08/14/2025
 Supervised By :Semsettin Yesilyurt 08/14/2025

Quant Time: Aug 13 01:55:24 2025
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y081225S.M
 Quant Title : SW846 8260
 QLast Update : Wed Aug 13 01:46:43 2025
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
41) Methacrylonitrile	7.213	41	261721	143.669	ug/l	90
42) 1,2-Dichloroethane	8.152	62	909030	151.078	ug/l	100
43) Isopropyl Acetate	8.195	43	1029854	161.596	ug/l	98
44) Trichloroethene	8.860	130	909510	152.126	ug/l	94
45) 1,2-Dichloropropane	9.134	63	822035	154.426	ug/l	99
46) Dibromomethane	9.225	93	480162	157.156	ug/l	100
47) Bromodichloromethane	9.420	83	1217658	154.884	ug/l	99
48) Methyl methacrylate	9.213	41	497527	163.144	ug/l	97
49) 1,4-Dioxane	9.225	88	117513	3280.235	ug/l	98
51) 4-Methyl-2-Pentanone	9.993	43	2677587	814.509	ug/l	99
52) Toluene	10.164	92	2332797	158.762	ug/l	99
53) t-1,3-Dichloropropene	10.390	75	1162952	163.355	ug/l	99
54) cis-1,3-Dichloropropene	9.853	75	1366797	162.359	ug/l	99
55) 1,1,2-Trichloroethane	10.567	97	642236	157.090	ug/l	98
56) Ethyl methacrylate	10.432	69	908662	173.693	ug/l	100
57) 1,3-Dichloropropane	10.713	76	1087297	156.818	ug/l	100
58) 2-Chloroethyl Vinyl ether	9.707	63	2167815	878.488	ug/l	99
59) 2-Hexanone	10.756	43	1848093	825.606	ug/l	100
60) Dibromochloromethane	10.908	129	860181	159.454	ug/l	99
61) 1,2-Dibromoethane	11.012	107	613069	159.546	ug/l	99
64) Tetrachloroethene	10.640	164	990664	146.682	ug/l	98
65) Chlorobenzene	11.438	112	2520874	154.514	ug/l	97
66) 1,1,1,2-Tetrachloroethane	11.511	131	871003	157.304	ug/l	99
67) Ethyl Benzene	11.511	91	4438665	158.093	ug/l	98
68) m/p-Xylenes	11.621	106	3511726	320.251	ug/l	96
69) o-Xylene	11.950	106	1683720	163.941	ug/l	100
70) Styrene	11.963	104	2846443	169.475	ug/l	99
71) Bromoform	12.127	173	523541	161.778	ug/l #	98
73) Isopropylbenzene	12.249	105	4269945	155.145	ug/l	99
74) N-amyl acetate	12.066	43	982090	168.265	ug/l	99
75) 1,1,2,2-Tetrachloroethane	12.499	83	717524	152.686	ug/l	100
76) 1,2,3-Trichloropropane	12.548	75	519276m	137.890	ug/l	
77) Bromobenzene	12.523	156	1021449	155.568	ug/l	99
78) n-propylbenzene	12.591	91	5048012	154.058	ug/l	99
79) 2-Chlorotoluene	12.676	91	2878647	153.331	ug/l	100
80) 1,3,5-Trimethylbenzene	12.731	105	3469329	155.973	ug/l	99
81) trans-1,4-Dichloro-2-b...	12.298	75	245958	158.203	ug/l	97
82) 4-Chlorotoluene	12.773	91	2981042	153.063	ug/l	99
83) tert-Butylbenzene	12.993	119	3161475	157.371	ug/l	99
84) 1,2,4-Trimethylbenzene	13.036	105	3501626	158.143	ug/l	100
85) sec-Butylbenzene	13.170	105	4541629	153.897	ug/l	99
86) p-Isopropyltoluene	13.286	119	3918969	159.987	ug/l	99
87) 1,3-Dichlorobenzene	13.279	146	2049060	158.251	ug/l	99
88) 1,4-Dichlorobenzene	13.359	146	1941716	151.172	ug/l	98
89) n-Butylbenzene	13.609	91	3578272	159.048	ug/l	100
90) Hexachloroethane	13.871	117	772603	154.073	ug/l	99
91) 1,2-Dichlorobenzene	13.651	146	1754100	154.469	ug/l	100
92) 1,2-Dibromo-3-Chloropr...	14.267	75	114505	156.498	ug/l	96
93) 1,2,4-Trichlorobenzene	14.913	180	1117401	166.397	ug/l	98
94) Hexachlorobutadiene	15.017	225	589351	149.352	ug/l	99
95) Naphthalene	15.139	128	2094983	182.954	ug/l	100
96) 1,2,3-Trichlorobenzene	15.322	180	975366	168.557	ug/l	99

Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY081225\
Data File : VY023055.D
Acq On : 12 Aug 2025 16:47
Operator : SY/MD
Sample : VSTDICC150
Misc : 5.00g/5.0mL/MSVOA_Y/SOIL
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_Y
ClientSampleId :
VSTDICC150

Manual Integrations
APPROVED

Reviewed By :Mahesh Dadoda 08/14/2025
Supervised By :Semsettin Yesilyurt 08/14/2025

Quant Time: Aug 13 01:55:24 2025
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y081225S.M
Quant Title : SW846 8260
QLast Update : Wed Aug 13 01:46:43 2025
Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
----------	------	------	----------	------	-------	----------

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY081225\
 Data File : VY023055.D
 Acq On : 12 Aug 2025 16:47
 Operator : SY/MD
 Sample : VSTDICC150
 Misc : 5.00g/5.0mL/MSVOA_Y/SOIL
 ALS Vial : 8 Sample Multiplier: 1

Instrument :

MSVOA_Y

ClientSampleId :

VSTDICC150

Manual Integrations

APPROVED

Reviewed By :Mahesh Dadoda 08/14/2025
 Supervised By :Semsettin Yesilyurt 08/14/2025


Quant Time: Aug 13 01:55:24 2025

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y081225S.M

Quant Title : SW846 8260

QLast Update : Wed Aug 13 01:46:43 2025

Response via : Initial Calibration

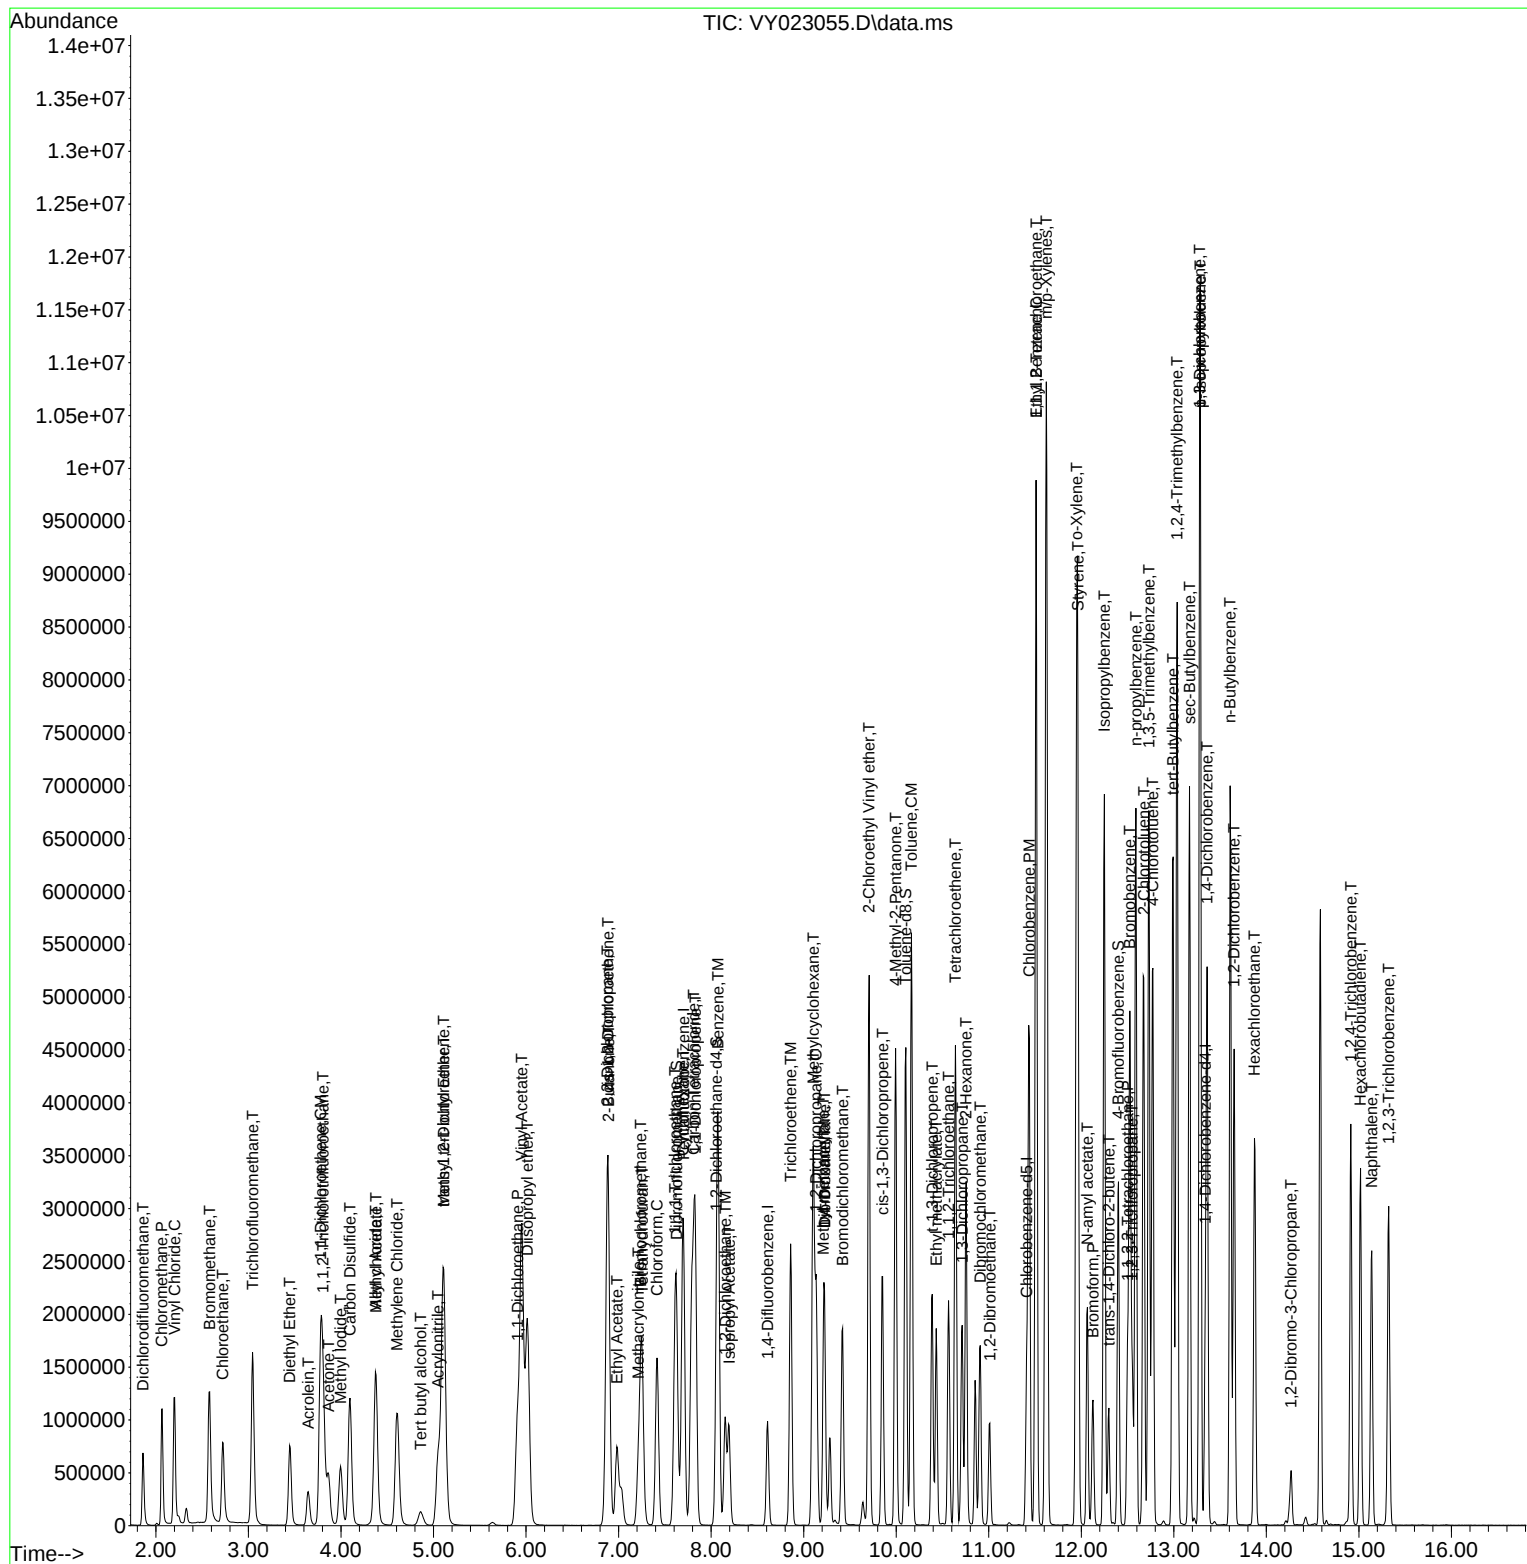

Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY081225\
 Data File : VY023057.D
 Acq On : 12 Aug 2025 17:53
 Operator : SY/MD
 Sample : VSTDICV050
 Misc : 5.00g/5.0mL/MSVOA_Y/SOIL
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 MSVOA_Y
 ClientSampleId :
 ICVVY081225

Manual Integrations
 APPROVED

Reviewed By :Mahesh Dadoda 08/14/2025
 Supervised By :Semsettin Yesilyurt 08/14/2025

Quant Time: Aug 13 02:14:27 2025
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y081225S.M
 Quant Title : SW846 8260
 QLast Update : Wed Aug 13 02:10:11 2025
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Pentafluorobenzene	7.707	168	528657	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	8.610	114	849851	50.000	ug/l	0.00
63) Chlorobenzene-d5	11.414	117	756555	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.340	152	376990	50.000	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	8.055	65	252116	50.038	ug/l	0.00
Spiked Amount 50.000	Range 50 - 163		Recovery = 100.080%			
35) Dibromofluoromethane	7.628	113	255171	50.179	ug/l	0.00
Spiked Amount 50.000	Range 54 - 147		Recovery = 100.360%			
50) Toluene-d8	10.103	98	979510	49.306	ug/l	0.00
Spiked Amount 50.000	Range 58 - 134		Recovery = 98.620%			
62) 4-Bromofluorobenzene	12.402	95	329022	51.500	ug/l	0.00
Spiked Amount 50.000	Range 30 - 143		Recovery = 103.000%			
Target Compounds						
					Qvalue	
2) Dichlorodifluoromethane	1.867	85	179421	41.579	ug/l	99
3) Chloromethane	2.068	50	340600	48.732	ug/l	100
4) Vinyl Chloride	2.202	62	416413	48.198	ug/l	99
5) Bromomethane	2.592	94	303147	46.983	ug/l	98
6) Chloroethane	2.733	64	281008	48.923	ug/l	99
7) Trichlorofluoromethane	3.050	101	493782	47.003	ug/l	100
8) Diethyl Ether	3.452	74	132818	47.787	ug/l	99
9) 1,1,2-Trichlorotrifluo...	3.812	101	247351	47.725	ug/l	99
10) Methyl Iodide	4.001	142	287126	51.340	ug/l	99
11) Tert butyl alcohol	4.860	59	84906	245.940	ug/l	98
12) 1,1-Dichloroethene	3.787	96	242931	47.686	ug/l	95
13) Acrolein	3.647	56	112246	222.008	ug/l	98
14) Allyl chloride	4.379	41	354691	47.317	ug/l	99
15) Acrylonitrile	5.055	53	274329	242.779	ug/l	99
16) Acetone	3.867	43	229985	210.695	ug/l	96
17) Carbon Disulfide	4.104	76	779852	46.948	ug/l	99
18) Methyl Acetate	4.385	43	168821	51.972	ug/l	99
19) Methyl tert-butyl Ether	5.116	73	658713	49.899	ug/l	100
20) Methylene Chloride	4.610	84	283386	49.960	ug/l	98
21) trans-1,2-Dichloroethene	5.110	96	279182	48.765	ug/l	98
22) Diisopropyl ether	6.019	45	814622	50.011	ug/l	97
23) Vinyl Acetate	5.958	43	2182924	242.360	ug/l	100
24) 1,1-Dichloroethane	5.915	63	483509	48.551	ug/l	100
25) 2-Butanone	6.890	43	341490	230.028	ug/l	99
26) 2,2-Dichloropropane	6.884	77	390777	45.475	ug/l	99
27) cis-1,2-Dichloroethene	6.884	96	322451	48.720	ug/l	99
28) Bromochloromethane	7.238	49	198640	50.275	ug/l	100
29) Tetrahydrofuran	7.262	42	227680	247.420	ug/l	100
30) Chloroform	7.421	83	497627	48.450	ug/l	97
31) Cyclohexane	7.695	56	436638	46.526	ug/l	98
32) 1,1,1-Trichloroethane	7.610	97	445943	48.933	ug/l	100
36) 1,1-Dichloropropene	7.829	75	364210	48.193	ug/l	99
37) Ethyl Acetate	6.982	43	157530	49.621	ug/l	99
38) Carbon Tetrachloride	7.817	117	394245	48.030	ug/l	99
39) Methylcyclohexane	9.103	83	493867	49.625	ug/l	98
40) Benzene	8.073	78	1128023	48.428	ug/l	100

Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY081225\
 Data File : VY023057.D
 Acq On : 12 Aug 2025 17:53
 Operator : SY/MD
 Sample : VSTDICV050
 Misc : 5.00g/5.0mL/MSVOA_Y/SOIL
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 MSVOA_Y
 ClientSampleId :
 ICVVY081225

Manual Integrations
 APPROVED

Reviewed By :Mahesh Dadoda 08/14/2025
 Supervised By :Semsettin Yesilyurt 08/14/2025

Quant Time: Aug 13 02:14:27 2025
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y081225S.M
 Quant Title : SW846 8260
 QLast Update : Wed Aug 13 02:10:11 2025
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
41) Methacrylonitrile	7.220	41	88437	48.269	ug/l	99
42) 1,2-Dichloroethane	8.152	62	291766	48.162	ug/l	100
43) Isopropyl Acetate	8.195	43	315013	49.094	ug/l	98
44) Trichloroethene	8.860	130	287745	47.803	ug/l	95
45) 1,2-Dichloropropane	9.140	63	262408	48.961	ug/l	98
46) Dibromomethane	9.225	93	149745	48.679	ug/l	99
47) Bromodichloromethane	9.420	83	391522	49.463	ug/l	98
48) Methyl methacrylate	9.219	41	155118	50.520	ug/l	99
49) 1,4-Dioxane	9.225	88	35050	971.749	ug/l	98
51) 4-Methyl-2-Pentanone	9.993	43	823949	248.943	ug/l	99
52) Toluene	10.164	92	724356	48.963	ug/l	100
53) t-1,3-Dichloropropene	10.390	75	356228	49.699	ug/l	99
54) cis-1,3-Dichloropropene	9.853	75	415017	48.965	ug/l	97
55) 1,1,2-Trichloroethane	10.567	97	201146	48.867	ug/l	98
56) Ethyl methacrylate	10.432	69	267458	50.779	ug/l	99
57) 1,3-Dichloropropane	10.713	76	343649	49.228	ug/l	99
58) 2-Chloroethyl Vinyl ether	9.707	63	678865	273.240	ug/l	100
59) 2-Hexanone	10.756	43	551743	244.812	ug/l	99
60) Dibromochloromethane	10.908	129	270536	49.810	ug/l	99
61) 1,2-Dibromoethane	11.012	107	190334	49.197	ug/l	100
64) Tetrachloroethene	10.640	164	307456	45.512	ug/l	98
65) Chlorobenzene	11.438	112	787799	48.275	ug/l	97
66) 1,1,1,2-Tetrachloroethane	11.512	131	270360	48.815	ug/l	99
67) Ethyl Benzene	11.512	91	1380648	49.163	ug/l	100
68) m/p-Xylenes	11.621	106	1080541	98.515	ug/l	99
69) o-Xylene	11.950	106	509991	49.645	ug/l	99
70) Styrene	11.963	104	852310	50.733	ug/l	99
71) Bromoform	12.127	173	157073	48.525	ug/l #	98
73) Isopropylbenzene	12.249	105	1327070	49.876	ug/l	100
74) N-amyl acetate	12.066	43	285118	50.529	ug/l	100
75) 1,1,2,2-Tetrachloroethane	12.499	83	224206	49.350	ug/l	98
76) 1,2,3-Trichloropropane	12.548	75	167859m	46.136	ug/l	
77) Bromobenzene	12.524	156	311065	49.004	ug/l	99
78) n-propylbenzene	12.591	91	1610911	50.853	ug/l	100
79) 2-Chlorotoluene	12.676	91	905657	49.898	ug/l	100
80) 1,3,5-Trimethylbenzene	12.731	105	1094902	50.916	ug/l	99
81) trans-1,4-Dichloro-2-b...	12.298	75	74263	49.409	ug/l	98
82) 4-Chlorotoluene	12.774	91	932114	49.505	ug/l	100
83) tert-Butylbenzene	12.993	119	979692	50.443	ug/l	99
84) 1,2,4-Trimethylbenzene	13.036	105	1092616	51.042	ug/l	100
85) sec-Butylbenzene	13.170	105	1459437	51.154	ug/l	100
86) p-Isopropyltoluene	13.286	119	1222900	51.639	ug/l	100
87) 1,3-Dichlorobenzene	13.280	146	621371	49.639	ug/l	98
88) 1,4-Dichlorobenzene	13.359	146	602429	48.514	ug/l	99
89) n-Butylbenzene	13.609	91	1122189	51.594	ug/l	100
90) Hexachloroethane	13.871	117	245386	50.617	ug/l	99
91) 1,2-Dichlorobenzene	13.651	146	540506	49.234	ug/l	99
92) 1,2-Dibromo-3-Chloropr...	14.267	75	35428	50.085	ug/l	98
93) 1,2,4-Trichlorobenzene	14.913	180	320472	49.363	ug/l	99
94) Hexachlorobutadiene	15.017	225	184430	48.344	ug/l	99
95) Naphthalene	15.139	128	571480	51.623	ug/l	100
96) 1,2,3-Trichlorobenzene	15.322	180	272638	48.735	ug/l	100

Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY081225\
Data File : VY023057.D
Acq On : 12 Aug 2025 17:53
Operator : SY/MD
Sample : VSTDICV050
Misc : 5.00g/5.0mL/MSVOA_Y/SOIL
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_Y
ClientSampleId :
ICVVY081225

Manual Integrations
APPROVED

Reviewed By :Mahesh Dadoda 08/14/2025
Supervised By :Semsettin Yesilyurt 08/14/2025

Quant Time: Aug 13 02:14:27 2025
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y081225S.M
Quant Title : SW846 8260
QLast Update : Wed Aug 13 02:10:11 2025
Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
----------	------	------	----------	------	-------	----------

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY081225\
Data File : VY023057.D
Acq On : 12 Aug 2025 17:53
Operator : SY/MD
Sample : VSTDICV050
Misc : 5.00g/5.0mL/MSVOA_Y/SOIL
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_Y
ClientSampleId :
ICVY081225

Manual Integrations APPROVED

Reviewed By :Mahesh Dadoda 08/14/2025
Supervised By :Semsettin Yesilyurt 08/14/2025

Quant Time: Aug 13 02:14:27 2025
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y081225S.M
Quant Title : SW846 8260
QLast Update : Wed Aug 13 02:10:11 2025
Response via : Initial Calibration

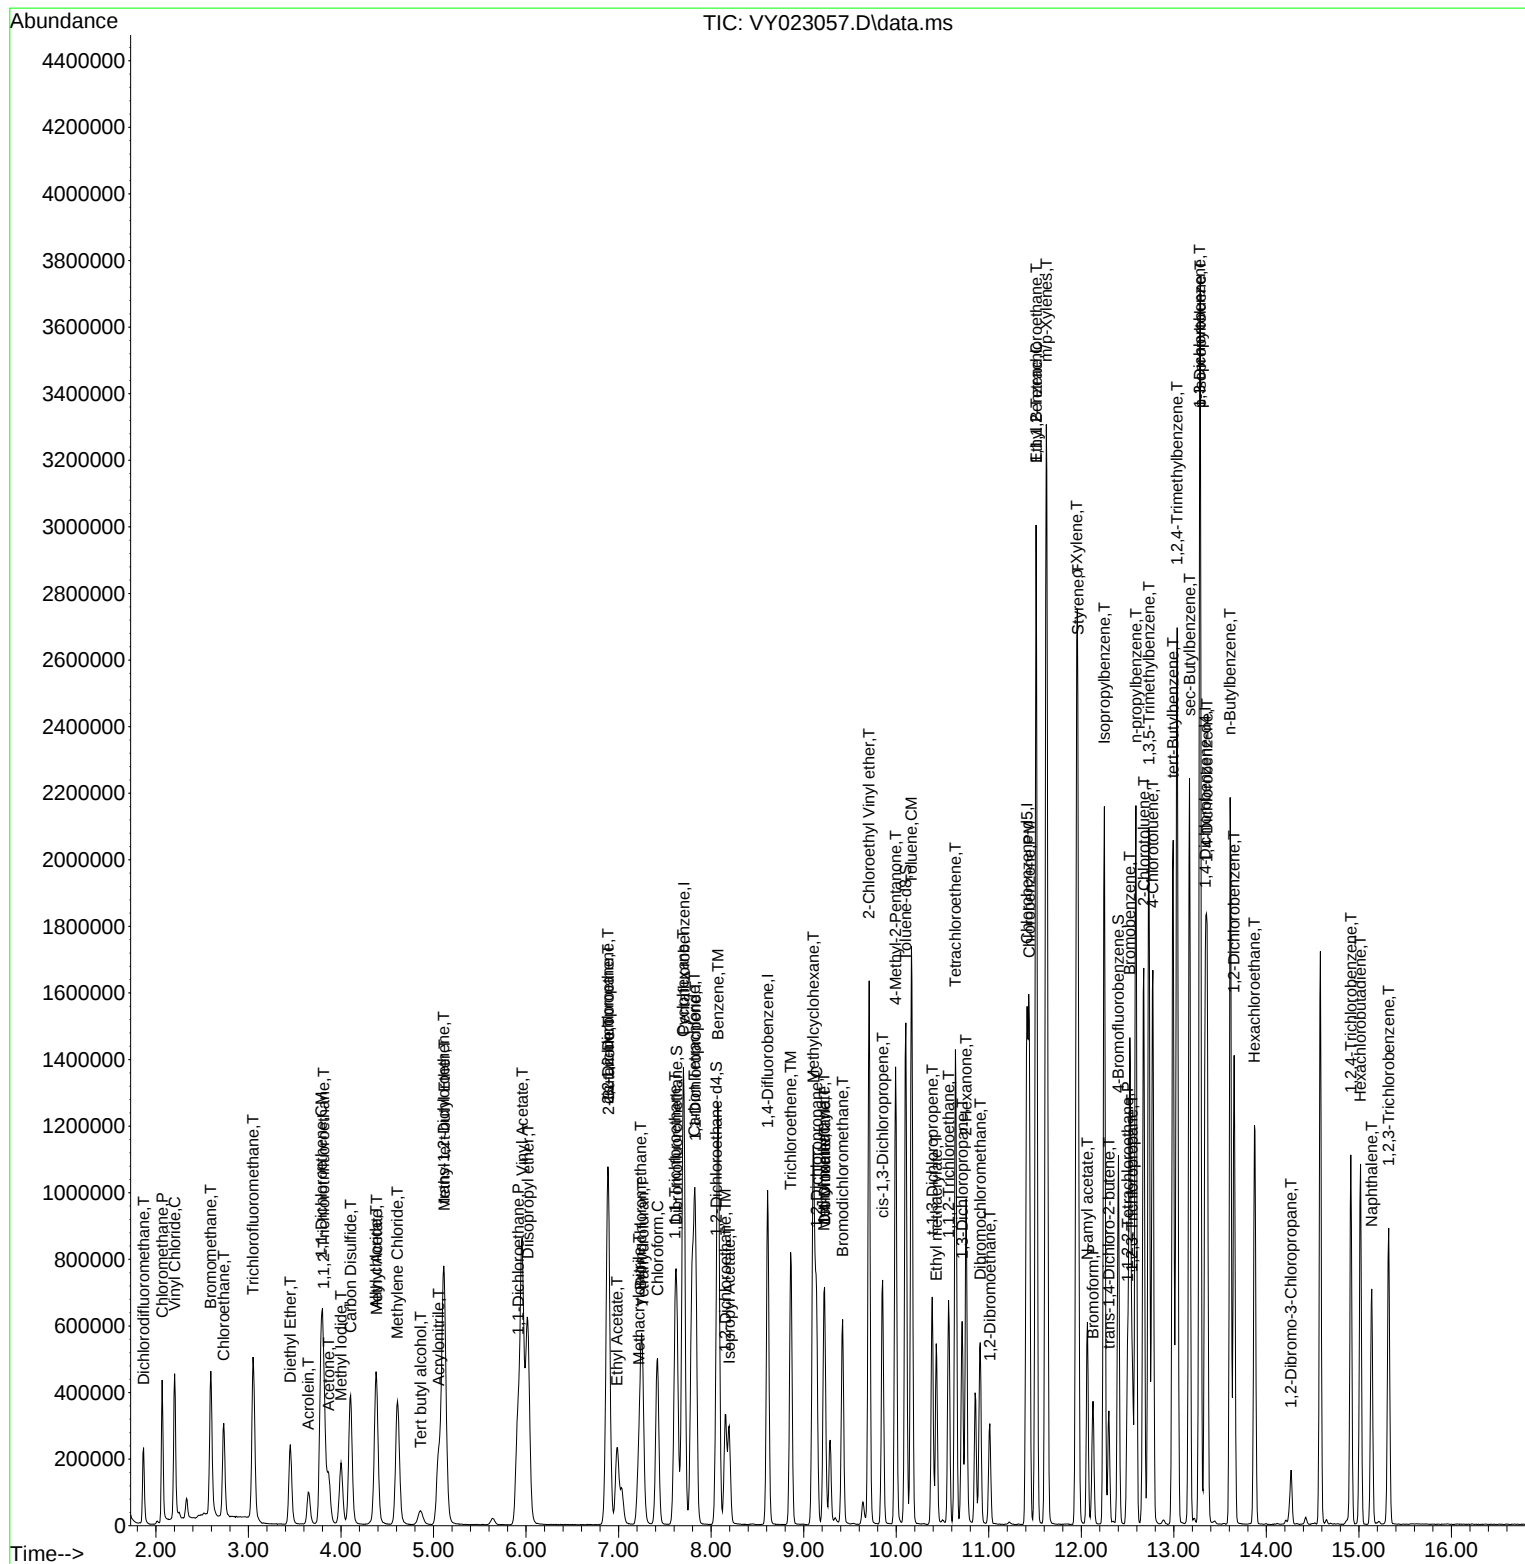

Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY081225\
 Data File : VY023057.D
 Acq On : 12 Aug 2025 17:53
 Operator : SY/MD
 Sample : VSTDICV050
 Misc : 5.00g/5.0mL/MSVOA_Y/SOIL
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 MSVOA_Y
 ClientSampleId :
 ICVVY081225

Quant Time: Aug 13 02:14:27 2025
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y081225S.M
 Quant Title : SW846 8260
 QLast Update : Wed Aug 13 02:10:11 2025
 Response via : Initial Calibration

Min. RRF : 0.000 Min. Rel. Area : 50% Max. R.T. Dev 0.50min
 Max. RRF Dev : 25% Max. Rel. Area : 150%

	Compound	AvgRF	CCRF	%Dev	Area%	Dev(min)
1 I	Pentafluorobenzene	1.000	1.000	0.0	98	0.00
2 T	Dichlorodifluoromethane	0.408	0.339	16.9	96	0.00
3 P	Chloromethane	0.661	0.644	2.6	104	0.00
4 C	Vinyl Chloride	0.817	0.788	3.5#	100	0.00
5 T	Bromomethane	0.610	0.573	6.1	104	0.00
6 T	Chloroethane	0.543	0.532	2.0	101	0.00
7 T	Trichlorofluoromethane	0.994	0.934	6.0	98	0.00
8 T	Diethyl Ether	0.263	0.251	4.6	98	0.00
9 T	1,1,2-Trichlorotrifluoroeth	0.490	0.468	4.5	99	0.00
10 T	Methyl Iodide	0.529	0.543	-2.6	97	0.00
11 T	Tert butyl alcohol	0.033	0.032	3.0	99	0.00
12 CM	1,1-Dichloroethene	0.482	0.460	4.6#	97	0.00
13 T	Acrolein	0.048	0.042	12.5	93	0.00
14 T	Allyl chloride	0.709	0.671	5.4	96	0.00
15 T	Acrylonitrile	0.107	0.104	2.8	96	0.00
16 T	Acetone	0.103	0.087	15.5	83	0.00
17 T	Carbon Disulfide	1.571	1.475	6.1	97	0.00
18 T	Methyl Acetate	0.307	0.319	-3.9	97	0.00
19 T	Methyl tert-butyl Ether	1.249	1.246	0.2	99	0.00
20 T	Methylene Chloride	0.620	0.536	13.5	103	0.00
21 T	trans-1,2-Dichloroethene	0.541	0.528	2.4	99	0.00
22 T	Diisopropyl ether	1.541	1.541	0.0	100	0.00
23 T	Vinyl Acetate	0.852	0.826	3.1	96	0.00
24 P	1,1-Dichloroethane	0.942	0.915	2.9	98	0.00
25 T	2-Butanone	0.140	0.129	7.9	89	0.00
26 T	2,2-Dichloropropane	0.813	0.739	9.1	92	0.00
27 T	cis-1,2-Dichloroethene	0.626	0.610	2.6	99	0.00
28 T	Bromochloromethane	0.374	0.376	-0.5	101	0.00
29 T	Tetrahydrofuran	0.087	0.086	1.1	97	0.00
30 C	Chloroform	0.971	0.941	3.1#	98	0.00
31 T	Cyclohexane	0.888	0.826	7.0	99	0.00
32 T	1,1,1-Trichloroethane	0.862	0.844	2.1	99	0.00
33 S	1,2-Dichloroethane-d4	0.477	0.477	0.0	101	0.00
34 I	1,4-Difluorobenzene	1.000	1.000	0.0	99	0.00
35 S	Dibromofluoromethane	0.299	0.300	-0.3	102	0.00
36 T	1,1-Dichloropropene	0.445	0.429	3.6	98	0.00
37 T	Ethyl Acetate	0.187	0.185	1.1	98	0.00
38 T	Carbon Tetrachloride	0.483	0.464	3.9	99	0.00
39 T	Methylcyclohexane	0.586	0.581	0.9	102	0.00
40 TM	Benzene	1.370	1.327	3.1	99	0.00
41 T	Methacrylonitrile	0.108	0.104	3.7	94	0.00
42 TM	1,2-Dichloroethane	0.356	0.343	3.7	98	0.00
43 T	Isopropyl Acetate	0.378	0.371	1.9	99	0.00
44 TM	Trichloroethene	0.354	0.339	4.2	98	0.00
45 C	1,2-Dichloropropane	0.315	0.309	1.9#	99	0.00
46 T	Dibromomethane	0.181	0.176	2.8	98	0.00
47 T	Bromodichloromethane	0.466	0.461	1.1	99	0.00
48 T	Methyl methacrylate	0.181	0.183	-1.1	96	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY081225\
 Data File : VY023057.D
 Acq On : 12 Aug 2025 17:53
 Operator : SY/MD
 Sample : VSTDICV050
 Misc : 5.00g/5.0mL/MSVOA_Y/SOIL
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 MSVOA_Y
 ClientSampleId :
 ICSVY081225

Quant Time: Aug 13 02:14:27 2025
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y081225S.M
 Quant Title : SW846 8260
 QLast Update : Wed Aug 13 02:10:11 2025
 Response via : Initial Calibration

Min. RRF : 0.000 Min. Rel. Area : 50% Max. R.T. Dev 0.50min
 Max. RRF Dev : 25% Max. Rel. Area : 150%

	Compound	AvgRF	CCRF	%Dev	Area%	Dev(min)
49 T	1,4-Dioxane	0.002	0.002	0.0	97	0.00
50 S	Toluene-d8	1.169	1.153	1.4	100	0.00
51 T	4-Methyl-2-Pentanone	0.195	0.194	0.5	97	0.00
52 CM	Toluene	0.870	0.852	2.1#	99	0.00
53 T	t-1,3-Dichloropropene	0.422	0.419	0.7	99	0.00
54 T	cis-1,3-Dichloropropene	0.499	0.488	2.2	98	0.00
55 T	1,1,2-Trichloroethane	0.242	0.237	2.1	98	0.00
56 T	Ethyl methacrylate	0.310	0.315	-1.6	98	0.00
57 T	1,3-Dichloropropane	0.411	0.404	1.7	99	0.00
58 T	2-Chloroethyl Vinyl ether	0.146	0.160	-9.6	102	0.00
59 T	2-Hexanone	0.133	0.130	2.3	94	0.00
60 T	Dibromochloromethane	0.320	0.318	0.6	99	0.00
61 T	1,2-Dibromoethane	0.228	0.224	1.8	98	0.00
62 S	4-Bromofluorobenzene	0.376	0.387	-2.9	104	0.00
63 I	Chlorobenzene-d5	1.000	1.000	0.0	101	0.00
64 T	Tetrachloroethene	0.446	0.406	9.0	94	0.00
65 PM	Chlorobenzene	1.079	1.041	3.5	99	0.00
66 T	1,1,1,2-Tetrachloroethane	0.366	0.357	2.5	99	0.00
67 C	Ethyl Benzene	1.856	1.825	1.7#	99	0.00
68 T	m/p-Xylenes	0.725	0.714	1.5	100	0.00
69 T	o-Xylene	0.679	0.674	0.7	99	0.00
70 T	Styrene	1.110	1.127	-1.5	101	0.00
71 P	Bromoform	0.214	0.208	2.8	98	0.00
72 I	1,4-Dichlorobenzene-d4	1.000	1.000	0.0	100	0.00
73 T	Isopropylbenzene	3.529	3.520	0.3	100	0.00
74 T	N-amyl acetate	0.748	0.756	-1.1	98	0.00
75 P	1,1,2,2-Tetrachloroethane	0.603	0.595	1.3	102	0.00
76 T	1,2,3-Trichloropropane	0.483	0.445	7.9	83	0.00
77 T	Bromobenzene	0.842	0.825	2.0	99	0.00
78 T	n-propylbenzene	4.201	4.273	-1.7	101	0.00
79 T	2-Chlorotoluene	2.407	2.402	0.2	101	0.00
80 T	1,3,5-Trimethylbenzene	2.852	2.904	-1.8	101	0.00
81 T	trans-1,4-Dichloro-2-butene	0.199	0.197	1.0	100	0.00
82 T	4-Chlorotoluene	2.497	2.473	1.0	100	0.00
83 T	tert-Butylbenzene	2.576	2.599	-0.9	100	0.00
84 T	1,2,4-Trimethylbenzene	2.839	2.898	-2.1	102	0.00
85 T	sec-Butylbenzene	3.784	3.871	-2.3	102	0.00
86 T	p-Isopropyltoluene	3.141	3.244	-3.3	102	0.00
87 T	1,3-Dichlorobenzene	1.660	1.648	0.7	102	0.00
88 T	1,4-Dichlorobenzene	1.647	1.598	3.0	100	0.00
89 T	n-Butylbenzene	2.885	2.977	-3.2	102	0.00
90 T	Hexachloroethane	0.643	0.651	-1.2	103	0.00
91 T	1,2-Dichlorobenzene	1.456	1.434	1.5	101	0.00
92 T	1,2-Dibromo-3-Chloropropane	0.094	0.094	0.0	99	0.00
93 T	1,2,4-Trichlorobenzene	0.861	0.850	1.3	100	0.00
94 T	Hexachlorobutadiene	0.506	0.489	3.4	99	0.00
95 T	Naphthalene	1.468	1.516	-3.3	102	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY081225\
Data File : VY023057.D
Acq On : 12 Aug 2025 17:53
Operator : SY/MD
Sample : VSTDICV050
Misc : 5.00g/5.0mL/MSVOA_Y/SOIL
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_Y
ClientSampleId :
ICVVY081225

Quant Time: Aug 13 02:14:27 2025
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y081225S.M
Quant Title : SW846 8260
QLast Update : Wed Aug 13 02:10:11 2025
Response via : Initial Calibration

Min. RRF : 0.000 Min. Rel. Area : 50% Max. R.T. Dev 0.50min
Max. RRF Dev : 25% Max. Rel. Area : 150%

	Compound	AvgRF	CCRF	%Dev	Area%	Dev(min)
96 T	1,2,3-Trichlorobenzene	0.742	0.723	2.6	100	0.00

(#) = Out of Range

SPCC's out = 0 CCC's out = 6

Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY081225\
 Data File : VY023057.D
 Acq On : 12 Aug 2025 17:53
 Operator : SY/MD
 Sample : VSTDICV050
 Misc : 5.00g/5.0mL/MSVOA_Y/SOIL
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 MSVOA_Y
 ClientSampleId :
 ICSVY081225

Quant Time: Aug 13 02:14:27 2025
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y081225S.M
 Quant Title : SW846 8260
 QLast Update : Wed Aug 13 02:10:11 2025
 Response via : Initial Calibration

Min. RRF : 0.000 Min. Rel. Area : 50% Max. R.T. Dev 0.50min
 Max. RRF Dev : 25% Max. Rel. Area : 150%

	Compound	Amount	Calc.	%Dev	Area%	Dev(min)
1 I	Pentafluorobenzene	50.000	50.000	0.0	98	0.00
2 T	Dichlorodifluoromethane	50.000	41.579	16.8	96	0.00
3 P	Chloromethane	50.000	48.732	2.5	104	0.00
4 C	Vinyl Chloride	50.000	48.198	3.6#	100	0.00
5 T	Bromomethane	50.000	46.983	6.0	104	0.00
6 T	Chloroethane	50.000	48.923	2.2	101	0.00
7 T	Trichlorofluoromethane	50.000	47.003	6.0	98	0.00
8 T	Diethyl Ether	50.000	47.787	4.4	98	0.00
9 T	1,1,2-Trichlorotrifluoroeth	50.000	47.725	4.5	99	0.00
10 T	Methyl Iodide	50.000	51.340	-2.7	97	0.00
11 T	Tert butyl alcohol	250.000	245.940	1.6	99	0.00
12 CM	1,1-Dichloroethene	50.000	47.686	4.6#	97	0.00
13 T	Acrolein	250.000	222.008	11.2	93	0.00
14 T	Allyl chloride	50.000	47.317	5.4	96	0.00
15 T	Acrylonitrile	250.000	242.779	2.9	96	0.00
16 T	Acetone	250.000	210.695	15.7	83	0.00
17 T	Carbon Disulfide	50.000	46.948	6.1	97	0.00
18 T	Methyl Acetate	50.000	51.972	-3.9	97	0.00
19 T	Methyl tert-butyl Ether	50.000	49.899	0.2	99	0.00
20 T	Methylene Chloride	50.000	49.960	0.1	103	0.00
21 T	trans-1,2-Dichloroethene	50.000	48.765	2.5	99	0.00
22 T	Diisopropyl ether	50.000	50.011	-0.0	100	0.00
23 T	Vinyl Acetate	250.000	242.360	3.1	96	0.00
24 P	1,1-Dichloroethane	50.000	48.551	2.9	98	0.00
25 T	2-Butanone	250.000	230.028	8.0	89	0.00
26 T	2,2-Dichloropropane	50.000	45.475	9.0	92	0.00
27 T	cis-1,2-Dichloroethene	50.000	48.720	2.6	99	0.00
28 T	Bromochloromethane	50.000	50.275	-0.5	101	0.00
29 T	Tetrahydrofuran	250.000	247.420	1.0	97	0.00
30 C	Chloroform	50.000	48.450	3.1#	98	0.00
31 T	Cyclohexane	50.000	46.526	6.9	99	0.00
32 T	1,1,1-Trichloroethane	50.000	48.933	2.1	99	0.00
33 S	1,2-Dichloroethane-d4	50.000	50.038	-0.1	101	0.00
34 I	1,4-Difluorobenzene	50.000	50.000	0.0	99	0.00
35 S	Dibromofluoromethane	50.000	50.179	-0.4	102	0.00
36 T	1,1-Dichloropropene	50.000	48.193	3.6	98	0.00
37 T	Ethyl Acetate	50.000	49.621	0.8	98	0.00
38 T	Carbon Tetrachloride	50.000	48.030	3.9	99	0.00
39 T	Methylcyclohexane	50.000	49.625	0.8	102	0.00
40 TM	Benzene	50.000	48.428	3.1	99	0.00
41 T	Methacrylonitrile	50.000	48.269	3.5	94	0.00
42 TM	1,2-Dichloroethane	50.000	48.162	3.7	98	0.00
43 T	Isopropyl Acetate	50.000	49.094	1.8	99	0.00
44 TM	Trichloroethene	50.000	47.803	4.4	98	0.00
45 C	1,2-Dichloropropane	50.000	48.961	2.1#	99	0.00
46 T	Dibromomethane	50.000	48.679	2.6	98	0.00
47 T	Bromodichloromethane	50.000	49.463	1.1	99	0.00
48 T	Methyl methacrylate	50.000	50.520	-1.0	96	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY081225\
 Data File : VY023057.D
 Acq On : 12 Aug 2025 17:53
 Operator : SY/MD
 Sample : VSTDICV050
 Misc : 5.00g/5.0mL/MSVOA_Y/SOIL
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 MSVOA_Y
 ClientSampleId :
 ICSVY081225

Quant Time: Aug 13 02:14:27 2025
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y081225S.M
 Quant Title : SW846 8260
 QLast Update : Wed Aug 13 02:10:11 2025
 Response via : Initial Calibration

Min. RRF : 0.000 Min. Rel. Area : 50% Max. R.T. Dev 0.50min
 Max. RRF Dev : 25% Max. Rel. Area : 150%

	Compound	Amount	Calc.	%Dev	Area%	Dev(min)
49 T	1,4-Dioxane	1000.000	971.749	2.8	97	0.00
50 S	Toluene-d8	50.000	49.306	1.4	100	0.00
51 T	4-Methyl-2-Pentanone	250.000	248.943	0.4	97	0.00
52 CM	Toluene	50.000	48.963	2.1#	99	0.00
53 T	t-1,3-Dichloropropene	50.000	49.699	0.6	99	0.00
54 T	cis-1,3-Dichloropropene	50.000	48.965	2.1	98	0.00
55 T	1,1,2-Trichloroethane	50.000	48.867	2.3	98	0.00
56 T	Ethyl methacrylate	50.000	50.779	-1.6	98	0.00
57 T	1,3-Dichloropropane	50.000	49.228	1.5	99	0.00
58 T	2-Chloroethyl Vinyl ether	250.000	273.240	-9.3	102	0.00
59 T	2-Hexanone	250.000	244.812	2.1	94	0.00
60 T	Dibromochloromethane	50.000	49.810	0.4	99	0.00
61 T	1,2-Dibromoethane	50.000	49.197	1.6	98	0.00
62 S	4-Bromofluorobenzene	50.000	51.500	-3.0	104	0.00
63 I	Chlorobenzene-d5	50.000	50.000	0.0	101	0.00
64 T	Tetrachloroethene	50.000	45.512	9.0	94	0.00
65 PM	Chlorobenzene	50.000	48.275	3.5	99	0.00
66 T	1,1,1,2-Tetrachloroethane	50.000	48.815	2.4	99	0.00
67 C	Ethyl Benzene	50.000	49.163	1.7#	99	0.00
68 T	m/p-Xylenes	100.000	98.515	1.5	100	0.00
69 T	o-Xylene	50.000	49.645	0.7	99	0.00
70 T	Styrene	50.000	50.733	-1.5	101	0.00
71 P	Bromoform	50.000	48.525	3.0	98	0.00
72 I	1,4-Dichlorobenzene-d4	50.000	50.000	0.0	100	0.00
73 T	Isopropylbenzene	50.000	49.876	0.2	100	0.00
74 T	N-ethyl acetate	50.000	50.529	-1.1	98	0.00
75 P	1,1,2,2-Tetrachloroethane	50.000	49.350	1.3	102	0.00
76 T	1,2,3-Trichloropropane	50.000	46.136	7.7	83	0.00
77 T	Bromobenzene	50.000	49.004	2.0	99	0.00
78 T	n-propylbenzene	50.000	50.853	-1.7	101	0.00
79 T	2-Chlorotoluene	50.000	49.898	0.2	101	0.00
80 T	1,3,5-Trimethylbenzene	50.000	50.916	-1.8	101	0.00
81 T	trans-1,4-Dichloro-2-butene	50.000	49.409	1.2	100	0.00
82 T	4-Chlorotoluene	50.000	49.505	1.0	100	0.00
83 T	tert-Butylbenzene	50.000	50.443	-0.9	100	0.00
84 T	1,2,4-Trimethylbenzene	50.000	51.042	-2.1	102	0.00
85 T	sec-Butylbenzene	50.000	51.154	-2.3	102	0.00
86 T	p-Isopropyltoluene	50.000	51.639	-3.3	102	0.00
87 T	1,3-Dichlorobenzene	50.000	49.639	0.7	102	0.00
88 T	1,4-Dichlorobenzene	50.000	48.514	3.0	100	0.00
89 T	n-Butylbenzene	50.000	51.594	-3.2	102	0.00
90 T	Hexachloroethane	50.000	50.617	-1.2	103	0.00
91 T	1,2-Dichlorobenzene	50.000	49.234	1.5	101	0.00
92 T	1,2-Dibromo-3-Chloropropane	50.000	50.085	-0.2	99	0.00
93 T	1,2,4-Trichlorobenzene	50.000	49.363	1.3	100	0.00
94 T	Hexachlorobutadiene	50.000	48.344	3.3	99	0.00
95 T	Naphthalene	50.000	51.623	-3.2	102	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY081225\
Data File : VY023057.D
Acq On : 12 Aug 2025 17:53
Operator : SY/MD
Sample : VSTDICV050
Misc : 5.00g/5.0mL/MSVOA_Y/SOIL
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_Y
ClientSampleId :
ICVVY081225

Quant Time: Aug 13 02:14:27 2025
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y081225S.M
Quant Title : SW846 8260
QLast Update : Wed Aug 13 02:10:11 2025
Response via : Initial Calibration

Min. RRF : 0.000 Min. Rel. Area : 50% Max. R.T. Dev 0.50min
Max. RRF Dev : 25% Max. Rel. Area : 150%

	Compound	Amount	Calc.	%Dev	Area%	Dev(min)
96 T	1,2,3-Trichlorobenzene	50.000	48.735	2.5	100	0.00

(#) = Out of Range SPCC's out = 0 CCC's out = 6



284 Sheffield Street, Mountainside, New Jersey 07092, Phone : 908 789 8900,
Fax : 908 789 8922

VOLATILE CONTINUING CALIBRATION CHECK

Lab Name:	<u>Alliance</u>	Contract:	<u>SCIA01</u>
Lab Code:	<u>ACE</u>	SDG No.:	<u>Q2868</u>
Instrument ID:	<u>MSVOA_Y</u>	Calibration Date/Time:	<u>08/15/2025 08:39</u>
Lab File ID:	<u>VY023111.D</u>	Init. Calib. Date(s):	<u>08/12/2025 08/12/2025</u>
Heated Purge: (Y/N)	<u>Y</u>	Init. Calib. Time(s):	<u>14:54 16:47</u>
GC Column:	<u>RXI-624</u>	ID:	<u>0.25</u> (mm)

COMPOUND	RRF	RRF050	MIN RRF	%D	MAX%D
Dichlorodifluoromethane	0.408	0.332		-18.63	20
Chloromethane	0.661	0.651	0.1	-1.51	20
Vinyl Chloride	0.817	0.876		7.22	20
Bromomethane	0.610	0.659		8.03	20
Chloroethane	0.543	0.599		10.31	20
Trichlorofluoromethane	0.994	0.982		-1.21	20
1,1,2-Trichlorotrifluoroethane	0.490	0.484		-1.22	20
1,1-Dichloroethene	0.482	0.471		-2.28	20
Acetone	0.103	0.116		12.62	20
Carbon Disulfide	1.571	1.520		-3.25	20
Methyl tert-butyl Ether	1.249	1.209		-3.2	20
Methyl Acetate	0.307	0.297		-3.26	20
Methylene Chloride	0.620	0.543		-12.42	20
trans-1,2-Dichloroethene	0.541	0.549		1.48	20
1,1-Dichloroethane	0.942	0.968	0.1	2.76	20
Cyclohexane	0.888	0.845		-4.84	20
2-Butanone	0.140	0.143		2.14	20
Carbon Tetrachloride	0.483	0.506		4.76	20
cis-1,2-Dichloroethene	0.626	0.643		2.72	20
Bromochloromethane	0.374	0.395		5.61	20
Chloroform	0.971	1.017		4.74	20
1,1,1-Trichloroethane	0.862	0.888		3.02	20
Methylcyclohexane	0.586	0.583		-0.51	20
Benzene	1.370	1.455		6.2	20
1,2-Dichloroethane	0.356	0.372		4.49	20
Trichloroethene	0.354	0.366		3.39	20
1,2-Dichloropropane	0.315	0.335		6.35	20
Bromodichloromethane	0.466	0.496		6.44	20
4-Methyl-2-Pentanone	0.195	0.194		-0.51	20
Toluene	0.870	0.928		6.67	20
t-1,3-Dichloropropene	0.422	0.434		2.84	20
cis-1,3-Dichloropropene	0.499	0.523		4.81	20
1,1,2-Trichloroethane	0.242	0.252		4.13	20
2-Hexanone	0.133	0.135		1.5	20
Dibromochloromethane	0.320	0.332		3.75	20
1,2-Dibromoethane	0.228	0.230		0.88	20
Tetrachloroethene	0.446	0.469		5.16	20
Chlorobenzene	1.079	1.142	0.3	5.84	20

All other compounds must meet a minimum RRF of 0.010.
RRF of 1,4-Dioxane = Value should be divide by 1000.



284 Sheffield Street, Mountainside, New Jersey 07092, Phone : 908 789 8900,
Fax : 908 789 8922

VOLATILE CONTINUING CALIBRATION CHECK

Lab Name:	<u>Alliance</u>	Contract:	<u>SCIA01</u>
Lab Code:	<u>ACE</u>	SDG No.:	<u>Q2868</u>
Instrument ID:	<u>MSVOA_Y</u>	Calibration Date/Time:	<u>08/15/2025</u> <u>08:39</u>
Lab File ID:	<u>VY023111.D</u>	Init. Calib. Date(s):	<u>08/12/2025</u> <u>08/12/2025</u>
Heated Purge: (Y/N)	<u>Y</u>	Init. Calib. Time(s):	<u>14:54</u> <u>16:47</u>
GC Column:	<u>RXI-624</u>	ID:	<u>0.25</u> (mm)

COMPOUND	RRF	RRF050	MIN RRF	%D	MAX%D
Ethyl Benzene	1.856	2.009		8.24	20
m/p-Xylenes	0.725	0.785		8.28	20
o-Xylene	0.679	0.736		8.4	20
Styrene	1.110	1.238		11.53	20
Bromoform	0.214	0.212	0.1	-0.94	20
Isopropylbenzene	3.529	3.734		5.81	20
1,1,2,2-Tetrachloroethane	0.603	0.595	0.3	-1.33	20
1,3-Dichlorobenzene	1.660	1.748		5.3	20
1,4-Dichlorobenzene	1.647	1.696		2.97	20
1,2-Dichlorobenzene	1.456	1.499		2.95	20
1,2-Dibromo-3-Chloropropane	0.094	0.090		-4.26	20
1,2,4-Trichlorobenzene	0.861	0.793		-7.9	20
1,2,3-Trichlorobenzene	0.742	0.679		-8.49	20
1,2-Dichloroethane-d4	0.477	0.480		0.63	20
Dibromofluoromethane	0.299	0.309		3.34	20
Toluene-d8	1.169	1.206		3.16	20
4-Bromofluorobenzene	0.376	0.376		0	20

All other compounds must meet a minimum RRF of 0.010.
RRF of 1,4-Dioxane = Value should be divide by 1000.

Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY081525\
 Data File : VY023111.D
 Acq On : 15 Aug 2025 08:39
 Operator : SY/MD
 Sample : VSTDCCC050
 Misc : 5.00g/5.0mL/MSVOA_Y/SOIL
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 MSVOA_Y
 ClientSampleId :
 VSTDCCC050

Manual Integrations
 APPROVED

Reviewed By : Semsettin Yesilyurt 08/19/2025
 Supervised By : Mahesh Dadoda 08/19/2025

Quant Time: Aug 18 02:22:29 2025
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y081225S.M
 Quant Title : SW846 8260
 QLast Update : Wed Aug 13 02:10:11 2025
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Pentafluorobenzene	7.707	168	443799	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	8.616	114	696916	50.000	ug/l	0.00
63) Chlorobenzene-d5	11.414	117	607348	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.347	152	306948	50.000	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	8.061	65	212960	50.349	ug/l	0.00
Spiked Amount 50.000	Range 50 - 163		Recovery = 100.700%			
35) Dibromofluoromethane	7.634	113	215688	51.722	ug/l	0.00
Spiked Amount 50.000	Range 54 - 147		Recovery = 103.440%			
50) Toluene-d8	10.103	98	840812	51.612	ug/l	0.00
Spiked Amount 50.000	Range 58 - 134		Recovery = 103.220%			
62) 4-Bromofluorobenzene	12.402	95	262368	50.079	ug/l	0.00
Spiked Amount 50.000	Range 30 - 143		Recovery = 100.160%			
Target Compounds					Qvalue	
2) Dichlorodifluoromethane	1.867	85	147210	40.637	ug/l	97
3) Chloromethane	2.068	50	288876	49.235	ug/l	97
4) Vinyl Chloride	2.202	62	388634	53.584	ug/l	99
5) Bromomethane	2.598	94	292335	53.970	ug/l	100
6) Chloroethane	2.733	64	266036	55.172	ug/l	99
7) Trichlorofluoromethane	3.050	101	435783	49.413	ug/l	97
8) Diethyl Ether	3.458	74	109033	46.730	ug/l	99
9) 1,1,2-Trichlorotrifluo...	3.812	101	214906	49.394	ug/l	98
10) Methyl Iodide	4.001	142	251096	53.482	ug/l	96
11) Tert butyl alcohol	4.866	59	59139	204.058	ug/l #	84
12) 1,1-Dichloroethene	3.793	96	209124	48.899	ug/l	94
13) Acrolein	3.647	56	67121	158.141	ug/l	99
14) Allyl chloride	4.379	41	305726	48.583	ug/l	98
15) Acrylonitrile	5.061	53	226259	238.524	ug/l	99
16) Acetone	3.866	43	257167	280.645	ug/l	99
17) Carbon Disulfide	4.104	76	674565	48.375	ug/l	100
18) Methyl Acetate	4.385	43	131808	48.336	ug/l	99
19) Methyl tert-butyl Ether	5.110	73	536488	48.411	ug/l	99
20) Methylene Chloride	4.610	84	241025	50.654	ug/l	98
21) trans-1,2-Dichloroethene	5.110	96	243549	50.676	ug/l	99
22) Diisopropyl ether	6.012	45	696767	50.954	ug/l	94
23) Vinyl Acetate	5.958	43	1859565	245.935	ug/l	99
24) 1,1-Dichloroethane	5.915	63	429668	51.394	ug/l	99
25) 2-Butanone	6.890	43	316503	253.961	ug/l	98
26) 2,2-Dichloropropane	6.884	77	379004	52.538	ug/l	99
27) cis-1,2-Dichloroethene	6.890	96	285339	51.356	ug/l	99
28) Bromochloromethane	7.244	49	175456	52.898	ug/l	97
29) Tetrahydrofuran	7.262	42	183118	237.044	ug/l	98
30) Chloroform	7.421	83	451255	52.336	ug/l	99
31) Cyclohexane	7.701	56	375108	47.613	ug/l	99
32) 1,1,1-Trichloroethane	7.616	97	394056	51.507	ug/l	99
36) 1,1-Dichloropropene	7.835	75	317586	51.245	ug/l	99
37) Ethyl Acetate	6.982	43	125483	48.201	ug/l	100
38) Carbon Tetrachloride	7.817	117	352681	52.395	ug/l	98
39) Methylcyclohexane	9.109	83	406063	49.756	ug/l	97
40) Benzene	8.079	78	1014264	53.099	ug/l	99

Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY081525\
 Data File : VY023111.D
 Acq On : 15 Aug 2025 08:39
 Operator : SY/MD
 Sample : VSTDCCC050
 Misc : 5.00g/5.0mL/MSVOA_Y/SOIL
 ALS Vial : 2 Sample Multiplier: 1

Instrument :

MSVOA_Y

ClientSampleId :

VSTDCCC050

Manual Integrations

APPROVED

Reviewed By :Semsettin Yesilyurt 08/19/2025

Supervised By :Mahesh Dadoda 08/19/2025

Quant Time: Aug 18 02:22:29 2025

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y081225S.M

Quant Title : SW846 8260

QLast Update : Wed Aug 13 02:10:11 2025

Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
41) Methacrylonitrile	7.220	41	77838m	51.807	ug/l	
42) 1,2-Dichloroethane	8.158	62	258937	52.122	ug/l	100
43) Isopropyl Acetate	8.195	43	250740	47.653	ug/l #	85
44) Trichloroethene	8.866	130	255103	51.680	ug/l	97
45) 1,2-Dichloropropane	9.140	63	233639	53.160	ug/l	99
46) Dibromomethane	9.225	93	131880	52.280	ug/l	99
47) Bromodichloromethane	9.420	83	345709	53.260	ug/l	98
48) Methyl methacrylate	9.219	41	121834	48.387	ug/l	96
49) 1,4-Dioxane	9.225	88	28081	949.382	ug/l	96
51) 4-Methyl-2-Pentanone	10.000	43	674267	248.424	ug/l	100
52) Toluene	10.170	92	646468	53.288	ug/l	99
53) t-1,3-Dichloropropene	10.390	75	302783	51.512	ug/l	99
54) cis-1,3-Dichloropropene	9.853	75	364333	52.418	ug/l	98
55) 1,1,2-Trichloroethane	10.573	97	175309	51.936	ug/l	98
56) Ethyl methacrylate	10.438	69	213704	49.477	ug/l	98
57) 1,3-Dichloropropane	10.713	76	293968	51.352	ug/l	100
58) 2-Chloroethyl Vinyl ether	9.707	63	531531	260.887	ug/l	100
59) 2-Hexanone	10.756	43	471343	255.032	ug/l	98
60) Dibromochloromethane	10.908	129	231138	51.895	ug/l	100
61) 1,2-Dibromoethane	11.012	107	160069	50.454	ug/l	100
64) Tetrachloroethene	10.646	164	284630	52.484	ug/l	99
65) Chlorobenzene	11.438	112	693667	52.949	ug/l	99
66) 1,1,1,2-Tetrachloroethane	11.511	131	239263	53.813	ug/l	98
67) Ethyl Benzene	11.518	91	1219913	54.111	ug/l	99
68) m/p-Xylenes	11.627	106	953446	108.283	ug/l	99
69) o-Xylene	11.950	106	446920	54.193	ug/l	100
70) Styrene	11.969	104	752144	55.770	ug/l	99
71) Bromoform	12.127	173	128745	49.544	ug/l #	99
73) Isopropylbenzene	12.249	105	1146162	52.906	ug/l	100
74) N-amyl acetate	12.066	43	226300	49.257	ug/l	99
75) 1,1,2,2-Tetrachloroethane	12.505	83	182753	49.405	ug/l	99
76) 1,2,3-Trichloropropane	12.554	75	151552m	51.159	ug/l	
77) Bromobenzene	12.530	156	262726	50.833	ug/l	98
78) n-propylbenzene	12.591	91	1396330	54.137	ug/l	100
79) 2-Chlorotoluene	12.676	91	783125	52.993	ug/l	99
80) 1,3,5-Trimethylbenzene	12.731	105	943980	53.915	ug/l	100
81) trans-1,4-Dichloro-2-b...	12.298	75	59917	48.961	ug/l	99
82) 4-Chlorotoluene	12.773	91	806542	52.611	ug/l	100
83) tert-Butylbenzene	12.993	119	825002	52.171	ug/l	99
84) 1,2,4-Trimethylbenzene	13.042	105	946009	54.277	ug/l	99
85) sec-Butylbenzene	13.170	105	1234484	53.143	ug/l	99
86) p-Isopropyltoluene	13.286	119	1047646	54.334	ug/l	100
87) 1,3-Dichlorobenzene	13.286	146	536529	52.641	ug/l	99
88) 1,4-Dichlorobenzene	13.365	146	520698	51.501	ug/l	99
89) n-Butylbenzene	13.615	91	955218	53.939	ug/l	98
90) Hexachloroethane	13.877	117	209441	53.061	ug/l	97
91) 1,2-Dichlorobenzene	13.657	146	460235	51.489	ug/l	100
92) 1,2-Dibromo-3-Chloropr...	14.273	75	27552	47.839	ug/l	95
93) 1,2,4-Trichlorobenzene	14.919	180	243376	46.042	ug/l	98
94) Hexachlorobutadiene	15.017	225	144679	46.578	ug/l	99
95) Naphthalene	15.139	128	408671	45.340	ug/l	100
96) 1,2,3-Trichlorobenzene	15.322	180	208542	45.784	ug/l	99

Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY081525\
Data File : VY023111.D
Acq On : 15 Aug 2025 08:39
Operator : SY/MD
Sample : VSTDCCC050
Misc : 5.00g/5.0mL/MSVOA_Y/SOIL
ALS Vial : 2 Sample Multiplier: 1

Instrument :
MSVOA_Y
ClientSampleId :
VSTDCCC050

Manual Integrations
APPROVED

Reviewed By :Semsettin Yesilyurt 08/19/2025
Supervised By :Mahesh Dadoda 08/19/2025

Quant Time: Aug 18 02:22:29 2025
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y081225S.M
Quant Title : SW846 8260
QLast Update : Wed Aug 13 02:10:11 2025
Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
----------	------	------	----------	------	-------	----------

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY081525\
Data File : VY023111.D
Acq On : 15 Aug 2025 08:39
Operator : SY/MD
Sample : VSTDCCC050
Misc : 5.00g/5.0mL/MSVOA_Y/SOIL
ALS Vial : 2 Sample Multiplier: 1

Instrument :
MSVOA_Y
ClientSampleId :
VSTDCCC050

Manual Integrations

Reviewed By :Semsettin Yesilyurt 08/19/2025
Supervised By :Mahesh Dadoda 08/19/2025

Quant Time: Aug 18 02:22:29 2025
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y081225S.M
Quant Title : SW846 8260
QLast Update : Wed Aug 13 02:10:11 2025
Response via : Initial Calibration

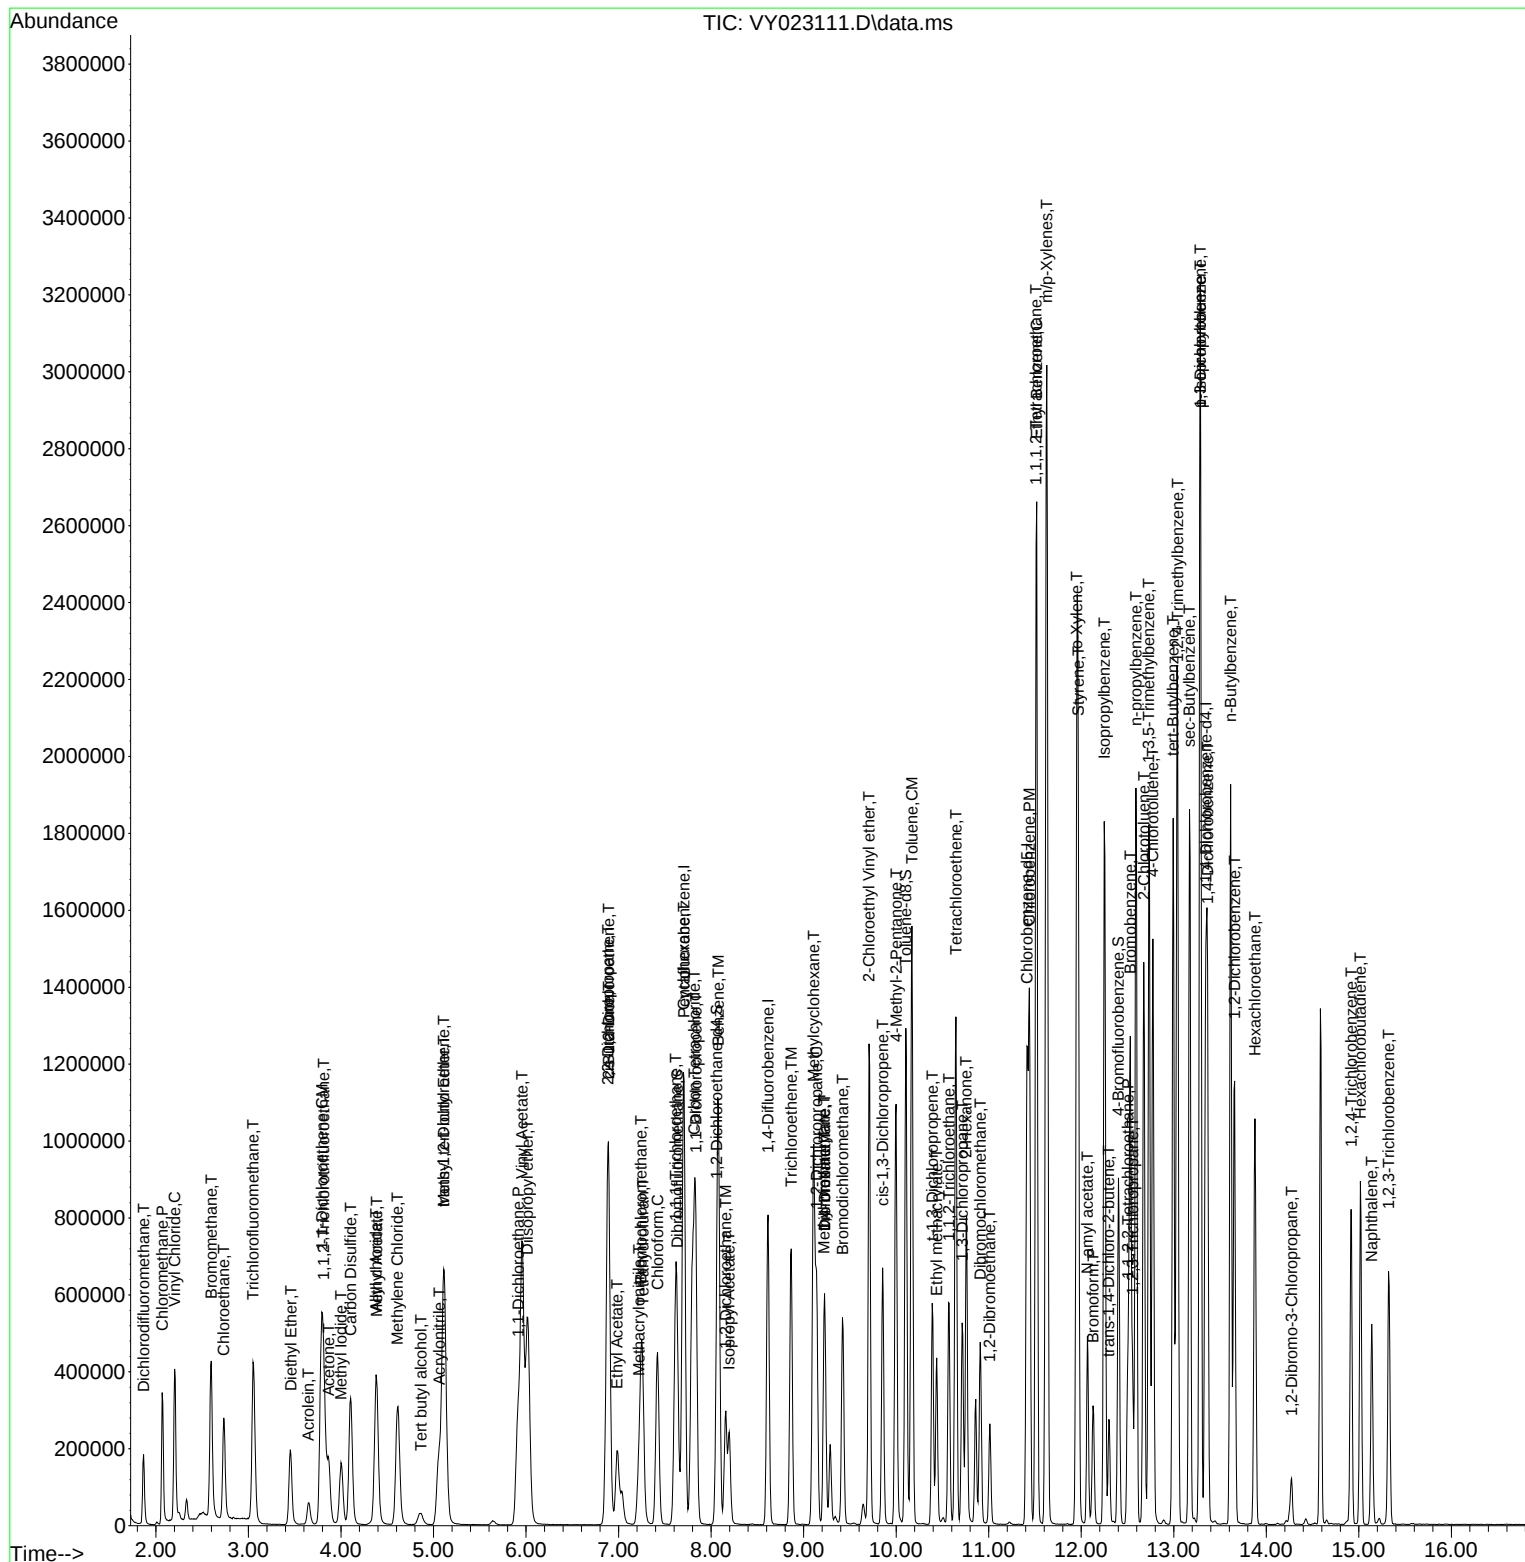

Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY081525\
 Data File : VY023111.D
 Acq On : 15 Aug 2025 08:39
 Operator : SY/MD
 Sample : VSTDCCC050
 Misc : 5.00g/5.0mL/MSVOA_Y/SOIL
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 MSVOA_Y
 LabSampleId :
 VSTDCCC050

Quant Time: Aug 18 02:22:29 2025
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y081225S.M
 Quant Title : SW846 8260
 QLast Update : Wed Aug 13 02:10:11 2025
 Response via : Initial Calibration

Min. RRF : 0.000 Min. Rel. Area : 50% Max. R.T. Dev 0.50min
 Max. RRF Dev : 25% Max. Rel. Area : 150%

	Compound	AvgRF	CCRF	%Dev	Area%	Dev(min)
1 I	Pentafluorobenzene	1.000	1.000	0.0	82	0.00
2 T	Dichlorodifluoromethane	0.408	0.332	18.6	78	0.00
3 P	Chloromethane	0.661	0.651	1.5	88	0.00
4 C	Vinyl Chloride	0.817	0.876	-7.2#	94	0.00
5 T	Bromomethane	0.610	0.659	-8.0	100	0.00
6 T	Chloroethane	0.543	0.599	-10.3	96	0.00
7 T	Trichlorofluoromethane	0.994	0.982	1.2	86	0.00
8 T	Diethyl Ether	0.263	0.246	6.5	81	0.01
9 T	1,1,2-Trichlorotrifluoroeth	0.490	0.484	1.2	86	0.00
10 T	Methyl Iodide	0.529	0.566	-7.0	85	0.00
11 T	Tert butyl alcohol	0.033	0.027	18.2	69	0.00
12 CM	1,1-Dichloroethene	0.482	0.471	2.3#	84	0.01
13 T	Acrolein	0.048	0.030	37.5#	55	0.00
14 T	Allyl chloride	0.709	0.689	2.8	83	0.00
15 T	Acrylonitrile	0.107	0.102	4.7	79	0.01
16 T	Acetone	0.103	0.116	-12.6	92	0.00
17 T	Carbon Disulfide	1.571	1.520	3.2	84	0.00
18 T	Methyl Acetate	0.307	0.297	3.3	76	0.00
19 T	Methyl tert-butyl Ether	1.249	1.209	3.2	80	0.00
20 T	Methylene Chloride	0.620	0.543	12.4	88	0.00
21 T	trans-1,2-Dichloroethene	0.541	0.549	-1.5	86	0.00
22 T	Diisopropyl ether	1.541	1.570	-1.9	85	0.00
23 T	Vinyl Acetate	0.852	0.838	1.6	82	0.00
24 P	1,1-Dichloroethane	0.942	0.968	-2.8	87	0.00
25 T	2-Butanone	0.140	0.143	-2.1	83	0.00
26 T	2,2-Dichloropropane	0.813	0.854	-5.0	89	0.00
27 T	cis-1,2-Dichloroethene	0.626	0.643	-2.7	87	0.00
28 T	Bromochloromethane	0.374	0.395	-5.6	89	0.00
29 T	Tetrahydrofuran	0.087	0.083	4.6	78	0.00
30 C	Chloroform	0.971	1.017	-4.7#	89	0.00
31 T	Cyclohexane	0.888	0.845	4.8	85	0.00
32 T	1,1,1-Trichloroethane	0.862	0.888	-3.0	87	0.00
33 S	1,2-Dichloroethane-d4	0.477	0.480	-0.6	86	0.00
34 I	1,4-Difluorobenzene	1.000	1.000	0.0	81	0.00
35 S	Dibromofluoromethane	0.299	0.309	-3.3	86	0.00
36 T	1,1-Dichloropropene	0.445	0.456	-2.5	86	0.00
37 T	Ethyl Acetate	0.187	0.180	3.7	78	0.00
38 T	Carbon Tetrachloride	0.483	0.506	-4.8	88	0.00
39 T	Methylcyclohexane	0.586	0.583	0.5	84	0.00
40 TM	Benzene	1.370	1.455	-6.2	89	0.00
41 T	Methacrylonitrile	0.108	0.112	-3.7	83	0.00
42 TM	1,2-Dichloroethane	0.356	0.372	-4.5	87	0.00
43 T	Isopropyl Acetate	0.378	0.360	4.8	78	0.00
44 TM	Trichloroethene	0.354	0.366	-3.4	87	0.00
45 C	1,2-Dichloropropane	0.315	0.335	-6.3#	88	0.00
46 T	Dibromomethane	0.181	0.189	-4.4	86	0.00
47 T	Bromodichloromethane	0.466	0.496	-6.4	88	0.00
48 T	Methyl methacrylate	0.181	0.175	3.3	76	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY081525\
 Data File : VY023111.D
 Acq On : 15 Aug 2025 08:39
 Operator : SY/MD
 Sample : VSTDCCC050
 Misc : 5.00g/5.0mL/MSVOA_Y/SOIL
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 MSVOA_Y
 LabSampleId :
 VSTDCCC050

Quant Time: Aug 18 02:22:29 2025
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y081225S.M
 Quant Title : SW846 8260
 QLast Update : Wed Aug 13 02:10:11 2025
 Response via : Initial Calibration

Min. RRF : 0.000 Min. Rel. Area : 50% Max. R.T. Dev 0.50min
 Max. RRF Dev : 25% Max. Rel. Area : 150%

	Compound	AvgRF	CCRF	%Dev	Area%	Dev(min)
49 T	1,4-Dioxane	0.002	0.002	0.0	77	0.00
50 S	Toluene-d8	1.169	1.206	-3.2	86	0.00
51 T	4-Methyl-2-Pentanone	0.195	0.194	0.5	79	0.00
52 CM	Toluene	0.870	0.928	-6.7#	88	0.00
53 T	t-1,3-Dichloropropene	0.422	0.434	-2.8	84	0.00
54 T	cis-1,3-Dichloropropene	0.499	0.523	-4.8	86	0.00
55 T	1,1,2-Trichloroethane	0.242	0.252	-4.1	86	0.00
56 T	Ethyl methacrylate	0.310	0.307	1.0	78	0.00
57 T	1,3-Dichloropropane	0.411	0.422	-2.7	85	0.00
58 T	2-Chloroethyl Vinyl ether	0.146	0.153	-4.8	80	0.00
59 T	2-Hexanone	0.133	0.135	-1.5	81	0.00
60 T	Dibromochloromethane	0.320	0.332	-3.8	85	0.00
61 T	1,2-Dibromoethane	0.228	0.230	-0.9	83	0.00
62 S	4-Bromofluorobenzene	0.376	0.376	0.0	83	0.00
63 I	Chlorobenzene-d5	1.000	1.000	0.0	81	0.00
64 T	Tetrachloroethene	0.446	0.469	-5.2	87	0.00
65 PM	Chlorobenzene	1.079	1.142	-5.8	87	0.00
66 T	1,1,1,2-Tetrachloroethane	0.366	0.394	-7.7	88	0.00
67 C	Ethyl Benzene	1.856	2.009	-8.2#	87	0.00
68 T	m/p-Xylenes	0.725	0.785	-8.3	88	0.00
69 T	o-Xylene	0.679	0.736	-8.4	87	0.00
70 T	Styrene	1.110	1.238	-11.5	89	0.00
71 P	Bromoform	0.214	0.212	0.9	80	0.00
72 I	1,4-Dichlorobenzene-d4	1.000	1.000	0.0	81	0.00
73 T	Isopropylbenzene	3.529	3.734	-5.8	87	0.00
74 T	N-amyl acetate	0.748	0.737	1.5	78	0.00
75 P	1,1,2,2-Tetrachloroethane	0.603	0.595	1.3	83	0.00
76 T	1,2,3-Trichloropropane	0.483	0.494	-2.3	75	0.00
77 T	Bromobenzene	0.842	0.856	-1.7	84	0.00
78 T	n-propylbenzene	4.201	4.549	-8.3	88	0.00
79 T	2-Chlorotoluene	2.407	2.551	-6.0	87	0.00
80 T	1,3,5-Trimethylbenzene	2.852	3.075	-7.8	87	0.00
81 T	trans-1,4-Dichloro-2-butene	0.199	0.195	2.0	80	0.00
82 T	4-Chlorotoluene	2.497	2.628	-5.2	87	0.00
83 T	tert-Butylbenzene	2.576	2.688	-4.3	84	0.00
84 T	1,2,4-Trimethylbenzene	2.839	3.082	-8.6	88	0.00
85 T	sec-Butylbenzene	3.784	4.022	-6.3	87	0.00
86 T	p-Isopropyltoluene	3.141	3.413	-8.7	88	0.00
87 T	1,3-Dichlorobenzene	1.660	1.748	-5.3	88	0.00
88 T	1,4-Dichlorobenzene	1.647	1.696	-3.0	86	0.00
89 T	n-Butylbenzene	2.885	3.112	-7.9	87	0.00
90 T	Hexachloroethane	0.643	0.682	-6.1	88	0.00
91 T	1,2-Dichlorobenzene	1.456	1.499	-3.0	86	0.00
92 T	1,2-Dibromo-3-Chloropropane	0.094	0.090	4.3	77	0.00
93 T	1,2,4-Trichlorobenzene	0.861	0.793	7.9	76	0.00
94 T	Hexachlorobutadiene	0.506	0.471	6.9	78	0.00
95 T	Naphthalene	1.468	1.331	9.3	73	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY081525\
Data File : VY023111.D
Acq On : 15 Aug 2025 08:39
Operator : SY/MD
Sample : VSTDCCC050
Misc : 5.00g/5.0mL/MSVOA_Y/SOIL
ALS Vial : 2 Sample Multiplier: 1

Instrument :
MSVOA_Y
LabSampleId :
VSTDCCC050

Quant Time: Aug 18 02:22:29 2025
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y081225S.M
Quant Title : SW846 8260
QLast Update : Wed Aug 13 02:10:11 2025
Response via : Initial Calibration

Min. RRF : 0.000 Min. Rel. Area : 50% Max. R.T. Dev 0.50min
Max. RRF Dev : 25% Max. Rel. Area : 150%

	Compound	AvgRF	CCRF	%Dev	Area%	Dev(min)
96 T	1,2,3-Trichlorobenzene	0.742	0.679	8.5	77	0.00

(#) = Out of Range

SPCC's out = 0 CCC's out = 6

Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY081525\
 Data File : VY023111.D
 Acq On : 15 Aug 2025 08:39
 Operator : SY/MD
 Sample : VSTDCCC050
 Misc : 5.00g/5.0mL/MSVOA_Y/SOIL
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 MSVOA_Y
 LabSampleId :
 VSTDCCC050

Quant Time: Aug 18 02:22:29 2025
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y081225S.M
 Quant Title : SW846 8260
 QLast Update : Wed Aug 13 02:10:11 2025
 Response via : Initial Calibration

Min. RRF : 0.000 Min. Rel. Area : 50% Max. R.T. Dev 0.50min
 Max. RRF Dev : 25% Max. Rel. Area : 150%

	Compound	Amount	Calc.	%Dev	Area%	Dev(min)
1 I	Pentafluorobenzene	50.000	50.000	0.0	82	0.00
2 T	Dichlorodifluoromethane	50.000	40.637	18.7	78	0.00
3 P	Chloromethane	50.000	49.235	1.5	88	0.00
4 C	Vinyl Chloride	50.000	53.584	-7.2#	94	0.00
5 T	Bromomethane	50.000	53.970	-7.9	100	0.00
6 T	Chloroethane	50.000	55.172	-10.3	96	0.00
7 T	Trichlorofluoromethane	50.000	49.413	1.2	86	0.00
8 T	Diethyl Ether	50.000	46.730	6.5	81	0.01
9 T	1,1,2-Trichlorotrifluoroeth	50.000	49.394	1.2	86	0.00
10 T	Methyl Iodide	50.000	53.482	-7.0	85	0.00
11 T	Tert butyl alcohol	250.000	204.058	18.4	69	0.00
12 CM	1,1-Dichloroethene	50.000	48.899	2.2#	84	0.01
13 T	Acrolein	250.000	158.141	36.7#	55	0.00
14 T	Allyl chloride	50.000	48.583	2.8	83	0.00
15 T	Acrylonitrile	250.000	238.524	4.6	79	0.01
16 T	Acetone	250.000	280.645	-12.3	92	0.00
17 T	Carbon Disulfide	50.000	48.375	3.3	84	0.00
18 T	Methyl Acetate	50.000	48.336	3.3	76	0.00
19 T	Methyl tert-butyl Ether	50.000	48.411	3.2	80	0.00
20 T	Methylene Chloride	50.000	50.654	-1.3	88	0.00
21 T	trans-1,2-Dichloroethene	50.000	50.676	-1.4	86	0.00
22 T	Diisopropyl ether	50.000	50.954	-1.9	85	0.00
23 T	Vinyl Acetate	250.000	245.935	1.6	82	0.00
24 P	1,1-Dichloroethane	50.000	51.394	-2.8	87	0.00
25 T	2-Butanone	250.000	253.961	-1.6	83	0.00
26 T	2,2-Dichloropropane	50.000	52.538	-5.1	89	0.00
27 T	cis-1,2-Dichloroethene	50.000	51.356	-2.7	87	0.00
28 T	Bromochloromethane	50.000	52.898	-5.8	89	0.00
29 T	Tetrahydrofuran	250.000	237.044	5.2	78	0.00
30 C	Chloroform	50.000	52.336	-4.7#	89	0.00
31 T	Cyclohexane	50.000	47.613	4.8	85	0.00
32 T	1,1,1-Trichloroethane	50.000	51.507	-3.0	87	0.00
33 S	1,2-Dichloroethane-d4	50.000	50.349	-0.7	86	0.00
34 I	1,4-Difluorobenzene	50.000	50.000	0.0	81	0.00
35 S	Dibromofluoromethane	50.000	51.722	-3.4	86	0.00
36 T	1,1-Dichloropropene	50.000	51.245	-2.5	86	0.00
37 T	Ethyl Acetate	50.000	48.201	3.6	78	0.00
38 T	Carbon Tetrachloride	50.000	52.395	-4.8	88	0.00
39 T	Methylcyclohexane	50.000	49.756	0.5	84	0.00
40 TM	Benzene	50.000	53.099	-6.2	89	0.00
41 T	Methacrylonitrile	50.000	51.807	-3.6	83	0.00
42 TM	1,2-Dichloroethane	50.000	52.122	-4.2	87	0.00
43 T	Isopropyl Acetate	50.000	47.653	4.7	78	0.00
44 TM	Trichloroethene	50.000	51.680	-3.4	87	0.00
45 C	1,2-Dichloropropane	50.000	53.160	-6.3#	88	0.00
46 T	Dibromomethane	50.000	52.280	-4.6	86	0.00
47 T	Bromodichloromethane	50.000	53.260	-6.5	88	0.00
48 T	Methyl methacrylate	50.000	48.387	3.2	76	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY081525\
 Data File : VY023111.D
 Acq On : 15 Aug 2025 08:39
 Operator : SY/MD
 Sample : VSTDCCC050
 Misc : 5.00g/5.0mL/MSVOA_Y/SOIL
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 MSVOA_Y
 LabSampleId :
 VSTDCCC050

Quant Time: Aug 18 02:22:29 2025
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y081225S.M
 Quant Title : SW846 8260
 QLast Update : Wed Aug 13 02:10:11 2025
 Response via : Initial Calibration

Min. RRF : 0.000 Min. Rel. Area : 50% Max. R.T. Dev 0.50min
 Max. RRF Dev : 25% Max. Rel. Area : 150%

	Compound	Amount	Calc.	%Dev	Area%	Dev(min)
49 T	1,4-Dioxane	1000.000	949.382	5.1	77	0.00
50 S	Toluene-d8	50.000	51.612	-3.2	86	0.00
51 T	4-Methyl-2-Pentanone	250.000	248.424	0.6	79	0.00
52 CM	Toluene	50.000	53.288	-6.6#	88	0.00
53 T	t-1,3-Dichloropropene	50.000	51.512	-3.0	84	0.00
54 T	cis-1,3-Dichloropropene	50.000	52.418	-4.8	86	0.00
55 T	1,1,2-Trichloroethane	50.000	51.936	-3.9	86	0.00
56 T	Ethyl methacrylate	50.000	49.477	1.0	78	0.00
57 T	1,3-Dichloropropane	50.000	51.352	-2.7	85	0.00
58 T	2-Chloroethyl Vinyl ether	250.000	260.887	-4.4	80	0.00
59 T	2-Hexanone	250.000	255.032	-2.0	81	0.00
60 T	Dibromochloromethane	50.000	51.895	-3.8	85	0.00
61 T	1,2-Dibromoethane	50.000	50.454	-0.9	83	0.00
62 S	4-Bromofluorobenzene	50.000	50.079	-0.2	83	0.00
63 I	Chlorobenzene-d5	50.000	50.000	0.0	81	0.00
64 T	Tetrachloroethene	50.000	52.484	-5.0	87	0.00
65 PM	Chlorobenzene	50.000	52.949	-5.9	87	0.00
66 T	1,1,1,2-Tetrachloroethane	50.000	53.813	-7.6	88	0.00
67 C	Ethyl Benzene	50.000	54.111	-8.2#	87	0.00
68 T	m/p-Xylenes	100.000	108.283	-8.3	88	0.00
69 T	o-Xylene	50.000	54.193	-8.4	87	0.00
70 T	Styrene	50.000	55.770	-11.5	89	0.00
71 P	Bromoform	50.000	49.544	0.9	80	0.00
72 I	1,4-Dichlorobenzene-d4	50.000	50.000	0.0	81	0.00
73 T	Isopropylbenzene	50.000	52.906	-5.8	87	0.00
74 T	N-ethyl acetate	50.000	49.257	1.5	78	0.00
75 P	1,1,2,2-Tetrachloroethane	50.000	49.405	1.2	83	0.00
76 T	1,2,3-Trichloropropane	50.000	51.159	-2.3	75	0.00
77 T	Bromobenzene	50.000	50.833	-1.7	84	0.00
78 T	n-propylbenzene	50.000	54.137	-8.3	88	0.00
79 T	2-Chlorotoluene	50.000	52.993	-6.0	87	0.00
80 T	1,3,5-Trimethylbenzene	50.000	53.915	-7.8	87	0.00
81 T	trans-1,4-Dichloro-2-butene	50.000	48.961	2.1	80	0.00
82 T	4-Chlorotoluene	50.000	52.611	-5.2	87	0.00
83 T	tert-Butylbenzene	50.000	52.171	-4.3	84	0.00
84 T	1,2,4-Trimethylbenzene	50.000	54.277	-8.6	88	0.00
85 T	sec-Butylbenzene	50.000	53.143	-6.3	87	0.00
86 T	p-Isopropyltoluene	50.000	54.334	-8.7	88	0.00
87 T	1,3-Dichlorobenzene	50.000	52.641	-5.3	88	0.00
88 T	1,4-Dichlorobenzene	50.000	51.501	-3.0	86	0.00
89 T	n-Butylbenzene	50.000	53.939	-7.9	87	0.00
90 T	Hexachloroethane	50.000	53.061	-6.1	88	0.00
91 T	1,2-Dichlorobenzene	50.000	51.489	-3.0	86	0.00
92 T	1,2-Dibromo-3-Chloropropane	50.000	47.839	4.3	77	0.00
93 T	1,2,4-Trichlorobenzene	50.000	46.042	7.9	76	0.00
94 T	Hexachlorobutadiene	50.000	46.578	6.8	78	0.00
95 T	Naphthalene	50.000	45.340	9.3	73	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY081525\
Data File : VY023111.D
Acq On : 15 Aug 2025 08:39
Operator : SY/MD
Sample : VSTDCCC050
Misc : 5.00g/5.0mL/MSVOA_Y/SOIL
ALS Vial : 2 Sample Multiplier: 1

Instrument :
MSVOA_Y
LabSampleId :
VSTDCCC050

Quant Time: Aug 18 02:22:29 2025
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y081225S.M
Quant Title : SW846 8260
QLast Update : Wed Aug 13 02:10:11 2025
Response via : Initial Calibration

Min. RRF : 0.000 Min. Rel. Area : 50% Max. R.T. Dev 0.50min
Max. RRF Dev : 25% Max. Rel. Area : 150%

	Compound	Amount	Calc.	%Dev	Area%	Dev(min)
96 T	1,2,3-Trichlorobenzene	50.000	45.784	8.4	77	0.00

(#) = Out of Range SPCC's out = 0 CCC's out = 6





QC SAMPLE DATA

Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY081225\
Data File : VY023048.D
Acq On : 12 Aug 2025 08:26
Operator : SY/MD
Sample : BFB
Misc : 5.00g/5.0mL/MSVOA_Y/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_Y
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y081225S.M
Title : SW846 8260
Last Update : Wed Aug 13 02:10:11 2025

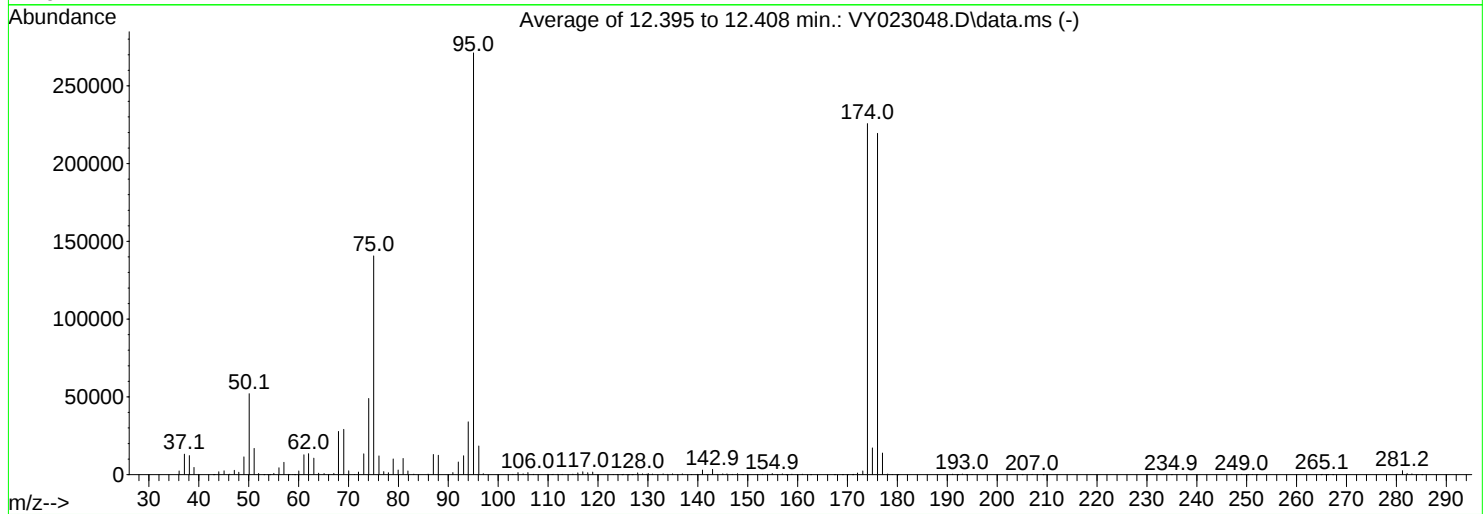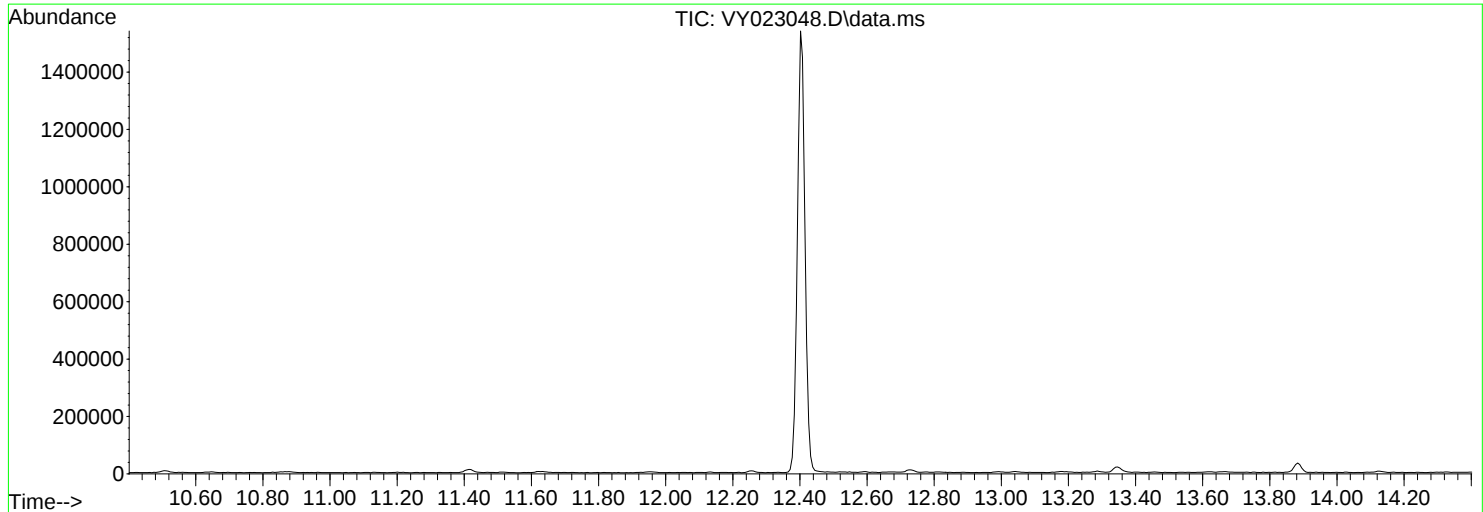

AutoFind: Scans 1751, 1752, 1753; Background Corrected with Scan 1743



Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	19.2	52107	PASS
75	95	30	60	51.9	140677	PASS
95	95	100	100	100.0	271211	PASS
96	95	5	9	6.8	18415	PASS
173	174	0.00	2	1.1	2383	PASS
174	95	50	100	83.2	225707	PASS
175	174	5	9	7.6	17158	PASS
176	174	95	101	97.2	219435	PASS
177	176	5	9	6.4	13937	PASS

Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY081525\
Data File : VY023110.D
Acq On : 15 Aug 2025 08:07
Operator : SY/MD
Sample : BFB
Misc : 5.00g/5.0mL/MSVOA_Y/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_Y
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y081225S.M
Title : SW846 8260
Last Update : Wed Aug 13 02:10:11 2025

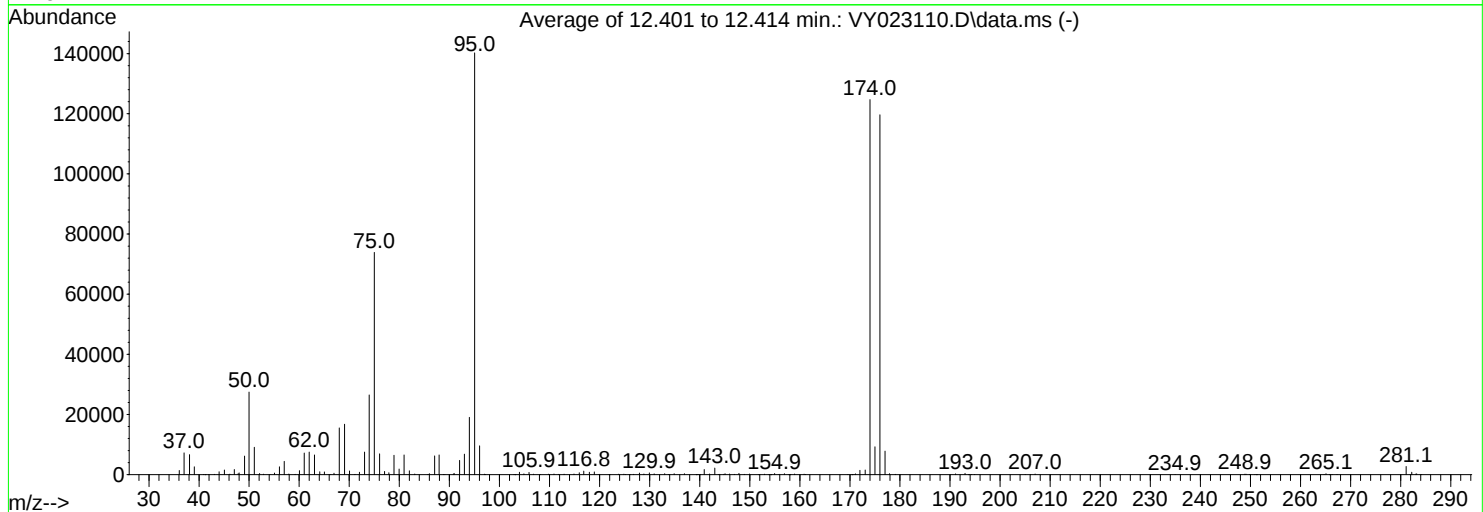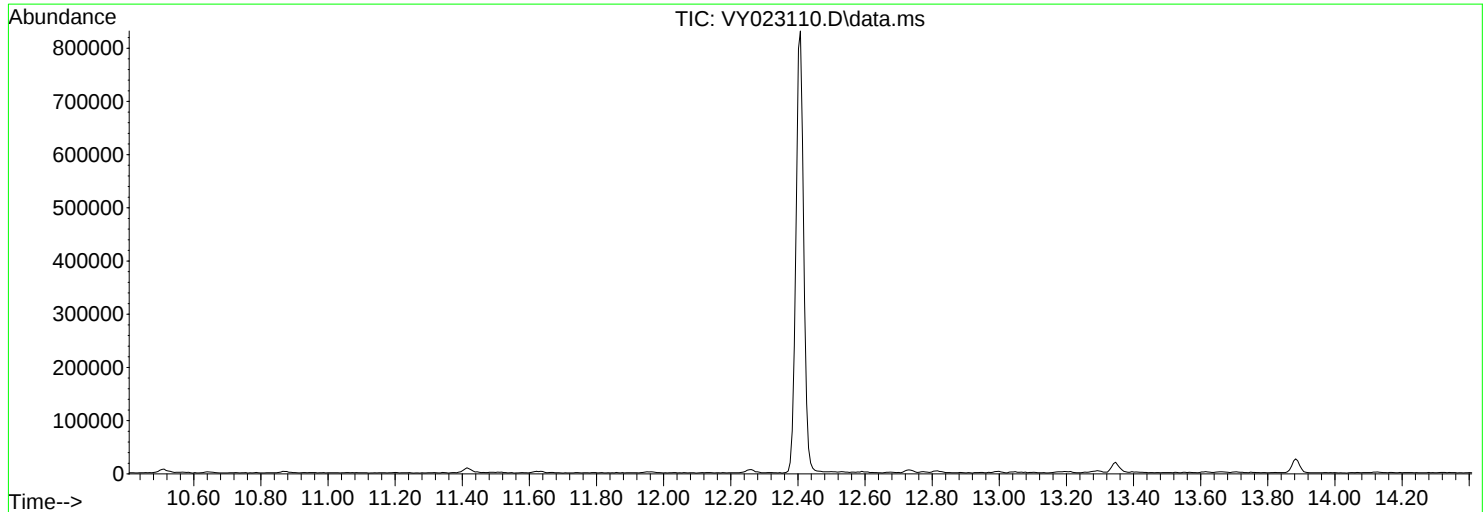

AutoFind: Scans 1752, 1753, 1754; Background Corrected with Scan 1743

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	19.6	27445	PASS
75	95	30	60	52.7	73891	PASS
95	95	100	100	100.0	140256	PASS
96	95	5	9	6.8	9601	PASS
173	174	0.00	2	1.2	1524	PASS
174	95	50	100	88.9	124701	PASS
175	174	5	9	7.4	9275	PASS
176	174	95	101	96.0	119685	PASS
177	176	5	9	6.5	7810	PASS

Report of Analysis

Client:	Sciaccia General Contractors, LLC			Date Collected:	
Project:	507 Franklin Ave			Date Received:	
Client Sample ID:	VY0815SBL01			SDG No.:	Q2868
Lab Sample ID:	VY0815SBL01			Matrix:	SOIL
Analytical Method:	8260D			% Solid:	100
Sample Wt/Vol:	5	Units:	g	Final Vol:	5000 uL
Soil Aliquot Vol:			uL	Test:	VOC-TCLVOA-10
GC Column:	RXI-624	ID :	0.25	Level :	LOW
Prep Method :					

File ID/Qc Batch:	Dilution:	Date Analyzed	Prep Batch ID
VY023112.D	1	08/15/25 09:08	VY081525

CAS Number	Parameter	Conc.	Qualifier	MDL	LOQ / CRQL	Units(Dry Weight)
TARGETS						
75-71-8	Dichlorodifluoromethane	1.10	U	1.10	5.00	ug/Kg
74-87-3	Chloromethane	1.10	U	1.10	5.00	ug/Kg
75-01-4	Vinyl Chloride	0.79	U	0.79	5.00	ug/Kg
74-83-9	Bromomethane	1.10	U	1.10	5.00	ug/Kg
75-00-3	Chloroethane	1.30	U	1.30	5.00	ug/Kg
75-69-4	Trichlorofluoromethane	1.20	U	1.20	5.00	ug/Kg
76-13-1	1,1,2-Trichlorotrifluoroethane	1.10	U	1.10	5.00	ug/Kg
75-35-4	1,1-Dichloroethene	1.00	U	1.00	5.00	ug/Kg
67-64-1	Acetone	4.70	U	4.70	25.0	ug/Kg
75-15-0	Carbon Disulfide	1.10	U	1.10	5.00	ug/Kg
1634-04-4	Methyl tert-butyl Ether	0.73	U	0.73	5.00	ug/Kg
79-20-9	Methyl Acetate	1.50	U	1.50	5.00	ug/Kg
75-09-2	Methylene Chloride	3.50	U	3.50	10.0	ug/Kg
156-60-5	trans-1,2-Dichloroethene	0.86	U	0.86	5.00	ug/Kg
75-34-3	1,1-Dichloroethane	0.80	U	0.80	5.00	ug/Kg
110-82-7	Cyclohexane	0.79	U	0.79	5.00	ug/Kg
78-93-3	2-Butanone	6.50	U	6.50	25.0	ug/Kg
56-23-5	Carbon Tetrachloride	0.97	U	0.97	5.00	ug/Kg
156-59-2	cis-1,2-Dichloroethene	0.75	U	0.75	5.00	ug/Kg
74-97-5	Bromochloromethane	1.20	U	1.20	5.00	ug/Kg
67-66-3	Chloroform	0.84	U	0.84	5.00	ug/Kg
71-55-6	1,1,1-Trichloroethane	0.93	U	0.93	5.00	ug/Kg
108-87-2	Methylcyclohexane	0.91	U	0.91	5.00	ug/Kg
71-43-2	Benzene	0.79	U	0.79	5.00	ug/Kg
107-06-2	1,2-Dichloroethane	0.79	U	0.79	5.00	ug/Kg
79-01-6	Trichloroethene	0.81	U	0.81	5.00	ug/Kg
78-87-5	1,2-Dichloropropane	0.91	U	0.91	5.00	ug/Kg
75-27-4	Bromodichloromethane	0.78	U	0.78	5.00	ug/Kg
108-10-1	4-Methyl-2-Pentanone	3.60	U	3.60	25.0	ug/Kg
108-88-3	Toluene	0.78	U	0.78	5.00	ug/Kg

Report of Analysis

Client:	Sciacca General Contractors, LLC		Date Collected:	
Project:	507 Franklin Ave		Date Received:	
Client Sample ID:	VY0815SBL01		SDG No.:	Q2868
Lab Sample ID:	VY0815SBL01		Matrix:	SOIL
Analytical Method:	8260D		% Solid:	100
Sample Wt/Vol:	5	Units: g	Final Vol:	5000 uL
Soil Aliquot Vol:		uL	Test:	VOC-TCLVOA-10
GC Column:	RXI-624	ID : 0.25	Level :	LOW
Prep Method :				

File ID/Qc Batch:	Dilution:	Date Analyzed	Prep Batch ID
VY023112.D	1	08/15/25 09:08	VY081525

CAS Number	Parameter	Conc.	Qualifier	MDL	LOQ / CRQL	Units(Dry Weight)
10061-02-6	t-1,3-Dichloropropene	0.65	U	0.65	5.00	ug/Kg
10061-01-5	cis-1,3-Dichloropropene	0.62	U	0.62	5.00	ug/Kg
79-00-5	1,1,2-Trichloroethane	0.92	U	0.92	5.00	ug/Kg
591-78-6	2-Hexanone	3.70	U	3.70	25.0	ug/Kg
124-48-1	Dibromochloromethane	0.87	U	0.87	5.00	ug/Kg
106-93-4	1,2-Dibromoethane	0.88	U	0.88	5.00	ug/Kg
127-18-4	Tetrachloroethene	1.10	U	1.10	5.00	ug/Kg
108-90-7	Chlorobenzene	0.91	U	0.91	5.00	ug/Kg
100-41-4	Ethyl Benzene	0.67	U	0.67	5.00	ug/Kg
179601-23-1	m/p-Xylenes	1.20	U	1.20	10.0	ug/Kg
95-47-6	o-Xylene	0.82	U	0.82	5.00	ug/Kg
100-42-5	Styrene	0.71	U	0.71	5.00	ug/Kg
75-25-2	Bromoform	0.86	U	0.86	5.00	ug/Kg
98-82-8	Isopropylbenzene	0.78	U	0.78	5.00	ug/Kg
79-34-5	1,1,2,2-Tetrachloroethane	1.20	U	1.20	5.00	ug/Kg
541-73-1	1,3-Dichlorobenzene	1.70	U	1.70	5.00	ug/Kg
106-46-7	1,4-Dichlorobenzene	1.60	U	1.60	5.00	ug/Kg
95-50-1	1,2-Dichlorobenzene	1.50	U	1.50	5.00	ug/Kg
96-12-8	1,2-Dibromo-3-Chloropropane	1.80	U	1.80	5.00	ug/Kg
120-82-1	1,2,4-Trichlorobenzene	3.00	U	3.00	5.00	ug/Kg
87-61-6	1,2,3-Trichlorobenzene	3.20	U	3.20	5.00	ug/Kg
SURROGATES						
17060-07-0	1,2-Dichloroethane-d4	59.8		63 - 155	120%	SPK: 50
1868-53-7	Dibromofluoromethane	52.7		70 - 134	105%	SPK: 50
2037-26-5	Toluene-d8	52.4		74 - 123	105%	SPK: 50
460-00-4	4-Bromofluorobenzene	47.5		17 - 146	95%	SPK: 50
INTERNAL STANDARDS						
363-72-4	Pentafluorobenzene	551000	7.707			
540-36-3	1,4-Difluorobenzene	1050000	8.616			
3114-55-4	Chlorobenzene-d5	953000	11.414			
3855-82-1	1,4-Dichlorobenzene-d4	371000	13.346			



284 Sheffield Street, Mountainside, New Jersey 07092, Phone : 908 789 8900,
Fax : 908 789 8922

Report of Analysis

Client:	Sciacca General Contractors, LLC		Date Collected:	
Project:	507 Franklin Ave		Date Received:	
Client Sample ID:	VY0815SBL01		SDG No.:	Q2868
Lab Sample ID:	VY0815SBL01		Matrix:	SOIL
Analytical Method:	8260D		% Solid:	100
Sample Wt/Vol:	5	Units: g	Final Vol:	5000 uL
Soil Aliquot Vol:		uL	Test:	VOC-TCLVOA-10
GC Column:	RXI-624	ID : 0.25	Level :	LOW
Prep Method :				

File ID/Qc Batch:	Dilution:	Date Analyzed	Prep Batch ID
VY023112.D	1	08/15/25 09:08	VY081525

CAS Number	Parameter	Conc.	Qualifier	MDL	LOQ / CRQL	Units
------------	-----------	-------	-----------	-----	------------	-------

U = Not Detected

LOQ = Limit of Quantitation

MDL = Method Detection Limit

LOD = Limit of Detection

E = Value Exceeds Calibration Range

Q = indicates LCS control criteria did not meet requirements

M = MS/MSD acceptance criteria did not meet requirements

J = Estimated Value

B = Analyte Found in Associated Method Blank

N = Presumptive Evidence of a Compound

* = Values outside of QC limits

D = Dilution

() = Laboratory InHouse Limit

A = Aldol-Condensation Reaction Products

Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY081525\
Data File : VY023112.D
Acq On : 15 Aug 2025 09:08
Operator : SY/MD
Sample : VY0815SBL01
Misc : 5.00g/5.0mL/MSVOA_Y/SOIL
ALS Vial : 3 Sample Multiplier: 1

Instrument :
MSVOA_Y
ClientSampleId :
VY0815SBL01

Quant Time: Aug 18 02:23:41 2025
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y081225S.M
Quant Title : SW846 8260
QLast Update : Wed Aug 13 02:10:11 2025
Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Pentafluorobenzene	7.707	168	550500	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	8.616	114	1049087	50.000	ug/l	0.00
63) Chlorobenzene-d5	11.414	117	953139	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.346	152	370974	50.000	ug/l	0.00

System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	8.061	65	313986	59.845	ug/l	0.00
Spiked Amount	50.000	Range	50 - 163	Recovery	=	119.700%
35) Dibromofluoromethane	7.634	113	330708	52.682	ug/l	0.00
Spiked Amount	50.000	Range	54 - 147	Recovery	=	105.360%
50) Toluene-d8	10.103	98	1285132	52.405	ug/l	0.00
Spiked Amount	50.000	Range	58 - 134	Recovery	=	104.800%
62) 4-Bromofluorobenzene	12.401	95	374958	47.544	ug/l	0.00
Spiked Amount	50.000	Range	30 - 143	Recovery	=	95.080%


Target Compounds	Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY081525\
Data File : VY023112.D
Acq On : 15 Aug 2025 09:08
Operator : SY/MD
Sample : VY0815SBL01
Misc : 5.00g/5.0mL/MSVOA_Y/SOIL
ALS Vial : 3 Sample Multiplier: 1

Instrument :
MSVOA_Y
ClientSampleId :
VY0815SBL01

Quant Time: Aug 18 02:23:41 2025
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y081225S.M
Quant Title : SW846 8260
QLast Update : Wed Aug 13 02:10:11 2025
Response via : Initial Calibration




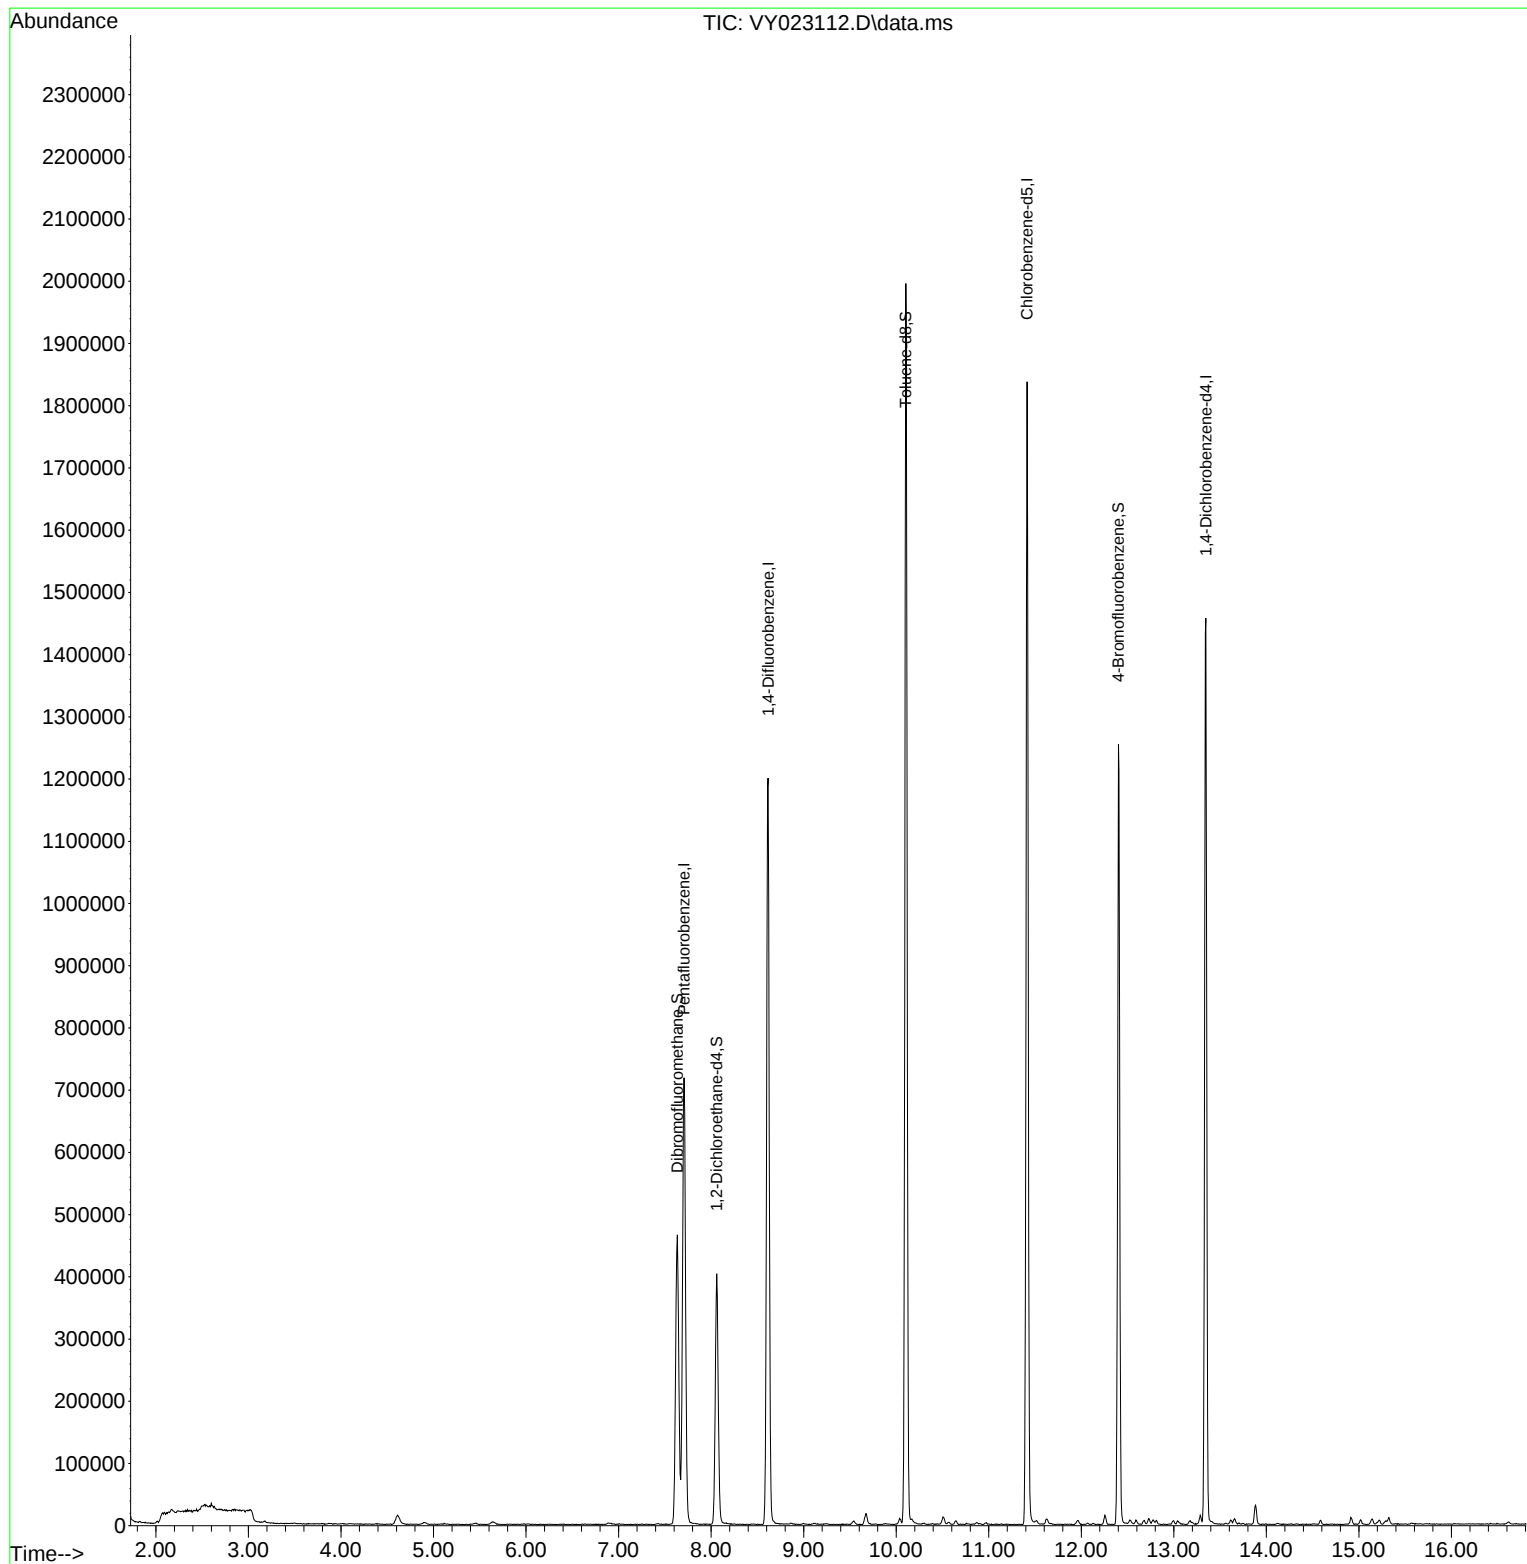


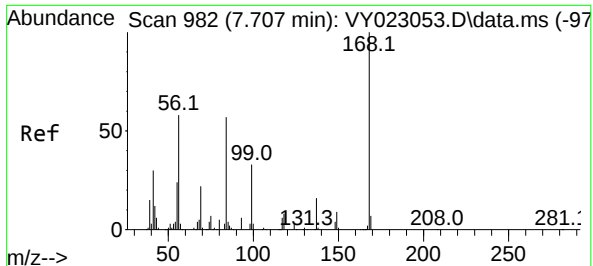

#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 7.707 min Scan# 91
Delta R.T. 0.000 min
Lab File: VY023112.D
Acq: 15 Aug 2025 09:08




Instrument :
MSVOA_Y
ClientSampleId :
VY0815SBL01


Tgt Ion:168 Resp: 550500
Ion Ratio Lower Upper
168 100
99 56.5 42.8 64.2

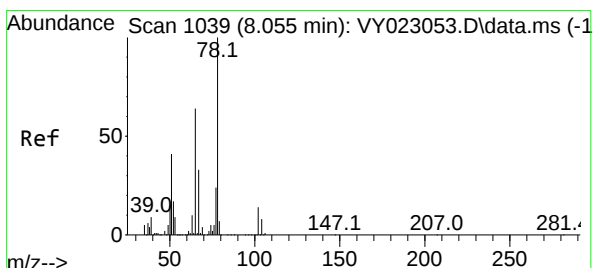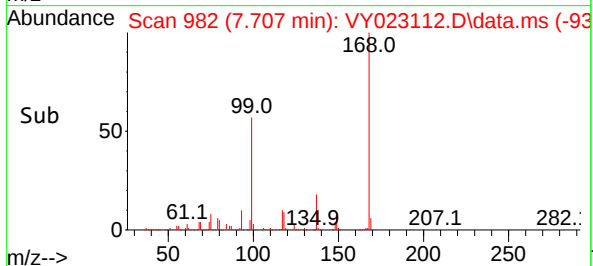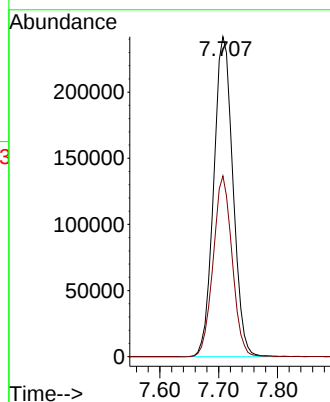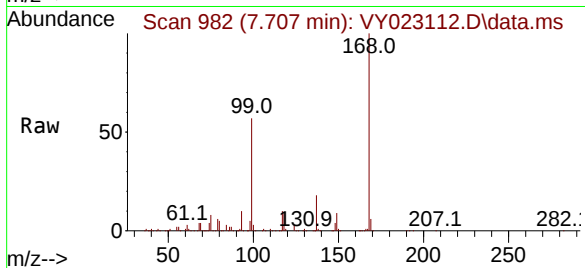

#33
1,2-Dichloroethane-d4
Concen: 59.845 ug/l
RT: 8.061 min Scan# 1040
Delta R.T. 0.006 min
Lab File: VY023112.D
Acq: 15 Aug 2025 09:08

Tgt Ion: 65 Resp: 313986
Ion Ratio Lower Upper
65 100
67 52.3 0.0 106.8

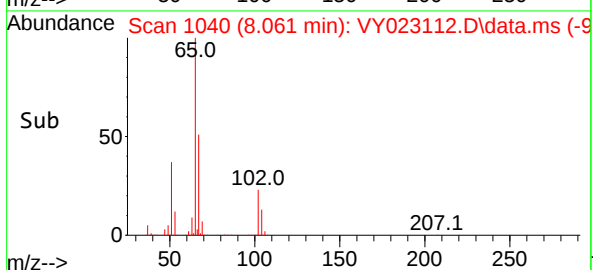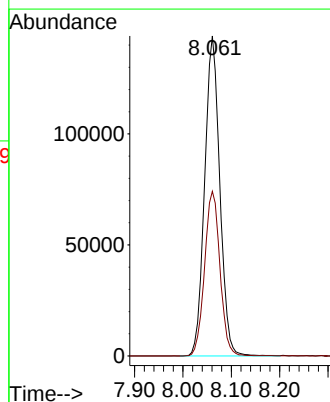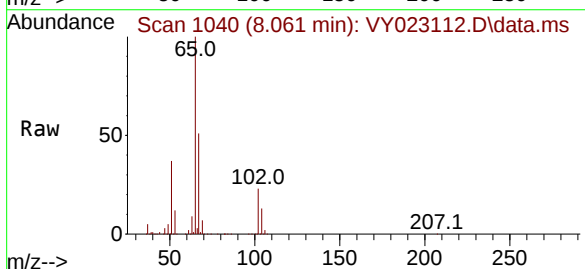

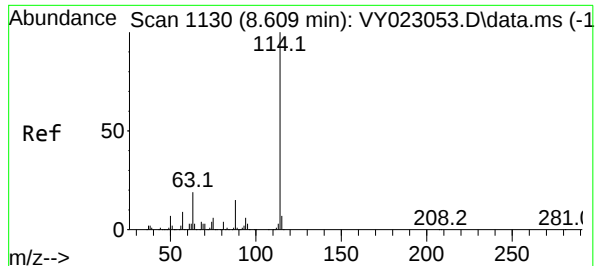

#34

1,4-Difluorobenzene

Concen: 50.000 ug/l

RT: 8.616 min Scan# 1131

Delta R.T. 0.006 min

Lab File: VY023112.D

Acq: 15 Aug 2025 09:08

Instrument :

MSVOA_Y

ClientSampleId :

VY0815SBL01





Tgt Ion:114 Resp: 1049087

Ion Ratio Lower Upper

114 100

63 19.0 0.0 38.4

88 14.6 0.0 30.0

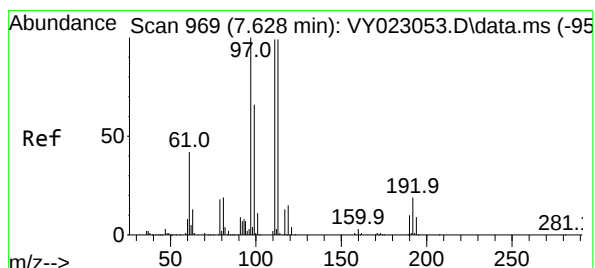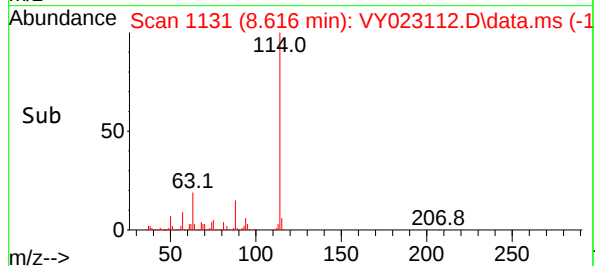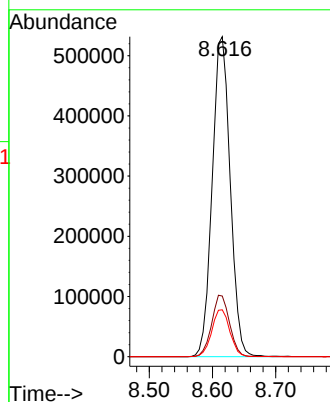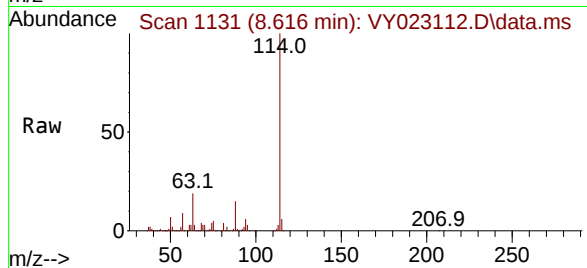

#35

Dibromofluoromethane

Concen: 52.682 ug/l

RT: 7.634 min Scan# 970

Delta R.T. 0.006 min

Lab File: VY023112.D

Acq: 15 Aug 2025 09:08




Tgt Ion:113 Resp: 330708


Ion Ratio Lower Upper

113 100

111 102.9 81.1 121.7

192 19.6 16.2 24.4


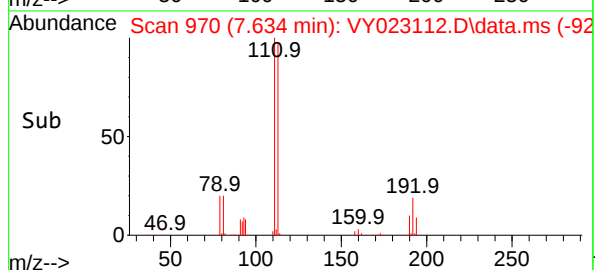
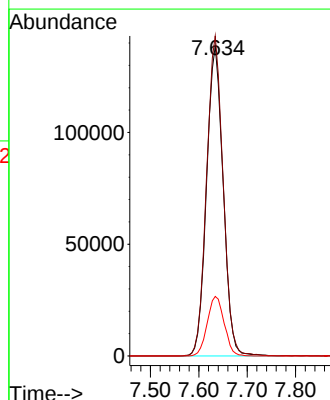
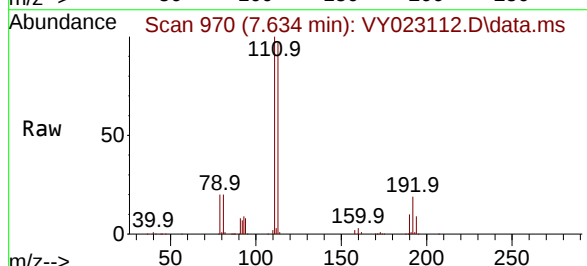


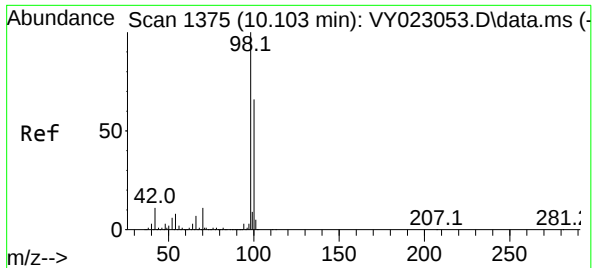

#50
Toluene-d8
Concen: 52.405 ug/l
RT: 10.103 min Scan# 1375
Delta R.T. 0.000 min
Lab File: VY023112.D
Acq: 15 Aug 2025 09:08




Instrument :
MSVOA_Y
ClientSampleId :
VY0815SBL01


Tgt Ion: 98 Resp: 1285132
Ion Ratio Lower Upper
98 100
100 64.8 52.3 78.5

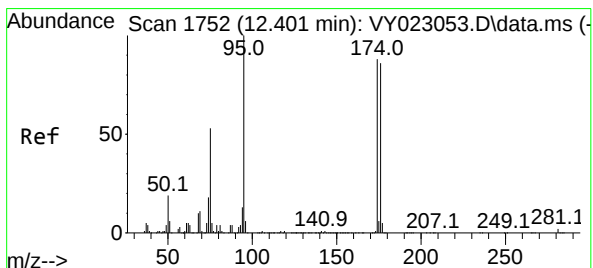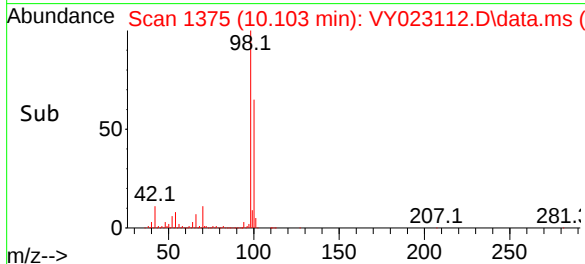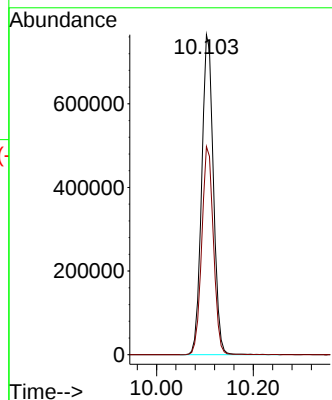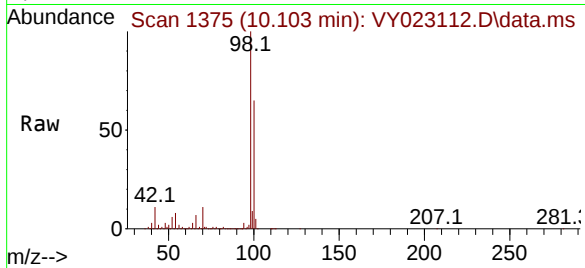

#62
4-Bromofluorobenzene
Concen: 47.544 ug/l
RT: 12.401 min Scan# 1752
Delta R.T. 0.000 min
Lab File: VY023112.D
Acq: 15 Aug 2025 09:08

Tgt Ion: 95 Resp: 374958
Ion Ratio Lower Upper
95 100
174 85.9 0.0 171.6
176 83.0 0.0 167.6

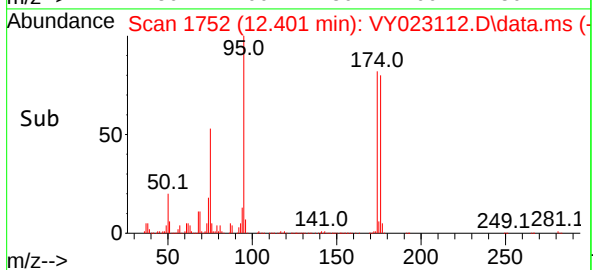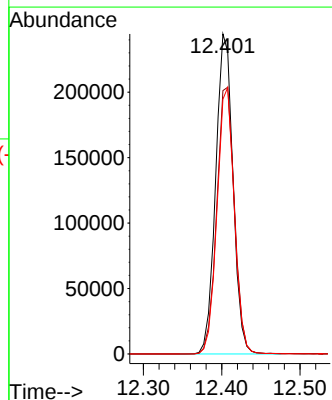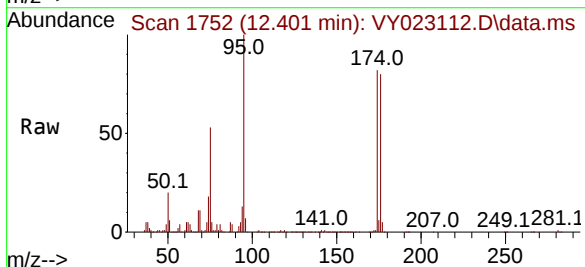

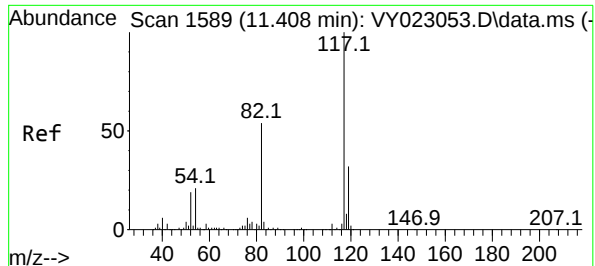

#63

Chlorobenzene-d5

Concen: 50.000 ug/l

RT: 11.414 min Scan# 117

Delta R.T. 0.006 min

Lab File: VY023112.D

Acq: 15 Aug 2025 09:08

Instrument :

MSVOA_Y

ClientSampleId :

VY0815SBL01





Tgt Ion:117 Resp: 953139

Ion Ratio Lower Upper

117 100

82 55.7 43.4 65.0

119 33.2 25.6 38.4

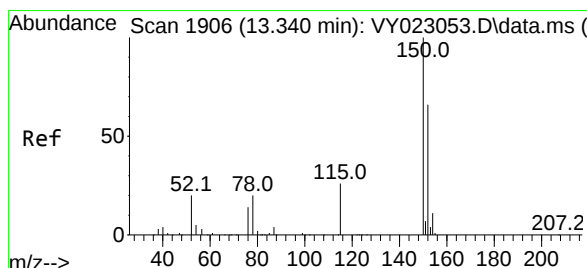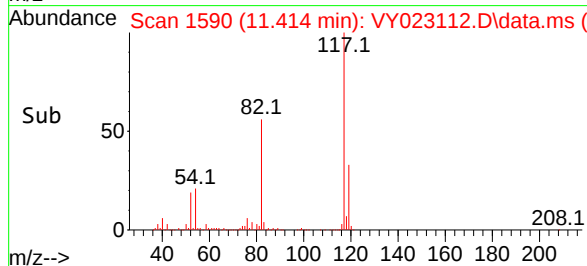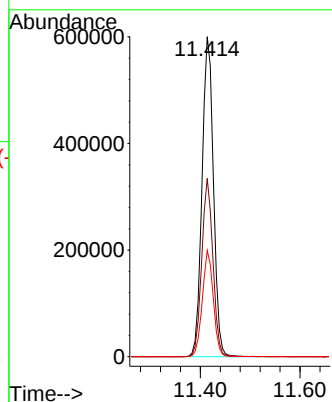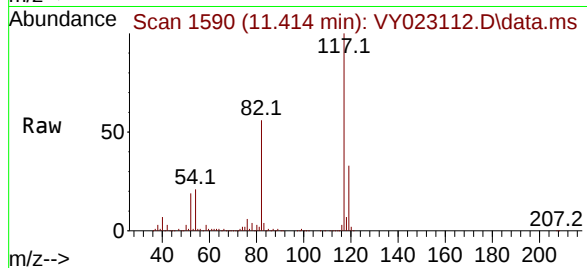

#72

1,4-Dichlorobenzene-d4

Concen: 50.000 ug/l

RT: 13.346 min Scan# 1907

Delta R.T. 0.006 min

Lab File: VY023112.D

Acq: 15 Aug 2025 09:08




Tgt Ion:152 Resp: 370974

Ion Ratio Lower Upper

152 100

115 56.8 28.2 84.6

150 157.6 0.0 348.0

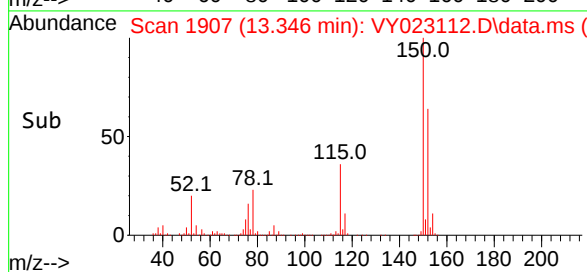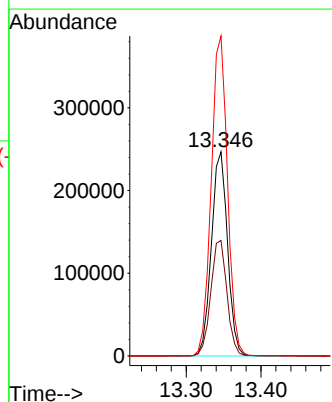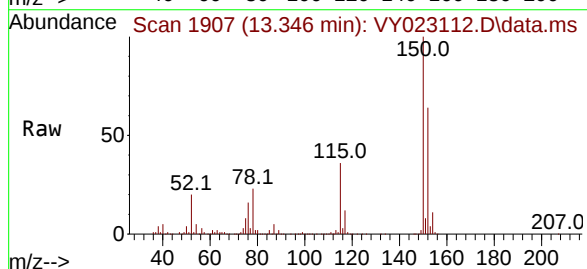

Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY081525\
 Data File : VY023112.D
 Acq On : 15 Aug 2025 09:08
 Operator : SY/MD
 Sample : VY0815SBL01
 Misc : 5.00g/5.0mL/MSVOA_Y/SOIL
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 MSVOA_Y
 ClientSampleId :
 VY0815SBL01

Integration Parameters: RTEINT.P

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y081225S.M

Title : SW846 8260

Signal : TIC: VY023112.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	4.610	463	474	487	rBV	14989	50337	1.51%	0.303%
2	7.634	960	970	976	rBV	464685	1112476	33.27%	6.688%
3	7.707	976	982	993	rVB	715479	1610606	48.17%	9.682%
4	8.061	1028	1040	1053	rBV	403205	890118	26.62%	5.351%
5	8.616	1121	1131	1144	rBV	1199454	2395578	71.65%	14.401%
6	9.676	1298	1305	1311	rBV	17461	37205	1.11%	0.224%
7	10.103	1368	1375	1384	rBV	1991604	3343501	100.00%	20.100%
8	11.414	1582	1590	1602	rBV	1836381	2914659	87.17%	17.522%
9	12.401	1745	1752	1763	rBV	1253322	1976340	59.11%	11.881%
10	13.346	1900	1907	1916	rVB	1452677	2248707	67.26%	13.518%
11	13.883	1988	1995	2004	rVB	30761	55163	1.65%	0.332%




Sum of corrected areas: 16634690

Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY081525\
Data File : VY023112.D
Acq On : 15 Aug 2025 09:08
Operator : SY/MD
Sample : VY0815SBL01
Misc : 5.00g/5.0mL/MSVOA_Y/SOIL
ALS Vial : 3 Sample Multiplier: 1

Instrument :
MSVOA_Y
ClientSampleId :
VY0815SBL01

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y081225S.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

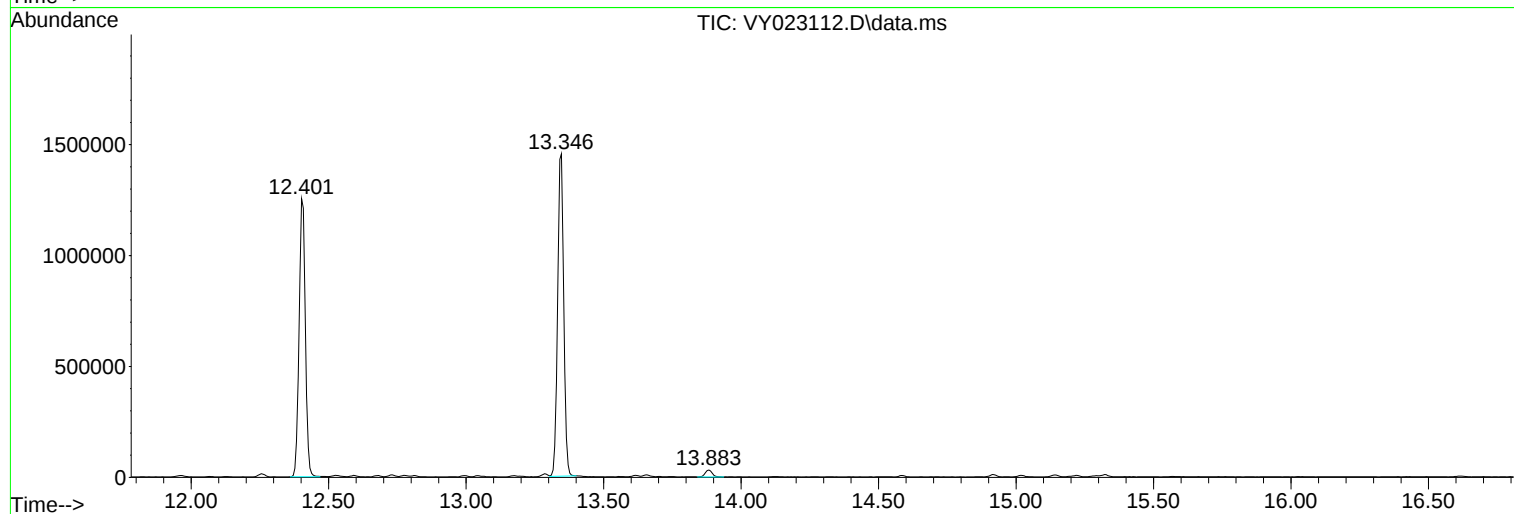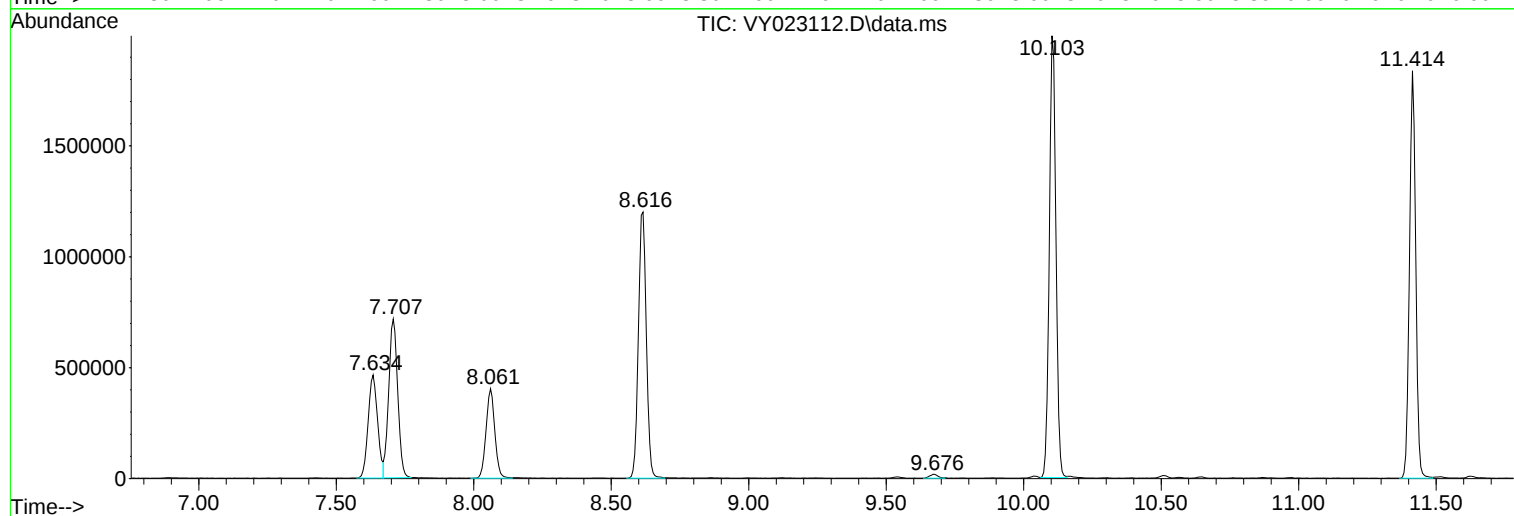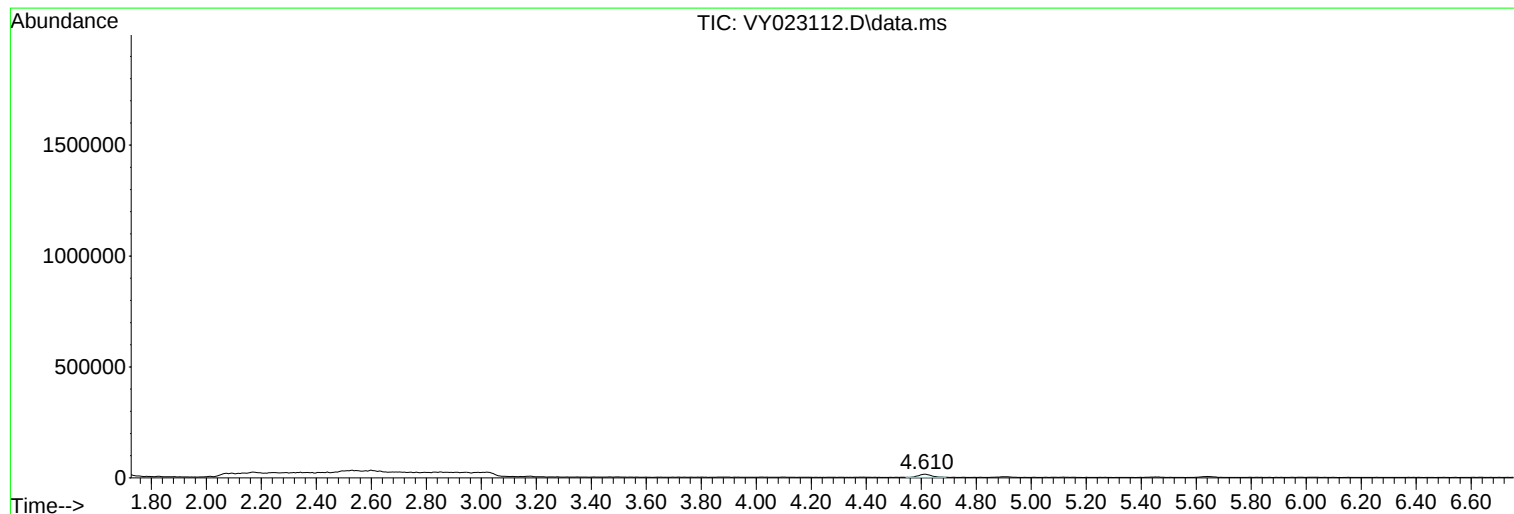

Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY081525\
Data File : VY023112.D
Acq On : 15 Aug 2025 09:08
Operator : SY/MD
Sample : VY0815SBL01
Misc : 5.00g/5.0mL/MSVOA_Y/SOIL
ALS Vial : 3 Sample Multiplier: 1

Instrument :
MSVOA_Y
ClientSampleId :
VY0815SBL01

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y081225S.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY081525\
Data File : VY023112.D
Acq On : 15 Aug 2025 09:08
Operator : SY/MD
Sample : VY0815SBL01
Misc : 5.00g/5.0mL/MSVOA_Y/SOIL
ALS Vial : 3 Sample Multiplier: 1

Instrument :
MSVOA_Y
ClientSampleId :
VY0815SBL01

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y081225S.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------

Report of Analysis

Client:	Sciaccia General Contractors, LLC			Date Collected:	
Project:	507 Franklin Ave			Date Received:	
Client Sample ID:	VY0815SBS01			SDG No.:	Q2868
Lab Sample ID:	VY0815SBS01			Matrix:	SOIL
Analytical Method:	8260D			% Solid:	100
Sample Wt/Vol:	5	Units:	g	Final Vol:	5000 uL
Soil Aliquot Vol:			uL	Test:	VOC-TCLVOA-10
GC Column:	RXI-624	ID :	0.25	Level :	LOW
Prep Method :					

File ID/Qc Batch:	Dilution:	Date Analyzed	Prep Batch ID
VY023113.D	1	08/15/25 09:37	VY081525

CAS Number	Parameter	Conc.	Qualifier	MDL	LOQ / CRQL	Units(Dry Weight)
TARGETS						
75-71-8	Dichlorodifluoromethane	19.7		1.10	5.00	ug/Kg
74-87-3	Chloromethane	22.2		1.10	5.00	ug/Kg
75-01-4	Vinyl Chloride	22.5		0.79	5.00	ug/Kg
74-83-9	Bromomethane	25.5		1.10	5.00	ug/Kg
75-00-3	Chloroethane	22.7		1.30	5.00	ug/Kg
75-69-4	Trichlorofluoromethane	21.1		1.20	5.00	ug/Kg
76-13-1	1,1,2-Trichlorotrifluoroethane	20.2		1.10	5.00	ug/Kg
75-35-4	1,1-Dichloroethene	19.8		1.00	5.00	ug/Kg
67-64-1	Acetone	110		4.70	25.0	ug/Kg
75-15-0	Carbon Disulfide	20.1		1.10	5.00	ug/Kg
1634-04-4	Methyl tert-butyl Ether	19.5		0.73	5.00	ug/Kg
79-20-9	Methyl Acetate	18.5		1.50	5.00	ug/Kg
75-09-2	Methylene Chloride	20.8		3.50	10.0	ug/Kg
156-60-5	trans-1,2-Dichloroethene	19.9		0.86	5.00	ug/Kg
75-34-3	1,1-Dichloroethane	20.4		0.80	5.00	ug/Kg
110-82-7	Cyclohexane	18.9		0.79	5.00	ug/Kg
78-93-3	2-Butanone	110		6.50	25.0	ug/Kg
56-23-5	Carbon Tetrachloride	19.6		0.97	5.00	ug/Kg
156-59-2	cis-1,2-Dichloroethene	20.1		0.75	5.00	ug/Kg
74-97-5	Bromochloromethane	21.9		1.20	5.00	ug/Kg
67-66-3	Chloroform	20.9		0.84	5.00	ug/Kg
71-55-6	1,1,1-Trichloroethane	20.3		0.93	5.00	ug/Kg
108-87-2	Methylcyclohexane	18.7		0.91	5.00	ug/Kg
71-43-2	Benzene	20.4		0.79	5.00	ug/Kg
107-06-2	1,2-Dichloroethane	20.6		0.79	5.00	ug/Kg
79-01-6	Trichloroethene	20.5		0.81	5.00	ug/Kg
78-87-5	1,2-Dichloropropane	20.5		0.91	5.00	ug/Kg
75-27-4	Bromodichloromethane	20.8		0.78	5.00	ug/Kg
108-10-1	4-Methyl-2-Pentanone	97.9		3.60	25.0	ug/Kg
108-88-3	Toluene	20.2		0.78	5.00	ug/Kg

Report of Analysis

Client:	Sciacca General Contractors, LLC	Date Collected:	
Project:	507 Franklin Ave	Date Received:	
Client Sample ID:	VY0815SBS01	SDG No.:	Q2868
Lab Sample ID:	VY0815SBS01	Matrix:	SOIL
Analytical Method:	8260D	% Solid:	100
Sample Wt/Vol:	5 Units: g	Final Vol:	5000 uL
Soil Aliquot Vol:	uL	Test:	VOC-TCLVOA-10
GC Column:	RXI-624 ID : 0.25	Level :	LOW
Prep Method :			

File ID/Qc Batch:	Dilution:	Date Analyzed	Prep Batch ID
VY023113.D	1	08/15/25 09:37	VY081525

CAS Number	Parameter	Conc.	Qualifier	MDL	LOQ / CRQL	Units(Dry Weight)
10061-02-6	t-1,3-Dichloropropene	19.9		0.65	5.00	ug/Kg
10061-01-5	cis-1,3-Dichloropropene	19.6		0.62	5.00	ug/Kg
79-00-5	1,1,2-Trichloroethane	20.2		0.92	5.00	ug/Kg
591-78-6	2-Hexanone	100		3.70	25.0	ug/Kg
124-48-1	Dibromochloromethane	20.1		0.87	5.00	ug/Kg
106-93-4	1,2-Dibromoethane	20.1		0.88	5.00	ug/Kg
127-18-4	Tetrachloroethene	21.8		1.10	5.00	ug/Kg
108-90-7	Chlorobenzene	19.5		0.91	5.00	ug/Kg
100-41-4	Ethyl Benzene	18.8		0.67	5.00	ug/Kg
179601-23-1	m/p-Xylenes	38.6		1.20	10.0	ug/Kg
95-47-6	o-Xylene	18.6		0.82	5.00	ug/Kg
100-42-5	Styrene	19.4		0.71	5.00	ug/Kg
75-25-2	Bromoform	18.7		0.86	5.00	ug/Kg
98-82-8	Isopropylbenzene	18.8		0.78	5.00	ug/Kg
79-34-5	1,1,2,2-Tetrachloroethane	18.1		1.20	5.00	ug/Kg
541-73-1	1,3-Dichlorobenzene	19.1		1.70	5.00	ug/Kg
106-46-7	1,4-Dichlorobenzene	19.3		1.60	5.00	ug/Kg
95-50-1	1,2-Dichlorobenzene	18.9		1.50	5.00	ug/Kg
96-12-8	1,2-Dibromo-3-Chloropropane	19.8		1.80	5.00	ug/Kg
120-82-1	1,2,4-Trichlorobenzene	18.2		3.00	5.00	ug/Kg
87-61-6	1,2,3-Trichlorobenzene	17.9		3.20	5.00	ug/Kg
SURROGATES						
17060-07-0	1,2-Dichloroethane-d4	51.7		63 - 155	103%	SPK: 50
1868-53-7	Dibromofluoromethane	49.3		70 - 134	99%	SPK: 50
2037-26-5	Toluene-d8	50.2		74 - 123	100%	SPK: 50
460-00-4	4-Bromofluorobenzene	48.5		17 - 146	97%	SPK: 50
INTERNAL STANDARDS						
363-72-4	Pentafluorobenzene	452000	7.707			
540-36-3	1,4-Difluorobenzene	727000	8.616			
3114-55-4	Chlorobenzene-d5	654000	11.414			
3855-82-1	1,4-Dichlorobenzene-d4	327000	13.341			



284 Sheffield Street, Mountainside, New Jersey 07092, Phone : 908 789 8900,
Fax : 908 789 8922

Report of Analysis

Client:	Sciacca General Contractors, LLC		Date Collected:	
Project:	507 Franklin Ave		Date Received:	
Client Sample ID:	VY0815SBS01		SDG No.:	Q2868
Lab Sample ID:	VY0815SBS01		Matrix:	SOIL
Analytical Method:	8260D		% Solid:	100
Sample Wt/Vol:	5	Units: g	Final Vol:	5000 uL
Soil Aliquot Vol:		uL	Test:	VOC-TCLVOA-10
GC Column:	RXI-624	ID : 0.25	Level :	LOW
Prep Method :				

File ID/Qc Batch:	Dilution:	Date Analyzed	Prep Batch ID
VY023113.D	1	08/15/25 09:37	VY081525

CAS Number	Parameter	Conc.	Qualifier	MDL	LOQ / CRQL	Units
------------	-----------	-------	-----------	-----	------------	-------

U = Not Detected

LOQ = Limit of Quantitation

MDL = Method Detection Limit

LOD = Limit of Detection

E = Value Exceeds Calibration Range

Q = indicates LCS control criteria did not meet requirements

M = MS/MSD acceptance criteria did not meet requirements

J = Estimated Value

B = Analyte Found in Associated Method Blank

N = Presumptive Evidence of a Compound

* = Values outside of QC limits

D = Dilution

() = Laboratory InHouse Limit

A = Aldol-Condensation Reaction Products

Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY081525\
 Data File : VY023113.D
 Acq On : 15 Aug 2025 09:37
 Operator : SY/MD
 Sample : VY0815SBS01
 Misc : 5.00g/5.0mL/MSVOA_Y/SOIL
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_Y
 ClientSampleId :
 VY0815SBS01

Manual Integrations
 APPROVED

Reviewed By :Semsettin Yesilyurt 08/19/2025
 Supervised By :Mahesh Dadoda 08/19/2025

Quant Time: Aug 18 02:24:07 2025
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y081225S.M
 Quant Title : SW846 8260
 QLast Update : Wed Aug 13 02:10:11 2025
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Pentafluorobenzene	7.707	168	452403	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	8.616	114	727202	50.000	ug/l	0.00
63) Chlorobenzene-d5	11.414	117	654458	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.341	152	327154	50.000	ug/l	0.00

System Monitoring Compounds

33) 1,2-Dichloroethane-d4	8.061	65	222883	51.692	ug/l	0.00
Spiked Amount	50.000	Range	50 - 163	Recovery	=	103.380%
35) Dibromofluoromethane	7.634	113	214583	49.314	ug/l	0.00
Spiked Amount	50.000	Range	54 - 147	Recovery	=	98.620%
50) Toluene-d8	10.103	98	852746	50.165	ug/l	0.00
Spiked Amount	50.000	Range	58 - 134	Recovery	=	100.320%
62) 4-Bromofluorobenzene	12.402	95	265399	48.547	ug/l	0.00
Spiked Amount	50.000	Range	30 - 143	Recovery	=	97.100%

Target Compounds

						Qvalue
2) Dichlorodifluoromethane	1.861	85	72666	19.678	ug/l	95
3) Chloromethane	2.068	50	133033	22.242	ug/l	99
4) Vinyl Chloride	2.202	62	166453	22.514	ug/l	99
5) Bromomethane	2.586	94	140731	25.487	ug/l	99
6) Chloroethane	2.733	64	111737	22.732	ug/l	98
7) Trichlorofluoromethane	3.050	101	189636	21.094	ug/l	99
8) Diethyl Ether	3.452	74	47224	19.855	ug/l	99
9) 1,1,2-Trichlorotrifluo...	3.812	101	89471	20.173	ug/l	98
10) Methyl Iodide	4.001	142	86732	18.122	ug/l	98
11) Tert butyl alcohol	4.860	59	27882	94.376	ug/l	99
12) 1,1-Dichloroethene	3.787	96	86211	19.775	ug/l	96
13) Acrolein	3.647	56	38871	89.841	ug/l	100
14) Allyl chloride	4.379	41	123002	19.175	ug/l	98
15) Acrylonitrile	5.055	53	97096	100.413	ug/l	99
16) Acetone	3.867	43	106046	113.526	ug/l	96
17) Carbon Disulfide	4.104	76	285962	20.117	ug/l	99
18) Methyl Acetate	4.379	43	51562	18.549	ug/l	98
19) Methyl tert-butyl Ether	5.116	73	220832	19.548	ug/l	98
20) Methylene Chloride	4.610	84	108703	20.808	ug/l	98
21) trans-1,2-Dichloroethene	5.110	96	97531	19.907	ug/l	98
22) Diisopropyl ether	6.019	45	280592	20.129	ug/l	95
23) Vinyl Acetate	5.958	43	767186	99.534	ug/l	98
24) 1,1-Dichloroethane	5.915	63	173658	20.377	ug/l	99
25) 2-Butanone	6.890	43	133656	105.206	ug/l	100
26) 2,2-Dichloropropane	6.884	77	149423	20.319	ug/l	100
27) cis-1,2-Dichloroethene	6.884	96	113605	20.058	ug/l	97
28) Bromochloromethane	7.238	49	74111	21.919	ug/l	96
29) Tetrahydrofuran	7.262	42	77082	97.884	ug/l	99
30) Chloroform	7.415	83	183779	20.909	ug/l	92
31) Cyclohexane	7.701	56	151804	18.902	ug/l	95
32) 1,1,1-Trichloroethane	7.616	97	157956	20.254	ug/l	99
36) 1,1-Dichloropropene	7.835	75	129384	20.008	ug/l	99
37) Ethyl Acetate	6.982	43	55493	20.428	ug/l	98
38) Carbon Tetrachloride	7.817	117	137873	19.630	ug/l	99
39) Methylcyclohexane	9.103	83	159285	18.705	ug/l	99
40) Benzene	8.079	78	405603	20.350	ug/l	100

Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY081525\
 Data File : VY023113.D
 Acq On : 15 Aug 2025 09:37
 Operator : SY/MD
 Sample : VY0815SBS01
 Misc : 5.00g/5.0mL/MSVOA_Y/SOIL
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_Y
 ClientSampleId :
 VY0815SBS01

Manual Integrations
 APPROVED

Reviewed By :Semsettin Yesilyurt 08/19/2025
 Supervised By :Mahesh Dadoda 08/19/2025

Quant Time: Aug 18 02:24:07 2025
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y081225S.M
 Quant Title : SW846 8260
 QLast Update : Wed Aug 13 02:10:11 2025
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
41) Methacrylonitrile	7.220	41	28150	17.956	ug/l	90
42) 1,2-Dichloroethane	8.152	62	106658	20.575	ug/l	98
43) Isopropyl Acetate	8.195	43	107344	19.551	ug/l	99
44) Trichloroethene	8.860	130	105377	20.459	ug/l	100
45) 1,2-Dichloropropane	9.140	63	93789	20.451	ug/l	100
46) Dibromomethane	9.231	93	54800	20.819	ug/l	97
47) Bromodichloromethane	9.420	83	141008	20.819	ug/l	100
48) Methyl methacrylate	9.219	41	49562	18.864	ug/l	98
49) 1,4-Dioxane	9.238	88	12370	400.796	ug/l	97
51) 4-Methyl-2-Pentanone	9.994	43	277163	97.864	ug/l	100
52) Toluene	10.170	92	255717	20.201	ug/l	99
53) t-1,3-Dichloropropene	10.390	75	121993	19.890	ug/l	97
54) cis-1,3-Dichloropropene	9.853	75	142316	19.623	ug/l	98
55) 1,1,2-Trichloroethane	10.567	97	71057	20.174	ug/l	98
56) Ethyl methacrylate	10.439	69	86412	19.173	ug/l	98
57) 1,3-Dichloropropane	10.713	76	118549	19.846	ug/l	99
58) 2-Chloroethyl Vinyl ether	9.707	63	208567	98.106	ug/l	100
59) 2-Hexanone	10.756	43	193382	100.277	ug/l	99
60) Dibromochloromethane	10.908	129	93374	20.091	ug/l	99
61) 1,2-Dibromoethane	11.012	107	66622	20.125	ug/l	98
64) Tetrachloroethene	10.646	164	127239	21.773	ug/l	93
65) Chlorobenzene	11.438	112	274616	19.453	ug/l	97
66) 1,1,1,2-Tetrachloroethane	11.512	131	93262	19.466	ug/l	98
67) Ethyl Benzene	11.518	91	456905	18.808	ug/l	98
68) m/p-Xylenes	11.627	106	365819	38.555	ug/l	98
69) o-Xylene	11.951	106	165713	18.648	ug/l	98
70) Styrene	11.969	104	281721	19.385	ug/l	99
71) Bromoform	12.127	173	52326	18.687	ug/l #	98
73) Isopropylbenzene	12.249	105	433053	18.755	ug/l	99
74) N-amyl acetate	12.066	43	91104	18.605	ug/l	98
75) 1,1,2,2-Tetrachloroethane	12.499	83	71400	18.110	ug/l	99
76) 1,2,3-Trichloropropane	12.554	75	61433m	19.457	ug/l	
77) Bromobenzene	12.530	156	104694	19.006	ug/l	97
78) n-propylbenzene	12.591	91	527930	19.204	ug/l	100
79) 2-Chlorotoluene	12.676	91	298409	18.946	ug/l	100
80) 1,3,5-Trimethylbenzene	12.731	105	351759	18.850	ug/l	100
81) trans-1,4-Dichloro-2-b...	12.298	75	24161	18.524	ug/l	95
82) 4-Chlorotoluene	12.774	91	307174	18.799	ug/l	99
83) tert-Butylbenzene	12.993	119	305956	18.153	ug/l	98
84) 1,2,4-Trimethylbenzene	13.042	105	356647	19.199	ug/l	99
85) sec-Butylbenzene	13.170	105	468353	18.917	ug/l	100
86) p-Isopropyltoluene	13.286	119	388353	18.897	ug/l	100
87) 1,3-Dichlorobenzene	13.286	146	206995	19.055	ug/l	100
88) 1,4-Dichlorobenzene	13.365	146	207638	19.268	ug/l	99
89) n-Butylbenzene	13.615	91	353333	18.720	ug/l	98
90) Hexachloroethane	13.877	117	82985	19.725	ug/l	97
91) 1,2-Dichlorobenzene	13.658	146	180503	18.946	ug/l	99
92) 1,2-Dibromo-3-Chloropr...	14.267	75	12160	19.809	ug/l	96
93) 1,2,4-Trichlorobenzene	14.913	180	102405	18.177	ug/l	99
94) Hexachlorobutadiene	15.017	225	61940	18.710	ug/l	98
95) Naphthalene	15.139	128	168145	17.503	ug/l	99
96) 1,2,3-Trichlorobenzene	15.322	180	86860	17.892	ug/l	99

Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY081525\
Data File : VY023113.D
Acq On : 15 Aug 2025 09:37
Operator : SY/MD
Sample : VY0815SBS01
Misc : 5.00g/5.0mL/MSVOA_Y/SOIL
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_Y
ClientSampleId :
VY0815SBS01

Manual Integrations
APPROVED

Reviewed By :Semsettin Yesilyurt 08/19/2025
Supervised By :Mahesh Dadoda 08/19/2025

Quant Time: Aug 18 02:24:07 2025
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y081225S.M
Quant Title : SW846 8260
QLast Update : Wed Aug 13 02:10:11 2025
Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
----------	------	------	----------	------	-------	----------

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY081525\
Data File : VY023113.D
Acq On : 15 Aug 2025 09:37
Operator : SY/MD
Sample : VY0815SBS01
Misc : 5.00g/5.0mL/MSVOA_Y/SOIL
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_Y
ClientSampleId :
VY0815SBS01

Manual Integrations APPROVED

Reviewed By :Semsettin Yesilyurt 08/19/2025
Supervised By :Mahesh Dadoda 08/19/2025

Quant Time: Aug 18 02:24:07 2025
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y081225S.M
Quant Title : SW846 8260
QLast Update : Wed Aug 13 02:10:11 2025
Response via : Initial Calibration

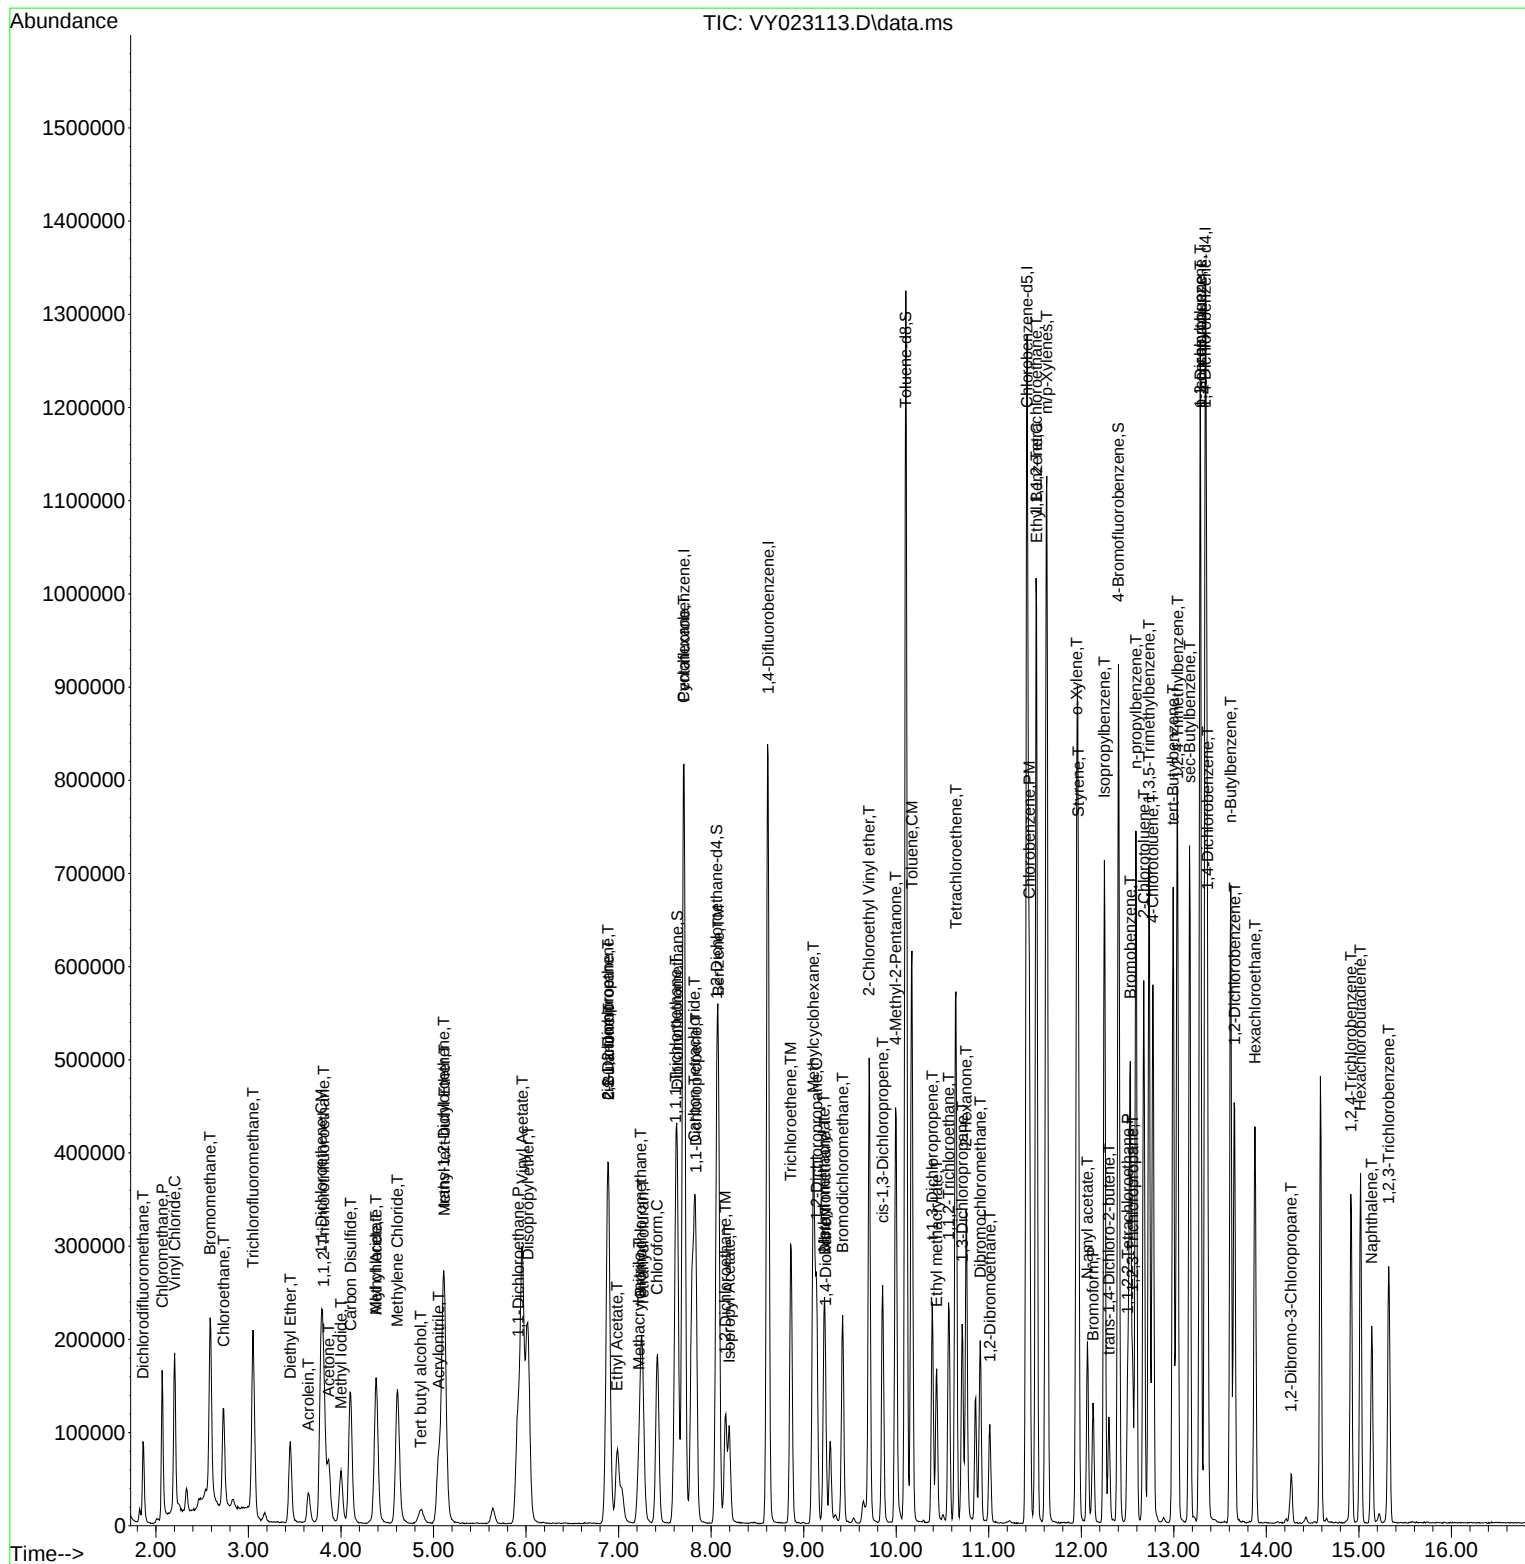

Report of Analysis

Client: Sciacca General Contractors, LLC

Date Collected:

Project: 507 Franklin Ave

Date Received:

Client Sample ID: VY0815SBSD01

SDG No.: Q2868

Lab Sample ID: VY0815SBSD01

Matrix: SOIL

Analytical Method: 8260D

% Solid: 100

Sample Wt/Vol: 5 Units: g

Final Vol: 5000 uL

Soil Aliquot Vol: _____ uL

Test: VOC-TCLVOA-10

GC Column: RXI-624 ID : 0.25

Level : LOW

Prep Method :

File ID/Qc Batch: Dilution:

Date Analyzed

Prep Batch ID

VY023114.D

1

08/15/25 09:59

VY081525

CAS Number	Parameter	Conc.	Qualifier	MDL	LOQ / CRQL	Units(Dry Weight)
TARGETS						
75-71-8	Dichlorodifluoromethane	21.3		1.10	5.00	ug/Kg
74-87-3	Chloromethane	22.8		1.10	5.00	ug/Kg
75-01-4	Vinyl Chloride	23.3		0.79	5.00	ug/Kg
74-83-9	Bromomethane	25.5		1.10	5.00	ug/Kg
75-00-3	Chloroethane	23.9		1.30	5.00	ug/Kg
75-69-4	Trichlorofluoromethane	22.3		1.20	5.00	ug/Kg
76-13-1	1,1,2-Trichlorotrifluoroethane	21.7		1.10	5.00	ug/Kg
75-35-4	1,1-Dichloroethene	20.9		1.00	5.00	ug/Kg
67-64-1	Acetone	110		4.70	25.0	ug/Kg
75-15-0	Carbon Disulfide	20.8		1.10	5.00	ug/Kg
1634-04-4	Methyl tert-butyl Ether	20.3		0.73	5.00	ug/Kg
79-20-9	Methyl Acetate	21.2		1.50	5.00	ug/Kg
75-09-2	Methylene Chloride	22.1		3.50	10.0	ug/Kg
156-60-5	trans-1,2-Dichloroethene	21.0		0.86	5.00	ug/Kg
75-34-3	1,1-Dichloroethane	21.0		0.80	5.00	ug/Kg
110-82-7	Cyclohexane	19.7		0.79	5.00	ug/Kg
78-93-3	2-Butanone	100		6.50	25.0	ug/Kg
56-23-5	Carbon Tetrachloride	20.5		0.97	5.00	ug/Kg
156-59-2	cis-1,2-Dichloroethene	20.5		0.75	5.00	ug/Kg
74-97-5	Bromochloromethane	21.8		1.20	5.00	ug/Kg
67-66-3	Chloroform	21.6		0.84	5.00	ug/Kg
71-55-6	1,1,1-Trichloroethane	21.0		0.93	5.00	ug/Kg
108-87-2	Methylcyclohexane	19.5		0.91	5.00	ug/Kg
71-43-2	Benzene	20.6		0.79	5.00	ug/Kg
107-06-2	1,2-Dichloroethane	20.9		0.79	5.00	ug/Kg
79-01-6	Trichloroethene	21.1		0.81	5.00	ug/Kg
78-87-5	1,2-Dichloropropane	20.6		0.91	5.00	ug/Kg
75-27-4	Bromodichloromethane	20.7		0.78	5.00	ug/Kg
108-10-1	4-Methyl-2-Pentanone	99.3		3.60	25.0	ug/Kg
108-88-3	Toluene	20.5		0.78	5.00	ug/Kg

Report of Analysis

Client:	Sciacca General Contractors, LLC	Date Collected:	
Project:	507 Franklin Ave	Date Received:	
Client Sample ID:	VY0815SBSD01	SDG No.:	Q2868
Lab Sample ID:	VY0815SBSD01	Matrix:	SOIL
Analytical Method:	8260D	% Solid:	100
Sample Wt/Vol:	5 Units: g	Final Vol:	5000 uL
Soil Aliquot Vol:	uL	Test:	VOC-TCLVOA-10
GC Column:	RXI-624 ID : 0.25	Level :	LOW
Prep Method :			

File ID/Qc Batch:	Dilution:	Date Analyzed	Prep Batch ID
VY023114.D	1	08/15/25 09:59	VY081525

CAS Number	Parameter	Conc.	Qualifier	MDL	LOQ / CRQL	Units(Dry Weight)
10061-02-6	t-1,3-Dichloropropene	19.7		0.65	5.00	ug/Kg
10061-01-5	cis-1,3-Dichloropropene	20.2		0.62	5.00	ug/Kg
79-00-5	1,1,2-Trichloroethane	20.4		0.92	5.00	ug/Kg
591-78-6	2-Hexanone	99.7		3.70	25.0	ug/Kg
124-48-1	Dibromochloromethane	20.6		0.87	5.00	ug/Kg
106-93-4	1,2-Dibromoethane	20.2		0.88	5.00	ug/Kg
127-18-4	Tetrachloroethene	22.8		1.10	5.00	ug/Kg
108-90-7	Chlorobenzene	21.1		0.91	5.00	ug/Kg
100-41-4	Ethyl Benzene	20.2		0.67	5.00	ug/Kg
179601-23-1	m/p-Xylenes	41.1		1.20	10.0	ug/Kg
95-47-6	o-Xylene	20.1		0.82	5.00	ug/Kg
100-42-5	Styrene	20.5		0.71	5.00	ug/Kg
75-25-2	Bromoform	19.8		0.86	5.00	ug/Kg
98-82-8	Isopropylbenzene	19.4		0.78	5.00	ug/Kg
79-34-5	1,1,2,2-Tetrachloroethane	19.0		1.20	5.00	ug/Kg
541-73-1	1,3-Dichlorobenzene	20.1		1.70	5.00	ug/Kg
106-46-7	1,4-Dichlorobenzene	19.8		1.60	5.00	ug/Kg
95-50-1	1,2-Dichlorobenzene	19.7		1.50	5.00	ug/Kg
96-12-8	1,2-Dibromo-3-Chloropropane	20.0		1.80	5.00	ug/Kg
120-82-1	1,2,4-Trichlorobenzene	18.5		3.00	5.00	ug/Kg
87-61-6	1,2,3-Trichlorobenzene	18.6		3.20	5.00	ug/Kg
SURROGATES						
17060-07-0	1,2-Dichloroethane-d4	52.1		63 - 155	104%	SPK: 50
1868-53-7	Dibromofluoromethane	50.3		70 - 134	101%	SPK: 50
2037-26-5	Toluene-d8	50.6		74 - 123	101%	SPK: 50
460-00-4	4-Bromofluorobenzene	48.7		17 - 146	97%	SPK: 50
INTERNAL STANDARDS						
363-72-4	Pentafluorobenzene	440000	7.707			
540-36-3	1,4-Difluorobenzene	718000	8.616			
3114-55-4	Chlorobenzene-d5	623000	11.414			
3855-82-1	1,4-Dichlorobenzene-d4	315000	13.34			



284 Sheffield Street, Mountainside, New Jersey 07092, Phone : 908 789 8900,
Fax : 908 789 8922

Report of Analysis

Client:	Sciacca General Contractors, LLC		Date Collected:	
Project:	507 Franklin Ave		Date Received:	
Client Sample ID:	VY0815SBSD01		SDG No.:	Q2868
Lab Sample ID:	VY0815SBSD01		Matrix:	SOIL
Analytical Method:	8260D		% Solid:	100
Sample Wt/Vol:	5	Units: g	Final Vol:	5000 uL
Soil Aliquot Vol:		uL	Test:	VOC-TCLVOA-10
GC Column:	RXI-624	ID : 0.25	Level :	LOW
Prep Method :				

File ID/Qc Batch:	Dilution:	Date Analyzed	Prep Batch ID
VY023114.D	1	08/15/25 09:59	VY081525

CAS Number	Parameter	Conc.	Qualifier	MDL	LOQ / CRQL	Units
------------	-----------	-------	-----------	-----	------------	-------

U = Not Detected

LOQ = Limit of Quantitation

MDL = Method Detection Limit

LOD = Limit of Detection

E = Value Exceeds Calibration Range

Q = indicates LCS control criteria did not meet requirements

M = MS/MSD acceptance criteria did not meet requirements

J = Estimated Value

B = Analyte Found in Associated Method Blank

N = Presumptive Evidence of a Compound

* = Values outside of QC limits

D = Dilution

() = Laboratory InHouse Limit

A = Aldol-Condensation Reaction Products

Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY081525\
 Data File : VY023114.D
 Acq On : 15 Aug 2025 09:59
 Operator : SY/MD
 Sample : VY0815SBS01
 Misc : 5.00g/5.0mL/MSVOA_Y/SOIL
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_Y
 ClientSampleId :
 VY0815SBS01

Manual Integrations
 APPROVED

Reviewed By :Semsettin Yesilyurt 08/19/2025
 Supervised By :Mahesh Dadoda 08/19/2025

Quant Time: Aug 18 02:25:28 2025
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y081225S.M
 Quant Title : SW846 8260
 QLast Update : Wed Aug 13 02:10:11 2025
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Pentafluorobenzene	7.707	168	440097	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	8.616	114	718363	50.000	ug/l	0.00
63) Chlorobenzene-d5	11.414	117	623331	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.340	152	315352	50.000	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	8.061	65	218582	52.112	ug/l	0.00
Spiked Amount	50.000	Range	50 - 163	Recovery	= 104.220%	
35) Dibromofluoromethane	7.634	113	216052	50.263	ug/l	0.00
Spiked Amount	50.000	Range	54 - 147	Recovery	= 100.520%	
50) Toluene-d8	10.103	98	848930	50.555	ug/l	0.00
Spiked Amount	50.000	Range	58 - 134	Recovery	= 101.100%	
62) 4-Bromofluorobenzene	12.401	95	263062	48.712	ug/l	0.00
Spiked Amount	50.000	Range	30 - 143	Recovery	= 97.420%	
Target Compounds						Qvalue
2) Dichlorodifluoromethane	1.861	85	76393	21.266	ug/l	99
3) Chloromethane	2.068	50	132852	22.833	ug/l	99
4) Vinyl Chloride	2.202	62	167480	23.286	ug/l	99
5) Bromomethane	2.586	94	136955	25.497	ug/l	99
6) Chloroethane	2.732	64	114091	23.860	ug/l	100
7) Trichlorofluoromethane	3.050	101	194616	22.253	ug/l	99
8) Diethyl Ether	3.452	74	48378	20.909	ug/l	94
9) 1,1,2-Trichlorotrifluo...	3.812	101	93467	21.663	ug/l	99
10) Methyl Iodide	4.001	142	95118	20.430	ug/l	98
11) Tert butyl alcohol	4.860	59	28033	97.541	ug/l	100
12) 1,1-Dichloroethene	3.781	96	88433	20.852	ug/l	97
13) Acrolein	3.647	56	36366	86.401	ug/l	100
14) Allyl chloride	4.379	41	121986	19.548	ug/l	98
15) Acrylonitrile	5.061	53	94706	100.680	ug/l	99
16) Acetone	3.866	43	99097	109.054	ug/l	97
17) Carbon Disulfide	4.098	76	288100	20.834	ug/l	99
18) Methyl Acetate	4.385	43	57336	21.203	ug/l	99
19) Methyl tert-butyl Ether	5.116	73	222672	20.262	ug/l	99
20) Methylene Chloride	4.610	84	111293	22.050	ug/l	99
21) trans-1,2-Dichloroethene	5.116	96	100236	21.032	ug/l	94
22) Diisopropyl ether	6.018	45	280376	20.676	ug/l	97
23) Vinyl Acetate	5.958	43	746169	99.514	ug/l	99
24) 1,1-Dichloroethane	5.915	63	173769	20.960	ug/l	98
25) 2-Butanone	6.890	43	127742	103.362	ug/l	98
26) 2,2-Dichloropropane	6.884	77	150177	20.993	ug/l	100
27) cis-1,2-Dichloroethene	6.890	96	113218	20.549	ug/l	100
28) Bromochloromethane	7.244	49	71693	21.797	ug/l	98
29) Tetrahydrofuran	7.256	42	75128	98.070	ug/l	99
30) Chloroform	7.421	83	184733	21.605	ug/l	98
31) Cyclohexane	7.701	56	153728	19.677	ug/l #	93
32) 1,1,1-Trichloroethane	7.616	97	159387	21.009	ug/l	98
36) 1,1-Dichloropropene	7.835	75	130154	20.374	ug/l	99
37) Ethyl Acetate	6.982	43	53108	19.791	ug/l	99
38) Carbon Tetrachloride	7.817	117	142469	20.534	ug/l	100
39) Methylcyclohexane	9.103	83	163971	19.492	ug/l	98
40) Benzene	8.079	78	406307	20.636	ug/l	97

Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY081525\
 Data File : VY023114.D
 Acq On : 15 Aug 2025 09:59
 Operator : SY/MD
 Sample : VY0815SBS01
 Misc : 5.00g/5.0mL/MSVOA_Y/SOIL
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_Y
 ClientSampleId :
 VY0815SBS01

Manual Integrations
 APPROVED

Reviewed By :Semsettin Yesilyurt 08/19/2025
 Supervised By :Mahesh Dadoda 08/19/2025

Quant Time: Aug 18 02:25:28 2025
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y081225S.M
 Quant Title : SW846 8260
 QLast Update : Wed Aug 13 02:10:11 2025
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
41) Methacrylonitrile	7.238	41	30597m	19.757	ug/l	
42) 1,2-Dichloroethane	8.158	62	106851	20.866	ug/l	98
43) Isopropyl Acetate	8.195	43	104154	19.203	ug/l	98
44) Trichloroethene	8.859	130	107257	21.080	ug/l	97
45) 1,2-Dichloropropane	9.140	63	93109	20.553	ug/l	100
46) Dibromomethane	9.231	93	55348	21.286	ug/l	96
47) Bromodichloromethane	9.420	83	138806	20.746	ug/l	97
48) Methyl methacrylate	9.219	41	48220	18.579	ug/l	93
49) 1,4-Dioxane	9.225	88	12812	420.225	ug/l	96
51) 4-Methyl-2-Pentanone	9.993	43	277745	99.276	ug/l	100
52) Toluene	10.170	92	256278	20.494	ug/l	98
53) t-1,3-Dichloropropene	10.390	75	119229	19.679	ug/l	96
54) cis-1,3-Dichloropropene	9.853	75	144778	20.208	ug/l	99
55) 1,1,2-Trichloroethane	10.566	97	70888	20.374	ug/l	97
56) Ethyl methacrylate	10.438	69	83239	18.696	ug/l	97
57) 1,3-Dichloropropane	10.713	76	119333	20.223	ug/l	99
58) 2-Chloroethyl Vinyl ether	9.707	63	207784	98.940	ug/l	99
59) 2-Hexanone	10.755	43	190027	99.749	ug/l	97
60) Dibromochloromethane	10.908	129	94653	20.617	ug/l	100
61) 1,2-Dibromoethane	11.011	107	65954	20.168	ug/l	99
64) Tetrachloroethene	10.646	164	126762	22.775	ug/l	99
65) Chlorobenzene	11.438	112	283100	21.056	ug/l	97
66) 1,1,1,2-Tetrachloroethane	11.511	131	94430	20.694	ug/l	98
67) Ethyl Benzene	11.518	91	466536	20.163	ug/l	99
68) m/p-Xylenes	11.627	106	371794	41.142	ug/l	97
69) o-Xylene	11.950	106	170235	20.113	ug/l	100
70) Styrene	11.963	104	283934	20.513	ug/l	99
71) Bromoform	12.127	173	52702	19.761	ug/l #	98
73) Isopropylbenzene	12.249	105	431158	19.372	ug/l	100
74) N-amyl acetate	12.066	43	89546	18.971	ug/l	99
75) 1,1,2,2-Tetrachloroethane	12.499	83	72067	18.963	ug/l	99
76) 1,2,3-Trichloropropane	12.554	75	62895m	20.665	ug/l	
77) Bromobenzene	12.530	156	104717	19.721	ug/l	99
78) n-propylbenzene	12.590	91	536311	20.239	ug/l	99
79) 2-Chlorotoluene	12.676	91	300425	19.787	ug/l	99
80) 1,3,5-Trimethylbenzene	12.731	105	355894	19.785	ug/l	100
81) trans-1,4-Dichloro-2-b...	12.298	75	23540	18.723	ug/l	94
82) 4-Chlorotoluene	12.773	91	318860	20.245	ug/l	100
83) tert-Butylbenzene	12.993	119	307259	18.913	ug/l	98
84) 1,2,4-Trimethylbenzene	13.042	105	355479	19.852	ug/l	99
85) sec-Butylbenzene	13.170	105	469710	19.682	ug/l	100
86) p-Isopropyltoluene	13.285	119	390935	19.735	ug/l	100
87) 1,3-Dichlorobenzene	13.285	146	210704	20.122	ug/l	98
88) 1,4-Dichlorobenzene	13.365	146	206023	19.834	ug/l	99
89) n-Butylbenzene	13.615	91	358048	19.679	ug/l	98
90) Hexachloroethane	13.877	117	81804	20.172	ug/l	97
91) 1,2-Dichlorobenzene	13.651	146	181214	19.733	ug/l	99
92) 1,2-Dibromo-3-Chloropr...	14.273	75	11846	20.020	ug/l	94
93) 1,2,4-Trichlorobenzene	14.913	180	100490	18.504	ug/l	97
94) Hexachlorobutadiene	15.017	225	59682	18.702	ug/l	97
95) Naphthalene	15.139	128	167894	18.131	ug/l	99
96) 1,2,3-Trichlorobenzene	15.322	180	86969	18.585	ug/l	99

Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY081525\
Data File : VY023114.D
Acq On : 15 Aug 2025 09:59
Operator : SY/MD
Sample : VY0815SBSD01
Misc : 5.00g/5.0mL/MSVOA_Y/SOIL
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_Y
ClientSampleId :
VY0815SBSD01

Manual Integrations
APPROVED

Reviewed By :Semsettin Yesilyurt 08/19/2025
Supervised By :Mahesh Dadoda 08/19/2025

Quant Time: Aug 18 02:25:28 2025
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y081225S.M
Quant Title : SW846 8260
QLast Update : Wed Aug 13 02:10:11 2025
Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
----------	------	------	----------	------	-------	----------

(#) = qualifier out of range (m) = manual integration (+) = signals summed


```
Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY081525\
Data File : VY023114.D
Acq On    : 15 Aug 2025   09:59
Operator  : SY/MD
Sample    : VY0815BSBD01
Misc      : 5.00g/5.0mL/MSVOA_Y/SOIL
ALS Vial  : 5      Sample Multiplier: 1
```

Instrument :
MSVOA_Y
ClientSampleId :
VY0815SBSD01

Manual Integrations APPROVED

Reviewed By :Semsettin Yesilyurt 08/19/2025
Supervised By :Mahesh Dadoda 08/19/2025

Quant Time: Aug 18 02:25:28 2025
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y081225S.M
Quant Title : SW846 8260
QLast Update : Wed Aug 13 02:10:11 2025
Response via : Initial Calibration

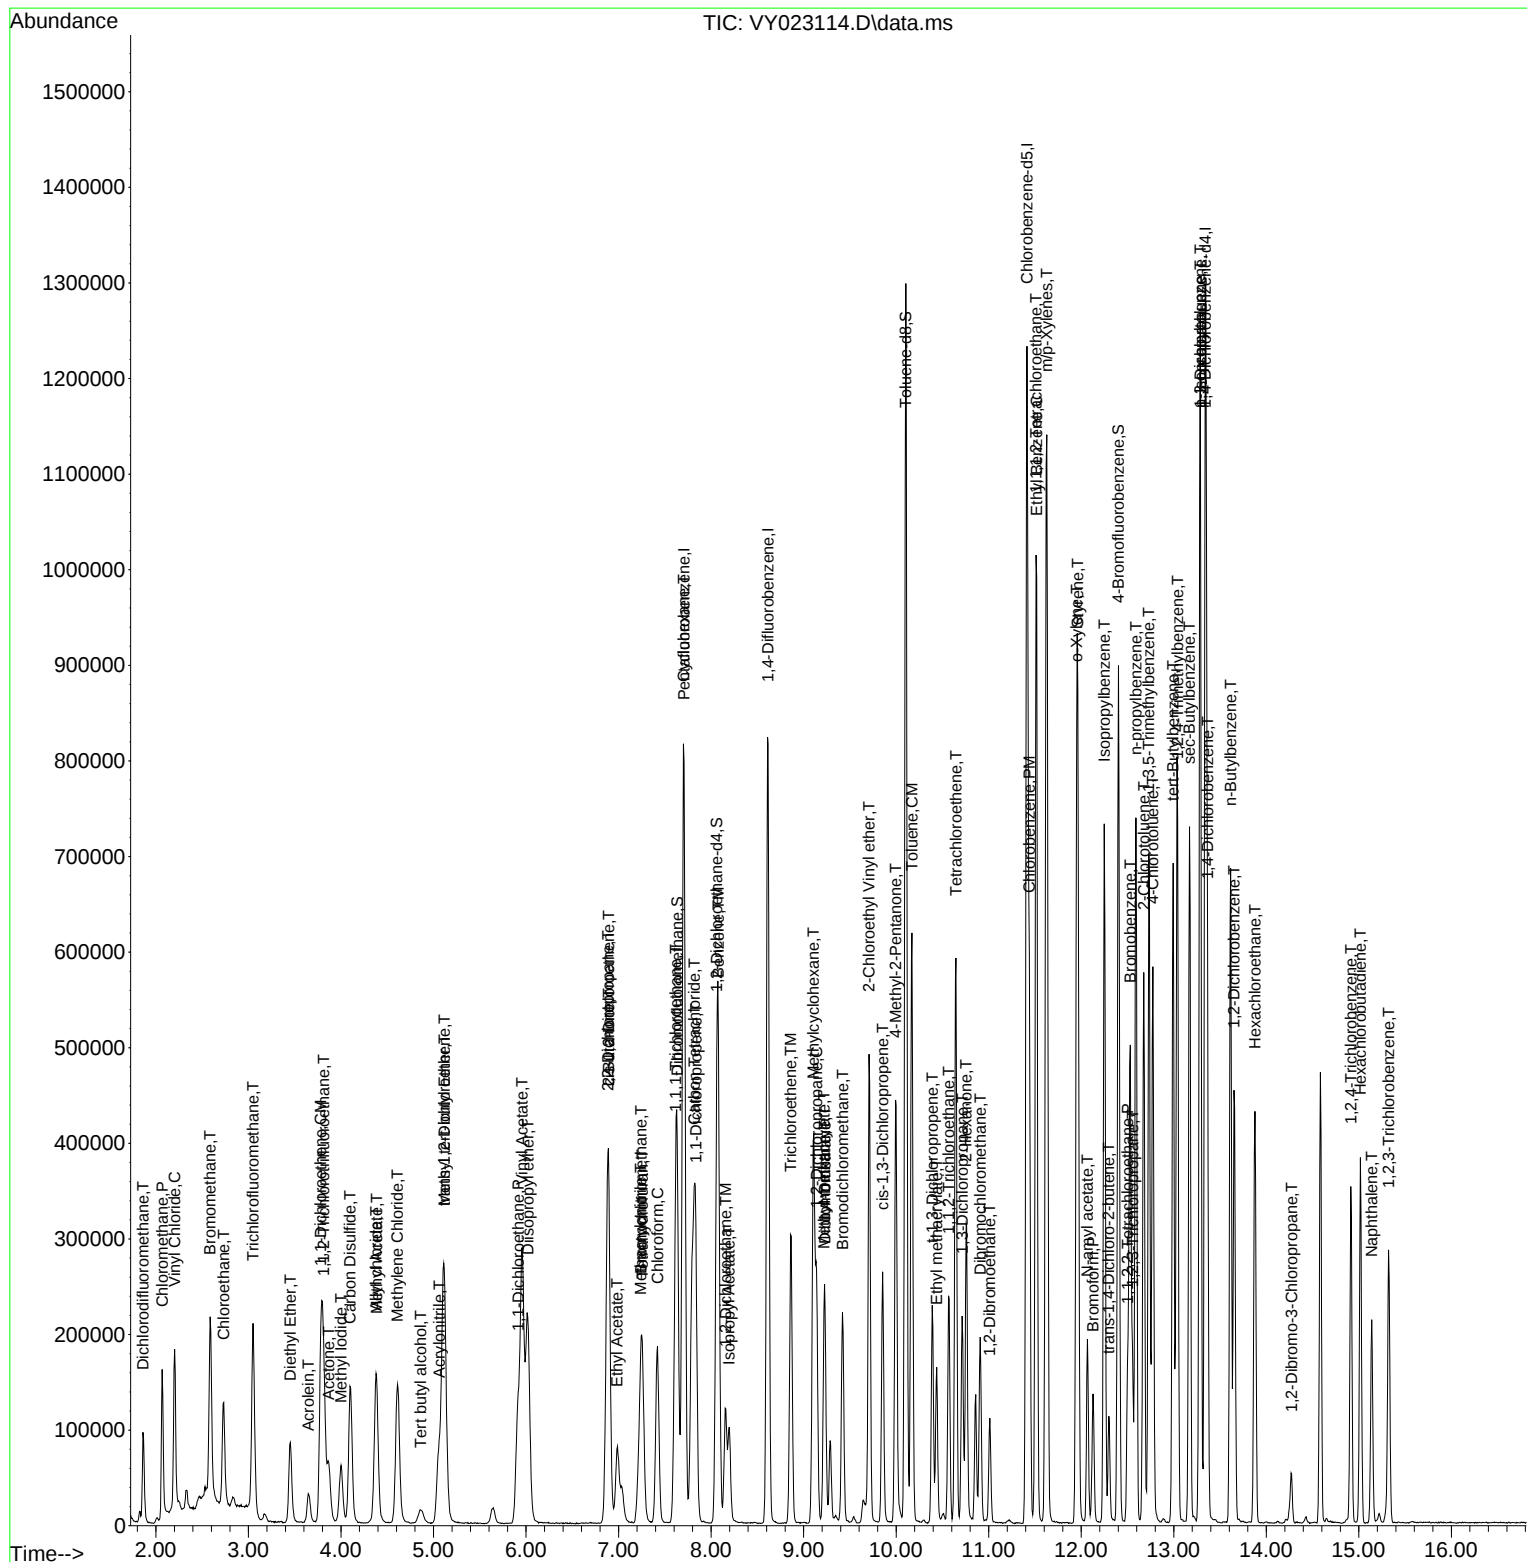

Manual Integration Report

Sequence:	VY081225	Instrument	MSVOA_y
-----------	----------	------------	---------

Sample ID	File ID	Parameter	Review By	Review On	Supervised By	Supervised On	Reason
VSTDICC005	VY023050.D	1,2,3-Trichloropropane	MMDadoda	8/14/2025 7:33:57 PM	SAM	8/14/2025 7:43:56 PM	Peak Integrated by Software
VSTDICC005	VY023050.D	Methacrylonitrile	MMDadoda	8/14/2025 7:33:57 PM	SAM	8/14/2025 7:43:56 PM	Peak Integrated by Software
VSTDICC010	VY023051.D	1,2,3-Trichloropropane	MMDadoda	8/14/2025 7:34:06 PM	SAM	8/14/2025 7:43:57 PM	Peak Integrated by Software
VSTDICC020	VY023052.D	1,2,3-Trichloropropane	MMDadoda	8/14/2025 7:34:08 PM	SAM	8/14/2025 7:43:59 PM	Peak Integrated by Software
VSTDICC020	VY023052.D	Methacrylonitrile	MMDadoda	8/14/2025 7:34:08 PM	SAM	8/14/2025 7:43:59 PM	Peak Integrated by Software
VSTDICCC050	VY023053.D	1,2,3-Trichloropropane	MMDadoda	8/14/2025 7:34:10 PM	SAM	8/14/2025 7:44:00 PM	Peak Integrated by Software
VSTDICC100	VY023054.D	1,2,3-Trichloropropane	MMDadoda	8/14/2025 7:34:12 PM	SAM	8/14/2025 7:44:02 PM	Peak Integrated by Software
VSTDICC150	VY023055.D	1,2,3-Trichloropropane	MMDadoda	8/14/2025 7:34:15 PM	SAM	8/14/2025 7:44:04 PM	Peak Integrated by Software
VSTDICV050	VY023057.D	1,2,3-Trichloropropane	MMDadoda	8/14/2025 7:34:16 PM	SAM	8/14/2025 7:44:06 PM	Peak Integrated by Software

Manual Integration Report

Sequence:	VY081525	Instrument	MSVOA_y
-----------	----------	------------	---------

Sample ID	File ID	Parameter	Review By	Review On	Supervised By	Supervised On	Reason
VSTDCCC050	VY023111.D	1,2,3-Trichloropropane	SAM	8/19/2025 4:19:46 AM	MMDadoda	8/19/2025 4:24:10 AM	Peak Integrated by Software
VSTDCCC050	VY023111.D	Methacrylonitrile	SAM	8/19/2025 4:19:46 AM	MMDadoda	8/19/2025 4:24:10 AM	Peak Integrated by Software
VY0815SBS01	VY023113.D	1,2,3-Trichloropropane	SAM	8/19/2025 4:19:47 AM	MMDadoda	8/19/2025 4:24:11 AM	Peak Integrated by Software
VY0815SBSD0 1	VY023114.D	1,2,3-Trichloropropane	SAM	8/19/2025 4:19:48 AM	MMDadoda	8/19/2025 4:24:12 AM	Peak Integrated by Software
VY0815SBSD0 1	VY023114.D	Methacrylonitrile	SAM	8/19/2025 4:19:48 AM	MMDadoda	8/19/2025 4:24:12 AM	Peak Integrated by Software
VSTDCCC050	VY023135.D	1,2,3-Trichloropropane	SAM	8/19/2025 4:19:49 AM	MMDadoda	8/19/2025 4:24:14 AM	Peak Integrated by Software

Instrument ID: **MSVOA_Y**

Daily Analysis Runlog For Sequence/QCBatch ID # VY081225

Review By	Mahesh Dadoda	Review On	8/14/2025 7:34:22 PM		
Supervise By	Semsettin Yesilyurt	Supervise On	8/14/2025 7:44:13 PM		
SubDirectory	VY081225	HP Acquire Method	MSVOA_Y	HP Processing Method	82y081225s.m
STD. NAME		STD REF.#			
Tune/Reschk		VP135083			
Initial Calibration Stds		VP135084,VP135085,VP135086,VP135087,VP135088,VP135089			
CCC					
Internal Standard/PEM		VP133934			
ICV/I.BLK		VP135090			
Surrogate Standard					
MS/MSD Standard					
LCS Standard					

Sr#	SampleId	Data File Name	Date-Time	Operator	Status
1	BFB	VY023048.D	12 Aug 2025 08:26	SY/MD	Ok
2	VSTDICC005	VY023049.D	12 Aug 2025 14:32	SY/MD	Not Ok
3	VSTDICC005	VY023050.D	12 Aug 2025 14:54	SY/MD	Ok,M
4	VSTDICC010	VY023051.D	12 Aug 2025 15:17	SY/MD	Ok,M
5	VSTDICC020	VY023052.D	12 Aug 2025 15:40	SY/MD	Ok,M
6	VSTDICCC050	VY023053.D	12 Aug 2025 16:02	SY/MD	Ok,M
7	VSTDICC100	VY023054.D	12 Aug 2025 16:25	SY/MD	Ok,M
8	VSTDICC150	VY023055.D	12 Aug 2025 16:47	SY/MD	Ok,M
9	VIBLK	VY023056.D	12 Aug 2025 17:31	SY/MD	Ok
10	VSTDICV050	VY023057.D	12 Aug 2025 17:53	SY/MD	Ok,M

M : Manual Integration

Instrument ID: **MSVOA_Y**

Daily Analysis Runlog For Sequence/QC Batch ID # VY081525

Review By	Semsettin Yesilyurt	Review On	8/19/2025 4:20:36 AM
Supervise By	Maresh Dadoda	Supervise On	8/19/2025 4:24:34 AM
SubDirectory	VY081525	HP Acquire Method	MSVOA_Y
		HP Processing Method	82y081225s.m
STD. NAME	STD REF.#		
Tune/Reschk Initial Calibration Stds	VP135149		
CCC Internal Standard/PEM ICV/I.BLK Surrogate Standard MS/MSD Standard LCS Standard	VP135150,VP135151 VP133934		

Sr#	SampleId	Data File Name	Date-Time	Operator	Status
1	BFB	VY023110.D	15 Aug 2025 08:07	SY/MD	Ok
2	VSTDCCC050	VY023111.D	15 Aug 2025 08:39	SY/MD	Ok,M
3	VY0815SBL01	VY023112.D	15 Aug 2025 09:08	SY/MD	Ok
4	VY0815SBS01	VY023113.D	15 Aug 2025 09:37	SY/MD	Ok,M
5	VY0815SBSD01	VY023114.D	15 Aug 2025 09:59	SY/MD	Ok,M
6	Q2876-01	VY023115.D	15 Aug 2025 10:44	SY/MD	Ok
7	Q2877-01	VY023116.D	15 Aug 2025 11:07	SY/MD	Ok
8	Q2853-01	VY023117.D	15 Aug 2025 11:31	SY/MD	Ok
9	Q2820-21	VY023118.D	15 Aug 2025 11:54	SY/MD	Ok
10	Q2820-22	VY023119.D	15 Aug 2025 12:18	SY/MD	Ok
11	Q2883-01	VY023120.D	15 Aug 2025 12:41	SY/MD	Ok
12	Q2820-23	VY023121.D	15 Aug 2025 13:05	SY/MD	ReRun
13	Q2820-24	VY023122.D	15 Aug 2025 13:28	SY/MD	Ok
14	Q2832-01	VY023123.D	15 Aug 2025 14:24	SY/MD	Ok
15	Q2832-03	VY023124.D	15 Aug 2025 14:47	SY/MD	Ok
16	Q2832-05	VY023125.D	15 Aug 2025 15:11	SY/MD	Ok
17	Q2832-07	VY023126.D	15 Aug 2025 15:34	SY/MD	Ok
18	Q2832-09	VY023127.D	15 Aug 2025 15:58	SY/MD	Ok
19	Q2844-02	VY023128.D	15 Aug 2025 16:21	SY/MD	Ok
20	Q2844-04	VY023129.D	15 Aug 2025 16:45	SY/MD	Ok
21	Q2844-06	VY023130.D	15 Aug 2025 17:08	SY/MD	Ok

Instrument ID: **MSVOA_Y**

Daily Analysis Runlog For Sequence/QCBatch ID # VY081525

Review By	Semsettin Yesilyurt	Review On	8/19/2025 4:20:36 AM		
Supervise By	Mahesh Dadoda	Supervise On	8/19/2025 4:24:34 AM		
SubDirectory	VY081525	HP Acquire Method	MSVOA_Y	HP Processing Method	82y081225s.m
STD. NAME		STD REF.#			
Tune/Reschk Initial Calibration Stds		VP135149			
CCC		VP135150,VP135151			
Internal Standard/PEM		VP133934			
ICV/I.BLK					
Surrogate Standard					
MS/MSD Standard					
LCS Standard					

22	Q2868-02	VY023131.D	15 Aug 2025 17:33	SY/MD	Ok
23	Q2865-01	VY023132.D	15 Aug 2025 17:56	SY/MD	Ok
24	Q2884-01	VY023133.D	15 Aug 2025 18:19	SY/MD	Ok
25	VIBLK	VY023134.D	15 Aug 2025 18:43	SY/MD	Ok
26	VSTDCCC050	VY023135.D	15 Aug 2025 19:06	SY/MD	Ok,M

M : Manual Integration

Instrument ID: MSVOA_Y

Daily Analysis Runlog For Sequence/QC Batch ID # VY081225

Review By	Maresh Dadoda	Review On	8/14/2025 7:34:22 PM
Supervise By	Semsettin Yesilyurt	Supervise On	8/14/2025 7:44:13 PM
SubDirectory	VY081225	HP Acquire Method	MSVOA_Y HP Processing Method 82y081225s.m

STD. NAME	STD REF.#
Tune/Reschk	VP135083
Initial Calibration Stds	VP135084,VP135085,VP135086,VP135087,VP135088,VP135089
CCC	
Internal Standard/PEM	VP133934
ICV/I.BLK	VP135090
Surrogate Standard	
MS/MSD Standard	
LCS Standard	

Sr#	Sampleld	ClientID	Data File Name	Date-Time	Comment	Operator	Status
1	BFB	BFB	VY023048.D	12 Aug 2025 08:26		SY/MD	Ok
2	VSTDICC005	VSTDICC005	VY023049.D	12 Aug 2025 14:32	Not used	SY/MD	Not Ok
3	VSTDICC005	VSTDICC005	VY023050.D	12 Aug 2025 14:54		SY/MD	Ok,M
4	VSTDICC010	VSTDICC010	VY023051.D	12 Aug 2025 15:17		SY/MD	Ok,M
5	VSTDICC020	VSTDICC020	VY023052.D	12 Aug 2025 15:40	LR-20	SY/MD	Ok,M
6	VSTDICCC050	VSTDICCC050	VY023053.D	12 Aug 2025 16:02		SY/MD	Ok,M
7	VSTDICC100	VSTDICC100	VY023054.D	12 Aug 2025 16:25		SY/MD	Ok,M
8	VSTDICC150	VSTDICC150	VY023055.D	12 Aug 2025 16:47		SY/MD	Ok,M
9	VIBLK	VIBLK	VY023056.D	12 Aug 2025 17:31		SY/MD	Ok
10	VSTDICV050	ICVVY081225	VY023057.D	12 Aug 2025 17:53		SY/MD	Ok,M

M : Manual Integration

Instrument ID: MSVOA_Y

Daily Analysis Runlog For Sequence/QC Batch ID # VY081525

Review By	Semsettin Yesilyurt	Review On	8/19/2025 4:20:36 AM		
Supervise By	Mahesh Dadoda	Supervise On	8/19/2025 4:24:34 AM		
SubDirectory	VY081525	HP Acquire Method	MSVOA_Y	HP Processing Method	82y081225s.m

STD. NAME	STD REF.#
Tune/Reschk Initial Calibration Stds	VP135149
CCC Internal Standard/PEM ICV/I.BLK Surrogate Standard MS/MSD Standard LCS Standard	VP135150,VP135151 VP133934

Sr#	SampleID	ClientID	Data File Name	Date-Time	Comment	Operator	Status
1	BFB	BFB	VY023110.D	15 Aug 2025 08:07		SY/MD	Ok
2	VSTDCCC050	VSTDCCC050	VY023111.D	15 Aug 2025 08:39		SY/MD	Ok,M
3	VY0815SBL01	VY0815SBL01	VY023112.D	15 Aug 2025 09:08		SY/MD	Ok
4	VY0815SBS01	VY0815SBS01	VY023113.D	15 Aug 2025 09:37		SY/MD	Ok,M
5	VY0815SBSD01	VY0815SBSD01	VY023114.D	15 Aug 2025 09:59		SY/MD	Ok,M
6	Q2876-01	CL-02-08142025	VY023115.D	15 Aug 2025 10:44	vial-A	SY/MD	Ok
7	Q2877-01	EO-02-08142025	VY023116.D	15 Aug 2025 11:07	vial-A	SY/MD	Ok
8	Q2853-01	TR-05-081325	VY023117.D	15 Aug 2025 11:31	vial-A	SY/MD	Ok
9	Q2820-21	22M-N	VY023118.D	15 Aug 2025 11:54	vial-A	SY/MD	Ok
10	Q2820-22	22M-W	VY023119.D	15 Aug 2025 12:18	vial-A	SY/MD	Ok
11	Q2883-01	RBR2520553	VY023120.D	15 Aug 2025 12:41	vial-A	SY/MD	Ok
12	Q2820-23	22M-E	VY023121.D	15 Aug 2025 13:05	vial-A Surrogate fail	SY/MD	ReRun
13	Q2820-24	22M-S	VY023122.D	15 Aug 2025 13:28	vial-A	SY/MD	Ok
14	Q2832-01	TG-S01	VY023123.D	15 Aug 2025 14:24	vial-A	SY/MD	Ok
15	Q2832-03	TG-S02	VY023124.D	15 Aug 2025 14:47	vial-A	SY/MD	Ok
16	Q2832-05	TG-S03	VY023125.D	15 Aug 2025 15:11	vial-A	SY/MD	Ok
17	Q2832-07	TG-S04	VY023126.D	15 Aug 2025 15:34	vial-A	SY/MD	Ok
18	Q2832-09	TG-S05	VY023127.D	15 Aug 2025 15:58	vial-A	SY/MD	Ok

Instrument ID: MSVOA_Y

Daily Analysis Runlog For Sequence/QC Batch ID # VY081525

Review By	Semsettin Yesilyurt	Review On	8/19/2025 4:20:36 AM		
Supervise By	Mahesh Dadoda	Supervise On	8/19/2025 4:24:34 AM		
SubDirectory	VY081525	HP Acquire Method	MSVOA_Y	HP Processing Method	82y081225s.m
STD. NAME	STD REF.#				
Tune/Reschk Initial Calibration Stds	VP135149				
CCC	VP135150,VP135151				
Internal Standard/PEM	VP133934				
ICV/I.BLK					
Surrogate Standard					
MS/MSD Standard					
LCS Standard					

19	Q2844-02	MOO-25-0224-0225	VY023128.D	15 Aug 2025 16:21	vial-A	SY/MD	Ok
20	Q2844-04	MOO-25-0234-0235	VY023129.D	15 Aug 2025 16:45	vial-A	SY/MD	Ok
21	Q2844-06	MOO-25-0223	VY023130.D	15 Aug 2025 17:08	vial-A	SY/MD	Ok
22	Q2868-02	VOC	VY023131.D	15 Aug 2025 17:33	vial-A	SY/MD	Ok
23	Q2865-01	ARS10-0047-VOC	VY023132.D	15 Aug 2025 17:56	vial-A	SY/MD	Ok
24	Q2884-01	VNJ-232	VY023133.D	15 Aug 2025 18:19	vial-A	SY/MD	Ok
25	VIBLK	VIBLK	VY023134.D	15 Aug 2025 18:43		SY/MD	Ok
26	VSTDCCC050	VSTDCCC050EC	VY023135.D	15 Aug 2025 19:06		SY/MD	Ok,M

M : Manual Integration

PERCENT SOLID

Supervisor: rubina
Analyst: jignesh
Date: 8/15/2025

OVENTEMP IN Celsius(°C): 107
Time IN: 17:25
In Date: 08/14/2025
Weight Check 1.0g: 1.00
Weight Check 10g: 10.00
OvenID: M OVEN#1

OVENTEMP OUT Celsius(°C): 104
Time OUT: 08:25
Out Date: 08/15/2025
Weight Check 1.0g: 1.00
Weight Check 10g: 10.00
BalanceID: M SC-4
Thermometer ID: % SOLID-OVEN

QC:LB136818

Lab ID	Client SampleID	Dish #	Dish Wt (g) (A)	Sample Wt (g)	Dish + Sample Wt (g) (B)	Dish+Dry Sample Wt (g) (C)	% Solid	Comments
Q2844-01	PAD-081325	1	1.14	9.98	11.12	10.42	93.0	
Q2844-02	MOO-25-0224-0225	2	1.14	10.90	12.04	11.08	91.2	
Q2844-04	MOO-25-0234-0235	3	1.19	10.42	11.61	10.82	92.4	
Q2844-06	MOO-25-0223	4	1.12	10.34	11.46	11.12	96.7	
Q2844-09	MOO-25-0226	5	1.00	1.00	2.00	2.00	100.0	debris
Q2844-11	MOO-25-0228	6	1.00	1.00	2.00	2.00	100.0	debris
Q2847-01	BUR-25-0069	7	1.17	10.42	11.59	10.1	85.7	
Q2847-02	BUR-25-0070	8	1.19	10.30	11.49	9.88	84.4	
Q2853-01	Tr-5-081325	9	1.18	10.34	11.52	11.22	97.1	
Q2853-02	Tr-5-081325-E2	10	1.19	10.38	11.57	11.18	96.2	
Q2865-01	ARS10-0047-VOC	44	1.14	10.85	11.99	9.2	74.3	
Q2865-02	ARS10-0047	45	1.15	10.35	11.5	8.23	68.4	
Q2866-01	Tre-2003	11	1.00	1.00	2.00	2.00	100.0	WIPE SAMPLE
Q2866-02	Tre-2004	12	1.00	1.00	2.00	2.00	100.0	WIPE SAMPLE
Q2868-01	WASTE	13	1.14	10.25	11.39	10.7	93.3	
Q2868-02	VOC	14	1.14	10.48	11.62	11.36	97.5	
Q2868-03	1	15	1.17	10.03	11.2	10.47	92.7	
Q2868-04	2	16	1.18	10.41	11.59	10.77	92.1	
Q2868-05	3	17	1.14	10.46	11.6	10.93	93.6	
Q2868-06	4	18	1.14	10.65	11.79	11.26	95.0	
Q2868-07	5	19	1.13	10.27	11.4	11.00	96.1	
Q2870-01	DRIL CUTTING 1-5 COMP	20	1.15	10.84	11.99	10.9	89.9	
Q2870-02	DRIL CUTTING 1-5 COMP-EPH-2	21	1.13	10.81	11.94	10.7	88.5	
Q2870-03	DRIL CUTTING 1-5 COMP-EPH-3	22	1.14	10.84	11.98	10.77	88.8	
Q2870-04	DRIL CUTTING 6-9 COMP	23	1.15	10.31	11.46	10.16	87.4	
Q2870-05	DRIL CUTTING 6-9 COMP-EPH-2	24	1.18	10.22	11.4	10.11	87.4	
Q2870-06	DRIL CUTTING 6-9 COMP-EPH-3	25	1.14	10.30	11.44	10.15	87.5	

PERCENT SOLID

Supervisor: rubina
Analyst: jignesh
Date: 8/15/2025

OVENTEMP IN Celsius(°C): 107
Time IN: 17:25
In Date: 08/14/2025
Weight Check 1.0g: 1.00
Weight Check 10g: 10.00
OvenID: M OVEN#1

OVENTEMP OUT Celsius(°C): 104
Time OUT: 08:25
Out Date: 08/15/2025
Weight Check 1.0g: 1.00
Weight Check 10g: 10.00
BalanceID: M SC-4
Thermometer ID: % SOLID-OVEN

QC:LB136818

Lab ID	Client SampleID	Dish #	Dish Wt (g) (A)	Sample Wt (g)	Dish + Sample Wt (g) (B)	Dish+Dry Sample Wt (g) (C)	% Solid	Comments
Q2871-01	DRIL CUTTING 1-3 COMP	26	1.18	10.39	11.57	9.71	82.1	
Q2871-02	DRIL CUTTING 1-3 -EPH-2	29	1.14	10.46	11.6	9.7	81.8	
Q2871-03	DRIL CUTTING 1-3-EPH3	30	1.18	10.71	11.89	9.72	79.7	
Q2871-04	DRIL CUTTING 4-6 COMP	27	1.19	10.58	11.77	9.81	81.5	
Q2871-05	DRIL CUTTING 4-6-EPH-2	31	1.19	10.55	11.74	9.98	83.3	
Q2871-06	DRIL CUTTING 4-6-EPH-3	32	1.14	10.65	11.79	11.00	92.6	
Q2871-07	DRIL CUTTING 1-5 COMP	28	1.16	10.52	11.68	10.2	85.9	
Q2871-08	DRIL CUTTING 1-5-EPH2	33	1.15	10.45	11.6	10.36	88.1	
Q2871-09	DRIL CUTTING 1-5-EPH3	34	1.16	10.67	11.83	10.55	88.0	
Q2872-01	DRIL CUTTING 1-2 COMP	35	1.14	10.45	11.59	9.9	83.8	
Q2872-02	DRIL CUTTING 1-2-EPH-2	36	1.19	10.22	11.41	9.56	81.9	
Q2872-03	DRIL CUTTING 1-2-EPH-3	37	1.18	10.34	11.52	9.79	83.3	
Q2873-01	DRIL CUTTING 1-3 COMP	38	1.18	10.64	11.82	10.42	86.8	
Q2873-02	DRIL CUTTING 1-3-EPH-2	39	1.14	10.13	11.27	10.04	87.9	
Q2873-03	DRIL CUTTING 1-3-EPH-3	40	1.17	10.62	11.79	10.24	85.4	
Q2873-04	DRIL CUTTING 4-6 COMP	41	1.15	10.33	11.48	10.35	89.1	
Q2873-05	DRIL CUTTING 4-6-EPH-2	42	1.14	10.76	11.9	10.7	88.8	
Q2873-06	DRIL CUTTING 4-6-EPH-3	43	1.11	10.78	11.89	10.68	88.8	
Q2874-01	COMP-1	46	1.00	1.00	2.00	2.00	100.0	debris
Q2874-02	ELI-25-0086	47	1.14	10.80	11.94	7.99	63.4	
Q2874-03	ELI-HQ-CONCRETE	48	1.14	10.43	11.57	10.92	93.8	
Q2875-01	SAND-BLAST-A	49	1.18	10.49	11.67	11.66	99.9	
Q2875-02	SAND-BLAST-B	50	1.19	10.50	11.69	11.66	99.7	
Q2876-01	CL-02-08142025	51	1.14	10.50	11.64	11.00	93.9	
Q2876-02	CL-02-08142025-E2	52	1.19	10.34	11.53	11.3	97.8	
Q2877-01	EO-02-08142025	53	1.14	10.76	11.9	11.36	95.0	
Q2877-02	EO-02-08142025-E2	54	1.12	10.50	11.62	11.17	95.7	

$$\% \text{ Solid} = \frac{(C-A) * 100}{(B-A)}$$

WORKLIST(Hardcopy Internal Chain)

8/13/25

WorkList Name : %1-081425

WorkList ID : 191267

Department : Wet-Chemistry

Date : 08-14-2025 08:39:26

Sample	Customer Sample	Matrix	Test	Preservative	Customer	Raw Sample Storage Location	Collect Date	Method
Q2844-01	PAD-081325	Solid	Percent Solids	Cool 4 deg C	PSEG03	J13	08/13/2025	Chemtech -SO
Q2844-02	MOO-25-0224-0225	Solid	Percent Solids	Cool 4 deg C	PSEG03	J13	08/13/2025	Chemtech -SO
Q2844-04	MOO-25-0234-0235	Solid	Percent Solids	Cool 4 deg C	PSEG03	J13	08/13/2025	Chemtech -SO
Q2844-06	MOO-25-0223	Solid	Percent Solids	Cool 4 deg C	PSEG03	J13	08/13/2025	Chemtech -SO
Q2844-09	MOO-25-0226	Solid	Percent Solids	Cool 4 deg C	PSEG03	J13	08/13/2025	Chemtech -SO
Q2844-11	MOO-25-0228	Solid	Percent Solids	Cool 4 deg C	PSEG03	J13	08/13/2025	Chemtech -SO
Q2847-01	BUR-25-0069	Solid	Percent Solids	Cool 4 deg C	PSEG03	J13	08/13/2025	Chemtech -SO
Q2847-02	BUR-25-0070	Solid	Percent Solids	Cool 4 deg C	PSEG03	J41	08/13/2025	Chemtech -SO
Q2853-01	Tr-5-081325	Solid	Percent Solids	Cool 4 deg C	PSEG03	J41	08/13/2025	Chemtech -SO
Q2853-02	Tr-5-081325-E2	Solid	Percent Solids	Cool 4 deg C	PSEG05	J33	08/13/2025	Chemtech -SO
Q2865-01	ARS10-0047-VOC	Solid	Percent Solids	Cool 4 deg C	PSEG05	J33	08/13/2025	Chemtech -SO
Q2865-02	ARS10-0047	Solid	Percent Solids	Cool 4 deg C	PSEG03	J41	08/13/2025	Chemtech -SO
Q2866-01	Tre-2003	Solid	Percent Solids	Cool 4 deg C	PSEG03	J41	08/13/2025	Chemtech -SO
Q2866-02	Tre-2004	Solid	Percent Solids	Cool 4 deg C	PSEG05	J11	08/13/2025	Chemtech -SO
Q2868-01	WASTE	Solid	Percent Solids	Cool 4 deg C	PSEG05	J11	08/13/2025	Chemtech -SO
Q2868-02	VOC	Solid	Percent Solids	Cool 4 deg C	SCIA01	J23	08/12/2025	Chemtech -SO
Q2868-03	1	Solid	Percent Solids	Cool 4 deg C	SCIA01	J23	08/12/2025	Chemtech -SO
Q2868-04	2	Solid	Percent Solids	Cool 4 deg C	SCIA01	J23	08/12/2025	Chemtech -SO
Q2868-05	3	Solid	Percent Solids	Cool 4 deg C	SCIA01	J23	08/12/2025	Chemtech -SO
Q2868-06	4	Solid	Percent Solids	Cool 4 deg C	SCIA01	J23	08/12/2025	Chemtech -SO
Q2868-07	5	Solid	Percent Solids	Cool 4 deg C	SCIA01	J23	08/12/2025	Chemtech -SO

Date/Time 08/14/25 15:00

Raw Sample Received by: [Signature]

Raw Sample Relinquished by: [Signature]

Date/Time 08/14/25 17:35

Raw Sample Received by: [Signature]

Raw Sample Relinquished by: [Signature]

WORKLIST(Hardcopy Internal Chain)

8196818

WorkList Name : %1-081425

WorkList ID : 191267

Department : Wet-Chemistry

Date : 08-14-2025 08:39:26

Sample	Customer Sample	Matrix	Test	Preservative	Customer	Raw Sample Storage Location	Collect Date	Method
Q2870-01	DRIL CUTTING 1-5 COMP	Solid	Percent Solids	Cool 4 deg C	PSEG03	J22	08/13/2025	Chemtech -SO
Q2870-02	DRIL CUTTING 1-5 COMP-EPT	Solid	Percent Solids	Cool 4 deg C	PSEG03	J22	08/13/2025	Chemtech -SO
Q2870-03	DRIL CUTTING 1-5 COMP-EPT	Solid	Percent Solids	Cool 4 deg C	PSEG03	J22	08/13/2025	Chemtech -SO
Q2870-04	DRIL CUTTING 6-9 COMP	Solid	Percent Solids	Cool 4 deg C	PSEG03	J22	08/13/2025	Chemtech -SO
Q2870-05	DRIL CUTTING 6-9 COMP-EPT	Solid	Percent Solids	Cool 4 deg C	PSEG03	J22	08/13/2025	Chemtech -SO
Q2870-06	DRIL CUTTING 6-9 COMP-EPT	Solid	Percent Solids	Cool 4 deg C	PSEG03	J22	08/13/2025	Chemtech -SO
Q2871-01	DRIL CUTTING 1-3 COMP	Solid	Percent Solids	Cool 4 deg C	PSEG03	J22	08/13/2025	Chemtech -SO
Q2871-02	DRIL CUTTING 1-3 -EPH-2	Solid	Percent Solids	Cool 4 deg C	PSEG03	J33	08/13/2025	Chemtech -SO
Q2871-03	DRIL CUTTING 1-3-EPH3	Solid	Percent Solids	Cool 4 deg C	PSEG03	J31	08/13/2025	Chemtech -SO
Q2871-04	DRIL CUTTING 4-6 COMP	Solid	Percent Solids	Cool 4 deg C	PSEG03	J31	08/13/2025	Chemtech -SO
Q2871-05	DRIL CUTTING 4-6-EPH-2	Solid	Percent Solids	Cool 4 deg C	PSEG03	J33	08/13/2025	Chemtech -SO
Q2871-06	DRIL CUTTING 4-6-EPH-3	Solid	Percent Solids	Cool 4 deg C	PSEG03	J31	08/13/2025	Chemtech -SO
Q2871-07	DRIL CUTTING 1-5 COMP	Solid	Percent Solids	Cool 4 deg C	PSEG03	J31	08/13/2025	Chemtech -SO
Q2871-08	DRIL CUTTING 1-5-EPH2	Solid	Percent Solids	Cool 4 deg C	PSEG03	J33	08/13/2025	Chemtech -SO
Q2871-09	DRIL CUTTING 1-5-EPH3	Solid	Percent Solids	Cool 4 deg C	PSEG03	J31	08/13/2025	Chemtech -SO
Q2872-01	DRIL CUTTING 1-2 COMP	Solid	Percent Solids	Cool 4 deg C	PSEG03	J31	08/13/2025	Chemtech -SO
Q2872-02	DRIL CUTTING 1-2-EPH-2	Solid	Percent Solids	Cool 4 deg C	PSEG03	J33	08/13/2025	Chemtech -SO
Q2872-03	DRIL CUTTING 1-2-EPH-3	Solid	Percent Solids	Cool 4 deg C	PSEG03	J33	08/13/2025	Chemtech -SO
Q2873-01	DRIL CUTTING 1-3 COMP	Solid	Percent Solids	Cool 4 deg C	PSEG03	J32	08/13/2025	Chemtech -SO
Q2873-02	DRIL CUTTING 1-3-EPH-2	Solid	Percent Solids	Cool 4 deg C	PSEG03	J32	08/13/2025	Chemtech -SO
Q2873-03	DRIL CUTTING 1-3-EPH-3	Solid	Percent Solids	Cool 4 deg C	PSEG03	J32	08/13/2025	Chemtech -SO

Date/Time 08-14-25 05:00
 Raw Sample Received by: [Signature]
 Raw Sample Relinquished by: [Signature]

Date/Time 08-14-25 17:35
 Raw Sample Received by: [Signature]
 Raw Sample Relinquished by: [Signature]

WORKLIST(Hardcopy Internal Chain)

87126818

WorkList Name : %1-081425 WorkList ID : 191267 Department : Wet-Chemistry Date : 08-14-2025 08:39:26

Sample	Customer Sample	Matrix	Test	Preservative	Customer	Raw Sample Storage Location	Collect Date	Method
Q2873-04	DRIL CUTTING 4-6 COMP	Solid	Percent Solids	Cool 4 deg C	PSEG03	J32	08/13/2025	Chemtech -SO
Q2873-05	DRIL CUTTING 4-6-EPH-2	Solid	Percent Solids	Cool 4 deg C	PSEG03	J32	08/13/2025	Chemtech -SO
Q2873-06	DRIL CUTTING 4-6-EPH-3	Solid	Percent Solids	Cool 4 deg C	PSEG03	J32	08/13/2025	Chemtech -SO
Q2874-01	COMP-1	Solid	Percent Solids	Cool 4 deg C	PSEG03	D31	08/14/2025	Chemtech -SO
Q2874-02	ELI-25-0086	Solid	Percent Solids	Cool 4 deg C	PSEG03	D31	08/14/2025	Chemtech -SO
Q2874-03	ELI-HQ-CONCRETE	Solid	Percent Solids	Cool 4 deg C	PSEG03	D31	08/14/2025	Chemtech -SO
Q2875-01	SAND-BLAST-A	Solid	Percent Solids	Cool 4 deg C	PSEG03	D21	08/14/2025	Chemtech -SO
Q2875-02	SAND-BLAST-B	Solid	Percent Solids	Cool 4 deg C	PSEG03	D21	08/14/2025	Chemtech -SO
Q2876-01	CL-02-08142025	Solid	Percent Solids	Cool 4 deg C	PSEG05	D31	08/14/2025	Chemtech -SO
Q2876-02	CL-02-08142025-E2	Solid	Percent Solids	Cool 4 deg C	PSEG05	D31	08/14/2025	Chemtech -SO
Q2877-01	EO-02-08142025	Solid	Percent Solids	Cool 4 deg C	PSEG05	D31	08/14/2025	Chemtech -SO
Q2877-02	EO-02-08142025-E2	Solid	Percent Solids	Cool 4 deg C	PSEG05	D31	08/14/2025	Chemtech -SO

Date/Time 08-14-25 15:00
 Raw Sample Received by: SP WWC
 Raw Sample Relinquished by: Am SM

Date/Time 08-14-25 17:35
 Raw Sample Received by: Am SM
 Raw Sample Relinquished by: SP WWC



SHIPPING DOCUMENTS

2 2868

507 Franklin Ave

CHEMTECH

CHAIN OF CUSTODY RECORD

284 Sheffield Street, Mountainside, NJ 07092
(908) 789-8900 Fax (908) 789-8922
www.chemtech.net

Chemtech Project Number N-111
COC Number

CLIENT INFORMATION			PROJECT INFORMATION		BILLING INFORMATION	
Report to be sent to:			PROJECT NAME:		BILL TO:	
COMPANY:			PROJECT #:		PO#:	
ADDRESS:			LOCATION:		ADDRESS:	
CITY:			PROJECT MANAGER:		CITY:	
STATE:			E-MAIL:		STATE:	
ZIP:			PHONE:		ZIP:	
ATTENTION:			FAX:		ATTENTION:	
PHONE:					PHONE:	

DATA TURNAROUND INFORMATION		DATA DELIVERABLE INFORMATION		ANALYSIS	
FAX (RUSH):	DAYS*	☐ Level 1 (Results Only)	☐ Level 4 (QC + Full Raw Data)		
HARDCOPY (DATA PACKAGE):	DAYS*	☐ Level 2 (Results + QC)	☐ NJ Reduced ☐ US EPA CLP		
EDD:	DAYS*	☐ Level 3 (Results + QC + Raw Data)	☐ NYS ASP A ☐ NYS ASP B		
*TO BE APPROVED BY CHEMTECH		☐ EDD FORMAT	☐ Other		
STANDARD HARDCOPY TURNAROUND TIME IS 10 BUSINESS DAYS					

CHEMTECH SAMPLE ID	PROJECT SAMPLE IDENTIFICATION	SAMPLE MATRIX	SAMPLE TYPE		SAMPLE COLLECTION		# of Bottles	PRESERVATIVES									COMMENTS ← Specify Preservatives A-HCl D-NaOH B-HNO3 E-ICE C-H2SO4 F-OTHER
			COMB	GRAS	DATE	TIME		1	2	3	4	5	6	7	8	9	
1.	WASTE				8-11-25	7:15	1	X									
2.	VOC				8-11-25	8:15	1		X								
3.	1				8-11-25	2:30	1			X							
4.	2				8-11-25	10:15	1			X							
5.	3				8-11-25	9:30	1			X							
6.	4				8-11-25	10:15	1			X							
7.	5				8-11-25	9:15	1			X							
8.																	
9.																	
10.																	

SAMPLE CUSTODY MUST BE DOCUMENTED BELOW EACH TIME SAMPLES CHANGE PROSESSION INCLUDING COURIER DELIVERY

RELINQUISHED BY SAMPLER	DATE/TIME 8-13-25	RECEIVED BY 1428	Conditions of bottles or collars at receipt: ☐ COMPLIANT ☐ NON COMPLIANT ☐ COOLER TEMP 3.8°
1.		1.	Comments:
RELINQUISHED BY	DATE/TIME	RECEIVED BY	
2.		2.	
RELINQUISHED BY	DATE/TIME 8-13-25	RECEIVED FOR LAB BY	CLIENT: ☐ Hand Delivered ☐ Other: _____
3.		3.	CHEMTECH: ☐ Picked Up
Page ____ of ____			Shipment Complete ☐ YES ☐ NO

WHITE - CHEMTECH COPY FOR RETURN TO CLIENT

YELLOW - CHEMTECH COPY

PINK - SAMPLER COPY

Laboratory Certification

Certified By	License No.
CAS EPA CLP Contract	68HERH20D0011
Connecticut	PH-0830
DOD ELAP (ANAB)	L2219
Maine	2024021
Maryland	296
New Hampshire	255424 Rev 1
New Jersey	20012
New York	11376
Pennsylvania	68-00548
Soil Permit	525-24-234-08441
Texas	TX-C25-00189
Virginia	460312

LOGIN REPORT/SAMPLE TRANSFER

Order ID : Q2868 SCIA01

Order Date : 8/14/2025 9:08:00 AM

Project Mgr :

Client Name : Sciacca General Contractor

Project Name : 11 Newman Ave Nutley

Report Type : Results Only

Client Contact : Rosanne Scirica

Receive DateTime : 8/13/2025 6:18:00 PM

EDD Type : EXCEL NJCLEANUP

Invoice Name : Sciacca General Contractor

Purchase Order :

Hard Copy Date :

Invoice Contact : Rosanne Scirica

Date Signoff :

LAB ID	CLIENT ID	MATRIX	SAMPLE DATE	SAMPLE TIME	TEST	TEST GROUP	METHOD	FAX DATE	DUE DATES
Q2868-02	VOC	Solid	08/12/2025	08:00	VOC-TCLVOA-10		8260D		10 Bus. Days

Relinquished By : 

Date / Time : 8/14/25 0930

Received By : 

Date / Time : 8/14/25 9:30

Storage Area : VOA Refridgerator Room

1286
C22