


Ident	Instrument IC-1			Analyst: NF		Method: 300.0 / 9056A		Initial Analyst		
	Con F-	Con CL-	Con NO2	Con BR-	Con NO3	Con HPO4	Con SO4			
STD1	0.000	0.000	0.000	0.000	0.000	0.000	0.000	IC1-080625	8/6/2025 10:18	10 RM/IZ
STD2	0.413	0.620	0.623	2.052	0.515	1.033	3.185	IC1-080625	8/6/2025 10:40	10 RM/IZ
STD3	0.794	1.184	1.185	3.953	0.990	2.067	5.931	IC1-080625	8/6/2025 11:01	10 RM/IZ
STD4	1.023	1.524	1.519	5.070	1.270	2.633	7.597	IC1-080625	8/6/2025 11:23	10 RM/IZ
STD5	1.972	2.981	2.982	9.960	2.483	4.695	14.838	IC1-080625	8/6/2025 11:44	10 RM/IZ
STD6	3.956	5.938	5.934	19.801	4.945	9.953	29.505	IC1-080625	8/6/2025 12:06	10 RM/IZ
STD7	5.041	7.553	7.556	25.165	6.298	12.620	37.443	IC1-080625	8/6/2025 12:27	10 RM/IZ
ICV	2.038	3.184	3.095	10.343	2.641	4.970	15.425	IC1-080625	8/6/2025 12:48	10 RM/IZ
ICB	0.000	0.000	0.000	0.000	0.000	0.000	0.000	IC1-080625	8/6/2025 13:10	10 RM/IZ
CCV	2.021	3.053	3.018	10.168	2.534	4.968	15.164	IC1-080625	8/15/2025 8:46	10 RM/IZ
CCB	0.000	0.000	0.000	0.000	0.000	0.000	0.000	IC1-080625	8/15/2025 9:07	10 RM/IZ
LB136833BLW	0.000	0.000	0.000	0.000	0.000	0.000	0.000	IC1-080625	8/15/2025 9:29	10 RM/IZ
LB136833BSW	2.033	3.052	3.022	10.177	2.541	5.126	15.268	IC1-080625	8/15/2025 9:50	10 RM/IZ
Q2869-01	0.231	39.025	0.000	0.216	0.000	0.000	211.494	IC1-080625	8/15/2025 10:12	10 RM/IZ
Q2869-05	0.234	40.693	0.000	0.109	0.062	0.000	207.570	IC1-080625	8/15/2025 10:55	10 RM/IZ
Q2869-07	0.075	0.128	0.000	0.000	0.000	0.000	0.000	IC1-080625	8/15/2025 11:59	10 RM/IZ
Q2878-01	0.228	18.953	0.000	0.210	0.000	0.000	156.413	IC1-080625	8/15/2025 12:42	10 RM/IZ
Q2878-01MS	2.340	21.563	3.101	10.537	2.620	8.338	167.938	IC1-080625	8/15/2025 13:04	10 RM/IZ
Q2878-01MSD	2.226	21.384	2.987	10.170	2.517	6.798	167.708	IC1-080625	8/15/2025 13:25	10 RM/IZ
Q2869-01DLX10	0.054	3.573	0.000	0.000	0.000	0.000	18.153	IC1-080625	8/15/2025 13:47	10 RM/IZ
Q2869-05DLX10	0.052	3.563	0.000	0.000	0.000	0.000	17.746	IC1-080625	8/15/2025 14:08	10 RM/IZ
CCV	2.003	3.054	3.031	10.190	2.542	4.578	15.227	IC1-080625	8/15/2025 14:30	10 RM/IZ
CCB	0.000	0.000	0.000	0.000	0.000	0.000	0.000	IC1-080625	8/15/2025 14:51	10 RM/IZ
Q2878-01DLX10	0.250	2.136	0.334	1.109	0.289	0.422	14.847	IC1-080625	8/15/2025 15:13	10 RM/IZ
CCV	2.032	3.057	3.021	10.173	2.542	5.193	15.147	IC1-080625	8/15/2025 15:56	10 RM/IZ
CCB	0.000	0.000	0.000	0.000	0.000	0.000	0.000	IC1-080625	8/15/2025 16:17	10 RM/IZ

Fluoride (Anions)

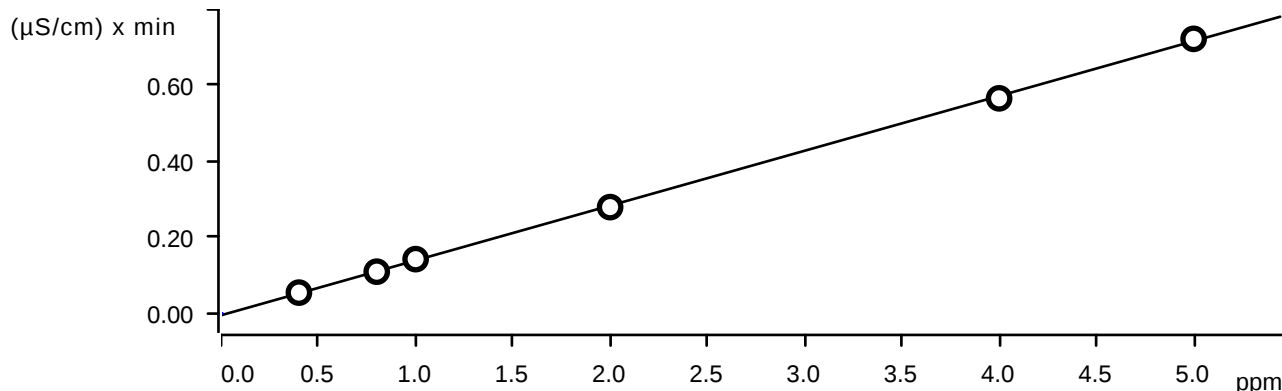


Function: $A = -5.18233\text{E-}3 + 0.0144368 \times Q$

Relative standard deviation 1.650446 %

Correlation coefficient 0.999856

Sample type	Index	Conc.	Volume	Dilution	Sample amount	Area	Ident	Date	Used
Standard 1	1	0.000	10.0	1.0	1.0	n. d.	STD1	2025-08-06 10:18:54 UTC-4	used
Standard 2	1	0.400	10.0	1.0	1.0	0.054	STD2	2025-08-06 10:40:18 UTC-4	used
Standard 3	1	0.800	10.0	1.0	1.0	0.110	STD3	2025-08-06 11:01:42 UTC-4	used
Standard 4	1	1.000	10.0	1.0	1.0	0.143	STD4	2025-08-06 11:23:08 UTC-4	used
Standard 5	1	2.000	10.0	1.0	1.0	0.280	STD5	2025-08-06 11:44:33 UTC-4	used
Standard 6	1	4.000	10.0	1.0	1.0	0.566	STD6	2025-08-06 12:06:00 UTC-4	used
Standard 7	1	5.000	10.0	1.0	1.0	0.723	STD7	2025-08-06 12:27:27 UTC-4	used

Chloride (Anions)

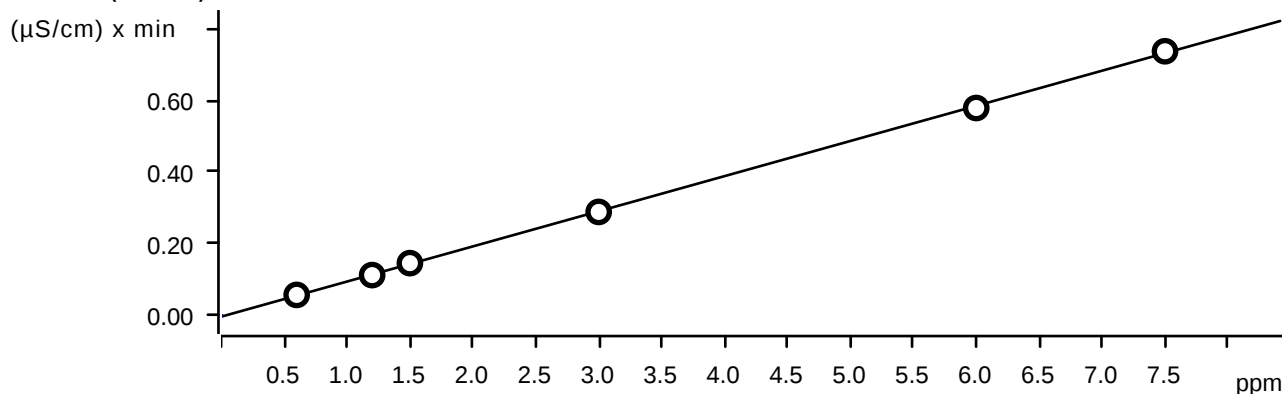

Function: $A = -3.45407\text{E-}3 + 9.79772\text{E-}3 \times Q$


Relative standard deviation 1.384132 %

Correlation coefficient 0.999898

Sample type	Index	Conc.	Volume	Dilution	Sample amount	Area	Ident	Date	Used
Standard 1	1	0.000	10.0	1.0	1.0	n. d.	STD1	2025-08-06 10:18:54 UTC-4	used
Standard 2	1	0.600	10.0	1.0	1.0	0.057	STD2	2025-08-06 10:40:18 UTC-4	used
Standard 3	1	1.200	10.0	1.0	1.0	0.113	STD3	2025-08-06 11:01:42 UTC-4	used
Standard 4	1	1.500	10.0	1.0	1.0	0.146	STD4	2025-08-06 11:23:08 UTC-4	used
Standard 5	1	3.000	10.0	1.0	1.0	0.289	STD5	2025-08-06 11:44:33 UTC-4	used
Standard 6	1	6.000	10.0	1.0	1.0	0.578	STD6	2025-08-06 12:06:00 UTC-4	used
Standard 7	1	7.500	10.0	1.0	1.0	0.737	STD7	2025-08-06 12:27:27 UTC-4	used

Nitrite (Anions)

(μS/cm) x min

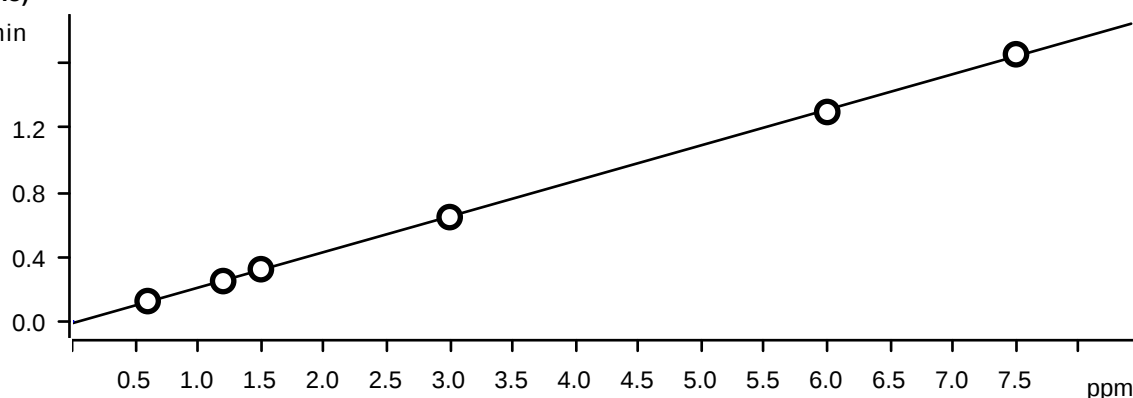Function: $A = -0.0116303 + 0.0220561 \times Q$


Relative standard deviation 1.449488 %

Correlation coefficient 0.999889

Sample type	Index	Conc.	Volume	Dilution	Sample amount	Area	Ident	Date	Used
Standard 1	1	0.000	10.0	1.0	1.0	n. d.	STD1	2025-08-06 10:18:54 UTC-4	used
Standard 2	1	0.600	10.0	1.0	1.0	0.126	STD2	2025-08-06 10:40:18 UTC-4	used
Standard 3	1	1.200	10.0	1.0	1.0	0.250	STD3	2025-08-06 11:01:42 UTC-4	used
Standard 4	1	1.500	10.0	1.0	1.0	0.323	STD4	2025-08-06 11:23:08 UTC-4	used
Standard 5	1	3.000	10.0	1.0	1.0	0.646	STD5	2025-08-06 11:44:33 UTC-4	used
Standard 6	1	6.000	10.0	1.0	1.0	1.297	STD6	2025-08-06 12:06:00 UTC-4	used
Standard 7	1	7.500	10.0	1.0	1.0	1.655	STD7	2025-08-06 12:27:27 UTC-4	used

Bromide (Anions)

($\mu\text{S}/\text{cm}$) $\times$ min

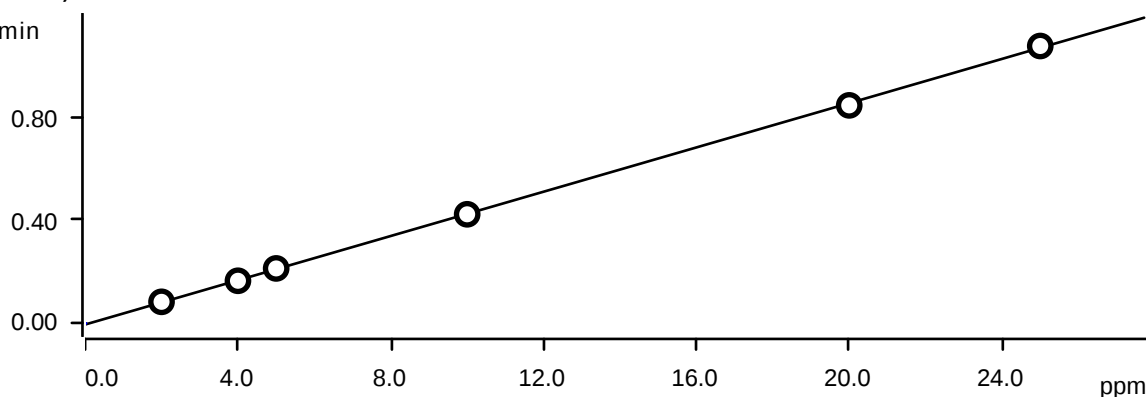

Function: $A = -4.59233\text{E-}3 + 4.28617\text{E-}3 \times Q$


Relative standard deviation: 1.283698 %

Correlation coefficient: 0.999912

Sample type	Index	Conc.	Volume	Dilution	Sample amount	Area	Ident	Date	Used
Standard 1	1	0.000	10.0	1.0	1.0	n. d.	STD1	2025-08-06 10:18:54 UTC-4	used
Standard 2	1	2.000	10.0	1.0	1.0	0.083	STD2	2025-08-06 10:40:18 UTC-4	used
Standard 3	1	4.000	10.0	1.0	1.0	0.165	STD3	2025-08-06 11:01:42 UTC-4	used
Standard 4	1	5.000	10.0	1.0	1.0	0.213	STD4	2025-08-06 11:23:08 UTC-4	used
Standard 5	1	10.000	10.0	1.0	1.0	0.422	STD5	2025-08-06 11:44:33 UTC-4	used
Standard 6	1	20.000	10.0	1.0	1.0	0.844	STD6	2025-08-06 12:06:00 UTC-4	used
Standard 7	1	25.000	10.0	1.0	1.0	1.074	STD7	2025-08-06 12:27:27 UTC-4	used

Nitrate (Anions)

($\mu\text{S}/\text{cm}$) $\times$ min

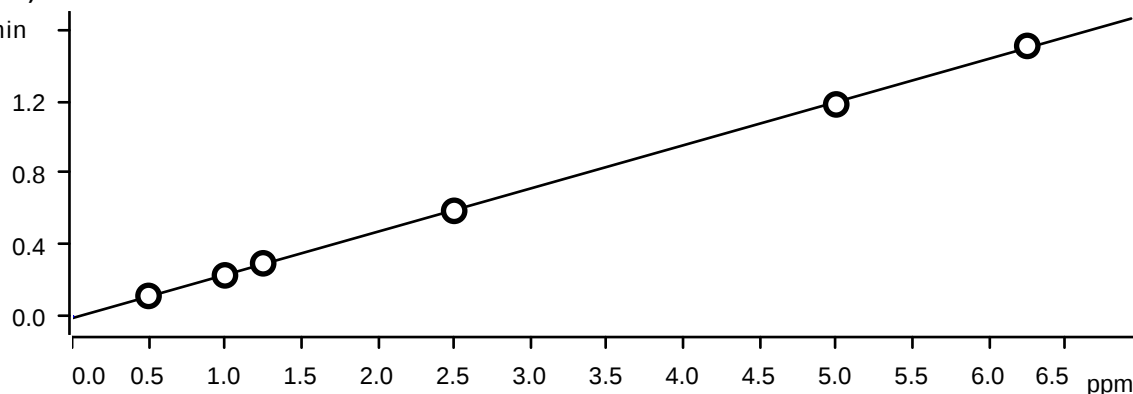

Function: $A = -9.68516\text{E-}3 + 0.0241085 \times Q$


Relative standard deviation: 1.469135 %

Correlation coefficient 0.999886

Sample type	Index	Conc.	Volume	Dilution	Sample amount	Area	Ident	Date	Used
Standard 1	1	0.000	10.0	1.0	1.0	n. d.	STD1	2025-08-06 10:18:54 UTC-4	used
Standard 2	1	0.500	10.0	1.0	1.0	0.115	STD2	2025-08-06 10:40:18 UTC-4	used
Standard 3	1	1.000	10.0	1.0	1.0	0.229	STD3	2025-08-06 11:01:42 UTC-4	used
Standard 4	1	1.250	10.0	1.0	1.0	0.296	STD4	2025-08-06 11:23:08 UTC-4	used
Standard 5	1	2.500	10.0	1.0	1.0	0.589	STD5	2025-08-06 11:44:33 UTC-4	used
Standard 6	1	5.000	10.0	1.0	1.0	1.182	STD6	2025-08-06 12:06:00 UTC-4	used
Standard 7	1	6.250	10.0	1.0	1.0	1.509	STD7	2025-08-06 12:27:27 UTC-4	used

Phosphate (Anions)

(μS/cm) x min

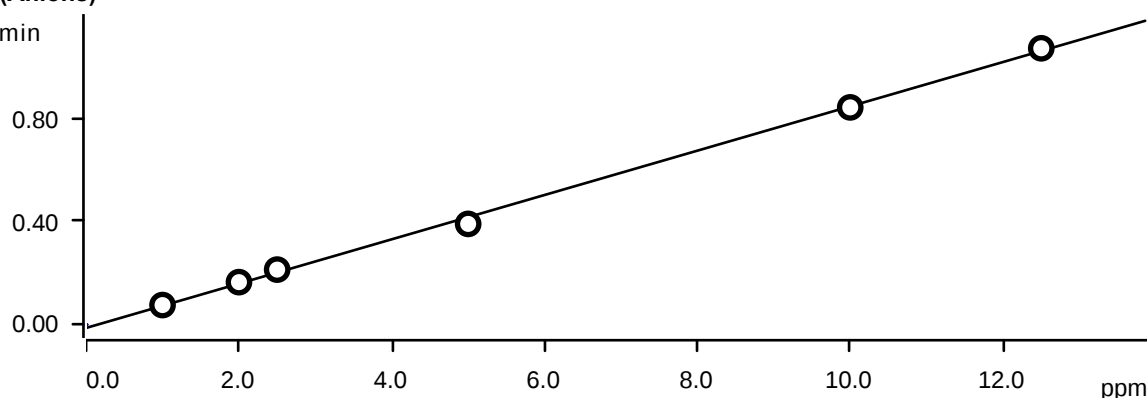
Function: $A = -0.0128563 + 8.58091E-3 \times Q$

Relative standard deviation 3.406332 %

Correlation coefficient 0.999402

Sample type	Index	Conc.	Volume	Dilution	Sample amount	Area	Ident	Date	Used
Standard 1	1	0.000	10.0	1.0	1.0	n. d.	STD1	2025-08-06 10:18:54 UTC-4	used
Standard 2	1	1.000	10.0	1.0	1.0	0.076	STD2	2025-08-06 10:40:18 UTC-4	used
Standard 3	1	2.000	10.0	1.0	1.0	0.164	STD3	2025-08-06 11:01:42 UTC-4	used
Standard 4	1	2.500	10.0	1.0	1.0	0.213	STD4	2025-08-06 11:23:08 UTC-4	used
Standard 5	1	5.000	10.0	1.0	1.0	0.390	STD5	2025-08-06 11:44:33 UTC-4	used
Standard 6	1	10.000	10.0	1.0	1.0	0.841	STD6	2025-08-06 12:06:00 UTC-4	used
Standard 7	1	12.500	10.0	1.0	1.0	1.070	STD7	2025-08-06 12:27:27 UTC-4	used

Sulfate (Anions)

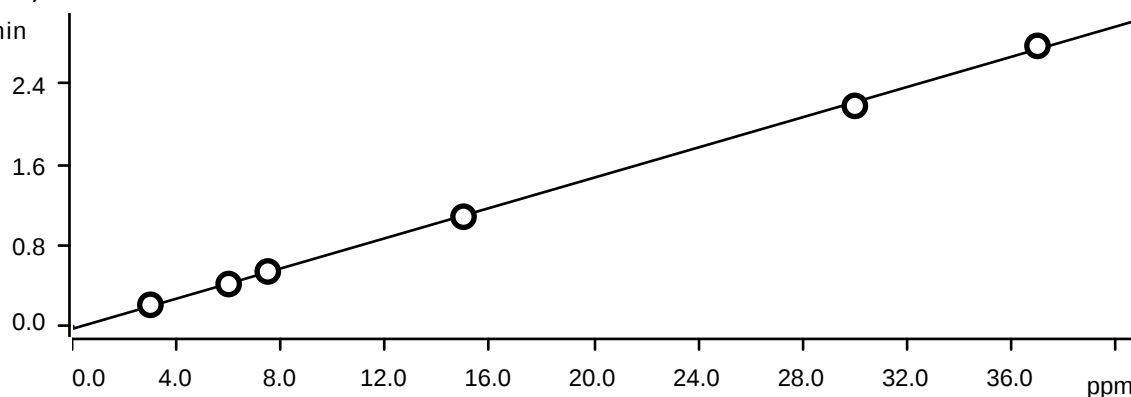 $(\mu\text{S}/\text{cm}) \times \text{min}$ Function: $A = -0.0267558 + 7.49232E-3 \times Q$

Relative standard deviation 2.236460 %

Correlation coefficient 0.999736


Sample type	Index	Conc.	Volume	Dilution	Sample amount	Area	Ident	Date	Used
Standard 1	1	0.000	10.0	1.0	1.0	n. d.	STD1	2025-08-06 10:18:54 UTC-4	used
Standard 2	1	3.000	10.0	1.0	1.0	0.212	STD2	2025-08-06 10:40:18 UTC-4	used
Standard 3	1	6.000	10.0	1.0	1.0	0.418	STD3	2025-08-06 11:01:42 UTC-4	used
Standard 4	1	7.500	10.0	1.0	1.0	0.542	STD4	2025-08-06 11:23:08 UTC-4	used
Standard 5	1	15.000	10.0	1.0	1.0	1.085	STD5	2025-08-06 11:44:33 UTC-4	used
Standard 6	1	30.000	10.0	1.0	1.0	2.184	STD6	2025-08-06 12:06:00 UTC-4	used
Standard 7	1	37.000	10.0	1.0	1.0	2.779	STD7	2025-08-06 12:27:27 UTC-4	used

Sample data

Ident STD1
Sample type Standard 1
Determination start 2025-08-06 10:18:54 UTC-4
Method IC1-080625
Operator

Anions

Data source Conductivity detector 1 (Eco IC 1)
Channel Conductivity
Recording time 19.0 min
Integration Automatically
Column type Metrosep A Supp 19 - 150/4.0
Eluent composition not defined
Flow 0.700 mL/min
Maximum flow monitored yes
Pressure 12.73 MPa
Maximum pressure monitored yes
Temperature ---- °C

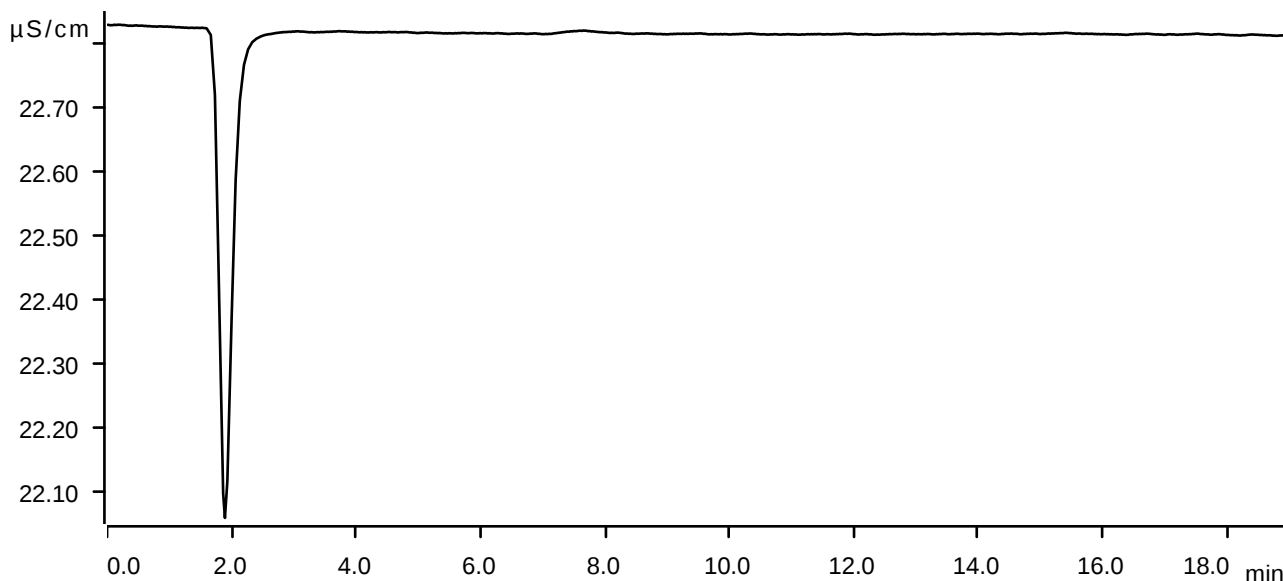Anions


Sample data

Ident STD2
Sample type Standard 2
Determination start 2025-08-06 10:40:18 UTC-4
Method IC1-080625
Operator

Anions

Data source Conductivity detector 1 (Eco IC 1)
Channel Conductivity
Recording time 19.0 min
Integration Automatically
Column type Metrosep A Supp 19 - 150/4.0
Eluent composition not defined
Flow 0.700 mL/min
Maximum flow monitored yes
Pressure 12.61 MPa
Maximum pressure monitored yes
Temperature ---- °C

Anions

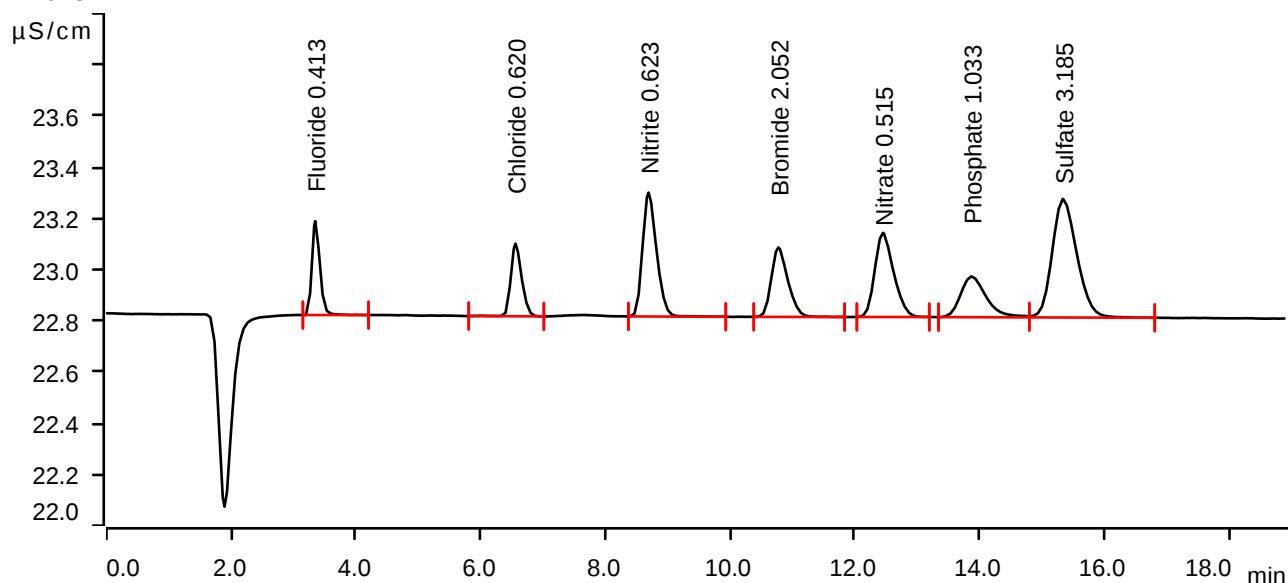

Peak number	Retention time min	Area (µS/cm) x min	Height µS/cm	Concentration ppm	Component name
1	3.350	0.0544	0.367	0.413	Fluoride
2	6.560	0.0573	0.284	0.620	Chloride
3	8.693	0.1258	0.484	0.623	Nitrite
4	10.775	0.0833	0.271	2.052	Bromide
5	12.452	0.1145	0.328	0.515	Nitrate
6	13.870	0.0758	0.159	1.033	Phosphate
7	15.340	0.2119	0.463	3.185	Sulfate


Sample data

Ident STD3
Sample type Standard 3
Determination start 2025-08-06 11:01:42 UTC-4
Method IC1-080625
Operator

Anions

Data source Conductivity detector 1 (Eco IC 1)
Channel Conductivity
Recording time 19.0 min
Integration Automatically
Column type Metrosep A Supp 19 - 150/4.0
Eluent composition not defined
Flow 0.700 mL/min
Maximum flow monitored yes
Pressure 12.61 MPa
Maximum pressure monitored yes
Temperature ---- °C

Anions

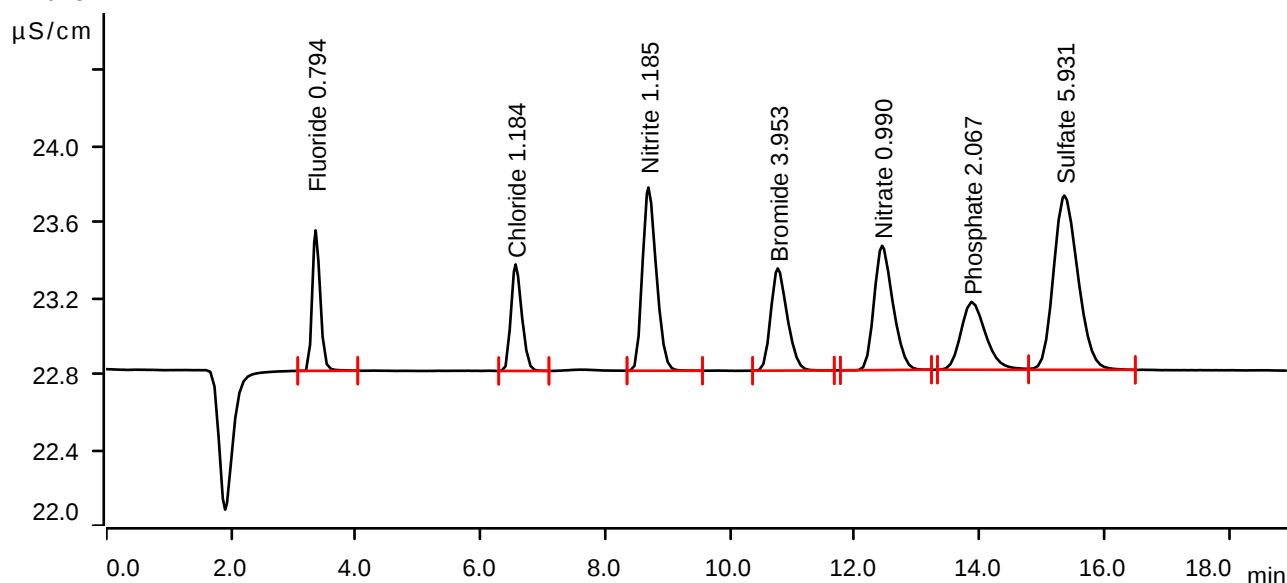

Peak number	Retention time min	Area (µS/cm) x min	Height µS/cm	Concentration ppm	Component name
1	3.357	0.1095	0.740	0.794	Fluoride
2	6.562	0.1125	0.561	1.184	Chloride
3	8.692	0.2498	0.966	1.185	Nitrite
4	10.765	0.1649	0.539	3.953	Bromide
5	12.438	0.2291	0.655	0.990	Nitrate
6	13.875	0.1645	0.358	2.067	Phosphate
7	15.360	0.4176	0.918	5.931	Sulfate


Sample data

Ident STD4
Sample type Standard 4
Determination start 2025-08-06 11:23:08 UTC-4
Method IC1-080625
Operator

Anions

Data source Conductivity detector 1 (Eco IC 1)
Channel Conductivity
Recording time 19.0 min
Integration Automatically
Column type Metrosep A Supp 19 - 150/4.0
Eluent composition not defined
Flow 0.700 mL/min
Maximum flow monitored yes
Pressure 12.44 MPa
Maximum pressure monitored yes
Temperature ---- °C

Anions

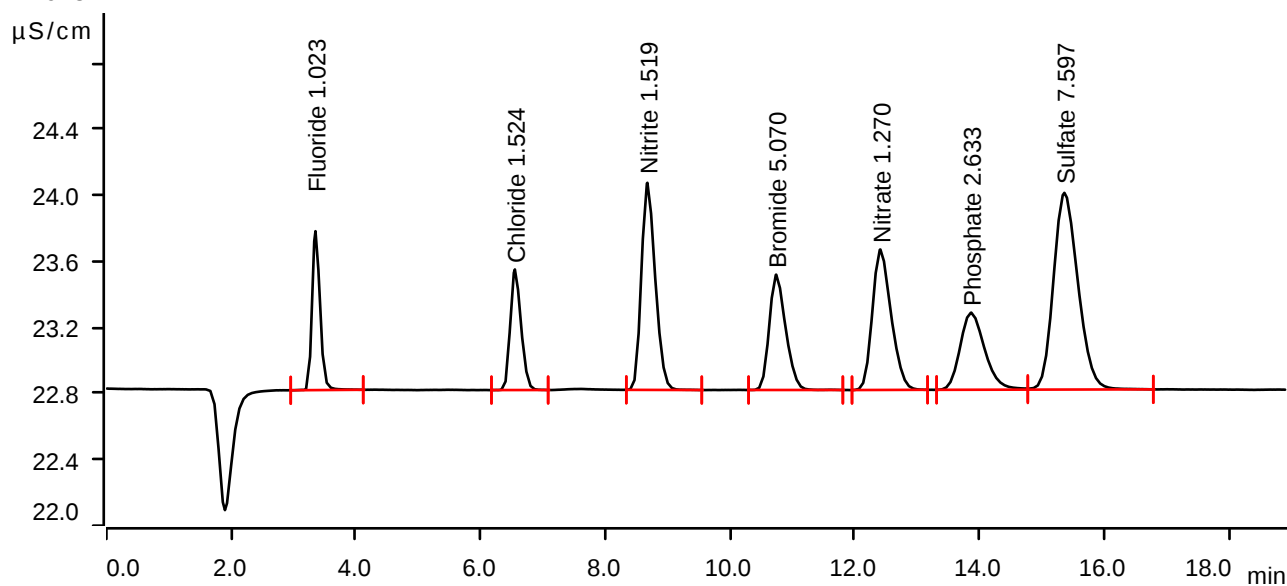

Peak number	Retention time min	Area (µS/cm) x min	Height µS/cm	Concentration ppm	Component name
1	3.353	0.1425	0.962	1.023	Fluoride
2	6.552	0.1459	0.730	1.524	Chloride
3	8.675	0.3233	1.254	1.519	Nitrite
4	10.740	0.2127	0.698	5.070	Bromide
5	12.410	0.2964	0.850	1.270	Nitrate
6	13.862	0.2131	0.467	2.633	Phosphate
7	15.360	0.5424	1.191	7.597	Sulfate


Sample data

Ident STD5
Sample type Standard 5
Determination start 2025-08-06 11:44:33 UTC-4
Method IC1-080625
Operator

Anions

Data source Conductivity detector 1 (Eco IC 1)
Channel Conductivity
Recording time 19.0 min
Integration Automatically
Column type Metrosep A Supp 19 - 150/4.0
Eluent composition not defined
Flow 0.700 mL/min
Maximum flow monitored yes
Pressure 12.44 MPa
Maximum pressure monitored yes
Temperature ---- °C

Anions

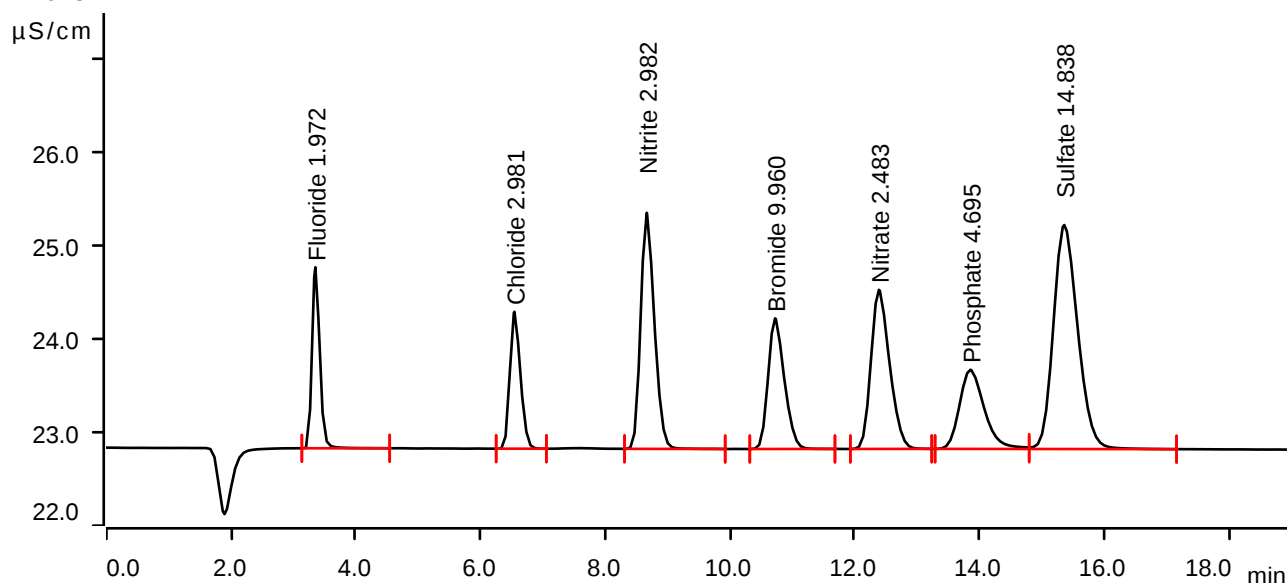

Peak number	Retention time min	Area (µS/cm) x min	Height µS/cm	Concentration ppm	Component name
1	3.352	0.2796	1.943	1.972	Fluoride
2	6.543	0.2887	1.470	2.981	Chloride
3	8.663	0.6461	2.534	2.982	Nitrite
4	10.722	0.4223	1.403	9.960	Bromide
5	12.387	0.5889	1.709	2.483	Nitrate
6	13.853	0.3900	0.850	4.695	Phosphate
7	15.358	1.0850	2.405	14.838	Sulfate


Sample data

Ident STD6
Sample type Standard 6
Determination start 2025-08-06 12:06:00 UTC-4
Method IC1-080625
Operator

Anions

Data source Conductivity detector 1 (Eco IC 1)
Channel Conductivity
Recording time 19.0 min
Integration Automatically
Column type Metrosep A Supp 19 - 150/4.0
Eluent composition not defined
Flow 0.700 mL/min
Maximum flow monitored yes
Pressure 12.39 MPa
Maximum pressure monitored yes
Temperature ---- °C

Anions

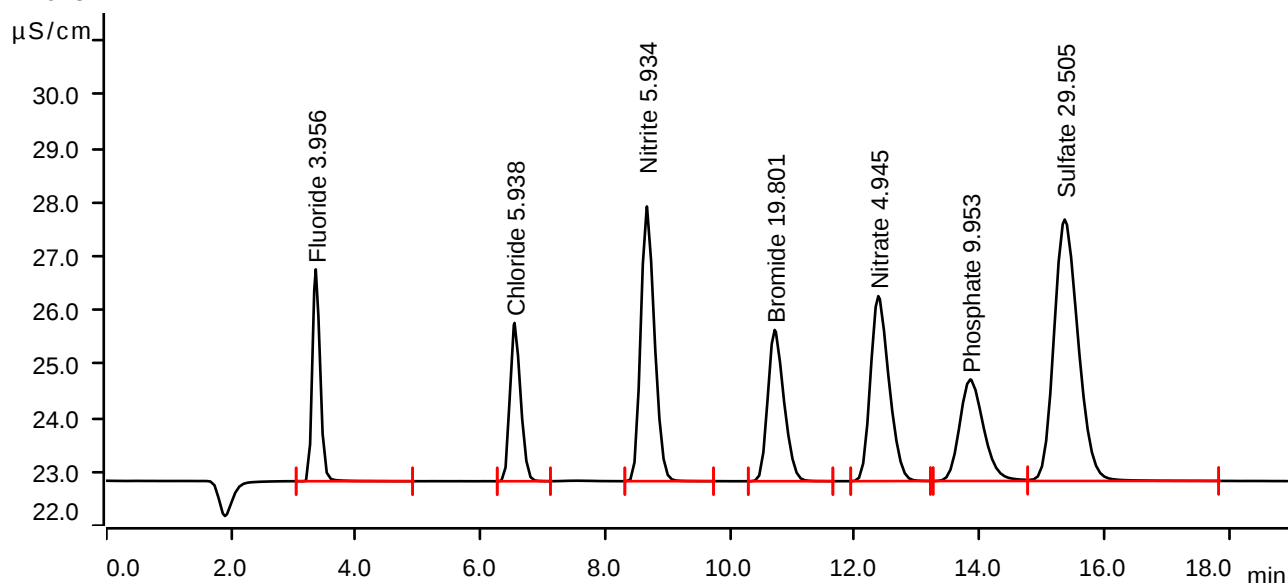

Peak number	Retention time min	Area (µS/cm) x min	Height µS/cm	Concentration ppm	Component name
1	3.358	0.5660	3.928	3.956	Fluoride
2	6.545	0.5784	2.936	5.938	Chloride
3	8.665	1.2973	5.095	5.934	Nitrite
4	10.715	0.8441	2.805	19.801	Bromide
5	12.377	1.1824	3.431	4.945	Nitrate
6	13.852	0.8412	1.884	9.953	Phosphate
7	15.365	2.1839	4.849	29.505	Sulfate


Sample data

Ident STD7
Sample type Standard 7
Determination start 2025-08-06 12:27:27 UTC-4
Method IC1-080625
Operator

Anions

Data source Conductivity detector 1 (Eco IC 1)
Channel Conductivity
Recording time 19.0 min
Integration Automatically
Column type Metrosep A Supp 19 - 150/4.0
Eluent composition not defined
Flow 0.700 mL/min
Maximum flow monitored yes
Pressure 12.39 MPa
Maximum pressure monitored yes
Temperature ---- °C

Anions

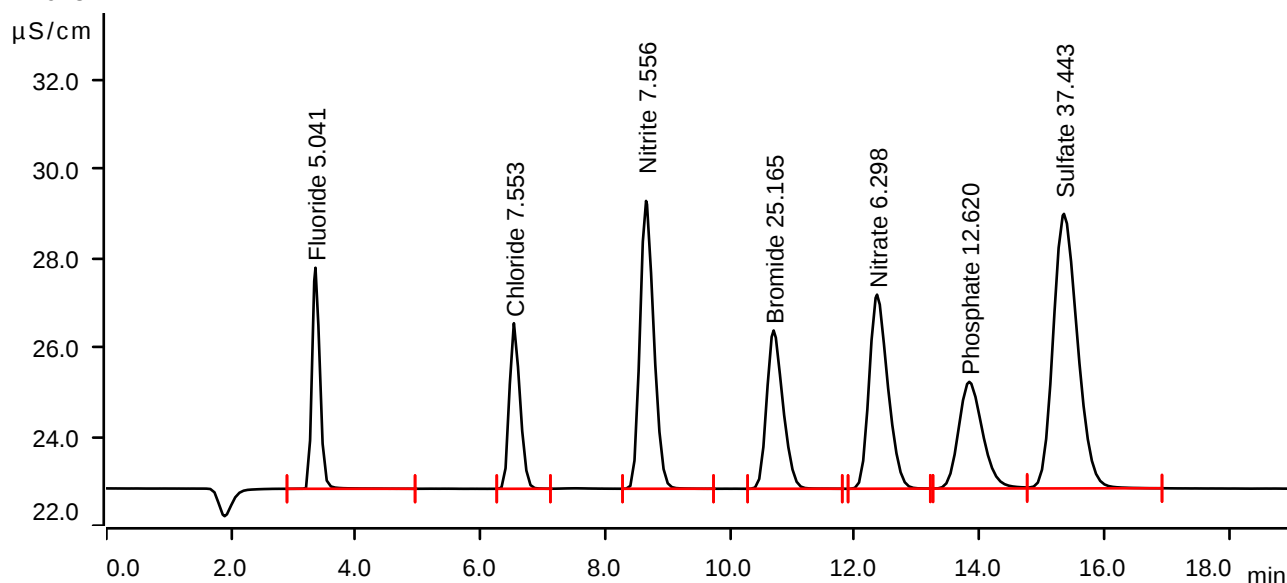

Peak number	Retention time min	Area (µS/cm) x min	Height µS/cm	Concentration ppm	Component name
1	3.353	0.7226	4.963	5.041	Fluoride
2	6.535	0.7366	3.716	7.553	Chloride
3	8.653	1.6550	6.462	7.556	Nitrite
4	10.698	1.0740	3.554	25.165	Bromide
5	12.357	1.5086	4.357	6.298	Nitrate
6	13.835	1.0700	2.396	12.620	Phosphate
7	15.353	2.7786	6.163	37.443	Sulfate


Sample data

Ident ICV
Sample type Check standard 1
Determination start 2025-08-06 12:48:56 UTC-4
Method IC1-080625
Operator

Anions

Data source Conductivity detector 1 (Eco IC 1)
Channel Conductivity
Recording time 19.0 min
Integration Automatically
Column type Metrosep A Supp 19 - 150/4.0
Eluent composition not defined
Flow 0.700 mL/min
Maximum flow monitored yes
Pressure 12.44 MPa
Maximum pressure monitored yes
Temperature ---- °C

Anions

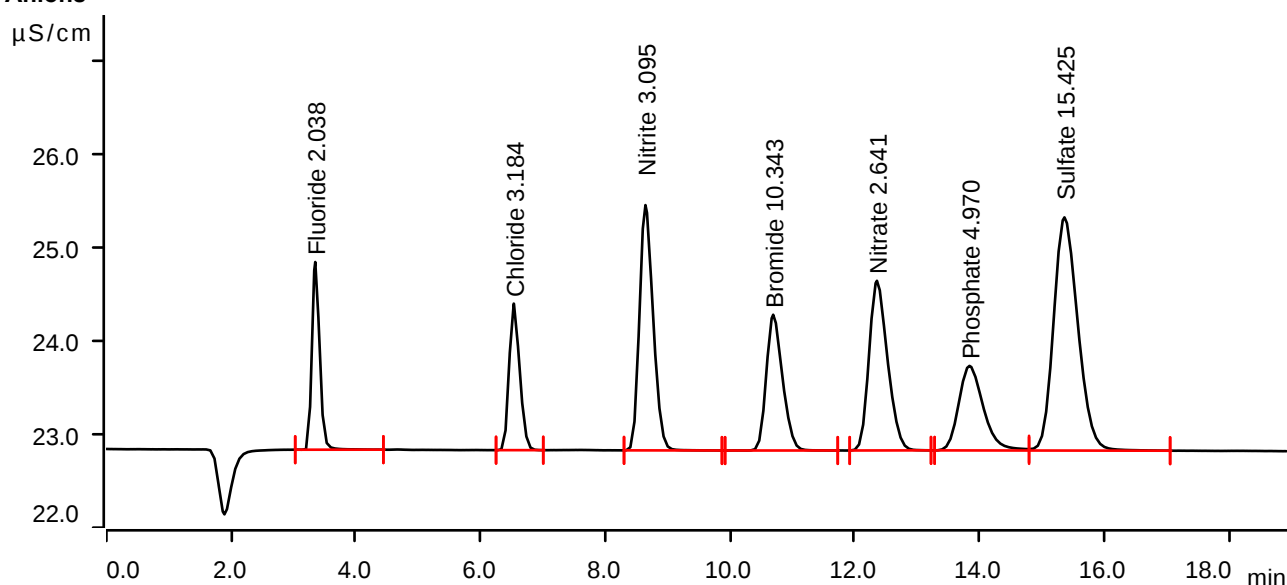

Peak number	Retention time min	Area (µS/cm) x min	Height µS/cm	Concentration ppm	Component name
1	3.350	0.2890	2.015	2.038	Fluoride
2	6.532	0.3085	1.574	3.184	Chloride
3	8.643	0.6711	2.634	3.095	Nitrite
4	10.692	0.4387	1.458	10.343	Bromide
5	12.355	0.6270	1.822	2.641	Nitrate
6	13.838	0.4136	0.908	4.970	Phosphate
7	15.362	1.1289	2.504	15.425	Sulfate


Sample data

Ident ICB
Sample type Sample
Determination start 2025-08-06 13:10:25 UTC-4
Method IC1-080625
Operator

Anions

Data source Conductivity detector 1 (Eco IC 1)
Channel Conductivity
Recording time 19.0 min
Integration Automatically
Column type Metrosep A Supp 19 - 150/4.0
Eluent composition not defined
Flow 0.700 mL/min
Maximum flow monitored yes
Pressure 12.33 MPa
Maximum pressure monitored yes
Temperature ---- °C

Anions

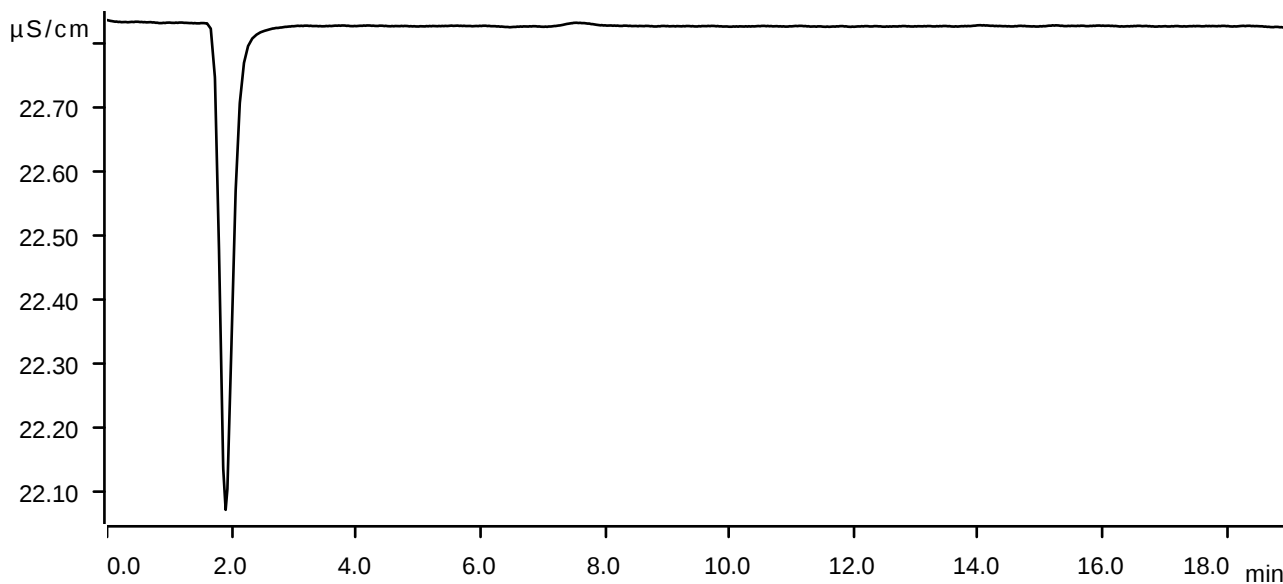


Sample data

Ident CCV
 Sample type Check standard 1
 Determination start 2025-08-15 08:46:08 UTC-4
 Method IC1-080625
 Operator

Anions

Data source Conductivity detector 1 (Eco IC 1)
 Channel Conductivity
 Recording time 19.0 min
 Integration Automatically
 Column type Metrosep A Supp 19 - 150/4.0
 Eluent composition not defined
 Flow 0.700 mL/min
 Maximum flow monitored yes
 Pressure 12.27 MPa
 Maximum pressure monitored yes
 Temperature ---- °C

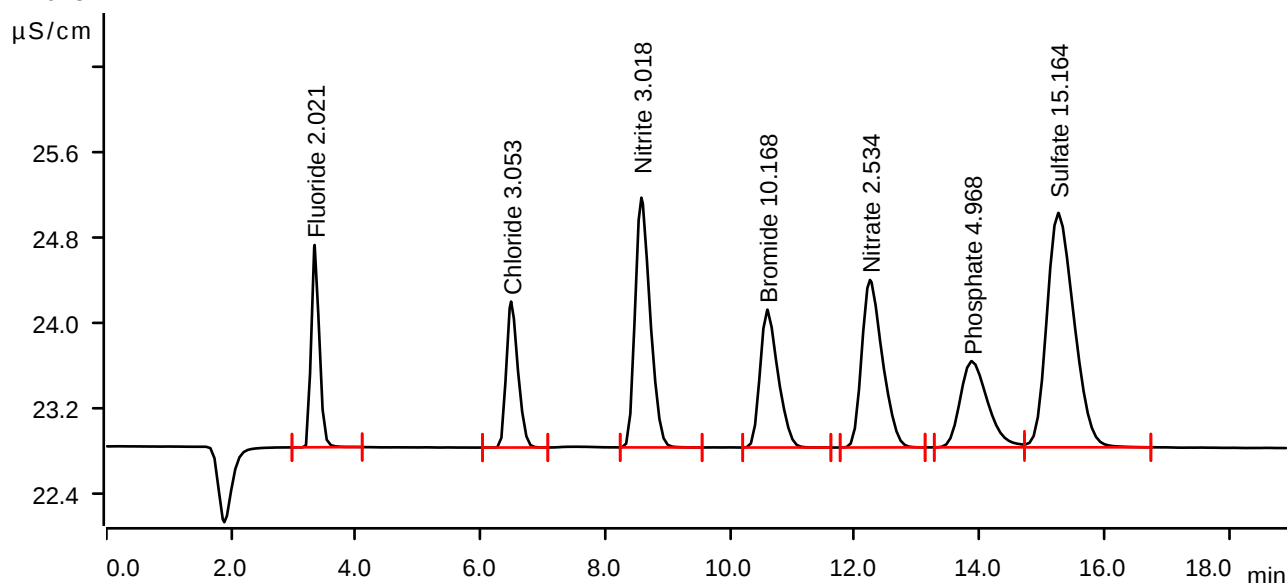Anions


Peak number	Retention time min	Area (µS/cm) x min	Height µS/cm	Concentration ppm	Component name
1	3.340	0.2866	1.895	2.021	Fluoride
2	6.490	0.2956	1.368	3.053	Chloride
3	8.578	0.6541	2.340	3.018	Nitrite
4	10.597	0.4312	1.292	10.168	Bromide
5	12.243	0.6013	1.570	2.534	Nitrate
6	13.873	0.4134	0.808	4.968	Phosphate
7	15.262	1.1094	2.197	15.164	Sulfate

Sample data

Ident CCB
Sample type Sample
Determination start 2025-08-15 09:07:38 UTC-4
Method IC1-080625
Operator

Anions

Data source Conductivity detector 1 (Eco IC 1)
Channel Conductivity
Recording time 19.0 min
Integration Automatically
Column type Metrosep A Supp 19 - 150/4.0
Eluent composition not defined
Flow 0.700 mL/min
Maximum flow monitored yes
Pressure 12.22 MPa
Maximum pressure monitored yes
Temperature ---- °C

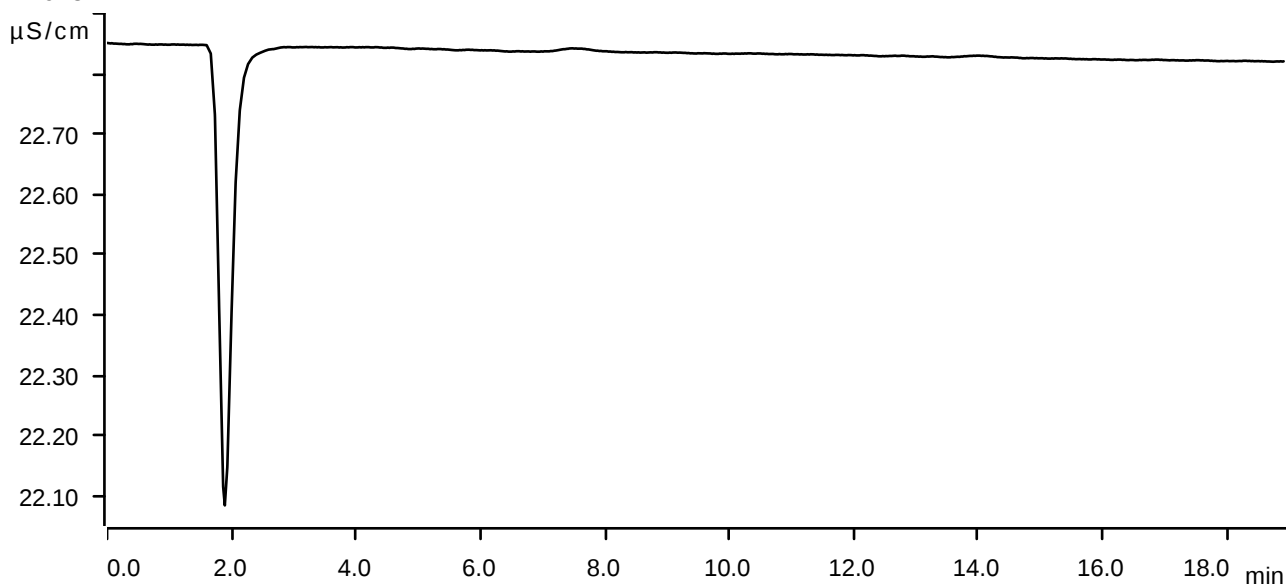
Anions

Sample data

Ident LB136833BLW
Sample type Sample
Determination start 2025-08-15 09:29:09 UTC-4
Method IC1-080625
Operator

Anions

Data source Conductivity detector 1 (Eco IC 1)
Channel Conductivity
Recording time 19.0 min
Integration Automatically
Column type Metrosep A Supp 19 - 150/4.0
Eluent composition not defined
Flow 0.700 mL/min
Maximum flow monitored yes
Pressure 12.11 MPa
Maximum pressure monitored yes
Temperature ---- °C

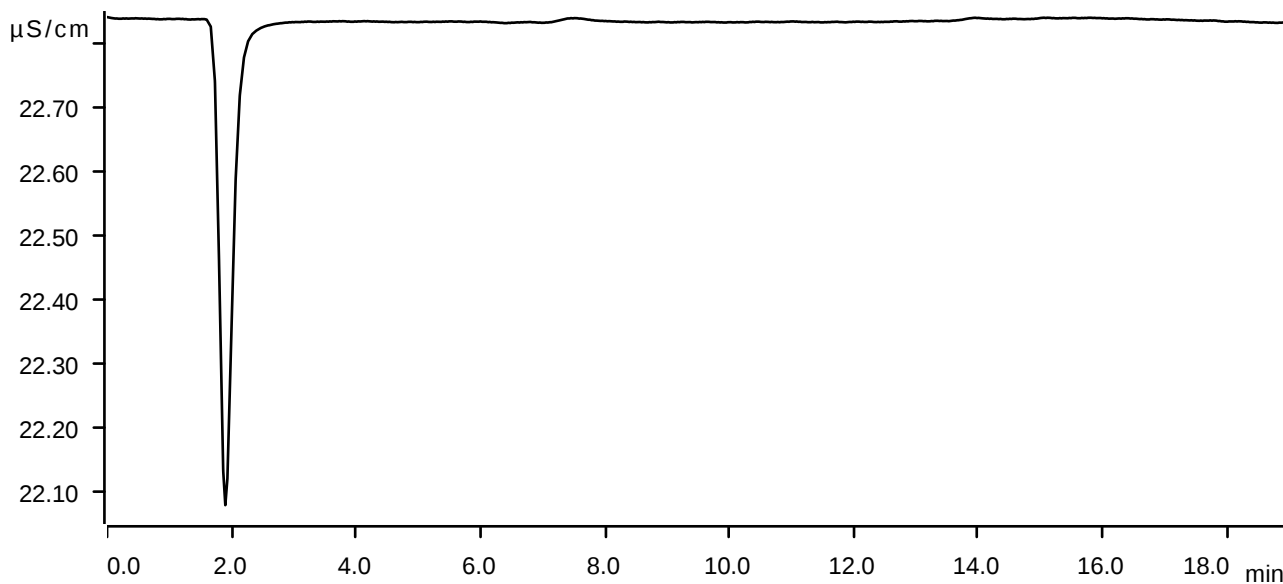Anions


Sample data

Ident LB136833BSW
Sample type Check standard 1
Determination start 2025-08-15 09:50:41 UTC-4
Method IC1-080625
Operator

Anions

Data source Conductivity detector 1 (Eco IC 1)
Channel Conductivity
Recording time 19.0 min
Integration Automatically
Column type Metrosep A Supp 19 - 150/4.0
Eluent composition not defined
Flow 0.700 mL/min
Maximum flow monitored yes
Pressure 12.05 MPa
Maximum pressure monitored yes
Temperature ---- °C

Anions

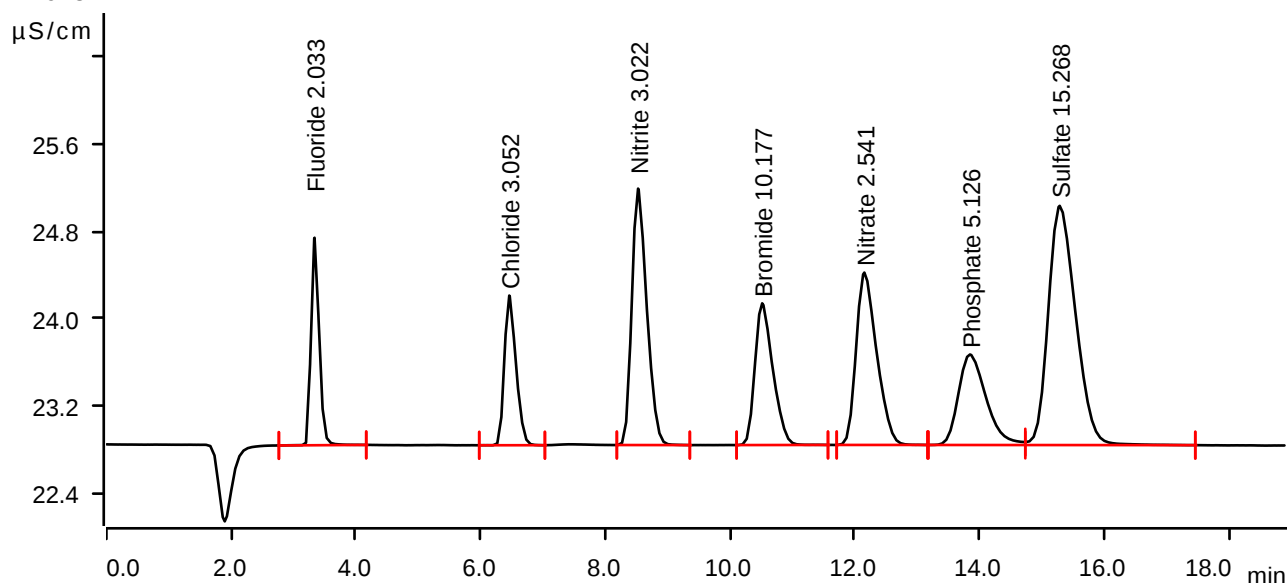

Peak number	Retention time min	Area (µS/cm) x min	Height µS/cm	Concentration ppm	Component name
1	3.338	0.2883	1.904	2.033	Fluoride
2	6.460	0.2956	1.373	3.052	Chloride
3	8.525	0.6548	2.353	3.022	Nitrite
4	10.515	0.4316	1.300	10.177	Bromide
5	12.153	0.6029	1.582	2.541	Nitrate
6	13.847	0.4270	0.830	5.126	Phosphate
7	15.285	1.1172	2.195	15.268	Sulfate


Sample data

Ident Q2869-01
Sample type Sample
Determination start 2025-08-15 10:12:14 UTC-4
Method IC1-080625
Operator

Anions

Data source Conductivity detector 1 (Eco IC 1)
Channel Conductivity
Recording time 19.0 min
Integration Automatically
Column type Metrosep A Supp 19 - 150/4.0
Eluent composition not defined
Flow 0.700 mL/min
Maximum flow monitored yes
Pressure 12.05 MPa
Maximum pressure monitored yes
Temperature ---- °C

Anions

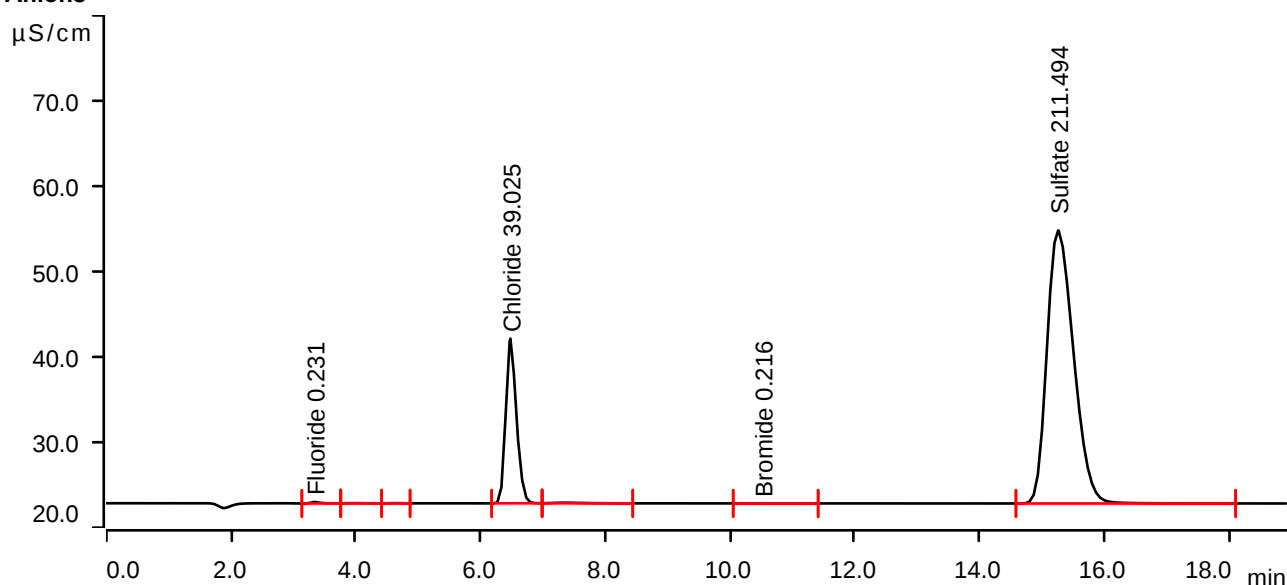

Peak number	Retention time min	Area (µS/cm) x min	Height µS/cm	Concentration ppm	Component name
1	3.337	0.0282	0.169	0.231	Fluoride
2	3.972	0.0044	0.017	invalid	
3	4.635	0.0036	0.019	invalid	
4	6.478	3.8201	19.288	39.025	Chloride
5	7.353	0.0346	0.067	invalid	Bromide
6	10.520	0.0047	0.012	0.216	
7	15.260	15.8191	31.991	211.494	


Sample data

Ident Q2869-05
Sample type Sample
Determination start 2025-08-15 10:55:09 UTC-4
Method IC1-080625
Operator

Anions

Data source Conductivity detector 1 (Eco IC 1)
Channel Conductivity
Recording time 19.0 min
Integration Automatically
Column type Metrosep A Supp 19 - 150/4.0
Eluent composition not defined
Flow 0.700 mL/min
Maximum flow monitored yes
Pressure 11.94 MPa
Maximum pressure monitored yes
Temperature ---- °C

Anions

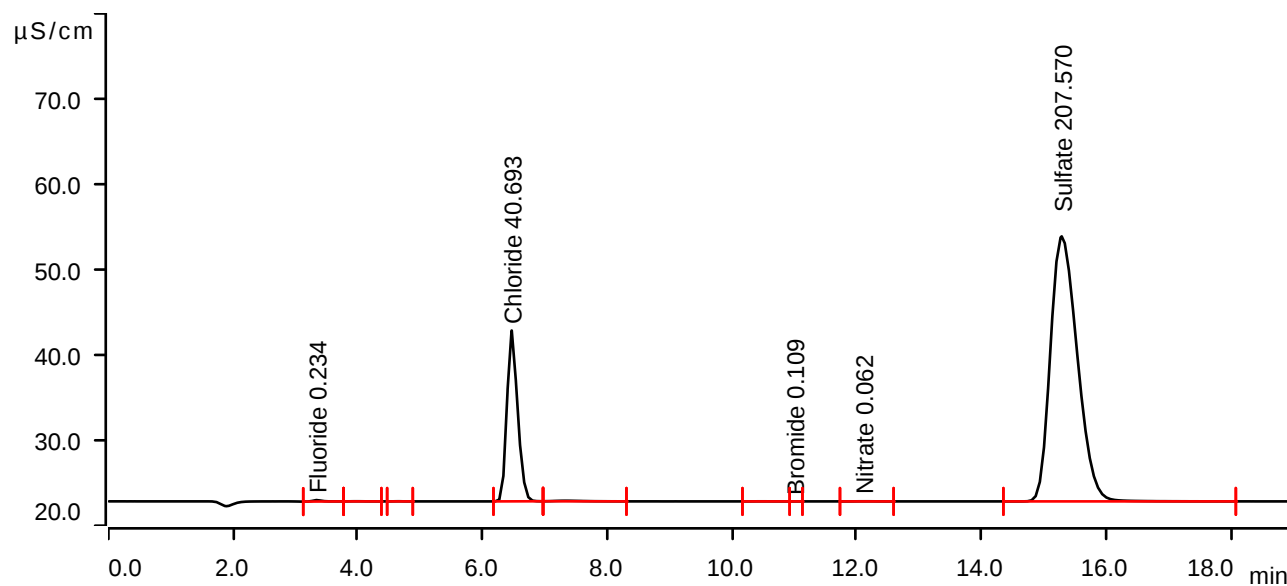

Peak number	Retention time min	Area ($\mu\text{S/cm}$) x min	Height $\mu\text{S/cm}$	Concentration ppm	Component name
1	3.338	0.0286	0.169	0.234	Fluoride
2	3.960	0.0040	0.016	invalid	
3	4.645	0.0028	0.016	invalid	
4	6.465	3.9835	20.011	40.693	Chloride
5	7.323	0.0336	0.065	invalid	
6	10.490	0.0036	0.011	invalid	
7	10.998	0.0001	0.001	0.109	Bromide
8	12.105	0.0052	0.014	0.062	Nitrate
9	15.285	15.5251	31.046	207.570	Sulfate


Sample data

Ident Q2869-07
Sample type Sample
Determination start 2025-08-15 11:59:40 UTC-4
Method IC1-080625
Operator

Anions

Data source Conductivity detector 1 (Eco IC 1)
Channel Conductivity
Recording time 19.0 min
Integration Automatically
Column type Metrosep A Supp 19 - 150/4.0
Eluent composition not defined
Flow 0.700 mL/min
Maximum flow monitored yes
Pressure 11.77 MPa
Maximum pressure monitored yes
Temperature ---- °C

Anions

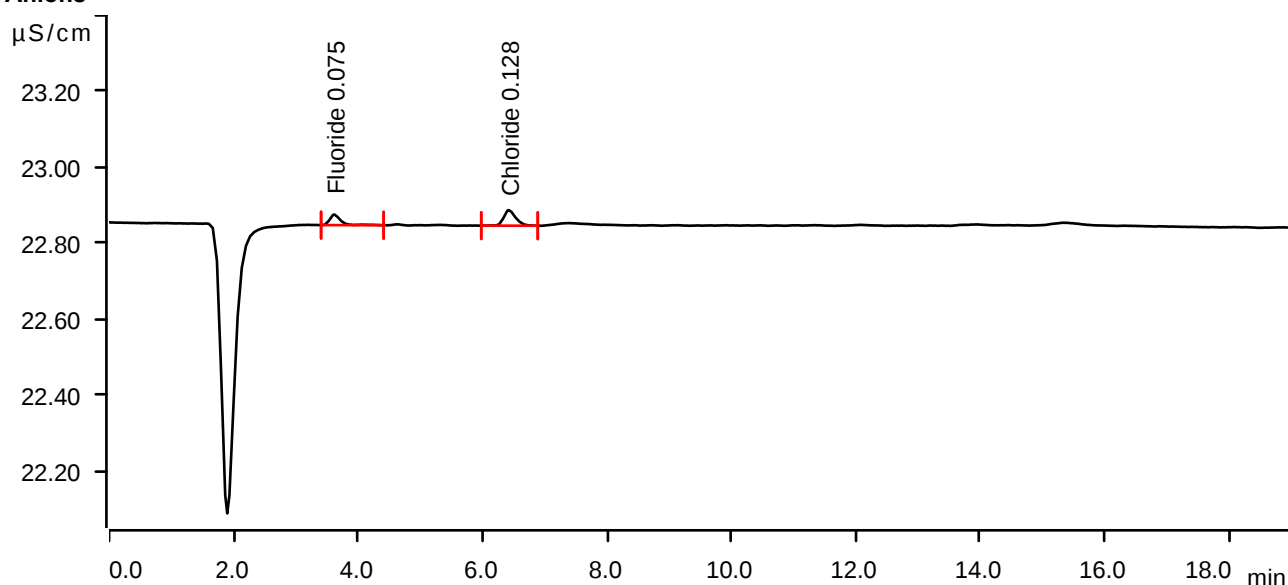

Peak number	Retention time min	Area (µS/cm) x min	Height µS/cm	Concentration ppm	Component name
1	3.623	0.0056	0.028	0.075	Fluoride
2	6.422	0.0090	0.041	0.128	Chloride


Sample data

Ident Q2878-01
Sample type Sample
Determination start 2025-08-15 12:42:36 UTC-4
Method IC1-080625
Operator

Anions

Data source Conductivity detector 1 (Eco IC 1)
Channel Conductivity
Recording time 19.0 min
Integration Automatically
Column type Metrosep A Supp 19 - 150/4.0
Eluent composition not defined
Flow 0.700 mL/min
Maximum flow monitored yes
Pressure 11.77 MPa
Maximum pressure monitored yes
Temperature ---- °C

Anions

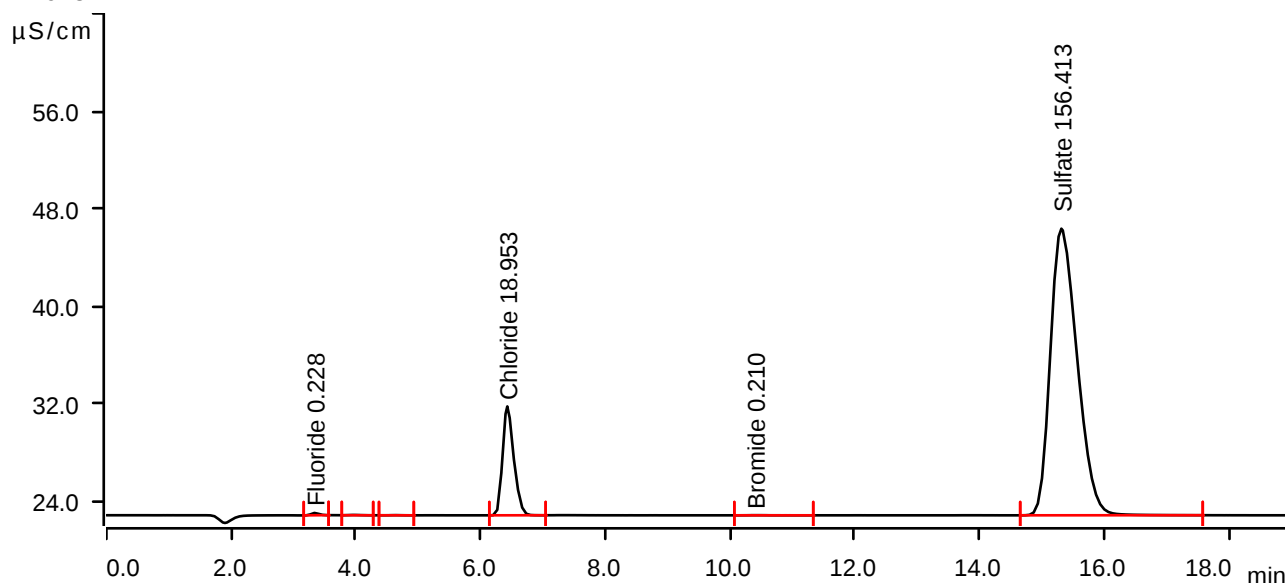

Peak number	Retention time min	Area (µS/cm) x min	Height µS/cm	Concentration ppm	Component name
1	3.340	0.0277	0.188	0.228	Fluoride
2	3.962	0.0054	0.025	invalid	
3	4.642	0.0027	0.014	invalid	
4	6.428	1.8535	8.930	18.953	Chloride
5	10.395	0.0044	0.012	0.210	Bromide
6	15.312	11.6922	23.503	156.413	Sulfate


Sample data

Ident Q2878-01MS
Sample type Sample
Determination start 2025-08-15 13:04:11 UTC-4
Method IC1-080625
Operator

Anions

Data source Conductivity detector 1 (Eco IC 1)
Channel Conductivity
Recording time 19.0 min
Integration Automatically
Column type Metrosep A Supp 19 - 150/4.0
Eluent composition not defined
Flow 0.700 mL/min
Maximum flow monitored yes
Pressure 11.71 MPa
Maximum pressure monitored yes
Temperature ---- °C

Anions

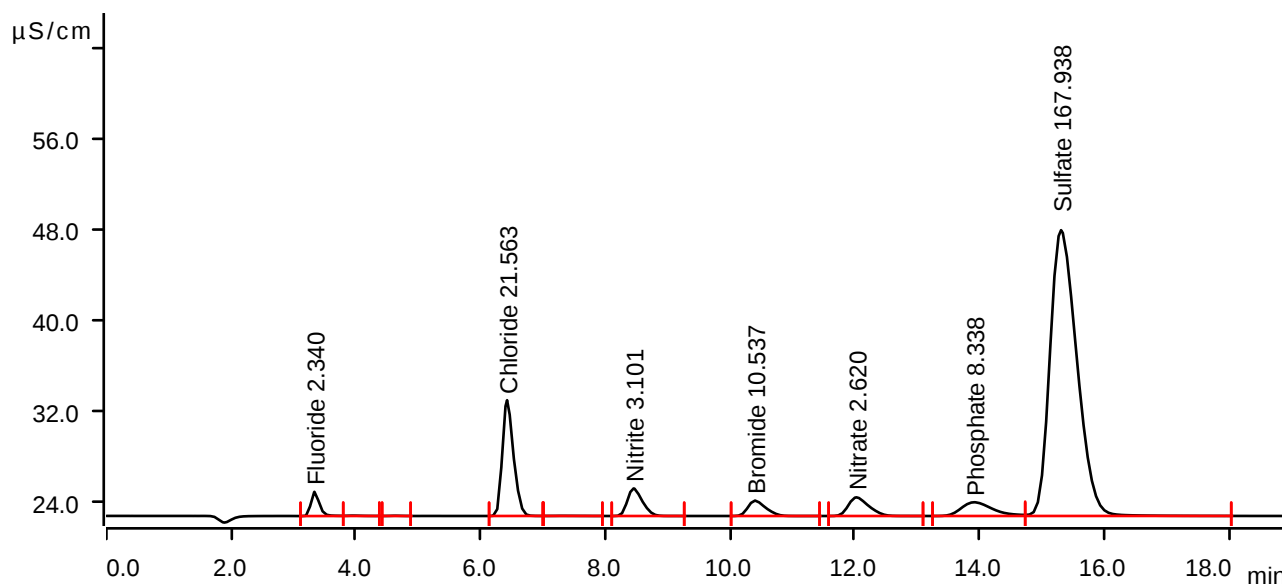

Peak number	Retention time min	Area ($\mu\text{S/cm}$) x min	Height $\mu\text{S/cm}$	Concentration ppm	Component name
1	3.337	0.3327	2.124	2.340	Fluoride
2	3.957	0.0086	0.033	invalid	
3	4.638	0.0038	0.021	invalid	
4	6.425	2.1092	10.175	21.563	Chloride
5	7.318	0.0046	0.010	invalid	
6	8.453	0.6724	2.422	3.101	Nitrite
7	10.400	0.4470	1.355	10.537	Bromide
8	12.027	0.6219	1.639	2.620	Nitrate
9	13.915	0.7026	1.207	8.338	Phosphate
10	15.307	12.5557	25.109	167.938	Sulfate


Sample data

Ident Q2878-01MSD
Sample type Sample
Determination start 2025-08-15 13:25:46 UTC-4
Method IC1-080625
Operator

Anions

Data source Conductivity detector 1 (Eco IC 1)
Channel Conductivity
Recording time 19.0 min
Integration Automatically
Column type Metrosep A Supp 19 - 150/4.0
Eluent composition not defined
Flow 0.700 mL/min
Maximum flow monitored yes
Pressure 11.71 MPa
Maximum pressure monitored yes
Temperature ---- °C

Anions

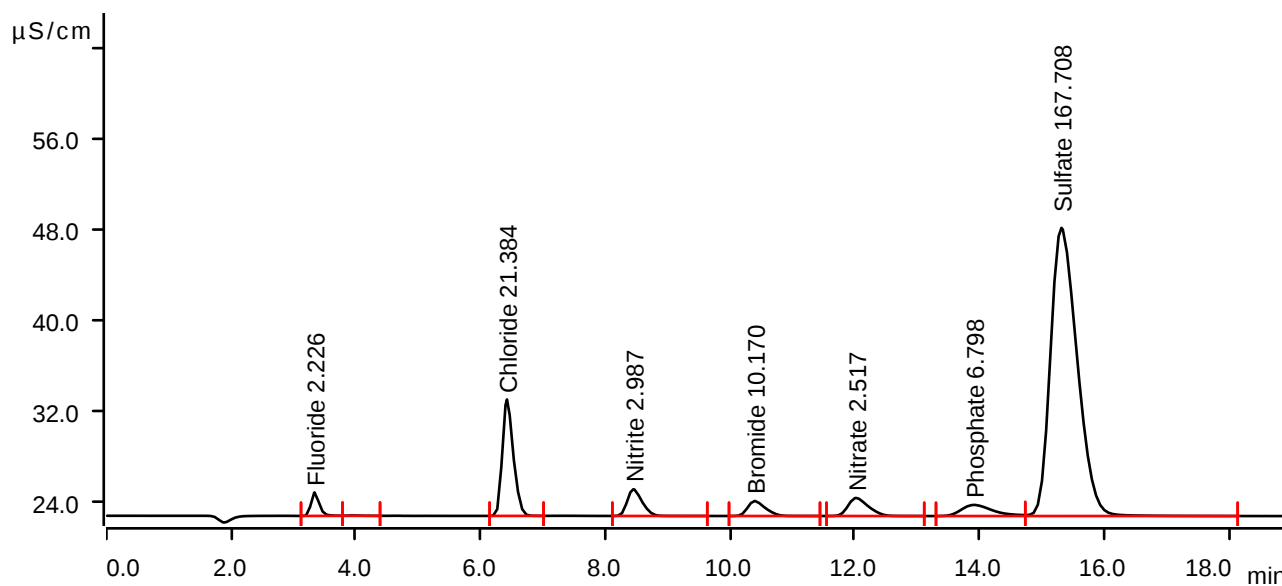

Peak number	Retention time min	Area (µS/cm) x min	Height µS/cm	Concentration ppm	Component name
1	3.338	0.3161	2.060	2.226	Fluoride
2	3.953	0.0087	0.033	invalid	
3	6.423	2.0917	10.230	21.384	Chloride
4	8.450	0.6472	2.353	2.987	Nitrite
5	10.395	0.4313	1.317	10.170	Bromide
6	12.022	0.5971	1.589	2.517	Nitrate
7	13.910	0.5705	0.976	6.798	Phosphate
8	15.313	12.5385	25.318	167.708	Sulfate


Sample data

Ident Q2869-01DLX10
Sample type Sample
Determination start 2025-08-15 13:47:20 UTC-4
Method IC1-080625
Operator

Anions

Data source Conductivity detector 1 (Eco IC 1)
Channel Conductivity
Recording time 19.0 min
Integration Automatically
Column type Metrosep A Supp 19 - 150/4.0
Eluent composition not defined
Flow 0.700 mL/min
Maximum flow monitored yes
Pressure 11.71 MPa
Maximum pressure monitored yes
Temperature ---- °C

Anions

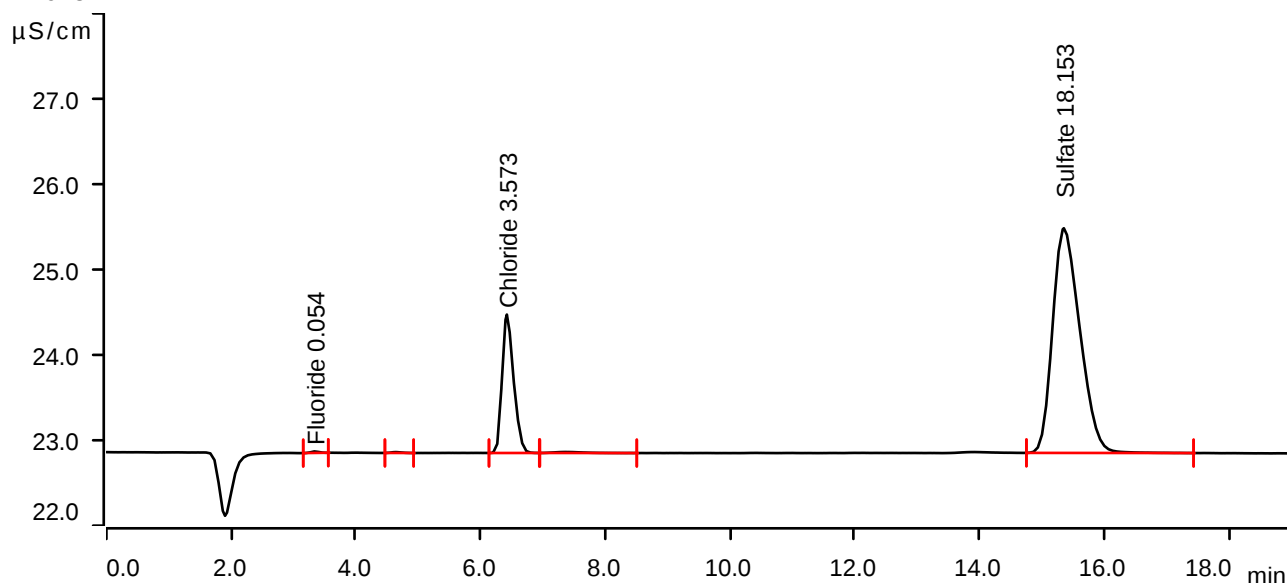

Peak number	Retention time min	Area (µS/cm) x min	Height µS/cm	Concentration ppm	Component name
1	3.338	0.0026	0.017	0.054	Fluoride
2	4.642	0.0019	0.010	invalid	
3	6.422	0.3466	1.622	3.573	Chloride
4	7.365	0.0063	0.012	invalid	
5	15.352	1.3333	2.632	18.153	Sulfate


Sample data

Ident Q2869-05DLX10
Sample type Sample
Determination start 2025-08-15 14:08:53 UTC-4
Method IC1-080625
Operator

Anions

Data source Conductivity detector 1 (Eco IC 1)
Channel Conductivity
Recording time 19.0 min
Integration Automatically
Column type Metrosep A Supp 19 - 150/4.0
Eluent composition not defined
Flow 0.700 mL/min
Maximum flow monitored yes
Pressure 11.88 MPa
Maximum pressure monitored yes
Temperature ---- °C

Anions

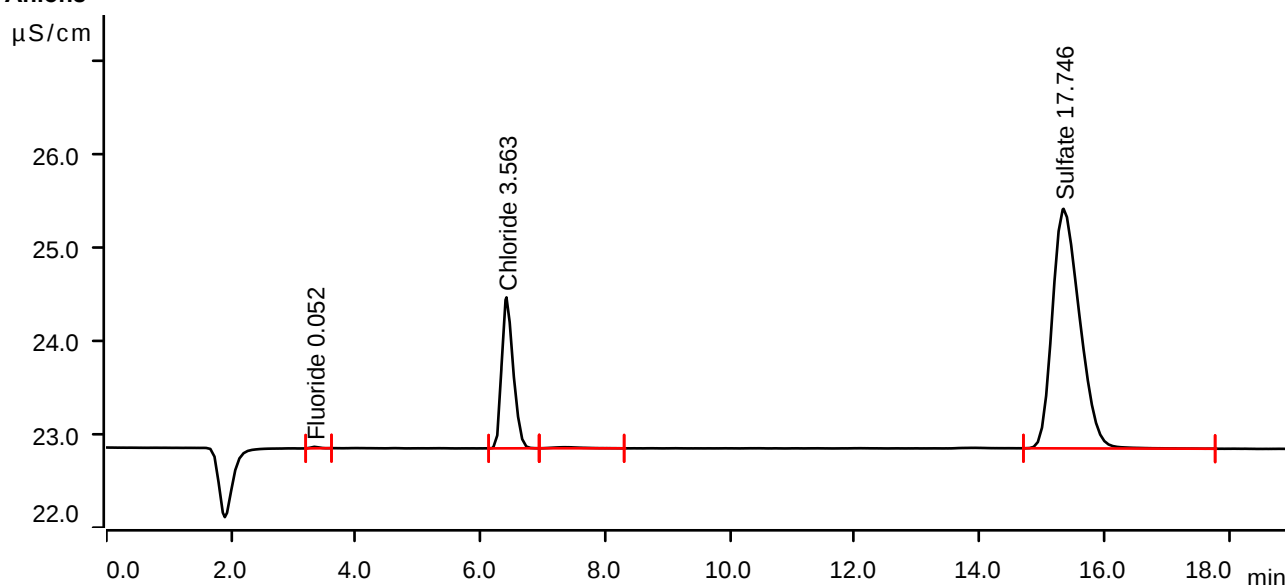

Peak number	Retention time min	Area (µS/cm) x min	Height µS/cm	Concentration ppm	Component name
1	3.335	0.0024	0.016	0.052	Fluoride
2	6.415	0.3456	1.621	3.563	Chloride
3	7.362	0.0064	0.011	invalid	
4	15.347	1.3029	2.573	17.746	Sulfate


Sample data

Ident CCV
Sample type Check standard 1
Determination start 2025-08-15 14:30:25 UTC-4
Method IC1-080625
Operator

Anions

Data source Conductivity detector 1 (Eco IC 1)
Channel Conductivity
Recording time 19.0 min
Integration Automatically
Column type Metrosep A Supp 19 - 150/4.0
Eluent composition not defined
Flow 0.700 mL/min
Maximum flow monitored yes
Pressure 11.71 MPa
Maximum pressure monitored yes
Temperature ---- °C

Anions

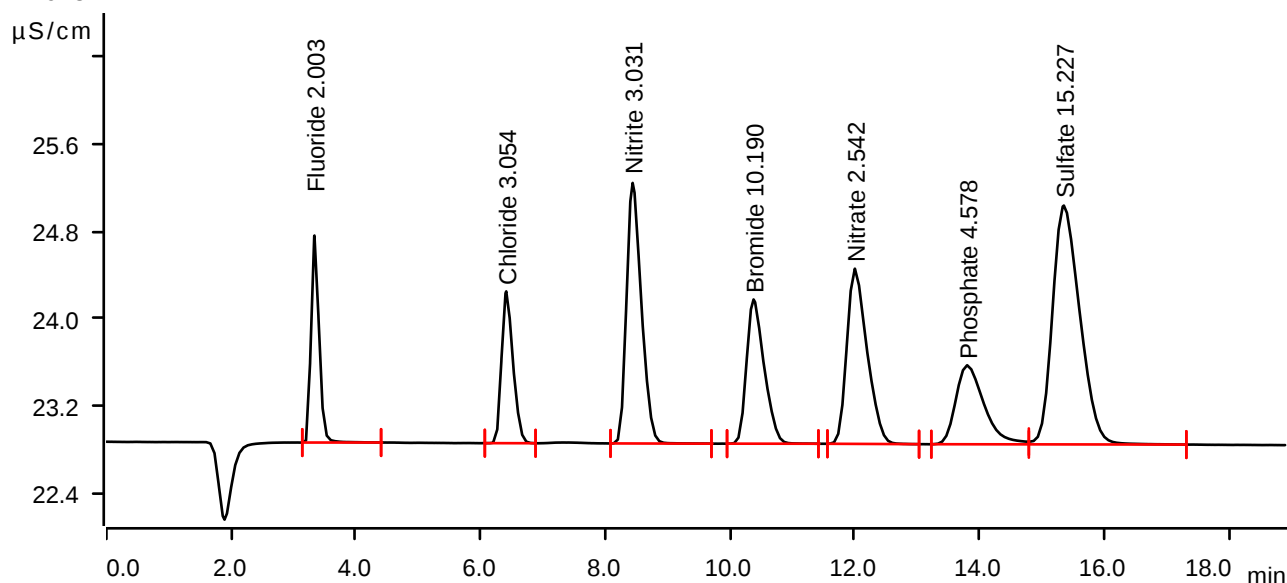


Peak number	Retention time min	Area (µS/cm) x min	Height µS/cm	Concentration ppm	Component name
1	3.337	0.2840	1.899	2.003	Fluoride
2	6.412	0.2957	1.393	3.054	Chloride
3	8.438	0.6570	2.391	3.031	Nitrite
4	10.377	0.4322	1.323	10.190	Bromide
5	12.002	0.6030	1.607	2.542	Nitrate
6	13.802	0.3800	0.725	4.578	Phosphate
7	15.352	1.1141	2.192	15.227	Sulfate

Sample data

Ident CCB
Sample type Sample
Determination start 2025-08-15 14:51:55 UTC-4
Method IC1-080625
Operator

Anions

Data source Conductivity detector 1 (Eco IC 1)
Channel Conductivity
Recording time 19.0 min
Integration Automatically
Column type Metrosep A Supp 19 - 150/4.0
Eluent composition not defined
Flow 0.700 mL/min
Maximum flow monitored yes
Pressure 11.71 MPa
Maximum pressure monitored yes
Temperature ---- °C

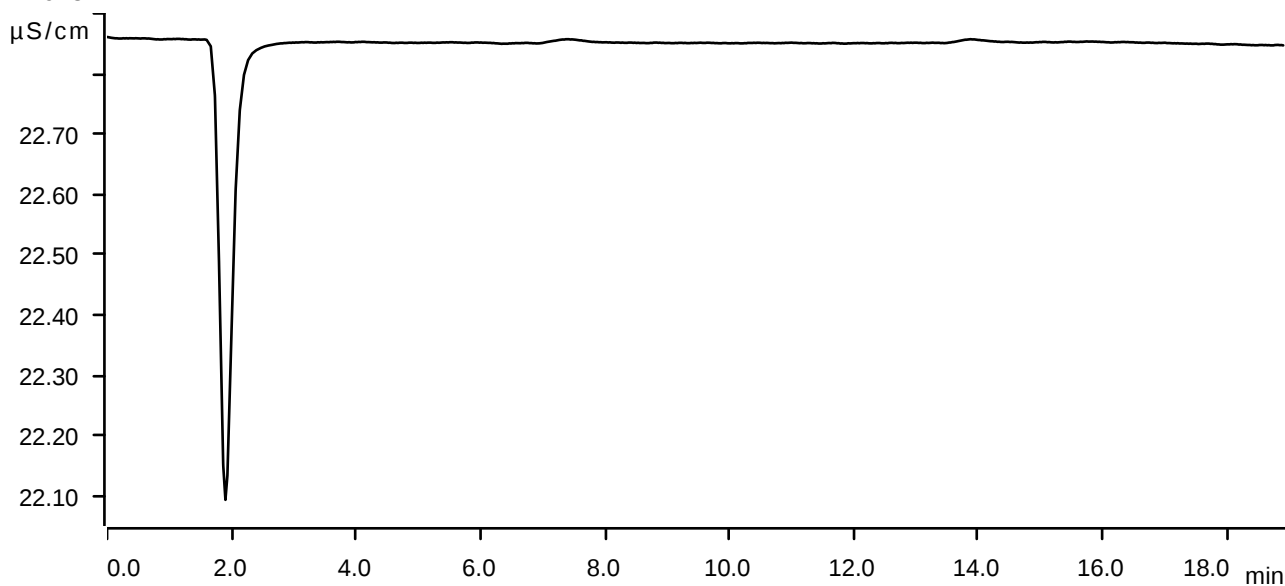Anions


Sample data

Ident Q2878-01DLX10
Sample type Sample
Determination start 2025-08-15 15:13:25 UTC-4
Method IC1-080625
Operator

Anions

Data source Conductivity detector 1 (Eco IC 1)
Channel Conductivity
Recording time 19.0 min
Integration Automatically
Column type Metrosep A Supp 19 - 150/4.0
Eluent composition not defined
Flow 0.700 mL/min
Maximum flow monitored yes
Pressure 11.99 MPa
Maximum pressure monitored yes
Temperature ---- °C

Anions

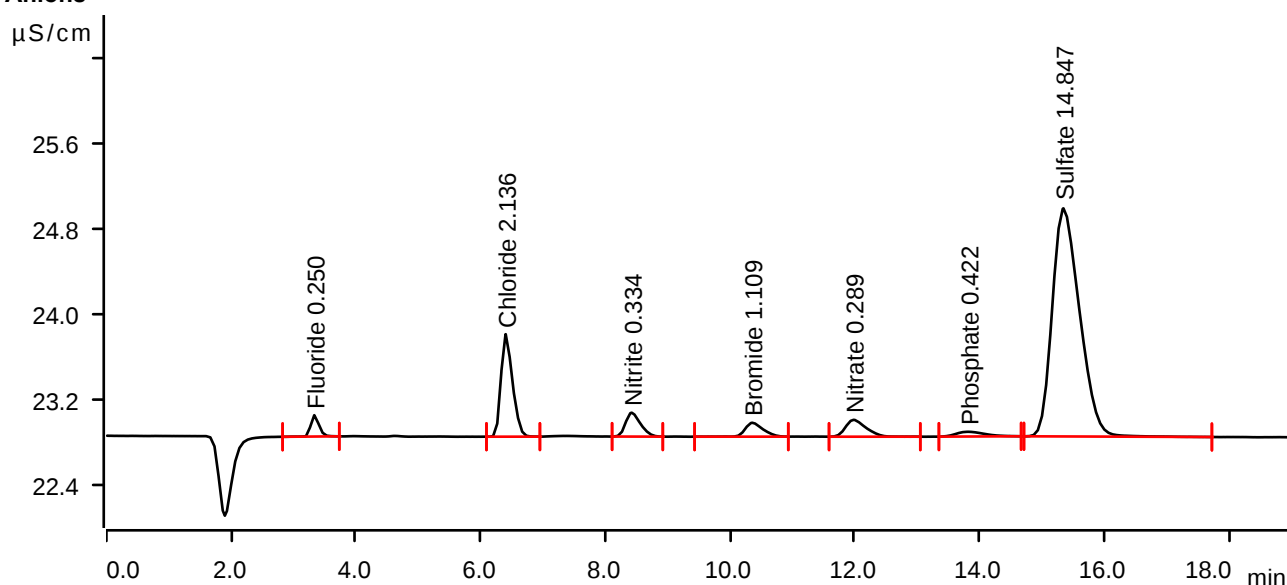

Peak number	Retention time min	Area (µS/cm) x min	Height µS/cm	Concentration ppm	Component name
1	3.335	0.0309	0.200	0.250	Fluoride
2	6.403	0.2058	0.961	2.136	Chloride
3	8.423	0.0621	0.224	0.334	Nitrite
4	10.355	0.0429	0.130	1.109	Bromide
5	11.980	0.0599	0.158	0.289	Nitrate
6	13.823	0.0234	0.044	0.422	Phosphate
7	15.345	1.0856	2.138	14.847	Sulfate


Sample data

Ident CCV
Sample type Check standard 1
Determination start 2025-08-15 15:56:28 UTC-4
Method IC1-080625
Operator

Anions

Data source Conductivity detector 1 (Eco IC 1)
Channel Conductivity
Recording time 19.0 min
Integration Automatically
Column type Metrosep A Supp 19 - 150/4.0
Eluent composition not defined
Flow 0.700 mL/min
Maximum flow monitored yes
Pressure 11.94 MPa
Maximum pressure monitored yes
Temperature ---- °C

Anions

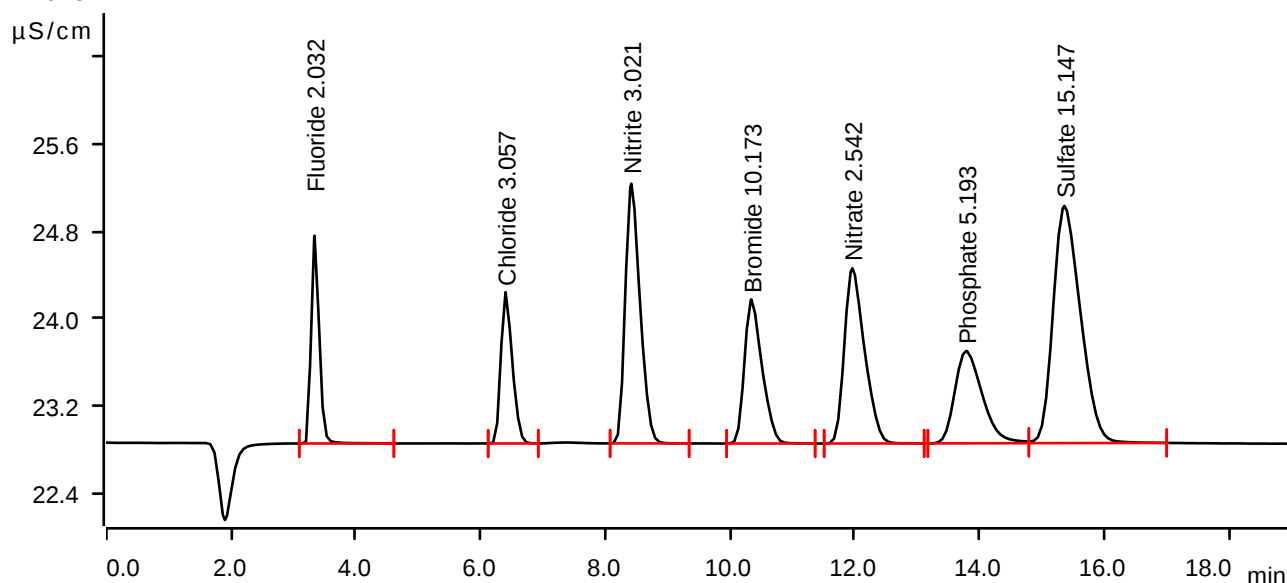

Peak number	Retention time min	Area (µS/cm) x min	Height µS/cm	Concentration ppm	Component name
1	3.338	0.2882	1.906	2.032	Fluoride
2	6.402	0.2960	1.389	3.057	Chloride
3	8.417	0.6547	2.384	3.021	Nitrite
4	10.342	0.4315	1.322	10.173	Bromide
5	11.960	0.6031	1.608	2.542	Nitrate
6	13.787	0.4328	0.848	5.193	Phosphate
7	15.360	1.1081	2.176	15.147	Sulfate

Sample data

Ident CCB
Sample type Sample
Determination start 2025-08-15 16:17:58 UTC-4
Method IC1-080625
Operator

Anions

Data source Conductivity detector 1 (Eco IC 1)
Channel Conductivity
Recording time 19.0 min
Integration Automatically
Column type Metrosep A Supp 19 - 150/4.0
Eluent composition not defined
Flow 0.700 mL/min
Maximum flow monitored yes
Pressure 11.77 MPa
Maximum pressure monitored yes
Temperature ---- °C

Anions