

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL072825\
 Data File : PL096612.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 28 Jul 2025 20:30
 Operator : AR\AJ
 Sample : PCHLORICV500
 Misc :
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 ICVPL072825CHLOR

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 29 08:55:57 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL072825.M
 Quant Title : GC Extractables
 QLast Update : Tue Jul 29 08:54:31 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.535	2.827	154.8E6	316.7E6	47.871	49.966
28)	SA Decachlor...	9.015	7.992	113.5E6	222.0E6	47.145	49.453
Target Compounds							
23)	Chlordane-1	4.690	3.838	80607891	104.0E6	473.847	496.105
24)	Chlordane-2	5.213	4.418	83986656	119.9E6	479.905	494.099
25)	Chlordane-3	5.916	5.052	326.6E6	350.0E6	488.971	503.359
26)	Chlordane-4	6.001	5.115	403.7E6	311.5E6	487.701	500.585
27)	Chlordane-5	6.837	6.009	65027237	126.7E6	492.093	496.824



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL072825\
Data File : PL096612.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 28 Jul 2025 20:30
Operator : AR\AJ
Sample : PCHLORICV500
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
ICVPL072825CHLOR

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 29 08:55:57 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL072825.M
Quant Title : GC Extractables
QLast Update : Tue Jul 29 08:54:31 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

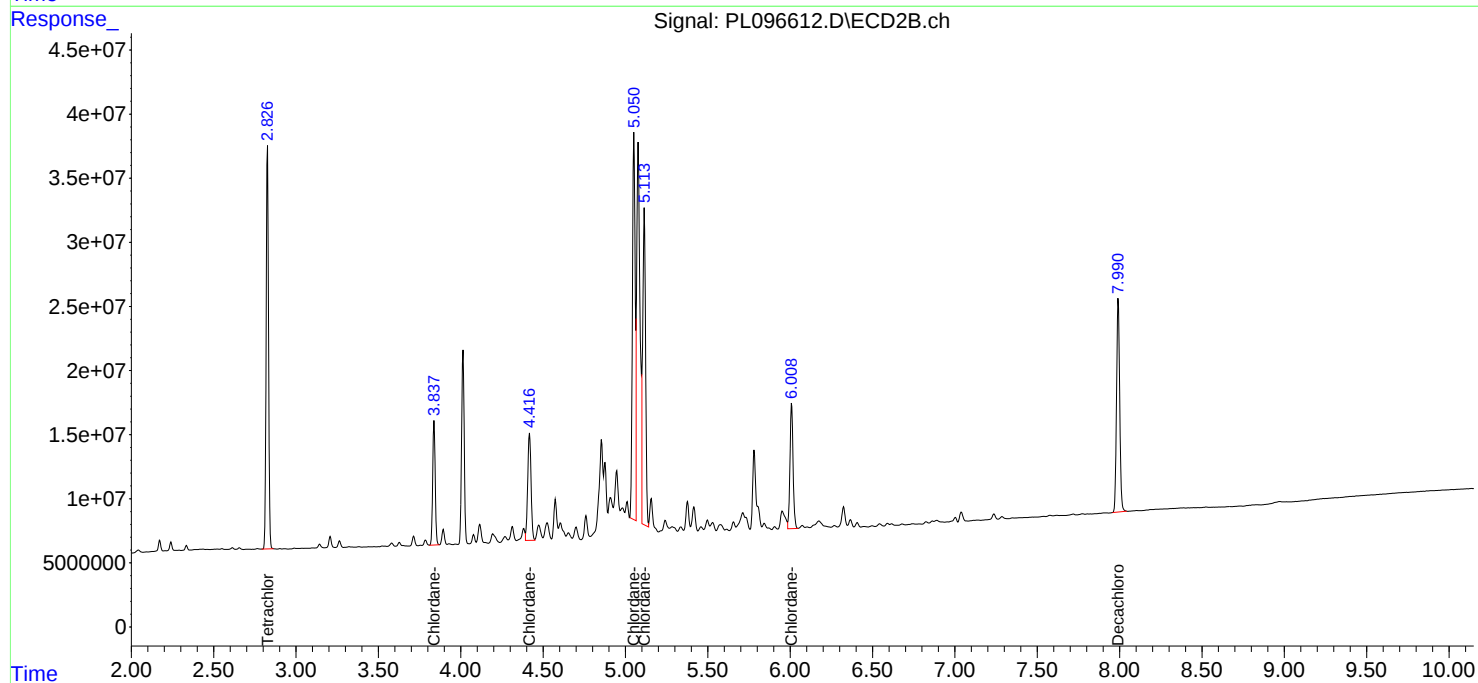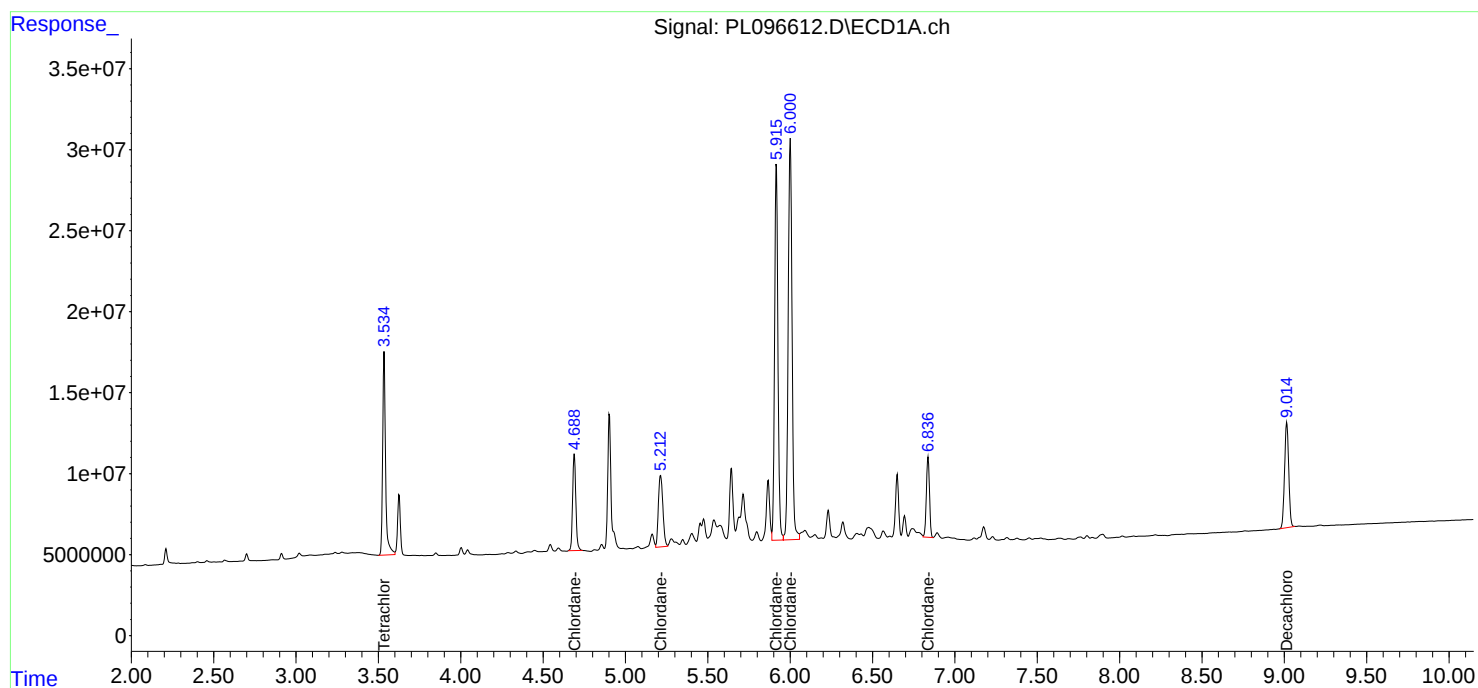


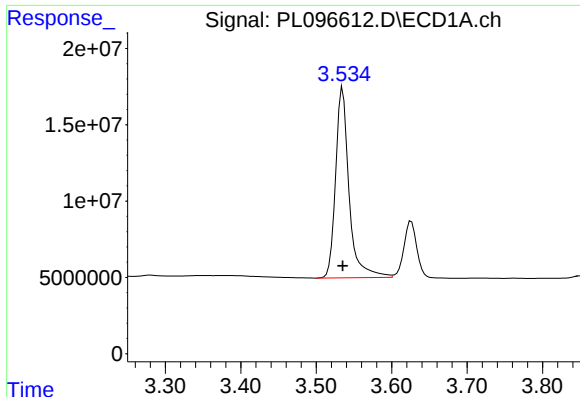

#1 Tetrachloro-m-xylene


R.T.: 3.535 min
Delta R.T.: 0.000 min
Response: 154829648
Conc: 47.87 ng/ml

Instrument :
ECD_L
ClientSampleId :
ICVPL072825CHLOR

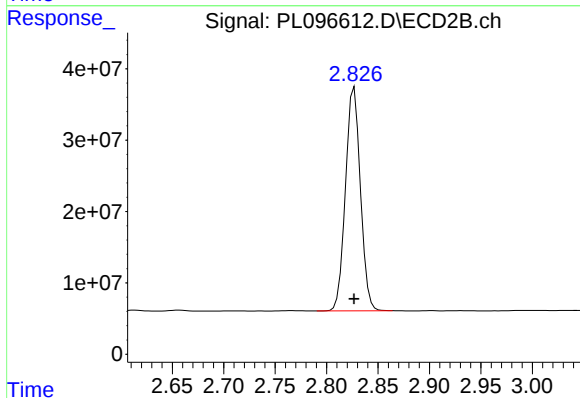


#1 Tetrachloro-m-xylene

R.T.: 2.827 min
Delta R.T.: 0.000 min
Response: 316660975
Conc: 49.97 ng/ml

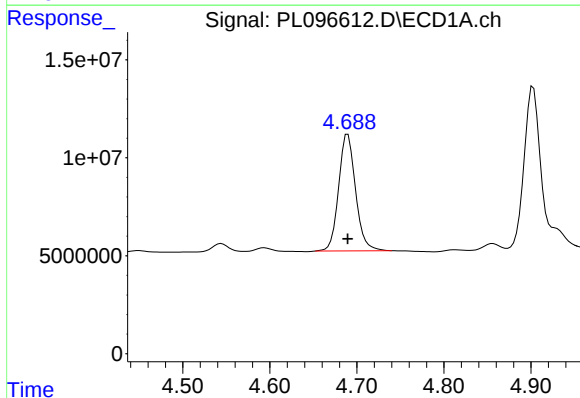


#23 Chlordane-1

R.T.: 4.690 min
Delta R.T.: 0.000 min
Response: 80607891
Conc: 473.85 ng/ml

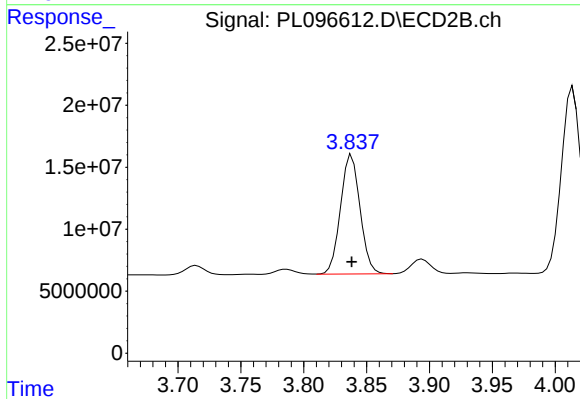

#23 Chlordane-1


R.T.: 3.838 min
Delta R.T.: 0.000 min
Response: 104002133
Conc: 496.10 ng/ml

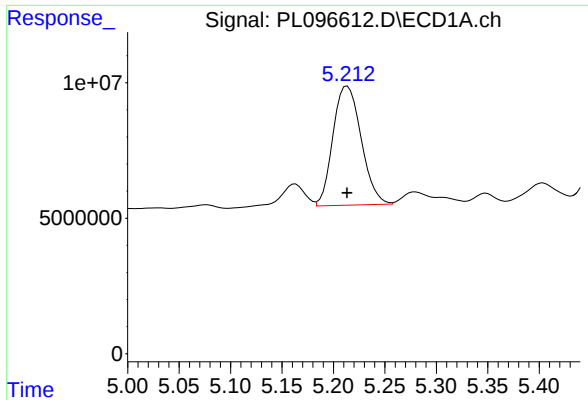

#24 Chlordane-2


R.T.: 5.213 min
Delta R.T.: 0.000 min
Response: 83986656
Conc: 479.90 ng/ml

Instrument :
ECD_L
ClientSampleId :
ICVPL072825CHLOR

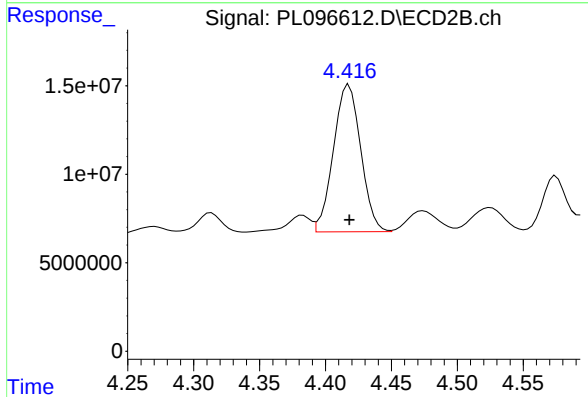


#24 Chlordane-2

R.T.: 4.418 min
Delta R.T.: 0.000 min
Response: 119863951
Conc: 494.10 ng/ml

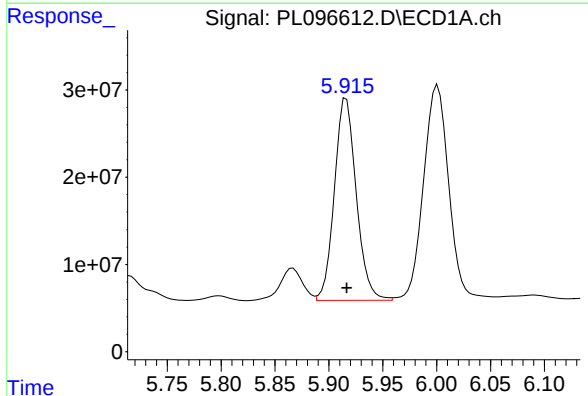


#25 Chlordane-3

R.T.: 5.916 min
Delta R.T.: 0.000 min
Response: 326602022
Conc: 488.97 ng/ml

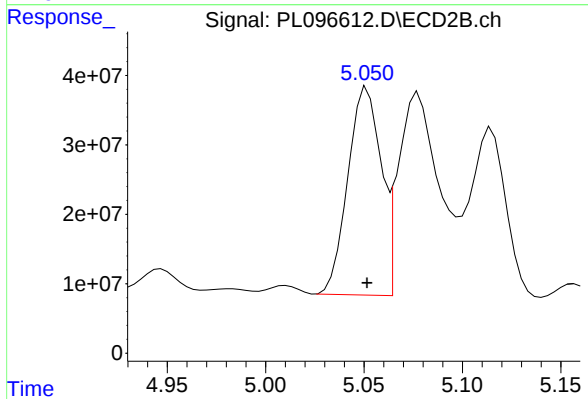

#25 Chlordane-3


R.T.: 5.052 min
Delta R.T.: 0.000 min
Response: 349986593
Conc: 503.36 ng/ml

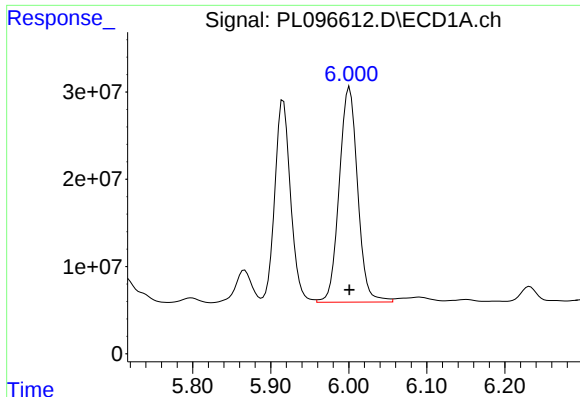

#26 Chlordane-4


R.T.: 6.001 min
Delta R.T.: 0.000 min
Response: 403669451
Conc: 487.70 ng/ml

Instrument :
ECD_L
ClientSampleId :
ICVPL072825CHLOR

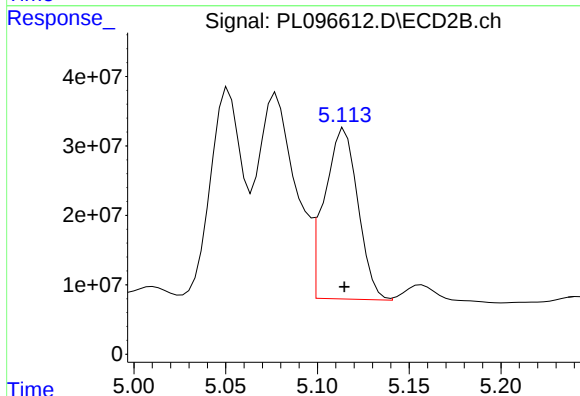


#26 Chlordane-4

R.T.: 5.115 min
Delta R.T.: 0.000 min
Response: 311530448
Conc: 500.59 ng/ml

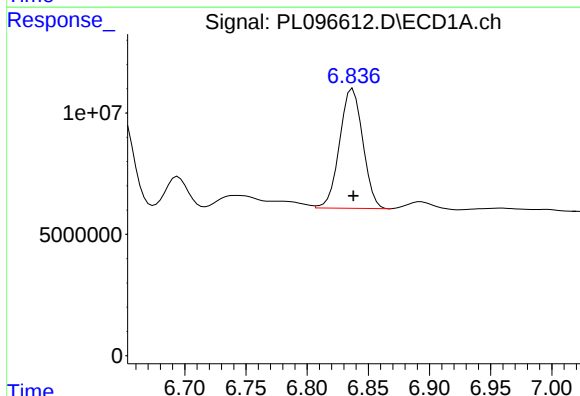


#27 Chlordane-5

R.T.: 6.837 min
Delta R.T.: 0.000 min
Response: 65027237
Conc: 492.09 ng/ml

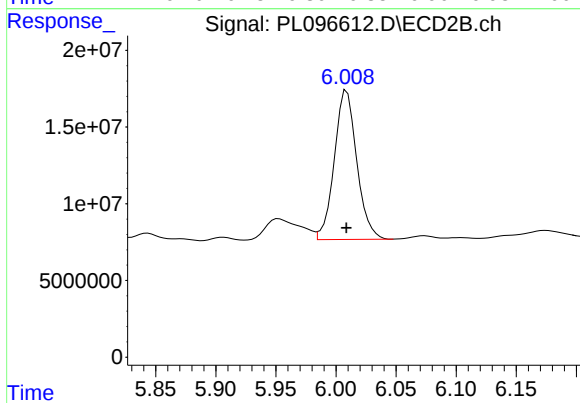

#27 Chlordane-5


R.T.: 6.009 min
Delta R.T.: 0.000 min
Response: 126745801
Conc: 496.82 ng/ml

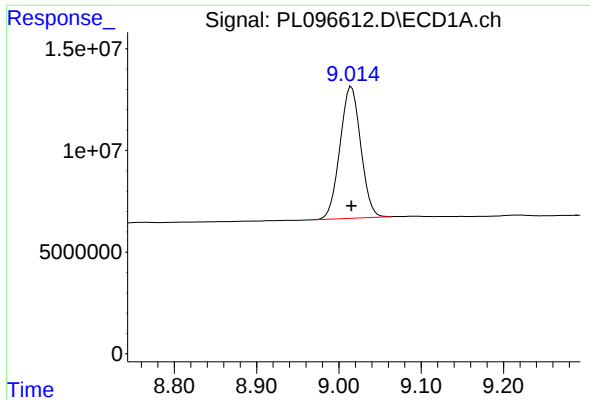

#28 Decachlorobiphenyl

R.T.: 9.015 min
Delta R.T.: 0.000 min
Response: 113455606
Conc: 47.15 ng/ml

Instrument :
ECD_L
ClientSampleId :
ICVPL072825CHLOR

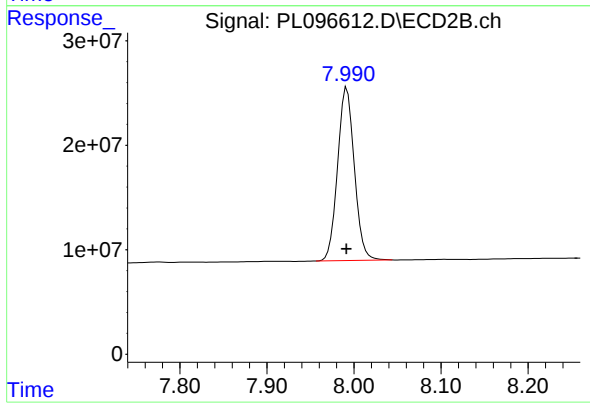

#28 Decachlorobiphenyl

R.T.: 7.992 min
Delta R.T.: 0.000 min
Response: 222009738
Conc: 49.45 ng/ml