
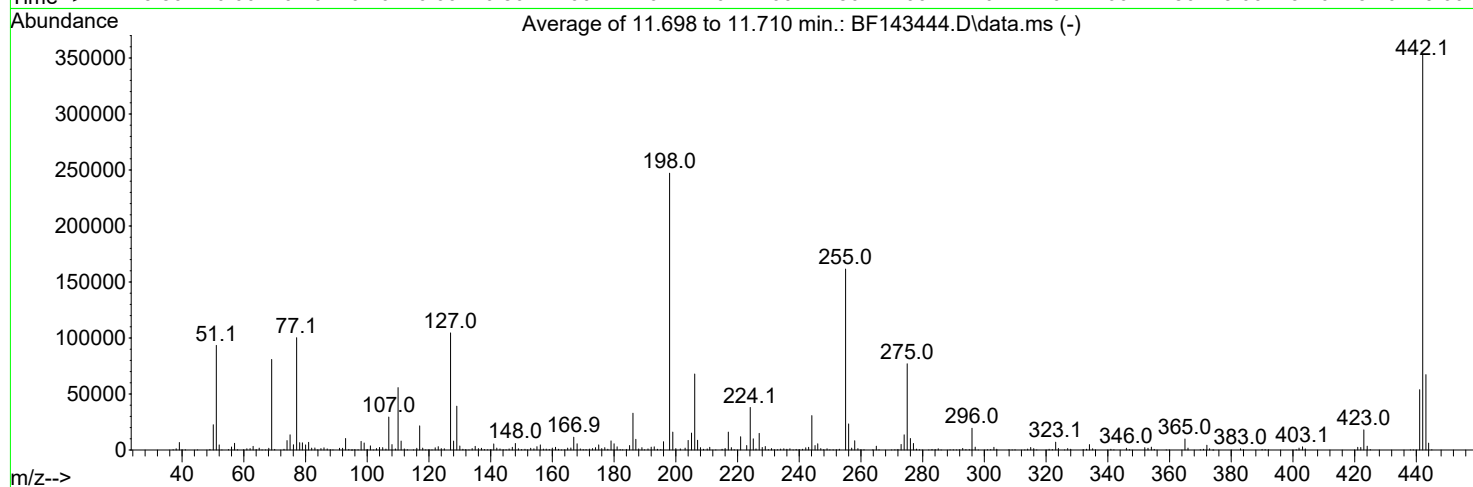


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF081925\
Data File : BF143444.D
Acq On : 19 Aug 2025 08:39
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF081525.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Mon Aug 18 04:40:19 2025

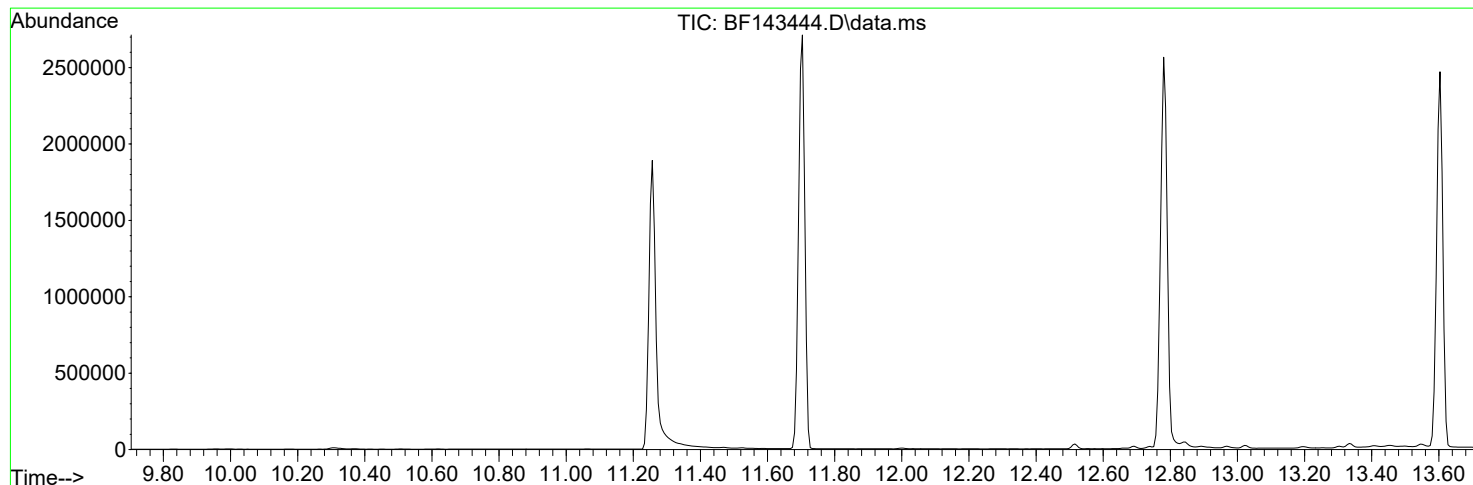

AutoFind: Scans 1616, 1617, 1618; Background Corrected with Scan 1609

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
68	69	0.00	2	1.9	1571	PASS
69	69	100	100	100.0	80784	PASS
70	69	0.00	2	0.7	567	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	247168	PASS
199	198	5	9	6.5	16017	PASS
365	198	1	100	4.0	9857	PASS
441	443	0.01	150	80.1	53915	PASS
442	442	100	100	100.0	352491	PASS
443	442	15	24	19.1	67315	PASS

DDT Breakdown




Date	Instrument Name	DFTPP Data File
8/19/2025	BNA_F	<u>BF143444.D</u>
Compound Name	Response	Retention Time
DDT	634271	13.604
DDD	11218	13.333
DDE	3577	12.968
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
14795	649066	2.28

Instrument :
BNA_F
ClientSampleId :
DFTPP

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF081925\
Data File : BF143444.D
Acq On : 19 Aug 2025 08:39
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Aug 19 12:05:45 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF081525.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Aug 18 04:40:19 2025
Response via : Initial Calibration

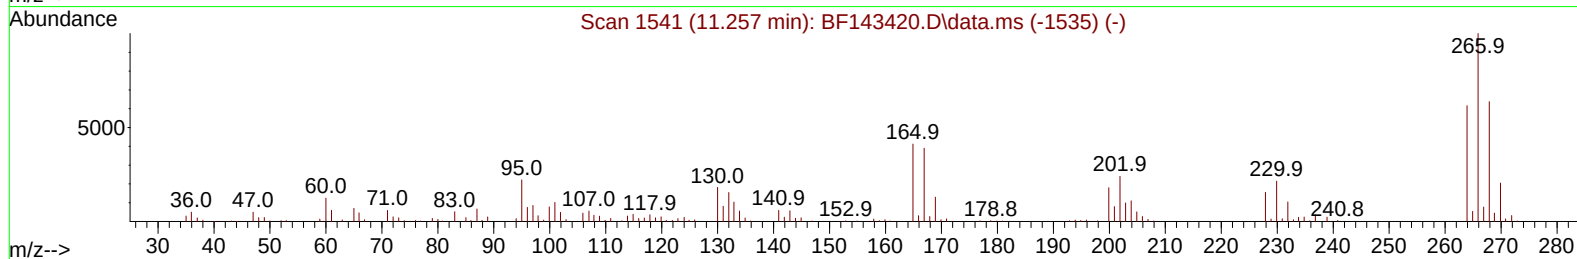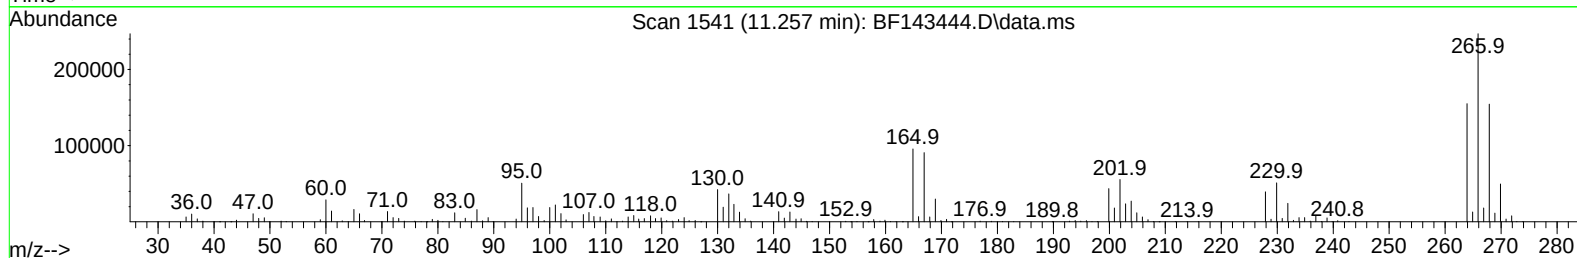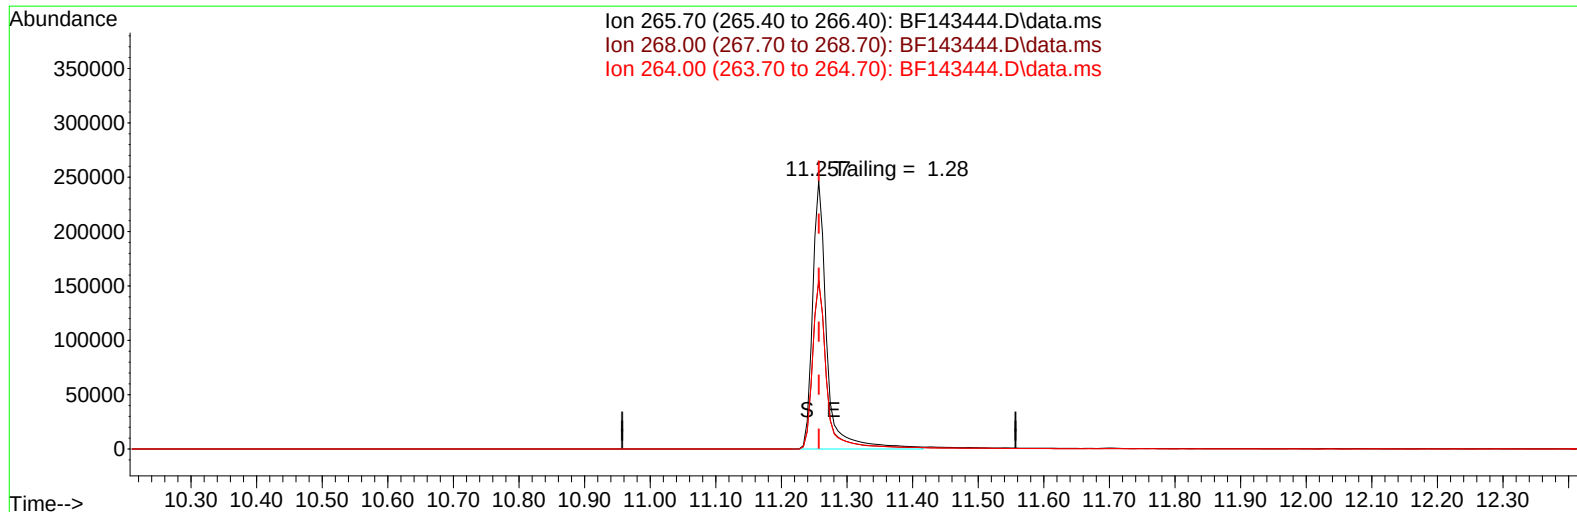

TIC: BF143444.D\data.ms

(70) Pentachlorophenol (C)

11.257min (-0.000) 503335.09 ng




response 372359

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.80	62.61
264.00	61.60	62.87
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF081925\
Data File : BF143444.D
Acq On : 19 Aug 2025 08:39
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Aug 19 12:05:45 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF081525.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Aug 18 04:40:19 2025
Response via : Initial Calibration

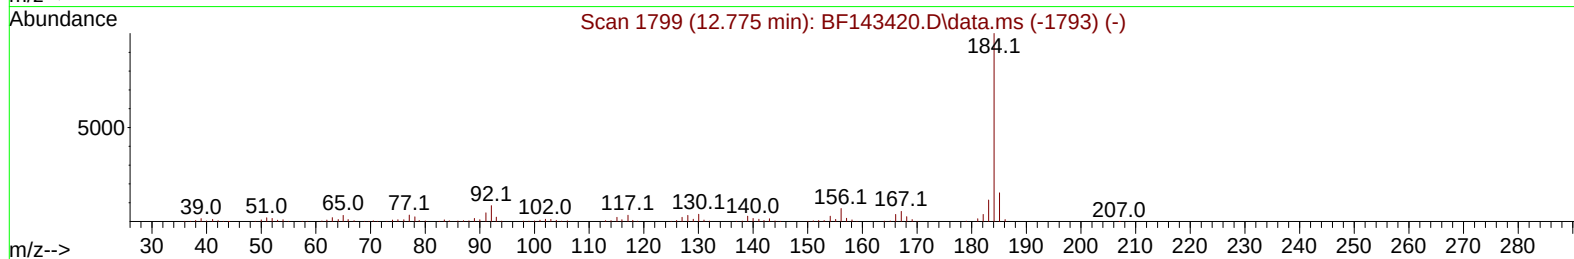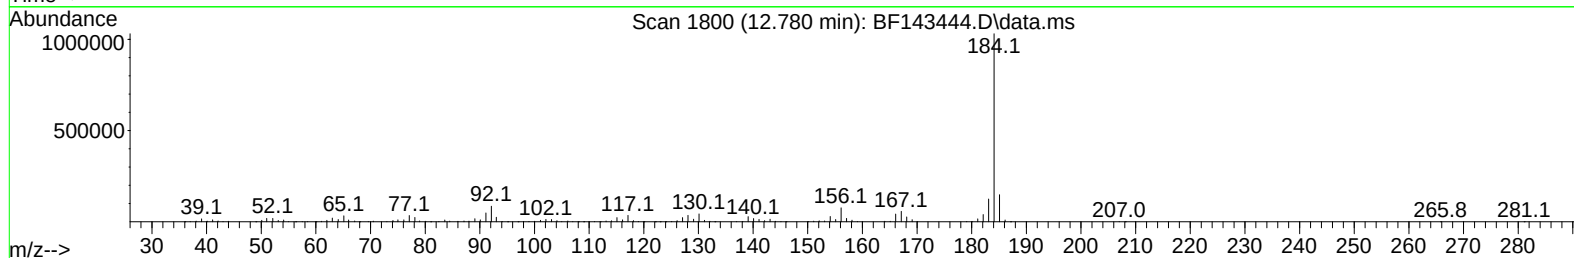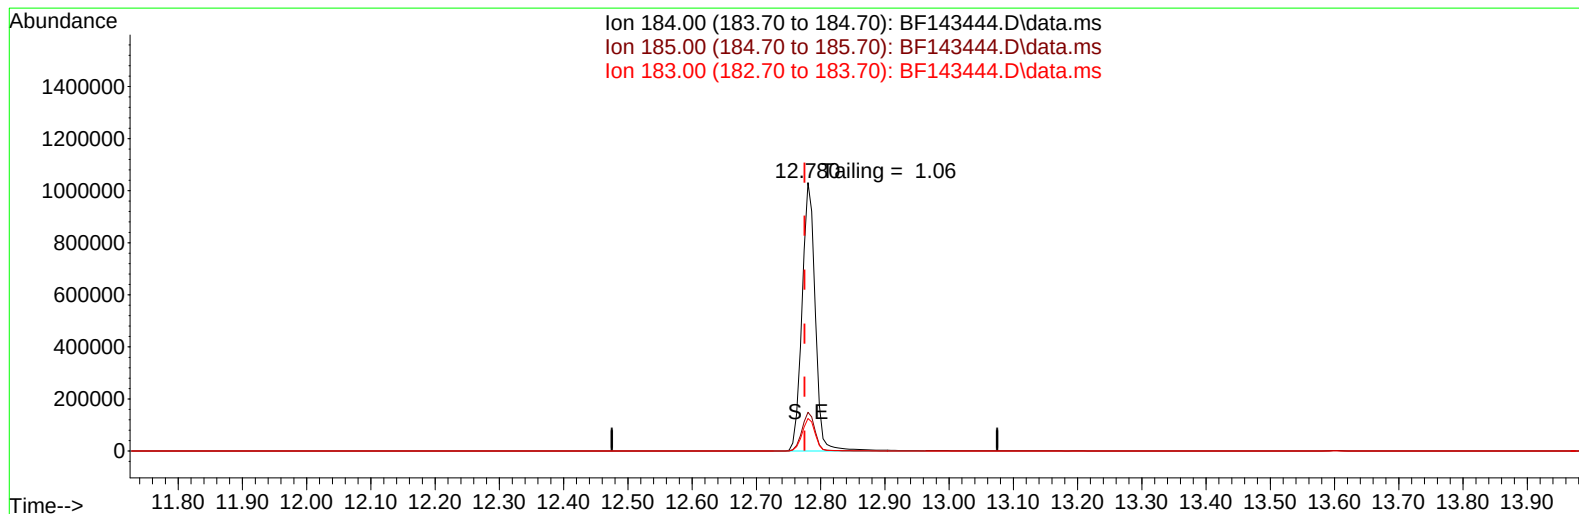

TIC: BF143444.D\data.ms

(77) Benzidine

12.780min (+ 0.005) 257789.28 ng

response 1485742

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.20	14.41
183.00	11.50	12.11
0.00	0.00	0.00