

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF081925\
 Data File : BF143446.D
 Acq On : 19 Aug 2025 10:05
 Operator : RC/JU
 Sample : PB169285BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 PB169285BL

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF081525.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BF143446.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	2.316	9	21	30	rVB	44728	80833	1.84%	0.301%
2	5.175	501	507	519	rBV	247929	402429	9.15%	1.496%
3	5.569	568	574	595	rBV	2639986	3603523	81.91%	13.399%
4	6.557	736	742	774	rBV	2521136	3637783	82.69%	13.526%
5	6.928	799	805	810	rBV	624215	788837	17.93%	2.933%
6	7.481	893	899	916	rBV	1716007	2495780	56.73%	9.280%
7	8.204	1017	1022	1041	rBV	771395	1043576	23.72%	3.880%
8	9.281	1198	1205	1210	rBV	3332665	4399230	100.00%	16.358%
9	9.957	1315	1320	1338	rBV	890475	1194857	27.16%	4.443%
10	10.751	1449	1455	1486	rBV	1884942	2643421	60.09%	9.829%
11	11.445	1568	1573	1590	rBV	899836	1178559	26.79%	4.382%
12	13.027	1836	1842	1859	rBV	2936646	3864203	87.84%	14.368%
13	14.086	2017	2022	2033	rBV	469440	652979	14.84%	2.428%
14	15.574	2269	2275	2291	rBV	377208	672130	15.28%	2.499%
15	17.292	2559	2567	2587	rVB4	50286	235727	5.36%	0.877%




Sum of corrected areas: 26893867

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF081925\
Data File : BF143446.D
Acq On : 19 Aug 2025 10:05
Operator : RC/JU
Sample : PB169285BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB169285BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF081525.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

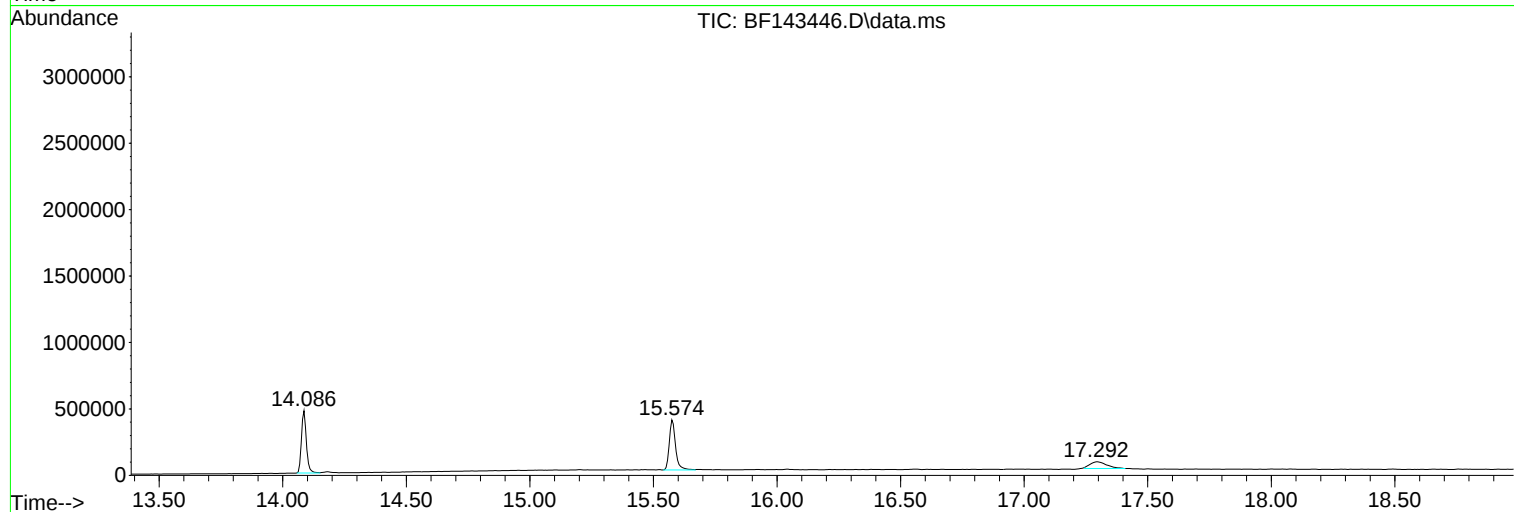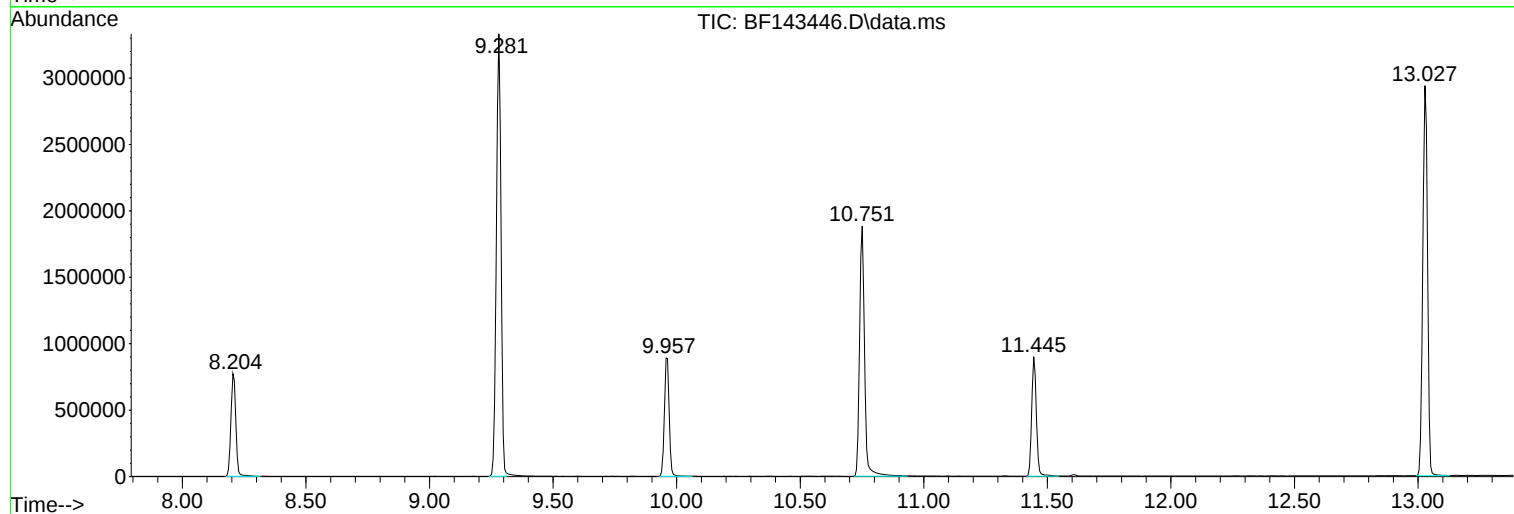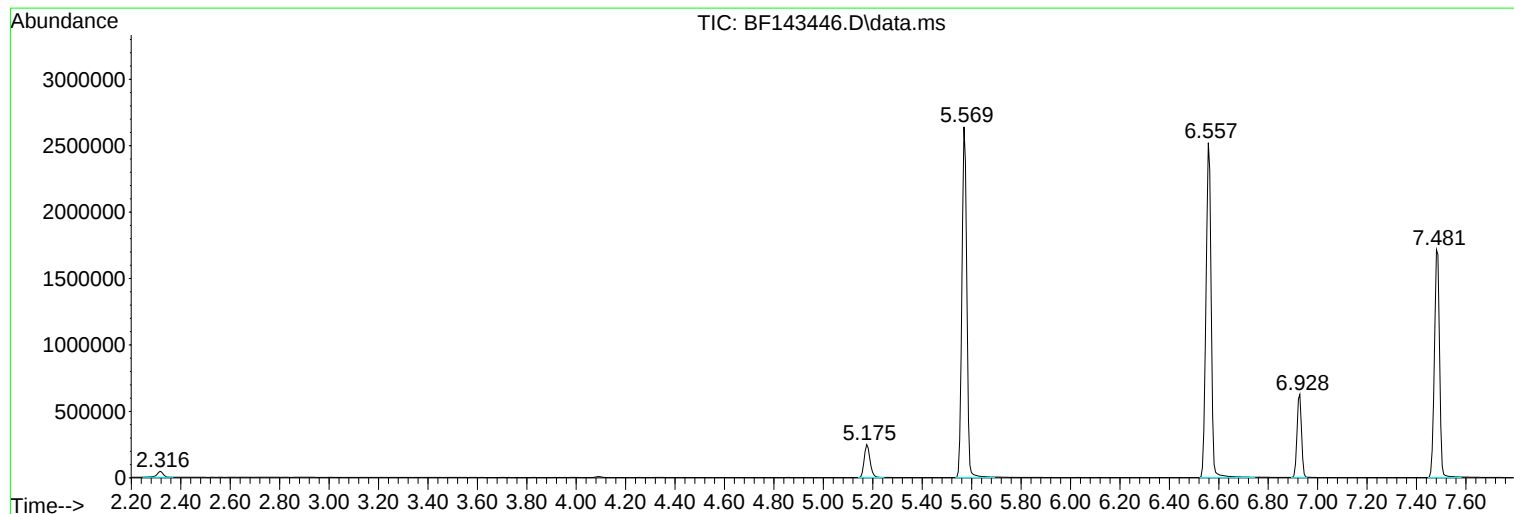

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF081925\
Data File : BF143446.D
Acq On : 19 Aug 2025 10:05
Operator : RC/JU
Sample : PB169285BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB169285BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF081525.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF081925\
Data File : BF143446.D
Acq On : 19 Aug 2025 10:05
Operator : RC/JU
Sample : PB169285BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB169285BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF081525.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------