

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF081925\
 Data File : BF143451.D
 Acq On : 19 Aug 2025 12:33
 Operator : RC/JU
 Sample : Q2879-01
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 OU4-TS-GRILLO-TSCP03-081425

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF081525.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BF143451.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	2.240	3	8	21	rVB	596671	973825	15.53%	2.135%
2	5.151	495	503	518	rBV	144753	231704	3.70%	0.508%
3	5.557	567	572	598	rBV	1372728	1900391	30.31%	4.167%
4	6.551	736	741	752	rBV	1283506	1752320	27.95%	3.842%
5	6.922	799	804	814	rBV	523240	671408	10.71%	1.472%
6	7.481	893	899	910	rBV	929419	1195154	19.06%	2.621%
7	8.204	1016	1022	1040	rVB	576101	757134	12.08%	1.660%
8	8.822	1113	1127	1136	rBV	98633	144564	2.31%	0.317%
9	9.275	1199	1204	1213	rBV	1446517	1848870	29.49%	4.054%
10	9.957	1315	1320	1333	rBV	532891	702888	11.21%	1.541%
11	10.669	1436	1441	1447	rBV	67221	91451	1.46%	0.201%
12	10.745	1449	1454	1470	rVB	670203	918597	14.65%	2.014%
13	11.445	1568	1573	1580	rBV2	482658	740450	11.81%	1.624%
14	11.969	1658	1662	1674	rVV2	330391	596977	9.52%	1.309%
15	12.057	1675	1677	1684	rVV2	39409	68666	1.10%	0.151%
16	12.145	1688	1692	1701	rVB6	47904	85310	1.36%	0.187%
17	12.604	1766	1770	1775	rBV2	65207	109046	1.74%	0.239%
18	12.657	1775	1779	1784	rBV	252664	365777	5.83%	0.802%
19	12.757	1792	1796	1809	rVB2	92745	165005	2.63%	0.362%
20	12.886	1813	1818	1824	rVB	225156	323324	5.16%	0.709%
21	13.027	1836	1842	1850	rBV	1534413	2032151	32.42%	4.456%
22	13.392	1900	1904	1909	rBV3	95391	191691	3.06%	0.420%
23	13.463	1913	1916	1926	rVB3	138403	267193	4.26%	0.586%
24	13.933	1992	1996	2005	rVB2	238482	508489	8.11%	1.115%
25	14.086	2014	2022	2029	rBV2	779055	1447020	23.08%	3.173%
26	14.545	2096	2100	2102	rBV	379025	501616	8.00%	1.100%
27	14.933	2162	2166	2173	rVB	375669	533079	8.50%	1.169%
28	15.004	2175	2178	2186	rVB2	108410	154101	2.46%	0.338%
29	15.092	2189	2193	2197	rVV	129071	213378	3.40%	0.468%
30	15.145	2197	2202	2203	rVV	225850	364415	5.81%	0.799%
31	15.204	2207	2212	2217	rVV	1699181	2569342	40.98%	5.634%
32	15.251	2217	2220	2232	rVB2	196974	474195	7.56%	1.040%
33	15.580	2271	2276	2286	rVB	438632	790541	12.61%	1.733%
34	15.798	2309	2313	2319	rBV2	144803	237334	3.79%	0.520%
35	15.939	2334	2337	2348	rVB	137177	276841	4.42%	0.607%
36	16.045	2349	2355	2362	rVB	1208843	2146984	34.25%	4.708%

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF081925\
Data File : BF143451.D
Acq On : 19 Aug 2025 12:33
Operator : RC/JU
Sample : Q2879-01
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
OU4-TS-GRILLO-TSCP03-081425

Integration Parameters: rteint.p
Integrator: RTE
Smoothing : ON Filtering: 5
Sampling : 1 Min Area: 3 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF081525.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

37	16.327	2398	2403	2416	rVB2	370321	880427	14.04%	1.931%
38	17.480	2593	2599	2609	rBV4	203089	575022	9.17%	1.261%
39	17.762	2634	2647	2658	rBV4	1549372	6268994	100.00%	13.747%
40	17.939	2672	2677	2684	rVB	484407	1083549	17.28%	2.376%
41	18.209	2715	2723	2732	rBV	1012197	3572115	56.98%	7.833%
42	18.303	2734	2739	2752	rVB5	773507	2491324	39.74%	5.463%
43	18.580	2776	2786	2804	rBV6	754922	4381341	69.89%	9.607%


Sum of corrected areas: 45604003

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF081925\
Data File : BF143451.D
Acq On : 19 Aug 2025 12:33
Operator : RC/JU
Sample : Q2879-01
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
OU4-TS-GRILLO-TSCP03-081425

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF081525.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

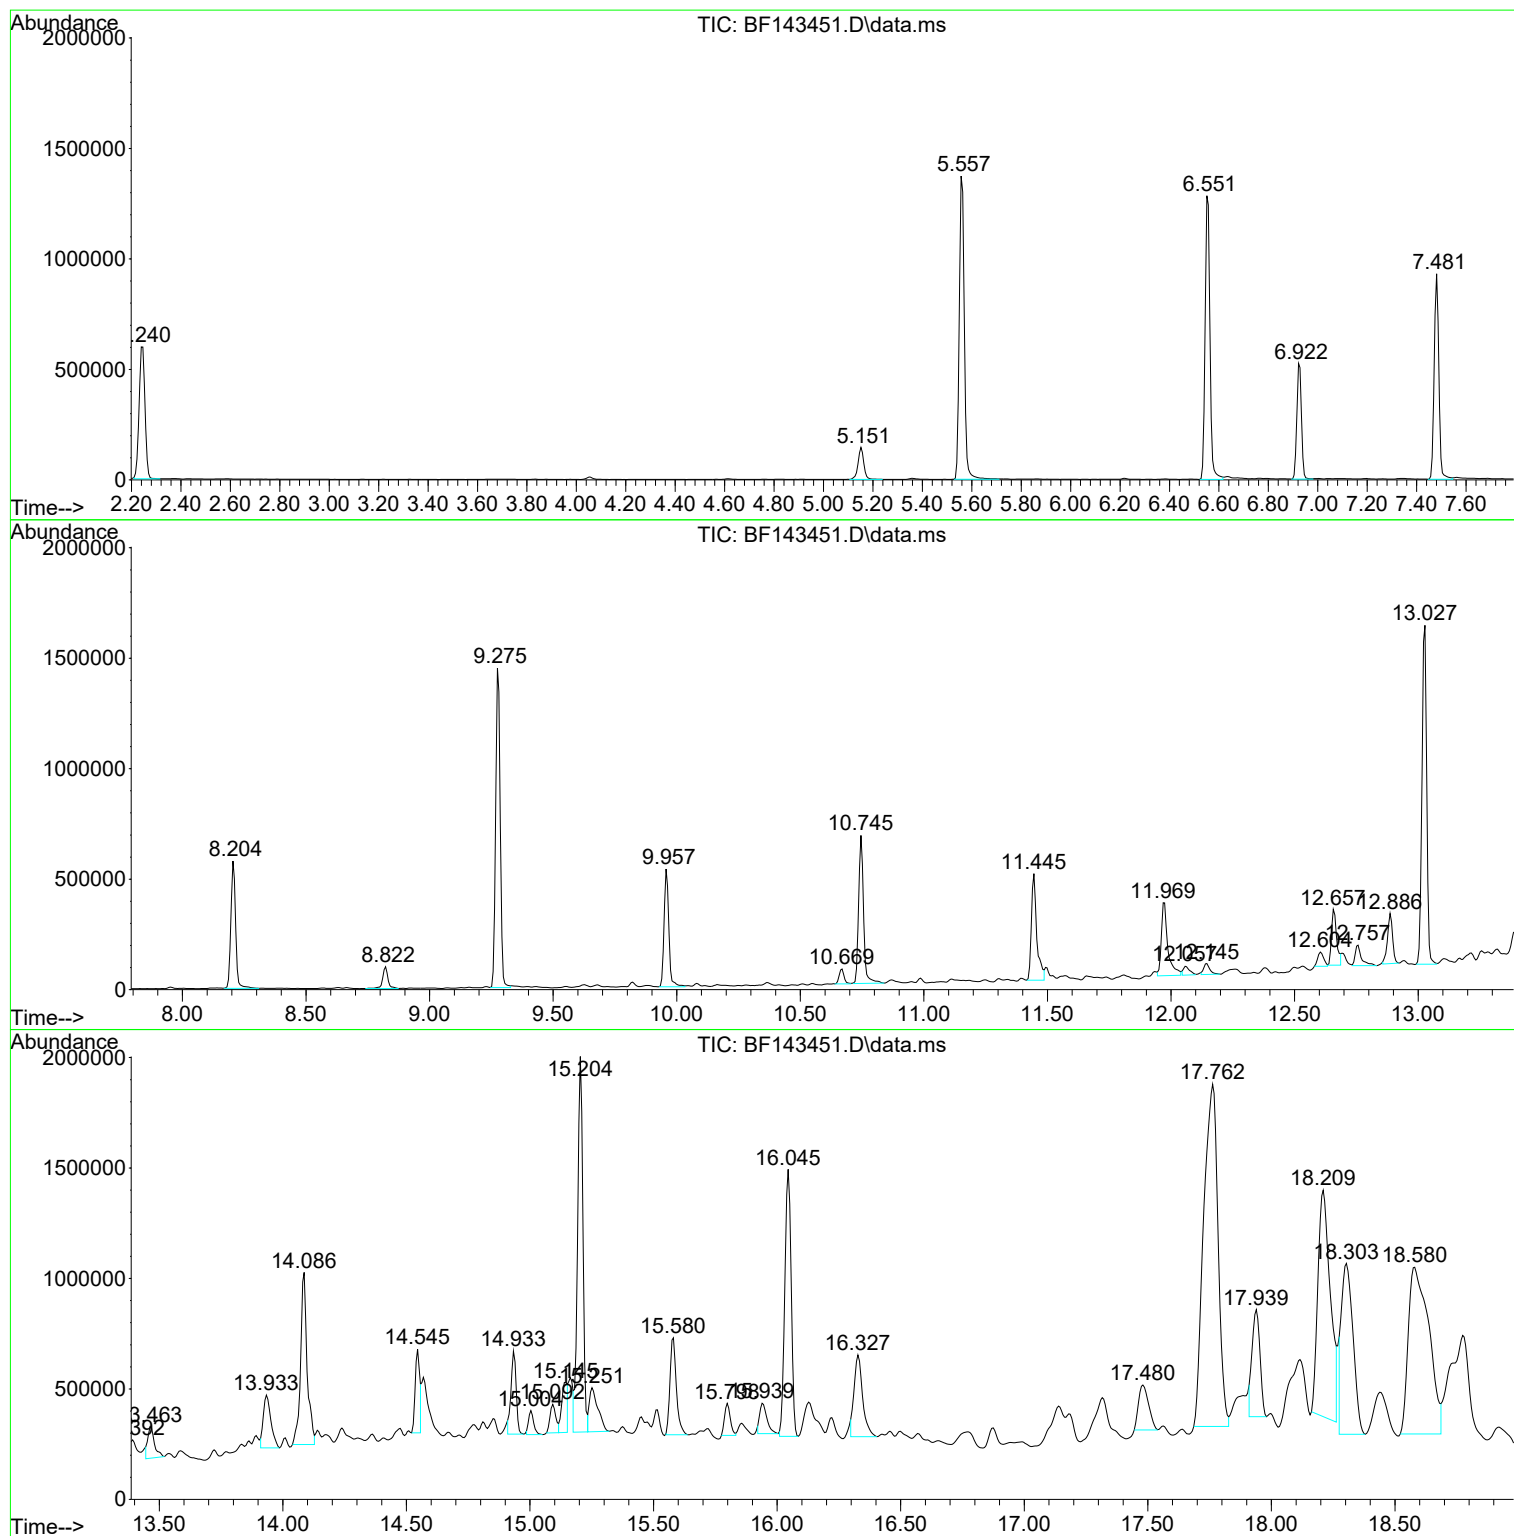

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF081925\
Data File : BF143451.D
Acq On : 19 Aug 2025 12:33
Operator : RC/JU
Sample : Q2879-01
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
OU4-TS-GRILLO-TSCP03-081425

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF081525.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF081925\
Data File : BF143451.D
Acq On : 19 Aug 2025 12:33
Operator : RC/JU
Sample : Q2879-01
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
OU4-TS-GRILLO-TSCP03-081425

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF081525.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------