

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF081925\
 Data File : BF143452.D
 Acq On : 19 Aug 2025 13:01
 Operator : RC/JU
 Sample : Q2879-03
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 OU4-TS-GRILLO-TSCP04-081425

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF081525.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BF143452.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	2.240	3	8	18	rVB	581282	912463	21.72%	2.523%
2	5.151	491	503	516	rVB	146068	230920	5.50%	0.638%
3	5.563	567	573	590	rBV	1352102	1872685	44.58%	5.177%
4	6.557	736	742	754	rBV	1325695	1764276	42.00%	4.878%
5	6.928	800	805	813	rBV	522110	672911	16.02%	1.860%
6	7.481	893	899	910	rBV	963937	1236892	29.44%	3.420%
7	8.204	1014	1022	1030	rBV	554644	715381	17.03%	1.978%
8	9.275	1199	1204	1213	rBV	1436820	1844204	43.90%	5.099%
9	9.622	1256	1263	1269	rBV5	21501	47787	1.14%	0.132%
10	9.822	1292	1297	1302	rBV	34928	50044	1.19%	0.138%
11	9.957	1315	1320	1325	rBV	514024	657908	15.66%	1.819%
12	10.669	1436	1441	1447	rBV	120308	163271	3.89%	0.451%
13	10.745	1449	1454	1470	rVB	758238	1022035	24.33%	2.826%
14	10.869	1470	1475	1482	rBV4	24045	49544	1.18%	0.137%
15	10.980	1490	1494	1499	rVB2	50800	71050	1.69%	0.196%
16	11.339	1552	1555	1561	rVB	28854	42391	1.01%	0.117%
17	11.445	1568	1573	1576	rBV	514187	746782	17.78%	2.065%
18	11.674	1606	1612	1619	rBV4	22523	68747	1.64%	0.190%
19	11.969	1653	1662	1673	rBV3	390315	792590	18.87%	2.191%
20	12.057	1674	1677	1680	rBV	69538	98183	2.34%	0.271%
21	12.145	1688	1692	1697	rBV5	67420	103816	2.47%	0.287%
22	12.498	1748	1752	1755	rBV	121276	179388	4.27%	0.496%
23	12.592	1764	1768	1775	rVB3	86865	163165	3.88%	0.451%
24	12.657	1775	1779	1784	rBV	383122	562320	13.39%	1.555%
25	12.757	1792	1796	1800	rBV	99820	144469	3.44%	0.399%
26	12.886	1813	1818	1825	rBV	412022	583833	13.90%	1.614%
27	13.027	1837	1842	1850	rVB	1592604	2054952	48.92%	5.681%
28	13.251	1877	1880	1884	rBV	75571	112392	2.68%	0.311%
29	13.321	1889	1892	1898	rVB2	77393	111423	2.65%	0.308%
30	13.927	1992	1995	2005	rVB2	478342	867403	20.65%	2.398%
31	14.086	2016	2022	2030	rBV2	800503	1606216	38.23%	4.441%
32	14.545	2096	2100	2117	rVB2	395966	1065940	25.37%	2.947%
33	14.933	2163	2166	2172	rVB	248857	334124	7.95%	0.924%
34	15.139	2197	2201	2204	rBV	296755	510702	12.16%	1.412%
35	15.204	2208	2212	2216	rVB	1286555	1756468	41.81%	4.856%
36	15.515	2262	2265	2270	rVB	172224	245903	5.85%	0.680%

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF081925\
Data File : BF143452.D
Acq On : 19 Aug 2025 13:01
Operator : RC/JU
Sample : Q2879-03
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
OU4-TS-GRILLO-TSCP04-081425

Integration Parameters: rteint.p
Integrator: RTE
Smoothing : ON Filtering: 5
Sampling : 1 Min Area: 3 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF081525.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

37	15.580	2271	2276	2292	rVV2	373476	709475	16.89%	1.961%
38	16.045	2349	2355	2361	rVB	931321	1609301	38.31%	4.449%
39	16.321	2399	2402	2417	rVB2	296373	666242	15.86%	1.842%
40	17.751	2633	2645	2657	rBV4	1083339	4200945	100.00%	11.614%
41	17.939	2672	2677	2684	rVB	355747	783984	18.66%	2.167%
42	18.198	2714	2721	2731	rBV	653907	2213197	52.68%	6.119%
43	18.568	2776	2784	2802	rBV9	447809	2524626	60.10%	6.980%


Sum of corrected areas: 36170348

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF081925\
Data File : BF143452.D
Acq On : 19 Aug 2025 13:01
Operator : RC/JU
Sample : Q2879-03
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
OU4-TS-GRILLO-TSCP04-081425

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF081525.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

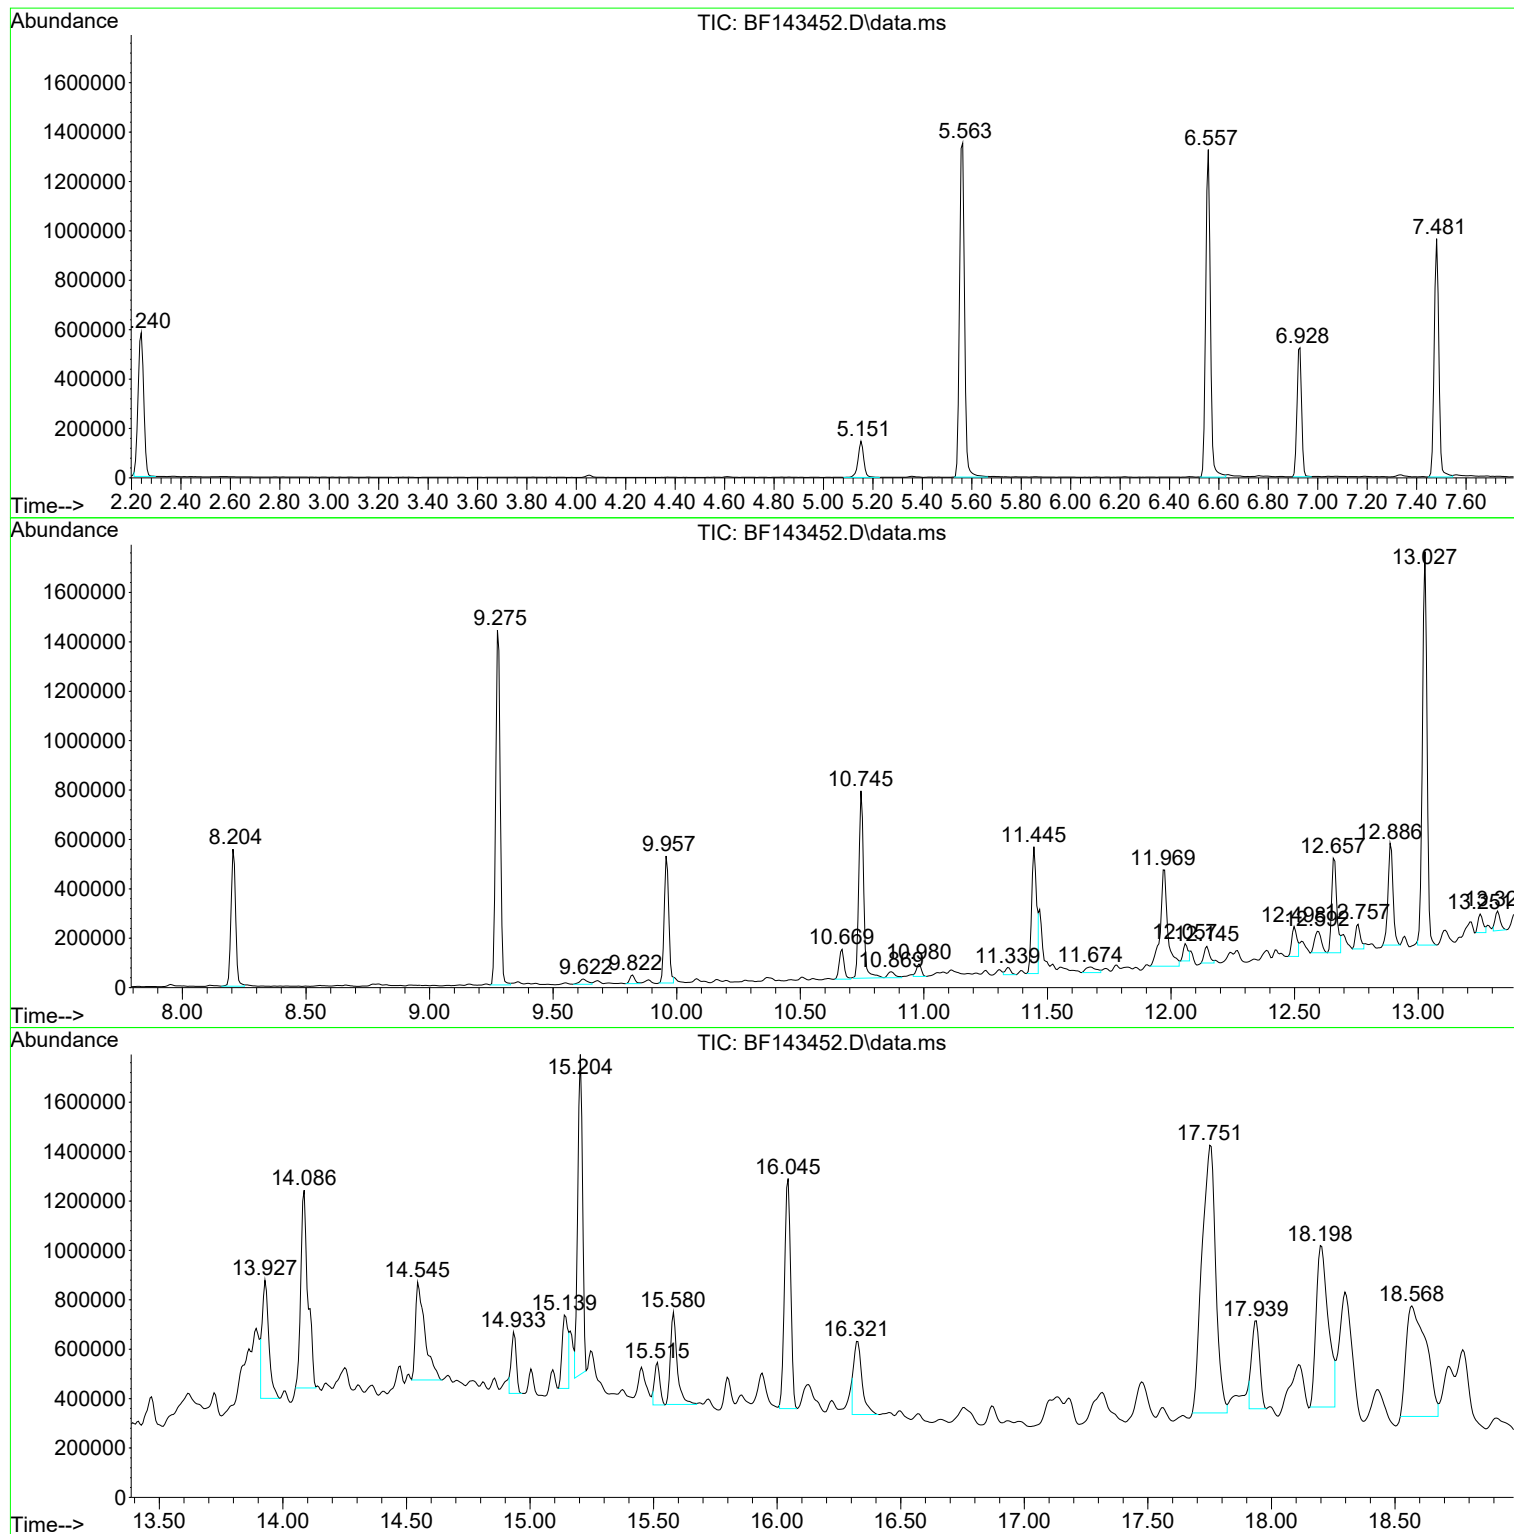

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF081925\
Data File : BF143452.D
Acq On : 19 Aug 2025 13:01
Operator : RC/JU
Sample : Q2879-03
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
OU4-TS-GRILLO-TSCP04-081425

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF081525.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF081925\
Data File : BF143452.D
Acq On : 19 Aug 2025 13:01
Operator : RC/JU
Sample : Q2879-03
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
OU4-TS-GRILLO-TSCP04-081425

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF081525.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------