

Data Path : Z:\svoasrv\HPCHEM1\BNA\_F\Data\BF081925\  
 Data File : BF143453.D  
 Acq On : 19 Aug 2025 13:30  
 Operator : RC/JU  
 Sample : Q2879-05  
 Misc :  
 ALS Vial : 10 Sample Multiplier: 1

Instrument :  
 BNA\_F  
 ClientSampleId :  
 OU4-TS-GRILLO-TSCP05-081425

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA\_F\Methods\8270-BF081525.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BF143453.D\data.ms

| peak<br># | R.T.<br>min | first<br>scan | max<br>scan | last<br>scan | PK<br>TY | peak<br>height | corr.<br>area | corr.<br>% max. | % of<br>total |
|-----------|-------------|---------------|-------------|--------------|----------|----------------|---------------|-----------------|---------------|
| 1         | 2.228       | 3             | 6           | 15           | rVB      | 509327         | 749943        | 16.15%          | 2.069%        |
| 2         | 5.151       | 495           | 503         | 515          | rVB      | 114410         | 177613        | 3.83%           | 0.490%        |
| 3         | 5.563       | 567           | 573         | 592          | rBV      | 1072618        | 1488914       | 32.07%          | 4.109%        |
| 4         | 6.557       | 737           | 742         | 753          | rBV      | 1049338        | 1370329       | 29.51%          | 3.781%        |
| 5         | 6.928       | 799           | 805         | 815          | rBV      | 436306         | 554083        | 11.93%          | 1.529%        |
| 6         | 7.481       | 893           | 899         | 909          | rBV      | 740696         | 949587        | 20.45%          | 2.620%        |
| 7         | 8.204       | 1015          | 1022        | 1030         | rBV      | 494183         | 646267        | 13.92%          | 1.783%        |
| 8         | 9.275       | 1199          | 1204        | 1213         | rBV      | 1157105        | 1477787       | 31.83%          | 4.078%        |
| 9         | 9.957       | 1315          | 1320        | 1325         | rBV      | 482565         | 630654        | 13.58%          | 1.740%        |
| 10        | 10.257      | 1366          | 1371        | 1381         | rBV      | 137126         | 181251        | 3.90%           | 0.500%        |
| 11        | 10.669      | 1436          | 1441        | 1447         | rBV      | 130793         | 179643        | 3.87%           | 0.496%        |
| 12        | 10.745      | 1449          | 1454        | 1460         | rBV      | 715802         | 951403        | 20.49%          | 2.625%        |
| 13        | 10.804      | 1460          | 1464        | 1469         | rVB2     | 31822          | 62704         | 1.35%           | 0.173%        |
| 14        | 10.980      | 1490          | 1494        | 1499         | rVB2     | 51168          | 72616         | 1.56%           | 0.200%        |
| 15        | 11.445      | 1568          | 1573        | 1580         | rBV2     | 548138         | 972187        | 20.94%          | 2.683%        |
| 16        | 11.580      | 1592          | 1596        | 1600         | rVB      | 157920         | 193896        | 4.18%           | 0.535%        |
| 17        | 11.675      | 1607          | 1612        | 1619         | rBV2     | 29401          | 54342         | 1.17%           | 0.150%        |
| 18        | 11.974      | 1658          | 1663        | 1674         | rVV3     | 425409         | 720642        | 15.52%          | 1.989%        |
| 19        | 12.063      | 1674          | 1678        | 1685         | rVB      | 54345          | 95937         | 2.07%           | 0.265%        |
| 20        | 12.145      | 1689          | 1692        | 1697         | rVB3     | 56039          | 81367         | 1.75%           | 0.225%        |
| 21        | 12.498      | 1749          | 1752        | 1756         | rBV2     | 38894          | 59653         | 1.28%           | 0.165%        |
| 22        | 12.592      | 1764          | 1768        | 1775         | rBV2     | 101980         | 176260        | 3.80%           | 0.486%        |
| 23        | 12.663      | 1775          | 1780        | 1792         | rBV2     | 517454         | 1320409       | 28.44%          | 3.644%        |
| 24        | 12.757      | 1793          | 1796        | 1804         | rVB      | 108517         | 168471        | 3.63%           | 0.465%        |
| 25        | 12.886      | 1812          | 1818        | 1825         | rBV      | 390138         | 614658        | 13.24%          | 1.696%        |
| 26        | 13.027      | 1837          | 1842        | 1850         | rVB      | 1579782        | 2018731       | 43.48%          | 5.571%        |
| 27        | 13.392      | 1901          | 1904        | 1907         | rBV      | 73671          | 113384        | 2.44%           | 0.313%        |
| 28        | 13.463      | 1913          | 1916        | 1920         | rBV3     | 162541         | 239934        | 5.17%           | 0.662%        |
| 29        | 13.604      | 1936          | 1940        | 1945         | rBV2     | 432184         | 637923        | 13.74%          | 1.760%        |
| 30        | 13.927      | 1992          | 1995        | 2005         | rVB2     | 442765         | 734599        | 15.82%          | 2.027%        |
| 31        | 14.086      | 2017          | 2022        | 2030         | rVB2     | 730546         | 1242257       | 26.75%          | 3.428%        |
| 32        | 14.551      | 2096          | 2101        | 2118         | rVB3     | 492827         | 1172118       | 25.24%          | 3.234%        |
| 33        | 14.933      | 2163          | 2166        | 2172         | rVB      | 315827         | 430807        | 9.28%           | 1.189%        |
| 34        | 15.145      | 2198          | 2202        | 2203         | rBV      | 170229         | 233706        | 5.03%           | 0.645%        |
| 35        | 15.204      | 2208          | 2212        | 2216         | rVB      | 1340687        | 1835596       | 39.53%          | 5.065%        |
| 36        | 15.580      | 2271          | 2276        | 2291         | rBV      | 371184         | 729583        | 15.71%          | 2.013%        |

Data Path : Z:\svoasrv\HPCHEM1\BNA\_F\Data\BF081925\  
Data File : BF143453.D  
Acq On : 19 Aug 2025 13:30  
Operator : RC/JU  
Sample : Q2879-05  
Misc :  
ALS Vial : 10 Sample Multiplier: 1

Instrument :  
BNA\_F  
ClientSampleId :  
OU4-TS-GRILLO-TSCP05-081425

Integration Parameters: rteint.p  
Integrator: RTE  
Smoothing : ON Filtering: 5  
Sampling : 1 Min Area: 3 % of largest Peak  
Start Thrs: 0.2 Max Peaks: 100  
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >  
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA\_F\Methods\8270-BF081525.M  
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

|    |        |      |      |      |      |         |         |         |         |
|----|--------|------|------|------|------|---------|---------|---------|---------|
| 37 | 16.045 | 2349 | 2355 | 2361 | rVB  | 1028034 | 1777601 | 38.28%  | 4.905%  |
| 38 | 16.327 | 2399 | 2403 | 2417 | rVB2 | 339007  | 727476  | 15.67%  | 2.007%  |
| 39 | 17.756 | 2632 | 2646 | 2656 | rBV4 | 1108848 | 4643323 | 100.00% | 12.813% |
| 40 | 17.933 | 2672 | 2676 | 2684 | rVB  | 336550  | 733344  | 15.79%  | 2.024%  |
| 41 | 18.198 | 2714 | 2721 | 2731 | rBV  | 632382  | 2122680 | 45.71%  | 5.858%  |
| 42 | 18.562 | 2775 | 2783 | 2802 | rBV7 | 515791  | 2894409 | 62.33%  | 7.987%  |




Sum of corrected areas: 36238087

Data Path : Z:\svoasrv\HPCHEM1\BNA\_F\Data\BF081925\  
Data File : BF143453.D  
Acq On : 19 Aug 2025 13:30  
Operator : RC/JU  
Sample : Q2879-05  
Misc :  
ALS Vial : 10 Sample Multiplier: 1

Instrument :  
BNA\_F  
ClientSampleId :  
OU4-TS-GRILLO-TSCP05-081425

Quant Method : Z:\svoasrv\HPCHEM1\BNA\_F\Methods\8270-BF081525.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L  
TIC Integration Parameters: LSCINT.P

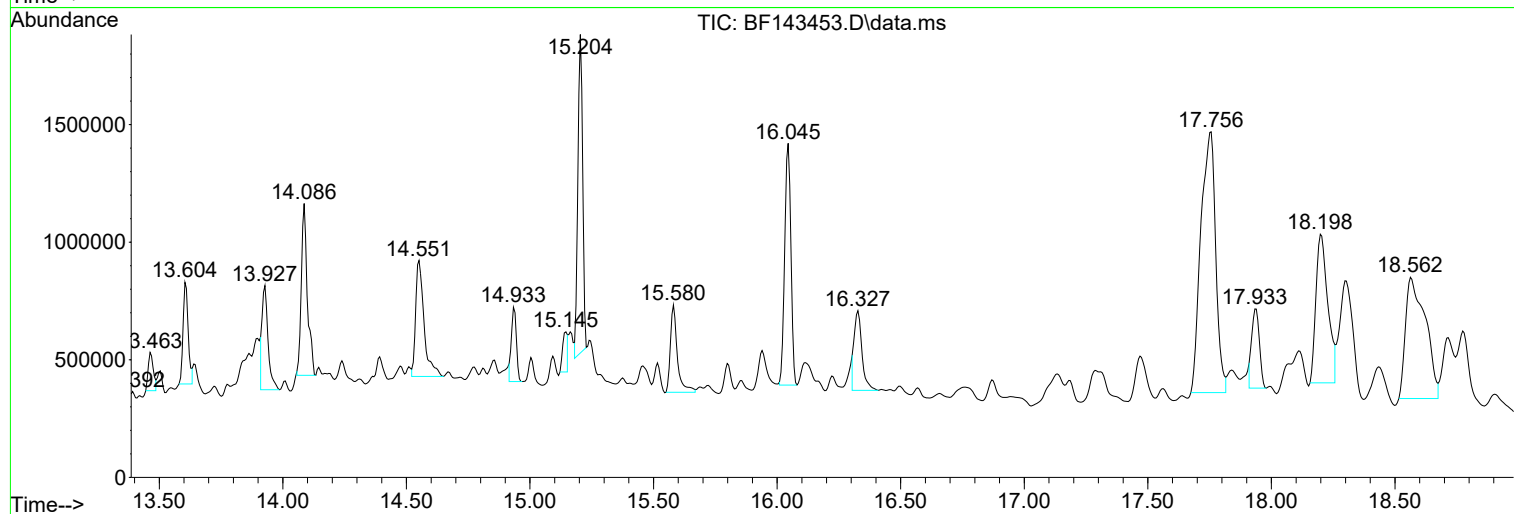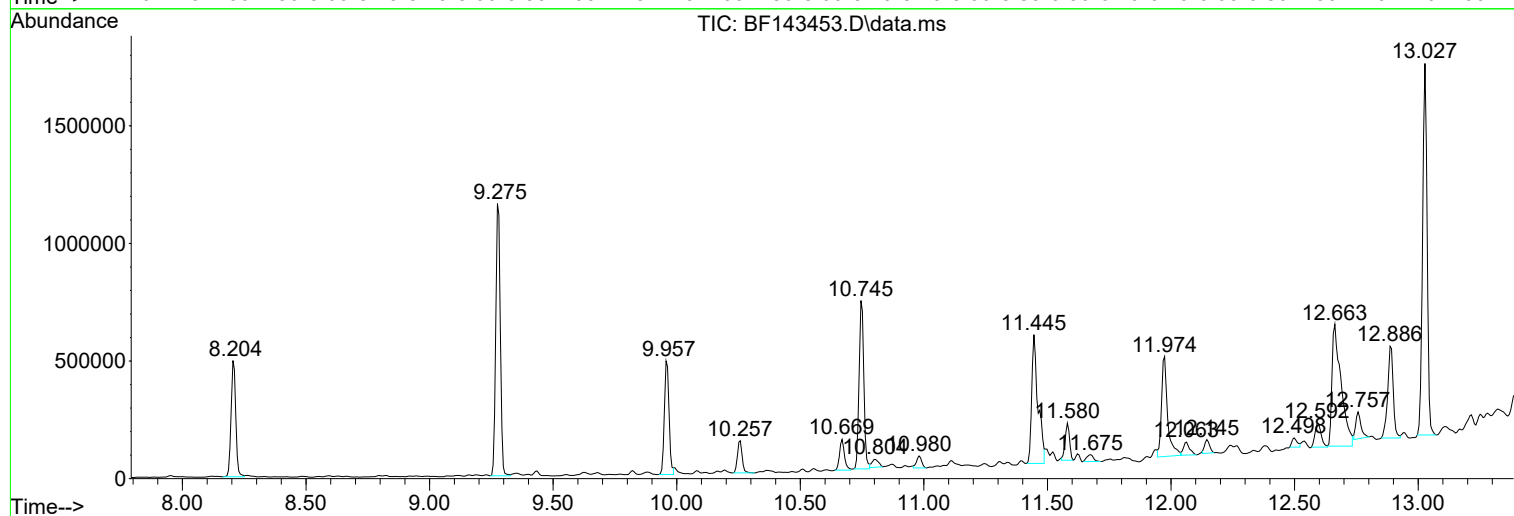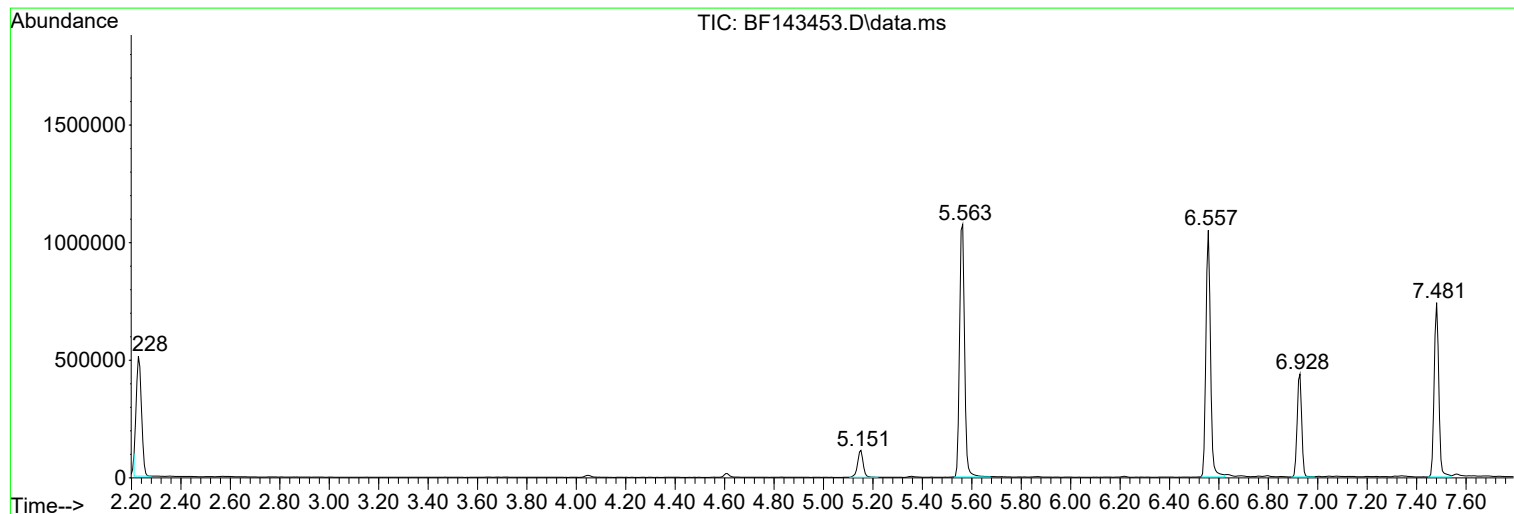

Data Path : Z:\svoasrv\HPCHEM1\BNA\_F\Data\BF081925\  
Data File : BF143453.D  
Acq On : 19 Aug 2025 13:30  
Operator : RC/JU  
Sample : Q2879-05  
Misc :  
ALS Vial : 10 Sample Multiplier: 1

Instrument :  
BNA\_F  
ClientSampleId :  
OU4-TS-GRILLO-TSCP05-081425

Quant Method : Z:\svoasrv\HPCHEM1\BNA\_F\Methods\8270-BF081525.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L  
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

\*\*\*\*\*

Data Path : Z:\svoasrv\HPCHEM1\BNA\_F\Data\BF081925\  
Data File : BF143453.D  
Acq On : 19 Aug 2025 13:30  
Operator : RC/JU  
Sample : Q2879-05  
Misc :  
ALS Vial : 10 Sample Multiplier: 1

Instrument :  
BNA\_F  
ClientSampleId :  
OU4-TS-GRILLO-TSCP05-081425

Quant Method : Z:\svoasrv\HPCHEM1\BNA\_F\Methods\8270-BF081525.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L  
TIC Integration Parameters: LSCINT.P

| TIC Top Hit name | RT | EstConc | Units | Response | # | RT | Resp | Conc |
|------------------|----|---------|-------|----------|---|----|------|------|
|------------------|----|---------|-------|----------|---|----|------|------|