

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF081925\
 Data File : BF143454.D
 Acq On : 19 Aug 2025 13:59
 Operator : RC/JU
 Sample : Q2879-07
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 OU4-TS-GRILLO-TSCP06-081425

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF081525.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BF143454.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	2.240	3	8	17	rVB	566095	879418	18.65%	2.195%
2	5.151	488	503	514	rBV	128050	198802	4.22%	0.496%
3	5.563	567	573	594	rBV	1217763	1615263	34.26%	4.032%
4	6.557	737	742	753	rBV	1195167	1569403	33.29%	3.917%
5	6.928	800	805	813	rBV	443433	553679	11.74%	1.382%
6	7.481	894	899	910	rBV	764896	979984	20.79%	2.446%
7	8.204	1015	1022	1030	rBV	438257	570699	12.11%	1.424%
8	9.275	1199	1204	1213	rBV	1208117	1573038	33.37%	3.926%
9	9.963	1315	1321	1325	rBV	446198	595266	12.63%	1.486%
10	10.669	1436	1441	1447	rBV	135000	179392	3.81%	0.448%
11	10.745	1449	1454	1463	rVV	742547	1019358	21.62%	2.544%
12	10.980	1490	1494	1499	rVB2	55207	78544	1.67%	0.196%
13	11.445	1568	1573	1581	rBV2	511410	911570	19.34%	2.275%
14	11.675	1606	1612	1620	rBV3	27911	72798	1.54%	0.182%
15	11.975	1658	1663	1674	rVV2	479371	773752	16.41%	1.931%
16	12.063	1675	1678	1685	rVB2	49604	83605	1.77%	0.209%
17	12.145	1689	1692	1701	rVB5	65813	111282	2.36%	0.278%
18	12.592	1764	1768	1775	rBV2	142570	218821	4.64%	0.546%
19	12.663	1775	1780	1792	rBV	464199	902712	19.15%	2.253%
20	12.757	1792	1796	1804	rVV	133484	207826	4.41%	0.519%
21	12.892	1813	1819	1825	rBV	343184	502225	10.65%	1.254%
22	13.027	1837	1842	1850	rBV	1636203	2112811	44.81%	5.274%
23	13.392	1901	1904	1908	rBV	82591	124554	2.64%	0.311%
24	13.469	1913	1917	1922	rVV5	122089	213452	4.53%	0.533%
25	13.927	1991	1995	2004	rVB2	470628	808638	17.15%	2.018%
26	14.004	2005	2008	2013	rVB2	195085	253153	5.37%	0.632%
27	14.086	2015	2022	2030	rBV2	727371	1375947	29.19%	3.434%
28	14.551	2096	2101	2108	rBV2	561420	1030960	21.87%	2.573%
29	14.939	2163	2167	2173	rVB	432372	602772	12.79%	1.505%
30	15.145	2199	2202	2203	rBV	121498	140918	2.99%	0.352%
31	15.204	2208	2212	2217	rVV	1411240	2019084	42.83%	5.040%
32	15.580	2272	2276	2291	rVB2	321465	598359	12.69%	1.494%
33	15.798	2310	2313	2319	rBV	113338	175001	3.71%	0.437%
34	16.045	2349	2355	2361	rVB	1034146	1765650	37.45%	4.407%
35	16.327	2398	2403	2416	rVB2	383854	875475	18.57%	2.185%
36	17.468	2592	2597	2608	rVB7	201548	563210	11.95%	1.406%

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF081925\
Data File : BF143454.D
Acq On : 19 Aug 2025 13:59
Operator : RC/JU
Sample : Q2879-07
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
OU4-TS-GRILLO-TSCP06-081425

Integration Parameters: rteint.p
Integrator: RTE
Smoothing : ON Filtering: 5
Sampling : 1 Min Area: 3 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF081525.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

37	17.762	2633	2647	2657	rBV4	1115340	4714537	100.00%	11.768%
38	17.939	2672	2677	2684	rVB	395512	888553	18.85%	2.218%
39	18.204	2715	2722	2732	rBV	794770	2572500	54.57%	6.421%
40	18.304	2735	2739	2751	rVB6	541929	1656501	35.14%	4.135%
41	18.568	2775	2784	2802	rBV7	632765	3354324	71.15%	8.373%
42	18.721	2804	2810	2815	rBV2	246204	619664	13.14%	1.547%




Sum of corrected areas: 40063500

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF081925\
Data File : BF143454.D
Acq On : 19 Aug 2025 13:59
Operator : RC/JU
Sample : Q2879-07
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
OU4-TS-GRILLO-TSCP06-081425

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF081525.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

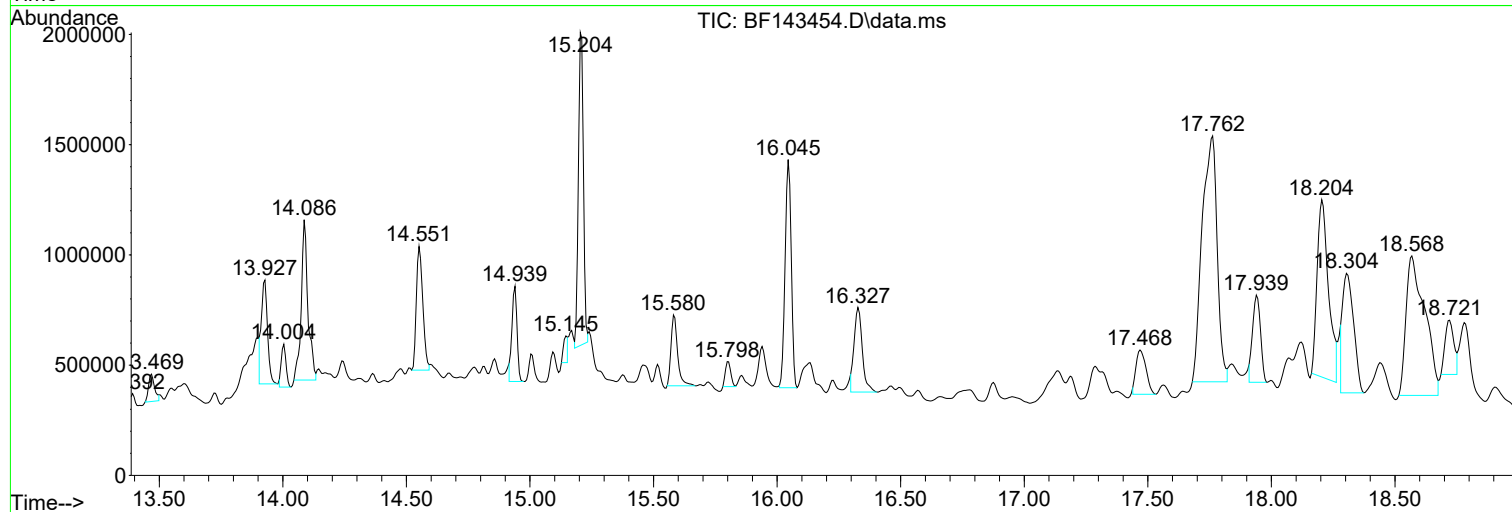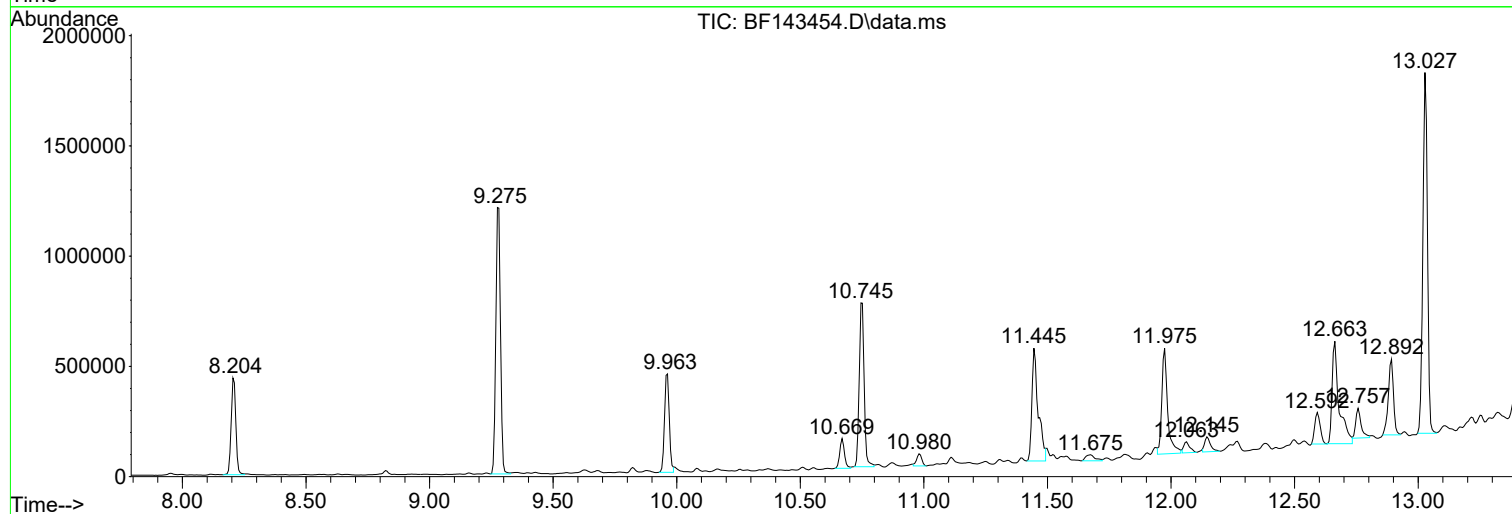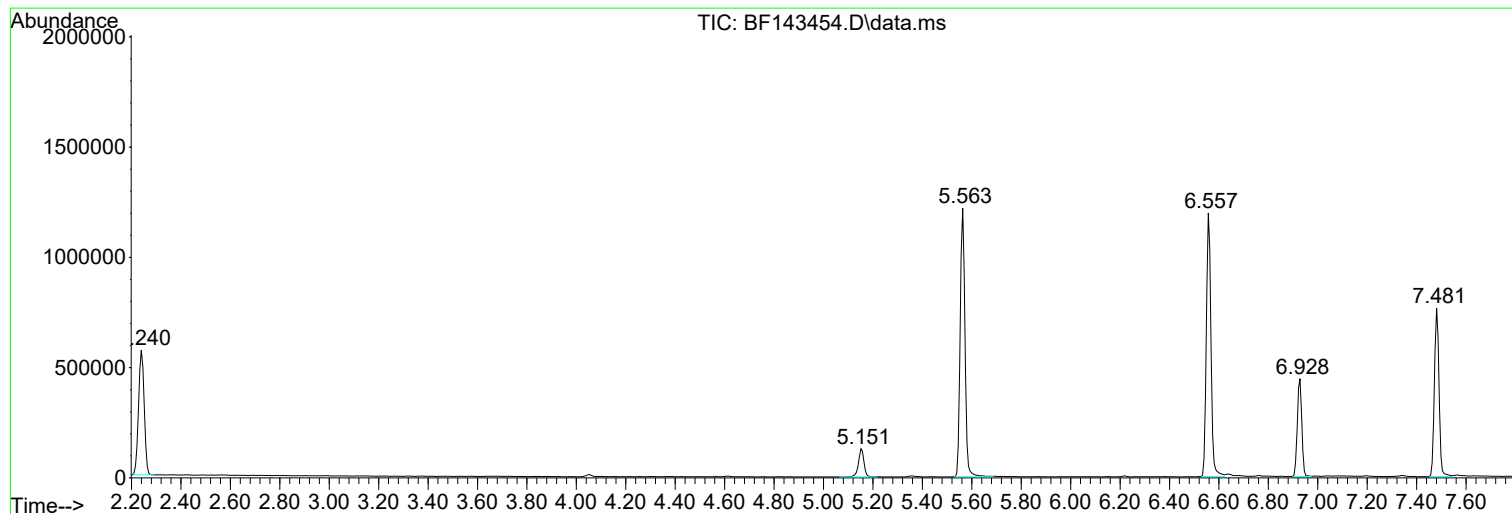

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF081925\
Data File : BF143454.D
Acq On : 19 Aug 2025 13:59
Operator : RC/JU
Sample : Q2879-07
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
OU4-TS-GRILLO-TSCP06-081425

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF081525.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF081925\
Data File : BF143454.D
Acq On : 19 Aug 2025 13:59
Operator : RC/JU
Sample : Q2879-07
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
OU4-TS-GRILLO-TSCP06-081425

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF081525.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------