

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF081925\
 Data File : BF143455.D
 Acq On : 19 Aug 2025 14:28
 Operator : RC/JU
 Sample : Q2879-09
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 OU4-TS-GRILLO-TSCP07-081425

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF081525.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BF143455.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	2.234	3	7	15	rVB	498614	762981	20.75%	2.475%
2	5.151	494	503	511	rBV	117486	178664	4.86%	0.580%
3	5.563	568	573	591	rBV	1113445	1478133	40.20%	4.796%
4	6.557	737	742	753	rBV	943754	1276484	34.71%	4.141%
5	6.928	800	805	813	rBV	391015	486916	13.24%	1.580%
6	7.481	894	899	910	rBV	652247	837671	22.78%	2.718%
7	8.204	1015	1022	1031	rBV	413191	547597	14.89%	1.777%
8	9.281	1199	1205	1213	rBV	1096497	1428150	38.84%	4.633%
9	9.957	1315	1320	1325	rBV	453448	602568	16.39%	1.955%
10	10.669	1436	1441	1447	rBV	122128	156739	4.26%	0.509%
11	10.751	1449	1455	1465	rVV	726095	988035	26.87%	3.206%
12	10.980	1490	1494	1499	rVB2	52740	71641	1.95%	0.232%
13	11.445	1568	1573	1580	rBV2	536384	821102	22.33%	2.664%
14	11.974	1658	1663	1674	rVB2	374015	629648	17.12%	2.043%
15	12.145	1689	1692	1698	rVB3	54179	73257	1.99%	0.238%
16	12.592	1764	1768	1775	rVB2	98306	147708	4.02%	0.479%
17	12.663	1776	1780	1792	rBV	279606	584164	15.89%	1.895%
18	12.757	1792	1796	1805	rBV	113291	190652	5.18%	0.619%
19	12.892	1814	1819	1825	rVB	202137	295440	8.03%	0.959%
20	13.027	1837	1842	1850	rBV	1574272	2011021	54.69%	6.525%
21	13.392	1901	1904	1908	rBV	77496	114373	3.11%	0.371%
22	13.469	1913	1917	1921	rVV3	107698	179170	4.87%	0.581%
23	13.921	1991	1994	2005	rVB2	484988	911002	24.77%	2.956%
24	14.063	2014	2018	2019	rBV	195429	259039	7.04%	0.840%
25	14.086	2019	2022	2030	rVB2	603048	922070	25.07%	2.992%
26	14.551	2096	2101	2108	rBV3	491983	921927	25.07%	2.991%
27	14.933	2163	2166	2173	rVB	262291	376585	10.24%	1.222%
28	15.204	2208	2212	2217	rBV	1208417	1661105	45.17%	5.389%
29	15.580	2272	2276	2291	rVB	308117	513679	13.97%	1.667%
30	16.045	2349	2355	2361	rVB	794906	1369692	37.25%	4.444%
31	16.327	2399	2403	2417	rVB2	292781	635721	17.29%	2.063%
32	17.756	2633	2646	2656	rBV4	926445	3677296	100.00%	11.931%
33	17.939	2672	2677	2684	rVB	308906	697903	18.98%	2.264%
34	18.203	2714	2722	2732	rBV	726140	2291083	62.30%	7.433%
35	18.562	2775	2783	2802	rBV6	527404	2723374	74.06%	8.836%

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF081925\
Data File : BF143455.D
Acq On : 19 Aug 2025 14:28
Operator : RC/JU
Sample : Q2879-09
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
OU4-TS-GRILLO-TSCP07-081425

Integration Parameters: rteint.p
Integrator: RTE
Smoothing : ON Filtering: 5
Sampling : 1 Min Area: 3 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF081525.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION




Sum of corrected areas: 30822590

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF081925\
Data File : BF143455.D
Acq On : 19 Aug 2025 14:28
Operator : RC/JU
Sample : Q2879-09
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
OU4-TS-GRILLO-TSCP07-081425

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF081525.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

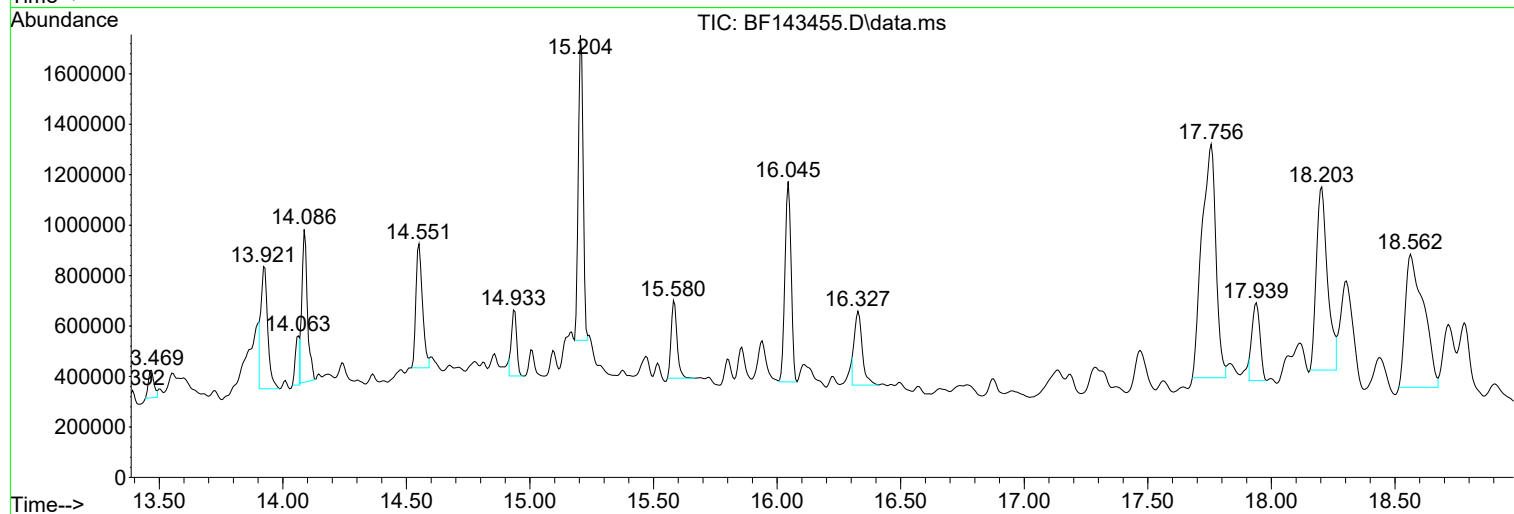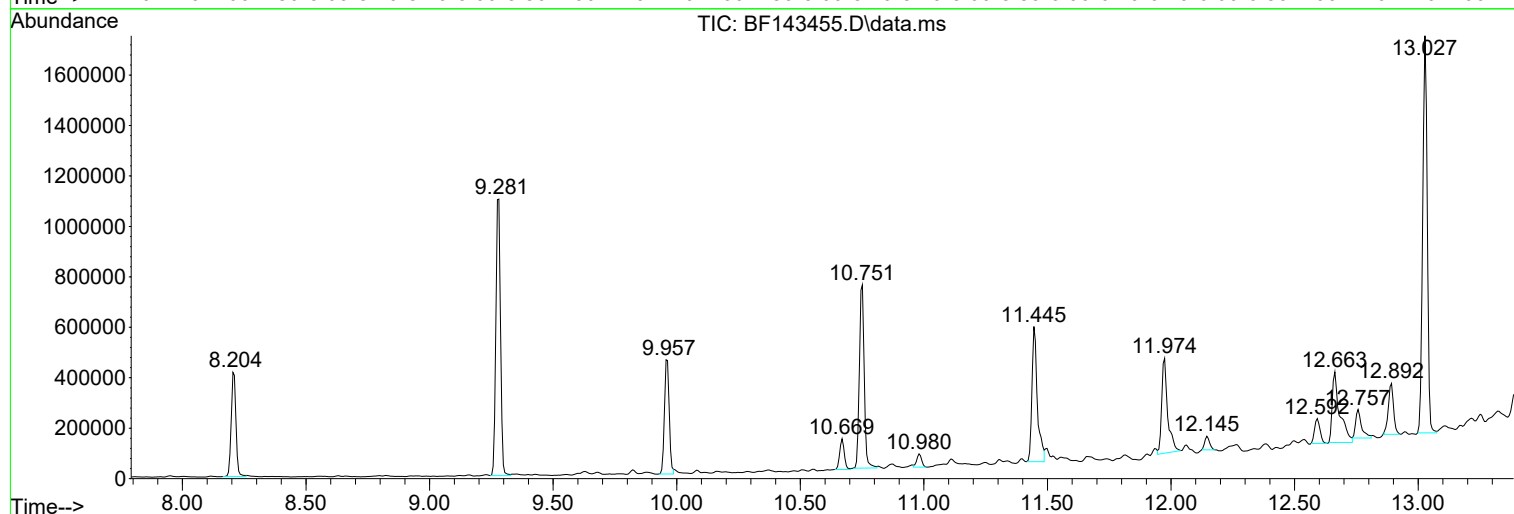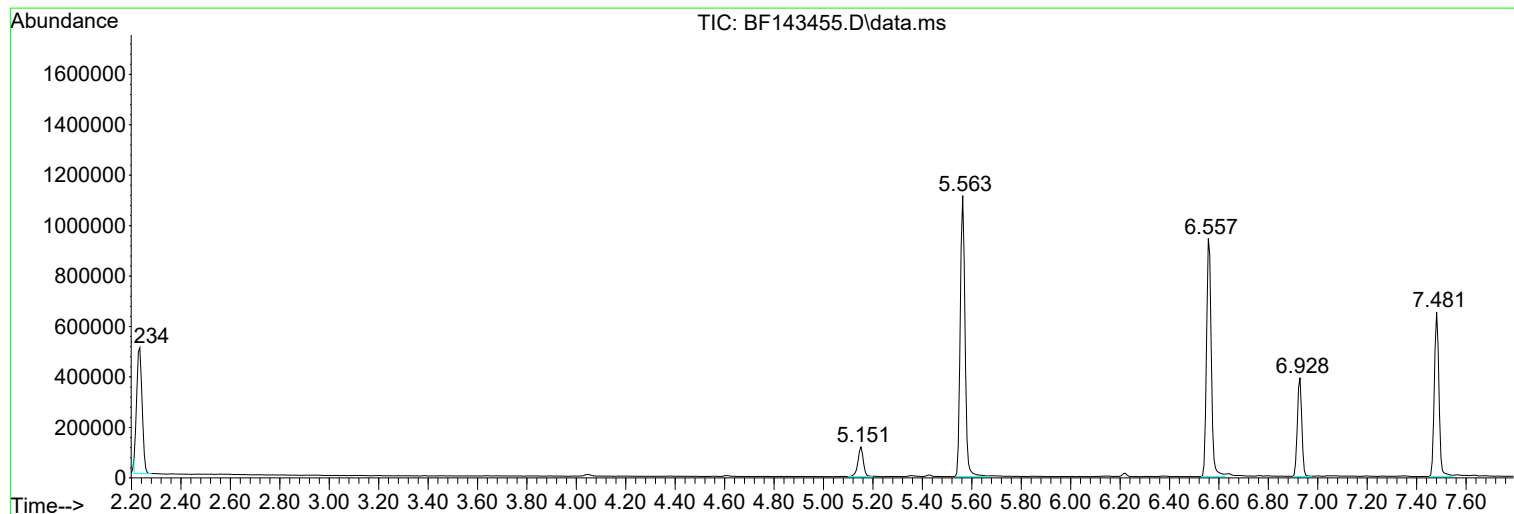

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF081925\
Data File : BF143455.D
Acq On : 19 Aug 2025 14:28
Operator : RC/JU
Sample : Q2879-09
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
OU4-TS-GRILLO-TSCP07-081425

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF081525.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF081925\
Data File : BF143455.D
Acq On : 19 Aug 2025 14:28
Operator : RC/JU
Sample : Q2879-09
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
OU4-TS-GRILLO-TSCP07-081425

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF081525.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------