

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF081925\
 Data File : BF143456.D
 Acq On : 19 Aug 2025 14:57
 Operator : RC/JU
 Sample : Q2879-11
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 OU4-TS-GRILLO-TSCP08-081425

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF081525.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BF143456.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	2.234	3	7	17	rVB	767551	1193396	25.43%	3.651%
2	5.151	495	503	512	rBV2	106038	164356	3.50%	0.503%
3	5.563	568	573	592	rBV	922531	1231234	26.24%	3.766%
4	6.557	737	742	753	rBV	855652	1173257	25.00%	3.589%
5	6.928	800	805	813	rBV	467515	575558	12.26%	1.761%
6	7.481	894	899	910	rBV	609241	786689	16.76%	2.407%
7	8.210	1014	1023	1030	rBV	479192	633736	13.50%	1.939%
8	9.281	1199	1205	1213	rBV	1043102	1340254	28.56%	4.100%
9	9.963	1315	1321	1335	rVV	526208	700839	14.93%	2.144%
10	10.669	1437	1441	1445	rBV	99946	126468	2.69%	0.387%
11	10.751	1450	1455	1464	rVB	613548	819869	17.47%	2.508%
12	10.981	1491	1494	1499	rVB2	47884	67531	1.44%	0.207%
13	11.445	1568	1573	1580	rBV2	547930	854068	18.20%	2.613%
14	11.975	1658	1663	1674	rBV2	405143	611752	13.04%	1.871%
15	12.063	1675	1678	1685	rVB	41556	65345	1.39%	0.200%
16	12.592	1764	1768	1775	rVB2	110992	166252	3.54%	0.509%
17	12.663	1776	1780	1792	rBV	304971	716424	15.27%	2.192%
18	12.757	1792	1796	1804	rVV	136988	218514	4.66%	0.668%
19	12.892	1815	1819	1825	rVB	212615	289540	6.17%	0.886%
20	13.027	1837	1842	1850	rBV	1423991	1865966	39.76%	5.708%
21	13.392	1900	1904	1911	rBV2	196929	403861	8.61%	1.235%
22	13.922	1992	1994	2005	rVB2	464411	765665	16.32%	2.342%
23	14.086	2019	2022	2029	rVB2	586597	874465	18.63%	2.675%
24	14.551	2097	2101	2108	rBV2	499939	872423	18.59%	2.669%
25	14.939	2164	2167	2173	rVB	251253	330226	7.04%	1.010%
26	15.204	2208	2212	2217	rBV	1028591	1447378	30.84%	4.428%
27	15.586	2272	2277	2288	rBV	323651	571900	12.19%	1.749%
28	16.045	2350	2355	2361	rVB	757088	1249806	26.63%	3.823%
29	16.327	2399	2403	2418	rVB	340745	760337	16.20%	2.326%
30	17.762	2633	2647	2657	rBV4	1058974	4692720	100.00%	14.355%
31	17.945	2673	2678	2685	rVB	379251	845996	18.03%	2.588%
32	18.204	2715	2722	2733	rBV	799812	2516934	53.63%	7.699%
33	18.574	2776	2785	2803	rBV6	587503	3166035	67.47%	9.685%
34	18.721	2805	2810	2816	rBV2	248244	590996	12.59%	1.808%

Sum of corrected areas: 32689790

Instrument :

BNA_F

ClientSampleId :


OU4-TS-GRILLO-TSCP08-081425

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF081925\
Data File : BF143456.D
Acq On : 19 Aug 2025 14:57
Operator : RC/JU
Sample : Q2879-11
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
OU4-TS-GRILLO-TSCP08-081425

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF081525.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

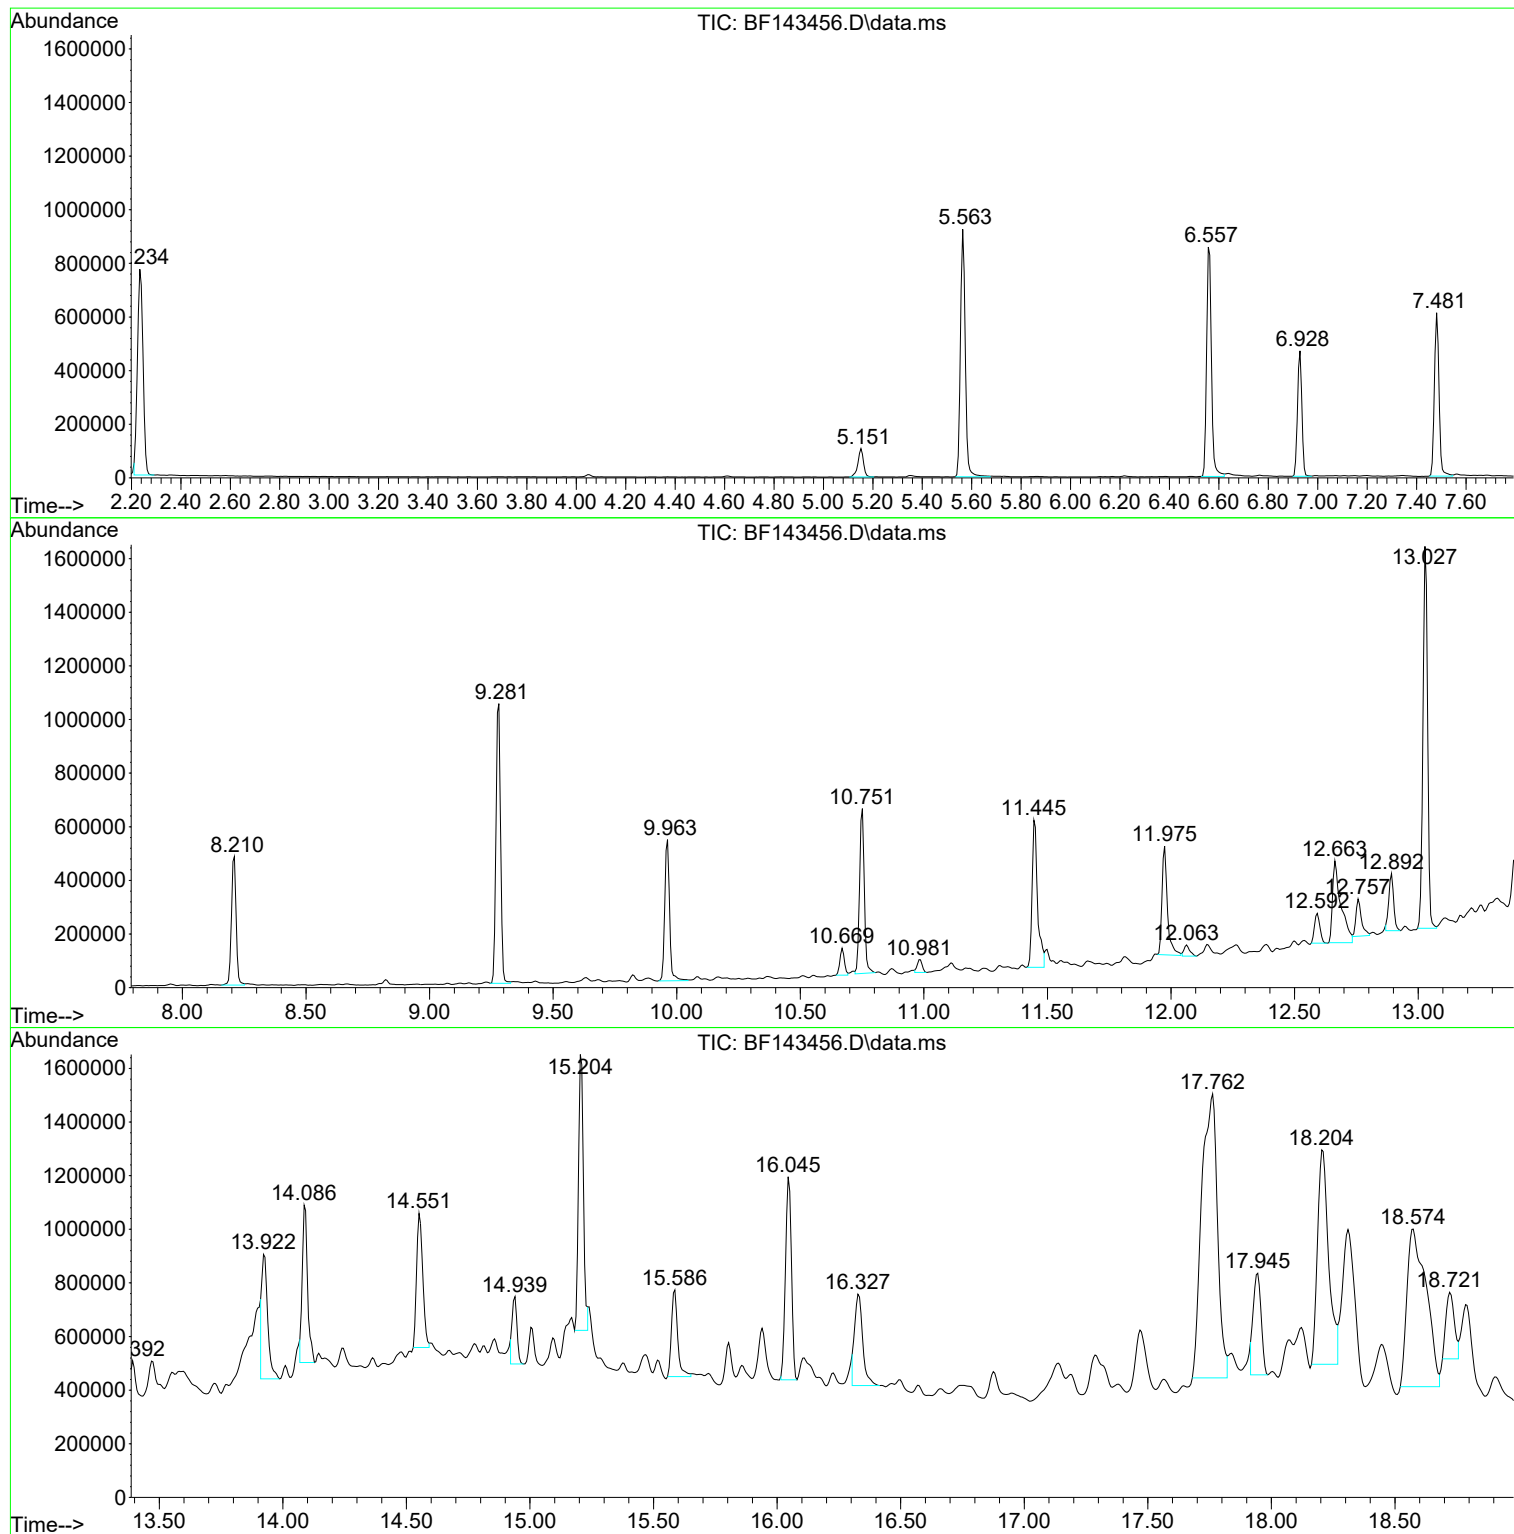

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF081925\
Data File : BF143456.D
Acq On : 19 Aug 2025 14:57
Operator : RC/JU
Sample : Q2879-11
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
OU4-TS-GRILLO-TSCP08-081425

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF081525.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF081925\
Data File : BF143456.D
Acq On : 19 Aug 2025 14:57
Operator : RC/JU
Sample : Q2879-11
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
OU4-TS-GRILLO-TSCP08-081425

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF081525.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------