

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF081925\
 Data File : BF143458.D
 Acq On : 19 Aug 2025 15:55
 Operator : RC/JU
 Sample : Q2879-15
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 OU4-TS-GRILLO-TSCP10-081425

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF081525.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BF143458.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	2.240	3	8	18	rVB	674862	1048611	22.80%	3.021%
2	5.157	493	504	511	rBV	118238	188834	4.11%	0.544%
3	5.569	568	574	590	rBV	1086361	1480275	32.18%	4.264%
4	6.563	738	743	752	rBV	1092241	1419764	30.86%	4.090%
5	6.928	800	805	812	rBV	500555	606082	13.18%	1.746%
6	7.481	894	899	910	rBV	680817	887287	19.29%	2.556%
7	8.210	1014	1023	1031	rBV	498118	640523	13.92%	1.845%
8	8.822	1119	1127	1136	rBV2	30374	48436	1.05%	0.140%
9	9.280	1199	1205	1212	rBV	1220812	1521715	33.08%	4.383%
10	9.963	1316	1321	1335	rVB	554372	721652	15.69%	2.079%
11	10.669	1437	1441	1446	rBV	110217	147699	3.21%	0.425%
12	10.751	1450	1455	1464	rVB	764057	990381	21.53%	2.853%
13	10.986	1491	1495	1499	rVB2	56172	76287	1.66%	0.220%
14	11.110	1513	1516	1523	rBV	39987	61161	1.33%	0.176%
15	11.451	1569	1574	1580	rBV	594039	898794	19.54%	2.589%
16	11.974	1659	1663	1675	rVV	590895	886952	19.28%	2.555%
17	12.592	1764	1768	1774	rVB	129147	185562	4.03%	0.535%
18	12.663	1776	1780	1792	rBV	293632	765123	16.63%	2.204%
19	12.757	1792	1796	1805	rVV	198867	330240	7.18%	0.951%
20	12.892	1815	1819	1825	rVB	219740	303808	6.60%	0.875%
21	13.033	1837	1843	1850	rBV	1650752	2230489	48.49%	6.425%
22	13.392	1900	1904	1909	rBV2	210579	365281	7.94%	1.052%
23	13.468	1914	1917	1926	rVB4	160464	325099	7.07%	0.936%
24	13.921	1991	1994	2006	rVB3	598423	1179774	25.65%	3.398%
25	14.063	2014	2018	2020	rBV	332027	489557	10.64%	1.410%
26	14.092	2020	2023	2029	rVB	592219	843743	18.34%	2.431%
27	14.551	2097	2101	2108	rBV2	630466	1029811	22.39%	2.966%
28	14.939	2164	2167	2174	rVB	308626	400087	8.70%	1.152%
29	15.010	2176	2179	2187	rVB	192862	269209	5.85%	0.775%
30	15.210	2208	2213	2217	rBV	1119430	1644450	35.75%	4.737%
31	15.586	2273	2277	2285	rVB	321697	495829	10.78%	1.428%
32	15.804	2311	2314	2319	rVB	154251	214811	4.67%	0.619%
33	16.045	2350	2355	2361	rVB	815638	1416811	30.80%	4.081%
34	16.333	2400	2404	2418	rVB	376711	767913	16.69%	2.212%
35	17.768	2634	2648	2657	rBV6	1040679	4600090	100.00%	13.251%
36	17.945	2674	2678	2686	rVB	356523	763370	16.59%	2.199%

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF081925\
Data File : BF143458.D
Acq On : 19 Aug 2025 15:55
Operator : RC/JU
Sample : Q2879-15
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
OU4-TS-GRILLO-TSCP10-081425

Integration Parameters: rteint.p
Integrator: RTE
Smoothing : ON Filtering: 5
Sampling : 1 Min Area: 3 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF081525.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

37	18.209	2716	2723	2733	rBV	683920	2049866	44.56%	5.905%
38	18.574	2777	2785	2790	rBV2	566159	1815250	39.46%	5.229%
39	18.721	2805	2810	2816	rBV2	252916	604121	13.13%	1.740%




Sum of corrected areas: 34714747

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF081925\
Data File : BF143458.D
Acq On : 19 Aug 2025 15:55
Operator : RC/JU
Sample : Q2879-15
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
OU4-TS-GRILLO-TSCP10-081425

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF081525.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

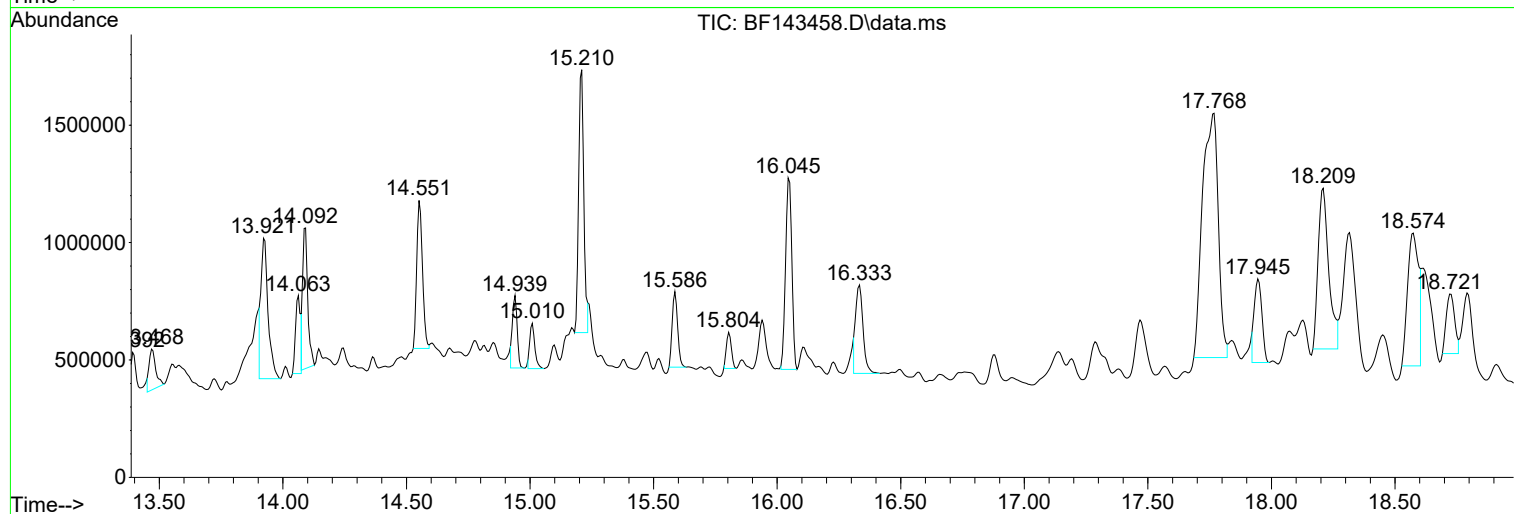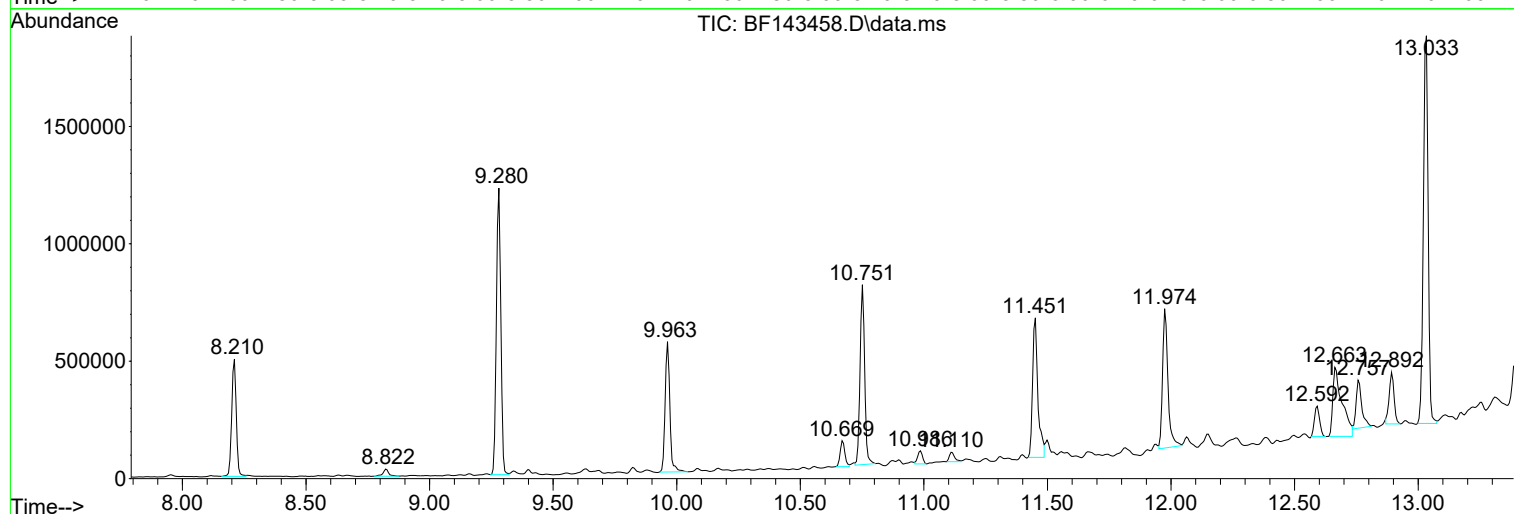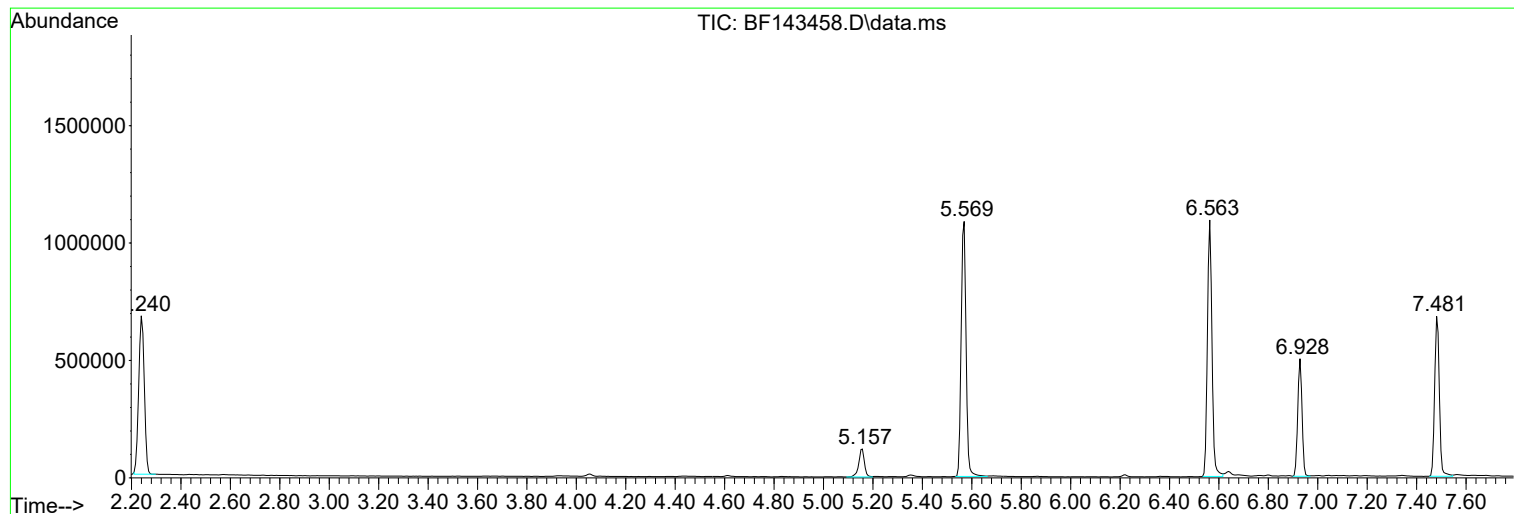

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF081925\
Data File : BF143458.D
Acq On : 19 Aug 2025 15:55
Operator : RC/JU
Sample : Q2879-15
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
OU4-TS-GRILLO-TSCP10-081425

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF081525.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF081925\
Data File : BF143458.D
Acq On : 19 Aug 2025 15:55
Operator : RC/JU
Sample : Q2879-15
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
OU4-TS-GRILLO-TSCP10-081425

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF081525.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc