

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF081925\
 Data File : BF143459.D
 Acq On : 19 Aug 2025 16:24
 Operator : RC/JU
 Sample : Q2879-17
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 OU4-TS-GRILLO-TSCP11-081425

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF081525.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BF143459.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	2.240	3	8	18	rVB	769486	1243974	17.29%	2.634%
2	5.157	495	504	512	rBV2	151071	235171	3.27%	0.498%
3	5.569	568	574	586	rBV	1426240	1871553	26.01%	3.963%
4	6.563	738	743	754	rBV	1361352	1863833	25.90%	3.947%
5	6.928	800	805	814	rBV	478567	586091	8.14%	1.241%
6	7.481	894	899	911	rBV	815636	1084666	15.07%	2.297%
7	8.210	1017	1023	1039	rVB	522817	684215	9.51%	1.449%
8	9.280	1199	1205	1210	rBV	1487190	1828687	25.41%	3.873%
9	9.963	1316	1321	1334	rBV	582888	770148	10.70%	1.631%
10	10.669	1437	1441	1447	rVB	129537	165005	2.29%	0.349%
11	10.751	1450	1455	1470	rVB	923664	1226335	17.04%	2.597%
12	10.986	1491	1495	1499	rVB	64052	87489	1.22%	0.185%
13	11.451	1569	1574	1580	rBV2	598992	935603	13.00%	1.981%
14	11.974	1659	1663	1675	rVB	470851	714837	9.93%	1.514%
15	12.145	1689	1692	1701	rVB4	114374	181640	2.52%	0.385%
16	12.592	1763	1768	1774	rBV	185344	286356	3.98%	0.606%
17	12.663	1776	1780	1792	rBV	343478	778994	10.82%	1.650%
18	12.757	1793	1796	1809	rVB2	125815	223749	3.11%	0.474%
19	12.892	1815	1819	1825	rVB	207611	292835	4.07%	0.620%
20	13.033	1837	1843	1850	rBV	1648103	2239434	31.12%	4.743%
21	13.345	1894	1896	1900	rVB2	100497	119883	1.67%	0.254%
22	13.392	1901	1904	1908	rBV	148153	212696	2.96%	0.450%
23	13.468	1913	1917	1921	rVV2	214211	317223	4.41%	0.672%
24	13.921	1991	1994	2005	rVB	604259	1064214	14.79%	2.254%
25	14.092	2019	2023	2030	rVB2	537928	813986	11.31%	1.724%
26	14.551	2096	2101	2108	rBV2	774583	1263185	17.55%	2.675%
27	14.939	2163	2167	2174	rVB	582320	813547	11.30%	1.723%
28	15.098	2190	2194	2198	rBV	183899	288520	4.01%	0.611%
29	15.209	2208	2213	2225	rVB	1855619	3067429	42.62%	6.496%
30	15.586	2273	2277	2291	rVB2	328636	577237	8.02%	1.222%
31	15.939	2334	2337	2348	rVB	243090	441542	6.14%	0.935%
32	16.051	2350	2356	2361	rVB	1146554	1953201	27.14%	4.136%
33	16.333	2399	2404	2416	rVB2	524263	1149353	15.97%	2.434%
34	17.468	2592	2597	2609	rVB5	339541	940547	13.07%	1.992%
35	17.780	2635	2650	2658	rBV4	1801997	7196392	100.00%	15.240%
36	17.950	2674	2679	2687	rVB	472435	1077044	14.97%	2.281%

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF081925\
Data File : BF143459.D
Acq On : 19 Aug 2025 16:24
Operator : RC/JU
Sample : Q2879-17
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
OU4-TS-GRILLO-TSCP11-081425

Integration Parameters: rteint.p
Integrator: RTE
Smoothing : ON Filtering: 5
Sampling : 1 Min Area: 3 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF081525.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

37	18.215	2717	2724	2735	rBV	965175	2992082	41.58%	6.336%
38	18.586	2777	2787	2805	rBV3	844142	4641423	64.50%	9.829%
39	18.733	2806	2812	2818	rBV2	381251	989995	13.76%	2.097%




Sum of corrected areas: 47220114

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF081925\
Data File : BF143459.D
Acq On : 19 Aug 2025 16:24
Operator : RC/JU
Sample : Q2879-17
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
OU4-TS-GRILLO-TSCP11-081425

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF081525.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

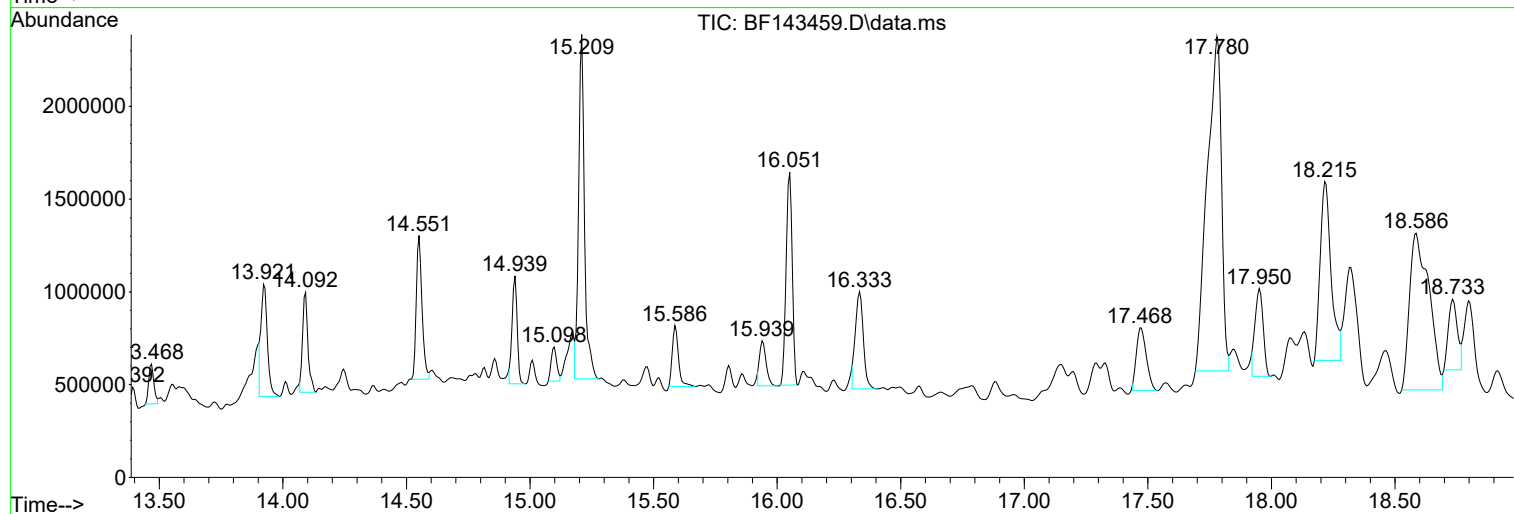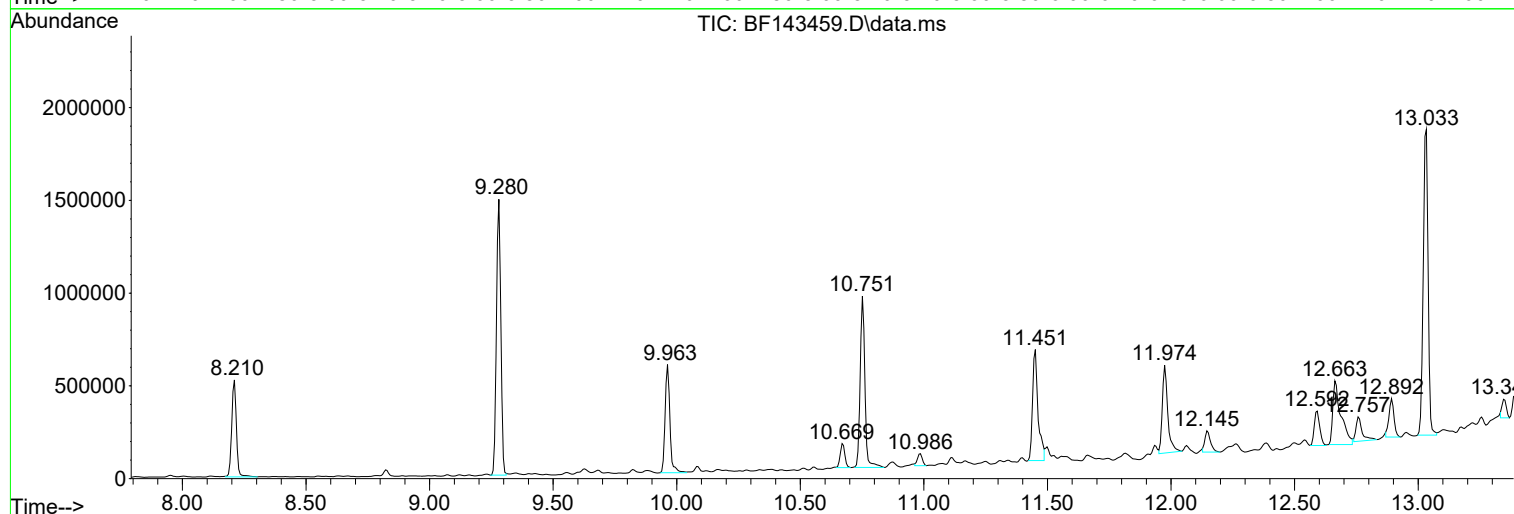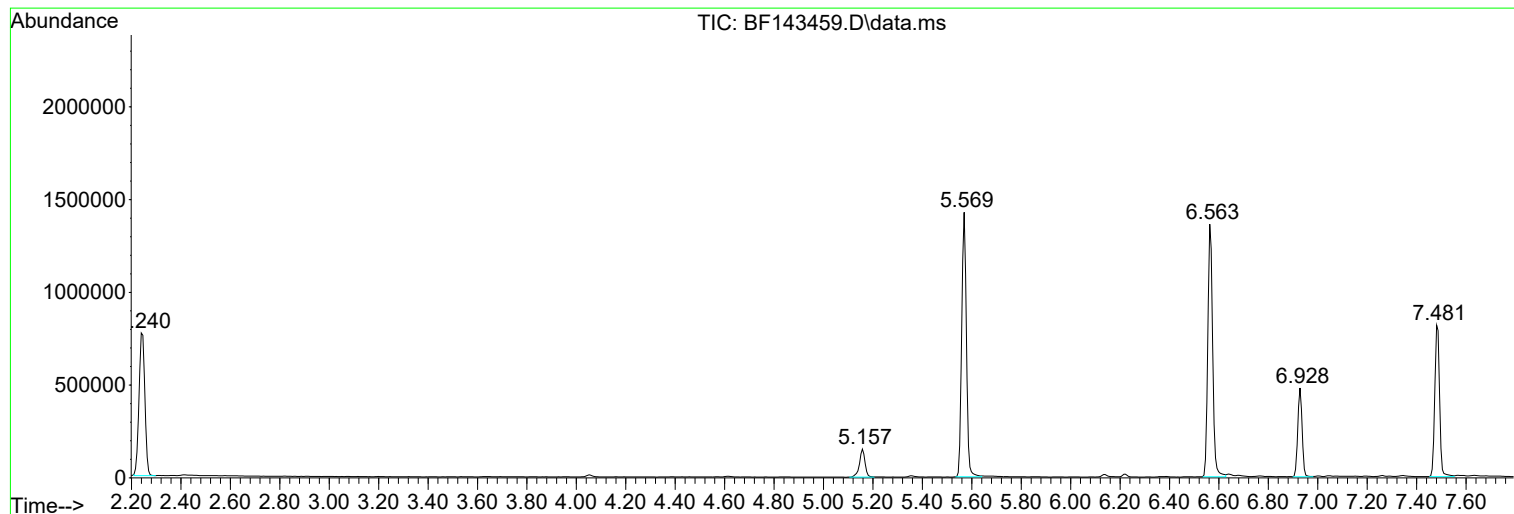

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF081925\
Data File : BF143459.D
Acq On : 19 Aug 2025 16:24
Operator : RC/JU
Sample : Q2879-17
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
OU4-TS-GRILLO-TSCP11-081425

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF081525.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF081925\
Data File : BF143459.D
Acq On : 19 Aug 2025 16:24
Operator : RC/JU
Sample : Q2879-17
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
OU4-TS-GRILLO-TSCP11-081425

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF081525.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------