

Data Path : Z:\svoasrv\HPCHEM1\BNA\_F\Data\BF081925\  
 Data File : BF143455.D  
 Acq On : 19 Aug 2025 14:28  
 Operator : RC/JU  
 Sample : Q2879-09  
 Misc :  
 ALS Vial : 12 Sample Multiplier: 1

Instrument :  
 BNA\_F  
 ClientSampleId :  
 OU4-TS-GRILLO-TSCP07-081425

Quant Time: Aug 19 14:51:40 2025  
 Quant Method : Z:\svoasrv\HPCHEM1\BNA\_F\Methods\8270-BF081525.M  
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
 QLast Update : Mon Aug 18 04:40:19 2025  
 Response via : Initial Calibration


| Compound                      | R.T.   | QIon | Response | Conc    | Units | Dev(Min) |
|-------------------------------|--------|------|----------|---------|-------|----------|
| -----                         |        |      |          |         |       |          |
| Internal Standards            |        |      |          |         |       |          |
| 1) 1,4-Dichlorobenzene-d4     | 6.928  | 152  | 81535    | 20.000  | ng    | 0.00     |
| 21) Naphthalene-d8            | 8.204  | 136  | 266043   | 20.000  | ng    | 0.00     |
| 39) Acenaphthene-d10          | 9.963  | 164  | 139719   | 20.000  | ng    | 0.00     |
| 64) Phenanthrene-d10          | 11.445 | 188  | 269890   | 20.000  | ng    | 0.00     |
| 76) Chrysene-d12              | 14.086 | 240  | 272023   | 20.000  | ng    | 0.00     |
| 86) Perylene-d12              | 15.580 | 264  | 174368   | 20.000  | ng    | 0.00     |
|                               |        |      |          |         |       |          |
| System Monitoring Compounds   |        |      |          |         |       |          |
| 5) 2-Fluorophenol             | 5.563  | 112  | 408333   | 87.057  | ng    | 0.00     |
| 7) Phenol-d6                  | 6.557  | 99   | 437182   | 73.960  | ng    | 0.00     |
| 23) Nitrobenzene-d5           | 7.481  | 82   | 275314   | 61.407  | ng    | 0.00     |
| 42) 2,4,6-Tribromophenol      | 10.751 | 330  | 128719   | 103.505 | ng    | 0.00     |
| 45) 2-Fluorobiphenyl          | 9.281  | 172  | 499605   | 60.144  | ng    | 0.00     |
| 79) Terphenyl-d14             | 13.027 | 244  | 755405   | 46.649  | ng    | 0.00     |
|                               |        |      |          |         |       |          |
| Target Compounds              |        |      |          |         |       | Qvalue   |
| 19) n-Nitroso-di-n-propyla... | 7.481  | 70   | 36852    | 10.070  | ng    | # 78     |
| 25) Isophorone                | 7.481  | 82   | 275311   | 32.084  | ng    | # 65     |
| 51) 2,6-Dinitrotoluene        | 9.957  | 165  | 18542    | 10.798  | ng    | # 24     |
| 57) 2,4-Dinitrotoluene        | 9.957  | 165  | 18543    | 8.099   | ng    | # 25     |
| 63) Azobenzene                | 10.669 | 77   | 30370    | 3.733   | ng    | # 1      |
| 67) 4-Bromophenyl-phenylether | 10.751 | 248  | 8482     | 2.661   | ng    | # 1      |
| 71) Phenanthrene              | 11.469 | 178  | 43999    | 3.011   | ng    | 99       |
| 72) Anthracene                | 11.469 | 178  | 43999    | 2.981   | ng    | 99       |
| 74) Di-n-butylphthalate       | 12.004 | 149  | 30134    | 2.424   | ng    | 98       |
| 75) Fluoranthene              | 12.663 | 202  | 136964   | 10.547  | ng    | 99       |
| 78) Pyrene                    | 12.892 | 202  | 122974   | 5.201   | ng    | 99       |
| 81) Benzo(a)anthracene        | 14.080 | 228  | 67916    | 3.922   | ng    | 93       |
| 83) Chrysene                  | 14.110 | 228  | 74599    | 4.659   | ng    | 97       |
| 84) Bis(2-ethylhexyl)phtha... | 14.057 | 149  | 74678    | 8.979   | ng    | 98       |
| 87) Indeno(1,2,3-cd)pyrene    | 17.098 | 276  | 29277    | 2.239   | ng    | 96       |
| 88) Benzo(b)fluoranthene      | 15.145 | 252  | 94459    | 10.108  | ng    | # 89     |
| 89) Benzo(k)fluoranthene      | 15.145 | 252  | 94459    | 10.248  | ng    | # 89     |
| 90) Benzo(a)pyrene            | 15.515 | 252  | 40917    | 4.597   | ng    | # 89     |
| 92) Benzo(g,h,i)perylene      | 17.562 | 276  | 29859    | 2.846   | ng    | # 91     |
| -----                         |        |      |          |         |       |          |


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA\_F\Data\BF081925\  
Data File : BF143455.D  
Acq On : 19 Aug 2025 14:28  
Operator : RC/JU  
Sample : Q2879-09  
Misc :  
ALS Vial : 12 Sample Multiplier: 1

Instrument :  
BNA\_F  
ClientSampleId :  
OU4-TS-GRILLO-TSCP07-081425


Quant Time: Aug 19 14:51:40 2025  
Quant Method : Z:\svoasrv\HPCHEM1\BNA\_F\Methods\8270-BF081525.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
QLast Update : Mon Aug 18 04:40:19 2025  
Response via : Initial Calibration

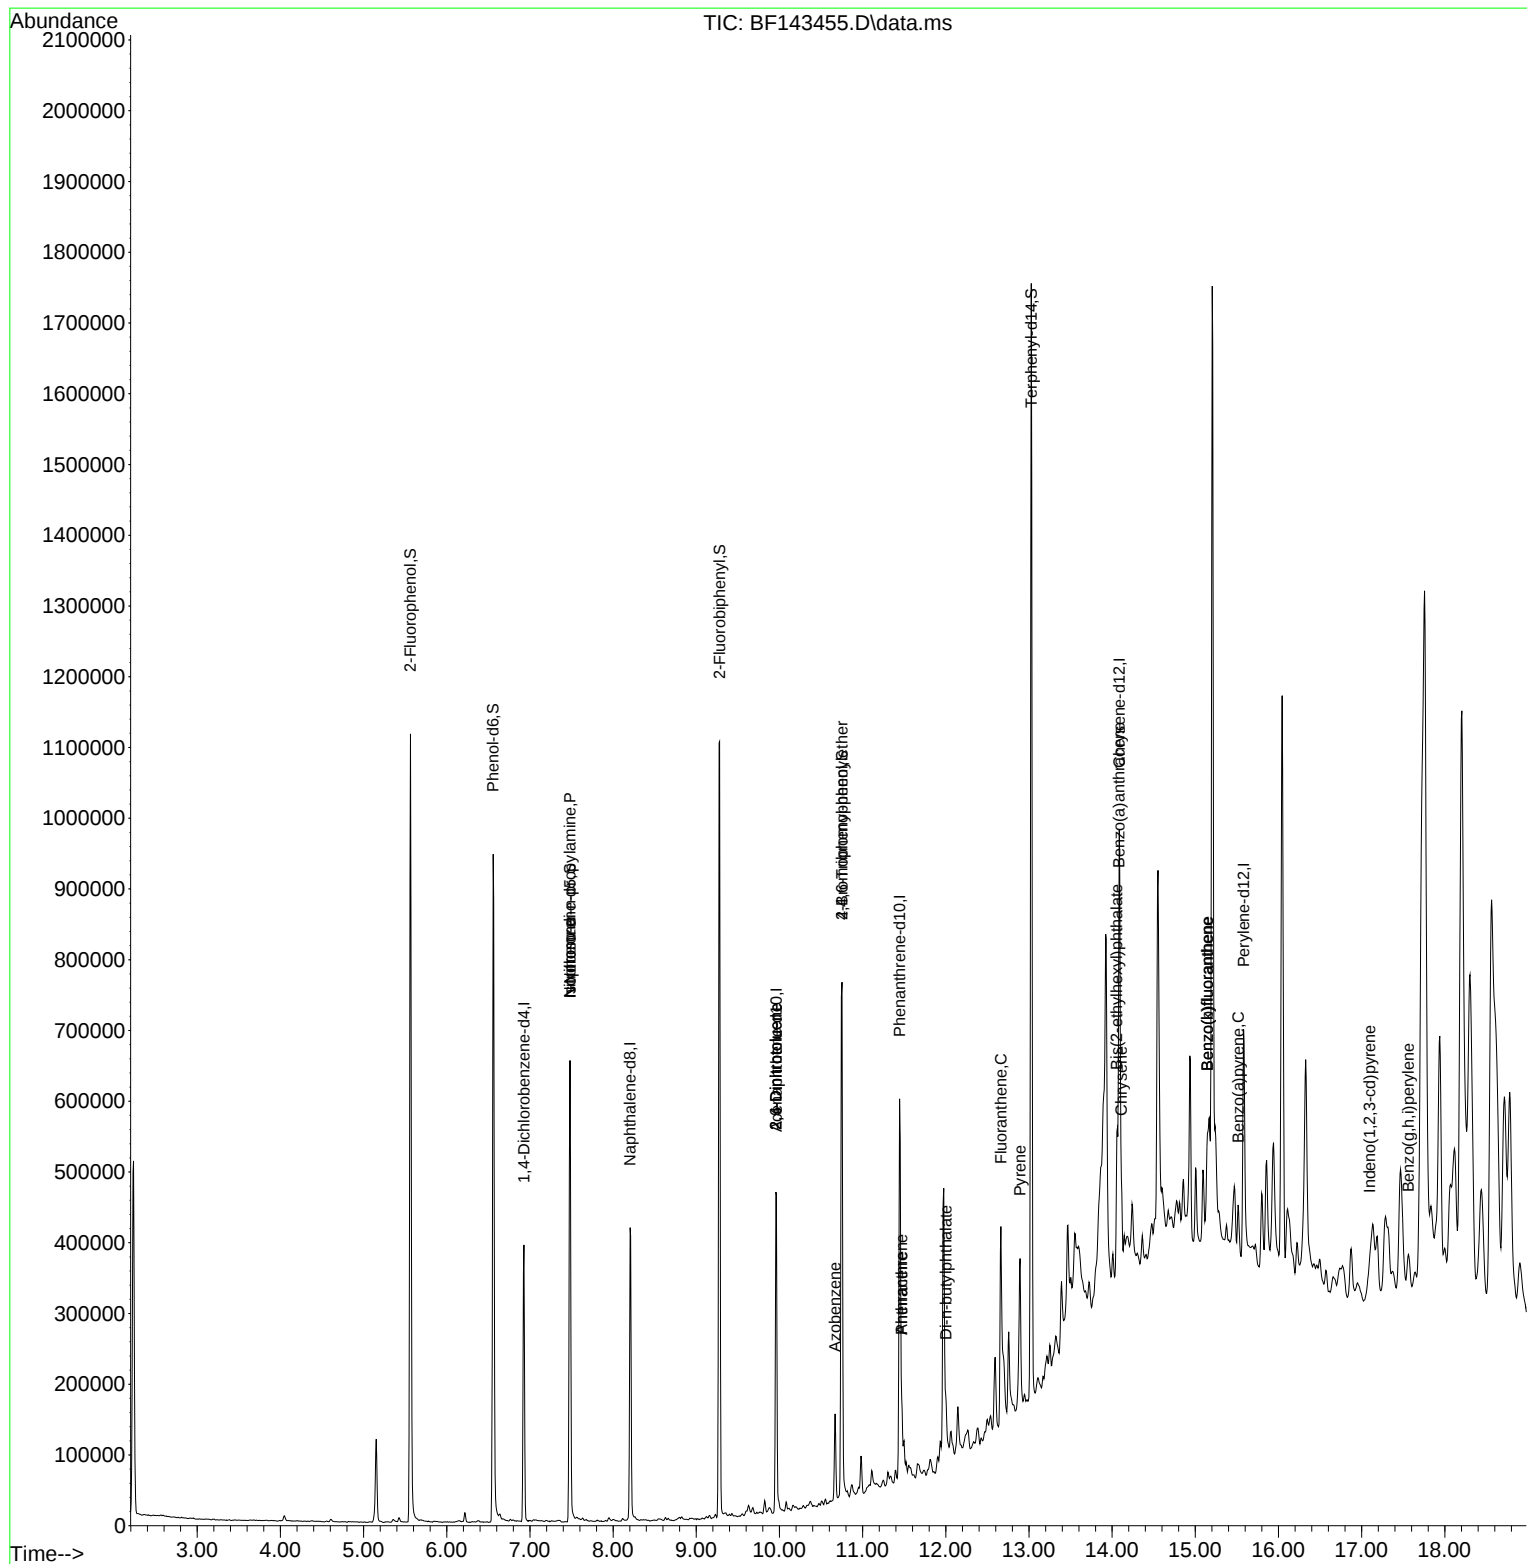






#1  
 1,4-Dichlorobenzene-d4  
 Concen: 20.000 ng  
 RT: 6.928 min Scan# 805  
 Delta R.T. -0.000 min  
 Lab File: BF143455.D  
 Acq: 19 Aug 2025 14:28


Instrument :  
 BNA\_F  
 ClientSampleId :  
 OU4-TS-GRILLO-TSCP07-081425





Tgt Ion:152 Resp: 81535  
 Ion Ratio Lower Upper  
 152 100  
 150 156.4 127.4 191.2  
 115 58.1 47.5 71.3

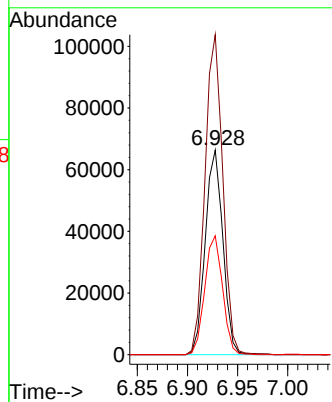


#5  
 2-Fluorophenol  
 Concen: 87.057 ng  
 RT: 5.563 min Scan# 573  
 Delta R.T. 0.006 min  
 Lab File: BF143455.D  
 Acq: 19 Aug 2025 14:28

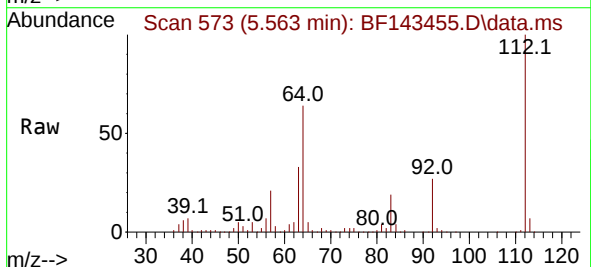

Tgt Ion:112 Resp: 408333  
 Ion Ratio Lower Upper  
 112 100  
 64 64.0 52.2 78.2  
 63 32.5 27.0 40.6



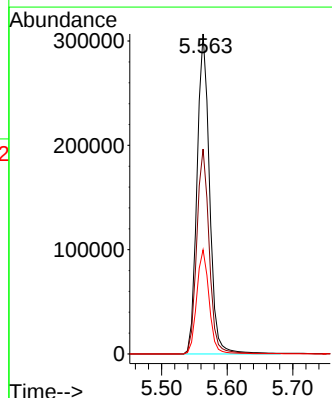





#7  
Phenol-d6  
Concen: 73.960 ng  
RT: 6.557 min Scan# 741  
Delta R.T. -0.000 min  
Lab File: BF143455.D  
Acq: 19 Aug 2025 14:28




Instrument :  
BNA\_F  
ClientSampleId :  
OU4-TS-GRILLO-TSCP07-081425


Tgt Ion: 99 Resp: 437182  
Ion Ratio Lower Upper  
99 100  
42 20.8 17.0 25.6  
71 34.5 27.4 41.2

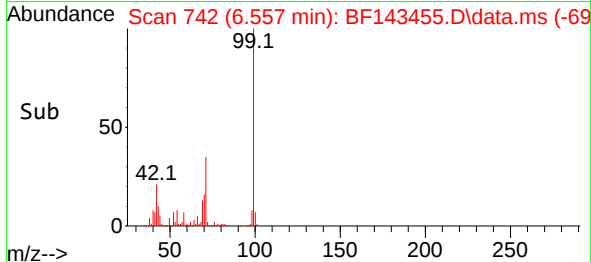

#19  
n-Nitroso-di-n-propylamine  
Concen: 10.070 ng  
RT: 7.481 min Scan# 899  
Delta R.T. 0.147 min  
Lab File: BF143455.D  
Acq: 19 Aug 2025 14:28

Tgt Ion: 70 Resp: 36852  
Ion Ratio Lower Upper  
70 100  
42 52.8 52.5 78.7  
101 0.0 7.9 11.9#  
130 2.5 16.0 24.0#

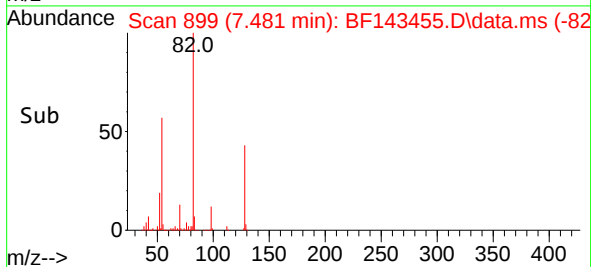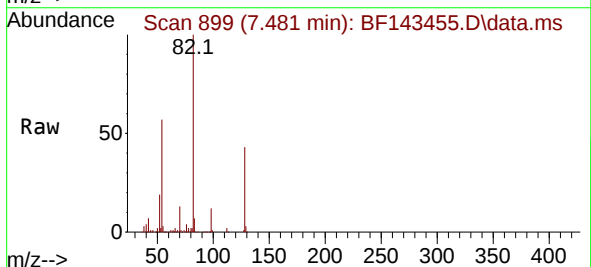



#21

Naphthalene-d8

Concen: 20.000 ng

RT: 8.204 min Scan# 1

Delta R.T. -0.006 min

Lab File: BF143455.D

Acq: 19 Aug 2025 14:28

Instrument :

BNA\_F

ClientSampleId :

OU4-TS-GRILLO-TSCP07-081425

Tgt Ion:136 Resp: 266043





Ion Ratio Lower Upper

136 100

137 11.0 8.8 13.2

54 10.0 7.8 11.8

68 6.4 5.2 7.8

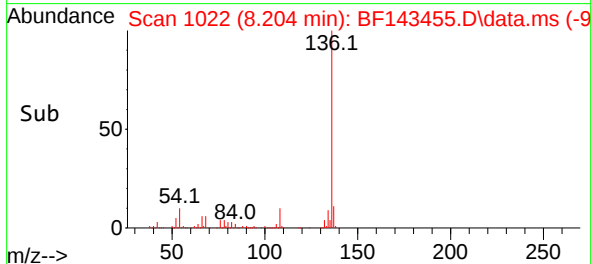

#23

Nitrobenzene-d5

Concen: 61.407 ng

RT: 7.481 min Scan# 899

Delta R.T. -0.006 min

Lab File: BF143455.D

Acq: 19 Aug 2025 14:28




Tgt Ion: 82 Resp: 275314


Ion Ratio Lower Upper

82 100

128 43.1 34.6 52.0

54 57.4 46.0 69.0




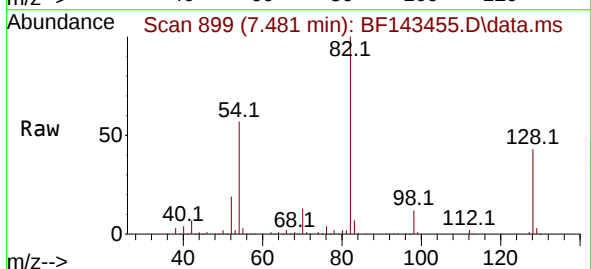




#25  
Isophorone  
Concen: 32.084 ng  
RT: 7.481 min Scan# 899  
Delta R.T. -0.265 min  
Lab File: BF143455.D  
Acq: 19 Aug 2025 14:28




Instrument :  
BNA\_F  
ClientSampleId :  
OU4-TS-GRILLO-TSCP07-081425


Tgt Ion: 82 Resp: 275311  
Ion Ratio Lower Upper  
82 100  
95 0.0 5.6 8.4#  
138 0.0 14.3 21.5#

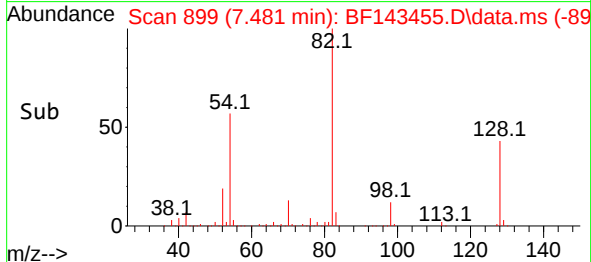

#39  
Acenaphthene-d10  
Concen: 20.000 ng  
RT: 9.963 min Scan# 1321  
Delta R.T. -0.000 min  
Lab File: BF143455.D  
Acq: 19 Aug 2025 14:28

Tgt Ion:164 Resp: 139719  
Ion Ratio Lower Upper  
164 100  
162 99.9 80.6 121.0  
160 42.9 34.6 51.8


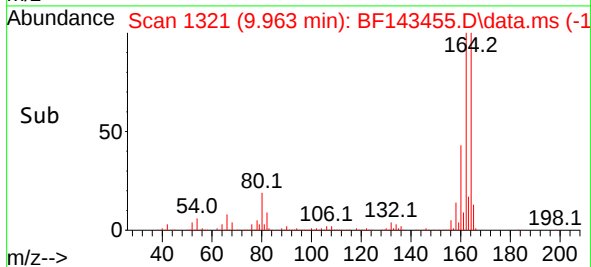

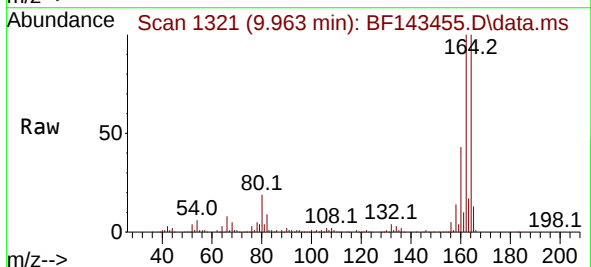




#42  
2,4,6-Tribromophenol  
Concen: 103.505 ng  
RT: 10.751 min Scan# 1455  
Delta R.T. -0.000 min  
Lab File: BF143455.D  
Acq: 19 Aug 2025 14:28




Instrument :  
BNA\_F  
ClientSampleId :  
OU4-TS-GRILLO-TSCP07-081425


Tgt Ion:330 Resp: 128719  
Ion Ratio Lower Upper  
330 100  
332 95.4 77.4 116.2  
141 30.6 24.1 36.1

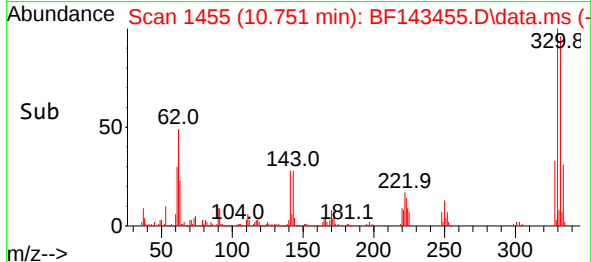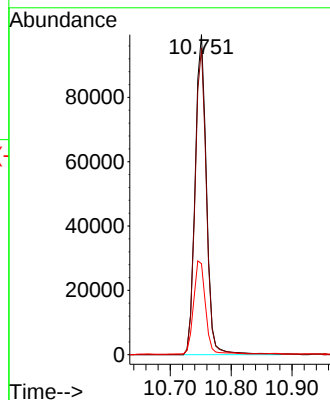

#45  
2-Fluorobiphenyl  
Concen: 60.144 ng  
RT: 9.281 min Scan# 1205  
Delta R.T. -0.000 min  
Lab File: BF143455.D  
Acq: 19 Aug 2025 14:28

Tgt Ion:172 Resp: 499605  
Ion Ratio Lower Upper  
172 100  
171 34.8 28.7 43.1  
170 23.0 19.0 28.6


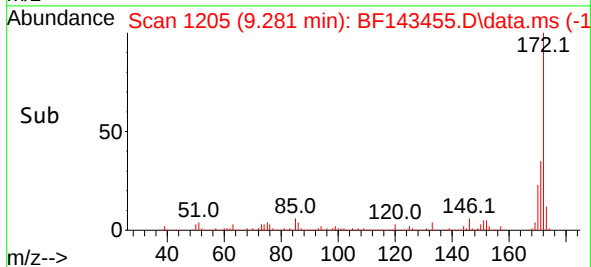
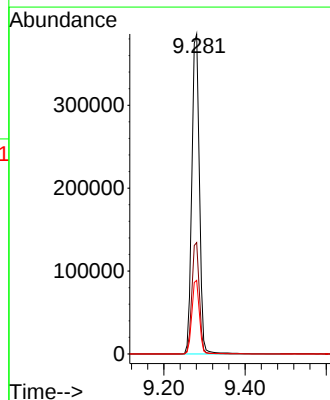
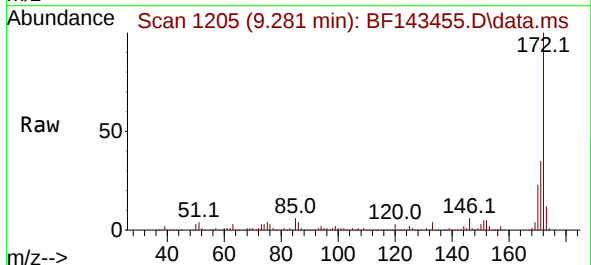




#51  
2,6-Dinitrotoluene  
Concen: 10.798 ng  
RT: 9.957 min Scan# 11  
Delta R.T. 0.218 min  
Lab File: BF143455.D  
Acq: 19 Aug 2025 14:28




Instrument :  
BNA\_F  
ClientSampleId :  
OU4-TS-GRILLO-TSCP07-081425


Tgt Ion:165 Resp: 18542  
Ion Ratio Lower Upper  
165 100  
63 1.8 48.2 72.2#  
89 1.3 44.2 66.2#

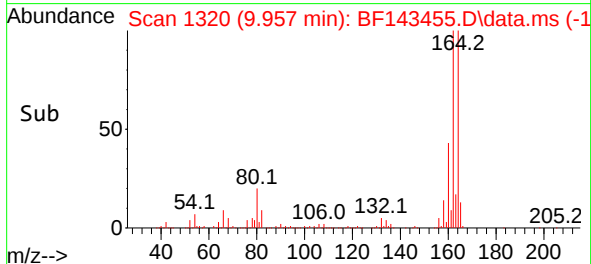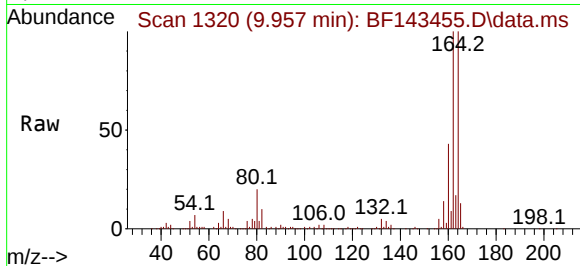

#57  
2,4-Dinitrotoluene  
Concen: 8.099 ng  
RT: 9.957 min Scan# 1320  
Delta R.T. -0.188 min  
Lab File: BF143455.D  
Acq: 19 Aug 2025 14:28

Tgt Ion:165 Resp: 18543  
Ion Ratio Lower Upper  
165 100  
63 1.8 37.0 55.6#  
89 1.3 55.4 83.0#  
182 0.0 2.3 3.5#

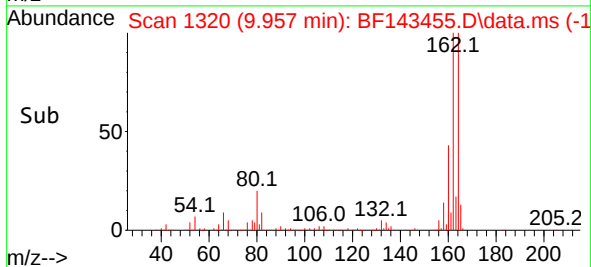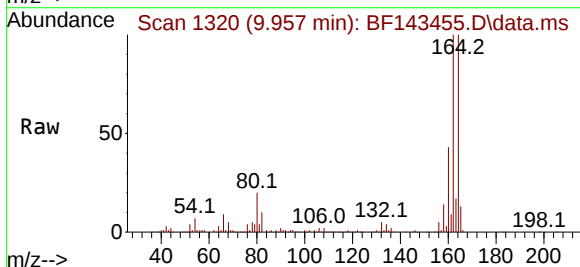



#63

Azobenzene

Concen: 3.733 ng

RT: 10.669 min Scan# 1440

Delta R.T. 0.006 min

Lab File: BF143455.D

Acq: 19 Aug 2025 14:28

Instrument :

BNA\_F

ClientSampleId :

OU4-TS-GRILLO-TSCP07-081425

Tgt Ion: 77 Resp: 30370





Ion Ratio Lower Upper

77 100

182 81.6 7.4 47.4#

105 148.4 1.7 41.7#

51 43.7 12.4 52.4

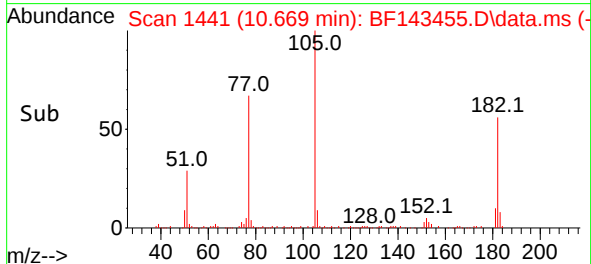

#64

Phenanthrene-d10

Concen: 20.000 ng

RT: 11.445 min Scan# 1573

Delta R.T. -0.006 min

Lab File: BF143455.D

Acq: 19 Aug 2025 14:28




Tgt Ion:188 Resp: 269890


Ion Ratio Lower Upper

188 100

94 10.1 8.0 12.0

80 11.2 8.6 12.8


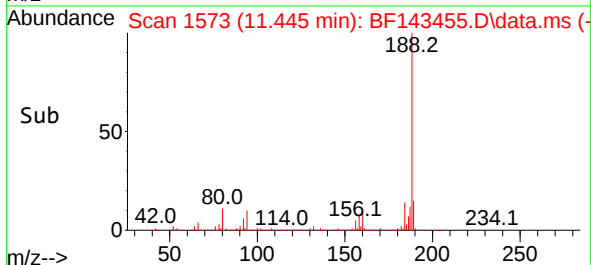
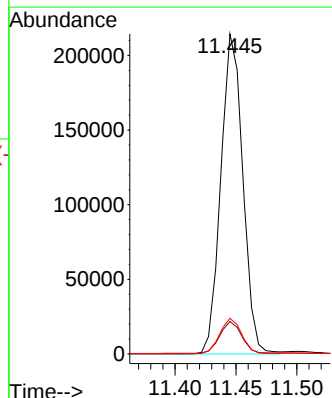
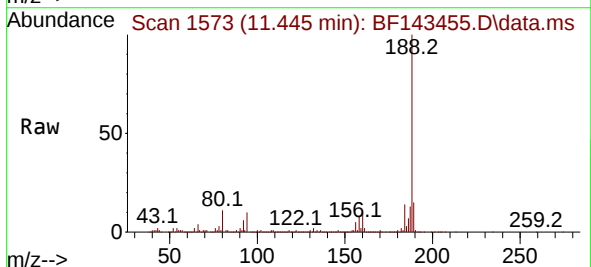




#67  
4-Bromophenyl-phenylether  
Concen: 2.661 ng  
RT: 10.751 min Scan# 1496  
Delta R.T. -0.241 min  
Lab File: BF143455.D  
Acq: 19 Aug 2025 14:28




Instrument :  
BNA\_F  
ClientSampleId :  
OU4-TS-GRILLO-TSCP07-081425


Tgt Ion:248 Resp: 8482  
Ion Ratio Lower Upper  
248 100  
250 206.4 78.6 118.0#  
141 436.7 54.9 82.3#

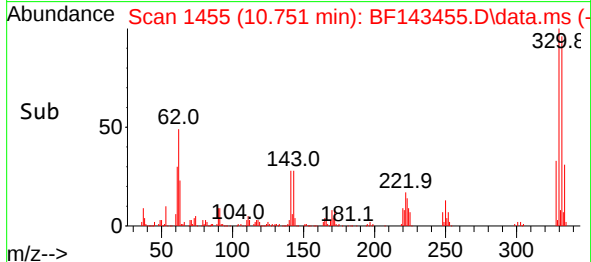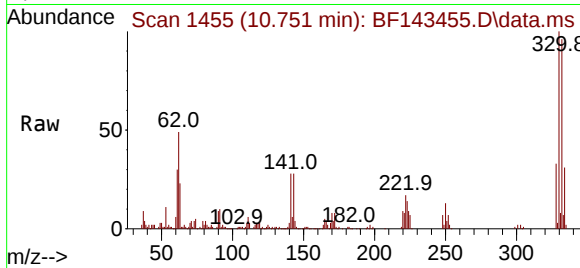

#71  
Phenanthrene  
Concen: 3.011 ng  
RT: 11.469 min Scan# 1577  
Delta R.T. -0.006 min  
Lab File: BF143455.D  
Acq: 19 Aug 2025 14:28

Tgt Ion:178 Resp: 43999  
Ion Ratio Lower Upper  
178 100  
176 19.1 15.4 23.0  
179 14.9 12.3 18.5


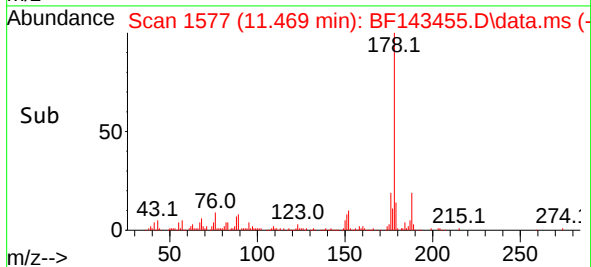

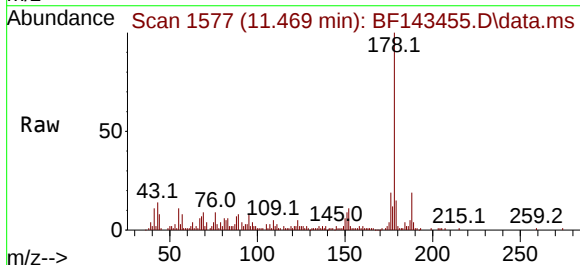




#72  
 Anthracene  
 Concen: 2.981 ng  
 RT: 11.469 min Scan# 1587  
 Delta R.T. -0.059 min  
 Lab File: BF143455.D  
 Acq: 19 Aug 2025 14:28




Instrument : BNA\_F  
 ClientSampleId : OU4-TS-GRILLO-TSCP07-081425


|             |       |           |
|-------------|-------|-----------|
| Tgt Ion:178 | Resp: | 43999     |
| Ion Ratio   | Lower | Upper     |
| 178         | 100   |           |
| 176         | 19.1  | 14.8 22.2 |
| 179         | 14.9  | 12.2 18.4 |

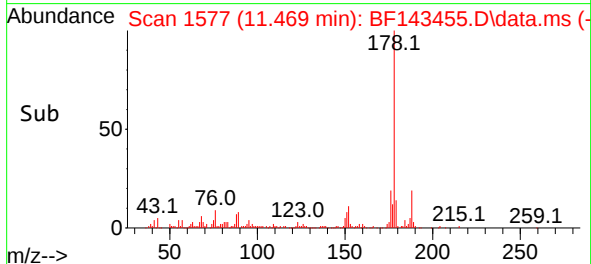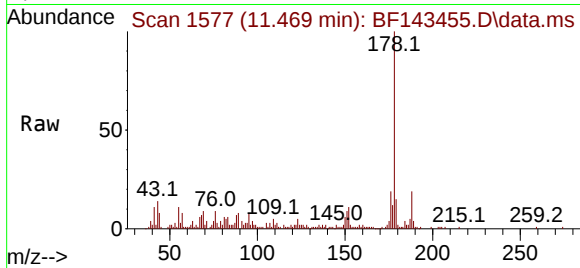

#74  
 Di-n-butylphthalate  
 Concen: 2.424 ng  
 RT: 12.004 min Scan# 1668  
 Delta R.T. -0.000 min  
 Lab File: BF143455.D  
 Acq: 19 Aug 2025 14:28

|             |       |          |
|-------------|-------|----------|
| Tgt Ion:149 | Resp: | 30134    |
| Ion Ratio   | Lower | Upper    |
| 149         | 100   |          |
| 150         | 10.4  | 7.3 10.9 |
| 104         | 4.8   | 3.8 5.6  |

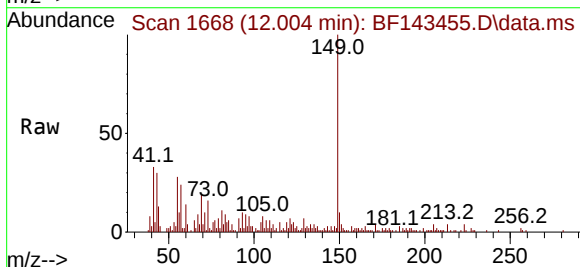



#75

Fluoranthene

Concen: 10.547 ng

RT: 12.663 min Scan# 1

Delta R.T. -0.000 min

Lab File: BF143455.D

Acq: 19 Aug 2025 14:28

Instrument :

BNA\_F

ClientSampleId :

OU4-TS-GRILLO-TSCP07-081425





Tgt Ion:202 Resp: 136964

Ion Ratio Lower Upper

202 100

101 10.8 0.0 31.5

203 18.0 0.0 37.5

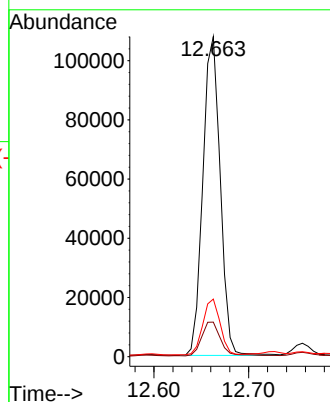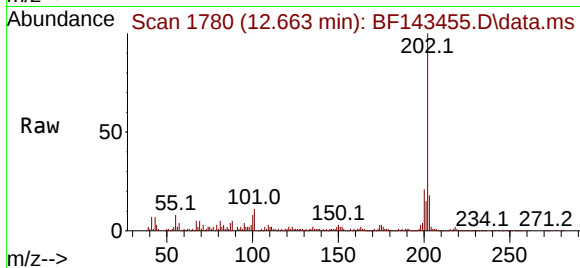

#76

Chrysene-d12

Concen: 20.000 ng

RT: 14.086 min Scan# 2022

Delta R.T. -0.000 min

Lab File: BF143455.D

Acq: 19 Aug 2025 14:28




Tgt Ion:240 Resp: 272023


Ion Ratio Lower Upper

240 100

120 11.2 9.0 13.4

236 25.4 20.2 30.2

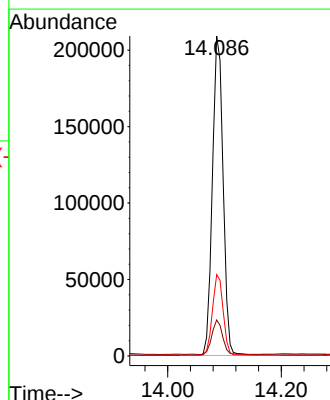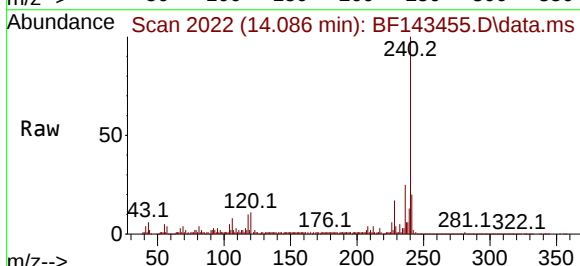



#78

Pyrene

Concen: 5.201 ng

RT: 12.892 min Scan# 1819

Delta R.T. -0.000 min

Lab File: BF143455.D

Acq: 19 Aug 2025 14:28

Instrument :

BNA\_F

ClientSampleId :

OU4-TS-GRILLO-TSCP07-081425





Tgt Ion:202 Resp: 122974

Ion Ratio Lower Upper

202 100

200 21.1 17.1 25.7

203 18.1 14.2 21.2

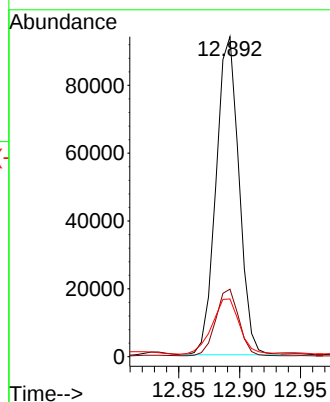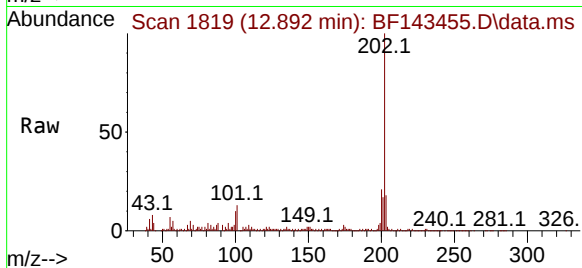

#79

Terphenyl-d14

Concen: 46.649 ng

RT: 13.027 min Scan# 1842

Delta R.T. -0.000 min

Lab File: BF143455.D

Acq: 19 Aug 2025 14:28




Tgt Ion:244 Resp: 755405


Ion Ratio Lower Upper

244 100

212 6.7 5.2 7.8

122 10.2 8.3 12.5

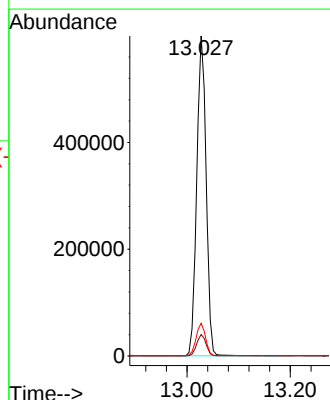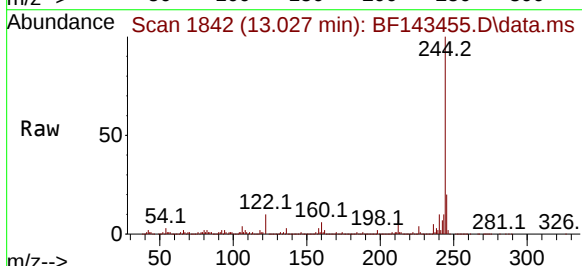



#81

Benzo(a)anthracene

Concen: 3.922 ng

RT: 14.080 min Scan# 2020

Delta R.T. 0.006 min

Lab File: BF143455.D

Acq: 19 Aug 2025 14:28

Instrument :

BNA\_F

ClientSampleId :

OU4-TS-GRILLO-TSCP07-081425





Tgt Ion:228 Resp: 67916

Ion Ratio Lower Upper

228 100

226 30.8 21.5 32.3

229 22.7 15.7 23.5

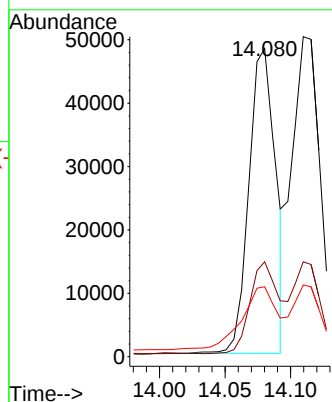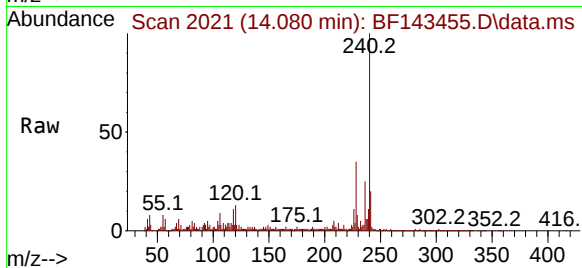

#83

Chrysene

Concen: 4.659 ng

RT: 14.110 min Scan# 2026

Delta R.T. -0.000 min

Lab File: BF143455.D

Acq: 19 Aug 2025 14:28




Tgt Ion:228 Resp: 74599


Ion Ratio Lower Upper

228 100

226 29.7 24.3 36.5

229 22.4 16.1 24.1




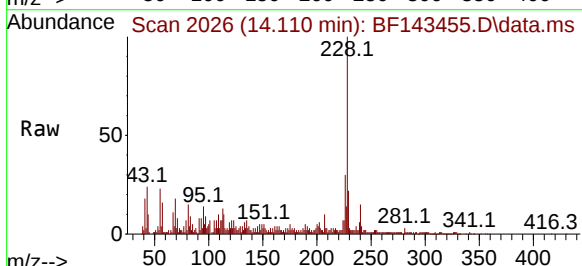




#84  
 Bis(2-ethylhexyl)phthalate  
 Concen: 8.979 ng  
 RT: 14.057 min Scan# 2017  
 Delta R.T. -0.000 min  
 Lab File: BF143455.D  
 Acq: 19 Aug 2025 14:28




Instrument :  
 BNA\_F  
 ClientSampleId :  
 OU4-TS-GRILLO-TSCP07-081425


|           |       |       |       |
|-----------|-------|-------|-------|
| Tgt Ion:  | 149   | Resp: | 74678 |
| Ion Ratio | Lower | Upper |       |
| 149       | 100   |       |       |
| 167       | 27.1  | 22.6  | 33.8  |
| 279       | 4.9   | 3.5   | 5.3   |

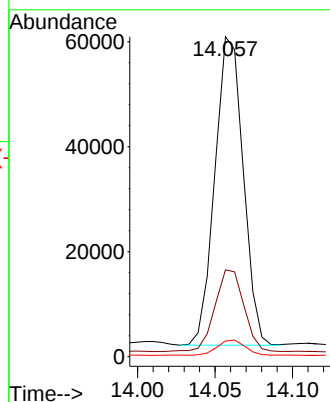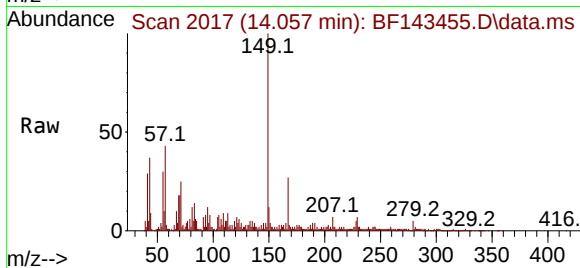

#86  
 Perylene-d12  
 Concen: 20.000 ng  
 RT: 15.580 min Scan# 2276  
 Delta R.T. 0.006 min  
 Lab File: BF143455.D  
 Acq: 19 Aug 2025 14:28

|           |       |       |        |
|-----------|-------|-------|--------|
| Tgt Ion:  | 264   | Resp: | 174368 |
| Ion Ratio | Lower | Upper |        |
| 264       | 100   |       |        |
| 260       | 22.4  | 18.8  | 28.2   |
| 265       | 21.6  | 17.4  | 26.0   |

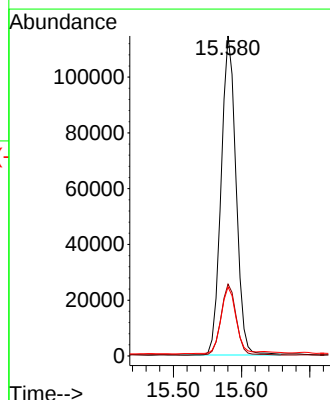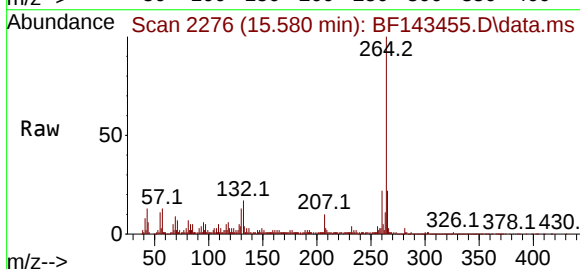



#87

Indeno(1,2,3-cd)pyrene

Concen: 2.239 ng

RT: 17.098 min Scan# 21

Delta R.T. -0.000 min

Lab File: BF143455.D

Acq: 19 Aug 2025 14:28





Instrument :

BNA\_F

ClientSampleId :

OU4-TS-GRILLO-TSCP07-081425

|          |       |       |       |
|----------|-------|-------|-------|
| Tgt Ion: | 276   | Resp: | 29277 |
| Ion      | Ratio | Lower | Upper |
| 276      | 100   |       |       |
| 138      | 21.5  | 20.2  | 30.4  |
| 277      | 25.2  | 20.2  | 30.2  |

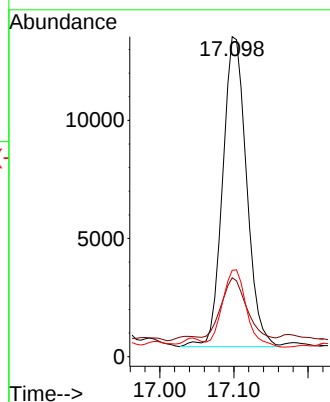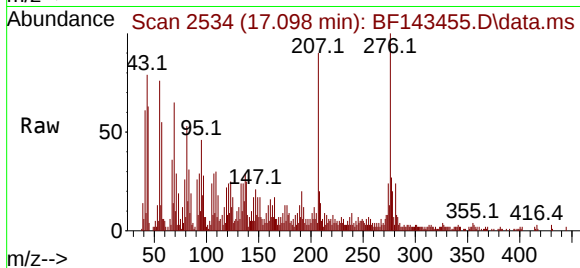

#88

Benzo(b)fluoranthene

Concen: 10.108 ng




RT: 15.145 min Scan# 2202


Delta R.T. 0.006 min

Lab File: BF143455.D

Acq: 19 Aug 2025 14:28

|          |       |       |       |
|----------|-------|-------|-------|
| Tgt Ion: | 252   | Resp: | 94459 |
| Ion      | Ratio | Lower | Upper |
| 252      | 100   |       |       |
| 253      | 24.3  | 17.1  | 25.7  |
| 125      | 17.9  | 7.5   | 11.3  |

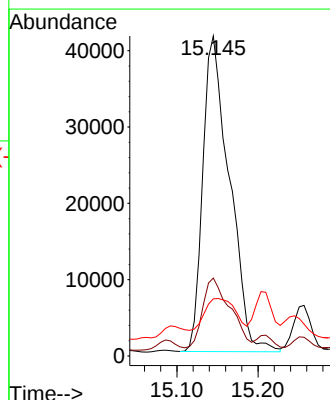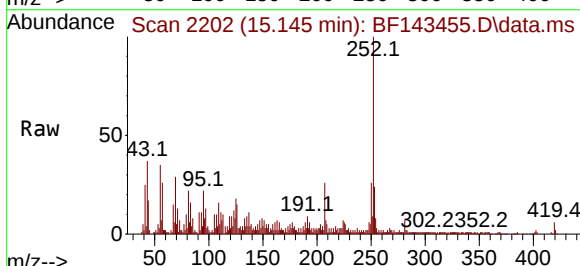



#89

Benzo(k)fluoranthene

Concen: 10.248 ng

RT: 15.145 min Scan# 21

Delta R.T. -0.024 min

Lab File: BF143455.D

Acq: 19 Aug 2025 14:28





Instrument :

BNA\_F

ClientSampleId :

OU4-TS-GRILLO-TSCP07-081425

|             |       |           |
|-------------|-------|-----------|
| Tgt Ion:252 | Resp: | 94459     |
| Ion Ratio   | Lower | Upper     |
| 252         | 100   |           |
| 253         | 24.3  | 17.2 25.8 |
| 125         | 17.9  | 7.4 11.2# |

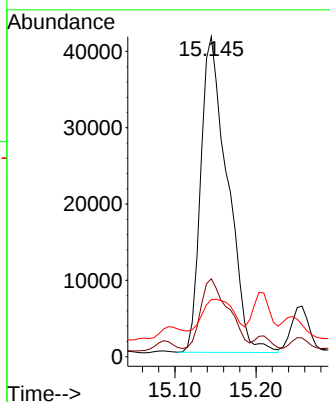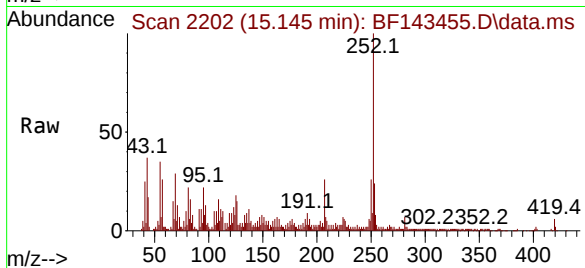

#90

Benzo(a)pyrene

Concen: 4.597 ng




RT: 15.515 min Scan# 2265


Delta R.T. 0.006 min

Lab File: BF143455.D

Acq: 19 Aug 2025 14:28


|             |       |            |
|-------------|-------|------------|
| Tgt Ion:252 | Resp: | 40917      |
| Ion Ratio   | Lower | Upper      |
| 252         | 100   |            |
| 253         | 26.3  | 17.4 26.2# |
| 125         | 16.1  | 8.6 12.8#  |

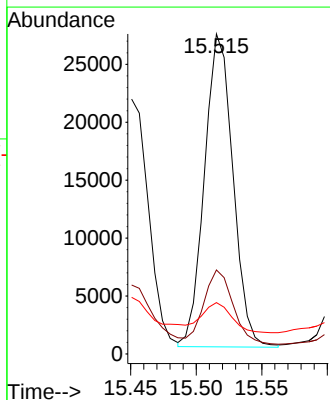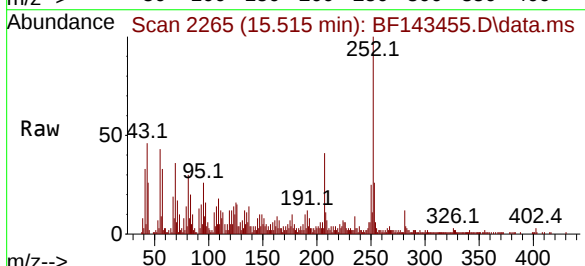



#92  
 Benzo(g,h,i)perylene  
 Concen: 2.846 ng  
 RT: 17.562 min Scan# 20  
 Delta R.T. 0.012 min  
 Lab File: BF143455.D  
 Acq: 19 Aug 2025 14:28

Instrument :  
 BNA\_F  
 ClientSampleId :  
 OU4-TS-GRILLO-TSCP07-081425

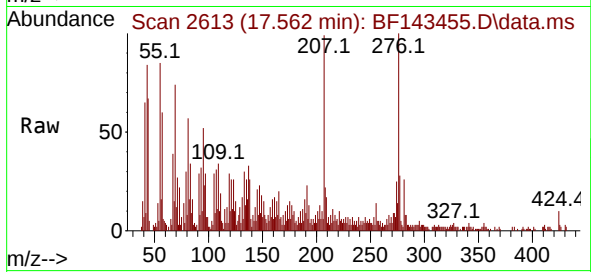

|           |       |       |       |
|-----------|-------|-------|-------|
| Tgt Ion:  | 276   | Resp: | 29859 |
| Ion Ratio | Lower | Upper |       |
| 276       | 100   |       |       |
| 277       | 27.8  | 18.7  | 28.1  |
| 138       | 26.4  | 17.5  | 26.3  |

