

Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY082025\
 Data File : VY023168.D
 Acq On : 20 Aug 2025 12:14
 Operator : SY/MD
 Sample : Q2879-09
 Misc : 4.25g/5.0mL/MSVOA_Y/SOIL/B
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 MSVOA_Y
 ClientSampleId :
 OU4-TS-GRILLO-TSCP07-081425

Quant Time: Aug 20 15:23:48 2025
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y081225S.M
 Quant Title : SW846 8260
 QLast Update : Wed Aug 13 02:10:11 2025
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Pentafluorobenzene	7.707	168	516659	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	8.616	114	966938	50.000	ug/l	0.00
63) Chlorobenzene-d5	11.414	117	789139	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.347	152	248201	50.000	ug/l	0.00

System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	8.061	65	276384	56.129	ug/l	0.00
Spiked Amount	50.000	Range	50 - 163	Recovery	=	112.260%
35) Dibromofluoromethane	7.634	113	310612	53.685	ug/l	0.00
Spiked Amount	50.000	Range	54 - 147	Recovery	=	107.360%
50) Toluene-d8	10.103	98	1144603	50.640	ug/l	0.00
Spiked Amount	50.000	Range	58 - 134	Recovery	=	101.280%
62) 4-Bromofluorobenzene	12.402	95	303850	41.801	ug/l	0.00
Spiked Amount	50.000	Range	30 - 143	Recovery	=	83.600%


Target Compounds	Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY082025\
Data File : VY023168.D
Acq On : 20 Aug 2025 12:14
Operator : SY/MD
Sample : Q2879-09
Misc : 4.25g/5.0mL/MSVOA_Y/SOIL/B
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_Y
ClientSampleId :
OU4-TS-GRILLO-TSCP07-081425

Quant Time: Aug 20 15:23:48 2025
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y081225S.M
Quant Title : SW846 8260
QLast Update : Wed Aug 13 02:10:11 2025
Response via : Initial Calibration




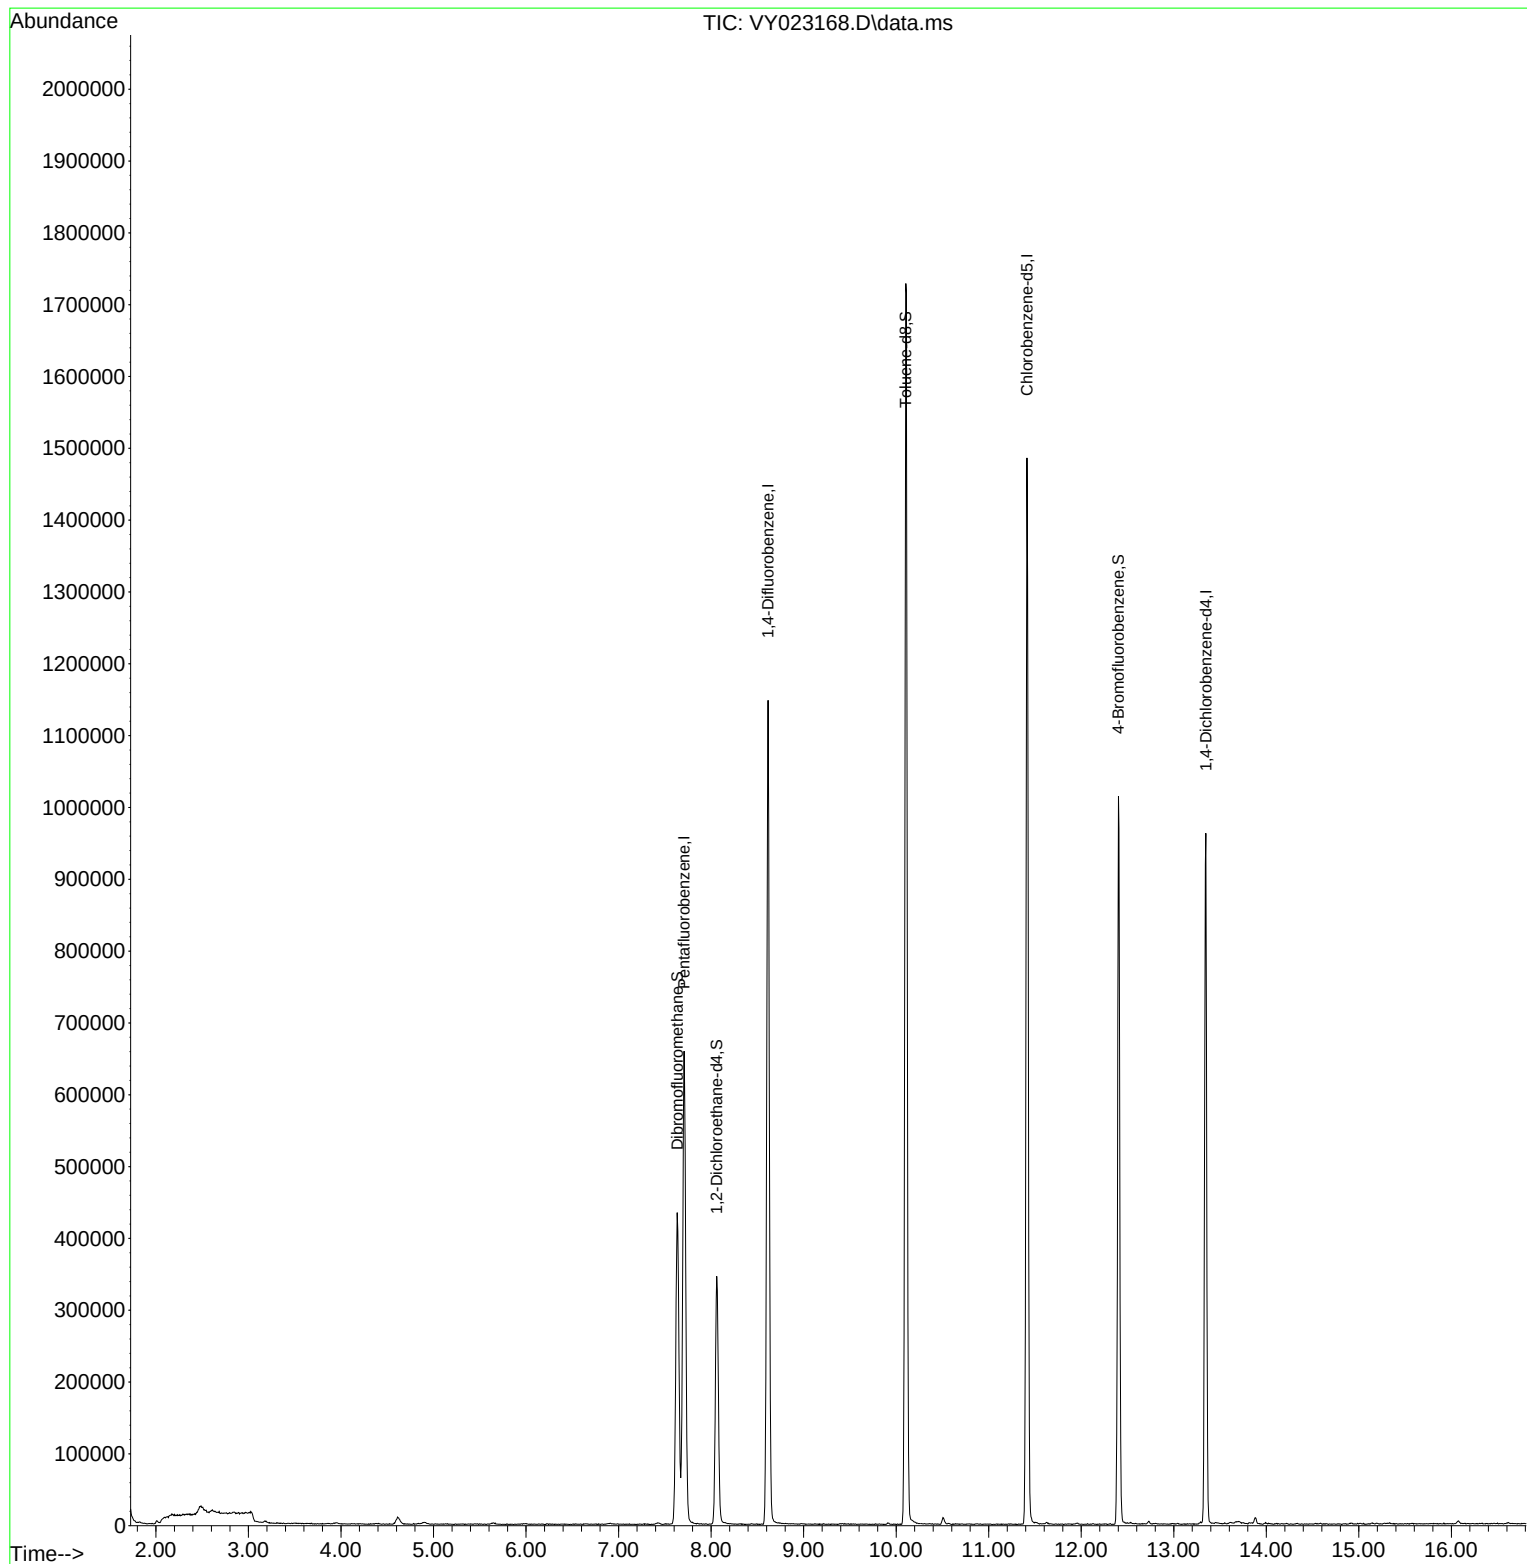


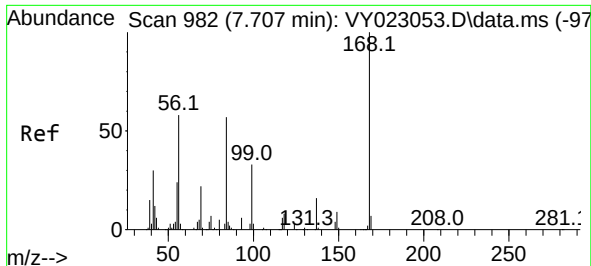

#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 7.707 min Scan# 91
Delta R.T. 0.000 min
Lab File: VY023168.D
Acq: 20 Aug 2025 12:14




Instrument :
MSVOA_Y
ClientSampleId :
OU4-TS-GRILLO-TSCP07-081425


Tgt Ion:168 Resp: 516659
Ion Ratio Lower Upper
168 100
99 54.0 42.8 64.2

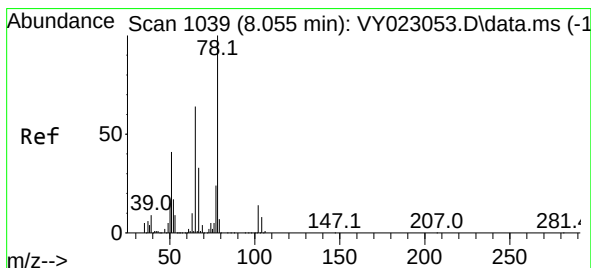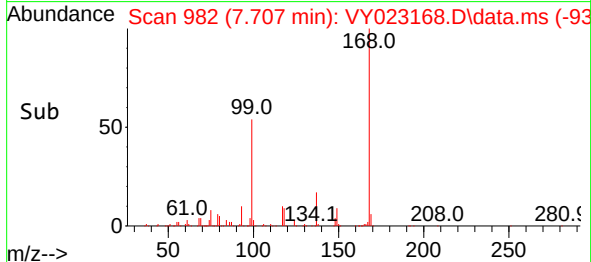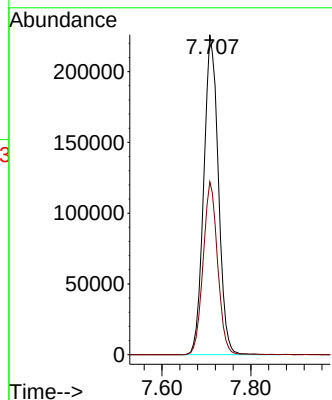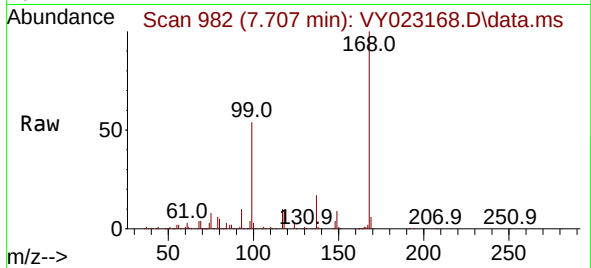

#33
1,2-Dichloroethane-d4
Concen: 56.129 ug/l
RT: 8.061 min Scan# 1040
Delta R.T. 0.006 min
Lab File: VY023168.D
Acq: 20 Aug 2025 12:14

Tgt Ion: 65 Resp: 276384
Ion Ratio Lower Upper
65 100
67 52.7 0.0 106.8


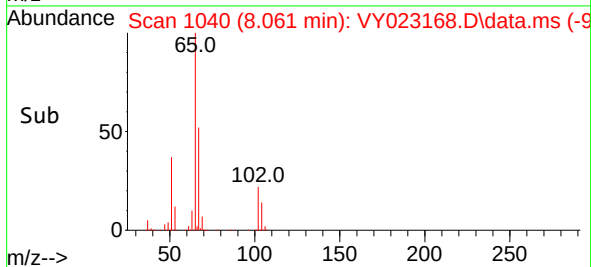
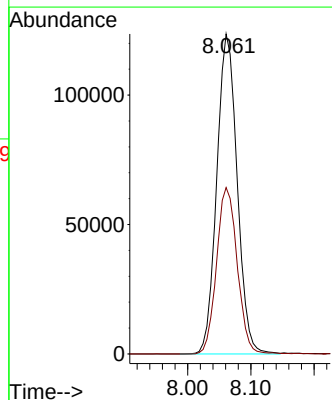
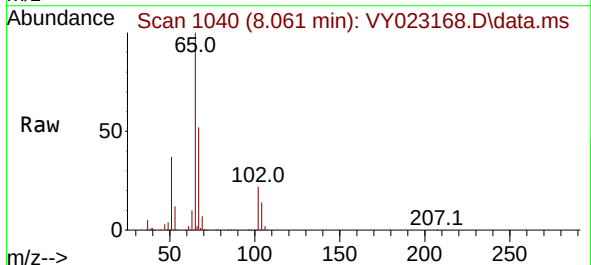


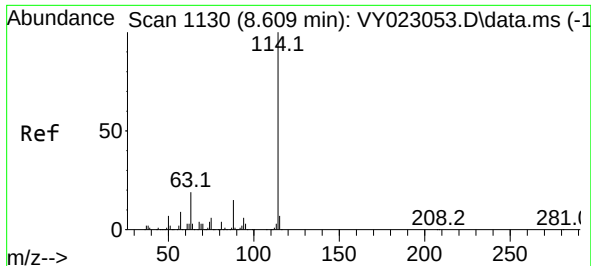

#34
1,4-Difluorobenzene
Concen: 50.000 ug/l
RT: 8.616 min Scan# 1131
Delta R.T. 0.006 min
Lab File: VY023168.D
Acq: 20 Aug 2025 12:14




Instrument :
MSVOA_Y
ClientSampleId :
OU4-TS-GRILLO-TSCP07-081425


Tgt Ion:114 Resp: 966938
Ion Ratio Lower Upper
114 100
63 18.1 0.0 38.4
88 14.7 0.0 30.0

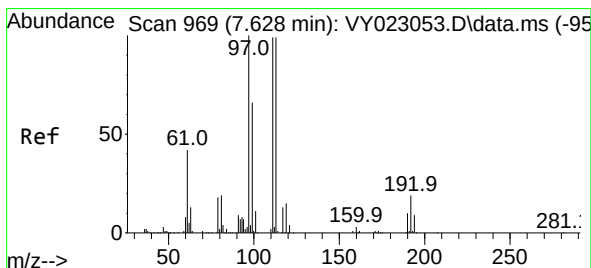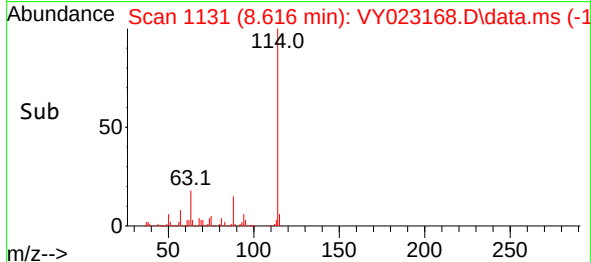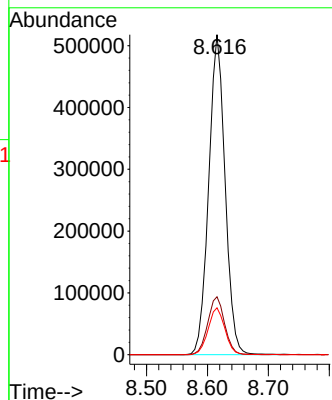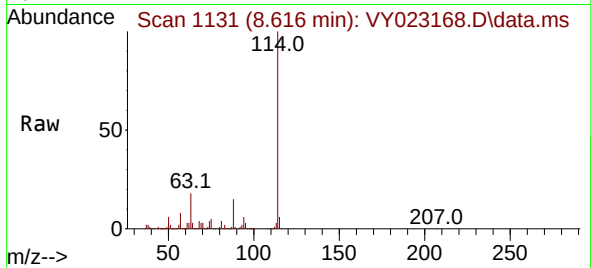

#35
Dibromofluoromethane
Concen: 53.685 ug/l
RT: 7.634 min Scan# 970
Delta R.T. 0.006 min
Lab File: VY023168.D
Acq: 20 Aug 2025 12:14

Tgt Ion:113 Resp: 310612
Ion Ratio Lower Upper
113 100
111 102.6 81.1 121.7
192 19.6 16.2 24.4


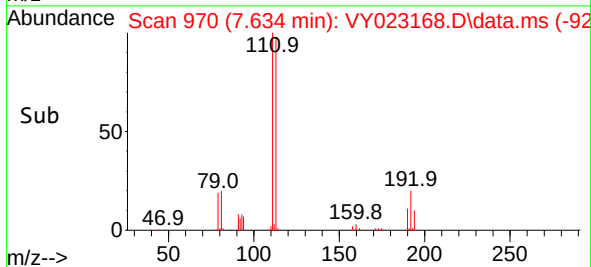
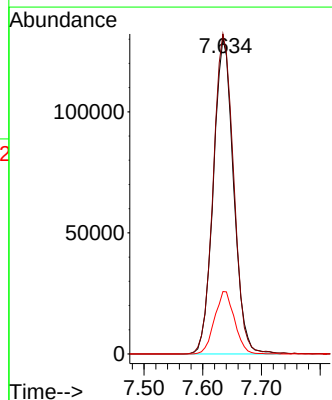
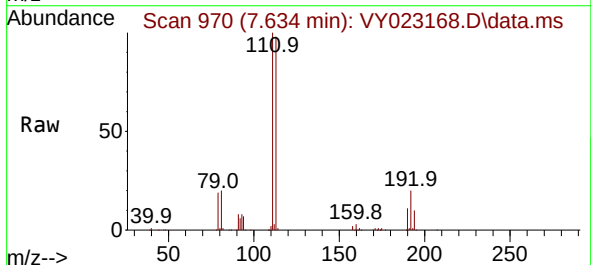


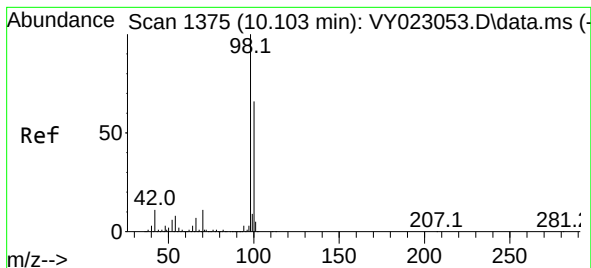

#50
Toluene-d8
Concen: 50.640 ug/l
RT: 10.103 min Scan# 11
Delta R.T. 0.000 min
Lab File: VY023168.D
Acq: 20 Aug 2025 12:14




Instrument :
MSVOA_Y
ClientSampleId :
OU4-TS-GRILLO-TSCP07-081425


Tgt Ion: 98 Resp: 1144603
Ion Ratio Lower Upper
98 100
100 65.4 52.3 78.5

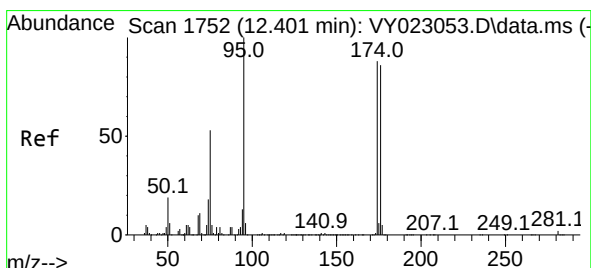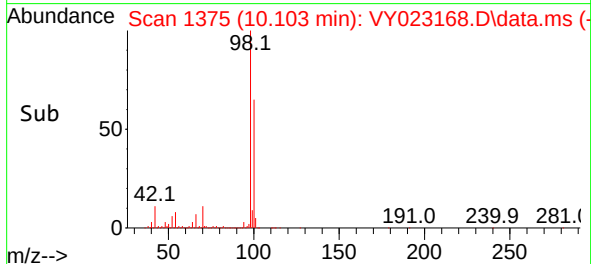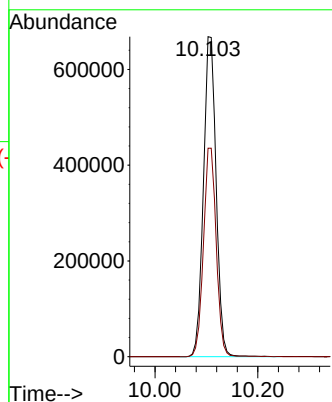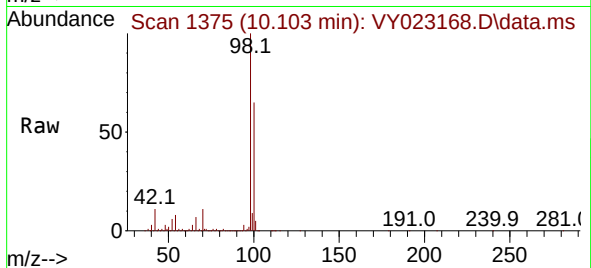

#62
4-Bromofluorobenzene
Concen: 41.801 ug/l
RT: 12.402 min Scan# 1752
Delta R.T. 0.000 min
Lab File: VY023168.D
Acq: 20 Aug 2025 12:14

Tgt Ion: 95 Resp: 303850
Ion Ratio Lower Upper
95 100
174 88.6 0.0 171.6
176 85.4 0.0 167.6


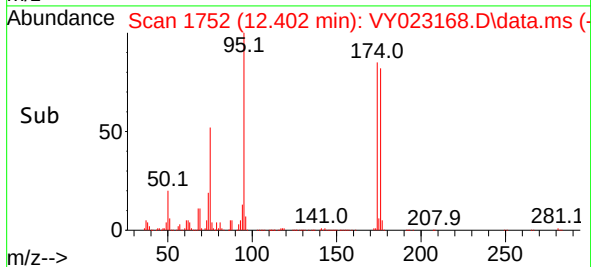
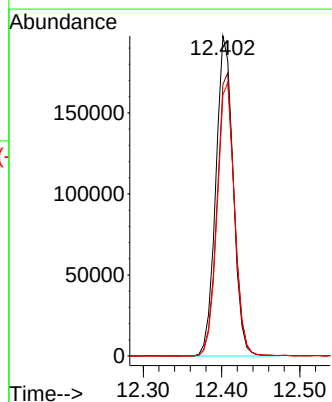
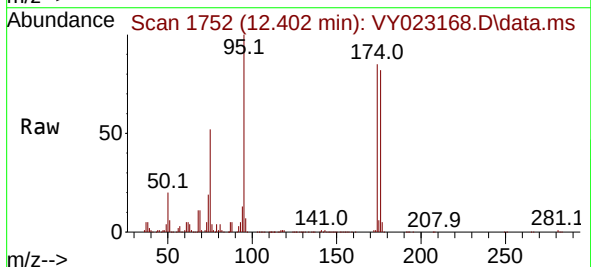


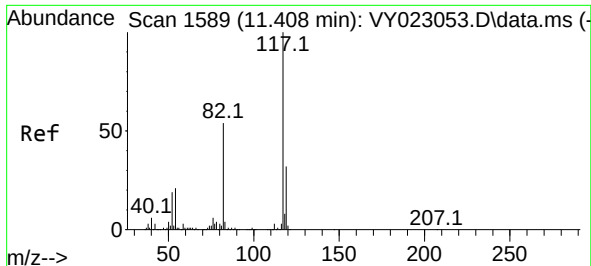

#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 11.414 min Scan# 11
Delta R.T. 0.006 min
Lab File: VY023168.D
Acq: 20 Aug 2025 12:14

Instrument :
MSVOA_Y
ClientSampleId :
OU4-TS-GRILLO-TSCP07-081425

Tgt Ion:117 Resp: 789139
Ion Ratio Lower Upper
117 100
82 54.5 43.4 65.0
119 32.1 25.6 38.4

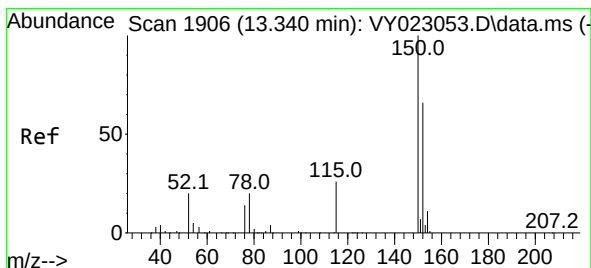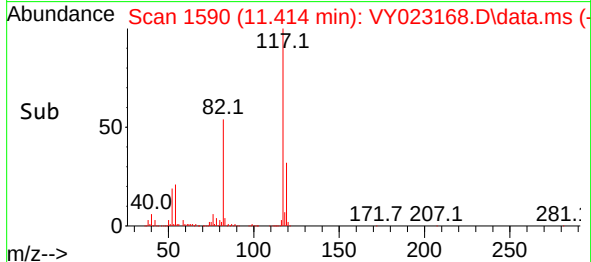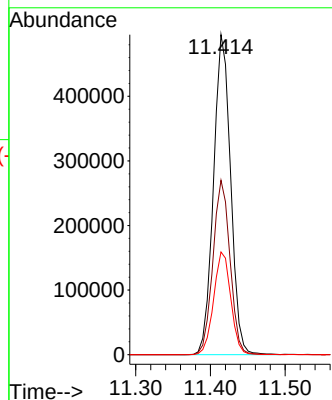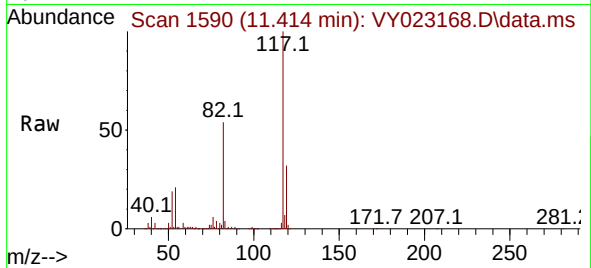

#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 13.347 min Scan# 1907
Delta R.T. 0.006 min
Lab File: VY023168.D
Acq: 20 Aug 2025 12:14

Tgt Ion:152 Resp: 248201
Ion Ratio Lower Upper
152 100
115 56.6 28.2 84.6
150 158.3 0.0 348.0

