


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN081925\
Data File : BN037617.D
Acq On : 20 Aug 2025 03:35
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270-SIM-BN081225.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Wed Aug 13 05:00:58 2025

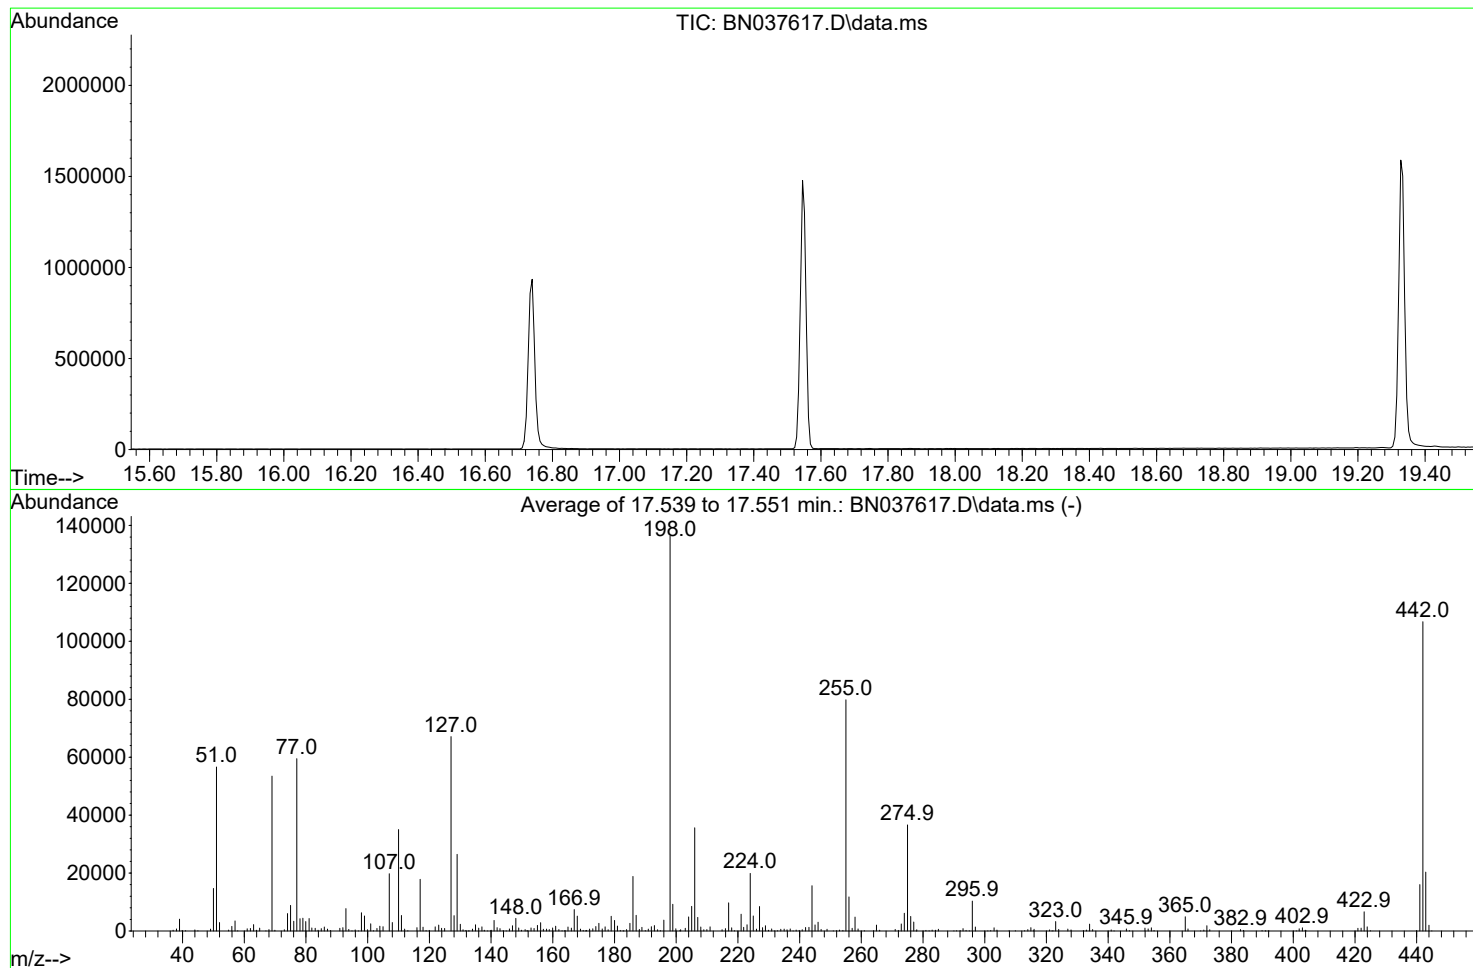

AutoFind: Scans 2457, 2458, 2459; Background Corrected with Scan 2451

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
68	69	0.00	2	0.9	485	PASS
69	69	100	100	100.0	53448	PASS
70	69	0.00	2	0.6	308	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	136293	PASS
199	198	5	9	6.8	9235	PASS
365	198	1	100	3.6	4939	PASS
441	443	0.01	150	79.0	16038	PASS
442	442	100	100	100.0	106744	PASS
443	442	15	24	19.0	20305	PASS

DDT Breakdown




Date	Instrument Name	DFTPP Data File
8/19/2025	BNA_N	<u>BN037617.D</u>
Compound Name	Response	Retention Time
DDT	466043	20.575
DDD	8008	20.133
DDE	521	19.628
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
8529	474572	1.80

Instrument :
BNA_N
ClientSampleId :
DFTPP

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN081925\
Data File : BN037617.D
Acq On : 20 Aug 2025 03:35
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: Aug 20 07:01:46 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Aug 06 01:49:15 2025
Response via : Initial Calibration

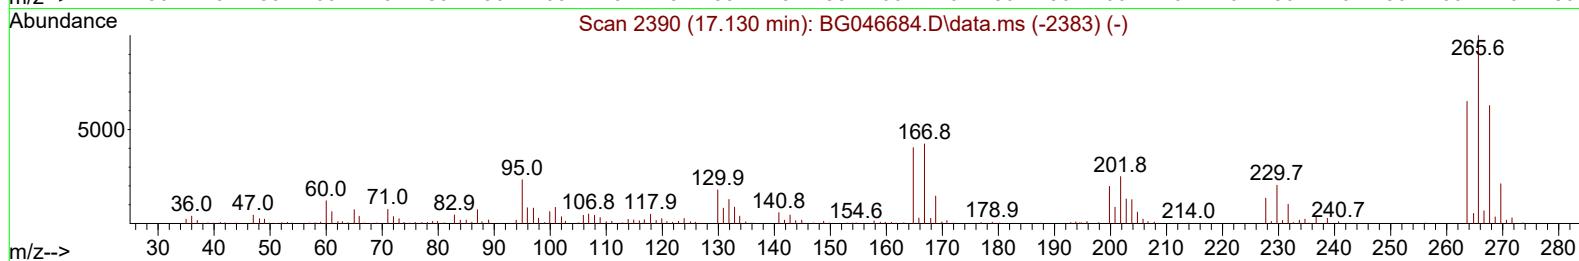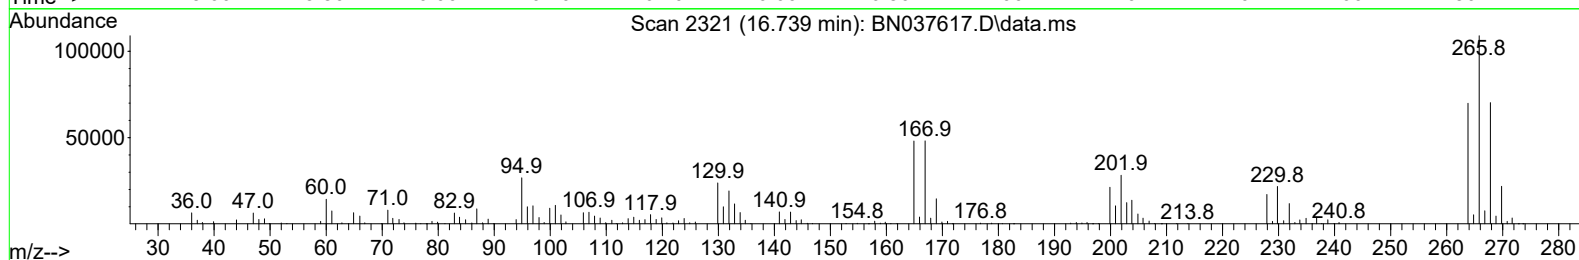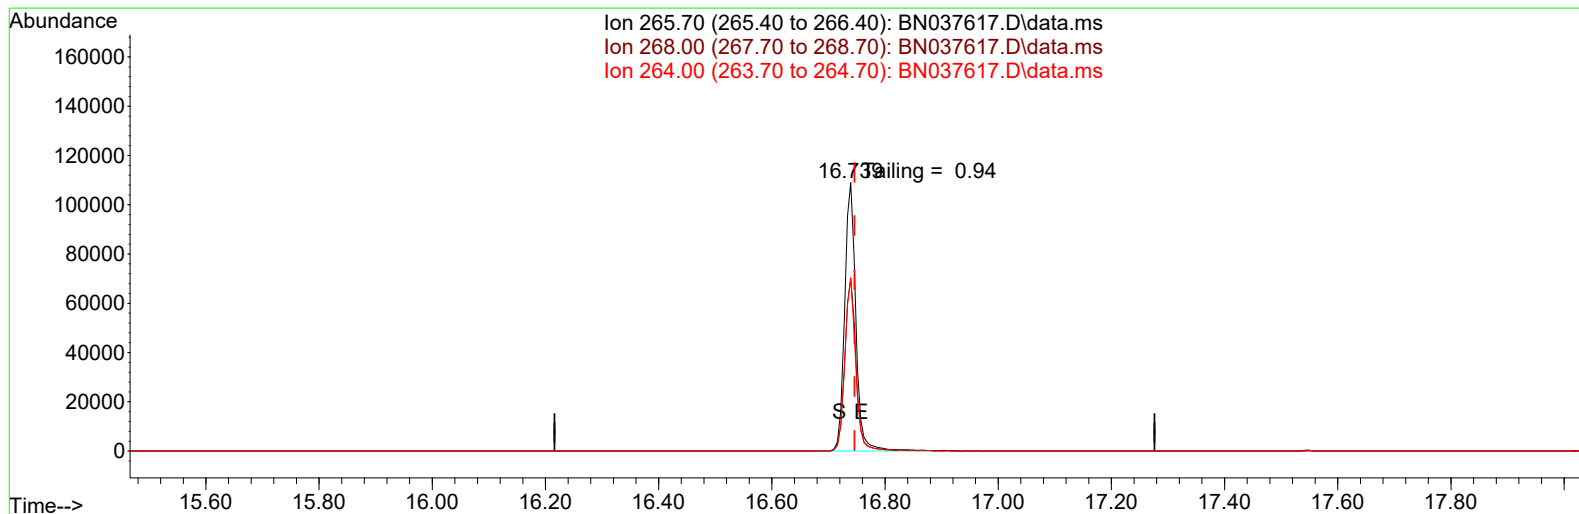

TIC: BN037617.D\data.ms

(70) Pentachlorophenol (C)

16.739min (-0.006) 24577.65 ng




response 150060

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	64.52
264.00	61.60	64.16
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN081925\
Data File : BN037617.D
Acq On : 20 Aug 2025 03:35
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: Aug 20 07:01:46 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Aug 06 01:49:15 2025
Response via : Initial Calibration

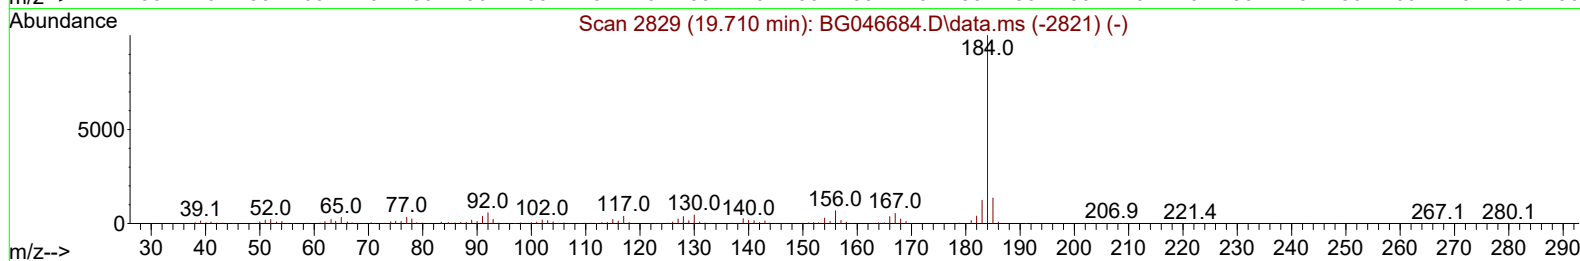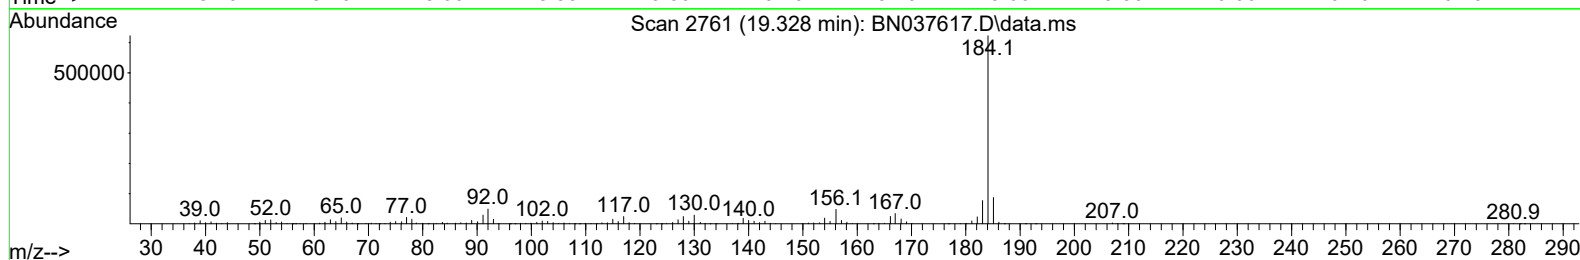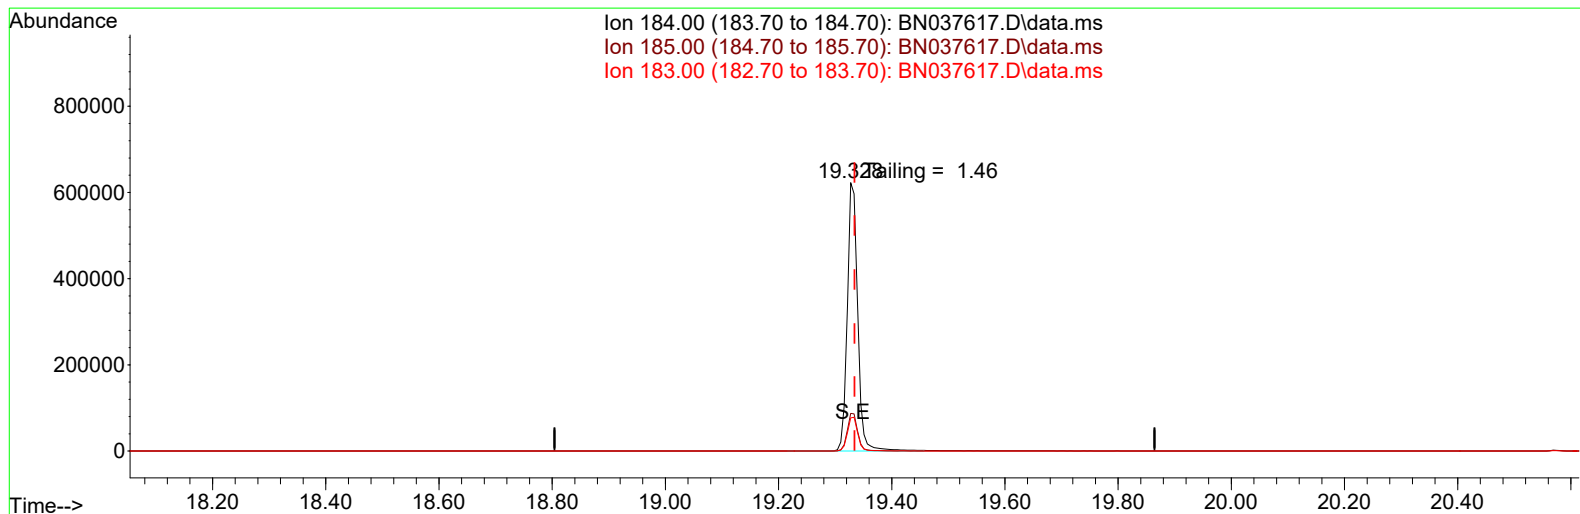

TIC: BN037617.D\data.ms

(77) Benzidine

19.328min (-0.006) 0.00 ng

response 801660

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	14.02
183.00	13.20	12.34
0.00	0.00	0.00