


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN082025\
Data File : BN037632.D
Acq On : 20 Aug 2025 16:18
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270-SIM-BN081225.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Wed Aug 13 05:00:58 2025

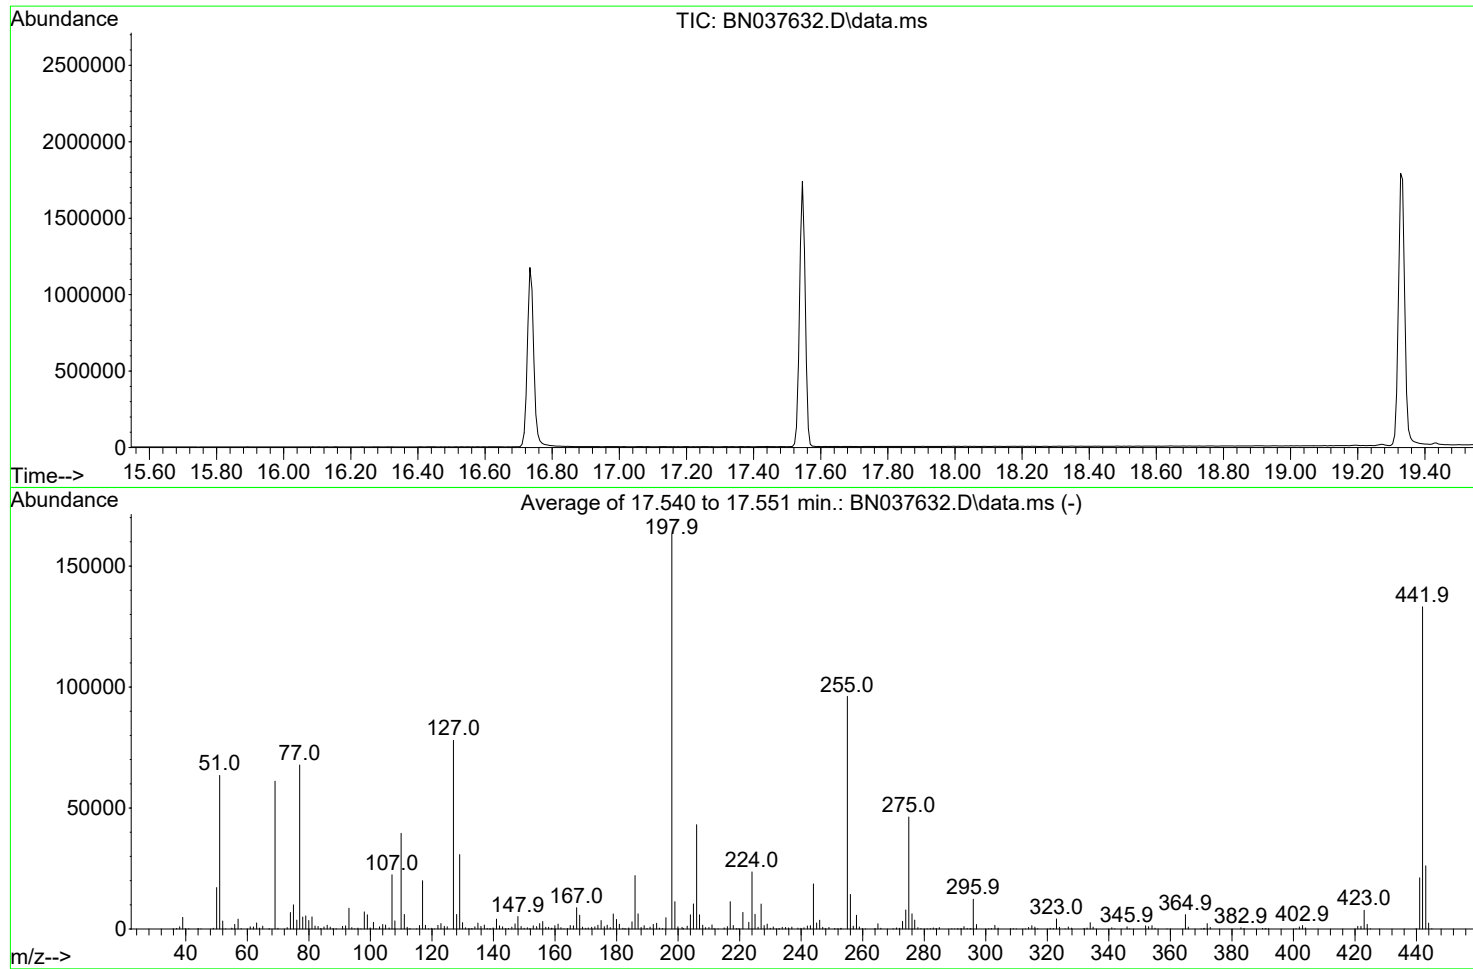

AutoFind: Scans 2457, 2458, 2459; Background Corrected with Scan 2450

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
68	69	0.00	2	0.0	0	PASS
69	69	100	100	100.0	61109	PASS
70	69	0.00	2	0.5	320	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	163179	PASS
199	198	5	9	6.9	11287	PASS
365	198	1	100	3.7	5979	PASS
441	443	0.01	150	81.1	21173	PASS
442	442	100	100	100.0	133187	PASS
443	442	15	24	19.6	26096	PASS

DDT Breakdown




Date	Instrument Name	DFTPP Data File
8/20/2025	BNA_N	<u>BN037632.D</u>
Compound Name	Response	Retention Time
DDT	551703	20.575
DDD	7513	20.134
DDE	470	19.628
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
7983	559686	1.43

Instrument :
BNA_N
ClientSampleId :
DFTPP

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN082025\
Data File : BN037632.D
Acq On : 20 Aug 2025 16:18
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: Aug 21 05:59:17 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Aug 06 01:49:15 2025
Response via : Initial Calibration

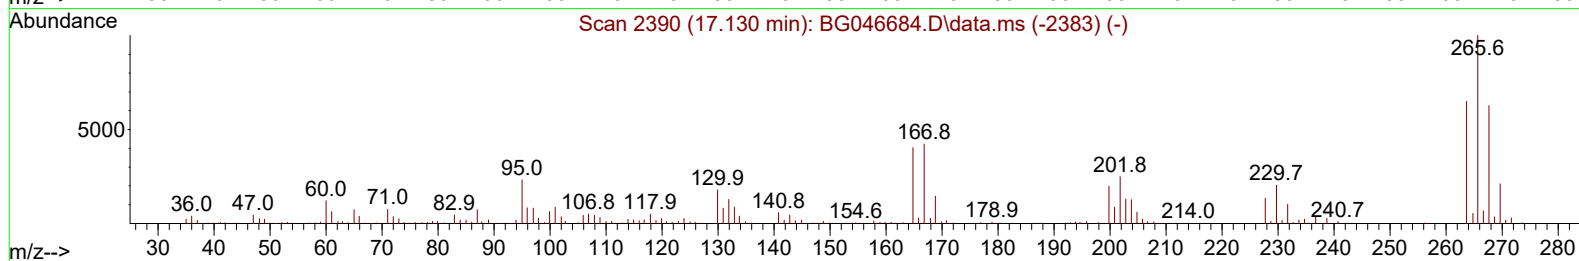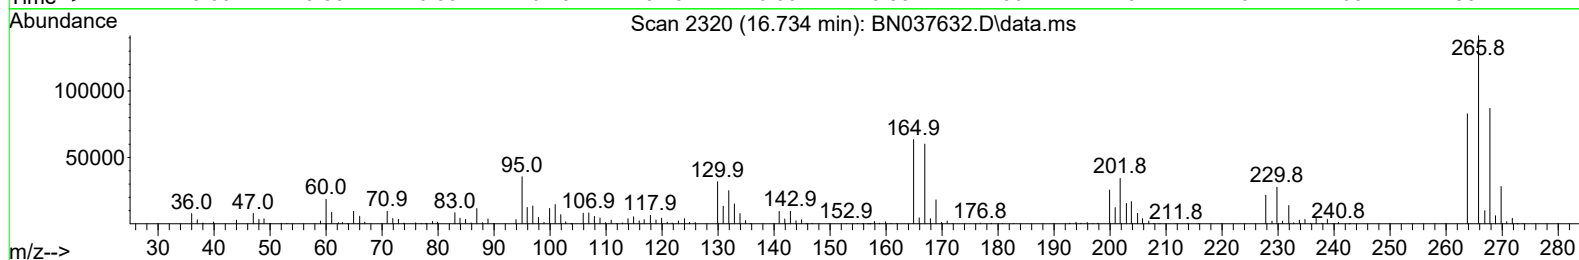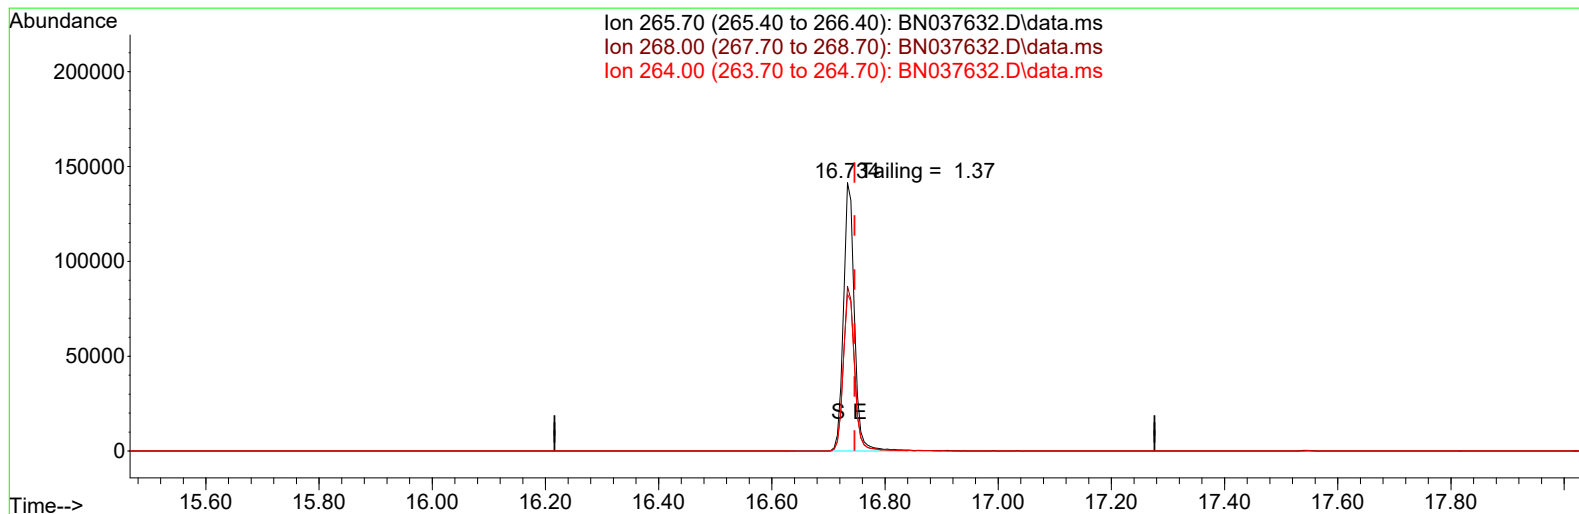

TIC: BN037632.D\data.ms

(70) Pentachlorophenol (C)

16.734min (-0.012) 25391.22 ng




response 190297

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	61.37
264.00	61.60	58.51
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN082025\
Data File : BN037632.D
Acq On : 20 Aug 2025 16:18
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: Aug 21 05:59:17 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Aug 06 01:49:15 2025
Response via : Initial Calibration

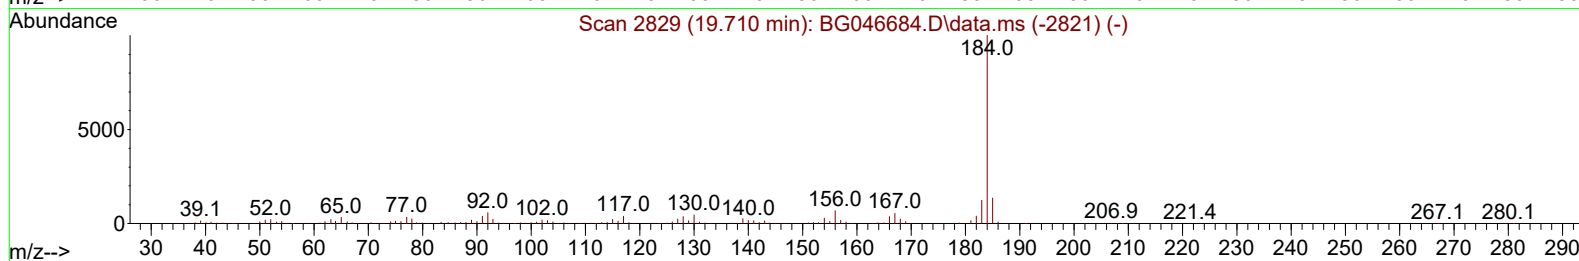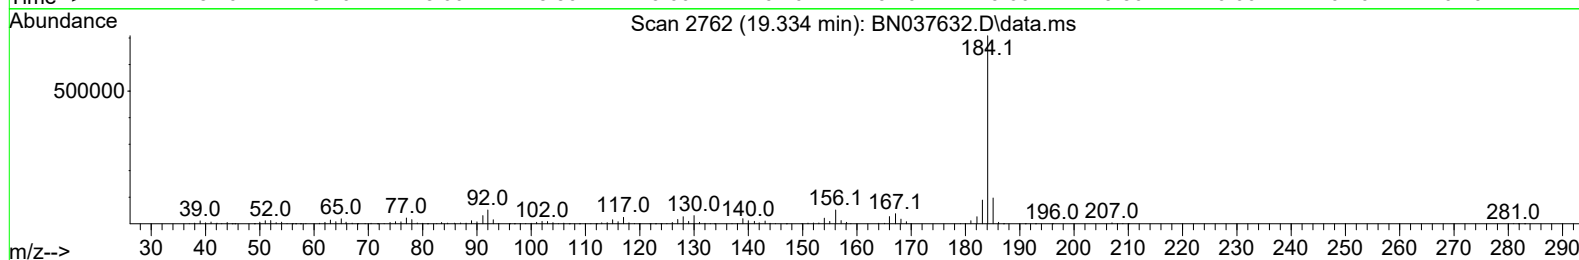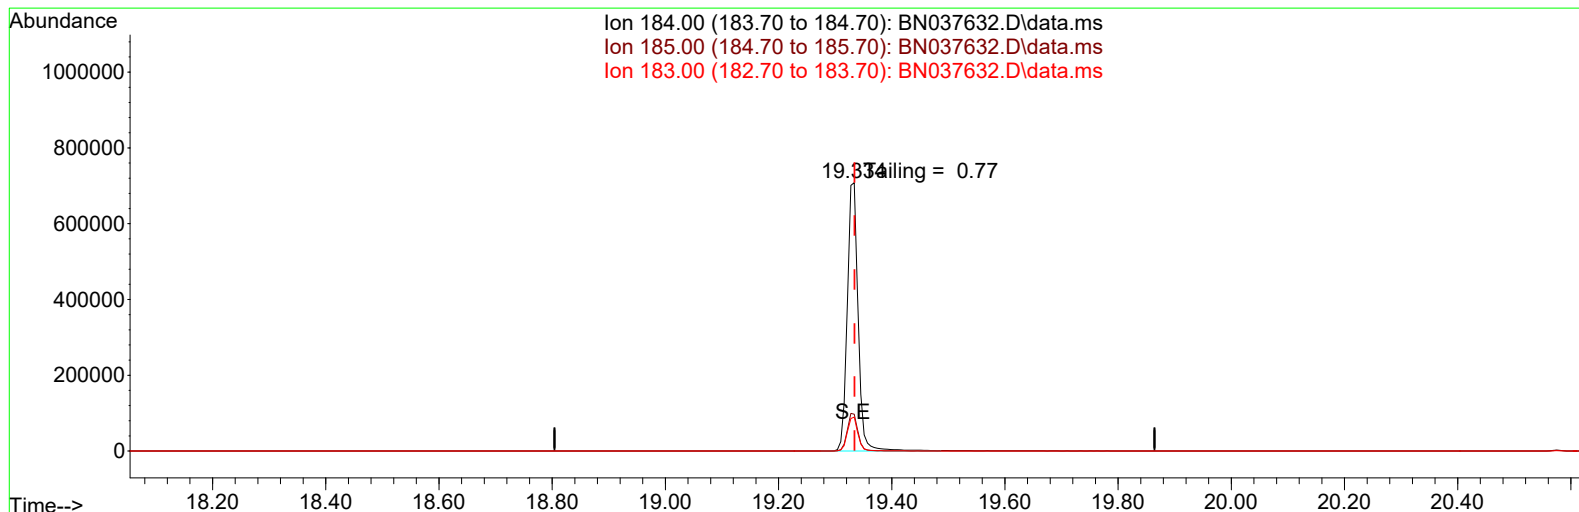

TIC: BN037632.D\data.ms

(77) Benzidine

19.334min (-0.001) 0.00 ng m

response 940808

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	13.76
183.00	13.20	12.63
0.00	0.00	0.00