


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN082025\
Data File : BN037642.D
Acq On : 21 Aug 2025 09:12
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270-SIM-BN081225.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Wed Aug 13 05:00:58 2025

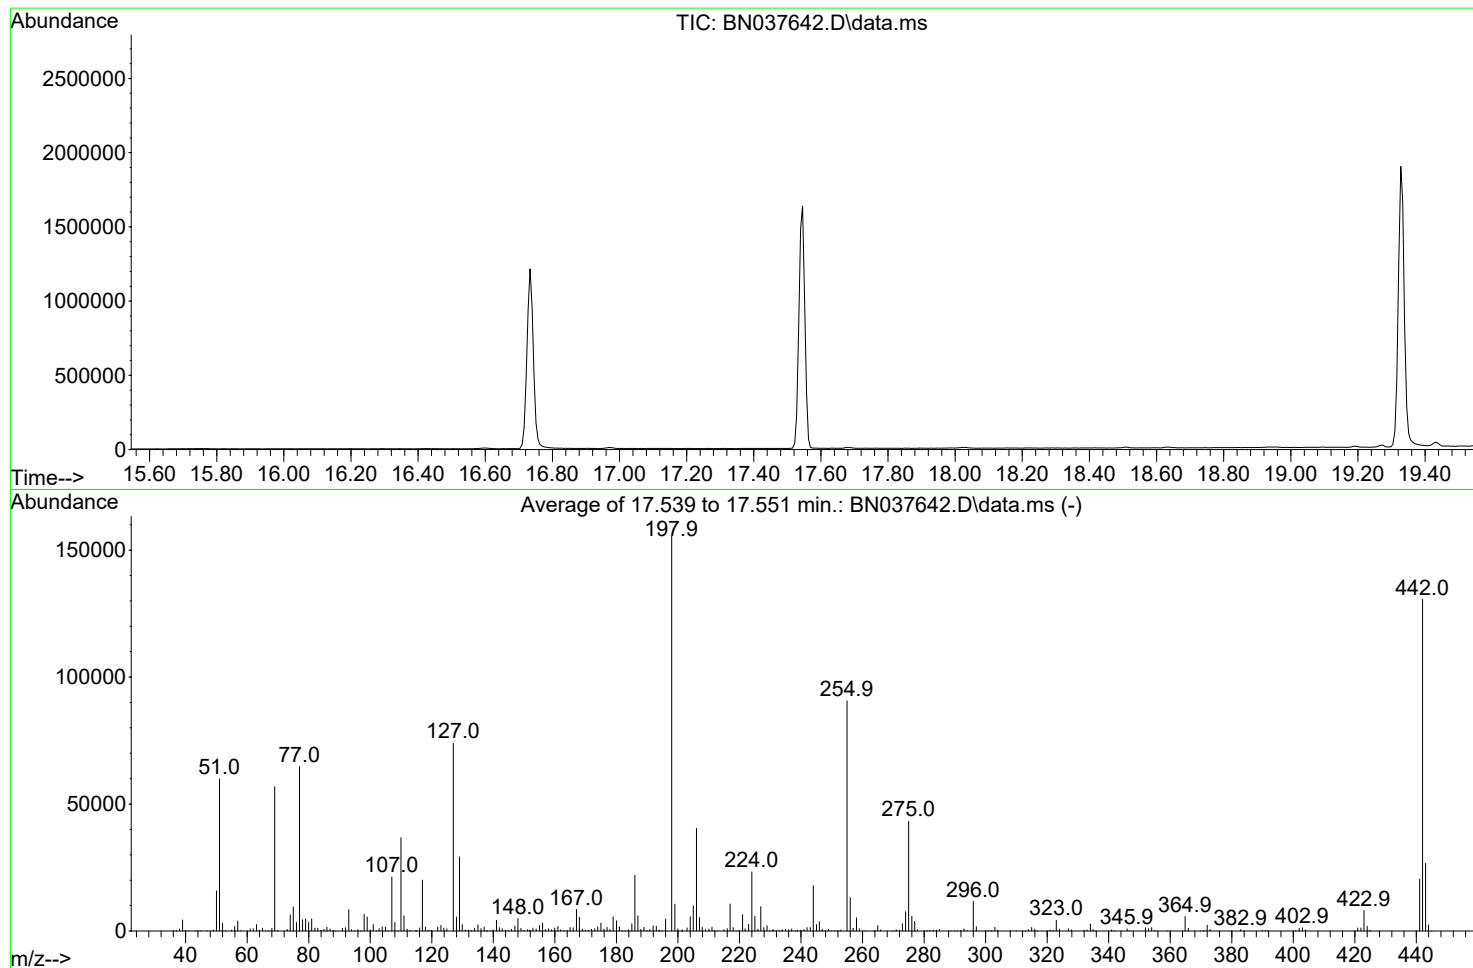

AutoFind: Scans 2457, 2458, 2459; Background Corrected with Scan 2450

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
68	69	0.00	2	1.9	1056	PASS
69	69	100	100	100.0	56869	PASS
70	69	0.00	2	0.5	266	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	155499	PASS
199	198	5	9	6.8	10621	PASS
365	198	1	100	3.7	5721	PASS
441	443	0.01	150	76.6	20443	PASS
442	442	100	100	100.0	130629	PASS
443	442	15	24	20.4	26688	PASS

DDT Breakdown




Date	Instrument Name	DFTPP Data File
8/20/2025	BNA_N	<u>BN037642.D</u>
Compound Name	Response	Retention Time
DDT	577409	20.133
DDD	7831	20.133
DDE	796	19.627
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
8627	586036	1.47

Instrument :
BNA_N
ClientSampleId :
DFTPP

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN082025\
Data File : BN037642.D
Acq On : 21 Aug 2025 09:12
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: Aug 22 08:25:22 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Aug 06 01:49:15 2025
Response via : Initial Calibration

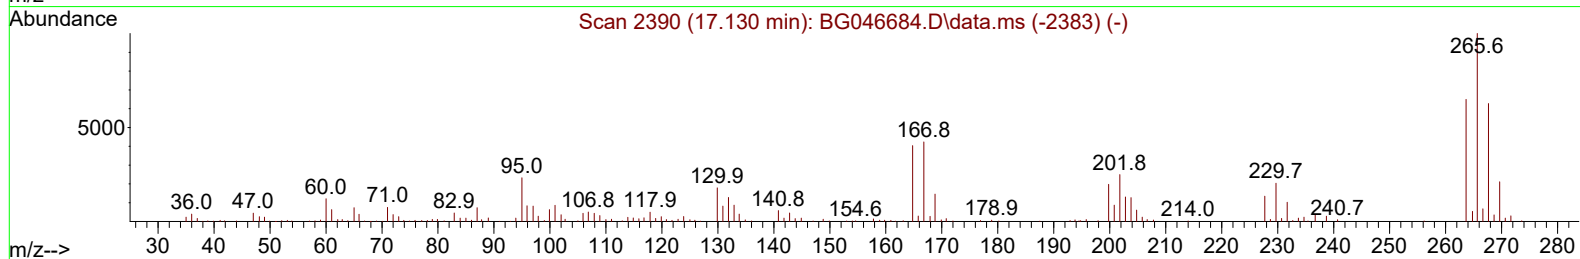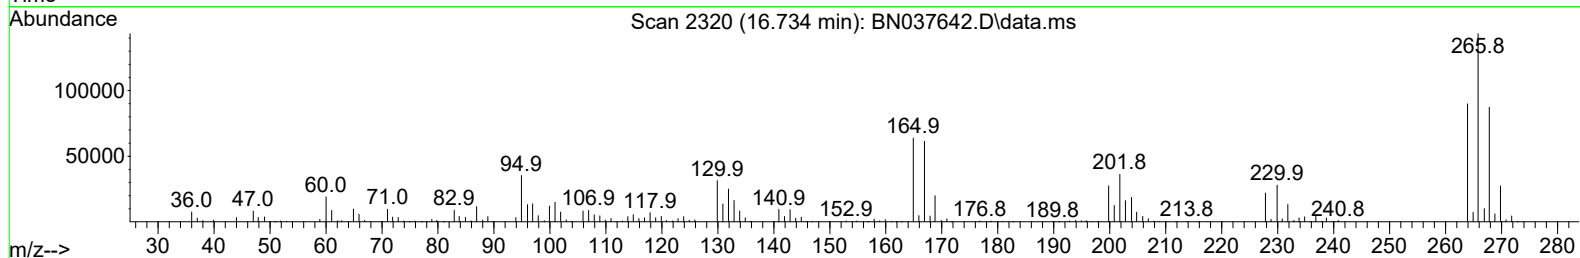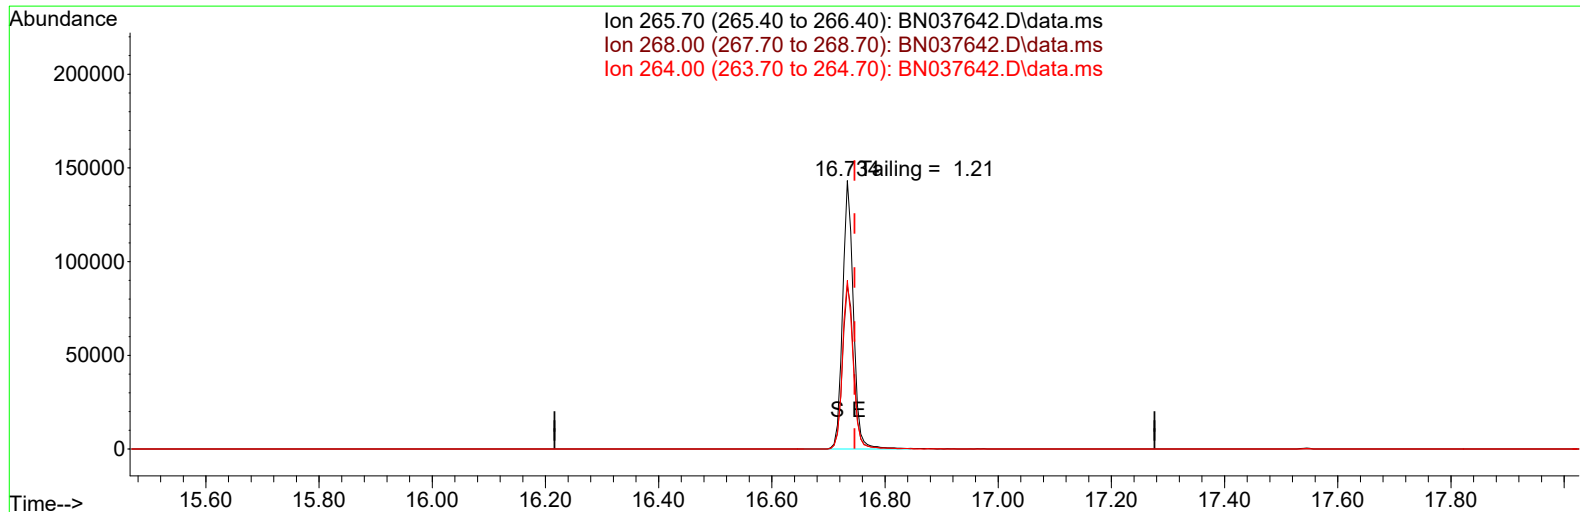

TIC: BN037642.D\data.ms

(70) Pentachlorophenol (C)

16.734min (-0.012) 30696.25 ng




response 188381

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	60.88
264.00	61.60	62.78
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN082025\
Data File : BN037642.D
Acq On : 21 Aug 2025 09:12
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: Aug 22 08:25:22 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Aug 06 01:49:15 2025
Response via : Initial Calibration

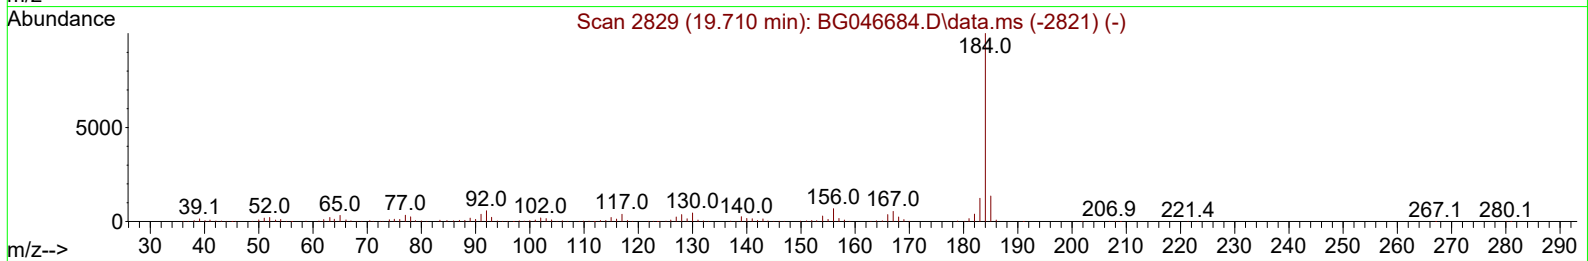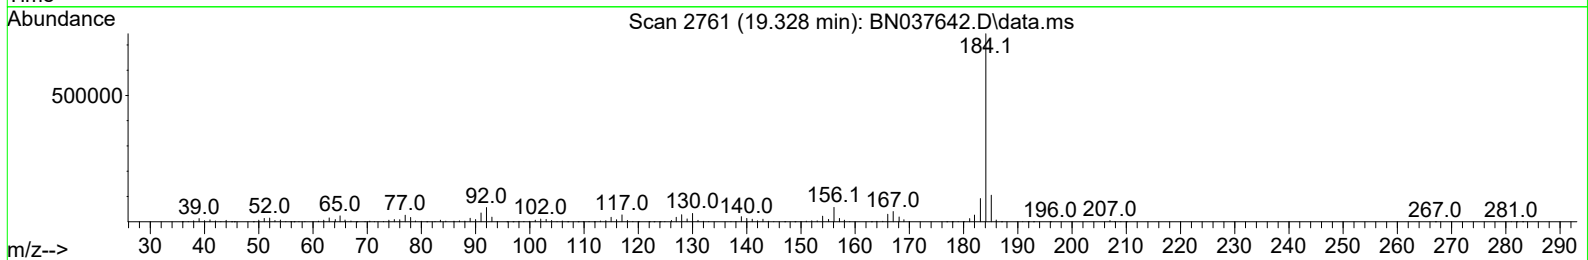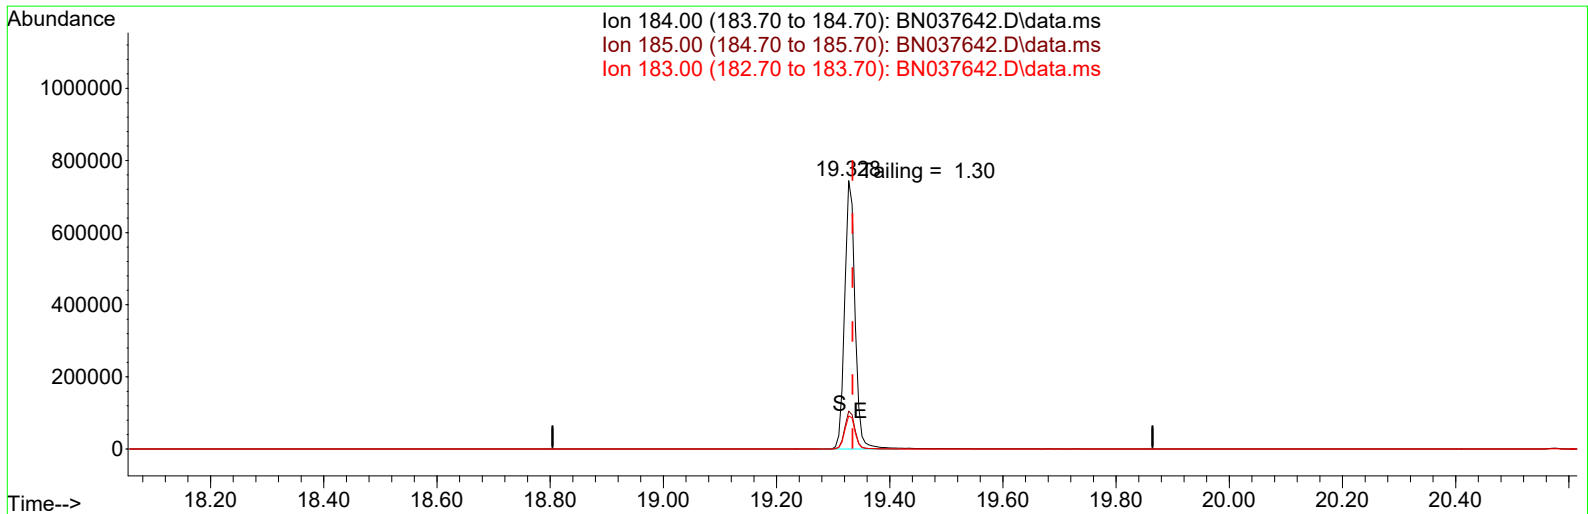

TIC: BN037642.D\data.ms

(77) Benzidine

19.328min (-0.007) 0.00 ng m

response 940363

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	14.12
183.00	13.20	12.35
0.00	0.00	0.00