


LB136873

7471B

INSTRUMENT ID: CV1

Linear

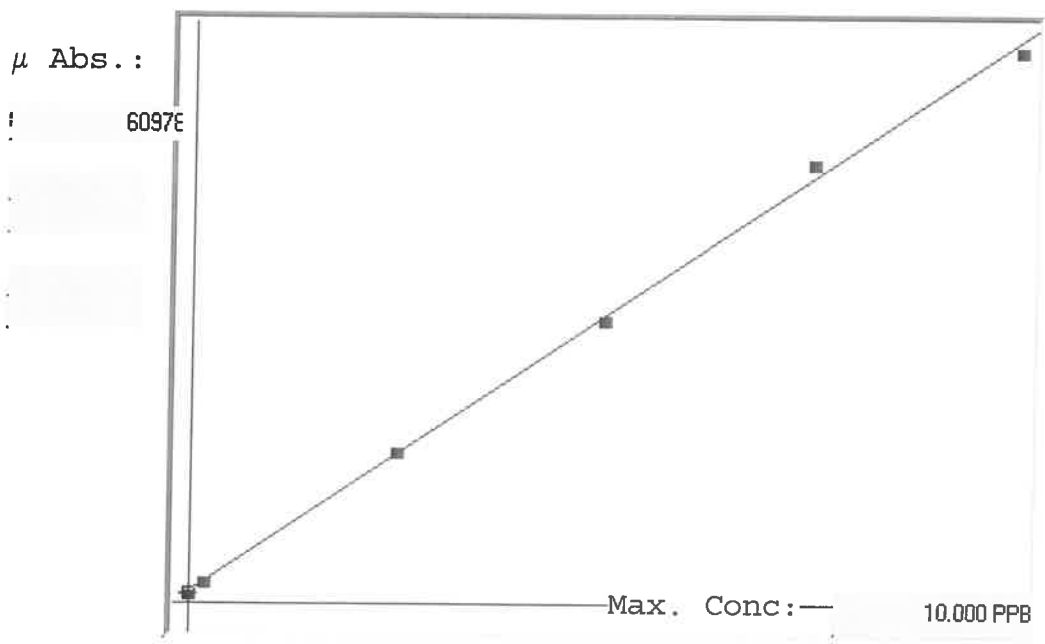

A= 0.0000e+000
B= 1.6447e-004
C= -2.1614e-001
Rho= 0.9992906
Accept=Accepted

Std ID	Conc.	Calc.	Dev.	Mean	SD or %RSD	Rep 1	Rep 2	Rep 3	Rep 4	Rep 5	6/0 1)
0.0	0.000	-0.039	-0.039	1079	0.000	1079					-
0.2	0.200	0.197	-0.003	2510	0.0 %	2510					-2
2.5	2.500	2.527	0.027	16680	0.0 %	16680					1
5.0	5.000	4.931	-0.069	31293	0.0 %	31293					-1
7.5	7.500	7.772	0.272	48567	0.0 %	48567					4
10.0	10.000	9.813	-0.187	60978	0.0 %	60978					-2

LB136873 INSTRUMENT ID : CV1

Method: 7471B

Operator: Admin

Date of Analysis: 19 Aug 2025 10:58:08

Type	Sample ID	Extended ID	Conc.	μ Abs	Units	Type	Std Cond/Method	Date
S	0.0 - 1	50	-	1079	PPB	Std	0.00007471B	19 Aug 2025 11:29:12
S	0.2 - 1	50.2	-	2510	PPB	Std	0.20007471B	19 Aug 2025 11:31:29
S	2.5 - 1	52.5	-	16680	PPB	Std	2.50007471B	19 Aug 2025 11:33:46
S	5.0 - 1	55	-	31293	PPB	Std	5.00007471B	19 Aug 2025 11:36:03
S	7.5 - 1	57.5	-	48567	PPB	Std	7.50007471B	19 Aug 2025 11:38:22
S	10.0 - 1	57.6	-	60978	PPB	Std	10.00007471B	19 Aug 2025 11:40:39
U	ICV22 - 1	ICV22	3.8610	24790	PPB	SMPL	-7471B	19 Aug 2025 11:44:26
U	ICB22 - 1	ICB22	0.0059	1350	PPB	SMPL	-7471B	19 Aug 2025 11:46:44
U	CCV68 - 1	CCV68	4.9328	31307	PPB	SMPL	-7471B	19 Aug 2025 11:49:01
U	CCB68 - 1	CCB68	-0.0214	1184	PPB	SMPL	-7471B	19 Aug 2025 11:51:17
U	CRA - 1	CRA	0.1694	2344	PPB	SMPL	-7471B	19 Aug 2025 11:53:36
U	HighStd - 1	HighStd	9.8116	60971	PPB	SMPL	-7471B	19 Aug 2025 11:55:50
U	ChkStd - 1	ChkStd	7.6993	48128	PPB	SMPL	-7471B	19 Aug 2025 11:58:06
U	PB169292BS - 1	PB169292BS	3.3498	21682	PPB	SMPL	-7471B	19 Aug 2025 12:05:58
U	Q2892-02 - 1	1-FLOOR-NORTH-EAST-CORNER-BACK-A	0.6182	5073	PPB	SMPL	-7471B	19 Aug 2025 12:08:15
U	Q2892-04 - 1	1-FLOOR-DRILL-B-BACK	1.0442	7663	PPB	SMPL	-7471B	19 Aug 2025 12:10:37
U	Q2892-06 - 1	BACK-1-FLOOR-CENTER-MIDDLE-C	0.2940	3102	PPB	SMPL	-7471B	19 Aug 2025 12:12:58
U	Q2892-08 - 1	3-FLOOR-NORTH-D	0.0633	1699	PPB	SMPL	-7471B	19 Aug 2025 12:15:17
U	Q2892-10 - 1	3-FLOOR-SOUTH-E	1.0050	7425	PPB	SMPL	-7471B	19 Aug 2025 12:17:34
U	CCV69 - 1	CCV69	4.8883	31036	PPB	SMPL	-7471B	19 Aug 2025 12:19:50
U	CCB69 - 1	CCB69	-0.0704	886	PPB	SMPL	-7471B	19 Aug 2025 12:22:06
U	Q2892-12 - 1	FRONT-1-FLOOR-F	1.0468	7679	PPB	SMPL	-7471B	19 Aug 2025 12:24:24
U	Q2897-01 - 1	HD-02-08182025	0.3672	3547	PPB	SMPL	-7471B	19 Aug 2025 12:33:25
U	Q2897-01DUP - 1	HD-02-08182025DUP	0.4069	3788	PPB	SMPL	-7471B	19 Aug 2025 12:39:21
U	Q2897-01MS - 1	HD-02-08182025MS	3.9363	25248	PPB	SMPL	-7471B	19 Aug 2025 12:41:38
U	Q2897-01MSD - 1	HD-02-08182025MSD	3.9645	25419	PPB	SMPL	-7471B	19 Aug 2025 12:43:55
U	PB69292BL - 1	PBS	-0.0222	1179	PPB	SMPL	-7471B	19 Aug 2025 12:49:03
U	Q2897-01LX5 - 1		-0.1454	430	PPB	SMPL	-7471B	19 Aug 2025 12:51:20
U	Q2897-01A - 1		4.1755	26702	PPB	SMPL	-7471B	19 Aug 2025 12:53:37
U	CCV70 - 1	CCV70	4.6754	29742	PPB	SMPL	-7471B	19 Aug 2025 12:55:55
U	CCB70 - 1	CCB70	-0.0790	834	PPB	SMPL	-7471B	19 Aug 2025 12:58:13