

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL081925\
 Data File : PL096901.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 19 Aug 2025 17:55
 Operator : AR\AJ
 Sample : PB169298BL
 Misc :
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 PB169298BL

Manual Integrations
 APPROVED

Reviewed By : Abdul Mirza 08/20/2025
 Supervised By : mohammad ahmed 08/21/2025

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 20 01:38:54 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL072825.M
 Quant Title : GC Extractables
 QLast Update : Fri Aug 08 15:43:38 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.530	2.826	58936358	89276745	18.529	18.686
28)	SA Decachlor...	9.001	7.986	48787189	82046735	20.459m	18.912

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL081925\
Data File : PL096901.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 19 Aug 2025 17:55
Operator : AR\AJ
Sample : PB169298BL
Misc :
ALS Vial : 20 Sample Multiplier: 1



Instrument :
ECD_L
ClientSampleId :
PB169298BL


Manual Integrations
APPROVED

Reviewed By : Abdul Mirza 08/20/2025
Supervised By : mohammad ahmed 08/21/2025

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 20 01:38:54 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL072825.M
Quant Title : GC Extractables
QLast Update : Fri Aug 08 15:43:38 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

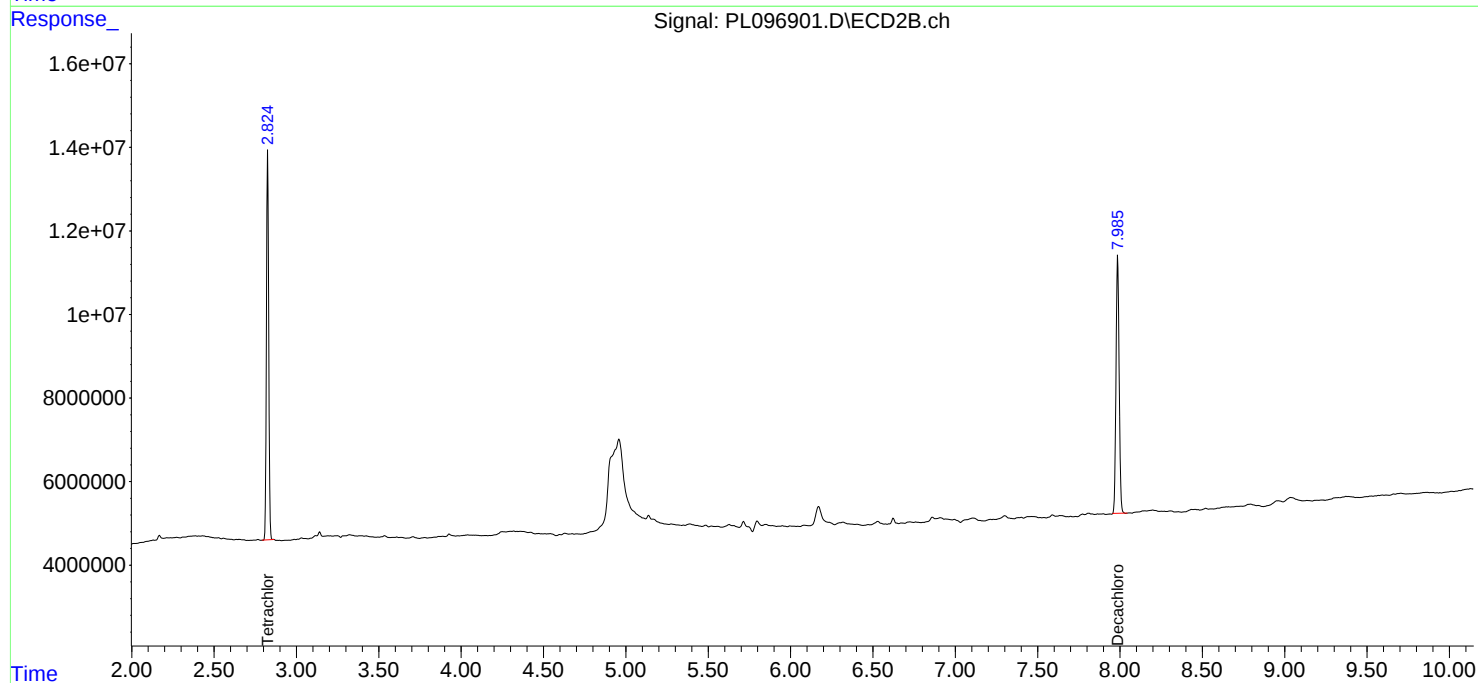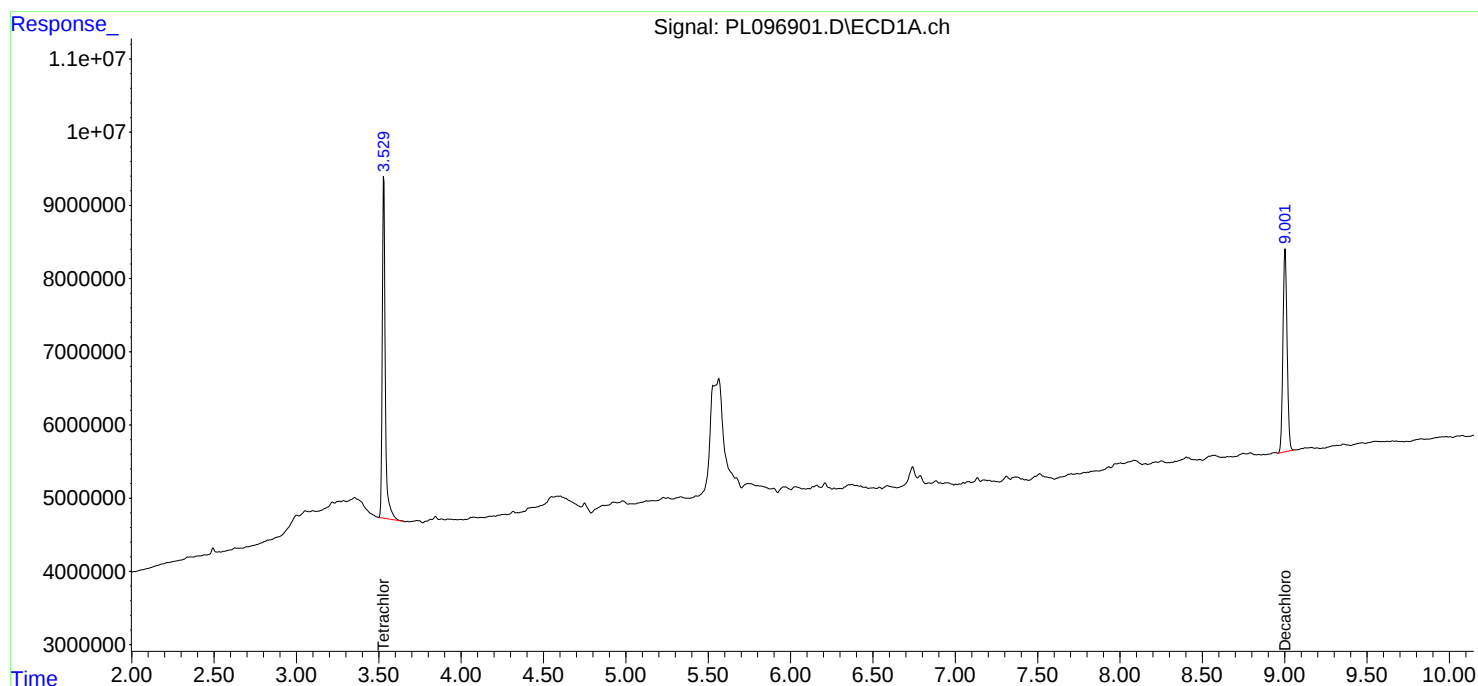

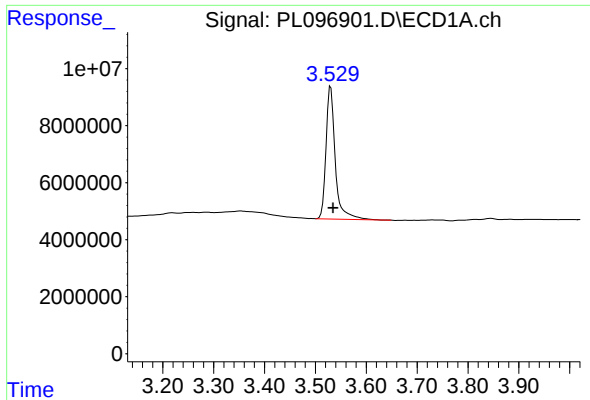


#1 Tetrachloro-m-xylene

R.T.: 3.530 min
Delta R.T.: -0.005 min
Response: 58936358
Conc: 18.53 ng/ml

Instrument :
ECD_L
ClientSampleId :
PB169298BL


Manual Integrations
APPROVED

Reviewed By :Abdul Mirza 08/20/2025
Supervised By :mohammad ahmed 08/21/2025

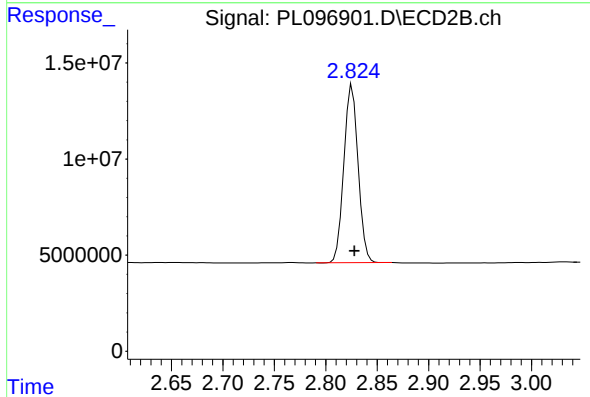


#1 Tetrachloro-m-xylene

R.T.: 2.826 min
Delta R.T.: -0.002 min
Response: 89276745
Conc: 18.69 ng/ml

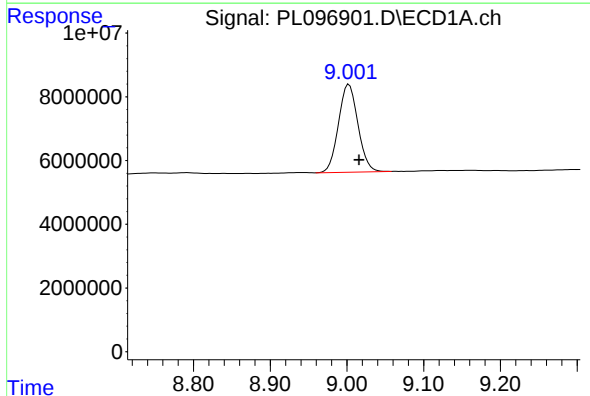

#28 Decachlorobiphenyl

R.T.: 9.001 min
Delta R.T.: -0.015 min
Response: 48787189
Conc: 20.46 ng/ml m

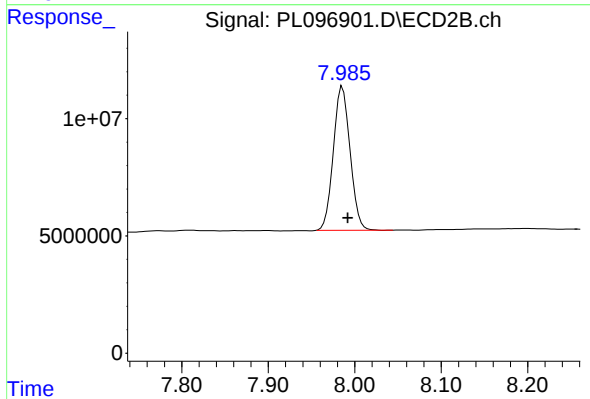

#28 Decachlorobiphenyl

R.T.: 7.986 min
Delta R.T.: -0.006 min
Response: 82046735
Conc: 18.91 ng/ml