

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL081925\
 Data File : PL096907.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 19 Aug 2025 19:17
 Operator : AR\AJ
 Sample : Q2892-04
 Misc :
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 1-FLOOR-DRILL-B-BACK

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 20 01:39:39 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL072825.M
 Quant Title : GC Extractables
 QLast Update : Fri Aug 08 15:43:38 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.530	2.826	89224352	95859753	28.051	20.064 #
28)	SA Decachlor...	9.004	7.986	42000865	76873056	17.613	17.720
Target Compounds							
9)	A Endosulfan I	0.000	5.185f	0	7881173	N.D.	1.425 #
12)	B 4,4'-DDE	6.159	5.299	7435317	12440732	2.315	2.256
13)	MA Dieldrin	0.000	5.431	0	9914164	N.D.	1.679 #
14)	MA Endrin	0.000	5.714	0	5845889	N.D.	1.081 #
15)	B Endosulfa...	6.785f	6.027f	8434463	7768932	2.634	1.513 #
17)	MA 4,4'-DDT	6.981	6.102	8008569	20556727	2.793	4.064 #
19)	B Endosulfa...	7.133f	6.391	14281429	14911570	4.970	2.932 #
20)	A Methoxychlor	0.000	6.702f	0	2548077	N.D.	0.930 #
21)	B Endrin ke...	7.575f	0.000	6041531	0	2.009	N.D. #
27)	Chlordane-5	0.000	6.027f	0	7768932	N.D.	30.453 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL081925\
Data File : PL096907.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 19 Aug 2025 19:17
Operator : AR\AJ
Sample : Q2892-04
Misc :
ALS Vial : 23 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
1-FLOOR-DRILL-B-BACK

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 20 01:39:39 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL072825.M
Quant Title : GC Extractables
QLast Update : Fri Aug 08 15:43:38 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

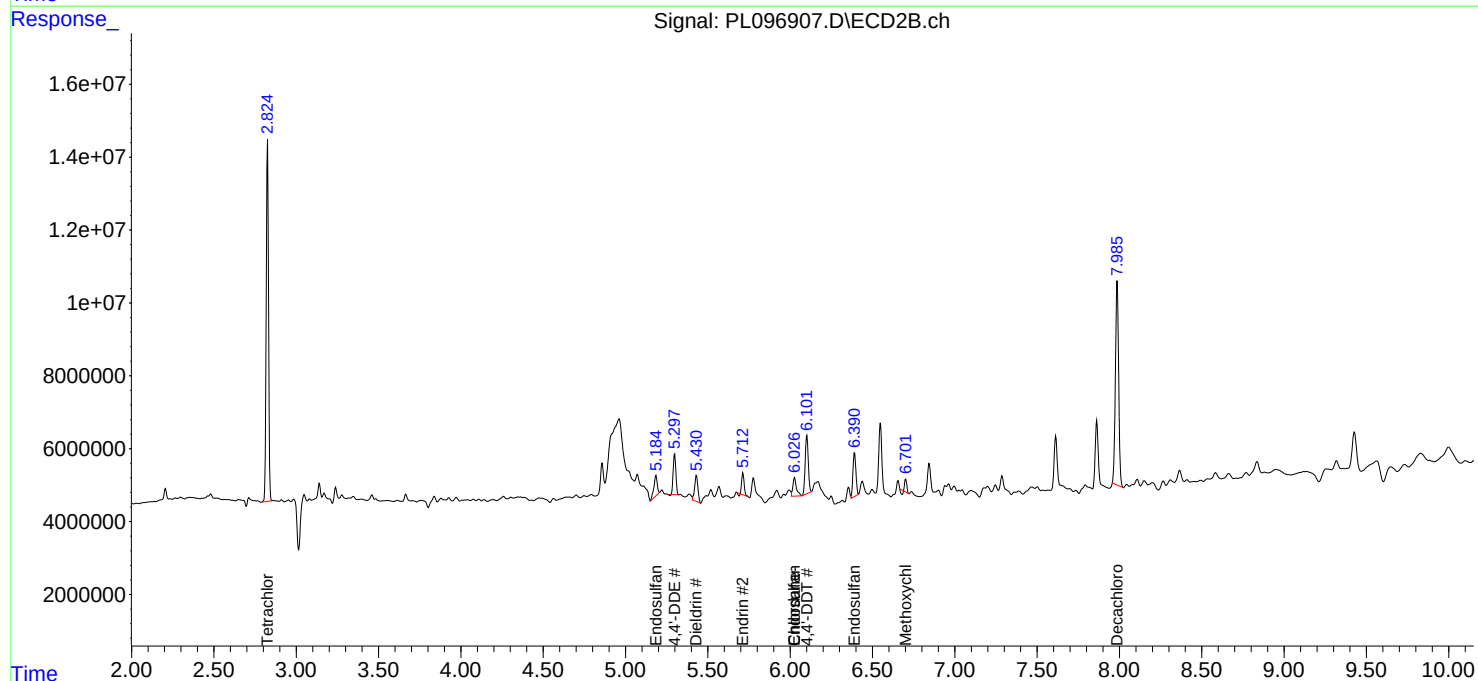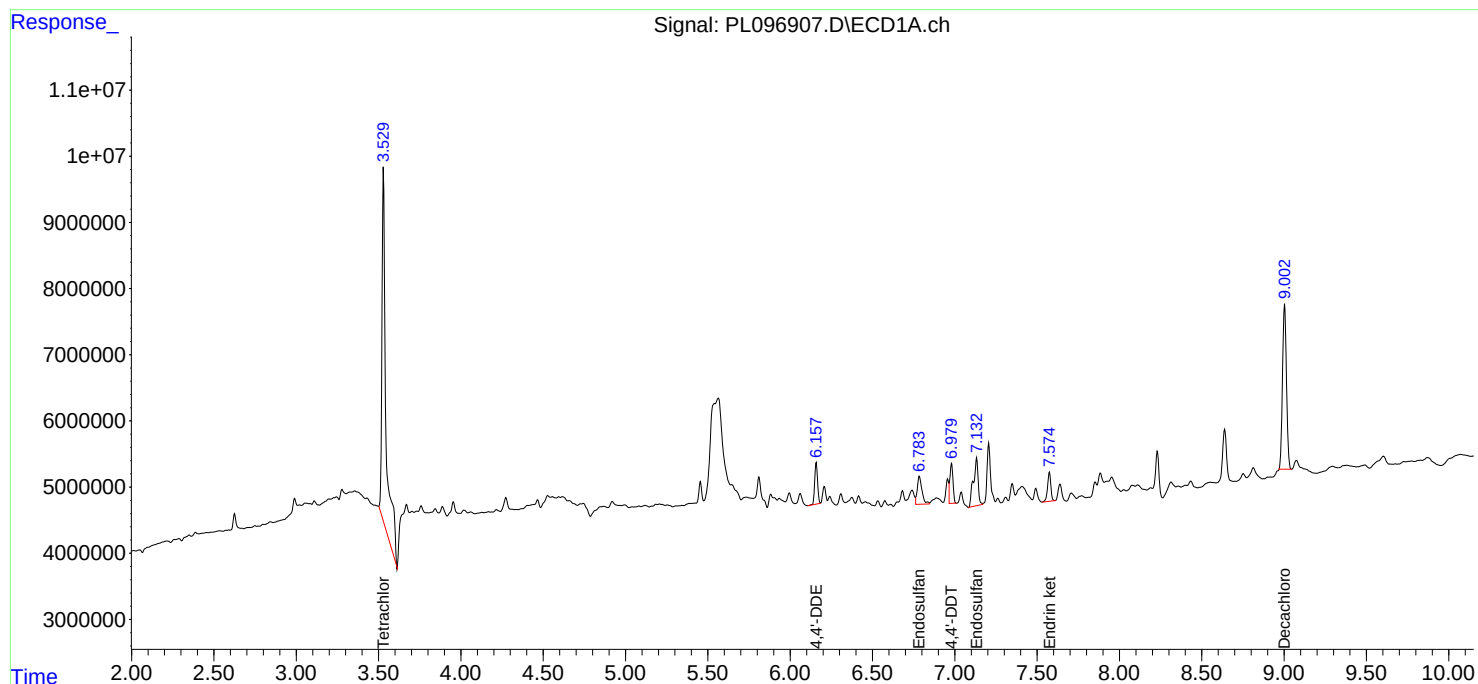


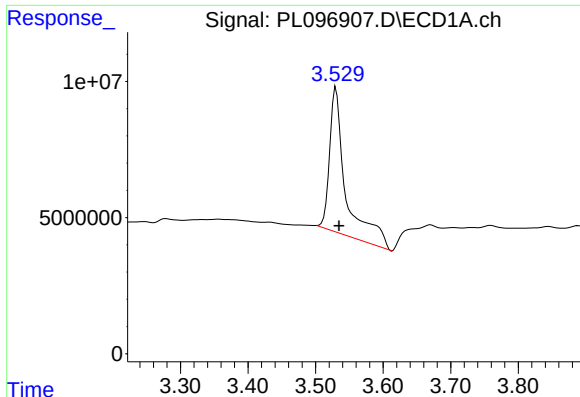

#1 Tetrachloro-m-xylene


R.T.: 3.530 min
Delta R.T.: -0.005 min
Response: 89224352
Conc: 28.05 ng/ml

Instrument :
ECD_L
ClientSampleId :
1-FLOOR-DRILL-B-BACK

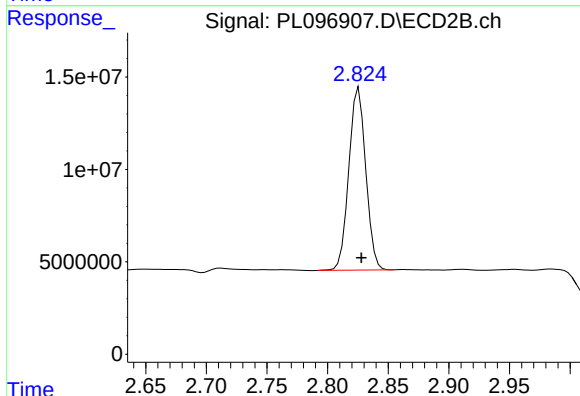


#1 Tetrachloro-m-xylene

R.T.: 2.826 min
Delta R.T.: -0.002 min
Response: 95859753
Conc: 20.06 ng/ml

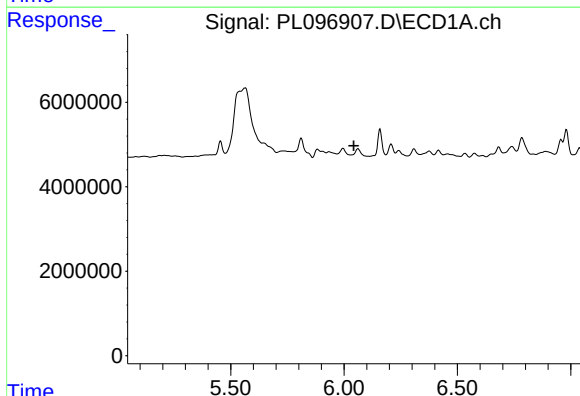


#9 Endosulfan I

R.T.: 0.000 min
Exp R.T. : 6.044 min
Response: 0
Conc: N.D.

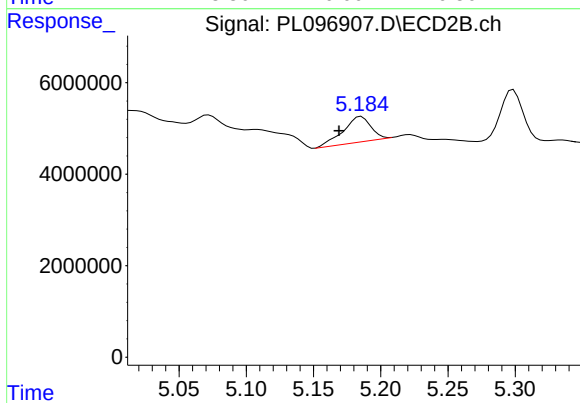

#9 Endosulfan I


R.T.: 5.185 min
Delta R.T.: 0.016 min
Response: 7881173
Conc: 1.42 ng/ml

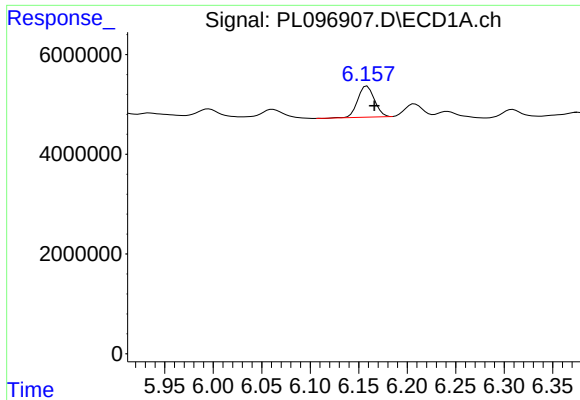

#12 4,4'-DDE


R.T.: 6.159 min
Delta R.T.: -0.007 min
Response: 7435317
Conc: 2.32 ng/ml

Instrument :
ECD_L
ClientSampleId :
1-FLOOR-DRILL-B-BACK

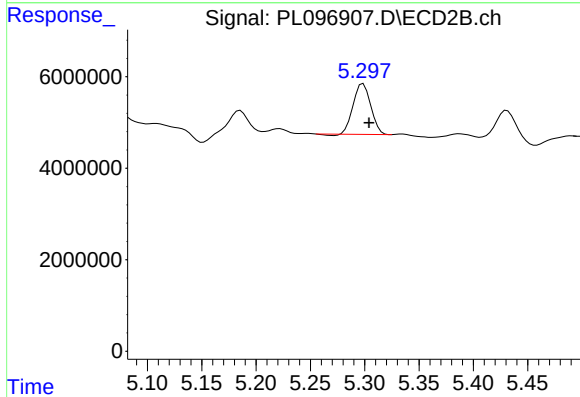


#12 4,4'-DDE

R.T.: 5.299 min
Delta R.T.: -0.005 min
Response: 12440732
Conc: 2.26 ng/ml

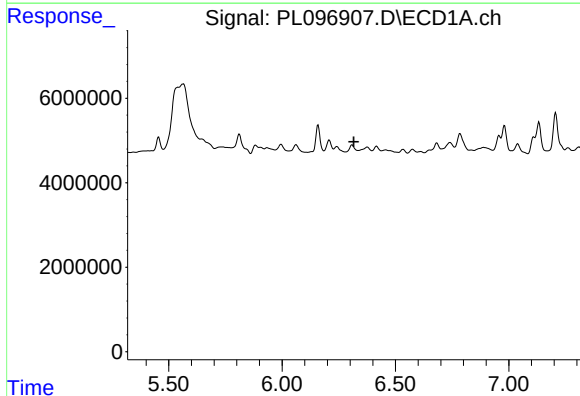


#13 Dieldrin

R.T.: 0.000 min
Exp R.T. : 6.316 min
Response: 0
Conc: N.D.

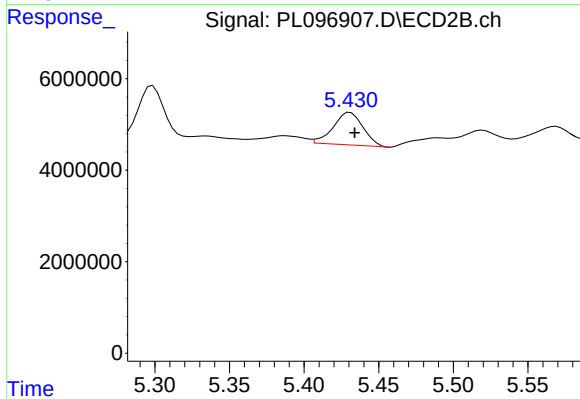

#13 Dieldrin


R.T.: 5.431 min
Delta R.T.: -0.003 min
Response: 9914164
Conc: 1.68 ng/ml

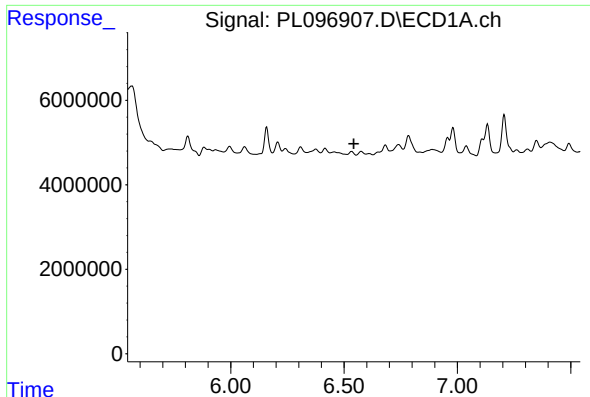

#14 Endrin


R.T.: 0.000 min
Exp R.T.: 6.542 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
1-FLOOR-DRILL-B-BACK

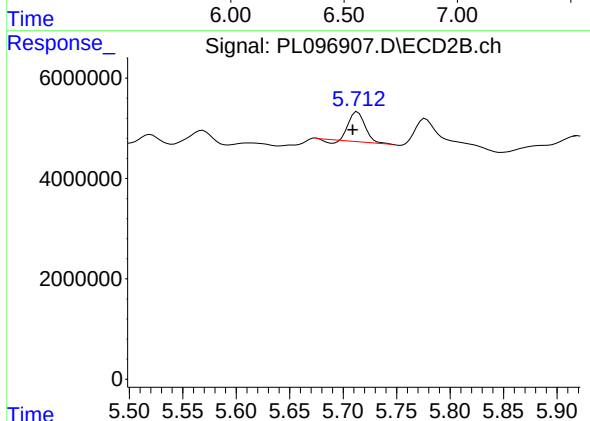


#14 Endrin

R.T.: 5.714 min
Delta R.T.: 0.005 min
Response: 5845889
Conc: 1.08 ng/ml

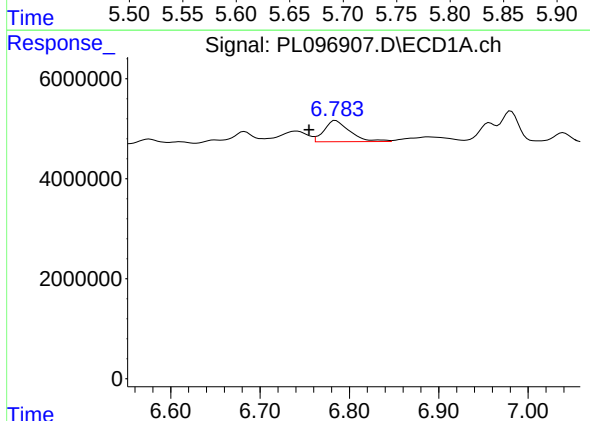


#15 Endosulfan II

R.T.: 6.785 min
Delta R.T.: 0.030 min
Response: 8434463
Conc: 2.63 ng/ml

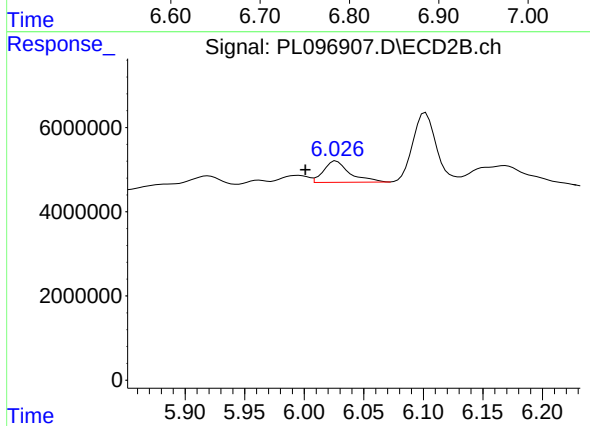

#15 Endosulfan II


R.T.: 6.027 min
Delta R.T.: 0.026 min
Response: 7768932
Conc: 1.51 ng/ml

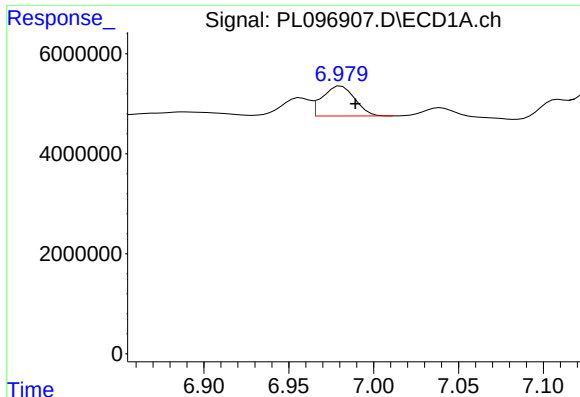

#17 4,4'-DDT


R.T.: 6.981 min
Delta R.T.: -0.008 min
Response: 8008569
Conc: 2.79 ng/ml

Instrument :
ECD_L
ClientSampleId :
1-FLOOR-DRILL-B-BACK

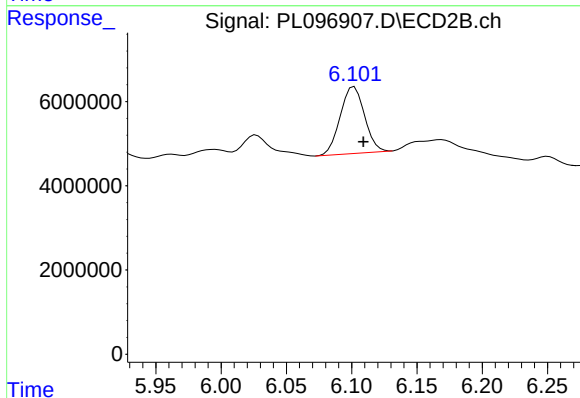


#17 4,4'-DDT

R.T.: 6.102 min
Delta R.T.: -0.007 min
Response: 20556727
Conc: 4.06 ng/ml

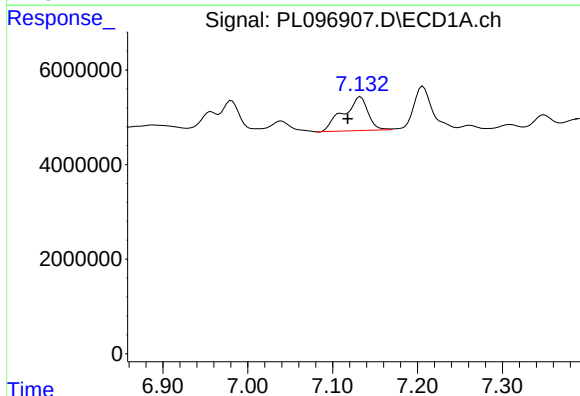


#19 Endosulfan Sulfate

R.T.: 7.133 min
Delta R.T.: 0.015 min
Response: 14281429
Conc: 4.97 ng/ml

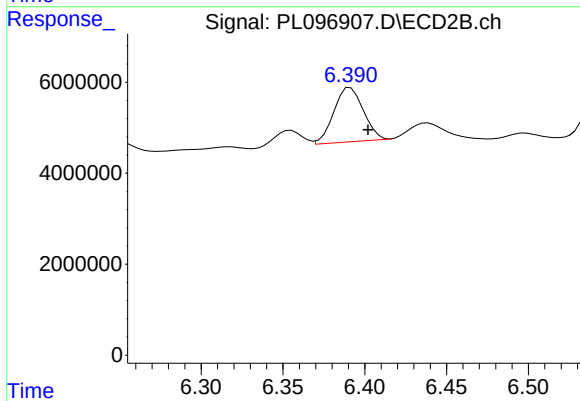

#19 Endosulfan Sulfate


R.T.: 6.391 min
Delta R.T.: -0.011 min
Response: 14911570
Conc: 2.93 ng/ml

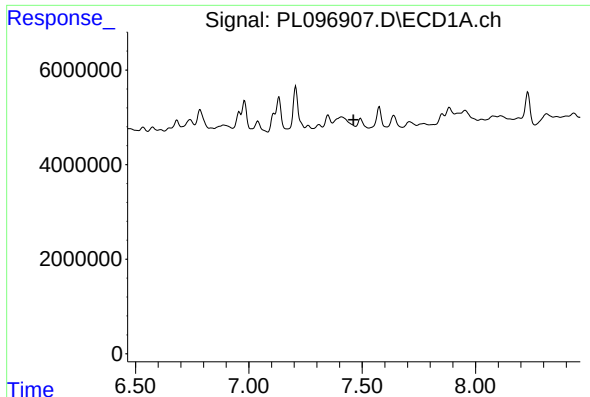

#20 Methoxychlor


R.T.: 0.000 min
Exp R.T.: 7.462 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
1-FLOOR-DRILL-B-BACK

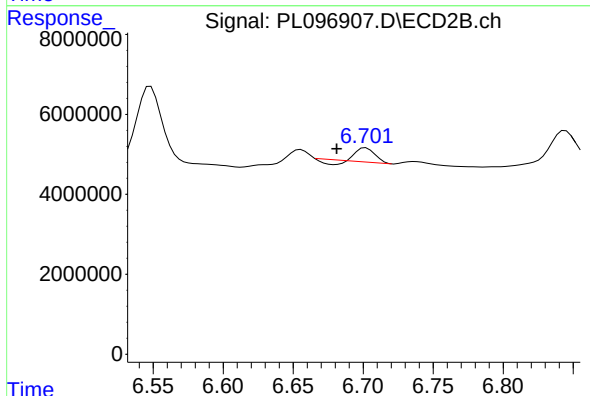


#20 Methoxychlor

R.T.: 6.702 min
Delta R.T.: 0.021 min
Response: 2548077
Conc: 0.93 ng/ml

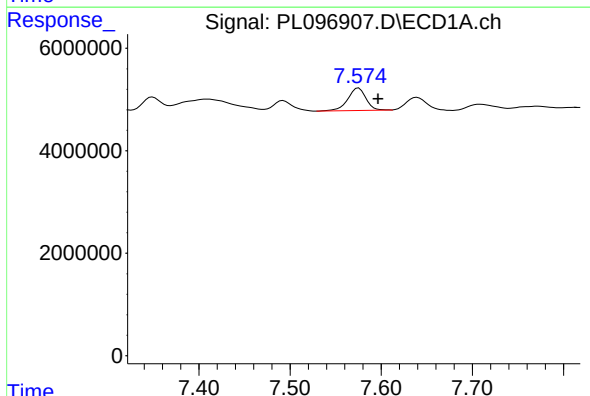


#21 Endrin ketone

R.T.: 7.575 min
Delta R.T.: -0.021 min
Response: 6041531
Conc: 2.01 ng/ml

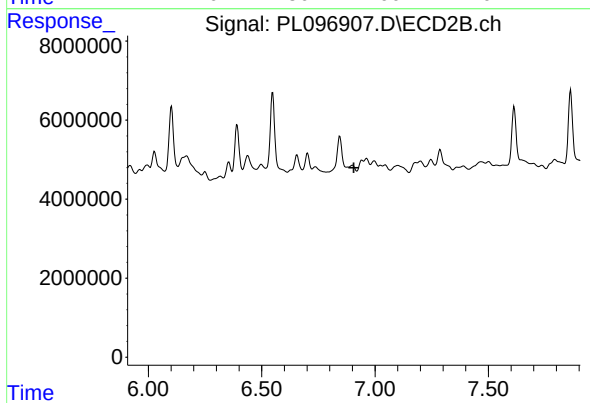

#21 Endrin ketone


R.T.: 0.000 min
Exp R.T.: 6.907 min
Response: 0
Conc: N.D.

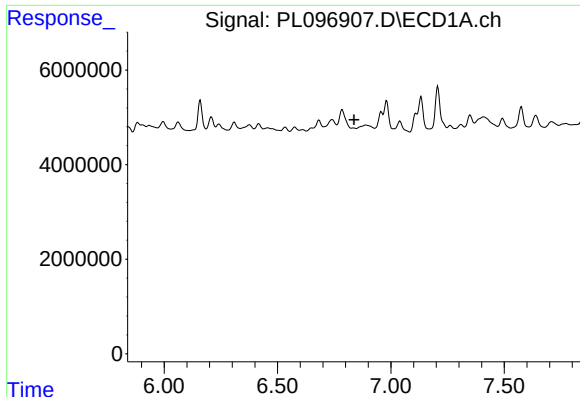

#27 Chlordane-5


R.T.: 0.000 min
Exp R.T.: 6.838 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
1-FLOOR-DRILL-B-BACK

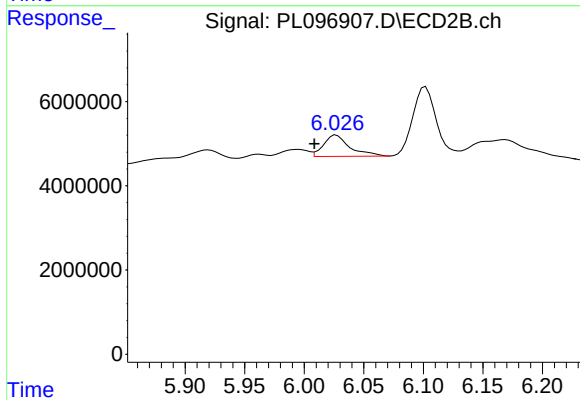


#27 Chlordane-5

R.T.: 6.027 min
Delta R.T.: 0.018 min
Response: 7768932
Conc: 30.45 ng/ml

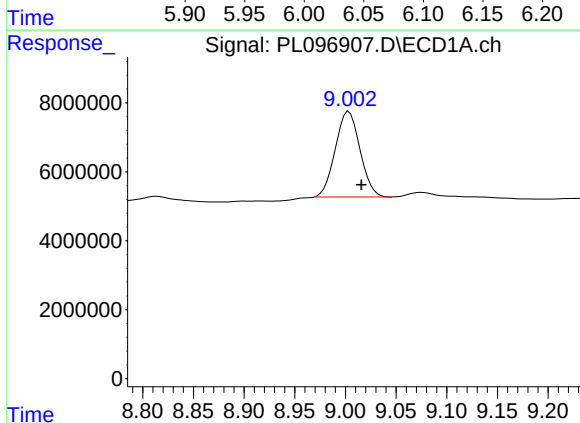

#28 Decachlorobiphenyl

R.T.: 9.004 min
Delta R.T.: -0.012 min
Response: 42000865
Conc: 17.61 ng/ml

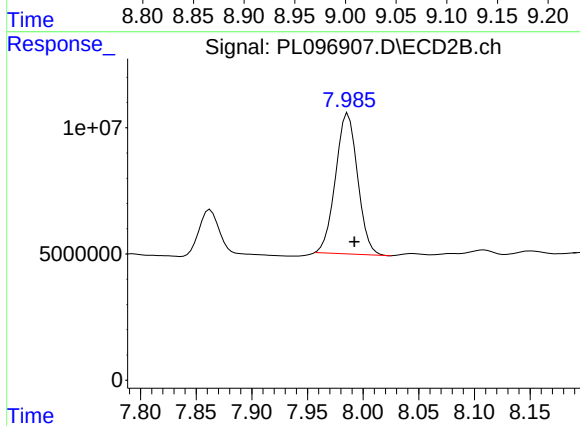

#28 Decachlorobiphenyl

R.T.: 7.986 min
Delta R.T.: -0.006 min
Response: 76873056
Conc: 17.72 ng/ml