
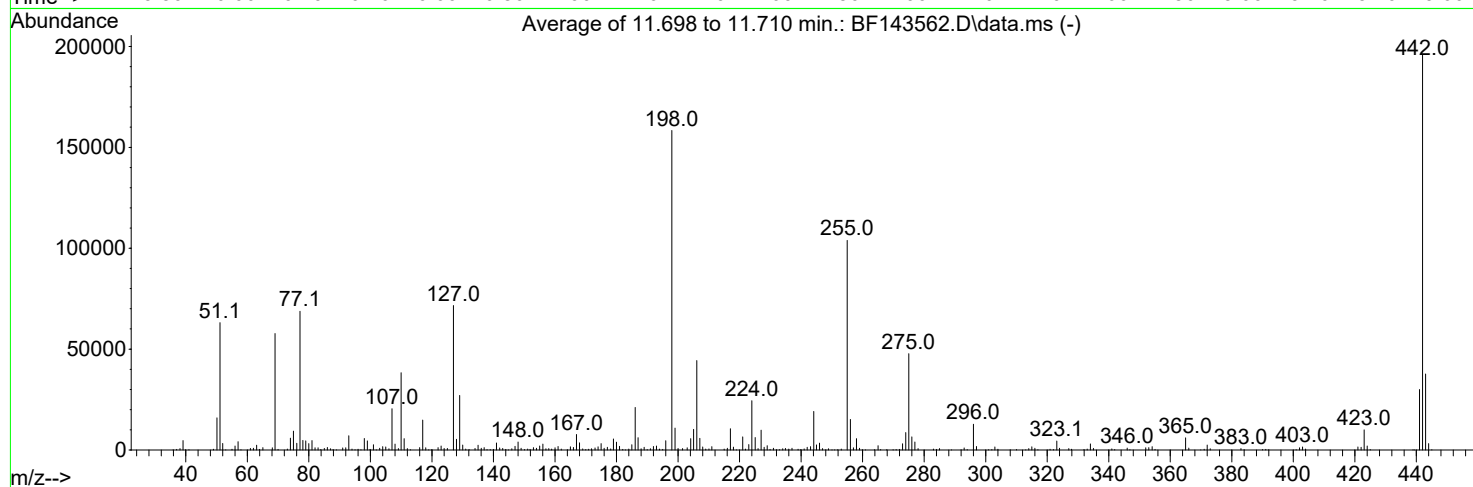


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF082225\
Data File : BF143562.D
Acq On : 22 Aug 2025 09:30
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF082025.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Thu Aug 21 06:12:21 2025

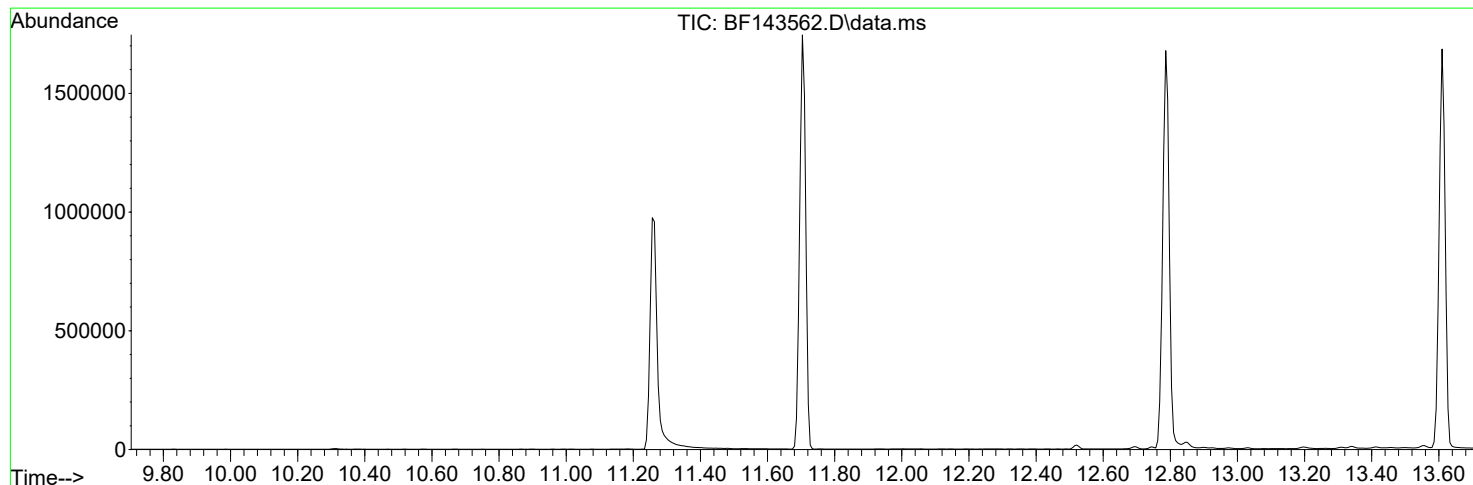

AutoFind: Scans 1616, 1617, 1618; Background Corrected with Scan 1610

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
68	69	0.00	2	2.0	1135	PASS
69	69	100	100	100.0	57712	PASS
70	69	0.00	2	0.6	333	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	158357	PASS
199	198	5	9	6.9	10882	PASS
365	198	1	100	3.8	6013	PASS
441	443	0.01	150	79.5	29981	PASS
442	442	100	100	100.0	195693	PASS
443	442	15	24	19.3	37699	PASS

DDT Breakdown




Date	Instrument Name	DFTPP Data File
8/22/2025	BNA_F	<u>BF143562.D</u>
Compound Name	Response	Retention Time
DDT	399110	13.61
DDD	5018	13.339
DDE	1337	12.974
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
6355	405465	1.57

Instrument :
BNA_F
ClientSampleId :
DFTPP

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF082225\
Data File : BF143562.D
Acq On : 22 Aug 2025 09:30
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Aug 22 09:53:54 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF082025.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Aug 21 06:12:21 2025
Response via : Initial Calibration

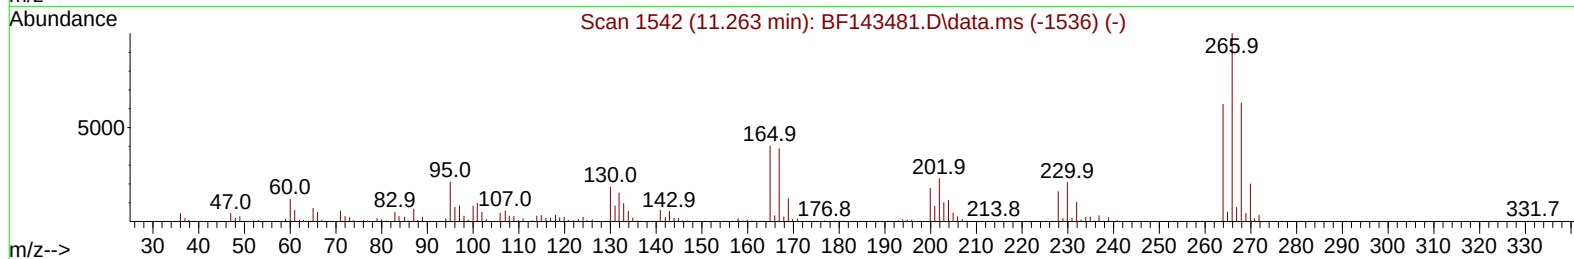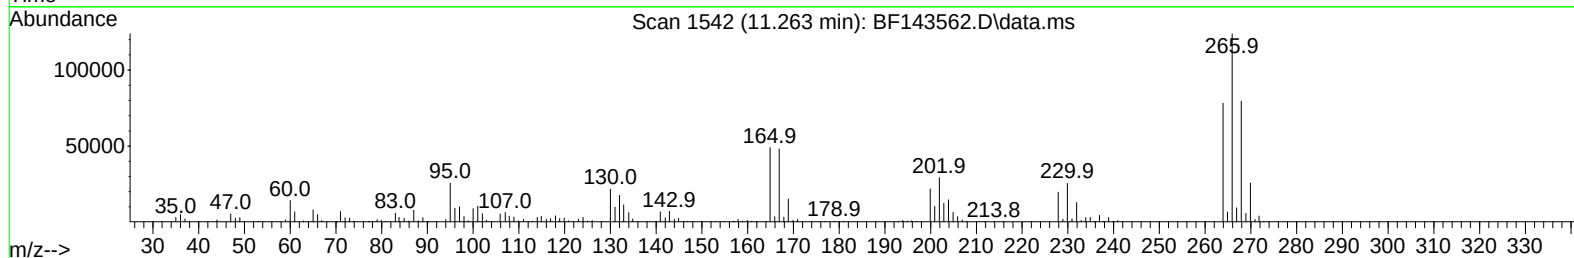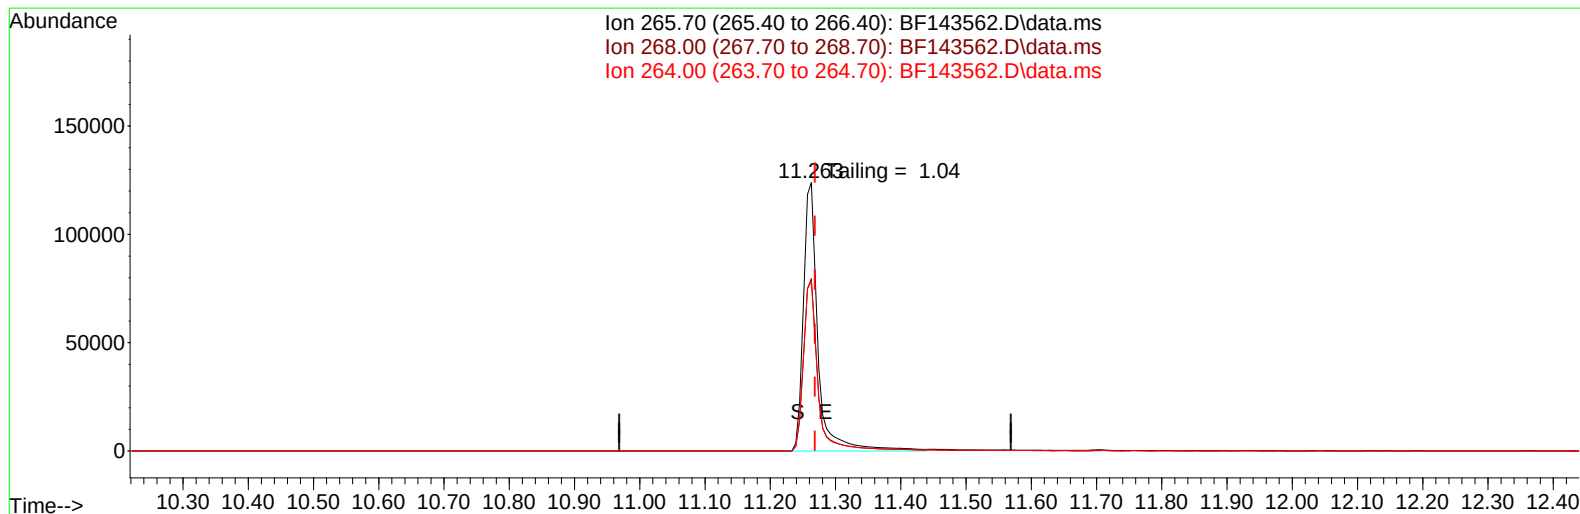

TIC: BF143562.D\data.ms

(70) Pentachlorophenol (C)

11.263min (-0.006) 106263.89 ng




response 193411

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.10	64.25
264.00	62.30	63.09
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF082225\
Data File : BF143562.D
Acq On : 22 Aug 2025 09:30
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Aug 22 09:53:54 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF082025.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Aug 21 06:12:21 2025
Response via : Initial Calibration

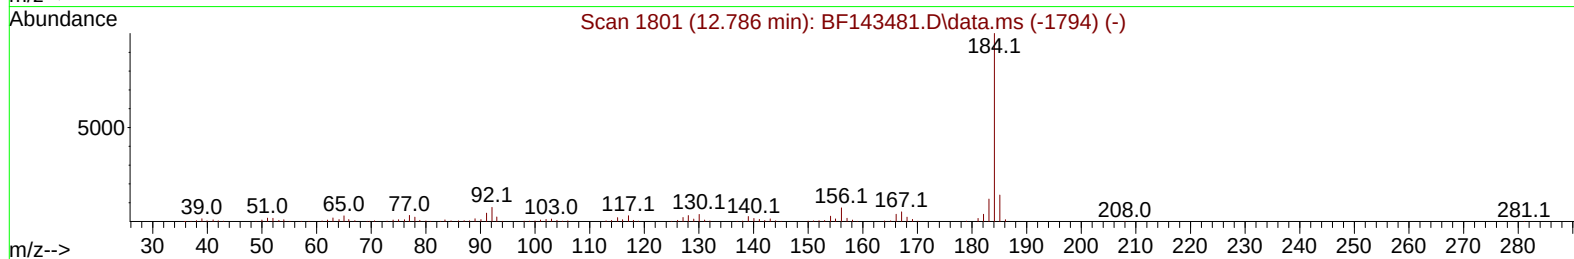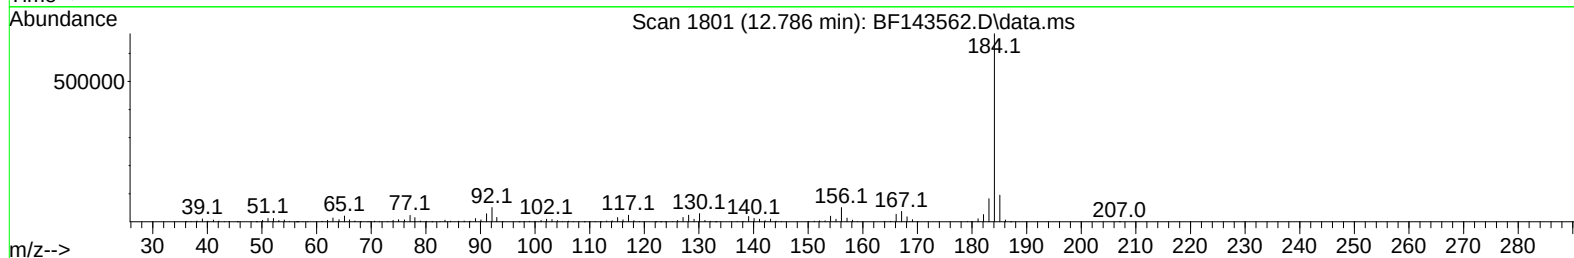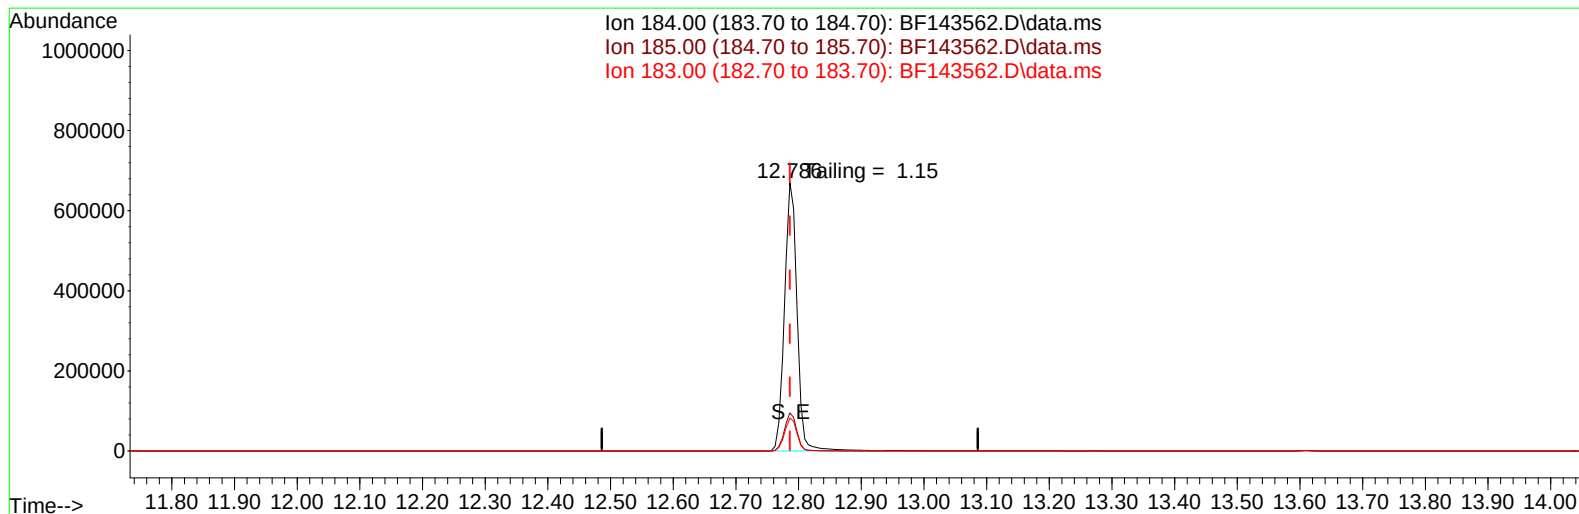

TIC: BF143562.D\data.ms

(77) Benzidine

12.786min (+ 0.000) 666495.20 ng

response 941621

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.10	14.18
183.00	11.90	12.27
0.00	0.00	0.00