

DATA REPORTING QUALIFIERS- ORGANIC

For reporting results, the following “ Results Qualifiers” are used:

Value	If the result is a value greater than or equal to the detection limit, report the value
U	Indicates the compound was analyzed for but was not detected. Report the minimum detection limit for the sample with the U, i.e. “10 U”. This is not necessarily the instrument detection limit attainable for this particular sample based on any concentration or dilution that may have been required.
ND	Indicates the analyte was analyzed for, but not detected
J	Indicates an estimated value. This flag is used: (1) When estimating a concentration for a tentatively identified compound (library search hits, where a 1:1 response is assumed.) (2) When the mass spectral data indicated the identification, however the result was less than the specified detection limit greater than zero. If the detection limit was 10ug/L and a concentration of 3 ug/L was calculated report as 3 J. This flag is used when similar situation arise on any organic parameter i.e. Pest, PCB and others.
B	Indicates the analyte was found in the blank as well as the sample report as “12 B”.
E	Indicates the analyte ‘s concentration exceeds the calibrated range of the instrument for that specific analysis.
D	This flag identifies all compounds identified in an analysis at a secondary dilution factor.
P	This flag is used for Pesticide/PCB target analyte when there is >25% difference for detected concentrations between the two GC columns. The lower of the two values is reported on Form 1 and flagged with a “P”.
N	This flag indicates presumptive evidence of a compound. This is only used for tentatively identified compounds (TICs), where the identification is based on a mass spectral library search. It applies to all TIC results. For generic characterization of a TIC, such as chlorinated hydrocarbon, the flag is not used.
A	This flag indicates that a Tentatively Identified Compound is a suspected aldol-condensation product.
Q	Indicates the LCS did not meet the control limits requirements

LAB CHRONICLE

OrderID: Q2894
Client: ATC Group Services LLC
Contact: Olga Seldinas

OrderDate: 8/18/2025 9:54:39 AM
Project: PS 190 BK - 2025SCA056
Location: J32

LabID	ClientID	Matrix	Test	Method	Sample Date	Prep Date	Anal Date	Received
Q2894-01	1A1B1C	CAULK	PCB	8082A	08/18/25	08/20/25	08/20/25	08/18/25
Q2894-02	2A2B2C	CAULK	PCB	8082A	08/18/25	08/20/25	08/20/25	08/18/25
Q2894-03	3A3B3C	CAULK	PCB	8082A	08/18/25	08/20/25	08/20/25	08/18/25
Q2894-04	4A4B4C	CAULK	PCB	8082A	08/18/25	08/20/25	08/20/25	08/18/25
Q2894-05	5A5B5C	CAULK	PCB	8082A	08/18/25	08/20/25	08/21/25	08/18/25



284 Sheffield Street, Mountainside, New Jersey 07092, Phone : 908 789 8900,
Fax : 908 789 8922

Hit Summary Sheet
SW-846

SDG No.: Q2894

Order ID: Q2894

Client: ATC Group Services LLC

Project ID: PS 190 BK - 2025SCA056

Sample ID	Client ID	Matrix	Parameter	Concentration	C	MDL	RDL	Units

Client ID :

Total Concentration: 0.000



QC SUMMARY

Surrogate Summary

SDG No.: **Q2894**

Client: **ATC Group Services LLC**

Analytical Method: **8082A**

Lab Sample ID	Client ID	Parameter	Column	Spike	Result	Recovery(%)	Qual	Limits(%)	
								Low	High
I.BLK-PO113002.D	PIBLK-PO113002.D	Tetrachloro-m-xyl	1	20	16.6	83		60	140
		Decachlorobiphen	1	20	17.2	86		60	140
		Tetrachloro-m-xyl	2	20	16.9	84		60	140
		Decachlorobiphen	2	20	18.1	91		60	140
I.BLK-PO113078.D	PIBLK-PO113078.D	Tetrachloro-m-xyl	1	20	18.1	91		60	140
		Decachlorobiphen	1	20	15.8	79		60	140
		Tetrachloro-m-xyl	2	20	17.5	88		60	140
		Decachlorobiphen	2	20	17.1	86		60	140
PB169322BS	PB169322BS	Tetrachloro-m-xyl	1	20	18.2	91		32	144
		Decachlorobiphen	1	20	17.9	90		32	175
		Tetrachloro-m-xyl	2	20	17.5	87		32	144
		Decachlorobiphen	2	20	19.0	95		32	175
Q2894-01	1A1B1C	Tetrachloro-m-xyl	1	20	21.6	108		32	144
		Decachlorobiphen	1	20	18.7	94		32	175
		Tetrachloro-m-xyl	2	20	24.0	120		32	144
		Decachlorobiphen	2	20	20.1	100		32	175
Q2894-02	2A2B2C	Tetrachloro-m-xyl	1	20	20.3	102		32	144
		Decachlorobiphen	1	20	19.7	99		32	175
		Tetrachloro-m-xyl	2	20	19.9	100		32	144
		Decachlorobiphen	2	20	20.9	104		32	175
Q2894-03	3A3B3C	Tetrachloro-m-xyl	1	20	20.7	103		32	144
		Decachlorobiphen	1	20	19.1	96		32	175
		Tetrachloro-m-xyl	2	20	20.4	102		32	144
		Decachlorobiphen	2	20	19.9	99		32	175
I.BLK-PO113093.D	PIBLK-PO113093.D	Tetrachloro-m-xyl	1	20	17.6	88		60	140
		Decachlorobiphen	1	20	19.0	95		60	140
		Tetrachloro-m-xyl	2	20	17.3	86		60	140
		Decachlorobiphen	2	20	18.3	92		60	140
PB169322BL	PB169322BL	Tetrachloro-m-xyl	1	20	18.8	94		32	144
		Decachlorobiphen	1	20	20.2	101		32	175
		Tetrachloro-m-xyl	2	20	18.1	91		32	144
		Decachlorobiphen	2	20	19.3	97		32	175
Q2894-04	4A4B4C	Tetrachloro-m-xyl	1	20	20.9	104		32	144
		Decachlorobiphen	1	20	22.1	111		32	175
		Tetrachloro-m-xyl	2	20	20.4	102		32	144
		Decachlorobiphen	2	20	20.5	103		32	175
I.BLK-PO113108.D	PIBLK-PO113108.D	Tetrachloro-m-xyl	1	20	17.9	90		60	140
		Decachlorobiphen	1	20	17.7	89		60	140
		Tetrachloro-m-xyl	2	20	17.5	88		60	140
		Decachlorobiphen	2	20	19.0	95		60	140
I.BLK-PO113118.D	PIBLK-PO113118.D	Tetrachloro-m-xyl	1	20	18.5	93		60	140

Surrogate Summary

SDG No.: Q2894

Client: ATC Group Services LLC

Analytical Method: 8082A

Lab Sample ID	Client ID	Parameter	Column	Spike	Result	Recovery(%)	Qual	Limits(%)	
								Low	High
I.BLK-PO113118.D	PIBLK-PO113118.D	Decachlorobiphen	1	20	18.9	95		60	140
		Tetrachloro-m-xyl	2	20	17.7	88		60	140
Q2894-05	5A5B5C	Decachlorobiphen	2	20	19.1	96		60	140
		Tetrachloro-m-xyl	1	20	19.0	95		32	144
		Decachlorobiphen	1	20	29.9	149		32	175
		Tetrachloro-m-xyl	2	20	18.1	91		32	144
		Decachlorobiphen	2	20	30.1	151		32	175
		Tetrachloro-m-xyl	1	20	18.3	92		60	140
I.BLK-PO113125.D	PIBLK-PO113125.D	Decachlorobiphen	1	20	18.8	94		60	140
		Tetrachloro-m-xyl	2	20	17.8	89		60	140
		Decachlorobiphen	2	20	18.8	94		60	140
		Tetrachloro-m-xyl	2	20	18.8	94		60	140



284 Sheffield Street, Mountainside, New Jersey 07092, Phone : 908 789 8900,
Fax : 908 789 8922

Laboratory Control Sample/Laboratory Control Sample Duplicate Summary

SW-846

SDG No.: Q2894

Analytical Method: 8082A

Client: ATC Group Services LLC

Datafile : PO113081.D

Lab Sample ID	Parameter	Spike	Result	Units	Rec	RPD	Qual	RPD	Low	Limits	RPD
								Qual		High	
PB169322BS (Column 1)	AR1016	166.6	178	ug/kg	107				71	120	
	AR1260	166.6	171	ug/kg	103				65	130	
PB169322BS (Column 2)	AR1016	166.6	166	ug/kg	100				71	120	
	AR1260	166.6	162	ug/kg	97				65	130	

4C

PESTICIDE METHOD BLANK SUMMARY

Client ID

PB169322BL

Lab Name: Alliance

Contract: ATCE02

Lab Code: ACE

SDG NO.: Q2894

Lab Sample ID: PB169322BL

Lab File ID: PO113094.D

Matrix: (soil/water) Solid

Extraction: (Type) SOXH

Sulfur Cleanup: (Y/N) N

Date Extracted: 08/20/2025

Date Analyzed (1): 08/20/2025

Date Analyzed (2): 08/20/2025

Time Analyzed (1): 17:09

Time Analyzed (2): 17:09

Instrument ID (1): ECD_O

Instrument ID (2): ECD_O

GC Column (1): ZB-MR1 ID: 0.32 (mm)

GC Column (2): ZB-MR2 ID: 0.32 (mm)

THIS METHOD BLANK APPLIES TO THE FOLLOWING SAMPLES, MS AND MSD:

EPA SAMPLE NO.	LAB SAMPLE ID	LAB FILE ID	DATE ANALYZED 1	DATE ANALYZED 2
PB169322BS	PB169322BS	PO113081.D	08/20/2025	08/20/2025
1A1B1C	Q2894-01	PO113082.D	08/20/2025	08/20/2025
2A2B2C	Q2894-02	PO113083.D	08/20/2025	08/20/2025
3A3B3C	Q2894-03	PO113084.D	08/20/2025	08/20/2025
4A4B4C	Q2894-04	PO113097.D	08/20/2025	08/20/2025
5A5B5C	Q2894-05	PO113120.D	08/21/2025	08/21/2025

COMMENTS: _____



SAMPLE DATA

Report of Analysis

Client:	ATC Group Services LLC	Date Collected:	08/18/25
Project:	PS 190 BK - 2025SCA056	Date Received:	08/18/25
Client Sample ID:	1A1B1C	SDG No.:	Q2894
Lab Sample ID:	Q2894-01	Matrix:	CAULK
Analytical Method:	8082A	% Solid:	100
Sample Wt/Vol:	8.42	Units:	g
Soil Aliquot Vol:			uL
Extraction Type:		Test:	PCB
GPC Factor :	1.0	PH :	
Prep Method :	SW3541B	Injection Volume :	

File ID/Qc Batch:	Dilution:	Prep Date	Date Analyzed	Prep Batch ID
PO113082.D	1	08/20/25 08:40	08/20/25 12:36	PB169322

CAS Number	Parameter	Conc.	Qualifier	MDL	LOQ / CRQL	Units
TARGETS						
12674-11-2	Aroclor-1016	14.1	U	14.1	60.6	ug/kg
11104-28-2	Aroclor-1221	14.4	U	14.4	60.6	ug/kg
11141-16-5	Aroclor-1232	13.3	U	13.3	60.6	ug/kg
53469-21-9	Aroclor-1242	14.3	U	14.3	60.6	ug/kg
12672-29-6	Aroclor-1248	21.1	U	21.1	60.6	ug/kg
11097-69-1	Aroclor-1254	11.4	U	11.4	60.6	ug/kg
37324-23-5	Aroclor-1262	17.9	U	17.9	60.6	ug/kg
11100-14-4	Aroclor-1268	12.8	U	12.8	60.6	ug/kg
11096-82-5	Aroclor-1260	11.5	U	11.5	60.6	ug/kg
SURROGATES						
877-09-8	Tetrachloro-m-xylene	24.0		32 - 144	120%	SPK: 20
2051-24-3	Decachlorobiphenyl	20.1		32 - 175	100%	SPK: 20

Comments:

U = Not Detected
 LOQ = Limit of Quantitation
 MDL = Method Detection Limit
 LOD = Limit of Detection
 E = Value Exceeds Calibration Range
 P = Indicates >25% difference for detected concentrations between the two GC columns
 Q = indicates LCS control criteria did not meet requirements
 M = MS/MSD acceptance criteria did not meet requirements

J = Estimated Value
 B = Analyte Found in Associated Method Blank
 N = Presumptive Evidence of a Compound
 * = Values outside of QC limits
 D = Dilution
 S = Indicates estimated value where valid five-point calibration was not performed prior to analyte detection in sample.
 () = Laboratory InHouse Limit

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0082025\
 Data File : PO113082.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 20 Aug 2025 12:36
 Operator : YP/AJ
 Sample : Q2894-01
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 1A1B1C

Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 08/21/2025
 Supervised By :mohammad ahmed 08/22/2025

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 20 13:06:14 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0081825.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Aug 19 06:08:32 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.661	3.655	177.0E6	121.2E6	21.619m	23.957m
2) SA Decachlor...	8.680	8.626	129.8E6	38058585	18.728	20.085

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO082025\
Data File : PO113082.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 20 Aug 2025 12:36
Operator : YP/AJ
Sample : Q2894-01
Misc :
ALS Vial : 10 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
1A1B1C


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 08/21/2025
Supervised By :mohammad ahmed 08/22/2025

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 20 13:06:14 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO081825.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Aug 19 06:08:32 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

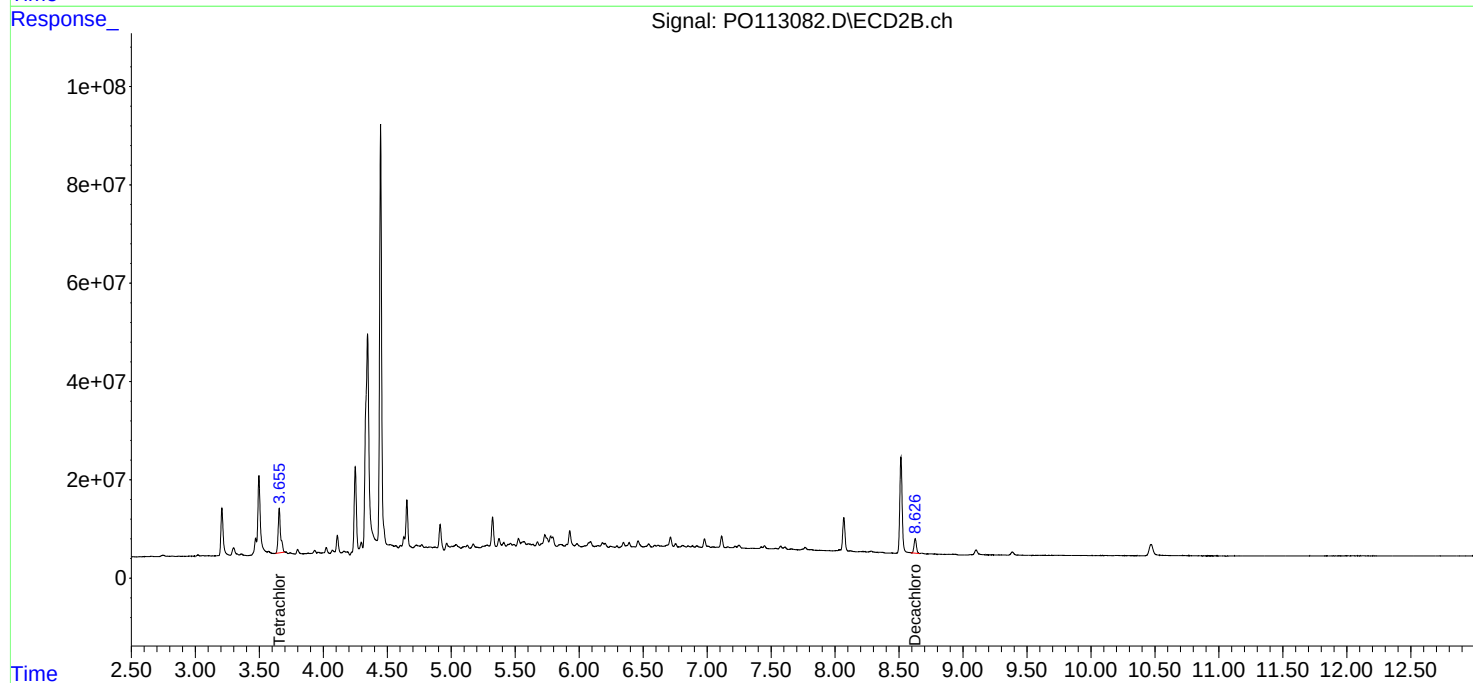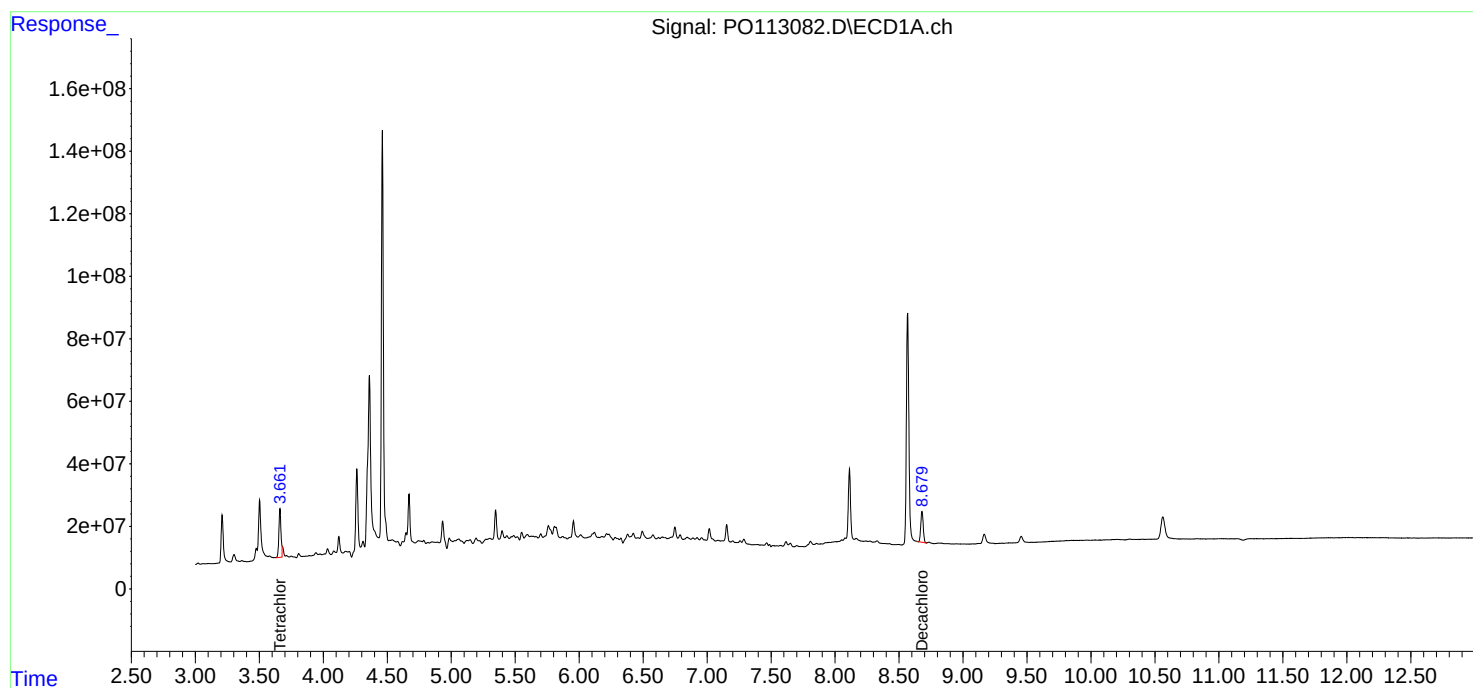

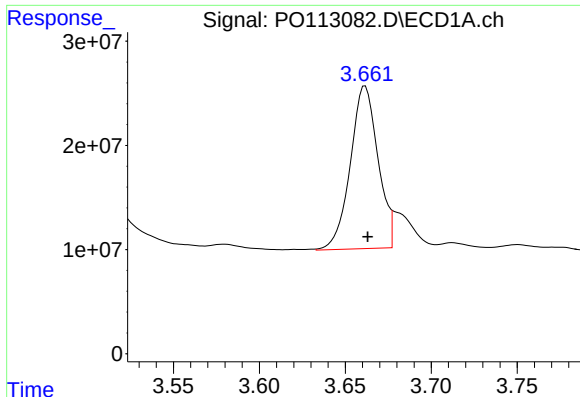


#1 Tetrachloro-m-xylene

R.T.: 3.661 min
Delta R.T.: -0.002 min
Response: 176982472
Conc: 21.62 ng/ml

Instrument :
ECD_O
ClientSampleId :
1A1B1C


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 08/21/2025
Supervised By :mohammad ahmed 08/22/2025

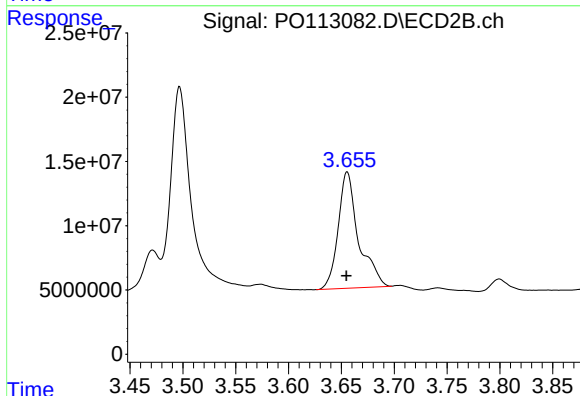


#1 Tetrachloro-m-xylene

R.T.: 3.655 min
Delta R.T.: 0.000 min
Response: 121237545
Conc: 23.96 ng/ml m

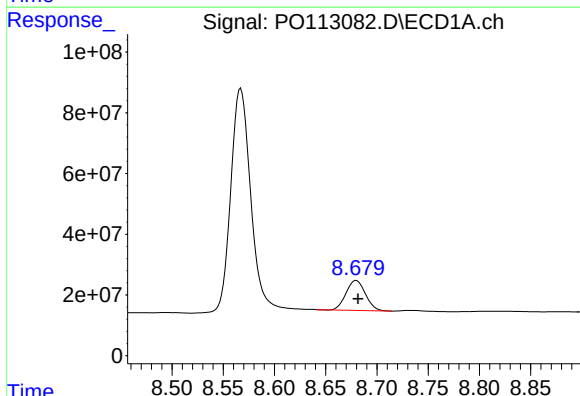

#2 Decachlorobiphenyl

R.T.: 8.680 min
Delta R.T.: -0.002 min
Response: 129810302
Conc: 18.73 ng/ml

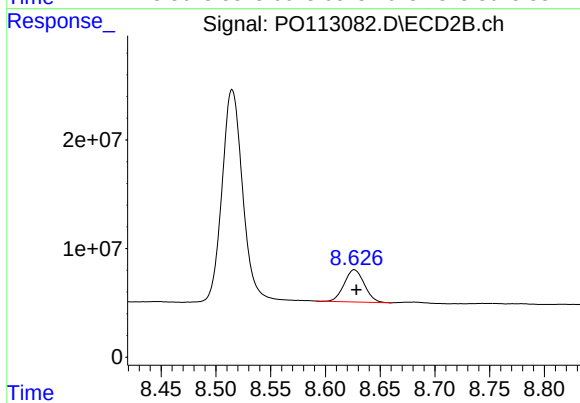

#2 Decachlorobiphenyl

R.T.: 8.626 min
Delta R.T.: -0.002 min
Response: 38058585
Conc: 20.09 ng/ml

Report of Analysis

Client:	ATC Group Services LLC	Date Collected:	08/18/25
Project:	PS 190 BK - 2025SCA056	Date Received:	08/18/25
Client Sample ID:	2A2B2C	SDG No.:	Q2894
Lab Sample ID:	Q2894-02	Matrix:	CAULK
Analytical Method:	8082A	% Solid:	100
Sample Wt/Vol:	2.19	Units:	g
Soil Aliquot Vol:			uL
Extraction Type:		Test:	PCB
GPC Factor :	1.0	PH :	
Prep Method :	SW3541B	Injection Volume :	

File ID/Qc Batch:	Dilution:	Prep Date	Date Analyzed	Prep Batch ID
PO113083.D	1	08/20/25 08:40	08/20/25 12:55	PB169322

CAS Number	Parameter	Conc.	Qualifier	MDL	LOQ / CRQL	Units
TARGETS						
12674-11-2	Aroclor-1016	54.1	U	54.1	233	ug/kg
11104-28-2	Aroclor-1221	55.2	U	55.2	233	ug/kg
11141-16-5	Aroclor-1232	51.0	U	51.0	233	ug/kg
53469-21-9	Aroclor-1242	54.9	U	54.9	233	ug/kg
12672-29-6	Aroclor-1248	81.1	U	81.1	233	ug/kg
11097-69-1	Aroclor-1254	44.0	U	44.0	233	ug/kg
37324-23-5	Aroclor-1262	68.8	U	68.8	233	ug/kg
11100-14-4	Aroclor-1268	49.3	U	49.3	233	ug/kg
11096-82-5	Aroclor-1260	44.2	U	44.2	233	ug/kg
SURROGATES						
877-09-8	Tetrachloro-m-xylene	20.3		32 - 144	102%	SPK: 20
2051-24-3	Decachlorobiphenyl	20.9		32 - 175	104%	SPK: 20

Comments:

U = Not Detected

LOQ = Limit of Quantitation

MDL = Method Detection Limit

LOD = Limit of Detection

E = Value Exceeds Calibration Range

P = Indicates >25% difference for detected concentrations between the two GC columns

Q = indicates LCS control criteria did not meet requirements

M = MS/MSD acceptance criteria did not meet requirements

J = Estimated Value

B = Analyte Found in Associated Method Blank

N = Presumptive Evidence of a Compound

* = Values outside of QC limits

D = Dilution

S = Indicates estimated value where valid five-point calibration was not performed prior to analyte detection in sample.

() = Laboratory InHouse Limit

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0082025\
 Data File : PO113083.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 20 Aug 2025 12:55
 Operator : YP/AJ
 Sample : Q2894-02
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 2A2B2C

Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 08/21/2025
 Supervised By :mohammad ahmed 08/22/2025

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 20 13:41:41 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0081825.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Aug 19 06:08:32 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.662	3.655	166.5E6	100.9E6	20.333m	19.945m
2) SA Decachlor...	8.681	8.627	136.7E6	39511998	19.723	20.852

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO082025\
Data File : PO113083.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 20 Aug 2025 12:55
Operator : YP/AJ
Sample : Q2894-02
Misc :
ALS Vial : 11 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
2A2B2C


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 08/21/2025
Supervised By :mohammad ahmed 08/22/2025

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 20 13:41:41 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO081825.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Aug 19 06:08:32 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

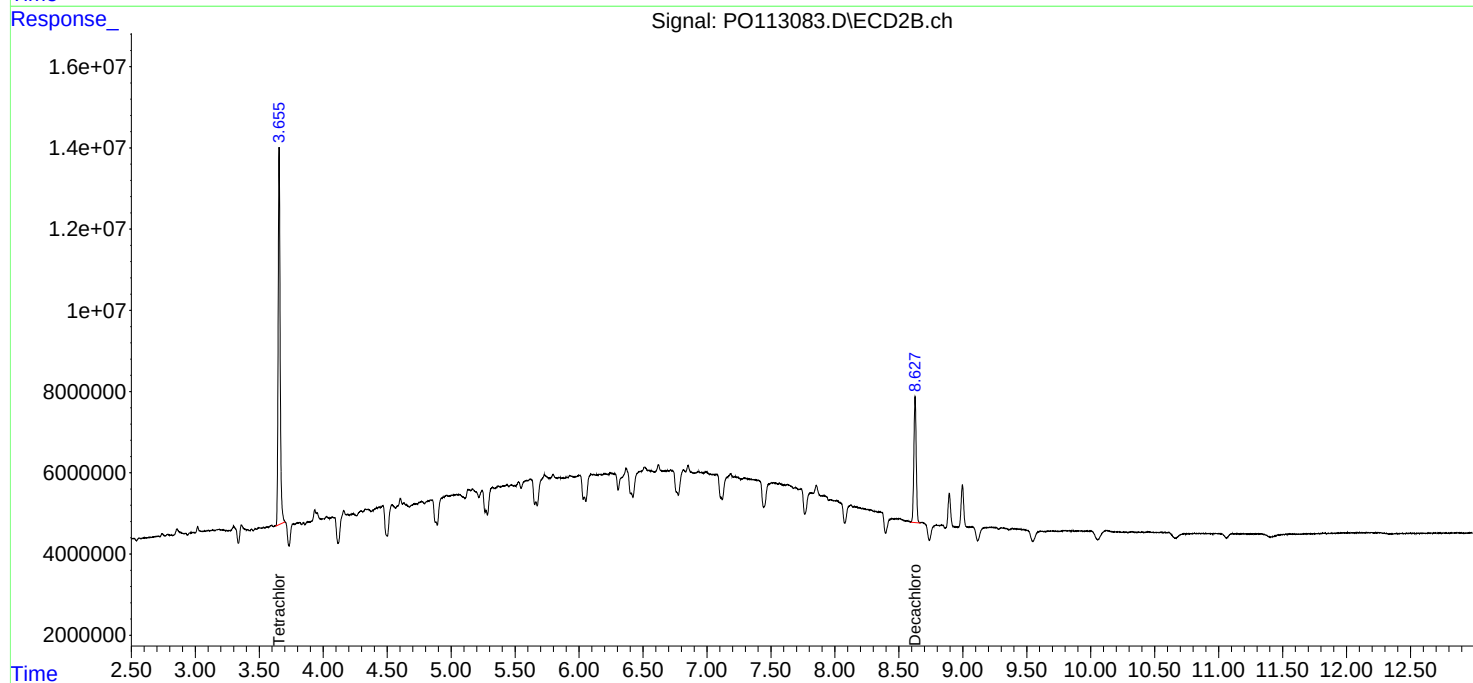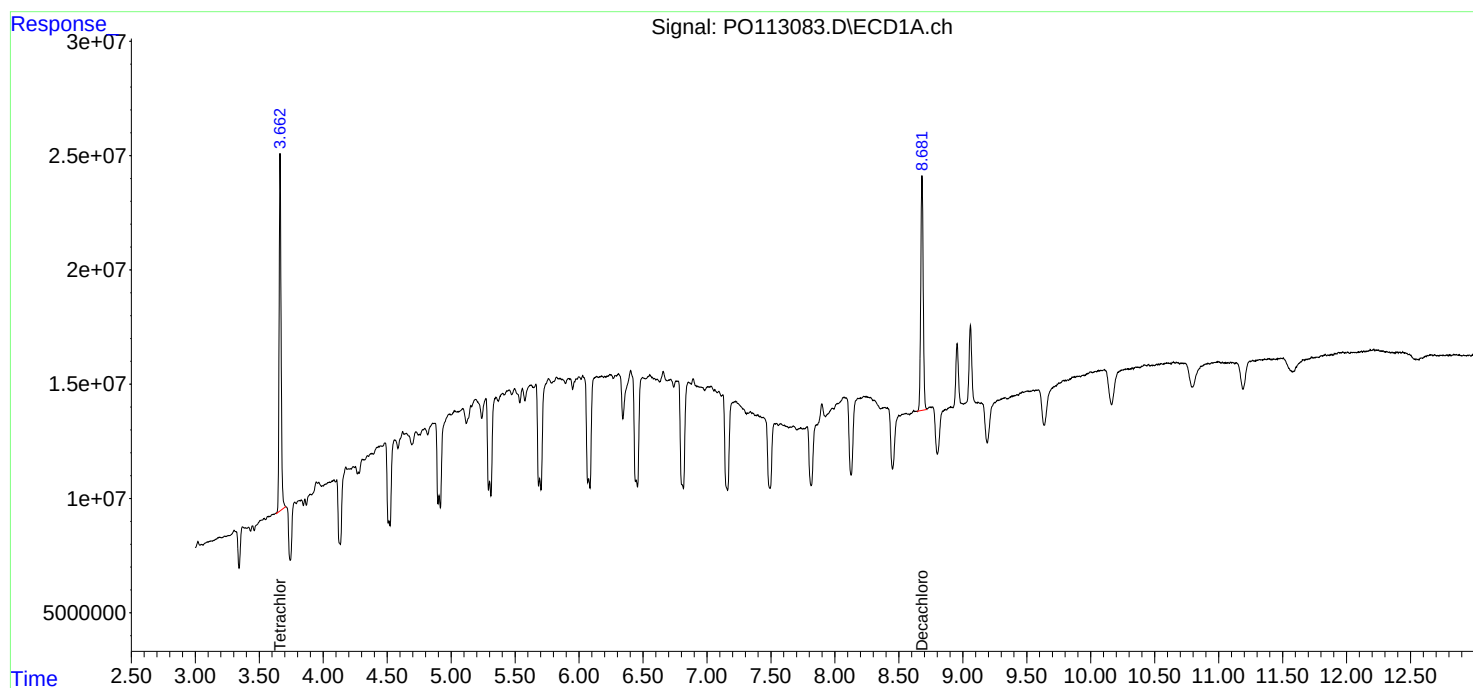

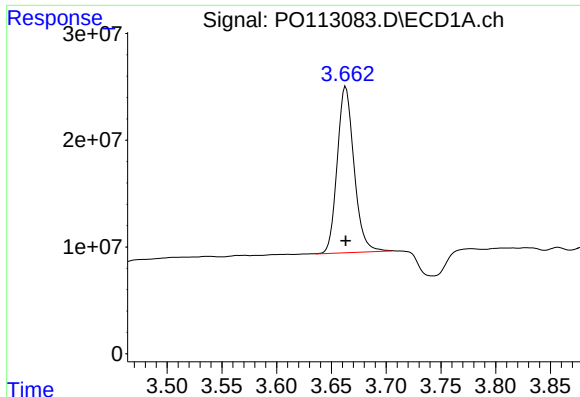


#1 Tetrachloro-m-xylene

R.T.: 3.662 min
Delta R.T.: 0.000 min
Response: 166459673
Conc: 20.33 ng/ml

Instrument :
ECD_O
ClientSampleId :
2A2B2C


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 08/21/2025
Supervised By :mohammad ahmed 08/22/2025

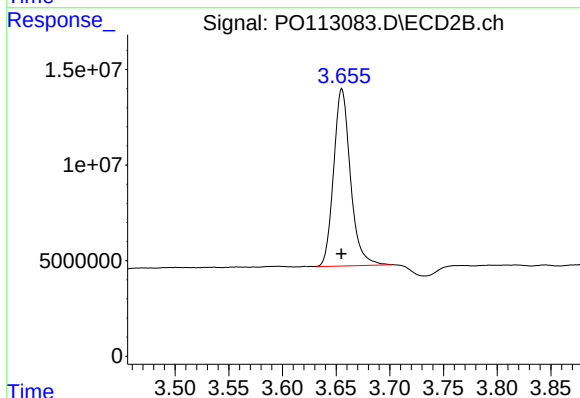


#1 Tetrachloro-m-xylene

R.T.: 3.655 min
Delta R.T.: 0.000 min
Response: 100936502
Conc: 19.95 ng/ml m

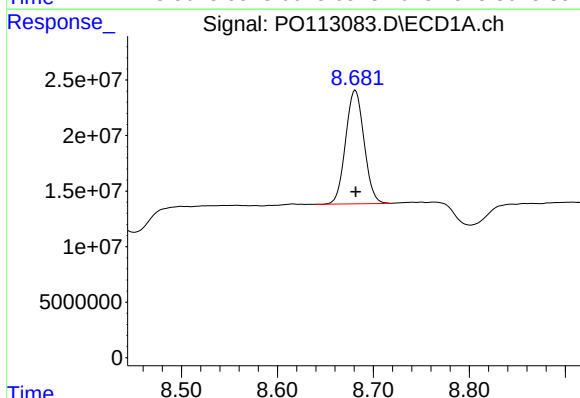

#2 Decachlorobiphenyl

R.T.: 8.681 min
Delta R.T.: 0.000 min
Response: 136711602
Conc: 19.72 ng/ml

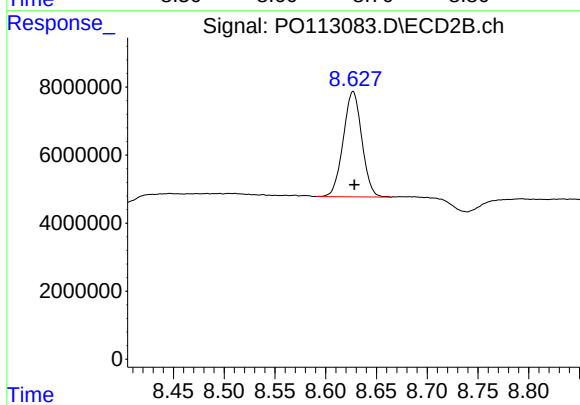

#2 Decachlorobiphenyl

R.T.: 8.627 min
Delta R.T.: -0.001 min
Response: 39511998
Conc: 20.85 ng/ml

Report of Analysis

Client:	ATC Group Services LLC		Date Collected:	08/18/25	
Project:	PS 190 BK - 2025SCA056		Date Received:	08/18/25	
Client Sample ID:	3A3B3C		SDG No.:	Q2894	
Lab Sample ID:	Q2894-03		Matrix:	CAULK	
Analytical Method:	8082A		% Solid:	100	Decanted:
Sample Wt/Vol:	1.83	Units: g	Final Vol:	10000	uL
Soil Aliquot Vol:		uL	Test:	PCB	
Extraction Type:			Injection Volume :		
GPC Factor :	1.0	PH :			
Prep Method :	SW3541B				

File ID/Qc Batch:	Dilution:	Prep Date	Date Analyzed	Prep Batch ID
PO113084.D	1	08/20/25 08:40	08/20/25 13:13	PB169322

CAS Number	Parameter	Conc.	Qualifier	MDL	LOQ / CRQL	Units
TARGETS						
12674-11-2	Aroclor-1016	64.8	U	64.8	279	ug/kg
11104-28-2	Aroclor-1221	66.1	U	66.1	279	ug/kg
11141-16-5	Aroclor-1232	61.0	U	61.0	279	ug/kg
53469-21-9	Aroclor-1242	65.7	U	65.7	279	ug/kg
12672-29-6	Aroclor-1248	97.0	U	97.0	279	ug/kg
11097-69-1	Aroclor-1254	52.6	U	52.6	279	ug/kg
37324-23-5	Aroclor-1262	82.3	U	82.3	279	ug/kg
11100-14-4	Aroclor-1268	59.0	U	59.0	279	ug/kg
11096-82-5	Aroclor-1260	53.0	U	53.0	279	ug/kg
SURROGATES						
877-09-8	Tetrachloro-m-xylene	20.7		32 - 144	103%	SPK: 20
2051-24-3	Decachlorobiphenyl	19.9		32 - 175	99%	SPK: 20

Comments:

U = Not Detected

LOQ = Limit of Quantitation

MDL = Method Detection Limit

LOD = Limit of Detection

E = Value Exceeds Calibration Range

P = Indicates >25% difference for detected concentrations between the two GC columns

Q = indicates LCS control criteria did not meet requirements

M = MS/MSD acceptance criteria did not meet requirements

J = Estimated Value

B = Analyte Found in Associated Method Blank

N = Presumptive Evidence of a Compound

* = Values outside of QC limits

D = Dilution

S = Indicates estimated value where valid five-point calibration was not performed prior to analyte detection in sample.

() = Laboratory InHouse Limit

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0082025\
 Data File : PO113084.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 20 Aug 2025 13:13
 Operator : YP/AJ
 Sample : Q2894-03
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 3A3B3C

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 20 13:42:20 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0081825.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Aug 19 06:08:32 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.664	3.655	169.4E6	103.1E6	20.693	20.374
2) SA Decachlor...	8.682	8.627	132.5E6	37685598	19.119	19.888

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO082025\
Data File : PO113084.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 20 Aug 2025 13:13
Operator : YP/AJ
Sample : Q2894-03
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
3A3B3C

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 20 13:42:20 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO081825.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Aug 19 06:08:32 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µm Signal #2 Info : 30M x 0.32mm x 0.25µm

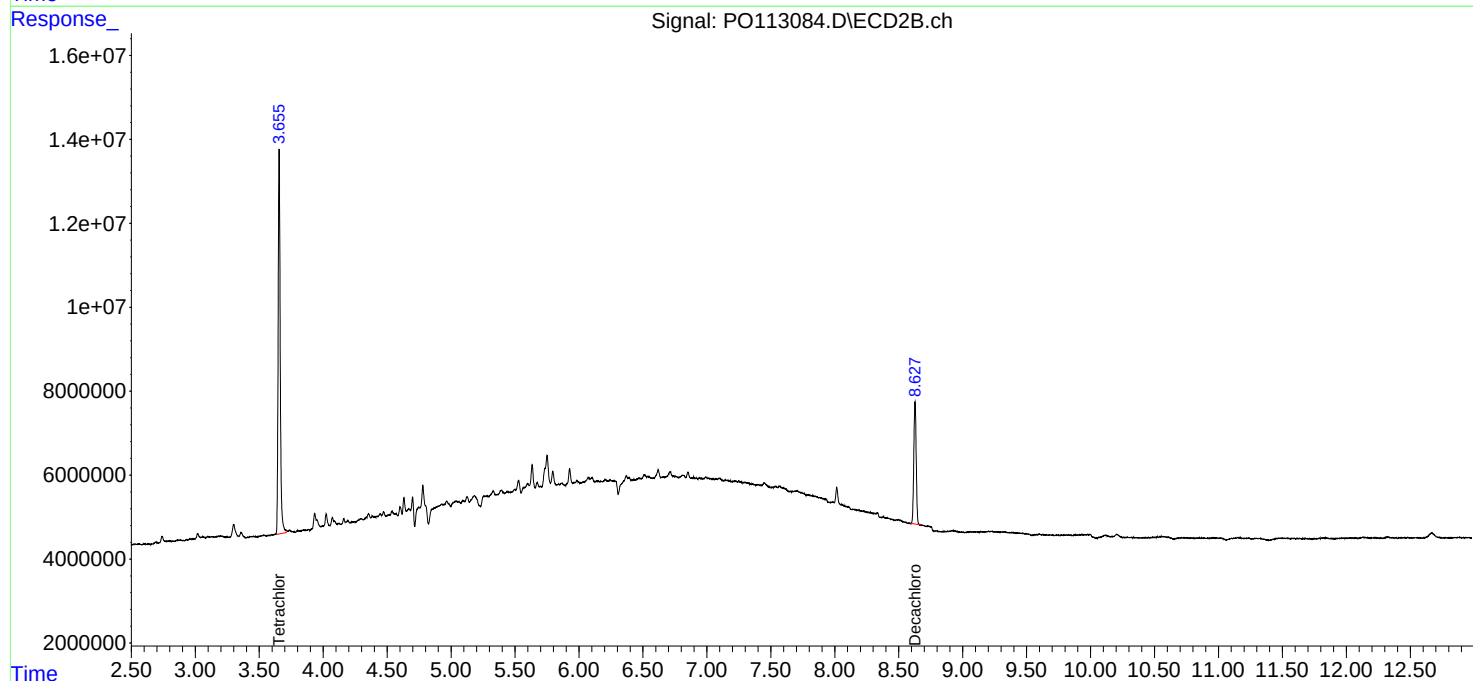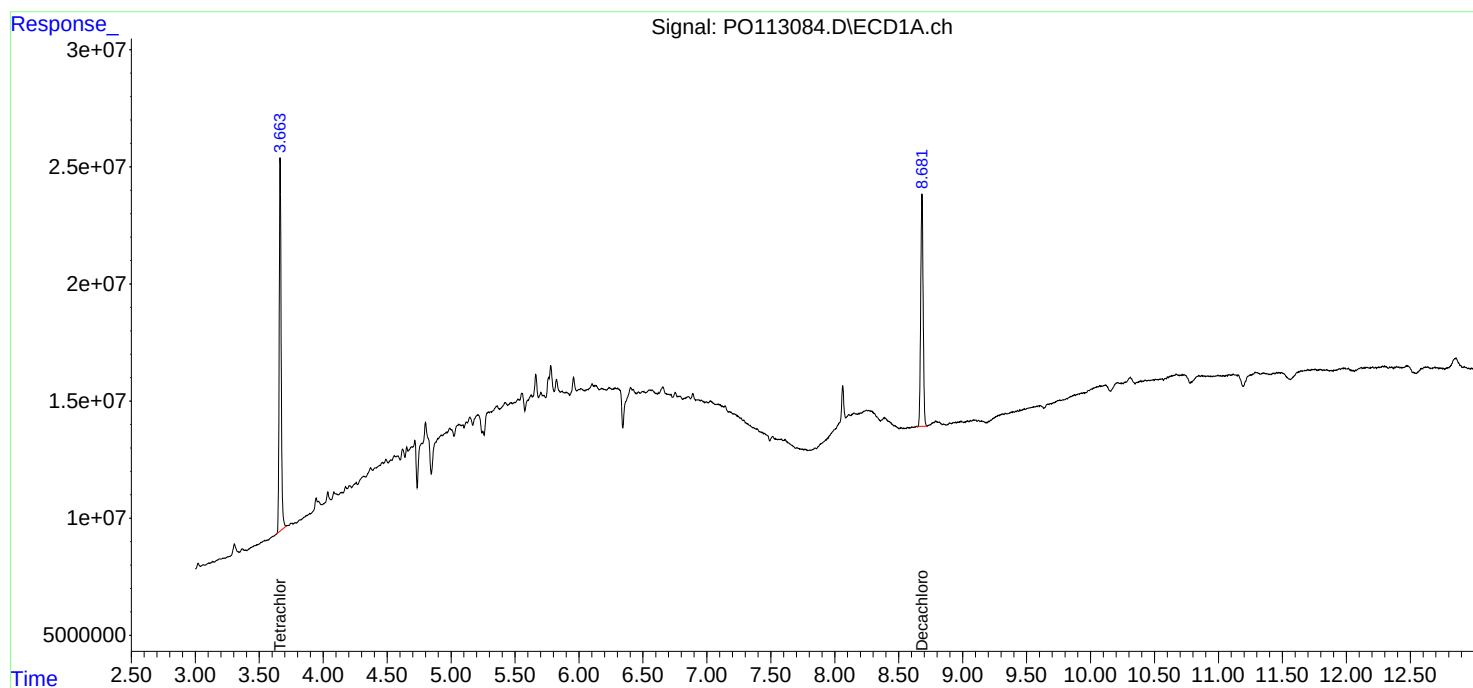


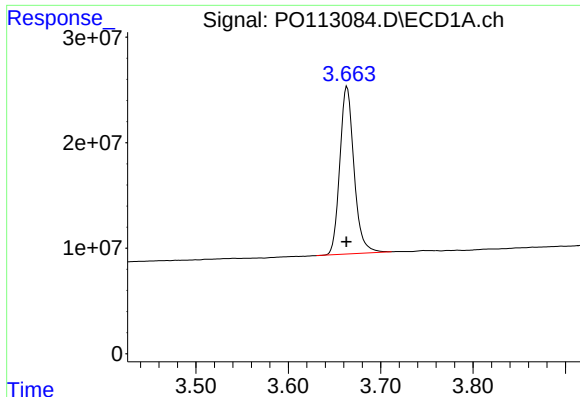

#1 Tetrachloro-m-xylene


R.T.: 3.664 min
Delta R.T.: 0.000 min
Response: 169401365
Conc: 20.69 ng/ml

Instrument :
ECD_O
ClientSampleId :
3A3B3C

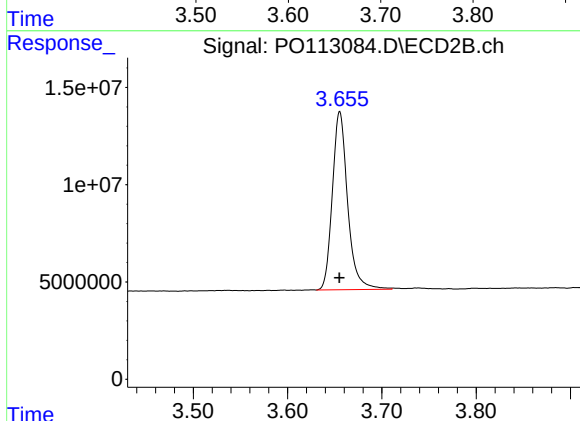


#1 Tetrachloro-m-xylene

R.T.: 3.655 min
Delta R.T.: 0.000 min
Response: 103105395
Conc: 20.37 ng/ml

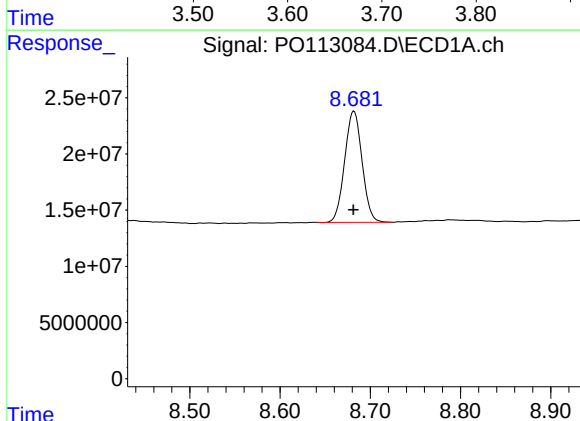

#2 Decachlorobiphenyl

R.T.: 8.682 min
Delta R.T.: 0.000 min
Response: 132524228
Conc: 19.12 ng/ml

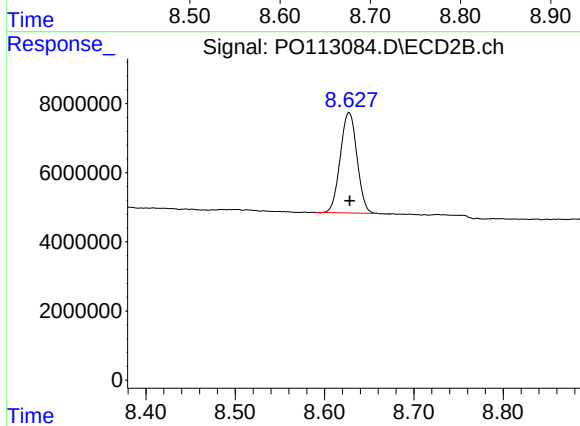

#2 Decachlorobiphenyl

R.T.: 8.627 min
Delta R.T.: 0.000 min
Response: 37685598
Conc: 19.89 ng/ml

Report of Analysis

Client:	ATC Group Services LLC	Date Collected:	08/18/25
Project:	PS 190 BK - 2025SCA056	Date Received:	08/18/25
Client Sample ID:	4A4B4C	SDG No.:	Q2894
Lab Sample ID:	Q2894-04	Matrix:	CAULK
Analytical Method:	8082A	% Solid:	100
Sample Wt/Vol:	2.3	Units:	g
Soil Aliquot Vol:			uL
Extraction Type:		Test:	PCB
GPC Factor :	1.0	PH :	
Prep Method :	SW3541B	Injection Volume :	

File ID/Qc Batch:	Dilution:	Prep Date	Date Analyzed	Prep Batch ID
PO113097.D	1	08/20/25 08:40	08/20/25 18:03	PB169322

CAS Number	Parameter	Conc.	Qualifier	MDL	LOQ / CRQL	Units
TARGETS						
12674-11-2	Aroclor-1016	51.5	U	51.5	222	ug/kg
11104-28-2	Aroclor-1221	52.6	U	52.6	222	ug/kg
11141-16-5	Aroclor-1232	48.5	U	48.5	222	ug/kg
53469-21-9	Aroclor-1242	52.3	U	52.3	222	ug/kg
12672-29-6	Aroclor-1248	77.2	U	77.2	222	ug/kg
11097-69-1	Aroclor-1254	41.9	U	41.9	222	ug/kg
37324-23-5	Aroclor-1262	65.5	U	65.5	222	ug/kg
11100-14-4	Aroclor-1268	47.0	U	47.0	222	ug/kg
11096-82-5	Aroclor-1260	42.1	U	42.1	222	ug/kg
SURROGATES						
877-09-8	Tetrachloro-m-xylene	20.9		32 - 144	104%	SPK: 20
2051-24-3	Decachlorobiphenyl	22.1		32 - 175	111%	SPK: 20

Comments:

U = Not Detected

LOQ = Limit of Quantitation

MDL = Method Detection Limit

LOD = Limit of Detection

E = Value Exceeds Calibration Range

P = Indicates >25% difference for detected concentrations between the two GC columns

Q = indicates LCS control criteria did not meet requirements

M = MS/MSD acceptance criteria did not meet requirements

J = Estimated Value

B = Analyte Found in Associated Method Blank

N = Presumptive Evidence of a Compound

* = Values outside of QC limits

D = Dilution

S = Indicates estimated value where valid five-point calibration was not performed prior to analyte detection in sample.

() = Laboratory InHouse Limit

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0082025\
 Data File : PO113097.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 20 Aug 2025 18:03
 Operator : YP/AJ
 Sample : Q2894-04
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 4A4B4C

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 21 01:41:59 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0081825.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Aug 19 06:08:32 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.664	3.655	170.7E6	103.1E6	20.845	20.369
2) SA Decachlor...	8.682	8.626	153.2E6	38895590	22.104	20.527

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO082025\
Data File : PO113097.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 20 Aug 2025 18:03
Operator : YP/AJ
Sample : Q2894-04
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
4A4B4C

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 21 01:41:59 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO081825.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Aug 19 06:08:32 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

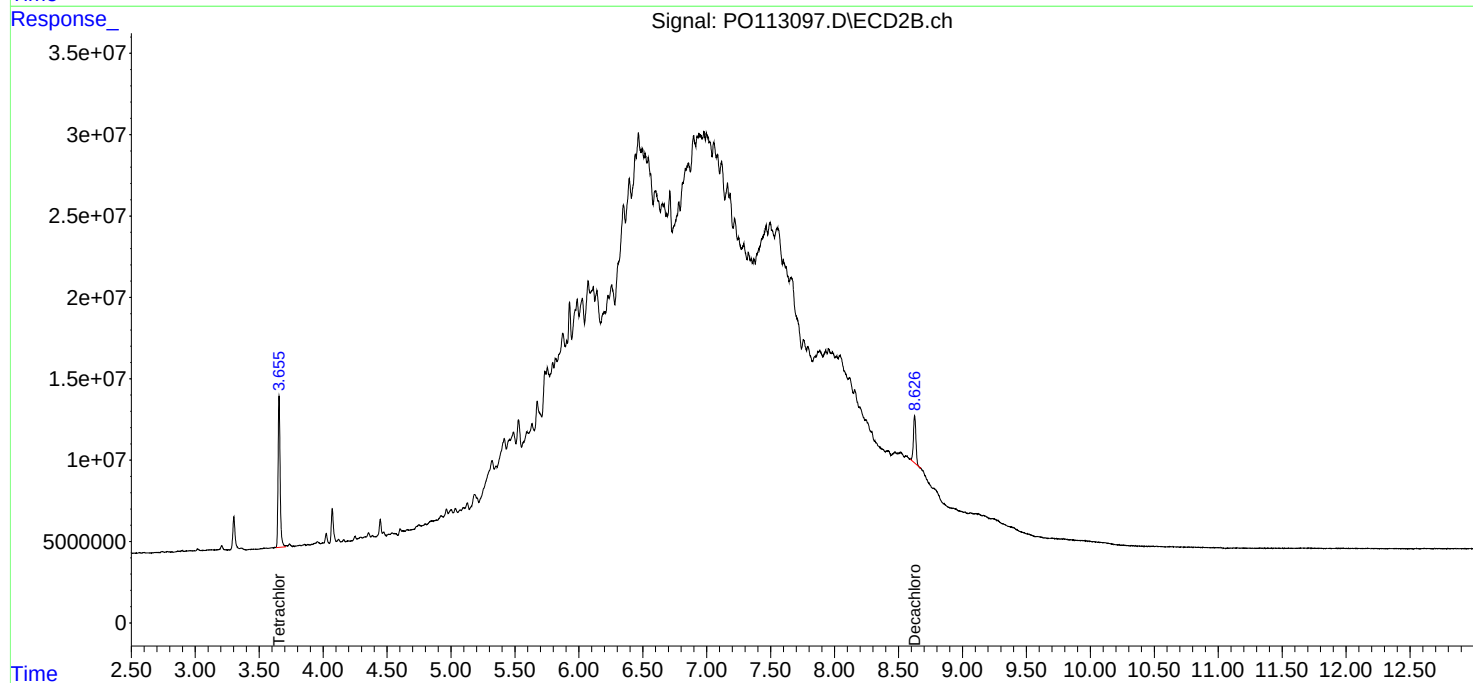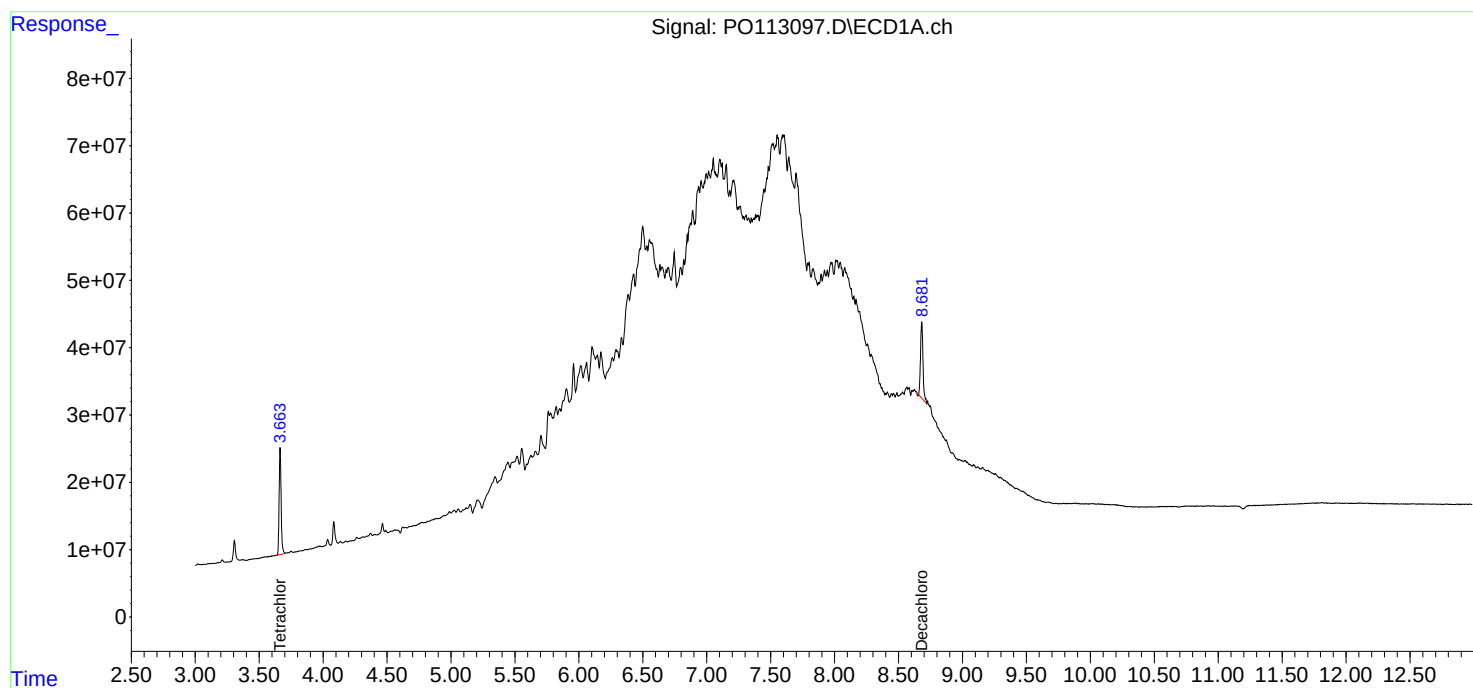


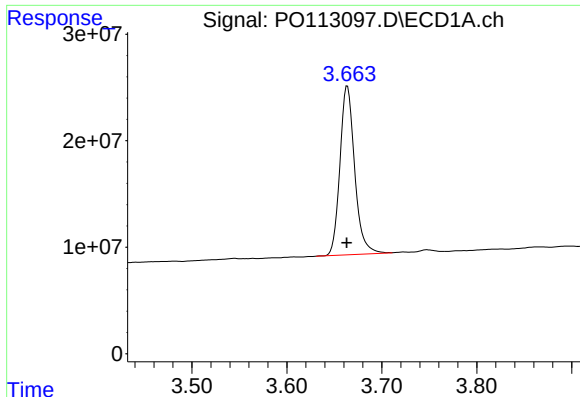

#1 Tetrachloro-m-xylene


R.T.: 3.664 min
Delta R.T.: 0.000 min
Response: 170653264
Conc: 20.85 ng/ml

Instrument :
ECD_O
ClientSampleId :
4A4B4C

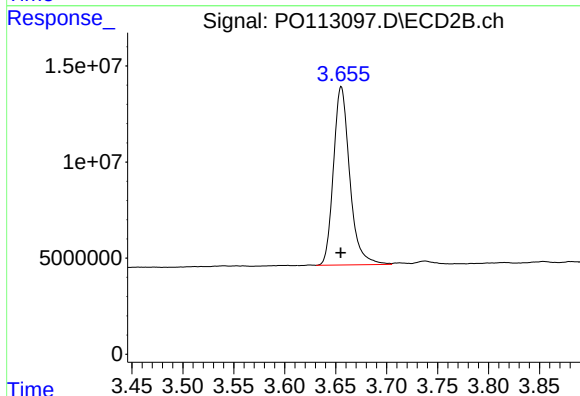


#1 Tetrachloro-m-xylene

R.T.: 3.655 min
Delta R.T.: 0.000 min
Response: 103080458
Conc: 20.37 ng/ml

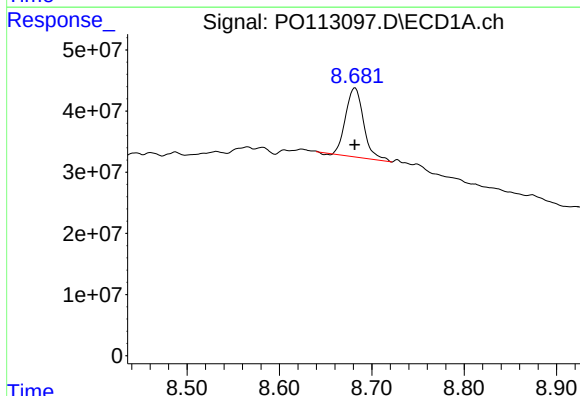

#2 Decachlorobiphenyl

R.T.: 8.682 min
Delta R.T.: 0.000 min
Response: 153215160
Conc: 22.10 ng/ml

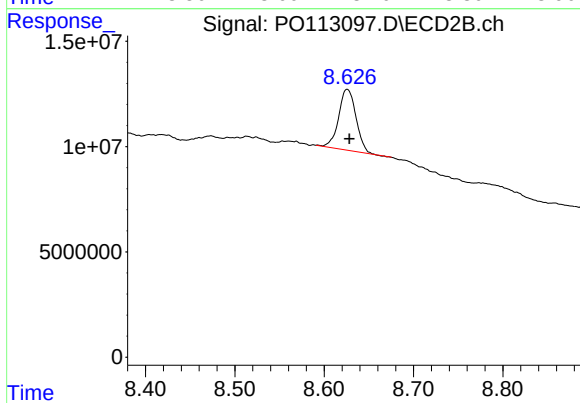

#2 Decachlorobiphenyl

R.T.: 8.626 min
Delta R.T.: -0.003 min
Response: 38895590
Conc: 20.53 ng/ml

Report of Analysis

Client:	ATC Group Services LLC		Date Collected:	08/18/25	
Project:	PS 190 BK - 2025SCA056		Date Received:	08/18/25	
Client Sample ID:	5A5B5C		SDG No.:	Q2894	
Lab Sample ID:	Q2894-05		Matrix:	CAULK	
Analytical Method:	8082A		% Solid:	100	Decanted:
Sample Wt/Vol:	7.8	Units: g	Final Vol:	10000	uL
Soil Aliquot Vol:		uL	Test:	PCB	
Extraction Type:			Injection Volume :		
GPC Factor :	1.0	PH :			
Prep Method :	SW3541B				

File ID/Qc Batch:	Dilution:	Prep Date	Date Analyzed	Prep Batch ID
PO113120.D	1	08/20/25 08:40	08/21/25 10:22	PB169322

CAS Number	Parameter	Conc.	Qualifier	MDL	LOQ / CRQL	Units
TARGETS						
12674-11-2	Aroclor-1016	15.2	U	15.2	65.4	ug/kg
11104-28-2	Aroclor-1221	15.5	U	15.5	65.4	ug/kg
11141-16-5	Aroclor-1232	14.3	U	14.3	65.4	ug/kg
53469-21-9	Aroclor-1242	15.4	U	15.4	65.4	ug/kg
12672-29-6	Aroclor-1248	22.8	U	22.8	65.4	ug/kg
11097-69-1	Aroclor-1254	12.3	U	12.3	65.4	ug/kg
37324-23-5	Aroclor-1262	19.3	U	19.3	65.4	ug/kg
11100-14-4	Aroclor-1268	13.8	U	13.8	65.4	ug/kg
11096-82-5	Aroclor-1260	12.4	U	12.4	65.4	ug/kg
SURROGATES						
877-09-8	Tetrachloro-m-xylene	19.0		32 - 144	95%	SPK: 20
2051-24-3	Decachlorobiphenyl	30.1		32 - 175	151%	SPK: 20

Comments:

U = Not Detected

LOQ = Limit of Quantitation

MDL = Method Detection Limit

LOD = Limit of Detection

E = Value Exceeds Calibration Range

P = Indicates >25% difference for detected concentrations between the two GC columns

Q = indicates LCS control criteria did not meet requirements

M = MS/MSD acceptance criteria did not meet requirements

J = Estimated Value

B = Analyte Found in Associated Method Blank

N = Presumptive Evidence of a Compound

* = Values outside of QC limits

D = Dilution

S = Indicates estimated value where valid five-point calibration was not performed prior to analyte detection in sample.

() = Laboratory InHouse Limit

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO082125\
 Data File : PO113120.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 21 Aug 2025 10:22
 Operator : YP/AJ
 Sample : Q2894-05RE
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 5A5B5C

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 21 11:34:37 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO081825.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Aug 19 06:08:32 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.662	3.654	155.3E6	91639135	18.974	18.108
2) SA Decachlor...	8.679	8.623	207.2E6	57109602	29.889	30.139

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO082125\
Data File : PO113120.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 21 Aug 2025 10:22
Operator : YP/AJ
Sample : Q2894-05RE
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
5A5B5C

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 21 11:34:37 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO081825.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Aug 19 06:08:32 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µm Signal #2 Info : 30M x 0.32mm x 0.25µm

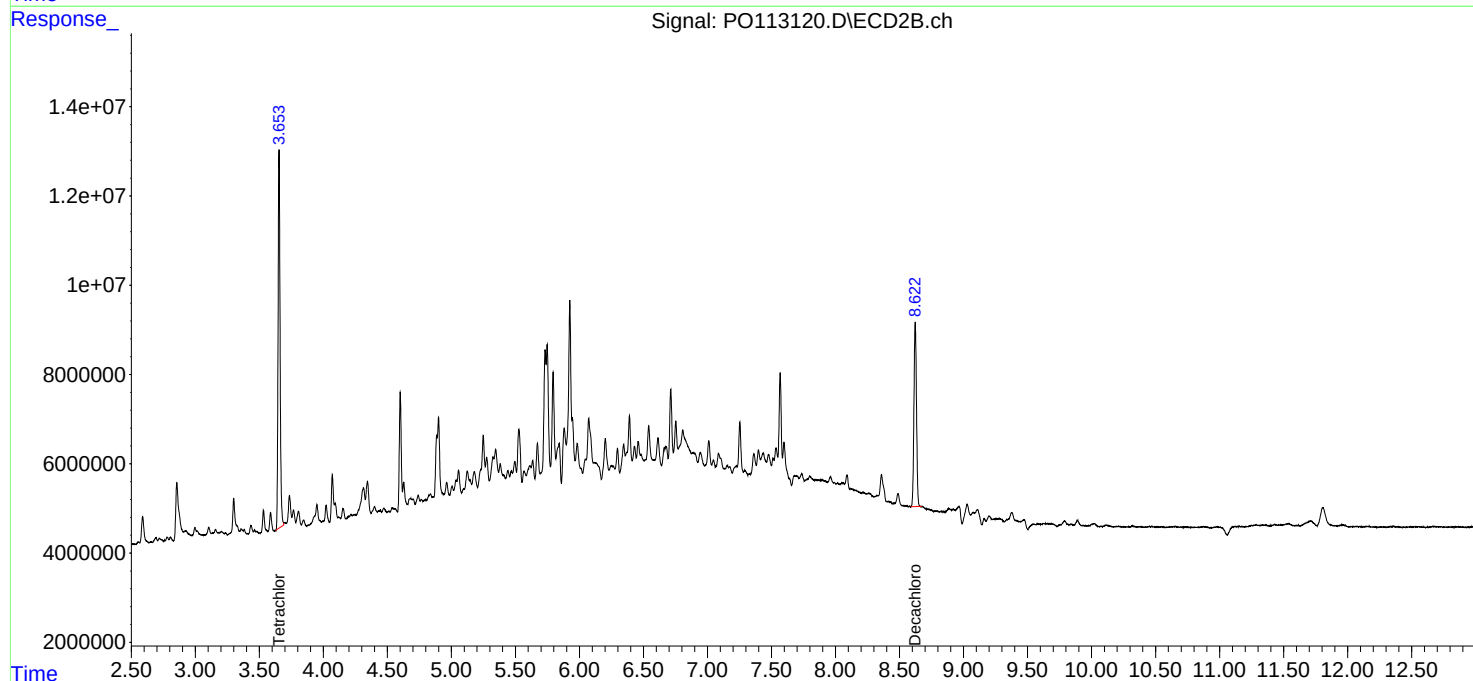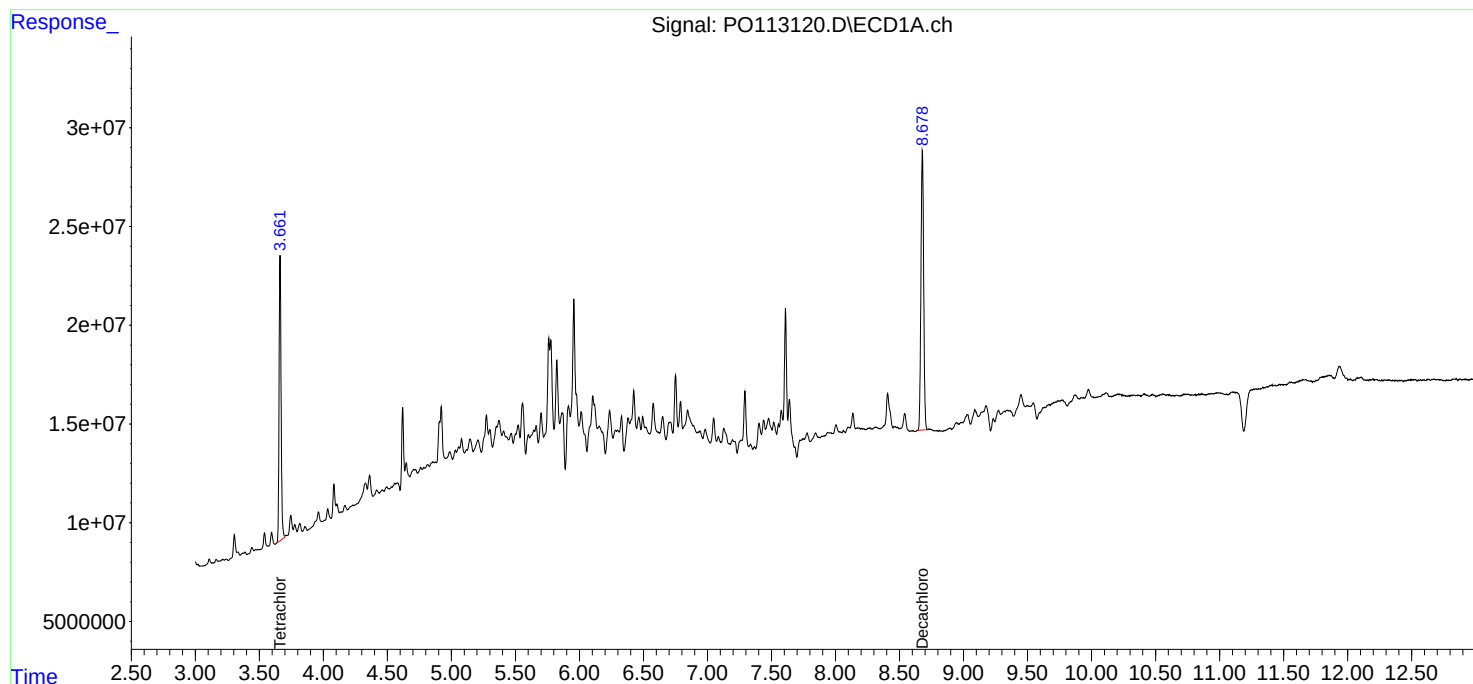


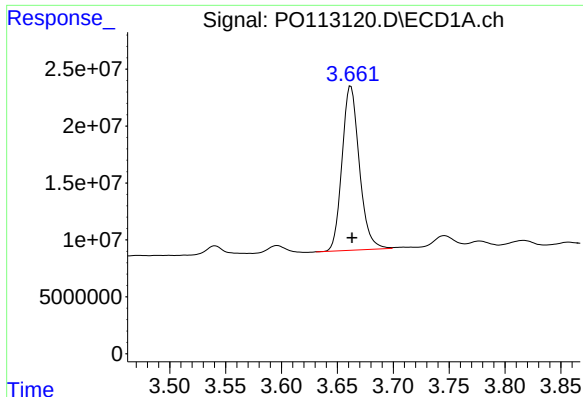

#1 Tetrachloro-m-xylene


R.T.: 3.662 min
Delta R.T.: 0.000 min
Response: 155329004
Conc: 18.97 ng/ml

Instrument :
ECD_O
ClientSampleId :
5A5B5C

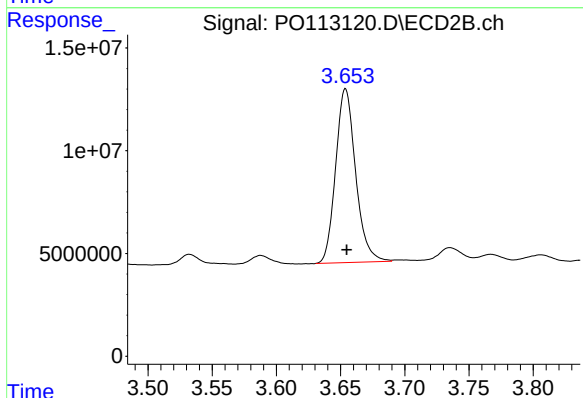


#1 Tetrachloro-m-xylene

R.T.: 3.654 min
Delta R.T.: 0.000 min
Response: 91639135
Conc: 18.11 ng/ml

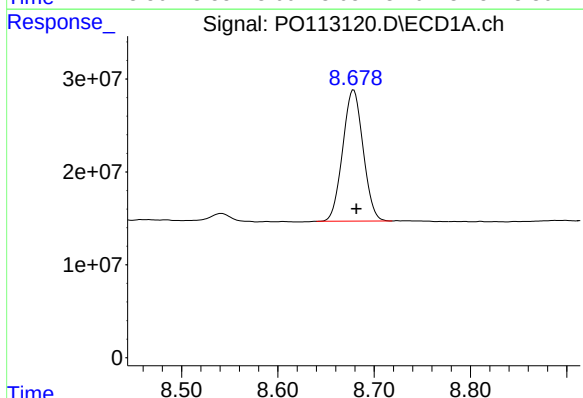

#2 Decachlorobiphenyl

R.T.: 8.679 min
Delta R.T.: -0.003 min
Response: 207173947
Conc: 29.89 ng/ml

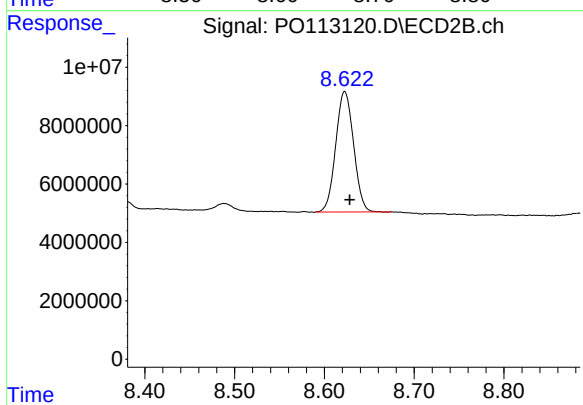

#2 Decachlorobiphenyl

R.T.: 8.623 min
Delta R.T.: -0.006 min
Response: 57109602
Conc: 30.14 ng/ml



CALIBRATION SUMMARY

Calibration Times: 09:53 18:24

LAB FILE ID: RT 1000 = PO113003.D RT 750 = PO113004.D
RT 500 = PO113005.D RT 250 = PO113006.D RT 050 = PO113007.D

[illegible]

[illegible]

Calibration Times: 09:53 18:24

LAB FILE ID: RT 1000 = PO113003.D RT 750 = PO113004.D
RT 500 = PO113005.D RT 250 = PO113006.D RT 050 = PO113007.D

[illegible]

[illegible]



284 Sheffield Street, Mountainside, New Jersey 07092, Phone : 908 789 8900,
Fax : 908 789 8922

CALIBRATION FACTOR OF INITIAL CALIBRATION

Lab Name: Alliance
Lab Code: ACE
Instrument ID: ECD_O

Contract: ATCE02
SDG NO.: Q2894

Calibration Date(s): 08/18/2025 08/18/2025
Calibration Times: 09:53 18:24

GC Column: ZB-MR1 ID: 0.32 (mm)

LAB FILE ID:		CF 1000 = <u>PO113003.D</u>		CF 750 = <u>PO113004.D</u>			
CF 500 = <u>PO113005.D</u>		CF 250 = <u>PO113006.D</u>		CF 050 = <u>PO113007.D</u>			
COMPOUND		CF 1000	CF 750	CF 500	CF 250	CF 050	% RSD
Aroclor-1016-1	(1)	255371052	268882561	275934040	276241276	258494960	266984778
Aroclor-1016-2	(2)	386597005	407445280	416148678	417991420	378975420	401431561
Aroclor-1016-3	(3)	240674907	253345352	260103296	260910040	260078600	255022439
Aroclor-1016-4	(4)	200488933	211018755	217396840	218446060	242989580	218068034
Aroclor-1016-5	(5)	201770173	209979241	223743332	226026380	246620380	221627901
Aroclor-1260-1	(1)	410428218	427895784	448350422	466101308	477127140	445980574
Aroclor-1260-2	(2)	647927331	671777743	694591256	718069576	701240300	686721241
Aroclor-1260-3	(3)	589701211	617064005	642929590	643696764	593976440	617473602
Aroclor-1260-4	(4)	414110693	436180457	452681312	475292936	461106740	447874428
Aroclor-1260-5	(5)	1160238835	1200115325	1238734248	1265998100	1188334440	1210684190
Decachlorobiphenyl		6690212690	6905027373	7141319640	7175759920	6744868400	6931437605
Tetrachloro-m-xylene		8029674340	8350369867	8441238500	8370538000	7741099400	8186584021
Aroclor-1242-1	(1)	219003807	233526197	242788968	240725264	213615160	229931879
Aroclor-1242-2	(2)	327976735	344946825	364718188	364178480	316305340	343625114
Aroclor-1242-3	(3)	205275217	218054489	227356174	226343432	232391780	221884218
Aroclor-1242-4	(4)	165269678	175377872	183337550	185157480	158170880	173462692
Aroclor-1242-5	(5)	180656505	196650337	209535050	215724772	198244940	200162321
Decachlorobiphenyl		6983751120	7199555547	7360295780	7264103480	6074426600	6976426505
Tetrachloro-m-xylene		7902542970	8274474280	8655126880	8517047440	6985096600	8066857634
Aroclor-1248-1	(1)	177555092	181269211	184034788	180488664	148983880	174466327
Aroclor-1248-2	(2)	240102006	246360772	247113578	251916636	223835260	241865650
Aroclor-1248-3	(3)	306109229	315711316	329615046	318673876	324209820	318863857
Aroclor-1248-4	(4)	475546851	491209784	508332020	505821844	517111680	499604436
Aroclor-1248-5	(5)	324226410	338835636	348307430	339859680	356228800	341491591
Decachlorobiphenyl		7181659070	7514737493	7570052300	7529287200	6075985600	7174344333
Tetrachloro-m-xylene		8381826150	8547750707	8588948580	8387451840	6708360600	8122867575
Aroclor-1254-1	(1)	499551241	515351475	527161470	563388796	594438580	539978312
Aroclor-1254-2	(2)	454632825	464341571	479773010	512965400	555557200	493454001
Aroclor-1254-3	(3)	711089310	727800197	738817928	777856740	738821820	738877199
Aroclor-1254-4	(4)	533028449	548551808	553178702	579063696	571175320	556999595
Aroclor-1254-5	(5)	687979747	697879139	702021496	740623884	676364320	700973717
Decachlorobiphenyl		7131515840	7330561920	7448714920	7630980560	6693328400	7247020328
Tetrachloro-m-xylene		8126881990	8349680347	8316489120	8586551360	7297838200	8135488203
Aroclor-1268-1	(1)	1761014831	1774598480	1803892944	1840793296	1424143680	1720888646



284 Sheffield Street, Mountainside, New Jersey 07092, Phone : 908 789 8900,
Fax : 908 789 8922

CALIBRATION FACTOR OF INITIAL CALIBRATION

Aroclor-1268-2	(2)	1477166466	1492439849	1517161498	1547779236	1206191000	1448147610	10
Aroclor-1268-3	(3)	1233609752	1245280741	1270713242	1291388356	990581680	1206314754	10
Aroclor-1268-4	(4)	475808490	479214719	476669802	493044724	378582420	460664031	10
Aroclor-1268-5	(5)	3340543820	3334721212	3351512988	3373775928	2541501700	3188411130	11
Decachlorobiphenyl		13573084670	13653631320	13924005880	14188212680	11035945600	13274976030	10
Tetrachloro-m-xylene		8383283840	8466545813	8477460740	8727640480	6548042000	8120594575	11



284 Sheffield Street, Mountainside, New Jersey 07092, Phone : 908 789 8900,
Fax : 908 789 8922

CALIBRATION FACTOR OF INITIAL CALIBRATION

Lab Name: Alliance
Lab Code: ACE
Instrument ID: ECD_O

Contract: ATCE02
SDG NO.: Q2894

Calibration Date(s): 08/18/2025 08/18/2025
Calibration Times: 09:53 18:24

GC Column: ZB-MR2 ID: 0.32 (mm)

LAB FILE ID:		CF 1000 = <u>PO113003.D</u>		CF 750 = <u>PO113004.D</u>			
CF 500 = <u>PO113005.D</u>		CF 250 = <u>PO113006.D</u>		CF 050 = <u>PO113007.D</u>			
COMPOUND		CF 1000	CF 750	CF 500	CF 250	CF 050	% RSD
Aroclor-1016-1	(1)	157648421	166338757	175029528	179513524	174338440	5
Aroclor-1016-2	(2)	242743120	252380695	260324992	267711416	265120000	4
Aroclor-1016-3	(3)	126993760	133087225	138404134	144167804	155418980	8
Aroclor-1016-4	(4)	100459724	106574292	112469896	119612944	144377780	15
Aroclor-1016-5	(5)	128106279	134710951	142286356	148407360	159139040	8
Aroclor-1260-1	(1)	228928107	240864928	252574738	272240464	280735880	8
Aroclor-1260-2	(2)	313918308	328124507	343910348	357024580	385581120	8
Aroclor-1260-3	(3)	262510074	276701705	293612640	313010736	341333940	10
Aroclor-1260-4	(4)	185941664	193924396	204255296	207408028	244718200	11
Aroclor-1260-5	(5)	425960236	439043723	465902736	470000160	541240260	10
Decachlorobiphenyl		1831064100	1917365987	1985856160	1994289280	1745675200	6
Tetrachloro-m-xylene		4916768960	5105759507	5187285900	5153639000	4939804600	2
Aroclor-1242-1	(1)	133881576	143118904	152394738	156445124	136681500	7
Aroclor-1242-2	(2)	203955870	217199904	228051544	234362648	200985900	7
Aroclor-1242-3	(3)	105689998	114133919	120912152	123685124	120400300	6
Aroclor-1242-4	(4)	101683397	110649877	117620438	123213288	135019900	11
Aroclor-1242-5	(5)	136091884	145976403	155166798	162502892	145926680	7
Decachlorobiphenyl		1868057120	1957140320	2005702880	2020794160	1772529000	5
Tetrachloro-m-xylene		4825813680	5071335853	5270165440	5270477280	4505798600	7
Aroclor-1248-1	(1)	108471143	113278465	116916398	117022156	101871080	6
Aroclor-1248-2	(2)	150794660	157713281	163410186	169101272	162475680	4
Aroclor-1248-3	(3)	159433549	166390719	173042032	176703836	172733300	4
Aroclor-1248-4	(4)	188271317	195815885	204890460	209017568	198105260	4
Aroclor-1248-5	(5)	194018440	203934763	211803632	222502412	229222700	7
Decachlorobiphenyl		1895882940	1980749933	2008729920	2044623040	1730989400	6
Tetrachloro-m-xylene		5046994300	5155202453	5203435340	5076525520	4220137200	8
Aroclor-1254-1	(1)	288848558	302797836	311612874	336218560	337291100	7
Aroclor-1254-2	(2)	255015428	266176108	276603524	303614928	300286060	8
Aroclor-1254-3	(3)	394658183	407977155	416043550	446405672	419527560	5
Aroclor-1254-4	(4)	258230294	268632580	273598908	289141772	284574380	5
Aroclor-1254-5	(5)	325480526	337925896	351521312	371760832	400764340	8
Decachlorobiphenyl		1855582740	1926836507	1973181280	2039405120	1846968600	4
Tetrachloro-m-xylene		4911279290	5066835907	5059128600	5241425160	4670568800	4
Aroclor-1268-1	(1)	505322959	499938980	529404120	551503232	461152840	7



284 Sheffield Street, Mountainside, New Jersey 07092, Phone : 908 789 8900,
Fax : 908 789 8922

CALIBRATION FACTOR OF INITIAL CALIBRATION

Aroclor-1268-2	(2)	411828393	408615411	431678690	446034816	378854460	415402354	6
Aroclor-1268-3	(3)	321714437	321009472	339466898	353051976	297302600	326509077	6
Aroclor-1268-4	(4)	120303152	122244828	123085728	129780148	106749080	120432587	7
Aroclor-1268-5	(5)	793658604	796742752	812678858	835111136	666596880	780957646	8
Decachlorobiphenyl		3468678600	3498241200	3592049560	3737387920	2992120000	3457695456	8
Tetrachloro-m-xylene		5091723140	5143743093	5120936720	5368398520	4128952800	4970750855	10



284 Sheffield Street, Mountainside, New Jersey 07092, Phone : 908 789 8900,
Fax : 908 789 8922

INITIAL CALIBRATION OF MULTICOMPONENT ANALYTES

Lab Name: Alliance **Contract:** ATCE02
Lab Code: ACE **SDG NO.:** Q2894
Instrument ID: ECD_O **Date(s) Analyzed:** 08/18/2025 08/18/2025
GC Column: ZB-MR1 **ID:** 0.32 (mm)

COMPOUND	AMOUNT (ng)	PEAK	RT	RT WINDOW		CALIBRATION FACTOR
				FROM	TO	
Aroclor-1221	500	1	3.87	3.77	3.97	93573200
		2	3.96	3.86	4.06	67550600
		3	4.04	3.94	4.14	221352000
		4	0.00			0
		5	0.00			0
Aroclor-1232	500	1	4.04	3.94	4.14	174006000
		2	4.53	4.43	4.63	99852400
		3	4.77	4.67	4.87	189475000
		4	4.94	4.84	5.04	94169600
		5	4.99	4.89	5.09	61943000
Aroclor-1262	500	1	6.79	6.69	6.89	915764000
		2	7.29	7.19	7.39	1512160000
		3	7.58	7.48	7.68	554108000
		4	7.64	7.54	7.74	977968000
		5	8.14	8.04	8.24	416878000



284 Sheffield Street, Mountainside, New Jersey 07092, Phone : 908 789 8900,
Fax : 908 789 8922

INITIAL CALIBRATION OF MULTICOMPONENT ANALYTES

Lab Name: Alliance **Contract:** ATCE02
Lab Code: ACE **SDG NO.:** Q2894
Instrument ID: ECD_O **Date(s) Analyzed:** 08/18/2025 08/18/2025
GC Column: ZB-MR2 **ID:** 0.32 (mm)

COMPOUND	AMOUNT (ng)	PEAK	RT	RT WINDOW		CALIBRATION FACTOR
				FROM	TO	
Aroclor-1221	500	1	3.86	3.76	3.96	63121200
		2	3.95	3.85	4.05	46673200
		3	4.02	3.92	4.12	148475000
		4	0.00			0
		5	0.00			0
Aroclor-1232	500	1	4.02	3.92	4.12	117403000
		2	4.75	4.65	4.85	122545000
		3	4.92	4.82	5.02	63345600
		4	5.01	4.91	5.11	56221200
		5	5.18	5.08	5.28	59863600
Aroclor-1262	500	1	6.76	6.66	6.86	414614000
		2	7.26	7.16	7.36	517670000
		3	7.54	7.44	7.64	179590000
		4	7.60	7.50	7.70	289902000
		5	8.09	7.99	8.19	108331000

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0081825\
 Data File : P0113003.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 18 Aug 2025 09:53
 Operator : YP/AJ
 Sample : AR1660ICC1000
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 AR1660ICC1000

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 18 10:58:58 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0081825.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Mon Aug 18 10:55:18 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.663	3.655	803.0E6	491.7E6	97.501	97.323
2) SA Decachlor...	8.682	8.628	669.0E6	183.1E6	96.739	95.945
Target Compounds						
3) L1 AR-1016-1	4.748	4.729	255.4E6	157.6E6	961.297	947.754
4) L1 AR-1016-2	4.767	4.747	386.6E6	242.7E6	963.187	965.051
5) L1 AR-1016-3	4.823	4.922	240.7E6	127.0E6	961.204	957.007
6) L1 AR-1016-4	4.943	4.964	200.5E6	100.5E6	959.539	943.596
7) L1 AR-1016-5	5.200	5.176	201.8E6	128.1E6	948.361	947.557
31) L7 AR-1260-1	6.236	6.204	410.4E6	228.9E6	955.842	950.890
32) L7 AR-1260-2	6.425	6.393	647.9E6	313.9E6	965.242	954.408
33) L7 AR-1260-3	6.792	6.544	589.7E6	262.5E6	956.817	944.072
34) L7 AR-1260-4	7.050	7.013	414.1E6	185.9E6	955.502	953.066
35) L7 AR-1260-5	7.294	7.255	1160.2E6	426.0E6	967.280	955.215



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO081825\
Data File : PO113003.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 18 Aug 2025 09:53
Operator : YP/AJ
Sample : AR1660ICC1000
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
AR1660ICC1000

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 18 10:58:58 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO081825.M
Quant Title : GC EXTRACTABLES
QLast Update : Mon Aug 18 10:55:18 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

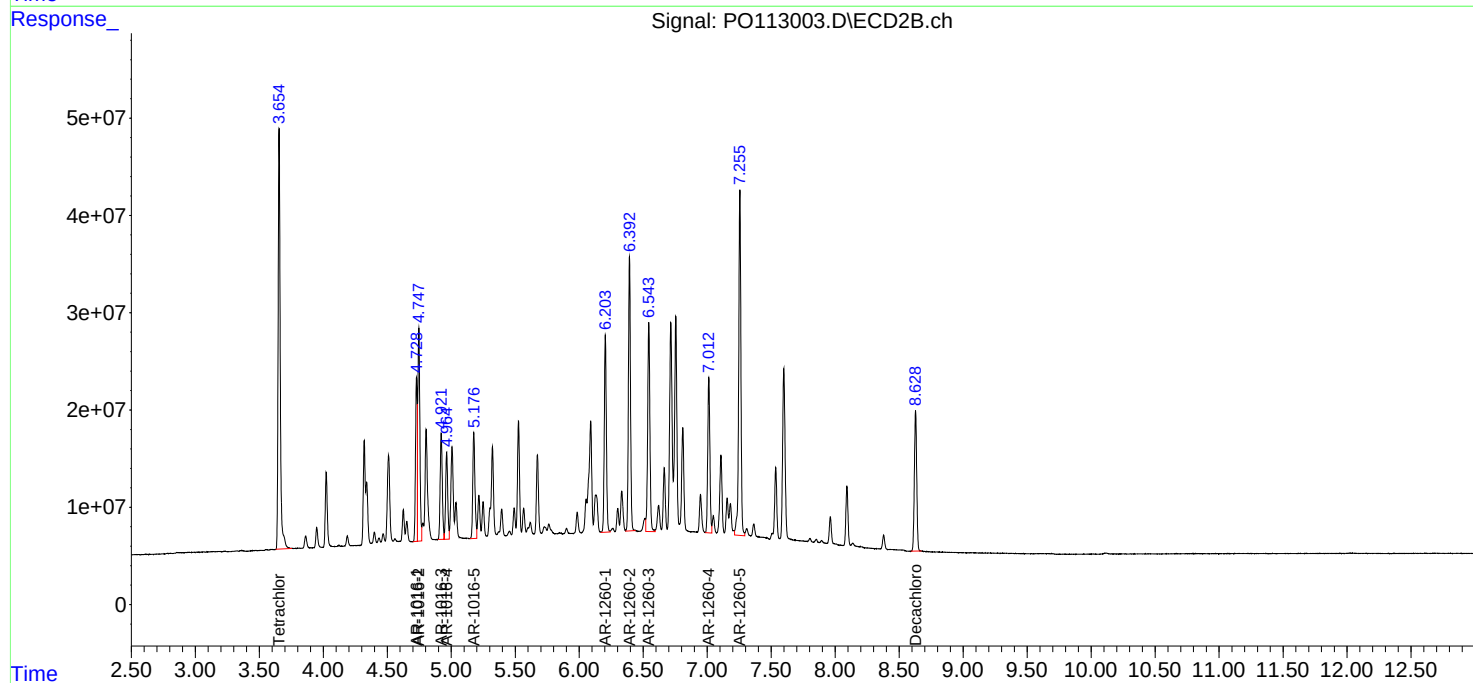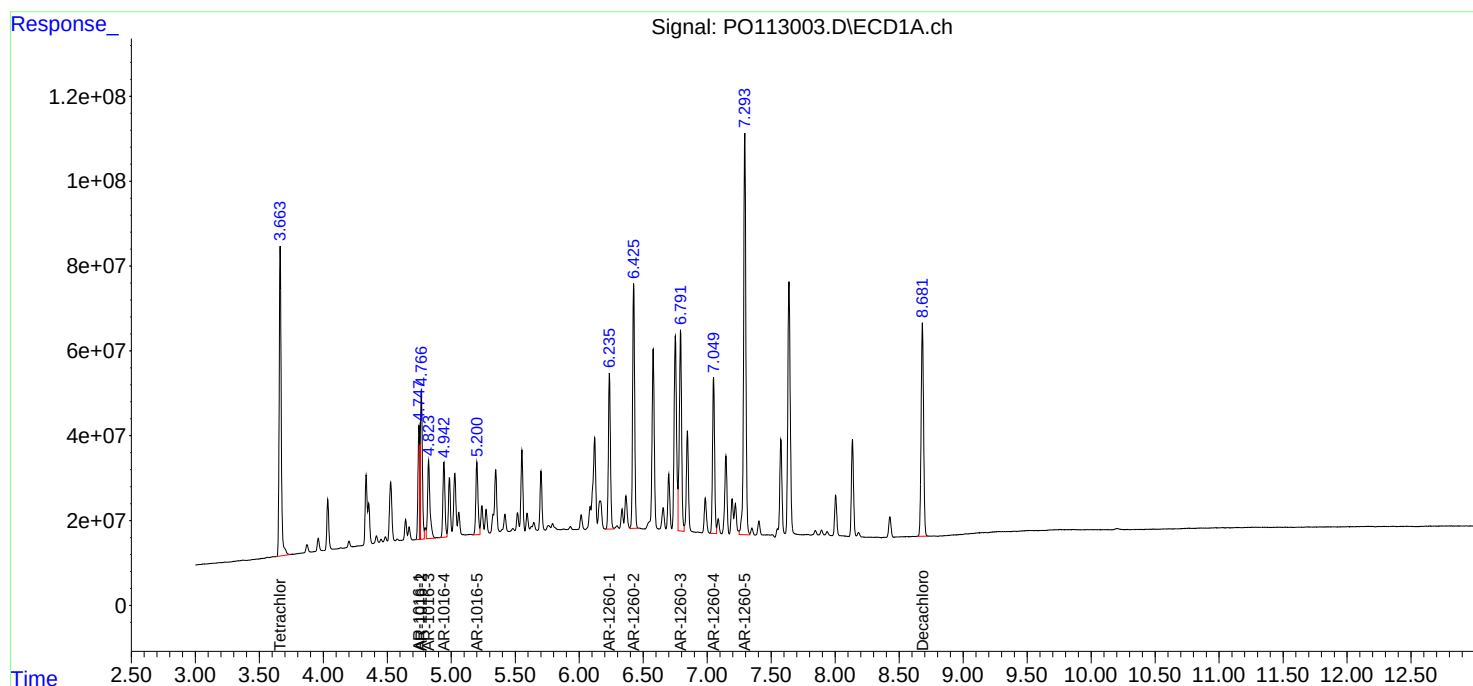

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0081825\
 Data File : P0113004.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 18 Aug 2025 10:11
 Operator : YP/AJ
 Sample : AR1660ICC750
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 AR1660ICC750

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 18 11:02:18 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0081825.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Mon Aug 18 10:55:18 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.663	3.655	626.3E6	382.9E6	75.694	75.530
2) SA Decachlor...	8.682	8.629	517.9E6	143.8E6	74.922	75.233
Target Compounds						
3) L1 AR-1016-1	4.747	4.729	201.7E6	124.8E6	756.055	749.999
4) L1 AR-1016-2	4.766	4.747	305.6E6	189.3E6	757.527	751.681
5) L1 AR-1016-3	4.823	4.922	190.0E6	99815419	755.880	751.462
6) L1 AR-1016-4	4.942	4.965	158.3E6	79930719	754.951	750.514
7) L1 AR-1016-5	5.199	5.177	157.5E6	101.0E6	743.444	748.203
31) L7 AR-1260-1	6.236	6.204	320.9E6	180.6E6	748.259	750.236
32) L7 AR-1260-2	6.426	6.393	503.8E6	246.1E6	750.386	748.798
33) L7 AR-1260-3	6.792	6.544	462.8E6	207.5E6	750.607	747.551
34) L7 AR-1260-4	7.050	7.014	327.1E6	145.4E6	753.206	746.985
35) L7 AR-1260-5	7.294	7.255	900.1E6	329.3E6	750.262	742.237



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO081825\
Data File : PO113004.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 18 Aug 2025 10:11
Operator : YP/AJ
Sample : AR1660ICC750
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
AR1660ICC750

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 18 11:02:18 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO081825.M
Quant Title : GC EXTRACTABLES
QLast Update : Mon Aug 18 10:55:18 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

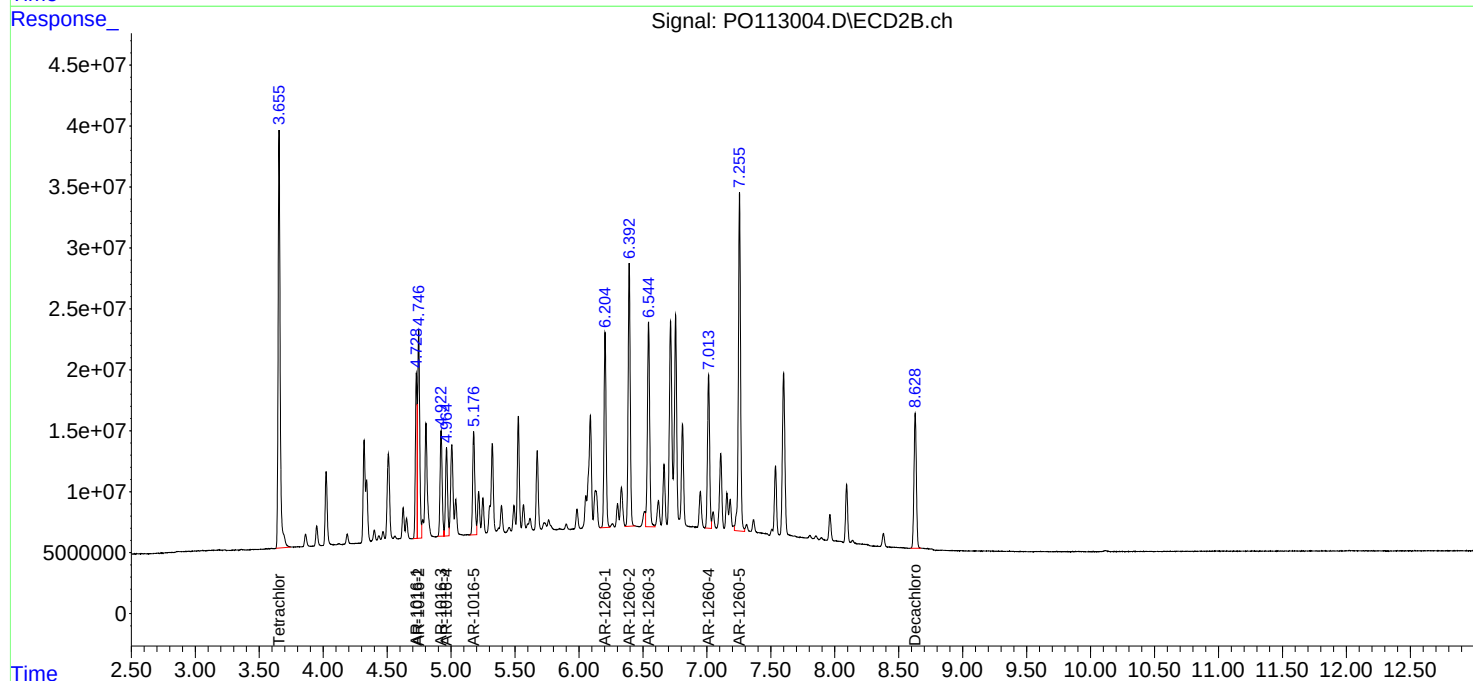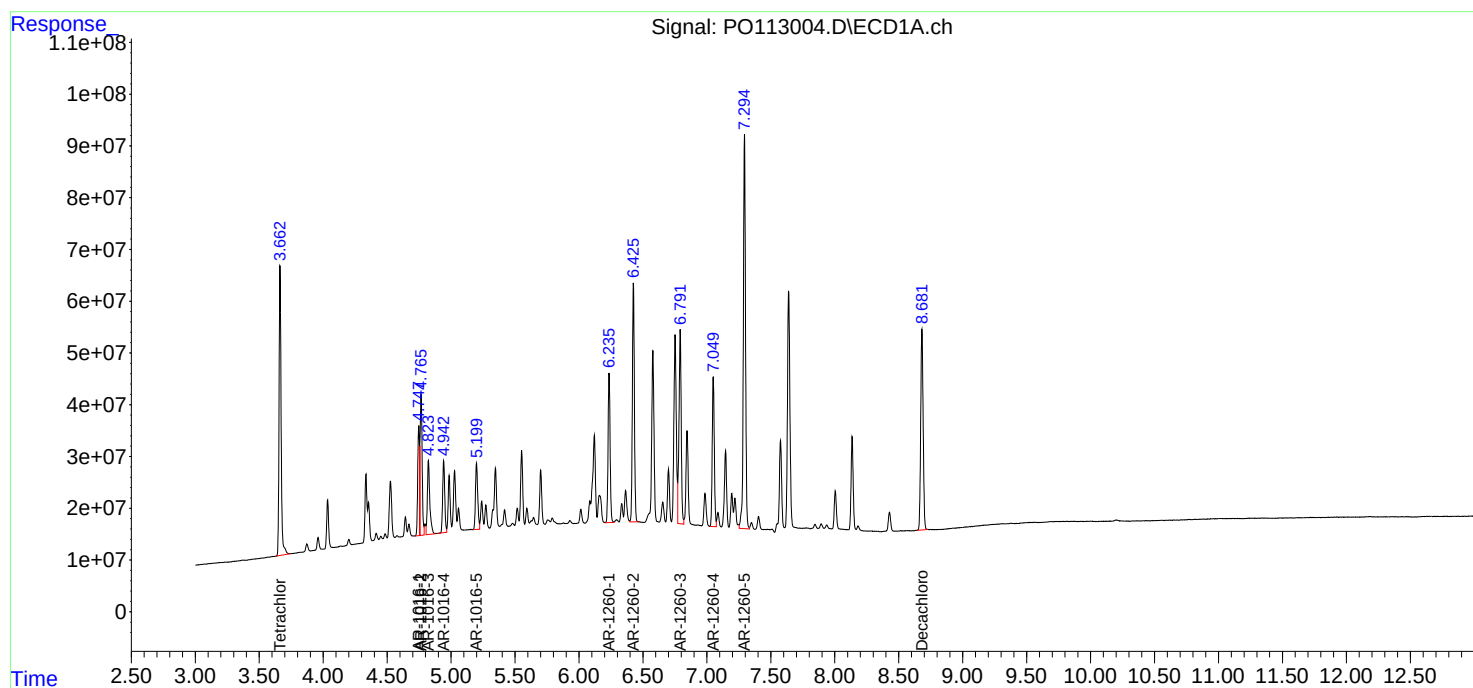

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0081825\
 Data File : P0113005.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 18 Aug 2025 10:29
 Operator : YP/AJ
 Sample : AR1660ICC500
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 AR1660ICC500

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 18 10:55:42 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0081825.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Mon Aug 18 10:55:18 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.663	3.655	422.1E6	259.4E6	50.000	50.000
2) SA Decachlor...	8.682	8.628	357.1E6	99292808	50.000	50.000
Target Compounds						
3) L1 AR-1016-1	4.748	4.729	138.0E6	87514764	500.000	500.000
4) L1 AR-1016-2	4.766	4.747	208.1E6	130.2E6	500.000	500.000
5) L1 AR-1016-3	4.824	4.922	130.1E6	69202067	500.000	500.000
6) L1 AR-1016-4	4.943	4.964	108.7E6	56234948	500.000	500.000
7) L1 AR-1016-5	5.199	5.176	111.9E6	71143178	500.000	500.000
31) L7 AR-1260-1	6.236	6.204	224.2E6	126.3E6	500.000	500.000
32) L7 AR-1260-2	6.426	6.392	347.3E6	172.0E6	500.000	500.000
33) L7 AR-1260-3	6.791	6.543	321.5E6	146.8E6	500.000	500.000
34) L7 AR-1260-4	7.051	7.012	226.3E6	102.1E6	500.000	500.000
35) L7 AR-1260-5	7.294	7.255	619.4E6	233.0E6	500.000	500.000



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO081825\
Data File : PO113005.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 18 Aug 2025 10:29
Operator : YP/AJ
Sample : AR1660ICC500
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
AR1660ICC500

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 18 10:55:42 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO081825.M
Quant Title : GC EXTRACTABLES
QLast Update : Mon Aug 18 10:55:18 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

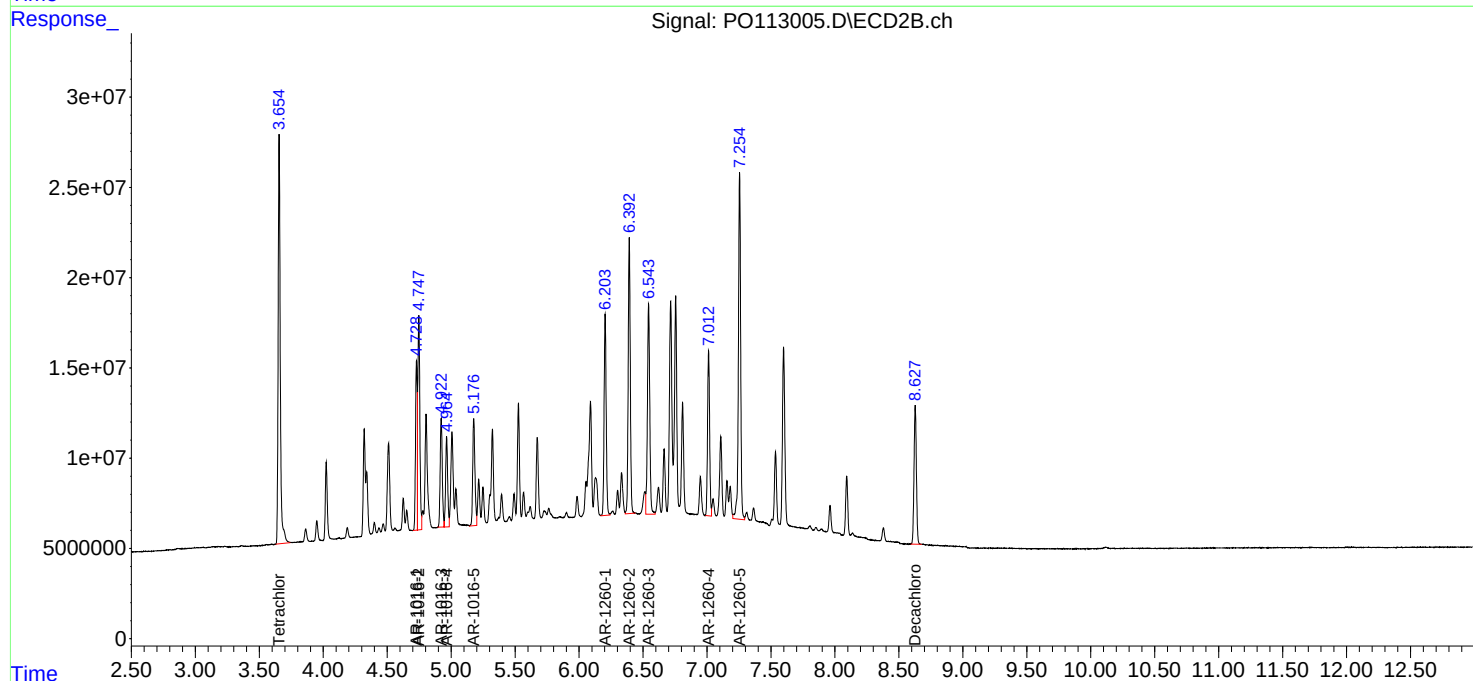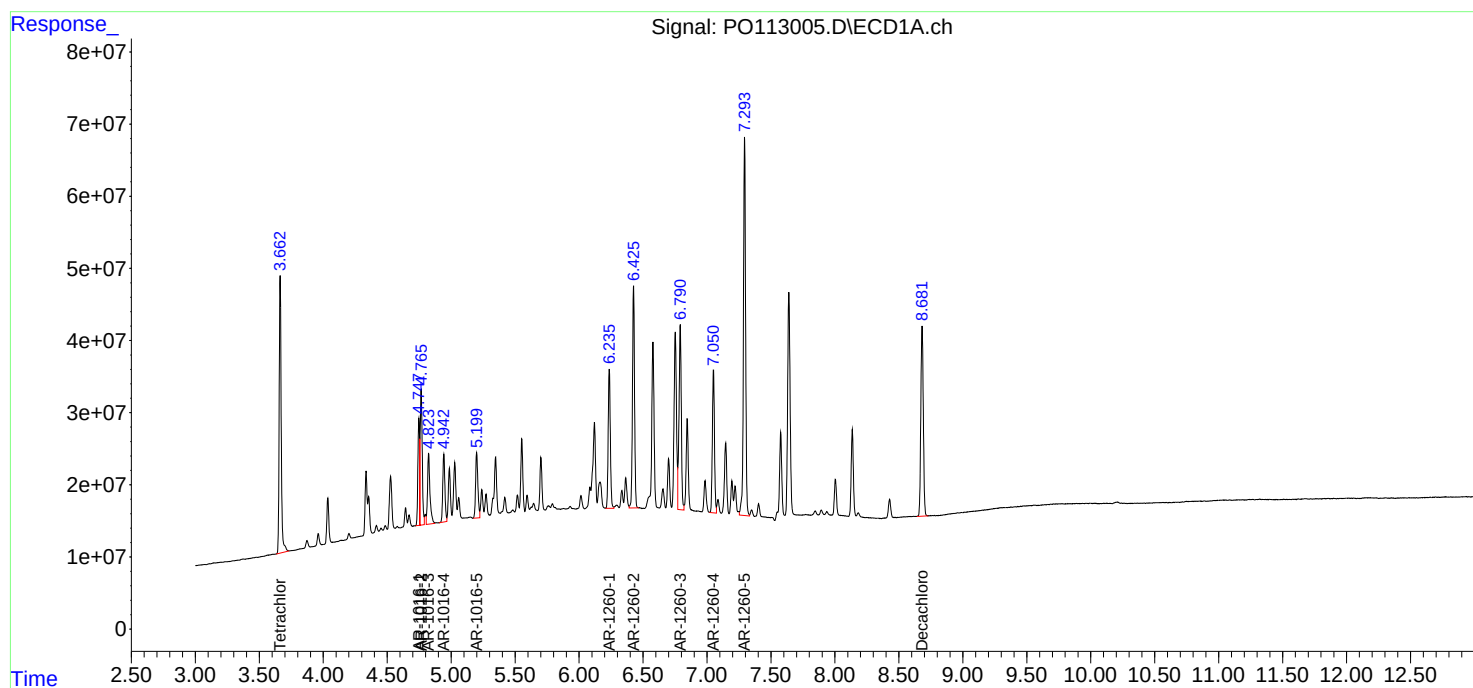

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0081825\
 Data File : P0113006.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 18 Aug 2025 10:48
 Operator : YP/AJ
 Sample : AR1660ICC250
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 AR1660ICC250

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 18 11:05:44 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0081825.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Mon Aug 18 10:55:18 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.663	3.655	209.3E6	128.8E6	25.219	25.308
2) SA Decachlor...	8.682	8.628	179.4E6	49857232	25.708	25.804
Target Compounds						
3) L1 AR-1016-1	4.748	4.729	69060319	44878381	256.628	264.562
4) L1 AR-1016-2	4.767	4.747	104.5E6	66927854	256.723	261.652
5) L1 AR-1016-3	4.824	4.922	65227510	36041951	257.046	265.672
6) L1 AR-1016-4	4.943	4.965	54611515	29903236	257.799	272.394
7) L1 AR-1016-5	5.200	5.176	56506595	37101840	262.358	268.120
31) L7 AR-1260-1	6.236	6.204	116.5E6	68060116	265.922	273.716
32) L7 AR-1260-2	6.426	6.392	179.5E6	89256145	262.801	265.845
33) L7 AR-1260-3	6.792	6.543	160.9E6	78252684	258.161	273.173
34) L7 AR-1260-4	7.051	7.013	118.8E6	51852007	267.279	262.035
35) L7 AR-1260-5	7.293	7.255	316.5E6	117.5E6	260.221	260.980


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO081825\
Data File : PO113006.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 18 Aug 2025 10:48
Operator : YP/AJ
Sample : AR1660ICC250
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
AR1660ICC250

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 18 11:05:44 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO081825.M
Quant Title : GC EXTRACTABLES
QLast Update : Mon Aug 18 10:55:18 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

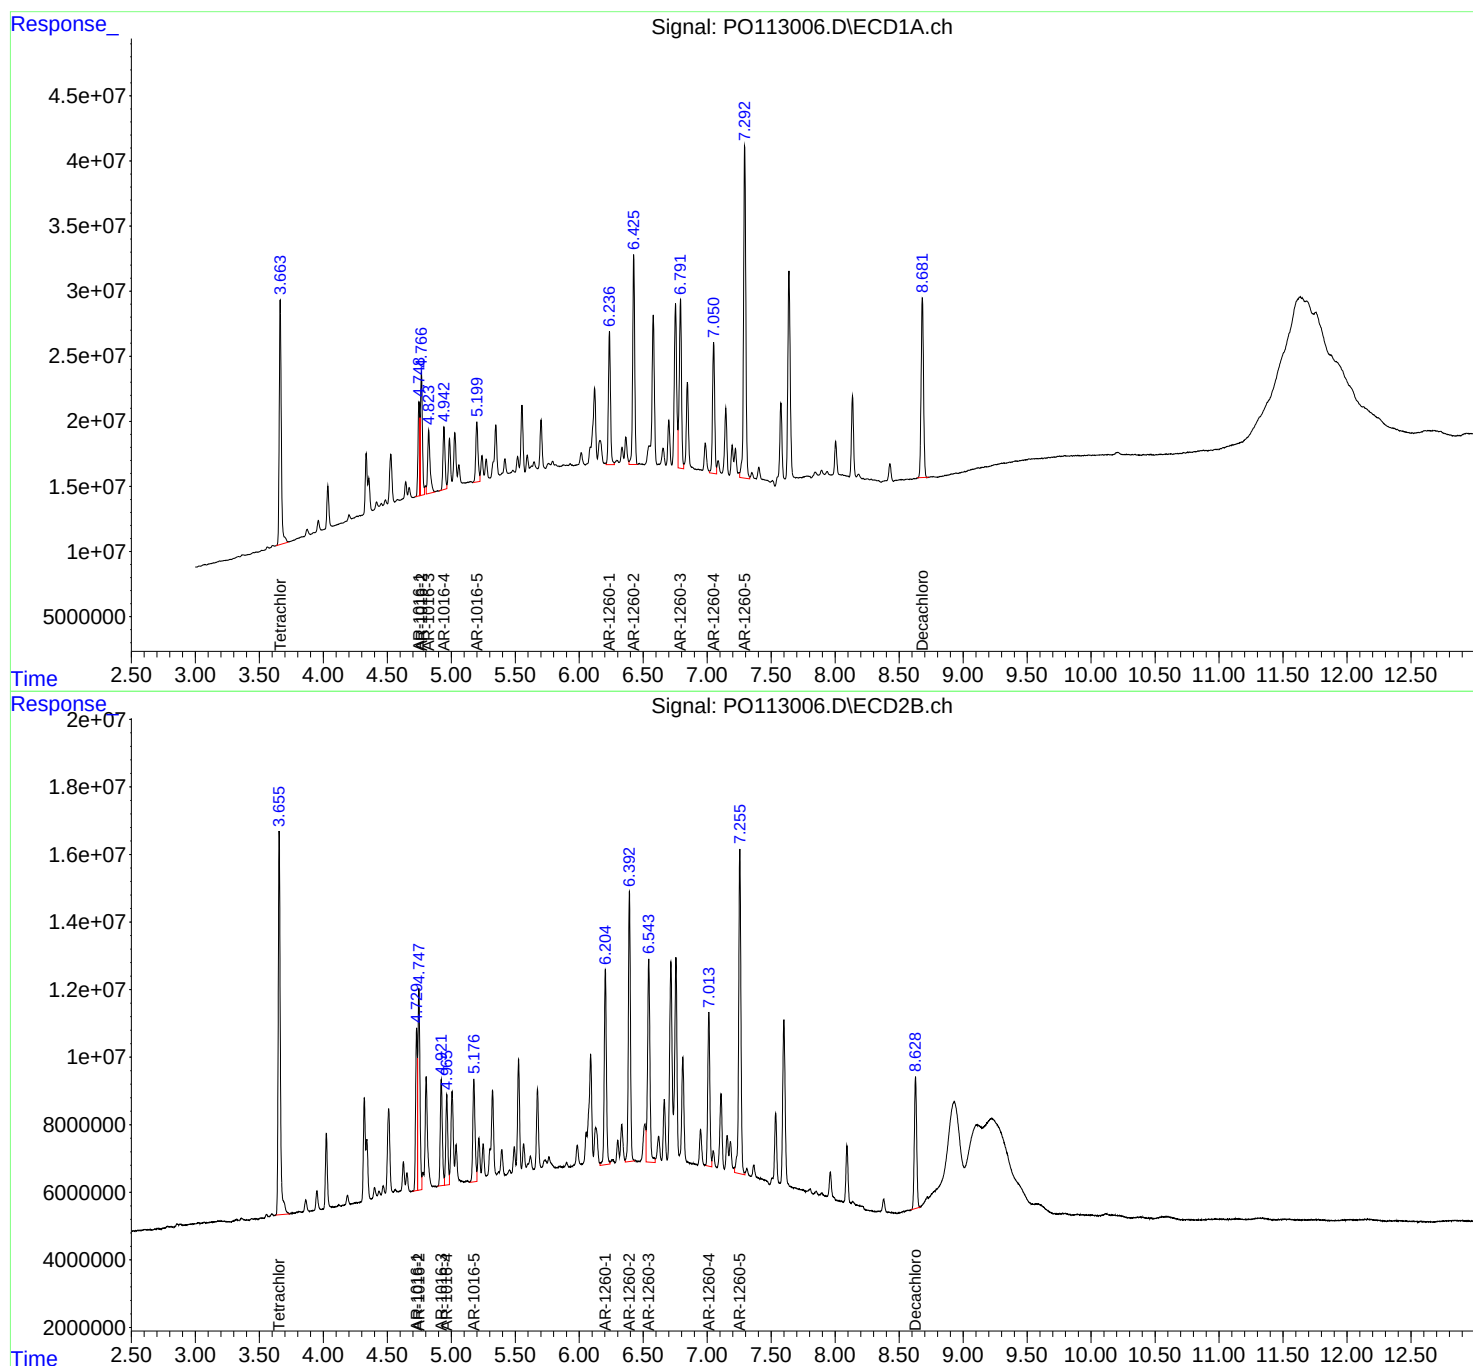

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0081825\
 Data File : P0113007.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 18 Aug 2025 11:06
 Operator : YP/AJ
 Sample : AR1660ICC050
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 AR1660ICC050

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 08/19/2025
 Supervised By :mohammad ahmed 08/20/2025

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 18 11:21:45 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0081825.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Mon Aug 18 11:21:34 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.663	3.654	38705497	24699023	4.728	4.881
2) SA Decachlor...	8.681	8.626	33724342	8728376	4.865	4.606
Target Compounds						
3) L1 AR-1016-1	4.747	4.728	12924748	8716922	48.963	51.104
4) L1 AR-1016-2	4.765	4.747	18948771	13256000	47.203	51.448
5) L1 AR-1016-3	4.823	4.922	13003930	7770949	50.991	55.660
6) L1 AR-1016-4	4.942	4.964	12149479	7218889	55.714	61.859
7) L1 AR-1016-5	5.199	5.176	12331019	7956952	55.638	55.827
31) L7 AR-1260-1	6.234	6.203	23856357	14036794	53.268m	55.031
32) L7 AR-1260-2	6.424	6.391	35062015	19279056	50.038m	55.766
33) L7 AR-1260-3	6.790	6.542	29698822	17066697	48.097	57.515m
34) L7 AR-1260-4	7.049	7.011	23055337	12235910	51.477	59.040
35) L7 AR-1260-5	7.292	7.253	59416722	27062013	49.077	57.772

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO081825\
Data File : PO113007.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 18 Aug 2025 11:06
Operator : YP/AJ
Sample : AR1660ICC050
Misc :
ALS Vial : 7 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
AR1660ICC050

Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 08/19/2025
Supervised By :mohammad ahmed 08/20/2025

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 18 11:21:45 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO081825.M
Quant Title : GC EXTRACTABLES
QLast Update : Mon Aug 18 11:21:34 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

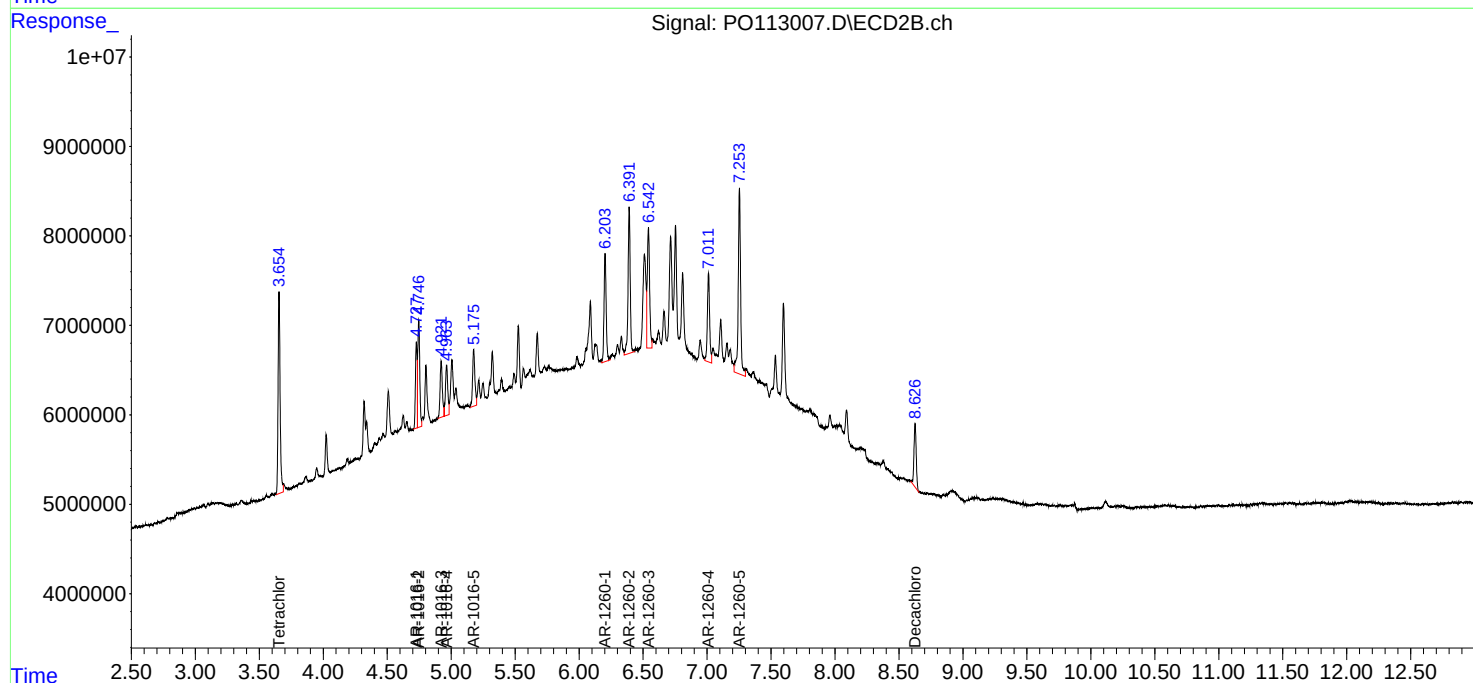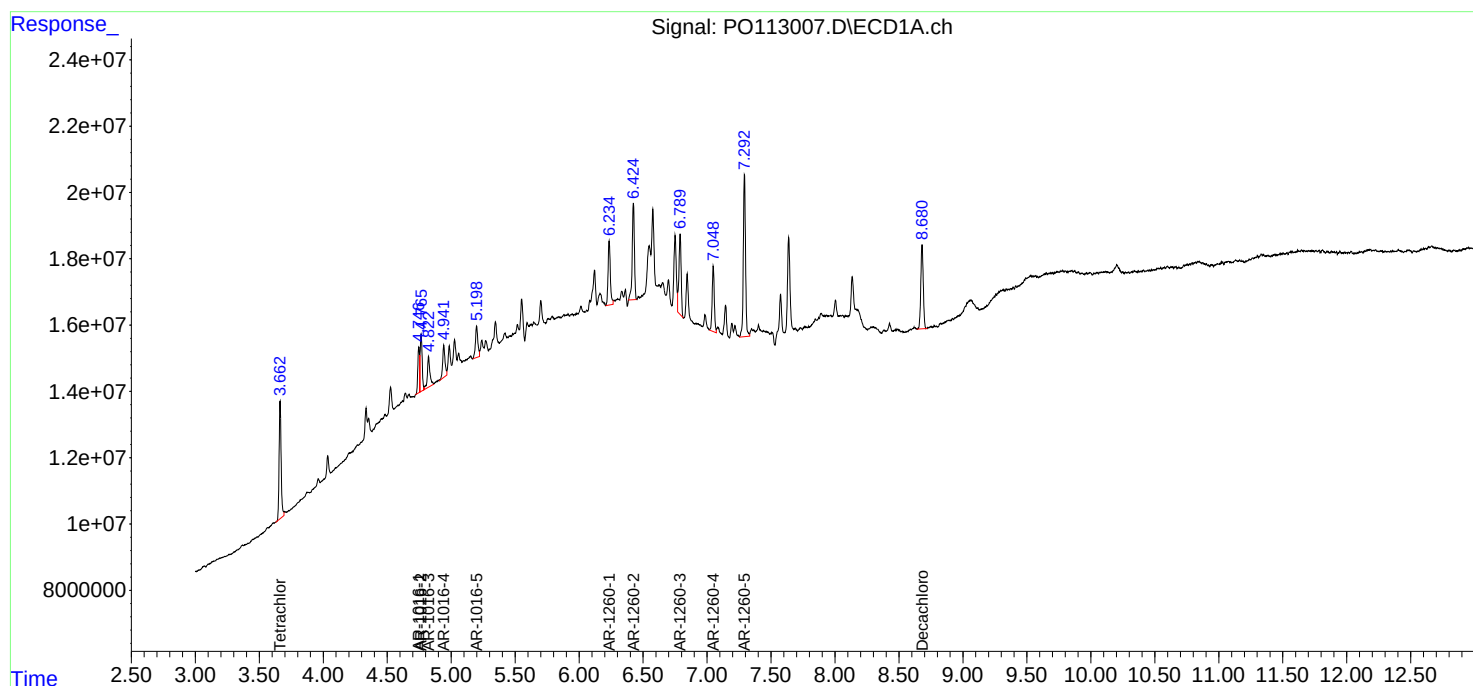

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0081825\
 Data File : P0113008.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 18 Aug 2025 11:25
 Operator : YP/AJ
 Sample : AR1221ICC500
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 AR1221ICC500

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 19 04:47:42 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0081825.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Aug 19 04:47:23 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.663	3.655	413.6E6	254.0E6	50.000	50.000
2) SA Decachlor...	8.682	8.627	342.9E6	94957632	50.000	50.000
Target Compounds						
8) L2 AR-1221-1	3.874	3.864	46786628	31560573	500.000	500.000
9) L2 AR-1221-2	3.960	3.950	33775329	23336608	500.000	500.000
10) L2 AR-1221-3	4.036	4.024	110.7E6	74237501	500.000	500.000



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO081825\
Data File : PO113008.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 18 Aug 2025 11:25
Operator : YP/AJ
Sample : AR1221ICC500
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
AR1221ICC500

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 19 04:47:42 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO081825.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Aug 19 04:47:23 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µm Signal #2 Info : 30M x 0.32mm x 0.25µm

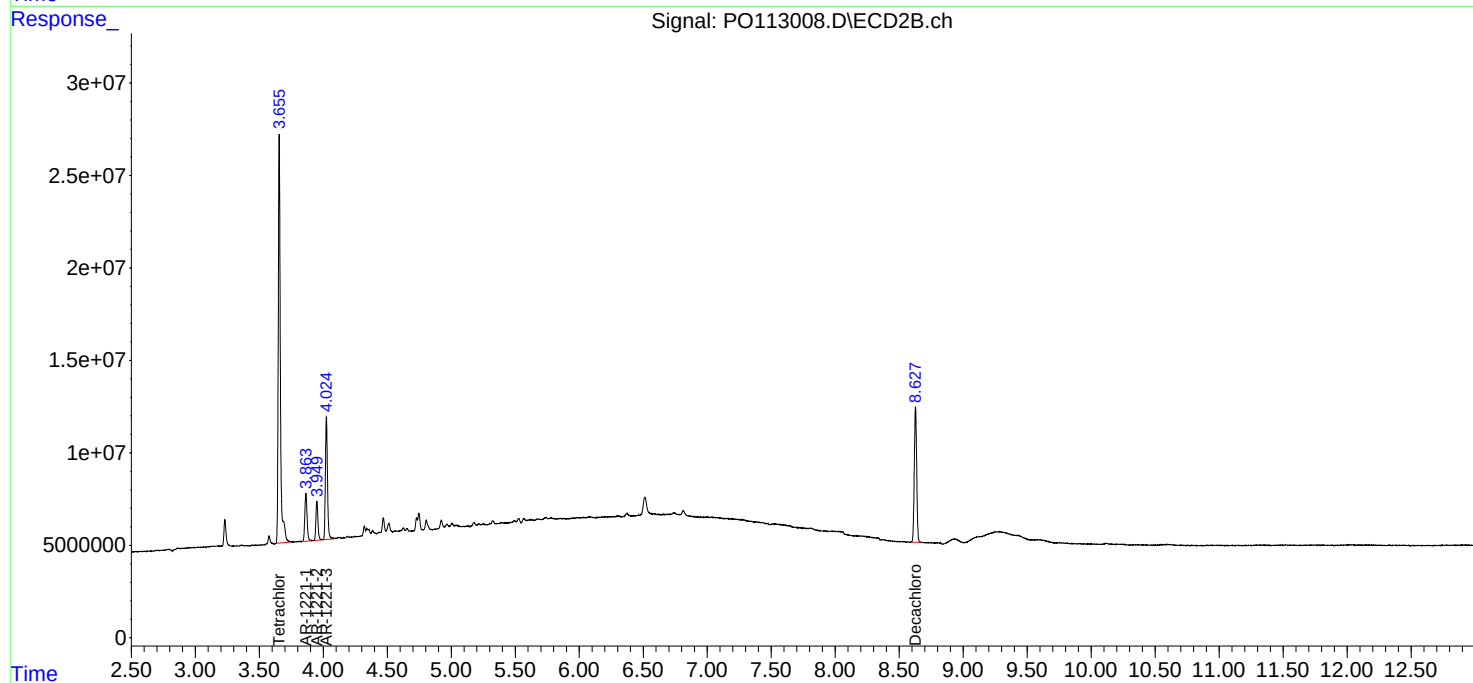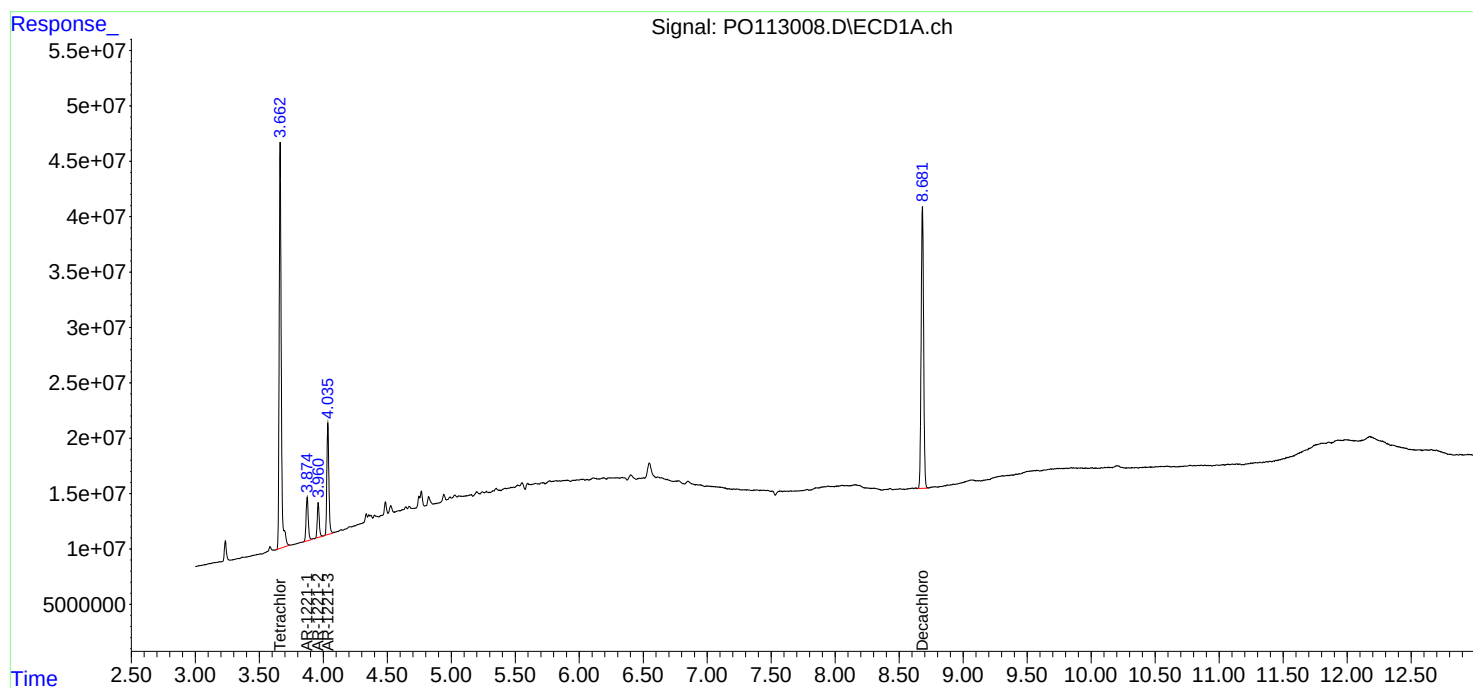

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0081825\
 Data File : P0113009.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 18 Aug 2025 11:43
 Operator : YP/AJ
 Sample : AR1232ICC500
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 AR1232ICC500

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 19 04:57:15 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0081825.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Aug 19 04:57:01 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.663	3.655	425.2E6	260.6E6	50.000	50.000
2) SA Decachlor...	8.682	8.628	358.9E6	97760702	50.000	50.000
Target Compounds						
11) L3 AR-1232-1	4.036	4.023	87003202	58701316	500.000	500.000
12) L3 AR-1232-2	4.527	4.747	49926230	61272548	500.000	500.000
13) L3 AR-1232-3	4.767	4.922	94737736	31672814	500.000	500.000
14) L3 AR-1232-4	4.942	5.006	47084775	28110590	500.000	500.000
15) L3 AR-1232-5	4.986	5.176	30971484	29931775	500.000	500.000



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO081825\
Data File : PO113009.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 18 Aug 2025 11:43
Operator : YP/AJ
Sample : AR1232ICC500
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
AR1232ICC500

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 19 04:57:15 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO081825.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Aug 19 04:57:01 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

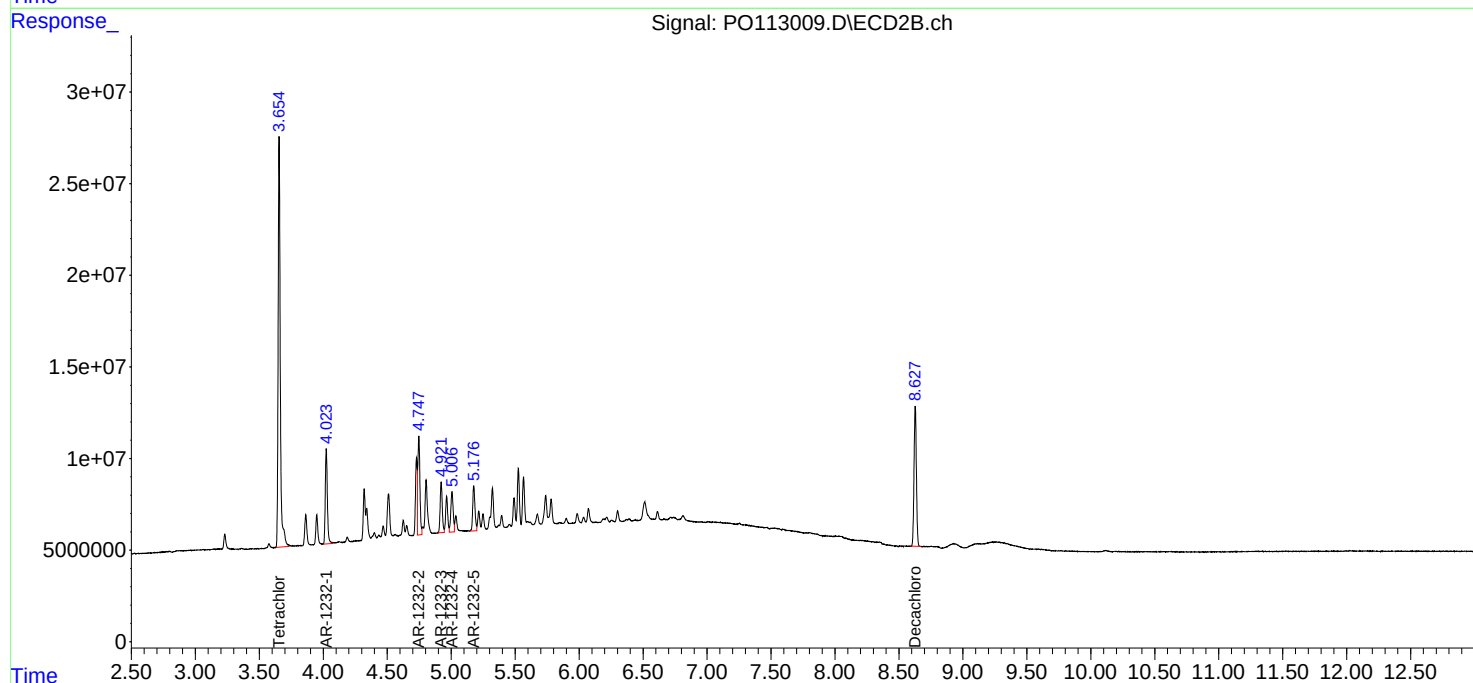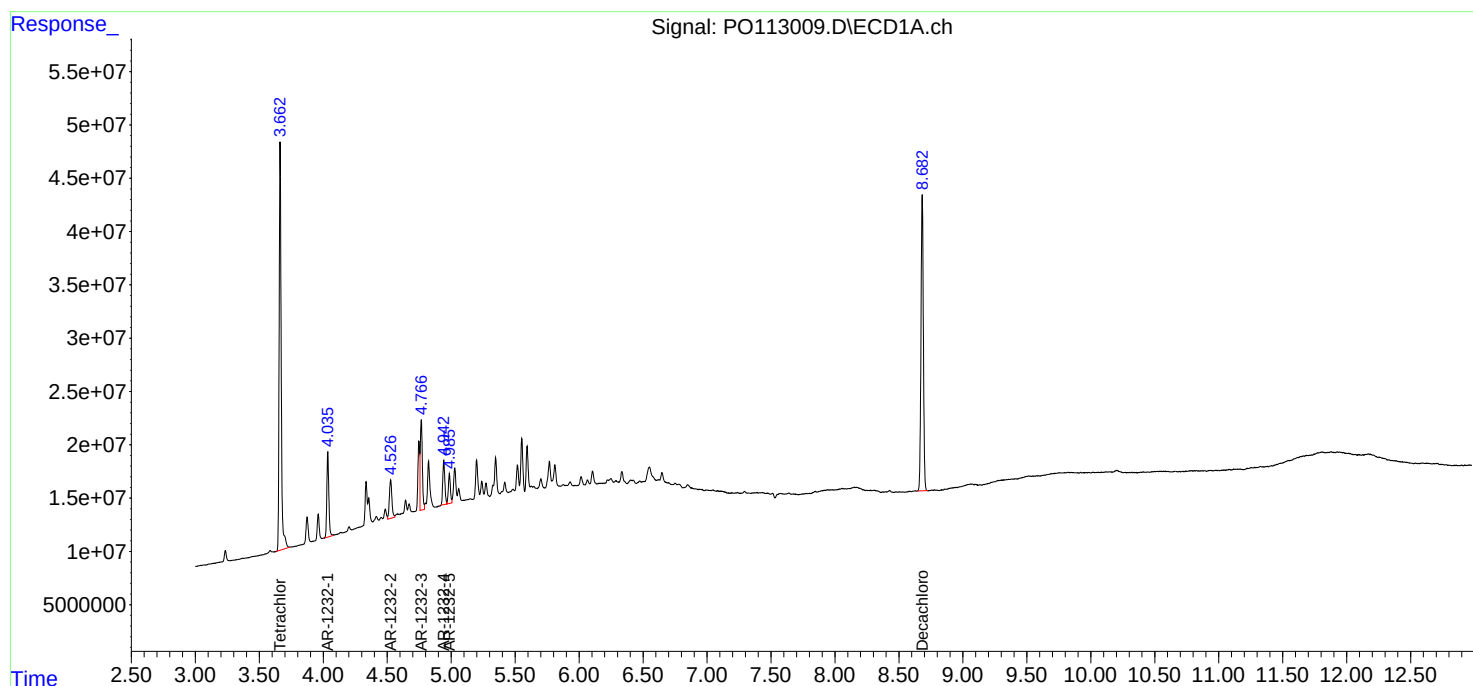

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0081825\
 Data File : P0113010.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 18 Aug 2025 12:01
 Operator : YP/AJ
 Sample : AR1242ICC1000
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 AR1242ICC1000

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 19 05:01:06 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0081825.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Aug 19 05:00:30 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.664	3.656	790.3E6	482.6E6	91.305	91.569
2) SA Decachlor...	8.682	8.629	698.4E6	186.8E6	94.884	93.137
Target Compounds						
16) L4 AR-1242-1	4.748	4.729	219.0E6	133.9E6	902.034	878.518
17) L4 AR-1242-2	4.767	4.747	328.0E6	204.0E6	899.261	894.341
18) L4 AR-1242-3	4.824	4.923	205.3E6	105.7E6	902.879	874.106
19) L4 AR-1242-4	4.943	5.007	165.3E6	101.7E6	901.450	864.505
20) L4 AR-1242-5	5.594	5.526	180.7E6	136.1E6	862.178	877.068



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO081825\
Data File : PO113010.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 18 Aug 2025 12:01
Operator : YP/AJ
Sample : AR1242ICC1000
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
AR1242ICC1000

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 19 05:01:06 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO081825.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Aug 19 05:00:30 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

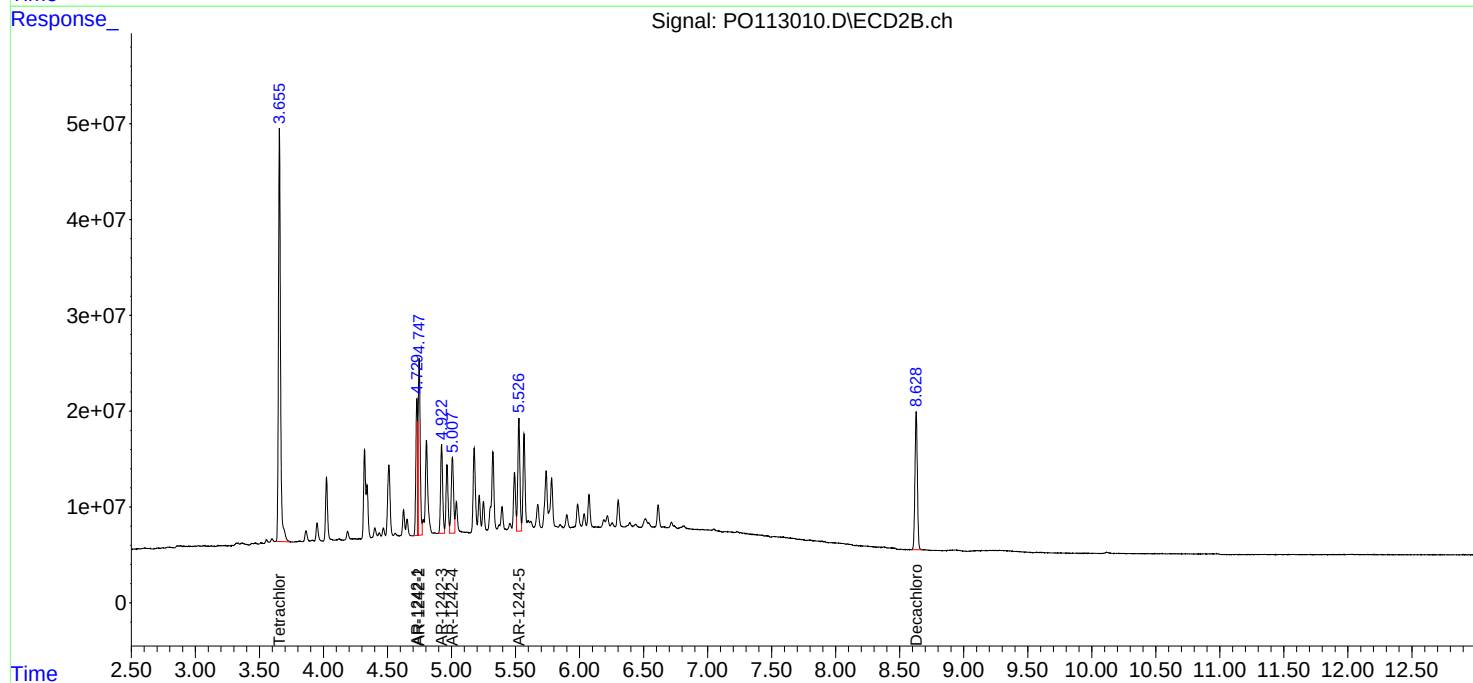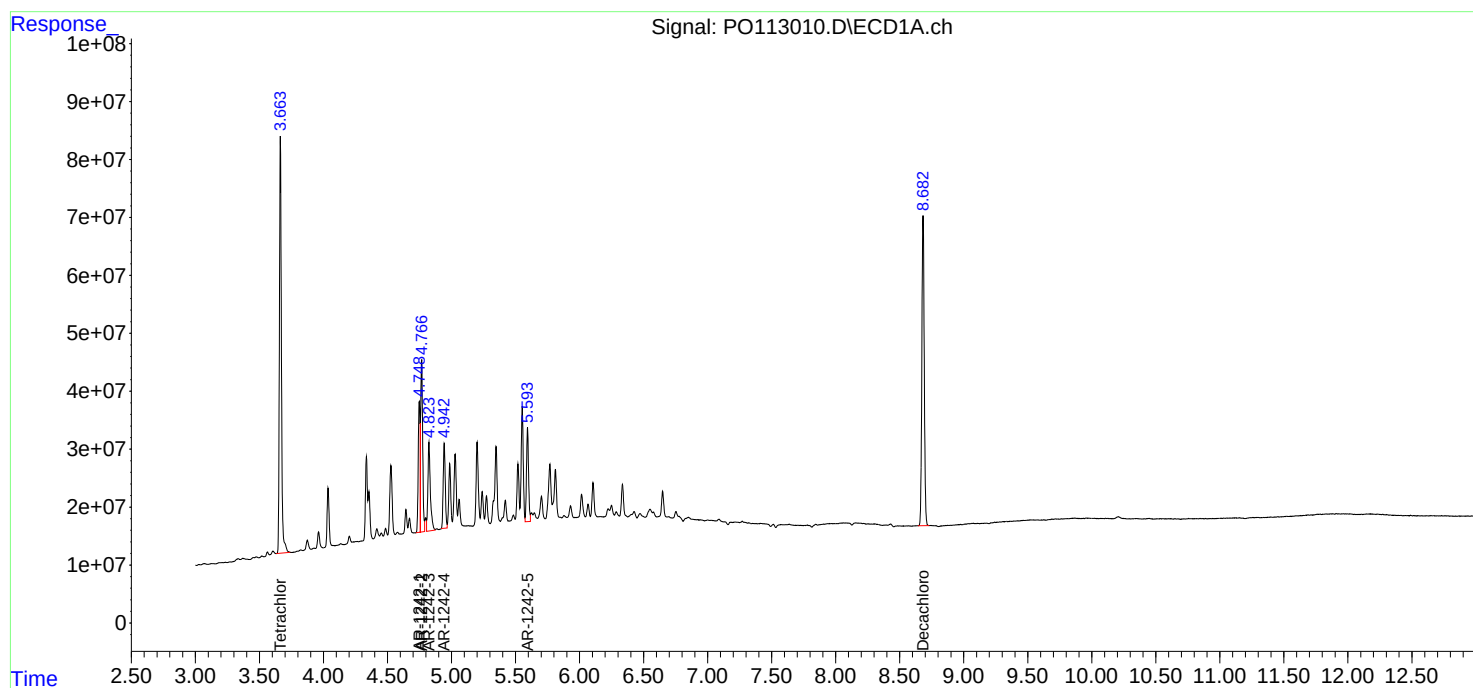

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0081825\
 Data File : P0113011.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 18 Aug 2025 12:20
 Operator : YP/AJ
 Sample : AR1242ICC750
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 AR1242ICC750

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 19 05:01:27 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0081825.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Aug 19 05:00:30 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.663	3.655	620.6E6	380.4E6	71.701	72.170
2) SA Decachlor...	8.682	8.627	540.0E6	146.8E6	73.362	73.184
Target Compounds						
16) L4 AR-1242-1	4.748	4.729	175.1E6	107.3E6	721.386	704.350
17) L4 AR-1242-2	4.766	4.746	258.7E6	162.9E6	709.343	714.312
18) L4 AR-1242-3	4.823	4.922	163.5E6	85600439	719.316	707.956
19) L4 AR-1242-4	4.943	5.006	131.5E6	82987408	717.438	705.553
20) L4 AR-1242-5	5.593	5.525	147.5E6	109.5E6	703.881	705.578



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO081825\
Data File : PO113011.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 18 Aug 2025 12:20
Operator : YP/AJ
Sample : AR1242ICC750
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
AR1242ICC750

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 19 05:01:27 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO081825.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Aug 19 05:00:30 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

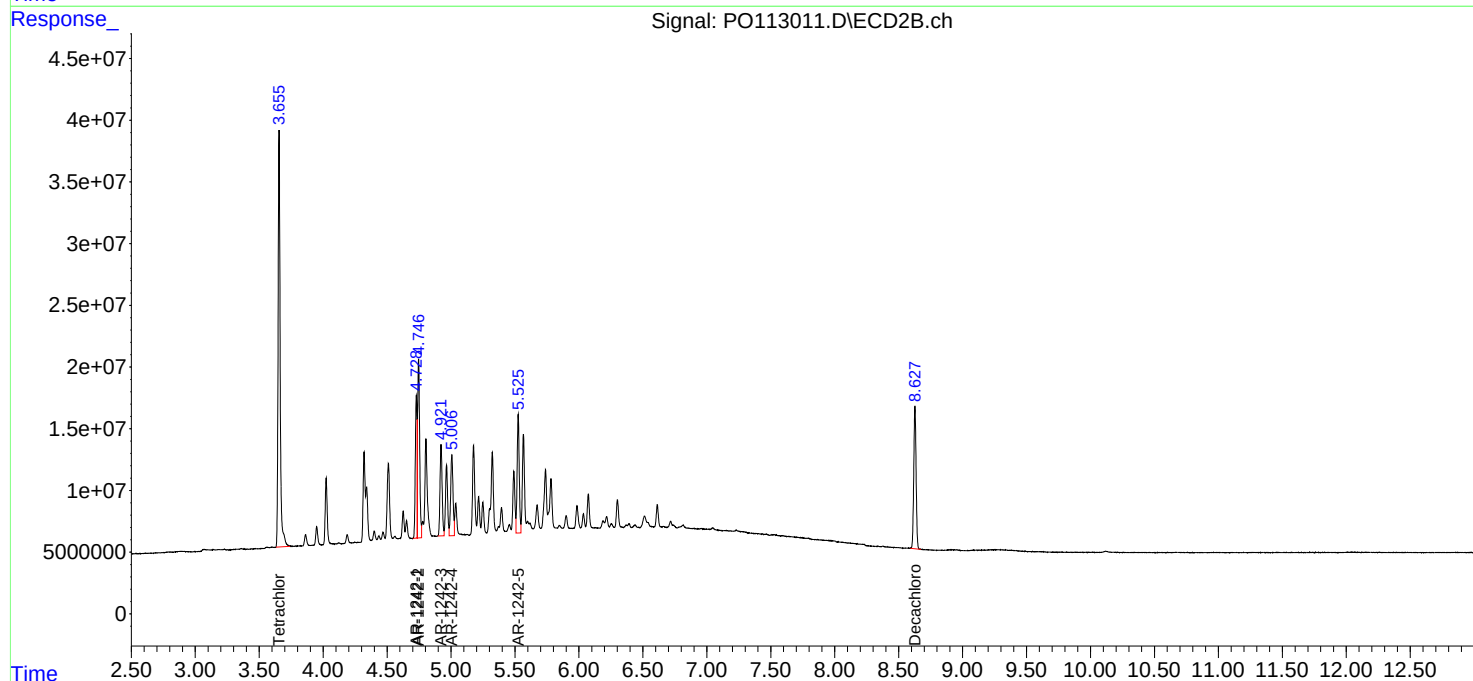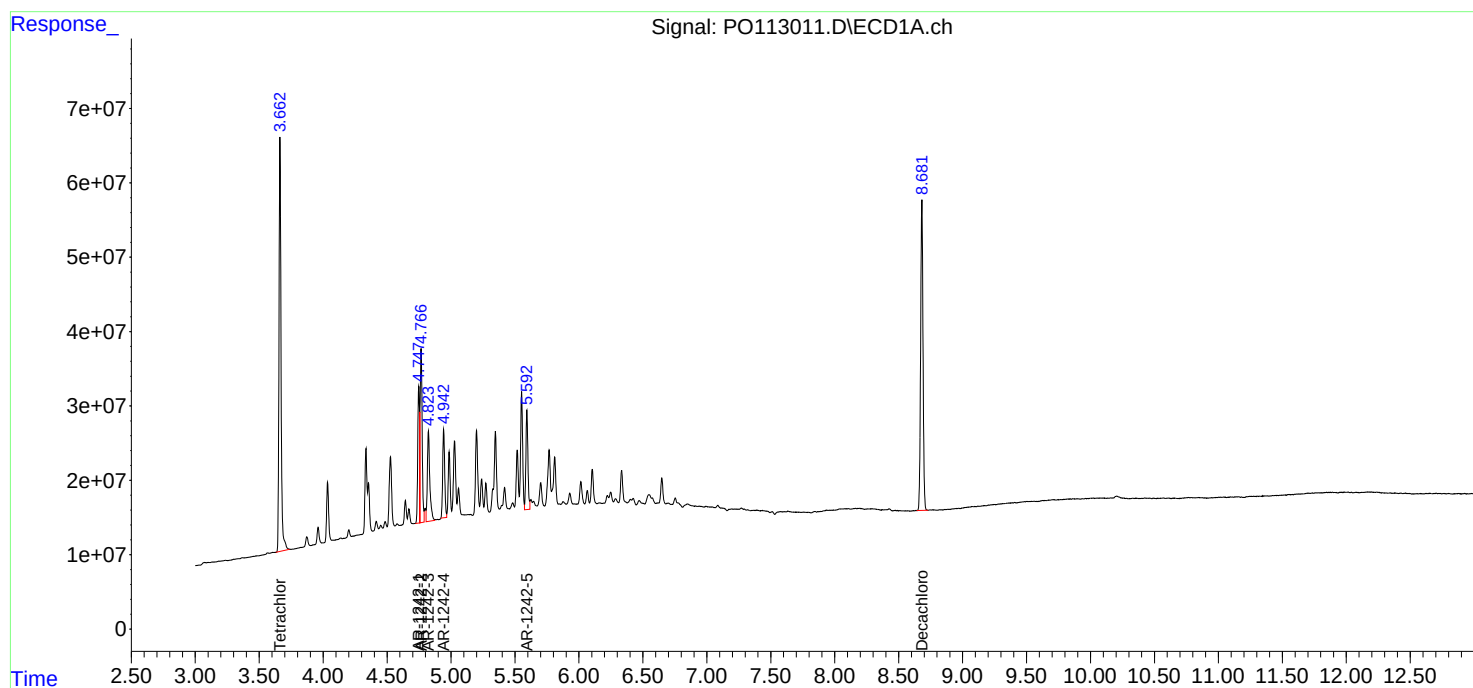

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0081825\
 Data File : P0113012.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 18 Aug 2025 12:38
 Operator : YP/AJ
 Sample : AR1242ICC500
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 AR1242ICC500

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 19 05:01:49 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0081825.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Aug 19 05:00:30 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.663	3.655	432.8E6	263.5E6	50.000	50.000
2) SA Decachlor...	8.681	8.626	368.0E6	100.3E6	50.000	50.000
Target Compounds						
16) L4 AR-1242-1	4.747	4.729	121.4E6	76197369	500.000	500.000
17) L4 AR-1242-2	4.766	4.747	182.4E6	114.0E6	500.000	500.000
18) L4 AR-1242-3	4.824	4.922	113.7E6	60456076	500.000	500.000
19) L4 AR-1242-4	4.942	5.006	91668775	58810219	500.000	500.000
20) L4 AR-1242-5	5.592	5.526	104.8E6	77583399	500.000	500.000



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO081825\
Data File : PO113012.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 18 Aug 2025 12:38
Operator : YP/AJ
Sample : AR1242ICC500
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
AR1242ICC500

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 19 05:01:49 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO081825.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Aug 19 05:00:30 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

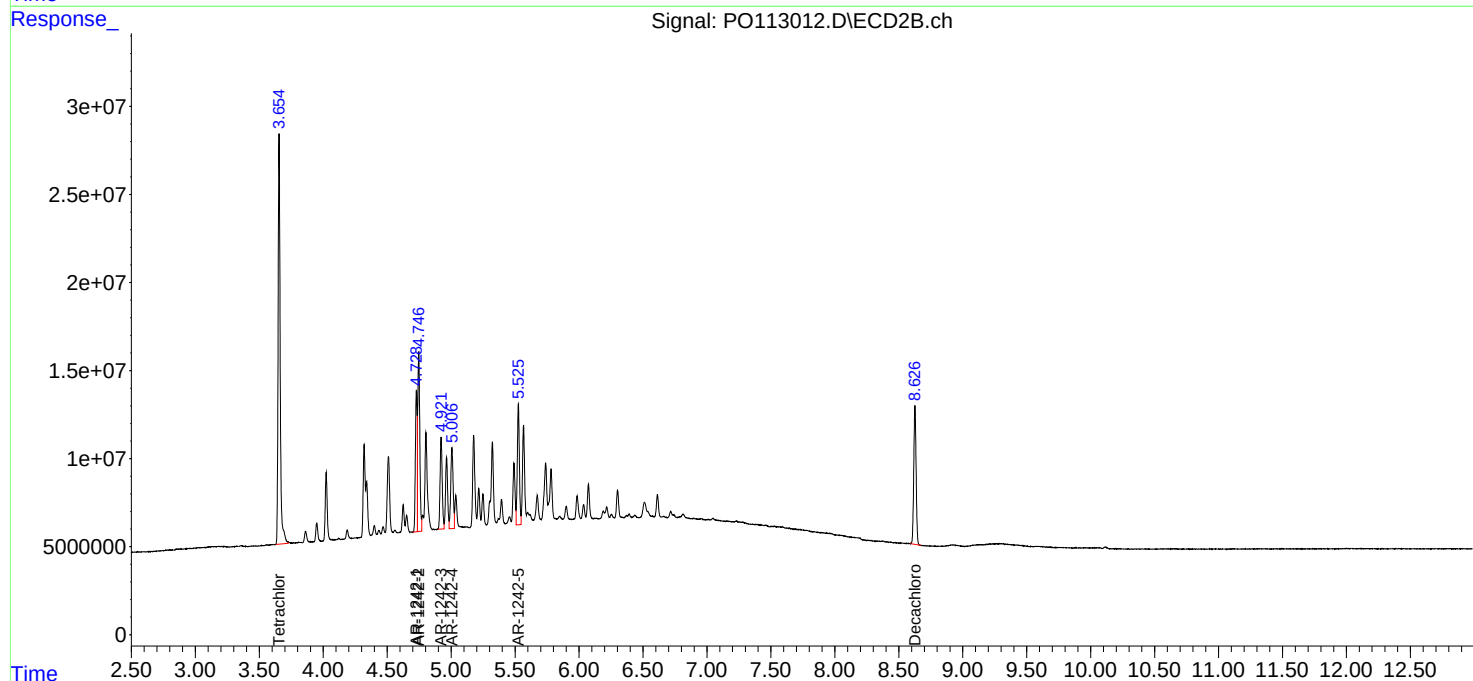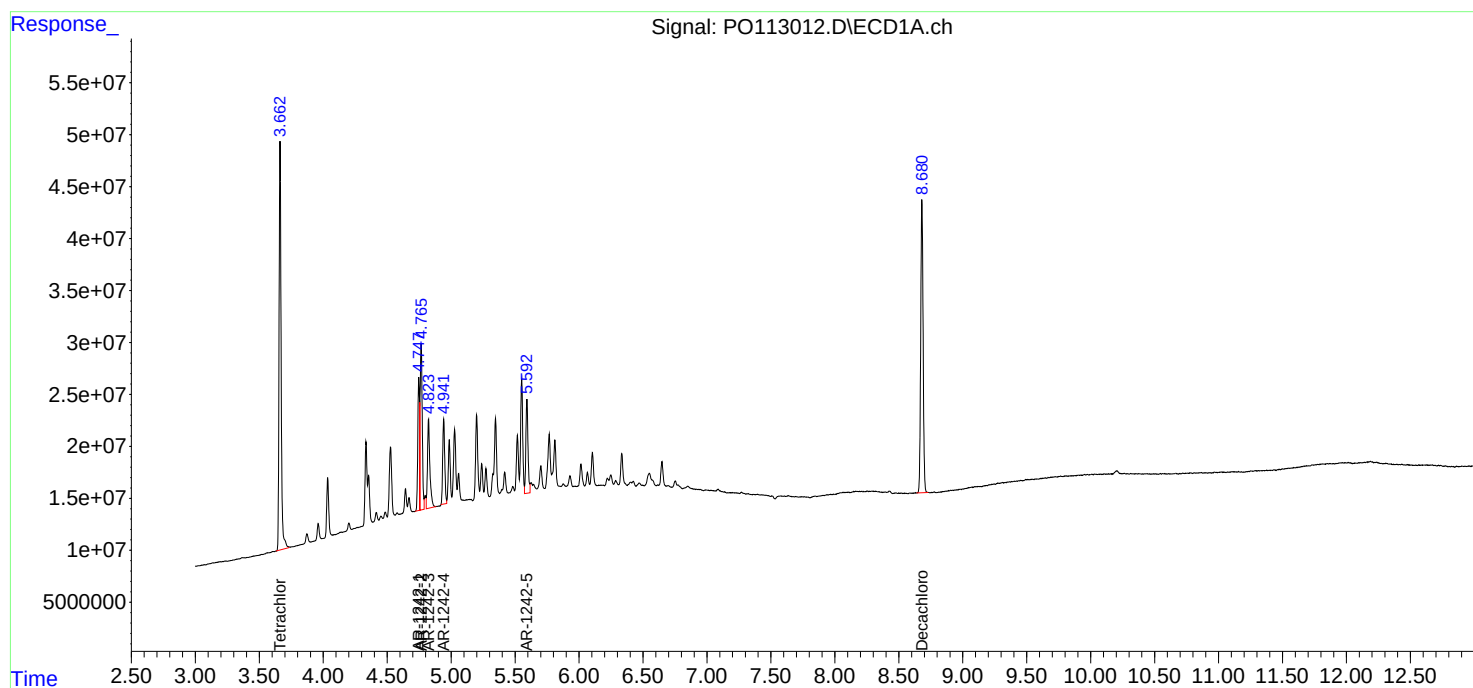

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0081825\
 Data File : P0113013.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 18 Aug 2025 12:57
 Operator : YP/AJ
 Sample : AR1242ICC250
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 AR1242ICC250

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 19 05:02:10 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0081825.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Aug 19 05:00:30 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.664	3.656	212.9E6	131.8E6	24.601	25.001
2)	SA Decachlor...	8.683	8.629	181.6E6	50519854	24.673	25.188
Target Compounds							
16)	L4 AR-1242-1	4.749	4.730	60181316	39111281	247.875	256.645
17)	L4 AR-1242-2	4.768	4.748	91044620	58590662	249.630	256.919
18)	L4 AR-1242-3	4.824	4.923	56585858	30921281	248.886	255.733
19)	L4 AR-1242-4	4.944	5.007	46289370	30803322	252.482	261.887
20)	L4 AR-1242-5	5.594	5.527	53931193	40625723	257.385	261.820



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO081825\
Data File : PO113013.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 18 Aug 2025 12:57
Operator : YP/AJ
Sample : AR1242ICC250
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
AR1242ICC250

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 19 05:02:10 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO081825.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Aug 19 05:00:30 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

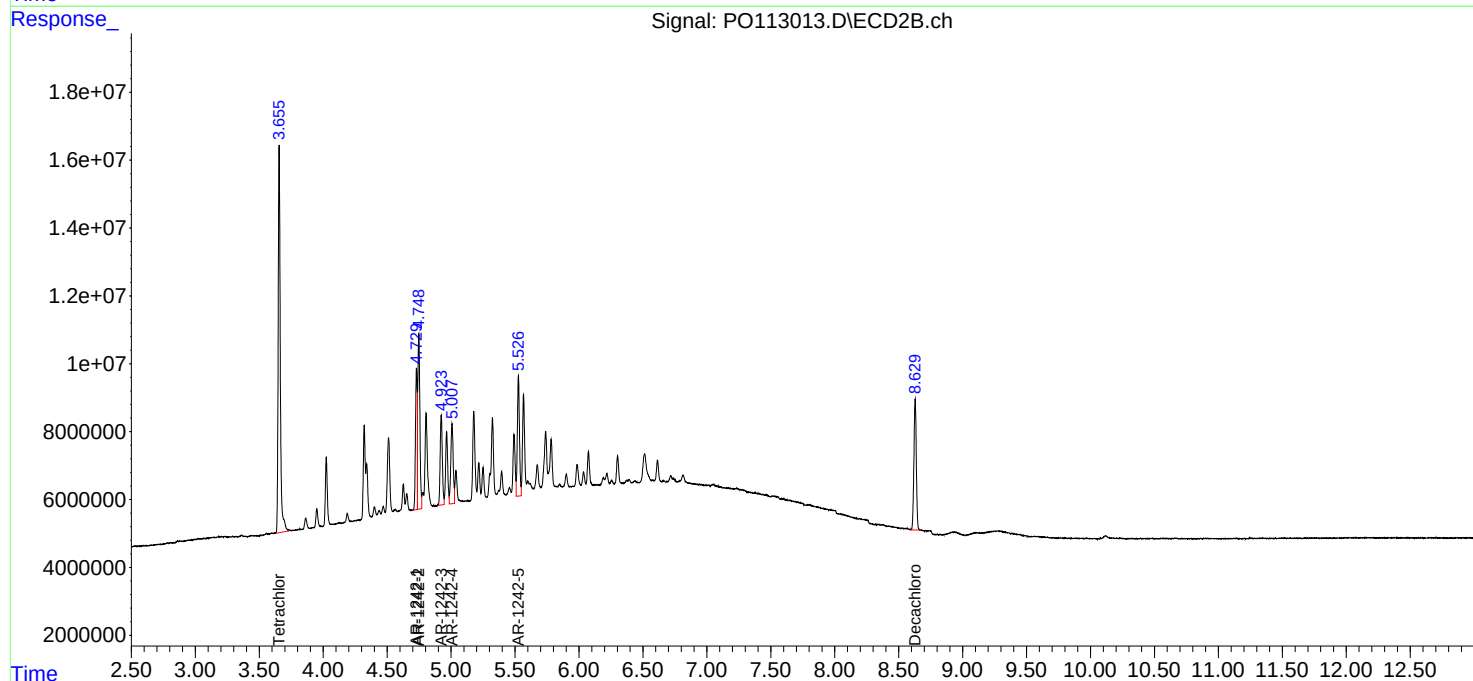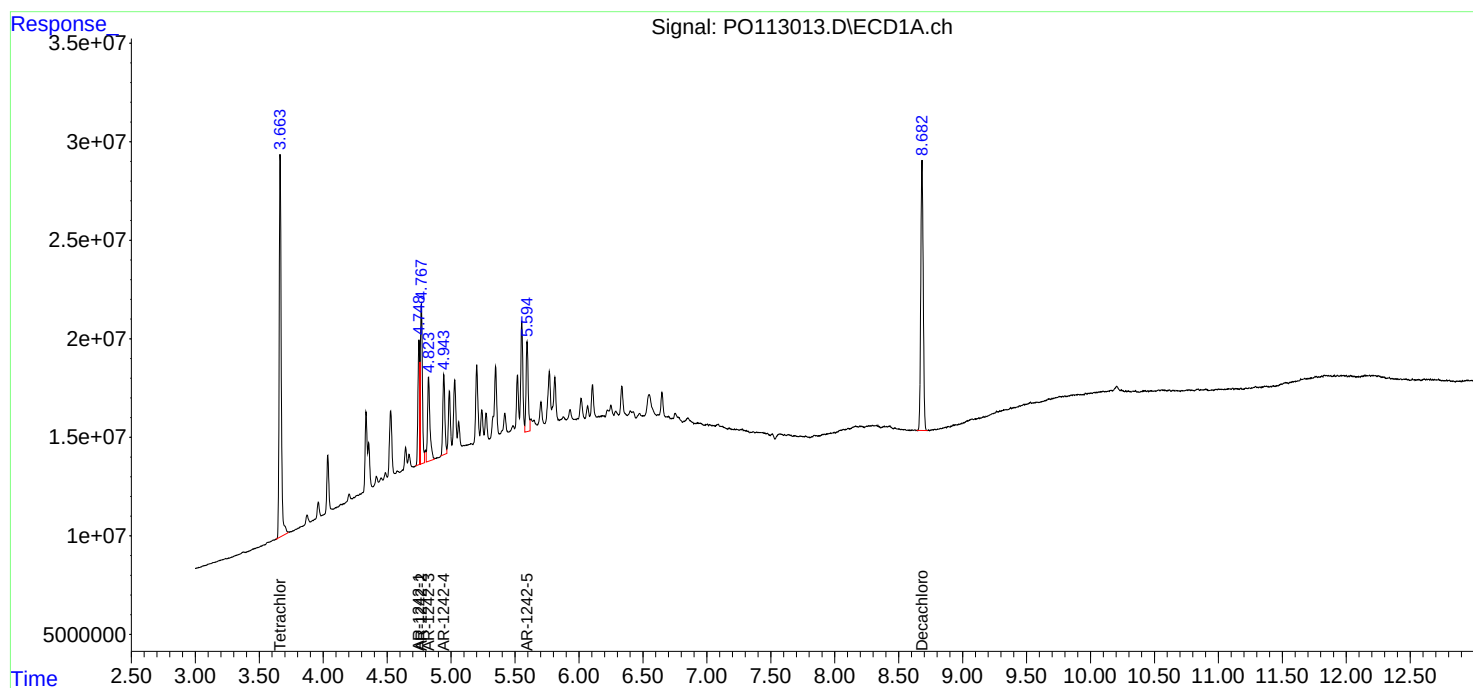

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0081825\
 Data File : P0113014.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 18 Aug 2025 13:15
 Operator : YP/AJ
 Sample : AR1242ICC050
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 AR1242ICC050

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 08/19/2025
 Supervised By :mohammad ahmed 08/20/2025

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 19 05:02:32 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0081825.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Aug 19 05:00:30 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.663	3.655	34925483	22528993	4.035	4.275
2)	SA Decachlor...	8.681	8.627	30372133	8862645	4.126	4.419
Target Compounds							
16)	L4 AR-1242-1	4.747	4.728	10680758	6834075	43.992m	44.845m
17)	L4 AR-1242-2	4.766	4.747	15815267	10049295	43.363m	44.066
18)	L4 AR-1242-3	4.824	4.922	11619589	6020015	51.107	49.788
19)	L4 AR-1242-4	4.943	5.007	7908544	6750995	43.137	57.396 #
20)	L4 AR-1242-5	5.592	5.526	9912247	7296334	47.306m	47.023m

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO081825\
Data File : PO113014.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 18 Aug 2025 13:15
Operator : YP/AJ
Sample : AR1242ICC050
Misc :
ALS Vial : 14 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
AR1242ICC050

Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 08/19/2025
Supervised By :mohammad ahmed 08/20/2025

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 19 05:02:32 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO081825.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Aug 19 05:00:30 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

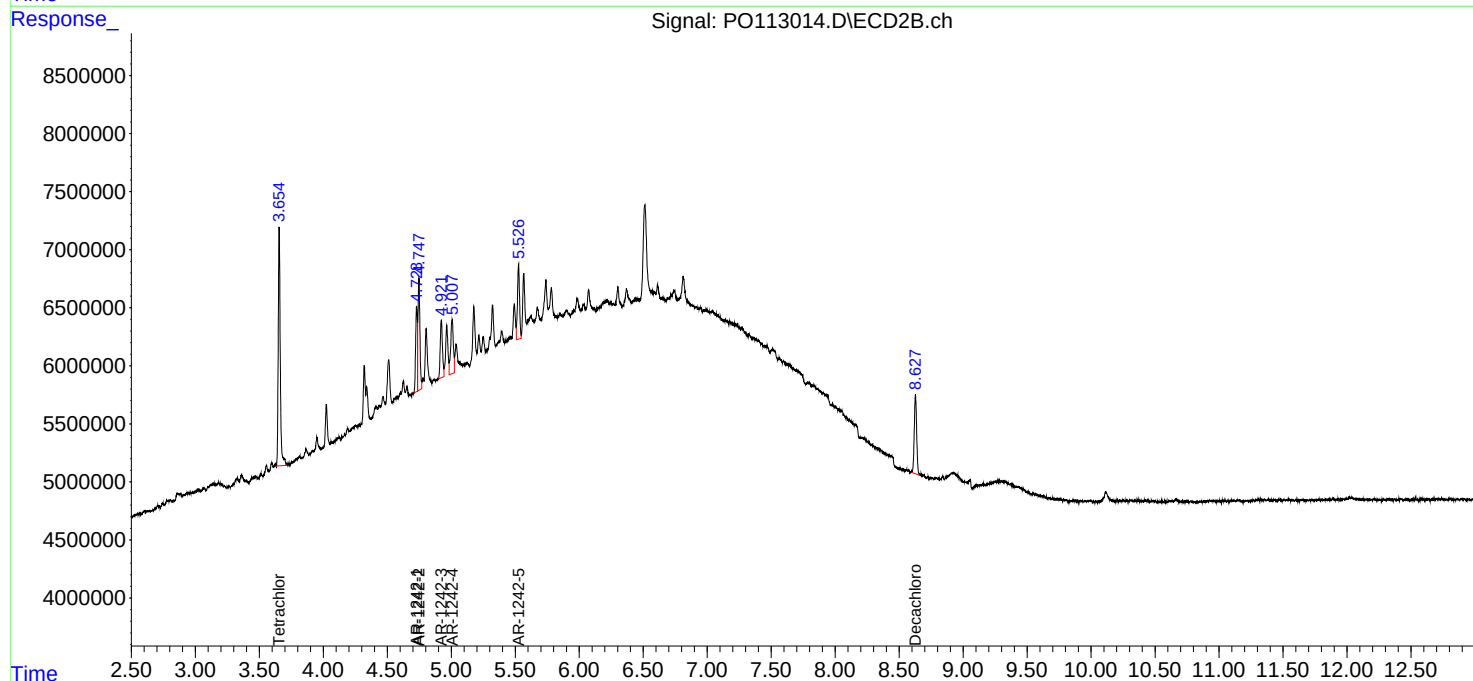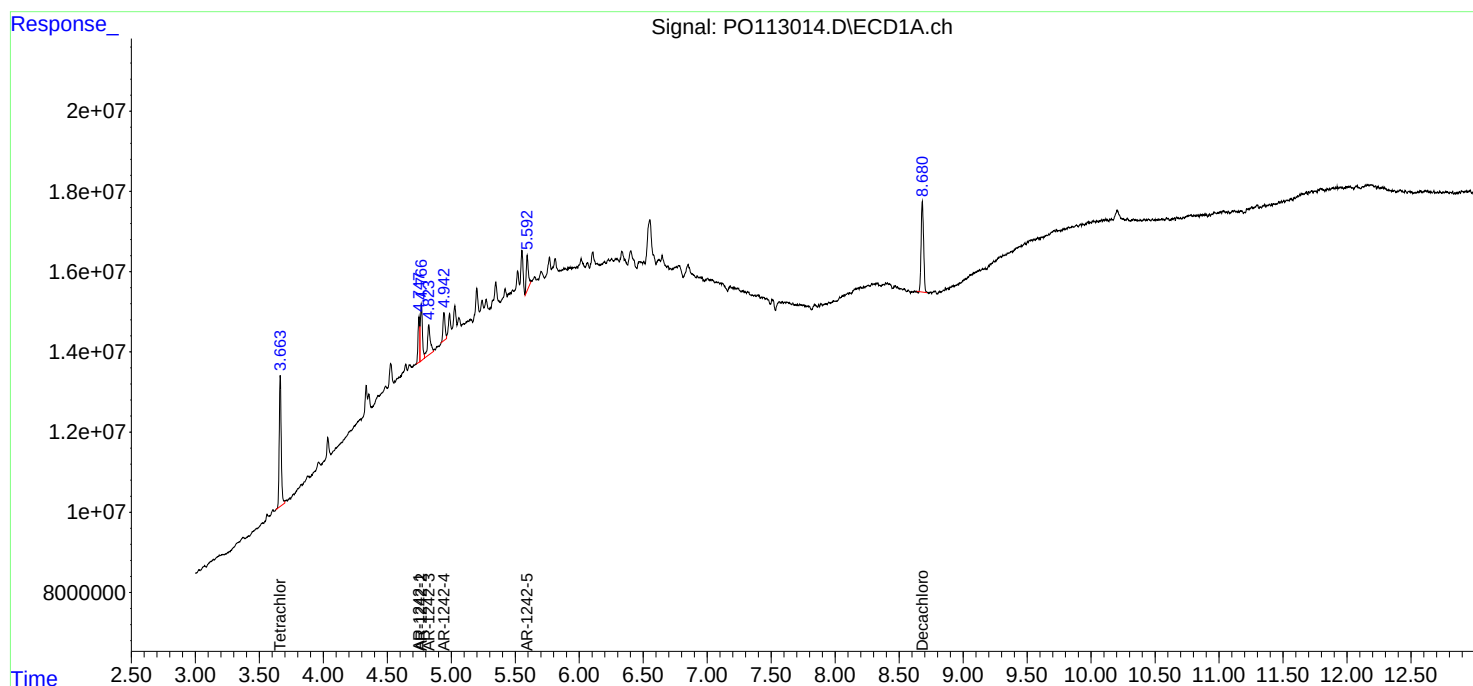

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0081825\
 Data File : P0113015.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 18 Aug 2025 13:34
 Operator : YP/AJ
 Sample : AR1248ICC1000
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 AR1248ICC1000

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 19 05:13:29 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0081825.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Aug 19 05:12:51 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.663	3.655	838.2E6	504.7E6	97.589	96.994
2) SA Decachlor...	8.683	8.627	718.2E6	189.6E6	94.869	94.382
Target Compounds						
21) L5 AR-1248-1	4.748	4.729	177.6E6	108.5E6	964.791	927.767
22) L5 AR-1248-2	4.986	4.965	240.1E6	150.8E6	971.626	922.798
23) L5 AR-1248-3	5.200	5.006	306.1E6	159.4E6	928.687	921.357
24) L5 AR-1248-4	5.552	5.177	475.5E6	188.3E6	935.504	918.888
25) L5 AR-1248-5	5.593	5.567	324.2E6	194.0E6	930.863	916.030



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO081825\
Data File : PO113015.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 18 Aug 2025 13:34
Operator : YP/AJ
Sample : AR1248ICC1000
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
AR1248ICC1000

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 19 05:13:29 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO081825.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Aug 19 05:12:51 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

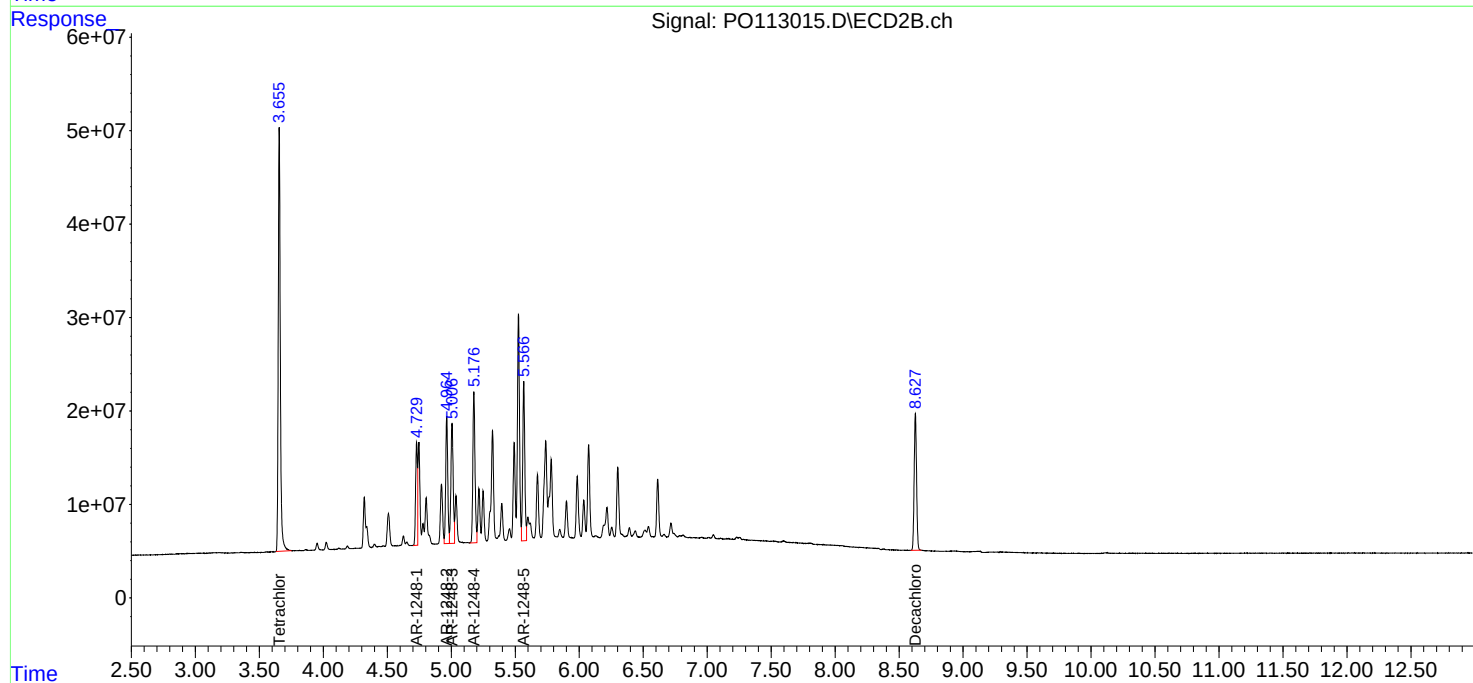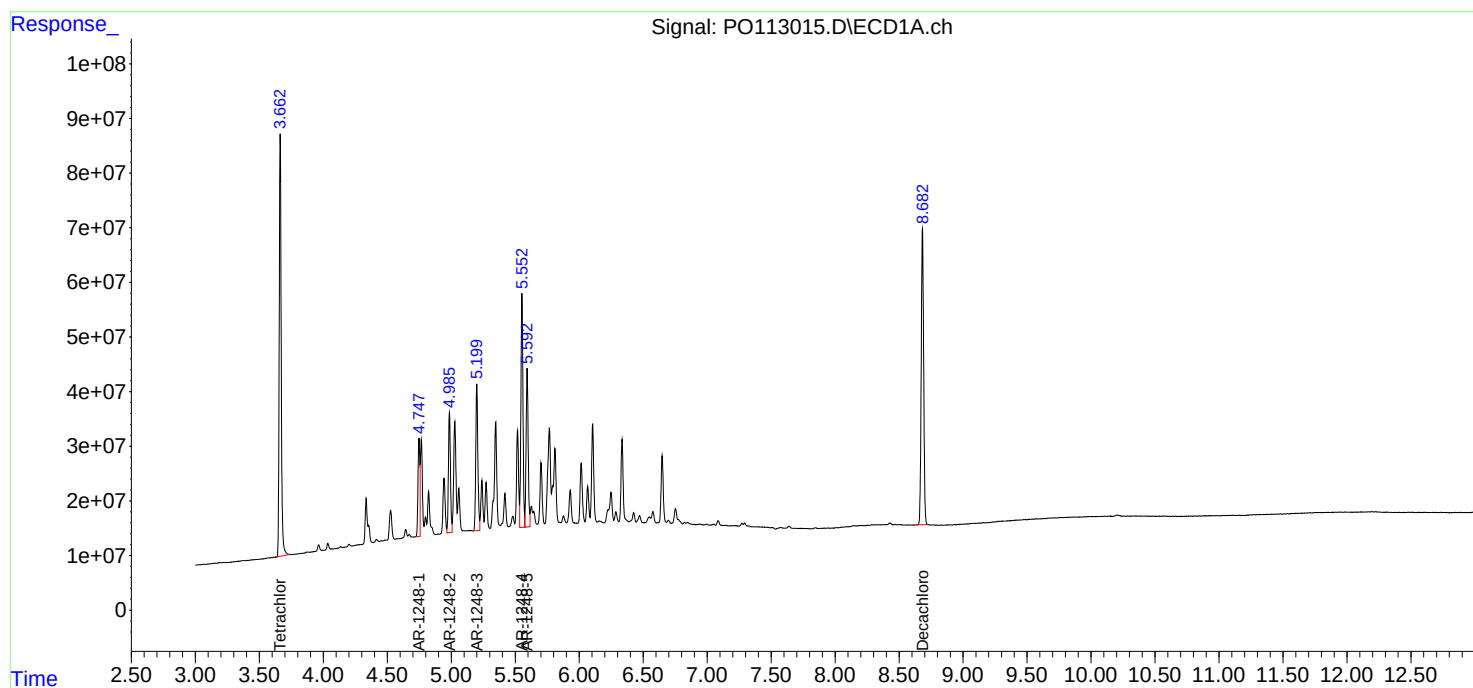

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0081825\
 Data File : P0113016.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 18 Aug 2025 13:52
 Operator : YP/AJ
 Sample : AR1248ICC750
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 AR1248ICC750

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 19 05:13:50 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0081825.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Aug 19 05:12:51 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.663	3.655	641.1E6	386.6E6	74.640	74.305
2) SA Decachlor...	8.682	8.628	563.6E6	148.6E6	74.452	73.955
Target Compounds						
21) L5 AR-1248-1	4.748	4.728	136.0E6	84958849	738.729	726.663
22) L5 AR-1248-2	4.986	4.964	184.8E6	118.3E6	747.715	723.853
23) L5 AR-1248-3	5.200	5.006	236.8E6	124.8E6	718.364	721.172
24) L5 AR-1248-4	5.552	5.176	368.4E6	146.9E6	724.738	716.783
25) L5 AR-1248-5	5.593	5.566	254.1E6	153.0E6	729.605	722.136



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO081825\
Data File : PO113016.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 18 Aug 2025 13:52
Operator : YP/AJ
Sample : AR1248ICC750
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
AR1248ICC750

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 19 05:13:50 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO081825.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Aug 19 05:12:51 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

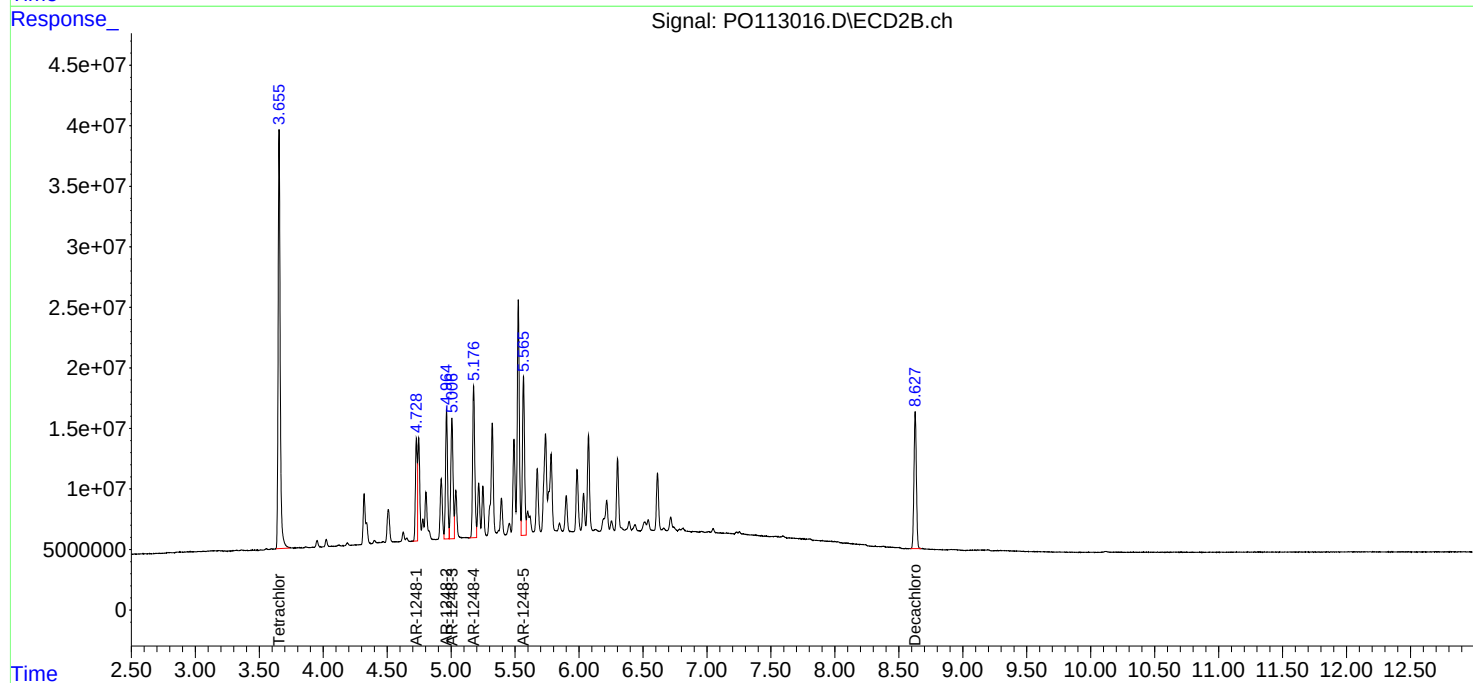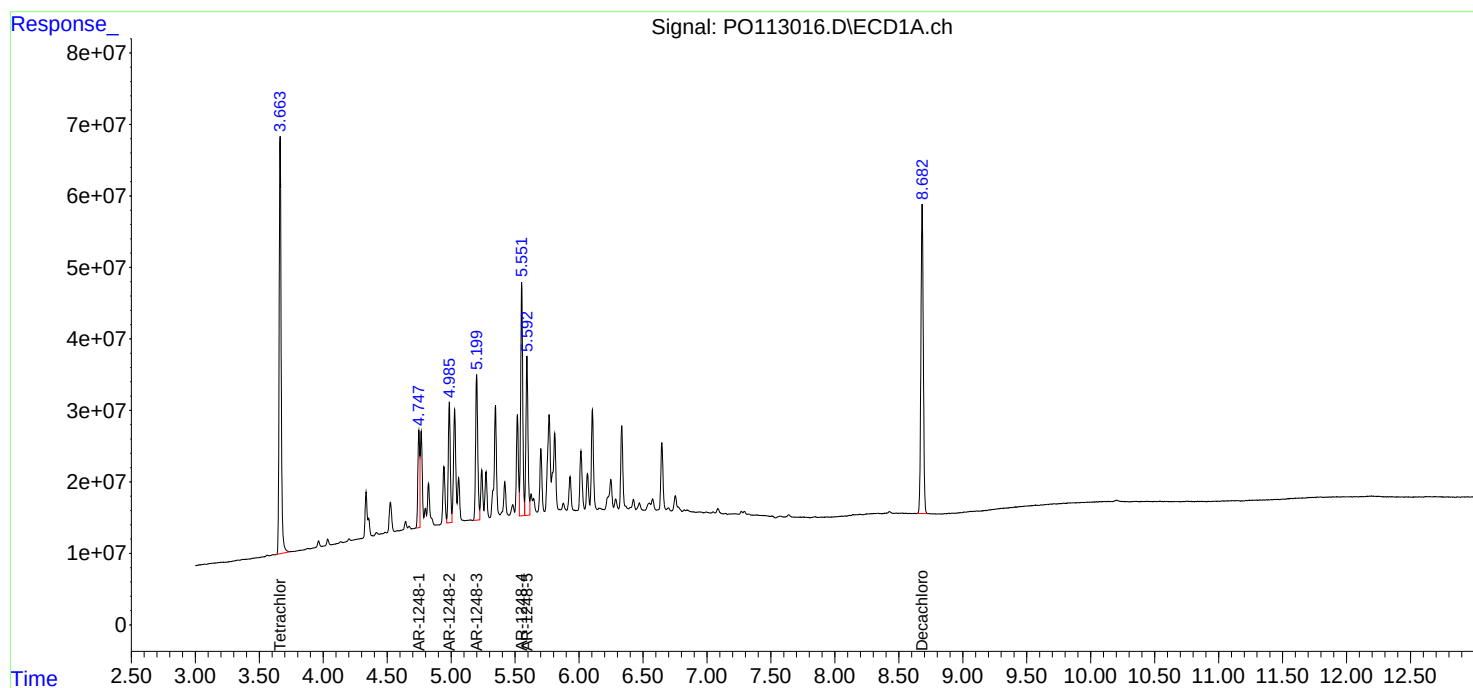

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0081825\
 Data File : P0113017.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 18 Aug 2025 14:09
 Operator : YP/AJ
 Sample : AR1248ICC500
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 AR1248ICC500

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 19 05:14:12 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0081825.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Aug 19 05:12:51 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.661	3.655	429.4E6	260.2E6	50.000	50.000
2) SA Decachlor...	8.682	8.627	378.5E6	100.4E6	50.000	50.000
Target Compounds						
21) L5 AR-1248-1	4.746	4.729	92017394	58458199	500.000	500.000
22) L5 AR-1248-2	4.983	4.964	123.6E6	81705093	500.000	500.000
23) L5 AR-1248-3	5.198	5.006	164.8E6	86521016	500.000	500.000
24) L5 AR-1248-4	5.550	5.176	254.2E6	102.4E6	500.000	500.000
25) L5 AR-1248-5	5.591	5.566	174.2E6	105.9E6	500.000	500.000



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO081825\
Data File : PO113017.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 18 Aug 2025 14:09
Operator : YP/AJ
Sample : AR1248ICC500
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
AR1248ICC500

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 19 05:14:12 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO081825.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Aug 19 05:12:51 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

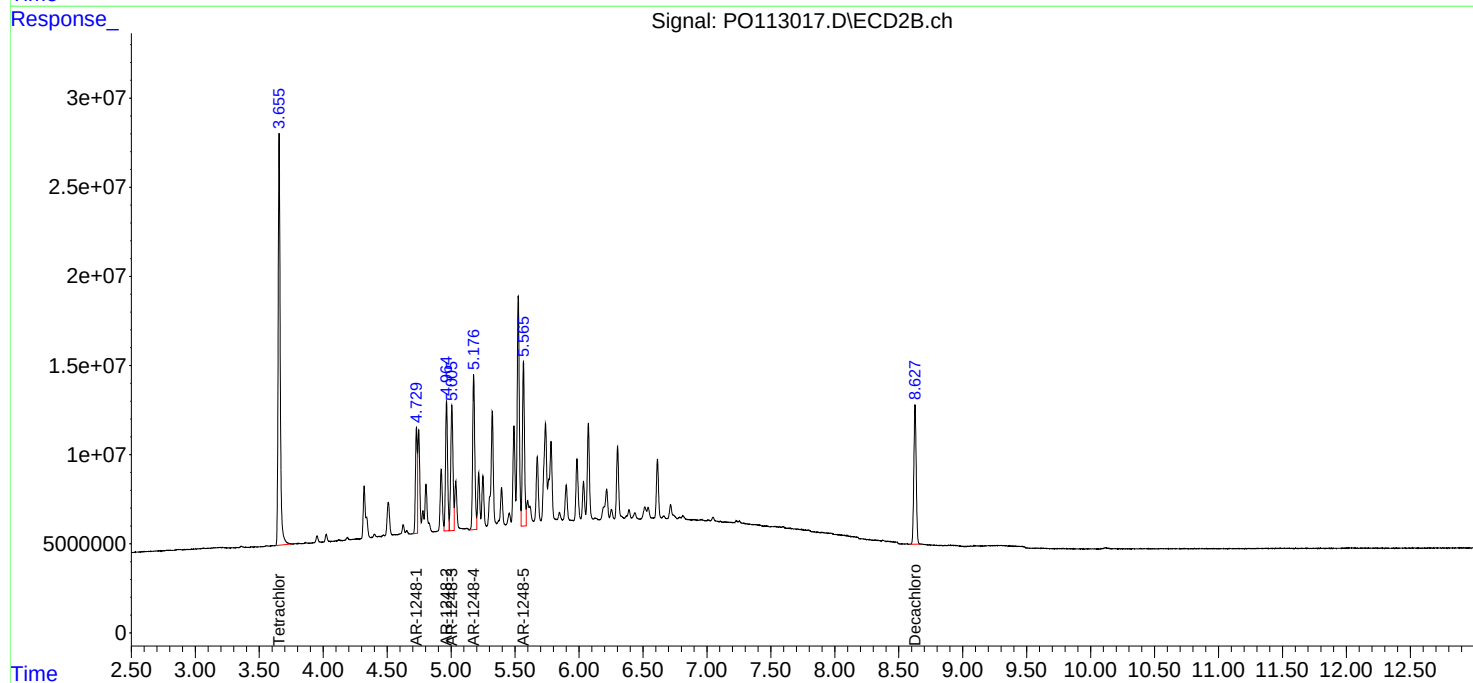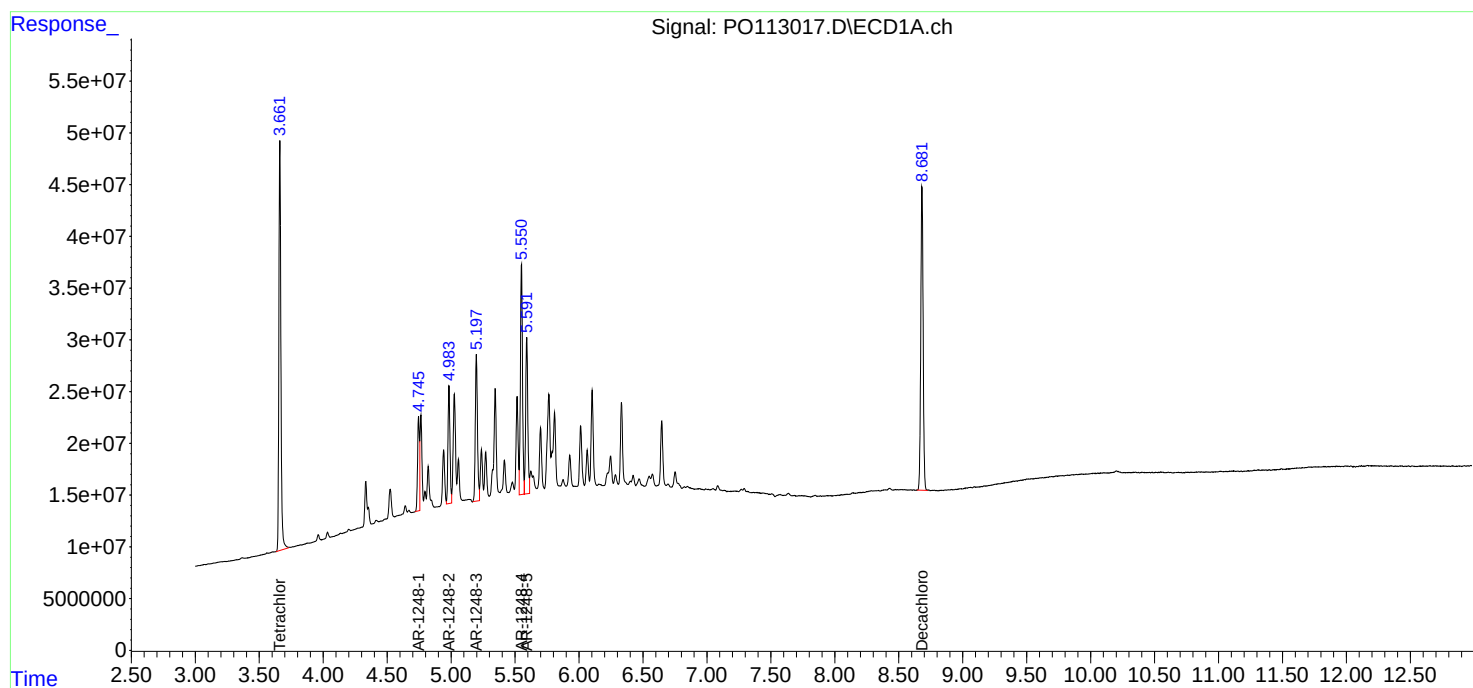

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0081825\
 Data File : P0113018.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 18 Aug 2025 14:28
 Operator : YP/AJ
 Sample : AR1248ICC250
 Misc :
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 AR1248ICC250

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 19 05:14:31 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0081825.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Aug 19 05:12:51 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.664	3.656	209.7E6	126.9E6	24.414	24.390
2) SA Decachlor...	8.682	8.627	188.2E6	51115576	24.865	25.447
Target Compounds						
21) L5 AR-1248-1	4.748	4.729	45122166	29255539	245.183	250.226
22) L5 AR-1248-2	4.986	4.965	62979159	42275318	254.859	258.707
23) L5 AR-1248-3	5.200	5.007	79668469	44175959	241.702	255.290
24) L5 AR-1248-4	5.553	5.178	126.5E6	52254392	248.765	255.036
25) L5 AR-1248-5	5.594	5.567	84964920	55625603	243.937	262.628


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO081825\
Data File : PO113018.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 18 Aug 2025 14:28
Operator : YP/AJ
Sample : AR1248ICC250
Misc :
ALS Vial : 18 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
AR1248ICC250

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 19 05:14:31 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO081825.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Aug 19 05:12:51 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

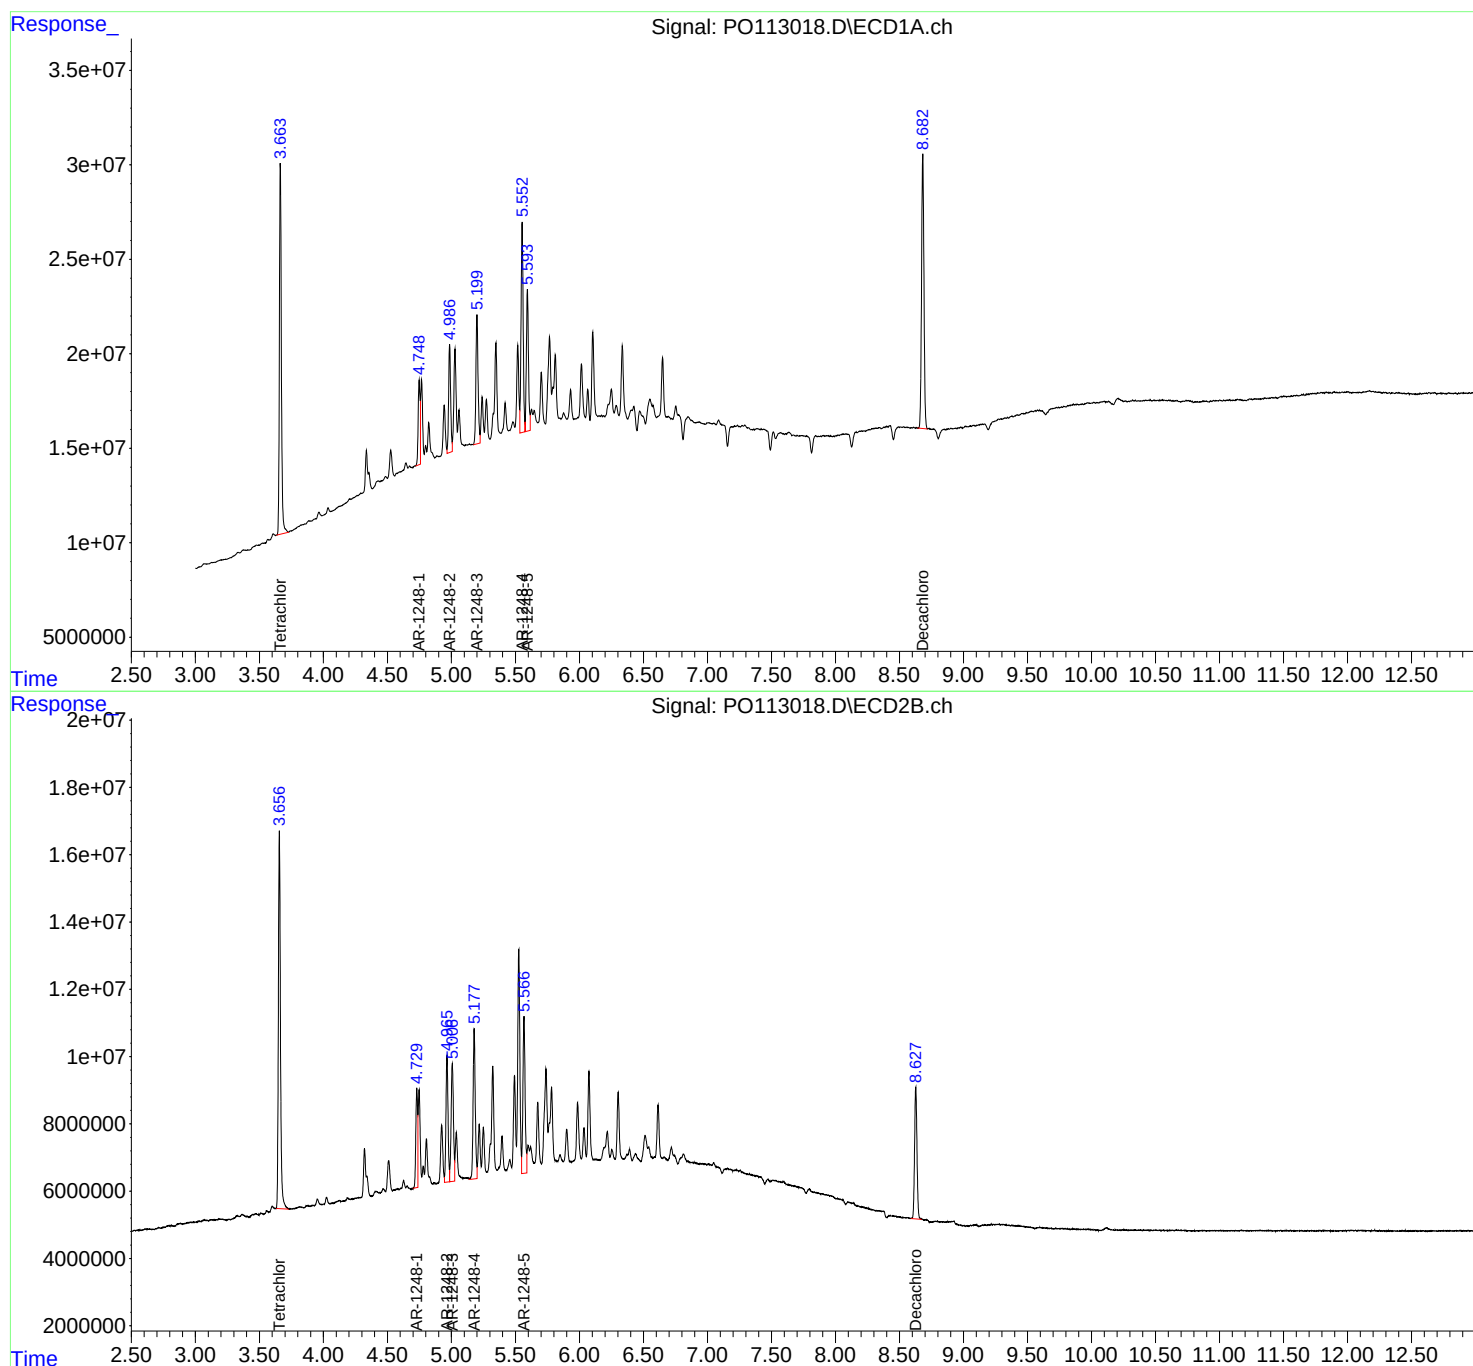

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0081825\
 Data File : P0113019.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 18 Aug 2025 14:46
 Operator : YP/AJ
 Sample : AR1248ICC050
 Misc :
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 AR1248ICC050

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 19 05:14:51 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0081825.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Aug 19 05:12:51 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.663	3.655	33541803	21100686	3.905	4.055
2) SA Decachlor...	8.683	8.627	30379928	8654947	4.013	4.309
Target Compounds						
21) L5 AR-1248-1	4.748	4.729	7449194	5093554	40.477	43.566
22) L5 AR-1248-2	4.986	4.964	11191763	8123784	45.290	49.714
23) L5 AR-1248-3	5.200	5.006	16210491	8636665	49.180	49.911
24) L5 AR-1248-4	5.553	5.176	25855584	9905263	50.864	48.344
25) L5 AR-1248-5	5.593	5.567	17811440	11461135	51.137	54.112



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO081825\
Data File : PO113019.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 18 Aug 2025 14:46
Operator : YP/AJ
Sample : AR1248ICC050
Misc :
ALS Vial : 19 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
AR1248ICC050

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 19 05:14:51 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO081825.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Aug 19 05:12:51 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

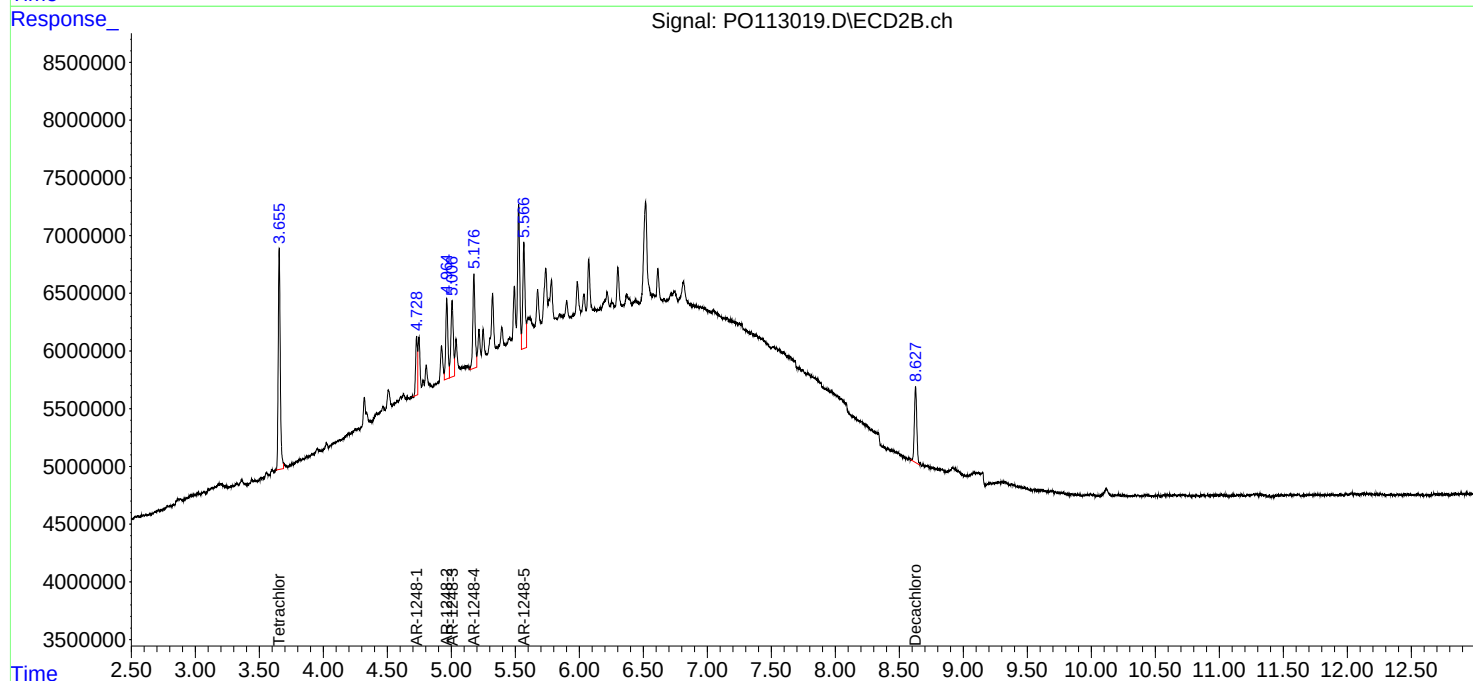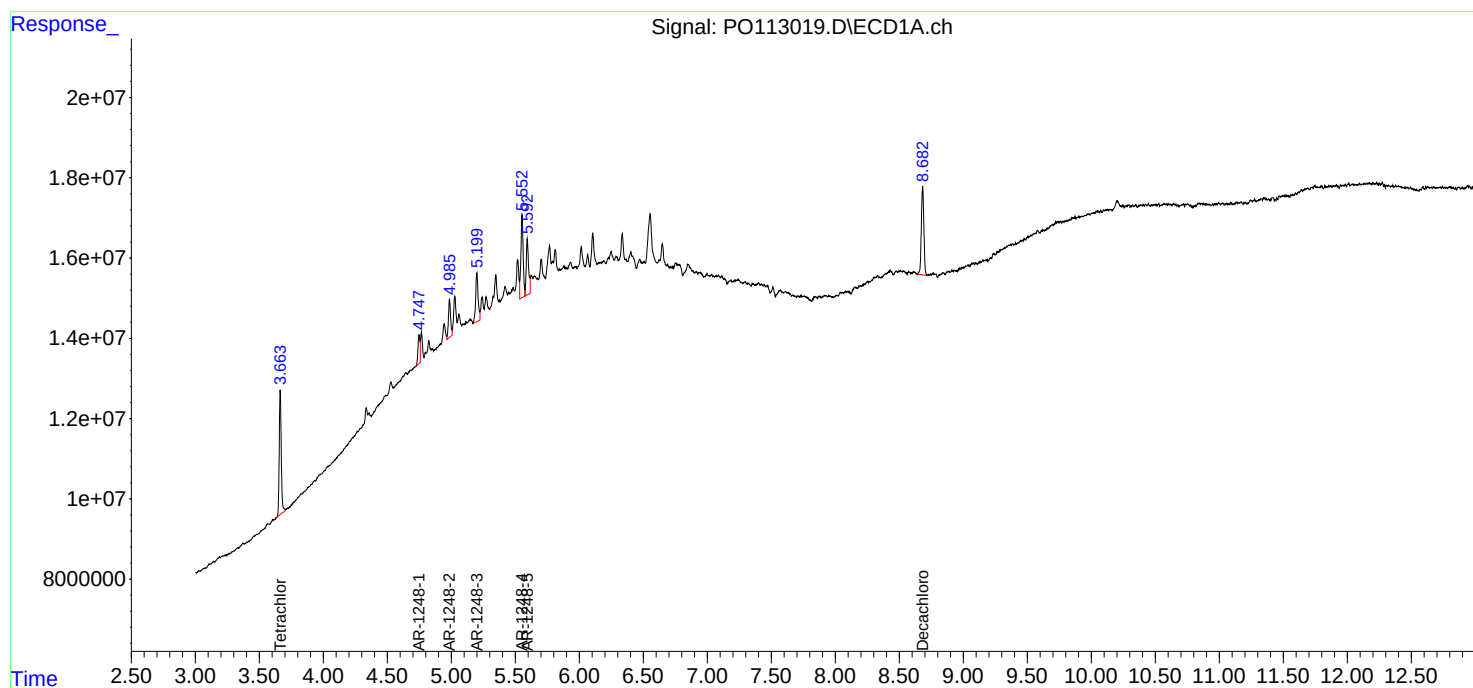

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0081825\
 Data File : P0113020.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 18 Aug 2025 15:05
 Operator : YP/AJ
 Sample : AR1254ICC1000
 Misc :
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 AR1254ICC1000

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 19 05:26:03 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0081825.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Aug 19 05:25:15 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.663	3.655	812.7E6	491.1E6	97.720	97.078
2)	SA Decachlor...	8.683	8.627	713.2E6	185.6E6	95.742	94.040
Target Compounds							
26)	L6 AR-1254-1	5.552	5.525	499.6E6	288.8E6	947.625	926.947
27)	L6 AR-1254-2	5.702	5.673	454.6E6	255.0E6	947.600	921.953
28)	L6 AR-1254-3	6.104	6.073	711.1E6	394.7E6	962.469	948.598
29)	L6 AR-1254-4	6.334	6.302	533.0E6	258.2E6	963.574	943.828
30)	L6 AR-1254-5	6.752	6.717	688.0E6	325.5E6	979.998	925.920



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO081825\
Data File : PO113020.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 18 Aug 2025 15:05
Operator : YP/AJ
Sample : AR1254ICC1000
Misc :
ALS Vial : 20 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
AR1254ICC1000

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 19 05:26:03 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO081825.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Aug 19 05:25:15 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µm Signal #2 Info : 30M x 0.32mm x 0.25µm

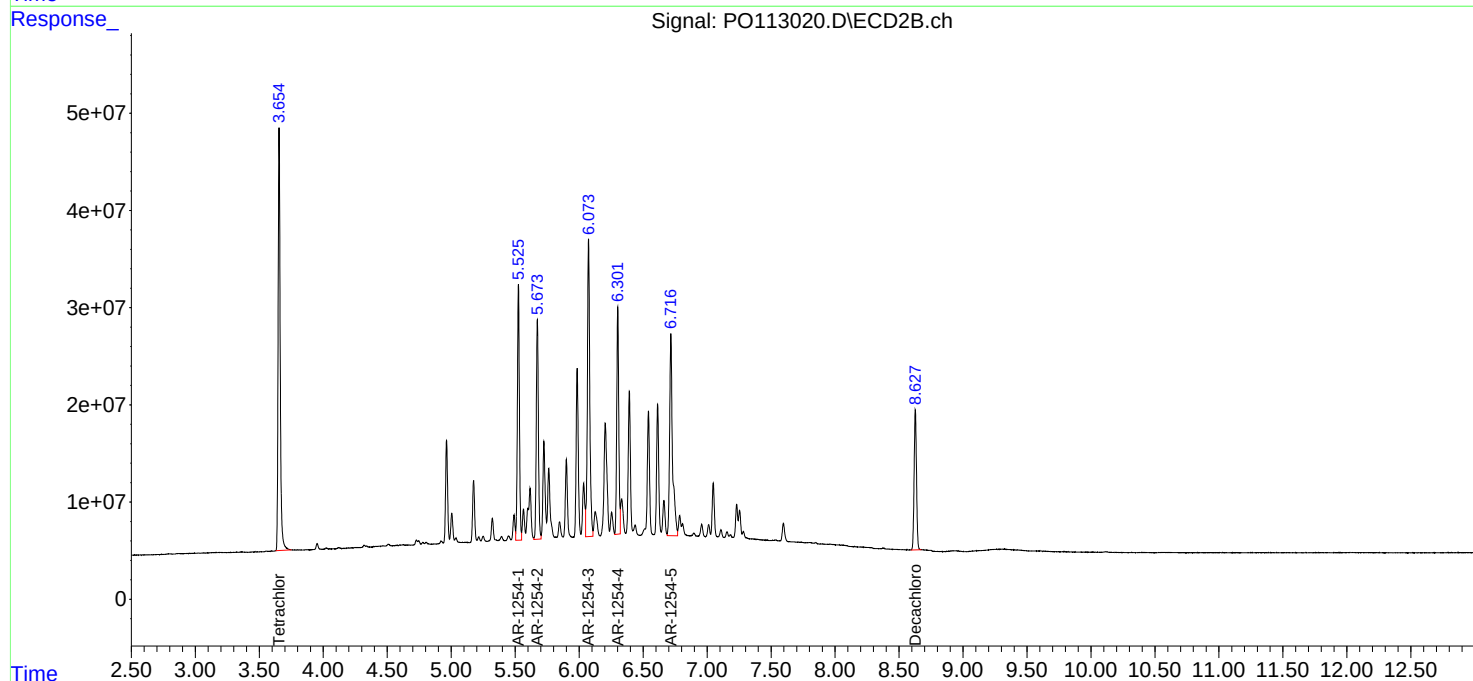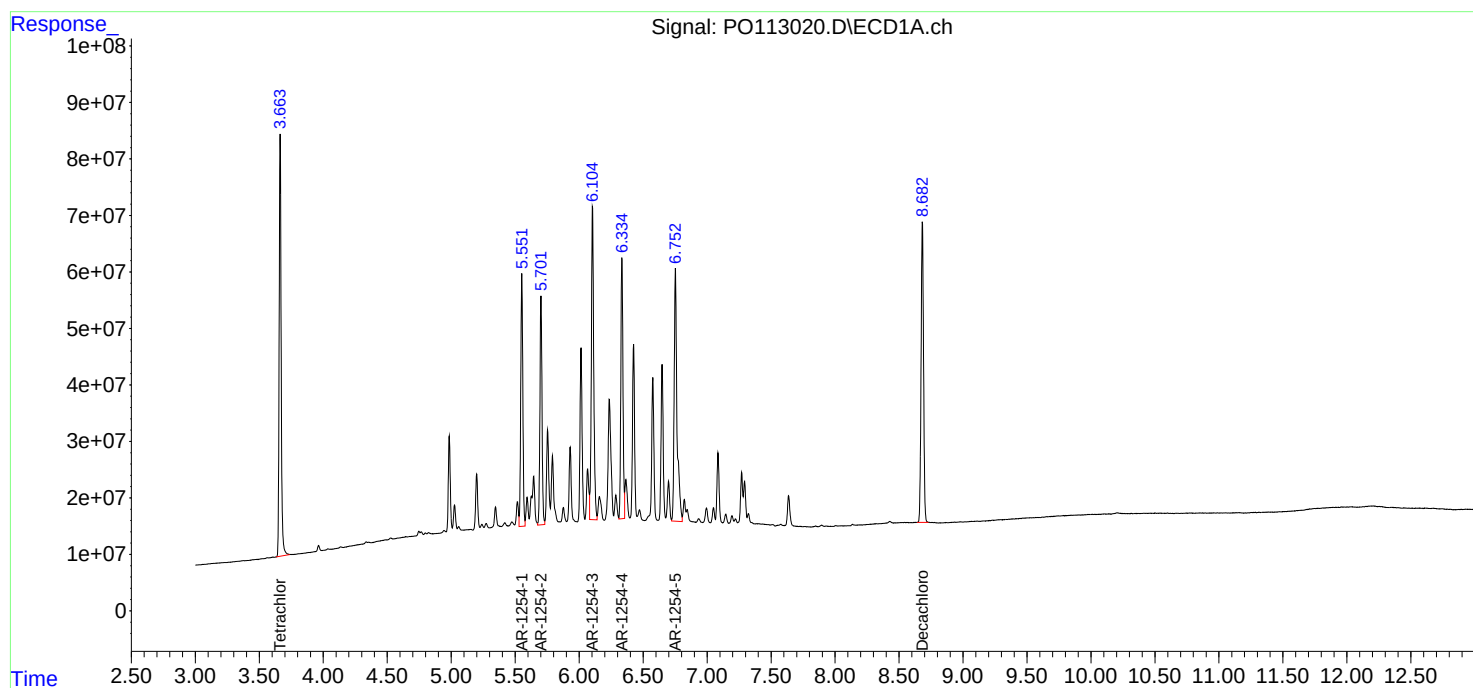

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0081825\
 Data File : P0113021.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 18 Aug 2025 15:23
 Operator : YP/AJ
 Sample : AR1254ICC750
 Misc :
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 AR1254ICC750

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 19 05:26:24 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0081825.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Aug 19 05:25:15 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.663	3.655	626.2E6	380.0E6	75.299	75.114
2) SA Decachlor...	8.682	8.627	549.8E6	144.5E6	73.810	73.238
Target Compounds						
26) L6 AR-1254-1	5.553	5.526	386.5E6	227.1E6	733.198	728.784
27) L6 AR-1254-2	5.702	5.674	348.3E6	199.6E6	725.877	721.726
28) L6 AR-1254-3	6.105	6.074	545.9E6	306.0E6	738.816	735.459
29) L6 AR-1254-4	6.335	6.302	411.4E6	201.5E6	743.727	736.386
30) L6 AR-1254-5	6.753	6.717	523.4E6	253.4E6	745.575	720.993



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO081825\
Data File : PO113021.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 18 Aug 2025 15:23
Operator : YP/AJ
Sample : AR1254ICC750
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
AR1254ICC750

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 19 05:26:24 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO081825.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Aug 19 05:25:15 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µm Signal #2 Info : 30M x 0.32mm x 0.25µm

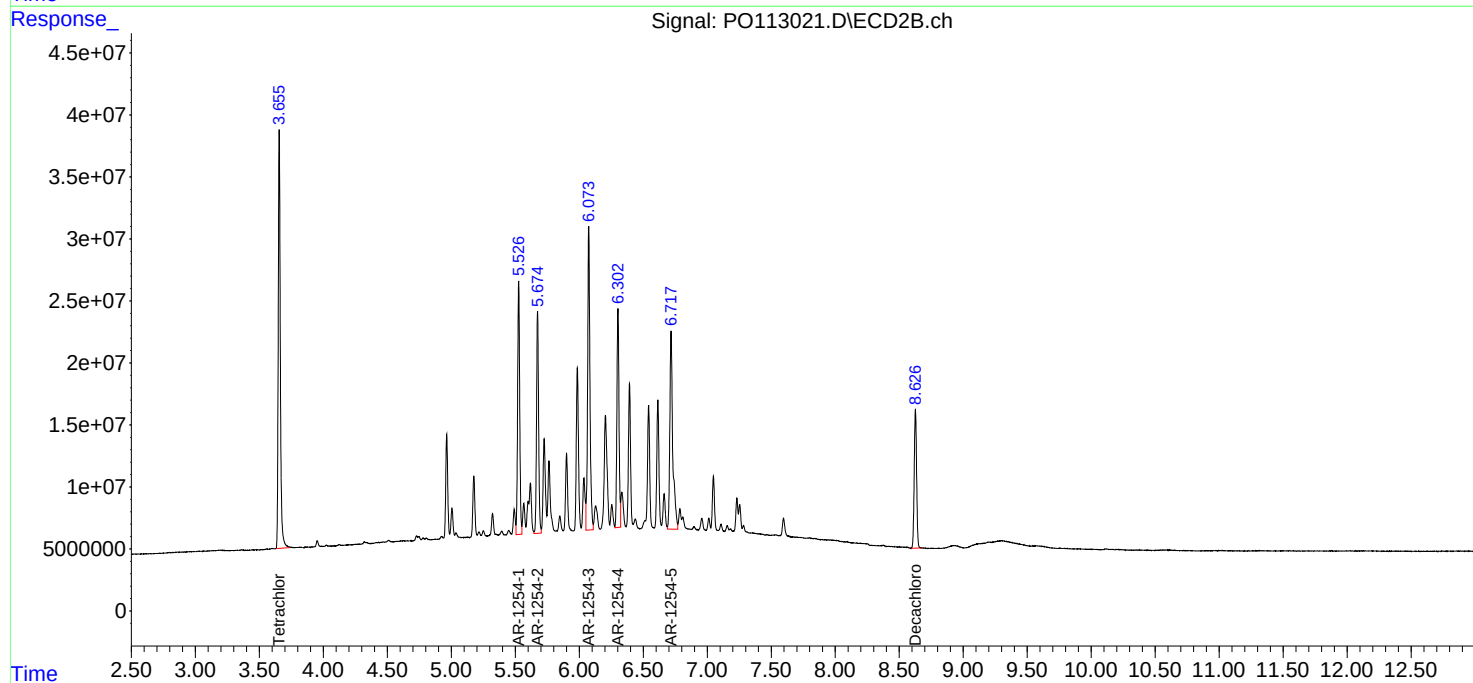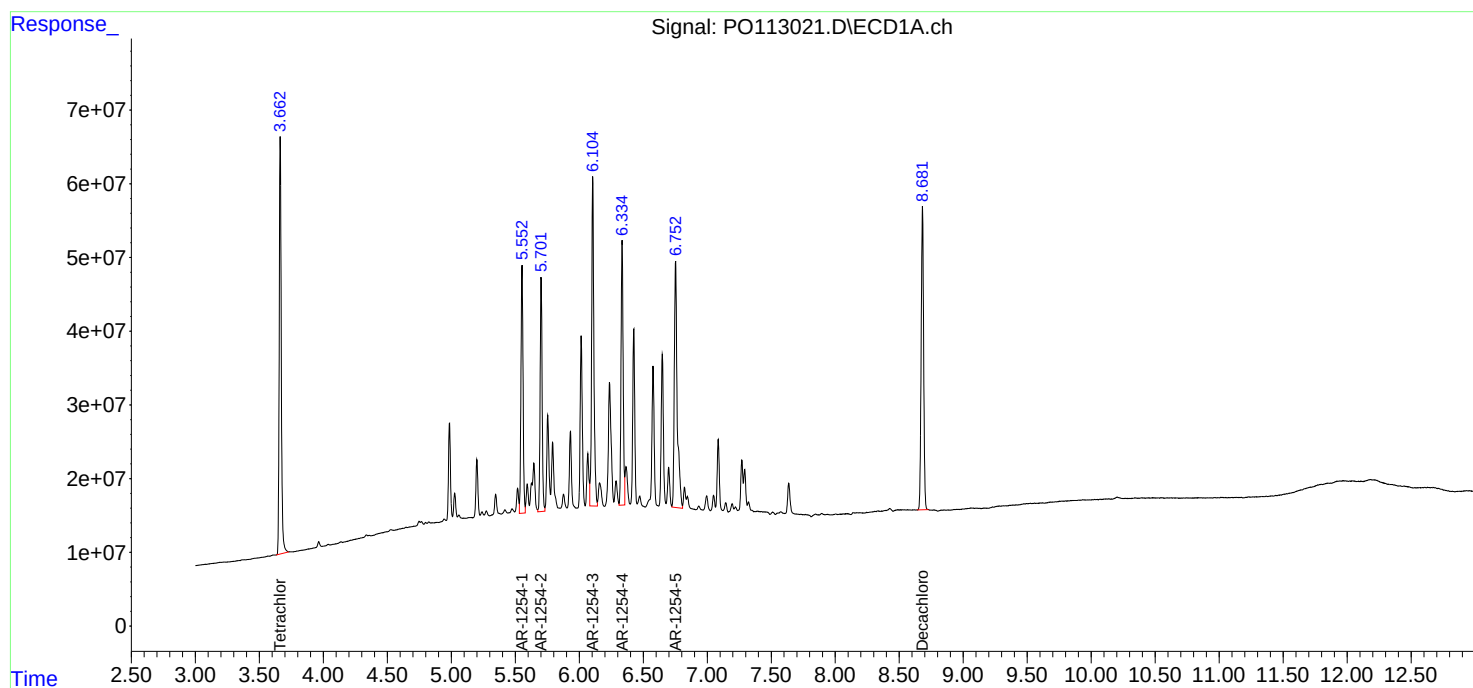

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0081825\
 Data File : P0113022.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 18 Aug 2025 15:41
 Operator : YP/AJ
 Sample : AR1254ICC500
 Misc :
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 AR1254ICC500

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 19 05:26:44 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0081825.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Aug 19 05:25:15 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.664	3.655	415.8E6	253.0E6	50.000	50.000
2) SA Decachlor...	8.682	8.628	372.4E6	98659064	50.000	50.000
Target Compounds						
26) L6 AR-1254-1	5.553	5.526	263.6E6	155.8E6	500.000	500.000
27) L6 AR-1254-2	5.703	5.674	239.9E6	138.3E6	500.000	500.000
28) L6 AR-1254-3	6.106	6.074	369.4E6	208.0E6	500.000	500.000
29) L6 AR-1254-4	6.335	6.302	276.6E6	136.8E6	500.000	500.000
30) L6 AR-1254-5	6.753	6.717	351.0E6	175.8E6	500.000	500.000



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO081825\
Data File : PO113022.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 18 Aug 2025 15:41
Operator : YP/AJ
Sample : AR1254ICC500
Misc :
ALS Vial : 22 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
AR1254ICC500

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 19 05:26:44 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO081825.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Aug 19 05:25:15 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µm Signal #2 Info : 30M x 0.32mm x 0.25µm

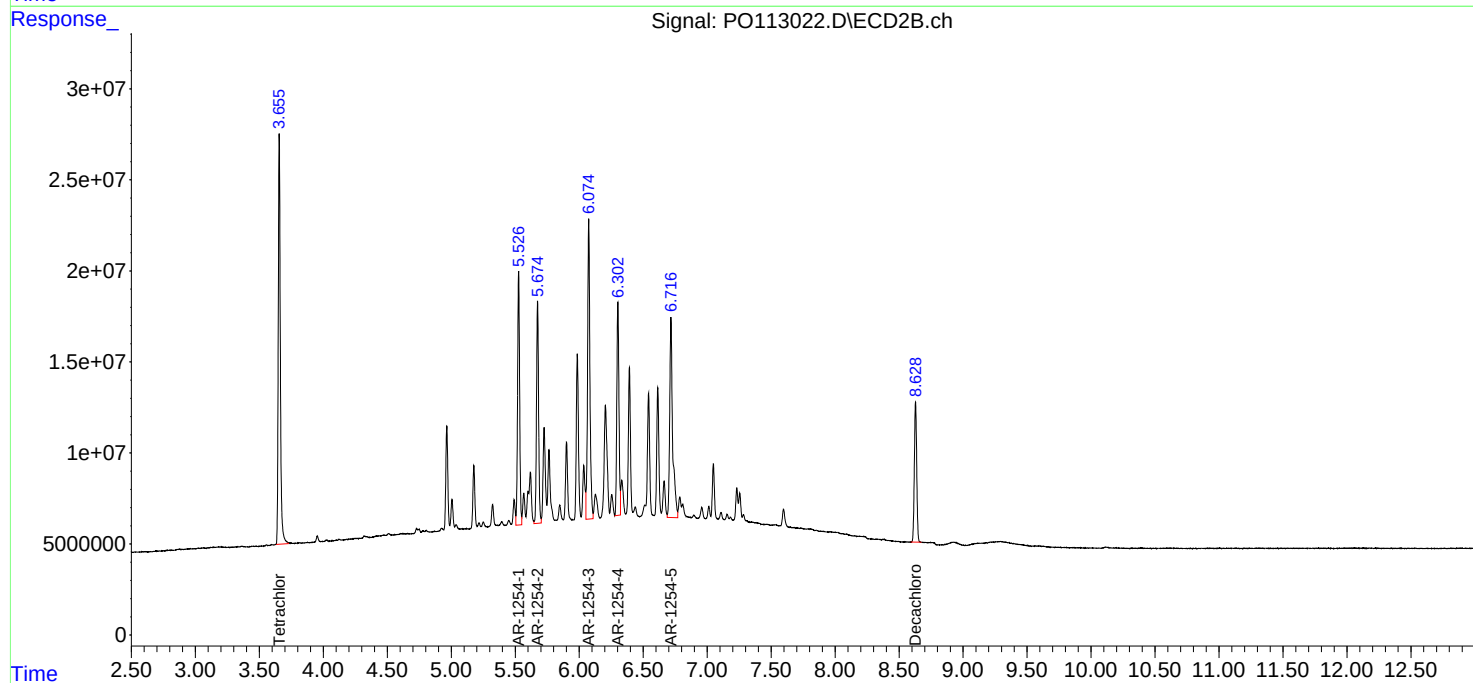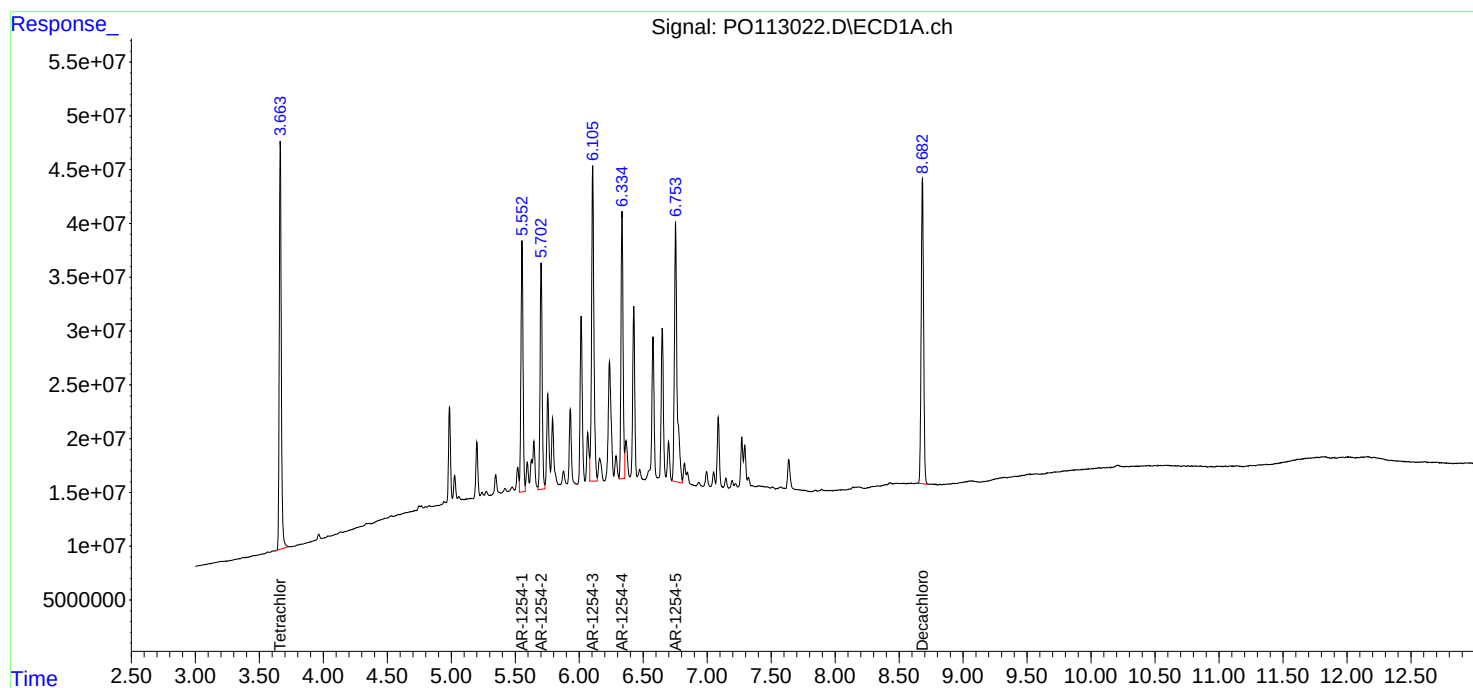

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0081825\
 Data File : P0113023.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 18 Aug 2025 16:00
 Operator : YP/AJ
 Sample : AR1254ICC250
 Misc :
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 AR1254ICC250

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 19 05:27:08 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0081825.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Aug 19 05:25:15 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.664	3.655	214.7E6	131.0E6	25.812	25.901
2) SA Decachlor...	8.683	8.628	190.8E6	50985128	25.612	25.839
Target Compounds						
26) L6 AR-1254-1	5.552	5.526	140.8E6	84054640	267.180	269.741
27) L6 AR-1254-2	5.702	5.674	128.2E6	75903732	267.296	274.413
28) L6 AR-1254-3	6.105	6.074	194.5E6	111.6E6	263.210	268.245
29) L6 AR-1254-4	6.335	6.301	144.8E6	72285443	261.698	264.202
30) L6 AR-1254-5	6.753	6.717	185.2E6	92940208	263.747	264.394



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO081825\
Data File : PO113023.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 18 Aug 2025 16:00
Operator : YP/AJ
Sample : AR1254ICC250
Misc :
ALS Vial : 23 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
AR1254ICC250

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 19 05:27:08 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO081825.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Aug 19 05:25:15 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µm Signal #2 Info : 30M x 0.32mm x 0.25µm

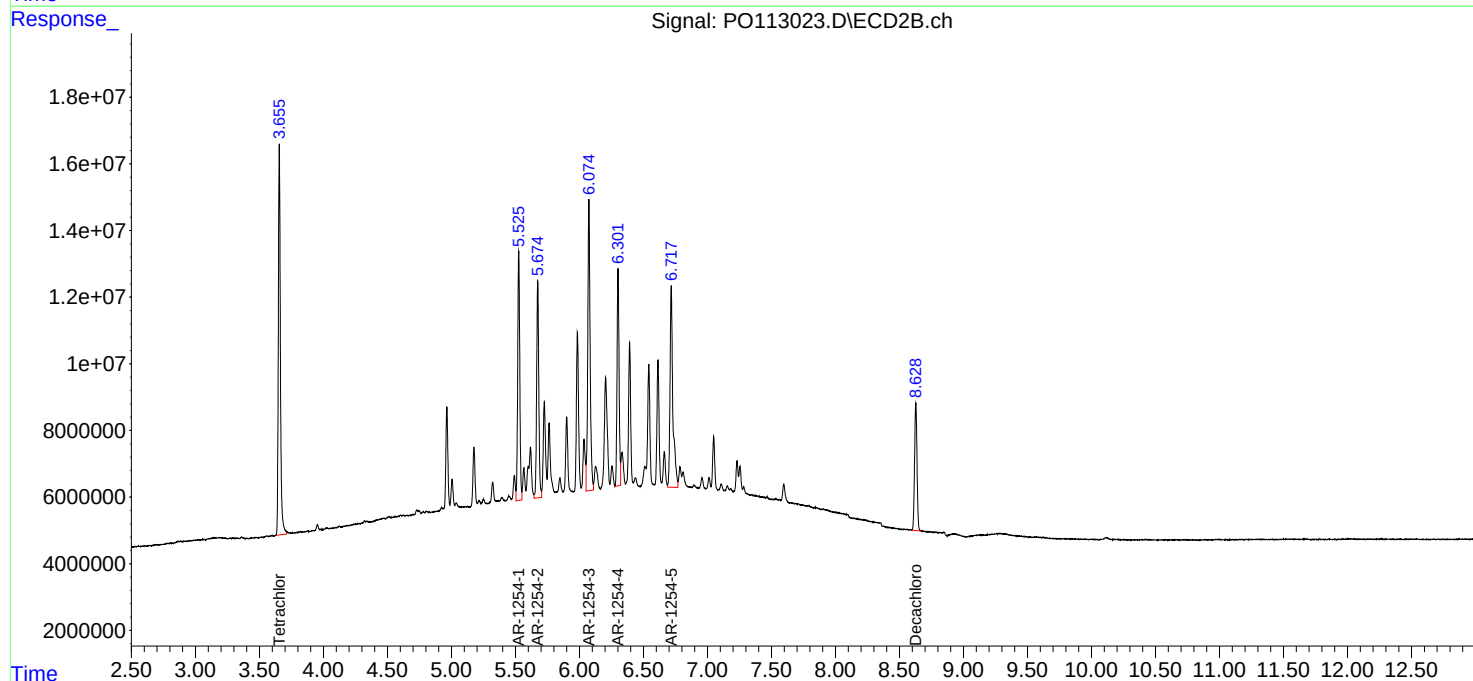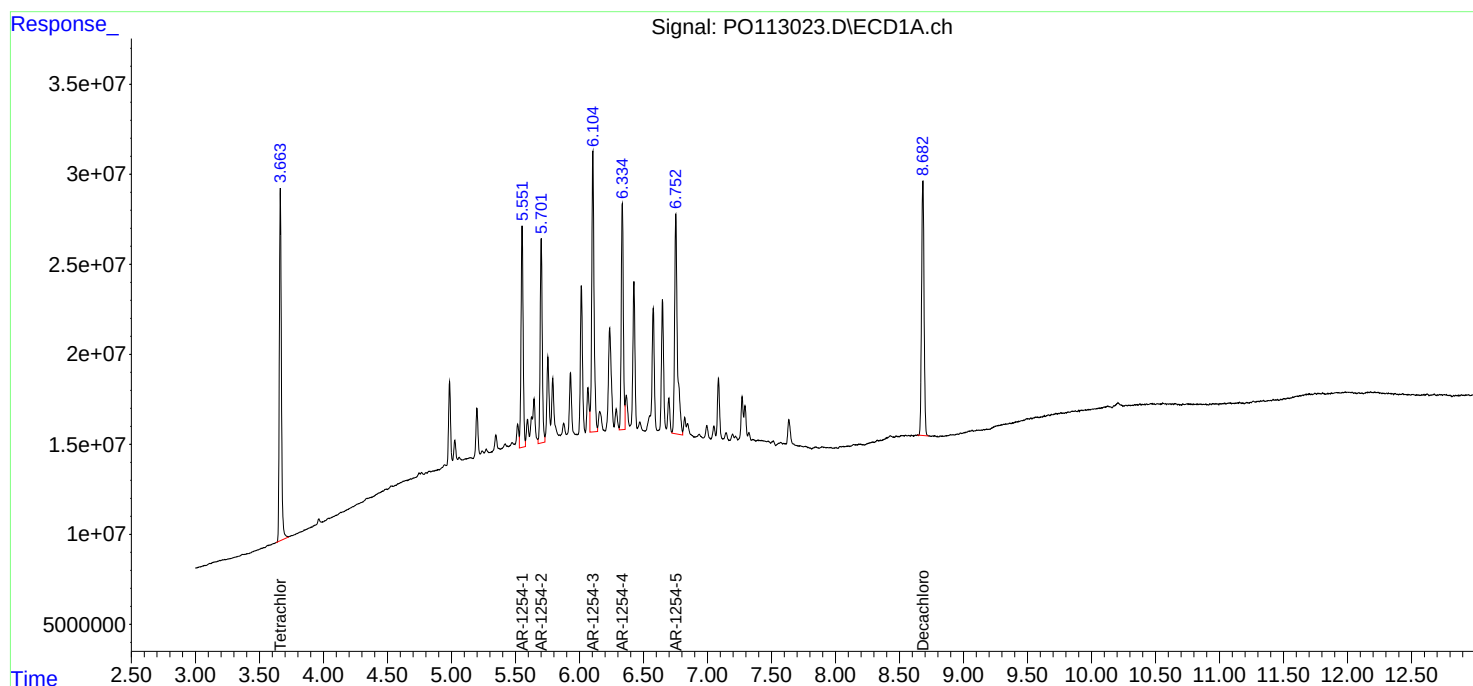

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_0\Data\P0081825\
 Data File : P0113024.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 18 Aug 2025 16:18
 Operator : YP/AJ
 Sample : AR1254ICC050
 Misc :
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 ECD_0
 ClientSampleId :
 AR1254ICC050

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 08/19/2025
 Supervised By :mohammad ahmed 08/20/2025

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 19 05:27:31 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_0\methods\P0081825.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Aug 19 05:25:15 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.663	3.655	36489191	23352844	4.388	4.616
2) SA Decachlor...	8.682	8.627	33466642	9234843	4.493	4.680
Target Compounds						
26) L6 AR-1254-1	5.553	5.525	29721929	16864555	56.381	54.120m
27) L6 AR-1254-2	5.702	5.673	27777860	15014303	57.898	54.281m
28) L6 AR-1254-3	6.105	6.073	36941091	20976378	50.000	50.419m
29) L6 AR-1254-4	6.335	6.302	28558766	14228719	51.627	52.006
30) L6 AR-1254-5	6.753	6.717	33818216	20038217	48.173	57.004

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO081825\
Data File : PO113024.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 18 Aug 2025 16:18
Operator : YP/AJ
Sample : AR1254ICC050
Misc :
ALS Vial : 24 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
AR1254ICC050

Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 08/19/2025
Supervised By :mohammad ahmed 08/20/2025

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 19 05:27:31 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO081825.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Aug 19 05:25:15 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µm Signal #2 Info : 30M x 0.32mm x 0.25µm

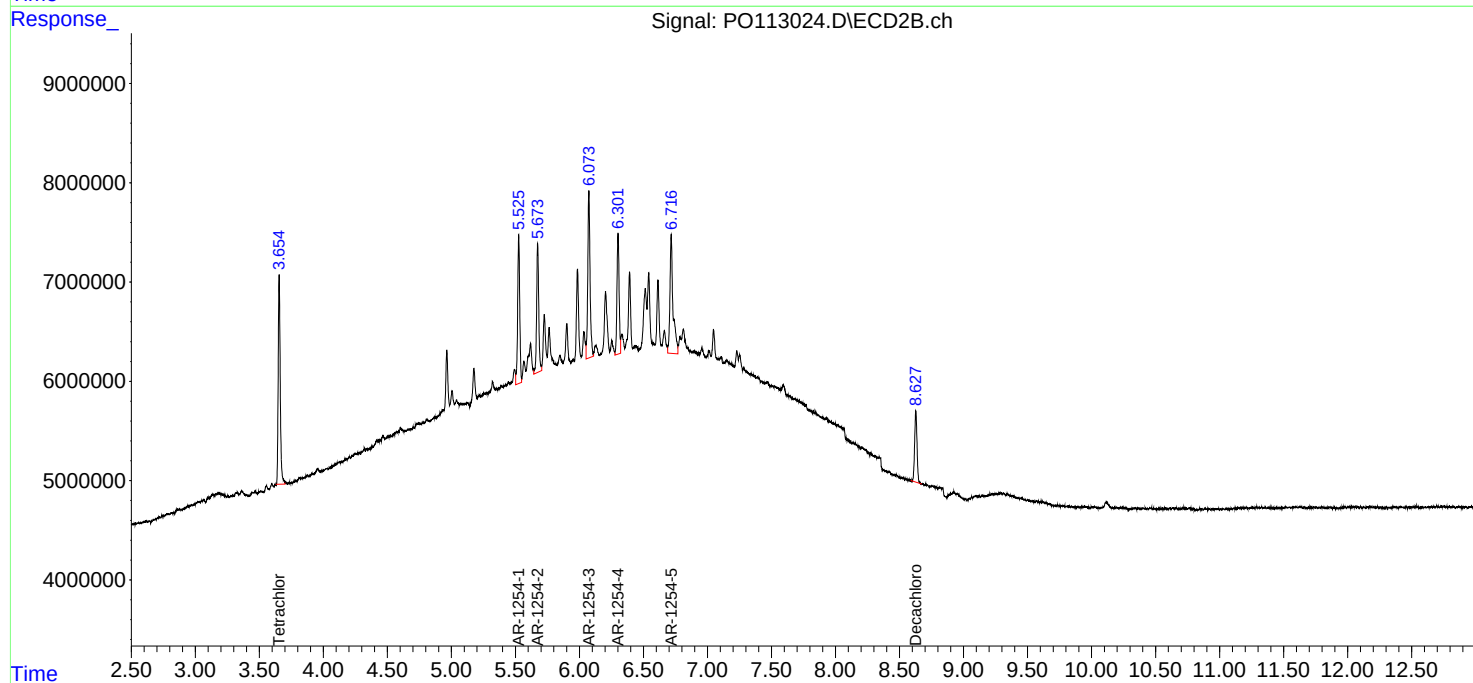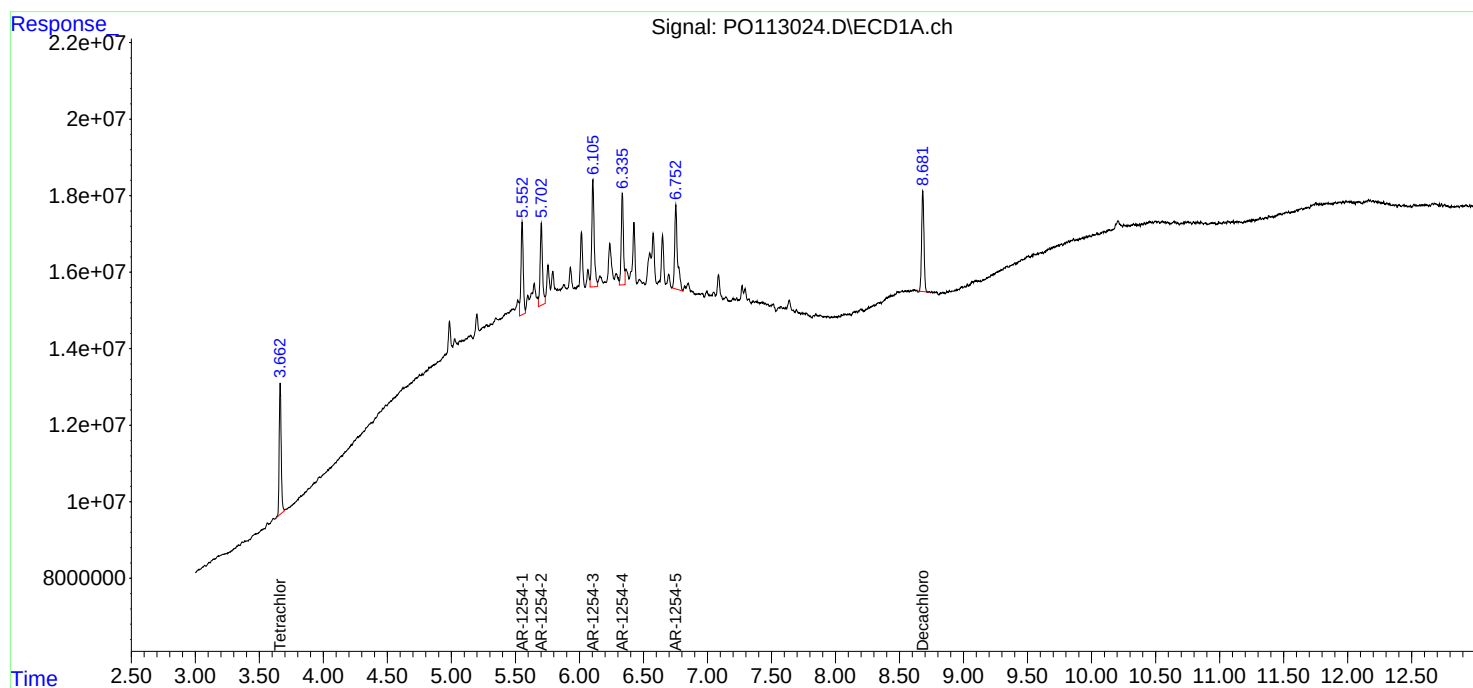

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0081825\
 Data File : P0113025.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 18 Aug 2025 16:54
 Operator : YP/AJ
 Sample : AR1262ICC500
 Misc :
 ALS Vial : 25 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 AR1262ICC500

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 19 05:39:43 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0081825.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Aug 19 05:39:26 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.662	3.656	406.7E6	247.5E6	50.000	50.000
2) SA Decachlor...	8.680	8.628	369.8E6	97697594	50.000	50.000
Target Compounds						
36) L8 AR-1262-1	6.790	6.755	457.9E6	207.3E6	500.000	500.000
37) L8 AR-1262-2	7.292	7.255	756.1E6	258.8E6	500.000	500.000
38) L8 AR-1262-3	7.575	7.536	277.1E6	89795239	500.000	500.000
39) L8 AR-1262-4	7.639	7.600	489.0E6	145.0E6	500.000	500.000
40) L8 AR-1262-5	8.135	8.092	208.4E6	54165644	500.000	500.000



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO081825\
Data File : PO113025.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 18 Aug 2025 16:54
Operator : YP/AJ
Sample : AR1262ICC500
Misc :
ALS Vial : 25 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
AR1262ICC500

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 19 05:39:43 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO081825.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Aug 19 05:39:26 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

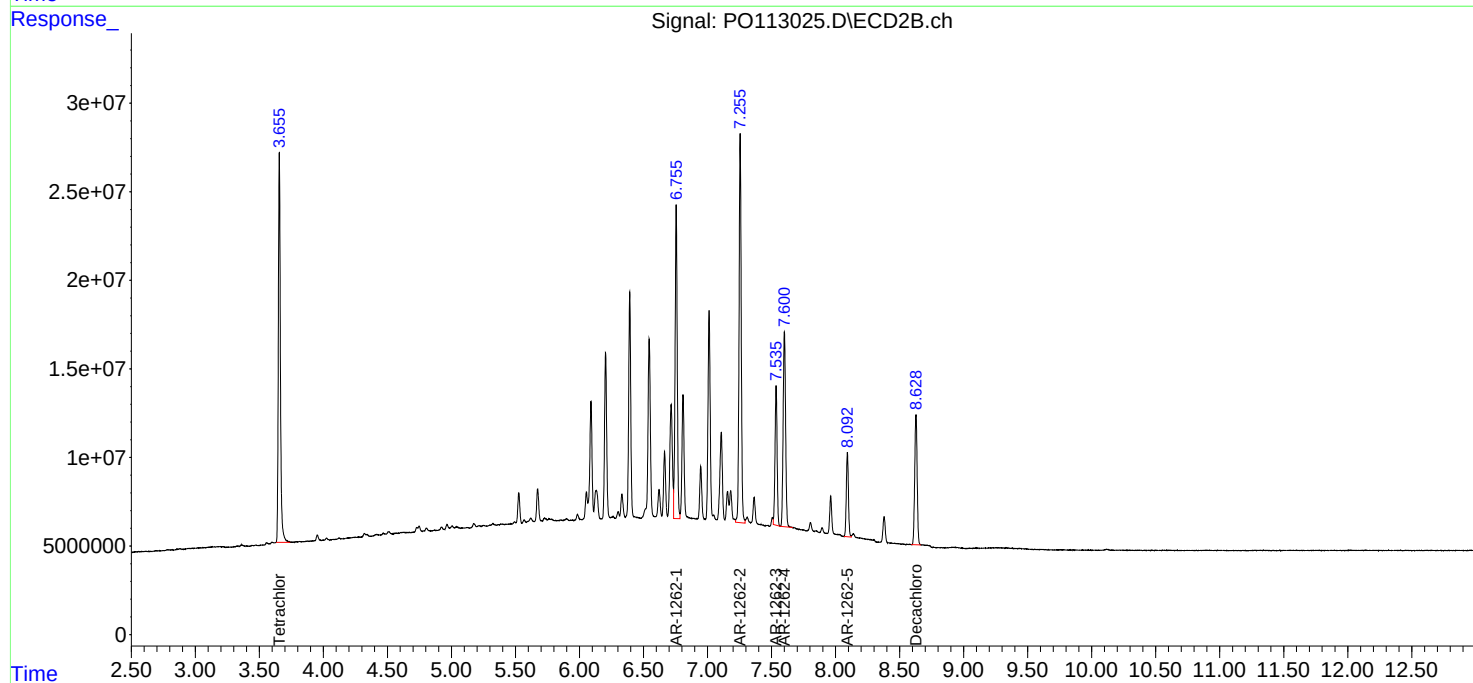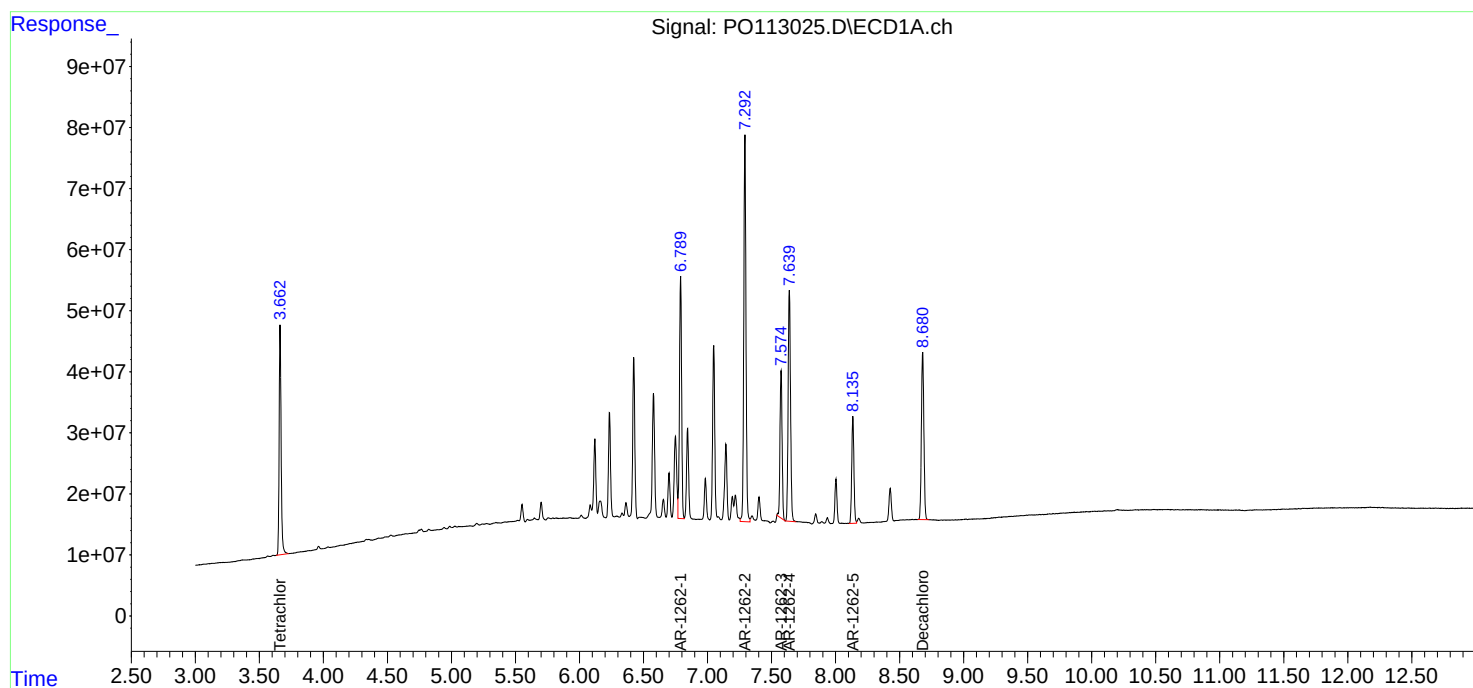

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0081825\
 Data File : P0113026.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 18 Aug 2025 17:12
 Operator : YP/AJ
 Sample : AR1268ICC1000
 Misc :
 ALS Vial : 26 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 AR1268ICC1000

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 19 05:48:40 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0081825.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Aug 19 05:48:08 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.664	3.656	838.3E6	509.2E6	98.889	99.430
2) SA Decachlor...	8.682	8.627	1357.3E6	346.9E6	97.480	96.565
Target Compounds						
41) L9 AR-1268-1	7.577	7.537	1761.0E6	505.3E6	976.230	954.513
42) L9 AR-1268-2	7.642	7.602	1477.2E6	411.8E6	973.638	954.016
43) L9 AR-1268-3	7.846	7.805	1233.6E6	321.7E6	970.801	947.705
44) L9 AR-1268-4	8.137	8.092	475.8E6	120.3E6	998.193	977.393
45) L9 AR-1268-5	8.428	8.379	3340.5E6	793.7E6	996.727	976.596



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO081825\
Data File : PO113026.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 18 Aug 2025 17:12
Operator : YP/AJ
Sample : AR1268ICC1000
Misc :
ALS Vial : 26 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
AR1268ICC1000

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 19 05:48:40 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO081825.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Aug 19 05:48:08 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

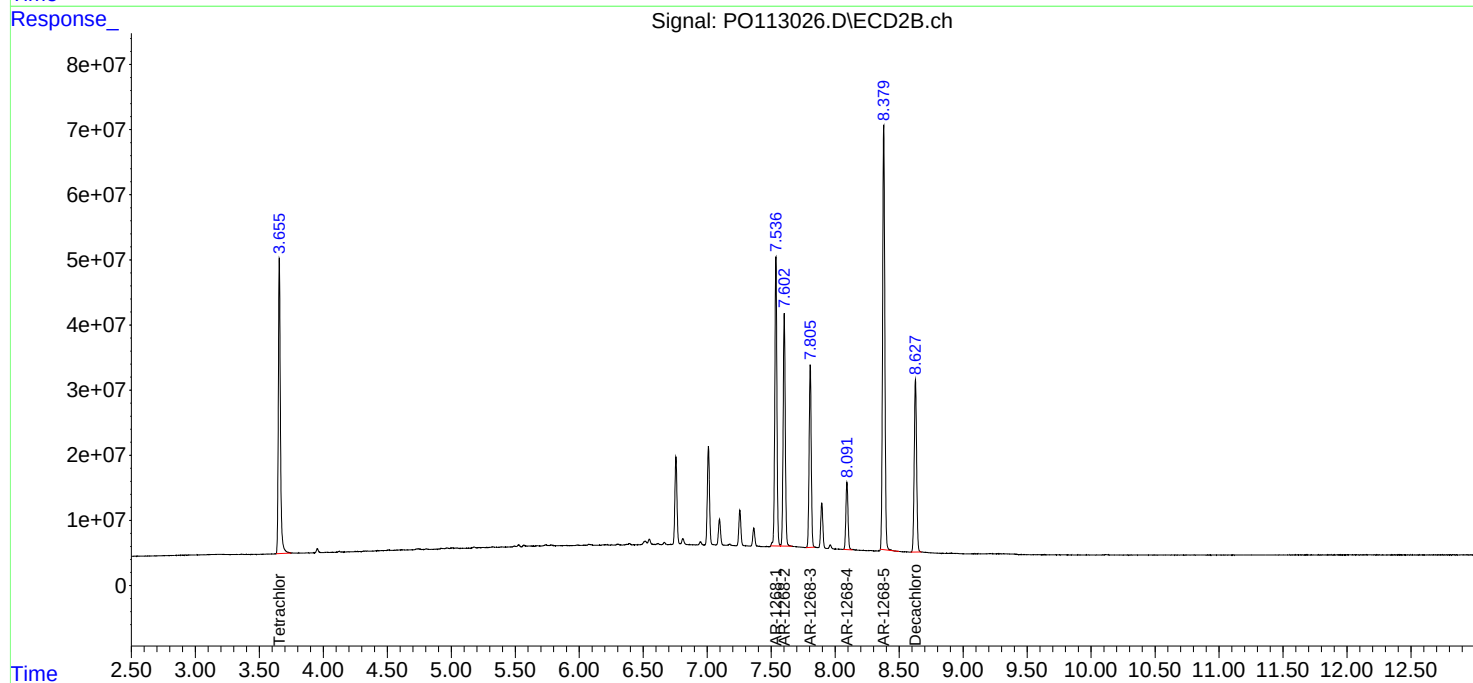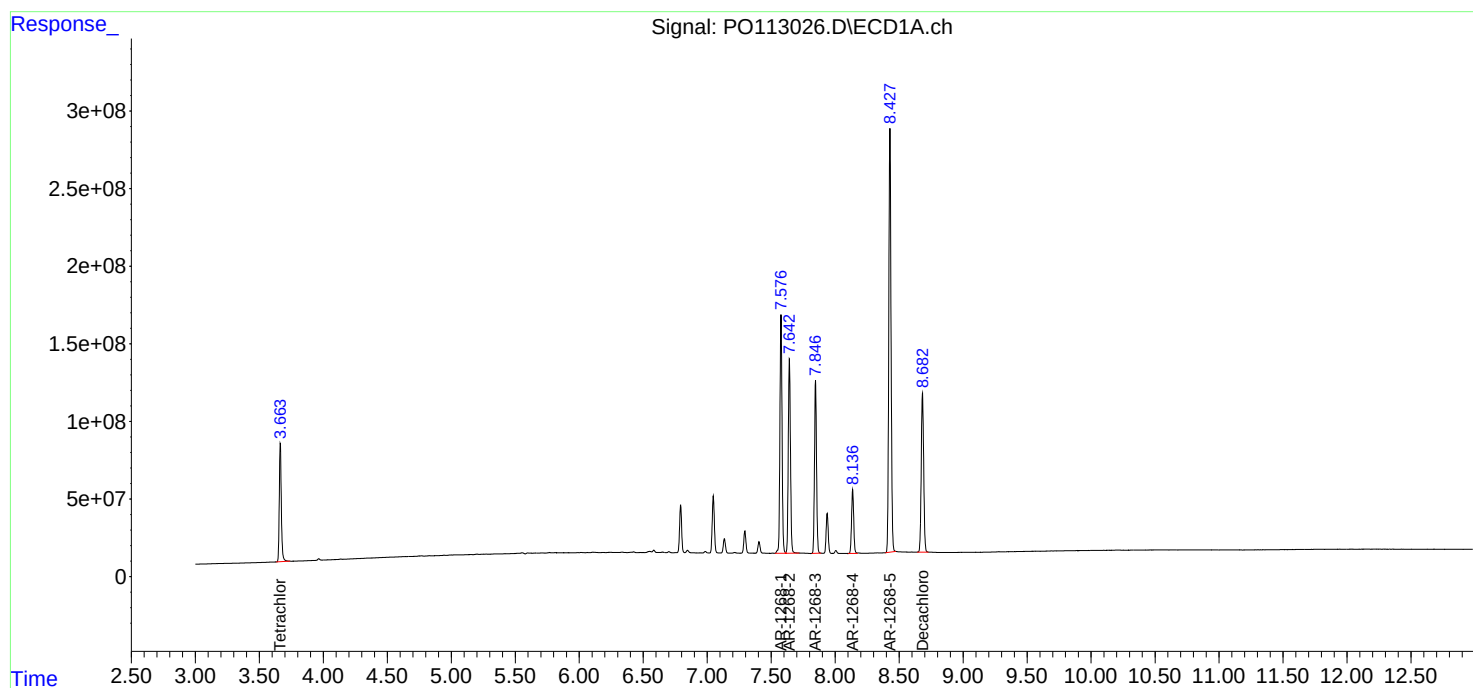

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0081825\
 Data File : P0113027.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 18 Aug 2025 17:30
 Operator : YP/AJ
 Sample : AR1268ICC750
 Misc :
 ALS Vial : 27 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 AR1268ICC750

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 19 05:49:00 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0081825.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Aug 19 05:48:08 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.661	3.655	635.0E6	385.8E6	74.903	75.334
2) SA Decachlor...	8.679	8.626	1024.0E6	262.4E6	73.544	73.041
Target Compounds						
41) L9 AR-1268-1	7.573	7.535	1330.9E6	375.0E6	737.820	708.257
42) L9 AR-1268-2	7.639	7.601	1119.3E6	306.5E6	737.779	709.930
43) L9 AR-1268-3	7.844	7.804	934.0E6	240.8E6	734.989	709.221
44) L9 AR-1268-4	8.133	8.092	359.4E6	91683621	754.004	744.876
45) L9 AR-1268-5	8.426	8.378	2501.0E6	597.6E6	746.242	735.293



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO081825\
Data File : PO113027.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 18 Aug 2025 17:30
Operator : YP/AJ
Sample : AR1268ICC750
Misc :
ALS Vial : 27 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
AR1268ICC750

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 19 05:49:00 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO081825.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Aug 19 05:48:08 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

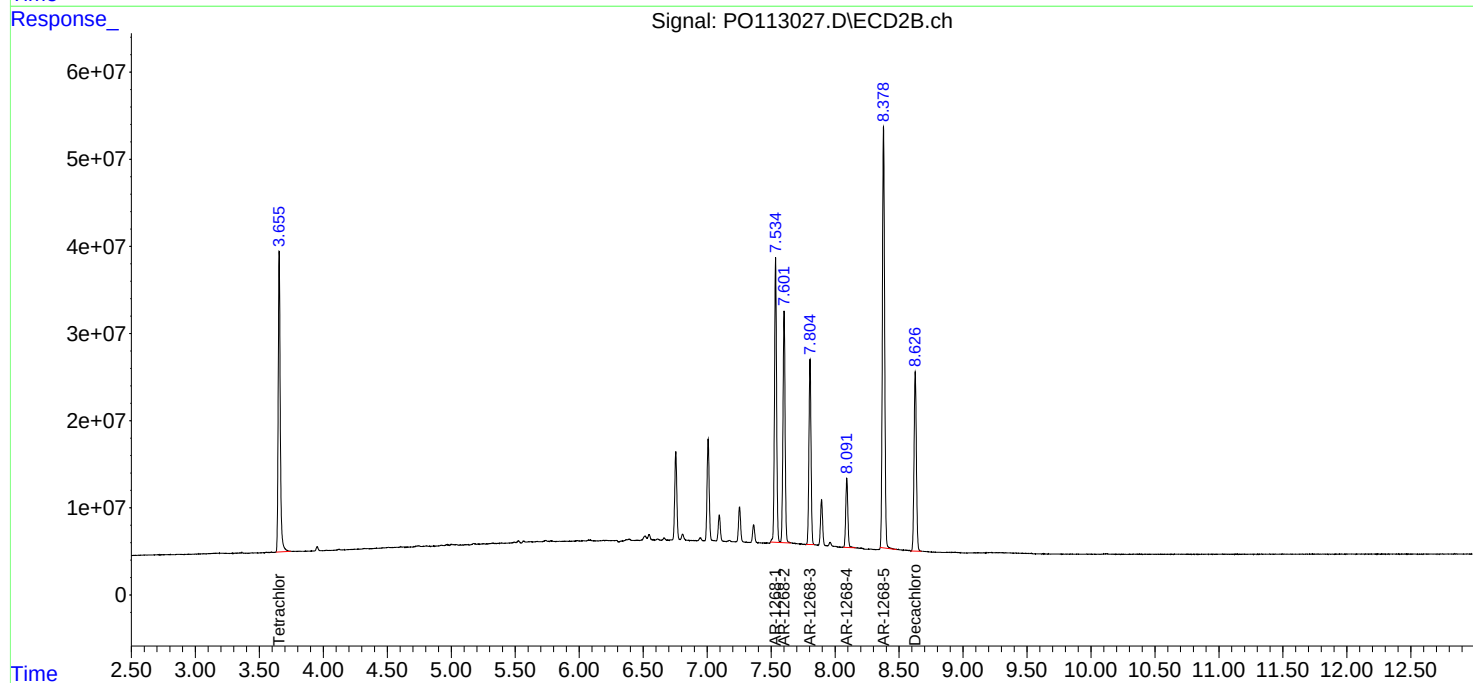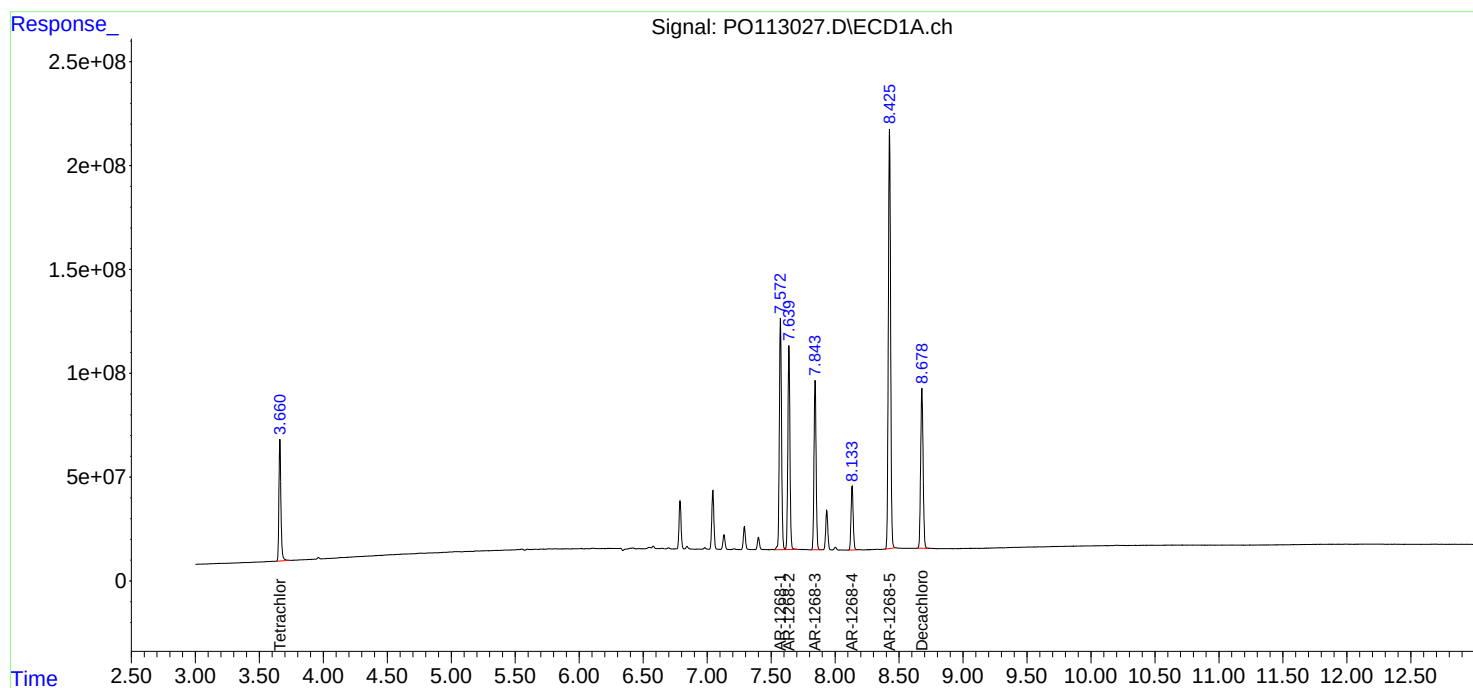

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0081825\
 Data File : P0113028.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 18 Aug 2025 17:48
 Operator : YP/AJ
 Sample : AR1268ICC500
 Misc :
 ALS Vial : 28 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 AR1268ICC500

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 19 05:49:21 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0081825.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Aug 19 05:48:08 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.663	3.655	423.9E6	256.0E6	50.000	50.000
2) SA Decachlor...	8.682	8.628	696.2E6	179.6E6	50.000	50.000
Target Compounds						
41) L9 AR-1268-1	7.575	7.536	901.9E6	264.7E6	500.000	500.000
42) L9 AR-1268-2	7.641	7.602	758.6E6	215.8E6	500.000	500.000
43) L9 AR-1268-3	7.846	7.805	635.4E6	169.7E6	500.000	500.000
44) L9 AR-1268-4	8.136	8.092	238.3E6	61542864	500.000	500.000
45) L9 AR-1268-5	8.428	8.379	1675.8E6	406.3E6	500.000	500.000



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO081825\
Data File : PO113028.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 18 Aug 2025 17:48
Operator : YP/AJ
Sample : AR1268ICC500
Misc :
ALS Vial : 28 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
AR1268ICC500

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 19 05:49:21 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO081825.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Aug 19 05:48:08 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

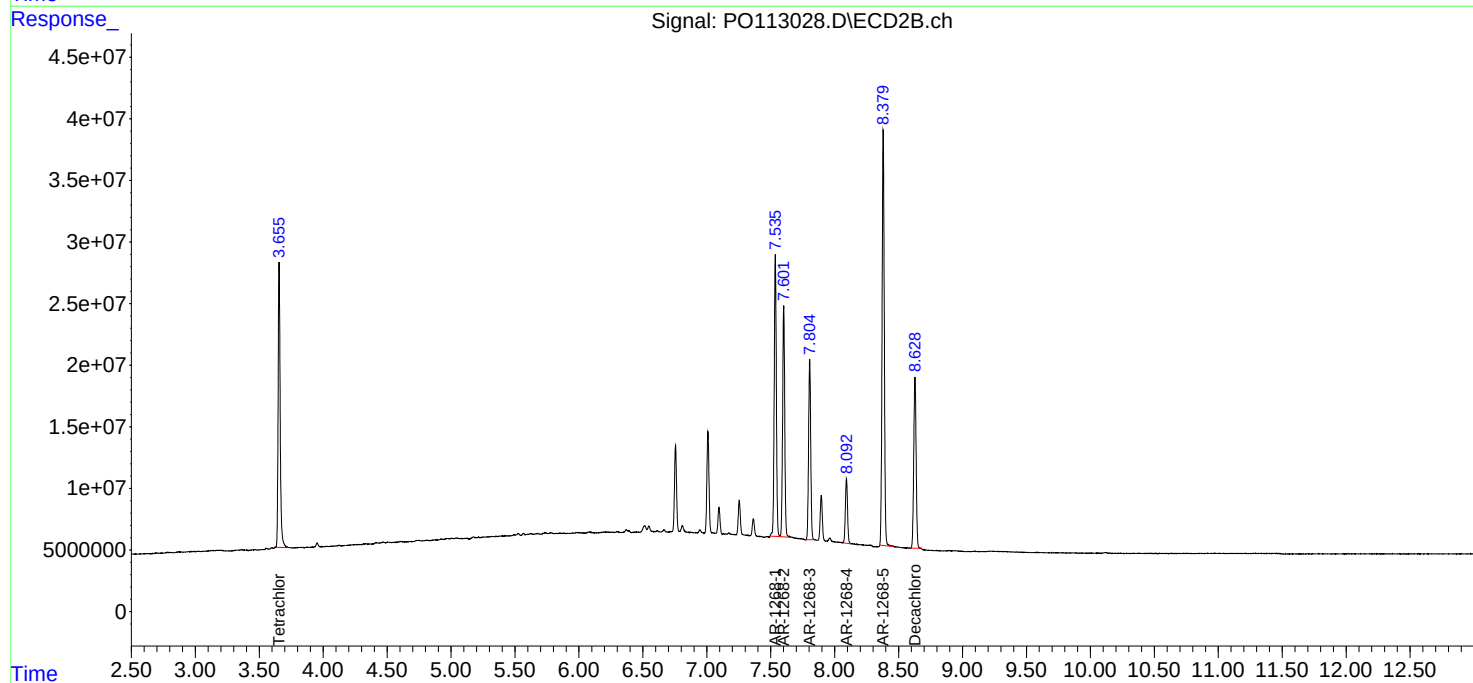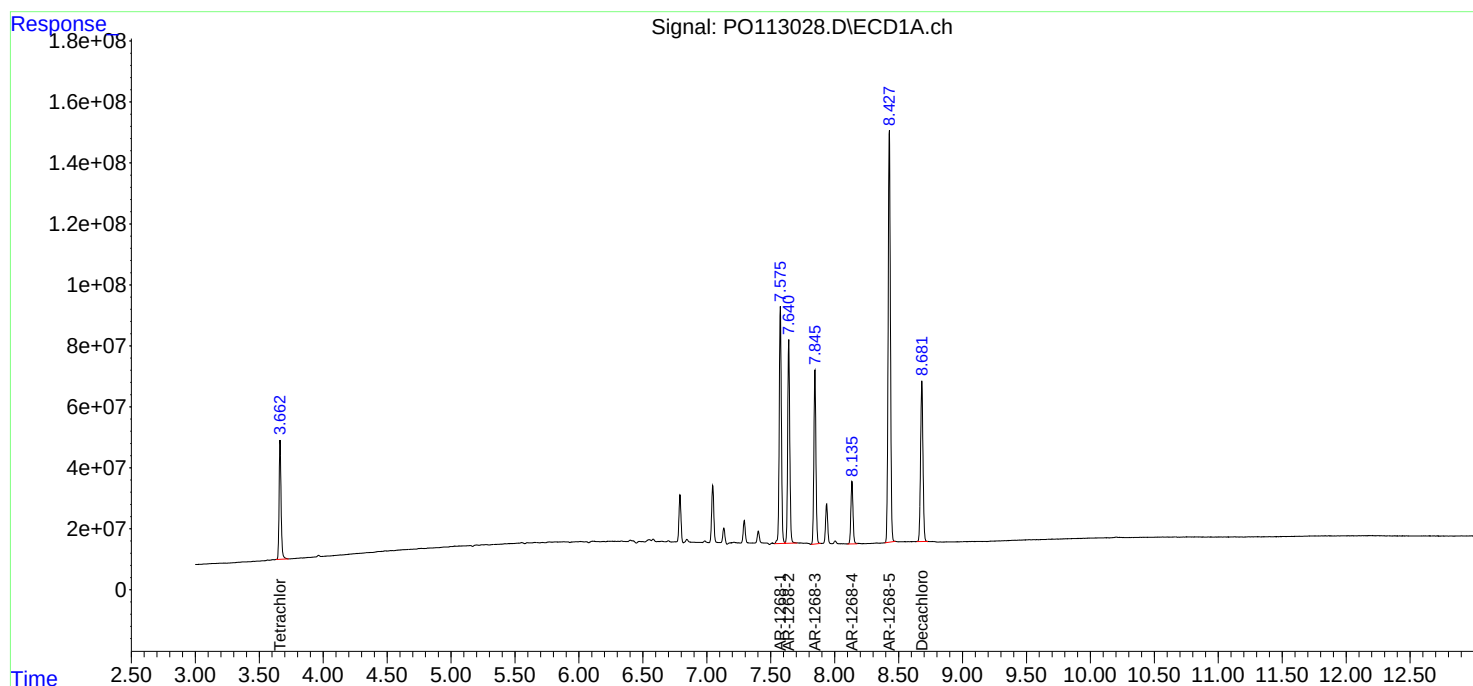

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0081825\
 Data File : P0113029.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 18 Aug 2025 18:06
 Operator : YP/AJ
 Sample : AR1268ICC250
 Misc :
 ALS Vial : 29 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 AR1268ICC250

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 19 05:49:41 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0081825.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Aug 19 05:48:08 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.662	3.655	218.2E6	134.2E6	25.738	26.208
2) SA Decachlor...	8.680	8.627	354.7E6	93434698	25.474	26.012
Target Compounds						
41) L9 AR-1268-1	7.575	7.535	460.2E6	137.9E6	255.114	260.436
42) L9 AR-1268-2	7.640	7.601	386.9E6	111.5E6	255.045	258.314
43) L9 AR-1268-3	7.845	7.804	322.8E6	88262994	254.068	260.005
44) L9 AR-1268-4	8.134	8.091	123.3E6	32445037	258.588	263.597
45) L9 AR-1268-5	8.427	8.378	843.4E6	208.8E6	251.661	256.901



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO081825\
Data File : PO113029.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 18 Aug 2025 18:06
Operator : YP/AJ
Sample : AR1268ICC250
Misc :
ALS Vial : 29 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
AR1268ICC250

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 19 05:49:41 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO081825.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Aug 19 05:48:08 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

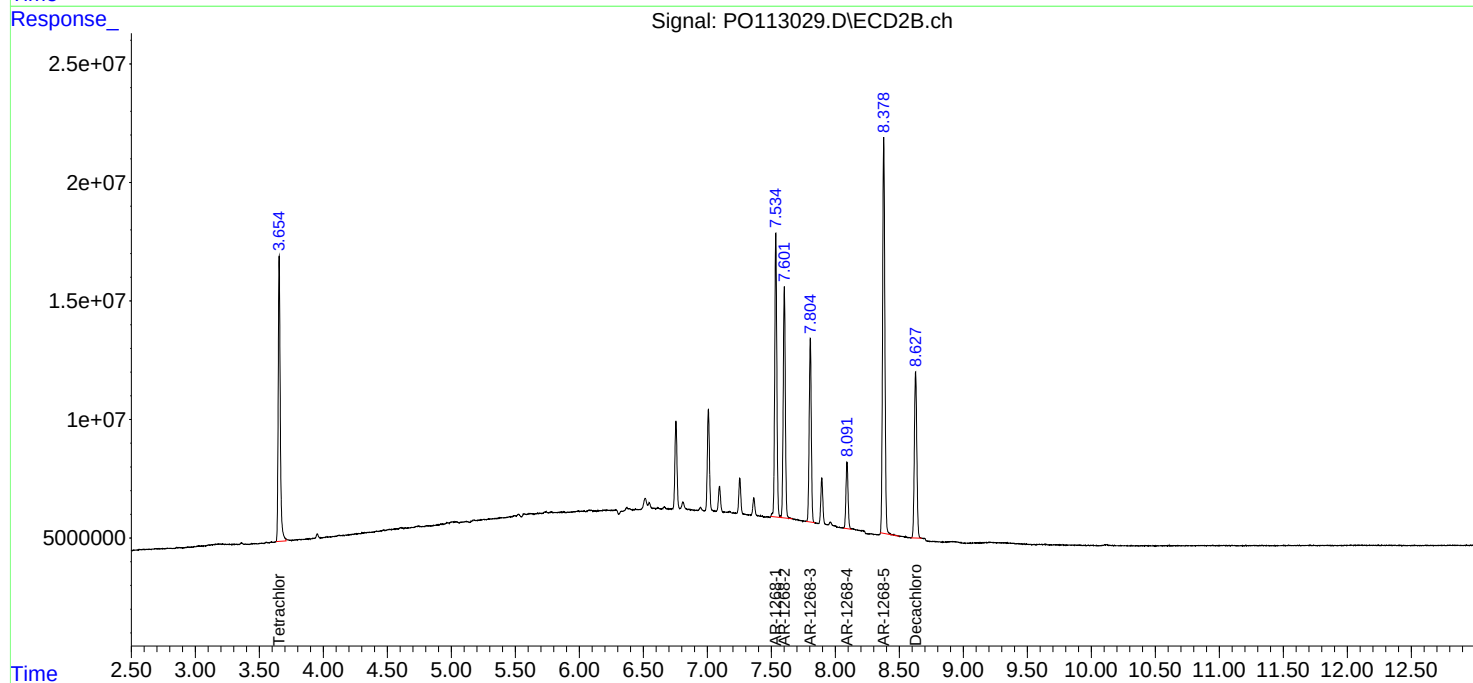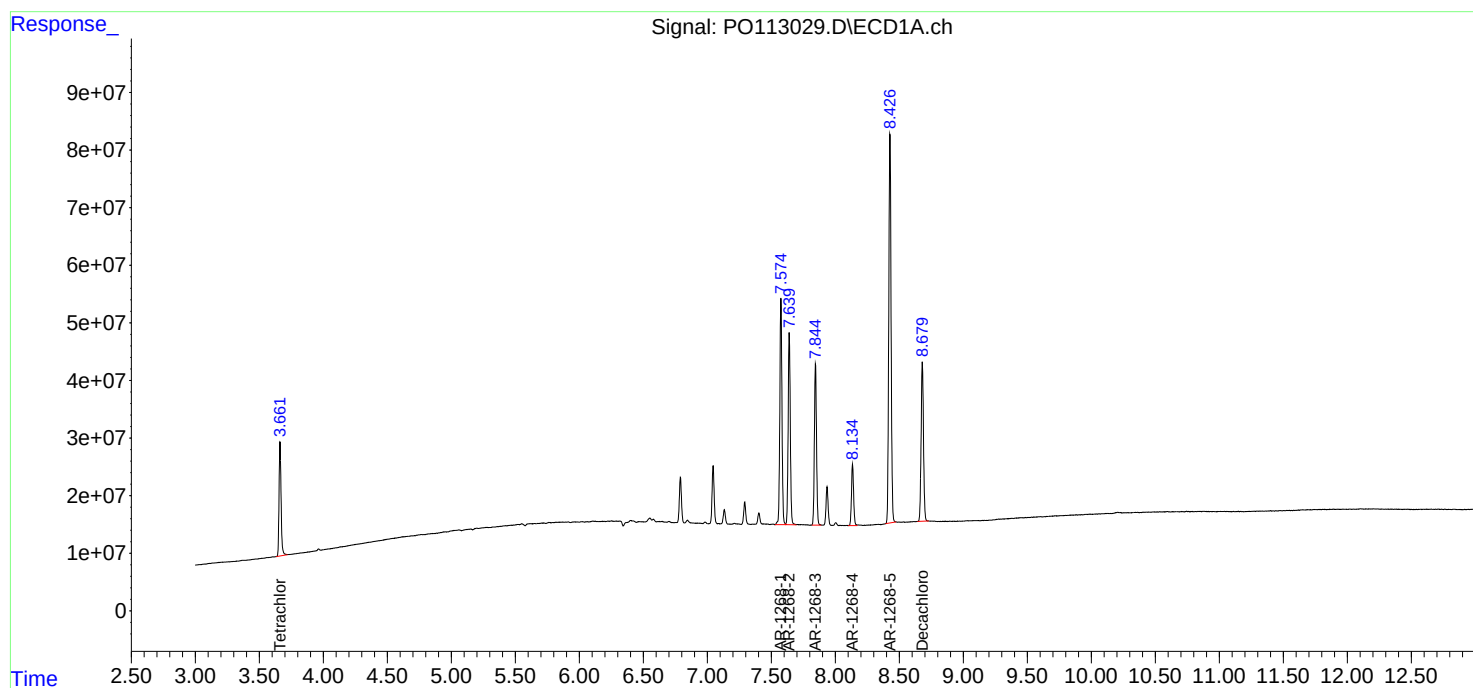

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0081825\
 Data File : P0113030.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 18 Aug 2025 18:24
 Operator : YP/AJ
 Sample : AR1268ICC050
 Misc :
 ALS Vial : 30 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 AR1268ICC050

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 08/19/2025
 Supervised By :mohammad ahmed 08/20/2025

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 19 05:50:03 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0081825.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Aug 19 05:48:08 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.663	3.656	32740210	20644764	3.862	4.031
2) SA Decachlor...	8.681	8.627	55179728	14960600	3.963	4.165
Target Compounds						
41) L9 AR-1268-1	7.575	7.535	71207184	23057642	39.474	43.554
42) L9 AR-1268-2	7.641	7.600	60309550	18942723	39.752	43.882
43) L9 AR-1268-3	7.845	7.803	49529084	14865130	38.977	43.790
44) L9 AR-1268-4	8.136	8.091	18929121	5337454	39.711	43.364
45) L9 AR-1268-5	8.426	8.378	127.1E6	33329844	37.916	41.012m

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO081825\
Data File : PO113030.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 18 Aug 2025 18:24
Operator : YP/AJ
Sample : AR1268ICC050
Misc :
ALS Vial : 30 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
AR1268ICC050

Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 08/19/2025
Supervised By :mohammad ahmed 08/20/2025

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 19 05:50:03 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO081825.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Aug 19 05:48:08 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µm Signal #2 Info : 30M x 0.32mm x 0.25µm

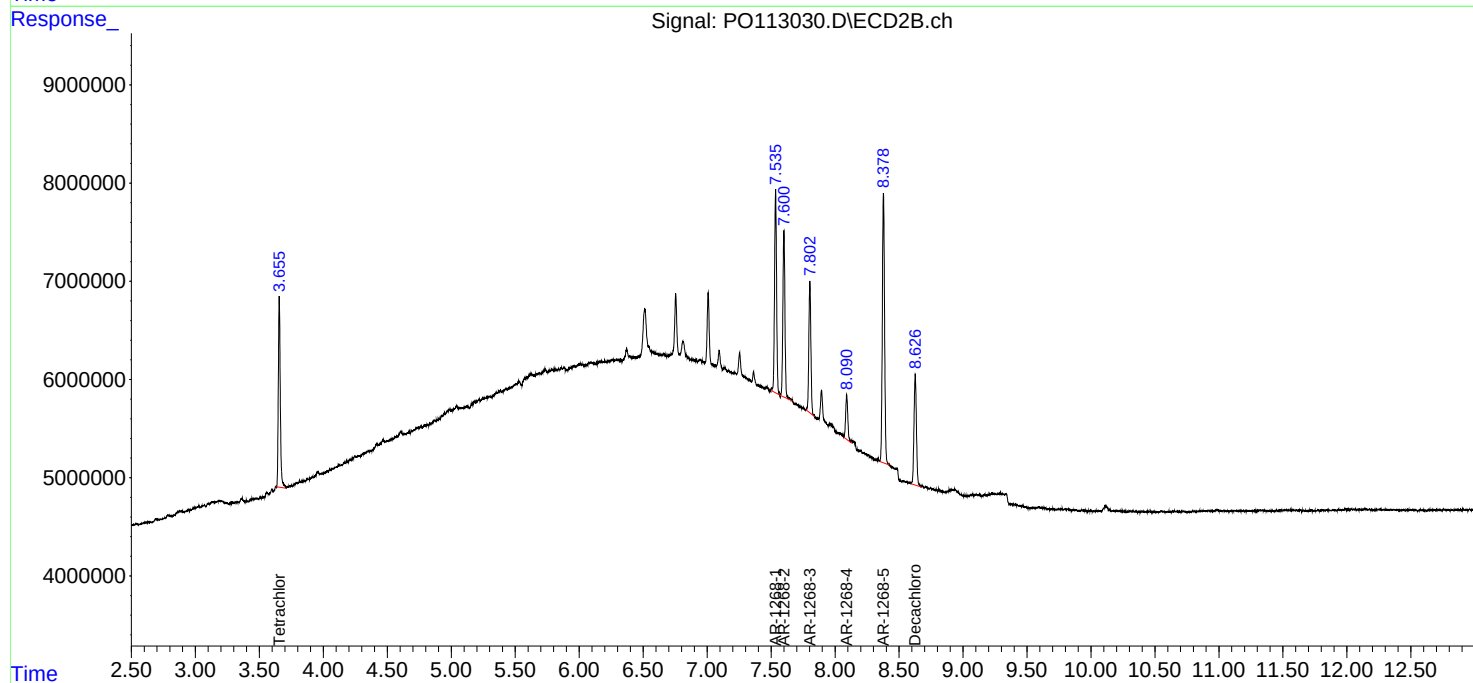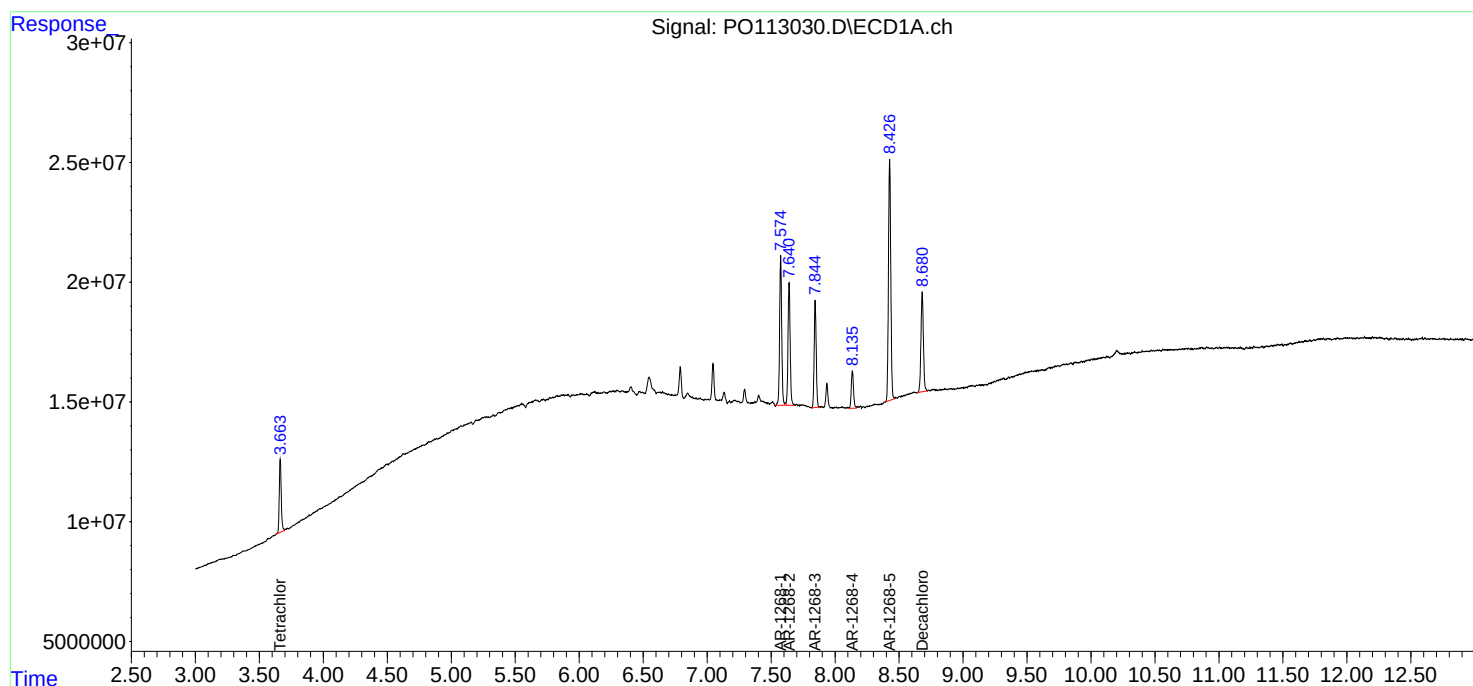

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0081825\
 Data File : P0113031.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 18 Aug 2025 18:43
 Operator : YP/AJ
 Sample : P0081825ICV500
 Misc :
 ALS Vial : 31 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 ICVPO081825

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 19 06:12:15 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0081825.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Aug 19 06:08:32 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.664	3.656	421.2E6	257.1E6	51.444	50.806
2)	SA Decachlor...	8.683	8.627	372.2E6	96647256	53.698	51.005
Target Compounds							
3)	L1 AR-1016-1	4.749	4.730	137.6E6	85391020	515.534	500.611
4)	L1 AR-1016-2	4.768	4.748	211.7E6	130.2E6	527.272	505.299
5)	L1 AR-1016-3	4.824	4.923	133.0E6	68472860	521.464	490.443
6)	L1 AR-1016-4	4.944	4.965	107.5E6	55300476	492.995	473.873
7)	L1 AR-1016-5	5.201	5.177	118.9E6	73202918	536.621	513.597
31)	L7 AR-1260-1	6.237	6.205	236.4E6	125.3E6	530.174	491.120
32)	L7 AR-1260-2	6.427	6.393	354.3E6	168.6E6	515.877	487.582
33)	L7 AR-1260-3	6.792	6.544	320.0E6	145.5E6	518.199	489.302
34)	L7 AR-1260-4	7.051	7.013	233.4E6	99741058	521.185	481.261
35)	L7 AR-1260-5	7.295	7.255	647.1E6	222.8E6	534.473	475.684



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO081825\
Data File : PO113031.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 18 Aug 2025 18:43
Operator : YP/AJ
Sample : PO081825ICV500
Misc :
ALS Vial : 31 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
ICVPO081825

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 19 06:12:15 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO081825.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Aug 19 06:08:32 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

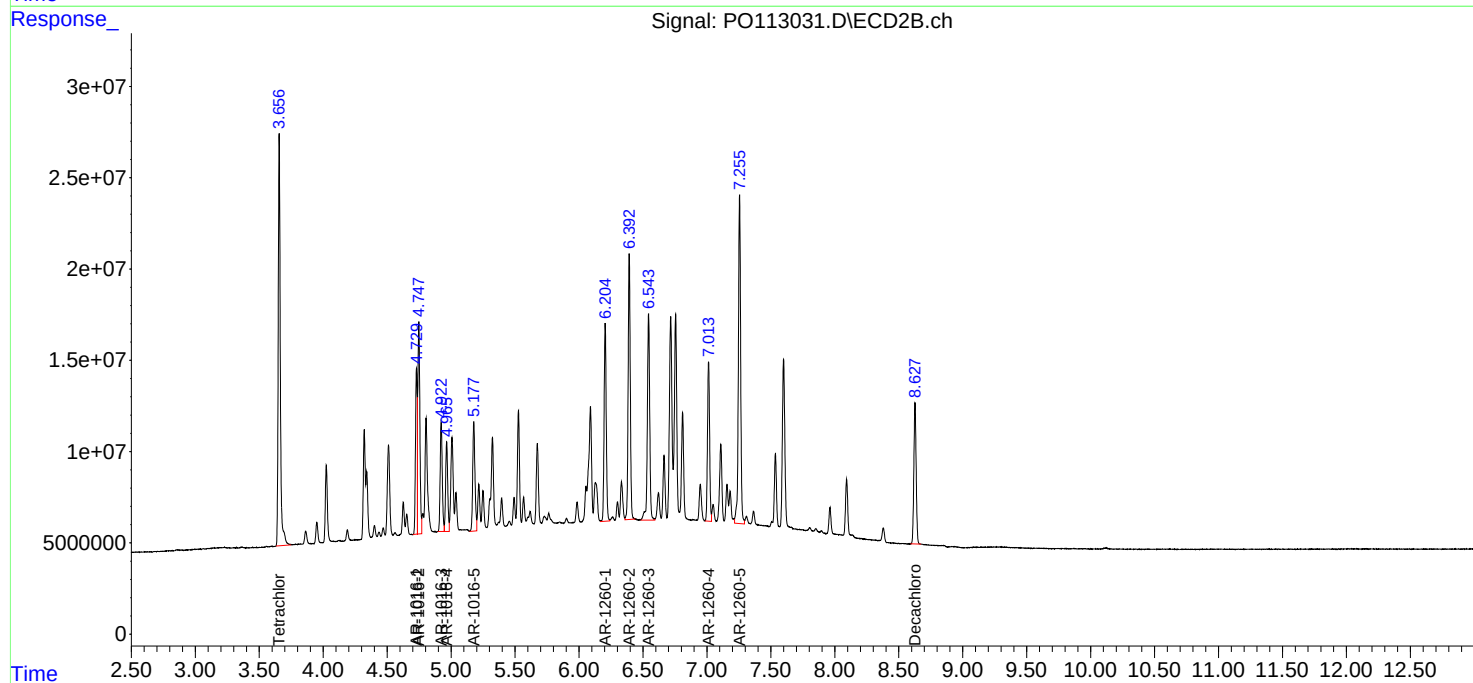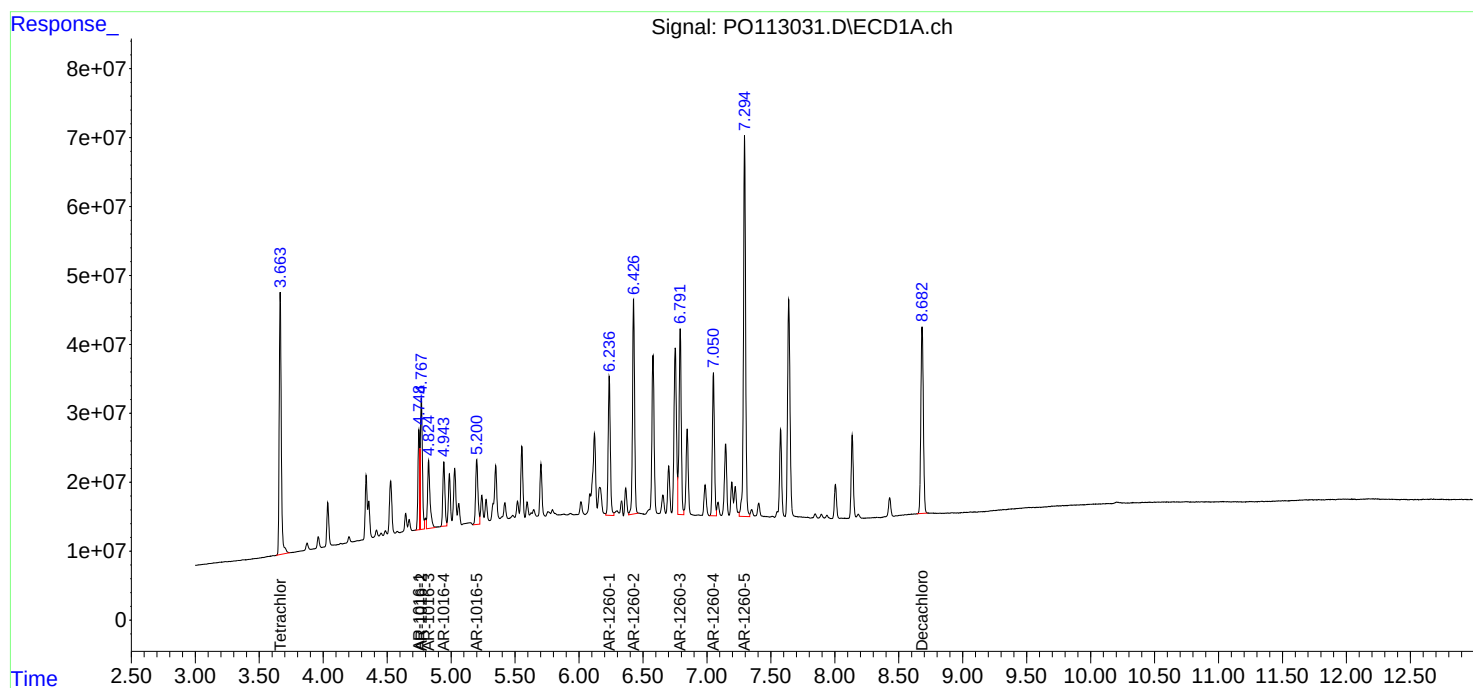

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0081825\
 Data File : P0113032.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 18 Aug 2025 19:37
 Operator : YP/AJ
 Sample : AR1242ICV500
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 ICVPO081825AR1242

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 19 06:20:37 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0081825.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Aug 19 06:08:32 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.664	3.656	429.6E6	262.9E6	52.476	51.959
2) SA Decachlor...	8.682	8.627	379.6E6	100.8E6	54.772	53.212
Target Compounds						
16) L4 AR-1242-1	4.750	4.730	118.2E6	75544744	513.948	522.785
17) L4 AR-1242-2	4.767	4.748	180.5E6	112.1E6	525.410	516.997
18) L4 AR-1242-3	4.825	4.923	114.2E6	58830110	514.501	502.975
19) L4 AR-1242-4	4.944	5.008	91221670	57727565	525.886	490.725
20) L4 AR-1242-5	5.594	5.526	103.3E6	75933701	515.841	509.168



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO081825\
Data File : PO113032.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 18 Aug 2025 19:37
Operator : YP/AJ
Sample : AR1242ICV500
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
ICVPO081825AR1242

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 19 06:20:37 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO081825.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Aug 19 06:08:32 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

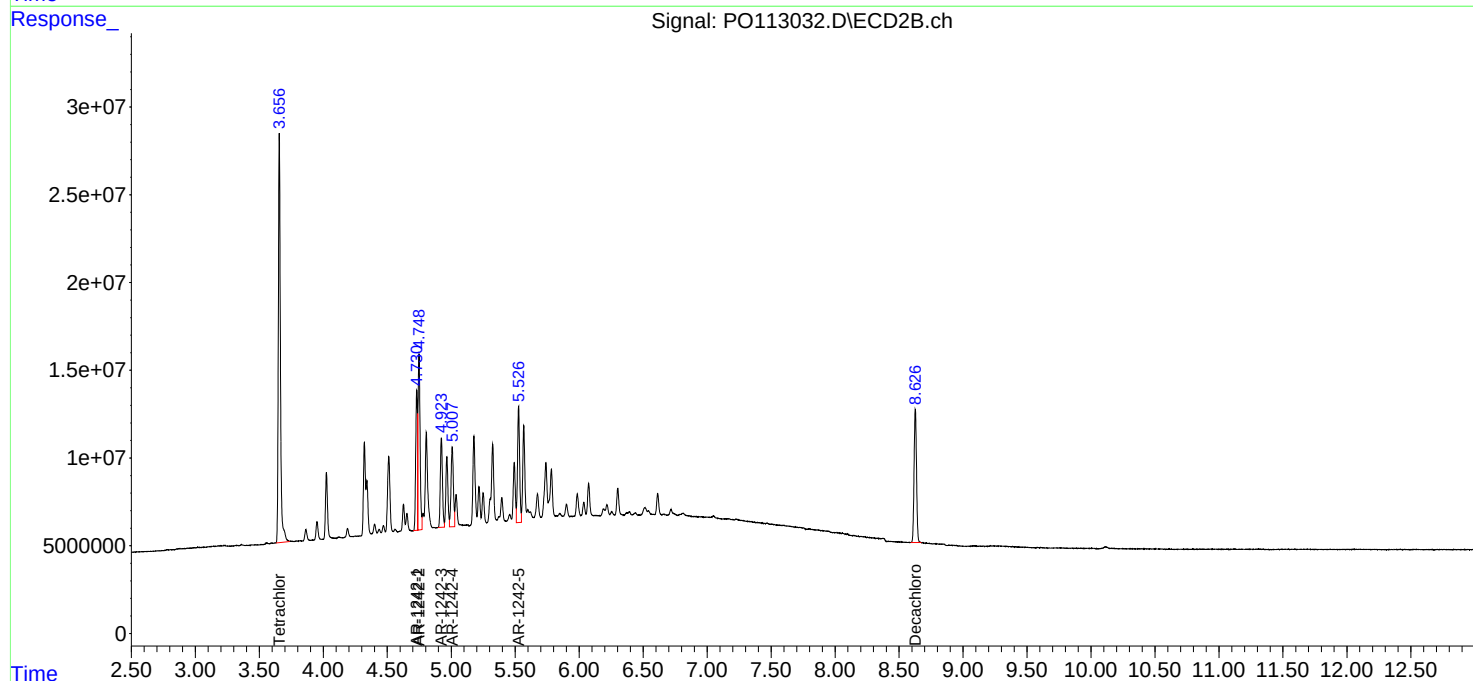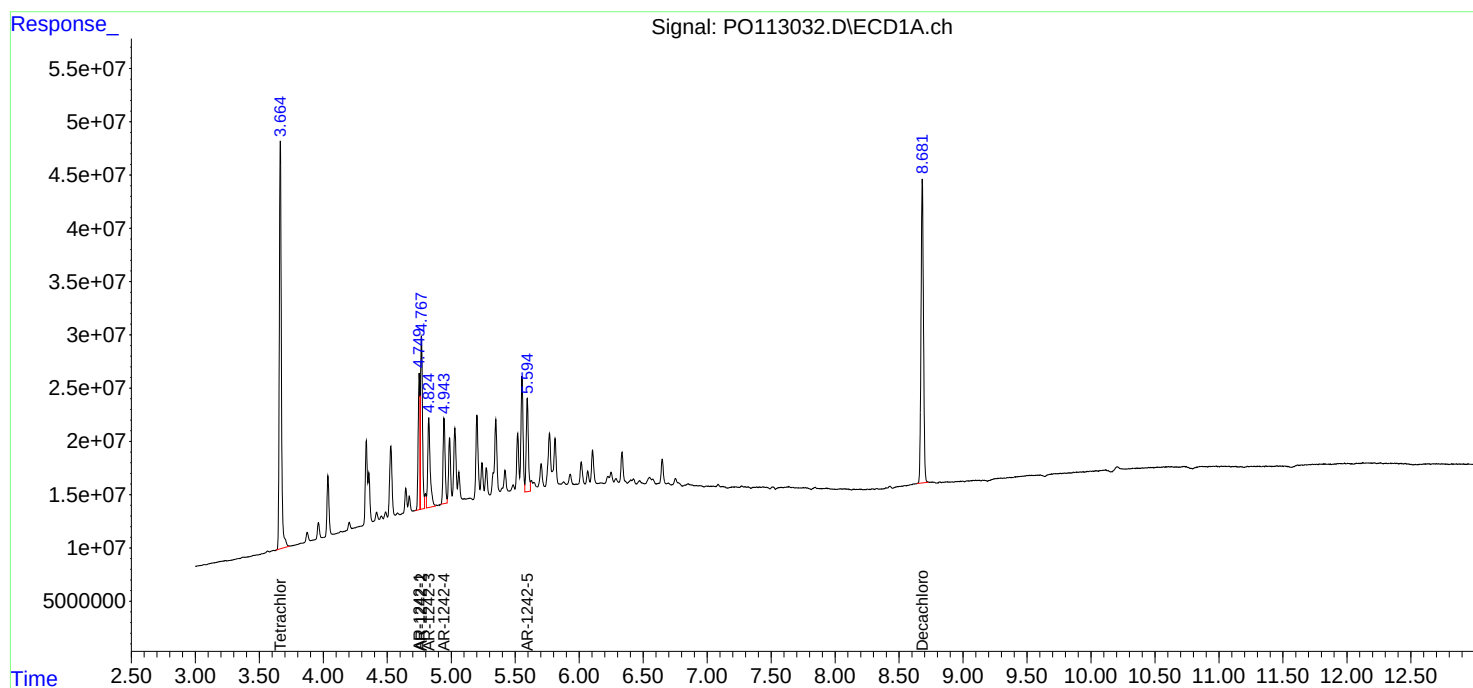

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0081825\
 Data File : P0113033.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 18 Aug 2025 19:54
 Operator : YP/AJ
 Sample : AR1248ICV500
 Misc :
 ALS Vial : 33 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 ICVPO081825AR1248

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 19 06:13:23 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0081825.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Aug 19 06:08:32 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.662	3.656	399.7E6	241.4E6	48.828	47.707
2) SA Decachlor...	8.680	8.627	370.4E6	97965710	53.439	51.701
Target Compounds						
21) L5 AR-1248-1	4.746	4.729	85766360	54333412	491.593	487.243
22) L5 AR-1248-2	4.984	4.965	115.6E6	76798982	478.136	477.906
23) L5 AR-1248-3	5.198	5.006	150.7E6	80662868	472.629	475.436
24) L5 AR-1248-4	5.551	5.177	233.0E6	95159179	466.303	477.659
25) L5 AR-1248-5	5.592	5.566	156.4E6	99002926	457.862	466.343



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO081825\
Data File : PO113033.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 18 Aug 2025 19:54
Operator : YP/AJ
Sample : AR1248ICV500
Misc :
ALS Vial : 33 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
ICVPO081825AR1248

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 19 06:13:23 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO081825.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Aug 19 06:08:32 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

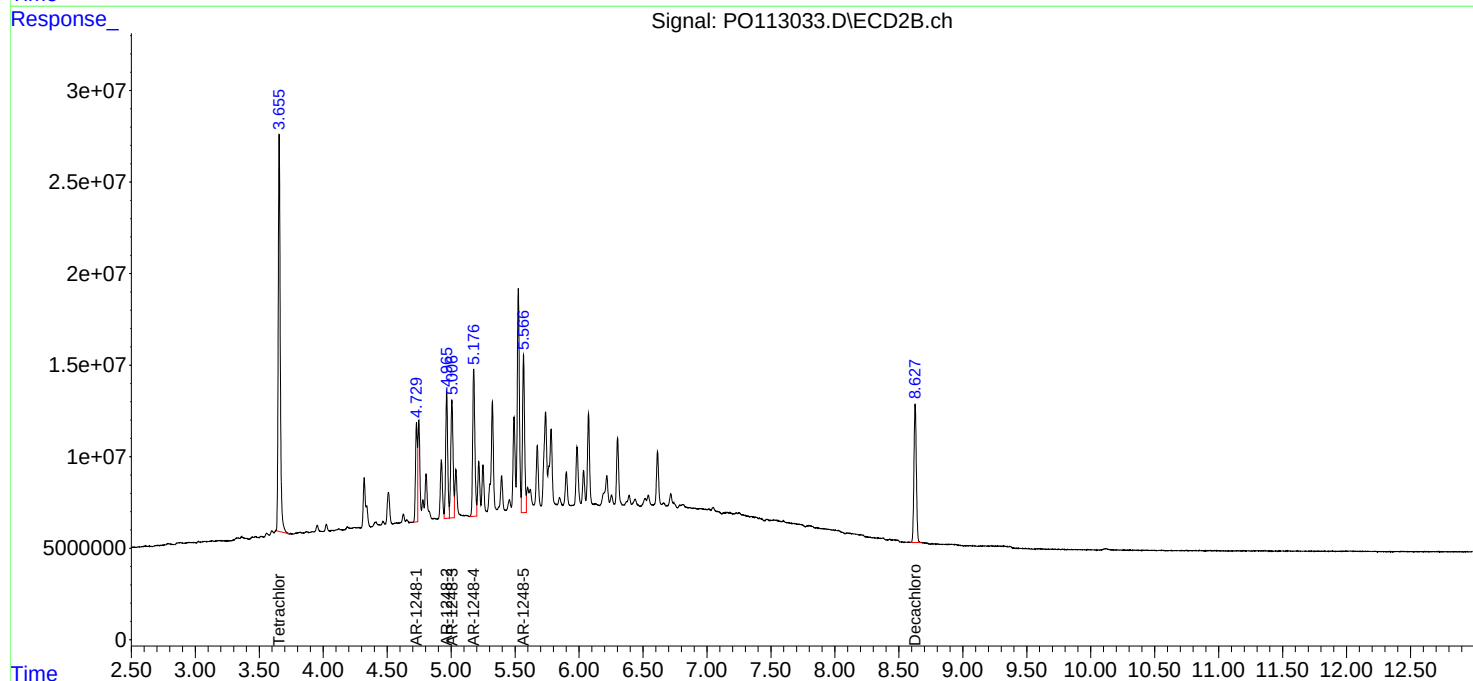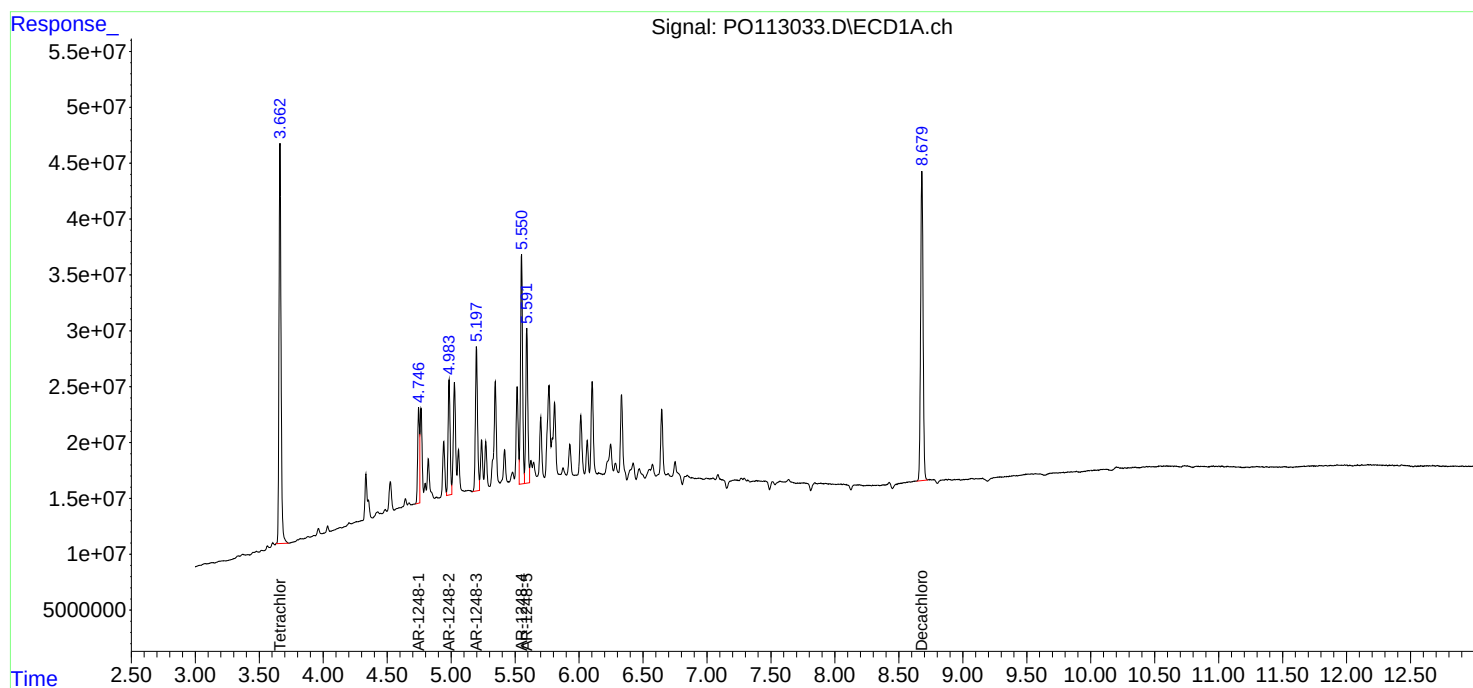

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0081825\
 Data File : P0113034.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 18 Aug 2025 20:31
 Operator : YP/AJ
 Sample : AR1254ICV500
 Misc :
 ALS Vial : 34 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 ICVPO081825AR1254

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 19 06:13:56 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0081825.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Aug 19 06:08:32 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.663	3.655	409.6E6	249.7E6	50.035	49.347
2) SA Decachlor...	8.681	8.628	369.2E6	98078894	53.271	51.761
Target Compounds						
26) L6 AR-1254-1	5.552	5.526	255.6E6	152.1E6	473.260	482.262
27) L6 AR-1254-2	5.701	5.673	233.3E6	135.4E6	472.888	482.834
28) L6 AR-1254-3	6.104	6.074	358.7E6	203.2E6	485.481	487.357
29) L6 AR-1254-4	6.334	6.301	267.7E6	131.5E6	480.676	478.371
30) L6 AR-1254-5	6.752	6.717	344.2E6	166.4E6	490.961	465.595



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO081825\
Data File : PO113034.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 18 Aug 2025 20:31
Operator : YP/AJ
Sample : AR1254ICV500
Misc :
ALS Vial : 34 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
ICVPO081825AR1254

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 19 06:13:56 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO081825.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Aug 19 06:08:32 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µm Signal #2 Info : 30M x 0.32mm x 0.25µm

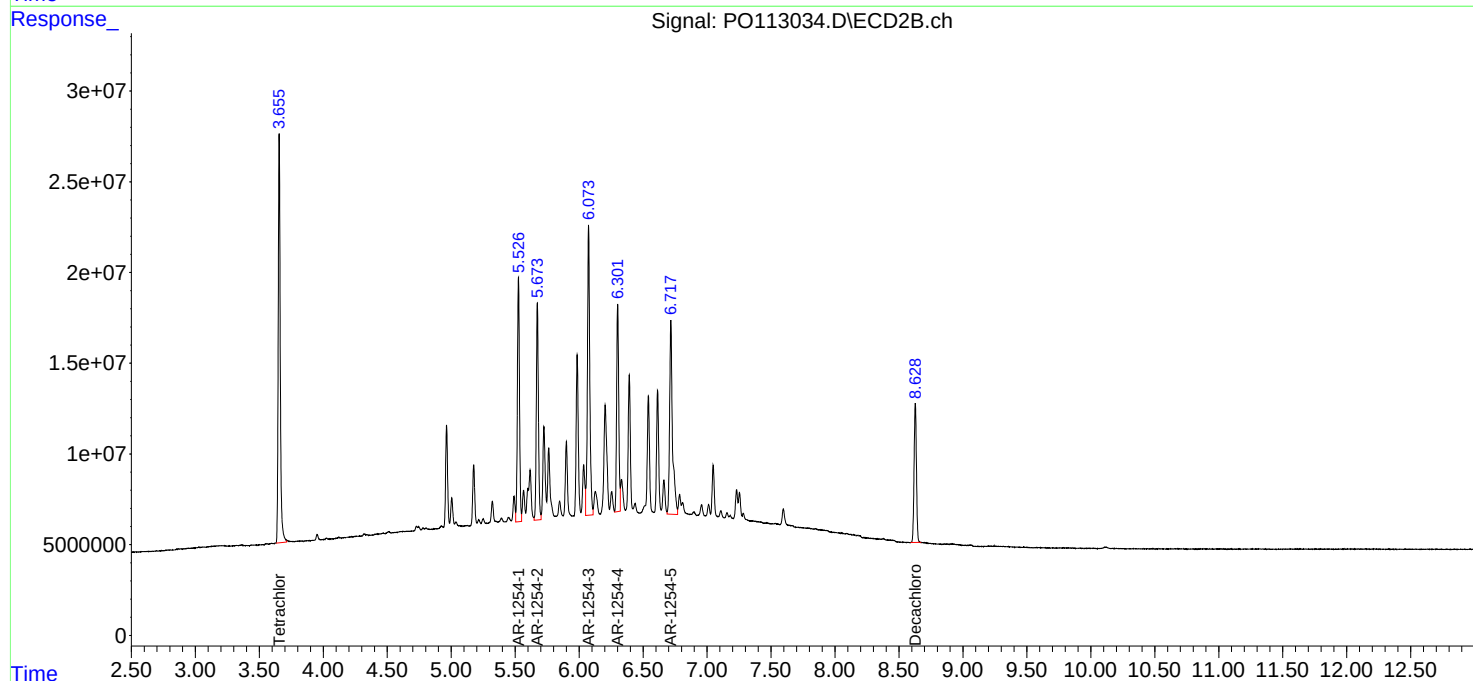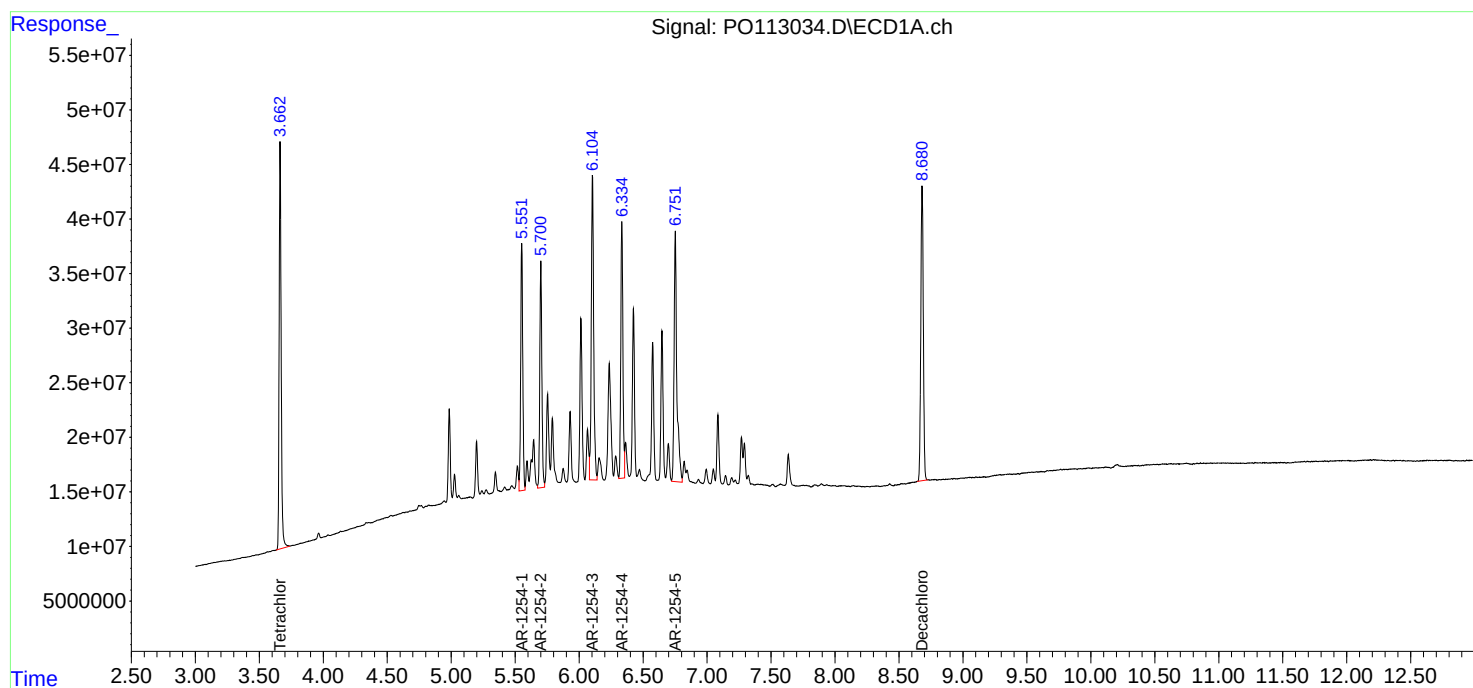

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0081825\
 Data File : P0113035.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 18 Aug 2025 21:07
 Operator : YP/AJ
 Sample : AR1268ICV500
 Misc :
 ALS Vial : 35 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 ICVPO081825AR1268

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 08/19/2025
 Supervised By :mohammad ahmed 08/20/2025

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 19 05:58:30 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0081825.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Aug 19 05:57:38 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.664	3.656	429.5E6	261.1E6	52.886	52.521
2) SA Decachlor...	8.682	8.627	678.8E6	177.0E6	51.133	51.189
Target Compounds						
41) L9 AR-1268-1	7.577	7.537	888.4E6	255.4E6	516.244	501.241
42) L9 AR-1268-2	7.642	7.602	745.6E6	207.2E6	514.846	498.702
43) L9 AR-1268-3	7.846	7.805	631.0E6	163.1E6	523.061	499.640
44) L9 AR-1268-4	8.137	8.092	241.9E6	62721591	525.077	520.802
45) L9 AR-1268-5	8.429	8.379	1632.4E6	402.4E6	511.965	515.245m

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_0\Data\PO081825\
Data File : PO113035.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 18 Aug 2025 21:07
Operator : YP/AJ
Sample : AR1268ICV500
Misc :
ALS Vial : 35 Sample Multiplier: 1



Instrument :
ECD_0
ClientSampleId :
ICVPO081825AR1268

Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 08/19/2025
Supervised By :mohammad ahmed 08/20/2025

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 19 05:58:30 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_0\methods\PO081825.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Aug 19 05:57:38 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

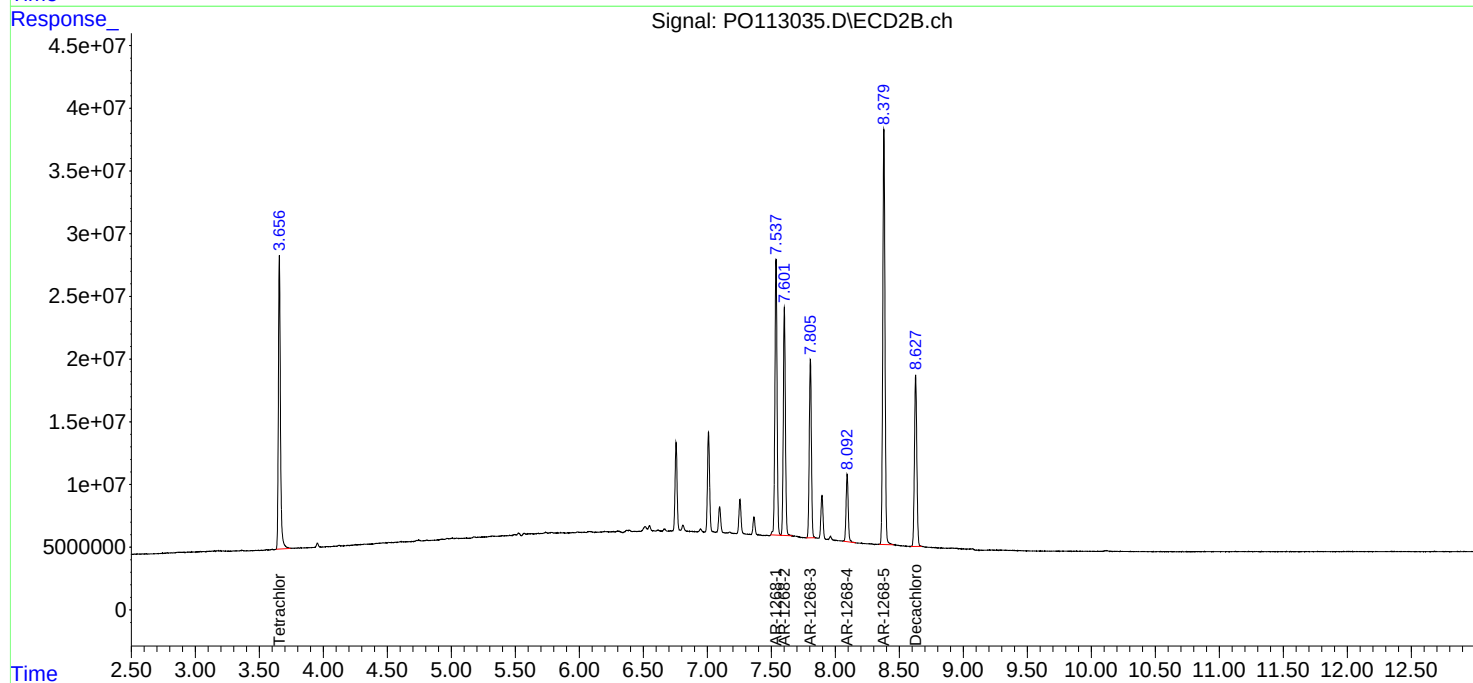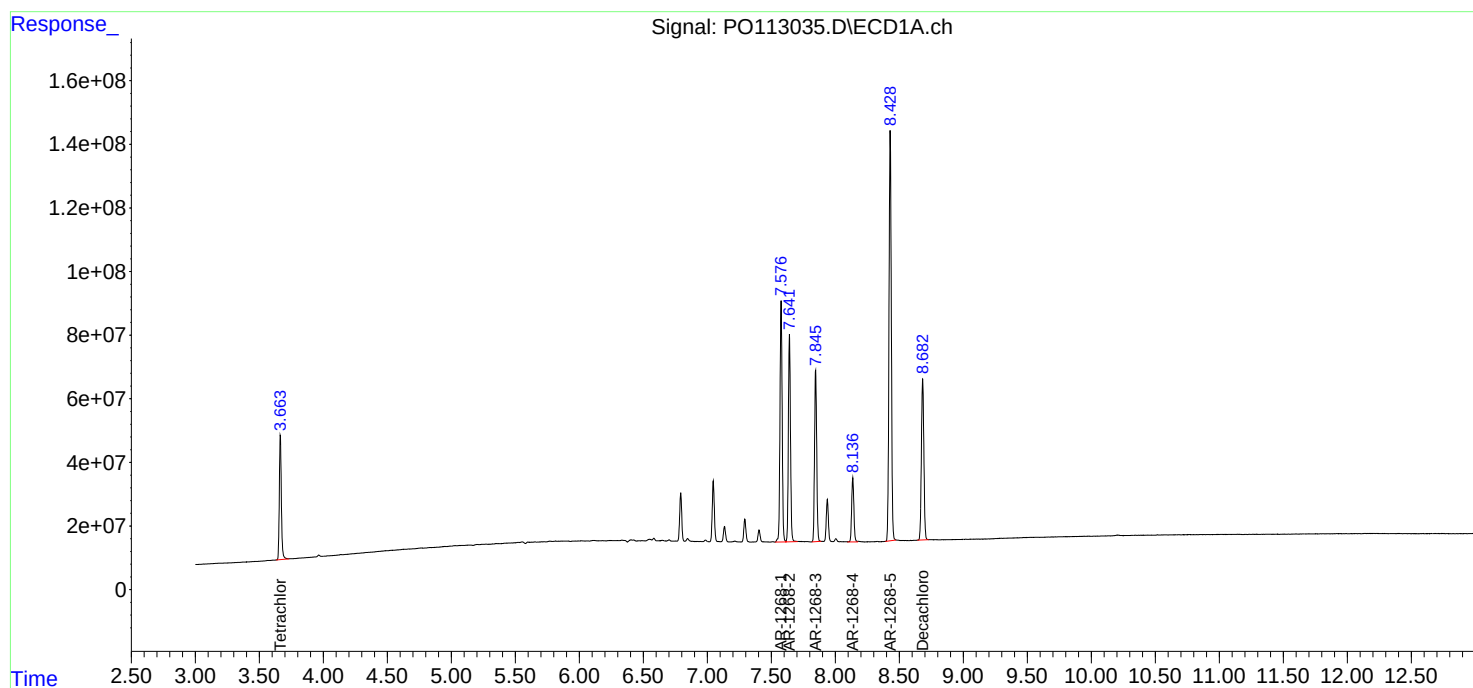



284 Sheffield Street, Mountainside, New Jersey 07092, Phone : 908 789 8900,
Fax : 908 789 8922

CALIBRATION VERIFICATION SUMMARY

Lab Name: Alliance

Contract: ATCE02

Lab Code: ACE

SDG NO.: Q2894

Continuing Calib Date: 08/20/2025

Initial Calibration Date(s): 08/18/2025 08/18/2025

Continuing Calib Time: 09:33

Initial Calibration Time(s): 09:53 18:24

GC Column: ZB-MR1 ID: 0.32 (mm)

COMPOUND		CCAL RT	AVG RT	RT WINDOW		DIFF RT
				FROM	TO	
Aroclor-1016-1	(1)	4.75	4.75	4.65	4.85	0.01
Aroclor-1016-2	(2)	4.76	4.77	4.67	4.87	0.01
Aroclor-1016-3	(3)	4.82	4.82	4.72	4.92	0.00
Aroclor-1016-4	(4)	4.94	4.94	4.84	5.04	0.00
Aroclor-1016-5	(5)	5.20	5.20	5.10	5.30	0.00
Aroclor-1260-1	(1)	6.23	6.24	6.14	6.34	0.01
Aroclor-1260-2	(2)	6.42	6.43	6.33	6.53	0.01
Aroclor-1260-3	(3)	6.79	6.79	6.69	6.89	0.00
Aroclor-1260-4	(4)	7.05	7.05	6.95	7.15	0.00
Aroclor-1260-5	(5)	7.29	7.29	7.19	7.39	0.00
Tetrachloro-m-xylene		3.66	3.66	3.56	3.76	0.00
Decachlorobiphenyl		8.68	8.68	8.58	8.78	0.00



284 Sheffield Street, Mountainside, New Jersey 07092, Phone : 908 789 8900,
Fax : 908 789 8922

CALIBRATION VERIFICATION SUMMARY

Lab Name: Alliance

Contract: ATCE02

Lab Code: ACE

SDG NO.: Q2894

Continuing Calib Date: 08/20/2025

Initial Calibration Date(s): 08/18/2025 08/18/2025

Continuing Calib Time: 09:33

Initial Calibration Time(s): 09:53 18:24

GC Column: ZB-MR2 ID: 0.32 (mm)

COMPOUND		CCAL RT	AVG RT	RT WINDOW		DIFF RT
				FROM	TO	
Aroclor-1016-1	(1)	4.73	4.73	4.63	4.83	0.00
Aroclor-1016-2	(2)	4.75	4.75	4.65	4.85	0.00
Aroclor-1016-3	(3)	4.92	4.92	4.82	5.02	0.00
Aroclor-1016-4	(4)	4.96	4.96	4.86	5.06	0.00
Aroclor-1016-5	(5)	5.18	5.18	5.08	5.28	0.00
Aroclor-1260-1	(1)	6.20	6.20	6.10	6.30	0.00
Aroclor-1260-2	(2)	6.39	6.39	6.29	6.49	0.00
Aroclor-1260-3	(3)	6.54	6.54	6.44	6.64	0.00
Aroclor-1260-4	(4)	7.01	7.01	6.91	7.11	0.00
Aroclor-1260-5	(5)	7.25	7.26	7.16	7.36	0.01
Tetrachloro-m-xylene		3.66	3.66	3.56	3.76	0.01
Decachlorobiphenyl		8.63	8.63	8.53	8.73	0.00



284 Sheffield Street, Mountainside, New Jersey 07092, Phone : 908 789 8900, Fax : 908 789 8922

CALIBRATION VERIFICATION SUMMARY

Lab Name: Alliance **Contract:** ATCE02
Lab Code: ACE **SDG NO.:** Q2894
GC Column: ZB-MR1 **ID:** 0.32 (mm) **Initi. Calib. Date(s):** 08/18/2025 08/18/2025

Client Sample No.: CCAL01 **Date Analyzed:** 08/20/2025
Lab Sample No.: AR1660CCC500 **Data File :** PO113074.D **Time Analyzed:** 09:33

COMPOUND	RT	RT WINDOW		CALC AMOUNT(ng)	NOM AMOUNT(ng)	%D
		FROM	TO			
Aroclor-1016-1	4.745	4.648	4.848	557.950	500.000	11.6
Aroclor-1016-2	4.764	4.666	4.866	569.590	500.000	13.9
Aroclor-1016-3	4.821	4.724	4.924	563.830	500.000	12.8
Aroclor-1016-4	4.939	4.843	5.043	536.000	500.000	7.2
Aroclor-1016-5	5.197	5.099	5.299	562.330	500.000	12.5
Aroclor-1260-1	6.233	6.136	6.336	573.260	500.000	14.7
Aroclor-1260-2	6.423	6.326	6.526	542.840	500.000	8.6
Aroclor-1260-3	6.788	6.691	6.891	473.310	500.000	-5.3
Aroclor-1260-4	7.047	6.951	7.151	440.650	500.000	-11.9
Aroclor-1260-5	7.291	7.194	7.394	520.410	500.000	4.1
Decachlorobiphenyl	8.680	8.582	8.782	44.730	50.000	-10.5
Tetrachloro-m-xylene	3.662	3.563	3.763	55.630	50.000	11.3



284 Sheffield Street, Mountainside, New Jersey 07092, Phone : 908 789 8900, Fax : 908 789 8922

CALIBRATION VERIFICATION SUMMARY

Lab Name: Alliance **Contract:** ATCE02
Lab Code: ACE **SDG NO.:** Q2894
GC Column: ZB-MR2 **ID:** 0.32 (mm) **Initi. Calib. Date(s):** 08/18/2025 08/18/2025

Client Sample No.: CCAL01 **Date Analyzed:** 08/20/2025
Lab Sample No.: AR1660CCC500 **Data File :** PO113074.D **Time Analyzed:** 09:33

COMPOUND	RT	RT WINDOW		CALC AMOUNT(ng)	NOM AMOUNT(ng)	%D
		FROM	TO			
Aroclor-1016-1	4.728	4.629	4.829	530.680	500.000	6.1
Aroclor-1016-2	4.746	4.647	4.847	520.840	500.000	4.2
Aroclor-1016-3	4.920	4.822	5.022	508.920	500.000	1.8
Aroclor-1016-4	4.963	4.864	5.064	492.130	500.000	-1.6
Aroclor-1016-5	5.175	5.076	5.276	532.190	500.000	6.4
Aroclor-1260-1	6.202	6.104	6.304	506.320	500.000	1.3
Aroclor-1260-2	6.390	6.292	6.492	504.370	500.000	0.9
Aroclor-1260-3	6.542	6.443	6.643	480.850	500.000	-3.8
Aroclor-1260-4	7.011	6.912	7.112	476.380	500.000	-4.7
Aroclor-1260-5	7.253	7.155	7.355	458.050	500.000	-8.4
Decachlorobiphenyl	8.626	8.528	8.728	48.290	50.000	-3.4
Tetrachloro-m-xylene	3.655	3.555	3.755	52.450	50.000	4.9

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0082025\
 Data File : PO113074.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 20 Aug 2025 09:33
 Operator : YP/AJ
 Sample : AR1660CCC500
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 AR1660CCC500

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 08/21/2025
 Supervised By :mohammad ahmed 08/22/2025

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 20 13:00:36 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0081825.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Aug 19 06:08:32 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.662	3.655	455.5E6	265.4E6	55.634	52.452
2) SA Decachlor...	8.680	8.626	310.1E6	91506016	44.733	48.292
Target Compounds						
3) L1 AR-1016-1	4.745	4.728	149.0E6	90519779	557.948	530.678
4) L1 AR-1016-2	4.764	4.746	228.6E6	134.2E6	569.586	520.837
5) L1 AR-1016-3	4.821	4.920	143.8E6	71052008	563.834	508.916
6) L1 AR-1016-4	4.939	4.963	116.9E6	57431542	536.001m	492.134
7) L1 AR-1016-5	5.197	5.175	124.6E6	75853388	562.332	532.192
31) L7 AR-1260-1	6.233	6.202	255.7E6	129.1E6	573.264	506.316
32) L7 AR-1260-2	6.423	6.390	372.8E6	174.4E6	542.845	504.371
33) L7 AR-1260-3	6.788	6.542	292.3E6	143.0E6	473.314	480.848
34) L7 AR-1260-4	7.047	7.011	197.4E6	98729668	440.648	476.381
35) L7 AR-1260-5	7.291	7.253	630.1E6	214.6E6	520.412	458.049

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO082025\
Data File : PO113074.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 20 Aug 2025 09:33
Operator : YP/AJ
Sample : AR1660CCC500
Misc :
ALS Vial : 3 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
AR1660CCC500

Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 08/21/2025
Supervised By :mohammad ahmed 08/22/2025

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 20 13:00:36 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO081825.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Aug 19 06:08:32 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

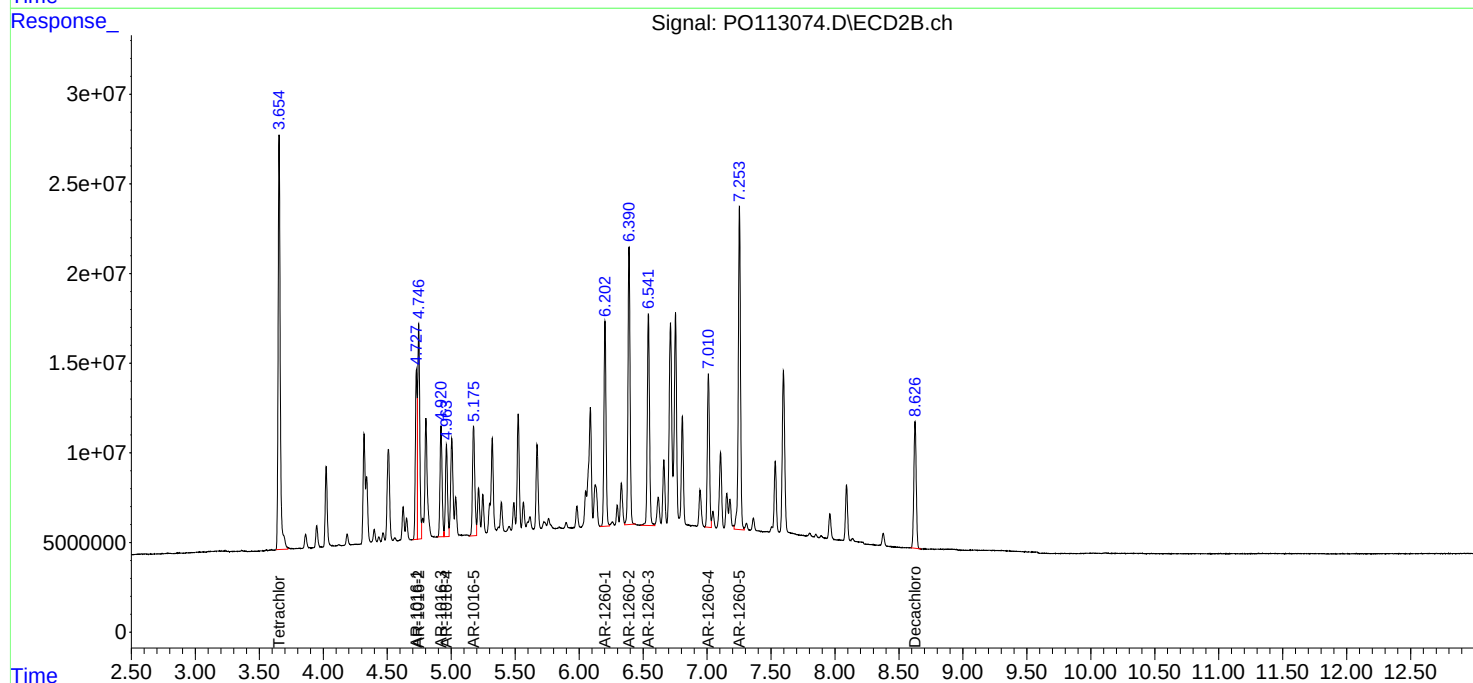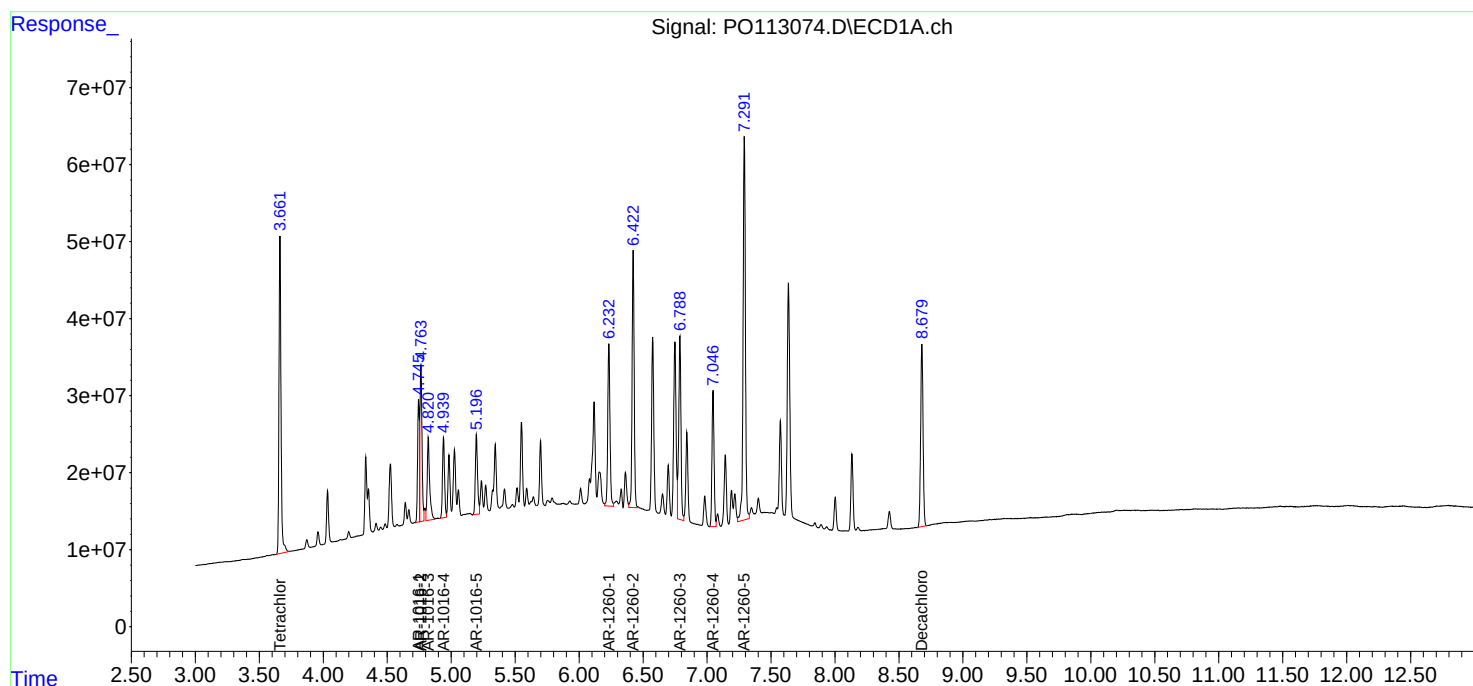



284 Sheffield Street, Mountainside, New Jersey 07092, Phone : 908 789 8900,
Fax : 908 789 8922

CALIBRATION VERIFICATION SUMMARY

Lab Name: Alliance

Contract: ATCE02

Lab Code: ACE

SDG NO.: Q2894

Continuing Calib Date: 08/20/2025

Initial Calibration Date(s): 08/18/2025 08/18/2025

Continuing Calib Time: 15:39

Initial Calibration Time(s): 09:53 18:24

GC Column: ZB-MR1 ID: 0.32 (mm)

COMPOUND		CCAL RT	AVG RT	RT WINDOW		DIFF RT
				FROM	TO	
Aroclor-1016-1	(1)	4.75	4.75	4.65	4.85	0.01
Aroclor-1016-2	(2)	4.76	4.77	4.67	4.87	0.01
Aroclor-1016-3	(3)	4.82	4.82	4.72	4.92	0.00
Aroclor-1016-4	(4)	4.94	4.94	4.84	5.04	0.00
Aroclor-1016-5	(5)	5.20	5.20	5.10	5.30	0.00
Aroclor-1260-1	(1)	6.23	6.24	6.14	6.34	0.01
Aroclor-1260-2	(2)	6.42	6.43	6.33	6.53	0.01
Aroclor-1260-3	(3)	6.79	6.79	6.69	6.89	0.00
Aroclor-1260-4	(4)	7.05	7.05	6.95	7.15	0.00
Aroclor-1260-5	(5)	7.29	7.29	7.19	7.39	0.00
Tetrachloro-m-xylene		3.66	3.66	3.56	3.76	0.00
Decachlorobiphenyl		8.68	8.68	8.58	8.78	0.00



284 Sheffield Street, Mountainside, New Jersey 07092, Phone : 908 789 8900,
Fax : 908 789 8922

CALIBRATION VERIFICATION SUMMARY

Lab Name: Alliance

Contract: ATCE02

Lab Code: ACE

SDG NO.: Q2894

Continuing Calib Date: 08/20/2025

Initial Calibration Date(s): 08/18/2025 08/18/2025

Continuing Calib Time: 15:39

Initial Calibration Time(s): 09:53 18:24

GC Column: ZB-MR2 ID: 0.32 (mm)

COMPOUND		CCAL RT	AVG RT	RT WINDOW		DIFF RT
				FROM	TO	
Aroclor-1016-1	(1)	4.73	4.73	4.63	4.83	0.00
Aroclor-1016-2	(2)	4.75	4.75	4.65	4.85	0.00
Aroclor-1016-3	(3)	4.92	4.92	4.82	5.02	0.00
Aroclor-1016-4	(4)	4.96	4.96	4.86	5.06	0.00
Aroclor-1016-5	(5)	5.18	5.18	5.08	5.28	0.00
Aroclor-1260-1	(1)	6.20	6.20	6.10	6.30	0.00
Aroclor-1260-2	(2)	6.39	6.39	6.29	6.49	0.00
Aroclor-1260-3	(3)	6.54	6.54	6.44	6.64	0.00
Aroclor-1260-4	(4)	7.01	7.01	6.91	7.11	0.00
Aroclor-1260-5	(5)	7.25	7.26	7.16	7.36	0.01
Tetrachloro-m-xylene		3.66	3.66	3.56	3.76	0.01
Decachlorobiphenyl		8.63	8.63	8.53	8.73	0.00



284 Sheffield Street, Mountainside, New Jersey 07092, Phone : 908 789 8900, Fax : 908 789 8922

CALIBRATION VERIFICATION SUMMARY

Lab Name: Alliance **Contract:** ATCE02
Lab Code: ACE **SDG NO.:** Q2894
GC Column: ZB-MR1 **ID:** 0.32 (mm) **Initi. Calib. Date(s):** 08/18/2025 08/18/2025

Client Sample No.: CCAL02 **Date Analyzed:** 08/20/2025
Lab Sample No.: AR1660CCC500 **Data File :** PO113089.D **Time Analyzed:** 15:39

COMPOUND	RT	RT WINDOW		CALC AMOUNT(ng)	NOM AMOUNT(ng)	%D
		FROM	TO			
Aroclor-1016-1	4.745	4.648	4.848	549.720	500.000	9.9
Aroclor-1016-2	4.764	4.666	4.866	557.770	500.000	11.6
Aroclor-1016-3	4.821	4.724	4.924	560.020	500.000	12.0
Aroclor-1016-4	4.940	4.843	5.043	521.460	500.000	4.3
Aroclor-1016-5	5.197	5.099	5.299	588.170	500.000	17.6
Aroclor-1260-1	6.233	6.136	6.336	578.100	500.000	15.6
Aroclor-1260-2	6.423	6.326	6.526	553.590	500.000	10.7
Aroclor-1260-3	6.789	6.691	6.891	548.020	500.000	9.6
Aroclor-1260-4	7.048	6.951	7.151	553.140	500.000	10.6
Aroclor-1260-5	7.291	7.194	7.394	559.300	500.000	11.9
Decachlorobiphenyl	8.680	8.582	8.782	53.560	50.000	7.1
Tetrachloro-m-xylene	3.662	3.563	3.763	55.020	50.000	10.0



284 Sheffield Street, Mountainside, New Jersey 07092, Phone : 908 789 8900, Fax : 908 789 8922

CALIBRATION VERIFICATION SUMMARY

Lab Name: Alliance **Contract:** ATCE02
Lab Code: ACE **SDG NO.:** Q2894
GC Column: ZB-MR2 **ID:** 0.32 (mm) **Initi. Calib. Date(s):** 08/18/2025 08/18/2025

Client Sample No.: CCAL02 **Date Analyzed:** 08/20/2025
Lab Sample No.: AR1660CCC500 **Data File :** PO113089.D **Time Analyzed:** 15:39

COMPOUND	RT	RT WINDOW		CALC AMOUNT(ng)	NOM AMOUNT(ng)	%D
		FROM	TO			
Aroclor-1016-1	4.728	4.629	4.829	525.810	500.000	5.2
Aroclor-1016-2	4.747	4.647	4.847	528.740	500.000	5.7
Aroclor-1016-3	4.921	4.822	5.022	517.620	500.000	3.5
Aroclor-1016-4	4.964	4.864	5.064	497.210	500.000	-0.6
Aroclor-1016-5	5.176	5.076	5.276	552.910	500.000	10.6
Aroclor-1260-1	6.203	6.104	6.304	512.480	500.000	2.5
Aroclor-1260-2	6.391	6.292	6.492	509.070	500.000	1.8
Aroclor-1260-3	6.543	6.443	6.643	478.950	500.000	-4.2
Aroclor-1260-4	7.012	6.912	7.112	498.110	500.000	-0.4
Aroclor-1260-5	7.254	7.155	7.355	490.130	500.000	-2.0
Decachlorobiphenyl	8.627	8.528	8.728	51.510	50.000	3.0
Tetrachloro-m-xylene	3.655	3.555	3.755	53.390	50.000	6.8

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0082025\
 Data File : PO113089.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 20 Aug 2025 15:39
 Operator : YP/AJ
 Sample : AR1660CCC500
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 AR1660CCC500

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 08/21/2025
 Supervised By :mohammad ahmed 08/22/2025

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 21 01:40:07 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0081825.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Aug 19 06:08:32 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.662	3.655	450.5E6	270.2E6	55.023	53.391
2) SA Decachlor...	8.680	8.627	371.3E6	97608949	53.564	51.513
Target Compounds						
3) L1 AR-1016-1	4.745	4.728	146.8E6	89689850	549.719	525.813
4) L1 AR-1016-2	4.764	4.747	223.9E6	136.2E6	557.772	528.736
5) L1 AR-1016-3	4.821	4.921	142.8E6	72267074	560.018	517.619
6) L1 AR-1016-4	4.940	4.964	113.7E6	58023335	521.458m	497.205
7) L1 AR-1016-5	5.197	5.176	130.4E6	78805833	588.174	552.907
31) L7 AR-1260-1	6.233	6.203	257.8E6	130.7E6	578.098	512.481
32) L7 AR-1260-2	6.423	6.391	380.2E6	176.0E6	553.586	509.068
33) L7 AR-1260-3	6.789	6.543	338.4E6	142.5E6	548.020	478.953
34) L7 AR-1260-4	7.048	7.012	247.7E6	103.2E6	553.145	498.111
35) L7 AR-1260-5	7.291	7.254	677.1E6	229.6E6	559.301	490.135

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO082025\
Data File : PO113089.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 20 Aug 2025 15:39
Operator : YP/AJ
Sample : AR1660CCC500
Misc :
ALS Vial : 3 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
AR1660CCC500

Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 08/21/2025
Supervised By :mohammad ahmed 08/22/2025

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 21 01:40:07 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO081825.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Aug 19 06:08:32 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

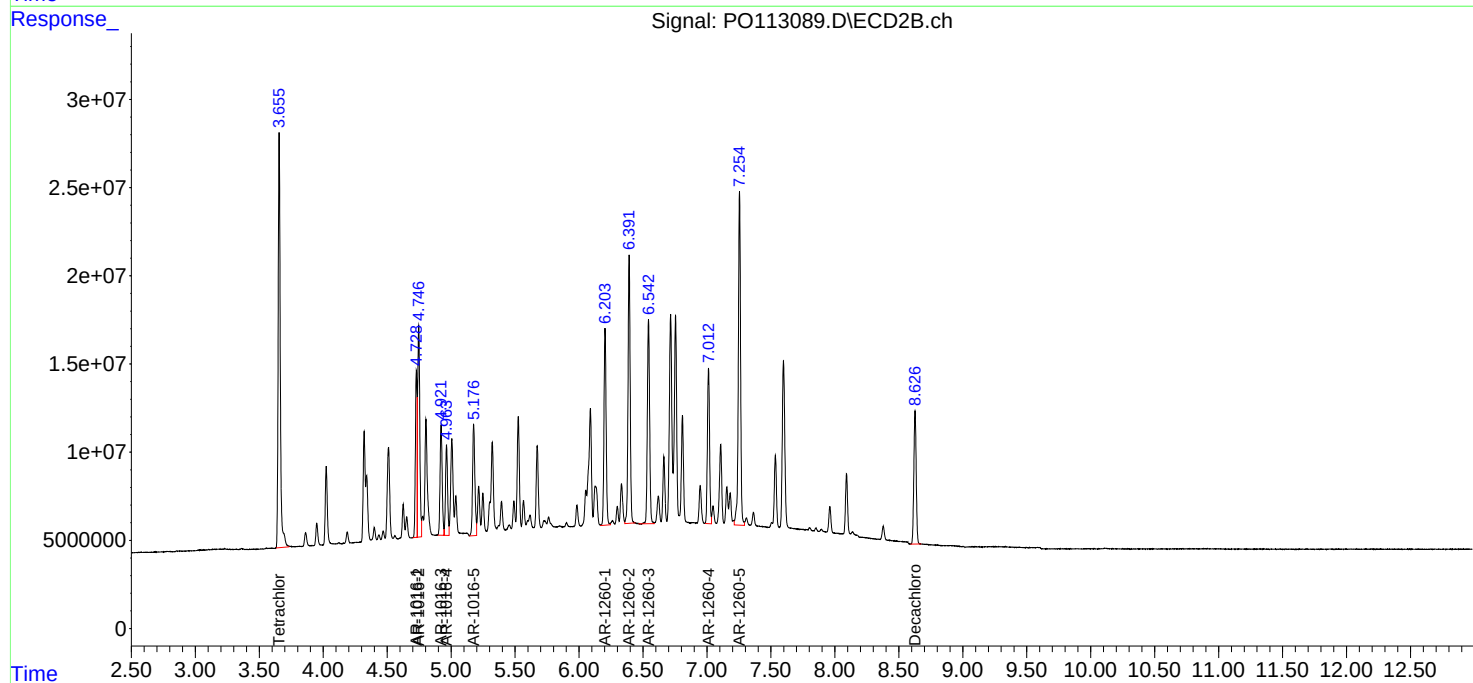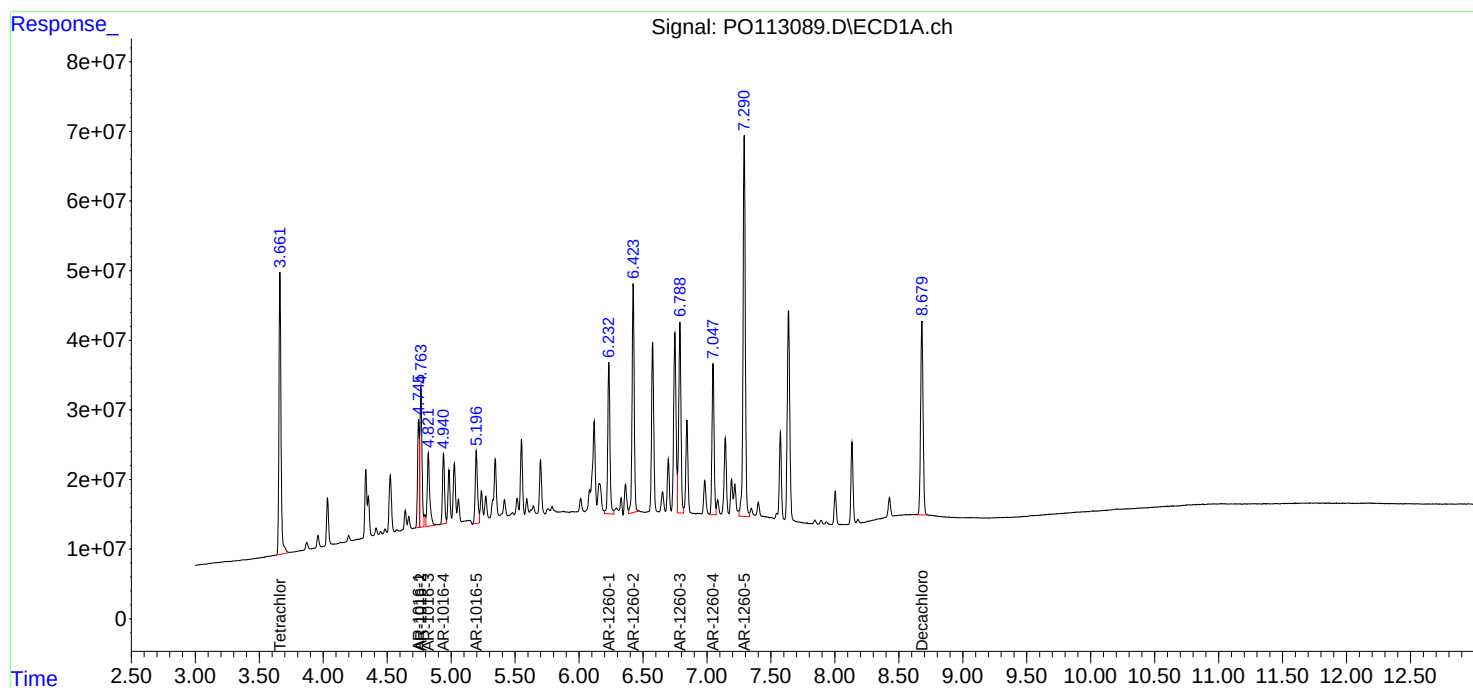



284 Sheffield Street, Mountainside, New Jersey 07092, Phone : 908 789 8900,
Fax : 908 789 8922

CALIBRATION VERIFICATION SUMMARY

Lab Name: Alliance

Contract: ATCE02

Lab Code: ACE

SDG NO.: Q2894

Continuing Calib Date: 08/20/2025

Initial Calibration Date(s): 08/18/2025 08/18/2025

Continuing Calib Time: 21:05

Initial Calibration Time(s): 09:53 18:24

GC Column: ZB-MR1 ID: 0.32 (mm)

COMPOUND		CCAL RT	AVG RT	RT WINDOW FROM TO		DIFF RT
Aroclor-1016-1	(1)	4.75	4.75	4.65	4.85	0.00
Aroclor-1016-2	(2)	4.77	4.77	4.67	4.87	0.01
Aroclor-1016-3	(3)	4.82	4.82	4.72	4.92	0.00
Aroclor-1016-4	(4)	4.94	4.94	4.84	5.04	0.00
Aroclor-1016-5	(5)	5.20	5.20	5.10	5.30	0.00
Aroclor-1260-1	(1)	6.23	6.24	6.14	6.34	0.01
Aroclor-1260-2	(2)	6.42	6.43	6.33	6.53	0.01
Aroclor-1260-3	(3)	6.79	6.79	6.69	6.89	0.00
Aroclor-1260-4	(4)	7.05	7.05	6.95	7.15	0.00
Aroclor-1260-5	(5)	7.29	7.29	7.19	7.39	0.00
Tetrachloro-m-xylene		3.66	3.66	3.56	3.76	0.00
Decachlorobiphenyl		8.68	8.68	8.58	8.78	0.00



284 Sheffield Street, Mountainside, New Jersey 07092, Phone : 908 789 8900,
Fax : 908 789 8922

CALIBRATION VERIFICATION SUMMARY

Lab Name: Alliance

Contract: ATCE02

Lab Code: ACE

SDG NO.: Q2894

Continuing Calib Date: 08/20/2025

Initial Calibration Date(s): 08/18/2025 08/18/2025

Continuing Calib Time: 21:05

Initial Calibration Time(s): 09:53 18:24

GC Column: ZB-MR2 ID: 0.32 (mm)

COMPOUND		CCAL RT	AVG RT	RT WINDOW		DIFF RT
				FROM	TO	
Aroclor-1016-1	(1)	4.73	4.73	4.63	4.83	0.00
Aroclor-1016-2	(2)	4.75	4.75	4.65	4.85	0.00
Aroclor-1016-3	(3)	4.92	4.92	4.82	5.02	0.00
Aroclor-1016-4	(4)	4.96	4.96	4.86	5.06	0.00
Aroclor-1016-5	(5)	5.18	5.18	5.08	5.28	0.00
Aroclor-1260-1	(1)	6.20	6.20	6.10	6.30	0.00
Aroclor-1260-2	(2)	6.39	6.39	6.29	6.49	0.00
Aroclor-1260-3	(3)	6.54	6.54	6.44	6.64	0.00
Aroclor-1260-4	(4)	7.01	7.01	6.91	7.11	0.00
Aroclor-1260-5	(5)	7.25	7.26	7.16	7.36	0.01
Tetrachloro-m-xylene		3.65	3.66	3.56	3.76	0.01
Decachlorobiphenyl		8.63	8.63	8.53	8.73	0.00



284 Sheffield Street, Mountainside, New Jersey 07092, Phone : 908 789 8900, Fax : 908 789 8922

CALIBRATION VERIFICATION SUMMARY

Lab Name: Alliance **Contract:** ATCE02
Lab Code: ACE **SDG NO.:** Q2894
GC Column: ZB-MR1 **ID:** 0.32 (mm) **Initi. Calib. Date(s):** 08/18/2025 08/18/2025

Client Sample No.: CCAL03 **Date Analyzed:** 08/20/2025
Lab Sample No.: AR1660CCC500 **Data File :** PO113104.D **Time Analyzed:** 21:05

COMPOUND	RT	RT WINDOW		CALC AMOUNT(ng)	NOM AMOUNT(ng)	%D
		FROM	TO			
Aroclor-1016-1	4.747	4.648	4.848	546.270	500.000	9.3
Aroclor-1016-2	4.765	4.666	4.866	558.770	500.000	11.8
Aroclor-1016-3	4.822	4.724	4.924	561.700	500.000	12.3
Aroclor-1016-4	4.941	4.843	5.043	508.020	500.000	1.6
Aroclor-1016-5	5.198	5.099	5.299	599.770	500.000	20.0
Aroclor-1260-1	6.234	6.136	6.336	545.420	500.000	9.1
Aroclor-1260-2	6.424	6.326	6.526	523.590	500.000	4.7
Aroclor-1260-3	6.790	6.691	6.891	503.040	500.000	0.6
Aroclor-1260-4	7.049	6.951	7.151	496.540	500.000	-0.7
Aroclor-1260-5	7.292	7.194	7.394	500.680	500.000	0.1
Decachlorobiphenyl	8.680	8.582	8.782	47.900	50.000	-4.2
Tetrachloro-m-xylene	3.662	3.563	3.763	55.180	50.000	10.4



284 Sheffield Street, Mountainside, New Jersey 07092, Phone : 908 789 8900, Fax : 908 789 8922

CALIBRATION VERIFICATION SUMMARY

Lab Name: Alliance **Contract:** ATCE02
Lab Code: ACE **SDG NO.:** Q2894
GC Column: ZB-MR2 **ID:** 0.32 (mm) **Initi. Calib. Date(s):** 08/18/2025 08/18/2025

Client Sample No.: CCAL03 **Date Analyzed:** 08/20/2025
Lab Sample No.: AR1660CCC500 **Data File :** PO113104.D **Time Analyzed:** 21:05

COMPOUND	RT	RT WINDOW		CALC AMOUNT(ng)	NOM AMOUNT(ng)	%D
		FROM	TO			
Aroclor-1016-1	4.728	4.629	4.829	525.020	500.000	5.0
Aroclor-1016-2	4.746	4.647	4.847	522.860	500.000	4.6
Aroclor-1016-3	4.921	4.822	5.022	513.260	500.000	2.7
Aroclor-1016-4	4.964	4.864	5.064	496.610	500.000	-0.7
Aroclor-1016-5	5.175	5.076	5.276	557.720	500.000	11.5
Aroclor-1260-1	6.203	6.104	6.304	490.130	500.000	-2.0
Aroclor-1260-2	6.391	6.292	6.492	488.970	500.000	-2.2
Aroclor-1260-3	6.542	6.443	6.643	453.790	500.000	-9.2
Aroclor-1260-4	7.012	6.912	7.112	473.090	500.000	-5.4
Aroclor-1260-5	7.254	7.155	7.355	471.190	500.000	-5.8
Decachlorobiphenyl	8.626	8.528	8.728	50.940	50.000	1.9
Tetrachloro-m-xylene	3.654	3.555	3.755	53.170	50.000	6.3

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0082025\
 Data File : PO113104.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 20 Aug 2025 21:05
 Operator : YP/AJ
 Sample : AR1660CCC500
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 AR1660CCC500

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 21 01:43:36 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0081825.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Aug 19 06:08:32 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.662	3.654	451.8E6	269.1E6	55.182	53.168
2) SA Decachlor...	8.680	8.626	332.0E6	96530730	47.904	50.944
Target Compounds						
3) L1 AR-1016-1	4.747	4.728	145.8E6	89554592	546.274	525.020
4) L1 AR-1016-2	4.765	4.746	224.3E6	134.7E6	558.765	522.862
5) L1 AR-1016-3	4.822	4.921	143.2E6	71658997	561.704	513.264
6) L1 AR-1016-4	4.941	4.964	110.8E6	57954190	508.025	496.613
7) L1 AR-1016-5	5.198	5.175	132.9E6	79491759	599.773	557.720
31) L7 AR-1260-1	6.234	6.203	243.2E6	125.0E6	545.419	490.127
32) L7 AR-1260-2	6.424	6.391	359.6E6	169.0E6	523.593	488.970
33) L7 AR-1260-3	6.790	6.542	310.6E6	135.0E6	503.038	453.787
34) L7 AR-1260-4	7.049	7.012	222.4E6	98047377	496.543	473.089
35) L7 AR-1260-5	7.292	7.254	606.2E6	220.7E6	500.685	471.188



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO082025\
Data File : PO113104.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 20 Aug 2025 21:05
Operator : YP/AJ
Sample : AR1660CCC500
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
AR1660CCC500

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 21 01:43:36 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO081825.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Aug 19 06:08:32 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

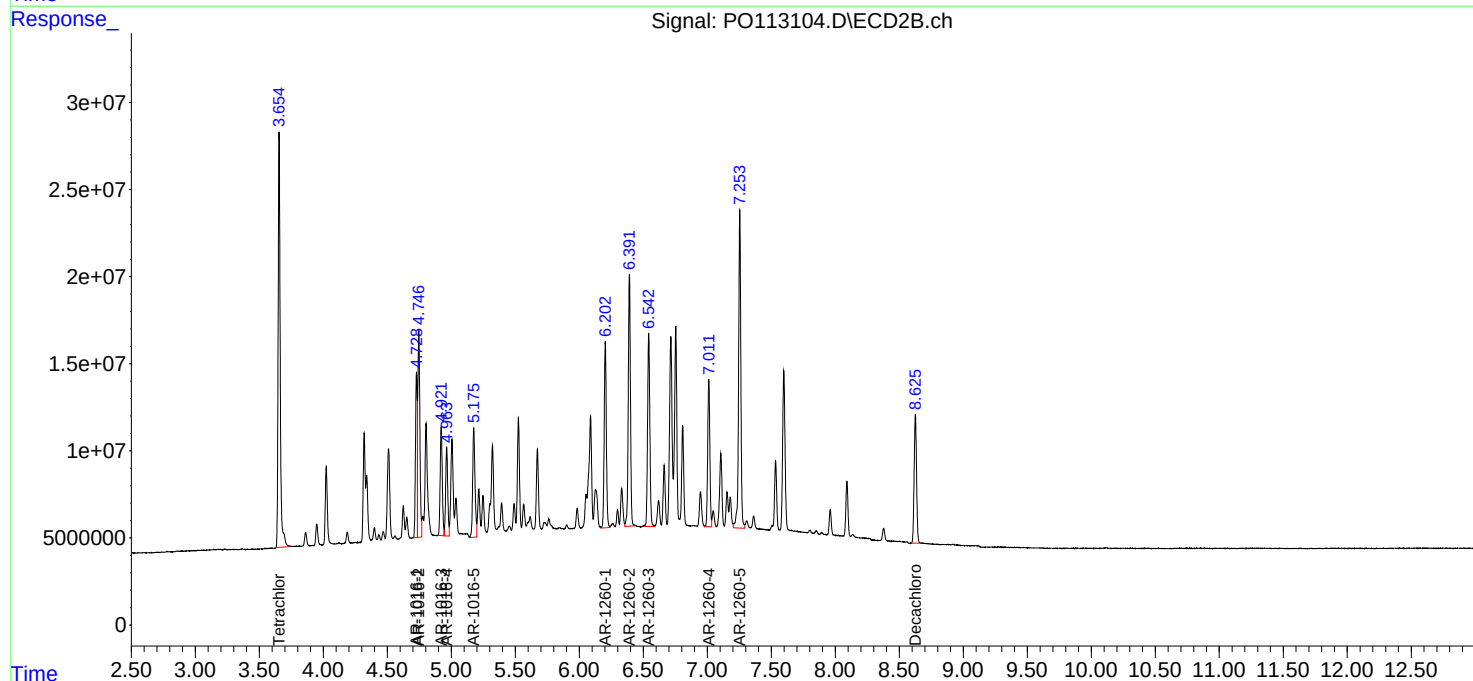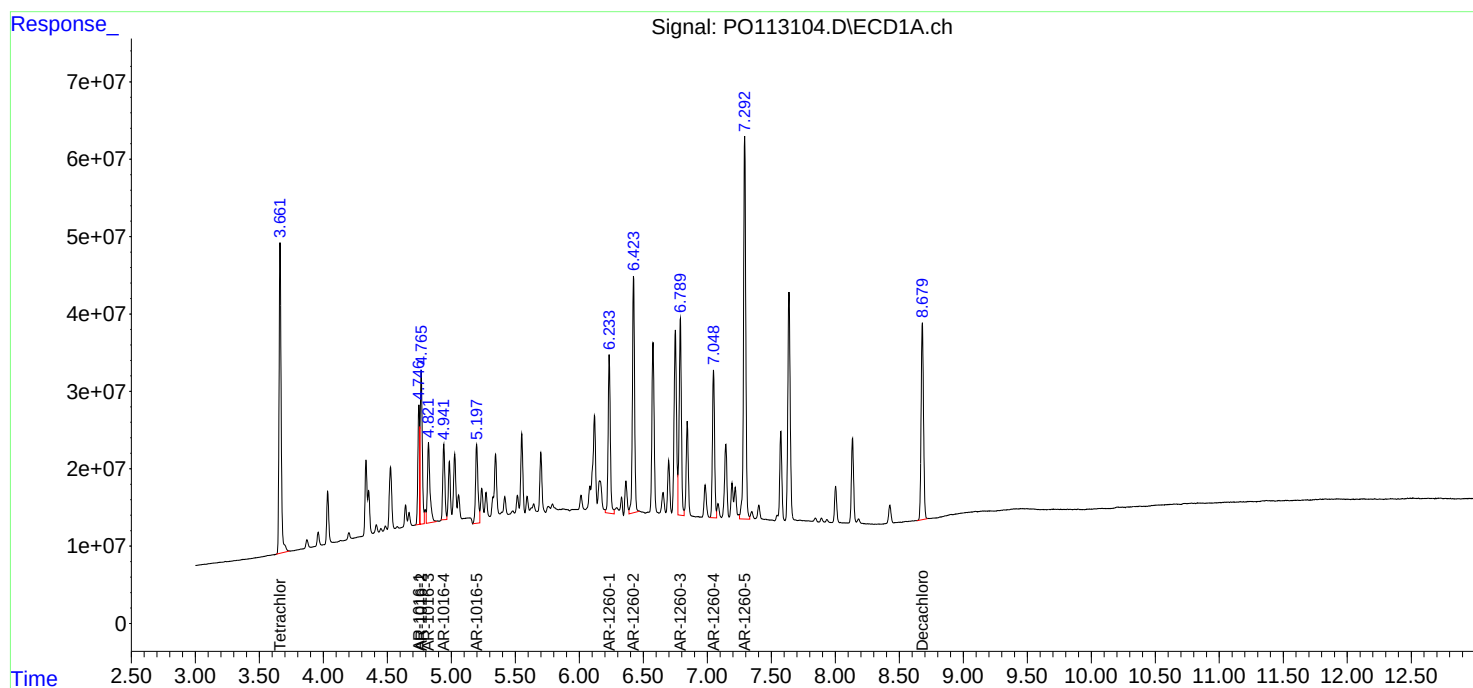



284 Sheffield Street, Mountainside, New Jersey 07092, Phone : 908 789 8900,
Fax : 908 789 8922

CALIBRATION VERIFICATION SUMMARY

Lab Name: Alliance

Contract: ATCE02

Lab Code: ACE

SDG NO.: Q2894

Continuing Calib Date: 08/21/2025

Initial Calibration Date(s): 08/18/2025 08/18/2025

Continuing Calib Time: 09:05

Initial Calibration Time(s): 09:53 18:24

GC Column: ZB-MR1 ID: 0.32 (mm)

COMPOUND		CCAL RT	AVG RT	RT WINDOW		DIFF RT
				FROM	TO	
Aroclor-1016-1	(1)	4.75	4.75	4.65	4.85	0.00
Aroclor-1016-2	(2)	4.77	4.77	4.67	4.87	0.01
Aroclor-1016-3	(3)	4.82	4.82	4.72	4.92	0.00
Aroclor-1016-4	(4)	4.94	4.94	4.84	5.04	0.00
Aroclor-1016-5	(5)	5.20	5.20	5.10	5.30	0.00
Aroclor-1260-1	(1)	6.24	6.24	6.14	6.34	0.00
Aroclor-1260-2	(2)	6.42	6.43	6.33	6.53	0.01
Aroclor-1260-3	(3)	6.79	6.79	6.69	6.89	0.00
Aroclor-1260-4	(4)	7.05	7.05	6.95	7.15	0.00
Aroclor-1260-5	(5)	7.29	7.29	7.19	7.39	0.00
Tetrachloro-m-xylene		3.66	3.66	3.56	3.76	0.00
Decachlorobiphenyl		8.68	8.68	8.58	8.78	0.00



284 Sheffield Street, Mountainside, New Jersey 07092, Phone : 908 789 8900,
Fax : 908 789 8922

CALIBRATION VERIFICATION SUMMARY

Lab Name: Alliance

Contract: ATCE02

Lab Code: ACE

SDG NO.: Q2894

Continuing Calib Date: 08/21/2025

Initial Calibration Date(s): 08/18/2025

08/18/2025

Continuing Calib Time: 09:05

Initial Calibration Time(s): 09:53

18:24

GC Column: ZB-MR2 ID: 0.32 (mm)

COMPOUND		CCAL RT	AVG RT	RT WINDOW		DIFF RT
				FROM	TO	
Aroclor-1016-1	(1)	4.73	4.73	4.63	4.83	0.00
Aroclor-1016-2	(2)	4.75	4.75	4.65	4.85	0.00
Aroclor-1016-3	(3)	4.92	4.92	4.82	5.02	0.00
Aroclor-1016-4	(4)	4.96	4.96	4.86	5.06	0.00
Aroclor-1016-5	(5)	5.18	5.18	5.08	5.28	0.00
Aroclor-1260-1	(1)	6.20	6.20	6.10	6.30	0.00
Aroclor-1260-2	(2)	6.39	6.39	6.29	6.49	0.00
Aroclor-1260-3	(3)	6.54	6.54	6.44	6.64	0.00
Aroclor-1260-4	(4)	7.01	7.01	6.91	7.11	0.00
Aroclor-1260-5	(5)	7.25	7.26	7.16	7.36	0.01
Tetrachloro-m-xylene		3.65	3.66	3.56	3.76	0.01
Decachlorobiphenyl		8.63	8.63	8.53	8.73	0.00



284 Sheffield Street, Mountainside, New Jersey 07092, Phone : 908 789 8900, Fax : 908 789 8922

CALIBRATION VERIFICATION SUMMARY

Lab Name: Alliance **Contract:** ATCE02
Lab Code: ACE **SDG NO.:** Q2894
GC Column: ZB-MR1 **ID:** 0.32 (mm) **Initi. Calib. Date(s):** 08/18/2025 08/18/2025

Client Sample No.: CCAL04 **Date Analyzed:** 08/21/2025
Lab Sample No.: AR1660CCC500 **Data File :** PO113117.D **Time Analyzed:** 09:05

COMPOUND	RT	RT WINDOW		CALC AMOUNT(ng)	NOM AMOUNT(ng)	%D
		FROM	TO			
Aroclor-1016-1	4.747	4.648	4.848	552.430	500.000	10.5
Aroclor-1016-2	4.765	4.666	4.866	552.440	500.000	10.5
Aroclor-1016-3	4.822	4.724	4.924	557.870	500.000	11.6
Aroclor-1016-4	4.942	4.843	5.043	510.680	500.000	2.1
Aroclor-1016-5	5.198	5.099	5.299	539.090	500.000	7.8
Aroclor-1260-1	6.235	6.136	6.336	537.520	500.000	7.5
Aroclor-1260-2	6.424	6.326	6.526	537.480	500.000	7.5
Aroclor-1260-3	6.790	6.691	6.891	542.040	500.000	8.4
Aroclor-1260-4	7.049	6.951	7.151	538.930	500.000	7.8
Aroclor-1260-5	7.291	7.194	7.394	542.160	500.000	8.4
Decachlorobiphenyl	8.680	8.582	8.782	51.280	50.000	2.6
Tetrachloro-m-xylene	3.662	3.563	3.763	54.750	50.000	9.5



284 Sheffield Street, Mountainside, New Jersey 07092, Phone : 908 789 8900, Fax : 908 789 8922

CALIBRATION VERIFICATION SUMMARY

Lab Name: Alliance **Contract:** ATCE02
Lab Code: ACE **SDG NO.:** Q2894
GC Column: ZB-MR2 **ID:** 0.32 (mm) **Initi. Calib. Date(s):** 08/18/2025 08/18/2025

Client Sample No.: CCAL04 **Date Analyzed:** 08/21/2025
Lab Sample No.: AR1660CCC500 **Data File :** PO113117.D **Time Analyzed:** 09:05

COMPOUND	RT	RT WINDOW		CALC AMOUNT(ng)	NOM AMOUNT(ng)	%D
		FROM	TO			
Aroclor-1016-1	4.728	4.629	4.829	510.640	500.000	2.1
Aroclor-1016-2	4.746	4.647	4.847	506.950	500.000	1.4
Aroclor-1016-3	4.920	4.822	5.022	494.770	500.000	-1.0
Aroclor-1016-4	4.963	4.864	5.064	483.490	500.000	-3.3
Aroclor-1016-5	5.175	5.076	5.276	515.140	500.000	3.0
Aroclor-1260-1	6.202	6.104	6.304	487.740	500.000	-2.5
Aroclor-1260-2	6.391	6.292	6.492	485.740	500.000	-2.9
Aroclor-1260-3	6.542	6.443	6.643	461.000	500.000	-7.8
Aroclor-1260-4	7.011	6.912	7.112	477.600	500.000	-4.5
Aroclor-1260-5	7.253	7.155	7.355	470.110	500.000	-6.0
Decachlorobiphenyl	8.626	8.528	8.728	51.090	50.000	2.2
Tetrachloro-m-xylene	3.654	3.555	3.755	51.540	50.000	3.1

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0082125\
 Data File : PO113117.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 21 Aug 2025 09:05
 Operator : YP/AJ
 Sample : AR1660CCC500
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 AR1660CCC500

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 21 11:32:34 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0081825.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Aug 19 06:08:32 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.662	3.654	448.2E6	260.8E6	54.746	51.538
2) SA Decachlor...	8.680	8.626	355.5E6	96801540	51.282	51.087
Target Compounds						
3) L1 AR-1016-1	4.747	4.728	147.5E6	87101839	552.427	510.640
4) L1 AR-1016-2	4.765	4.746	221.8E6	130.6E6	552.441	506.952
5) L1 AR-1016-3	4.822	4.920	142.3E6	69077533	557.875	494.774
6) L1 AR-1016-4	4.942	4.963	111.4E6	56422466	510.678	483.487
7) L1 AR-1016-5	5.198	5.175	119.5E6	73423229	539.087	515.142
31) L7 AR-1260-1	6.235	6.202	239.7E6	124.4E6	537.519	487.738
32) L7 AR-1260-2	6.424	6.391	369.1E6	167.9E6	537.475	485.745
33) L7 AR-1260-3	6.790	6.542	334.7E6	137.1E6	542.037	460.999
34) L7 AR-1260-4	7.049	7.011	241.4E6	98982024	538.931	477.598
35) L7 AR-1260-5	7.291	7.253	656.4E6	220.2E6	542.163	470.110



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO082125\
Data File : PO113117.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 21 Aug 2025 09:05
Operator : YP/AJ
Sample : AR1660CCC500
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
AR1660CCC500

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 21 11:32:34 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO081825.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Aug 19 06:08:32 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

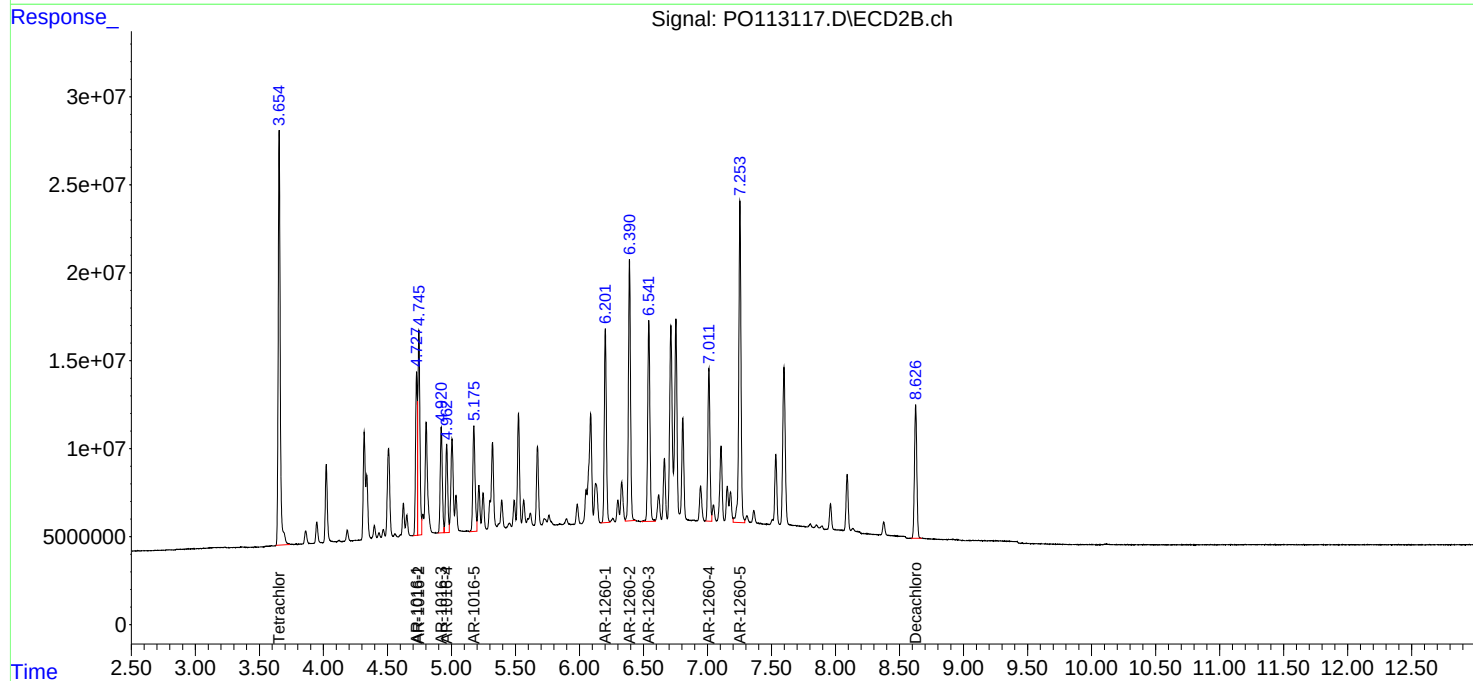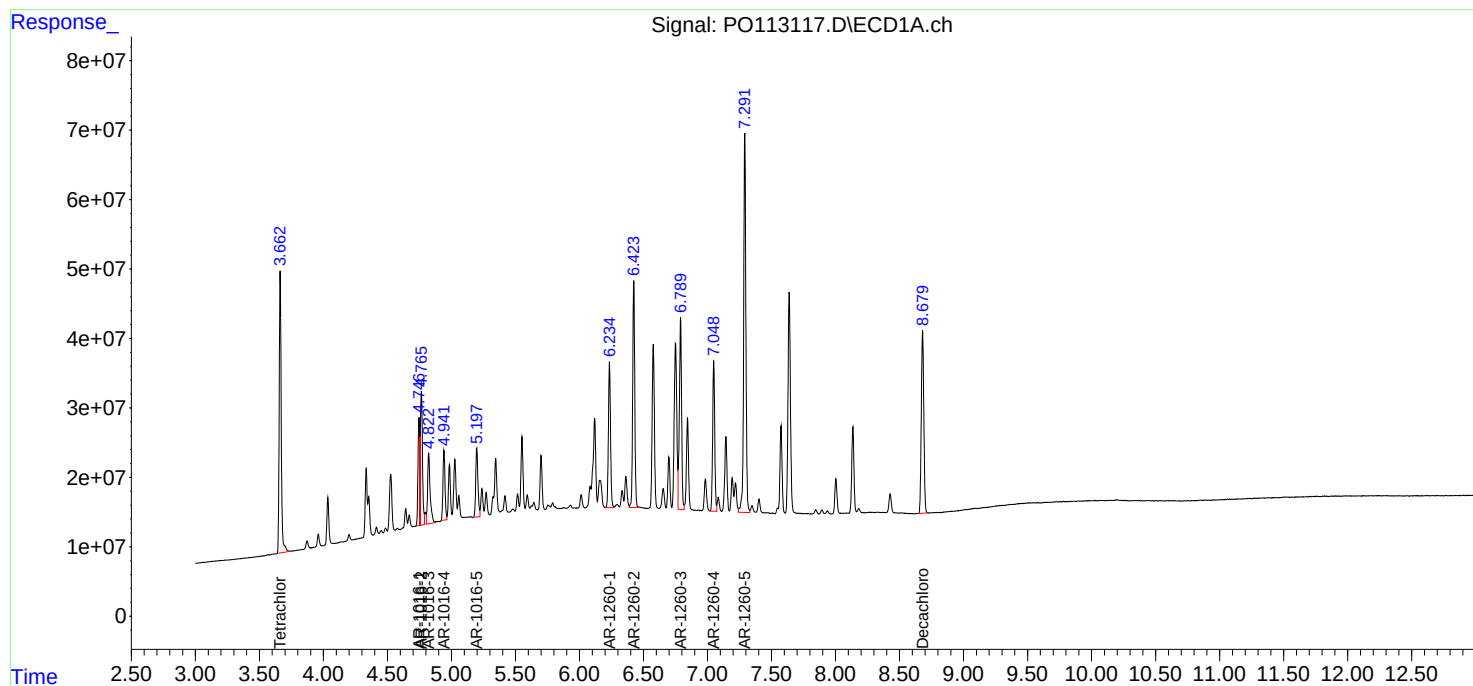



284 Sheffield Street, Mountainside, New Jersey 07092, Phone : 908 789 8900,
Fax : 908 789 8922

CALIBRATION VERIFICATION SUMMARY

Lab Name: Alliance

Contract: ATCE02

Lab Code: ACE

SDG NO.: Q2894

Continuing Calib Date: 08/21/2025

Initial Calibration Date(s): 08/18/2025 08/18/2025

Continuing Calib Time: 11:17

Initial Calibration Time(s): 09:53 18:24

GC Column: ZB-MR1 ID: 0.32 (mm)

COMPOUND		CCAL RT	AVG RT	RT WINDOW		DIFF RT
				FROM	TO	
Aroclor-1016-1	(1)	4.75	4.75	4.65	4.85	0.00
Aroclor-1016-2	(2)	4.77	4.77	4.67	4.87	0.01
Aroclor-1016-3	(3)	4.82	4.82	4.72	4.92	0.00
Aroclor-1016-4	(4)	4.94	4.94	4.84	5.04	0.00
Aroclor-1016-5	(5)	5.20	5.20	5.10	5.30	0.00
Aroclor-1260-1	(1)	6.23	6.24	6.14	6.34	0.01
Aroclor-1260-2	(2)	6.42	6.43	6.33	6.53	0.01
Aroclor-1260-3	(3)	6.79	6.79	6.69	6.89	0.00
Aroclor-1260-4	(4)	7.05	7.05	6.95	7.15	0.00
Aroclor-1260-5	(5)	7.29	7.29	7.19	7.39	0.00
Tetrachloro-m-xylene		3.66	3.66	3.56	3.76	0.00
Decachlorobiphenyl		8.68	8.68	8.58	8.78	0.00



284 Sheffield Street, Mountainside, New Jersey 07092, Phone : 908 789 8900,
Fax : 908 789 8922

CALIBRATION VERIFICATION SUMMARY

Lab Name: Alliance

Contract: ATCE02

Lab Code: ACE

SDG NO.: Q2894

Continuing Calib Date: 08/21/2025

Initial Calibration Date(s): 08/18/2025 08/18/2025

Continuing Calib Time: 11:17

Initial Calibration Time(s): 09:53 18:24

GC Column: ZB-MR2 ID: 0.32 (mm)

COMPOUND		CCAL RT	AVG RT	RT WINDOW		DIFF RT
				FROM	TO	
Aroclor-1016-1	(1)	4.73	4.73	4.63	4.83	0.00
Aroclor-1016-2	(2)	4.75	4.75	4.65	4.85	0.01
Aroclor-1016-3	(3)	4.92	4.92	4.82	5.02	0.00
Aroclor-1016-4	(4)	4.96	4.96	4.86	5.06	0.00
Aroclor-1016-5	(5)	5.18	5.18	5.08	5.28	0.00
Aroclor-1260-1	(1)	6.20	6.20	6.10	6.30	0.00
Aroclor-1260-2	(2)	6.39	6.39	6.29	6.49	0.00
Aroclor-1260-3	(3)	6.54	6.54	6.44	6.64	0.00
Aroclor-1260-4	(4)	7.01	7.01	6.91	7.11	0.00
Aroclor-1260-5	(5)	7.25	7.26	7.16	7.36	0.01
Tetrachloro-m-xylene		3.65	3.66	3.56	3.76	0.01
Decachlorobiphenyl		8.63	8.63	8.53	8.73	0.00



284 Sheffield Street, Mountainside, New Jersey 07092, Phone : 908 789 8900, Fax : 908 789 8922

CALIBRATION VERIFICATION SUMMARY

Lab Name: Alliance **Contract:** ATCE02
Lab Code: ACE **SDG NO.:** Q2894
GC Column: ZB-MR1 **ID:** 0.32 (mm) **Initi. Calib. Date(s):** 08/18/2025 08/18/2025

Client Sample No.: CCAL05 **Date Analyzed:** 08/21/2025
Lab Sample No.: AR1660CCC500 **Data File :** PO113121.D **Time Analyzed:** 11:17

COMPOUND	RT	RT WINDOW		CALC AMOUNT(ng)	NOM AMOUNT(ng)	%D
		FROM	TO			
Aroclor-1016-1	4.747	4.648	4.848	539.080	500.000	7.8
Aroclor-1016-2	4.765	4.666	4.866	539.140	500.000	7.8
Aroclor-1016-3	4.822	4.724	4.924	544.630	500.000	8.9
Aroclor-1016-4	4.941	4.843	5.043	497.690	500.000	-0.5
Aroclor-1016-5	5.198	5.099	5.299	530.520	500.000	6.1
Aroclor-1260-1	6.234	6.136	6.336	522.410	500.000	4.5
Aroclor-1260-2	6.424	6.326	6.526	524.960	500.000	5.0
Aroclor-1260-3	6.789	6.691	6.891	530.520	500.000	6.1
Aroclor-1260-4	7.049	6.951	7.151	528.340	500.000	5.7
Aroclor-1260-5	7.293	7.194	7.394	531.270	500.000	6.3
Decachlorobiphenyl	8.681	8.582	8.782	50.780	50.000	1.6
Tetrachloro-m-xylene	3.662	3.563	3.763	53.320	50.000	6.6



284 Sheffield Street, Mountainside, New Jersey 07092, Phone : 908 789 8900, Fax : 908 789 8922

CALIBRATION VERIFICATION SUMMARY

Lab Name: Alliance **Contract:** ATCE02
Lab Code: ACE **SDG NO.:** Q2894
GC Column: ZB-MR2 **ID:** 0.32 (mm) **Initi. Calib. Date(s):** 08/18/2025 08/18/2025

Client Sample No.: CCAL05 **Date Analyzed:** 08/21/2025
Lab Sample No.: AR1660CCC500 **Data File :** PO113121.D **Time Analyzed:** 11:17

COMPOUND	RT	RT WINDOW		CALC AMOUNT(ng)	NOM AMOUNT(ng)	%D
		FROM	TO			
Aroclor-1016-1	4.727	4.629	4.829	495.730	500.000	-0.9
Aroclor-1016-2	4.745	4.647	4.847	503.750	500.000	0.8
Aroclor-1016-3	4.920	4.822	5.022	486.710	500.000	-2.7
Aroclor-1016-4	4.963	4.864	5.064	477.370	500.000	-4.5
Aroclor-1016-5	5.175	5.076	5.276	505.560	500.000	1.1
Aroclor-1260-1	6.202	6.104	6.304	483.430	500.000	-3.3
Aroclor-1260-2	6.391	6.292	6.492	484.400	500.000	-3.1
Aroclor-1260-3	6.542	6.443	6.643	451.820	500.000	-9.6
Aroclor-1260-4	7.012	6.912	7.112	474.760	500.000	-5.0
Aroclor-1260-5	7.254	7.155	7.355	466.870	500.000	-6.6
Decachlorobiphenyl	8.626	8.528	8.728	50.470	50.000	0.9
Tetrachloro-m-xylene	3.654	3.555	3.755	50.740	50.000	1.5

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0082125\
 Data File : PO113121.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 21 Aug 2025 11:17
 Operator : YP/AJ
 Sample : AR1660CCC500
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 AR1660CCC500

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 21 11:39:50 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0081825.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Aug 19 06:08:32 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.662	3.654	436.5E6	256.8E6	53.321	50.739
2) SA Decachlor...	8.681	8.626	352.0E6	95627816	50.779	50.467
Target Compounds						
3) L1 AR-1016-1	4.747	4.727	143.9E6	84558715	539.077	495.731
4) L1 AR-1016-2	4.765	4.745	216.4E6	129.8E6	539.144	503.750
5) L1 AR-1016-3	4.822	4.920	138.9E6	67951488	544.629	486.708
6) L1 AR-1016-4	4.941	4.963	108.5E6	55708850	497.694	477.372
7) L1 AR-1016-5	5.198	5.175	117.6E6	72057111	530.524	505.558
31) L7 AR-1260-1	6.234	6.202	233.0E6	123.3E6	522.405	483.428
32) L7 AR-1260-2	6.424	6.391	360.5E6	167.5E6	524.963	484.404
33) L7 AR-1260-3	6.789	6.542	327.6E6	134.4E6	530.519	451.823
34) L7 AR-1260-4	7.049	7.012	236.6E6	98393332	528.342	474.758
35) L7 AR-1260-5	7.293	7.254	643.2E6	218.7E6	531.267	466.868



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO082125\
Data File : PO113121.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 21 Aug 2025 11:17
Operator : YP/AJ
Sample : AR1660CCC500
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
AR1660CCC500

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 21 11:39:50 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO081825.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Aug 19 06:08:32 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

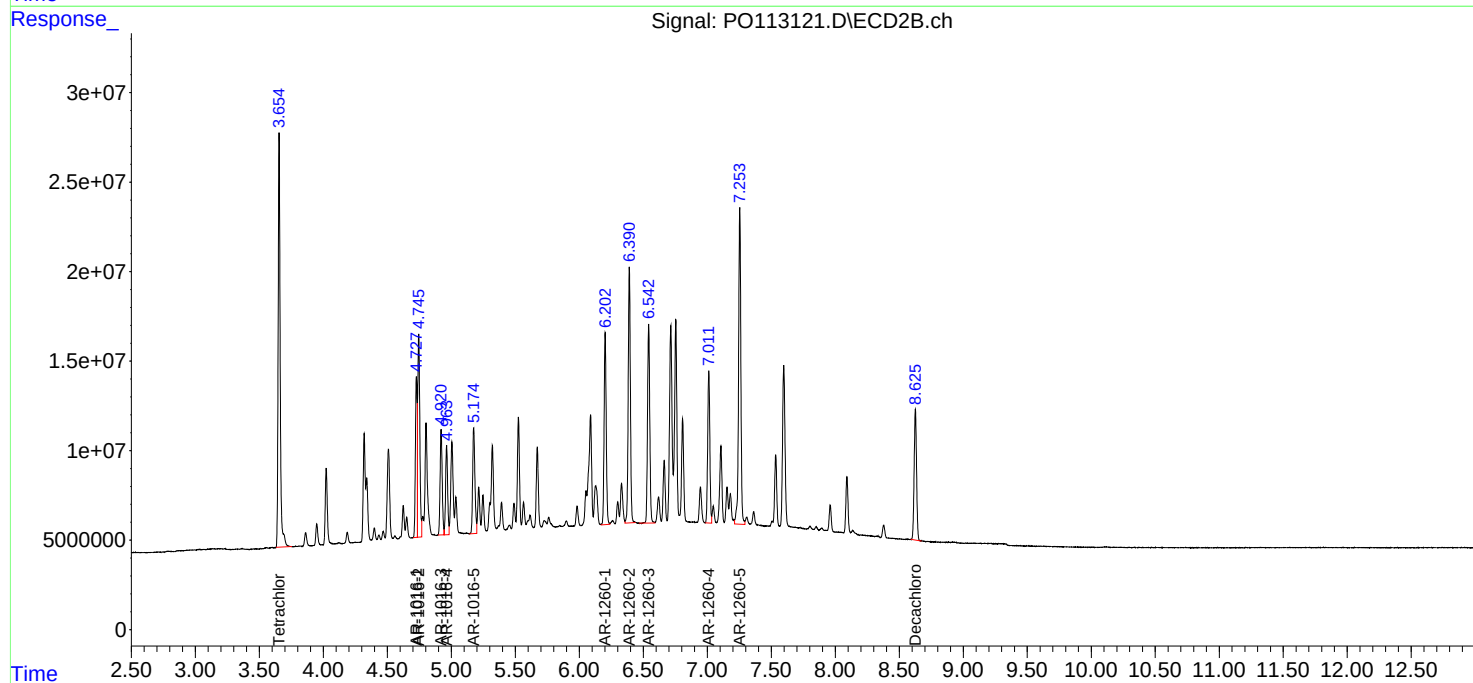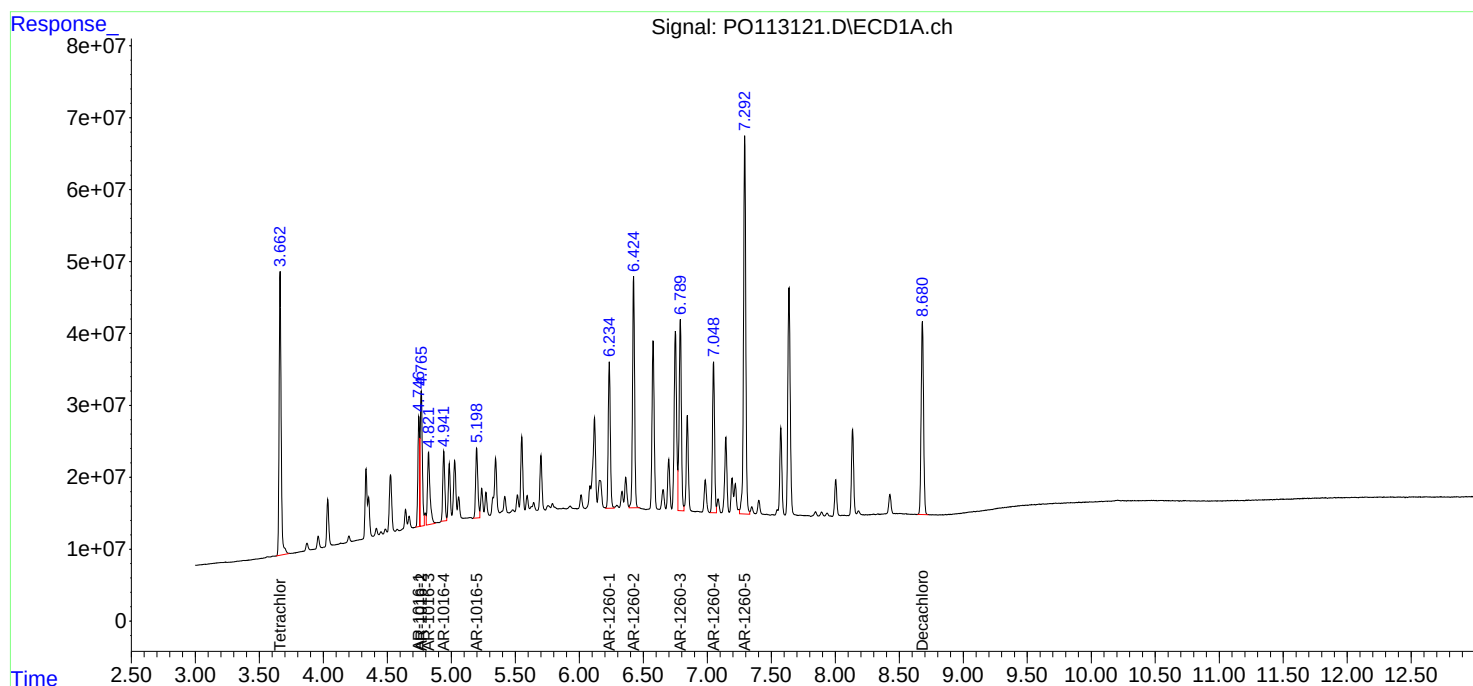

Analytical Sequence

Client: ATC Group Services LLC

SDG No.: Q2894

Project: PS 190 BK - 2025SCA056

Instrument ID: ECD_O

GC Column: ZB-MR1

ID: 0.32 (mm)

Inst. Calib. Date(s): 08/18/2025

08/18/2025

THE ANALYTICAL SEQUENCE OF PERFORMANCE EVALUATION MIXTURES, BLANKS, SAMPLES,
AND STANDARDS IS GIVEN BELOW:

CLIENT ID	LAB SAMPLE ID	DATE ANALYZED	TIME ANALYZED	DATAFILE	DCB RT #	TCX RT #
IBLK	IBLK	08/18/2025	09:34	PO113002.D	8.68	3.66
AR1660ICC1000	AR1660ICC1000	08/18/2025	09:53	PO113003.D	8.68	3.66
AR1660ICC750	AR1660ICC750	08/18/2025	10:11	PO113004.D	8.68	3.66
AR1660ICC500	AR1660ICC500	08/18/2025	10:29	PO113005.D	8.68	3.66
AR1660ICC250	AR1660ICC250	08/18/2025	10:48	PO113006.D	8.68	3.66
AR1660ICC050	AR1660ICC050	08/18/2025	11:06	PO113007.D	8.68	3.66
AR1221ICC500	AR1221ICC500	08/18/2025	11:25	PO113008.D	8.68	3.66
AR1232ICC500	AR1232ICC500	08/18/2025	11:43	PO113009.D	8.68	3.66
AR1242ICC1000	AR1242ICC1000	08/18/2025	12:01	PO113010.D	8.68	3.66
AR1242ICC750	AR1242ICC750	08/18/2025	12:20	PO113011.D	8.68	3.66
AR1242ICC500	AR1242ICC500	08/18/2025	12:38	PO113012.D	8.68	3.66
AR1242ICC250	AR1242ICC250	08/18/2025	12:57	PO113013.D	8.68	3.66
AR1242ICC050	AR1242ICC050	08/18/2025	13:15	PO113014.D	8.68	3.66
AR1248ICC1000	AR1248ICC1000	08/18/2025	13:34	PO113015.D	8.68	3.66
AR1248ICC750	AR1248ICC750	08/18/2025	13:52	PO113016.D	8.68	3.66
AR1248ICC500	AR1248ICC500	08/18/2025	14:09	PO113017.D	8.68	3.66
AR1248ICC250	AR1248ICC250	08/18/2025	14:28	PO113018.D	8.68	3.66
AR1248ICC050	AR1248ICC050	08/18/2025	14:46	PO113019.D	8.68	3.66
AR1254ICC1000	AR1254ICC1000	08/18/2025	15:05	PO113020.D	8.68	3.66
AR1254ICC750	AR1254ICC750	08/18/2025	15:23	PO113021.D	8.68	3.66
AR1254ICC500	AR1254ICC500	08/18/2025	15:41	PO113022.D	8.68	3.66
AR1254ICC250	AR1254ICC250	08/18/2025	16:00	PO113023.D	8.68	3.66
AR1254ICC050	AR1254ICC050	08/18/2025	16:18	PO113024.D	8.68	3.66
AR1262ICC500	AR1262ICC500	08/18/2025	16:54	PO113025.D	8.68	3.66
AR1268ICC1000	AR1268ICC1000	08/18/2025	17:12	PO113026.D	8.68	3.66
AR1268ICC750	AR1268ICC750	08/18/2025	17:30	PO113027.D	8.68	3.66
AR1268ICC500	AR1268ICC500	08/18/2025	17:48	PO113028.D	8.68	3.66
AR1268ICC250	AR1268ICC250	08/18/2025	18:06	PO113029.D	8.68	3.66
AR1268ICC050	AR1268ICC050	08/18/2025	18:24	PO113030.D	8.68	3.66
AR1660CCC500	AR1660CCC500	08/20/2025	09:33	PO113074.D	8.68	3.66
IBLK	IBLK	08/20/2025	10:47	PO113078.D	8.68	3.66
PB169322BS	PB169322BS	08/20/2025	12:19	PO113081.D	8.68	3.66
1A1B1C	Q2894-01	08/20/2025	12:36	PO113082.D	8.68	3.66
2A2B2C	Q2894-02	08/20/2025	12:55	PO113083.D	8.68	3.66
3A3B3C	Q2894-03	08/20/2025	13:13	PO113084.D	8.68	3.66
AR1660CCC500	AR1660CCC500	08/20/2025	15:39	PO113089.D	8.68	3.66
IBLK	IBLK	08/20/2025	16:50	PO113093.D	8.68	3.67
PB169322BL	PB169322BL	08/20/2025	17:09	PO113094.D	8.68	3.66
4A4B4C	Q2894-04	08/20/2025	18:03	PO113097.D	8.68	3.66
AR1660CCC500	AR1660CCC500	08/20/2025	21:05	PO113104.D	8.68	3.66
IBLK	IBLK	08/20/2025	22:37	PO113108.D	8.68	3.66
AR1660CCC500	AR1660CCC500	08/21/2025	09:05	PO113117.D	8.68	3.66

Analytical Sequence

I.BLK	I.BLK	08/21/2025	09:46	PO113118.D	8.69	3.67
5A5B5C	Q2894-05	08/21/2025	10:22	PO113120.D	8.68	3.66
AR1660CCC500	AR1660CCC500	08/21/2025	11:17	PO113121.D	8.68	3.66
I.BLK	I.BLK	08/21/2025	12:34	PO113125.D	8.68	3.66

Analytical Sequence

Client: ATC Group Services LLC

SDG No.: Q2894

Project: PS 190 BK - 2025SCA056

Instrument ID: ECD_O

GC Column: ZB-MR2

ID: 0.32 (mm)

Inst. Calib. Date(s): 08/18/2025 08/18/2025

THE ANALYTICAL SEQUENCE OF PERFORMANCE EVALUATION MIXTURES, BLANKS, SAMPLES,
AND STANDARDS IS GIVEN BELOW:

CLIENT ID	LAB SAMPLE ID	DATE ANALYZED	TIME ANALYZED	DATAFILE	DCB RT #	TCX RT #
IBLK	IBLK	08/18/2025	09:34	PO113002.D	8.63	3.66
AR1660ICC1000	AR1660ICC1000	08/18/2025	09:53	PO113003.D	8.63	3.66
AR1660ICC750	AR1660ICC750	08/18/2025	10:11	PO113004.D	8.63	3.66
AR1660ICC500	AR1660ICC500	08/18/2025	10:29	PO113005.D	8.63	3.66
AR1660ICC250	AR1660ICC250	08/18/2025	10:48	PO113006.D	8.63	3.66
AR1660ICC050	AR1660ICC050	08/18/2025	11:06	PO113007.D	8.63	3.65
AR1221ICC500	AR1221ICC500	08/18/2025	11:25	PO113008.D	8.63	3.66
AR1232ICC500	AR1232ICC500	08/18/2025	11:43	PO113009.D	8.63	3.66
AR1242ICC1000	AR1242ICC1000	08/18/2025	12:01	PO113010.D	8.63	3.66
AR1242ICC750	AR1242ICC750	08/18/2025	12:20	PO113011.D	8.63	3.66
AR1242ICC500	AR1242ICC500	08/18/2025	12:38	PO113012.D	8.63	3.66
AR1242ICC250	AR1242ICC250	08/18/2025	12:57	PO113013.D	8.63	3.66
AR1242ICC050	AR1242ICC050	08/18/2025	13:15	PO113014.D	8.63	3.66
AR1248ICC1000	AR1248ICC1000	08/18/2025	13:34	PO113015.D	8.63	3.66
AR1248ICC750	AR1248ICC750	08/18/2025	13:52	PO113016.D	8.63	3.66
AR1248ICC500	AR1248ICC500	08/18/2025	14:09	PO113017.D	8.63	3.66
AR1248ICC250	AR1248ICC250	08/18/2025	14:28	PO113018.D	8.63	3.66
AR1248ICC050	AR1248ICC050	08/18/2025	14:46	PO113019.D	8.63	3.66
AR1254ICC1000	AR1254ICC1000	08/18/2025	15:05	PO113020.D	8.63	3.66
AR1254ICC750	AR1254ICC750	08/18/2025	15:23	PO113021.D	8.63	3.66
AR1254ICC500	AR1254ICC500	08/18/2025	15:41	PO113022.D	8.63	3.66
AR1254ICC250	AR1254ICC250	08/18/2025	16:00	PO113023.D	8.63	3.66
AR1254ICC050	AR1254ICC050	08/18/2025	16:18	PO113024.D	8.63	3.66
AR1262ICC500	AR1262ICC500	08/18/2025	16:54	PO113025.D	8.63	3.66
AR1268ICC1000	AR1268ICC1000	08/18/2025	17:12	PO113026.D	8.63	3.66
AR1268ICC750	AR1268ICC750	08/18/2025	17:30	PO113027.D	8.63	3.66
AR1268ICC500	AR1268ICC500	08/18/2025	17:48	PO113028.D	8.63	3.66
AR1268ICC250	AR1268ICC250	08/18/2025	18:06	PO113029.D	8.63	3.66
AR1268ICC050	AR1268ICC050	08/18/2025	18:24	PO113030.D	8.63	3.66
AR1660CCC500	AR1660CCC500	08/20/2025	09:33	PO113074.D	8.63	3.66
IBLK	IBLK	08/20/2025	10:47	PO113078.D	8.63	3.66
PB169322BS	PB169322BS	08/20/2025	12:19	PO113081.D	8.63	3.66
1A1B1C	Q2894-01	08/20/2025	12:36	PO113082.D	8.63	3.66
2A2B2C	Q2894-02	08/20/2025	12:55	PO113083.D	8.63	3.66
3A3B3C	Q2894-03	08/20/2025	13:13	PO113084.D	8.63	3.66
AR1660CCC500	AR1660CCC500	08/20/2025	15:39	PO113089.D	8.63	3.66
IBLK	IBLK	08/20/2025	16:50	PO113093.D	8.63	3.66
PB169322BL	PB169322BL	08/20/2025	17:09	PO113094.D	8.63	3.66
4A4B4C	Q2894-04	08/20/2025	18:03	PO113097.D	8.63	3.66
AR1660CCC500	AR1660CCC500	08/20/2025	21:05	PO113104.D	8.63	3.65
IBLK	IBLK	08/20/2025	22:37	PO113108.D	8.63	3.66
AR1660CCC500	AR1660CCC500	08/21/2025	09:05	PO113117.D	8.63	3.65

Analytical Sequence

I.BLK	I.BLK	08/21/2025	09:46	PO113118.D	8.63	3.65
5A5B5C	Q2894-05	08/21/2025	10:22	PO113120.D	8.62	3.65
AR1660CCC500	AR1660CCC500	08/21/2025	11:17	PO113121.D	8.63	3.65
I.BLK	I.BLK	08/21/2025	12:34	PO113125.D	8.63	3.65



284 Sheffield Street, Mountainside, New Jersey 07092, Phone : 908 789 8900,
Fax : 908 789 8922

IDENTIFICATION SUMMARY
FOR MULTICOMPONENT ANALYTES

SAMPLE NO.

PB169322BS

Lab Name: Alliance

Contract: ATCE02

Lab Code: ACE

SDG NO.: Q2894

Lab Sample ID: PB169322BS

Date(s) Analyzed: 08/20/2025 08/20/2025

Instrument ID (1): ECD_O

Instrument ID (2): ECD_O

GC Column: (1): ZB-MR1 ID: 0.32 (mm)

GC Column: (2): ZB-MR2 ID: 0.32 (mm)

Data file PO113081.D

ANALYTE	COL	RT	RT WINDOW		CONCENTRATION	MEAN CONCENTRATION	%RPD
			FROM	TO			
Aroclor-1016	1	4.748	4.698	4.798	181	178	6.98
COLUMN 1	2	4.766	4.716	4.816	185		
	3	4.823	4.773	4.873	182		
	4	4.942	4.892	4.992	170		
	5	5.199	5.149	5.249	172		
COLUMN 2	1	4.728	4.678	4.778	173	166	
	2	4.746	4.696	4.796	168		
	3	4.921	4.871	4.971	164		
	4	4.964	4.914	5.014	157		
	5	5.175	5.125	5.225	166		
Aroclor-1260	1	6.235	6.185	6.285	188	171	5.41
COLUMN 1	2	6.425	6.375	6.475	185		
	3	6.79	6.74	6.84	163		
	4	7.049	6.999	7.099	167		
	5	7.292	7.242	7.342	151		
COLUMN 2	1	6.202	6.152	6.252	173	162	
	2	6.391	6.341	6.441	171		
	3	6.542	6.492	6.592	165		
	4	7.011	6.961	7.061	150		
	5	7.253	7.203	7.303	152		



QC SAMPLE DATA

Report of Analysis

Client:	ATC Group Services LLC	Date Collected:	
Project:	PS 190 BK - 2025SCA056	Date Received:	
Client Sample ID:	PB169322BL	SDG No.:	Q2894
Lab Sample ID:	PB169322BL	Matrix:	SOIL
Analytical Method:	8082A	% Solid:	100
Sample Wt/Vol:	30.01	Units:	g
Soil Aliquot Vol:			uL
Extraction Type:		Test:	PCB
GPC Factor :	1.0	PH :	
Prep Method :	SW3541B	Injection Volume :	

File ID/Qc Batch:	Dilution:	Prep Date	Date Analyzed	Prep Batch ID
PO113094.D	1	08/20/25 08:40	08/20/25 17:09	PB169322

CAS Number	Parameter	Conc.	Qualifier	MDL	LOQ / CRQL	Units(Dry Weight)
TARGETS						
12674-11-2	Aroclor-1016	3.90	U	3.90	17.0	ug/kg
11104-28-2	Aroclor-1221	4.00	U	4.00	17.0	ug/kg
11141-16-5	Aroclor-1232	3.70	U	3.70	17.0	ug/kg
53469-21-9	Aroclor-1242	4.00	U	4.00	17.0	ug/kg
12672-29-6	Aroclor-1248	5.90	U	5.90	17.0	ug/kg
11097-69-1	Aroclor-1254	3.20	U	3.20	17.0	ug/kg
37324-23-5	Aroclor-1262	5.00	U	5.00	17.0	ug/kg
11100-14-4	Aroclor-1268	3.60	U	3.60	17.0	ug/kg
11096-82-5	Aroclor-1260	3.20	U	3.20	17.0	ug/kg
SURROGATES						
877-09-8	Tetrachloro-m-xylene	18.8		32 - 144	94%	SPK: 20
2051-24-3	Decachlorobiphenyl	20.2		32 - 175	101%	SPK: 20

Comments:

U = Not Detected

LOQ = Limit of Quantitation

MDL = Method Detection Limit

LOD = Limit of Detection

E = Value Exceeds Calibration Range

P = Indicates >25% difference for detected concentrations between the two GC columns

Q = indicates LCS control criteria did not meet requirements

M = MS/MSD acceptance criteria did not meet requirements

J = Estimated Value

B = Analyte Found in Associated Method Blank

N = Presumptive Evidence of a Compound

* = Values outside of QC limits

D = Dilution

S = Indicates estimated value where valid five-point calibration was not performed prior to analyte detection in sample.

() = Laboratory InHouse Limit

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0082025\
Data File : P0113094.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 20 Aug 2025 17:09
Operator : YP/AJ
Sample : PB169322BL
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
PB169322BL

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 21 01:41:17 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0081825.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Aug 19 06:08:32 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.664	3.656	153.6E6	91636566	18.759	18.108
2) SA Decachlor...	8.681	8.627	140.0E6	36609486	20.192	19.321

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO082025\
Data File : PO113094.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 20 Aug 2025 17:09
Operator : YP/AJ
Sample : PB169322BL
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
PB169322BL

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 21 01:41:17 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO081825.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Aug 19 06:08:32 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

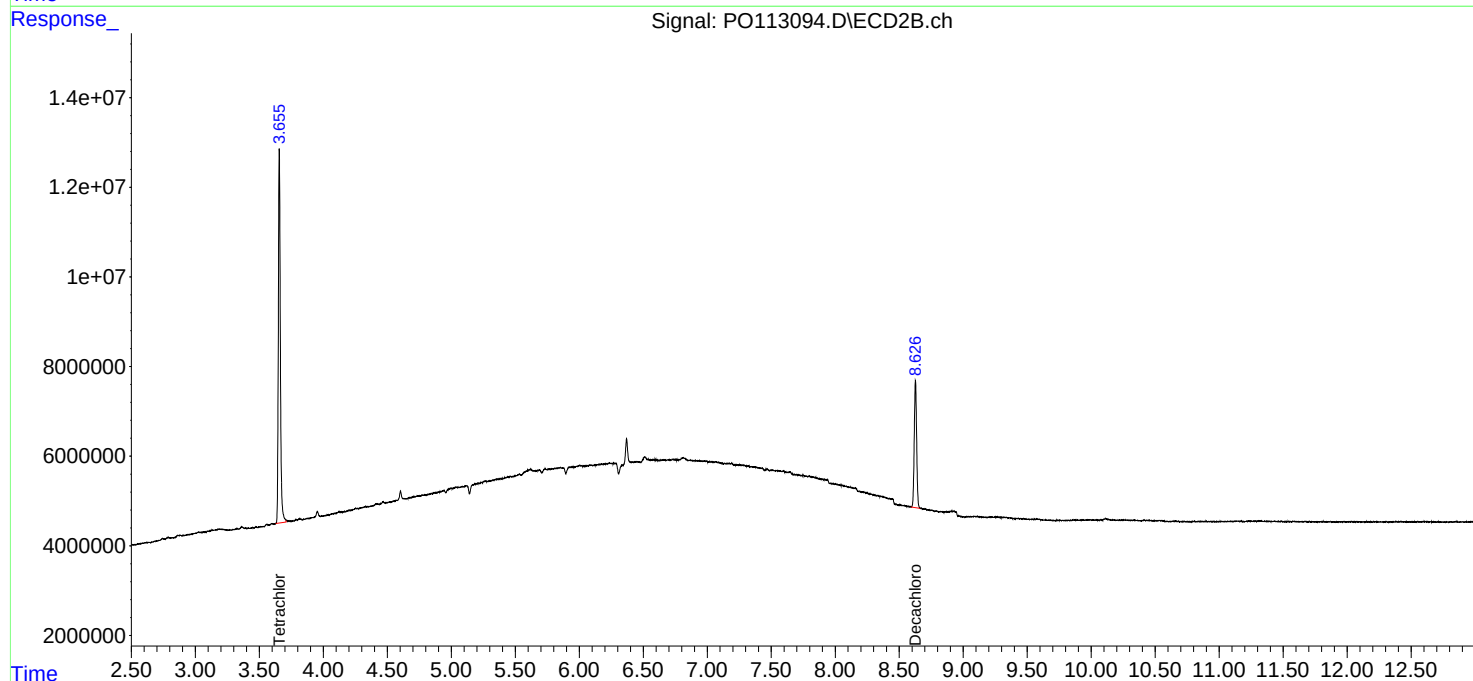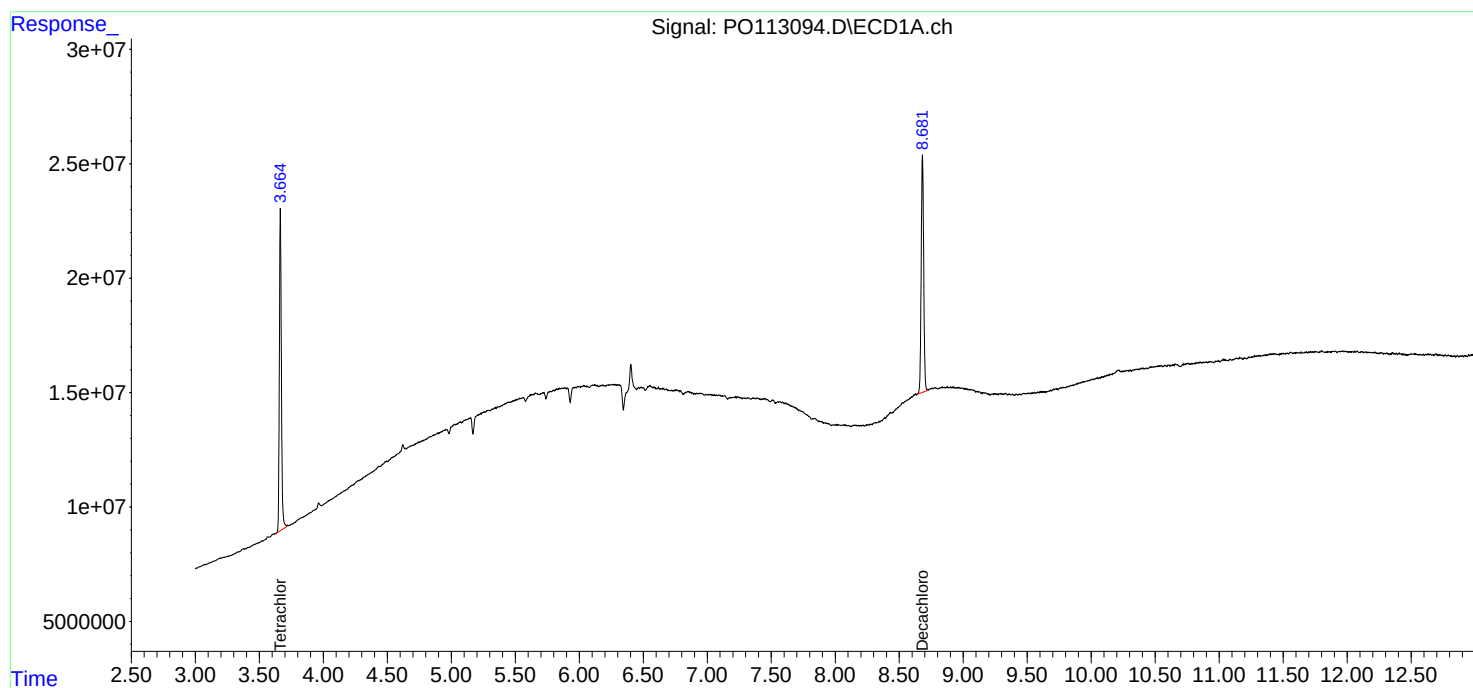


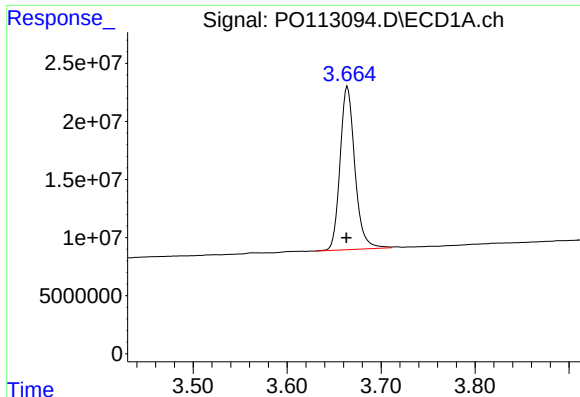

#1 Tetrachloro-m-xylene


R.T.: 3.664 min
Delta R.T.: 0.001 min
Response: 153572084
Conc: 18.76 ng/ml

Instrument :
ECD_O
ClientSampleId :
PB169322BL

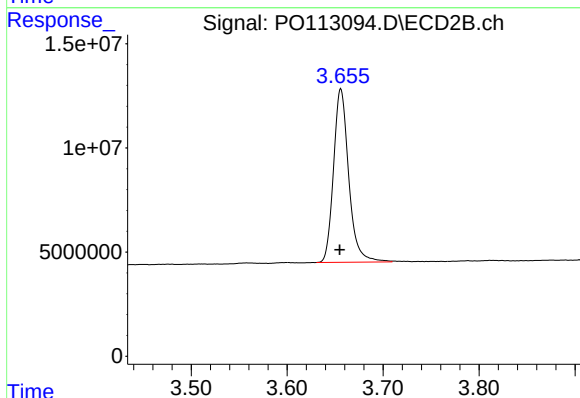


#1 Tetrachloro-m-xylene

R.T.: 3.656 min
Delta R.T.: 0.000 min
Response: 91636566
Conc: 18.11 ng/ml

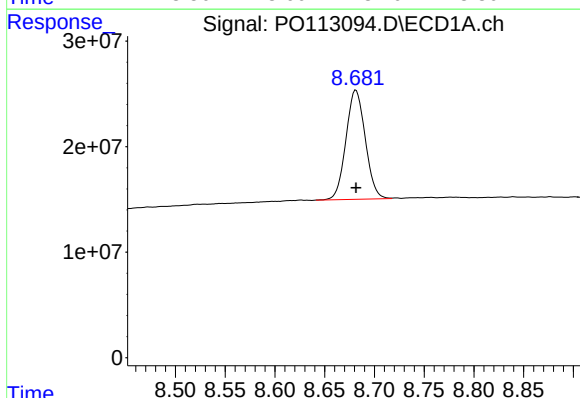

#2 Decachlorobiphenyl

R.T.: 8.681 min
Delta R.T.: 0.000 min
Response: 139957236
Conc: 20.19 ng/ml

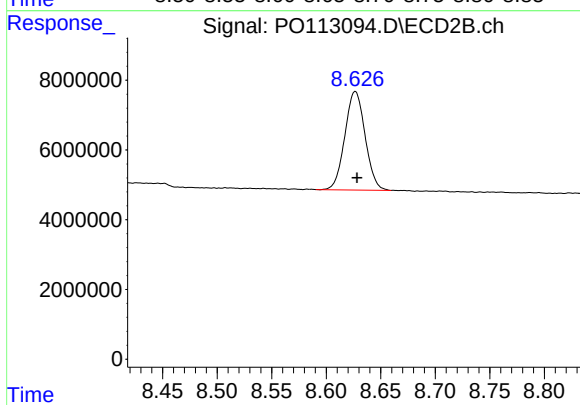

#2 Decachlorobiphenyl

R.T.: 8.627 min
Delta R.T.: -0.002 min
Response: 36609486
Conc: 19.32 ng/ml

Report of Analysis

Client:	ATC Group Services LLC		Date Collected:	08/18/25	
Project:	PS 190 BK - 2025SCA056		Date Received:	08/18/25	
Client Sample ID:	PIBLK-PO113002.D		SDG No.:	Q2894	
Lab Sample ID:	I.BLK-PO113002.D		Matrix:	WATER	
Analytical Method:	8082A		% Solid:	0	Decanted:
Sample Wt/Vol:	1000	Units: mL	Final Vol:	10000	uL
Soil Aliquot Vol:		uL	Test:	PCB	
Extraction Type:			Injection Volume :		
GPC Factor :	1.0	PH :			
Prep Method :	5030				

File ID/Qc Batch:	Dilution:	Prep Date	Date Analyzed	Prep Batch ID
PO113002.D	1		08/18/25	PO081825

CAS Number	Parameter	Conc.	Qualifier	MDL	LOQ / CRQL	Units
TARGETS						
12674-11-2	Aroclor-1016	0.097	U	0.097	0.50	ug/L
11104-28-2	Aroclor-1221	0.13	U	0.13	0.50	ug/L
11141-16-5	Aroclor-1232	0.096	U	0.096	0.50	ug/L
53469-21-9	Aroclor-1242	0.12	U	0.12	0.50	ug/L
12672-29-6	Aroclor-1248	0.071	U	0.071	0.50	ug/L
11097-69-1	Aroclor-1254	0.094	U	0.094	0.50	ug/L
11096-82-5	Aroclor-1260	0.081	U	0.081	0.50	ug/L
37324-23-5	Aroclor-1262	0.14	U	0.14	0.50	ug/L
11100-14-4	Aroclor-1268	0.11	U	0.11	0.50	ug/L
SURROGATES						
877-09-8	Tetrachloro-m-xylene	16.6		60 - 140	83%	SPK: 20
2051-24-3	Decachlorobiphenyl	17.2		60 - 140	86%	SPK: 20

Comments:

U = Not Detected
 LOQ = Limit of Quantitation
 MDL = Method Detection Limit
 LOD = Limit of Detection
 E = Value Exceeds Calibration Range
 P = Indicates >25% difference for detected concentrations between the two GC columns
 Q = indicates LCS control criteria did not meet requirements
 M = MS/MSD acceptance criteria did not meet requirements

J = Estimated Value
 B = Analyte Found in Associated Method Blank
 N = Presumptive Evidence of a Compound
 * = Values outside of QC limits
 D = Dilution
 S = Indicates estimated value where valid five-point calibration was not performed prior to analyte detection in sample.
 () = Laboratory InHouse Limit

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO081825\
 Data File : PO113002.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 18 Aug 2025 09:34
 Operator : YP/AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 I.BLK

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 19 06:11:43 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO081825.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Aug 19 06:08:32 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.663	3.655	136.1E6	85350797	16.620	16.866
2) SA Decachlor...	8.682	8.627	119.0E6	34312580	17.168	18.108

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO081825\
Data File : PO113002.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 18 Aug 2025 09:34
Operator : YP/AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
I.BLK

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 19 06:11:43 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO081825.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Aug 19 06:08:32 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

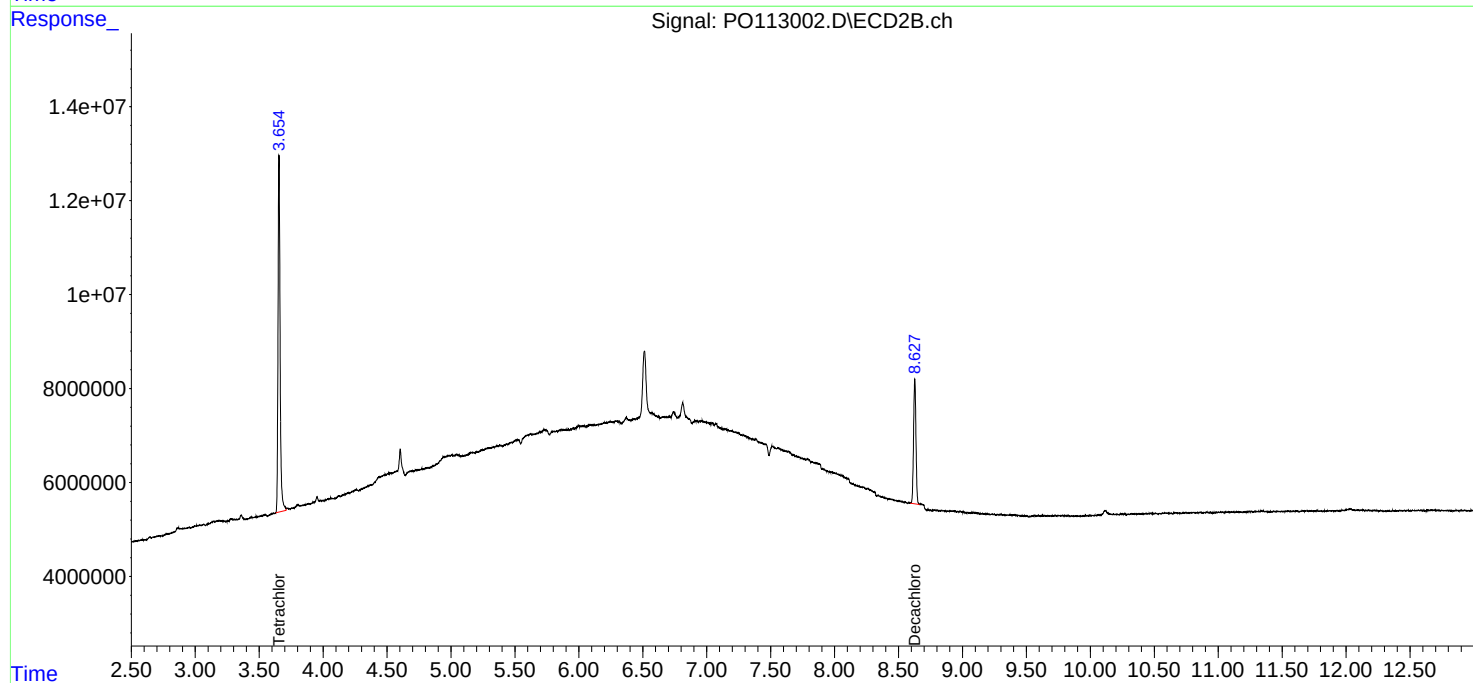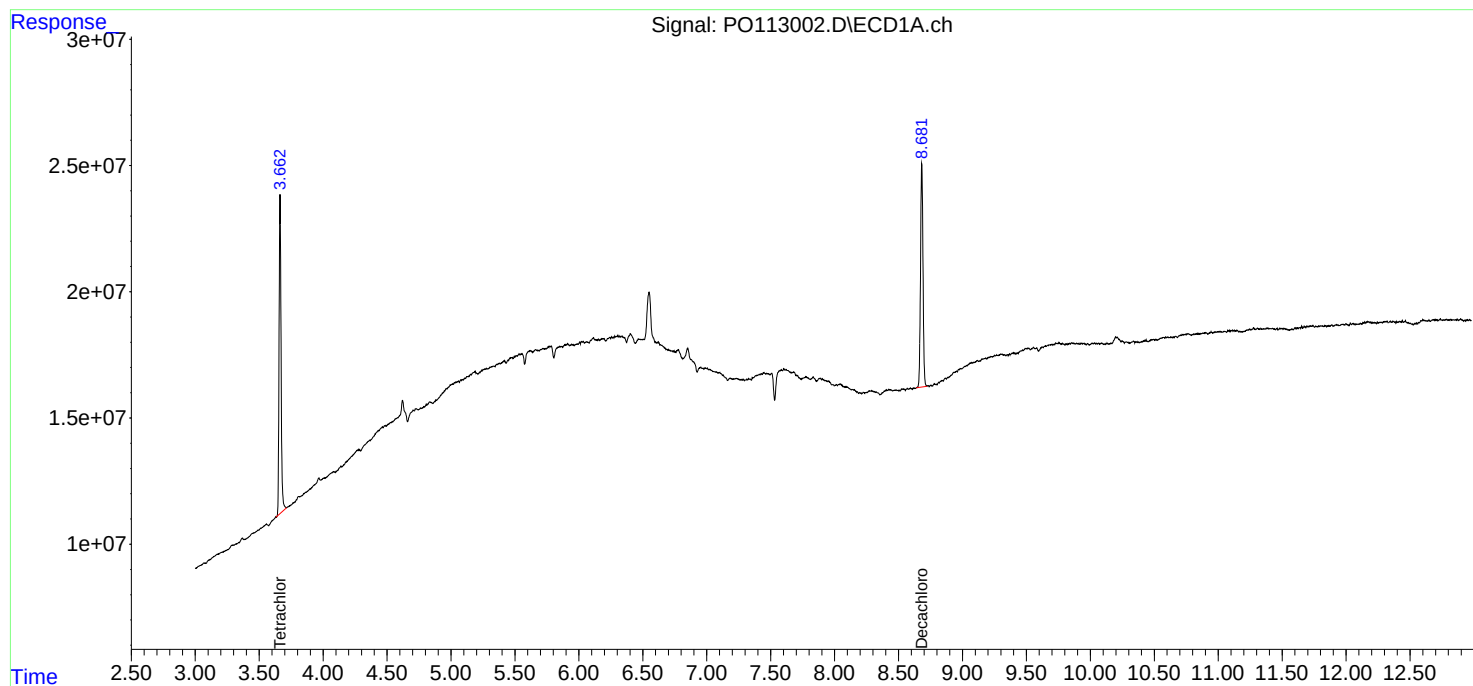


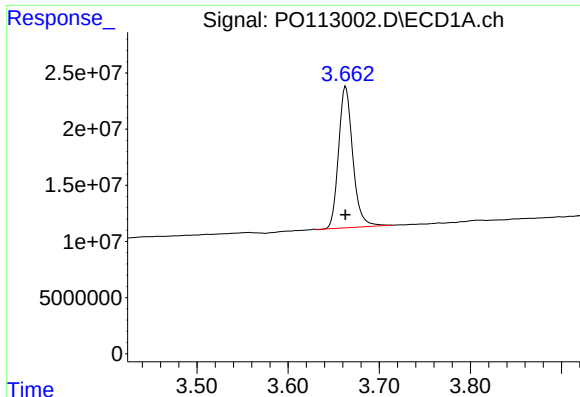

#1 Tetrachloro-m-xylene


R.T.: 3.663 min
Delta R.T.: 0.000 min
Response: 136059721
Conc: 16.62 ng/ml

Instrument :
ECD_O
ClientSampleId :
I.BLK

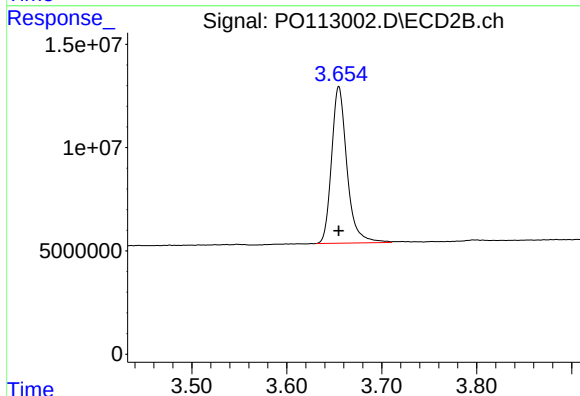


#1 Tetrachloro-m-xylene

R.T.: 3.655 min
Delta R.T.: 0.000 min
Response: 85350797
Conc: 16.87 ng/ml

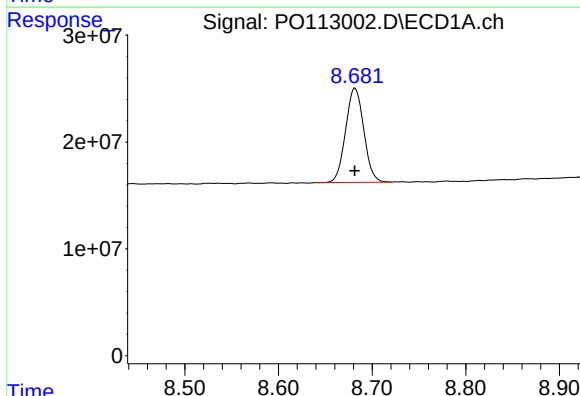

#2 Decachlorobiphenyl

R.T.: 8.682 min
Delta R.T.: 0.000 min
Response: 119000321
Conc: 17.17 ng/ml

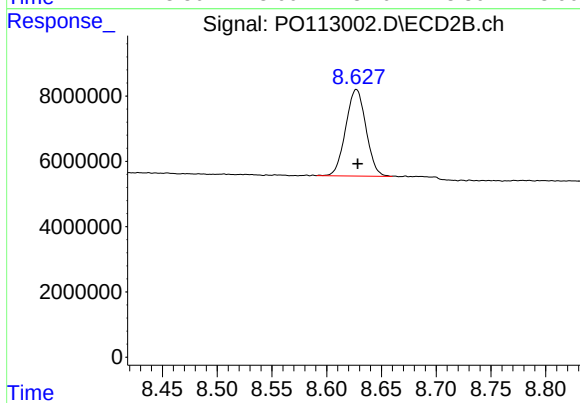

#2 Decachlorobiphenyl

R.T.: 8.627 min
Delta R.T.: -0.001 min
Response: 34312580
Conc: 18.11 ng/ml

Report of Analysis

Client:	ATC Group Services LLC	Date Collected:	08/20/25
Project:	PS 190 BK - 2025SCA056	Date Received:	08/20/25
Client Sample ID:	PIBLK-PO113078.D	SDG No.:	Q2894
Lab Sample ID:	I.BLK-PO113078.D	Matrix:	WATER
Analytical Method:	8082A	% Solid:	0
Sample Wt/Vol:	1000	Units:	mL
Soil Aliquot Vol:			uL
Extraction Type:		Test:	PCB
GPC Factor :	1.0	PH :	
Prep Method :	5030	Injection Volume :	

File ID/Qc Batch:	Dilution:	Prep Date	Date Analyzed	Prep Batch ID
PO113078.D	1		08/20/25	PO082025

CAS Number	Parameter	Conc.	Qualifier	MDL	LOQ / CRQL	Units
TARGETS						
12674-11-2	Aroclor-1016	0.097	U	0.097	0.50	ug/L
11104-28-2	Aroclor-1221	0.13	U	0.13	0.50	ug/L
11141-16-5	Aroclor-1232	0.096	U	0.096	0.50	ug/L
53469-21-9	Aroclor-1242	0.12	U	0.12	0.50	ug/L
12672-29-6	Aroclor-1248	0.071	U	0.071	0.50	ug/L
11097-69-1	Aroclor-1254	0.094	U	0.094	0.50	ug/L
11096-82-5	Aroclor-1260	0.081	U	0.081	0.50	ug/L
37324-23-5	Aroclor-1262	0.14	U	0.14	0.50	ug/L
11100-14-4	Aroclor-1268	0.11	U	0.11	0.50	ug/L
SURROGATES						
877-09-8	Tetrachloro-m-xylene	17.5		60 - 140	88%	SPK: 20
2051-24-3	Decachlorobiphenyl	15.8		60 - 140	79%	SPK: 20

Comments:

U = Not Detected

LOQ = Limit of Quantitation

MDL = Method Detection Limit

LOD = Limit of Detection

E = Value Exceeds Calibration Range

P = Indicates >25% difference for detected concentrations between the two GC columns

Q = indicates LCS control criteria did not meet requirements

M = MS/MSD acceptance criteria did not meet requirements

J = Estimated Value

B = Analyte Found in Associated Method Blank

N = Presumptive Evidence of a Compound

* = Values outside of QC limits

D = Dilution

S = Indicates estimated value where valid five-point calibration was not performed prior to analyte detection in sample.

() = Laboratory InHouse Limit

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0082025\
Data File : PO113078.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 20 Aug 2025 10:47
Operator : YP/AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
I.BLK

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 20 13:03:38 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0081825.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Aug 19 06:08:32 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.664	3.656	148.3E6	88565651	18.118	17.501
2) SA Decachlor...	8.680	8.627	109.6E6	32428852	15.811	17.114

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO082025\
Data File : PO113078.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 20 Aug 2025 10:47
Operator : YP/AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
I.BLK

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 20 13:03:38 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO081825.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Aug 19 06:08:32 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

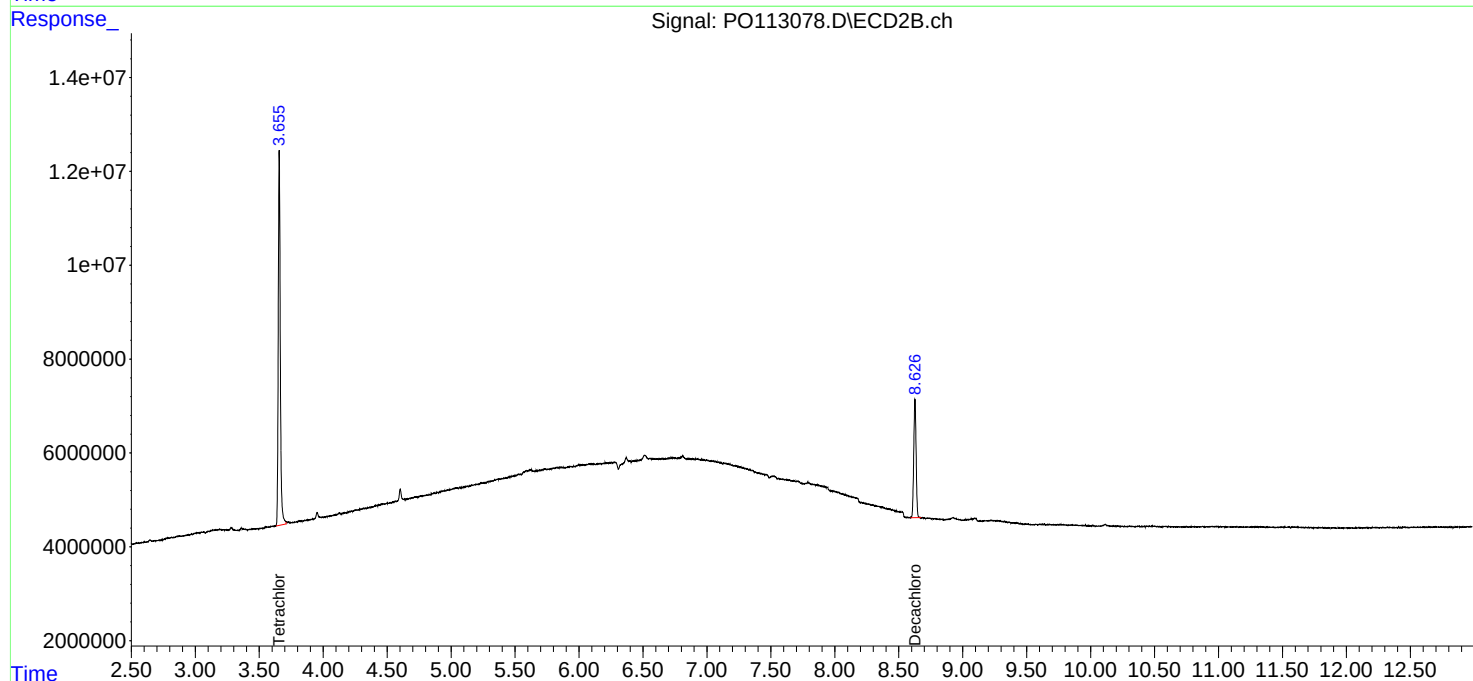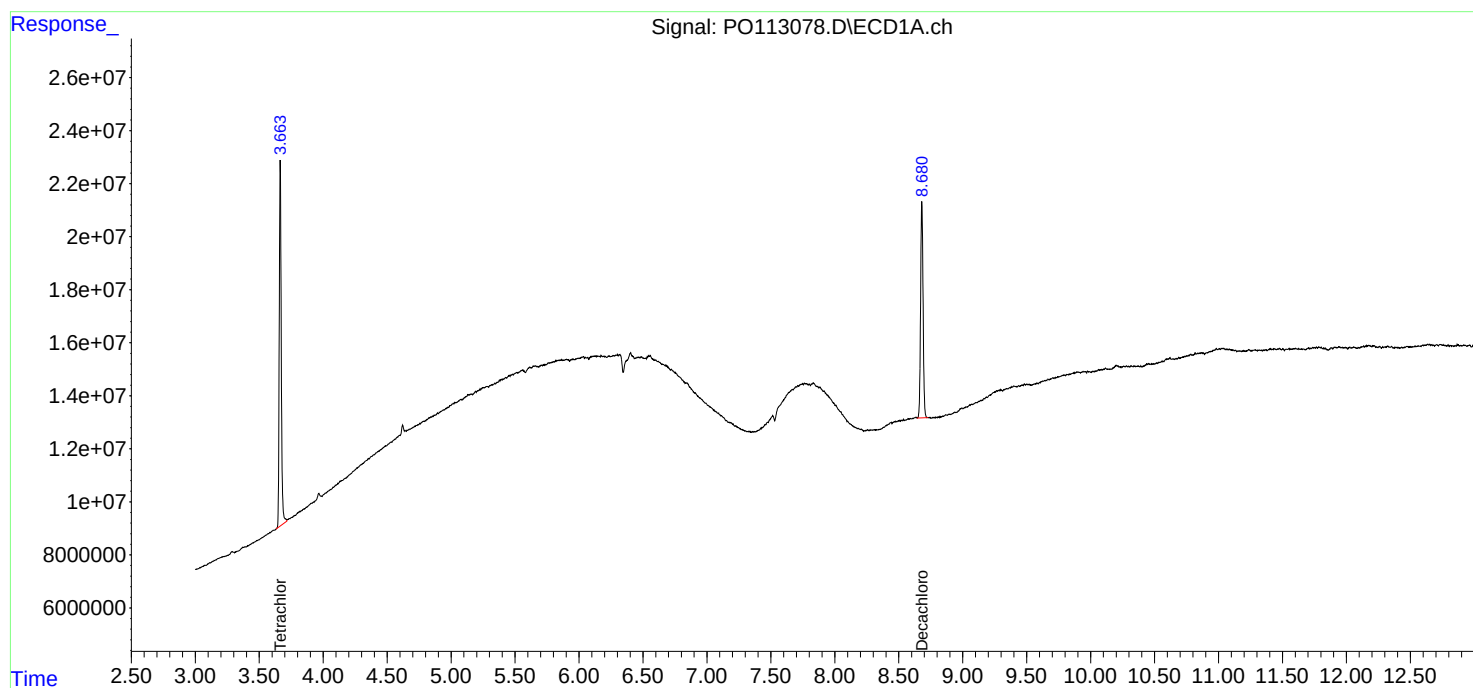


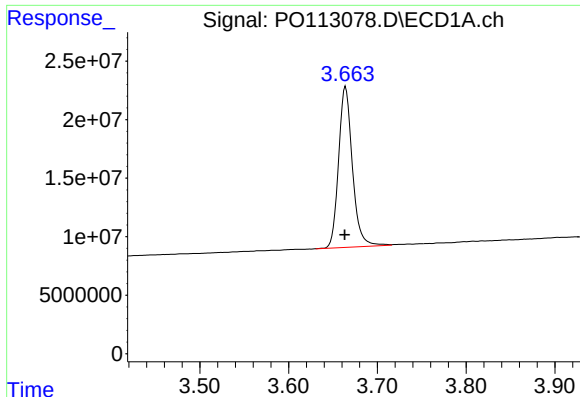

#1 Tetrachloro-m-xylene


R.T.: 3.664 min
Delta R.T.: 0.001 min
Response: 148323427
Conc: 18.12 ng/ml

Instrument :
ECD_O
ClientSampleId :
I.BLK

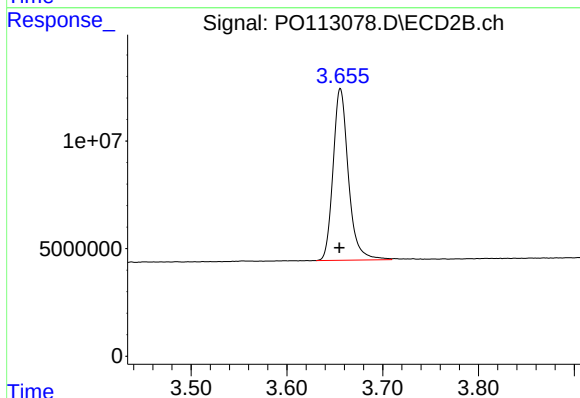


#1 Tetrachloro-m-xylene

R.T.: 3.656 min
Delta R.T.: 0.001 min
Response: 88565651
Conc: 17.50 ng/ml

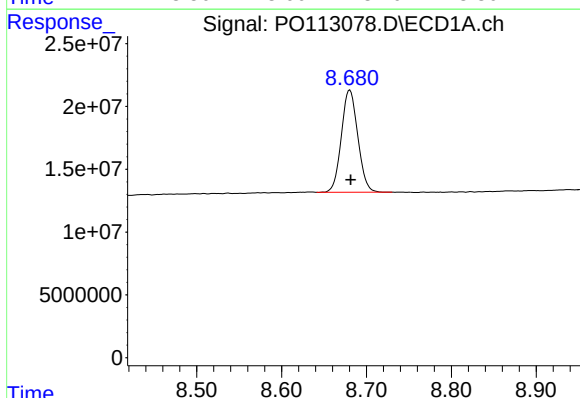

#2 Decachlorobiphenyl

R.T.: 8.680 min
Delta R.T.: -0.001 min
Response: 109595923
Conc: 15.81 ng/ml

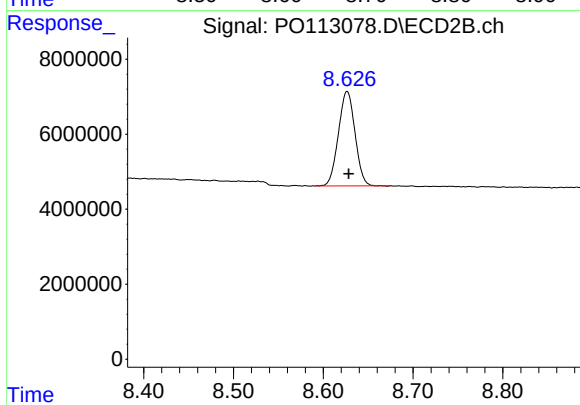

#2 Decachlorobiphenyl

R.T.: 8.627 min
Delta R.T.: -0.002 min
Response: 32428852
Conc: 17.11 ng/ml

Report of Analysis

Client:	ATC Group Services LLC	Date Collected:	08/20/25
Project:	PS 190 BK - 2025SCA056	Date Received:	08/20/25
Client Sample ID:	PIBLK-PO113093.D	SDG No.:	Q2894
Lab Sample ID:	I.BLK-PO113093.D	Matrix:	WATER
Analytical Method:	8082A	% Solid:	0
Sample Wt/Vol:	1000	Units:	mL
Soil Aliquot Vol:			uL
Extraction Type:		Test:	PCB
GPC Factor :	1.0	PH :	
Prep Method :	5030	Injection Volume :	

File ID/Qc Batch:	Dilution:	Prep Date	Date Analyzed	Prep Batch ID
PO113093.D	1		08/20/25	po082025

CAS Number	Parameter	Conc.	Qualifier	MDL	LOQ / CRQL	Units
TARGETS						
12674-11-2	Aroclor-1016	0.097	U	0.097	0.50	ug/L
11104-28-2	Aroclor-1221	0.13	U	0.13	0.50	ug/L
11141-16-5	Aroclor-1232	0.096	U	0.096	0.50	ug/L
53469-21-9	Aroclor-1242	0.12	U	0.12	0.50	ug/L
12672-29-6	Aroclor-1248	0.071	U	0.071	0.50	ug/L
11097-69-1	Aroclor-1254	0.094	U	0.094	0.50	ug/L
11096-82-5	Aroclor-1260	0.081	U	0.081	0.50	ug/L
37324-23-5	Aroclor-1262	0.14	U	0.14	0.50	ug/L
11100-14-4	Aroclor-1268	0.11	U	0.11	0.50	ug/L
SURROGATES						
877-09-8	Tetrachloro-m-xylene	17.3		60 - 140	86%	SPK: 20
2051-24-3	Decachlorobiphenyl	18.3		60 - 140	92%	SPK: 20

Comments:

U = Not Detected

LOQ = Limit of Quantitation

MDL = Method Detection Limit

LOD = Limit of Detection

E = Value Exceeds Calibration Range

P = Indicates >25% difference for detected concentrations between the two GC columns

Q = indicates LCS control criteria did not meet requirements

M = MS/MSD acceptance criteria did not meet requirements

J = Estimated Value

B = Analyte Found in Associated Method Blank

N = Presumptive Evidence of a Compound

* = Values outside of QC limits

D = Dilution

S = Indicates estimated value where valid five-point calibration was not performed prior to analyte detection in sample.

() = Laboratory InHouse Limit

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0082025\
Data File : PO113093.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 20 Aug 2025 16:50
Operator : YP/AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
I.BLK

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 21 01:41:03 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0081825.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Aug 19 06:08:32 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.665	3.657	144.5E6	87439348	17.654	17.278
2) SA Decachlor...	8.681	8.627	131.7E6	34729368	18.998	18.328

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO082025\
Data File : PO113093.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 20 Aug 2025 16:50
Operator : YP/AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
I.BLK

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 21 01:41:03 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO081825.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Aug 19 06:08:32 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

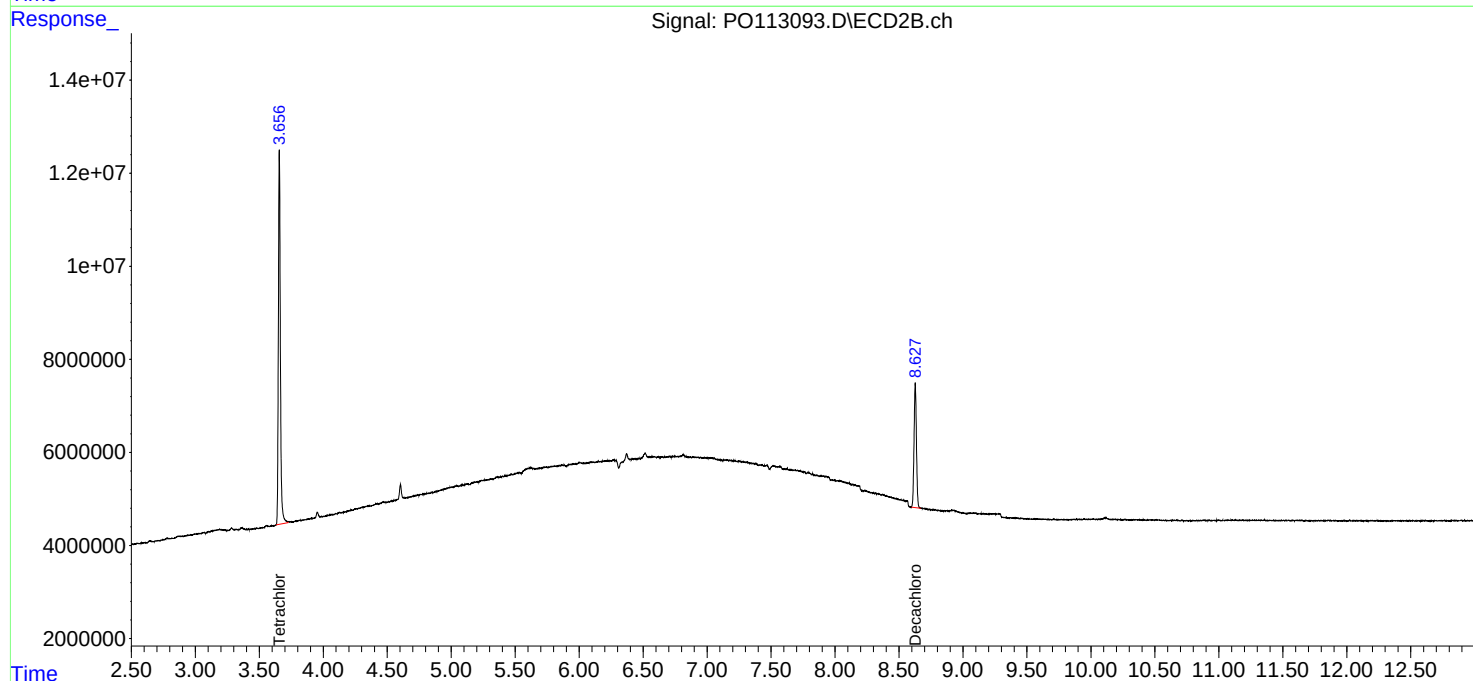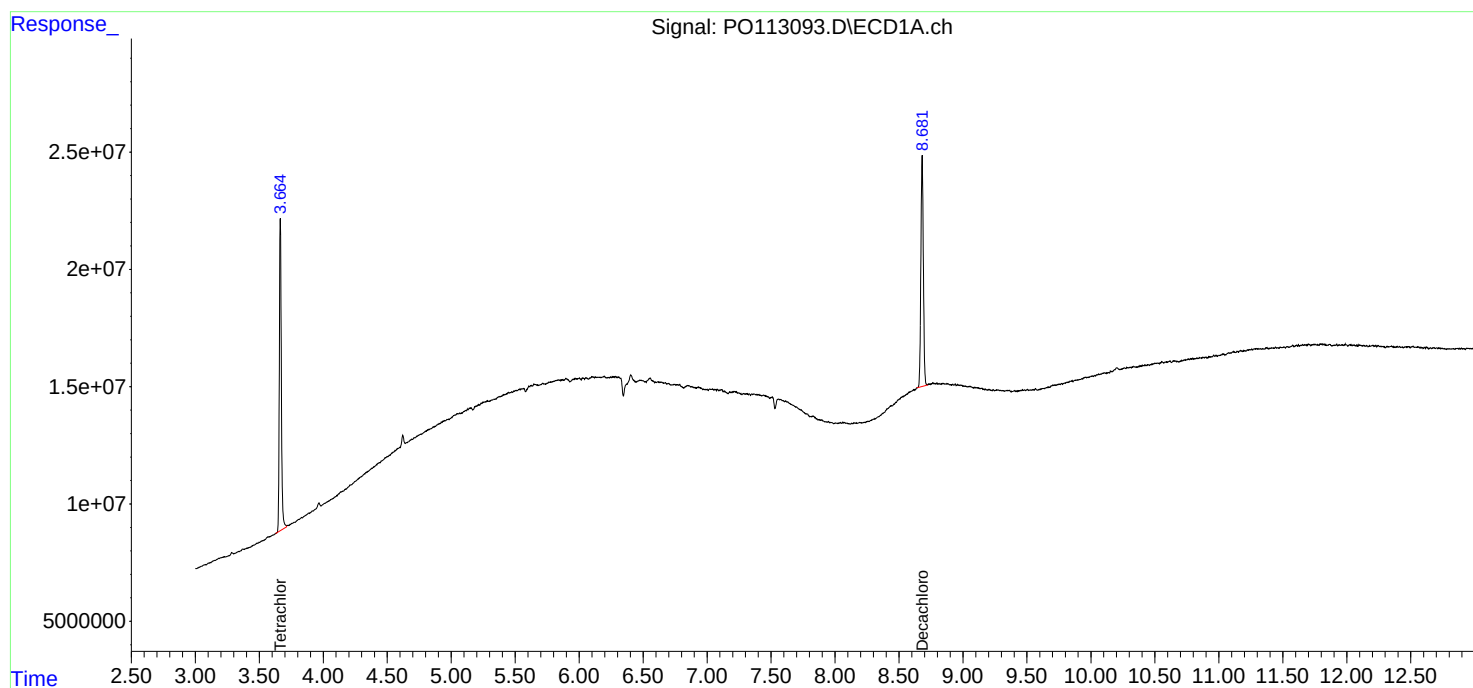


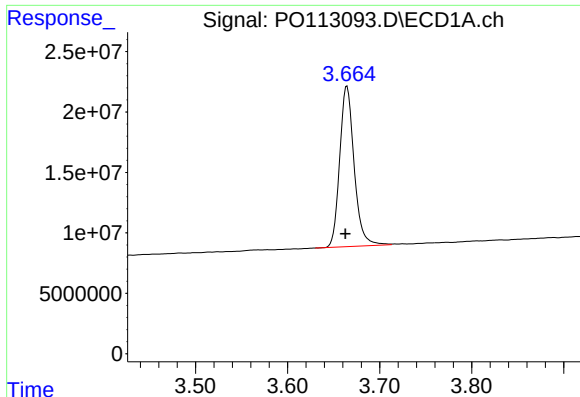

#1 Tetrachloro-m-xylene


R.T.: 3.665 min
Delta R.T.: 0.002 min
Response: 144525587
Conc: 17.65 ng/ml

Instrument :
ECD_O
ClientSampleId :
I.BLK

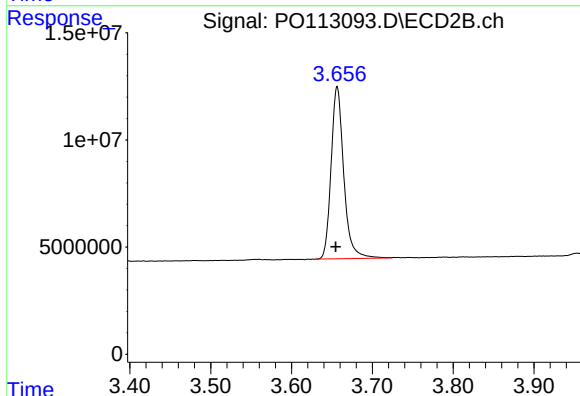


#1 Tetrachloro-m-xylene

R.T.: 3.657 min
Delta R.T.: 0.002 min
Response: 87439348
Conc: 17.28 ng/ml

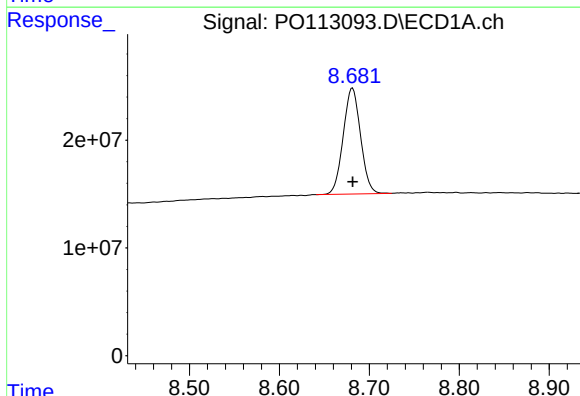

#2 Decachlorobiphenyl

R.T.: 8.681 min
Delta R.T.: 0.000 min
Response: 131684261
Conc: 19.00 ng/ml

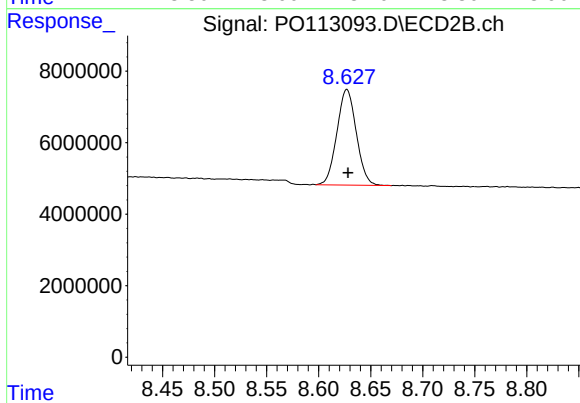

#2 Decachlorobiphenyl

R.T.: 8.627 min
Delta R.T.: -0.001 min
Response: 34729368
Conc: 18.33 ng/ml

Report of Analysis

Client:	ATC Group Services LLC		Date Collected:	08/20/25	
Project:	PS 190 BK - 2025SCA056		Date Received:	08/20/25	
Client Sample ID:	PIBLK-PO113108.D		SDG No.:	Q2894	
Lab Sample ID:	I.BLK-PO113108.D		Matrix:	WATER	
Analytical Method:	8082A		% Solid:	0	Decanted:
Sample Wt/Vol:	1000	Units: mL	Final Vol:	10000	uL
Soil Aliquot Vol:		uL	Test:	PCB	
Extraction Type:			Injection Volume :		
GPC Factor :	1.0	PH :			
Prep Method :	5030				

File ID/Qc Batch:	Dilution:	Prep Date	Date Analyzed	Prep Batch ID
PO113108.D	1		08/20/25	po082025

CAS Number	Parameter	Conc.	Qualifier	MDL	LOQ / CRQL	Units
TARGETS						
12674-11-2	Aroclor-1016	0.097	U	0.097	0.50	ug/L
11104-28-2	Aroclor-1221	0.13	U	0.13	0.50	ug/L
11141-16-5	Aroclor-1232	0.096	U	0.096	0.50	ug/L
53469-21-9	Aroclor-1242	0.12	U	0.12	0.50	ug/L
12672-29-6	Aroclor-1248	0.071	U	0.071	0.50	ug/L
11097-69-1	Aroclor-1254	0.094	U	0.094	0.50	ug/L
11096-82-5	Aroclor-1260	0.081	U	0.081	0.50	ug/L
37324-23-5	Aroclor-1262	0.14	U	0.14	0.50	ug/L
11100-14-4	Aroclor-1268	0.11	U	0.11	0.50	ug/L
SURROGATES						
877-09-8	Tetrachloro-m-xylene	17.5		60 - 140	88%	SPK: 20
2051-24-3	Decachlorobiphenyl	17.7		60 - 140	89%	SPK: 20

Comments:

U = Not Detected

LOQ = Limit of Quantitation

MDL = Method Detection Limit

LOD = Limit of Detection

E = Value Exceeds Calibration Range

P = Indicates >25% difference for detected concentrations between the two GC columns

Q = indicates LCS control criteria did not meet requirements

M = MS/MSD acceptance criteria did not meet requirements

J = Estimated Value

B = Analyte Found in Associated Method Blank

N = Presumptive Evidence of a Compound

* = Values outside of QC limits

D = Dilution

S = Indicates estimated value where valid five-point calibration was not performed prior to analyte detection in sample.

() = Laboratory InHouse Limit

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0082025\
Data File : PO113108.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 20 Aug 2025 22:37
Operator : YP/AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
I.BLK

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 21 01:44:32 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0081825.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Aug 19 06:08:32 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.662	3.655	146.9E6	88590318	17.939	17.506
2)	SA Decachlor...	8.681	8.626	122.9E6	36029884	17.738	19.015

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO082025\
Data File : PO113108.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 20 Aug 2025 22:37
Operator : YP/AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
I.BLK

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 21 01:44:32 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO081825.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Aug 19 06:08:32 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

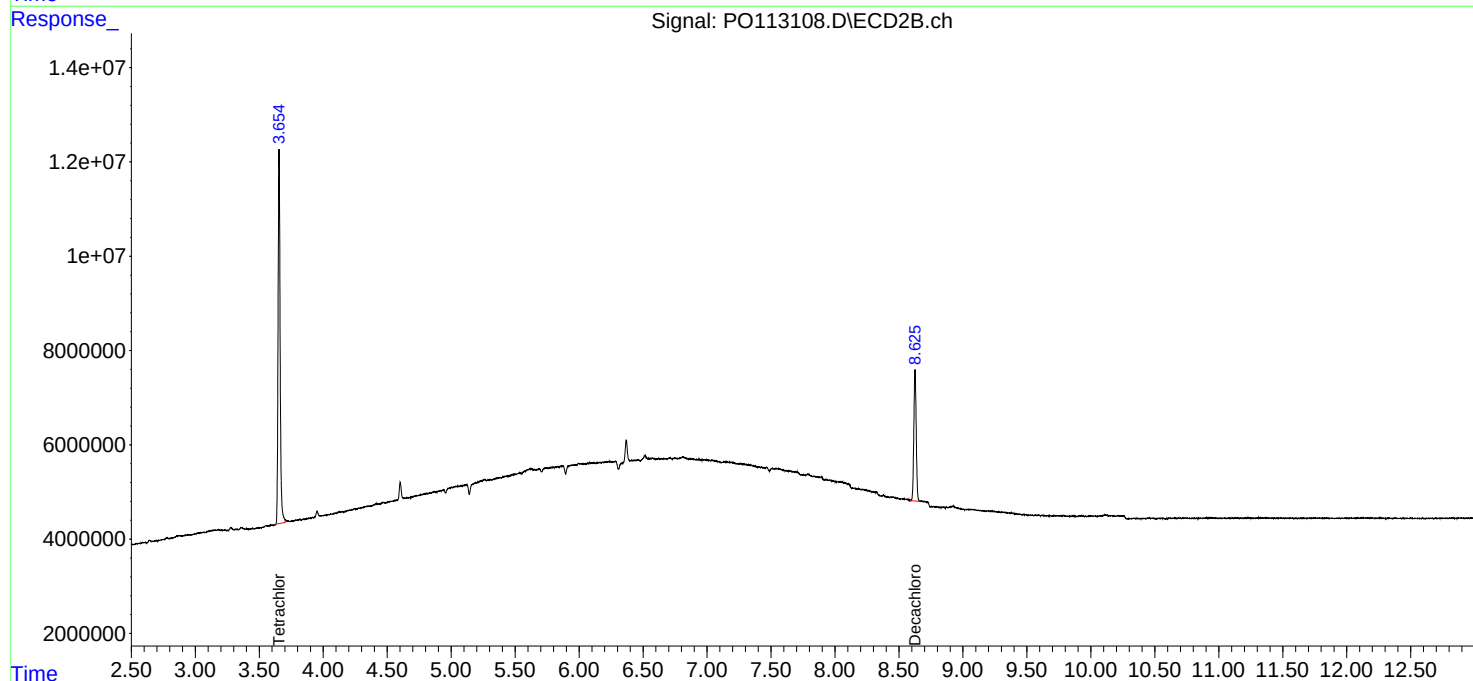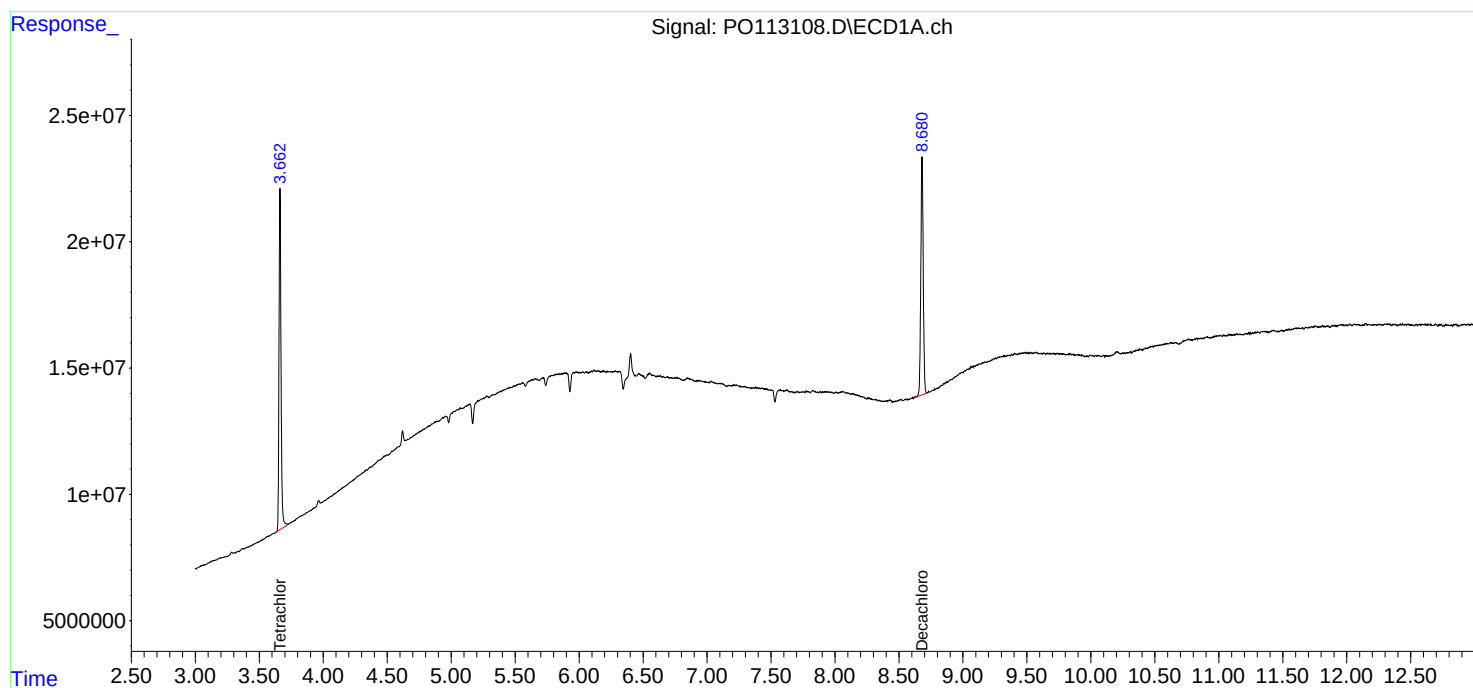


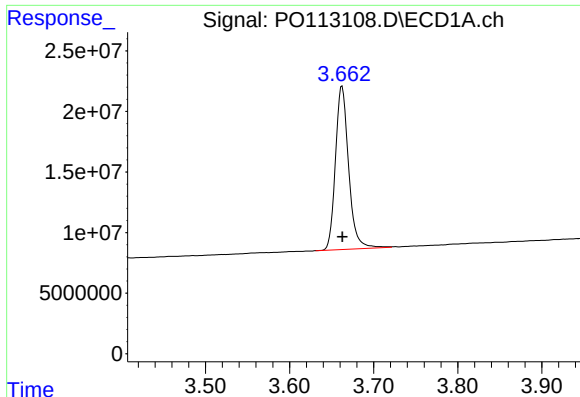

#1 Tetrachloro-m-xylene


R.T.: 3.662 min
Delta R.T.: 0.000 min
Response: 146857474
Conc: 17.94 ng/ml

Instrument :
ECD_O
ClientSampleId :
I.BLK

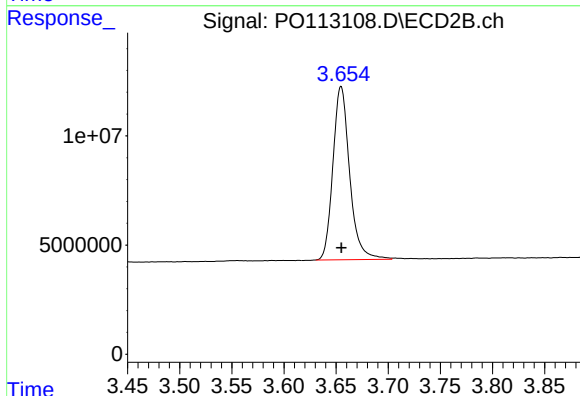


#1 Tetrachloro-m-xylene

R.T.: 3.655 min
Delta R.T.: 0.000 min
Response: 88590318
Conc: 17.51 ng/ml

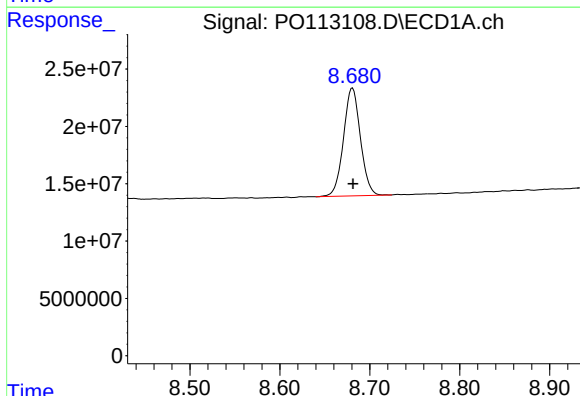

#2 Decachlorobiphenyl

R.T.: 8.681 min
Delta R.T.: 0.000 min
Response: 122948042
Conc: 17.74 ng/ml

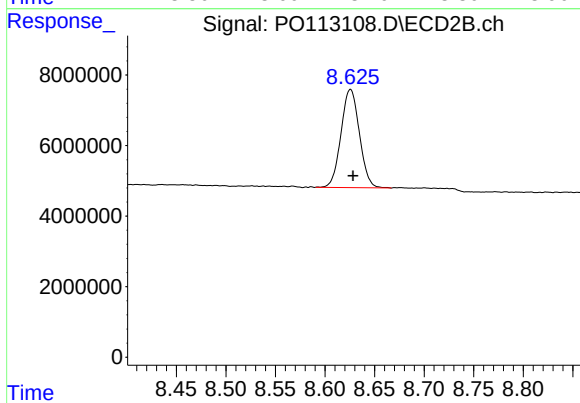

#2 Decachlorobiphenyl

R.T.: 8.626 min
Delta R.T.: -0.003 min
Response: 36029884
Conc: 19.01 ng/ml

Report of Analysis

Client:	ATC Group Services LLC		Date Collected:	08/21/25	
Project:	PS 190 BK - 2025SCA056		Date Received:	08/21/25	
Client Sample ID:	PIBLK-PO113118.D		SDG No.:	Q2894	
Lab Sample ID:	I.BLK-PO113118.D		Matrix:	WATER	
Analytical Method:	8082A		% Solid:	0	Decanted:
Sample Wt/Vol:	1000	Units: mL	Final Vol:	10000	uL
Soil Aliquot Vol:		uL	Test:	PCB	
Extraction Type:			Injection Volume :		
GPC Factor :	1.0	PH :			
Prep Method :	5030				

File ID/Qc Batch:	Dilution:	Prep Date	Date Analyzed	Prep Batch ID
PO113118.D	1		08/21/25	po082125

CAS Number	Parameter	Conc.	Qualifier	MDL	LOQ / CRQL	Units
TARGETS						
12674-11-2	Aroclor-1016	0.097	U	0.097	0.50	ug/L
11104-28-2	Aroclor-1221	0.13	U	0.13	0.50	ug/L
11141-16-5	Aroclor-1232	0.096	U	0.096	0.50	ug/L
53469-21-9	Aroclor-1242	0.12	U	0.12	0.50	ug/L
12672-29-6	Aroclor-1248	0.071	U	0.071	0.50	ug/L
11097-69-1	Aroclor-1254	0.094	U	0.094	0.50	ug/L
11096-82-5	Aroclor-1260	0.081	U	0.081	0.50	ug/L
37324-23-5	Aroclor-1262	0.14	U	0.14	0.50	ug/L
11100-14-4	Aroclor-1268	0.11	U	0.11	0.50	ug/L
SURROGATES						
877-09-8	Tetrachloro-m-xylene	17.7		60 - 140	88%	SPK: 20
2051-24-3	Decachlorobiphenyl	18.9		60 - 140	95%	SPK: 20

Comments:

U = Not Detected

LOQ = Limit of Quantitation

MDL = Method Detection Limit

LOD = Limit of Detection

E = Value Exceeds Calibration Range

P = Indicates >25% difference for detected concentrations between the two GC columns

Q = indicates LCS control criteria did not meet requirements

M = MS/MSD acceptance criteria did not meet requirements

J = Estimated Value

B = Analyte Found in Associated Method Blank

N = Presumptive Evidence of a Compound

* = Values outside of QC limits

D = Dilution

S = Indicates estimated value where valid five-point calibration was not performed prior to analyte detection in sample.

() = Laboratory InHouse Limit

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0082125\
Data File : PO113118.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 21 Aug 2025 09:46
Operator : YP/AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
I.BLK

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 21 11:33:17 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0081825.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Aug 19 06:08:32 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.668	3.654	151.7E6	89377599	18.535	17.661
2) SA Decachlor...	8.691	8.628	131.3E6	36237578	18.945	19.124

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO082125\
Data File : PO113118.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 21 Aug 2025 09:46
Operator : YP/AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
I.BLK

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 21 11:33:17 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO081825.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Aug 19 06:08:32 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

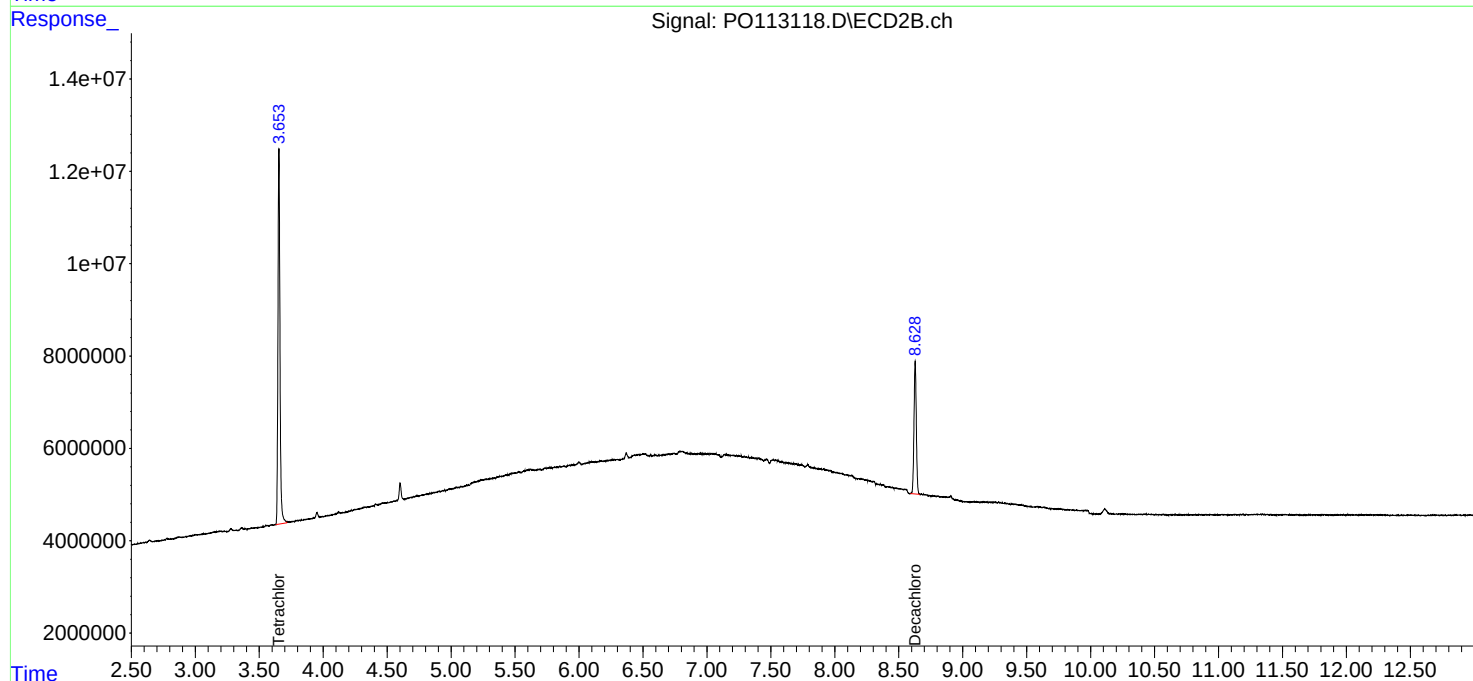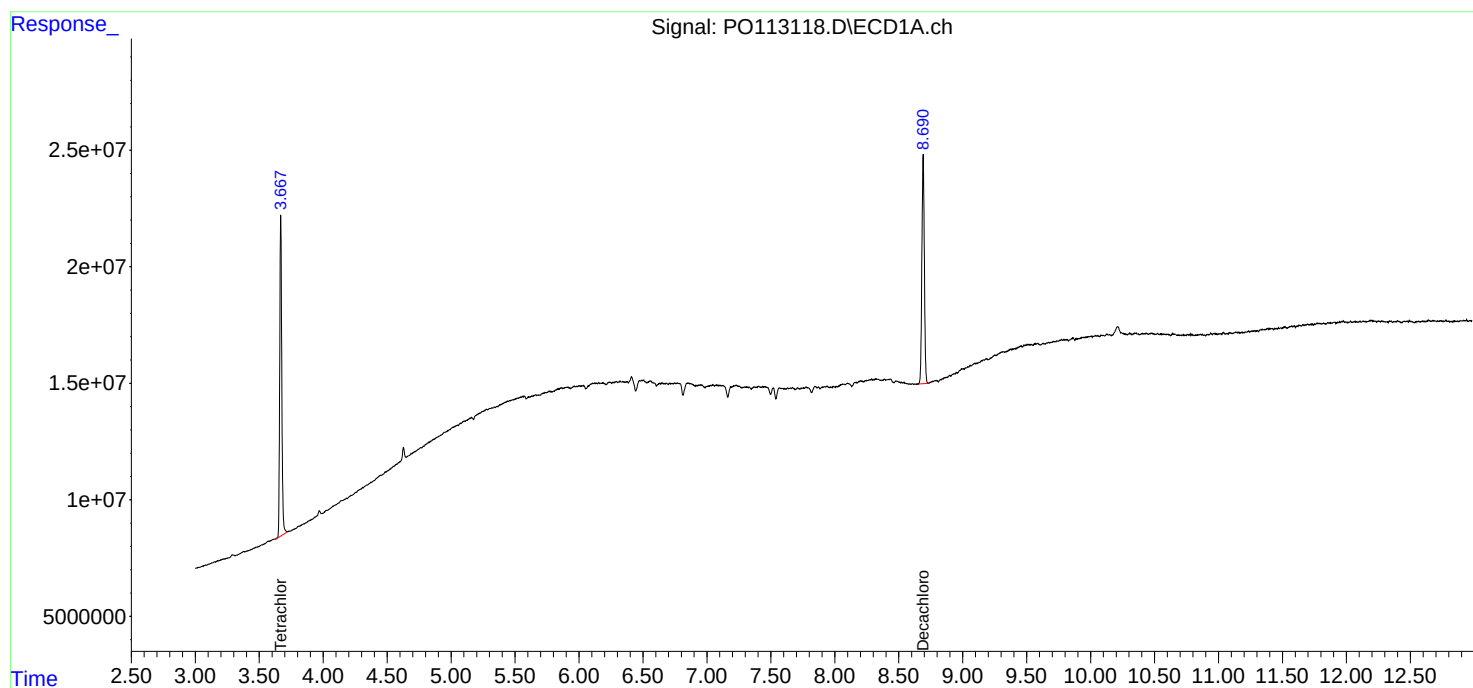


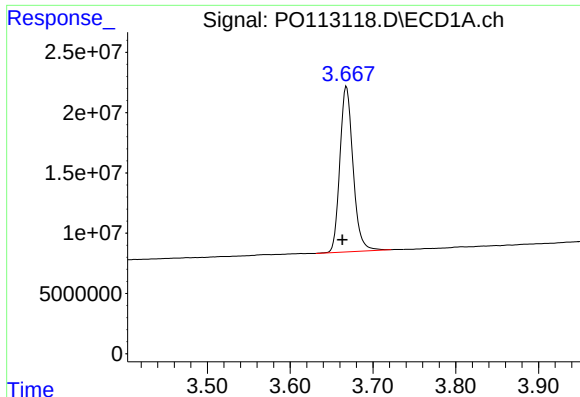

#1 Tetrachloro-m-xylene


R.T.: 3.668 min
Delta R.T.: 0.005 min
Response: 151738724
Conc: 18.54 ng/ml

Instrument :
ECD_O
ClientSampleId :
I.BLK

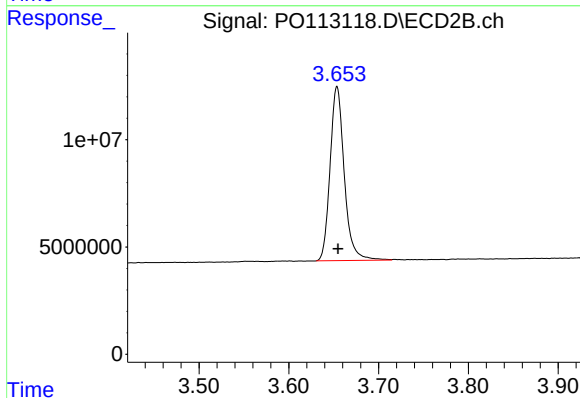


#1 Tetrachloro-m-xylene

R.T.: 3.654 min
Delta R.T.: -0.001 min
Response: 89377599
Conc: 17.66 ng/ml

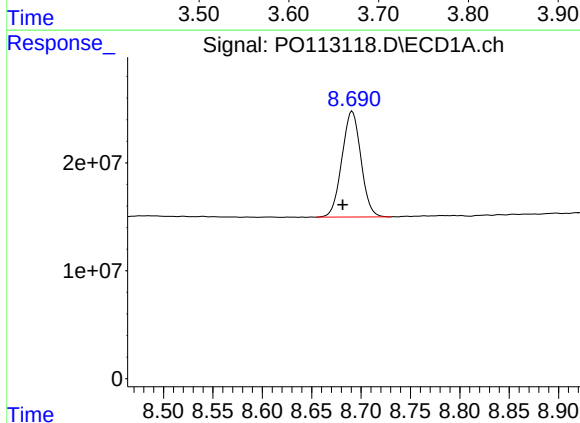

#2 Decachlorobiphenyl

R.T.: 8.691 min
Delta R.T.: 0.009 min
Response: 131315337
Conc: 18.94 ng/ml

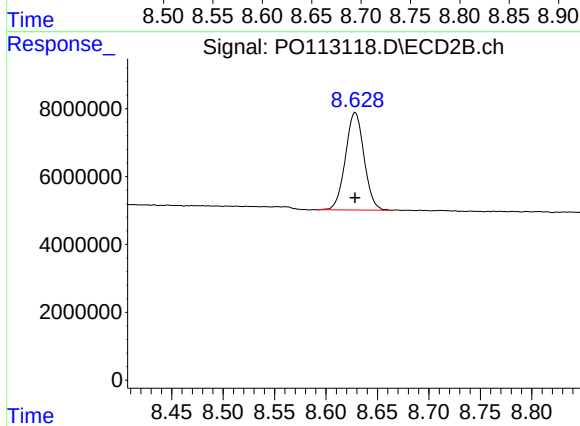

#2 Decachlorobiphenyl

R.T.: 8.628 min
Delta R.T.: 0.000 min
Response: 36237578
Conc: 19.12 ng/ml

Report of Analysis

Client:	ATC Group Services LLC		Date Collected:	08/21/25	
Project:	PS 190 BK - 2025SCA056		Date Received:	08/21/25	
Client Sample ID:	PIBLK-PO113125.D		SDG No.:	Q2894	
Lab Sample ID:	I.BLK-PO113125.D		Matrix:	WATER	
Analytical Method:	8082A		% Solid:	0	Decanted:
Sample Wt/Vol:	1000	Units: mL	Final Vol:	10000	uL
Soil Aliquot Vol:		uL	Test:	PCB	
Extraction Type:			Injection Volume :		
GPC Factor :	1.0	PH :			
Prep Method :	5030				

File ID/Qc Batch:	Dilution:	Prep Date	Date Analyzed	Prep Batch ID
PO113125.D	1		08/21/25	po082125

CAS Number	Parameter	Conc.	Qualifier	MDL	LOQ / CRQL	Units
TARGETS						
12674-11-2	Aroclor-1016	0.097	U	0.097	0.50	ug/L
11104-28-2	Aroclor-1221	0.13	U	0.13	0.50	ug/L
11141-16-5	Aroclor-1232	0.096	U	0.096	0.50	ug/L
53469-21-9	Aroclor-1242	0.12	U	0.12	0.50	ug/L
12672-29-6	Aroclor-1248	0.071	U	0.071	0.50	ug/L
11097-69-1	Aroclor-1254	0.094	U	0.094	0.50	ug/L
11096-82-5	Aroclor-1260	0.081	U	0.081	0.50	ug/L
37324-23-5	Aroclor-1262	0.14	U	0.14	0.50	ug/L
11100-14-4	Aroclor-1268	0.11	U	0.11	0.50	ug/L
SURROGATES						
877-09-8	Tetrachloro-m-xylene	17.8		60 - 140	89%	SPK: 20
2051-24-3	Decachlorobiphenyl	18.8		60 - 140	94%	SPK: 20

Comments:

U = Not Detected

LOQ = Limit of Quantitation

MDL = Method Detection Limit

LOD = Limit of Detection

E = Value Exceeds Calibration Range

P = Indicates >25% difference for detected concentrations between the two GC columns

Q = indicates LCS control criteria did not meet requirements

M = MS/MSD acceptance criteria did not meet requirements

J = Estimated Value

B = Analyte Found in Associated Method Blank

N = Presumptive Evidence of a Compound

* = Values outside of QC limits

D = Dilution

S = Indicates estimated value where valid five-point calibration was not performed prior to analyte detection in sample.

() = Laboratory InHouse Limit

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO082125\
Data File : PO113125.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 21 Aug 2025 12:34
Operator : YP/AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
I.BLK

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 21 12:51:48 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO081825.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Aug 19 06:08:32 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.663	3.654	150.0E6	89896556	18.320	17.764
2) SA Decachlor...	8.681	8.626	130.1E6	35683718	18.774	18.832

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO082125\
Data File : PO113125.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 21 Aug 2025 12:34
Operator : YP/AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
I.BLK

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 21 12:51:48 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO081825.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Aug 19 06:08:32 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

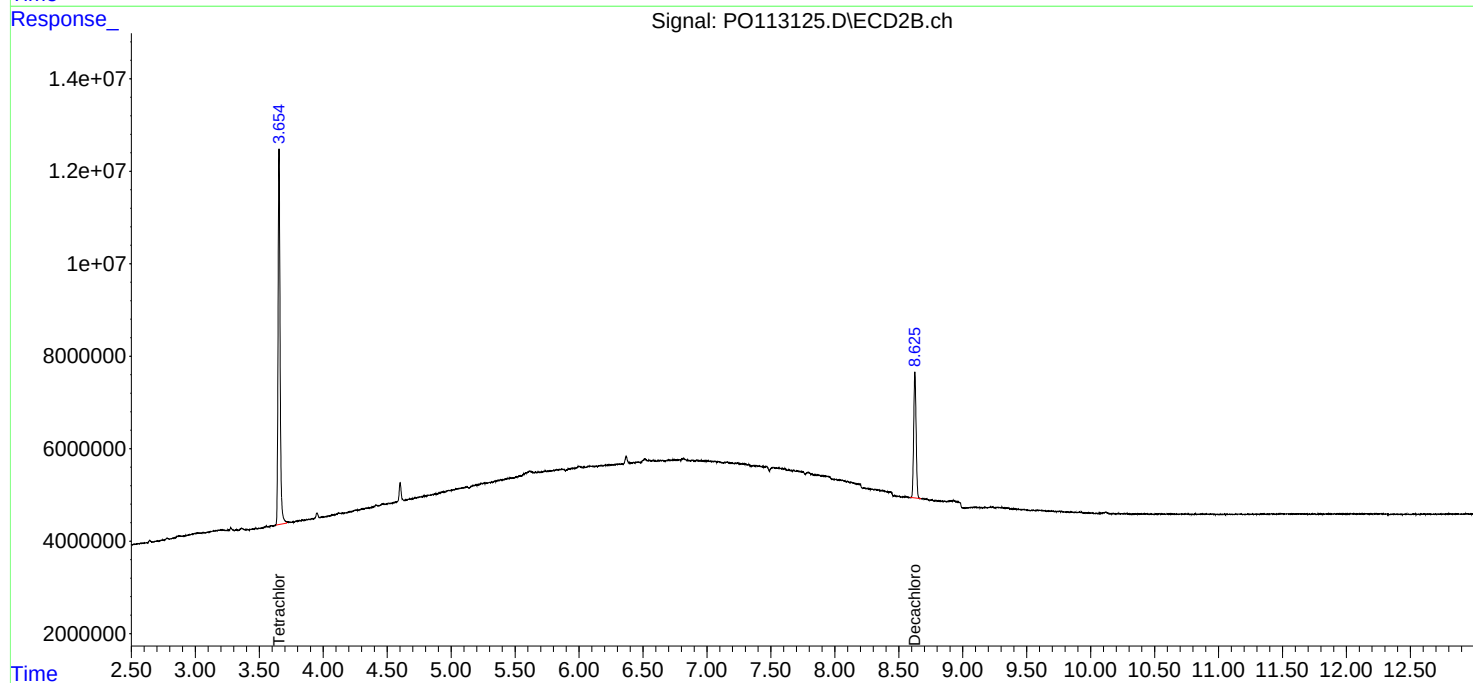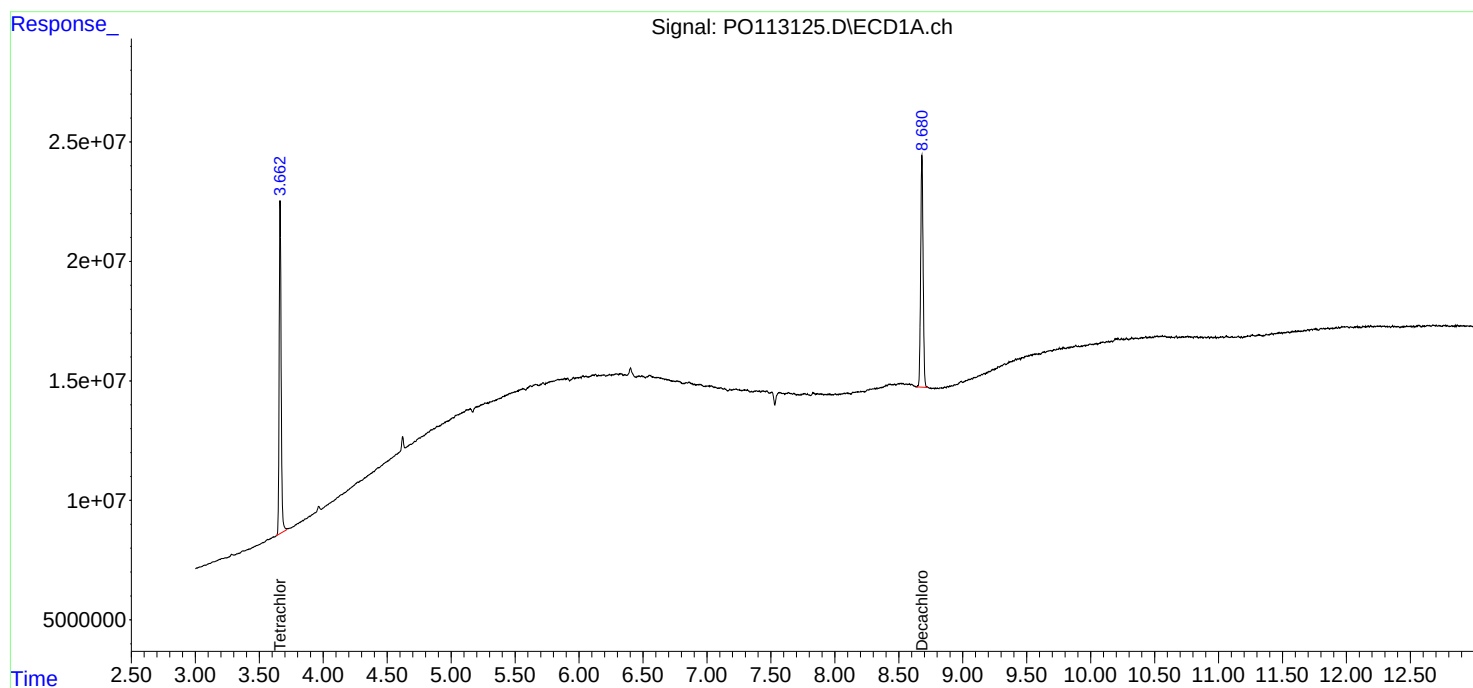


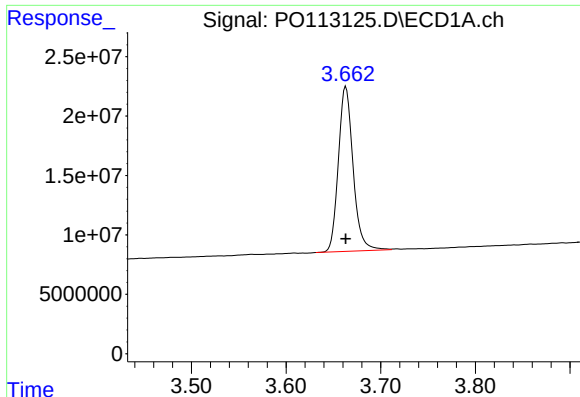

#1 Tetrachloro-m-xylene


R.T.: 3.663 min
Delta R.T.: 0.000 min
Response: 149977214
Conc: 18.32 ng/ml

Instrument :
ECD_O
ClientSampleId :
I.BLK

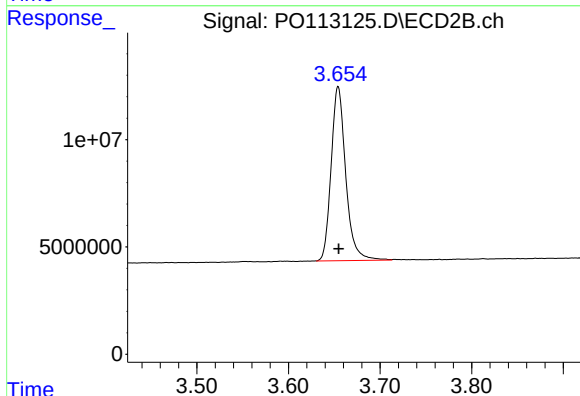


#1 Tetrachloro-m-xylene

R.T.: 3.654 min
Delta R.T.: 0.000 min
Response: 89896556
Conc: 17.76 ng/ml

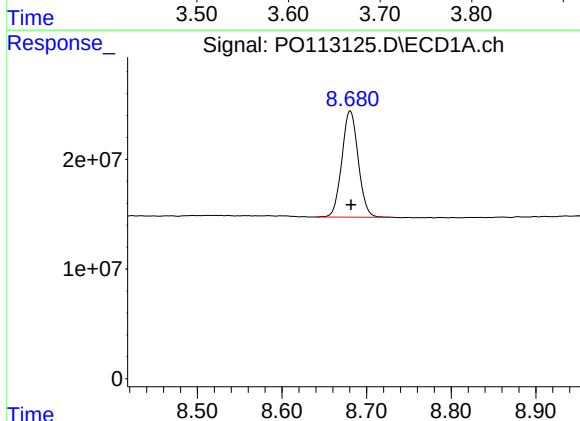

#2 Decachlorobiphenyl

R.T.: 8.681 min
Delta R.T.: 0.000 min
Response: 130132799
Conc: 18.77 ng/ml

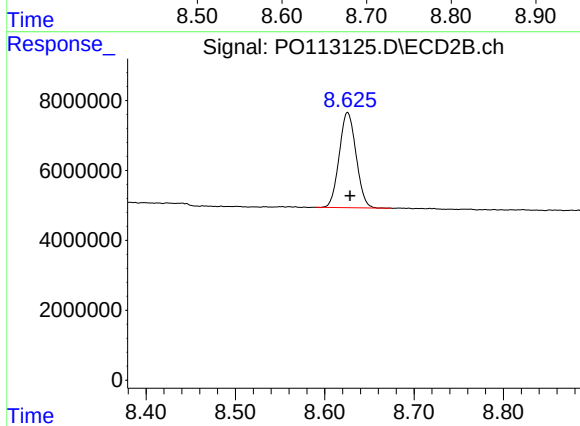

#2 Decachlorobiphenyl

R.T.: 8.626 min
Delta R.T.: -0.003 min
Response: 35683718
Conc: 18.83 ng/ml

Report of Analysis

Client:	ATC Group Services LLC		Date Collected:		
Project:	PS 190 BK - 2025SCA056		Date Received:		
Client Sample ID:	PB169322BS		SDG No.:	Q2894	
Lab Sample ID:	PB169322BS		Matrix:	SOIL	
Analytical Method:	8082A		% Solid:	100	Decanted:
Sample Wt/Vol:	30.02	Units: g	Final Vol:	10000	uL
Soil Aliquot Vol:		uL	Test:	PCB	
Extraction Type:			Injection Volume :		
GPC Factor :	1.0	PH :			
Prep Method :	SW3541B				

File ID/Qc Batch:	Dilution:	Prep Date	Date Analyzed	Prep Batch ID
PO113081.D	1	08/20/25 08:40	08/20/25 12:19	PB169322

CAS Number	Parameter	Conc.	Qualifier	MDL	LOQ / CRQL	Units(Dry Weight)
TARGETS						
12674-11-2	Aroclor-1016	178		3.90	17.0	ug/kg
11104-28-2	Aroclor-1221	4.00	U	4.00	17.0	ug/kg
11141-16-5	Aroclor-1232	3.70	U	3.70	17.0	ug/kg
53469-21-9	Aroclor-1242	4.00	U	4.00	17.0	ug/kg
12672-29-6	Aroclor-1248	5.90	U	5.90	17.0	ug/kg
11097-69-1	Aroclor-1254	3.20	U	3.20	17.0	ug/kg
37324-23-5	Aroclor-1262	5.00	U	5.00	17.0	ug/kg
11100-14-4	Aroclor-1268	3.60	U	3.60	17.0	ug/kg
11096-82-5	Aroclor-1260	171		3.20	17.0	ug/kg
SURROGATES						
877-09-8	Tetrachloro-m-xylene	18.2		32 - 144	91%	SPK: 20
2051-24-3	Decachlorobiphenyl	19.0		32 - 175	95%	SPK: 20

Comments:

U = Not Detected

LOQ = Limit of Quantitation

MDL = Method Detection Limit

LOD = Limit of Detection

E = Value Exceeds Calibration Range

P = Indicates >25% difference for detected concentrations between the two GC columns

Q = indicates LCS control criteria did not meet requirements

M = MS/MSD acceptance criteria did not meet requirements

J = Estimated Value

B = Analyte Found in Associated Method Blank

N = Presumptive Evidence of a Compound

* = Values outside of QC limits

D = Dilution

S = Indicates estimated value where valid five-point calibration was not performed prior to analyte detection in sample.

() = Laboratory InHouse Limit

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0082025\
 Data File : PO113081.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 20 Aug 2025 12:19
 Operator : YP/AJ
 Sample : PB169322BS
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 PB169322BS

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 20 13:05:34 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0081825.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Aug 19 06:08:32 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.664	3.655	149.1E6	88345618	18.214	17.457
2) SA Decachlor...	8.681	8.627	124.2E6	35981458	17.916	18.989
Target Compounds						
3) L1 AR-1016-1	4.748	4.728	145.2E6	88659221	543.787	519.771
4) L1 AR-1016-2	4.766	4.746	222.8E6	129.9E6	554.921	504.111
5) L1 AR-1016-3	4.823	4.921	139.7E6	68785520	547.756	492.682
6) L1 AR-1016-4	4.942	4.964	111.6E6	54986476	511.541	471.182
7) L1 AR-1016-5	5.199	5.175	114.1E6	70940426	515.037	497.723
31) L7 AR-1260-1	6.235	6.202	252.3E6	132.5E6	565.783	519.482
32) L7 AR-1260-2	6.425	6.391	381.0E6	177.4E6	554.810	513.139
33) L7 AR-1260-3	6.790	6.542	301.9E6	147.0E6	488.893	494.202
34) L7 AR-1260-4	7.049	7.011	224.7E6	93229029	501.631	449.840
35) L7 AR-1260-5	7.292	7.253	549.6E6	213.3E6	453.972	455.361



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO082025\
Data File : PO113081.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 20 Aug 2025 12:19
Operator : YP/AJ
Sample : PB169322BS
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
PB169322BS

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 20 13:05:34 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO081825.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Aug 19 06:08:32 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

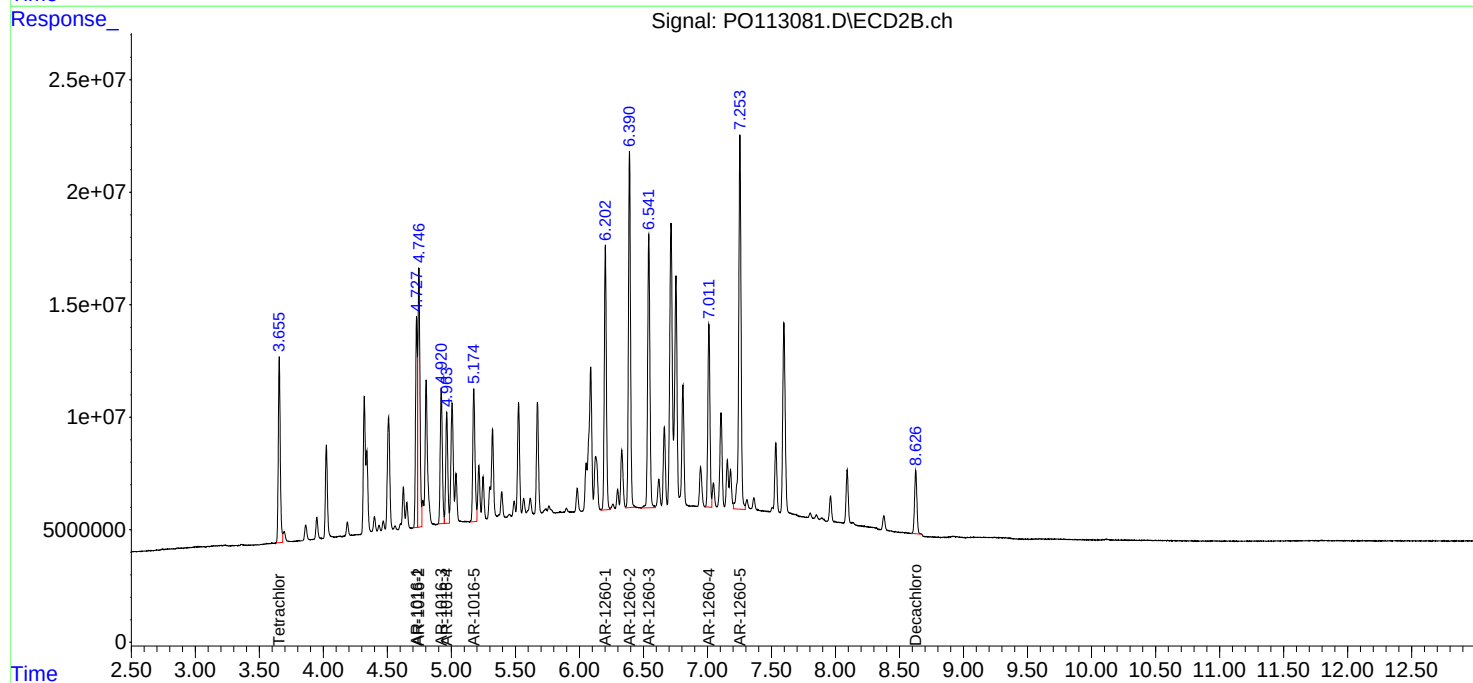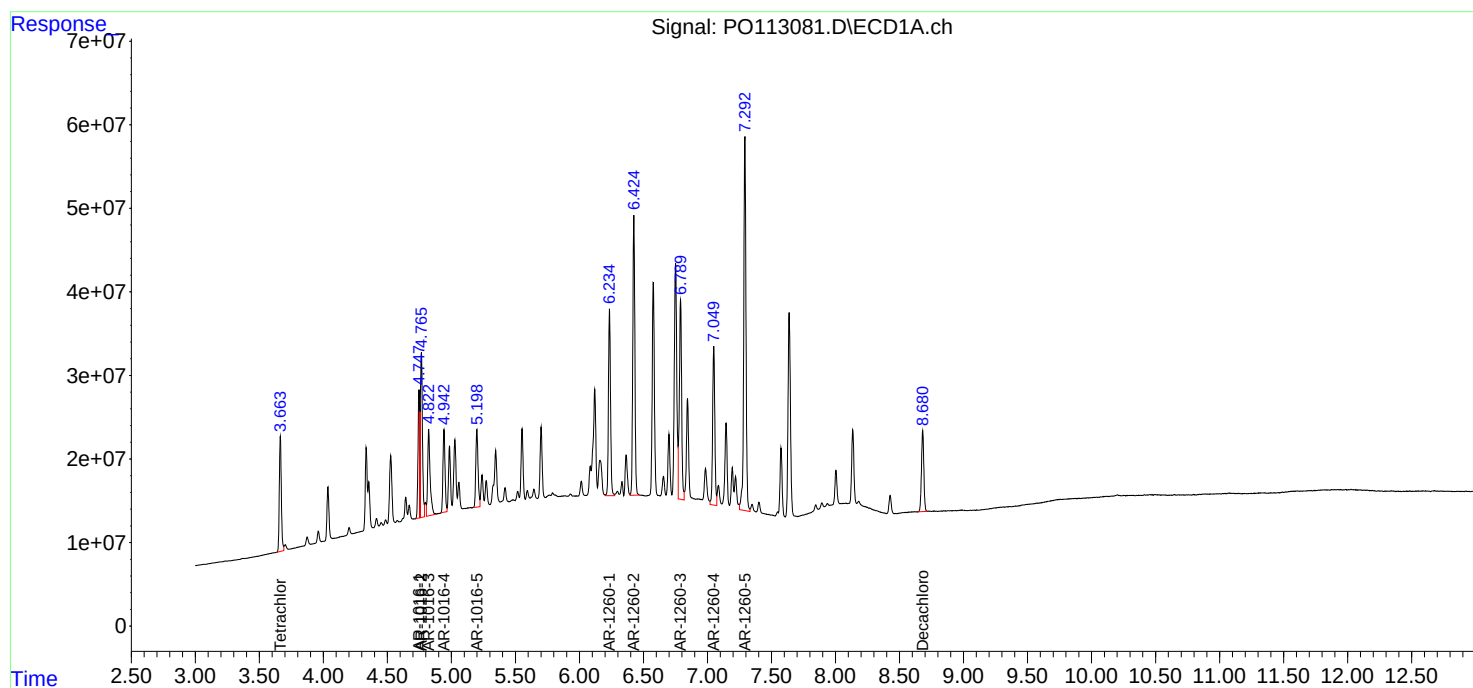

Manual Integration Report

Sequence:	PO081825	Instrument	ECD_o

Sample ID	File ID	Parameter	Review By	Review On	Supervised By	Supervised On	Reason
AR1660ICC050	PO113007.D	AR-1260-1	yogesh	8/19/2025 7:25:57 AM	mohammad	8/20/2025 3:04:50	Peak Integrated by Software
AR1660ICC050	PO113007.D	AR-1260-2	yogesh	8/19/2025 7:25:57 AM	mohammad	8/20/2025 3:04:50	Peak Integrated by Software
AR1660ICC050	PO113007.D	AR-1260-3 #2	yogesh	8/19/2025 7:25:57 AM	mohammad	8/20/2025 3:04:50	Peak Integrated by Software
AR1242ICC050	PO113014.D	AR-1242-1	yogesh	8/19/2025 7:25:59 AM	mohammad	8/20/2025 3:04:50	Peak Integrated by Software
AR1242ICC050	PO113014.D	AR-1242-1 #2	yogesh	8/19/2025 7:25:59 AM	mohammad	8/20/2025 3:04:50	Peak Integrated by Software
AR1242ICC050	PO113014.D	AR-1242-2	yogesh	8/19/2025 7:25:59 AM	mohammad	8/20/2025 3:04:50	Peak Integrated by Software
AR1242ICC050	PO113014.D	AR-1242-5	yogesh	8/19/2025 7:25:59 AM	mohammad	8/20/2025 3:04:50	Peak Integrated by Software
AR1242ICC050	PO113014.D	AR-1242-5 #2	yogesh	8/19/2025 7:25:59 AM	mohammad	8/20/2025 3:04:50	Peak Integrated by Software
AR1254ICC050	PO113024.D	AR-1254-1 #2	yogesh	8/19/2025 7:26:00 AM	mohammad	8/20/2025 3:04:50	Peak Integrated by Software
AR1254ICC050	PO113024.D	AR-1254-2 #2	yogesh	8/19/2025 7:26:00 AM	mohammad	8/20/2025 3:04:50	Peak Integrated by Software
AR1254ICC050	PO113024.D	AR-1254-3 #2	yogesh	8/19/2025 7:26:00 AM	mohammad	8/20/2025 3:04:50	Peak Integrated by Software
AR1268ICC050	PO113030.D	AR-1268-5 #2	yogesh	8/19/2025 7:26:02 AM	mohammad	8/20/2025 3:04:50	Peak Integrated by Software
AR1268ICV500	PO113035.D	AR-1268-5 #2	yogesh	8/19/2025 7:26:03 AM	mohammad	8/20/2025 3:04:50	Peak Integrated by Software



284 Sheffield Street, Mountainside, New Jersey 07092, Phone : 908 789 8900, Fax : 908 789 8922

Manual Integration Report

Sequence:

PO081825

Instrument

ECD_o

Sample ID

File ID

Parameter

Review By

Review On

Supervised
By

Supervised On

Reason

Manual Integration Report

Sequence:

PO082025

Instrument

ECD_o

Sample ID	File ID	Parameter	Review By	Review On	Supervised By	Supervised On	Reason
AR1660CCC500	PO113074.D	AR-1016-4	yogesh	8/21/2025 7:57:50 AM	mohammad	8/22/2025 2:04:33	Peak Integrated by Software
Q2894-01	PO113082.D	Tetrachloro-m-xylene	yogesh	8/21/2025 7:57:55 AM	mohammad	8/22/2025 2:04:33	Peak Integrated by Software
Q2894-01	PO113082.D	Tetrachloro-m-xylene #2	yogesh	8/21/2025 7:57:55 AM	mohammad	8/22/2025 2:04:33	Peak Integrated by Software
Q2894-02	PO113083.D	Tetrachloro-m-xylene	yogesh	8/21/2025 7:57:54 AM	mohammad	8/22/2025 2:04:33	Peak Integrated by Software
Q2894-02	PO113083.D	Tetrachloro-m-xylene #2	yogesh	8/21/2025 7:57:54 AM	mohammad	8/22/2025 2:04:33	Peak Integrated by Software
AR1660CCC500	PO113089.D	AR-1016-4	yogesh	8/21/2025 8:36:01 AM	mohammad	8/22/2025 2:04:33	Peak Integrated by Software
AR1660CCC500	PO113111.D	AR-1016-5	yogesh	8/21/2025 8:37:27 AM	mohammad	8/22/2025 2:04:33	Peak Integrated by Software

Manual Integration Report

Sequence:

po082125

Instrument

ECD_o

Sample ID	File ID	Parameter	Review By	Review On	Supervised By	Supervised On	Reason
AR1660CCC500	PO113148.D	AR-1016-5	yogesh	8/22/2025 7:26:24 AM	 	 	Peak Integrated by Software
AR1660CCC500	PO113157.D	AR-1016-5	yogesh	8/22/2025 7:26:25 AM	 	 	Peak Integrated by Software
AR1242CCC500	PO113158.D	AR-1242-5	yogesh	8/22/2025 7:26:27 AM	 	 	Peak Integrated by Software
AR1254CCC500	PO113160.D	AR-1254-1	yogesh	8/22/2025 7:26:29 AM	 	 	Peak Integrated by Software
AR1254CCC500	PO113160.D	AR-1254-2	yogesh	8/22/2025 7:26:29 AM	 	 	Peak Integrated by Software

Instrument ID: ECD_O

Daily Analysis Runlog For Sequence/QC Batch ID # PO081825

Review By	yogesh	Review On	8/18/2025 10:23:59 AM
Supervise By	mohammad	Supervise On	8/20/2025 3:04:50 AM
SubDirectory	PO081825	HP Acquire Method	HP Processing Method PO081825
STD. NAME	STD REF.#		
Tune/Reschk	PP24815,PP2416,PP24817,PP24818,PP24819,PP24820,PP24821,PP24822,PP24823,PP24824,PP24825,PP24826,PP24827,PP24828,PP24829,PP24830,PP24831,PP24832,PP24833,PP24834,PP24835,PP24836,PP24837,PP24838,PP24839,PP24840,PP24841,PP24842,PP24843,PP24844,PP24845,PP24846,PP24847,PP24848,PP24849,PP24850,PP24851,PP24852,PP24853,PP24854		
Initial Calibration Stds			
CCC			
Internal Standard/PEM			
ICV/I.BLK			
Surrogate Standard			
MS/MSD Standard	PP24815,PP24816,PP24817,PP24818,PP24819,PP24820,PP24821,PP24822,PP24855,PP24856,PP24857,PP24858,PP24859,PP24860,PP24861,PP24862		
LCS Standard			

Sr#	Sampleld	Data File Name	Date-Time	Operator	Status
1	HEXANE	PO113001.D	18 Aug 2025 09:16	YP/AJ	Ok
2	I.BLK	PO113002.D	18 Aug 2025 09:34	YP/AJ	Ok
3	AR1660ICC1000	PO113003.D	18 Aug 2025 09:53	YP/AJ	Ok
4	AR1660ICC750	PO113004.D	18 Aug 2025 10:11	YP/AJ	Ok
5	AR1660ICC500	PO113005.D	18 Aug 2025 10:29	YP/AJ	Ok
6	AR1660ICC250	PO113006.D	18 Aug 2025 10:48	YP/AJ	Ok
7	AR1660ICC050	PO113007.D	18 Aug 2025 11:06	YP/AJ	Ok,M
8	AR1221ICC500	PO113008.D	18 Aug 2025 11:25	YP/AJ	Ok
9	AR1232ICC500	PO113009.D	18 Aug 2025 11:43	YP/AJ	Ok
10	AR1242ICC1000	PO113010.D	18 Aug 2025 12:01	YP/AJ	Ok
11	AR1242ICC750	PO113011.D	18 Aug 2025 12:20	YP/AJ	Ok
12	AR1242ICC500	PO113012.D	18 Aug 2025 12:38	YP/AJ	Ok
13	AR1242ICC250	PO113013.D	18 Aug 2025 12:57	YP/AJ	Ok
14	AR1242ICC050	PO113014.D	18 Aug 2025 13:15	YP/AJ	Ok,M
15	AR1248ICC1000	PO113015.D	18 Aug 2025 13:34	YP/AJ	Ok
16	AR1248ICC750	PO113016.D	18 Aug 2025 13:52	YP/AJ	Ok
17	AR1248ICC500	PO113017.D	18 Aug 2025 14:09	YP/AJ	Ok
18	AR1248ICC250	PO113018.D	18 Aug 2025 14:28	YP/AJ	Ok
19	AR1248ICC050	PO113019.D	18 Aug 2025 14:46	YP/AJ	Ok
20	AR1254ICC1000	PO113020.D	18 Aug 2025 15:05	YP/AJ	Ok
21	AR1254ICC750	PO113021.D	18 Aug 2025 15:23	YP/AJ	Ok

Instrument ID: ECD_O

Daily Analysis Runlog For Sequence/QC Batch ID # PO081825

Review By	yogesh	Review On	8/18/2025 10:23:59 AM
Supervise By	mohammad	Supervise On	8/20/2025 3:04:50 AM
SubDirectory	PO081825	HP Acquire Method	HP Processing Method PO081825
STD. NAME	STD REF.#		
Tune/Reschk			
Initial Calibration Stds	PP24815,PP2416,PP24817,PP24818,PP24819,PP24820,PP24821,PP24822,PP24823,PP24824,PP24825,PP24826,PP24827,PP24828,PP24829,PP24830,PP24831,PP24832,PP24833,PP24834,PP24835,PP24836,PP24837,PP24838,PP24839,PP24840,PP24841,PP24842,PP24843,PP24844,PP24845,PP24846,PP24847,PP24848,PP24849,PP24850,PP24851,PP24852,PP24853,PP24854		
CCC			
Internal Standard/PEM			
ICV/I.BLK	PP24815,PP24816,PP24817,PP24818,PP24819,PP24820,PP24821,PP24822,PP24855,PP24856,PP24857,PP24858,PP24859,PP24860,PP24861,PP24862		
Surrogate Standard			
MS/MSD Standard			
LCS Standard			

22	AR1254ICC500	PO113022.D	18 Aug 2025 15:41	YP/AJ	Ok
23	AR1254ICC250	PO113023.D	18 Aug 2025 16:00	YP/AJ	Ok
24	AR1254ICC050	PO113024.D	18 Aug 2025 16:18	YP/AJ	Ok,M
25	AR1262ICC500	PO113025.D	18 Aug 2025 16:54	YP/AJ	Ok
26	AR1268ICC1000	PO113026.D	18 Aug 2025 17:12	YP/AJ	Ok
27	AR1268ICC750	PO113027.D	18 Aug 2025 17:30	YP/AJ	Ok
28	AR1268ICC500	PO113028.D	18 Aug 2025 17:48	YP/AJ	Ok
29	AR1268ICC250	PO113029.D	18 Aug 2025 18:06	YP/AJ	Ok
30	AR1268ICC050	PO113030.D	18 Aug 2025 18:24	YP/AJ	Ok,M
31	PO081825ICV500	PO113031.D	18 Aug 2025 18:43	YP/AJ	Ok
32	AR1242ICV500	PO113032.D	18 Aug 2025 19:37	YP/AJ	Ok
33	AR1248ICV500	PO113033.D	18 Aug 2025 19:54	YP/AJ	Ok
34	AR1254ICV500	PO113034.D	18 Aug 2025 20:31	YP/AJ	Ok
35	AR1268ICV500	PO113035.D	18 Aug 2025 21:07	YP/AJ	Ok,M
36	DDT ANALOG	PO113036.D	18 Aug 2025 21:44	YP/AJ	Ok

M : Manual Integration

Instrument ID: ECD_O

Daily Analysis Runlog For Sequence/QC Batch ID # PO082025

Review By	yogesh	Review On	8/20/2025 11:41:48 AM
Supervise By	mohammad	Supervise On	8/22/2025 2:04:33 AM
SubDirectory	PO082025	HP Acquire Method	HP Processing Method PO081825
STD. NAME	STD REF.#		
Tune/Reschk			
Initial Calibration Stds	PP24815,PP2416,PP24817,PP24818,PP24819,PP24820,PP24821,PP24822,PP24823,PP24824,PP24825,PP24826,PP24827,PP24828,PP24829,PP24830,PP24831,PP24832,PP24833,PP24834,PP24835,PP24836,PP24837,PP24838,PP24839,PP24840,PP24841,PP24842,PP24843,PP24844,PP24845,PP24846,PP24847,PP24848,PP24849,PP24850,PP24851,PP24852,PP24853,PP24854		
CCC	PP24824,PP24828,PP24832,PP24836,PP24840,PP24844,PP24852		
Internal Standard/PEM			
ICV/I.BLK	PP24815,PP24816,PP24817,PP24818,PP24819,PP24820,PP24821,PP24822,PP24855,PP24856,PP24857,PP24858,PP24859,PP24860,PP24861,PP24862		
Surrogate Standard			
MS/MSD Standard			
LCS Standard			

Sr#	SampleId	Data File Name	Date-Time	Operator	Status
1	HEXANE	PO113073.D	20 Aug 2025 09:16	YP/AJ	Ok
2	AR1660CCC500	PO113074.D	20 Aug 2025 09:33	YP/AJ	Ok,M
3	AR1242CCC500	PO113075.D	20 Aug 2025 09:52	YP/AJ	Ok
4	AR1248CCC500	PO113076.D	20 Aug 2025 10:10	YP/AJ	Ok
5	AR1254CCC500	PO113077.D	20 Aug 2025 10:28	YP/AJ	Ok
6	I.BLK	PO113078.D	20 Aug 2025 10:47	YP/AJ	Ok
7	DDT ANALOG	PO113079.D	20 Aug 2025 11:05	YP/AJ	Ok
8	PB169322BL	PO113080.D	20 Aug 2025 12:01	YP/AJ	Not Ok
9	PB169322BS	PO113081.D	20 Aug 2025 12:19	YP/AJ	Ok
10	Q2894-01	PO113082.D	20 Aug 2025 12:36	YP/AJ	Ok,M
11	Q2894-02	PO113083.D	20 Aug 2025 12:55	YP/AJ	Ok,M
12	Q2894-03	PO113084.D	20 Aug 2025 13:13	YP/AJ	Ok
13	Q2894-04	PO113085.D	20 Aug 2025 13:32	YP/AJ	Not Ok
14	Q2894-05	PO113086.D	20 Aug 2025 13:50	YP/AJ	Dilution
15	Q2901-01	PO113087.D	20 Aug 2025 14:09	YP/AJ	Dilution
16	Q2901-02	PO113088.D	20 Aug 2025 14:27	YP/AJ	Dilution
17	AR1660CCC500	PO113089.D	20 Aug 2025 15:39	YP/AJ	Ok,M
18	AR1242CCC500	PO113090.D	20 Aug 2025 15:57	YP/AJ	Ok
19	AR1248CCC500	PO113091.D	20 Aug 2025 16:14	YP/AJ	Ok
20	AR1254CCC500	PO113092.D	20 Aug 2025 16:32	YP/AJ	Ok
21	I.BLK	PO113093.D	20 Aug 2025 16:50	YP/AJ	Ok

Instrument ID: ECD_O

Daily Analysis Runlog For Sequence/QC Batch ID # PO082025

Review By	yogesh	Review On	8/20/2025 11:41:48 AM
Supervise By	mohammad	Supervise On	8/22/2025 2:04:33 AM
SubDirectory	PO082025	HP Acquire Method	HP Processing Method PO081825
STD. NAME	STD REF.#		
Tune/Reschk			
Initial Calibration Stds	PP24815,PP2416,PP24817,PP24818,PP24819,PP24820,PP24821,PP24822,PP24823,PP24824,PP24825,PP24826,PP24827,PP24828,PP24829,PP24830,PP24831,PP24832,PP24833,PP24834,PP24835,PP24836,PP24837,PP24838,PP24839,PP24840,PP24841,PP24842,PP24843,PP24844,PP24845,PP24846,PP24847,PP24848,PP24849,PP24850,PP24851,PP24852,PP24853,PP24854		
CCC	PP24824,PP24828,PP24832,PP24836,PP24840,PP24844,PP24852		
Internal Standard/PEM			
ICV/I.BLK	PP24815,PP24816,PP24817,PP24818,PP24819,PP24820,PP24821,PP24822,PP24855,PP24856,PP24857,PP24858,PP24859,PP24860,PP24861,PP24862		
Surrogate Standard			
MS/MSD Standard			
LCS Standard			

22	PB169322BL	PO113094.D	20 Aug 2025 17:09	YP/AJ	Ok
23	PB169326BL	PO113095.D	20 Aug 2025 17:27	YP/AJ	Ok
24	PB169326BS	PO113096.D	20 Aug 2025 17:45	YP/AJ	Ok
25	Q2894-04	PO113097.D	20 Aug 2025 18:03	YP/AJ	Ok
26	Q2907-01	PO113098.D	20 Aug 2025 18:21	YP/AJ	Ok,M
27	Q2907-02	PO113099.D	20 Aug 2025 18:40	YP/AJ	Ok,M
28	Q2907-03	PO113100.D	20 Aug 2025 18:57	YP/AJ	Ok,M
29	Q2907-04	PO113101.D	20 Aug 2025 19:16	YP/AJ	Ok,M
30	Q2908-01	PO113102.D	20 Aug 2025 19:33	YP/AJ	Ok,M
31	Q2908-02	PO113103.D	20 Aug 2025 19:51	YP/AJ	Ok,M
32	AR1660CCC500	PO113104.D	20 Aug 2025 21:05	YP/AJ	Ok
33	AR1242CCC500	PO113105.D	20 Aug 2025 21:42	YP/AJ	Ok
34	AR1248CCC500	PO113106.D	20 Aug 2025 22:00	YP/AJ	Ok
35	AR1254CCC500	PO113107.D	20 Aug 2025 22:19	YP/AJ	Ok
36	I.BLK	PO113108.D	20 Aug 2025 22:37	YP/AJ	Ok
37	Q2901-01DL	PO113109.D	20 Aug 2025 22:55	YP/AJ	Ok
38	Q2901-02DL	PO113110.D	20 Aug 2025 23:14	YP/AJ	Ok,M
39	AR1660CCC500	PO113111.D	21 Aug 2025 00:27	YP/AJ	Ok,M
40	AR1242CCC500	PO113112.D	21 Aug 2025 01:04	YP/AJ	Ok
41	AR1248CCC500	PO113113.D	21 Aug 2025 01:22	YP/AJ	Ok
42	AR1254CCC500	PO113114.D	21 Aug 2025 01:41	YP/AJ	Ok
43	I.BLK	PO113115.D	21 Aug 2025 01:59	YP/AJ	Ok

M : Manual Integration

Instrument ID: ECD_O

Daily Analysis Runlog For Sequence/QC Batch ID # PO082125

Review By	yogesh	Review On	8/21/2025 10:42:36 AM
Supervise By		Supervise On	
SubDirectory	PO082125	HP Acquire Method	HP Processing Method PO081825
STD. NAME	STD REF.#		
Tune/Reschk			
Initial Calibration Stds	PP24815,PP24816,PP24817,PP24818,PP24819,PP24820,PP24821,PP24822,PP24823,PP24824,PP24825,PP24826,PP24827,PP24828,PP24829,PP24830,PP24831,PP24832,PP24833,PP24834,PP24835,PP24836,PP24837,PP24838,PP24839,PP24840,PP24841,PP24842,PP24843,PP24844,PP24845,PP24846,PP24847,PP24848,PP24849,PP24850,PP24851,PP24852,PP24853,PP24854		
CCC	PP24824,PP24828,PP24832,PP24836,PP24840,PP24844,PP24852		
Internal Standard/PEM			
ICV/I.BLK	PP24815,PP24816,PP24817,PP24818,PP24819,PP24820,PP24821,PP24822,PP24855,PP24856,PP24857,PP24858,PP24859,PP24860,PP24861,PP24862		
Surrogate Standard			
MS/MSD Standard			
LCS Standard			

Sr#	SampleId	Data File Name	Date-Time	Operator	Status
1	HEXANE	PO113116.D	21 Aug 2025 08:47	YP/AJ	Ok
2	AR1660CCC500	PO113117.D	21 Aug 2025 09:05	YP/AJ	Ok
3	I.BLK	PO113118.D	21 Aug 2025 09:46	YP/AJ	Ok
4	DDT ANALOG	PO113119.D	21 Aug 2025 10:04	YP/AJ	Ok
5	Q2894-05	PO113120.D	21 Aug 2025 10:22	YP/AJ	Ok
6	AR1660CCC500	PO113121.D	21 Aug 2025 11:17	YP/AJ	Ok
7	AR1242CCC500	PO113122.D	21 Aug 2025 11:39	YP/AJ	Ok
8	AR1248CCC500	PO113123.D	21 Aug 2025 11:57	YP/AJ	Ok
9	AR1254CCC500	PO113124.D	21 Aug 2025 12:16	YP/AJ	Ok
10	I.BLK	PO113125.D	21 Aug 2025 12:34	YP/AJ	Ok
11	Q2896-08	PO113126.D	21 Aug 2025 12:53	YP/AJ	Ok
12	Q2896-09	PO113127.D	21 Aug 2025 13:11	YP/AJ	Ok,NS
13	Q2896-10	PO113128.D	21 Aug 2025 13:30	YP/AJ	Ok
14	Q2914-01	PO113129.D	21 Aug 2025 13:48	YP/AJ	ReRun
15	Q2914-04	PO113130.D	21 Aug 2025 14:06	YP/AJ	Ok
16	Q2914-07	PO113131.D	21 Aug 2025 14:25	YP/AJ	ReRun
17	Q2914-10	PO113132.D	21 Aug 2025 14:43	YP/AJ	ReRun
18	Q2914-13	PO113133.D	21 Aug 2025 15:02	YP/AJ	ReRun
19	Q2914-13MS	PO113134.D	21 Aug 2025 15:20	YP/AJ	Not Ok
20	Q2914-13MSD	PO113135.D	21 Aug 2025 15:37	YP/AJ	Not Ok
21	AR1660CCC500	PO113136.D	21 Aug 2025 17:09	YP/AJ	Ok

Instrument ID: ECD_O

Daily Analysis Runlog For Sequence/QC Batch ID # PO082125

Review By	yogesh	Review On	8/21/2025 10:42:36 AM
Supervise By		Supervise On	
SubDirectory	PO082125	HP Acquire Method	HP Processing Method PO081825
STD. NAME	STD REF.#		
Tune/Reschk			
Initial Calibration Stds	PP24815,PP24816,PP24817,PP24818,PP24819,PP24820,PP24821,PP24822,PP24823,PP24824,PP24825,PP24826,PP24827,PP24828,PP24829,PP24830,PP24831,PP24832,PP24833,PP24834,PP24835,PP24836,PP24837,PP24838,PP24839,PP24840,PP24841,PP24842,PP24843,PP24844,PP24845,PP24846,PP24847,PP24848,PP24849,PP24850,PP24851,PP24852,PP24853,PP24854		
CCC	PP24824,PP24828,PP24832,PP24836,PP24840,PP24844,PP24852		
Internal Standard/PEM			
ICV/I.BLK	PP24815,PP24816,PP24817,PP24818,PP24819,PP24820,PP24821,PP24822,PP24855,PP24856,PP24857,PP24858,PP24859,PP24860,PP24861,PP24862		
Surrogate Standard			
MS/MSD Standard			
LCS Standard			

22	AR1242CCC500	PO113137.D	21 Aug 2025 17:45	YP/AJ	Ok
23	AR1248CCC500	PO113138.D	21 Aug 2025 18:04	YP/AJ	Ok
24	AR1254CCC500	PO113139.D	21 Aug 2025 18:22	YP/AJ	Ok
25	I.BLK	PO113140.D	21 Aug 2025 18:41	YP/AJ	Ok
26	PB169337BL	PO113141.D	21 Aug 2025 18:59	YP/AJ	Ok
27	PB169337BS	PO113142.D	21 Aug 2025 19:17	YP/AJ	Ok
28	Q2914-16	PO113143.D	21 Aug 2025 19:36	YP/AJ	ReRun
29	Q2914-19	PO113144.D	21 Aug 2025 19:54	YP/AJ	ReRun
30	Q2922-02	PO113145.D	21 Aug 2025 20:13	YP/AJ	Ok,NS
31	Q2922-05	PO113146.D	21 Aug 2025 20:31	YP/AJ	Ok,NS
32	Q2922-08	PO113147.D	21 Aug 2025 20:49	YP/AJ	Ok,NS
33	AR1660CCC500	PO113148.D	21 Aug 2025 22:03	YP/AJ	Ok,NS
34	AR1242CCC500	PO113149.D	21 Aug 2025 22:58	YP/AJ	Ok
35	AR1248CCC500	PO113150.D	21 Aug 2025 23:17	YP/AJ	Ok
36	AR1254CCC500	PO113151.D	21 Aug 2025 23:35	YP/AJ	Ok
37	I.BLK	PO113152.D	21 Aug 2025 23:53	YP/AJ	Ok
38	Q2914-01RE	PO113153.D	22 Aug 2025 00:12	YP/AJ	Confirms
39	Q2914-04RE	PO113154.D	22 Aug 2025 00:30	YP/AJ	Not Ok
40	Q2914-07RE	PO113155.D	22 Aug 2025 00:49	YP/AJ	Confirms
41	Q2914-10RE	PO113156.D	22 Aug 2025 01:07	YP/AJ	Confirms
42	AR1660CCC500	PO113157.D	22 Aug 2025 02:21	YP/AJ	Ok,NS
43	AR1242CCC500	PO113158.D	22 Aug 2025 03:16	YP/AJ	Ok,NS
44	AR1248CCC500	PO113159.D	22 Aug 2025 03:33	YP/AJ	Ok

Instrument ID: ECD_O

Daily Analysis Runlog For Sequence/QC Batch ID # PO082125

Review By	yogesh	Review On	8/21/2025 10:42:36 AM
Supervise By		Supervise On	
SubDirectory	PO082125	HP Acquire Method	HP Processing Method PO081825
STD. NAME	STD REF.#		
Tune/Reschk			
Initial Calibration Stds	PP24815,PP24816,PP24817,PP24818,PP24819,PP24820,PP24821,PP24822,PP24823,PP24824,PP24825,PP24826,PP24827,PP24828,PP24829,PP24830,PP24831,PP24832,PP24833,PP24834,PP24835,PP24836,PP24837,PP24838,PP24839,PP24840,PP24841,PP24842,PP24843,PP24844,PP24845,PP24846,PP24847,PP24848,PP24849,PP24850,PP24851,PP24852,PP24853,PP24854		
CCC	PP24824,PP24828,PP24832,PP24836,PP24840,PP24844,PP24852		
Internal Standard/PEM			
ICV/I.BLK	PP24815,PP24816,PP24817,PP24818,PP24819,PP24820,PP24821,PP24822,PP24855,PP24856,PP24857,PP24858,PP24859,PP24860,PP24861,PP24862		
Surrogate Standard			
MS/MSD Standard			
LCS Standard			

45	AR1254CCC500	PO113160.D	22 Aug 2025 03:52	YP/AJ	Ok,NS
46	I.BLK	PO113161.D	22 Aug 2025 04:10	YP/AJ	Ok

M : Manual Integration

Instrument ID: ECD_O

Daily Analysis Runlog For Sequence/QC Batch ID # PO081825

Review By	yogesh	Review On	8/18/2025 10:23:59 AM
Supervise By	mohammad	Supervise On	8/20/2025 3:04:50 AM
SubDirectory	PO081825	HP Acquire Method	HP Processing Method PO081825

STD. NAME	STD REF.#
Tune/Reschk	
Initial Calibration Stds	PP24815,PP2416,PP24817,PP24818,PP24819,PP24820,PP24821,PP24822,PP24823,PP24824,PP24825,PP24826,PP24827,PP24828,PP24829,P P24830,PP24831,PP24832,PP24833,PP24834,PP24835,PP24836,PP24837,PP24838,PP24839,PP24840,PP24841,PP24842,PP24843,PP24844,PP 24845,PP24846,PP24847,PP24848,PP24849,PP24850,PP24851,PP24852,PP24853,PP24854
CCC	
Internal Standard/PEM	
ICV/I.BLK	PP24815,PP24816,PP24817,PP24818,PP24819,PP24820,PP24821,PP24822,PP24855,PP24856,PP24857,PP24858,PP24859,PP24860,PP24861,PP24862
Surrogate Standard	
MS/MSD Standard	
LCS Standard	

Sr#	SampleId	ClientID	Data File Name	Date-Time	Comment	Operator	Status
1	HEXANE	HEXANE	PO113001.D	18 Aug 2025 09:16		YP/AJ	Ok
2	I.BLK	I.BLK	PO113002.D	18 Aug 2025 09:34		YP/AJ	Ok
3	AR1660ICC1000	AR1660ICC1000	PO113003.D	18 Aug 2025 09:53		YP/AJ	Ok
4	AR1660ICC750	AR1660ICC750	PO113004.D	18 Aug 2025 10:11		YP/AJ	Ok
5	AR1660ICC500	AR1660ICC500	PO113005.D	18 Aug 2025 10:29		YP/AJ	Ok
6	AR1660ICC250	AR1660ICC250	PO113006.D	18 Aug 2025 10:48		YP/AJ	Ok
7	AR1660ICC050	AR1660ICC050	PO113007.D	18 Aug 2025 11:06		YP/AJ	Ok,M
8	AR1221ICC500	AR1221ICC500	PO113008.D	18 Aug 2025 11:25		YP/AJ	Ok
9	AR1232ICC500	AR1232ICC500	PO113009.D	18 Aug 2025 11:43		YP/AJ	Ok
10	AR1242ICC1000	AR1242ICC1000	PO113010.D	18 Aug 2025 12:01		YP/AJ	Ok
11	AR1242ICC750	AR1242ICC750	PO113011.D	18 Aug 2025 12:20		YP/AJ	Ok
12	AR1242ICC500	AR1242ICC500	PO113012.D	18 Aug 2025 12:38		YP/AJ	Ok
13	AR1242ICC250	AR1242ICC250	PO113013.D	18 Aug 2025 12:57		YP/AJ	Ok
14	AR1242ICC050	AR1242ICC050	PO113014.D	18 Aug 2025 13:15		YP/AJ	Ok,M
15	AR1248ICC1000	AR1248ICC1000	PO113015.D	18 Aug 2025 13:34		YP/AJ	Ok
16	AR1248ICC750	AR1248ICC750	PO113016.D	18 Aug 2025 13:52		YP/AJ	Ok
17	AR1248ICC500	AR1248ICC500	PO113017.D	18 Aug 2025 14:09		YP/AJ	Ok
18	AR1248ICC250	AR1248ICC250	PO113018.D	18 Aug 2025 14:28		YP/AJ	Ok

Instrument ID: ECD_O

Daily Analysis Runlog For Sequence/QC Batch ID # PO081825

Review By	yogesh	Review On	8/18/2025 10:23:59 AM
Supervise By	mohammad	Supervise On	8/20/2025 3:04:50 AM
SubDirectory	PO081825	HP Acquire Method	HP Processing Method PO081825
STD. NAME	STD REF.#		
Tune/Reschk	PP24815,PP2416,PP24817,PP24818,PP24819,PP24820,PP24821,PP24822,PP24823,PP24824,PP24825,PP24826,PP24827,PP24828,PP24829,P P24830,PP24831,PP24832,PP24833,PP24834,PP24835,PP24836,PP24837,PP24838,PP24839,PP24840,PP24841,PP24842,PP24843,PP24844,PP 24845,PP24846,PP24847,PP24848,PP24849,PP24850,PP24851,PP24852,PP24853,PP24854		
Initial Calibration Stds			
CCC			
Internal Standard/PEM			
ICV/I.BLK			
Surrogate Standard			
MS/MSD Standard	PP24815,PP24816,PP24817,PP24818,PP24819,PP24820,PP24821,PP24822,PP24855,PP24856,PP24857,PP24858,PP24859,PP24860,PP24861,PP24862		
LCS Standard			

19	AR1248ICC050	AR1248ICC050	PO113019.D	18 Aug 2025 14:46		YP/AJ	Ok
20	AR1254ICC1000	AR1254ICC1000	PO113020.D	18 Aug 2025 15:05		YP/AJ	Ok
21	AR1254ICC750	AR1254ICC750	PO113021.D	18 Aug 2025 15:23		YP/AJ	Ok
22	AR1254ICC500	AR1254ICC500	PO113022.D	18 Aug 2025 15:41		YP/AJ	Ok
23	AR1254ICC250	AR1254ICC250	PO113023.D	18 Aug 2025 16:00		YP/AJ	Ok
24	AR1254ICC050	AR1254ICC050	PO113024.D	18 Aug 2025 16:18		YP/AJ	Ok,M
25	AR1262ICC500	AR1262ICC500	PO113025.D	18 Aug 2025 16:54		YP/AJ	Ok
26	AR1268ICC1000	AR1268ICC1000	PO113026.D	18 Aug 2025 17:12		YP/AJ	Ok
27	AR1268ICC750	AR1268ICC750	PO113027.D	18 Aug 2025 17:30		YP/AJ	Ok
28	AR1268ICC500	AR1268ICC500	PO113028.D	18 Aug 2025 17:48		YP/AJ	Ok
29	AR1268ICC250	AR1268ICC250	PO113029.D	18 Aug 2025 18:06		YP/AJ	Ok
30	AR1268ICC050	AR1268ICC050	PO113030.D	18 Aug 2025 18:24		YP/AJ	Ok,M
31	PO081825ICV500	ICVPO081825	PO113031.D	18 Aug 2025 18:43		YP/AJ	Ok
32	AR1242ICV500	ICVPO081825AR1242	PO113032.D	18 Aug 2025 19:37		YP/AJ	Ok
33	AR1248ICV500	ICVPO081825AR1248	PO113033.D	18 Aug 2025 19:54		YP/AJ	Ok
34	AR1254ICV500	ICVPO081825AR1254	PO113034.D	18 Aug 2025 20:31		YP/AJ	Ok
35	AR1268ICV500	ICVPO081825AR1268	PO113035.D	18 Aug 2025 21:07		YP/AJ	Ok,M
36	DDT ANALOG	DDT ANALOG	PO113036.D	18 Aug 2025 21:44		YP/AJ	Ok

M : Manual Integration

Instrument ID: ECD_O

Daily Analysis Runlog For Sequence/QC Batch ID # PO082025

Review By	yogesh	Review On	8/20/2025 11:41:48 AM
Supervise By	mohammad	Supervise On	8/22/2025 2:04:33 AM
SubDirectory	PO082025	HP Acquire Method	HP Processing Method PO081825

STD. NAME	STD REF.#
Tune/Reschk	
Initial Calibration Stds	PP24815,PP2416,PP24817,PP24818,PP24819,PP24820,PP24821,PP24822,PP24823,PP24824,PP24825,PP24826,PP24827,PP24828,PP24829,P P24830,PP24831,PP24832,PP24833,PP24834,PP24835,PP24836,PP24837,PP24838,PP24839,PP24840,PP24841,PP24842,PP24843,PP24844,PP 24845,PP24846,PP24847,PP24848,PP24849,PP24850,PP24851,PP24852,PP24853,PP24854
CCC	PP24824,PP24828,PP24832,PP24836,PP24840,PP24844,PP24852
Internal Standard/PEM	
ICV/I.BLK	PP24815,PP24816,PP24817,PP24818,PP24819,PP24820,PP24821,PP24822,PP24855,PP24856,PP24857,PP24858,PP24859,PP24860,PP24861,PP24862
Surrogate Standard	
MS/MSD Standard	
LCS Standard	

Sr#	SampleId	ClientID	Data File Name	Date-Time	Comment	Operator	Status
1	HEXANE	HEXANE	PO113073.D	20 Aug 2025 09:16		YP/AJ	Ok
2	AR1660CCC500	AR1660CCC500	PO113074.D	20 Aug 2025 09:33		YP/AJ	Ok,M
3	AR1242CCC500	AR1242CCC500	PO113075.D	20 Aug 2025 09:52		YP/AJ	Ok
4	AR1248CCC500	AR1248CCC500	PO113076.D	20 Aug 2025 10:10		YP/AJ	Ok
5	AR1254CCC500	AR1254CCC500	PO113077.D	20 Aug 2025 10:28		YP/AJ	Ok
6	I.BLK	I.BLK	PO113078.D	20 Aug 2025 10:47		YP/AJ	Ok
7	DDT ANALOG	DDT ANALOG	PO113079.D	20 Aug 2025 11:05		YP/AJ	Ok
8	PB169322BL	PB169322BL	PO113080.D	20 Aug 2025 12:01	Run with cleanup sample	YP/AJ	Not Ok
9	PB169322BS	PB169322BS	PO113081.D	20 Aug 2025 12:19		YP/AJ	Ok
10	Q2894-01	1A1B1C	PO113082.D	20 Aug 2025 12:36		YP/AJ	Ok,M
11	Q2894-02	2A2B2C	PO113083.D	20 Aug 2025 12:55		YP/AJ	Ok,M
12	Q2894-03	3A3B3C	PO113084.D	20 Aug 2025 13:13		YP/AJ	Ok
13	Q2894-04	4A4B4C	PO113085.D	20 Aug 2025 13:32	need cleanup	YP/AJ	Not Ok
14	Q2894-05	5A5B5C	PO113086.D	20 Aug 2025 13:50	DCB high in both column	YP/AJ	Dilution
15	Q2901-01	HVAC DUCT SEALANT	PO113087.D	20 Aug 2025 14:09	AR1254 Hit, Need Dilution,	YP/AJ	Dilution
16	Q2901-02	EXTERIOR WINDOW C	PO113088.D	20 Aug 2025 14:27	AR1260 Hit	YP/AJ	Dilution
17	AR1660CCC500	AR1660CCC500	PO113089.D	20 Aug 2025 15:39		YP/AJ	Ok,M
18	AR1242CCC500	AR1242CCC500	PO113090.D	20 Aug 2025 15:57		YP/AJ	Ok

Instrument ID: ECD_O

Daily Analysis Runlog For Sequence/QC Batch ID # PO082025

Review By	yogesh	Review On	8/20/2025 11:41:48 AM
Supervise By	mohammad	Supervise On	8/22/2025 2:04:33 AM
SubDirectory	PO082025	HP Acquire Method	HP Processing Method PO081825
STD. NAME	STD REF.#		
Tune/Reschk			
Initial Calibration Stds	PP24815,PP2416,PP24817,PP24818,PP24819,PP24820,PP24821,PP24822,PP24823,PP24824,PP24825,PP24826,PP24827,PP24828,PP24829,P P24830,PP24831,PP24832,PP24833,PP24834,PP24835,PP24836,PP24837,PP24838,PP24839,PP24840,PP24841,PP24842,PP24843,PP24844,PP 24845,PP24846,PP24847,PP24848,PP24849,PP24850,PP24851,PP24852,PP24853,PP24854		
CCC	PP24824,PP24828,PP24832,PP24836,PP24840,PP24844,PP24852		
Internal Standard/PEM			
ICV/I.BLK	PP24815,PP24816,PP24817,PP24818,PP24819,PP24820,PP24821,PP24822,PP24855,PP24856,PP24857,PP24858,PP24859,PP24860,PP24861,PP24862		
Surrogate Standard			
MS/MSD Standard			
LCS Standard			

19	AR1248CCC500	AR1248CCC500	PO113091.D	20 Aug 2025 16:14		YP/AJ	Ok
20	AR1254CCC500	AR1254CCC500	PO113092.D	20 Aug 2025 16:32		YP/AJ	Ok
21	I.BLK	I.BLK	PO113093.D	20 Aug 2025 16:50		YP/AJ	Ok
22	PB169322BL	PB169322BL	PO113094.D	20 Aug 2025 17:09		YP/AJ	Ok
23	PB169326BL	PB169326BL	PO113095.D	20 Aug 2025 17:27		YP/AJ	Ok
24	PB169326BS	PB169326BS	PO113096.D	20 Aug 2025 17:45		YP/AJ	Ok
25	Q2894-04	4A4B4C	PO113097.D	20 Aug 2025 18:03		YP/AJ	Ok
26	Q2907-01	JEI0237-1-1	PO113098.D	20 Aug 2025 18:21		YP/AJ	Ok,M
27	Q2907-02	JEI0237-1-2	PO113099.D	20 Aug 2025 18:40	AR1260 Hit	YP/AJ	Ok,M
28	Q2907-03	BC271336-1-1	PO113100.D	20 Aug 2025 18:57	DCB high in 2nd column	YP/AJ	Ok,M
29	Q2907-04	BC271336-1-2	PO113101.D	20 Aug 2025 19:16		YP/AJ	Ok,M
30	Q2908-01	GHA571Y-1-1	PO113102.D	20 Aug 2025 19:33		YP/AJ	Ok,M
31	Q2908-02	GHA571Y-1-2	PO113103.D	20 Aug 2025 19:51		YP/AJ	Ok,M
32	AR1660CCC500	AR1660CCC500	PO113104.D	20 Aug 2025 21:05		YP/AJ	Ok
33	AR1242CCC500	AR1242CCC500	PO113105.D	20 Aug 2025 21:42		YP/AJ	Ok
34	AR1248CCC500	AR1248CCC500	PO113106.D	20 Aug 2025 22:00		YP/AJ	Ok
35	AR1254CCC500	AR1254CCC500	PO113107.D	20 Aug 2025 22:19		YP/AJ	Ok
36	I.BLK	I.BLK	PO113108.D	20 Aug 2025 22:37		YP/AJ	Ok
37	Q2901-01DL	HVAC DUCT SEALANT	PO113109.D	20 Aug 2025 22:55	AR1254 Hit	YP/AJ	Ok

Instrument ID: ECD_O

Daily Analysis Runlog For Sequence/QC Batch ID # PO082025

Review By	yogesh	Review On	8/20/2025 11:41:48 AM
Supervise By	mohammad	Supervise On	8/22/2025 2:04:33 AM
SubDirectory	PO082025	HP Acquire Method	HP Processing Method PO081825
STD. NAME	STD REF.#		
Tune/Reschk			
Initial Calibration Stds	PP24815,PP2416,PP24817,PP24818,PP24819,PP24820,PP24821,PP24822,PP24823,PP24824,PP24825,PP24826,PP24827,PP24828,PP24829,P P24830,PP24831,PP24832,PP24833,PP24834,PP24835,PP24836,PP24837,PP24838,PP24839,PP24840,PP24841,PP24842,PP24843,PP24844,PP 24845,PP24846,PP24847,PP24848,PP24849,PP24850,PP24851,PP24852,PP24853,PP24854		
CCC	PP24824,PP24828,PP24832,PP24836,PP24840,PP24844,PP24852		
Internal Standard/PEM			
ICV/I.BLK	PP24815,PP24816,PP24817,PP24818,PP24819,PP24820,PP24821,PP24822,PP24855,PP24856,PP24857,PP24858,PP24859,PP24860,PP24861,PP24862		
Surrogate Standard			
MS/MSD Standard			
LCS Standard			

38	Q2901-02DL	EXTERIOR WINDOW	PO113110.D	20 Aug 2025 23:14	AR1260 Hit	YP/AJ	Ok,M
39	AR1660CCC500	AR1660CCC500	PO113111.D	21 Aug 2025 00:27		YP/AJ	Ok,M
40	AR1242CCC500	AR1242CCC500	PO113112.D	21 Aug 2025 01:04		YP/AJ	Ok
41	AR1248CCC500	AR1248CCC500	PO113113.D	21 Aug 2025 01:22		YP/AJ	Ok
42	AR1254CCC500	AR1254CCC500	PO113114.D	21 Aug 2025 01:41		YP/AJ	Ok
43	I.BLK	I.BLK	PO113115.D	21 Aug 2025 01:59		YP/AJ	Ok

M : Manual Integration

Instrument ID: ECD_O

Daily Analysis Runlog For Sequence/QC Batch ID # PO082125

Review By	yogesh	Review On	8/21/2025 10:42:36 AM
Supervise By		Supervise On	
SubDirectory	PO082125	HP Acquire Method	HP Processing Method PO081825

STD. NAME	STD REF.#
Tune/Reschk	
Initial Calibration Stds	PP24815,PP24816,PP24817,PP24818,PP24819,PP24820,PP24821,PP24822,PP24823,PP24824,PP24825,PP24826,PP24827,PP24828,PP24829,P P24830,PP24831,PP24832,PP24833,PP24834,PP24835,PP24836,PP24837,PP24838,PP24839,PP24840,PP24841,PP24842,PP24843,PP24844,PP 24845,PP24846,PP24847,PP24848,PP24849,PP24850,PP24851,PP24852,PP24853,PP24854
CCC	PP24824,PP24828,PP24832,PP24836,PP24840,PP24844,PP24852
Internal Standard/PEM	
ICV/I.BLK	PP24815,PP24816,PP24817,PP24818,PP24819,PP24820,PP24821,PP24822,PP24855,PP24856,PP24857,PP24858,PP24859,PP24860,PP24861,PP24862
Surrogate Standard	
MS/MSD Standard	
LCS Standard	

Sr#	SampleId	ClientID	Data File Name	Date-Time	Comment	Operator	Status
1	HEXANE	HEXANE	PO113116.D	21 Aug 2025 08:47		YP/AJ	Ok
2	AR1660CCC500	AR1660CCC500	PO113117.D	21 Aug 2025 09:05		YP/AJ	Ok
3	I.BLK	I.BLK	PO113118.D	21 Aug 2025 09:46		YP/AJ	Ok
4	DDT ANALOG	DDT ANALOG	PO113119.D	21 Aug 2025 10:04		YP/AJ	Ok
5	Q2894-05	5A5B5C	PO113120.D	21 Aug 2025 10:22		YP/AJ	Ok
6	AR1660CCC500	AR1660CCC500	PO113121.D	21 Aug 2025 11:17		YP/AJ	Ok
7	AR1242CCC500	AR1242CCC500	PO113122.D	21 Aug 2025 11:39		YP/AJ	Ok
8	AR1248CCC500	AR1248CCC500	PO113123.D	21 Aug 2025 11:57		YP/AJ	Ok
9	AR1254CCC500	AR1254CCC500	PO113124.D	21 Aug 2025 12:16		YP/AJ	Ok
10	I.BLK	I.BLK	PO113125.D	21 Aug 2025 12:34		YP/AJ	Ok
11	Q2896-08	8	PO113126.D	21 Aug 2025 12:53		YP/AJ	Ok
12	Q2896-09	9	PO113127.D	21 Aug 2025 13:11		YP/AJ	Ok,NS
13	Q2896-10	10	PO113128.D	21 Aug 2025 13:30		YP/AJ	Ok
14	Q2914-01	K262-9A	PO113129.D	21 Aug 2025 13:48	DCB high in both column	YP/AJ	ReRun
15	Q2914-04	K262-10A	PO113130.D	21 Aug 2025 14:06	DCB high in 2nd column	YP/AJ	Ok
16	Q2914-07	K262-11A	PO113131.D	21 Aug 2025 14:25	DCB high in both column	YP/AJ	ReRun
17	Q2914-10	K262-12A	PO113132.D	21 Aug 2025 14:43	DCB high in both column	YP/AJ	ReRun
18	Q2914-13	K262-13A	PO113133.D	21 Aug 2025 15:02	DCB high in both column	YP/AJ	ReRun

Instrument ID: ECD_O

Daily Analysis Runlog For Sequence/QC Batch ID # PO082125

Review By	yogesh	Review On	8/21/2025 10:42:36 AM
Supervise By		Supervise On	
SubDirectory	PO082125	HP Acquire Method	HP Processing Method PO081825
STD. NAME	STD REF.#		
Tune/Reschk			
Initial Calibration Stds	PP24815,PP24816,PP24817,PP24818,PP24819,PP24820,PP24821,PP24822,PP24823,PP24824,PP24825,PP24826,PP24827,PP24828,PP24829,PP24830,PP24831,PP24832,PP24833,PP24834,PP24835,PP24836,PP24837,PP24838,PP24839,PP24840,PP24841,PP24842,PP24843,PP24844,PP24845,PP24846,PP24847,PP24848,PP24849,PP24850,PP24851,PP24852,PP24853,PP24854		
CCC	PP24824,PP24828,PP24832,PP24836,PP24840,PP24844,PP24852		
Internal Standard/PEM			
ICV/I.BLK	PP24815,PP24816,PP24817,PP24818,PP24819,PP24820,PP24821,PP24822,PP24855,PP24856,PP24857,PP24858,PP24859,PP24860,PP24861,PP24862		
Surrogate Standard			
MS/MSD Standard			
LCS Standard			

19	Q2914-13MS	K262-13AMS	PO113134.D	21 Aug 2025 15:20	No clear peak	YP/AJ	Not Ok
20	Q2914-13MSD	K262-13AMSD	PO113135.D	21 Aug 2025 15:37	No clear peak	YP/AJ	Not Ok
21	AR1660CCC500	AR1660CCC500	PO113136.D	21 Aug 2025 17:09		YP/AJ	Ok
22	AR1242CCC500	AR1242CCC500	PO113137.D	21 Aug 2025 17:45		YP/AJ	Ok
23	AR1248CCC500	AR1248CCC500	PO113138.D	21 Aug 2025 18:04		YP/AJ	Ok
24	AR1254CCC500	AR1254CCC500	PO113139.D	21 Aug 2025 18:22		YP/AJ	Ok
25	I.BLK	I.BLK	PO113140.D	21 Aug 2025 18:41		YP/AJ	Ok
26	PB169337BL	PB169337BL	PO113141.D	21 Aug 2025 18:59		YP/AJ	Ok
27	PB169337BS	PB169337BS	PO113142.D	21 Aug 2025 19:17		YP/AJ	Ok
28	Q2914-16	K262-14A	PO113143.D	21 Aug 2025 19:36	DCB high in both column	YP/AJ	ReRun
29	Q2914-19	K262-15A	PO113144.D	21 Aug 2025 19:54	DCB high in both column	YP/AJ	ReRun
30	Q2922-02	K262-16A	PO113145.D	21 Aug 2025 20:13	AR1254 Hit	YP/AJ	Ok,NS
31	Q2922-05	K262-17A	PO113146.D	21 Aug 2025 20:31	AR1254 Hit	YP/AJ	Ok,NS
32	Q2922-08	K262-18A	PO113147.D	21 Aug 2025 20:49	AR1254 Hit	YP/AJ	Ok,NS
33	AR1660CCC500	AR1660CCC500	PO113148.D	21 Aug 2025 22:03		YP/AJ	Ok,NS
34	AR1242CCC500	AR1242CCC500	PO113149.D	21 Aug 2025 22:58		YP/AJ	Ok
35	AR1248CCC500	AR1248CCC500	PO113150.D	21 Aug 2025 23:17		YP/AJ	Ok
36	AR1254CCC500	AR1254CCC500	PO113151.D	21 Aug 2025 23:35		YP/AJ	Ok
37	I.BLK	I.BLK	PO113152.D	21 Aug 2025 23:53		YP/AJ	Ok

Instrument ID: ECD_O

Daily Analysis Runlog For Sequence/QC Batch ID # PO082125

Review By	yogesh	Review On	8/21/2025 10:42:36 AM
Supervise By		Supervise On	
SubDirectory	PO082125	HP Acquire Method	HP Processing Method PO081825
STD. NAME	STD REF.#		
Tune/Reschk			
Initial Calibration Stds	PP24815,PP24816,PP24817,PP24818,PP24819,PP24820,PP24821,PP24822,PP24823,PP24824,PP24825,PP24826,PP24827,PP24828,PP24829,P P24830,PP24831,PP24832,PP24833,PP24834,PP24835,PP24836,PP24837,PP24838,PP24839,PP24840,PP24841,PP24842,PP24843,PP24844,PP 24845,PP24846,PP24847,PP24848,PP24849,PP24850,PP24851,PP24852,PP24853,PP24854		
CCC	PP24824,PP24828,PP24832,PP24836,PP24840,PP24844,PP24852		
Internal Standard/PEM			
ICV/I.BLK	PP24815,PP24816,PP24817,PP24818,PP24819,PP24820,PP24821,PP24822,PP24855,PP24856,PP24857,PP24858,PP24859,PP24860,PP24861,PP24862		
Surrogate Standard			
MS/MSD Standard			
LCS Standard			

38	Q2914-01RE	K262-9ARE	PO113153.D	22 Aug 2025 00:12	DCB high in both column	YP/AJ	Confirms
39	Q2914-04RE	K262-10ARE	PO113154.D	22 Aug 2025 00:30	not needed	YP/AJ	Not Ok
40	Q2914-07RE	K262-11ARE	PO113155.D	22 Aug 2025 00:49	DCB high in both column	YP/AJ	Confirms
41	Q2914-10RE	K262-12ARE	PO113156.D	22 Aug 2025 01:07	DCB high in both column	YP/AJ	Confirms
42	AR1660CCC500	AR1660CCC500	PO113157.D	22 Aug 2025 02:21		YP/AJ	Ok,NS
43	AR1242CCC500	AR1242CCC500	PO113158.D	22 Aug 2025 03:16		YP/AJ	Ok,NS
44	AR1248CCC500	AR1248CCC500	PO113159.D	22 Aug 2025 03:33		YP/AJ	Ok
45	AR1254CCC500	AR1254CCC500	PO113160.D	22 Aug 2025 03:52		YP/AJ	Ok,NS
46	I.BLK	I.BLK	PO113161.D	22 Aug 2025 04:10		YP/AJ	Ok

M : Manual Integration

PERCENT SOLID

Supervisor: rubina
Analyst: jignesh
Date: 8/19/2025

OVENTEMP IN Celsius(°C): 107
Time IN: 17:00
In Date: 08/18/2025
Weight Check 1.0g: 1.00
Weight Check 10g: 10.00
OvenID: M OVEN#1

OVENTEMP OUT Celsius(°C): 104
Time OUT: 08:25
Out Date: 08/19/2025
Weight Check 1.0g: 1.00
Weight Check 10g: 10.00
BalanceID: M SC-4
Thermometer ID: % SOLID-OVEN

QC:LB136862

Lab ID	Client SampleID	Dish #	Dish Wt(g) (A)	Sample Wt(g)	Dish + Sample Wt(g) (B)	Dish+Dry Sample Wt(g) (C)	% Solid	Comments
Q2891-01	BARRICADE	1	1.00	1.00	2.00	2.00	100.0	STONE SAMPLE, 100% SOLIDS
Q2891-02	WALL-1	2	1.00	1.00	2.00	2.00	100.0	Concreate sample
Q2891-03	WALL-2	3	1.00	1.00	2.00	2.00	100.0	STONE SAMPLE, 100% SOLIDS
Q2891-04	WALL-3	4	1.00	1.00	2.00	2.00	100.0	STONE SAMPLE, 100% SOLIDS
Q2892-01	1ST-FLOOR-NORTH-EAST-C ONRNER-BACK-A	5	1.18	10.03	11.21	10.19	89.8	
Q2892-02	1ST-FLOOR-NORTH-EAST-C ONRNER-BACK-A	6	1.16	9.97	11.13	10.22	90.9	
Q2892-03	1ST-FLOOR-DRILL-B-BACK	7	1.19	10.43	11.62	10.54	89.6	
Q2892-04	1ST-FLOOR-DRILL-B-BACK	8	1.16	10.39	11.55	10.48	89.7	
Q2892-05	BACK-1-FLOOR-CENTER-MI DDLE-C	9	1.18	10.41	11.59	10.39	88.5	
Q2892-06	BACK-1-FLOOR-CENTER-MI DDLE-C	10	1.19	10.38	11.57	10.52	89.9	
Q2892-07	3-FLOOR-NORTH-D	11	1.15	10.68	11.83	11.09	93.1	
Q2892-08	3-FLOOR-NORTH-D	12	1.13	10.24	11.37	10.77	94.1	
Q2892-09	3-FLOOR-SOUTH-E	13	1.17	10.21	11.38	10.48	91.2	
Q2892-10	3-FLOOR-SOUTH-E	14	1.18	10.34	11.52	10.65	91.6	
Q2892-11	FRONT-1-FLOOR-F	15	1.16	10.21	11.37	10.42	90.7	
Q2892-12	FRONT-1-FLOOR-F	16	1.14	10.64	11.78	10.52	88.2	
Q2893-01	LOD-MDL-SOIL-01-QT3-20 25	36	1.00	1.00	2.00	2.00	100.0	
Q2893-02	LOQ-SOIL-02-QT3-2025	37	1.00	1.00	2.00	2.00	100.0	
Q2893-03	MDL-SOIL-03-QT3-2025	38	1.00	1.00	2.00	2.00	100.0	
Q2893-04	LOD-MDL-SOIL-04-QT3-20 25	39	1.00	1.00	2.00	2.00	100.0	
Q2893-05	LOQ-SOIL-05-QT3-2025	40	1.00	1.00	2.00	2.00	100.0	
Q2893-06	MDL-SOIL-06-QT3-2025	41	1.00	1.00	2.00	2.00	100.0	
Q2893-16	LLOQ-SOIL-QT3-2025	42	1.00	1.00	2.00	2.00	100.0	
Q2894-01	1A1B1C	17	1.00	1.00	2.00	2.00	100.0	Caulk sample
Q2894-02	2A2B2C	18	1.00	1.00	2.00	2.00	100.0	Caulk sample
Q2894-03	3A3B3C	19	1.00	1.00	2.00	2.00	100.0	Caulk sample

PERCENT SOLID

Supervisor: rubina
Analyst: jignesh
Date: 8/19/2025

OVENTEMP IN Celsius(°C): 107
Time IN: 17:00
In Date: 08/18/2025
Weight Check 1.0g: 1.00
Weight Check 10g: 10.00
OvenID: M OVEN#1

OVENTEMP OUT Celsius(°C): 104
Time OUT: 08:25
Out Date: 08/19/2025
Weight Check 1.0g: 1.00
Weight Check 10g: 10.00
BalanceID: M SC-4
Thermometer ID: % SOLID-OVEN

QC:LB136862

Lab ID	Client SampleID	Dish #	Dish Wt(g) (A)	Sample Wt(g)	Dish + Sample Wt(g) (B)	Dish+Dry Sample Wt(g) (C)	% Solid	Comments
Q2894-04	4A4B4C	20	1.00	1.00	2.00	2.00	100.0	Caulk sample
Q2894-05	5A5B5C	21	1.00	1.00	2.00	2.00	100.0	Caulk sample
Q2895-01	1104	22	1.00	1.00	2.00	2.00	100.0	oil sample
Q2895-03	1204	23	1.00	1.00	2.00	2.00	100.0	debris
Q2896-01	1	24	1.00	1.00	2.00	2.00	100.0	WIPE SAMPLE
Q2896-02	2	25	1.00	1.00	2.00	2.00	100.0	WIPE SAMPLE
Q2896-03	3	26	1.00	1.00	2.00	2.00	100.0	WIPE SAMPLE
Q2896-04	4	27	1.00	1.00	2.00	2.00	100.0	WIPE SAMPLE
Q2896-05	5	28	1.00	1.00	2.00	2.00	100.0	WIPE SAMPLE
Q2896-06	6	29	1.00	1.00	2.00	2.00	100.0	WIPE SAMPLE
Q2896-07	7	30	1.00	1.00	2.00	2.00	100.0	WIPE SAMPLE
Q2896-08	8	31	1.00	1.00	2.00	2.00	100.0	WIPE SAMPLE
Q2896-09	9	32	1.00	1.00	2.00	2.00	100.0	WIPE SAMPLE
Q2896-10	10	33	1.00	1.00	2.00	2.00	100.0	WIPE SAMPLE
Q2897-01	HD-02-08182025	34	1.15	10.84	11.99	10.64	87.5	
Q2897-02	HD-02-08182025-E2	35	1.17	10.35	11.52	10.29	88.1	
Q2899-03	MDL-SOIL-QT3-2025-05	43	1.00	1.00	2.00	2.00	100.0	
Q2899-04	MDL-SOIL-QT3-2025-06	44	1.00	1.00	2.00	2.00	100.0	
Q2899-05	MDL-MED-SOIL-QT3-2025-05	45	1.00	1.00	2.00	2.00	100.0	
Q2899-06	MDL-MED-SOIL-QT3-2025-06	46	1.00	1.00	2.00	2.00	100.0	

$$\% \text{ Solid} = \frac{(C-A) * 100}{(B-A)}$$

WORKLIST(Hardcopy Internal Chain)

17136862

WorkList Name : %1-081825 WorkList ID : 191322 Department : Wet-Chemistry Date : 08-18-2025 08:19:10

Sample	Customer Sample	Matrix	Test	Preservative	Customer	Raw Sample Storage Location	Collect Date	Method
Q2891-01	BARRICADE	Solid	Percent Solids	Cool 4 deg C	PSEG03	D31	08/15/2025	Chemtech -SO
Q2891-02	WALL-1	Solid	Percent Solids	Cool 4 deg C	PSEG03	D31	08/15/2025	Chemtech -SO
Q2891-03	WALL-2	Solid	Percent Solids	Cool 4 deg C	PSEG03	D31	08/15/2025	Chemtech -SO
Q2891-04	WALL-3	Solid	Percent Solids	Cool 4 deg C	PSEG03	D31	08/15/2025	Chemtech -SO
Q2892-01	1ST-FLOOR-NORTH-EAST-CC	Solid	Percent Solids	Cool 4 deg C	BAPS03	D31	08/15/2025	Chemtech -SO
Q2892-02	1ST-FLOOR-NORTH-EAST-CC	Solid	Percent Solids	Cool 4 deg C	BAPS03	D31	08/15/2025	Chemtech -SO
Q2892-03	1ST-FLOOR-DRILL-B-BACK	Solid	Percent Solids	Cool 4 deg C	BAPS03	D31	08/15/2025	Chemtech -SO
Q2892-04	1ST-FLOOR-DRILL-B-BACK	Solid	Percent Solids	Cool 4 deg C	BAPS03	D31	08/15/2025	Chemtech -SO
Q2892-05	BACK-1-FLOOR-CENTER-MID	Solid	Percent Solids	Cool 4 deg C	BAPS03	D31	08/15/2025	Chemtech -SO
Q2892-06	BACK-1-FLOOR-CENTER-MID	Solid	Percent Solids	Cool 4 deg C	BAPS03	D31	08/15/2025	Chemtech -SO
Q2892-07	3-FLOOR-NORTH-D	Solid	Percent Solids	Cool 4 deg C	BAPS03	D31	08/15/2025	Chemtech -SO
Q2892-08	3-FLOOR-NORTH-D	Solid	Percent Solids	Cool 4 deg C	BAPS03	D31	08/15/2025	Chemtech -SO
Q2892-09	3-FLOOR-SOUTH-E	Solid	Percent Solids	Cool 4 deg C	BAPS03	D31	08/15/2025	Chemtech -SO
Q2892-10	3-FLOOR-SOUTH-E	Solid	Percent Solids	Cool 4 deg C	BAPS03	D31	08/15/2025	Chemtech -SO
Q2892-11	FRONT-1-FLOOR-F	Solid	Percent Solids	Cool 4 deg C	BAPS03	D31	08/15/2025	Chemtech -SO
Q2892-12	FRONT-1-FLOOR-F	Solid	Percent Solids	Cool 4 deg C	BAPS03	D31	08/15/2025	Chemtech -SO
Q2893-01	LOD-MDL-SOIL-01-QT3-2025	Solid	Percent Solids	NONE	ALLI03	QA Of	08/18/2025	Chemtech -SO
Q2893-02	LOQ-SOIL-02-QT3-2025	Solid	Percent Solids	NONE	ALLI03	QA Of	08/18/2025	Chemtech -SO
Q2893-03	MDL-SOIL-03-QT3-2025	Solid	Percent Solids	NONE	ALLI03	QA Of	08/18/2025	Chemtech -SO
Q2893-04	LOD-MDL-SOIL-04-QT3-2025	Solid	Percent Solids	NONE	ALLI03	QA Of	08/18/2025	Chemtech -SO
Q2893-05	LOQ-SOIL-05-QT3-2025	Solid	Percent Solids	NONE	ALLI03	QA Of	08/18/2025	Chemtech -SO

Date/Time 08/18/25 13:00
 Raw Sample Received by: [Signature]
 Raw Sample Relinquished by: [Signature]
 Date/Time 08/18/25 17:10
 Raw Sample Received by: [Signature]
 Raw Sample Relinquished by: [Signature]

WORKLIST(Hardcopy Internal Chain)

136862

WorkList Name : %1-081825 WorkList ID : 191322 Department : Wet-Chemistry Date : 08-18-2025 08:19:10

Sample	Customer Sample	Matrix	Test	Preservative	Customer	Raw Sample Storage Location	Collect Date	Method
Q2893-06	MDL-SOIL-06-QT3-2025	Solid	Percent Solids	NONE	ALLI03	QA Of	08/18/2025	Chemtech -SO
Q2893-16	LLOQ-SOIL-QT3-2025	Solid	Percent Solids	NONE	ALLI03	QA Of	08/18/2025	Chemtech -SO
Q2894-01	1A1B1C	Solid	Percent Solids	Cool 4 deg C	ATCE02	J32	08/07/2025	Chemtech -SO
Q2894-02	2A2B2C	Solid	Percent Solids	Cool 4 deg C	ATCE02	J32	08/07/2025	Chemtech -SO
Q2894-03	3A3B3C	Solid	Percent Solids	Cool 4 deg C	ATCE02	J32	08/07/2025	Chemtech -SO
Q2894-04	4A4B4C	Solid	Percent Solids	Cool 4 deg C	ATCE02	J32	08/07/2025	Chemtech -SO
Q2894-05	5A5B5C	Solid	Percent Solids	Cool 4 deg C	ATCE02	J32	08/07/2025	Chemtech -SO
Q2895-01	1104	Solid	Percent Solids	Cool 4 deg C	PSEG03	D31	08/18/2025	Chemtech -SO
Q2895-03	1204	Solid	Percent Solids	Cool 4 deg C	PSEG03	D31	08/18/2025	Chemtech -SO
Q2896-01	1	Solid	Percent Solids	Cool 4 deg C	PSEG03	D31	08/18/2025	Chemtech -SO
Q2896-02	2	Solid	Percent Solids	Cool 4 deg C	PSEG03	D31	08/18/2025	Chemtech -SO
Q2896-03	3	Solid	Percent Solids	Cool 4 deg C	PSEG03	D31	08/18/2025	Chemtech -SO
Q2896-04	4	Solid	Percent Solids	Cool 4 deg C	PSEG03	D31	08/18/2025	Chemtech -SO
Q2896-05	5	Solid	Percent Solids	Cool 4 deg C	PSEG03	D31	08/18/2025	Chemtech -SO
Q2896-06	6	Solid	Percent Solids	Cool 4 deg C	PSEG03	D31	08/18/2025	Chemtech -SO
Q2896-07	7	Solid	Percent Solids	Cool 4 deg C	PSEG03	D31	08/18/2025	Chemtech -SO
Q2896-08	8	Solid	Percent Solids	Cool 4 deg C	PSEG03	D31	08/18/2025	Chemtech -SO
Q2896-09	9	Solid	Percent Solids	Cool 4 deg C	PSEG03	D31	08/18/2025	Chemtech -SO
Q2896-10	10	Solid	Percent Solids	Cool 4 deg C	PSEG03	D31	08/18/2025	Chemtech -SO
Q2897-01	HD-02-08182025	Solid	Percent Solids	Cool 4 deg C	PSEG05	D21	08/18/2025	Chemtech -SO
Q2897-02	HD-02-08182025-E2	Solid	Percent Solids	Cool 4 deg C	PSEG05	D21	08/18/2025	Chemtech -SO

Date/Time 08/18/25 15:00 Date/Time 08/18/25 17:10
 Raw Sample Received by: SB WOC Raw Sample Received by: [Signature]
 Raw Sample Relinquished by: [Signature] Raw Sample Relinquished by: [Signature]

WORKLIST(Hardcopy Internal Chain)

873682

WorkList Name : %1-081825

WorkList ID : 191322

Department : Wet-Chemistry

Date : 08-18-2025 08:19:10

Sample	Customer Sample	Matrix	Test	Preservative	Customer	Raw Sample Storage Location	Collect Date	Method
Q2899-03	MDL-SOIL-QT3-2025-05	Solid	Percent Solids	Cool 4 deg C	ALLI03	QA Of	08/18/2025	Chemtech -SO
Q2899-04	MDL-SOIL-QT3-2025-06	Solid	Percent Solids	Cool 4 deg C	ALLI03	QA Of	08/18/2025	Chemtech -SO
Q2899-05	MDL-MED-SOIL-QT3-2025-05	Solid	Percent Solids	Cool 4 deg C	ALLI03	QA Of	08/18/2025	Chemtech -SO
Q2899-06	MDL-MED-SOIL-QT3-2025-06	Solid	Percent Solids	Cool 4 deg C	ALLI03	QA Of	08/18/2025	Chemtech -SO

Date/Time 08/18/25 13:00

Raw Sample Received by: Sh wcy

Raw Sample Relinquished by: Sh wcy

Date/Time 08-18-25 17:10

Raw Sample Received by: Sh wcy

Raw Sample Relinquished by: Sh wcy

SOP ID: M3541-ASE Extraction-15

Clean Up SOP #: Acid Cleanup

Extraction Start Date : 08/20/2025

Matrix : Solid

Extraction Start Time : 08:40

Weigh By: EH

Extraction By: RJ

Extraction End Date : 08/20/2025

Balance check: RJ

Filter By: RJ

Extraction End Time : 11:45

Balance ID: EX-SC-2

pH Meter ID: N/A

Concentration By: EH

pH Strip Lot#: N/A

Hood ID: 3,7

Supervisor By : RUPESH

Extraction Method: ☐ Separatory Funnel

☐ Continuous Liquid/Liquid

☐ Sonication

☐ Waste Dilution

☒ Soxhlet

Standard Name	MLS USED	Concentration ug/mL	STD REF. # FROM LOG
Spike Sol 1	1.0ML	5000 PPB	PP24799
Surrogate	1.0ML	200 PPB	PP24663
N/A	N/A	N/A	N/A
N/A	N/A	N/A	N/A
N/A	N/A	N/A	N/A

Chemical Used	ML/SAMPLE USED	Lot Number
Hexane/Acetone/1:1	N/A	EP2627
Baked Na2SO4	N/A	EP2632
Hexane	N/A	E3962
H2SO4 1:1	N/A	EP2610
Sand	N/A	E3951
N/A	N/A	N/A
N/A	N/A	N/A
N/A	N/A	N/A
N/A	N/A	N/A
N/A	N/A	N/A
N/A	N/A	N/A
N/A	N/A	N/A
N/A	N/A	N/A
N/A	N/A	N/A

Extraction Conformance/Non-Conformance Comments:

40ML Vial Lot # 03-40BTS721, No MS/MSD Performed as sample are Caulk Mat. With Limited Volume.

KD Bath ID: N/A

Envap ID: NEVAP-02

KD Bath Temperature: N/A

Envap Temperature: 40 °C

Date / Time	Prepped Sample Relinquished By/Location	Received By/Location
8/20/25	RS (EH Lab)	Y. P. Pestil PuB.
11:50	Preparation Group	Analysis Group

Analytical Method: M3541-ASE Extraction-15

Concentration Date: 08/20/2025

Sample ID	Client Sample ID	Test	g/ mL	PH	Surr/Spike By:		Final Vol. (mL)	JarID	Comments	Prep Pos
					AddedBy	VerifiedBy				
PB169322BL	ABLK322	PCB	30.01	N/A	ritesh	Evelyn	10			U3-1
PB169322BS	ALCS322	PCB	30.02	N/A	ritesh	Evelyn	10			2
Q2894-01	1A1B1C	PCB	8.42	N/A	ritesh	Evelyn	10		Caulk Mat.	3
Q2894-02	2A2B2C	PCB	2.19	N/A	ritesh	Evelyn	10		Caulk Mat.	4
Q2894-03	3A3B3C	PCB	1.83	N/A	ritesh	Evelyn	10		Caulk Mat.	5
Q2894-04	4A4B4C	PCB	2.30	N/A	ritesh	Evelyn	10		Caulk Mat.	6
Q2894-05	5A5B5C	PCB	7.80	N/A	ritesh	Evelyn	10		Caulk Mat.	U6-1
Q2901-01	HVAC DUCT SEALANT	PCB Group1	4.25	N/A	ritesh	Evelyn	10		Caulk Mat.	2
Q2901-02	EXTERIOR WINDOW CAULK	PCB Group1	0.68	N/A	ritesh	Evelyn	10		Caulk Mat.	3

16932
8:40

WORKLIST(Hardcopy Internal Chain)

WorkList Name : Q2894 WorkList ID : 191362 Department : Extraction Date : 08-20-2025 08:25:59

Sample	Customer Sample	Matrix	Test	Preservative	Customer	Raw Sample Storage Location	Collect Date	Method
Q2894-01	1A1B1C	Solid	PCB	Cool 4 deg C	ATCE02	J32	08/18/2025	8082A
Q2894-02	2A2B2C	Solid	PCB	Cool 4 deg C	ATCE02	J32	08/07/2025	8082A
Q2894-03	3A3B3C	Solid	PCB	Cool 4 deg C	ATCE02	J32	08/07/2025	8082A
Q2894-04	4A4B4C	Solid	PCB	Cool 4 deg C	ATCE02	J32	08/07/2025	8082A
Q2894-05	5A5B5C	Solid	PCB	Cool 4 deg C	ATCE02	J32	08/07/2025	8082A
Q2901-01	HVAC DUCT SEALANT	Solid	PCB Group1	Cool 4 deg C	ATCE02	J11	08/13/2025	8082A
Q2901-02	EXTERIOR WINDOW CAULK	Solid	PCB Group1	Cool 4 deg C	ATCE02	J11	08/13/2025	8082A

Date/Time 08/20/25 8:35
Raw Sample Received by: RJ (EXT-106b)
Raw Sample Relinquished by: [Signature]

Date/Time 08/20/25 8:50
Raw Sample Received by: [Signature]
Raw Sample Relinquished by: RJ (EXT-106b)

Prep Standard - Chemical Standard Summary

Order ID : Q2894

Test : PCB

Prepbatch ID : PB169322,

Sequence ID/Qc Batch ID: PO082025,PO082125,

Standard ID :

EP2610,EP2627,EP2632,PP2414,PP2416,PP24329,PP24330,PP24381,PP24663,PP24799,PP24805,PP24806,PP24807,PP24808,PP24809,PP24810,PP24811,PP24812,PP24814,PP24815,PP24816,PP24817,PP24818,PP24819,PP24820,PP24821,PP24822,PP24823,PP24824,PP24825,PP24826,PP24827,PP24828,PP24829,PP24830,PP24831,PP24832,PP24833,PP24834,PP24835,PP24836,PP24837,PP24838,PP24839,PP24840,PP24841,PP24842,PP24843,PP24844,PP24845,PP24846,PP24847,PP24848,PP24849,PP24850,PP24851,PP24852,PP24853,PP24854,PP24855,PP24856,PP24857,PP24858,PP24859,PP24860,PP24861,PP24862,

Chemical ID :

E3804,E3875,E3944,E3949,E3950,E3951,E3955,E3962,E3963,M6157,P11522,P11592,P12700,P12703,P12951,P12952,P12957,P13356,P13373,P13375,P13590,P13592,P13695,P13697,P13706,P13786,P13789,P13833,P13879,P13881,P13885,P2258,P2287,W3112,W3177,W3234,



<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
314	1.1 H2SO4 SOLN	EP2610	05/07/2025	11/07/2025	RUPESHKUMAR SHAH	Extraction_SCALE_2 (EX-SC-2)	None	Riteshkumar Patel 05/07/2025
<u>FROM</u>	1000.00000ml of M6157 + 1000.00000ml of W3112 = Final Quantity: 2000.000 ml							

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
230	1:1ACETONE/HEXANE	EP2627	07/15/2025	01/15/2026	RUPESHKUMAR SHAH	None	None	Riteshkumar Patel 07/15/2025
<u>FROM</u> 4000.00000ml of E3949 + 4000.00000ml of E3950 = Final Quantity: 8000.000 ml								



<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
3923	Baked Sodium Sulfate	EP2632	08/11/2025	01/28/2026	RUPESHKUMAR SHAH	Extraction_SCALE_2 (EX-SC-2)	None	Riteshkumar Patel 08/11/2025
<u>FROM</u> 4000.00000gram of E3875 = Final Quantity: 4000.000 gram								

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipettelID</u>	<u>Supervised By</u>
1534	Pesticides Intermediate 5ppm	PP2414	07/26/2009	07/26/2011				Yogesh Patel 07/24/2025
<u>FROM</u> 0.02500ml of P2258 + 0.12500ml of P2287 = Final Quantity: 10.000 ml								

Pest/Pcb STANDARD PREPARATION LOG

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
1536	Pesticides calibration level-5	PP2416	07/26/2010	07/26/2011				Yogesh Patel
								07/24/2025

FROM 0.37500ml of PP2414 = Final Quantity: 25.000 ml

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
84	Pest/PCB Surrogate Stock 20 PPM	PP24329	03/18/2025	08/22/2025	Yogesh Patel	None	None	Abdul Mirza
								04/03/2025

FROM 1.00000ml of P13356 + 9.00000ml of W3177 = Final Quantity: 10.000 ml

Pest/Pcb STANDARD PREPARATION LOG

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
202	AR1660 1000/100 ppb working solution 1st source	PP24330	03/18/2025	08/22/2025	Yogesh Patel	None	None	Abdul Mirza
								04/03/2025

FROM 0.10000ml of P13697 + 99.40000ml of W3177 + 0.50000ml of PP24329 = Final Quantity: 100.000 ml

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
1893	AR1254 1000 PPB Working Sol. 2nd Source	PP24381	03/18/2025	08/22/2025	Yogesh Patel	None	None	Abdul Mirza
								04/03/2025

FROM 1.00000ml of P12957 + 98.50000ml of W3177 + 0.50000ml of PP24329 = Final Quantity: 100.000 ml

Pest/Pcb STANDARD PREPARATION LOG

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
465	200 PPB Pest/PCB Surrogate Spike	PP24663	06/24/2025	12/24/2025	Abdul Mirza	None	None	Yogesh Patel
								07/21/2025

FROM 1.00000ml of P13786 + 999.00000ml of E3944 = Final Quantity: 1000.000 ml

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
3857	5000 PPB PCB SPIKE SOLUTION 2ND SOURCE	PP24799	08/12/2025	02/12/2026	Abdul Mirza	None	None	Yogesh Patel
								08/19/2025

FROM 0.50000ml of P12951 + 99.50000ml of E3955 = Final Quantity: 100.000 ml

Pest/Pcb STANDARD PREPARATION LOG

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
84	Pest/PCB Surrogate Stock 20 PPM	PP24805	08/18/2025	02/18/2026	Yogesh Patel	None	None	Abdul Mirza
								08/19/2025

FROM 1.00000ml of P13789 + 9.00000ml of E3962 = Final Quantity: 10.000 ml

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
213	AR1221 1000 PPB WORKING SOLUTION	PP24806	08/18/2025	02/18/2026	Yogesh Patel	None	None	Abdul Mirza
								08/19/2025

FROM 0.10000ml of P13375 + 99.40000ml of E3962 + 0.50000ml of PP24805 = Final Quantity: 100.000 ml

Pest/Pcb STANDARD PREPARATION LOG

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
214	AR1232 1000 PPB WORKING SOLUTION	PP24807	08/18/2025	02/18/2026	Yogesh Patel	None	None	Abdul Mirza
								08/19/2025

FROM 0.10000ml of P13879 + 99.40000ml of E3962 + 0.50000ml of PP24805 = Final Quantity: 100.000 ml

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
215	AR1242 1000 PPB WORKING STD	PP24808	08/18/2025	02/18/2026	Yogesh Patel	None	None	Abdul Mirza
								08/19/2025

FROM 0.10000ml of P13706 + 99.40000ml of E3962 + 0.50000ml of PP24805 = Final Quantity: 100.000 ml

Pest/Pcb STANDARD PREPARATION LOG

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
216	AR1248 1000 PPB WORKING STD	PP24809	08/18/2025	02/18/2026	Yogesh Patel	None	None	Abdul Mirza
								08/19/2025

FROM 0.10000ml of P13695 + 99.40000ml of E3962 + 0.50000ml of PP24805 = Final Quantity: 100.000 ml

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
217	AR1254 1000 PPB WORKING STD	PP24810	08/18/2025	02/18/2026	Yogesh Patel	None	None	Abdul Mirza
								08/19/2025

FROM 0.10000ml of P11592 + 99.40000ml of E3962 + 0.50000ml of PP24805 = Final Quantity: 100.000 ml



284 Sheffield Street, Mountainside, New Jersey 07092, Phone : 908 789 8900,
Fax : 908 789 8922

284 Sheffield Street, Mountainside, New Jersey 07092, Phone : 908 789 8900,
Fax : 908 789 8922

284 Sheffield Street, Mountainside, New Jersey 07092, Phone : 908 789 8900,
Fax : 908 789 8922

284 Sheffield Street, Mountainside, New Jersey 07092, Phone : 908 789 8900,
Fax : 908 789 8922

284 Sheffield Street, Mountainside, New Jersey 07092, Phone : 908 789 8900,
Fax : 908 789 8922

Pest/Pcb STANDARD PREPARATION LOG

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
404	AR1660 100 PPM Stock Solution 2nd Source	PP24814	08/18/2025	02/18/2026	Yogesh Patel	None	None	Abdul Mirza
								08/19/2025

FROM 1.00000ml of P12952 + 9.00000ml of E3804 = Final Quantity: 10.000 ml

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
405	AR1660 1000/100 PPB ICV STD	PP24815	08/18/2025	02/18/2026	Yogesh Patel	None	None	Abdul Mirza
								08/19/2025

FROM 98.50000ml of E3962 + 0.50000ml of PP24805 + 1.00000ml of PP24814 = Final Quantity: 100.000 ml

Pest/Pcb STANDARD PREPARATION LOG

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
3789	AR1221 1000 PPB WORKING SOL.2ND SOURCE(AGILENT)	PP24816	08/18/2025	09/18/2025	Yogesh Patel	None	None	Abdul Mirza
								08/19/2025

FROM 1.00000ml of P13373 + 98.50000ml of E3962 + 0.50000ml of PP24805 = Final Quantity: 100.000 ml

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
1887	AR1232 1000 PPB Working Sol. 2nd Source	PP24817	08/18/2025	02/18/2026	Yogesh Patel	None	None	Abdul Mirza
								08/19/2025

FROM 1.00000ml of P12700 + 98.50000ml of E3962 + 0.50000ml of PP24805 = Final Quantity: 100.000 ml

Pest/Pcb STANDARD PREPARATION LOG

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
1889	AR1242 1000 PPB Working Sol. 2nd Source	PP24818	08/18/2025	02/18/2026	Yogesh Patel	None	None	Abdul Mirza
								08/19/2025

FROM 1.00000ml of P13590 + 98.50000ml of E3962 + 0.50000ml of PP24805 = Final Quantity: 100.000 ml

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
1890	AR1248 1000 PPB Working Sol. 2nd Source	PP24819	08/18/2025	02/18/2026	Yogesh Patel	None	None	Abdul Mirza
								08/19/2025

FROM 1.00000ml of P13592 + 98.50000ml of E3962 + 0.50000ml of PP24805 = Final Quantity: 100.000 ml

Pest/Pcb STANDARD PREPARATION LOG

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
2193	AR1254 100 PPM STOCK SOLUTION	PP24820	08/18/2025	02/15/2026	Yogesh Patel	None	None	Abdul Mirza
								08/19/2025

FROM 1.00000ml of P13833 + 9.00000ml of E3963 = Final Quantity: 10.000 ml

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
3757	AR1262 1000 PPB Working Solution second source	PP24821	08/18/2025	02/18/2026	Yogesh Patel	None	None	Abdul Mirza
								08/19/2025

FROM 1.00000ml of P12703 + 98.50000ml of E3962 + 0.50000ml of PP24805 = Final Quantity: 100.000 ml

Pest/Pcb STANDARD PREPARATION LOG

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
3817	AR1268 1000 ppb Working Soln. 2nd source	PP24822	08/18/2025	09/18/2025	Yogesh Patel	None	None	Abdul Mirza
								08/19/2025

FROM 1.00000ml of P11522 + 98.50000ml of E3962 + 0.50000ml of PP24805 = Final Quantity: 100.000 ml

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
203	AR1660 750 PPB STD	PP24823	08/18/2025	02/18/2026	Yogesh Patel	None	None	Abdul Mirza
								08/19/2025

FROM 0.25000ml of W3234 + 0.75000ml of PP24330 = Final Quantity: 1.000 ml

Pest/Pcb STANDARD PREPARATION LOG

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
204	AR1660 500 PPB STD	PP24824	08/18/2025	02/18/2026	Yogesh Patel	None	None	Abdul Mirza
								08/19/2025

FROM 0.50000ml of W3234 + 0.50000ml of PP24330 = Final Quantity: 1.000 ml

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
205	AR1660 250 PPB STD	PP24825	08/18/2025	02/18/2026	Yogesh Patel	None	None	Abdul Mirza
								08/19/2025

FROM 0.75000ml of W3234 + 0.25000ml of PP24330 = Final Quantity: 1.000 ml

Pest/Pcb STANDARD PREPARATION LOG

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
206	AR1660 50 PPB STD	PP24826	08/18/2025	02/18/2026	Yogesh Patel	None	None	Abdul Mirza
								08/19/2025

FROM 0.90000ml of W3234 + 0.10000ml of PP24824 = Final Quantity: 1.000 ml

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
1079	AR1221 750 PPB STD	PP24827	08/18/2025	02/18/2026	Yogesh Patel	None	None	Abdul Mirza
								08/19/2025

FROM 0.25000ml of W3234 + 0.75000ml of PP24806 = Final Quantity: 1.000 ml

Pest/Pcb STANDARD PREPARATION LOG

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
222	AR1221 500 PPB STD	PP24828	08/18/2025	02/18/2026	Yogesh Patel	None	None	Abdul Mirza
								08/19/2025

FROM 0.50000ml of W3234 + 0.50000ml of PP24806 = Final Quantity: 1.000 ml

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
1080	AR1221 250 PPB STD	PP24829	08/18/2025	02/18/2026	Yogesh Patel	None	None	Abdul Mirza
								08/19/2025

FROM 0.75000ml of W3234 + 0.25000ml of PP24806 = Final Quantity: 1.000 ml

Pest/Pcb STANDARD PREPARATION LOG

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
1081	AR1221 50 PPB STD	PP24830	08/18/2025	02/18/2026	Yogesh Patel	None	None	Abdul Mirza
								08/19/2025

FROM 0.90000ml of W3234 + 0.10000ml of PP24828 = Final Quantity: 1.000 ml

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
1063	AR1232 750 PPB STD	PP24831	08/18/2025	02/18/2026	Yogesh Patel	None	None	Abdul Mirza
								08/19/2025

FROM 0.25000ml of W3234 + 0.75000ml of PP24807 = Final Quantity: 1.000 ml

Pest/Pcb STANDARD PREPARATION LOG

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
223	AR1232 500 PPB STD	PP24832	08/18/2025	02/18/2026	Yogesh Patel	None	None	Abdul Mirza
								08/19/2025

FROM 0.50000ml of W3234 + 0.50000ml of PP24807 = Final Quantity: 1.000 ml

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
1064	AR1232 250 PPB STD	PP24833	08/18/2025	02/18/2026	Yogesh Patel	None	None	Abdul Mirza
								08/19/2025

FROM 0.75000ml of W3234 + 0.25000ml of PP24807 = Final Quantity: 1.000 ml

Pest/Pcb STANDARD PREPARATION LOG

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
1065	AR1232 50 PPB STD	PP24834	08/18/2025	02/18/2026	Yogesh Patel	None	None	Abdul Mirza
								08/19/2025

FROM 0.90000ml of W3234 + 0.10000ml of PP24832 = Final Quantity: 1.000 ml

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
1067	AR1242 750 PPB STD	PP24835	08/18/2025	02/18/2026	Yogesh Patel	None	None	Abdul Mirza
								08/19/2025

FROM 0.25000ml of W3234 + 0.75000ml of PP24808 = Final Quantity: 1.000 ml

Pest/Pcb STANDARD PREPARATION LOG

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
224	AR1242 500 PPB STD	PP24836	08/18/2025	02/18/2026	Yogesh Patel	None	None	Abdul Mirza
								08/19/2025

FROM 0.50000ml of W3234 + 0.50000ml of PP24808 = Final Quantity: 1.000 ml

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
1068	AR1242 250 PPB STD	PP24837	08/18/2025	02/18/2026	Yogesh Patel	None	None	Abdul Mirza
								08/19/2025

FROM 0.75000ml of W3234 + 0.25000ml of PP24808 = Final Quantity: 1.000 ml

Pest/Pcb STANDARD PREPARATION LOG

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
1069	AR1242 50 PPB STD	PP24838	08/18/2025	02/18/2026	Yogesh Patel	None	None	Abdul Mirza
								08/19/2025

FROM 0.90000ml of W3234 + 0.10000ml of PP24836 = Final Quantity: 1.000 ml

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
1075	AR1248 750 PPB STD	PP24839	08/18/2025	02/18/2026	Yogesh Patel	None	None	Abdul Mirza
								08/19/2025

FROM 0.25000ml of W3234 + 0.75000ml of PP24809 = Final Quantity: 1.000 ml

Pest/Pcb STANDARD PREPARATION LOG

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
225	AR1248 500 PPB STD	PP24840	08/18/2025	02/18/2026	Yogesh Patel	None	None	Abdul Mirza
								08/19/2025

FROM 0.50000ml of W3234 + 0.50000ml of PP24809 = Final Quantity: 1.000 ml

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
1076	AR1248 250 PPB STD	PP24841	08/18/2025	02/18/2026	Yogesh Patel	None	None	Abdul Mirza
								08/19/2025

FROM 0.75000ml of W3234 + 0.25000ml of PP24809 = Final Quantity: 1.000 ml

Pest/Pcb STANDARD PREPARATION LOG

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
1077	AR1248 50 PPB STD	PP24842	08/18/2025	02/18/2026	Yogesh Patel	None	None	Abdul Mirza
								08/19/2025

FROM 0.90000ml of W3234 + 0.10000ml of PP24840 = Final Quantity: 1.000 ml

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
1071	AR1254 750 PPB STD	PP24843	08/18/2025	02/18/2026	Yogesh Patel	None	None	Abdul Mirza
								08/19/2025

FROM 0.25000ml of W3234 + 0.75000ml of PP24810 = Final Quantity: 1.000 ml

Pest/Pcb STANDARD PREPARATION LOG

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
226	AR1254 500 PPB STD	PP24844	08/18/2025	02/18/2026	Yogesh Patel	None	None	Abdul Mirza
								08/19/2025

FROM 0.50000ml of W3234 + 0.50000ml of PP24810 = Final Quantity: 1.000 ml

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
1072	AR1254 250 PPB STD	PP24845	08/18/2025	02/18/2026	Yogesh Patel	None	None	Abdul Mirza
								08/19/2025

FROM 0.75000ml of W3234 + 0.25000ml of PP24810 = Final Quantity: 1.000 ml

Pest/Pcb STANDARD PREPARATION LOG

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
1073	AR1254 50 PPB STD	PP24846	08/18/2025	02/18/2026	Yogesh Patel	None	None	Abdul Mirza
								08/19/2025

FROM 0.90000ml of W3234 + 0.10000ml of PP24844 = Final Quantity: 1.000 ml

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
3753	AR1262 750 PPB STD	PP24847	08/18/2025	02/18/2026	Yogesh Patel	None	None	Abdul Mirza
								08/19/2025

FROM 0.25000ml of W3234 + 0.75000ml of PP24811 = Final Quantity: 1.000 ml

Pest/Pcb STANDARD PREPARATION LOG

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
1530	AR1262 500 PPB STD	PP24848	08/18/2025	02/18/2026	Yogesh Patel	None	None	Abdul Mirza
								08/19/2025

FROM 0.50000ml of W3234 + 0.50000ml of PP24811 = Final Quantity: 1.000 ml

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
3754	AR1262 250 PPB STD	PP24849	08/18/2025	02/18/2026	Yogesh Patel	None	None	Abdul Mirza
								08/19/2025

FROM 0.75000ml of W3234 + 0.25000ml of PP24811 = Final Quantity: 1.000 ml

Pest/Pcb STANDARD PREPARATION LOG

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
3755	AR1262 50 PPB STD	PP24850	08/18/2025	02/18/2026	Yogesh Patel	None	None	Abdul Mirza
								08/19/2025

FROM 0.90000ml of W3234 + 0.10000ml of PP24848 = Final Quantity: 1.000 ml

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
3820	AR1268 750 PPB STD	PP24851	08/18/2025	02/18/2026	Yogesh Patel	None	None	Abdul Mirza
								08/19/2025

FROM 0.25000ml of W3234 + 0.75000ml of PP24812 = Final Quantity: 1.000 ml

Pest/Pcb STANDARD PREPARATION LOG

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
1533	AR1268 500 PPB STD	PP24852	08/18/2025	02/18/2026	Yogesh Patel	None	None	Abdul Mirza
								08/19/2025

FROM 0.50000ml of W3234 + 0.50000ml of PP24812 = Final Quantity: 1.000 ml

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
3821	AR1268 250 PPB STD	PP24853	08/18/2025	02/18/2026	Yogesh Patel	None	None	Abdul Mirza
								08/19/2025

FROM 0.75000ml of W3234 + 0.25000ml of PP24812 = Final Quantity: 1.000 ml

Pest/Pcb STANDARD PREPARATION LOG

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
3822	AR1268 50 PPB STD	PP24854	08/18/2025	02/18/2026	Yogesh Patel	None	None	Abdul Mirza
								08/19/2025

FROM 0.90000ml of W3234 + 0.10000ml of PP24852 = Final Quantity: 1.000 ml

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
406	AR1660 500 PPB ICV	PP24855	08/18/2025	02/18/2026	Yogesh Patel	None	None	Abdul Mirza
								08/19/2025

FROM 0.50000ml of W3234 + 0.50000ml of PP24815 = Final Quantity: 1.000 ml

Pest/Pcb STANDARD PREPARATION LOG

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
3790	AR1221 500 PPB ICV(AGILENT)	PP24856	08/18/2025	09/18/2025	Yogesh Patel	None	None	Abdul Mirza
								08/19/2025

FROM 0.50000ml of W3234 + 0.50000ml of PP24816 = Final Quantity: 1.000 ml

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
1888	AR1232 500 PPB ICV	PP24857	08/18/2025	02/18/2026	Yogesh Patel	None	None	Abdul Mirza
								08/19/2025

FROM 0.50000ml of W3234 + 0.50000ml of PP24817 = Final Quantity: 1.000 ml

Pest/Pcb STANDARD PREPARATION LOG

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
1891	AR1242 500 PPB ICV	PP24858	08/18/2025	02/18/2026	Yogesh Patel	None	None	Abdul Mirza
								08/19/2025

FROM 0.50000ml of W3234 + 0.50000ml of PP24818 = Final Quantity: 1.000 ml

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
1892	AR1248 500 PPB ICV	PP24859	08/18/2025	02/18/2026	Yogesh Patel	None	None	Abdul Mirza
								08/19/2025

FROM 0.50000ml of W3234 + 0.50000ml of PP24819 = Final Quantity: 1.000 ml

Pest/Pcb STANDARD PREPARATION LOG

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
1894	AR1254 500 PPB ICV	PP24860	08/18/2025	02/18/2026	Yogesh Patel	None	None	Abdul Mirza
								08/19/2025

FROM 0.50000ml of W3234 + 0.50000ml of PP24381 = Final Quantity: 1.000 ml

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
3758	AR1262 500 PPB STD ICV	PP24861	08/18/2025	02/18/2026	Yogesh Patel	None	None	Abdul Mirza
								08/19/2025

FROM 0.50000ml of W3234 + 0.50000ml of PP24821 = Final Quantity: 1.000 ml

Pest/Pcb STANDARD PREPARATION LOG

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
3823	AR1268 500 PPB STD ICV	PP24862	08/18/2025	09/18/2025	Yogesh Patel	None	None	Abdul Mirza
								08/19/2025

FROM 0.50000ml of W3234 + 0.50000ml of PP24822 = Final Quantity: 1.000 ml

CHEMICAL RECEIPT LOG BOOK

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
Seidler Chemical	9005-05 / Acetone Ultra (cs/4x4L)	24E0761004	02/18/2026	10/01/2024 / Rajesh	09/25/2024 / Rajesh	E3804

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
PCI Scientific Supply, Inc.	PC19631-100 / SODIUM SULFATE, ANHYDROUS, PEST GRADE, 1	417203	01/28/2026	07/28/2025 / RUPESH	01/29/2025 / Rajesh	E3875

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
Seidler Chemical	BA-9254-03 / Acetone, Ultra Resi (cs/4x4L)	24H1462005	05/24/2027	06/20/2025 / RUPESH	05/14/2025 / RUPESH	E3944

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
Seidler Chemical	BA-9254-03 / Acetone, Ultra Resi (cs/4x4L)	24H2762008	04/18/2027	07/08/2025 / RITESHKUMAR	07/03/2025 / RUPESH	E3949

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
Seidler Chemical	BA-9262-03 / Hexane, Ultra-Resi (cs/4x4L)	25C0362005	04/30/2026	07/08/2025 / RITESHKUMAR	07/03/2025 / RUPESH	E3950

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
Seidler Chemical	BA-3382-05 / Sand, Purified (cs/4x2.5kg)	25A2756718	12/31/2028	07/09/2025 / RUPESH	04/28/2020 / RUPESH	E3951

CHEMICAL RECEIPT LOG BOOK

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
Seidler Chemical	BA-9254-03 / Acetone, Ultra Resi (cs/4x4L)	24H2762008	04/18/2027	07/16/2025 / RUPESH	07/16/2025 / RUPESH	E3955

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
Seidler Chemical	BA-9262-03 / Hexane, Ultra-Resi (cs/4x4L)	25C0362005	04/30/2026	08/05/2025 / RUPESH	07/30/2025 / RUPESH	E3962

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
Seidler Chemical	BA-9254-03 / Acetone, Ultra Resi (cs/4x4L)	24H2762008	02/15/2026	08/15/2025 / RUPESH	08/07/2025 / RUPESH	E3963

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
Seidler Chemical	BA-9673-33 / Sulfuric Acid, Instra-Analyzed (cs/6c2.5L)	24i1262013	11/07/2025	05/07/2025 / RUPESH	02/18/2025 / Mohan	M6157

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
Agilent Technologies	PP-382-1 / Aroclor 1268	0006587800	09/18/2025	03/18/2025 / yogesh	02/21/2022 / Ankita	P11522

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
Restek	32011 / PCB Mix, Aroclor 1254, 1000ug/mL, Hexane, 1mL/ampul	A0175403	02/18/2026	08/18/2025 / yogesh	03/18/2022 / Abdul	P11592

CHEMICAL RECEIPT LOG BOOK

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
Absolute Standards, Inc	91867 / Aroclor 1232 100 ug/mL	020823	02/18/2026	08/18/2025 / yogesh	08/07/2023 / Ankita	P12700

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
Absolute Standards, Inc	x9166 / Aroclor 1262 100 ug/mL	060523	02/18/2026	08/18/2025 / yogesh	08/07/2023 / Ankita	P12703

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
Absolute Standards, Inc.	20064 / Aroclor 1016/1260	022023	02/12/2026	08/12/2025 / Abdul	12/20/2023 / Yogesh	P12951

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
Absolute Standards, Inc.	20064 / Aroclor 1016/1260	022023	02/18/2026	08/18/2025 / yogesh	12/20/2023 / Yogesh	P12952

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
Absolute Standards, Inc.	/ Arochlor 1254	121823	04/03/2025	10/03/2024 / Ankita	12/20/2023 / Yogesh	P12957

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
Restek	32000 / Pesticide Mix, CLP method, Pesticide Surrogate Mix, 200ug/mL, Acetone, 1mL	A0206810	09/18/2025	03/18/2025 / yogesh	04/22/2024 / Abdul	P13356

CHEMICAL RECEIPT LOG BOOK

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
Agilent Technologies	PP-292-1 / Aroclor 1221	0006783205	09/18/2025	03/18/2025 / yogesh	05/02/2024 / Ankita	P13373

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
Restek	32007 / PCB Mix, Aroclor 1221, 1000ug/mL, Hexane, 1mL/ampul	A0207511	02/18/2026	08/18/2025 / yogesh	05/03/2024 / Abdul	P13375

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
Agilent Technologies	PP-312-1 / Aroclor 1242	0006665550	02/18/2026	08/18/2025 / yogesh	10/14/2024 / Ankita	P13590

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
Agilent Technologies	PP-342-1 / Aroclor 1248	0006726317	02/18/2026	08/18/2025 / yogesh	10/14/2024 / Ankita	P13592

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
Restek	32010 / PCB Mix, Aroclor 1248, 1000ug/mL, Hexane, 1mL/ampul	A0214733	02/18/2026	08/18/2025 / yogesh	10/17/2024 / yogesh	P13695

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
Restek	32039 / PCB Mix, Aroclor 1016/1260, 1000ug/mL, hexane, 1mL/ampul	A0210629	09/18/2025	03/18/2025 / yogesh	10/17/2024 / yogesh	P13697

CHEMICAL RECEIPT LOG BOOK

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
Restek	32009 / PCB Mix, Aroclor 1242, 1000ug/mL, Hexane, 1mL/ampul	A0210232	02/18/2026	08/18/2025 / yogesh	10/17/2024 / yogesh	P13706

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
Restek	32000 / Pesticide Mix, CLP method, Pesticide Surrogate Mix, 200ug/mL, Acetone, 1mL	A0214495	12/24/2025	06/24/2025 / Abdul	11/19/2024 / Ankita	P13786

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
Restek	32000 / Pesticide Mix, CLP method, Pesticide Surrogate Mix, 200ug/mL, Acetone, 1mL	A0214495	02/18/2026	08/18/2025 / yogesh	11/19/2024 / Ankita	P13789

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
Restek	32011 / PCB Mix, Aroclor 1254, 1000ug/mL, Hexane, 1mL/ampul	a0217391	02/18/2026	08/18/2025 / yogesh	12/09/2024 / Ankita	P13833

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
Restek	32008 / PCB Mix, Aroclor 1232, 1000ug/mL, Hexane, 1mL/ampul	A0219655	02/18/2026	08/18/2025 / yogesh	01/23/2025 / Ankita	P13879

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
Restek	32409 / PCB Stock Solution, Aroclor 1262 Std, 1mL, Hexane	A0217041	02/18/2026	08/18/2025 / yogesh	01/23/2025 / Ankita	P13881

CHEMICAL RECEIPT LOG BOOK

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
Restek	32410 / PCB Stock Solution, Aroclor 1268 Std, 1mL, Hexane	A0217264	02/18/2026	08/18/2025 / yogesh	01/23/2025 / Ankita	P13885

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
Absolute Standards, Inc	/ CLP pesticide surrogate standard	051209	05/12/2014	07/23/2010 / rpatel	07/29/2009 / rpatel	P2287

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
Seidler Chemical	DIW / DI Water	Daily Lab-Certified	07/03/2029	07/03/2024 / lwona	07/03/2024 / lwona	W3112

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
Seidler Chemical	BA-9262-03 / Hexane, Ultra-Resi (cs/4x4L)	24G1962003	08/22/2025	02/03/2025 / jignesh	01/31/2025 / jignesh	W3177

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
Seidler Chemical	BA-9262-03 / Hexane, Ultra-Resi (cs/4x4L)	25C0362005	04/30/2026	07/28/2025 / jignesh	07/25/2025 / jignesh	W3234

Material No.: 9005-05
Batch No.: 24E0761004
Manufactured Date: 2024-05-02
Retest Date: 2029-05-01
Revision No.: 0

Certificate of Analysis

Test	Specification	Result
Assay ((CH ₃) ₂ CO) (by GC, corrected for water)	≥ 99.5 %	99.8 %
Color (APHA)	≤ 10	< 5
Residue after Evaporation	≤ 5 ppm	< 1 ppm
Titration Acid (μeq/g)	≤ 0.3	0.1
Titration Base (μeq/g)	≤ 0.5	0.1
Water (H ₂ O)	≤ 0.5 %	0.1 %
Solubility in H ₂ O	Passes Test	Passes Test
Chloride (Cl)	≤ 0.2 ppm	< 0.2 ppm
Phosphate (PO ₄)	≤ 0.05 ppm	< 0.05 ppm
Trace Impurities – Aluminum (Al)	≤ 50.0 ppb	< 5.0 ppb
Arsenic and Antimony (as As)	≤ 5.0 ppb	< 5.0 ppb
Trace Impurities – Barium (Ba)	≤ 20.0 ppb	< 1.0 ppb
Trace Impurities – Beryllium (Be)	≤ 10.0 ppb	< 1.0 ppb
Trace Impurities – Bismuth (Bi)	≤ 20.0 ppb	< 10.0 ppb
Trace Impurities – Boron (B)	≤ 10.0 ppb	< 5.0 ppb
Trace Impurities – Cadmium (Cd)	≤ 10.0 ppb	< 1.0 ppb
Trace Impurities – Calcium (Ca)	≤ 25.0 ppb	3.6 ppb
Trace Impurities – Chromium (Cr)	≤ 10.0 ppb	< 1.0 ppb
Trace Impurities – Cobalt (Co)	≤ 10.0 ppb	< 1.0 ppb
Trace Impurities – Copper (Cu)	≤ 10.0 ppb	< 1.0 ppb
Trace Impurities – Gallium (Ga)	≤ 10.0 ppb	< 1.0 ppb
Trace Impurities – Germanium (Ge)	≤ 10.0 ppb	< 10.0 ppb
Trace Impurities – Gold (Au)	≤ 20 ppb	< 5 ppb
Trace Impurities – Iron (Fe)	≤ 20.0 ppb	< 1.0 ppb
Trace Impurities – Lead (Pb)	≤ 10.0 ppb	< 10.0 ppb
Trace Impurities – Lithium (Li)	≤ 10.0 ppb	< 1.0 ppb
Trace Impurities – Magnesium (Mg)	≤ 20 ppb	< 1 ppb
Trace Impurities – Manganese (Mn)	≤ 10.0 ppb	< 1.0 ppb

Recd by RP on 9/25/24

E 3804

>>> Continued on page 2 >>>

Acetone
CMOS

 **avantor™**



Material No.: 9005-05
Batch No.: 24E0761004

Test	Specification	Result
Trace Impurities – Molybdenum (Mo)	≤ 10.0 ppb	< 5.0 ppb
Trace Impurities – Nickel (Ni)	≤ 10.0 ppb	< 5.0 ppb
Trace Impurities – Niobium (Nb)	≤ 50.0 ppb	< 1.0 ppb
Trace Impurities – Potassium (K)	≤ 10.0 ppb	< 10.0 ppb
Trace Impurities – Silicon (Si)	≤ 50 ppb	< 10 ppb
Trace Impurities – Silver (Ag)	≤ 10.0 ppb	< 1.0 ppb
Trace Impurities – Sodium (Na)	≤ 10.0 ppb	< 1.0 ppb
Trace Impurities – Strontium (Sr)	≤ 10.0 ppb	< 1.0 ppb
Trace Impurities – Tantalum (Ta)	≤ 50.0 ppb	< 5.0 ppb
Trace Impurities – Thallium (Tl)	≤ 10.0 ppb	< 5.0 ppb
Trace Impurities – Tin (Sn)	≤ 20.0 ppb	< 10.0 ppb
Trace Impurities – Titanium (Ti)	≤ 10.0 ppb	< 1.0 ppb
Trace Impurities – Vanadium (V)	≤ 10.0 ppb	< 1.0 ppb
Trace Impurities – Zinc (Zn)	≤ 20.0 ppb	7.9 ppb
Trace Impurities – Zirconium (Zr)	≤ 10.0 ppb	< 1.0 ppb
Particle Count – 0.5 µm and greater (Rion KS42AF)	≤ 100 par/ml	8 par/ml
Particle Count – 1.0 µm and greater (Rion KS42AF)	≤ 8 par/ml	2 par/ml

>>> Continued on page 3 >>>

Acetone
CMOS

 **avantor™**



Material No.: 9005-05
Batch No.: 24E0761004

Test	Specification	Result

For Microelectronic Use

Country of Origin: USA
Packaging Site: Paris Mfg Ctr & DC



Michelle Bales
Sr. Manager, Quality Assurance



**PRODUCTOS
QUÍMICOS
MONTERREY, S.A. DE C.V.**

MIRADOR 201, COL. MIRADOR
MONTERREY, N.L. MÉXICO
CP 64070
TEL +52 81 13 52 67 67
www.pqm.com.mx

CERTIFICATE OF ANALYSIS

PRODUCT :	SODIUM SULFATE CRYSTALS ANHYDROUS		
QUALITY :	ACS (CODE RMB3375)	FORMULA :	Na ₂ SO ₄
SPECIFICATION NUMBER:	6399	RELEASE DATE:	MAY/23/2024
LOT NUMBER :	417203		

TEST	SPECIFICATIONS	LOT VALUES
Assay (Na ₂ SO ₄)	Min. 99.0%	99.8 %
pH of a 5% solution at 25°C	5.2 - 9.2	6.2
Insoluble matter	Max. 0.01%	0.001 %
Loss on ignition	Max. 0.5%	0.1 %
Chloride (Cl)	Max. 0.001%	<0.001 %
Nitrogen compounds (as N)	Max. 5 ppm	<5 ppm
Phosphate (PO ₄)	Max. 0.001%	<0.001 %
Heavy metals (as Pb)	Max. 5 ppm	<5 ppm
Iron (Fe)	Max. 0.001%	<0.001 %
Calcium (Ca)	Max. 0.01%	0.001 %
Magnesium (Mg)	Max. 0.005%	0.001 %
Potassium (K)	Max. 0.008%	0.001 %
Extraction-concentration suitability	Passes test	Passes test
Appearance	Passes test	Passes test
Identification	Passes test	Passes test
Solubility and foreign matter	Passes test	Passes test
Retained on US Standard No. 10 sieve	Max. 1%	0.2 %
Retained on US Standard No. 60 sieve	Min. 94%	96.2 %
Through US Standard No. 60 sieve	Max. 5%	3.5 %
Through US Standard No. 100 sieve	Max. 10%	0.1 %

COMMENTS

QC: PhC Irma Belmares

If you need further details, please call our factory or contact our local distributor.

RE-02-01, Ed. 3

E 3875

Acetone
BAKER RESI-ANALYZED® Reagent
For Organic Residue Analysis

Avantor™



Material No.: 9254-03

Batch No.: 24H1462005

Manufactured Date: 2024-05-24

Expiration Date: 2027-05-24

Revision No.: 0

Certificate of Analysis

Test	Specification	Result
Assay ((CH ₃) ₂ CO) (by GC, corrected for water)	>= 99.4 %	99.8 %
Color (APHA)	<= 10	5
Residue after Evaporation	<= 1.0 ppm	0.2 ppm
Substances Reducing Permanganate	Passes Test	Passes Test
Titration Acid (μeq/g)	<= 0.3	0.2
Titration Base (μeq/g)	<= 0.6	<0.1
Water (H ₂ O)	<= 0.5 %	0.2 %
FID-Sensitive Impurities (as 2-Octanol) Single Impurity Peak (ng/mL)	<= 5	<1
ECD Sensitive Impurities (as Heptachlor Epoxide) Single Peak (pg/mL)	<= 10	1

For Laboratory, Research, or Manufacturing Use
MEETS SPECIFICATIONS WITHIN THE EXPIRATION PERIOD

Country of Origin: United States
Packaging Site: Phillipsburg Mfg Ctr & DC

E3944

Jamie Croak
Director Quality Operations, Bioscience Production

For questions on this Certificate of Analysis please contact Technical Services at 855.282.6867 or +1.610.386.1700

Avantor Performance Materials LLC

Acetone

BAKER RESI-ANALYZED® Reagent
For Organic Residue Analysis

Avantor™



Material No.: 9254-03

Batch No.: 24H2762008

Manufactured Date: 2024-04-18

Expiration Date: 2027-04-18

Revision No.: 0

Certificate of Analysis

Test	Specification	Result
Assay ((CH ₃) ₂ CO) (by GC, corrected for water)	>= 99.4 %	100.0 %
Color (APHA)	<= 10	5
Residue after Evaporation	<= 1.0 ppm	0.0 ppm
Substances Reducing Permanganate	Passes Test	Passes Test
Titration Acid (µeq/g)	<= 0.3	0.2
Titration Base (µeq/g)	<= 0.6	<0.1
Water (H ₂ O)	<= 0.5 %	<0.1 %
FID-Sensitive Impurities (as 2-Octanol) Single Impurity Peak (ng/mL)	<= 5	1
ECD Sensitive Impurities (as Heptachlor Epoxide) Single Peak (pg/mL)	<= 10	1

For Laboratory, Research, or Manufacturing Use

MEETS SPECIFICATIONS WITHIN THE EXPIRATION PERIOD

Country of Origin: United States

Packaging Site: Phillipsburg Mfg Ctr & DC

Reel on 7/2/25

E3949

J. Croak

Jamie Croak

Director Quality Operations, Bioscience Production

For questions on this Certificate of Analysis please contact Technical Services at 855.282.6867 or +1.610.386.1700

Avantor Performance Materials LLC

n-Hexane 95%
ULTRA RESI-ANALYZED
For Organic Residue Analysis



Material No.: 9262-03

Batch No.: 25C0362005

Manufactured Date: 2025-01-29

Expiration Date: 2026-04-30

Revision No.: 0

Certificate of Analysis

Test	Specification	Result
FID-Sensitive Impurities (as 2-Octanol) Single Impurity Peak (ng/mL)	≤ 5	1
ECD Sensitive Impurities (as Heptachlor Epoxide) Single Peak (pg/mL)	≤ 10	6
ECD-Sensitive Impurities (as Ethylene Dibromide) - Single Impurity Peak (ng/mL)	≤ 5	5
Assay (Total Saturated C ₆ Isomers) (by GC, corrected for water)	$\geq 99.5 \%$	100.0 %
Assay (as n-Hexane) (by GC, corrected for water)	$\geq 95 \%$	100 %
Color (APHA)	≤ 10	10
Residue after Evaporation	≤ 1.0 ppm	0.1 ppm
Substances Darkened by H ₂ SO ₄	Passes Test	Passes Test
Water (by KF, coulometric)	$\leq 0.05 \%$	$< 0.01 \%$

For Laboratory, Research, or Manufacturing Use

MEETS SPECIFICATIONS WITHIN THE EXPIRATION PERIOD

Country of Origin: United States

Packaging Site: Phillipsburg Mfg Ctr & DC

3950

Recd on 7/02/25

Jamie Croak
Director Quality Operations, Bioscience Production



Material	BDH9274-2.5KG
Material Description	BDH SAND STDD OTTAWA W+I 2.5KG
Grade	NOT APPLICABLE
Batch	25A2756718
Reassay Date	12/31/2028
CAS Number	14808-60-7
Molecular Formula	SiO ₂
Molecular Mass	60.09
Date of Manufacture	12/05/2024
Storage	Room Temperature

Characteristics	Specifications	Measured Values
Appearance	Beige granules.	Beige granules.
Moisture	<= 0.1 %	0.1 %
Particle Size 30-40 mesh	>= 80 %	99 %
CUSTOMER PART # BDH9274-2.5KG		

Received on 1/12/25.

E3951

Internal ID #: 793

Signature	Additional Information
We certify that this batch conforms to the specifications listed above. This document has been electronically produced and is valid without a signature. Leona Edwardson, Quality Control Sr. Manager - Solon VWR Chemicals, LLC. 28600 Fountain Parkway, Solon OH 44139 USA	Analysis may have been rounded to significant digits in specification limits Product meets analytical specifications of the grades listed.

Acetone
BAKER RESI-ANALYZED® Reagent
For Organic Residue Analysis



Material No.: 9254-03
Batch No.: 24H2762008
Manufactured Date: 2024-04-18
Expiration Date: 2027-04-18
Revision No.: 0

Certificate of Analysis

Test	Specification	Result
Assay ((CH ₃) ₂ CO) (by GC, corrected for water)	>= 99.4 %	100.0 %
Color (APHA)	<= 10	5
Residue after Evaporation	<= 1.0 ppm	0.0 ppm
Substances Reducing Permanganate	Passes Test	Passes Test
Titration Acid (µeq/g)	<= 0.3	0.2
Titration Base (µeq/g)	<= 0.6	<0.1
Water (H ₂ O)	<= 0.5 %	<0.1 %
FID-Sensitive Impurities (as 2-Octanol) Single Impurity Peak (ng/mL)	<= 5	1
ECD Sensitive Impurities (as Heptachlor Epoxide) Single Peak (pg/mL)	<= 10	1

For Laboratory, Research, or Manufacturing Use
MEETS SPECIFICATIONS WITHIN THE EXPIRATION PERIOD

Country of Origin: United States
Packaging Site: Phillipsburg Mfg Ctr & DC

Received on 7/16/25

E 3955

Jamie Croak
Director Quality Operations, Bioscience Production

For questions on this Certificate of Analysis please contact Technical Services at 855.282.6867 or +1.610.386.1700

Avantor Performance Materials, LLC

100 Matsonford Rd, Suite 200, Radnor, PA, 19087, U.S.A. Phone 610.386.1700

n-Hexane 95%
ULTRA RESI-ANALYZED
For Organic Residue Analysis



Material No.: 9262-03
Batch No.: 25C0362005
Manufactured Date: 2025-01-29
Expiration Date: 2026-04-30
Revision No.: 0

Certificate of Analysis

Test	Specification	Result
FID-Sensitive Impurities (as 2-Octanol) Single Impurity Peak (ng/mL)	≤ 5	1
ECD Sensitive Impurities (as HeptachlorEpoxide) Single Peak (pg/mL)	≤ 10	6
ECD-Sensitive Impurities (as EthyleneDibromide) - Single Impurity Peak (ng/mL)	≤ 5	5
Assay (Total Saturated C ₆ Isomers) (by GC, corrected for water)	$\geq 99.5 \%$	100.0 %
Assay (as n-Hexane) (by GC, corrected for water)	$\geq 95 \%$	100 %
Color (APHA)	≤ 10	10
Residue after Evaporation	≤ 1.0 ppm	0.1 ppm
Substances Darkened by H ₂ SO ₄	Passes Test	Passes Test
Water (by KF, coulometric)	$\leq 0.05 \%$	$< 0.01 \%$

For Laboratory, Research, or Manufacturing Use
MEETS SPECIFICATIONS WITHIN THE EXPIRATION PERIOD

Country of Origin: United States
Packaging Site: Phillipsburg Mfg Ctr & DC

Received on 7/30/25

E3962

Jamie Croak
Director Quality Operations, Bioscience Production

Acetone.
BAKER RESI-ANALYZED® Reagent
For Organic Residue Analysis

Avantor™



Material No.: 9254-03
Batch No.: 24H2762008
Manufactured Date: 2024-04-18
Expiration Date: 2027-04-18
Revision No.: 0

Certificate of Analysis

Test	Specification	Result
Assay ((CH ₃) ₂ CO) (by GC, corrected for water)	>= 99.4 %	100.0 %
Color (APHA)	<= 10	5
Residue after Evaporation	<= 1.0 ppm	0.0 ppm
Substances Reducing Permanganate	Passes Test	Passes Test
Titration Acid (μeq/g)	<= 0.3	0.2
Titration Base (μeq/g)	<= 0.6	<0.1
Water (H ₂ O)	<= 0.5 %	<0.1 %
FID-Sensitive Impurities (as 2-Octanol) Single Impurity Peak (ng/mL)	<= 5	1
ECD Sensitive Impurities (as Heptachlor Epoxide) Single Peak (pg/mL)	<= 10	1

For Laboratory, Research, or Manufacturing Use
MEETS SPECIFICATIONS WITHIN THE EXPIRATION PERIOD

Country of Origin: United States
Packaging Site: Phillipsburg Mfg Ctr & DC

Received on 8/6/25

E 3963

J. Croak

Jamie Croak
Director Quality Operations, Bioscience Production

For questions on this Certificate of Analysis please contact Technical Services at 855.282.6867 or +1.610.386.1700

Avantor Performance Materials, LLC

100 Matsonford Rd, Suite 200, Radnor, PA, 19087, U.S.A. Phone 610.386.1700

Sulfuric Acid
BAKER INSTRA-ANALYZED® Reagent
For Trace Metal Analysis
Low Selenium

avantor™



MG157
MS

Material No.: 9673-33

Batch No.: 24I1262013

Manufactured Date: 2024-08-07

Retest Date: 2029-08-06

Revision No.: 0

Certificate of Analysis

Test	Specification	Result
ACS – Assay (H ₂ SO ₄)	95.0 – 98.0 %	96.2 %
Appearance	Passes Test	Passes Test
ACS – Color (APHA)	<= 10	5
ACS – Residue after Ignition	<= 3 ppm	<1 ppm
ACS – Substances Reducing Permanganate(as SO ₂)	<= 2 ppm	<2 ppm
Ammonium (NH ₄)	<= 1 ppm	<1 ppm
Chloride (Cl)	<= 0.1 ppm	<0.1 ppm
Nitrate (NO ₃)	<= 0.2 ppm	0.1 ppm
Phosphate (PO ₄)	<= 0.5 ppm	<0.1 ppm
Trace Impurities – Aluminum (Al)	<= 30.0 ppb	<5.0 ppb
Arsenic & Antimony (as As)	<= 4.0 ppb	<2.0 ppb
Trace Impurities – Boron (B)	<= 10.0 ppb	<5.0 ppb
Trace Impurities – Cadmium (Cd)	<= 2.0 ppb	<1.0 ppb
Trace Impurities – Chromium (Cr)	<= 6.0 ppb	<1.0 ppb
Trace Impurities – Cobalt (Co)	<= 0.5 ppb	<0.3 ppb
Trace Impurities – Copper (Cu)	<= 1.0 ppb	<1.0 ppb
Trace Impurities – Gold (Au)	<= 10.0 ppb	<5.0 ppb
Heavy Metals (as Pb)	<= 500.0 ppb	<100.0 ppb
Trace Impurities – Iron (Fe)	<= 50.0 ppb	<1.0 ppb
Trace Impurities – Lead (Pb)	<= 0.5 ppb	<0.5 ppb
Trace Impurities – Magnesium (Mg)	<= 7.0 ppb	<1.0 ppb
Trace Impurities – Manganese (Mn)	<= 1.0 ppb	<1.0 ppb
Trace Impurities – Mercury (Hg)	<= 0.5 ppb	<0.1 ppb
Trace Impurities – Nickel (Ni)	<= 2.0 ppb	<0.3 ppb
Trace Impurities – Potassium (K)	<= 500.0 ppb	<10.0 ppb
Trace Impurities – Selenium (Se)	<= 50.0 ppb	7.2 ppb
Trace Impurities – Silicon (Si)	<= 100.0 ppb	12.8 ppb
Trace Impurities – Silver (Ag)	<= 1.0 ppb	<1.0 ppb

For questions on this Certificate of Analysis please contact Technical Services at 855.282.6867 or +1.610.386.1700

Avantor Performance Materials LLC

Sulfuric Acid

BAKER INSTRA-ANALYZED® Reagent

For Trace Metal Analysis

Low Selenium

 **avantors**™



Material No.: 9673-33

Batch No.: 2411262013

Test	Specification	Result
Trace Impurities – Sodium (Na)	≤ 500.0 ppb	< 5.0 ppb
Trace Impurities – Strontium (Sr)	≤ 5.0 ppb	< 1.0 ppb
Trace Impurities – Tin (Sn)	≤ 5.0 ppb	1.1 ppb
Trace Impurities – Zinc (Zn)	≤ 5.0 ppb	< 1.0 ppb

For Laboratory, Research, or Manufacturing Use

Country of Origin: United States

Packaging Site: Phillipsburg Mfg Ctr & DC



Jamie Croak

Director Quality Operations, Bioscience Production

For questions on this Certificate of Analysis please contact Technical Services at 855.282.6867 or +1.610.386.1700

Avantor Performance Materials LLC



Certificate of Analysis

P11518
↓
P11522
AJ
02/21/22

Product Name: Aroclor 1268 Standard

Product Number: PP-382-1

Lot Issue Date: 09-Feb-2021

Lot Number: 0006587800

Expiration Date: 31-Mar-2029

Description:

This analytical reference material (RM) was manufactured and verified in accordance with an ISO 9001 registered quality system and analyte concentrations were verified by an ISO 17025 accredited laboratory. The concentration and uncertainty value at the 95% confidence level for each analyte, determined gravimetrically, is listed below.

Analyte	CAS#	Analyte Lot	Concentration ± Uncertainty
Aroclor 1268	011100-14-4	RM00937	100.0 ± 0.5 µg/mL

Matrix: isooctane (2,2,4-trimethylpentane)

Storage Conditions: Store at Room Temperature (15° to 30°C).

Traceability:

The balances used for these measurements are calibrated with weights traceable to NIST in compliance with ANSI/NCSL Z540.3, ISO 9001, ISO 17025, and ISO 17034. Calibrated Class A glassware is used for volumetric measurements. Thermometers are calibrated against a NIST traceable thermometer in accordance with NIST Special Publication 1088.

Homogeneity:

This RM was unitized according to an in-house procedure and is guaranteed to be homogeneous. There is no minimum sub-sample size required.

Intended Use:

This RM is intended for the preparation of working reference samples for use in routine laboratory analyses, calibration of instruments, validation of analytical methods, assessments of measurement methods, and continuing calibration verification.

Instructions for Use:

Sample aliquots for analysis should be withdrawn at 20°C to 25°C immediately after opening the container and should be processed without delay for the certified values to be valid within the stated uncertainties.

Hazards:

Refer to the Safety Data Sheet on www.agilent.com for information regarding this RM.


Expiration of Certification:

The certification of this RM is valid until the expiration date specified above, provided the RM is handled and stored in accordance with the instructions given in this certificate. This certification is nullified if the RM is damaged, contaminated, or otherwise modified.

Maintenance of Certification:

If substantive changes are noted that affect the certification before the expiration of this certificate, Agilent will notify the purchaser.

Sample lot approver:


Monica Bourgeois
QMS Representative



ISO 17034 Cert
No. AR-1936

RM was produced in accordance with TUV USA Inc registered ISO 9001 Quality Management System. Cert # 56 100 18560026
Page: 1 of 1

www.agilent.com/quality/
CSD-QA-015.1



ISO 17025 Cert
No. AT-1937



CERTIFIED REFERENCE MATERIAL

110 Benner Circle
Bellefonte, PA 16823-8812
Tel: (800)356-1688
Fax: (814)353-1309

www.restek.com

Certificate of Analysis



FOR LABORATORY USE ONLY-READ SDS PRIOR TO USE.

This Reference Material is intended for Laboratory Use Only as a standard for the qualitative and/or quantitative determination of the analyte(s) listed.

Catalog No. : 32011 Lot No.: A0175403
Description : Aroclor® 1254 Standard
Aroclor® 1254 Standard 1,000 µg/mL, Hexane, 1mL/ampul
Container Size : 2 mL Pkg Amt: > 1 mL
Expiration Date : November 30, 2027 Storage: 25°C nominal
Handling: This product contains PCBs. Ship: Ambient

CERTIFIED VALUES

Elution Order	Compound	Grav. Conc. (weight/volume)	Expanded Uncertainty (95% C.L.; K=2)
1	Aroclor 1254 CAS # 11097-69-1 (Lot 124-191-B) Purity ----%	1,000.7 µg/mL	+/- 5.9437 µg/mL Gravimetric +/- 31.7284 µg/mL Unstressed +/- 41.4406 µg/mL Stressed

Solvent: Hexane
CAS # 110-54-3
Purity 99%

P11588
↓
P11592 / (S)

AR
04/30/2022

Column:

30m x .25mm x .2um
Rtx-CLP II (cat.# 11323)

Carrier Gas:

helium-constant pressure 20 psi.

Temp. Program:

200°C to 300°C
@ 25°C/min. (hold 10 min.)

Inj. Temp:


250°C

Det. Temp:

300°C

Det. Type:

ECD

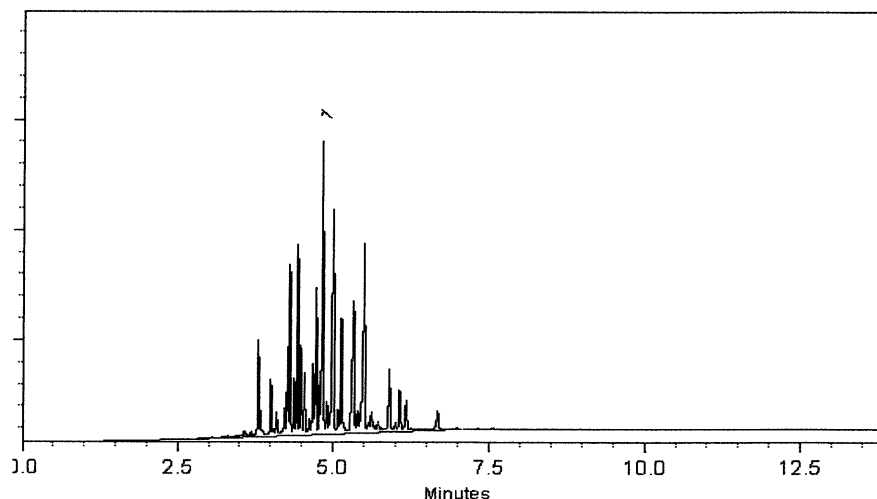

This chromatogram represents a general set of testing conditions chosen for product acceptance. For optimal results in your lab, conditions should be adjusted for your specific instrument, method, and application.

Cathleen Soltis

Cathleen Soltis - Mix Technician

Date Mixed: 15-Aug-2021

Balance: 1128360905

Alexis Shelow

Alexis Shelow - Operations Tech I

Date Passed: 17-Aug-2021

Manufactured under Restek's ISO 9001:2015
Registered Quality System
Certificate #FM 80397

P11588
↓
P11592 / (5)

AR
04/30/22



CERTIFIED WEIGHT REPORT

Part Number: **91867**
 Lot Number: **020823**
 Description: **WP 037 - Aroclor 1232**
PCB Technical Mixture
 Expiration Date: **020833**
 Recommended Storage: **Ambient (20 °C)**
 Nominal Concentration ($\mu\text{g/mL}$): **100**
 NIST Test ID#: **6UTB**

Solvent(
Aceton


Weight(s) shown below were combined and diluted to (mL): **100.0**
 5E-05 Balance Uncertainty
 0.057 Flask Uncertainty

Compound	RM#	Lot Number	Nominal Conc ($\mu\text{g/mL}$)	Purity (%)	Uncertainty Purity	Target Weight (g)
1. Aroclor 1232	17	45-6A	100	100	0.5	0.01000

- The certified value is the concentration calculated from gravimetric and volumetric measurements unless otherwise stated.
- Standards are prepared gravimetrically using balances that are calibrated with weights traceable to NIST (see above).
- Standards are certified (+/-) 0.5% of the stated value, unless otherwise stated.
- All Standards, after opening ampule, should be stored with caps tight and under appropriate laboratory conditions.
- Uncertainty Reference: Taylor, B.N. and Kuyat, C.E., "Guidelines for Evaluating and Expressing the Uncertainty of NIST Measure Technical Note 1297, U.S. Government Printing Office, Washington, DC, (1994).

Comments

GC3-M1 Analysis by Melissa Stonier
 Column ID SPB-608 30 meter X 0.53mm X 5 μm film thickness
 Flow rates: Helium (carrier) = 5mL/min, Helium (make-up) = 25mL/min
 Hydrogen (make-up) = 30mL/min, Air (make-up) = 350mL/min
 Oven Profile: Temp 1 = 150°C (Time 1 = 4 min), Temp 2 = 290°C (Time 2 = 13.5 min)
 Rate = 8°C/min, Total run time = 35 min
 Injector temp. = 200°C, FID Temp. = 300°C. FID Signal = Edaq Channel 1
 Standard injection = 1.5 μL , Range=3

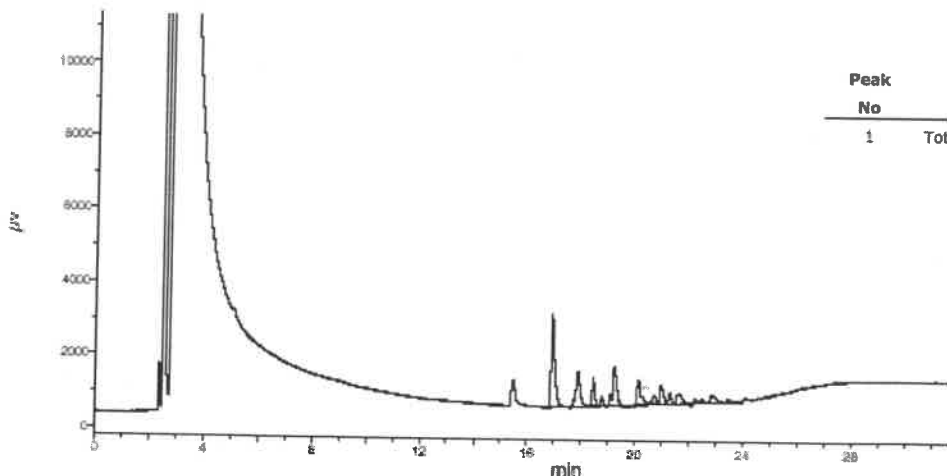



CERTIFIED WEIGHT REPORT

Part Number: X9166
Lot Number: 060523
Description: Aroclor 1262

Solvent(s):
Methanol

Appendix IX Compound

Expiration Date: 060533

Recommended Storage: Ambient (20 °C)

Nominal Concentration (µg/mL): 100


NIST Test ID#: 6UTB

5E-05 Balance Uncertainty

Volume(s) shown below were combined and diluted to (mL): 20.0 0.002 Flask Uncertainty

Compound	Part Number	Lot Number	Dil. Factor	Initial Vol. (mL)	Uncertainty Pipette (mL)	Co
1. Aroclor 1262	70444	080322	0.10	2.00	0.017	

Method GC7MSD-7.M: Column:(30m X 0.25mm ID X 0.25µm film thickn min.), Rate = 8°C/min., Injector B= 200°C, Detector B = 290°C.

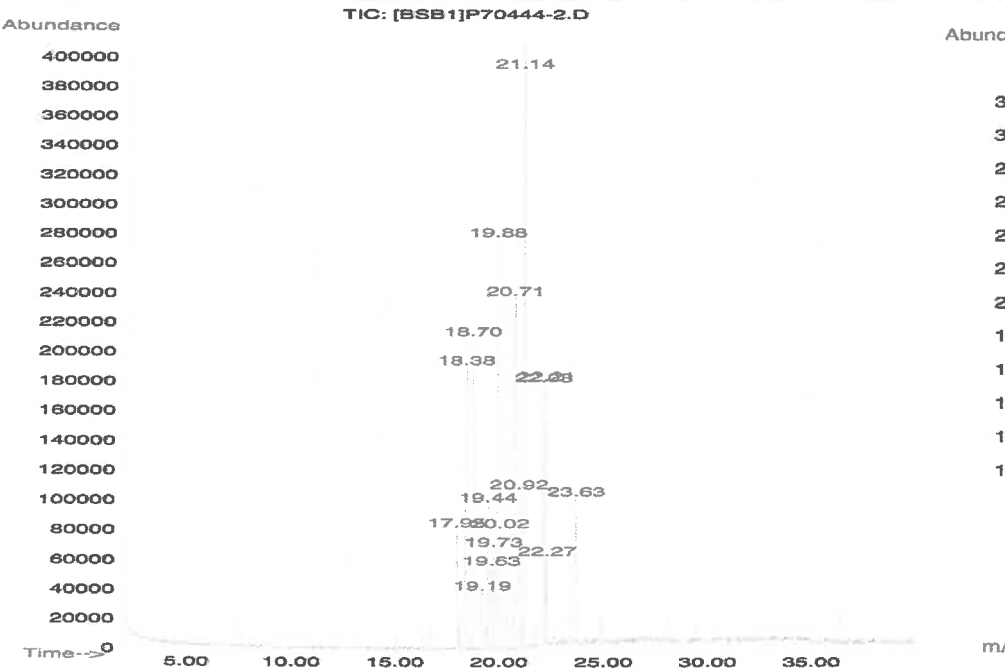

- The certified value is the concentration calculated from gravimetric and volumetric me
- Standards are prepared gravimetrically using balances that are calibrated with weight
- Standards are certified (+/-) 0.5% of the stated value, unless otherwise stated.
- All Standards, after opening ampule, should be stored with caps tight and under appro
- Uncertainty Reference: Taylor, B.N. and Kuyat, C.E., "Guidelines for Evaluating and NIST Technical Note 1297, U.S. Government Printing Office, Washington, DC, (1994).



Certified Reference Material CRM

CERTIFIED WEIGHT REPORT

Part Number:
20064

Lot Number:
022023

Description:
CLP PCB'S - Aroclor Mix
Aroclors 1016 & 1260

Expiration Date:
022033

Recommended Storage:
Ambient (20 °C)

Nominal Concentration (µg/mL):
1000

NIST Test ID#:
6UTB

Solvent(s):
Hexane

Lot#:
273615

Formulated By:
Benson Chan

Reviewed By:
Pedro L. Rentas

DATE:
022023

DATE:
022023

Weight(s) shown below were combined and diluted to (mL.):
200.0

Balance Uncertainty:
0.010

Flask Uncertainty:
0.010

Part Number:
20064

Lot Number:
022023

Description:
CLP PCB'S - Aroclor Mix
Aroclors 1016 & 1260

Expiration Date:
022033

Recommended Storage:
Ambient (20 °C)

Nominal Concentration (µg/mL):
1000

NIST Test ID#:
6UTB

Solvent(s):
Hexane

Lot#:
273615

Formulated By:
Benson Chan

Reviewed By:
Pedro L. Rentas

DATE:
022023

DATE:
022023

Weight(s) shown below were combined and diluted to (mL.):
200.0


Balance Uncertainty:
0.010

Flask Uncertainty:
0.010

Compound	RM#	Lot Number	Nominal Conc (µg/mL)	Purity (%)	Purity Uncertainty	Target Weight(g)	Actual Weight(g)	Actual Conc (µg/mL)	Expanded Uncertainty (+/-) (µg/mL)	CAS#	OSHA PEL (TWA)	LD50
1. Aroclor 1016	15	020491JC	1000	100	0.2	0.20004	0.20060	1002.8	4.0	12674-11-2	N/A	N/A
2. Aroclor 1260	21	020491JC	1000	100	0.2	0.20004	0.20081	1003.9	4.0	11086-82-5	0.5mg/m3	orl-rat 1315mg/kg

* The certified value is the concentration calculated from gravimetric and volumetric measurements unless otherwise stated.
* Standards are prepared gravimetrically using balances that are calibrated with weights traceable to NIST (see above).
* All Standards, after opening ampule, should be stored with caps tight and under appropriate laboratory conditions.
* Uncertainty Reference: Taylor, B.N. and Kuyat, C.E., "Guidelines for Evaluating and Expressing the Uncertainty of NIST Measurement Result," NIST Technical Note 1297, U.S. Government Printing Office, Washington, DC, (1994).

Comments
GC3-M1 Analysis by Melissa Stortier
Column ID SPB-608 30 meter X 0.53mm X5µm film thickness
Flow rates: Helium (carrier) = 5mL/min, Helium (make-up) = 25mL/min
Hydrogen (make-up) = 30mL/min, Air (make-up) = 350mL/min
Oven Profile: Temp 1 = 150°C (Time 1 = 4 min), Temp 2 = 280°C (Time 2 = 13.5 min)
Rate = 8°C/min, Total run time = 35 min
Injector temp. = 200°C, FID Temp. = 300°C, FID Signal = Etdaq Channel 1
Standard Injection = 1.5µL, Range=3

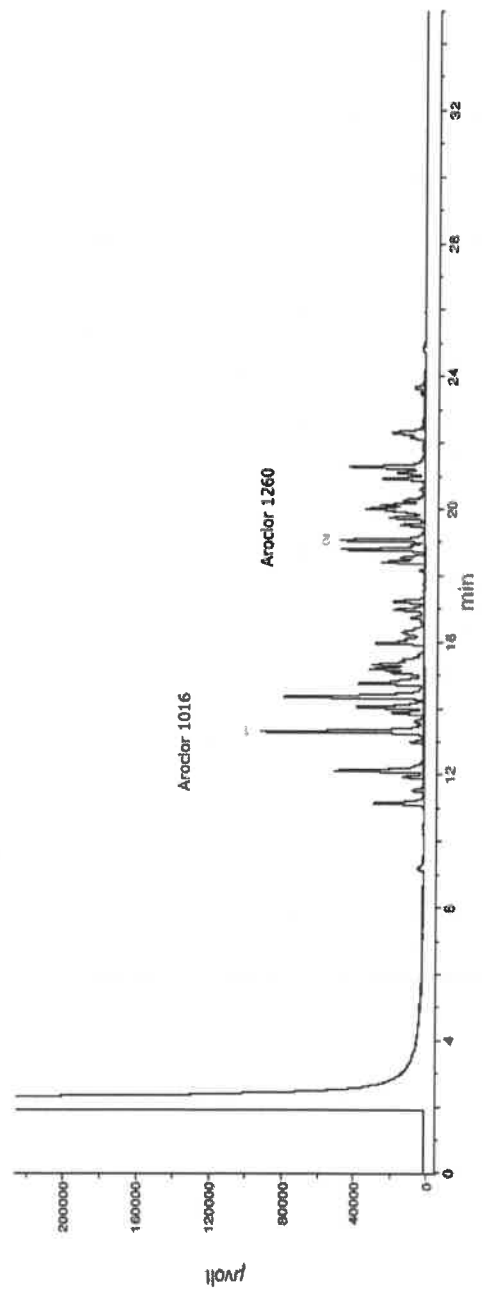



Certified Reference Material CRM

CERTIFIED WEIGHT REPORT

Part Number:
20064

Solvent(s):
Hexane

Lot#
273615

Lot Number:
022023

Formulated By:
Benson Chan

DATE
022023

Description:
CLP PCB'S - Aroclor Mix
Aroclors 1016 & 1260

Reviewed By:
Pedro L. Rentas

DATE
022023

Expiration Date:
022033

Expanded
Uncertainty
(+/-) (µg/mL)

4.0

Recommended Storage:
Ambient (20 °C)

Actual
Conc (µg/mL)

1002.8

Nominal Concentration (µg/mL):
1000

Actual
Weight(g)

0.20060

NIST Test ID#:
6UTB

Target
Weight(g)

0.20004

Weight(s) shown below were combined and diluted to (mL.):
200.0

Purity
(%)

100

5E-05 Balance Uncertainty
0.010 Flask Uncertainty

Conc (µg/mL)

1000

SDS Information
(Solvent Safety Info. On Attached pg.)

OSHA PEL (TWA)


LD50

PR2946 7/18
↓
12/20/23
P12955

Compound	RM#	Lot Number	Nominal Conc (µg/mL)	Purity (%)	Expanded Uncertainty (+/-) (µg/mL)	Actual Conc (µg/mL)	Actual Weight(g)	Target Weight(g)
1. Aroclor 1016	15	020491JC	1000	100	4.0	1002.8	0.20060	0.20004
2. Aroclor 1260	21	020491JC	1000	100	4.0	1003.9	0.20081	0.20004

* The certified value is the concentration calculated from gravimetric and volumetric measurements unless otherwise stated.
* Standards are prepared gravimetrically using balances that are calibrated with weights traceable to NIST (see above).
* All Standards, after opening ampule, should be stored with caps tight and under appropriate laboratory conditions.
* Uncertainty Reference: Taylor, B.N. and Kuyat, C.E., "Guidelines for Evaluating and Expressing the Uncertainty of NIST Measurement Result," NIST Technical Note 1297, U.S. Government Printing Office, Washington, DC, (1994).

Comments
GC3-M1 Analysis by Melissa Stortier
Column ID SPB-608 30 meter X 0.53mm X5µm film thickness
Flow rates: Helium (carrier) = 5mL/min, Helium (make-up) = 25mL/min
Hydrogen (make-up) = 30mL/min, Air (make-up) = 350mL/min
Oven Profile: Temp 1 = 150°C (Time 1 = 4 min), Temp 2 = 280°C (Time 2 = 13.5 min)
Rate = 8°C/min, Total run time = 35 min
Injector temp. = 200°C, FID Temp. = 300°C, FID Signal = Etdaq Channel 1
Standard Injection = 1.5µL, Range=3

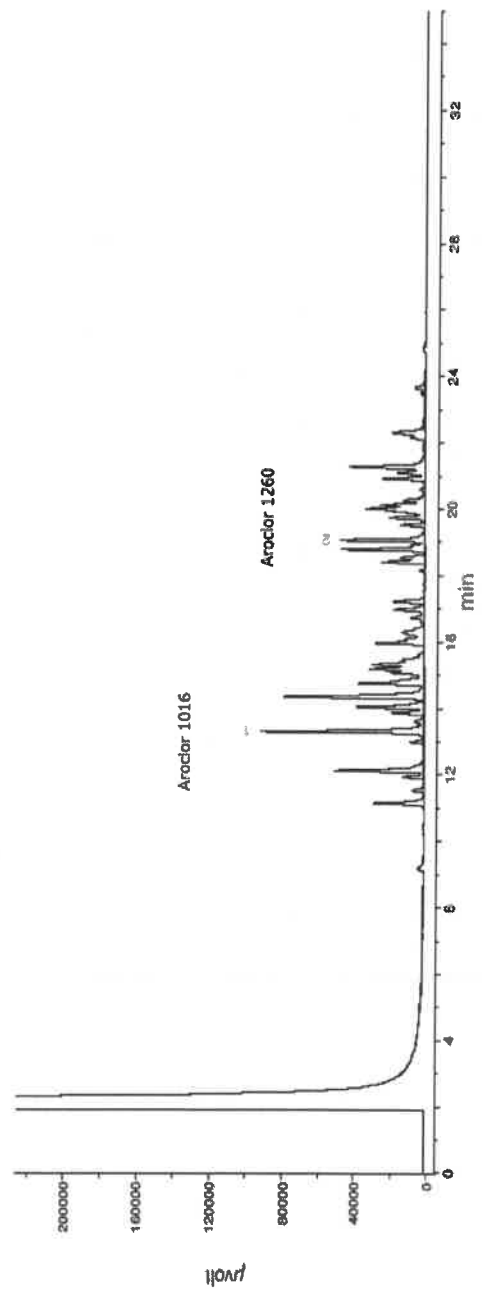



CERTIFIED WEIGHT REPORT

Part Number: 99139
Lot Number: 121823
Description: Aroclor 1254

Expiration Date: 121833
Recommended Storage: Ambient (20 °C)
Nominal Concentration (µg/mL): 100
NIST Test ID#: 6UTB

Volume(s) shown below were combined and diluted to (mL): 20.0
Note: Aroclor 1254 is a mix of isomers.

Solvent(s): Iso-octane
Lot#: 82227

Formulated By: Anthony Mahoney	121823	DATE
Reviewed By: Pedro L. Rentas	121823	DATE


P12956 / Y.P.
12/18/23
P12957

Compound	Part Number	Lot Number	Dilution Factor	Initial Vol. (mL)	Initial Uncertainty	Pipette (mL)	Conc. (µg/mL)	Initial Conc. (µg/mL)	Final Conc. (µg/mL)	Expanded Uncertainty (+/-) (µg/mL)	SDS Information		
											(Solvent Safety Info. On Attached pg.)	CAS#	OSHA PEL (TWA) LD50
1. Aroclor 1254	79100	121823	0.10	2.00	0.017	0.017	1003.3	100.1	1.8	11097-69-1	0.5mg/m3 (skin)		or-rat 1295mg/kg

* The certified value is the concentration calculated from gravimetric and volumetric measurements unless otherwise stated.
* Standards are prepared gravimetrically using balances that are calibrated with weights traceable to NIST (see above).
* Standards are certified (+/-) 0.5% of the stated value, unless otherwise stated.
* All Standards, after opening ampule, should be stored with caps tight and under appropriate laboratory conditions.
* Uncertainty Reference: Taylor, B.N. and Kuyat, C.E., "Guidelines for Evaluating and Expressing the Uncertainty of NIST Measurement Result," NIST Technical Note 1297, U.S. Government Printing Office, Washington, DC, (1994).

Comments
GC3-M1 Analysis by Melissa Stonier
Column ID SPB-608 30 meter X 0.53mm X 5µm film thickness
Flow rates: Helium (carrier) = 5mL/min, Helium (make-up) = 25mL/min
Hydrogen (make-up) = 30mL/min, Air (make-up) = 350mL/min
Oven Profile: Temp 1 = 150 °C (Time 1 = 4 min), Temp 2 = 250 °C (Time 2 = 13.5 min)
Rate = 8 °C/min, Total run time = 35 min
Injector temp. = 200 °C, FID Temp. = 300 °C, FID Signal = EDAQ Channel 1
Standard injection = 1.5µL, Range=3

Peak No.	Name	FID RT (min.)
1	Total Aroclor 1254	18.12

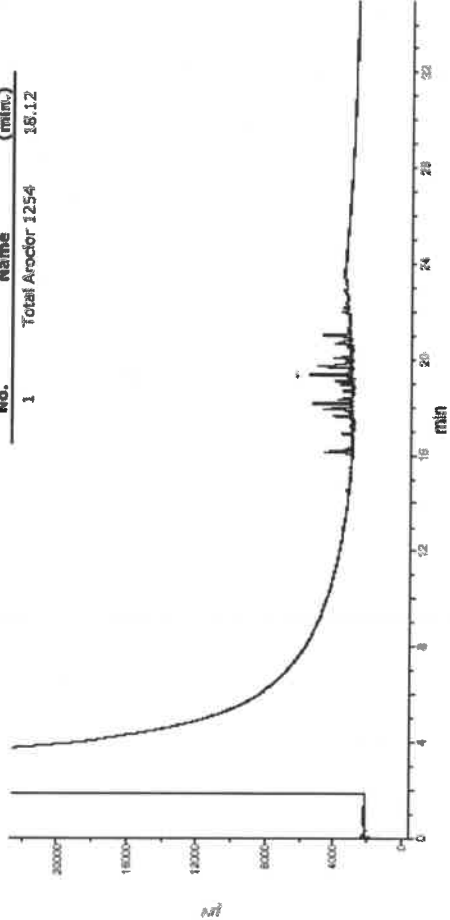



110 Benner Circle
Bellefonte, PA 16823-8812
Tel: 1-814-353-1300
Fax: 1-814-353-1309

www.restek.com

CERTIFIED REFERENCE MATERIAL

Certificate of Analysis

chromatographic plus



FOR LABORATORY USE ONLY-READ SDS PRIOR TO USE.

This Reference Material is intended for Laboratory Use Only as a standard for the qualitative and/or quantitative determination of the analyte(s) listed.

Catalog No. : 32000 **Lot No.:** A0206810

Description : Pesticide Surrogate Mix
Pesticide Surrogate Mix 200 µg/mL, Acetone, 1mL/ampul

Container Size : 2 mL **Pkg Amt:** > 1 mL

Expiration Date : April 30, 2030 **Storage:** 10°C or colder

Handling: Contains PCBs - sonicate prior to use. **Ship:** Ambient

P13348
↓
P13357
10
DAUF
04/25/2024

CERTIFIED VALUES

Elution Order	Compound	CAS #	Lot #	Purity	Grav. Conc. (weight/volume)	Expanded Uncertainty * (95% C.L.; K=2)
1	2,4,5,6-Tetrachloro-m-xylene	877-09-8	RP220407	99%	200.3 µg/mL	+/- 11.1143
2	Decachlorobiphenyl (BZ# 209)	2051-24-3	30638	99%	200.6 µg/mL	+/- 11.1298

* Expanded Uncertainty displayed in same units as Grav. Conc.

Solvent: Acetone
CAS # 67-64-1
Purity 99%

Tech Tips:

Decachlorobiphenyl has poor solubility in most organic solvents. The maximum concentration that can be prepared in acetone, hexane, or isooctane is 200µg/mL. Temperature will affect the solubility as well. Storing solutions at reduced temperatures will cause decachlorobiphenyl to precipitate.

Products containing decachlorobiphenyl must be sonicated for a minimum of 10 minutes prior to opening the ampul. Because each ultrasonic bath operates at a different energy level, 10 minutes is a guideline only. Longer sonication time will not affect product quality.

These precautions apply to working solutions prepared in your laboratory as well. The amount of compound that precipitates depends on concentration AND temperature. If you store your standards at a temperature lower than 4°C (even dilute solutions), allow extra sonication time.

Quality Confirmation Test

Column:

30m x .25mm x .2um
Rtx-CLP II (cat.# 11323)

Carrier Gas:

helium-constant pressure 20 psi.

Temp. Program:

200°C to 300°C
@ 25°C/min. (hold 10 min.)

Inj. Temp:

250°C

Det. Temp:

300°C

Det. Type:


ECD

Split Vent:


10 ml/min.

Inj. Vol

1µl

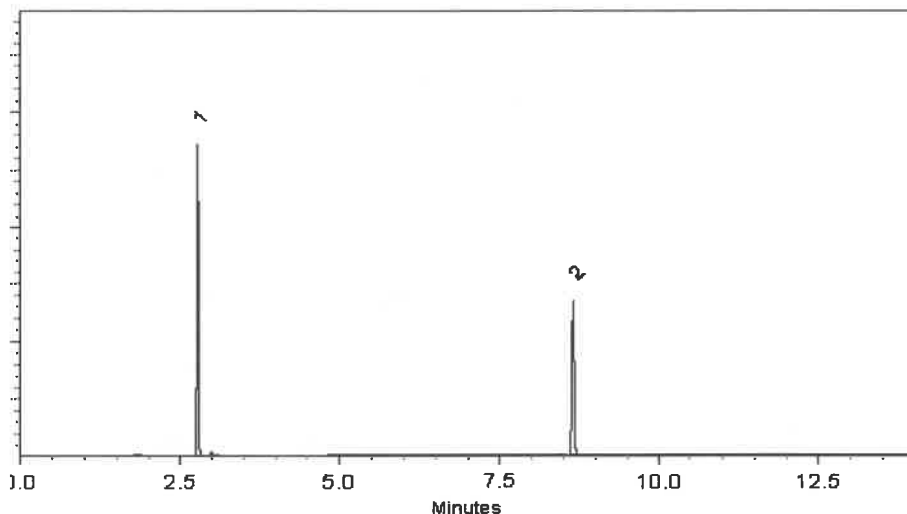


This chromatogram represents a general set of testing conditions chosen for product acceptance. For optimal results in your lab, conditions should be adjusted for your specific instrument, method, and application.


Laith Clemente - Operations Technician I

Date Mixed: 22-Jan-2024


Balance Serial # 1128360905


Jennifer Pollino - Operations Tech III - ARM QC

Date Passed: 24-Jan-2024

Manufactured under Restek's ISO 9001:2015
Registered Quality System
Certificate #FM 80397

P 13348
↓
P 13357
10


SAUF
04/25/2025



110 Benner Circle
Bellefonte, PA 16823-8812
Tel: 1-814-353-1300
Fax: 1-814-353-1309

www.restek.com

CERTIFIED REFERENCE MATERIAL

Certificate of Analysis

chromatographic plus



FOR LABORATORY USE ONLY-READ SDS PRIOR TO USE.

This Reference Material is intended for Laboratory Use Only as a standard for the qualitative and/or quantitative determination of the analyte(s) listed.

Catalog No. : 32007 **Lot No.:** A0207511

Description : Aroclor® 1221 Standard

Aroclor® 1221 Standard 1,000 µg/mL, Hexane, 1mL/ampul

Container Size : 2 mL **Pkg Amt:** > 1 mL

Expiration Date : May 31, 2030 **Storage:** 25°C nominal

Handling: This product contains PCBs. **Ship:** Ambient

CERTIFIED VALUES

Elution Order	Compound	CAS #	Lot #	Purity	Grav. Conc. (weight/volume)	Expanded Uncertainty * (95% C.L.; K=2)
1	Aroclor 1221	11104-28-2	13192500	----%	1,002.7 µg/mL	+/- 55.6424

* Expanded Uncertainty displayed in same units as Grav. Conc.

Solvent: Hexane
CAS # 110-54-3
Purity 99%

P 13374
↓
P 13375
/

[Signature]
05/6/2024

Quality Confirmation Test

Column:

30m x .25mm x .2um
Rtx-CLP II (cat.# 11323)

Carrier Gas:

helium-constant pressure 20 psi.

Temp. Program:

200°C to 300°C
@ 25°C/min. (hold 10 min.)

Inj. Temp:

250°C

Det. Temp:

300°C

Det. Type:


ECD

Split Vent:


10 ml/min.

Inj. Vol

1µl

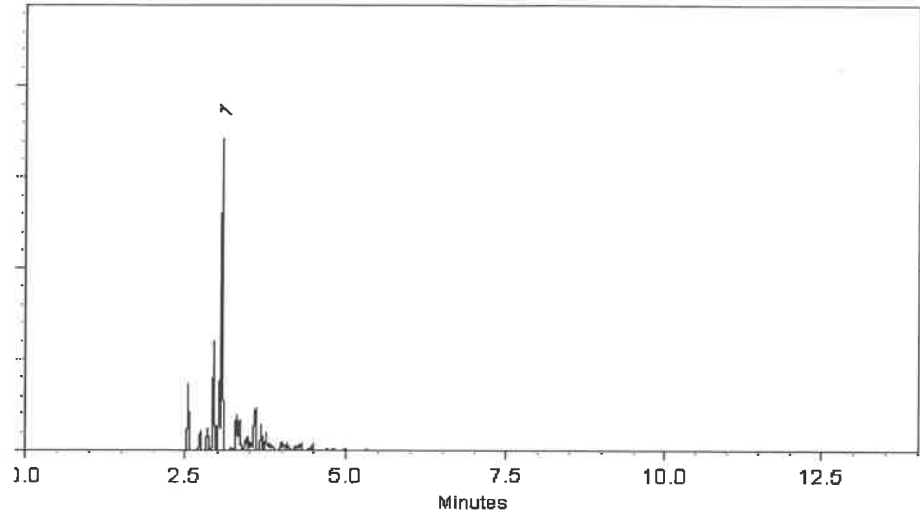

This chromatogram represents a general set of testing conditions chosen for product acceptance. For optimal results in your lab, conditions should be adjusted for your specific instrument, method, and application.


Laith Clemente - Operations Technician I

Date Mixed: 06-Feb-2024


Balance Serial # 1128360905


Jennifer Pollino - Operations Tech III - ARM QC


Date Passed: 08-Feb-2024

Manufactured under Restek's ISO 9001:2015
Registered Quality System
Certificate #FM 80397

P 13374 } ②
↓
P 13375 }


05/6/2024

ISO 17034



Agilent

Trusted Answers

Reference Material Certificate

Product Name: Aroclor 1242 Standard

Lot Number: 0006665550

Product Number: PP-312-1

Lot Issue Date: 08-Feb-2022

Storage Conditions: Store at Room Temperature (15° to 30°C).

Expiration Date: 31-Jan-2027

Component Name	CERTIFIED VALUES		CAS#	Analyte Lot
	Concentration	Expanded Uncertainty		
Aroclor 1242	100.4	± 0.5 µg/mL	053469-21-9	NT01020

Matrix: isooctane (2,2,4-trimethylpentane)

Description:

This document is prepared in accordance with ISO 17034 and Guide 31. This analytical reference material standard was manufactured and verified in accordance with an ISO 9001 registered quality system and analyte concentrations were verified by an ISO 17025 accredited laboratory. The concentration and uncertainty value at the 95% confidence level for each analyte, determined gravimetrically, is listed above.

Traceability:

The balances used for these measurements are calibrated with weights traceable to NIST in compliance with ANSI/NCSL Z540.3, ISO 9001, ISO 17025, and ISO 17034. Calibrated Class A glassware is used for volumetric measurements. Thermometers are calibrated against a NIST traceable thermometer in accordance with NIST Special Publication 1088.

Homogeneity:

This analytical reference standard was unitized according to an in-house procedure and is guaranteed to be homogeneous. There is no minimum sub-sample size required.

Instructions for Use:

Sample aliquots for analysis should be withdrawn at 20°C to 25°C immediately after opening the container and should be processed without delay for the certified values to be valid within the stated uncertainties.

Safety:

Refer to the Safety Data Sheet on www.agilent.com for information regarding this analytical reference material.

Intended Use:

This analytical reference standard is intended for the preparation of working reference samples for use in routine laboratory analyses, calibration of instruments, validation of analytical methods, assessments of measurement methods, and continuing calibration verification.

Expiration of Certification:

The certification of this analytical reference standard is valid until the expiration date specified above, provided the material is handled and stored in accordance with the instructions given in this certificate. This certification is nullified if the material is damaged, contaminated, or otherwise modified.

P13589
↓
P13590AJ
10/14/24

ISO 17034



Maintenance of Certification:

If substantive changes are noted that affect the certification before the expiration of this certificate, Agilent will notify the purchaser.

Sample lot approver:

Monica Bourgeois
QMS Representative



ISO 17034 Cert
No. AR-1936

RM was produced in accordance with the TUV/SUD registered ISO 9001:2015
Quality Management System. Cert# 951215321

Page: 2 of 2

www.agilent.com/quality/

CSD-QA-015.1



ISO 17025
Cert No. AT-

Reference Material Certificate
Product Information Sheet

Product Name: Aroclor 1248 Standard

Lot Number: 0006726317

Product Number: PP-342-1

Lot Issue Date: 27-Jan-2023

Storage Conditions: Store at Room Temperature (15° to 30°C).

Expiration Date: 28-Feb-2031

Component Name	Concentration	Uncertainty	CAS#	Analyte Lot
Aroclor 1248	100.3 ±	0.5 µg/mL	012672-29-6	NT01582

Matrix: isooctane (2,2,4-trimethylpentane)

Description:

This document is prepared in accordance with ISO 17034 and Guide 31. This analytical reference material (RM) standard was manufactured and verified in accordance with an ISO 9001 registered quality system and analyte concentrations were verified by an ISO 17025 accredited laboratory. The concentration and uncertainty value at the 95% confidence level for each analyte, determined gravimetrically, is listed above. Purity values are taken from approved vendor raw material certificates.

Traceability:

The balances used for these measurements are calibrated with weights traceable to NIST in compliance with ANSI/NCSL Z540.3, ISO 9001, ISO 17025, and ISO 17034. Calibrated Class A glassware is used for volumetric measurements. Thermometers are calibrated against a NIST traceable thermometer in accordance with NIST Special Publication 1088.

Homogeneity:

This analytical reference (RM) standard was unitized according to an in-house procedure and is guaranteed to be homogeneous. There is no minimum sub-sample size required.

Instructions for Use:

Sample aliquots for analysis should be withdrawn at 20°C to 25°C immediately after opening the container and should be processed without delay for the certified values to be valid within the stated uncertainties.

Safety:

Refer to the Safety Data Sheet on www.agilent.com for information regarding this analytical reference material.

Intended Use:

This analytical reference (RM) standard is intended for the preparation of working reference samples for use in routine laboratory analyses, calibration of instruments, validation of analytical methods, assessments of measurement methods, and continuing calibration verification.

Expiration of Certification:

The certification of this analytical reference standard (RM) is valid until the expiration date specified above, provided the material is handled and stored in accordance with the instructions given in this certificate. This certification is nullified if the material is damaged, contaminated, or otherwise modified.

P13591
↓
P13592

AS
10/14/2024



Maintenance of Certification:

If substantive changes are noted that affect the certification before the expiration of this certificate, Agilent will notify the purchaser.

Sample lot approver:

Monica Bourgeois
QMS Representative



ISO 17034 Cert
No. AR-1936

RM was produced in accordance with the TUV/SUD registered ISO
9001:2015 Quality Management System. Cert# 951215321

Page: 2 of 2

www.agilent.com/quality/

CSD-QA-015.1

ISO 17025



110 Benner Circle
Bellefonte, PA 16823-8812
Tel: 1-814-353-1300
Fax: 1-814-353-1309

www.restek.com

CERTIFIED REFERENCE MATERIAL

Certificate of Analysis

chromatographic plus



FOR LABORATORY USE ONLY-READ SDS PRIOR TO USE.

This Reference Material is intended for Laboratory Use Only as a standard for the qualitative and/or quantitative determination of the analyte(s) listed.

Catalog No. : 32010 **Lot No.:** A0214733

Description : Aroclor® 1248 Standard

Aroclor® 1248 Standard 1,000µg/mL, Hexane, 1mL/ampul

Container Size : 2 mL **Pkg Amt:** > 1 mL

Expiration Date : November 30, 2030 **Storage:** 25°C nominal

Handling: This product contains PCBs. **Ship:** Ambient

P13695 } Y.P.
P13696 } 10/17/24

CERTIFIED VALUES

Elution Order	Compound	CAS #	Lot #	Purity	Grav. Conc. (weight/volume)	Expanded Uncertainty * (95% C.L.; K=2)
1	Aroclor 1248	12672-29-6	15242800	----%	1,005.0 µg/mL	+/- 55.7700

* Expanded Uncertainty displayed in same units as Grav. Conc.

Solvent: Hexane
CAS # 110-54-3
Purity 99%

Quality Confirmation Test

Column:

30m x .25mm x .2um
Rtx-CLP II (cat.# 11323)

Carrier Gas:

helium-constant pressure 20 psi.

Temp. Program:

200°C to 300°C
@ 25°C/min. (hold 10 min.)

Inj. Temp:

250°C

Det. Temp:

300°C

Det. Type:


ECD

Split Vent:

10 ml/min.

Inj. Vol

0.2µl

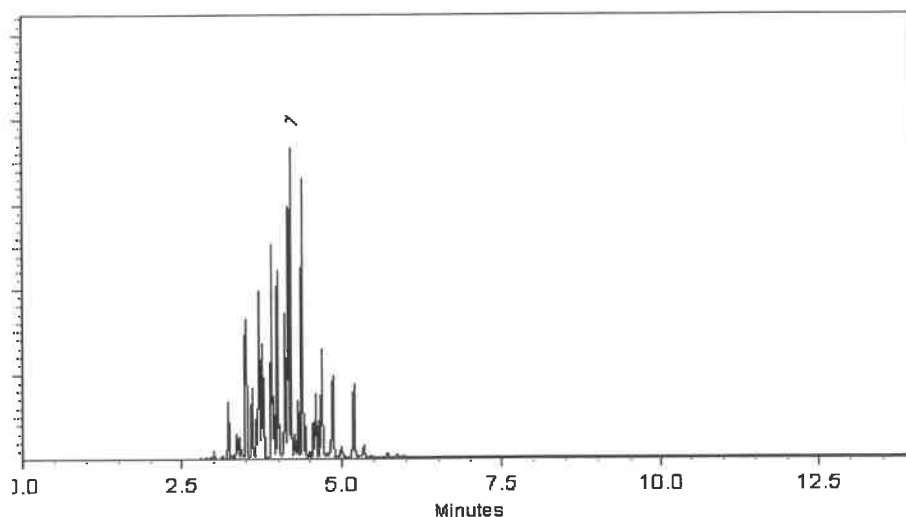

This chromatogram represents a general set of testing conditions chosen for product acceptance. For optimal results in your lab, conditions should be adjusted for your specific instrument, method, and application.

Rebecca Gingerich - Operations Tech II

Date Mixed: 02-Aug-2024

Balance Serial # C322230531

Jennifer Pollino - Operations Tech III - ARM QC

Date Passed: 13-Aug-2024

Manufactured under Restek's ISO 9001:2015
Registered Quality System
Certificate #FM 80397

General Certified Reference Material Notes

Expiration Notes:

- Expiration date valid for unopened ampul stored in compliance with the recommended conditions.
- Uncertainty, concentration, and expiration of the CRM are based on the unopened product being stored according to the recommended condition found in the storage field.

Purity Notes:

- Purity and/or chemical identity are determined by one or more of the following techniques: GC/FID, HPLC, GC/μECD, GC/MS, LC/MS, RI, and/or melting point.
- Compounds with a listed purity of less than 99% have been weight corrected to compensate for impurities and/or salts. A correction factor is used to calculate the amount of compound necessary to achieve the desired concentration of the parent compound in solution.
- Purity of isomeric compounds is reported as the sum of the isomers.
- Purity values are rounded to the nearest whole number.

Certified Uncertainty Value Notes:

- The uncertainties are determined in accordance with ISO 17034 and Guide 35. The certified expanded uncertainty value includes gravimetric uncertainty, homogeneity between-ampul uncertainty, storage stability uncertainty and shipping stability uncertainty and were combined using the following formula:

$$U_{combined\ uncertainty} = k \sqrt{u_{gravimetric}^2 + u_{homogeneity}^2 + u_{storage\ stability}^2 + u_{shipping\ stability}^2}$$

k is a coverage factor of 2, which gives a level of confidence of approximately 95%.

- The packaged amount is the minimum sample size for which uncertainty is valid. The ampuls are over-filled to ensure that the minimum packaged amount can be sufficiently transferred.

Manufacturing Notes:

- Concentration is based upon gravimetric preparation using either a balance whose calibration has been verified daily using NIST traceable weights, and/or dilutions with Class A glassware.

Handling Notes:

- Stability of the unopened product, when stored in compliance with the recommended conditions, is guaranteed through the expiration displayed on the product label and certificate. Contact Restek for additional opened product stability information, with the knowledge/understanding that open product stability is subject to the specific handling and environmental conditions to which the product is exposed. For your convenience Restek supplies deactivated vials with most standards packed in 2mL ampuls. Larger volume deactivated vials are available through Restek as a custom ordered item. Additionally, Restek sells DMDCS for the purpose of glassware deactivation as catalog number 31861, which includes complete instructions.
- If any undissolved material is visible inside the ampul, sonicate the unopened ampul until the material is completely dissolved.



110 Benner Circle
Bellefonte, PA 16823-8812
Tel: 1-814-353-1300
Fax: 1-814-353-1309

www.restek.com

CERTIFIED REFERENCE MATERIAL

Certificate of Analysis

chromatographic plus



FOR LABORATORY USE ONLY-READ SDS PRIOR TO USE.

This Reference Material is intended for Laboratory Use Only as a standard for the qualitative and/or quantitative determination of the analyte(s) listed.

Catalog No. : 32039 **Lot No.:** A0210629

Description : Aroclor® 1016/1260 Mix
Aroclor® 1016/1260 Mix 1,000 µg/mL, Hexane, 1mL/ampul

Container Size : 2 mL **Pkg Amt:** > 1 mL

Expiration Date : July 31, 2030 **Storage:** 25°C nominal

Handling: This product contains PCBs. **Ship:** Ambient

P13697
↓
P13701 } Y.P.
10/19/24

CERTIFIED VALUES

Elution Order	Compound	CAS #	Lot #	Purity	Grav. Conc. (weight/volume)	Expanded Uncertainty * (95% C.L.; K=2)
1	Aroclor 1016	12674-11-2	07	----%	1,005.3 µg/mL	+/- 55.7809
2	Aroclor 1260	11096-82-5	1320657	----%	1,000.0 µg/mL	+/- 55.4850

* Expanded Uncertainty displayed in same units as Grav. Conc.

Solvent: Hexane
CAS # 110-54-3
Purity 99%

Quality Confirmation Test

Column:

30m x .25mm x .2um
Rtx-CLP II (cat.# 11323)

Carrier Gas:

helium-constant pressure 20 psi.

Temp. Program:

200°C to 300°C
@ 25°C/min. (hold 10 min.)

Inj. Temp:

250°C

Det. Temp:

300°C

Det. Type:


ECD

Split Vent:


10 ml/min.

Inj. Vol

0.2µl

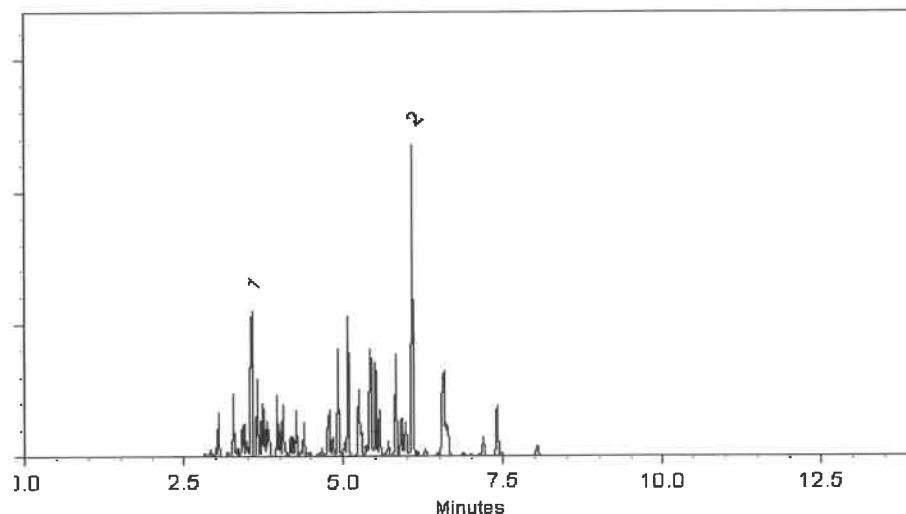


This chromatogram represents a general set of testing conditions chosen for product acceptance. For optimal results in your lab, conditions should be adjusted for your specific instrument, method, and application.


Laith Clemente - Operations Technician I

Date Mixed: 22-Apr-2024

Balance Serial # B442140311


Dillan Murphy - Operations Technician I

Date Passed: 24-Apr-2024

Manufactured under Restek's ISO 9001:2015
Registered Quality System
Certificate #FM 80397

General Certified Reference Material Notes

Expiration Notes:

- Expiration date valid for unopened ampul stored in compliance with the recommended conditions.
- Uncertainty, concentration, and expiration of the CRM are based on the unopened product being stored according to the recommended condition found in the storage field.

Purity Notes:

- Purity and/or chemical identity are determined by one or more of the following techniques: GC/FID, HPLC, GC/μECD, GC/MS, LC/MS, RI, and/or melting point.
- Compounds with a listed purity of less than 99% have been weight corrected to compensate for impurities and/or salts. A correction factor is used to calculate the amount of compound necessary to achieve the desired concentration of the parent compound in solution.
- Purity of isomeric compounds is reported as the sum of the isomers.
- Purity values are rounded to the nearest whole number.

Certified Uncertainty Value Notes:

- The uncertainties are determined in accordance with ISO 17034 and Guide 35. The certified expanded uncertainty value includes gravimetric uncertainty, homogeneity between-ampul uncertainty, storage stability uncertainty and shipping stability uncertainty and were combined using the following formula:

$$U_{combined\ uncertainty} = k \sqrt{u_{gravimetric}^2 + u_{homogeneity}^2 + u_{storage\ stability}^2 + u_{shipping\ stability}^2}$$

k is a coverage factor of 2, which gives a level of confidence of approximately 95%.

- The packaged amount is the minimum sample size for which uncertainty is valid. The ampuls are over-filled to ensure that the minimum packaged amount can be sufficiently transferred.

Manufacturing Notes:

- Concentration is based upon gravimetric preparation using either a balance whose calibration has been verified daily using NIST traceable weights, and/or dilutions with Class A glassware.

Handling Notes:

- Stability of the unopened product, when stored in compliance with the recommended conditions, is guaranteed through the expiration displayed on the product label and certificate. Contact Restek for additional opened product stability information, with the knowledge/understanding that open product stability is subject to the specific handling and environmental conditions to which the product is exposed. For your convenience Restek supplies deactivated vials with most standards packed in 2mL ampuls. Larger volume deactivated vials are available through Restek as a custom ordered item. Additionally, Restek sells DMDCS for the purpose of glassware deactivation as catalog number 31861, which includes complete instructions.
- If any undissolved material is visible inside the ampul, sonicate the unopened ampul until the material is completely dissolved.



110 Benner Circle
Bellefonte, PA 16823-8812
Tel: 1-814-353-1300
Fax: 1-814-353-1309

www.restek.com

CERTIFIED REFERENCE MATERIAL

Certificate of Analysis

chromatographic plus



FOR LABORATORY USE ONLY-READ SDS PRIOR TO USE.

This Reference Material is intended for Laboratory Use Only as a standard for the qualitative and/or quantitative determination of the analyte(s) listed.

Catalog No. : 32009 **Lot No.:** A0210232
Description : Aroclor® 1242 Standard
Aroclor® 1242 Standard 1,000 µg/mL, Hexane, 1mL/ampul
Container Size : 2 mL **Pkg Amt:** > 1 mL
Expiration Date : July 31, 2030 **Storage:** 25°C nominal
Handling: This product contains PCBs. **Ship:** Ambient

P13706 } y.p.
P13707 } 10/17/24

CERTIFIED VALUES

Elution Order	Compound	CAS #	Lot #	Purity	Grav. Conc. (weight/volume)	Expanded Uncertainty * (95% C.L.; K=2)
1	Aroclor 1242	53469-21-9	01141	----%	1,000.7 µg/mL	+/- 55.5295

* Expanded Uncertainty displayed in same units as Grav. Conc.

Solvent: Hexane
CAS # 110-54-3
Purity 99%

Quality Confirmation Test

Column:

30m x .25mm x .2um
Rtx-CLP II (cat.# 11323)

Carrier Gas:

helium-constant pressure 20 psi.

Temp. Program:

200°C to 300°C
@ 25°C/min. (hold 10 min.)

Inj. Temp:

250°C

Det. Temp:

300°C

Det. Type:


ECD

Split Vent:

10 ml/min.

Inj. Vol

0.2µl

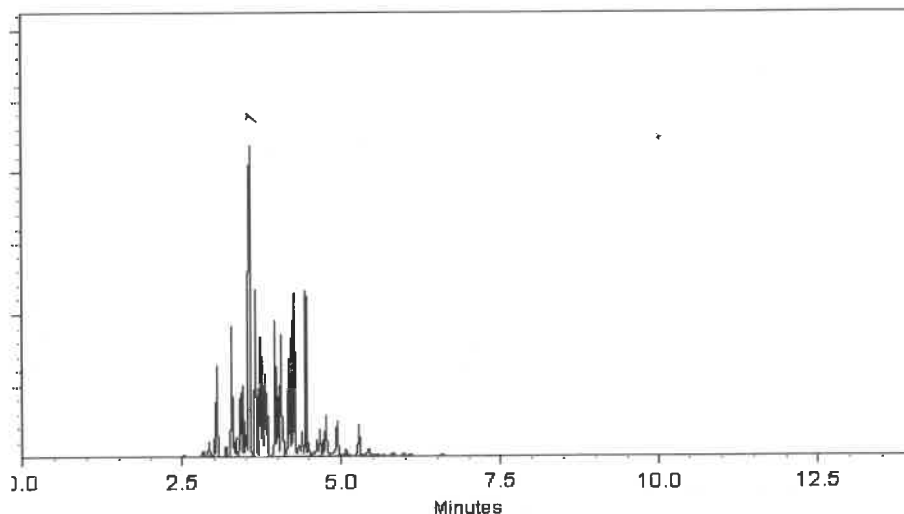

This chromatogram represents a general set of testing conditions chosen for product acceptance. For optimal results in your lab, conditions should be adjusted for your specific instrument, method, and application.


Amanda Miller - Operations Tech III - ARM QC

Date Mixed: 11-Apr-2024

Balance Serial # B442140311


Christie Mills - Operations Lead Tech - ARM QC

Date Passed: 17-Apr-2024

Manufactured under Restek's ISO 9001:2015
Registered Quality System
Certificate #FM 80397

General Certified Reference Material Notes

Expiration Notes:

- Expiration date valid for unopened ampul stored in compliance with the recommended conditions.
- Uncertainty, concentration, and expiration of the CRM are based on the unopened product being stored according to the recommended condition found in the storage field.

Purity Notes:

- Purity and/or chemical identity are determined by one or more of the following techniques: GC/FID, HPLC, GC/μECD, GC/MS, LC/MS, RI, and/or melting point.
- Compounds with a listed purity of less than 99% have been weight corrected to compensate for impurities and/or salts. A correction factor is used to calculate the amount of compound necessary to achieve the desired concentration of the parent compound in solution.
- Purity of isomeric compounds is reported as the sum of the isomers.
- Purity values are rounded to the nearest whole number.

Certified Uncertainty Value Notes:

- The uncertainties are determined in accordance with ISO 17034 and Guide 35. The certified expanded uncertainty value includes gravimetric uncertainty, homogeneity between-ampul uncertainty, storage stability uncertainty and shipping stability uncertainty and were combined using the following formula:

$$U_{combined\ uncertainty} = k \sqrt{u_{gravimetric}^2 + u_{homogeneity}^2 + u_{storage\ stability}^2 + u_{shipping\ stability}^2}$$

k is a coverage factor of 2, which gives a level of confidence of approximately 95%.

- The packaged amount is the minimum sample size for which uncertainty is valid. The ampuls are over-filled to ensure that the minimum packaged amount can be sufficiently transferred.

Manufacturing Notes:

- Concentration is based upon gravimetric preparation using either a balance whose calibration has been verified daily using NIST traceable weights, and/or dilutions with Class A glassware.

Handling Notes:

- Stability of the unopened product, when stored in compliance with the recommended conditions, is guaranteed through the expiration displayed on the product label and certificate. Contact Restek for additional opened product stability information, with the knowledge/understanding that open product stability is subject to the specific handling and environmental conditions to which the product is exposed. For your convenience Restek supplies deactivated vials with most standards packed in 2mL ampuls. Larger volume deactivated vials are available through Restek as a custom ordered item. Additionally, Restek sells DMDCS for the purpose of glassware deactivation as catalog number 31861, which includes complete instructions.
- If any undissolved material is visible inside the ampul, sonicate the unopened ampul until the material is completely dissolved.




110 Benner Circle
Bellefonte, PA 16823-8812
Tel: 1-814-353-1300
Fax: 1-814-353-1309

www.restek.com

CERTIFIED REFERENCE MATERIAL

Certificate of Analysis

chromatographic plus



FOR LABORATORY USE ONLY-READ SDS PRIOR TO USE.

This Reference Material is intended for Laboratory Use Only as a standard for the qualitative and/or quantitative determination of the analyte(s) listed.

Catalog No. : 32000 **Lot No.:** A0214495

Description : Pesticide Surrogate Mix

Pesticide Surrogate Mix 200 µg/mL, Acetone, 1mL/ampul

Container Size : 2 mL **Pkg Amt:** > 1 mL

Expiration Date : October 31, 2030 **Storage:** 10°C or colder

Handling: Contains PCBs - sonicate prior to use. **Ship:** Ambient

P19785
AJ
11/19/24
P19789

CERTIFIED VALUES

Elution Order	Compound	CAS #	Lot #	Purity	Grav. Conc. (weight/volume)	Expanded Uncertainty * (95% C.L.; K=2)
1	2,4,5,6-Tetrachloro-m-xylene	877-09-8	RP220407	99%	200.2 µg/mL	+/- 11.1087
2	Decachlorobiphenyl (BZ# 209)	2051-24-3	30679	99%	201.4 µg/mL	+/- 11.1753

* Expanded Uncertainty displayed in same units as Grav. Conc.

Solvent: Acetone
CAS # 67-64-1
Purity 99%

Tech Tips:

Decachlorobiphenyl has poor solubility in most organic solvents. The maximum concentration that can be prepared in acetone, hexane, or isooctane is 200µg/mL. Temperature will affect the solubility as well. Storing solutions at reduced temperatures will cause decachlorobiphenyl to precipitate.

Products containing decachlorobiphenyl must be sonicated for a minimum of 10 minutes prior to opening the ampul. Because each ultrasonic bath operates at a different energy level, 10 minutes is a guideline only. Longer sonication time will not affect product quality.

These precautions apply to working solutions prepared in your laboratory as well. The amount of compound that precipitates depends on concentration AND temperature. If you store your standards at a temperature lower than 4°C (even dilute solutions), allow extra sonication time.

Quality Confirmation Test

Column:
30m x 25mm x 2um
Rtx-CLP II (cat.# 11323)

Carrier Gas:
helium-constant pressure 20 psi.

Temp. Program:
200°C to 300°C
@ 25°C/min. (hold 10 min.)


Inj. Temp:
250°C

Det. Temp:
300°C

Det. Type:
ECD

Split Vent:
10 ml/min.

Inj. Vol
1µl

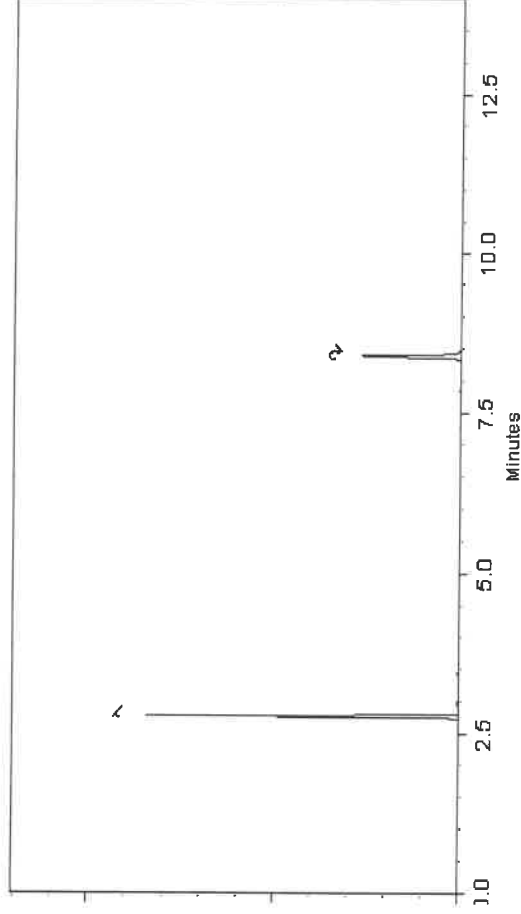

This chromatogram represents a general set of testing conditions chosen for product acceptance. For optimal results in your lab, conditions should be adjusted for your specific instrument, method, and application.

A. O. P.
Aaron Enyart - Operations Tech I

Date Mixed: 29-Jul-2024 Balance Serial # B345965662

Jennifer Pollino
Jennifer Pollino - Operations Tech III - ARM QC

Date Passed: 01-Aug-2024

Manufactured under Restek's ISO 9001:2015
Registered Quality System
Certificate #FM 80397




110 Benner Circle
Bellefonte, PA 16823-8812
Tel: 1-814-353-1300
Fax: 1-814-353-1309

www.restek.com

CERTIFIED REFERENCE MATERIAL

Certificate of Analysis

chromatographic plus



FOR LABORATORY USE ONLY-READ SDS PRIOR TO USE.

This Reference Material is intended for Laboratory Use Only as a standard for the qualitative and/or quantitative determination of the analyte(s) listed.

Catalog No. : 32000 **Lot No.:** A0214495

Description : Pesticide Surrogate Mix

Pesticide Surrogate Mix 200 µg/mL, Acetone, 1mL/ampul

Container Size : 2 mL **Pkg Amt:** > 1 mL

Expiration Date : October 31, 2030 **Storage:** 10°C or colder

Handling: Contains PCBs - sonicate prior to use. **Ship:** Ambient

P19785
AJ
11/19/24
P19789

CERTIFIED VALUES

Elution Order	Compound	CAS #	Lot #	Purity	Grav. Conc. (weight/volume)	Expanded Uncertainty * (95% C.L.; K=2)
1	2,4,5,6-Tetrachloro-m-xylene	877-09-8	RP220407	99%	200.2 µg/mL	+/- 11.1087
2	Decachlorobiphenyl (BZ# 209)	2051-24-3	30679	99%	201.4 µg/mL	+/- 11.1753

* Expanded Uncertainty displayed in same units as Grav. Conc.

Solvent: Acetone
CAS # 67-64-1
Purity 99%

Tech Tips:

Decachlorobiphenyl has poor solubility in most organic solvents. The maximum concentration that can be prepared in acetone, hexane, or isooctane is 200µg/mL. Temperature will affect the solubility as well. Storing solutions at reduced temperatures will cause decachlorobiphenyl to precipitate.

Products containing decachlorobiphenyl must be sonicated for a minimum of 10 minutes prior to opening the ampul. Because each ultrasonic bath operates at a different energy level, 10 minutes is a guideline only. Longer sonication time will not affect product quality.

These precautions apply to working solutions prepared in your laboratory as well. The amount of compound that precipitates depends on concentration AND temperature. If you store your standards at a temperature lower than 4°C (even dilute solutions), allow extra sonication time.

Quality Confirmation Test

Column:
30m x 25mm x 2um
Rtx-CLP II (cat.# 11323)

Carrier Gas:
helium-constant pressure 20 psi.

Temp. Program:
200°C to 300°C
@ 25°C/min. (hold 10 min.)


Inj. Temp:
250°C

Det. Temp:
300°C

Det. Type:
ECD

Split Vent:
10 ml/min.

Inj. Vol
1µl

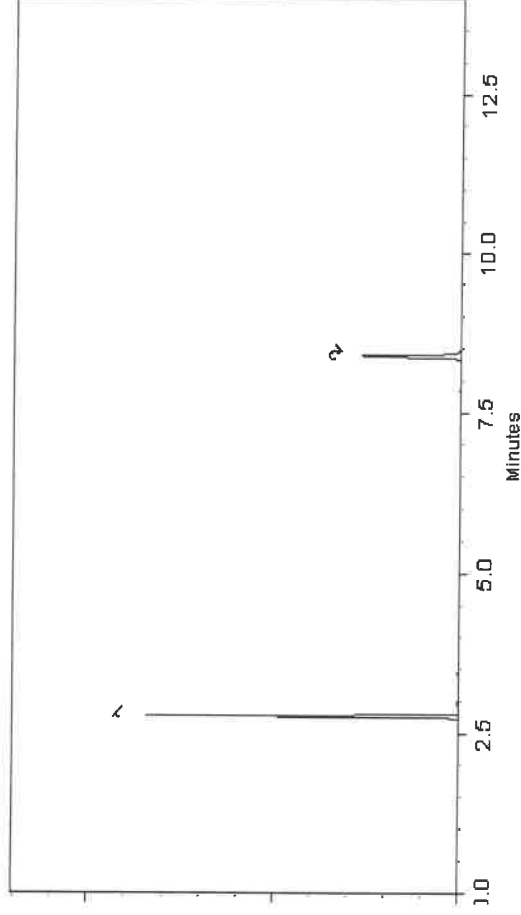

This chromatogram represents a general set of testing conditions chosen for product acceptance. For optimal results in your lab, conditions should be adjusted for your specific instrument, method, and application.

A. O. P.
Aaron Enyart - Operations Tech I

Date Mixed: 29-Jul-2024 Balance Serial # B345965662

Jennifer Pollino
Jennifer Pollino - Operations Tech III - ARM QC

Date Passed: 01-Aug-2024

Manufactured under Restek's ISO 9001:2015
Registered Quality System
Certificate #FM 80397



110 Benner Circle
Bellefonte, PA 16823-8812
Tel: 1-814-353-1300
Fax: 1-814-353-1309

www.restek.com

CERTIFIED REFERENCE MATERIAL

Certificate of Analysis

chromatographic plus



FOR LABORATORY USE ONLY-READ SDS PRIOR TO USE.

This Reference Material is intended for Laboratory Use Only as a standard for the qualitative and/or quantitative determination of the analyte(s) listed.

Catalog No. : 32011 **Lot No.:** A0217391
Description : Aroclor® 1254 Standard
Aroclor® 1254 Standard 1,000 µg/mL, Hexane, 1mL/ampul
Container Size : 2 mL **Pkg Amt:** > 1 mL
Expiration Date : January 31, 2031 **Storage:** 25°C nominal
Handling: This product contains PCBs. **Ship:** Ambient

CERTIFIED VALUES

Elution Order	Compound	CAS #	Lot #	Purity	Grav. Conc. (weight/volume)	Expanded Uncertainty * (95% C.L.; K=2)
1	Aroclor 1254	11097-69-1	124-191-B	----%	1,004.7 µg/mL	+/- 55.7515

* Expanded Uncertainty displayed in same units as Grav. Conc.

Solvent: Hexane
CAS # 110-54-3
Purity 99%

P13830
↓
P13832
↓
P13834
AJ
12/09/24

Quality Confirmation Test

Column:

30m x .25mm x .2um
Rtx-CLP II (cat.# 11323)

Carrier Gas:

helium-constant pressure 20 psi.

Temp. Program:

200°C to 300°C
@ 25°C/min. (hold 10 min.)

Inj. Temp:

250°C

Det. Temp:

300°C

Det. Type:


ECD

Split Vent:

300 ml/min.

Inj. Vol

1µl

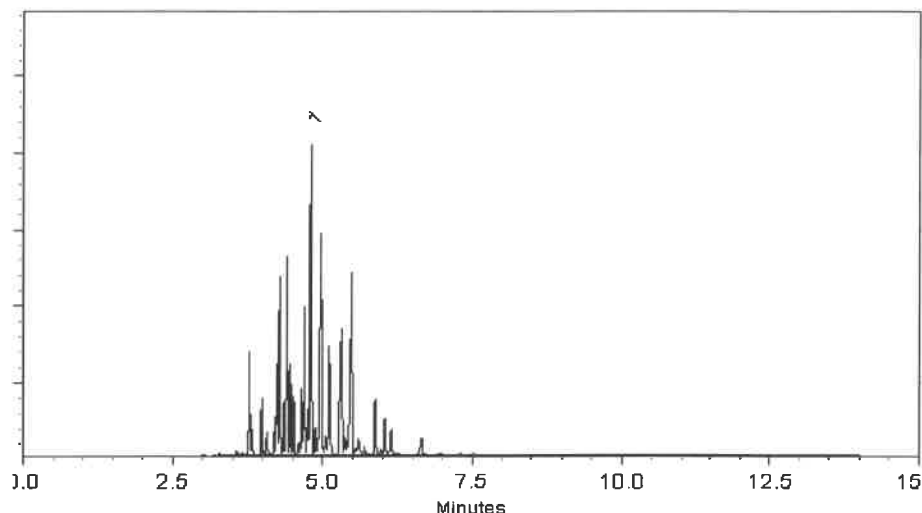

This chromatogram represents a general set of testing conditions chosen for product acceptance. For optimal results in your lab, conditions should be adjusted for your specific instrument, method, and application.

Michael Maye
Michael Maye - Operations Tech I

Date Mixed: 02-Oct-2024

Balance Serial # C322230531

Jennifer Pollino
Jennifer Pollino - Operations Tech III - ARM QC

Date Passed: 07-Oct-2024

Manufactured under Restek's ISO 9001:2015
Registered Quality System
Certificate #FM 80397



110 Benner Circle
Bellefonte, PA 16823-8812
Tel: 1-814-353-1300
Fax: 1-814-353-1309

www.restek.com

CERTIFIED REFERENCE MATERIAL

Certificate of Analysis

chromatographic plus



FOR LABORATORY USE ONLY-READ SDS PRIOR TO USE.

This Reference Material is intended for Laboratory Use Only as a standard for the qualitative and/or quantitative determination of the analyte(s) listed.

Catalog No. : 32008 **Lot No.:** A0219655

Description : Aroclor® 1232 Standard

Container Size : 2 mL

Expiration Date : March 31, 2031

Handling: This product contains PCBs.

Aroclor® 1232 Standard 1,000 µg/mL, Hexane, 1mL/ampul

Pkg Amt: > 1 mL

Storage: 25°C nominal

Ship: Ambient

CERTIFIED VALUES

Elution Order	Compound	CAS #	Lot #	Purity	Grav. Conc. (weight/volume)	Expanded Uncertainty * (95% C.L.; K=2)
1	Aroclor 1232	11141-16-5	15665-01	---%	1,007.0 µg/mL	+/- 55.8810

Solvent: Hexane

CAS # 110-54-3

Purity 99%

* Expanded Uncertainty displayed in same units as Grav. Conc.

P13878
↓
P13880

AJ
01/28/25

Quality Confirmation Test

Column:

30m x .25mm x .2um
Rtx-CLP II (cat.# 11323)

Carrier Gas:

helium-constant pressure 20 psi.

Temp. Program:

200°C to 300°C
@ 25°C/min. (hold 10 min.)

Inj. Temp:

250°C

Det. Temp:

300°C

Det. Type:


ECD

Split Vent:

10 ml/min.

Inj. Vol

1µl

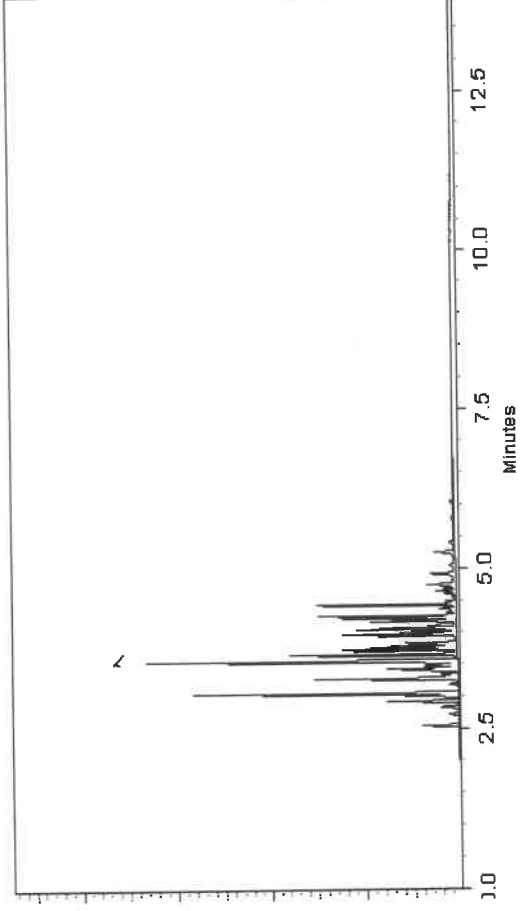

This chromatogram represents a general set of testing conditions chosen for product acceptance. For optimal results in your lab, conditions should be adjusted for your specific instrument, method, and application.

Michael Maye
Michael Maye - Operations Tech I

Date Mixed: 02-Dec-2024

Balance Serial #

C322230531

Brittany Federhik
Brittany Federhiko - Operations Tech I

Date Passed: 05-Dec-2024

Manufactured under Restek's ISO 9001:2015
Registered Quality System
Certificate #FM 80397



CERTIFIED REFERENCE MATERIAL

110 Benner Circle
Bellefonte, PA 16823-8812
Tel: 1-814-353-1300
Fax: 1-814-353-1309

www.restek.com



Certificate of Analysis

chromatographic plus



FOR LABORATORY USE ONLY-READ SDS PRIOR TO USE.

This Reference Material is intended for Laboratory Use Only as a standard for the qualitative and/or quantitative determination of the analyte(s) listed.

Catalog No. : 32409 **Lot No.:** A0217041

Description : Aroclor® 1262 Standard

Container Size : 2 mL **Pkg Amt:** > 1 mL

Expiration Date : December 31, 2030 **Storage:** 25°C nominal

Handling: This product contains PCBs. **Ship:** Ambient

CERTIFIED VALUES

Elution Order	Compound	CAS #	Lot #	Purity	Grav. Conc. (weight/volume)	Expanded Uncertainty * (95% C.L.; K=2)
1	Aroclor 1262	37324-23-5	10849100	----%	1,000.0 µg/mL	+/- 55.4925

Solvent: Hexane
CAS # 110-54-3
Purity 99%

* Expanded Uncertainty displayed in same units as Grav. Conc.

P13881

AJ
01128125

~~PT3880~~

Quality Confirmation Test

Column:
30m x .25mm x .2um
Rtx-CLP II (cat.# 11323)

Carrier Gas:
helium-constant pressure 20 psi.

Temp. Program:
200°C to 300°C
@ 25°C/min. (hold 10 min.)


Inj. Temp:
250°C

Det. Temp:
300°C

Det. Type:
ECD

Split Vent:
300 ml/min.

Inj. Vol
0.2µl

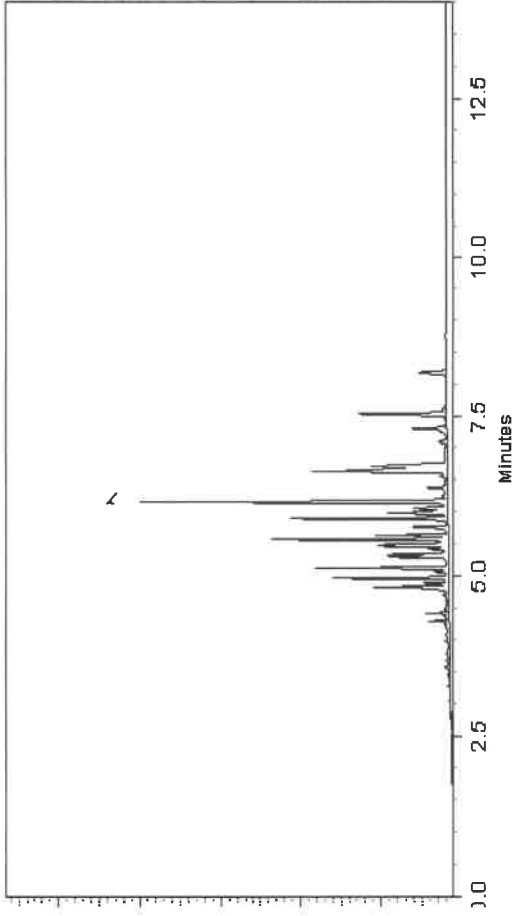

This chromatogram represents a general set of testing conditions chosen for product acceptance. For optimal results in your lab, conditions should be adjusted for your specific instrument, method, and application.


Rebecca Gingerich - Operations Tech II


Jennifer Pollino - Operations Tech III - ARM QC

Date Mixed: 25-Sep-2024 Balance Serial # C322230531

Date Passed: 30-Sep-2024

Manufactured under Restek's ISO 9001:2015
Registered Quality System
Certificate #FM 80397




110 Benner Circle
Bellefonte, PA 16823-8812
Tel: 1-814-353-1300
Fax: 1-814-353-1309

www.restek.com

CERTIFIED REFERENCE MATERIAL

Certificate of Analysis

chromatographic plus



FOR LABORATORY USE ONLY-READ SDS PRIOR TO USE.

This Reference Material is intended for Laboratory Use Only as a standard for the qualitative and/or quantitative determination of the analyte(s) listed.

Catalog No. : 32410

Lot No.: A0217264

Description : Aroclor® 1268 Standard

Aroclor® 1268 Standard 1,000 µg/mL, 1mL/ampul, Hexane

Container Size : 2 mL

Pkg Amt: > 1 mL

Expiration Date : January 31, 2031

Storage: 25°C nominal

Handling:

This product contains PCBs.

Ship: Ambient

CERTIFIED VALUES

Elution Order	Compound	CAS #	Lot #	Purity	Grav. Conc. (weight/volume)	Expanded Uncertainty * (95% C.L.; K=2)
1	Aroclor 1268	11100-14-4	12353400	----%	1,009.8 µg/mL	+/- 56.0364

Solvent: Hexane

CAS # 110-54-3

Purity 99%

* Expanded Uncertainty displayed in same units as Grav. Conc.

P13884

+

AJ
01/28/25

P13886

Quality Confirmation Test

Column:

30m x .25mm x .2um
Rtx-CLP II (cat.# 11323)

Carrier Gas:

helium-constant pressure 20 psi.

Temp. Program:

200°C to 300°C
@ 25°C/min. (hold 10 min.)

Inj. Temp:

250°C

Det. Temp:

300°C

Det. Type:


ECD

Split Vent:

Split ratio 500:1

Inj. Vol

0.2µl

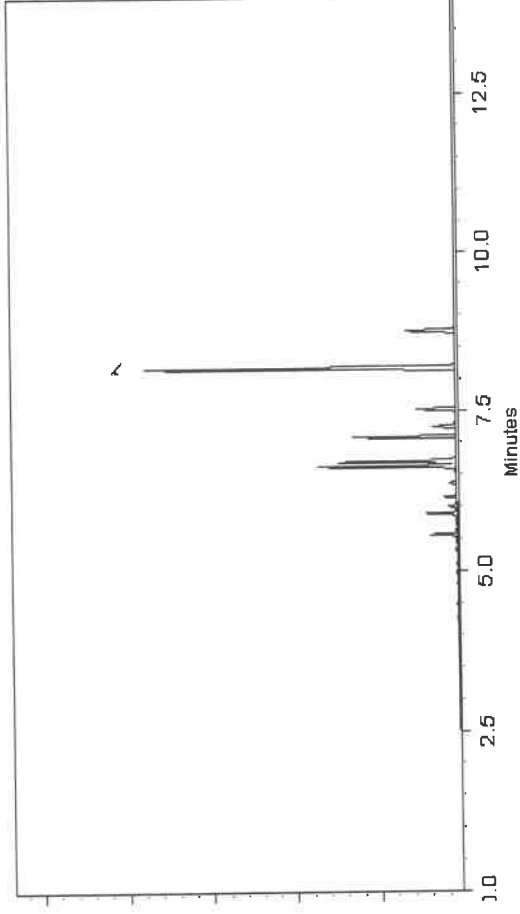

This chromatogram represents a general set of testing conditions chosen for product acceptance. For optimal results in your lab, conditions should be adjusted for your specific instrument, method, and application.

Stacey Wanner - Operations Technician I

Date Mixed: 01-Oct-2024

Balance Serial #

1128360905

Jennifer Pollino - Operations Tech III - ARM QC

Date Passed: 02-Oct-2024

Manufactured under Restek's ISO 9001:2015
Registered Quality System
Certificate #FM 80397

n-Hexane 95%
ULTRA RESI-ANALYZED
For Organic Residue Analysis



Material No.: 9262-03
Batch No.: 24G1962003
Manufactured Date: 2024-05-23
Expiration Date: 2025-08-22
Revision No.: 0

Certificate of Analysis

Test	Specification	Result
FID-Sensitive Impurities (as 2-Octanol) Single Impurity Peak (ng/mL)	≤ 5	3
ECD Sensitive Impurities (as Heptachlor Epoxide) Single Peak (pg/mL)	≤ 10	1
ECD-Sensitive Impurities (as Ethylene Dibromide) - Single Impurity Peak (ng/mL)	≤ 5	1
Assay (Total Saturated C ₆ Isomers) (by GC, corrected for water)	$\geq 99.5 \%$	99.7 %
Assay (as n-Hexane) (by GC, corrected for water)	$\geq 95 \%$	98 %
Color (APHA)	≤ 10	5
Residue after Evaporation	≤ 1.0 ppm	0.1 ppm
Substances Darkened by H ₂ SO ₄	Passes Test	Passes Test
Water (by KF, coulometric)	$\leq 0.05 \%$	< 0.01 %

For Laboratory, Research, or Manufacturing Use
MEETS SPECIFICATIONS WITHIN THE EXPIRATION PERIOD

Country of Origin: USA
Packaging Site: Phillipsburg Mfg Ctr & DC

Jamie Croak
Director Quality Operations, Bioscience Production

n-Hexane 95%
ULTRA RESI-ANALYZED
For Organic Residue Analysis

 **avantor**™



Material No.: 9262-03

Batch No.: 25C0362005

Manufactured Date: 2025-01-29

Expiration Date: 2026-04-30

Revision No.: 0

W3234 JB
OP4421 07/28/2025

Certificate of Analysis

Test	Specification	Result
FID-Sensitive Impurities (as 2-Octanol) Single Impurity Peak (ng/mL)	<= 5	1
ECD Sensitive Impurities (as HeptachlorEpoxide) Single Peak (pg/mL)	<= 10	6
ECD-Sensitive Impurities (as EthyleneDibromide) - Single Impurity Peak (ng/mL)	<= 5	5
Assay (Total Saturated C ₆ Isomers) (by GC, corrected for water)	>= 99.5 %	100.0 %
Assay (as n-Hexane) (by GC, corrected for water)	>= 95 %	100 %
Color (APHA)	<= 10	10
Residue after Evaporation	<= 1.0 ppm	0.1 ppm
Substances Darkened by H ₂ SO ₄	Passes Test	Passes Test
Water (by KF, coulometric)	<= 0.05 %	<0.01 %

For Laboratory, Research, or Manufacturing Use

MEETS SPECIFICATIONS WITHIN THE EXPIRATION PERIOD

Country of Origin: United States

Packaging Site: Phillipsburg Mfg Ctr & DC



Jamie Croak
Director Quality Operations, Bioscience Production

For questions on this Certificate of Analysis please contact Technical Services at 855.282.6867 or +1.610.386.1700

Avantor Performance Materials LLC



SHIPPING DOCUMENTS

CHEMTECH

CHAIN OF CUSTODY RECORD

284 Sheffield Street, Mountainside, NJ 07092
(908) 789-8900 Fax (908) 789-8922

www.chemtech.net

Chemtech Project Number

COC Number

22894

CLIENT INFORMATION

Report to be sent to:
COMPANY: ATC Group Services
ADDRESS:
CITY:
STATE: ZIP:
ATTENTION:
PHONE: FAX:

PROJECT INFORMATION

PROJECT NAME: PS 190-Brooklyn
PROJECT #: 2025SCA036 LOCATION: Brooklyn
PROJECT MANAGER: Olga Seldina
E-MAIL: olga.seldina@oneath.com
PHONE: 912.104.0619 FAX:
BILL TO: PO#
ADDRESS:
CITY: STATE: ZIP:
ATTENTION:
PHONE:

DATA TURNAROUND INFORMATION

FAX (RUSH) 5 days
HARDCOPY (DATA PACKAGE) _____
EDD: _____
STANDARD HARDCOPY TURNAROUND TIME IS 10 BUSINESS DAYS

DATA DELIVERABLE INFORMATION

☐ Level 1 (Results Only)
☐ Level 2 (Results + QC)
☐ Level 3 (Results + QC + Raw Data)
☐ EDD FORMAT

ANALYSIS

1 2 3 4 5 6 7 8 9
PRESERVATIVES

COMMENTS

CHEMTECH SAMPLE ID	PROJECT IDENTIFICATION	SAMPLE MATRIX	SAMPLE TYPE		DATE	TIME	# of Bottles	PRESERVATIVES											
			TYPE	COLLECTION				1	2	3	4	5	6	7	8	9			
1. 18131C - butyltin chloride - 600g		caustic	✓		8/16/00 PM														
2. 2A215 2C - 1000g		caustic	✓		8/16/00 12:30 PM														
3. 3A215 3C - 1000g		caustic	✓		8/16/00 1:15 PM														
4. 4A215 4C - 1000g		caustic	✓		8/16/00 1:15 PM														
5. 5A215 5C - 1000g		caustic	✓		8/16/00 1:15 PM														
6. 6A215 6C - 1000g		caustic	✓		8/16/00 1:15 PM														
7. 7A215 7C - 1000g		caustic	✓		8/16/00 1:15 PM														
8. 8A215 8C - 1000g		caustic	✓		8/16/00 1:15 PM														
9. 9A215 9C - 1000g		caustic	✓		8/16/00 1:15 PM														
10. 10A215 10C - 1000g		caustic	✓		8/16/00 1:15 PM														

CHEMTECH SAMPLE ID	PROJECT IDENTIFICATION	SAMPLE MATRIX	SAMPLE TYPE		DATE	TIME	# of Bottles	PRESERVATIVES											
			TYPE	COLLECTION				1	2	3	4	5	6	7	8	9			
1. 18131C - butyltin chloride - 600g		caustic	✓		8/16/00 PM														
2. 2A215 2C - 1000g		caustic	✓		8/16/00 12:30 PM														
3. 3A215 3C - 1000g		caustic	✓		8/16/00 1:15 PM														
4. 4A215 4C - 1000g		caustic	✓		8/16/00 1:15 PM														
5. 5A215 5C - 1000g		caustic	✓		8/16/00 1:15 PM														
6. 6A215 6C - 1000g		caustic	✓		8/16/00 1:15 PM														
7. 7A215 7C - 1000g		caustic	✓		8/16/00 1:15 PM														
8. 8A215 8C - 1000g		caustic	✓		8/16/00 1:15 PM														
9. 9A215 9C - 1000g		caustic	✓		8/16/00 1:15 PM														
10. 10A215 10C - 1000g		caustic	✓		8/16/00 1:15 PM														

SAMPLE CUSTODY MUST BE DOCUMENTED BELOW EACH TIME SAMPLES CHANGE PROSESSION INCLUDING COURIER DELIVERY

RELINQUISHED BY SAMPLER: Olga Seldina DATE/TIME: 8/15/05
RELINQUISHED BY: [Signature] DATE/TIME: 8/15/05
RECEIVED FOR LAB BY: [Signature] DATE/TIME: 8/15/05
RECEIVED BY: [Signature] DATE/TIME: 8/15/05
Comments: 21.1.5
Conditions of bottles or collars at receipt: ☐ COMPLIANT ☐ NON COMPLIANT ☐ COOLER TEMP 21.1.5
CLIENT: ☐ Hand Delivered ☐ Other: _____
CHEMTECH: ☐ Picked Up ☐ _____
Page _____ of _____

RELINQUISHED BY: _____ DATE/TIME: _____
RECEIVED FOR LAB BY: _____ DATE/TIME: _____
RECEIVED BY: _____ DATE/TIME: _____
Comments: _____
Conditions of bottles or collars at receipt: ☐ COMPLIANT ☐ NON COMPLIANT ☐ COOLER TEMP _____
CLIENT: ☐ Hand Delivered ☐ Other: _____
CHEMTECH: ☐ Picked Up ☐ _____
Page _____ of _____

10/20/21

WHITE - CHEMTECH COPY FOR RETURN TO CLIENT

YELLOW - CHEMTECH COPY

PINK - SAMPLER COPY

Laboratory Composite Sample log

Lab Project number: Q2894Date: 8-18-25Client Name: ATC Group ServicesClient Project Name: PS 190 - BrooklynInstructions: Composite all Samples (3:1)Sample Custodian: C. Peña

Client Sample ID	Weigh /Volume used	New ID	Sample Description	Sample Composite time	Comments
1A	2.48g	1A1B1C	Caulk	9:35	Total weight (7.44g)
1B	2.47g	↓	↓	↓	↓
1C	2.49g	↓	↓	↓	↓
2A	0.74g	2A2B2C		9:40	Total weight (2.22g)
2B	0.76g	↓	↓	↓	↓
2C	0.72g	↓	↓	↓	↓
3A	0.60g	3A3B3C		9:45	Total weight (1.80g)
3B	0.59g	↓	↓	↓	↓
3C	0.61g	↓	↓	↓	↓
4A	0.77g	4A4B4C		9:50	Total weight (2.33g)
4B	0.76g	↓	↓	↓	↓

Lab Project number: Q 2894

Date: 8-18-25

Client Name: ATC Group Services

Client Project Name : PS 190 - Brooklyn

Instructions: Composite all sample (3:1)

Sample Custodian: C. Peña

QA Control # A3041251

Laboratory Certification

Certified By	License No.
CAS EPA CLP Contract	68HERH20D0011
Connecticut	PH-0830
DOD ELAP (ANAB)	L2219
Maine	2024021
Maryland	296
New Hampshire	255424 Rev 1
New Jersey	20012
New York	11376
Pennsylvania	68-00548
Soil Permit	525-24-234-08441
Texas	TX-C25-00189
Virginia	460312