


Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP082225\
Data File : BP025543.D
Acq On : 22 Aug 2025 10:08
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP081425.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Thu Aug 14 18:14:31 2025

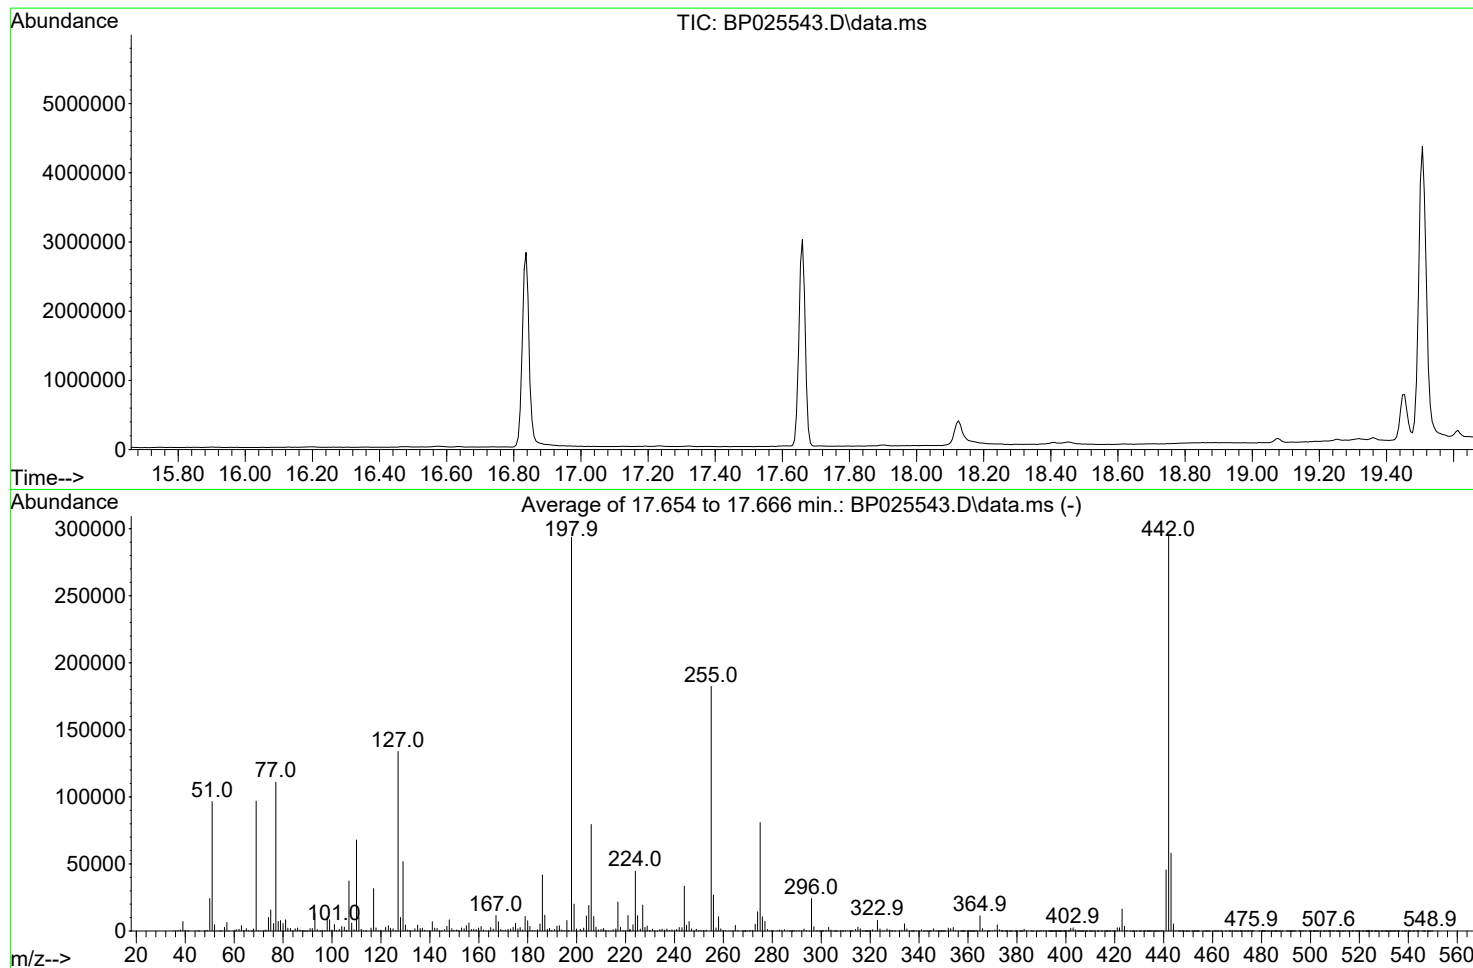

AutoFind: Scans 2502, 2503, 2504; Background Corrected with Scan 2494

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
68	69	0.00	2	1.6	1519	PASS
69	69	100	100	100.0	96945	PASS
70	69	0.00	2	0.4	396	PASS
197	198	0.00	2	0.2	468	PASS
198	198	100	100	100.0	293657	PASS
199	198	5	9	6.8	20111	PASS
365	198	1	100	3.8	11295	PASS
441	443	0.01	150	78.6	45599	PASS
442	442	100	100	100.0	294439	PASS
443	442	15	24	19.7	58043	PASS

DDT Breakdown




Date	Instrument Name	DFTPP Data File
8/22/2025	BNA_P	<u>BP025543.D</u>
Compound Name	Response	Retention Time
DDT	1433027	20.801
DDD	19562	20.348
DDE	2885	19.813
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
22447	1455474	1.54

Instrument :
BNA_P
ClientSampleId :
DFTPP

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP082225\
Data File : BP025543.D
Acq On : 22 Aug 2025 10:08
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DFTPP

Quant Time: Aug 22 10:56:13 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP081425.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Aug 14 18:14:31 2025
Response via : Initial Calibration

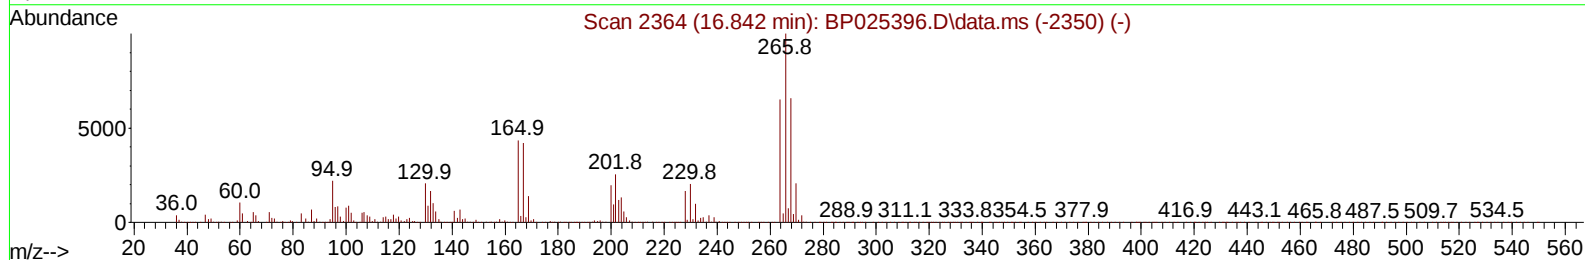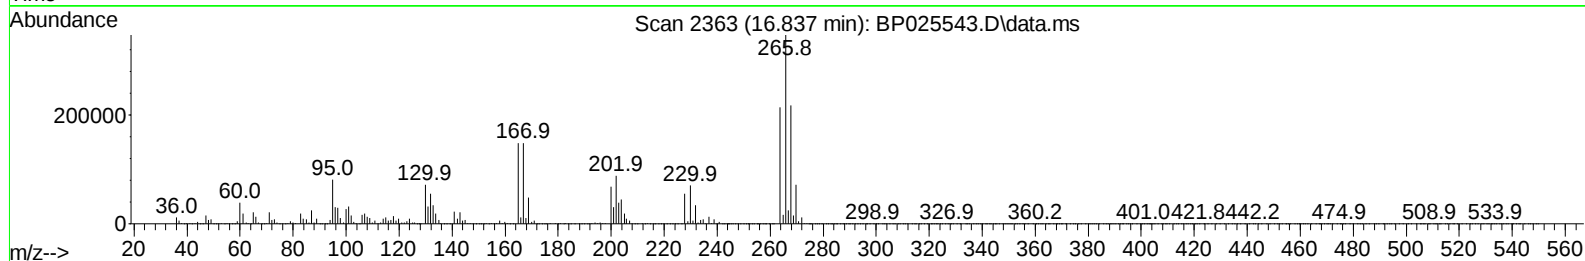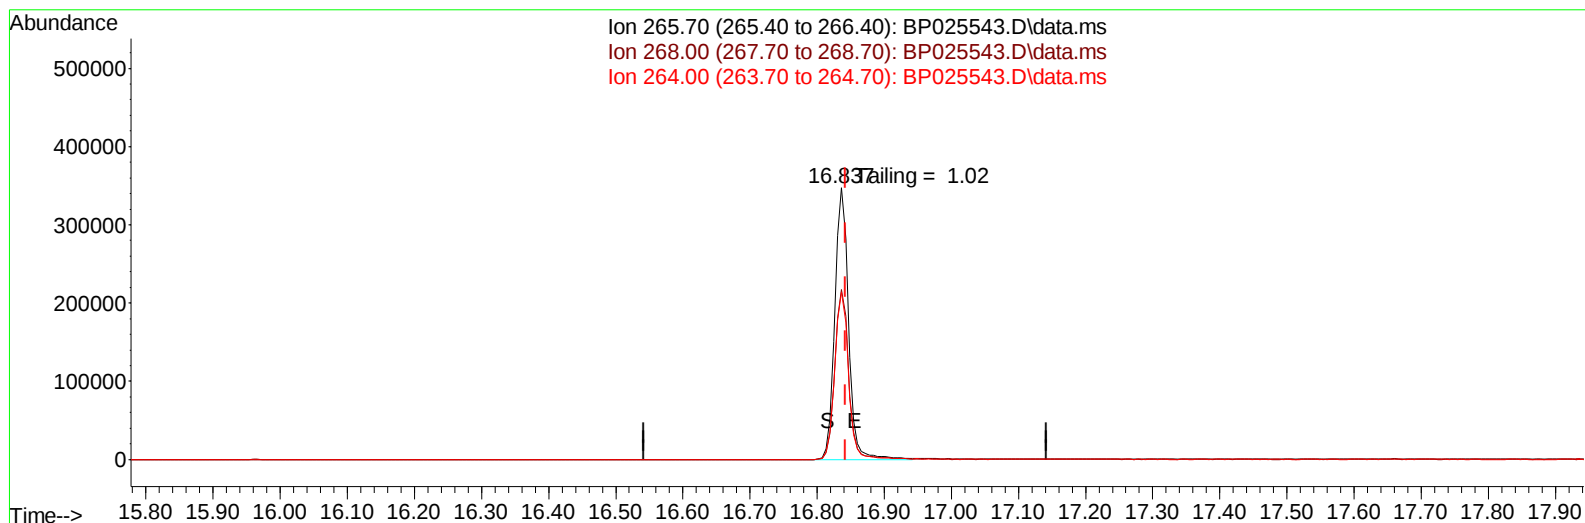

TIC: BP025543.D\data.ms

(70) Pentachlorophenol (C)

16.837min (-0.006) 24379.55 ng




response 490511

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	65.80	62.65
264.00	65.00	61.62
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP082225\
Data File : BP025543.D
Acq On : 22 Aug 2025 10:08
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DFTPP

Quant Time: Aug 22 10:56:13 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP081425.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Aug 14 18:14:31 2025
Response via : Initial Calibration

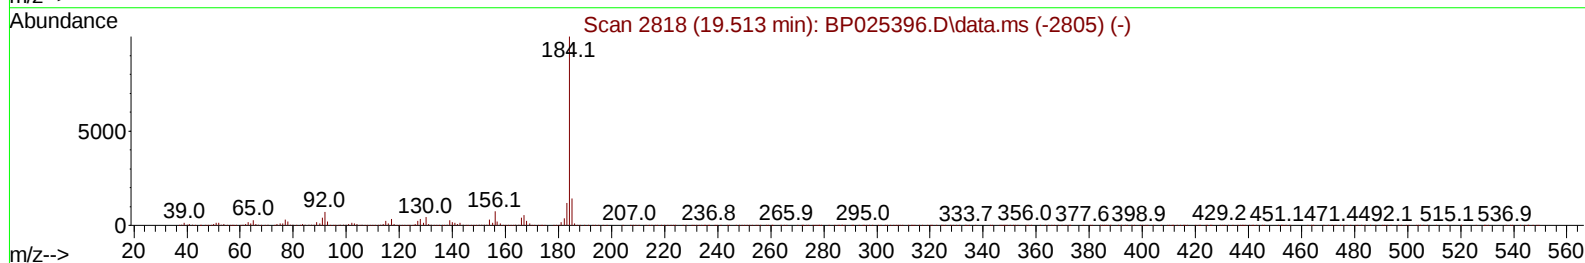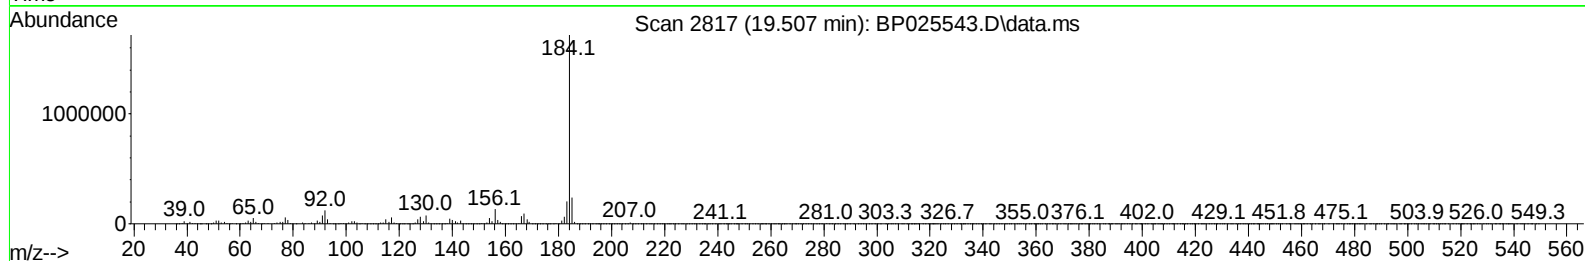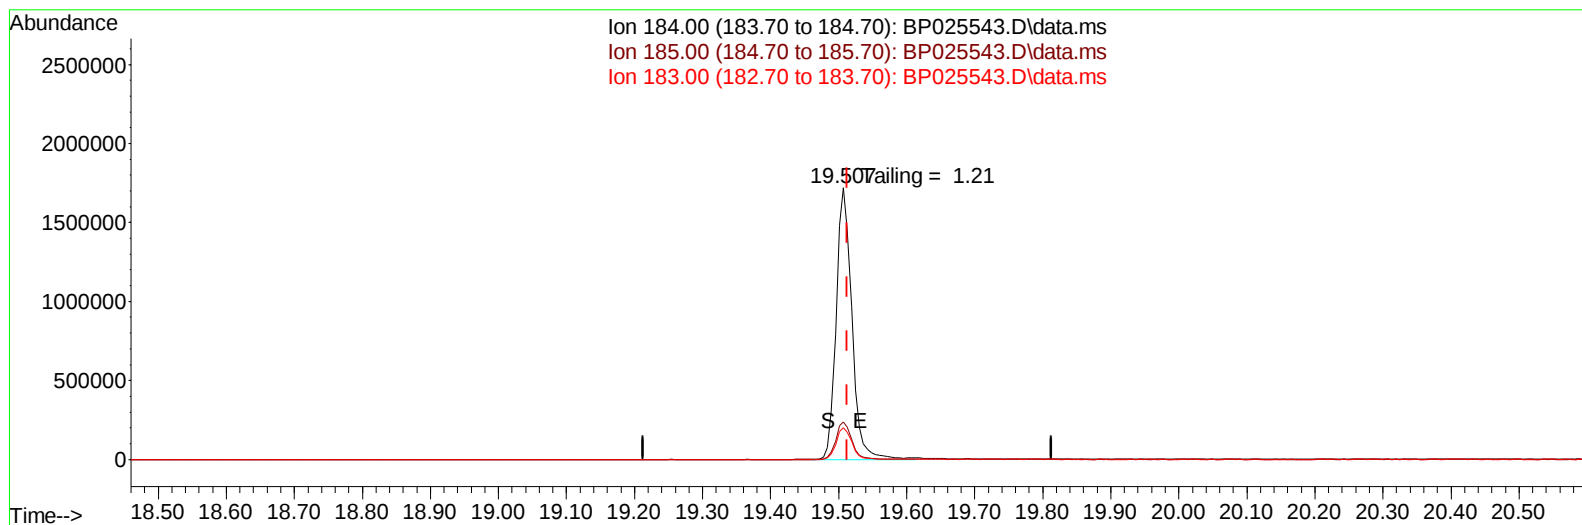

TIC: BP025543.D\data.ms

(77) Benzidine

19.507min (-0.006) 16182.04 ng

response 2751355

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.40	13.92
183.00	11.80	11.76
0.00	0.00	0.00