

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF082225\
 Data File : BF143566.D
 Acq On : 22 Aug 2025 12:02
 Operator : RC/JU
 Sample : Q2903-01
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 MW-6A-081925

Quant Time: Aug 22 12:23:59 2025
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF082025.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Aug 21 06:12:21 2025
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	6.922	152	108481	20.000	ng	0.00
21) Naphthalene-d8	8.204	136	426866	20.000	ng	0.00
39) Acenaphthene-d10	9.963	164	257748	20.000	ng	0.00
64) Phenanthrene-d10	11.451	188	457617	20.000	ng	0.00
76) Chrysene-d12	14.098	240	250701	20.000	ng	0.00
86) Perylene-d12	15.592	264	223630	20.000	ng	0.00
System Monitoring Compounds						
5) 2-Fluorophenol	5.563	112	438580	70.596	ng	0.00
7) Phenol-d6	6.557	99	372380	48.556	ng	-0.02
23) Nitrobenzene-d5	7.487	82	720621	98.513	ng	-0.01
42) 2,4,6-Tribromophenol	10.757	330	408642	170.320	ng	0.00
45) 2-Fluorobiphenyl	9.281	172	1337994	85.792	ng	0.00
79) Terphenyl-d14	13.039	244	1549381	107.847	ng	0.00


Target Compounds	Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF082225\
Data File : BF143566.D
Acq On : 22 Aug 2025 12:02
Operator : RC/JU
Sample : Q2903-01
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
MW-6A-081925

Quant Time: Aug 22 12:23:59 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF082025.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Aug 21 06:12:21 2025
Response via : Initial Calibration




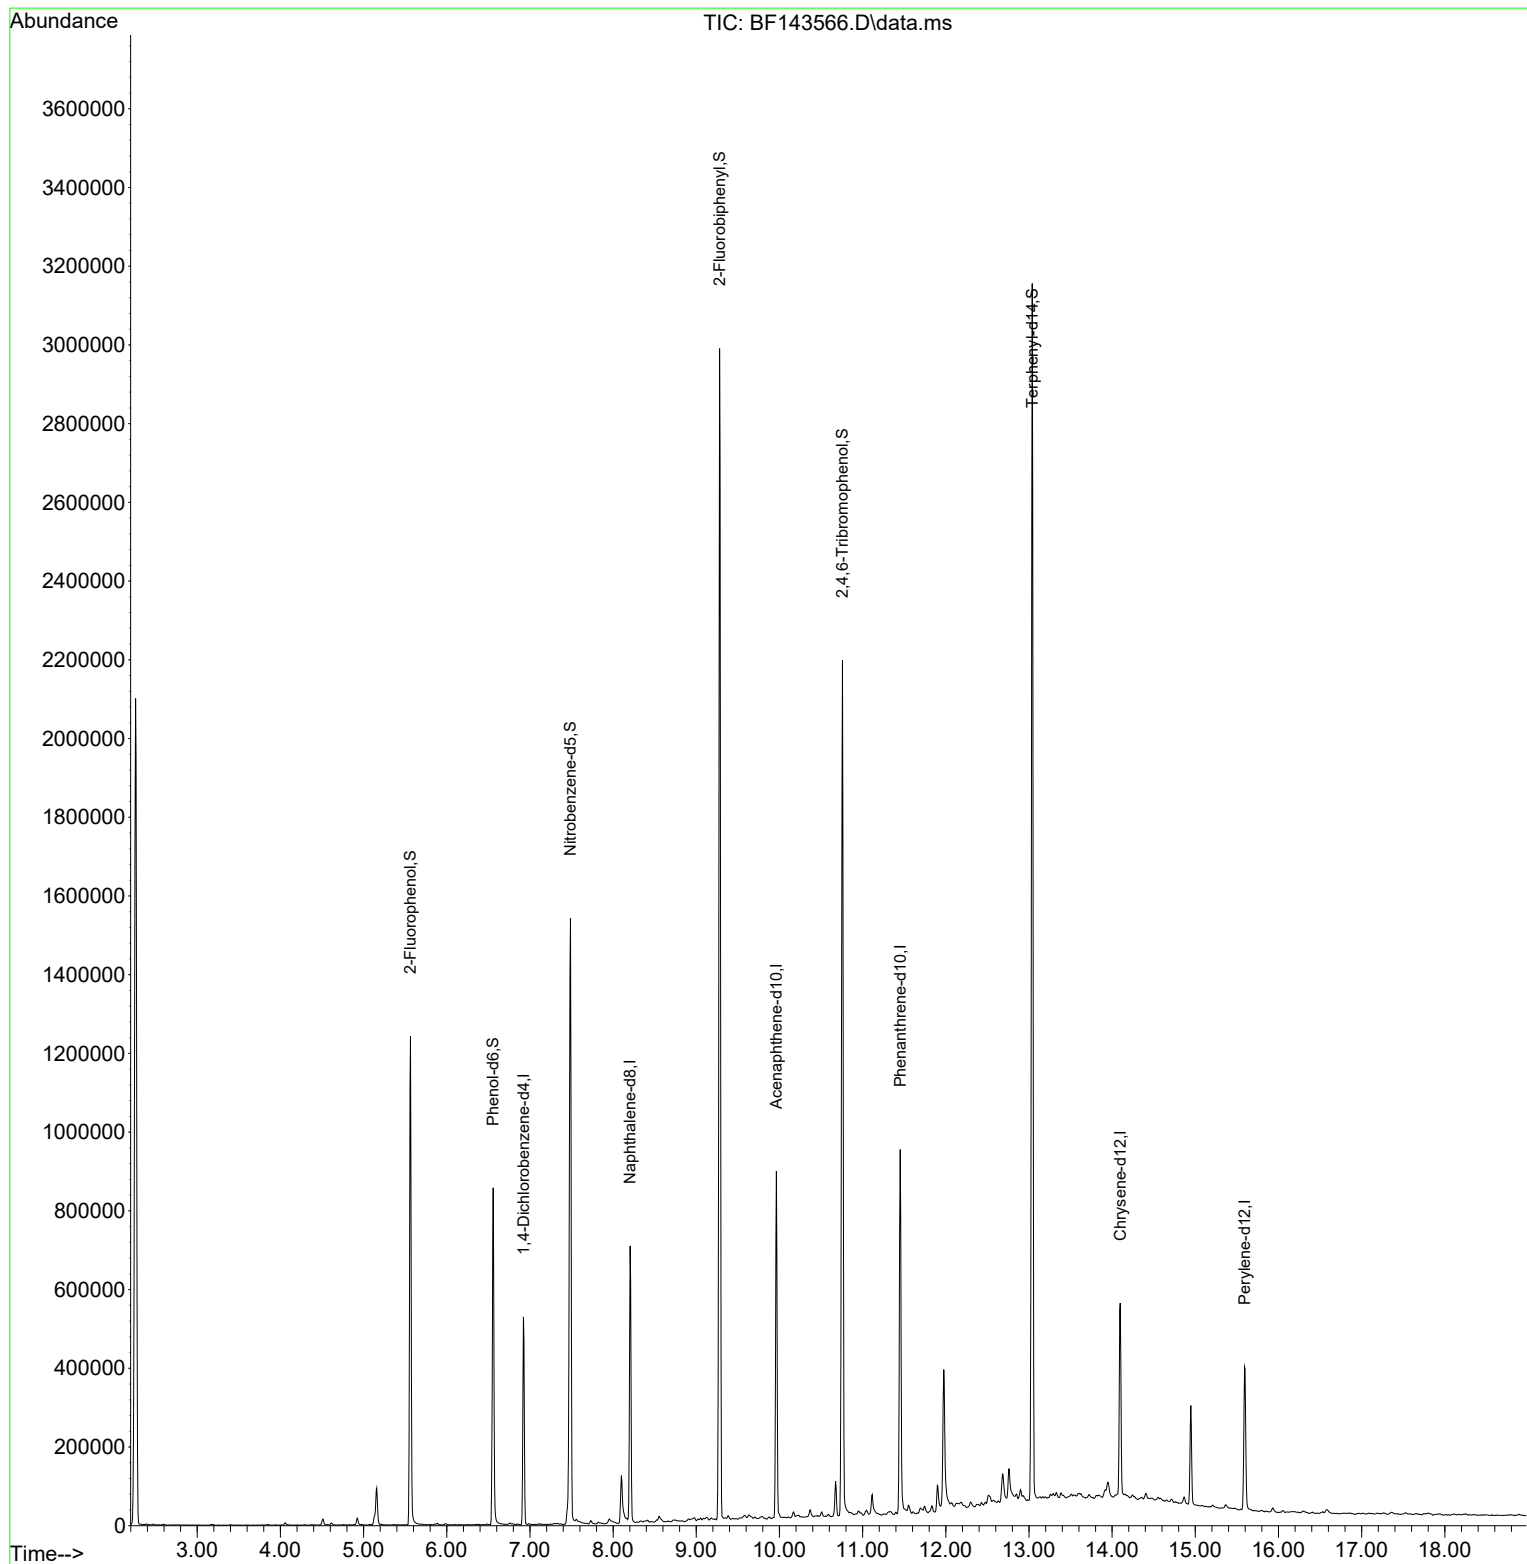


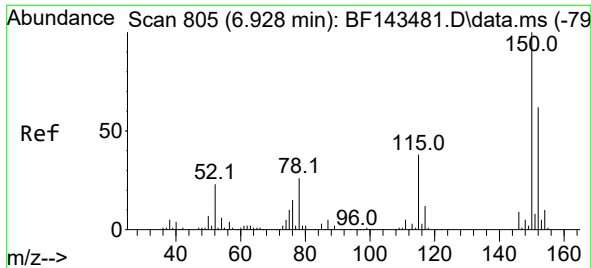

#1
1,4-Dichlorobenzene-d4
Concen: 20.000 ng
RT: 6.922 min Scan# 805
Delta R.T. -0.006 min
Lab File: BF143566.D
Acq: 22 Aug 2025 12:02




Instrument :
BNA_F
ClientSampleId :
MW-6A-081925


Tgt Ion:152 Resp: 108481
Ion Ratio Lower Upper
152 100
150 156.4 128.9 193.3
115 62.9 49.2 73.8

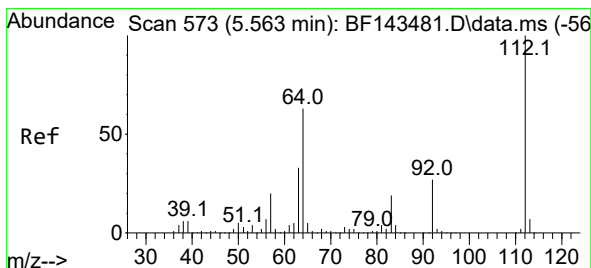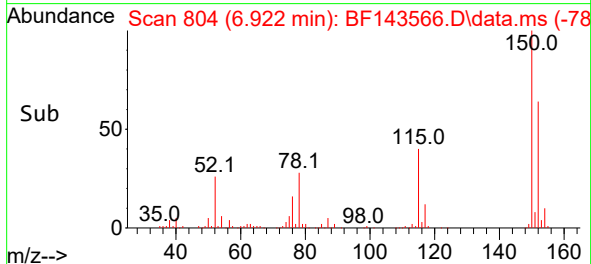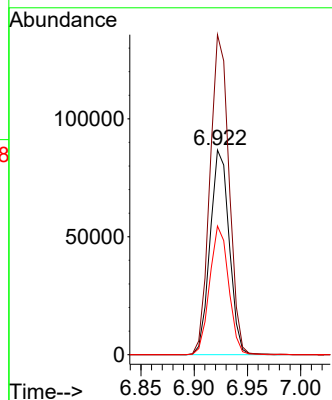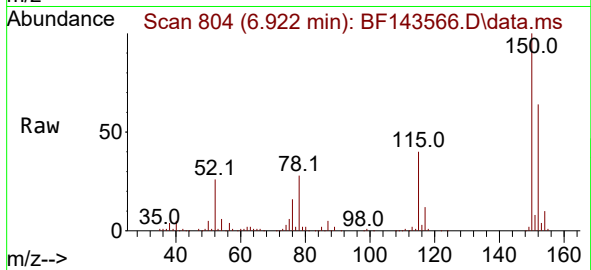

#5
2-Fluorophenol
Concen: 70.596 ng
RT: 5.563 min Scan# 573
Delta R.T. -0.000 min
Lab File: BF143566.D
Acq: 22 Aug 2025 12:02

Tgt Ion:112 Resp: 438580
Ion Ratio Lower Upper
112 100
64 65.2 50.4 75.6
63 34.5 26.4 39.6


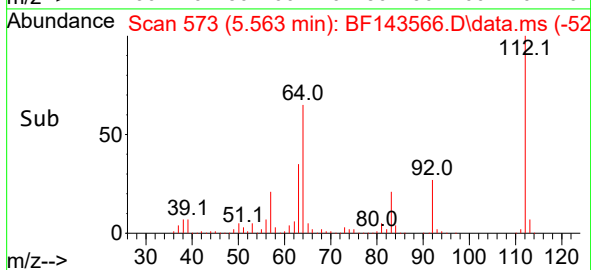
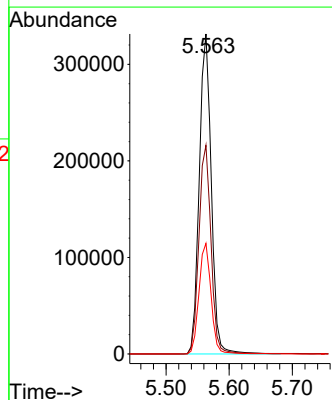
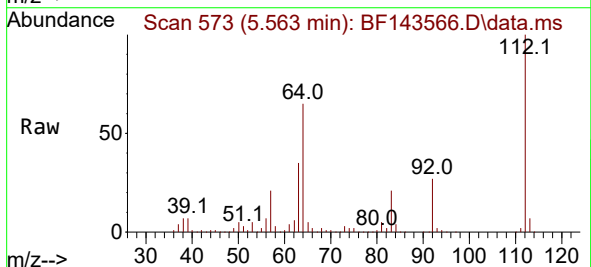


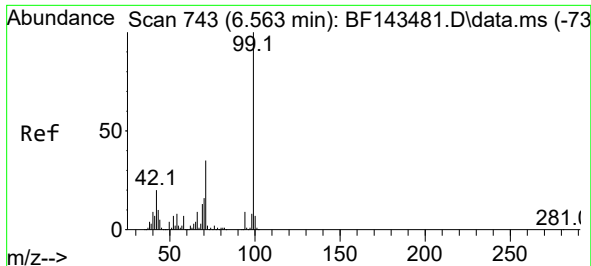

#7
Phenol-d6
Concen: 48.556 ng
RT: 6.557 min Scan# 74
Delta R.T. -0.018 min
Lab File: BF143566.D
Acq: 22 Aug 2025 12:02




Instrument :
BNA_F
ClientSampleId :
MW-6A-081925


Tgt Ion: 99 Resp: 372380
Ion Ratio Lower Upper
99 100
42 21.0 16.3 24.5
71 38.4 28.2 42.2

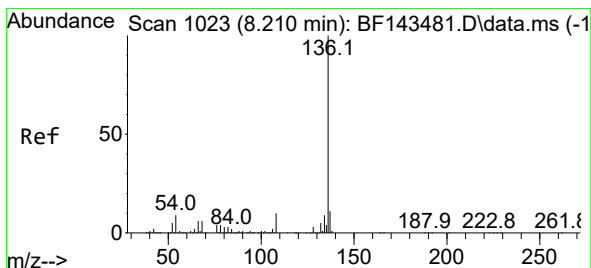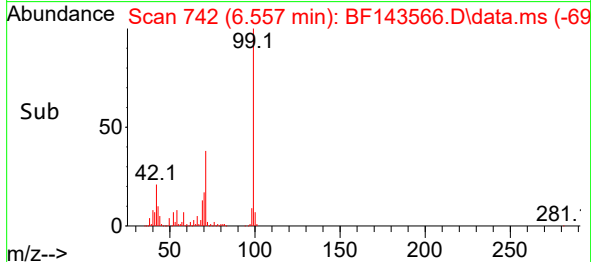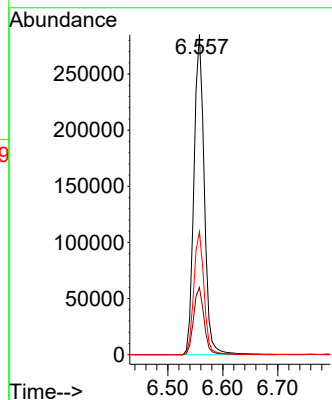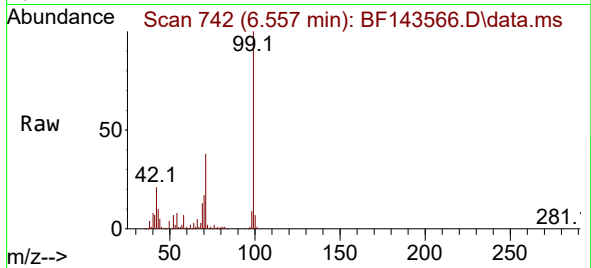

#21
Naphthalene-d8
Concen: 20.000 ng
RT: 8.204 min Scan# 1022
Delta R.T. -0.006 min
Lab File: BF143566.D
Acq: 22 Aug 2025 12:02

Tgt Ion: 136 Resp: 426866
Ion Ratio Lower Upper
136 100
137 11.0 9.0 13.4
54 9.2 7.4 11.2
68 5.6 5.0 7.4


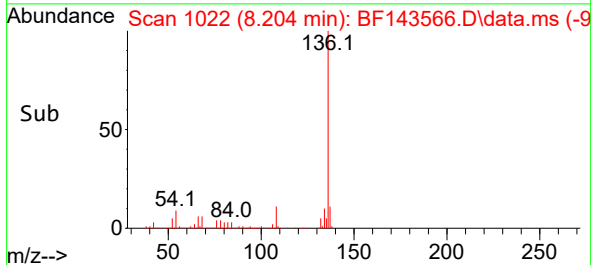
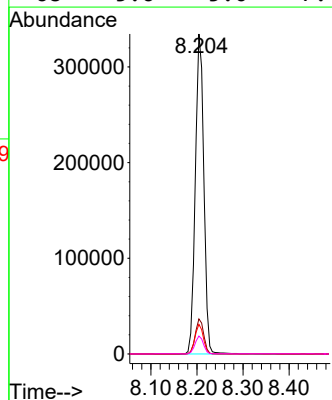
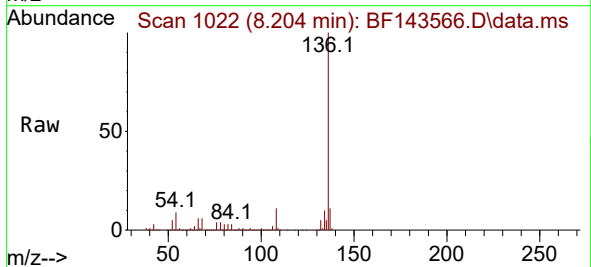


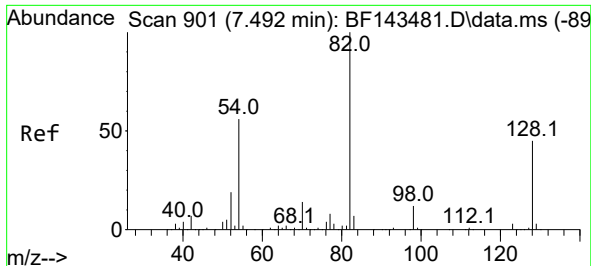

#23
 Nitrobenzene-d5
 Concen: 98.513 ng
 RT: 7.487 min Scan# 901
 Delta R.T. -0.012 min
 Lab File: BF143566.D
 Acq: 22 Aug 2025 12:02




Instrument :
 BNA_F
 ClientSampleId :
 MW-6A-081925


Tgt Ion: 82 Resp: 720621
 Ion Ratio Lower Upper
 82 100
 128 42.8 35.5 53.3
 54 56.2 44.3 66.5

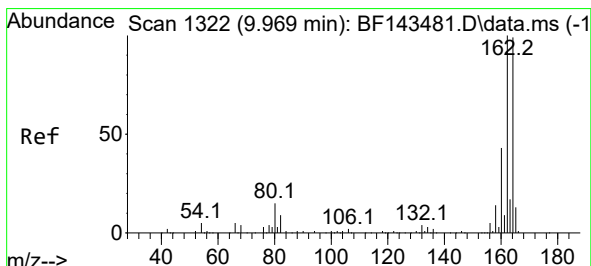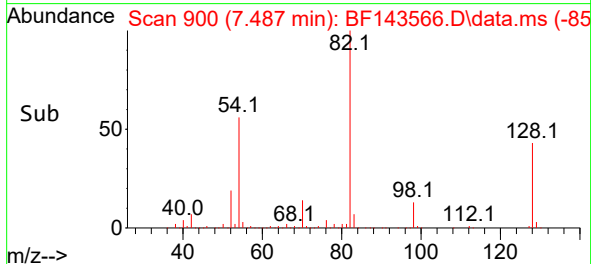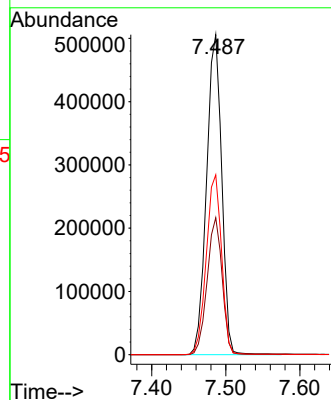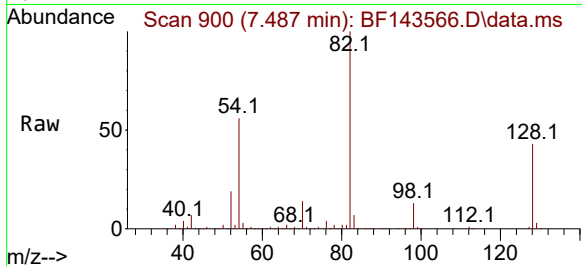

#39
 Acenaphthene-d10
 Concen: 20.000 ng
 RT: 9.963 min Scan# 1321
 Delta R.T. -0.006 min
 Lab File: BF143566.D
 Acq: 22 Aug 2025 12:02

Tgt Ion:164 Resp: 257748
 Ion Ratio Lower Upper
 164 100
 162 101.6 80.5 120.7
 160 42.7 34.3 51.5


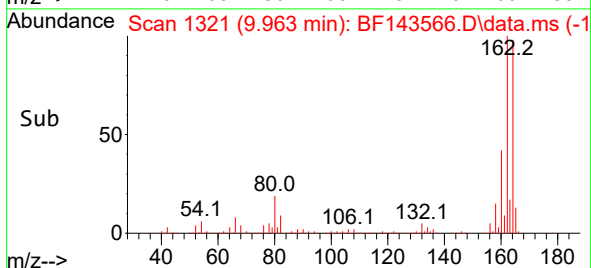
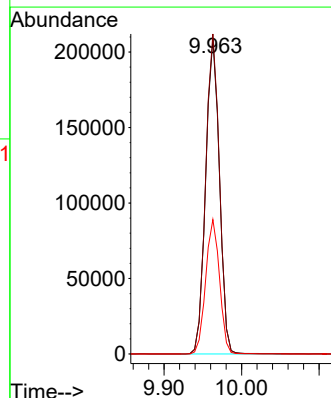
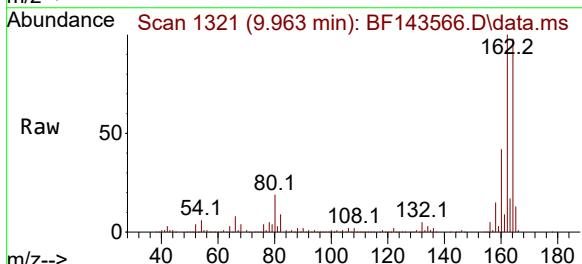


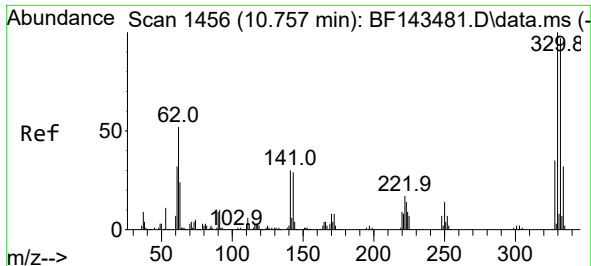

#42
2,4,6-Tribromophenol
Concen: 170.320 ng
RT: 10.757 min Scan# 1456
Delta R.T. -0.006 min
Lab File: BF143566.D
Acq: 22 Aug 2025 12:02




Instrument :
BNA_F
ClientSampleId :
MW-6A-081925


Tgt Ion:330 Resp: 408642
Ion Ratio Lower Upper
330 100
332 96.6 78.0 117.0
141 28.9 23.7 35.5

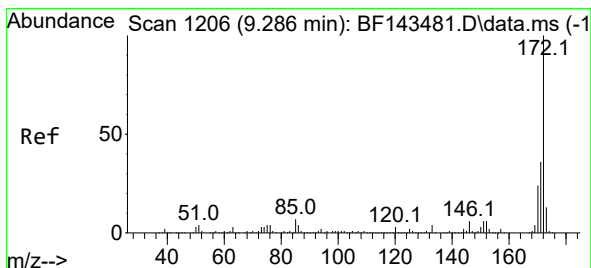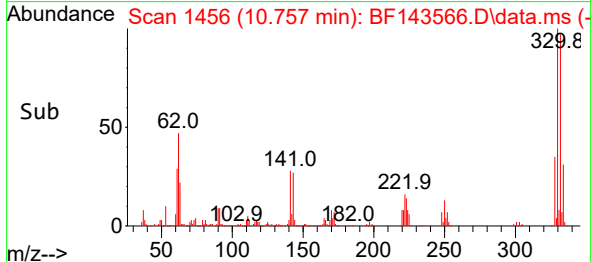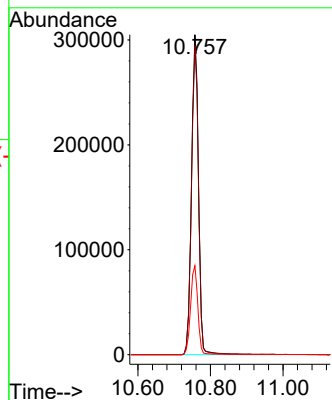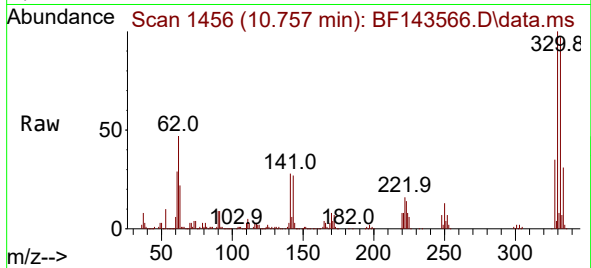

#45
2-Fluorobiphenyl
Concen: 85.792 ng
RT: 9.281 min Scan# 1205
Delta R.T. -0.006 min
Lab File: BF143566.D
Acq: 22 Aug 2025 12:02

Tgt Ion:172 Resp: 1337994
Ion Ratio Lower Upper
172 100
171 36.1 28.8 43.2
170 23.9 18.8 28.2


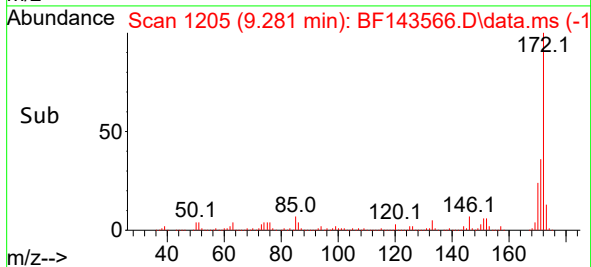
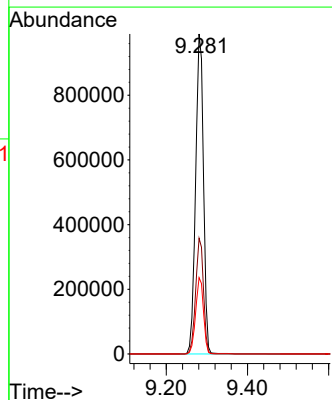
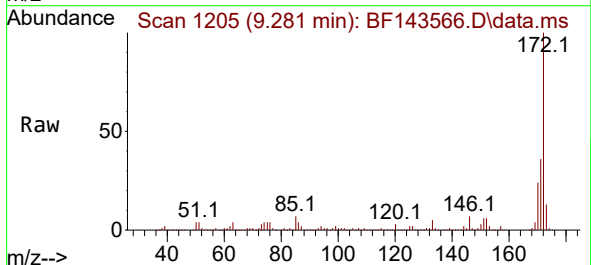


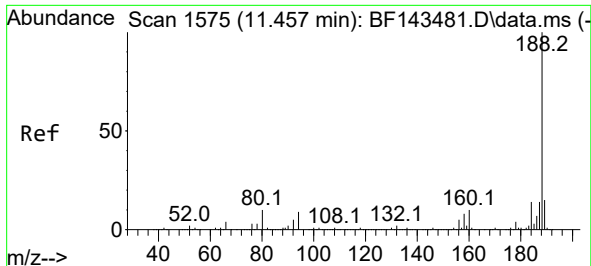

#64
Phenanthrene-d10
Concen: 20.000 ng
RT: 11.451 min Scan# 1
Delta R.T. -0.006 min
Lab File: BF143566.D
Acq: 22 Aug 2025 12:02




Instrument :
BNA_F
ClientSampleId :
MW-6A-081925


Tgt Ion:188 Resp: 457617
Ion Ratio Lower Upper
188 100
94 9.4 7.4 11.2
80 10.3 8.2 12.4

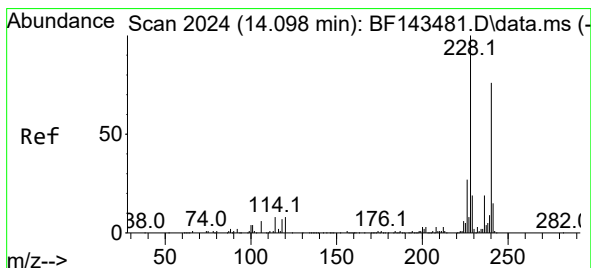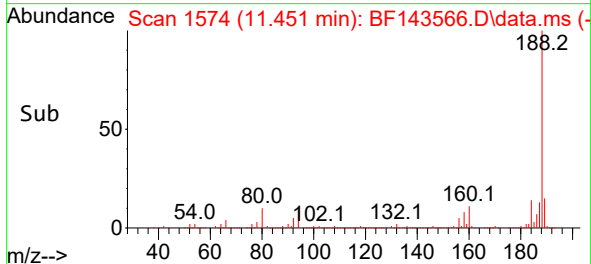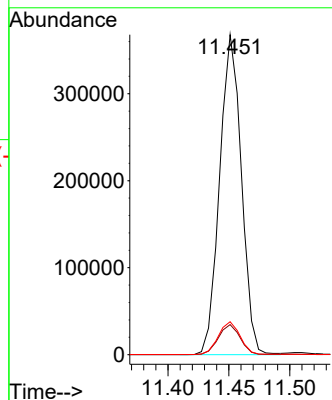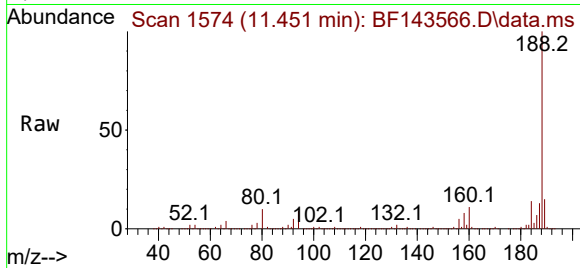

#76
Chrysene-d12
Concen: 20.000 ng
RT: 14.098 min Scan# 2024
Delta R.T. -0.006 min
Lab File: BF143566.D
Acq: 22 Aug 2025 12:02

Tgt Ion:240 Resp: 250701
Ion Ratio Lower Upper
240 100
120 9.1 8.6 12.8
236 25.1 20.4 30.6


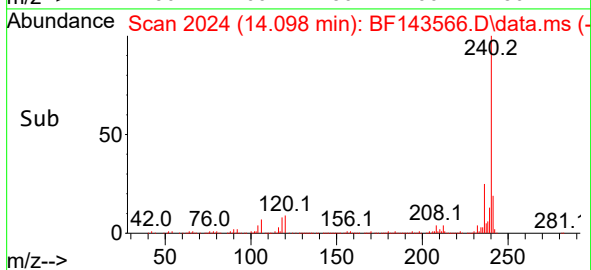
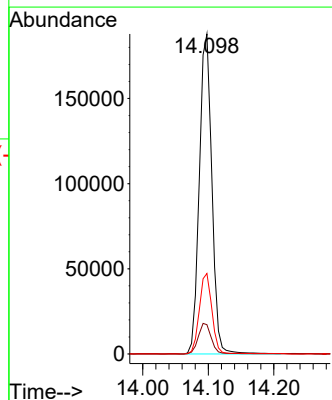
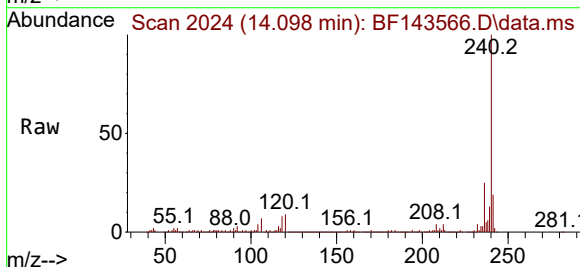


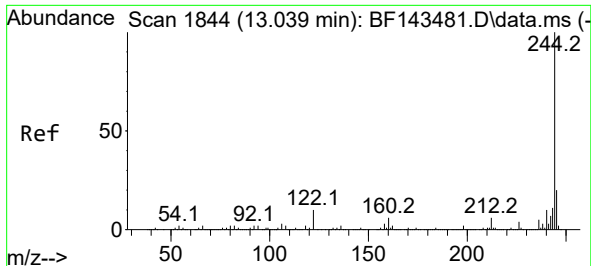

#79
 Terphenyl-d14
 Concen: 107.847 ng
 RT: 13.039 min Scan# 1844
 Delta R.T. -0.000 min
 Lab File: BF143566.D
 Acq: 22 Aug 2025 12:02

Instrument :
 BNA_F
 ClientSampleId :
 MW-6A-081925

Tgt Ion:244 Resp: 1549381
 Ion Ratio Lower Upper
 244 100
 212 7.1 5.2 7.8
 122 9.7 7.9 11.9

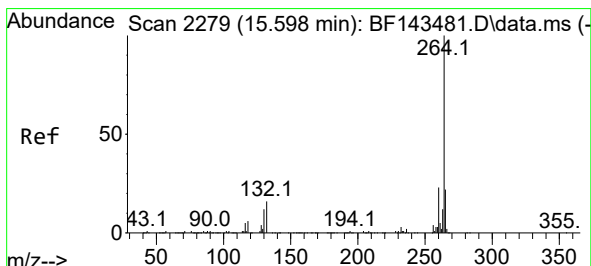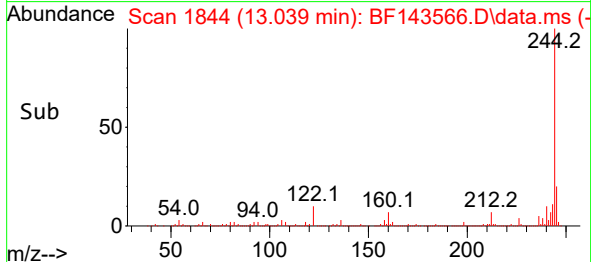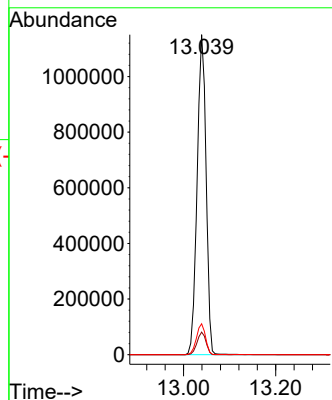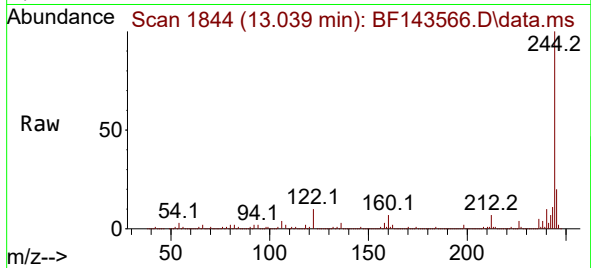

#86
 Perylene-d12
 Concen: 20.000 ng
 RT: 15.592 min Scan# 2278
 Delta R.T. -0.006 min
 Lab File: BF143566.D
 Acq: 22 Aug 2025 12:02

Tgt Ion:264 Resp: 223630
 Ion Ratio Lower Upper
 264 100
 260 23.3 18.7 28.1
 265 21.3 17.6 26.4

