

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP082525\
 Data File : PP074634.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 25 Aug 2025 12:04
 Operator : YP\AJ
 Sample : Q2911-12
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 K262-4C

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 08/26/2025
 Supervised By :mohammad ahmed 08/27/2025

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 25 12:39:13 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP081925.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Aug 20 06:20:44 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.660	3.803	21079297	66393103	17.226m	13.731
2) SA Decachlor...	10.445	8.810	15428244	211.4E6	15.623m	28.185 #

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP082525\
Data File : PP074634.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 25 Aug 2025 12:04
Operator : YP\AJ
Sample : Q2911-12
Misc :
ALS Vial : 11 Sample Multiplier: 1



Instrument :
ECD_P
ClientSampleId :
K262-4C


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 08/26/2025
Supervised By :mohammad ahmed 08/27/2025

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 25 12:39:13 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP081925.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Aug 20 06:20:44 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

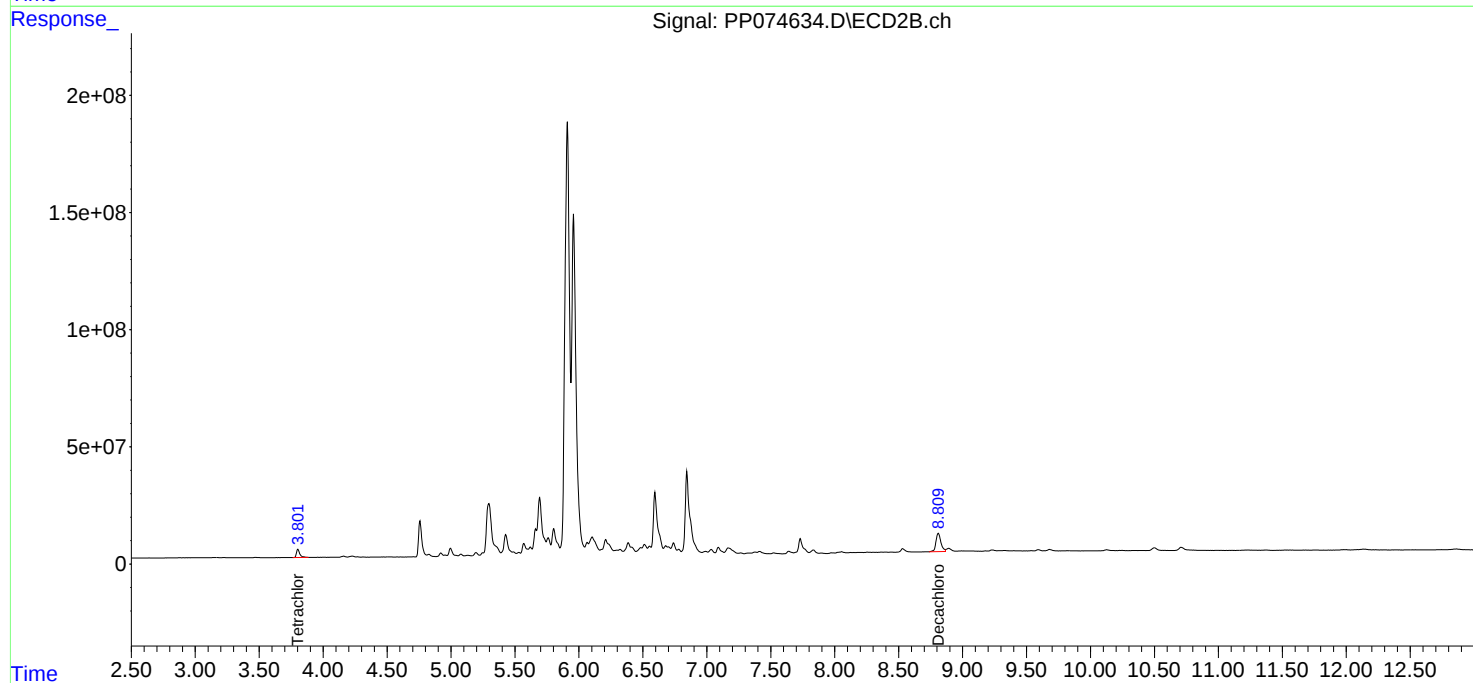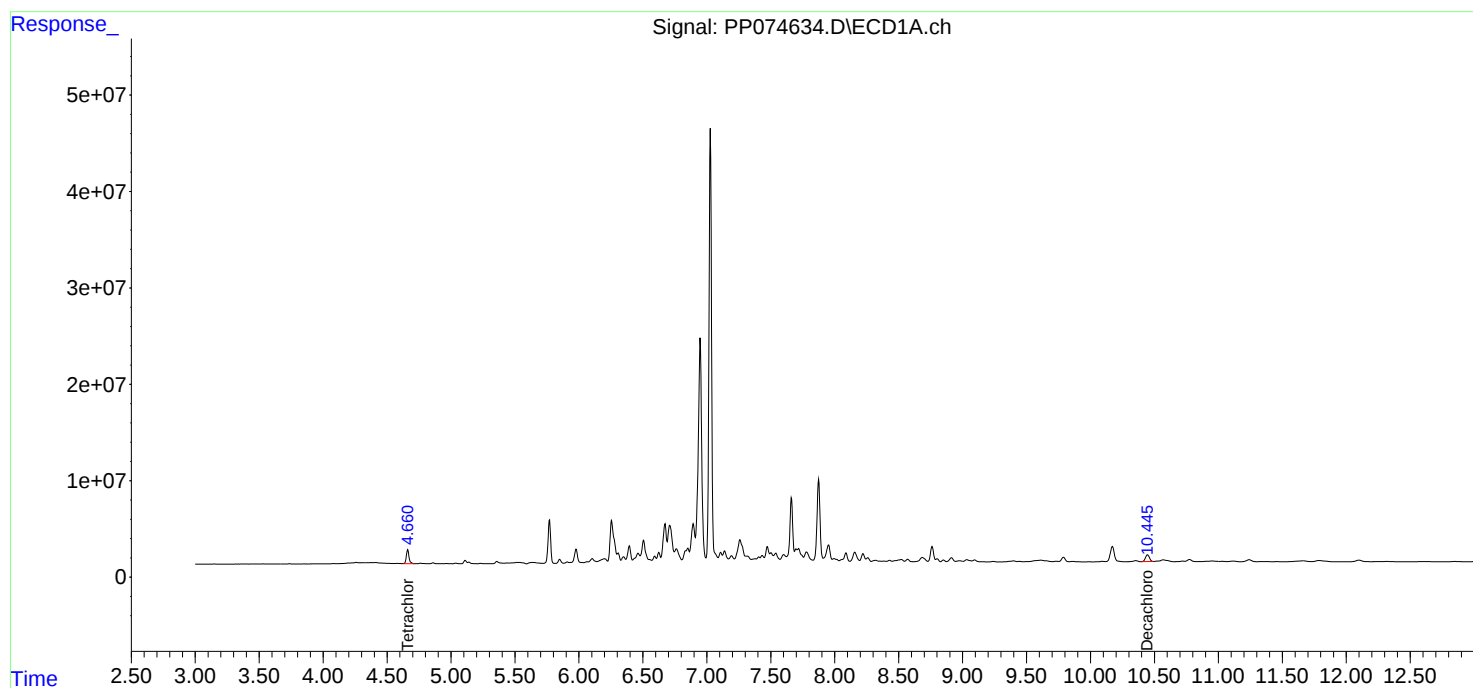

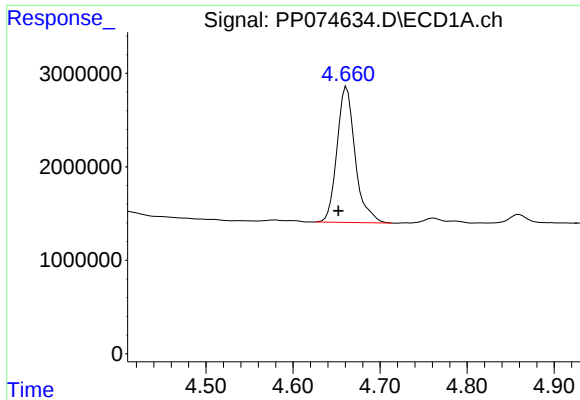


#1 Tetrachloro-m-xylene

R.T.: 4.660 min
Delta R.T.: 0.008 min
Response: 21079297
Conc: 17.23 ng/ml

Instrument :
ECD_P
ClientSampleId :
K262-4C


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 08/26/2025
Supervised By :mohammad ahmed 08/27/2025

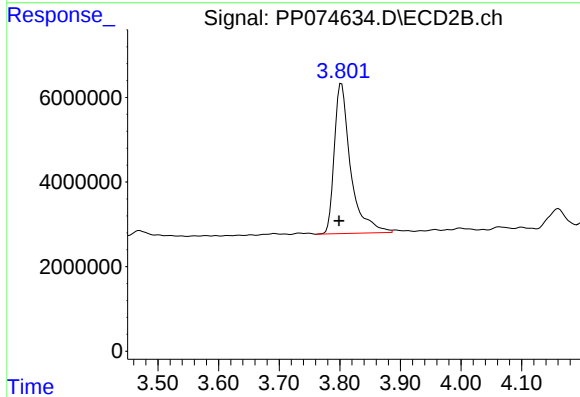


#1 Tetrachloro-m-xylene

R.T.: 3.803 min
Delta R.T.: 0.004 min
Response: 66393103
Conc: 13.73 ng/ml

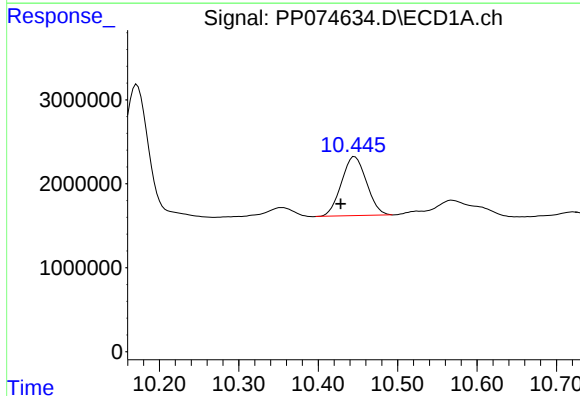

#2 Decachlorobiphenyl

R.T.: 10.445 min
Delta R.T.: 0.016 min
Response: 15428244
Conc: 15.62 ng/ml m

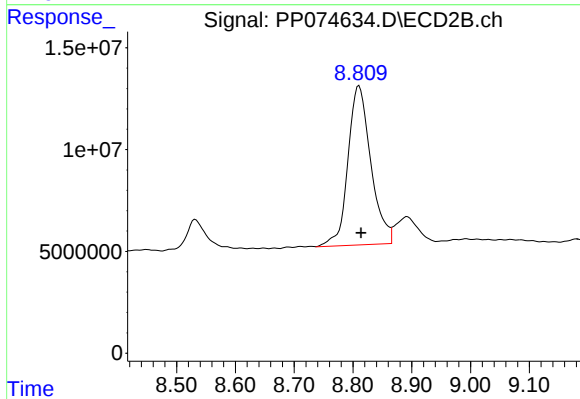

#2 Decachlorobiphenyl

R.T.: 8.810 min
Delta R.T.: -0.004 min
Response: 211367342
Conc: 28.19 ng/ml