


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF082625\
Data File : BF143584.D
Acq On : 26 Aug 2025 08:36
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF082625.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Tue Aug 26 16:30:52 2025

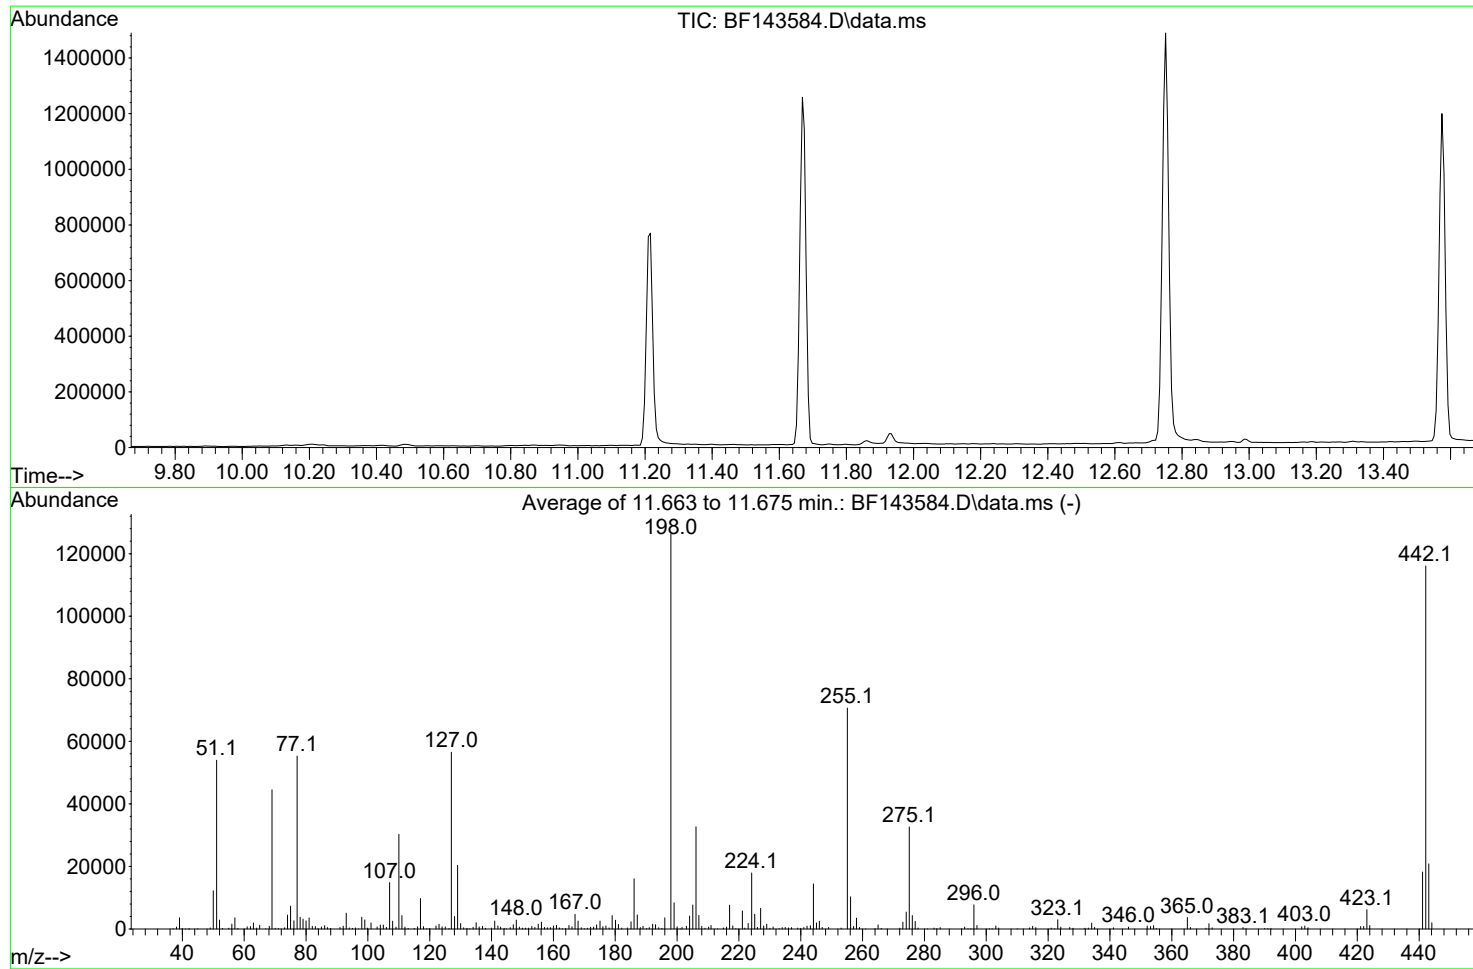

AutoFind: Scans 1610, 1611, 1612; Background Corrected with Scan 1604

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
68	69	0.00	2	1.9	866	PASS
69	69	100	100	100.0	44507	PASS
70	69	0.00	2	0.6	286	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	126253	PASS
199	198	5	9	6.7	8415	PASS
365	198	1	100	2.9	3677	PASS
441	443	0.01	150	87.5	18206	PASS
442	442	100	100	100.0	116075	PASS
443	442	15	24	17.9	20814	PASS

DDT Breakdown




Date	Instrument Name	DFTPP Data File
8/26/2025	BNA_F	<u>BF143584.D</u>
Compound Name	Response	Retention Time
DDT	230164	13.574
DDD	919	13.31
DDE	0	12.974
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
919	231083	0.40

Instrument :
BNA_F
ClientSampleId :
DFTPP

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF082625\
Data File : BF143584.D
Acq On : 26 Aug 2025 08:36
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Aug 26 16:49:14 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF082625.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Aug 26 16:30:52 2025
Response via : Initial Calibration

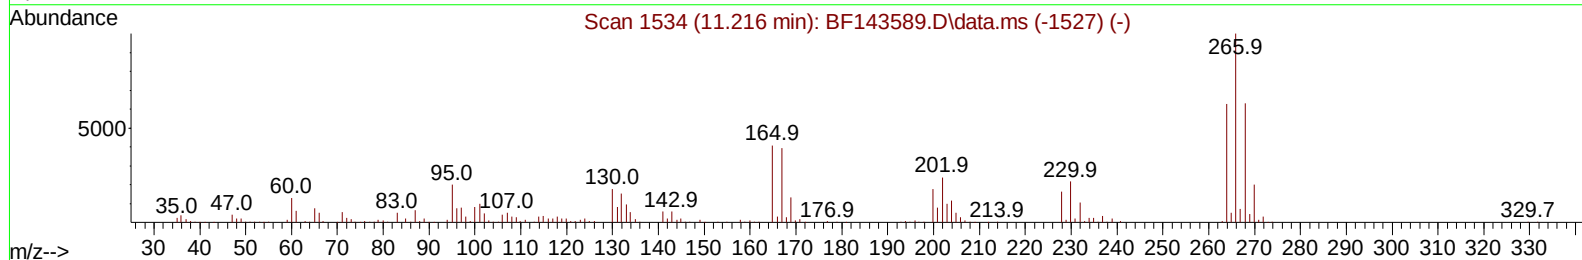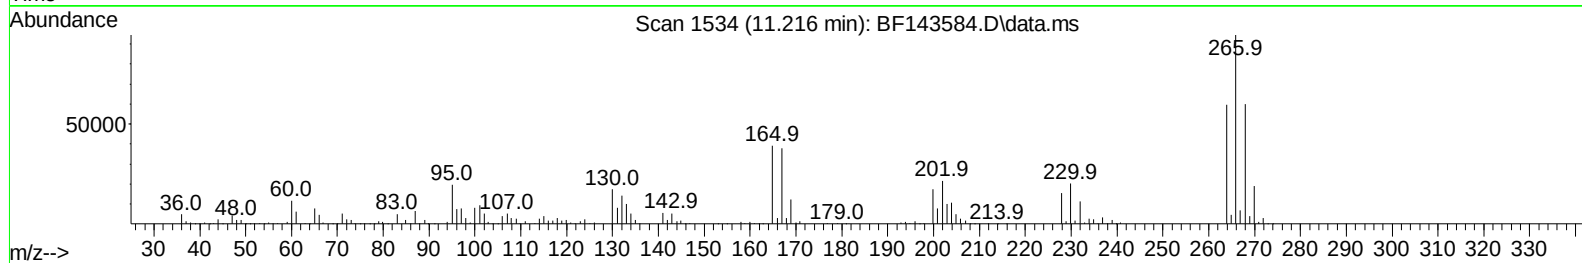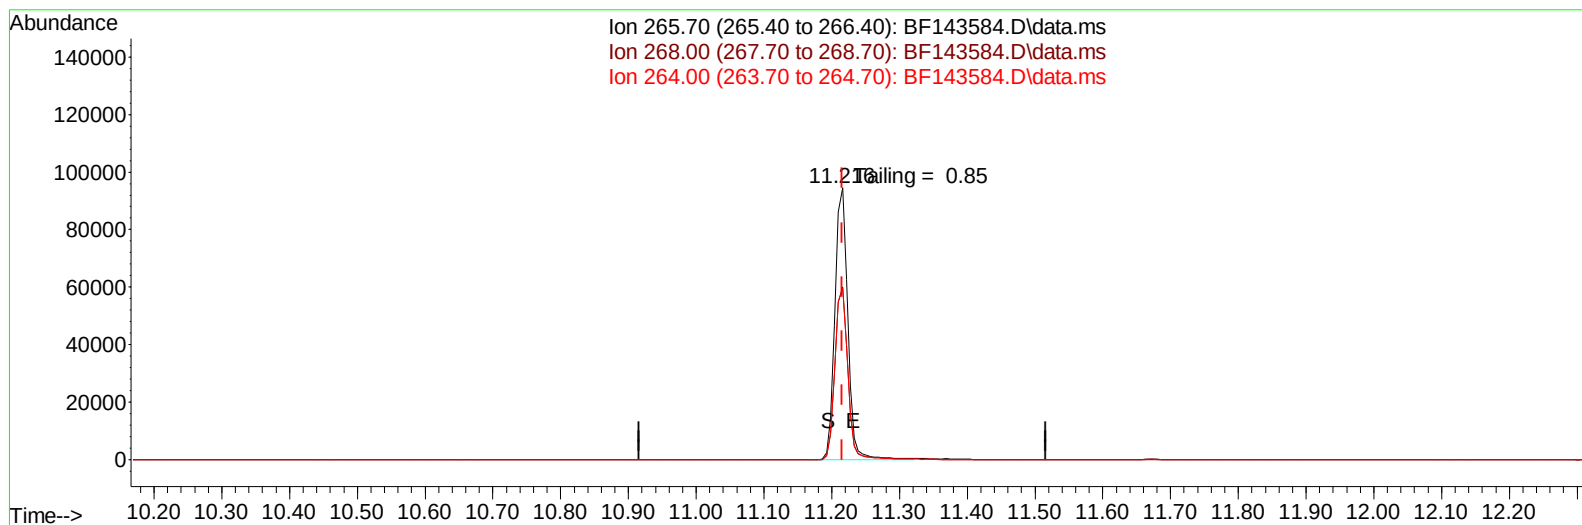

TIC: BF143584.D\data.ms

(70) Pentachlorophenol (C)

11.216min (-0.000) 43843.49 ng




response 124332

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.00	63.55
264.00	62.60	63.20
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF082625\
Data File : BF143584.D
Acq On : 26 Aug 2025 08:36
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Aug 26 16:49:14 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF082625.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Aug 26 16:30:52 2025
Response via : Initial Calibration

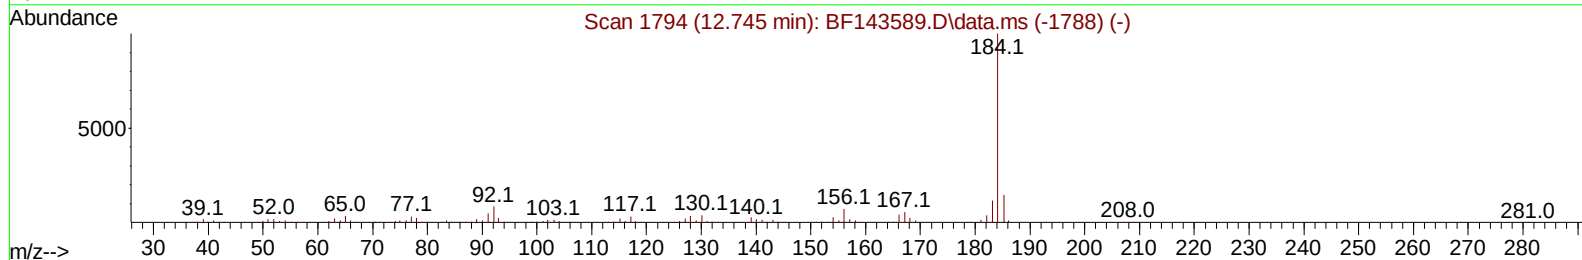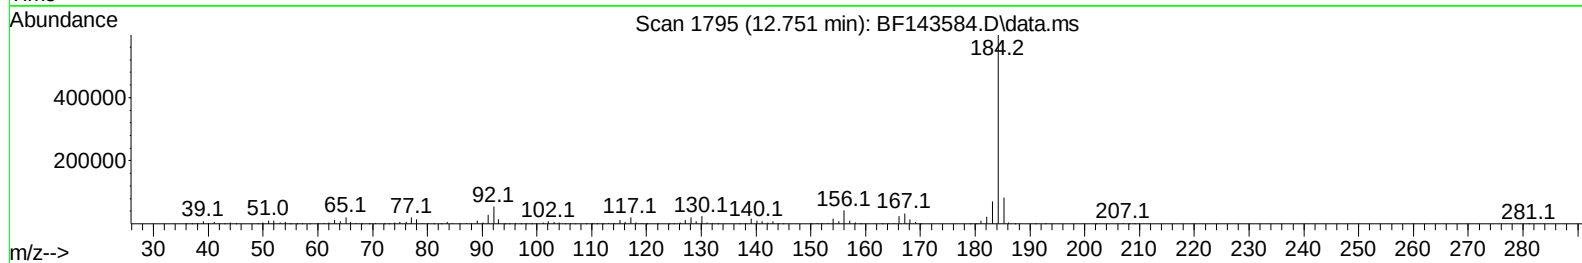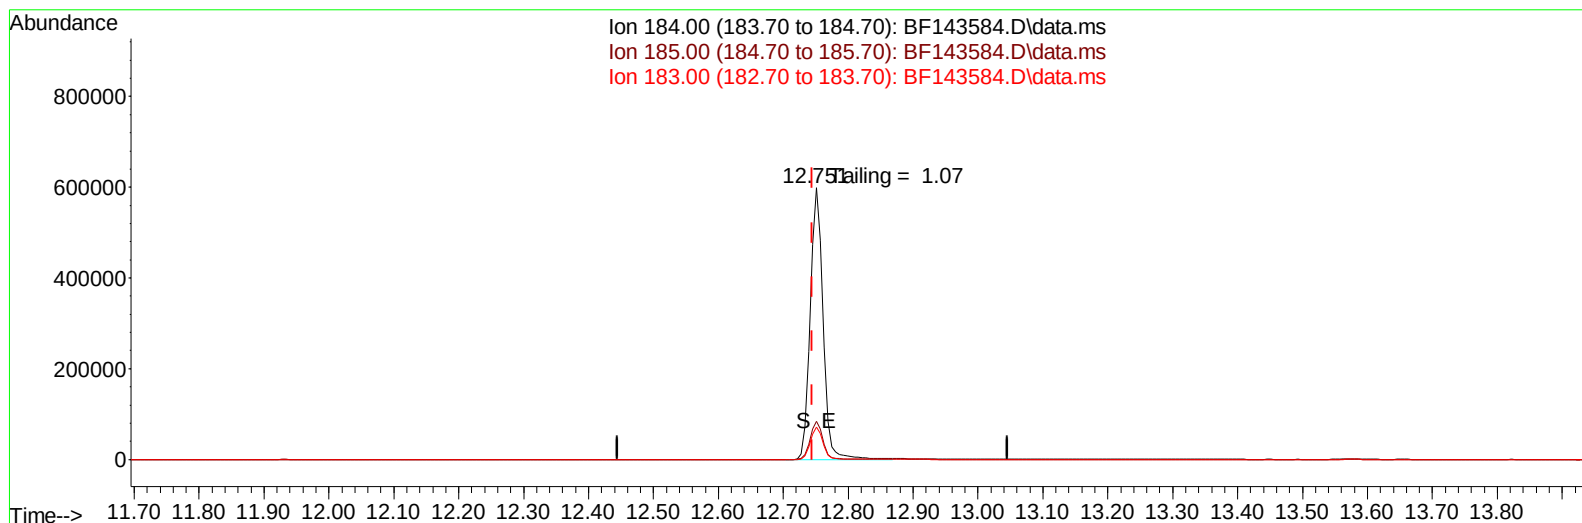

TIC: BF143584.D\data.ms

(77) Benzidine

12.751min (+ 0.006) 32424.16 ng

response 824131

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.70	14.06
183.00	11.40	11.84
0.00	0.00	0.00