


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF082725\
Data File : BF143595.D
Acq On : 27 Aug 2025 08:48
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF082625.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Tue Aug 26 16:30:52 2025

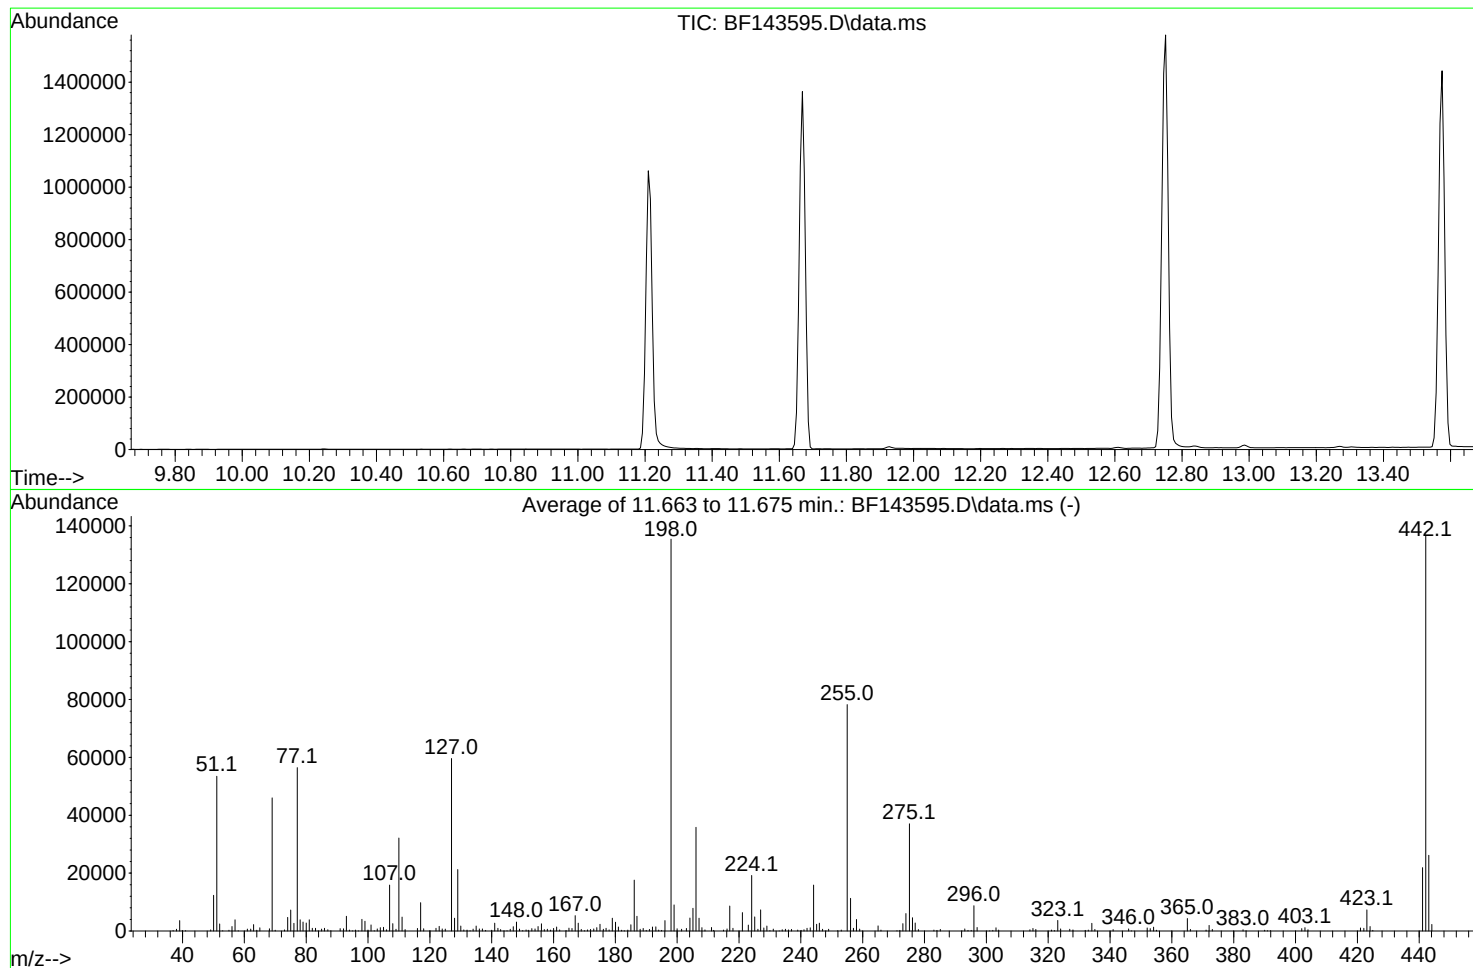




AutoFind: Scans 1610, 1611, 1612; Background Corrected with Scan 1603

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
68	69	0.00	2	1.6	756	PASS
69	69	100	100	100.0	45984	PASS
70	69	0.00	2	0.6	286	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	135429	PASS
199	198	5	9	6.6	8998	PASS
365	198	1	100	3.2	4332	PASS
441	443	0.01	150	83.6	21883	PASS
442	442	100	100	100.0	136464	PASS
443	442	15	24	19.2	26173	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF082725\
Data File : BF143595.D
Acq On : 27 Aug 2025 08:48
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Aug 27 11:27:53 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF082625.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Aug 26 16:30:52 2025
Response via : Initial Calibration

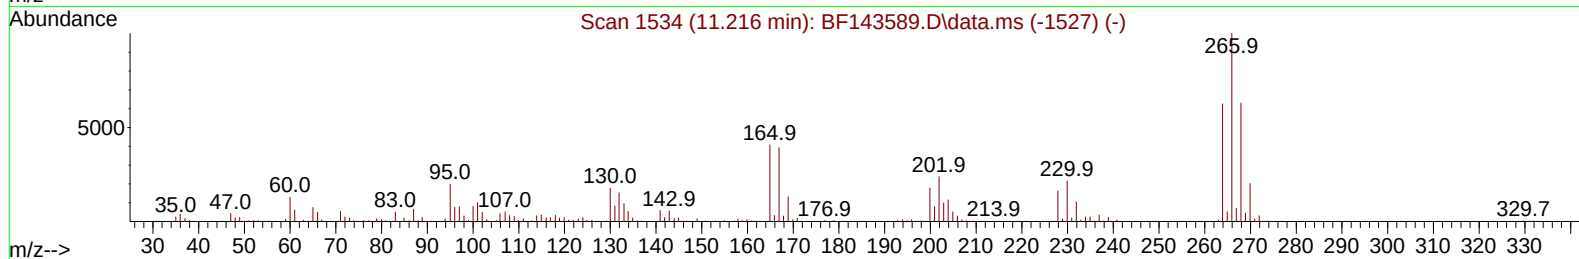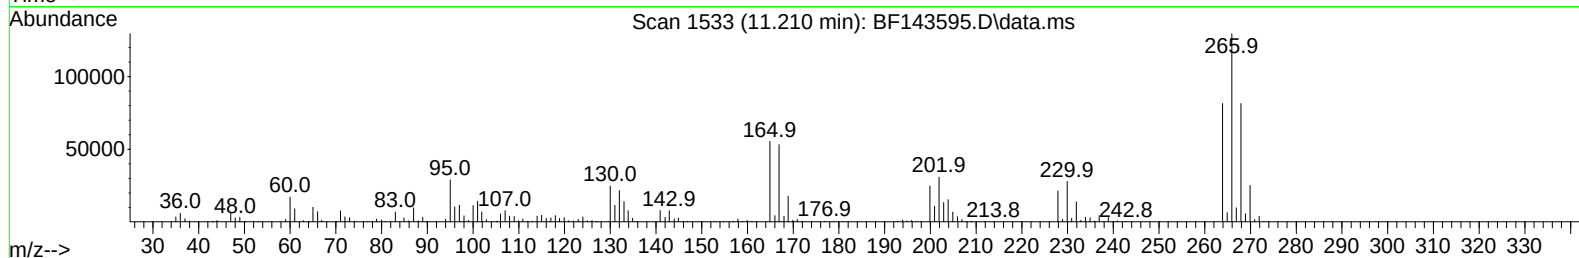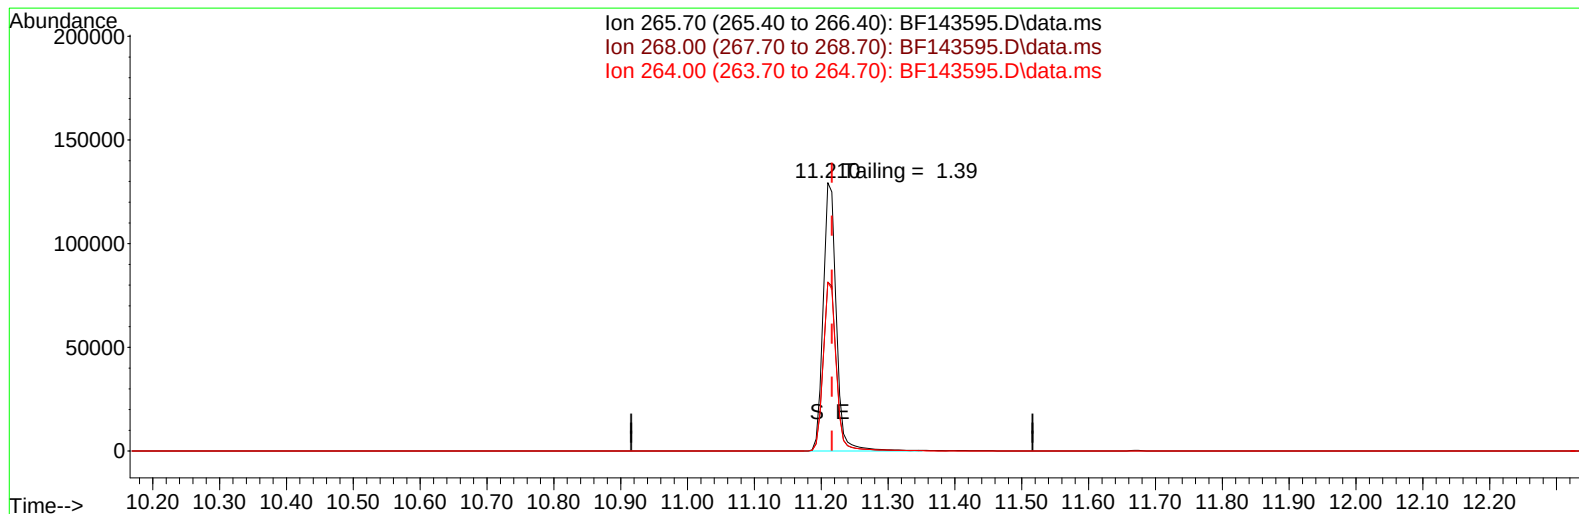

TIC: BF143595.D\data.ms

(70) Pentachlorophenol (C)

11.210min (-0.006) 54326.76 ng




response 177044

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.00	62.96
264.00	62.60	62.92
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF082725\
Data File : BF143595.D
Acq On : 27 Aug 2025 08:48
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Aug 27 11:27:53 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF082625.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Aug 26 16:30:52 2025
Response via : Initial Calibration

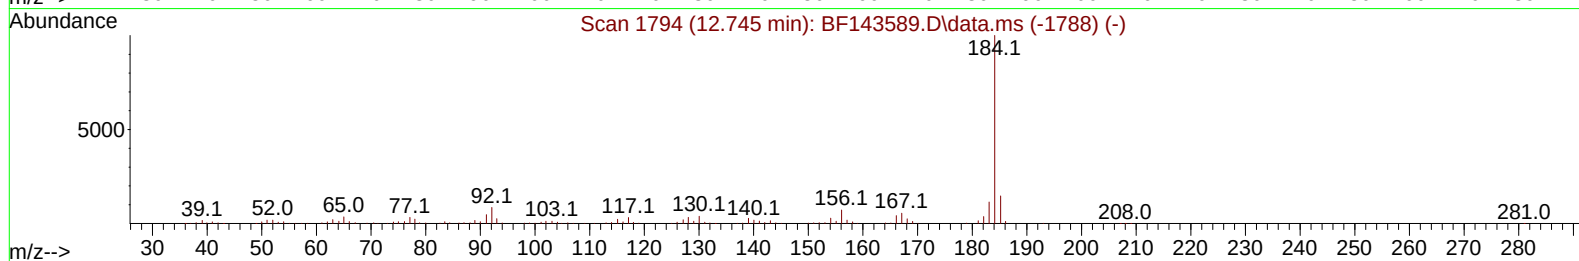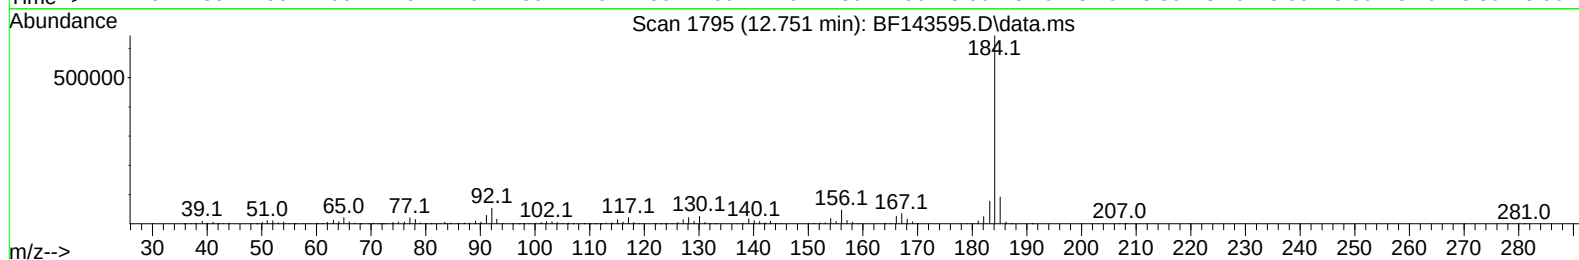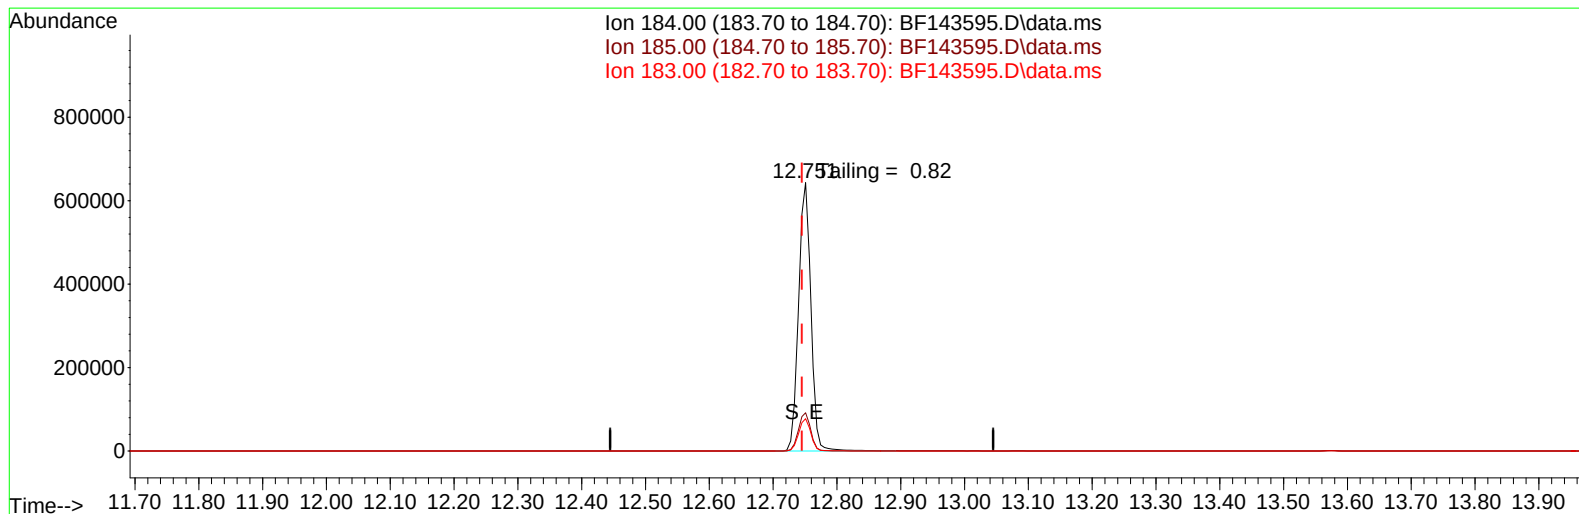

TIC: BF143595.D\data.ms

(77) Benzidine

12.751min (+ 0.006) 57519.20 ng

response 866062

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.70	14.27
183.00	11.40	12.04
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
8/27/2025	BNA_F	<u>BF143595.D</u>
Compound Name	Response	Retention Time
DDT	347516	13.574
DDD	2772	13.269
DDE	0	12.974
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
2772	350288	0.79

Instrument :
BNA_F
ClientSampleId :
DFTPP