
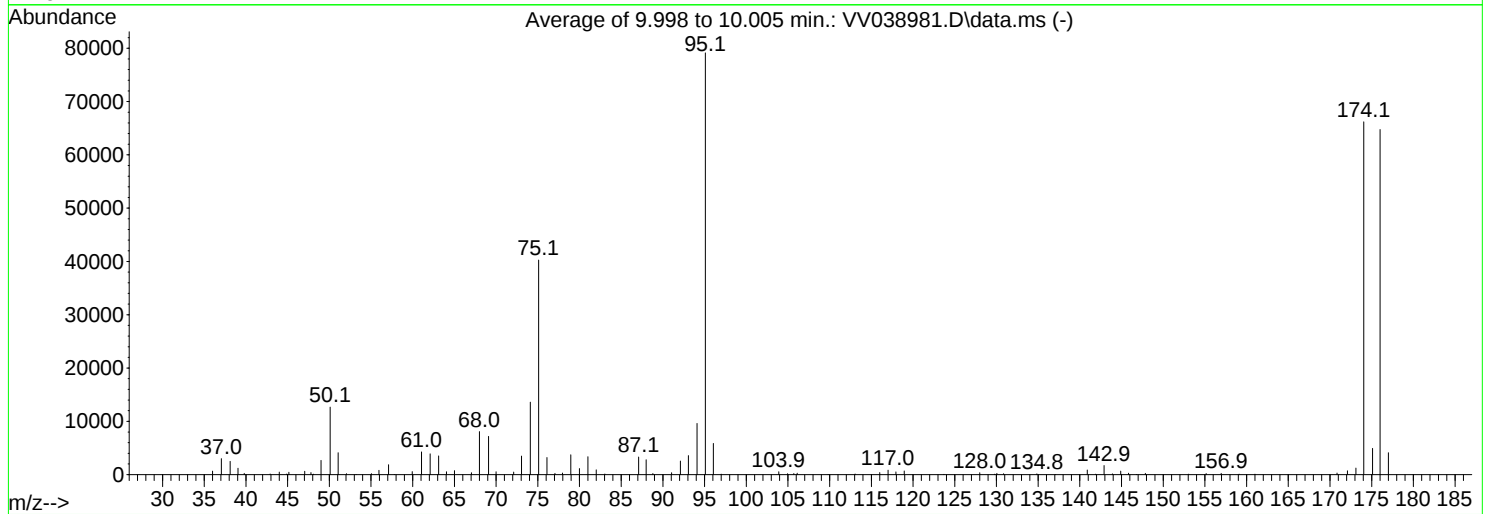


Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV082125\
Data File : VV038981.D
Acq On : 21 Aug 2025 15:11
Operator : SY/MD
Sample : BFB
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\82V082125W.M
Title : SW846 8260
Last Update : Fri Aug 22 04:15:04 2025

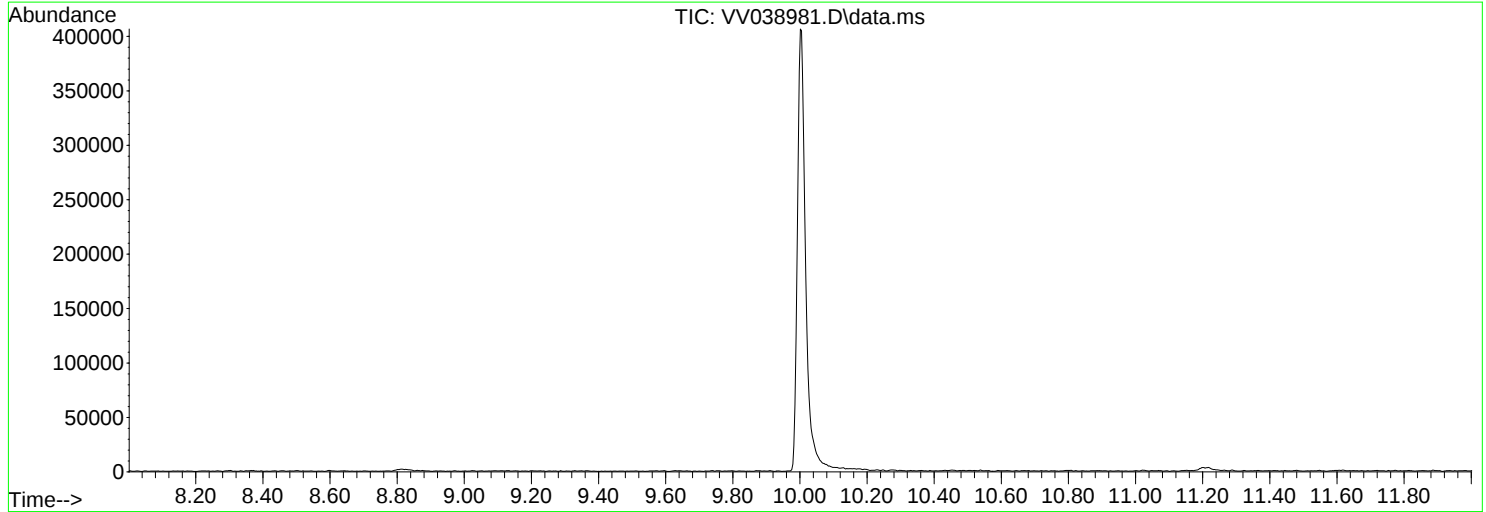

AutoFind: Scans 2786, 2787, 2788; Background Corrected with Scan 2776

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	15	40	16.0	12677	PASS
75	95	30	60	50.9	40256	PASS
95	95	100	100	100.0	79139	PASS
96	95	5	9	7.4	5845	PASS
173	174	0.00	2	1.8	1222	PASS
174	95	50	100	83.7	66211	PASS
175	174	5	9	7.4	4925	PASS
176	174	95	101	97.8	64765	PASS
177	176	5	9	6.4	4126	PASS