


BFB

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV082225\
Data File : VV039008.D
Acq On : 22 Aug 2025 07:56
Operator : SY/MD
Sample : BFB
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\82V082125W.M
Title : SW846 8260
Last Update : Fri Aug 22 04:15:04 2025

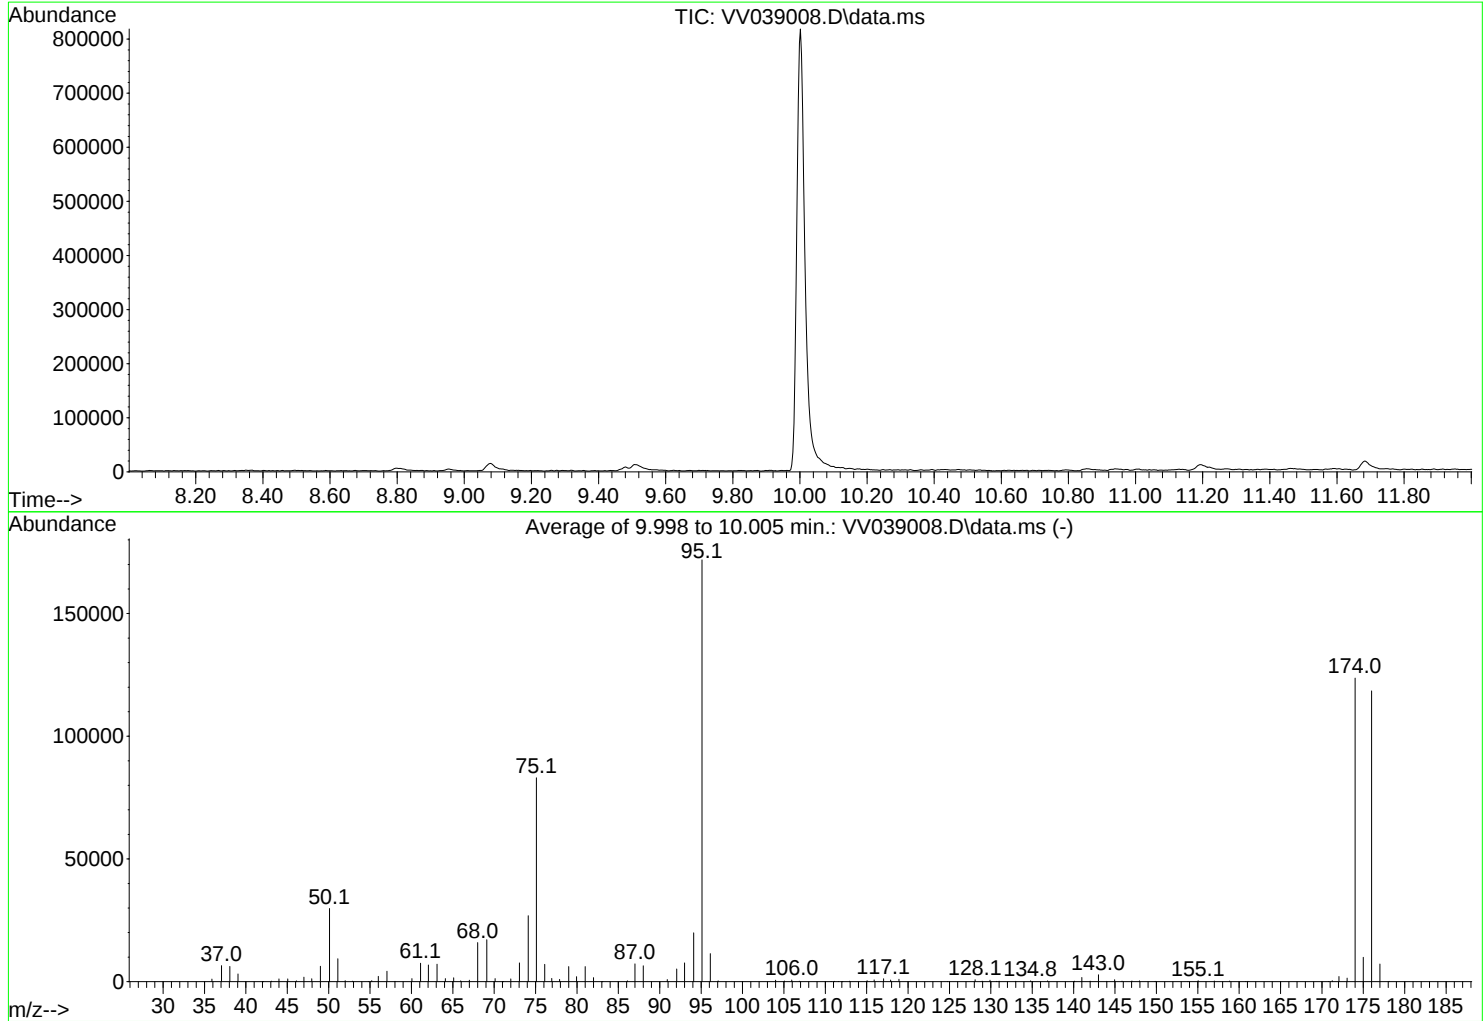

AutoFind: Scans 2786, 2787, 2788; Background Corrected with Scan 2774

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	15	40	17.3	29773	PASS
75	95	30	60	48.3	83061	PASS
95	95	100	100	100.0	171883	PASS
96	95	5	9	6.6	11417	PASS
173	174	0.00	2	1.1	1416	PASS
174	95	50	100	72.0	123715	PASS
175	174	5	9	8.0	9904	PASS
176	174	95	101	95.8	118488	PASS
177	176	5	9	6.1	7173	PASS