


Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV082125\
Data File : VV038972.D
Acq On : 21 Aug 2025 08:34
Operator : SY/MD
Sample : BFB
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\82V082125W.M
Title : SW846 8260
Last Update : Fri Aug 22 04:15:04 2025

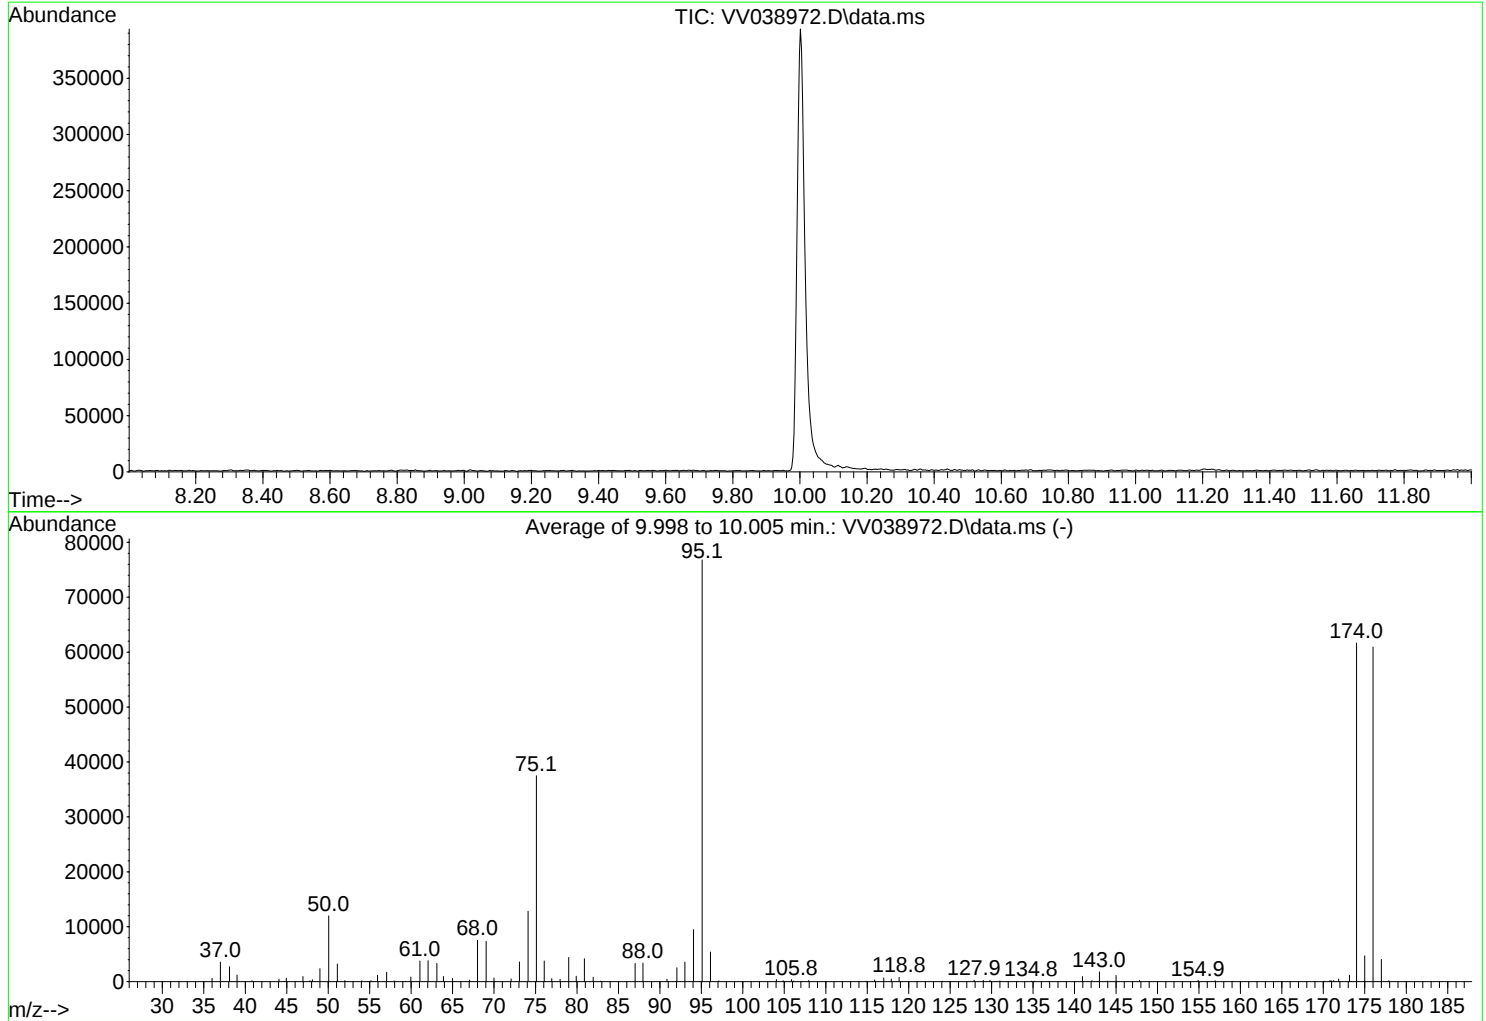

AutoFind: Scans 2786, 2787, 2788; Background Corrected with Scan 2775

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	15.6	11976	PASS
75	95	30	60	48.8	37496	PASS
95	95	100	100	100.0	76808	PASS
96	95	5	9	7.0	5392	PASS
173	174	0.00	2	1.9	1161	PASS
174	95	50	100	80.3	61643	PASS
175	174	5	9	7.6	4704	PASS
176	174	95	101	98.8	60933	PASS
177	176	5	9	6.6	4042	PASS