
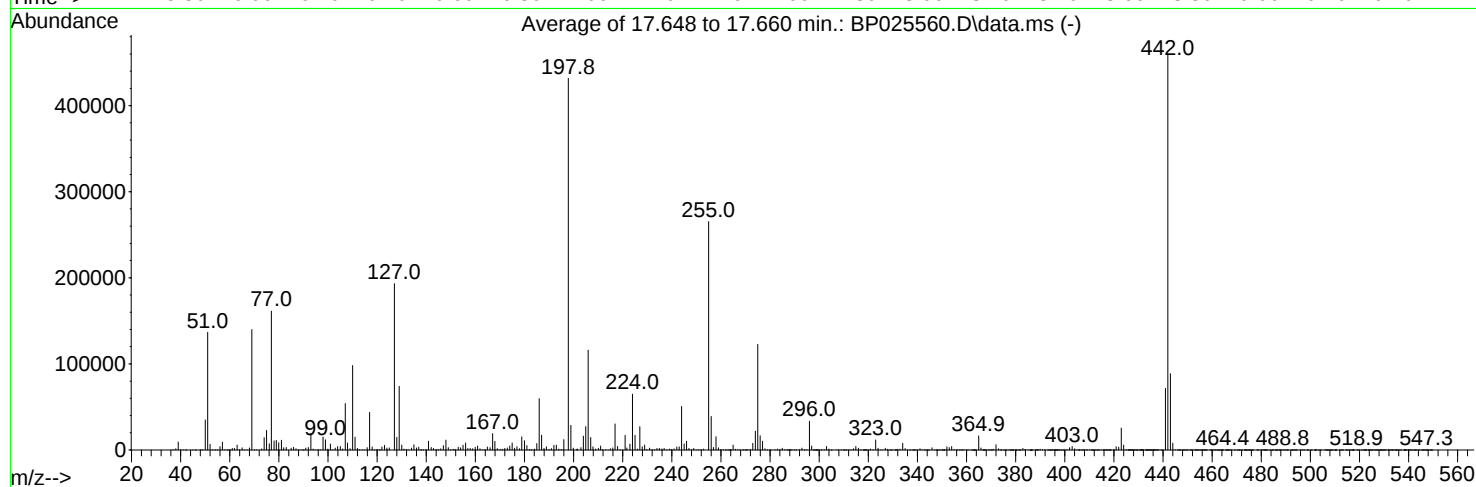


Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP082525\
Data File : BP025560.D
Acq On : 25 Aug 2025 10:24
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP081425.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Thu Aug 14 18:14:31 2025

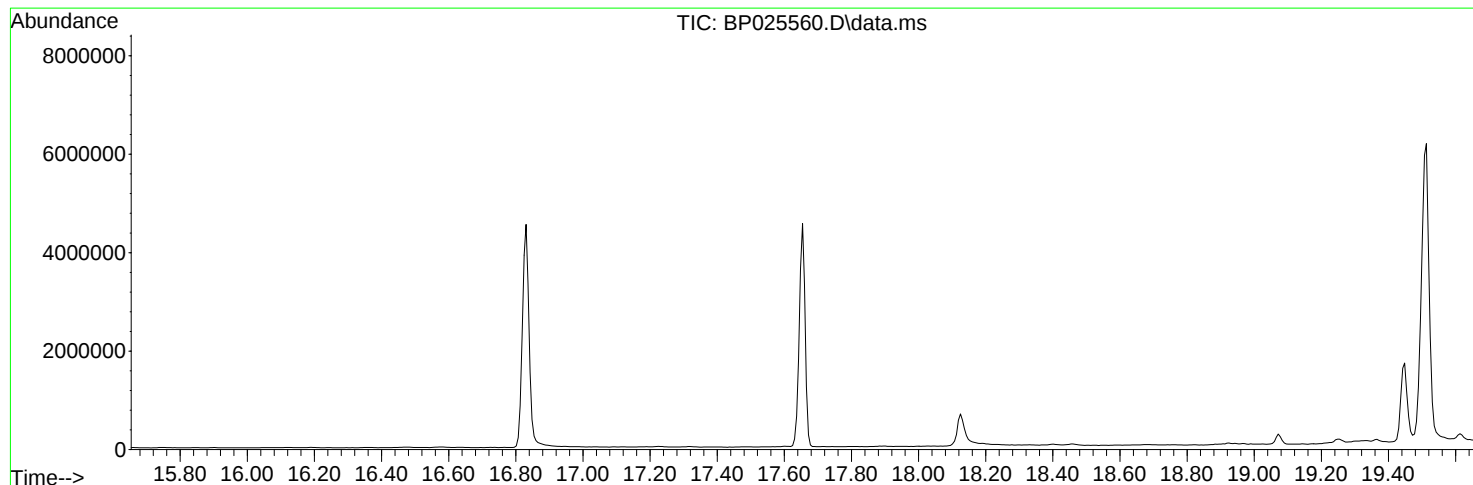




AutoFind: Scans 2501, 2502, 2503; Background Corrected with Scan 2491

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
68	69	0.00	2	1.7	2382	PASS
69	69	100	100	100.0	139943	PASS
70	69	0.00	2	0.3	445	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	431644	PASS
199	198	5	9	6.6	28690	PASS
365	198	1	100	3.8	16344	PASS
441	443	0.01	150	80.8	71635	PASS
442	442	100	100	100.0	458603	PASS
443	442	15	24	19.3	88643	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP082525\
Data File : BP025560.D
Acq On : 25 Aug 2025 10:24
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DFTPP

Quant Time: Aug 25 12:41:12 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP081425.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Aug 14 18:14:31 2025
Response via : Initial Calibration

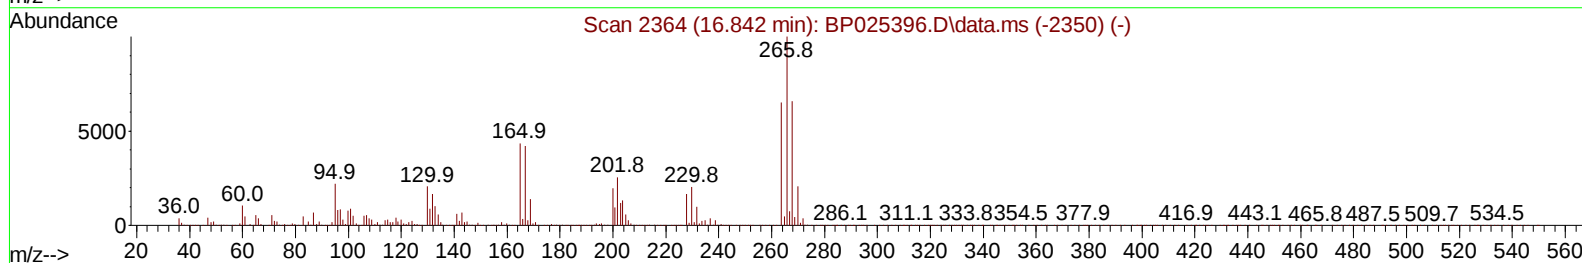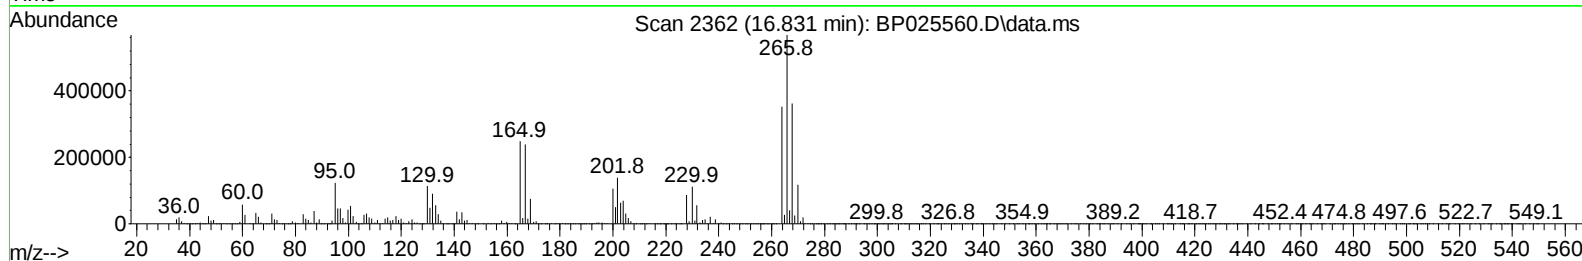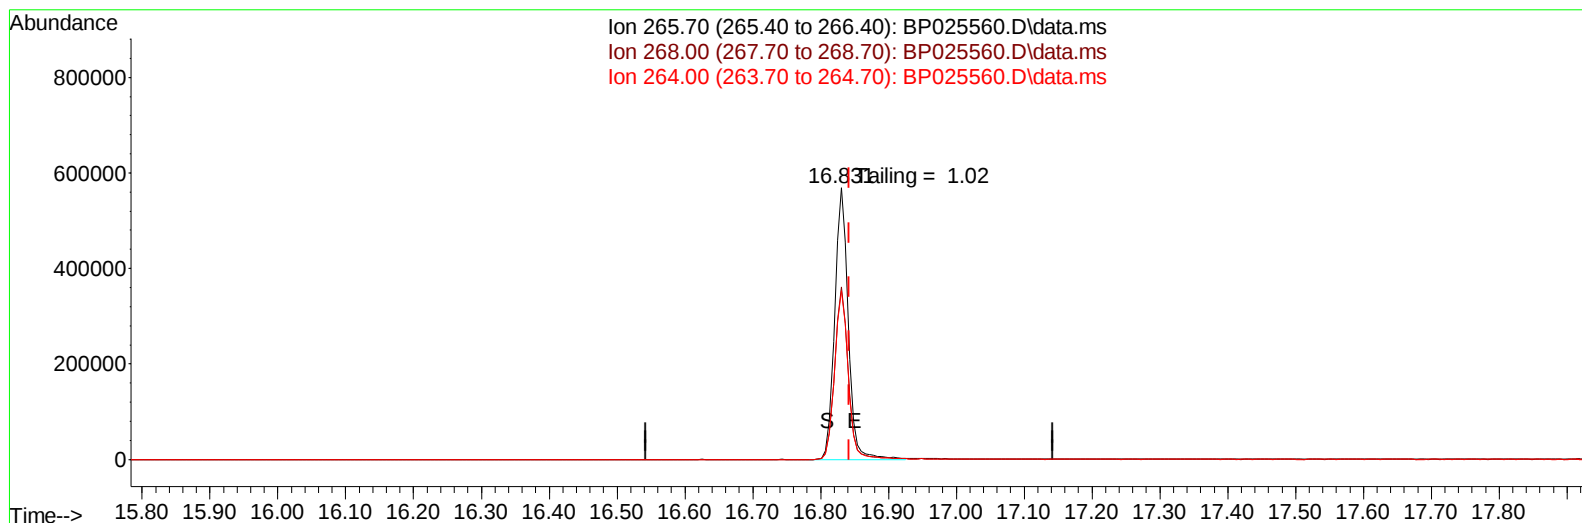

TIC: BP025560.D\data.ms

(70) Pentachlorophenol (C)

16.831min (-0.012) 30402.24 ng




response 788586

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	65.80	63.60
264.00	65.00	62.15
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP082525\
Data File : BP025560.D
Acq On : 25 Aug 2025 10:24
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DFTPP

Quant Time: Aug 25 12:41:12 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP081425.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Aug 14 18:14:31 2025
Response via : Initial Calibration

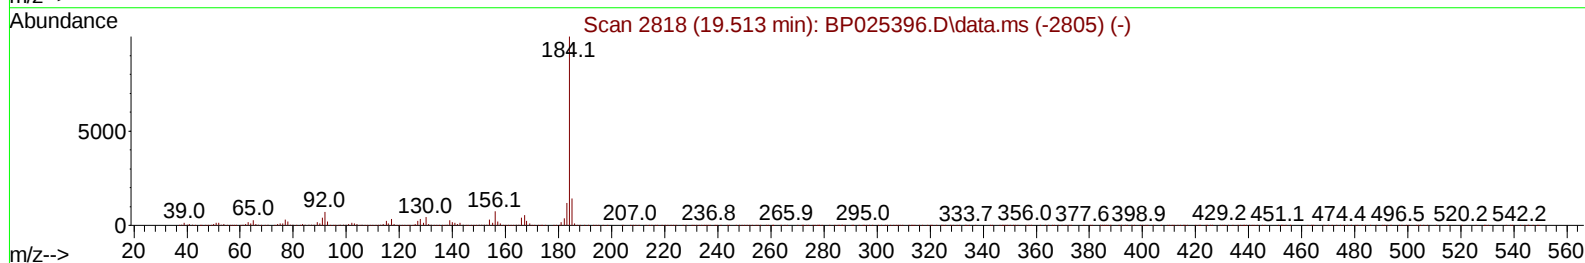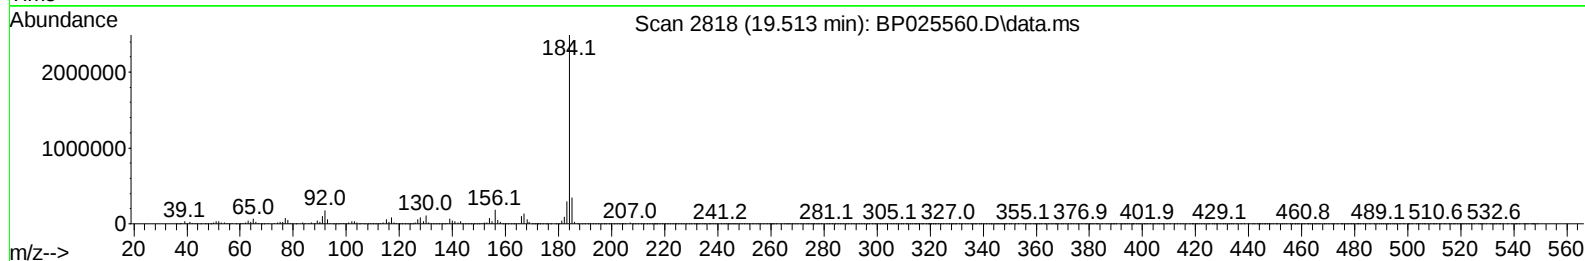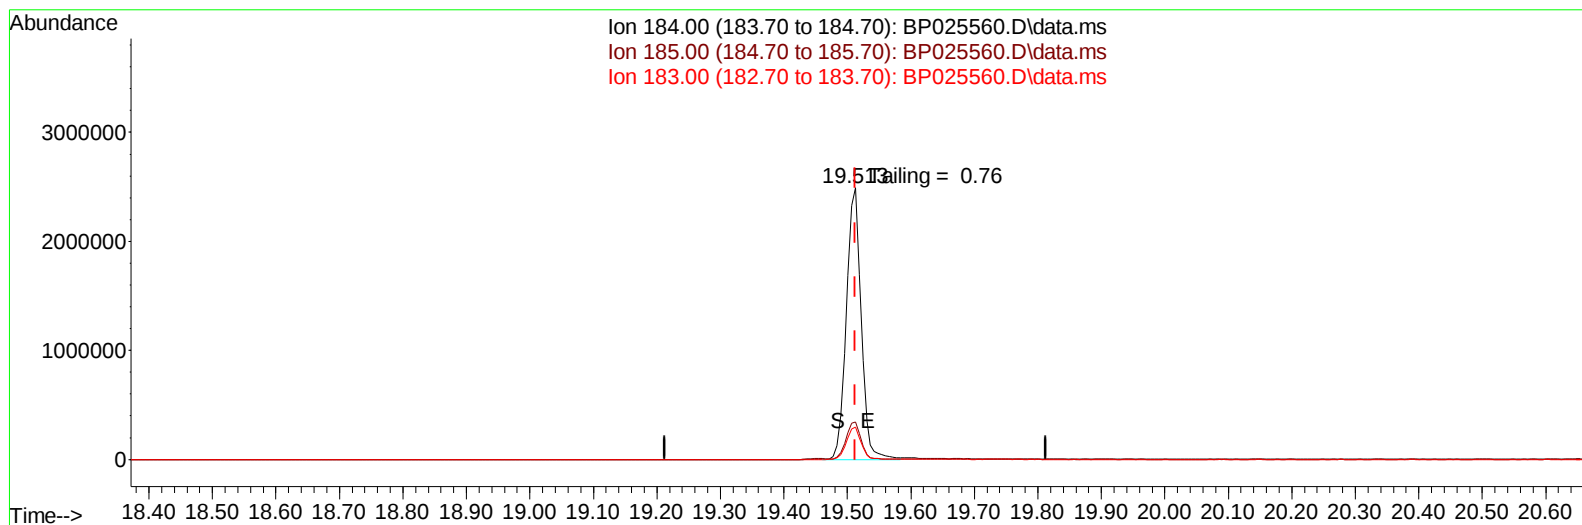

TIC: BP025560.D\data.ms

(77) Benzidine

19.513min (+ 0.000) 18802.33 ng

response 4079827

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.40	13.93
183.00	11.80	12.00
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
8/25/2025	BNA_P	<u>BP025560.D</u>
Compound Name	Response	Retention Time
DDT	2097133	20.807
DDD	38651	20.342
DDE	4733	19.819
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
43384	2140517	2.03

Instrument :
BNA_P
ClientSampleId :
DFTPP