
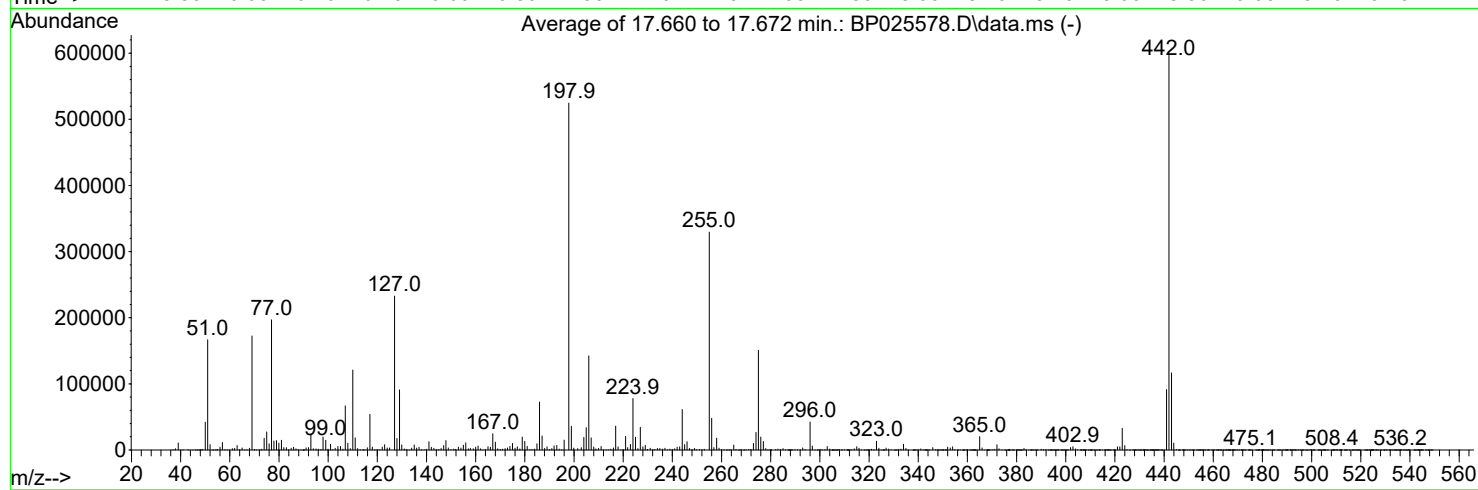


Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP082625\
Data File : BP025578.D
Acq On : 26 Aug 2025 08:59
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP081425.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Thu Aug 14 18:14:31 2025

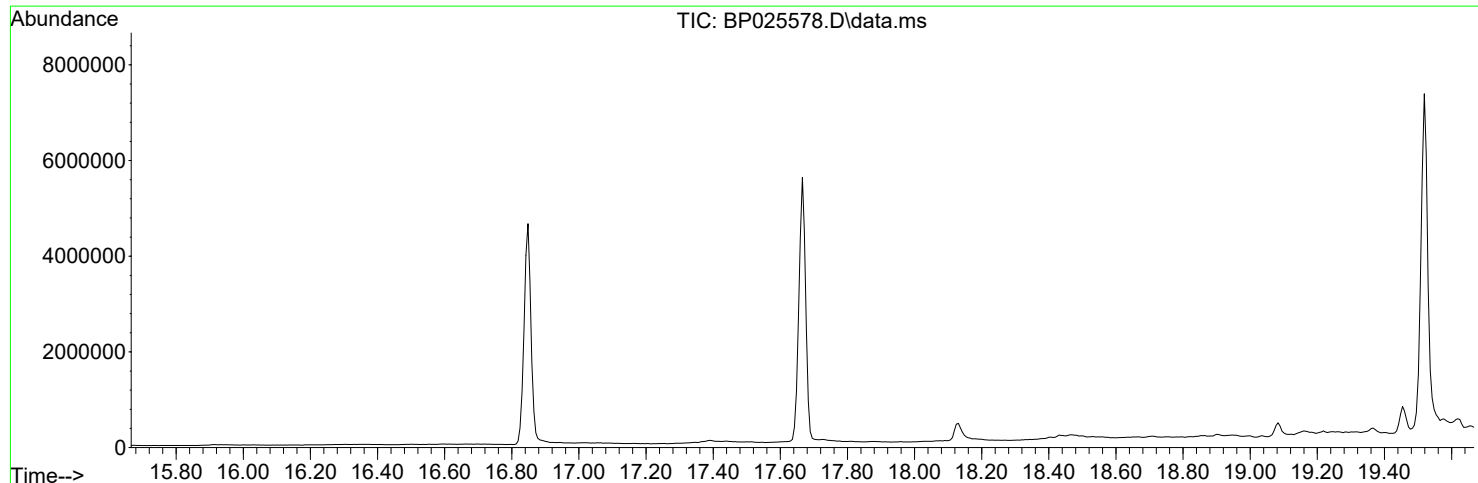

AutoFind: Scans 2503, 2504, 2505; Background Corrected with Scan 2493

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
68	69	0.00	2	1.6	2756	PASS
69	69	100	100	100.0	172546	PASS
70	69	0.00	2	0.6	1035	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	524501	PASS
199	198	5	9	6.8	35733	PASS
365	198	1	100	3.9	20440	PASS
441	443	0.01	150	78.3	91453	PASS
442	442	100	100	100.0	597035	PASS
443	442	15	24	19.6	116747	PASS

DDT Breakdown




Date	Instrument Name	DFTPP Data File
8/26/2025	BNA_P	<u>BP025578.D</u>
Compound Name	Response	Retention Time
DDT	2136201	20.813
DDD	101241	20.354
DDE	5903	19.819
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
107144	2243345	4.78

Instrument :
BNA_P
ClientSampleId :
DFTPP

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP082625\
Data File : BP025578.D
Acq On : 26 Aug 2025 08:59
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DFTPP

Quant Time: Aug 26 09:35:45 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP081425.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Aug 14 18:14:31 2025
Response via : Initial Calibration

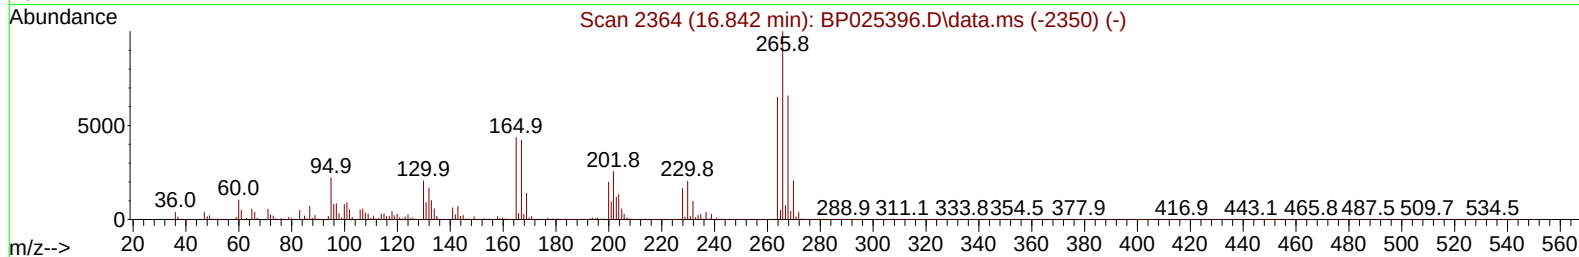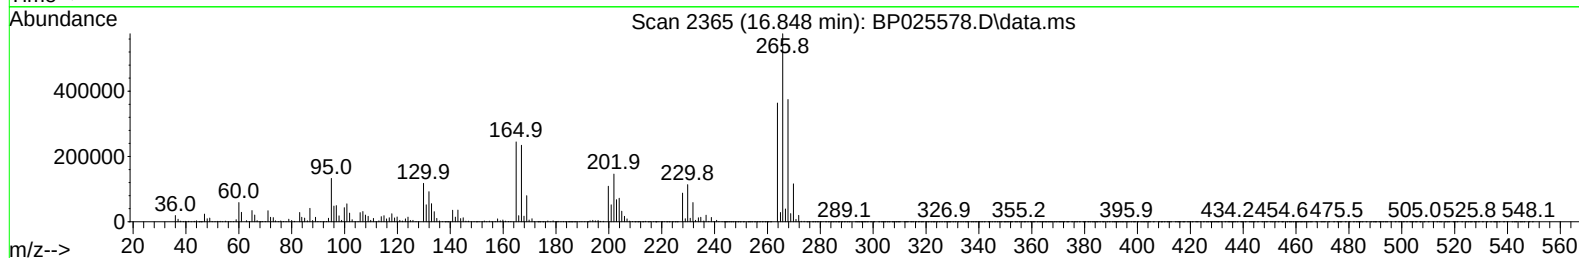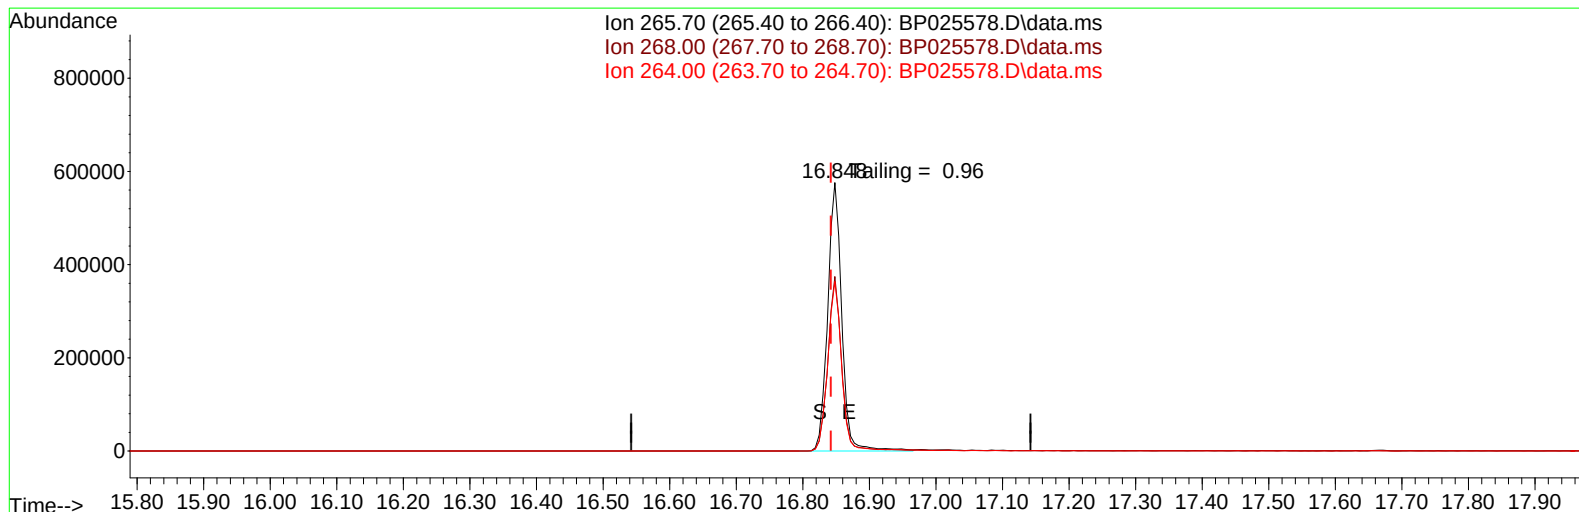

TIC: BP025578.D\data.ms

(70) Pentachlorophenol (C)

16.848min (+ 0.006) 901788.49 ng




response 849129

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	65.80	64.98
264.00	65.00	63.17
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP082625\
Data File : BP025578.D
Acq On : 26 Aug 2025 08:59
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DFTPP

Quant Time: Aug 26 09:35:45 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP081425.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Aug 14 18:14:31 2025
Response via : Initial Calibration

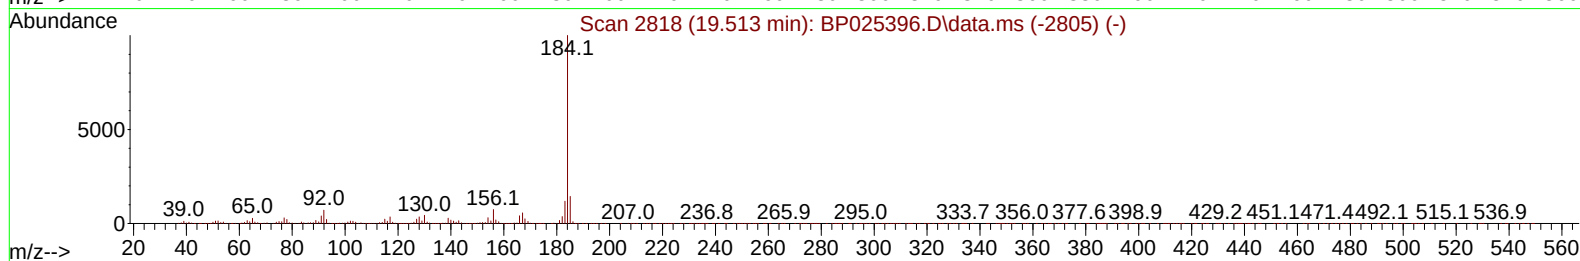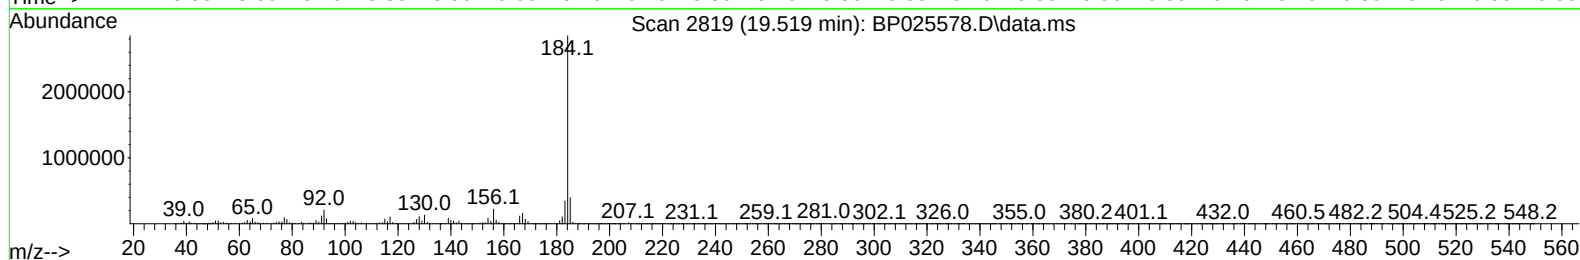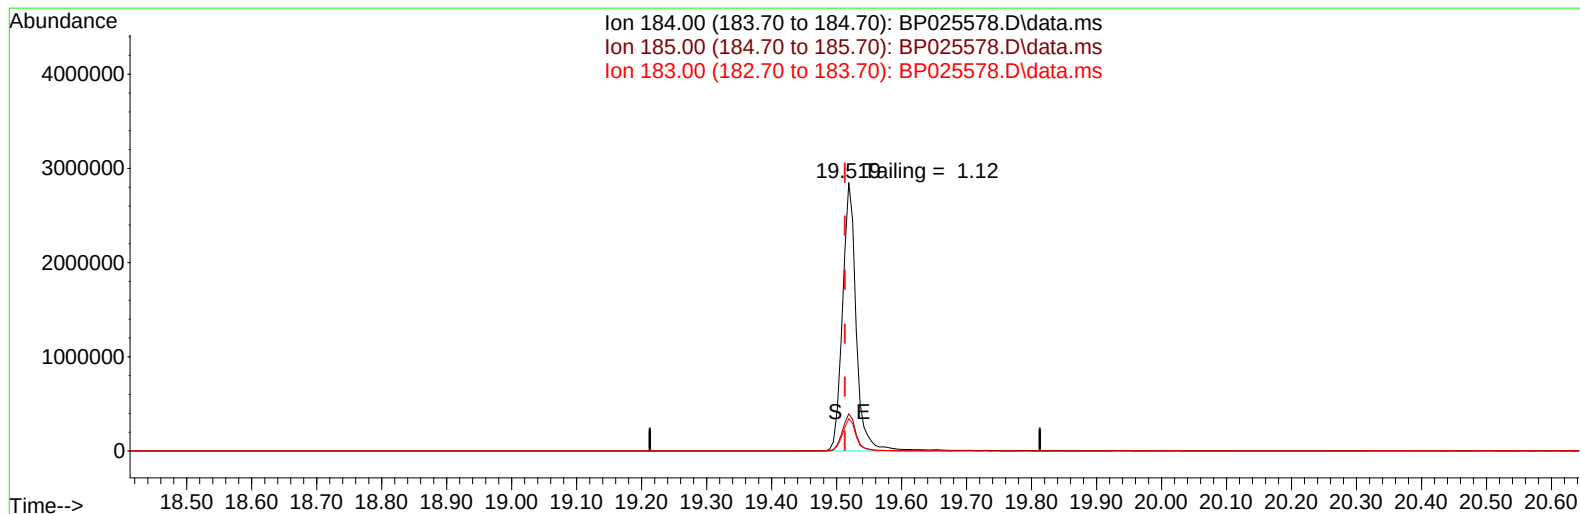

TIC: BP025578.D\data.ms

(77) Benzidine

19.519min (+ 0.006) 262076.27 ng

response 4167956

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.40	13.88
183.00	11.80	12.08
0.00	0.00	0.00