
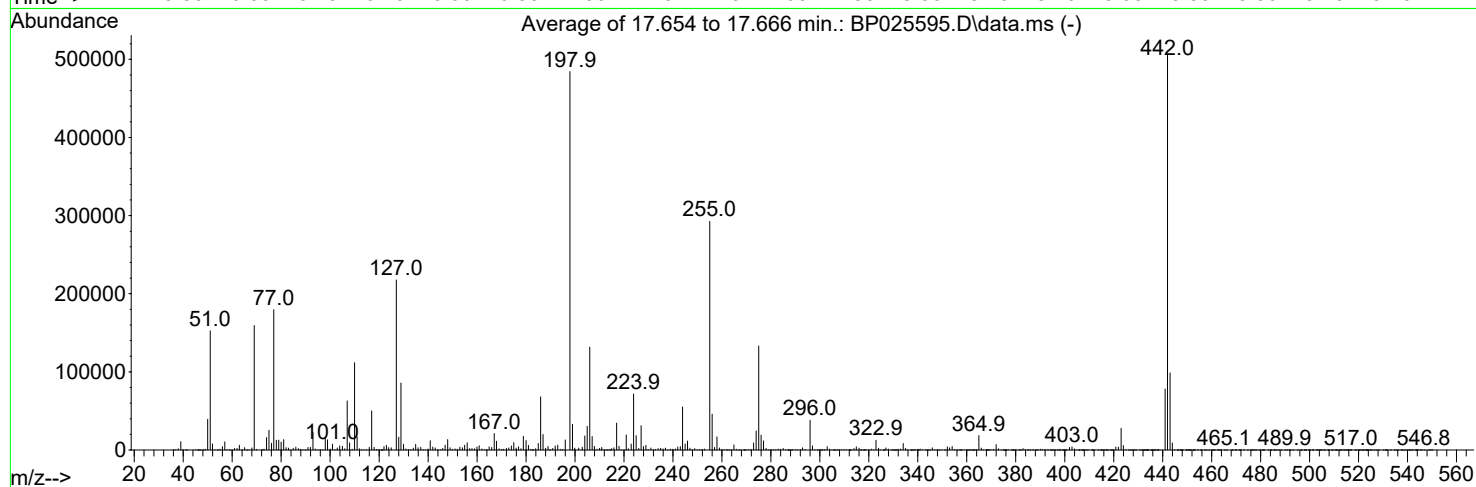


Data Path : Z:\svoasrv\HPCHEM1\BNA\_P\Data\BP082725\  
Data File : BP025595.D  
Acq On : 27 Aug 2025 08:58  
Operator : CG/JU  
Sample : DFTPP  
Misc :  
ALS Vial : 1 Sample Multiplier: 1

Instrument :  
BNA\_P  
ClientSampleId :  
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA\_P\Methods\8270E-BP081425.M  
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
Last Update : Thu Aug 14 18:14:31 2025

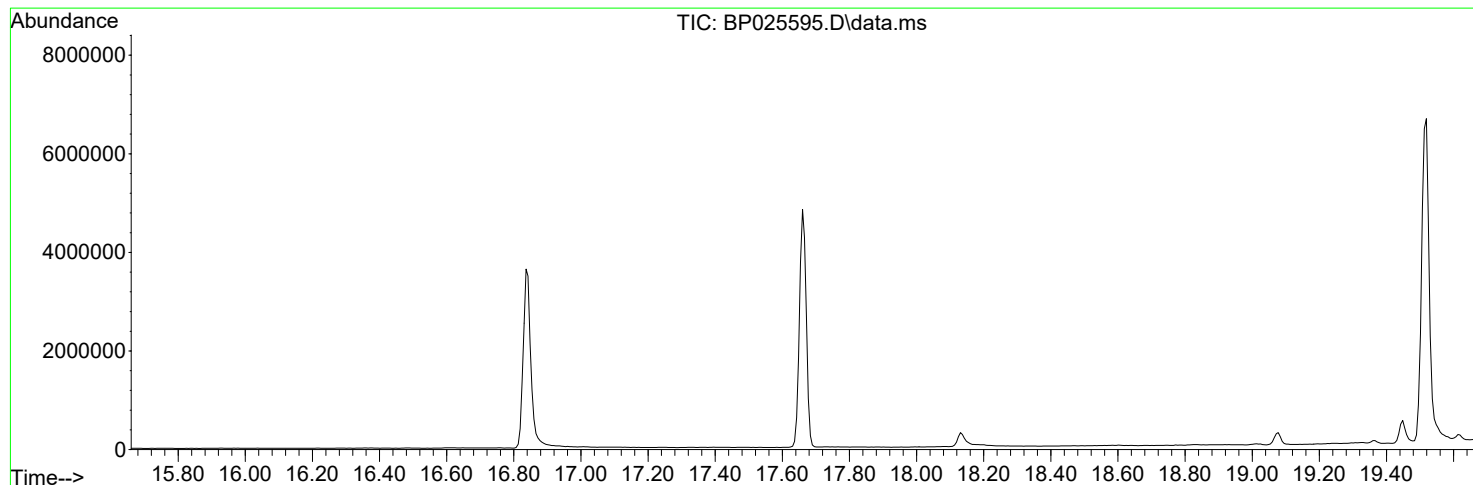

AutoFind: Scans 2502, 2503, 2504; Background Corrected with Scan 2495

| Target | Rel. to | Lower  | Upper  | Rel.  | Raw    | Result    |
|--------|---------|--------|--------|-------|--------|-----------|
| Mass   | Mass    | Limit% | Limit% | Abn%  | Abn    | Pass/Fail |
| 68     | 69      | 0.00   | 2      | 1.7   | 2647   | PASS      |
| 69     | 69      | 100    | 100    | 100.0 | 159279 | PASS      |
| 70     | 69      | 0.00   | 2      | 0.6   | 914    | PASS      |
| 197    | 198     | 0.00   | 2      | 0.0   | 0      | PASS      |
| 198    | 198     | 100    | 100    | 100.0 | 484263 | PASS      |
| 199    | 198     | 5      | 9      | 6.8   | 33059  | PASS      |
| 365    | 198     | 1      | 100    | 3.8   | 18407  | PASS      |
| 441    | 443     | 0.01   | 150    | 79.2  | 78301  | PASS      |
| 442    | 442     | 100    | 100    | 100.0 | 505318 | PASS      |
| 443    | 442     | 15     | 24     | 19.6  | 98803  | PASS      |

# DDT Breakdown




| Date          | Instrument Name  | DFTPP Data File    |
|---------------|------------------|--------------------|
| 8/27/2025     | BNA_P            | <u>BP025595.D</u>  |
|               |                  |                    |
|               |                  |                    |
| Compound Name | Response         | Retention Time     |
|               |                  |                    |
| DDT           | 2242813          | 20.807             |
| DDD           | 65606            | 20.342             |
| DDE           | 9202             | 19.819             |
|               |                  |                    |
|               |                  |                    |
| SUM(DDD+DDE)  | SUM(DDT+DDD+DDE) | % Breakdown Of DDT |
|               |                  |                    |
| 74808         | 2317621          | 3.23               |
|               |                  |                    |

Instrument :  
BNA\_P  
ClientSampleId :  
DFTPP

Data Path : Z:\svoasrv\HPCHEM1\BNA\_P\Data\BP082725\  
Data File : BP025595.D  
Acq On : 27 Aug 2025 08:58  
Operator : CG/JU  
Sample : DFTPP  
Misc :  
ALS Vial : 1 Sample Multiplier: 1

Instrument :  
BNA\_P  
ClientSampleId :  
DFTPP

Quant Time: Aug 27 16:26:25 2025  
Quant Method : Z:\svoasrv\HPCHEM1\BNA\_P\Methods\8270E-BP081425.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
QLast Update : Thu Aug 14 18:14:31 2025  
Response via : Initial Calibration

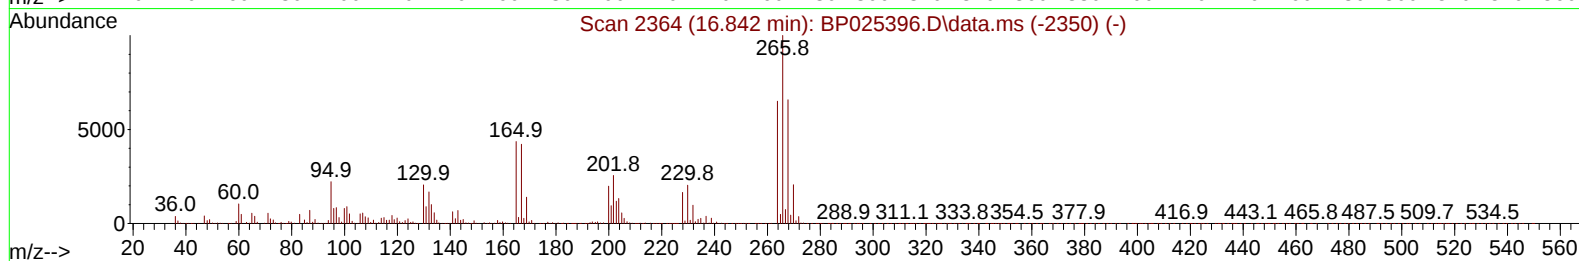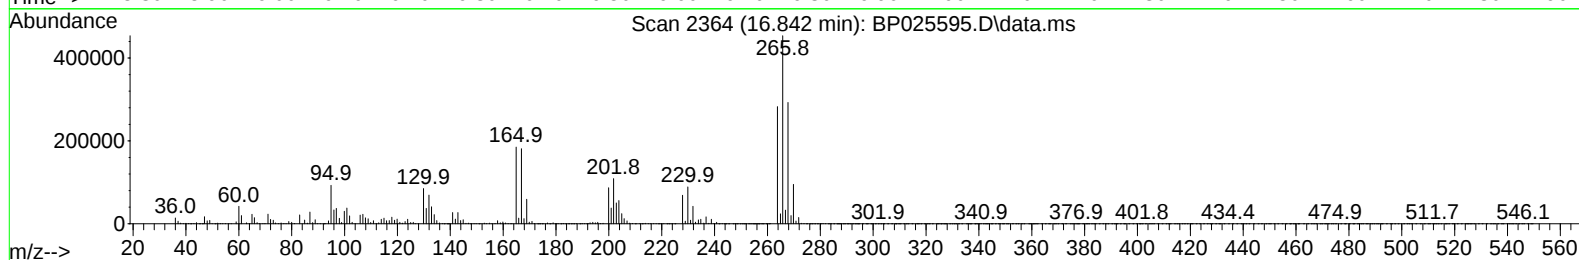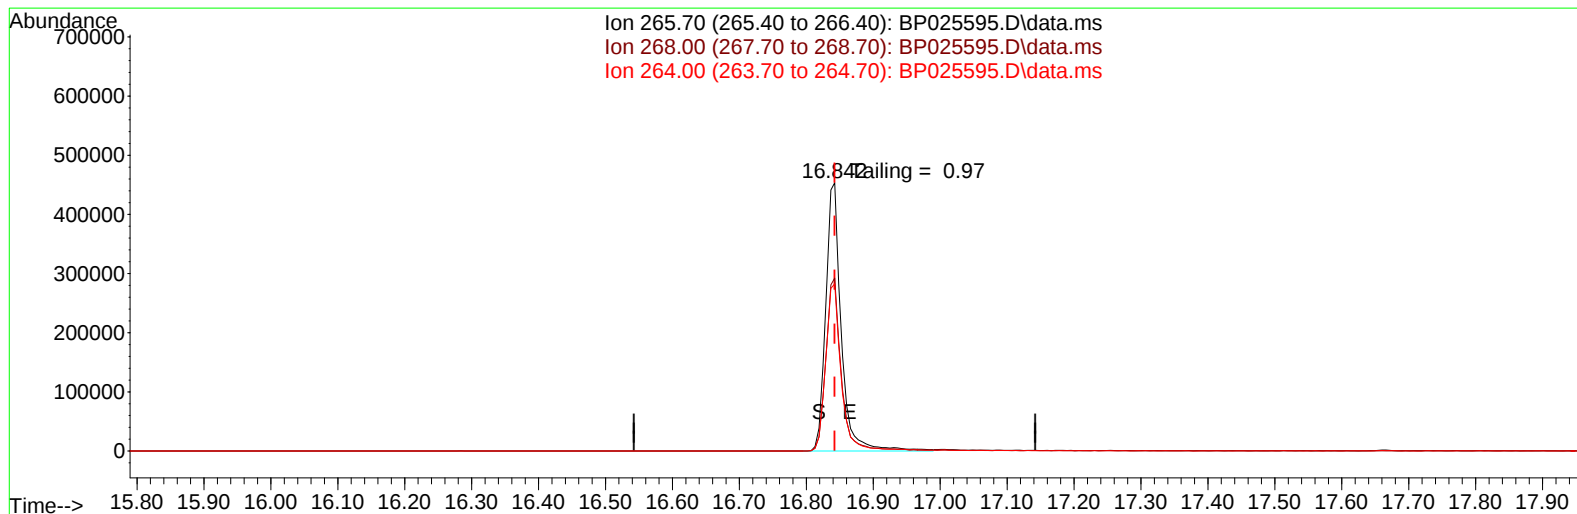

TIC: BP025595.D\data.ms

**(70) Pentachlorophenol (C)**

**16.842min (+ 0.000) 1966640.70 ng**




**response 728058**

| Ion    | Exp%   | Act%   |
|--------|--------|--------|
| 265.70 | 100.00 | 100.00 |
| 268.00 | 65.80  | 64.47  |
| 264.00 | 65.00  | 62.33  |
| 0.00   | 0.00   | 0.00   |

Data Path : Z:\svoasrv\HPCHEM1\BNA\_P\Data\BP082725\  
Data File : BP025595.D  
Acq On : 27 Aug 2025 08:58  
Operator : CG/JU  
Sample : DFTPP  
Misc :  
ALS Vial : 1 Sample Multiplier: 1

Instrument :  
BNA\_P  
ClientSampleId :  
DFTPP

Quant Time: Aug 27 16:26:25 2025  
Quant Method : Z:\svoasrv\HPCHEM1\BNA\_P\Methods\8270E-BP081425.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
QLast Update : Thu Aug 14 18:14:31 2025  
Response via : Initial Calibration

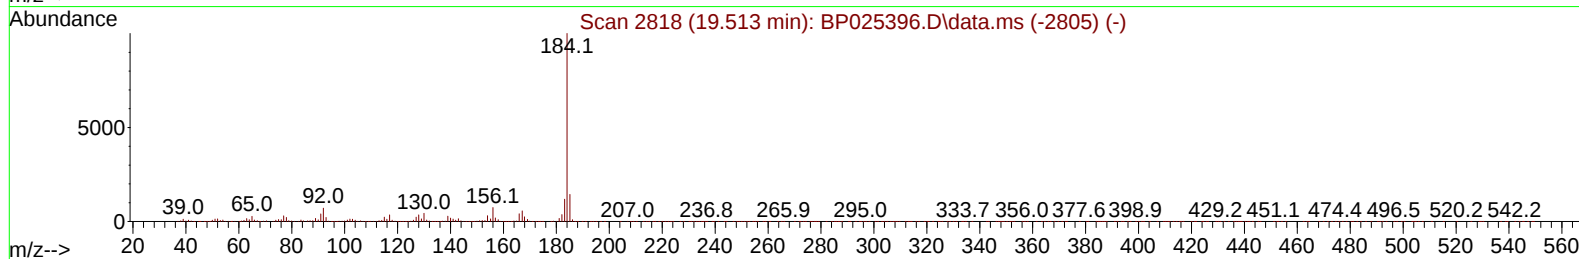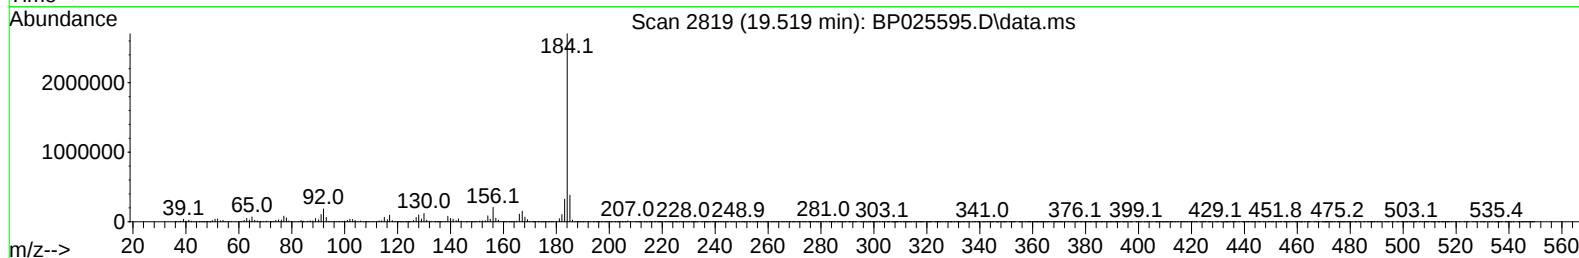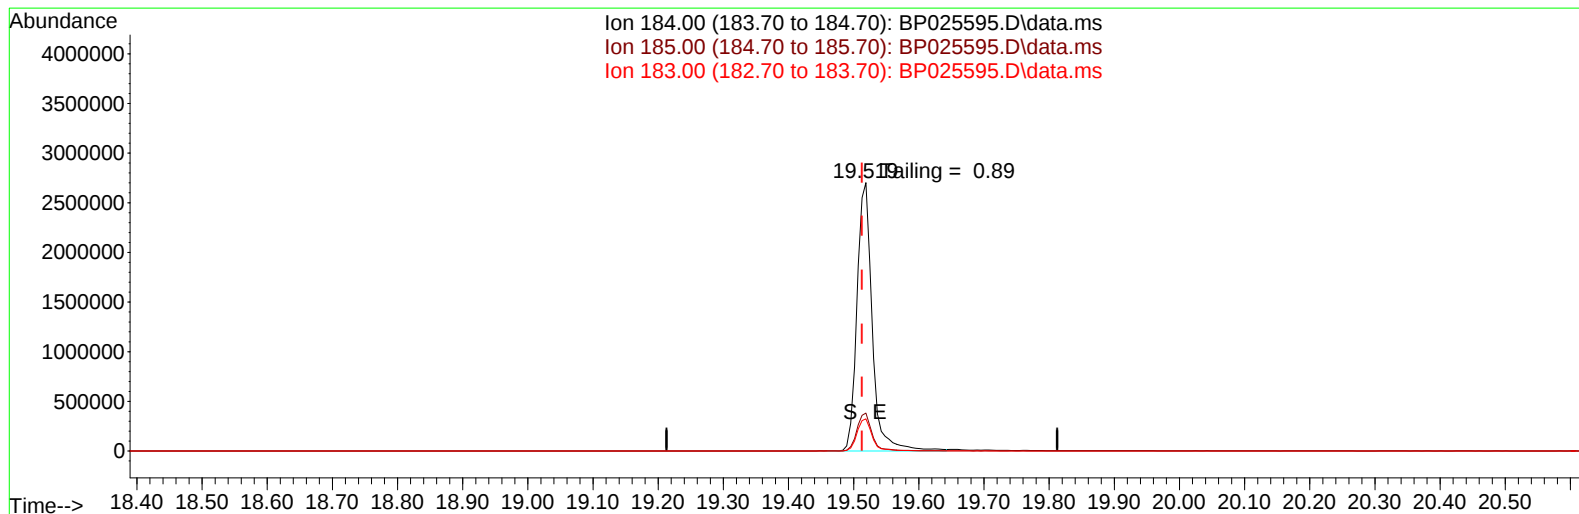

TIC: BP025595.D\data.ms

(77) Benzidine

19.519min (+ 0.006) 862145.80 ng

response 4384060

| Ion    | Exp%   | Act%   |
|--------|--------|--------|
| 184.00 | 100.00 | 100.00 |
| 185.00 | 14.40  | 14.17  |
| 183.00 | 11.80  | 11.99  |
| 0.00   | 0.00   | 0.00   |