

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP082625\
 Data File : BP025594.D
 Acq On : 26 Aug 2025 20:44
 Operator : CG/JU
 Sample : Q2928-01
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 27-BELL

Manual Integrations
 APPROVED

Reviewed By :Rahul Chavli 08/27/2025
 Supervised By :Jagrut Upadhyay 08/27/2025

Quant Time: Aug 27 01:04:05 2025
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP081425.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Aug 14 18:14:31 2025
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.778	152	209024	20.000	ng	-0.02
21) Naphthalene-d8	10.549	136	844005	20.000	ng	-0.01
39) Acenaphthene-d10	14.389	164	543820	20.000	ng	-0.02
64) Phenanthrene-d10	17.195	188	1107950	20.000	ng	0.00
76) Chrysene-d12	21.636	240	1177876	20.000	ng	-0.01
86) Perylene-d12	25.018	264	1387698	20.000	ng	-0.01
System Monitoring Compounds						
5) 2-Fluorophenol	5.408	112	979361	77.810	ng	0.00
7) Phenol-d6	6.972	99	1255837	77.824	ng	0.00
23) Nitrobenzene-d5	8.919	82	810516	48.578	ng	-0.02
42) 2,4,6-Tribromophenol	15.913	330	625675	85.476	ng	0.00
45) 2-Fluorobiphenyl	13.007	172	1851674	46.535	ng	-0.01
79) Terphenyl-d14	19.907	244	2887144	44.845	ng	-0.01
Target Compounds						Qvalue
49) Acenaphthylene	14.119	152	101788	2.001	ng	99
71) Phenanthrene	17.236	178	449521	7.386	ng	99
72) Anthracene	17.336	178	167691	2.698	ng	99
75) Fluoranthene	19.319	202	1569842	21.623	ng	99
78) Pyrene	19.695	202	1463678	19.118	ng	99
81) Benzo(a)anthracene	21.619	228	947450	12.197	ng	97
83) Chrysene	21.683	228	965816m	13.276	ng	
87) Indeno(1,2,3-cd)pyrene	28.865	276	743117	7.302	ng	# 90
88) Benzo(b)fluoranthene	23.948	252	1397978	17.084	ng	96
89) Benzo(k)fluoranthene	24.007	252	441415	5.391	ng	94
90) Benzo(a)pyrene	24.854	252	988740	12.413	ng	97
91) Dibenzo(a,h)anthracene	28.936	278	190610	2.292	ng	96
92) Benzo(g,h,i)perylene	30.047	276	686707	8.400	ng	99

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP082625\
Data File : BP025594.D
Acq On : 26 Aug 2025 20:44
Operator : CG/JU
Sample : Q2928-01
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
27-BELL

Manual Integrations
APPROVED

Reviewed By :Rahul Chavli 08/27/2025
Supervised By :Jagrut Upadhyay 08/27/2025


Quant Time: Aug 27 01:04:05 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP081425.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Aug 14 18:14:31 2025
Response via : Initial Calibration

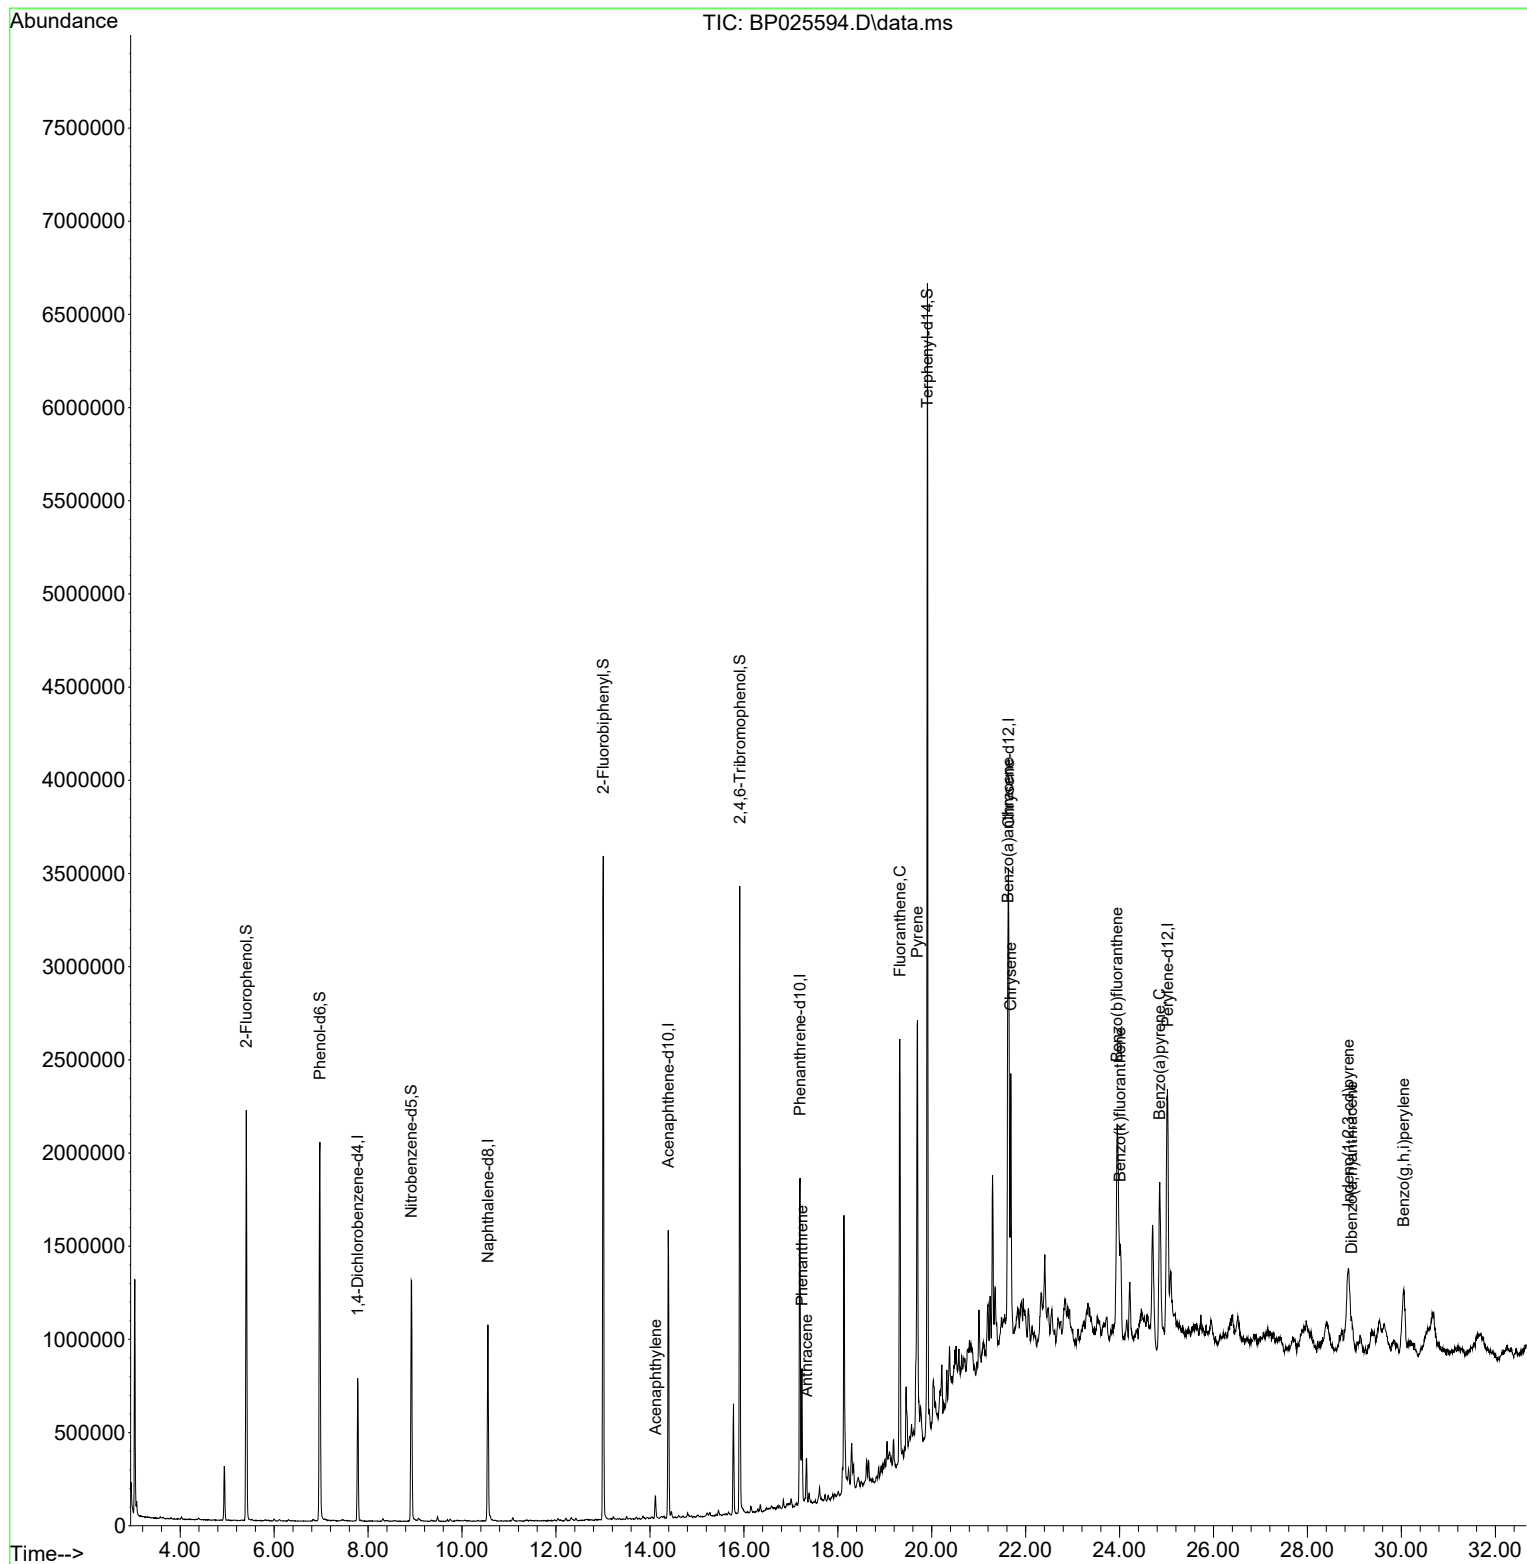



#1
1,4-Dichlorobenzene-d4
Concen: 20.000 ng
RT: 7.778 min Scan# 81
Delta R.T. -0.018 min
Lab File: BP025594.D
Acq: 26 Aug 2025 20:44




Instrument :
BNA_P
ClientSampleId :
27-BELL



Tgt Ion:152 Resp: 209024
Ion Ratio Lower Upper
152 100
150 155.5 125.9 188.9
115 62.8 48.5 72.7




Manual Integrations
APPROVED


Reviewed By :Rahul Chavli 08/27/2025
Supervised By :Jagrut Upadhyay 08/27/2025

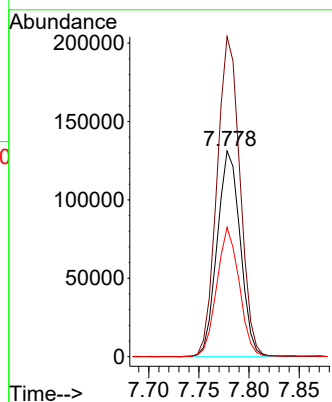

#5
2-Fluorophenol
Concen: 77.810 ng
RT: 5.408 min Scan# 420
Delta R.T. 0.000 min
Lab File: BP025594.D
Acq: 26 Aug 2025 20:44


Tgt Ion:112 Resp: 979361
Ion Ratio Lower Upper
112 100
64 55.9 43.8 65.8
63 29.4 22.7 34.1

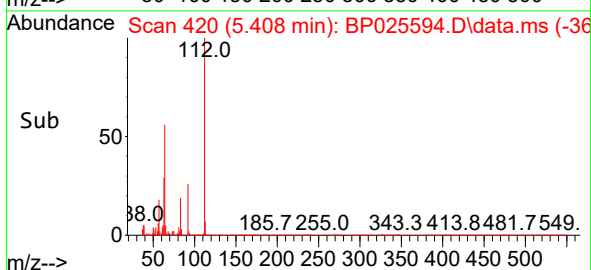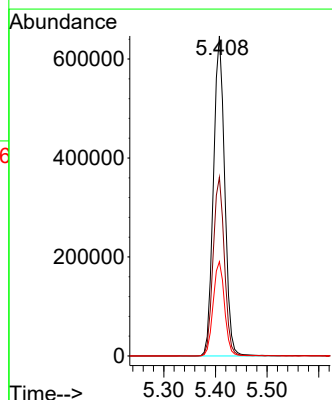



#7
Phenol-d6
Concen: 77.824 ng
RT: 6.972 min Scan# 61
Delta R.T. 0.006 min
Lab File: BP025594.D
Acq: 26 Aug 2025 20:44




Instrument :
BNA_P
ClientSampleId :
27-BELL




Tgt Ion: 99 Resp: 125583
Ion Ratio Lower Upper
99 100
42 16.9 13.7 20.5
71 34.4 28.2 42.4

Manual Integrations
APPROVED



Reviewed By :Rahul Chavli 08/27/2025
Supervised By :Jagrut Upadhyay 08/27/2025

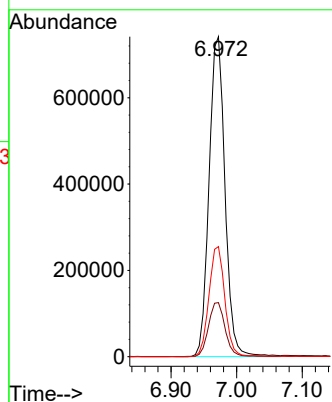


#21
Naphthalene-d8
Concen: 20.000 ng
RT: 10.549 min Scan# 1294
Delta R.T. -0.012 min
Lab File: BP025594.D
Acq: 26 Aug 2025 20:44




Tgt Ion:136 Resp: 844005
Ion Ratio Lower Upper
136 100
137 10.7 9.2 13.8
54 7.8 6.0 9.0
68 5.6 4.3 6.5

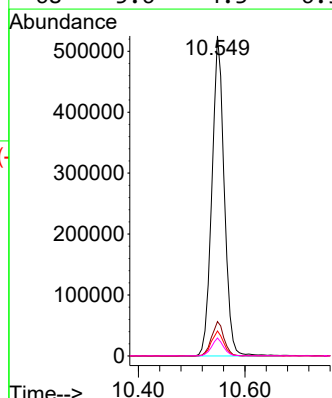

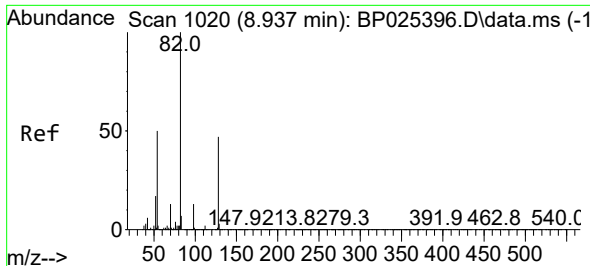

#23
Nitrobenzene-d5
Concen: 48.578 ng
RT: 8.919 min Scan# 1020
Delta R.T. -0.018 min
Lab File: BP025594.D
Acq: 26 Aug 2025 20:44




Instrument :
BNA_P
ClientSampleId :
27-BELL

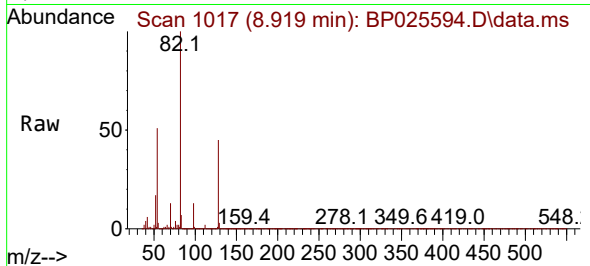


Tgt Ion: 82 Resp: 810510
Ion Ratio Lower Upper
82 100
128 44.6 37.7 56.5
54 51.0 39.8 59.6

Manual Integrations
APPROVED



Reviewed By :Rahul Chavli 08/27/2025
Supervised By :Jagrut Upadhyay 08/27/2025

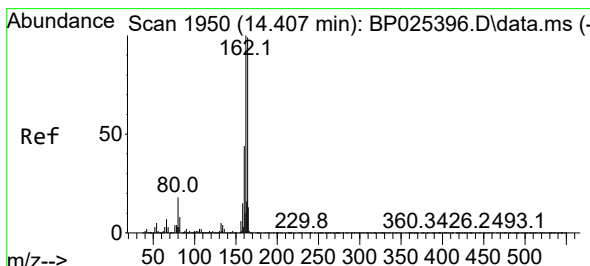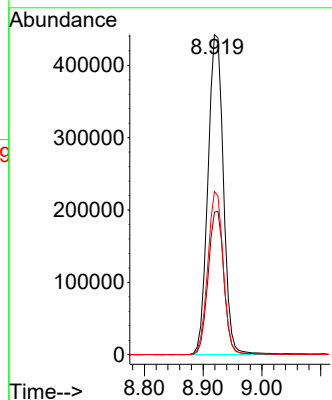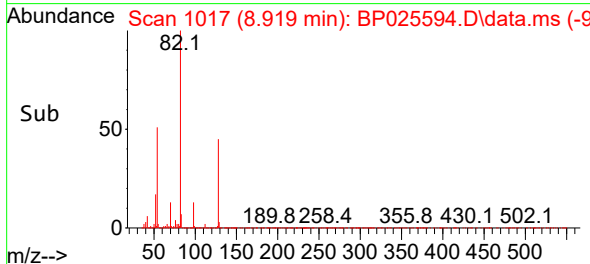

#39
Acenaphthene-d10
Concen: 20.000 ng
RT: 14.389 min Scan# 1947
Delta R.T. -0.018 min
Lab File: BP025594.D
Acq: 26 Aug 2025 20:44

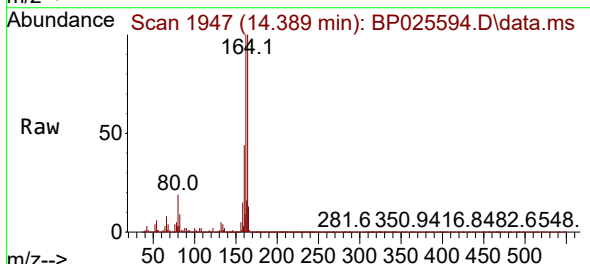


Tgt Ion:164 Resp: 543820
Ion Ratio Lower Upper
164 100
162 100.1 81.0 121.6
160 44.0 35.4 53.2

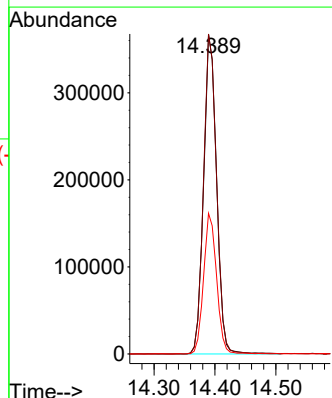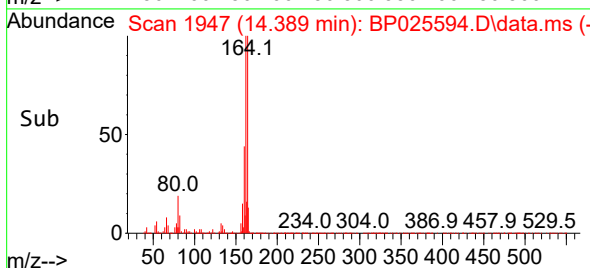



#42
2,4,6-Tribromophenol
Concen: 85.476 ng
RT: 15.913 min Scan# 21
Delta R.T. 0.000 min
Lab File: BP025594.D
Acq: 26 Aug 2025 20:44




Instrument :
BNA_P
ClientSampleId :
27-BELL




Tgt Ion: 330 Resp: 625674
Ion Ratio Lower Upper
330 100
332 97.1 77.3 115.9
141 32.6 26.6 39.8

Manual Integrations
APPROVED



Reviewed By :Rahul Chavli 08/27/2025
Supervised By :Jagrut Upadhyay 08/27/2025

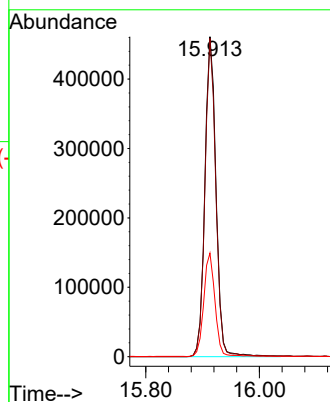


#45
2-Fluorobiphenyl
Concen: 46.535 ng
RT: 13.007 min Scan# 1712
Delta R.T. -0.012 min
Lab File: BP025594.D
Acq: 26 Aug 2025 20:44




Tgt Ion: 172 Resp: 1851674
Ion Ratio Lower Upper
172 100
171 35.1 28.1 42.1
170 23.2 18.6 28.0

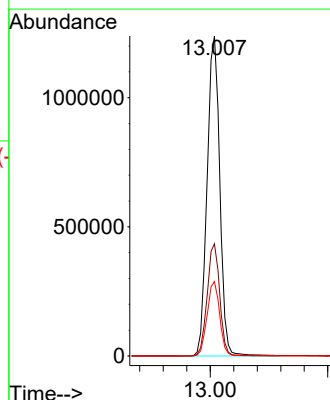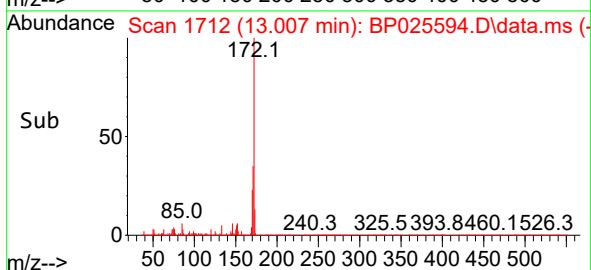

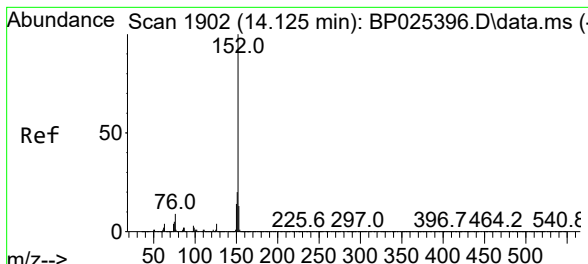

#49
 Acenaphthylene
 Concen: 2.001 ng
 RT: 14.119 min Scan# 1901
 Delta R.T. -0.006 min
 Lab File: BP025594.D
 Acq: 26 Aug 2025 20:44




Instrument :
 BNA_P
 ClientSampleId :
 27-BELL

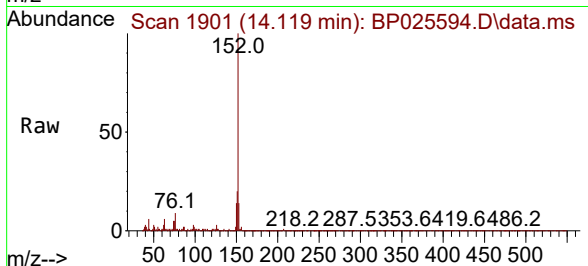

Tgt Ion:152 Resp: 101788
 Ion Ratio Lower Upper
 152 100
 151 20.1 16.0 24.0
 153 14.3 10.6 15.8




Manual Integrations
 APPROVED


Reviewed By :Rahul Chavli 08/27/2025
 Supervised By :Jagrut Upadhyay 08/27/2025

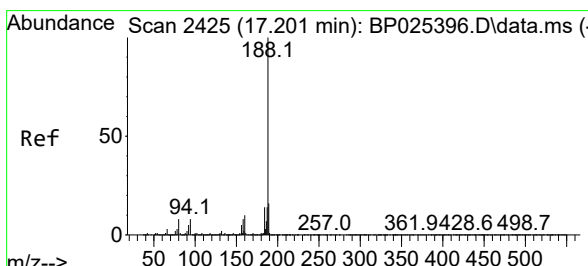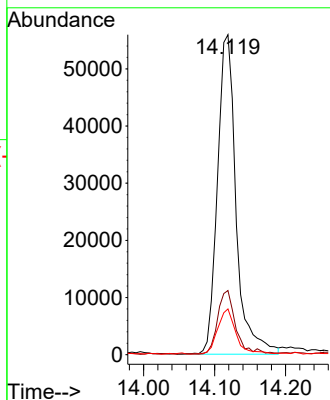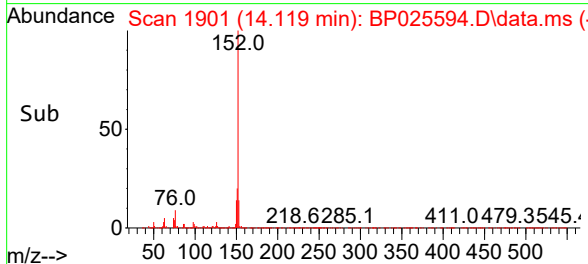

#64
 Phenanthrene-d10
 Concen: 20.000 ng
 RT: 17.195 min Scan# 2424
 Delta R.T. -0.006 min
 Lab File: BP025594.D
 Acq: 26 Aug 2025 20:44

Tgt Ion:188 Resp: 1107950
 Ion Ratio Lower Upper
 188 100
 94 8.6 6.6 10.0
 80 9.5 6.7 10.1

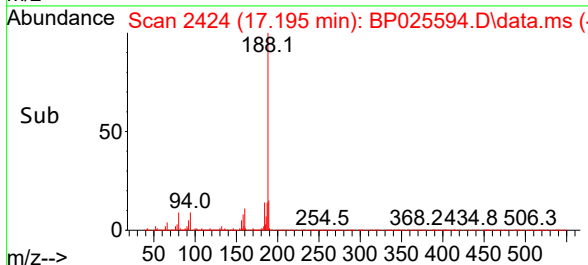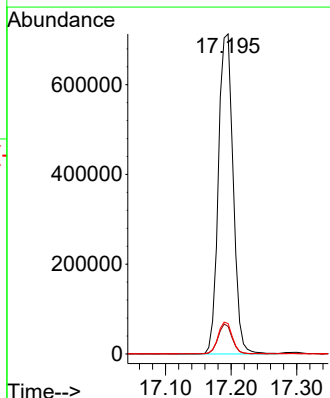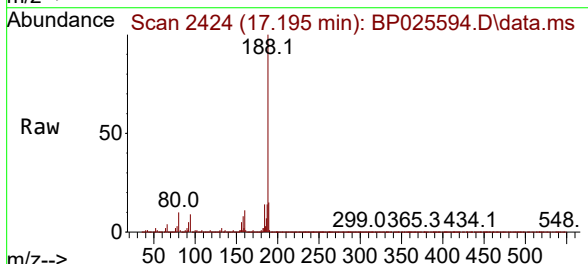

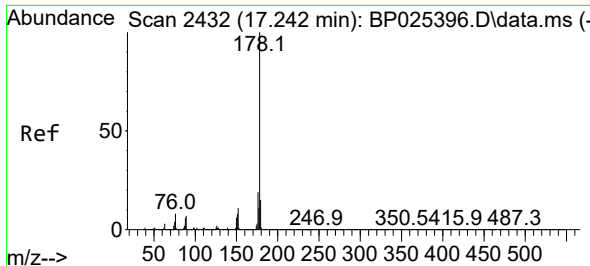





#71
Phenanthrene
Concen: 7.386 ng
RT: 17.236 min Scan# 2432
Delta R.T. -0.006 min
Lab File: BP025594.D
Acq: 26 Aug 2025 20:44

Instrument :
BNA_P
ClientSampleId :
27-BELL

Tgt Ion:178 Resp: 44952
Ion Ratio Lower Upper
178 100
176 19.0 15.5 23.3
179 15.4 12.2 18.4




Manual Integrations
APPROVED


Reviewed By :Rahul Chavli 08/27/2025
Supervised By :Jagrut Upadhyay 08/27/2025

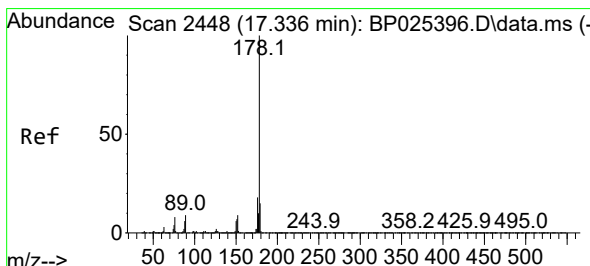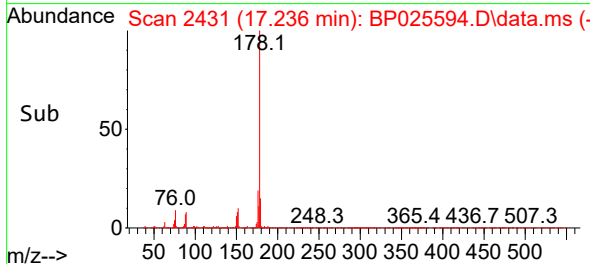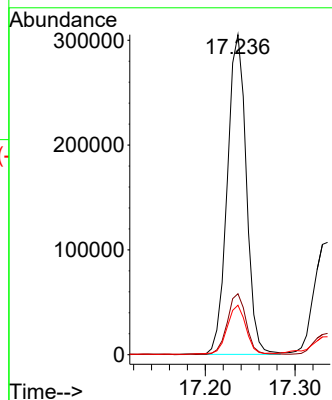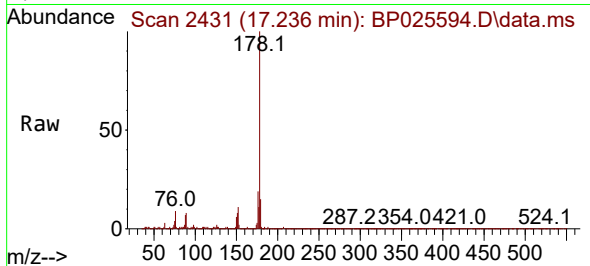

#72
Anthracene
Concen: 2.698 ng
RT: 17.336 min Scan# 2448
Delta R.T. 0.000 min
Lab File: BP025594.D
Acq: 26 Aug 2025 20:44


Tgt Ion:178 Resp: 167691
Ion Ratio Lower Upper
178 100
176 18.9 14.7 22.1
179 16.0 12.2 18.2

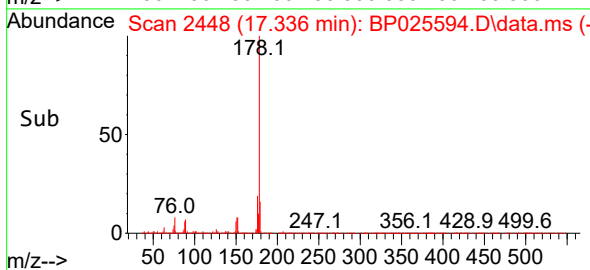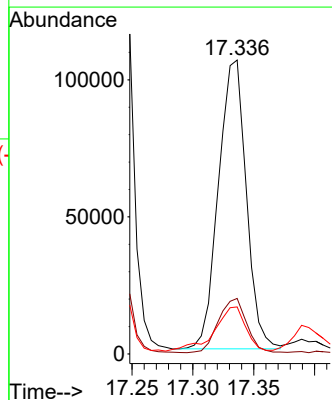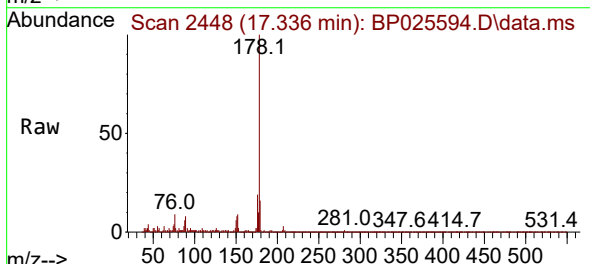



#75
Fluoranthene
Concen: 21.623 ng
RT: 19.319 min Scan# 21
Delta R.T. -0.006 min
Lab File: BP025594.D
Acq: 26 Aug 2025 20:44




Instrument :
BNA_P
ClientSampleId :
27-BELL



Tgt Ion:202 Resp: 156984
Ion Ratio Lower Upper
202 100
101 10.7 0.0 31.1
203 17.6 0.0 37.3




Manual Integrations
APPROVED


Reviewed By :Rahul Chavli 08/27/2025
Supervised By :Jagrut Upadhyay 08/27/2025

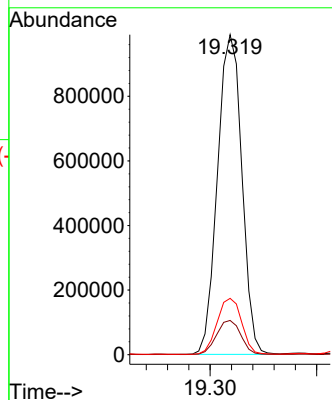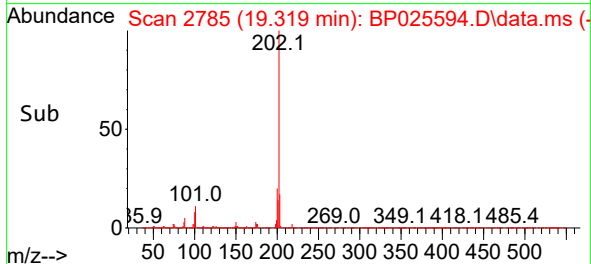

#76
Chrysene-d12
Concen: 20.000 ng
RT: 21.636 min Scan# 3179
Delta R.T. -0.012 min
Lab File: BP025594.D
Acq: 26 Aug 2025 20:44

Tgt Ion:240 Resp: 1177876
Ion Ratio Lower Upper
240 100
120 10.0 8.9 13.3
236 25.5 19.8 29.8

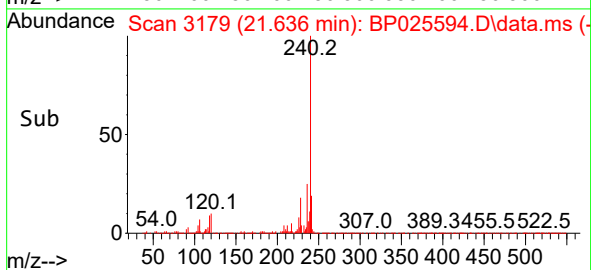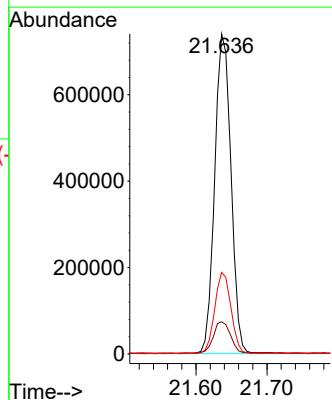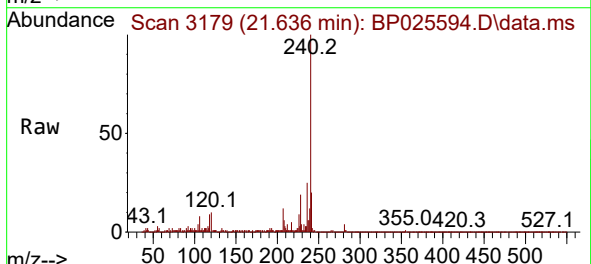



#78

Pyrene

Concen: 19.118 ng

RT: 19.695 min Scan# 2849

Delta R.T. -0.006 min

Lab File: BP025594.D

Acq: 26 Aug 2025 20:44

Instrument :

BNA_P

ClientSampleId :

27-BELL

Tgt Ion:202 Resp: 1463678

Ion Ratio Lower Upper

202 100

200 20.6 16.9 25.3





203 17.8 14.2 21.2

Manual Integrations

APPROVED

Reviewed By :Rahul Chavli 08/27/2025

Supervised By :Jagrut Upadhyay 08/27/2025

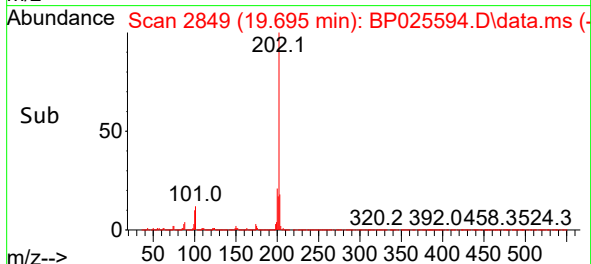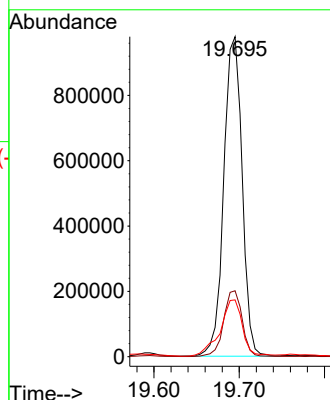

#79

Terphenyl-d14

Concen: 44.845 ng

RT: 19.907 min Scan# 2885

Delta R.T. -0.012 min

Lab File: BP025594.D

Acq: 26 Aug 2025 20:44




Tgt Ion:244 Resp: 2887144


Ion Ratio Lower Upper

244 100

212 7.0 5.8 8.6


122 10.0 7.4 11.2

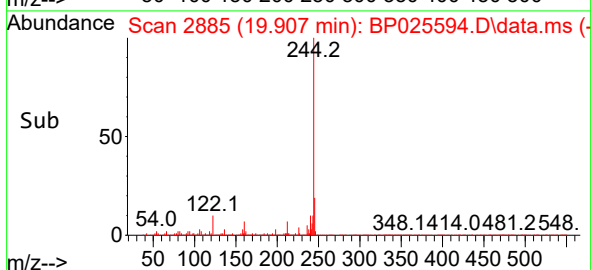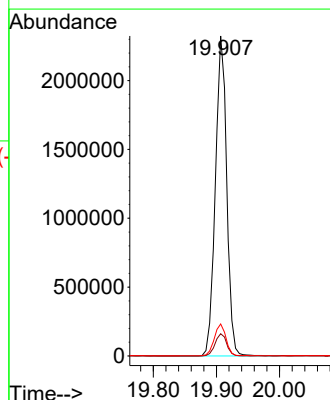



#81
Benzo(a)anthracene
Concen: 12.197 ng
RT: 21.619 min Scan# 3176
Delta R.T. -0.012 min
Lab File: BP025594.D
Acq: 26 Aug 2025 20:44




Instrument :
BNA_P
ClientSampleId :
27-BELL




Tgt Ion:228 Resp: 947450
Ion Ratio Lower Upper
228 100
226 28.8 21.7 32.5
229 20.2 15.6 23.4

Manual Integrations
APPROVED



Reviewed By :Rahul Chavli 08/27/2025
Supervised By :Jagrut Upadhyay 08/27/2025

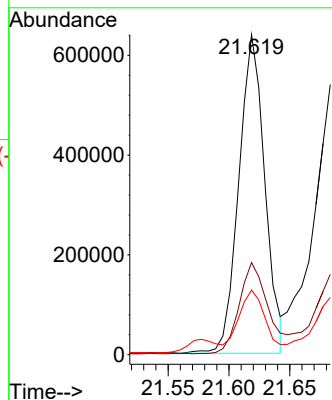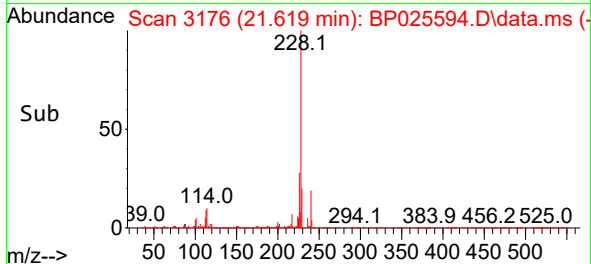


#83
Chrysene
Concen: 13.276 ng m
RT: 21.683 min Scan# 3187
Delta R.T. -0.012 min
Lab File: BP025594.D
Acq: 26 Aug 2025 20:44

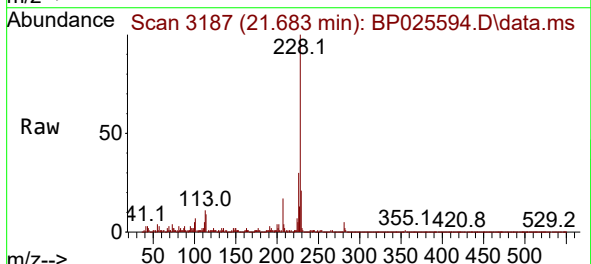

Tgt Ion:228 Resp: 965816
Ion Ratio Lower Upper
228 100
226 29.7 23.2 34.8
229 21.2 15.6 23.4

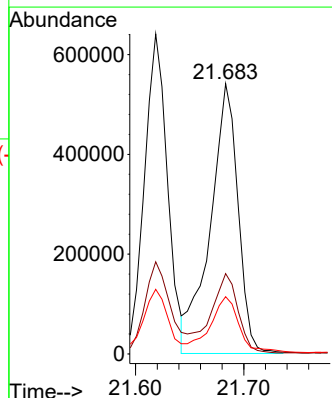



#86

Perylene-d12

Concen: 20.000 ng

RT: 25.018 min Scan# 31

Delta R.T. -0.012 min

Lab File: BP025594.D

Acq: 26 Aug 2025 20:44

Instrument :

BNA_P

ClientSampleId :

27-BELL

Tgt Ion:264 Resp: 1387698

Ion Ratio Lower Upper

264 100

260 23.6 19.3 28.9





265 22.0 17.4 26.0

Manual Integrations

APPROVED

Reviewed By :Rahul Chavli 08/27/2025

Supervised By :Jagrut Upadhyay 08/27/2025

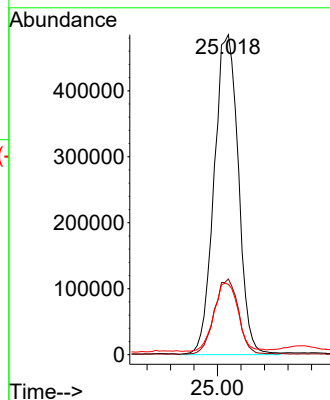

#87

Indeno(1,2,3-cd)pyrene

Concen: 7.302 ng

RT: 28.865 min Scan# 4408

Delta R.T. 0.000 min

Lab File: BP025594.D

Acq: 26 Aug 2025 20:44




Tgt Ion:276 Resp: 743117


Ion Ratio Lower Upper

276 100

138 20.7 12.9 19.3#

277 25.5 17.0 25.6

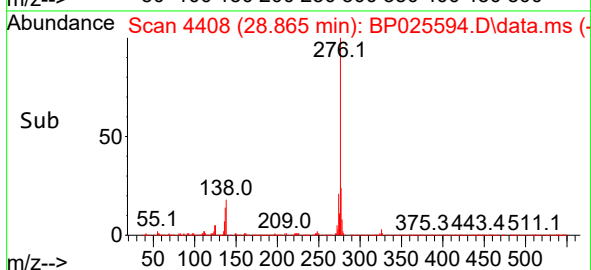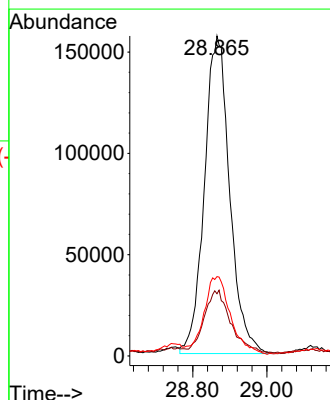



#88

Benzo(b)fluoranthene

Concen: 17.084 ng

RT: 23.948 min Scan# 3573

Delta R.T. -0.006 min

Lab File: BP025594.D

Acq: 26 Aug 2025 20:44

Instrument :

BNA_P

ClientSampleId :

27-BELL

Tgt Ion:252 Resp: 1397978

Ion Ratio Lower Upper

252 100

253 23.7 17.7 26.5





125 11.7 7.9 11.9

Manual Integrations

APPROVED

Reviewed By :Rahul Chavli 08/27/2025

Supervised By :Jagrut Upadhyay 08/27/2025

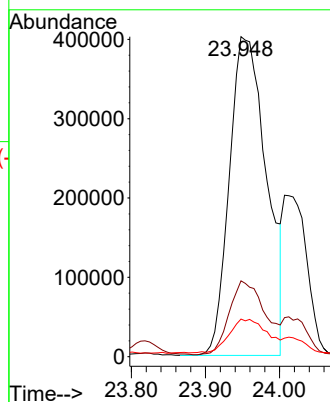

#89

Benzo(k)fluoranthene

Concen: 5.391 ng

RT: 24.007 min Scan# 3582

Delta R.T. -0.023 min

Lab File: BP025594.D

Acq: 26 Aug 2025 20:44




Tgt Ion:252 Resp: 441415


Ion Ratio Lower Upper

252 100

253 24.1 17.1 25.7

125 11.5 7.8 11.6

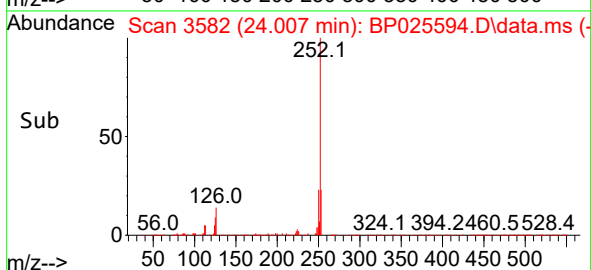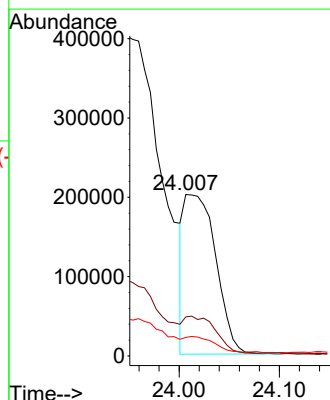



#90

Benzo(a)pyrene

Concen: 12.413 ng

RT: 24.854 min Scan# 31

Delta R.T. 0.000 min

Lab File: BP025594.D

Acq: 26 Aug 2025 20:44

Instrument :

BNA_P

ClientSampleId :

27-BELL

Tgt Ion:252 Resp: 988740

Ion Ratio Lower Upper

252 100

253 23.8 17.5 26.3





125 11.3 8.7 13.1

Manual Integrations

APPROVED

Reviewed By :Rahul Chavli 08/27/2025

Supervised By :Jagrut Upadhyay 08/27/2025

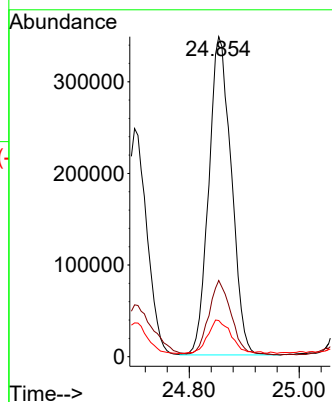

#91

Dibenzo(a,h)anthracene

Concen: 2.292 ng

RT: 28.936 min Scan# 4420

Delta R.T. -0.018 min

Lab File: BP025594.D

Acq: 26 Aug 2025 20:44




Tgt Ion:278 Resp: 190610


Ion Ratio Lower Upper

278 100

139 17.6 13.0 19.4

279 26.7 19.4 29.2

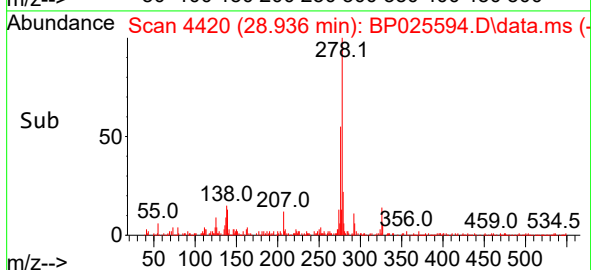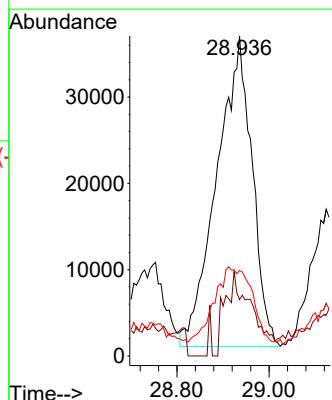



#92

Benzo(g,h,i)perylene

Concen: 8.400 ng

RT: 30.047 min Scan# 4

Delta R.T. -0.012 min

Lab File: BP025594.D


Acq: 26 Aug 2025 20:44

Instrument :

BNA_P

ClientSampleId :

27-BELL

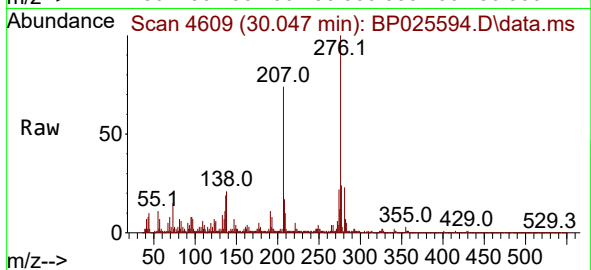

Tgt Ion:276 Resp: 68670

Ion Ratio Lower Upper

276 100

277 23.5 19.4 29.0

138 20.7 16.7 25.1

Manual Integrations

APPROVED

Reviewed By :Rahul Chavli 08/27/2025

Supervised By :Jagrut Upadhyay 08/27/2025

