
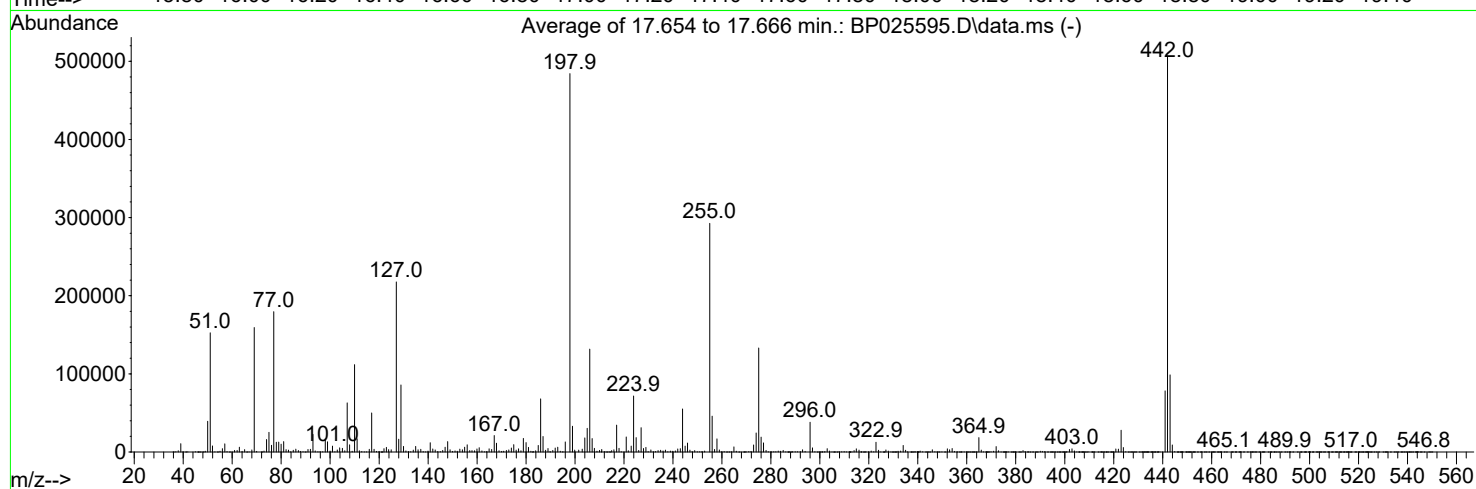


Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP082725\
Data File : BP025595.D
Acq On : 27 Aug 2025 08:58
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP081425.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Thu Aug 14 18:14:31 2025

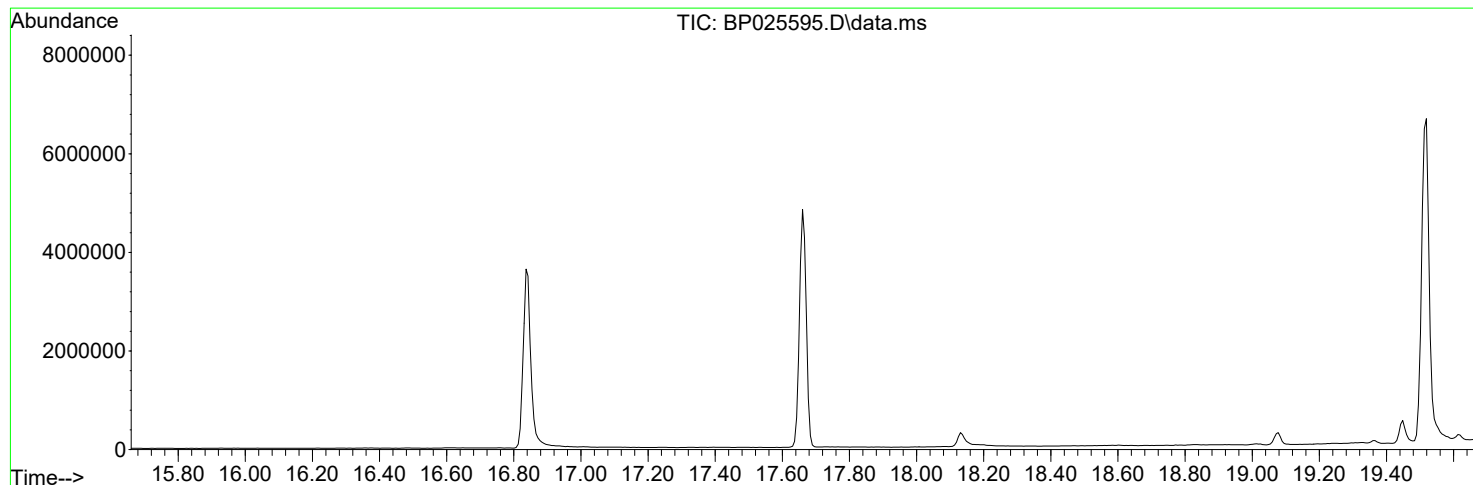

AutoFind: Scans 2502, 2503, 2504; Background Corrected with Scan 2495

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
68	69	0.00	2	1.7	2647	PASS
69	69	100	100	100.0	159279	PASS
70	69	0.00	2	0.6	914	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	484263	PASS
199	198	5	9	6.8	33059	PASS
365	198	1	100	3.8	18407	PASS
441	443	0.01	150	79.2	78301	PASS
442	442	100	100	100.0	505318	PASS
443	442	15	24	19.6	98803	PASS

DDT Breakdown




Date	Instrument Name	DFTPP Data File
8/27/2025	BNA_P	<u>BP025595.D</u>
Compound Name	Response	Retention Time
DDT	2242813	20.807
DDD	65606	20.342
DDE	9202	19.819
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
74808	2317621	3.23

Instrument :
BNA_P
ClientSampleId :
DFTPP

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP082725\
Data File : BP025595.D
Acq On : 27 Aug 2025 08:58
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DFTPP

Quant Time: Aug 27 16:26:25 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP081425.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Aug 14 18:14:31 2025
Response via : Initial Calibration

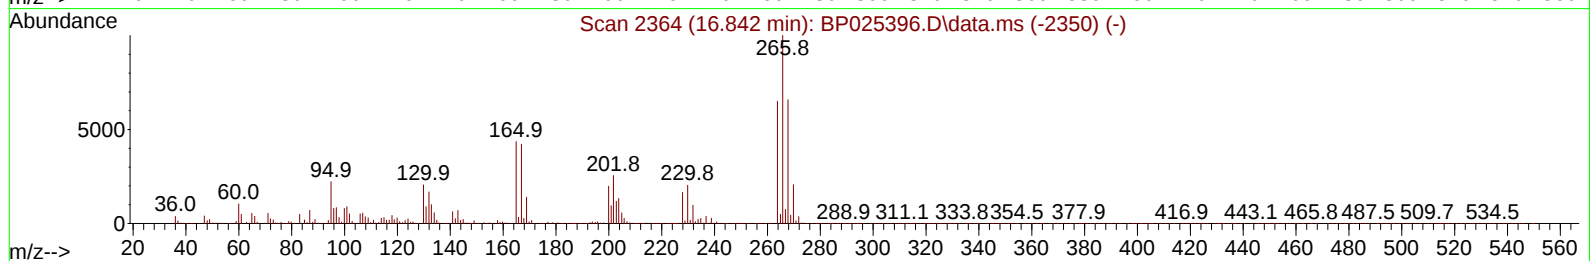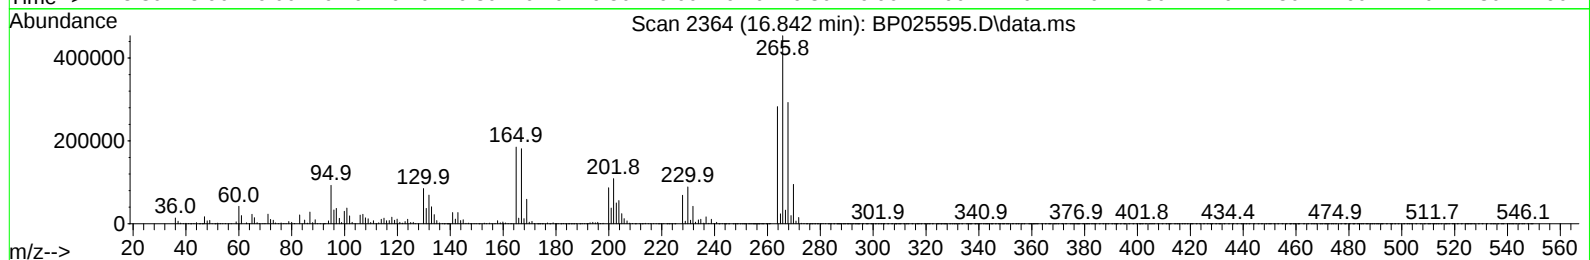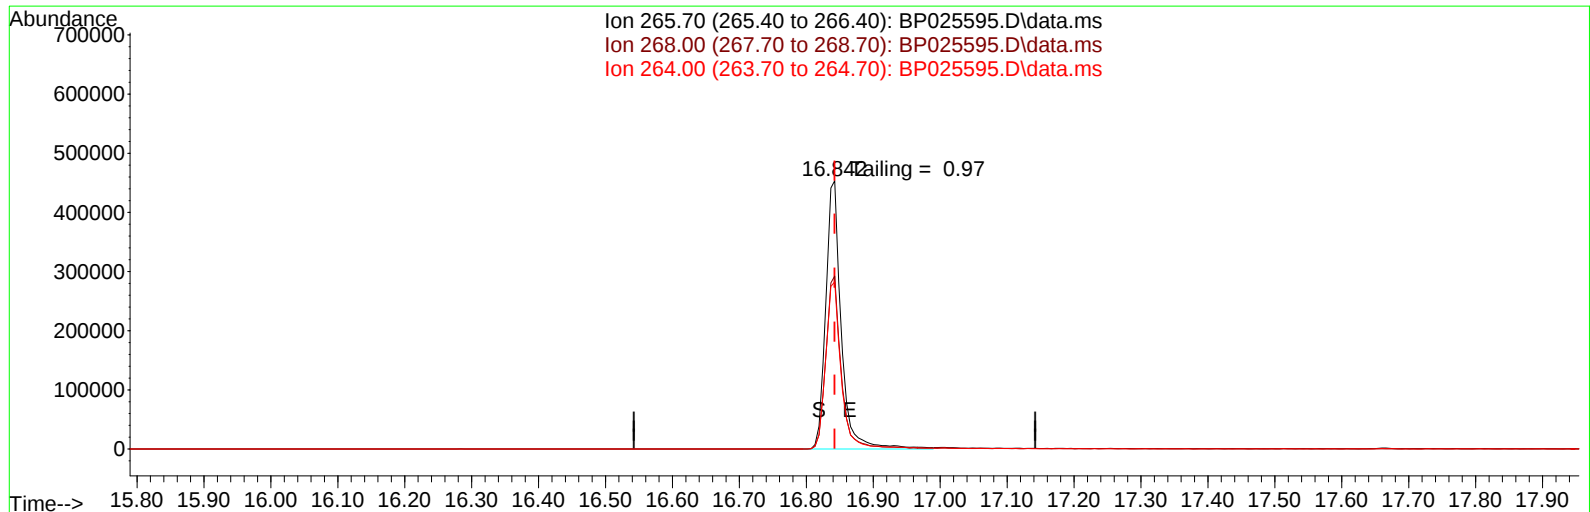

TIC: BP025595.D\data.ms

(70) Pentachlorophenol (C)

16.842min (+ 0.000) 1966640.70 ng




response 728058

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	65.80	64.47
264.00	65.00	62.33
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP082725\
Data File : BP025595.D
Acq On : 27 Aug 2025 08:58
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DFTPP

Quant Time: Aug 27 16:26:25 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP081425.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Aug 14 18:14:31 2025
Response via : Initial Calibration

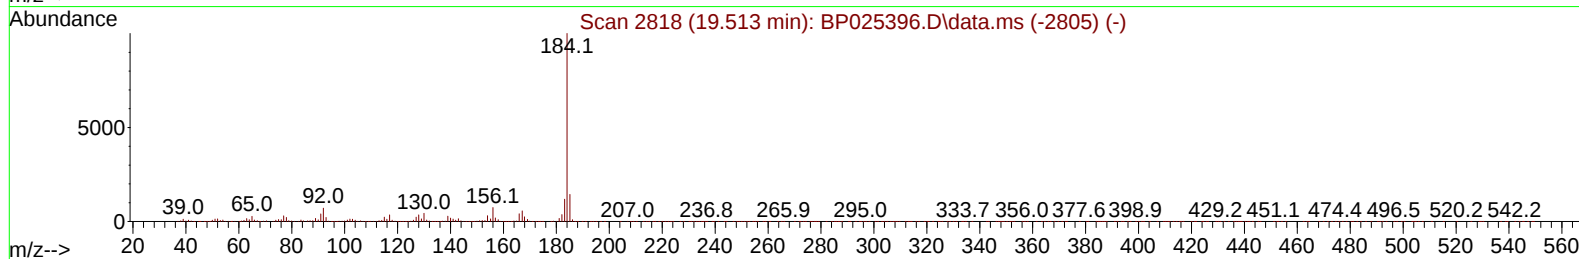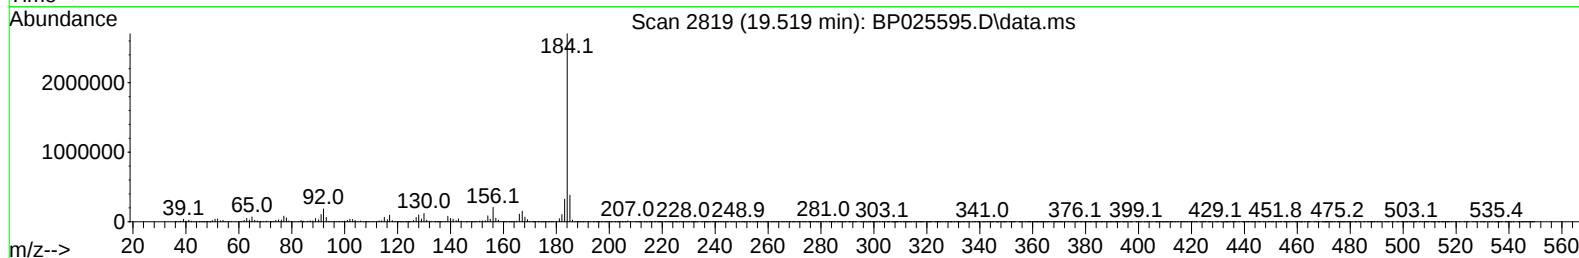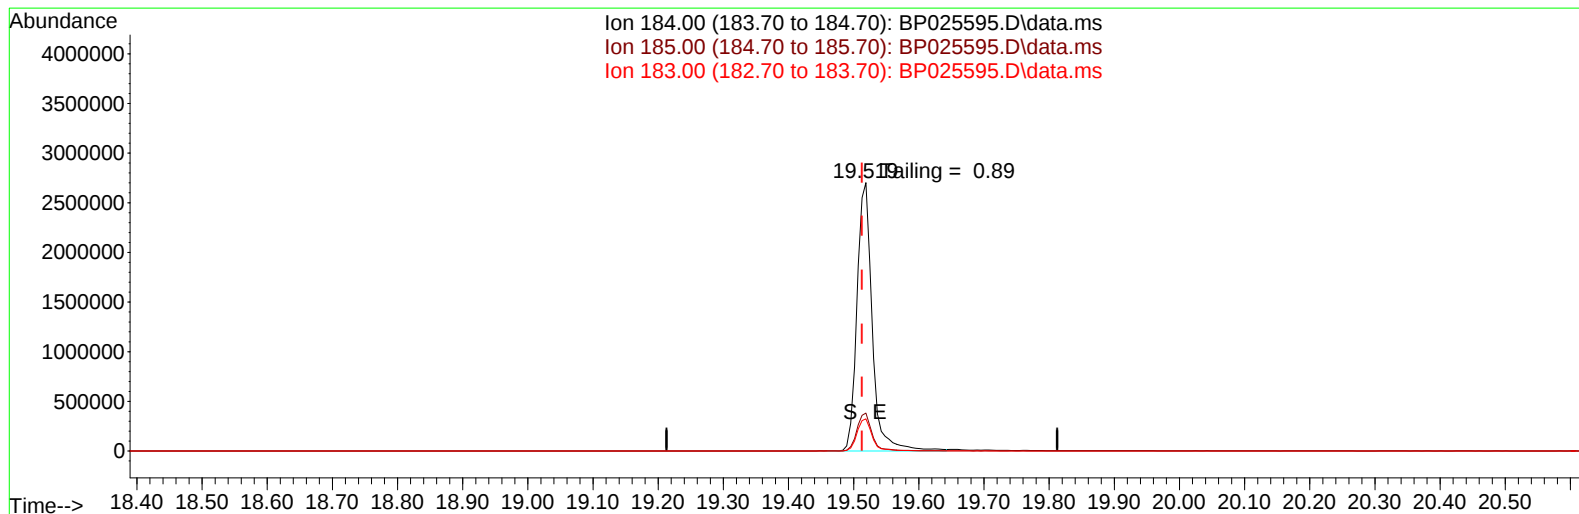

TIC: BP025595.D\data.ms

(77) Benzidine

19.519min (+ 0.006) 862145.80 ng

response 4384060

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.40	14.17
183.00	11.80	11.99
0.00	0.00	0.00